
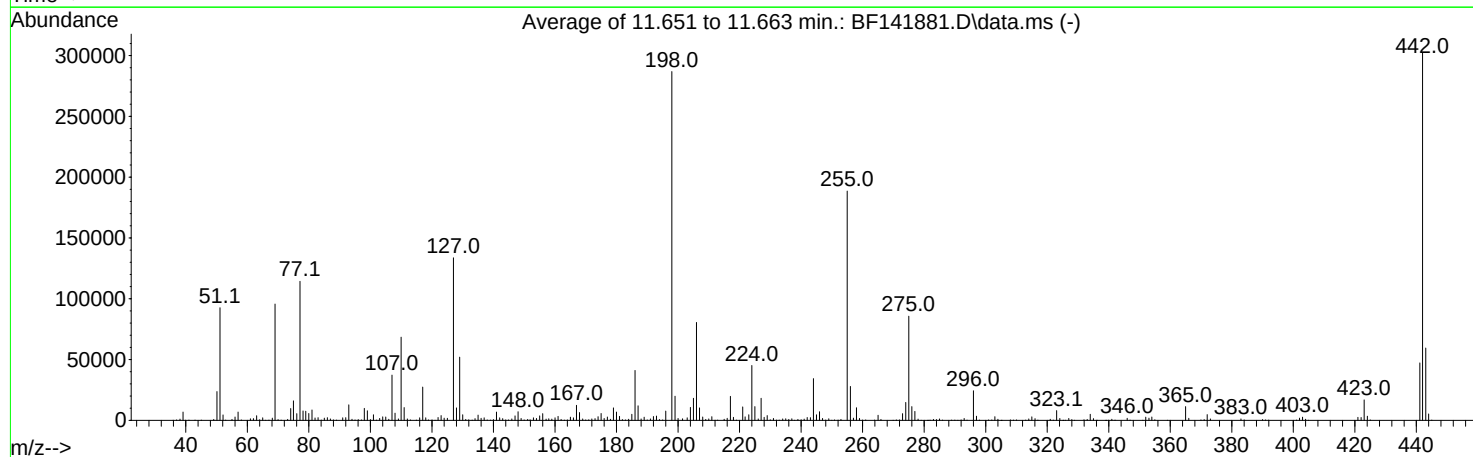


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030725\
Data File : BF141881.D
Acq On : 07 Mar 2025 08:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 28 01:48:16 2025

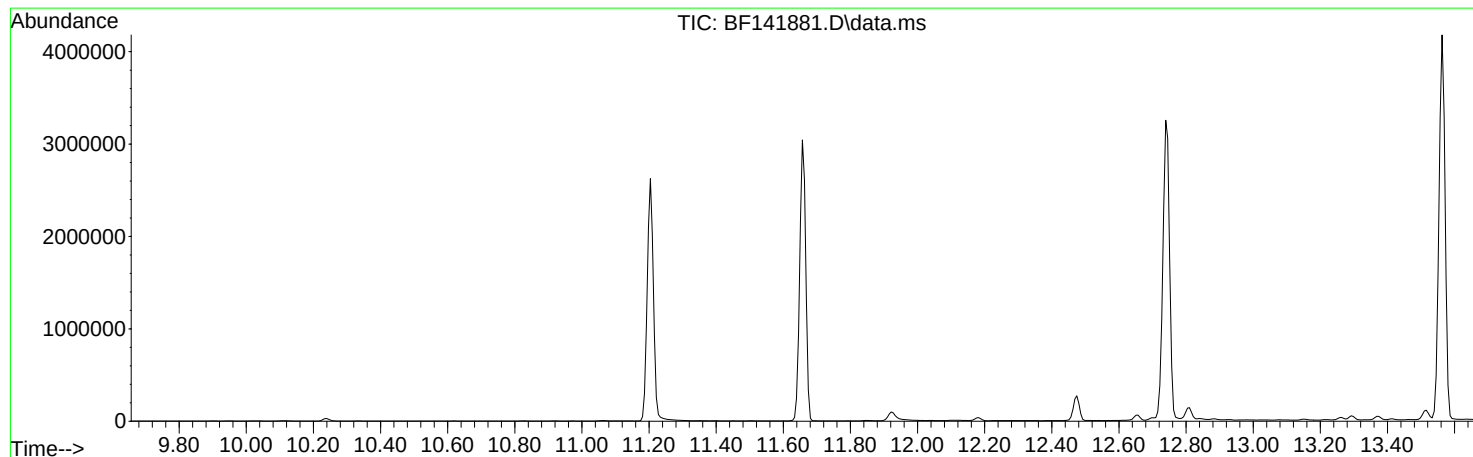

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	92640	PASS
68	69	0.00	2	2.0	1892	PASS
69	198	0.00	100	33.4	95707	PASS
70	69	0.00	2	0.8	730	PASS
127	198	10	80	46.6	133723	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	286869	PASS
199	198	5	9	6.9	19893	PASS
275	198	10	60	29.9	85757	PASS
365	198	1	100	4.0	11387	PASS
441	198	0.01	100	16.5	47280	PASS
442	442	50	100	100.0	302571	PASS
443	442	15	24	19.7	59485	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/7/2025	BNA_F	<u>BF141881.D</u>
Compound Name	Response	Retention Time
DDT	1053294	13.563
DDD	17562	13.292
DDE	1240	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18802	1072096	1.75

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030725\
Data File : BF141881.D
Acq On : 07 Mar 2025 08:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 07 09:59:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

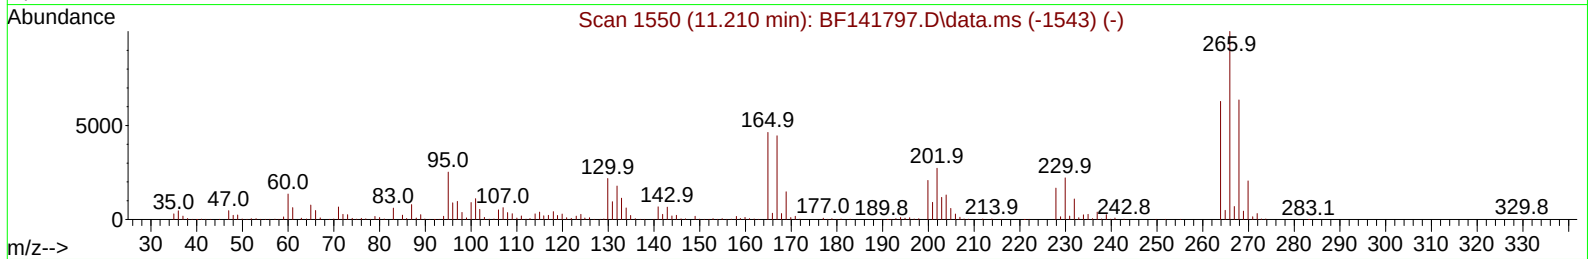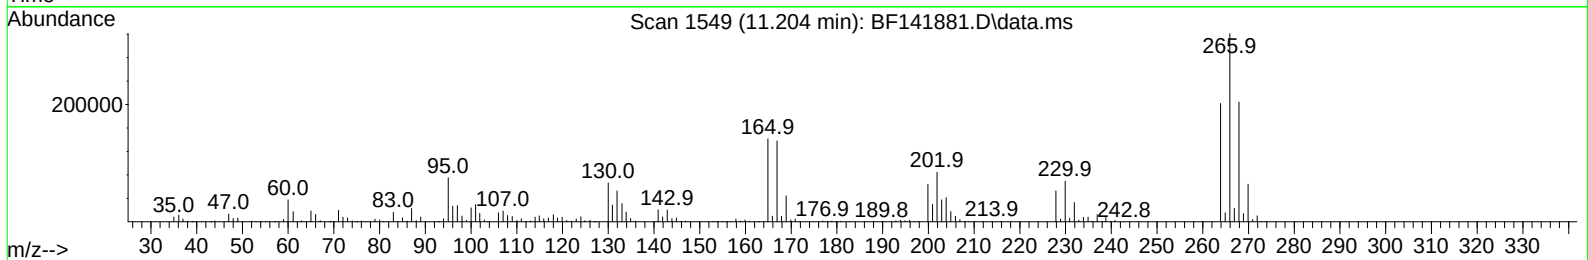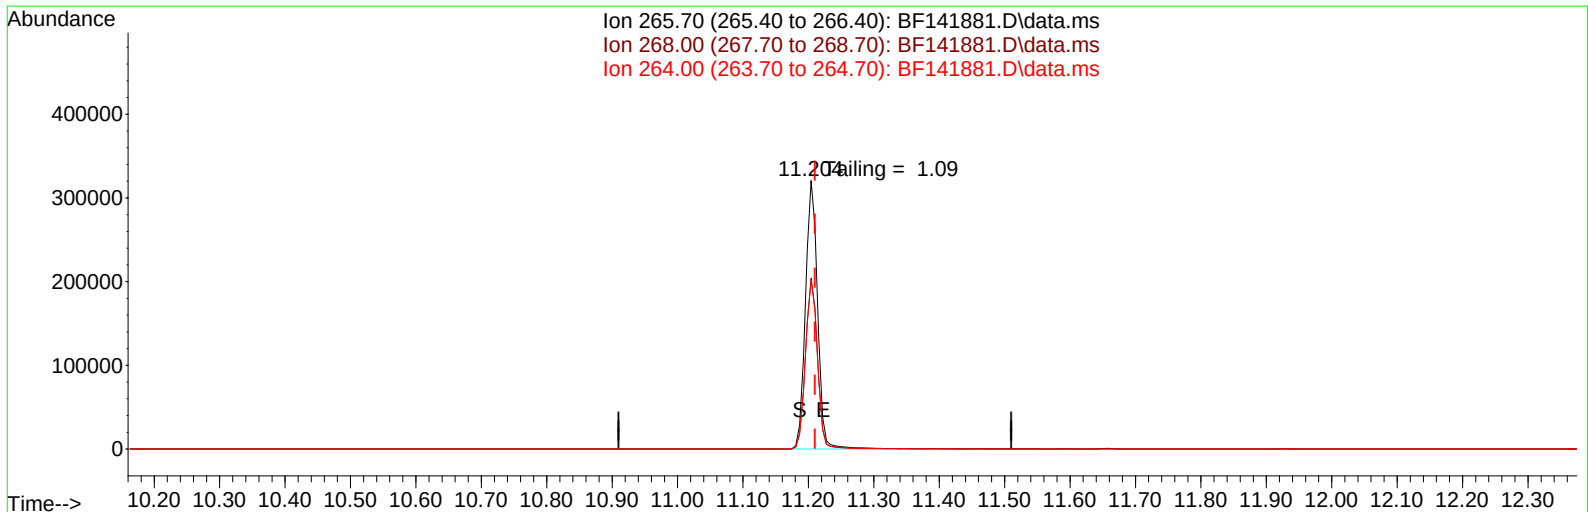

TIC: BF141881.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 136401.80 ng




response 416145

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.68
264.00	62.80	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030725\
Data File : BF141881.D
Acq On : 07 Mar 2025 08:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 07 09:59:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

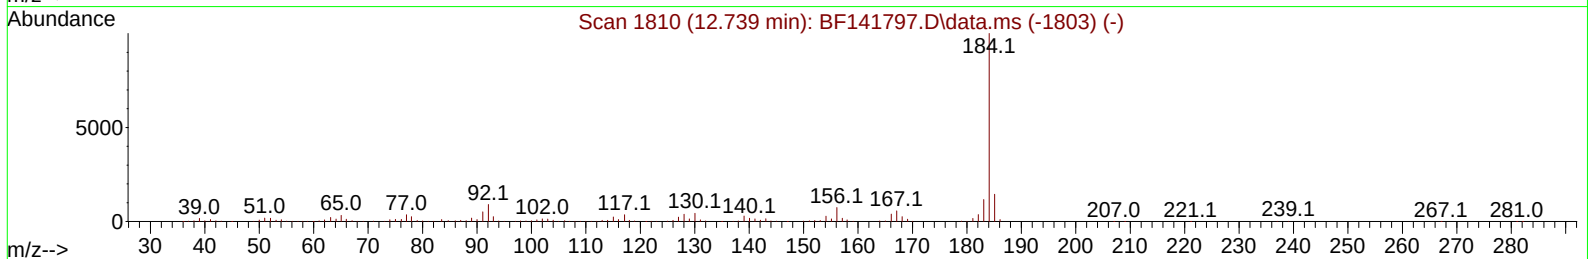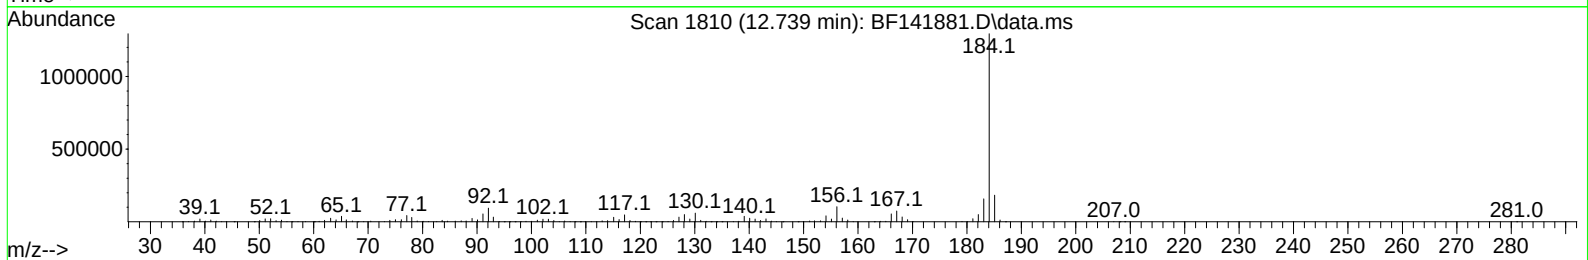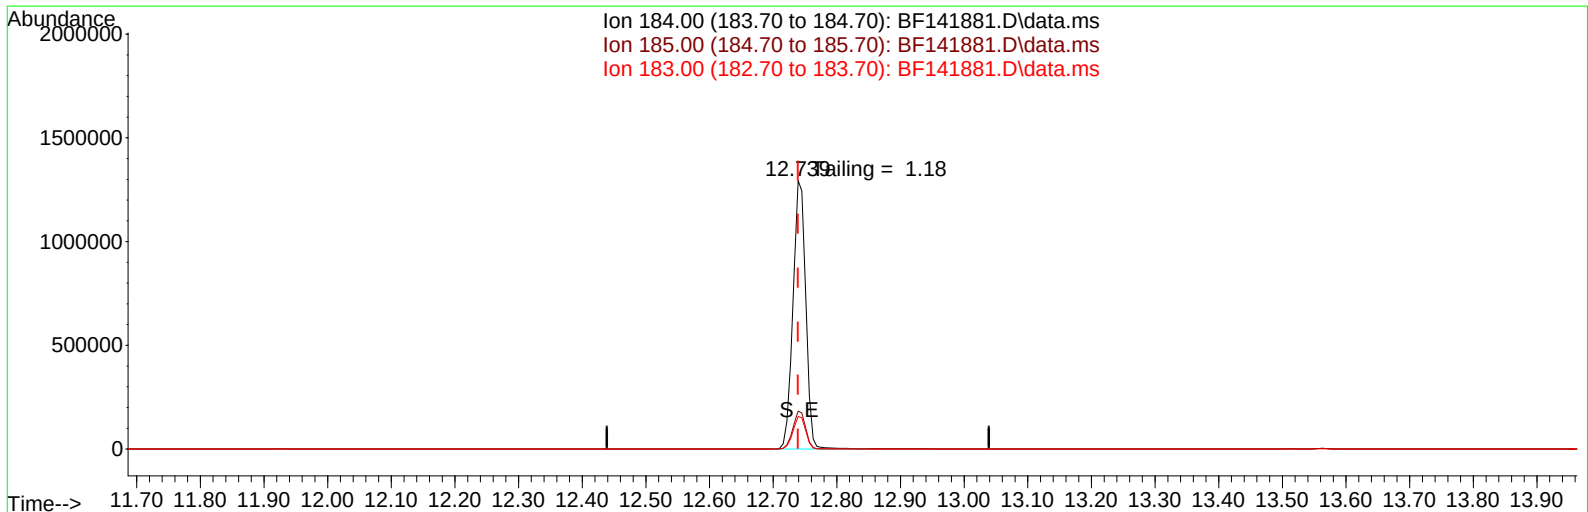

TIC: BF141881.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 161104.25 ng

response 1816840

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.17
183.00	11.70	12.15
0.00	0.00	0.00