


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX030625\
Data File : VX045154.D
Acq On : 06 Mar 2025 09:09
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Title : SW846 8260
Last Update : Fri Feb 28 06:45:16 2025

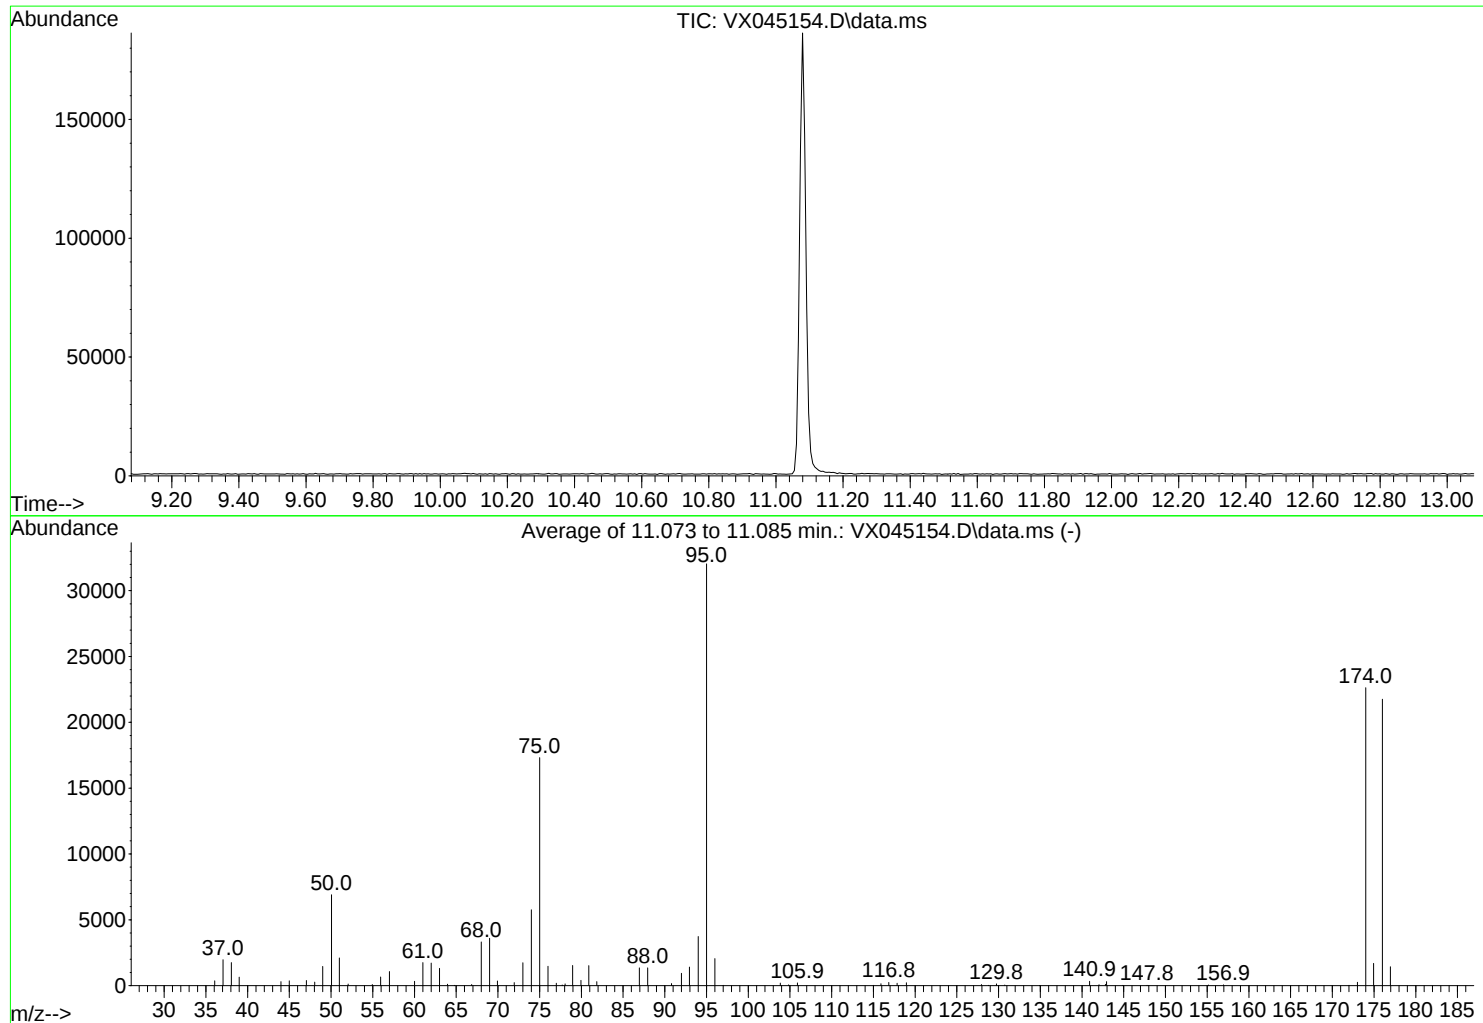

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.5	6899	PASS
75	95	30	60	54.0	17313	PASS
95	95	100	100	100.0	32037	PASS
96	95	5	9	6.4	2059	PASS
173	174	0.00	2	1.1	256	PASS
174	95	50	100	70.6	22629	PASS
175	174	5	9	7.5	1688	PASS
176	174	95	101	96.1	21751	PASS
177	176	5	9	6.6	1434	PASS