

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030625\
 Data File : P0109655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2025 13:06
 Operator : YP/AJ
 Sample : Q1498-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 4A-4B-4C-1928 BLD-WINDOW

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/07/2025
 Supervised By :mohammad ahmed 03/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 13:43:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.694	217.3E6	124.6E6	22.954m	23.813m
2) SA Decachlor...	8.756	8.707	178.3E6	71992286	20.728	22.609m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030625\
Data File : PO109655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2025 13:06
Operator : YP/AJ
Sample : Q1498-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
4A-4B-4C-1928 BLD-WINDOW


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2025
Supervised By :mohammad ahmed 03/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 13:43:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

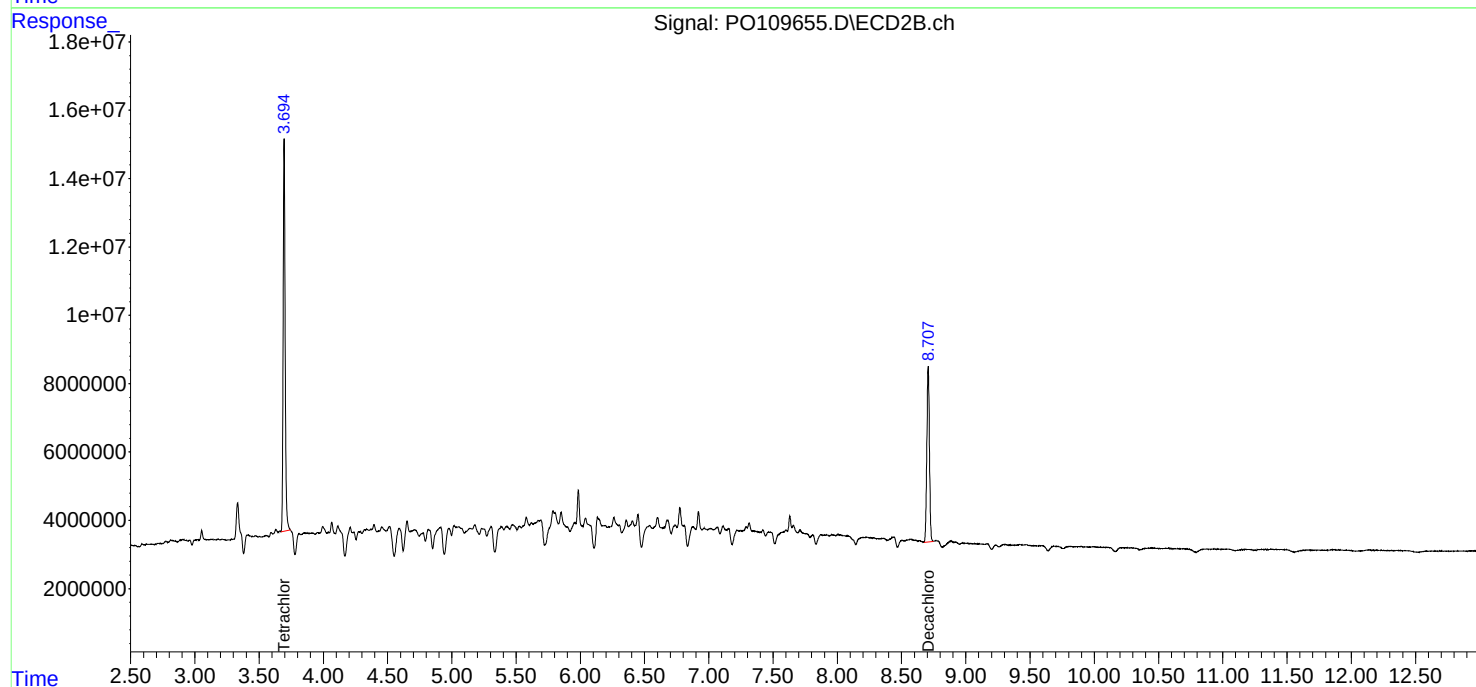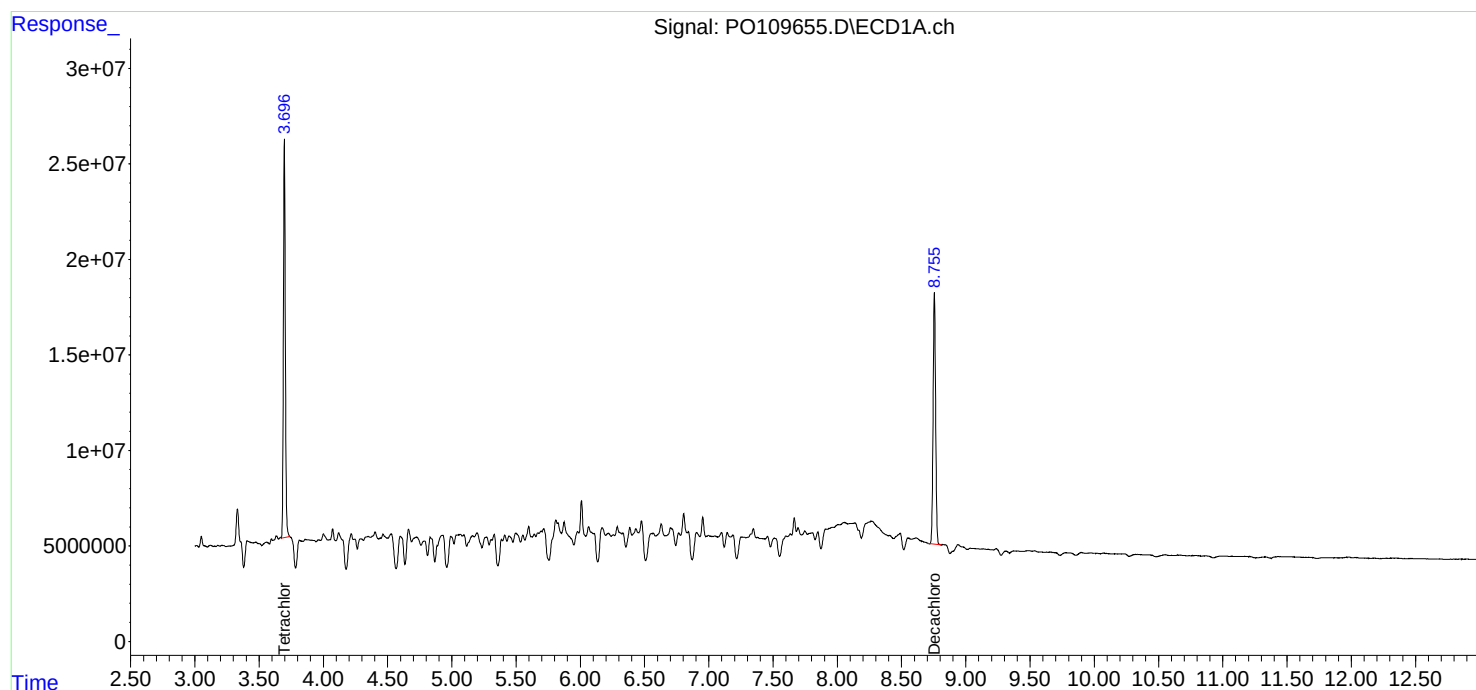

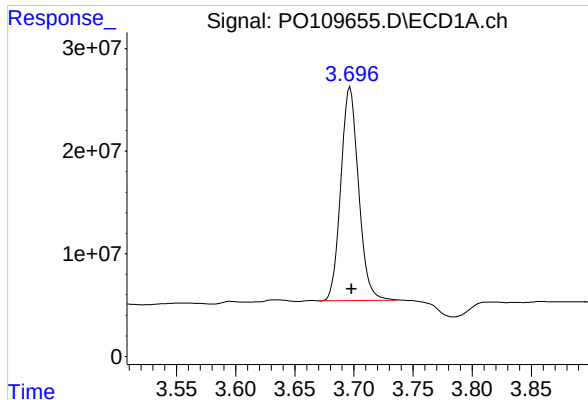


#1 Tetrachloro-m-xylene

R.T.: 3.696 min
Delta R.T.: -0.002 min
Response: 217262573
Conc: 22.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
4A-4B-4C-1928 BLD-WINDOW


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2025
Supervised By :mohammad ahmed 03/08/2025

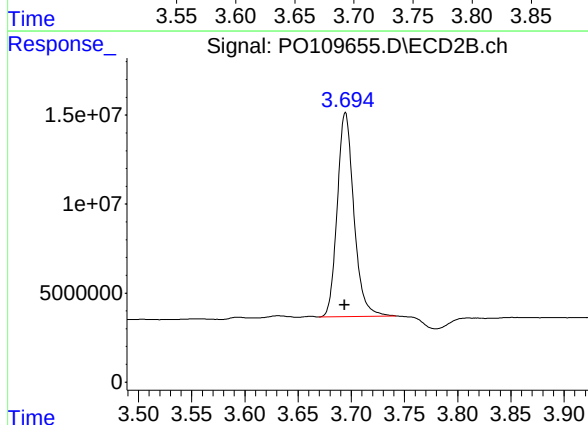


#1 Tetrachloro-m-xylene

R.T.: 3.694 min
Delta R.T.: 0.000 min
Response: 124640148
Conc: 23.81 ng/ml m

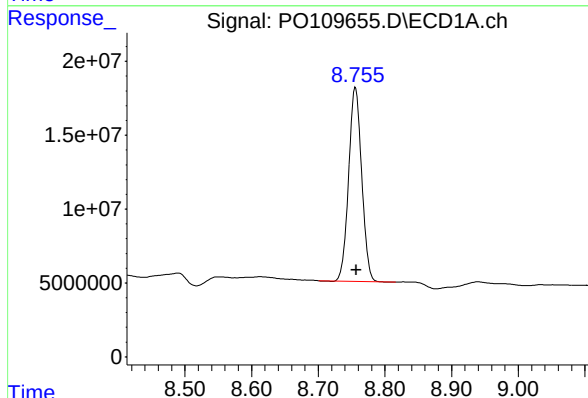

#2 Decachlorobiphenyl

R.T.: 8.756 min
Delta R.T.: 0.000 min
Response: 178301089
Conc: 20.73 ng/ml

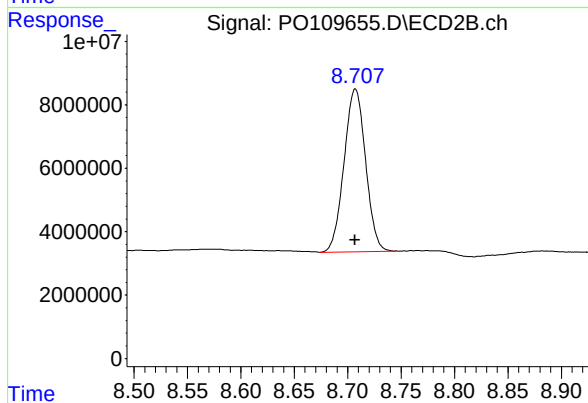

#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: 0.000 min
Response: 71992286
Conc: 22.61 ng/ml m