

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030625\
 Data File : P0109658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2025 14:01
 Operator : YP/AJ
 Sample : Q1498-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 7A-7B-7C-ROOF-5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/07/2025
 Supervised By :mohammad ahmed 03/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 00:08:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.695	200.2E6	119.7E6	21.148	22.869
2) SA Decachlor...	8.756	8.708	157.2E6	61306445	18.274m	19.253m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030625\
Data File : PO109658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2025 14:01
Operator : YP/AJ
Sample : Q1498-04
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
7A-7B-7C-ROOF-5


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2025
Supervised By :mohammad ahmed 03/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:08:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

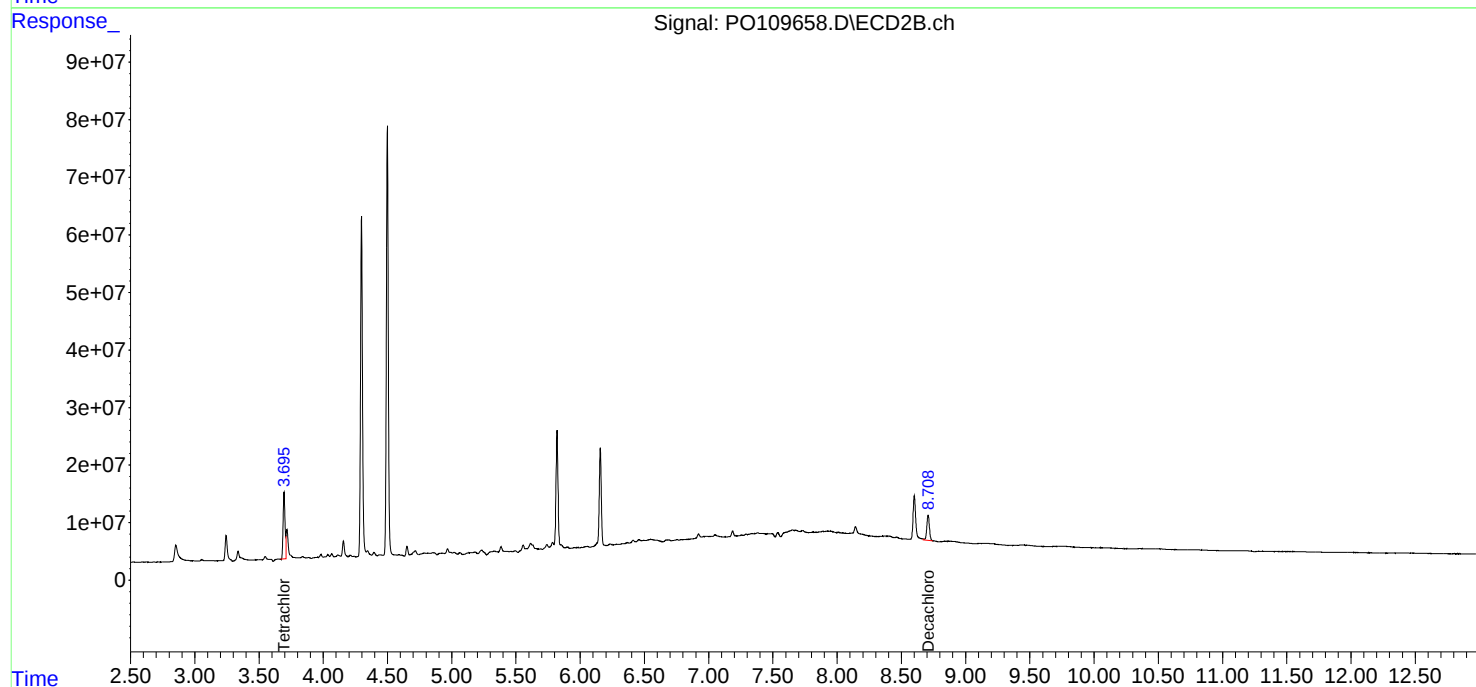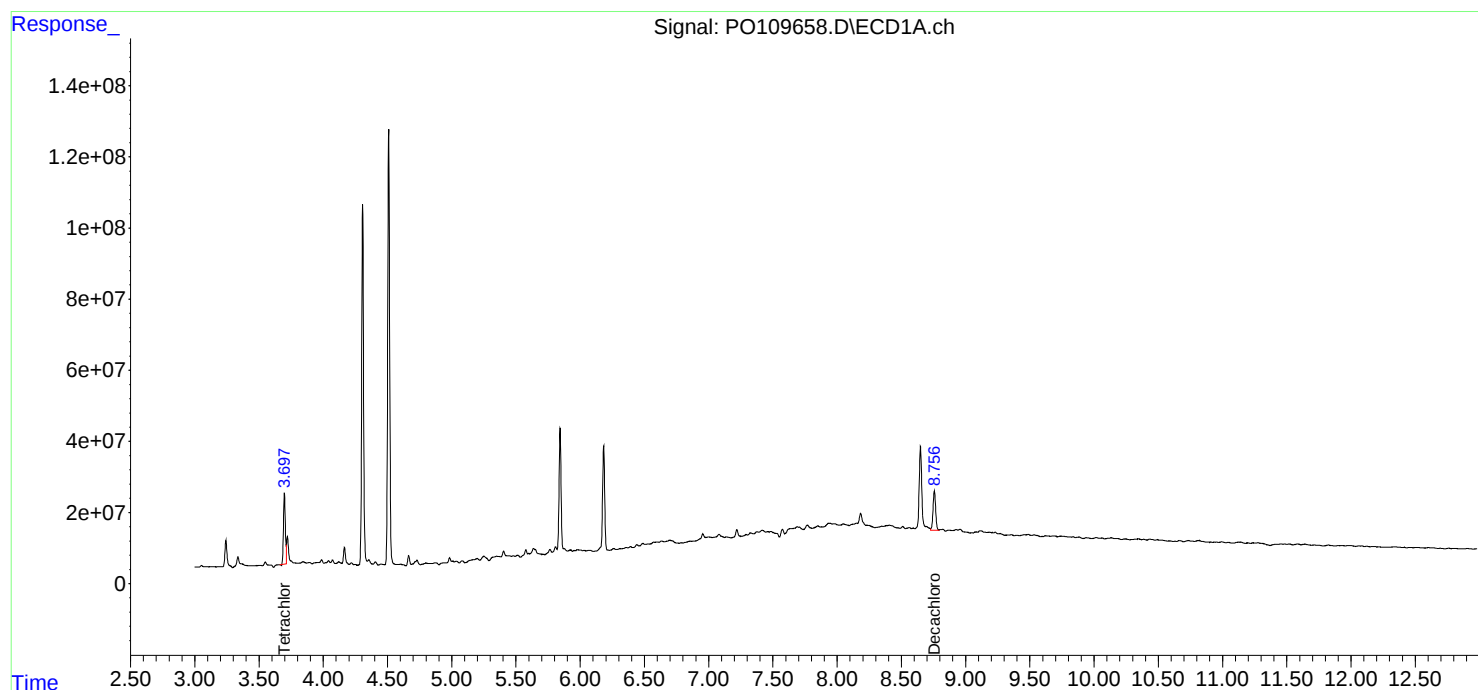

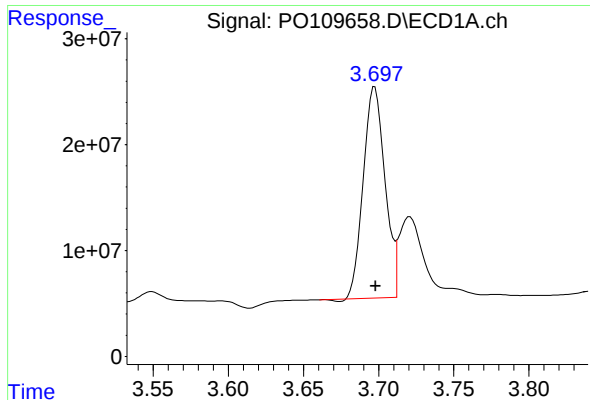


#1 Tetrachloro-m-xylene

R.T.: 3.697 min
Delta R.T.: 0.000 min
Response: 200164376
Conc: 21.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
7A-7B-7C-ROOF-5


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2025
Supervised By :mohammad ahmed 03/08/2025

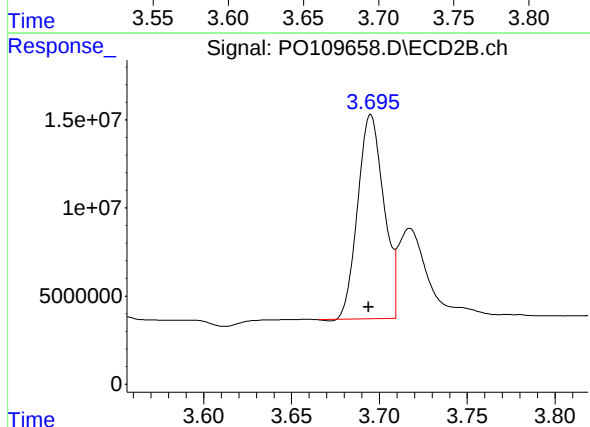


#1 Tetrachloro-m-xylene

R.T.: 3.695 min
Delta R.T.: 0.001 min
Response: 119703127
Conc: 22.87 ng/ml

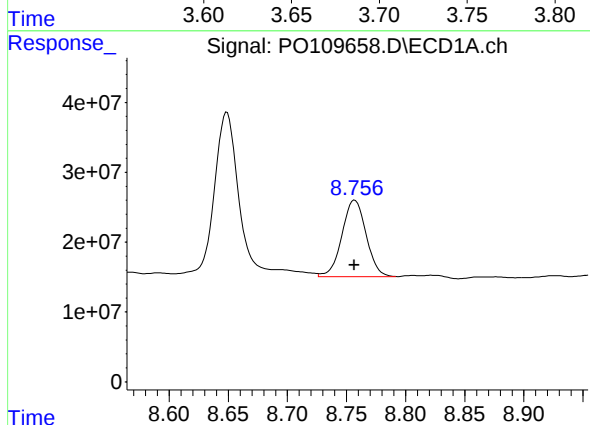

#2 Decachlorobiphenyl

R.T.: 8.756 min
Delta R.T.: 0.000 min
Response: 157188792
Conc: 18.27 ng/ml m

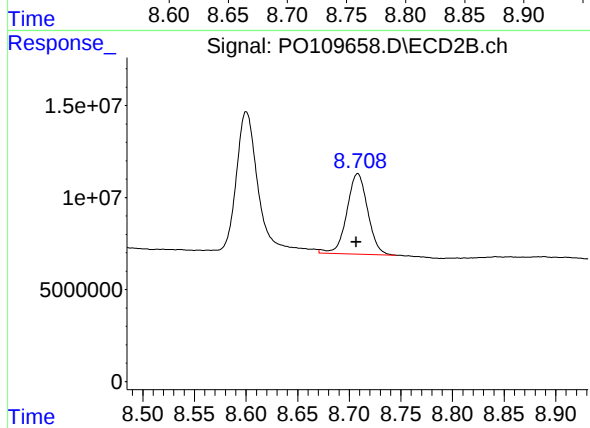

#2 Decachlorobiphenyl

R.T.: 8.708 min
Delta R.T.: 0.001 min
Response: 61306445
Conc: 19.25 ng/ml m