

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0030625\
 Data File : P0109661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2025 14:55
 Operator : YP/AJ
 Sample : Q1498-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 10A-10B-10C-ROOF-6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/07/2025
 Supervised By :mohammad ahmed 03/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 00:09:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.695	179.8E6	108.8E6	18.991	20.778
2) SA Decachlor...	8.756	8.707	168.6E6	71983275	19.595m	22.606m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO030625\
Data File : PO109661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2025 14:55
Operator : YP/AJ
Sample : Q1498-07
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
10A-10B-10C-ROOF-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2025
Supervised By :mohammad ahmed 03/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 00:09:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

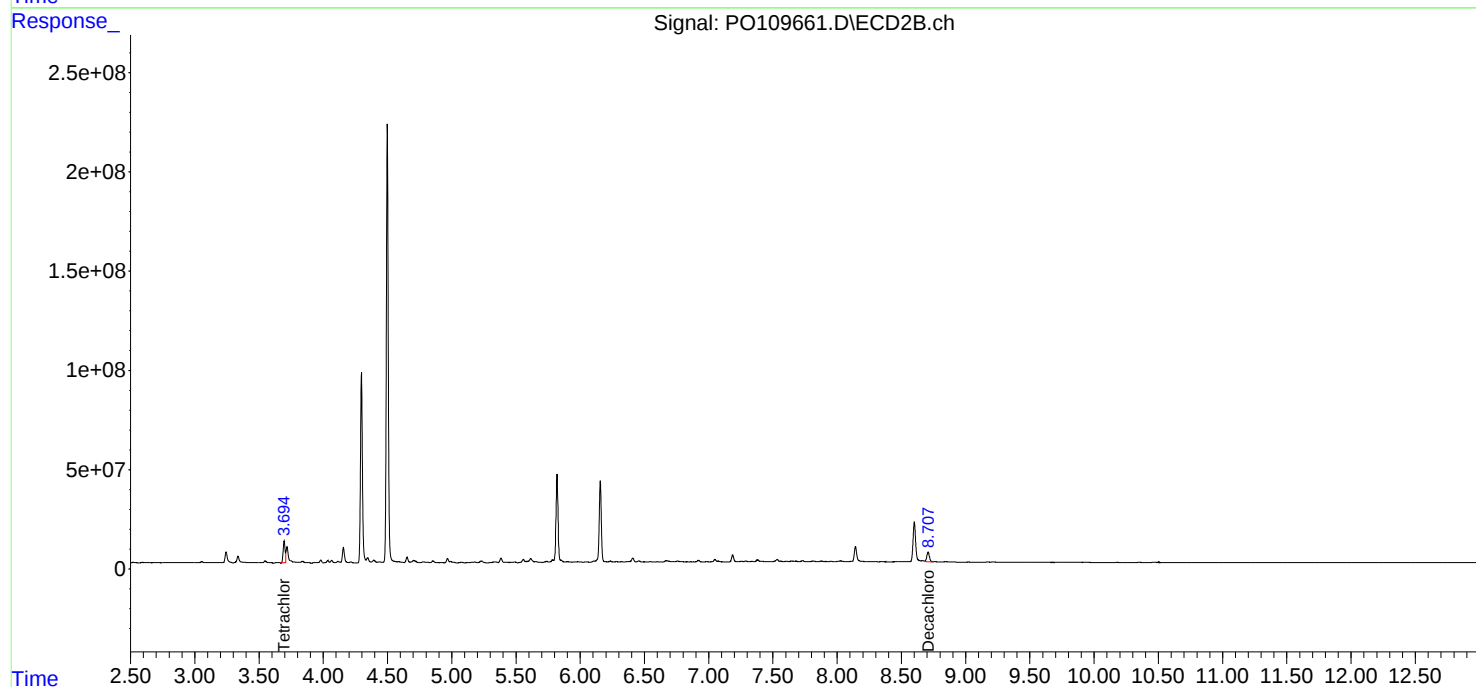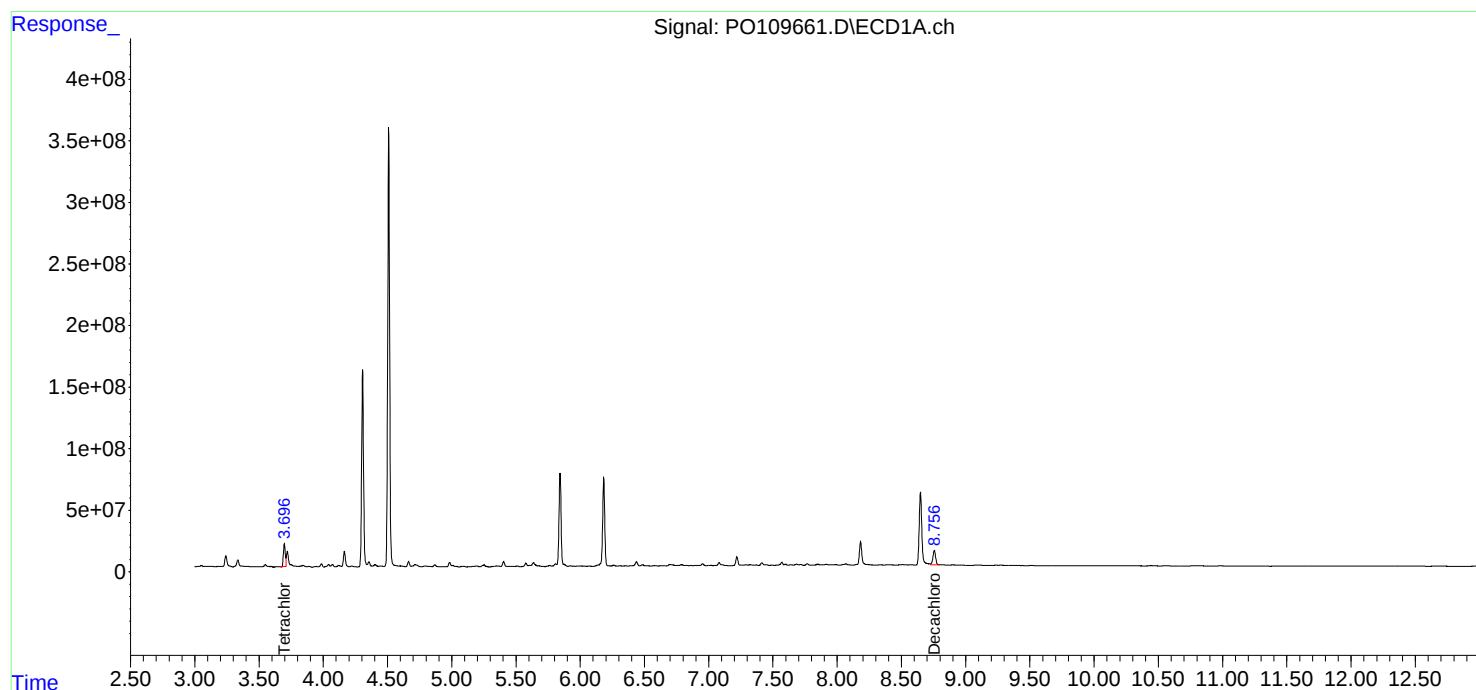

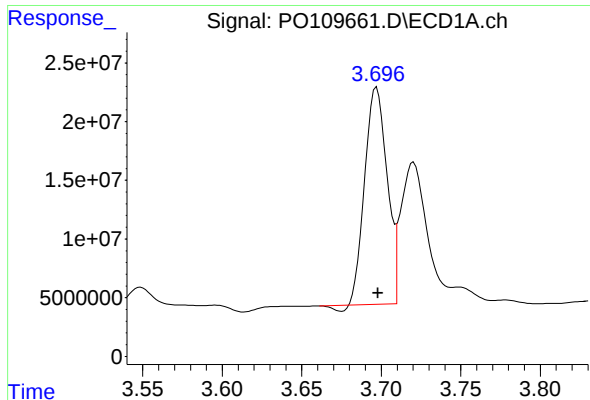


#1 Tetrachloro-m-xylene

R.T.: 3.697 min
Delta R.T.: 0.000 min
Response: 179750153
Conc: 18.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
10A-10B-10C-ROOF-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2025
Supervised By :mohammad ahmed 03/08/2025

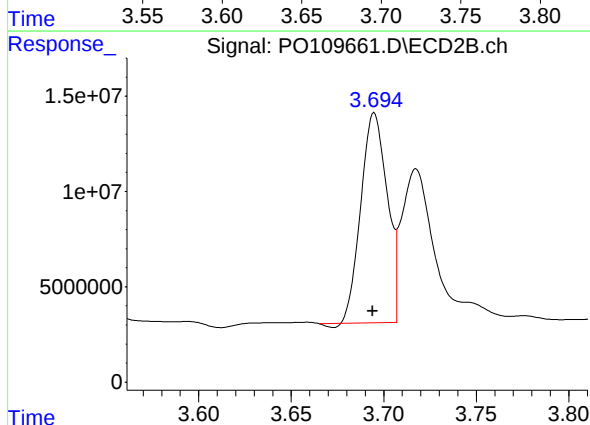


#1 Tetrachloro-m-xylene

R.T.: 3.695 min
Delta R.T.: 0.001 min
Response: 108755502
Conc: 20.78 ng/ml

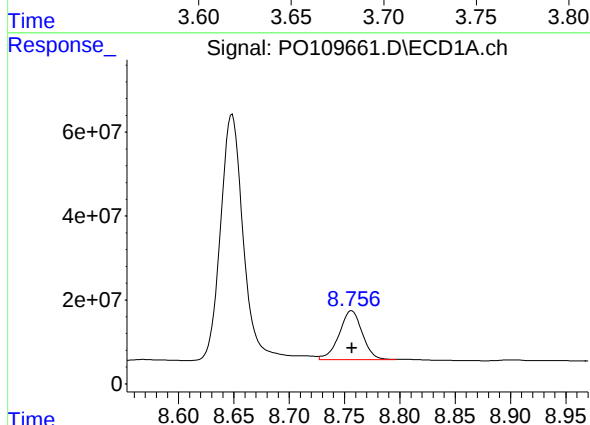

#2 Decachlorobiphenyl

R.T.: 8.756 min
Delta R.T.: 0.000 min
Response: 168556543
Conc: 19.60 ng/ml m

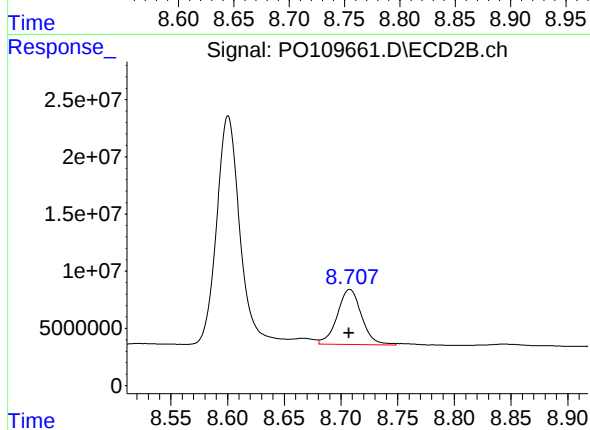

#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: 0.000 min
Response: 71983275
Conc: 22.61 ng/ml m