


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030725\
Data File : BN036543.D
Acq On : 07 Mar 2025 12:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN021025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 05 16:08:57 2025

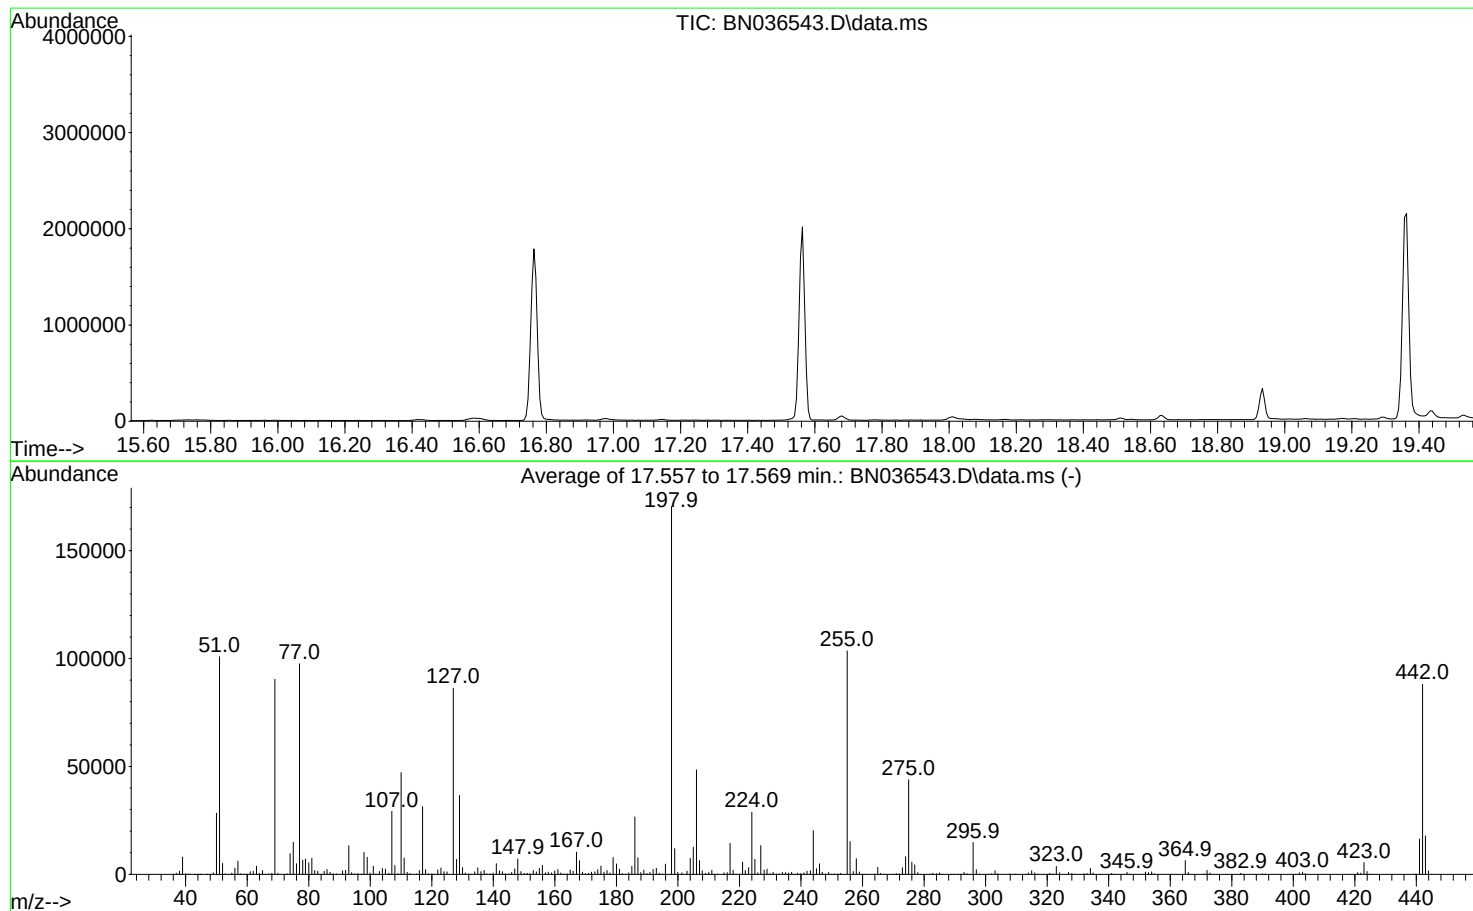

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	59.1	100816	PASS
68	69	0.00	2	0.6	506	PASS
69	198	0.00	100	53.0	90409	PASS
70	69	0.00	2	0.6	534	PASS
127	198	10	80	50.6	86237	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	170475	PASS
199	198	5	9	7.0	11922	PASS
275	198	10	60	25.7	43816	PASS
365	198	1	100	3.8	6410	PASS
441	198	0.01	100	9.6	16431	PASS
442	442	50	100	100.0	88096	PASS
443	442	15	24	20.2	17795	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/7/2025	BNA_N	<u>BN036543.D</u>
Compound Name	Response	Retention Time
DDT	743928	20.598
DDD	12190	20.157
DDE	771	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12961	756889	1.71

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030725\
Data File : BN036543.D
Acq On : 07 Mar 2025 12:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 07 17:45:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

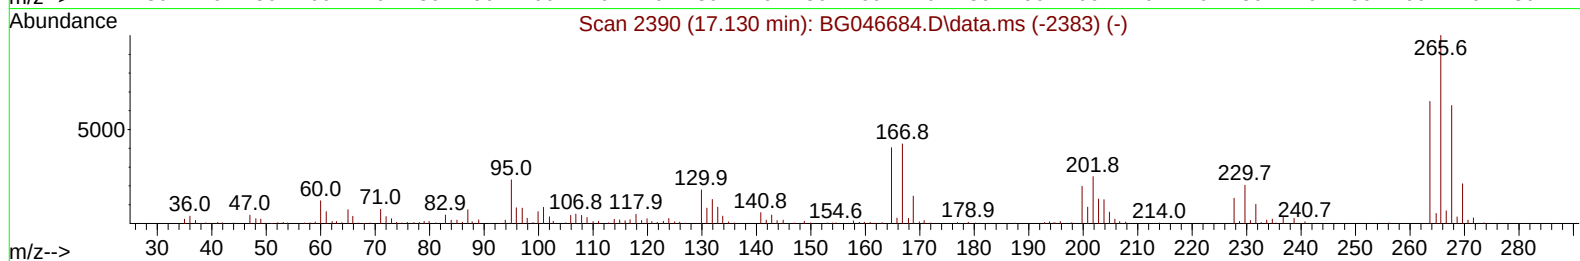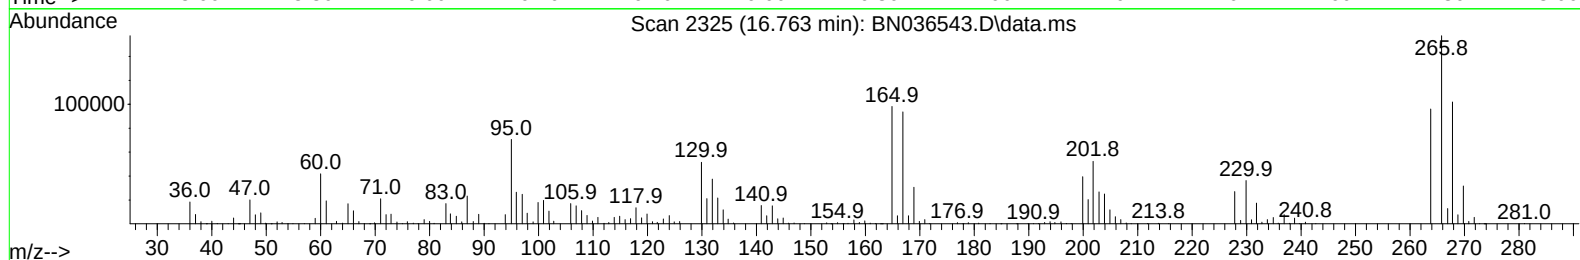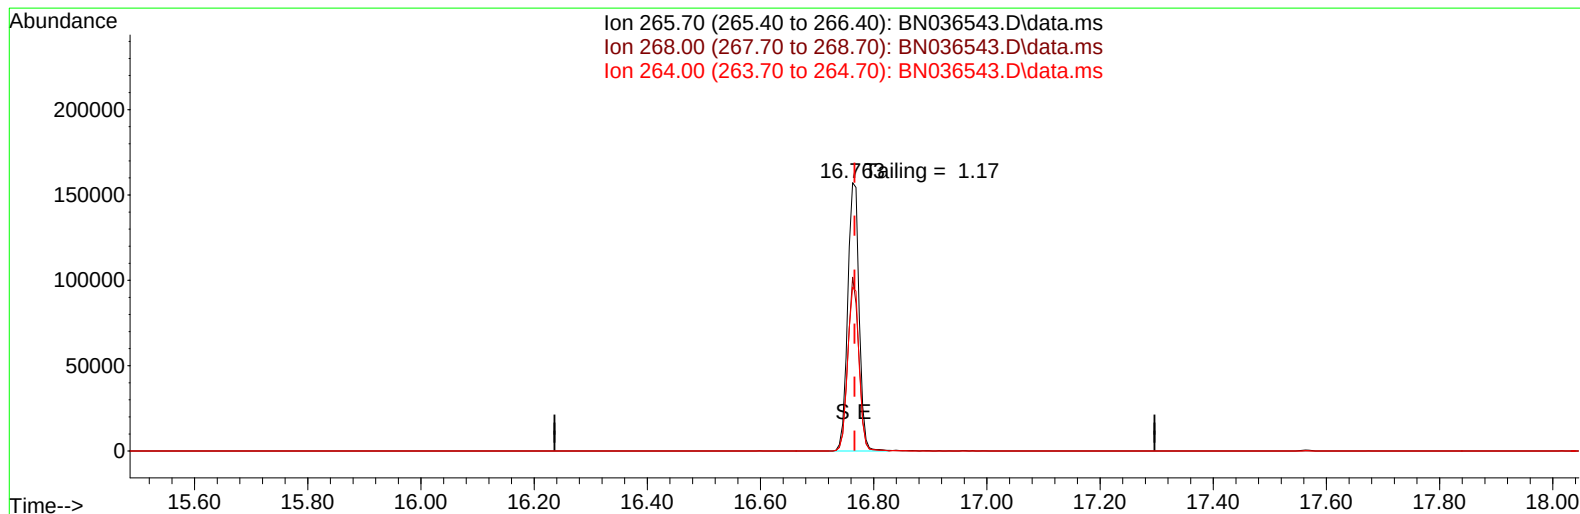

TIC: BN036543.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.003) 25175.33 ng




response 219895

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.78
264.00	61.60	61.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN030725\
Data File : BN036543.D
Acq On : 07 Mar 2025 12:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 07 17:45:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

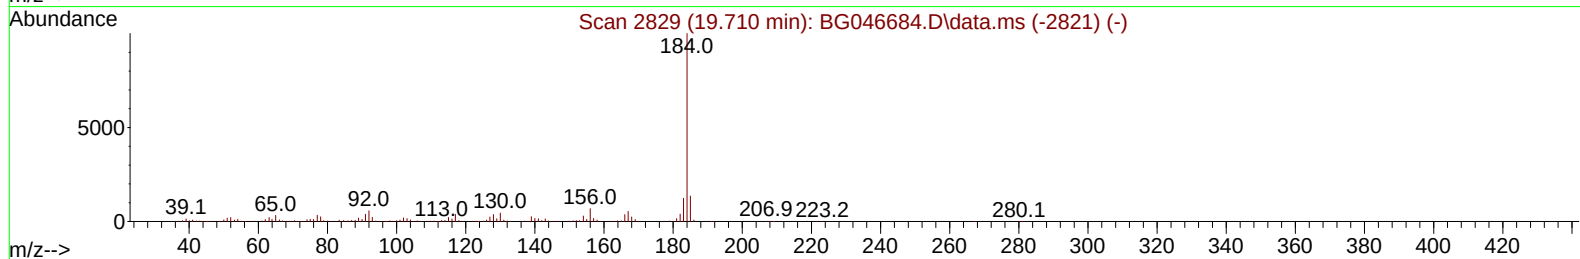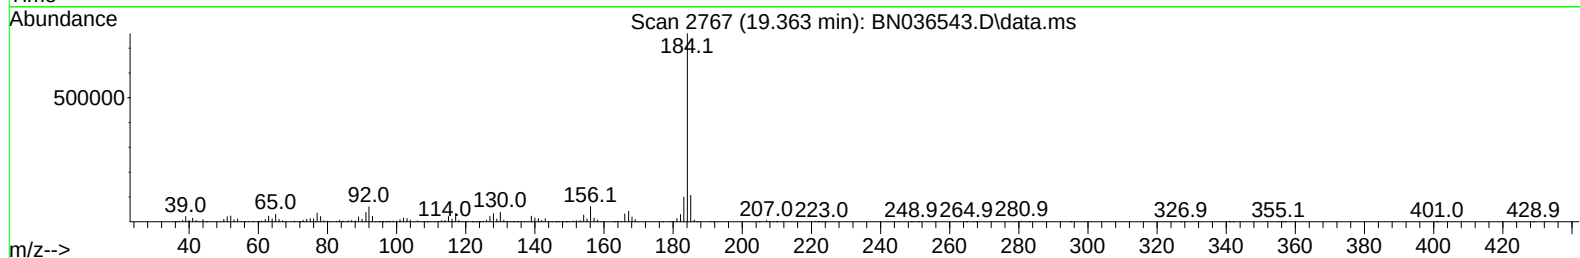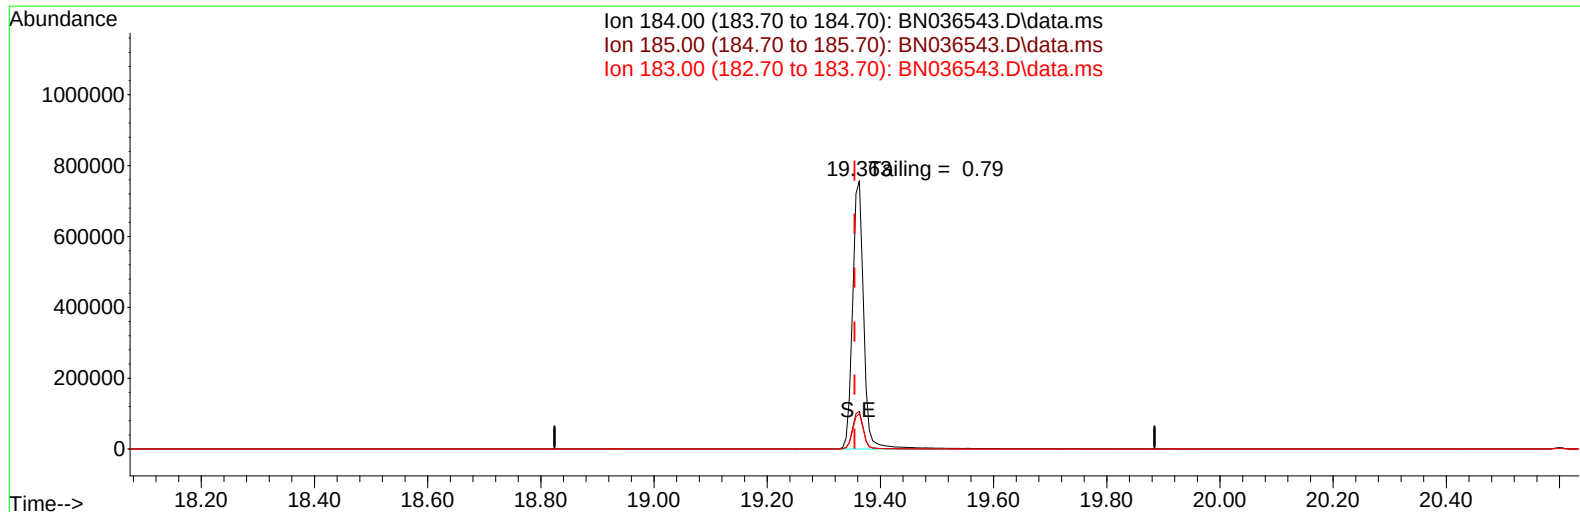

TIC: BN036543.D\data.ms

(77) Benzidine

19.363min (+ 0.009) 0.00 ng

response 1030323

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.03
183.00	13.20	13.20
0.00	0.00	0.00