
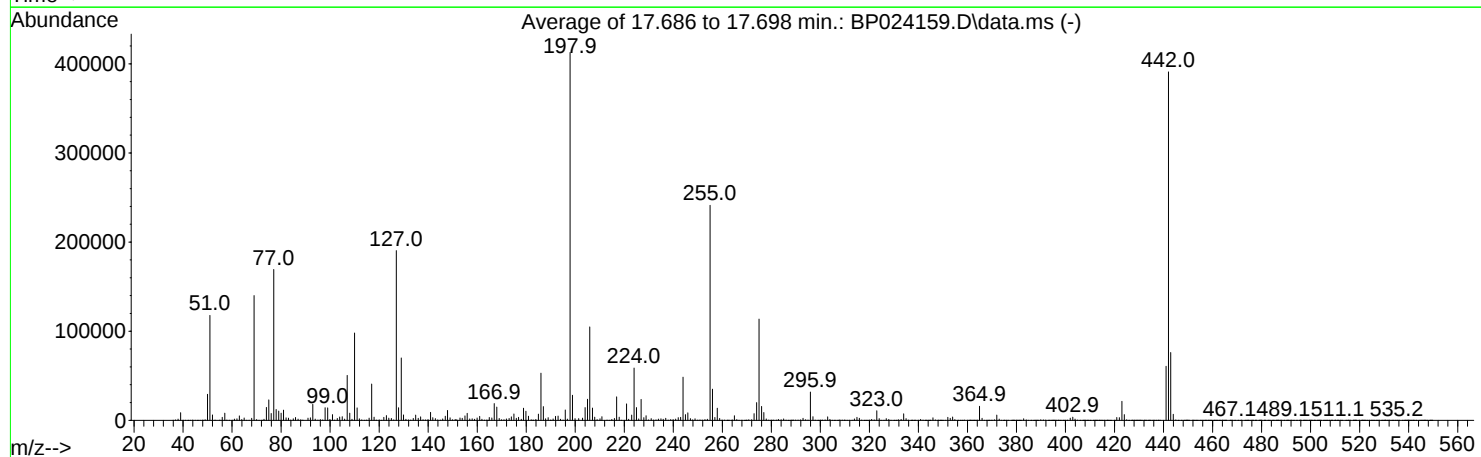


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031225\
Data File : BP024159.D
Acq On : 12 Mar 2025 15:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 13 05:55:58 2025

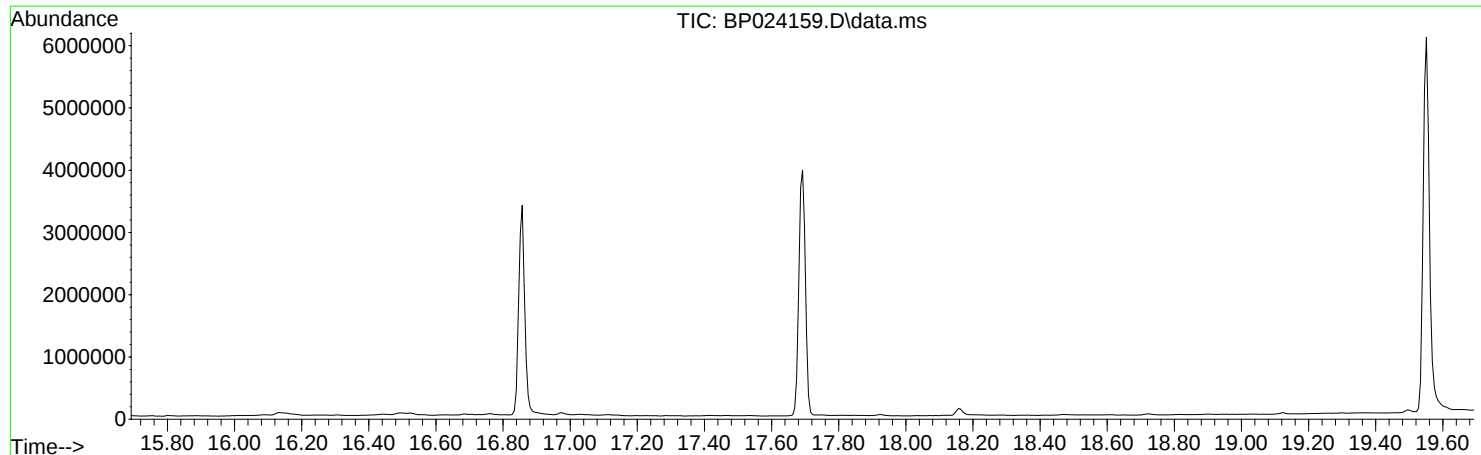

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	117822	PASS
68	69	0.00	2	1.6	2280	PASS
69	198	0.00	100	33.9	139938	PASS
70	69	0.00	2	0.6	822	PASS
127	198	10	80	46.1	190399	PASS
197	198	0.00	2	0.4	1468	PASS
198	198	100	100	100.0	412716	PASS
199	198	5	9	6.8	28114	PASS
275	198	10	60	27.5	113624	PASS
365	198	1	100	3.8	15804	PASS
441	198	0.01	100	14.7	60679	PASS
442	442	100	100	100.0	391061	PASS
443	442	15	24	19.5	76081	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/12/2025	BNA_P	<u>BP024159.D</u>
Compound Name	Response	Retention Time
DDT	1535436	20.851
DDD	16722	20.439
DDE	443	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17165	1552601	1.11

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031225\
Data File : BP024159.D
Acq On : 12 Mar 2025 15:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 13 05:56:16 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

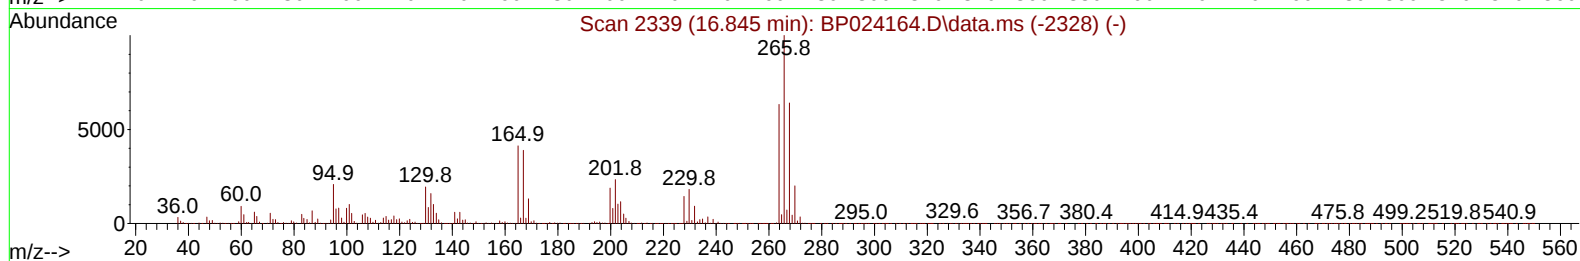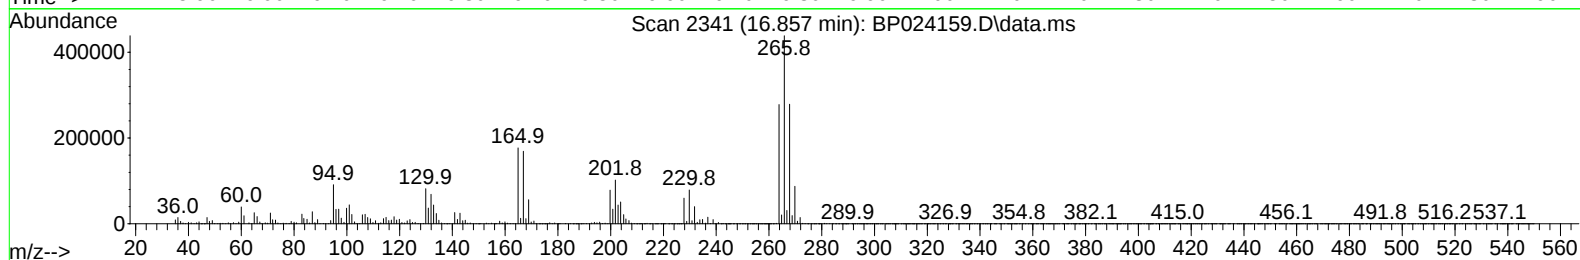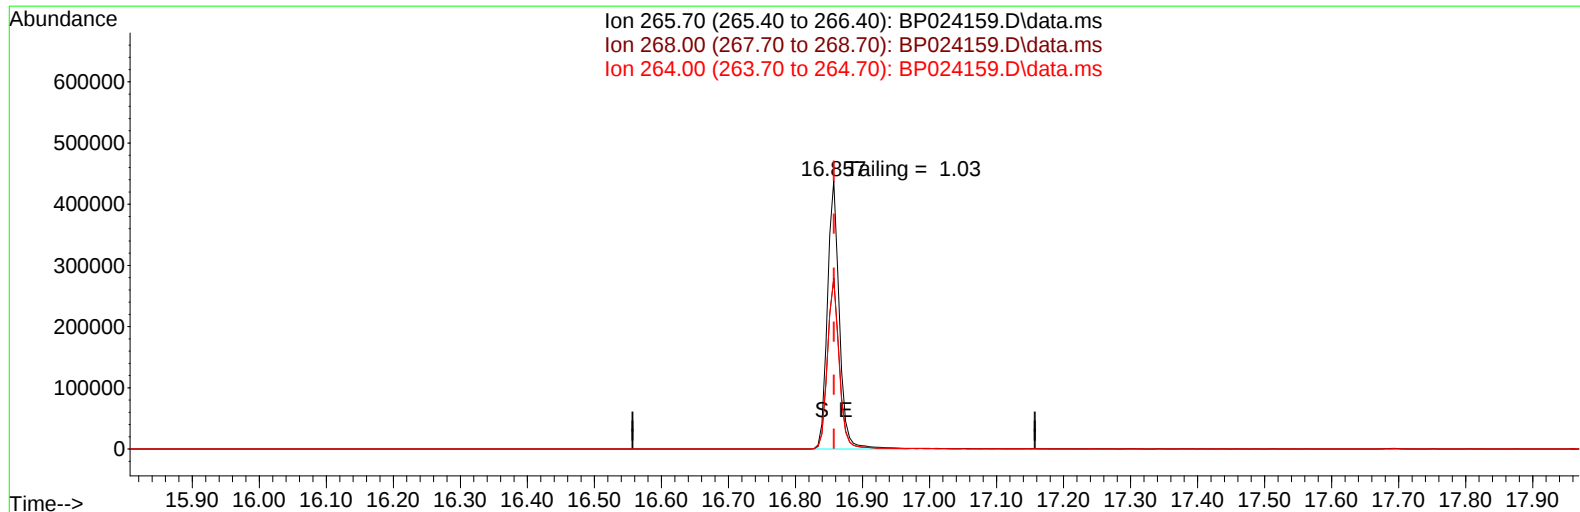

TIC: BP024159.D\data.ms

(70) Pentachlorophenol (C)

16.857min (0.000) 4607317.61 ng




response 542052

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.56
264.00	63.30	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031225\
 Data File : BP024159.D
 Acq On : 12 Mar 2025 15:36
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 13 05:56:16 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 13 05:55:58 2025
 Response via : Initial Calibration

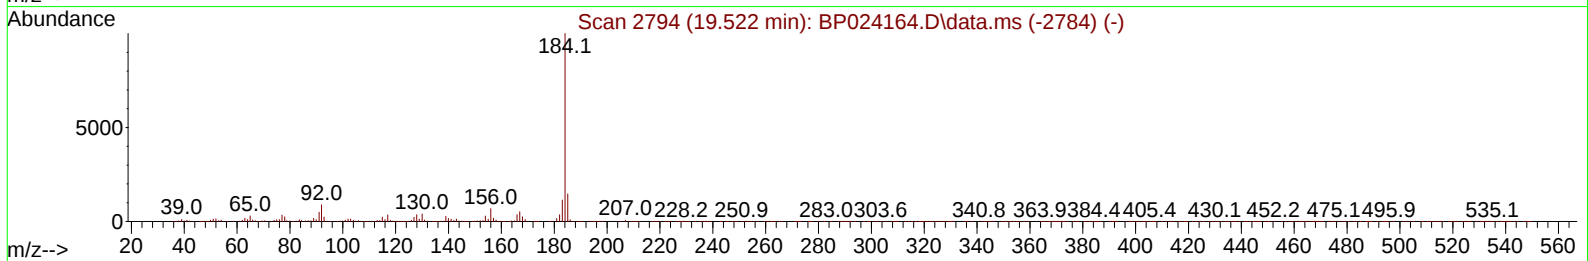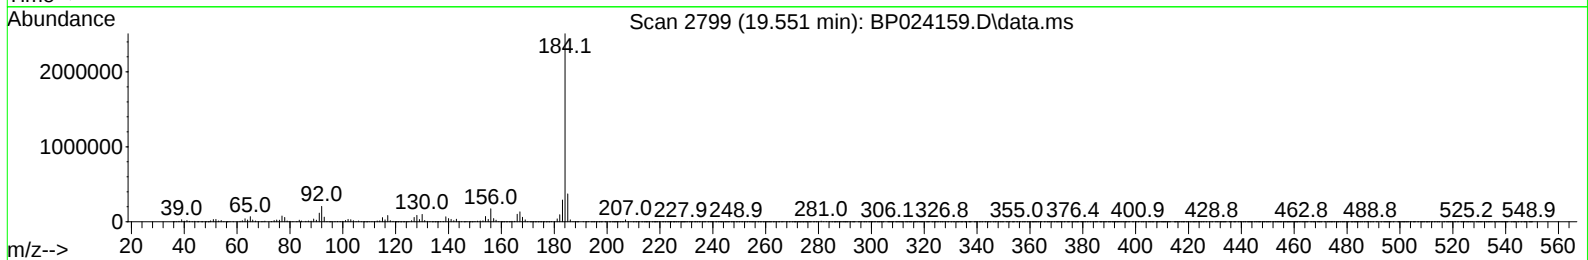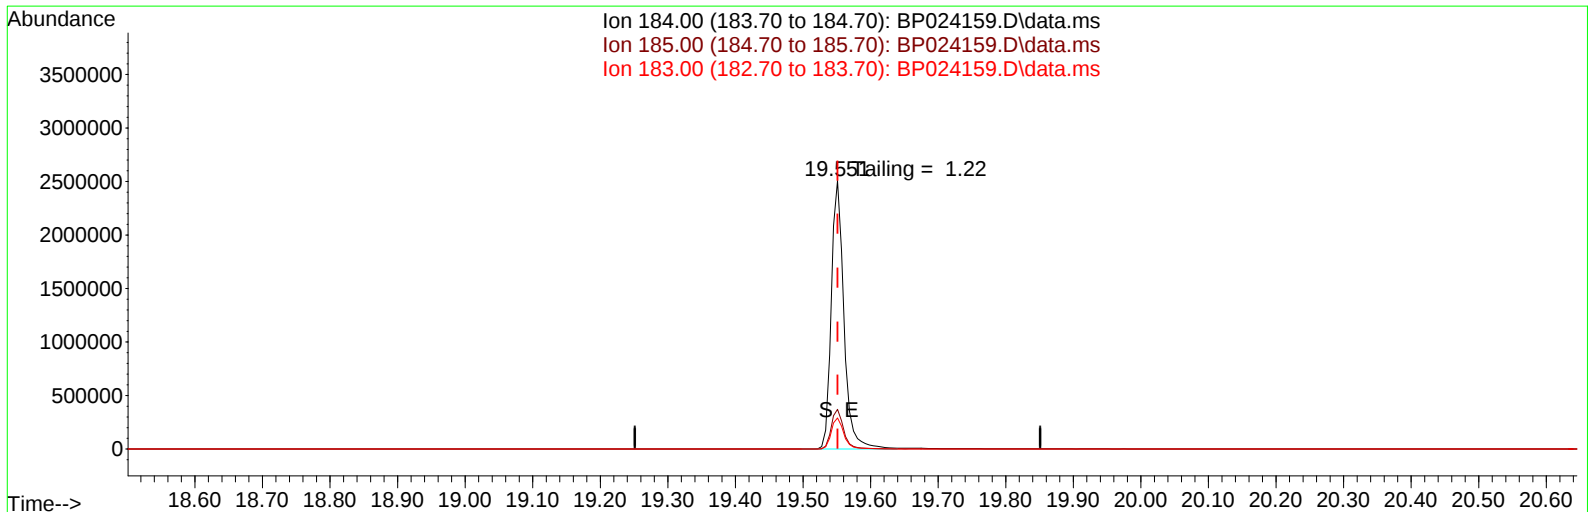

TIC: BP024159.D\data.ms

(77) Benzidine

19.551min (0.000) 3117449.49 ng

response 3272103

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.81
183.00	11.40	11.59
0.00	0.00	0.00