


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031025\
Data File : BN036556.D
Acq On : 10 Mar 2025 11:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

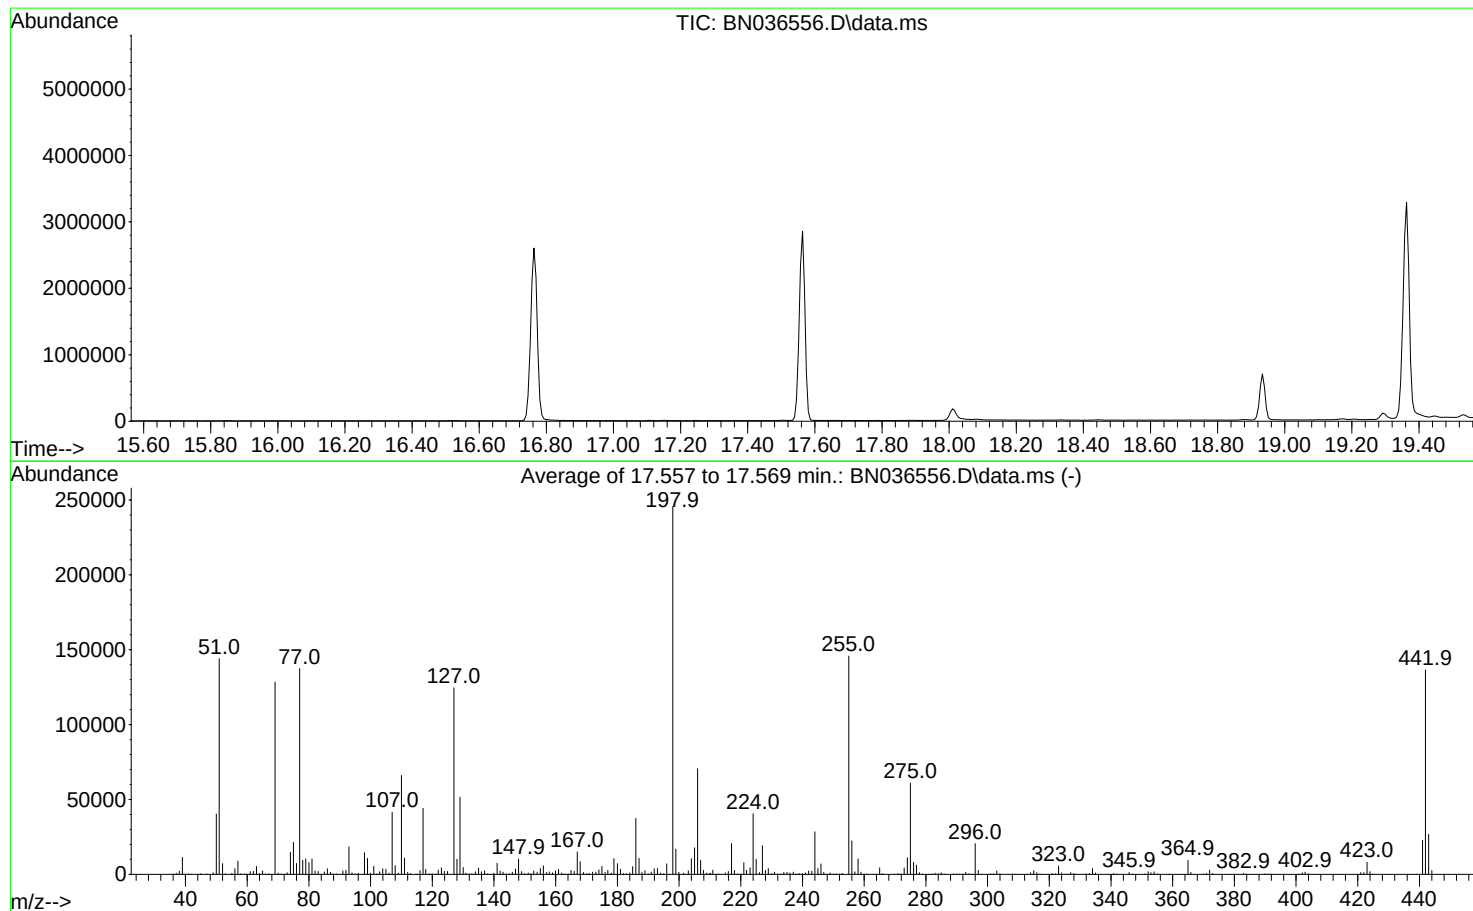

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.6	144050	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.3	128410	PASS
70	69	0.00	2	0.7	835	PASS
127	198	10	80	50.7	124576	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	245632	PASS
199	198	5	9	6.9	16887	PASS
275	198	10	60	24.8	60997	PASS
365	198	1	100	3.8	9349	PASS
441	198	0.01	100	9.3	22761	PASS
442	442	50	100	100.0	136488	PASS
443	442	15	24	19.6	26765	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/10/2025	BNA_N	<u>BN036556.D</u>
Compound Name	Response	Retention Time
DDT	1110406	20.598
DDD	11596	20.21
DDE	530	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12126	1122532	1.08

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031025\
Data File : BN036556.D
Acq On : 10 Mar 2025 11:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 10 17:07:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

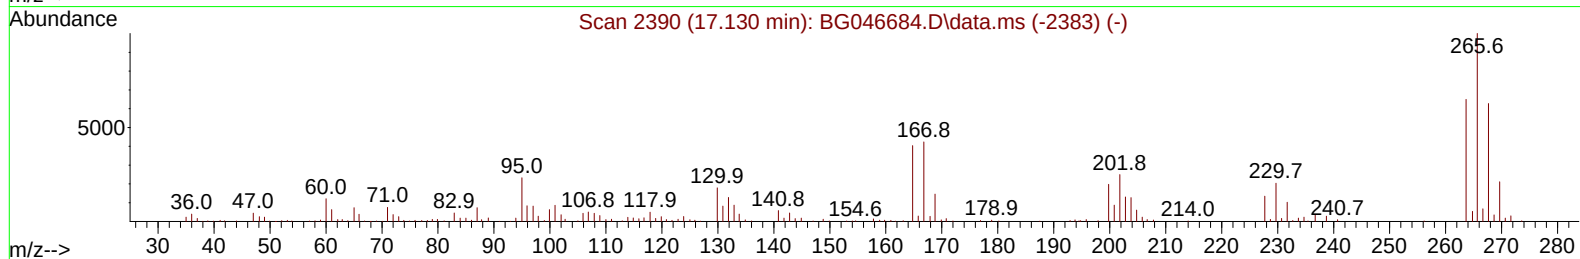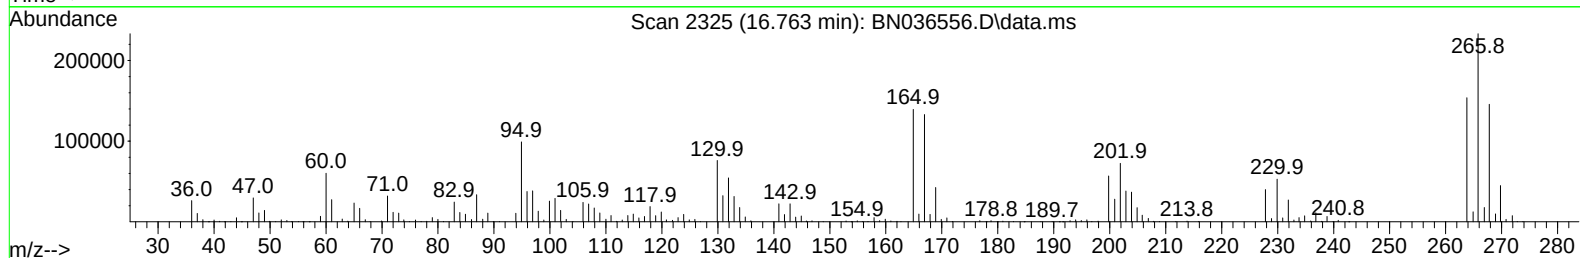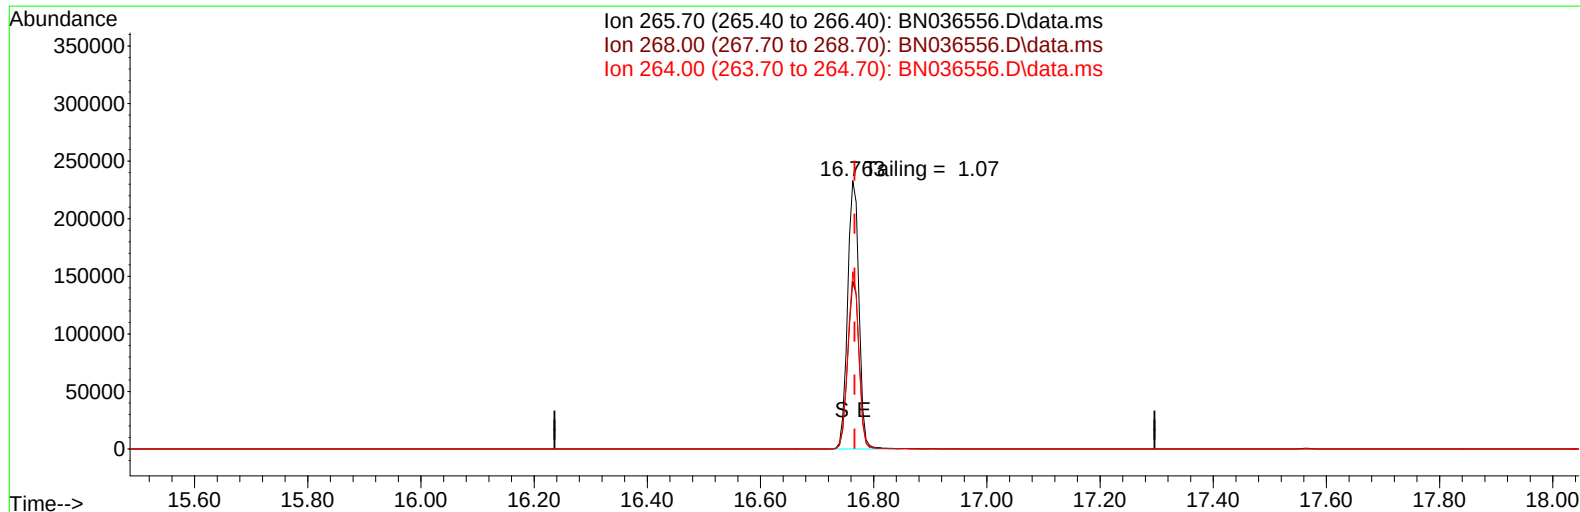

TIC: BN036556.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.003) 23577.14 ng




response 323613

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.52
264.00	61.60	66.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031025\
Data File : BN036556.D
Acq On : 10 Mar 2025 11:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 10 17:07:28 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

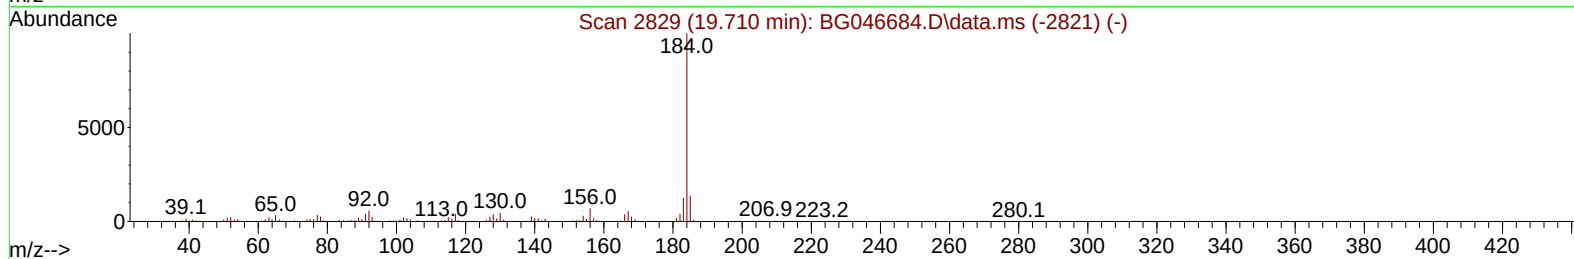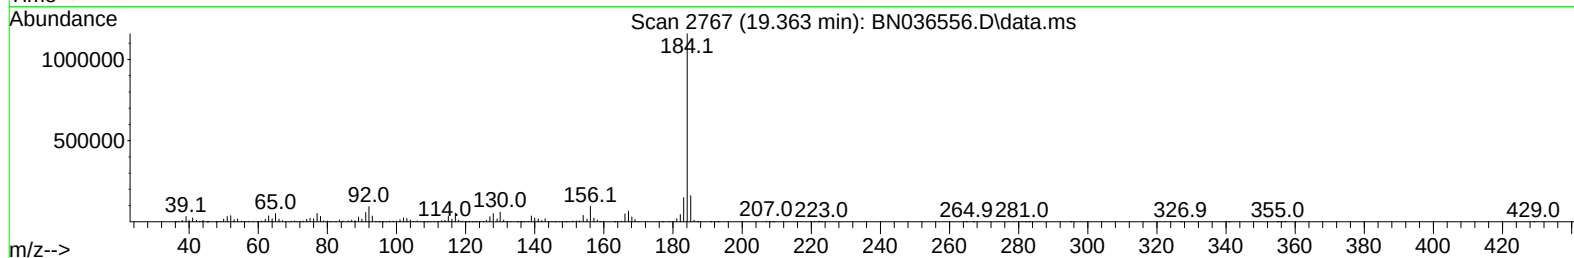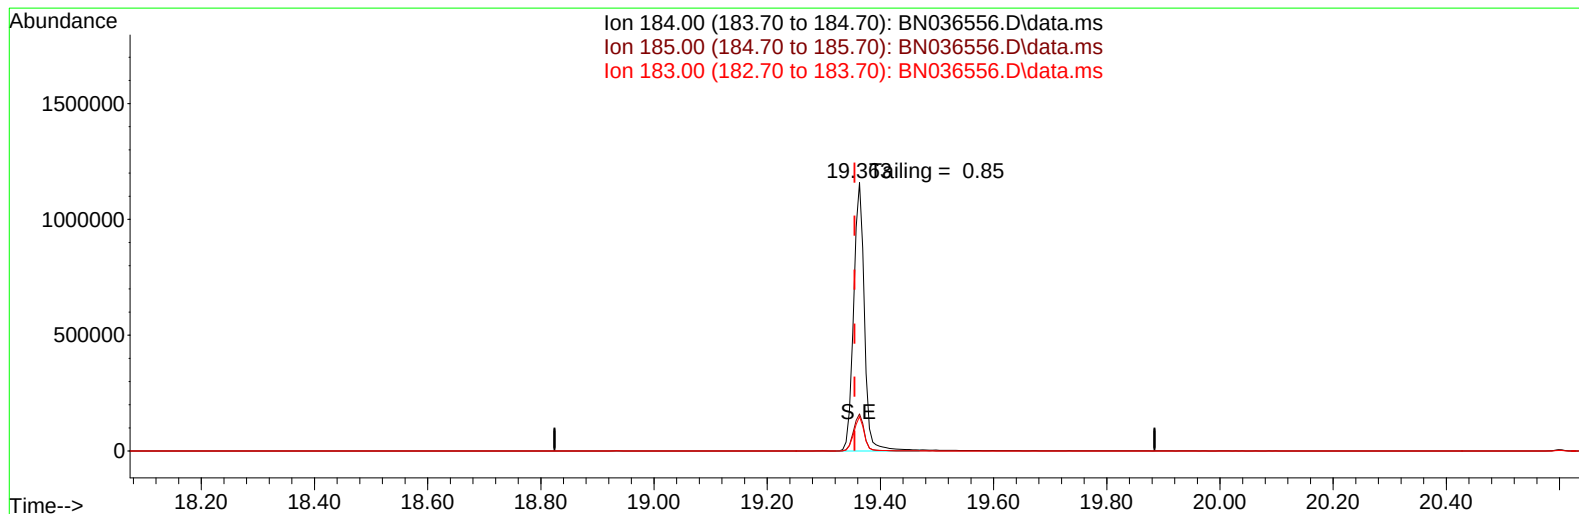

TIC: BN036556.D\data.ms

(77) Benzidine

19.363min (+ 0.009) 0.00 ng

response 1553313

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.86
183.00	13.20	12.85
0.00	0.00	0.00