


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036600.D
Acq On : 14 Mar 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

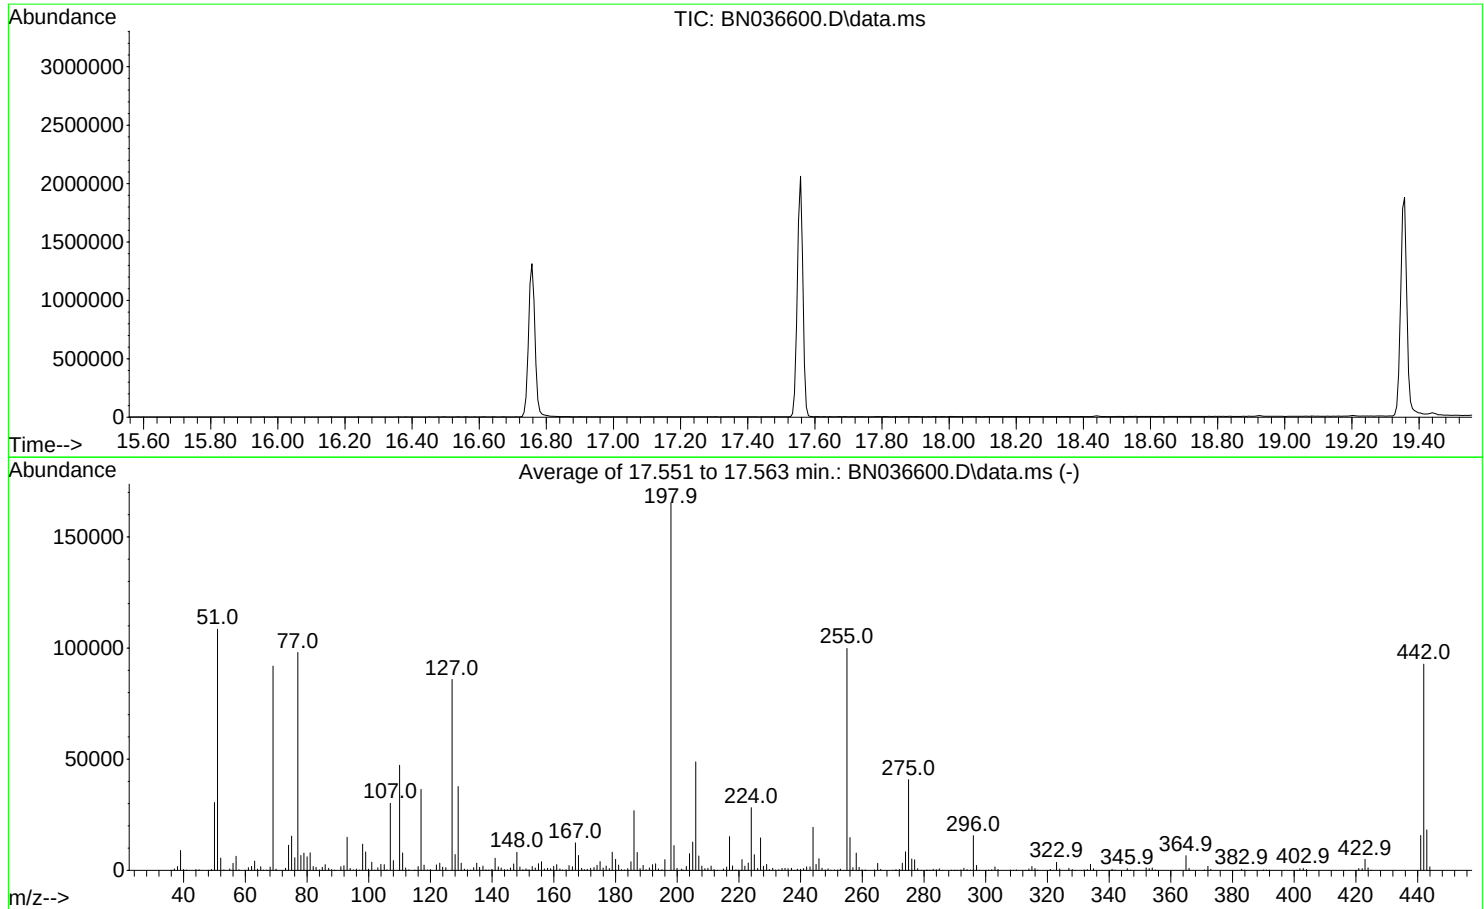

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.5	108445	PASS
68	69	0.00	2	1.6	1504	PASS
69	198	0.00	100	55.5	91899	PASS
70	69	0.00	2	0.6	558	PASS
127	198	10	80	51.9	85880	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	165483	PASS
199	198	5	9	6.7	11147	PASS
275	198	10	60	24.7	40816	PASS
365	198	1	100	4.0	6612	PASS
441	198	0.01	100	9.5	15668	PASS
442	442	50	100	100.0	92771	PASS
443	442	15	24	19.7	18237	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/14/2025	BNA_N	<u>BN036600.D</u>
Compound Name	Response	Retention Time
DDT	534890	20.592
DDD	6130	20.204
DDE	455	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6585	541475	1.22

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036600.D
Acq On : 14 Mar 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 15 00:26:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 15 00:26:30 2025
Response via : Initial Calibration

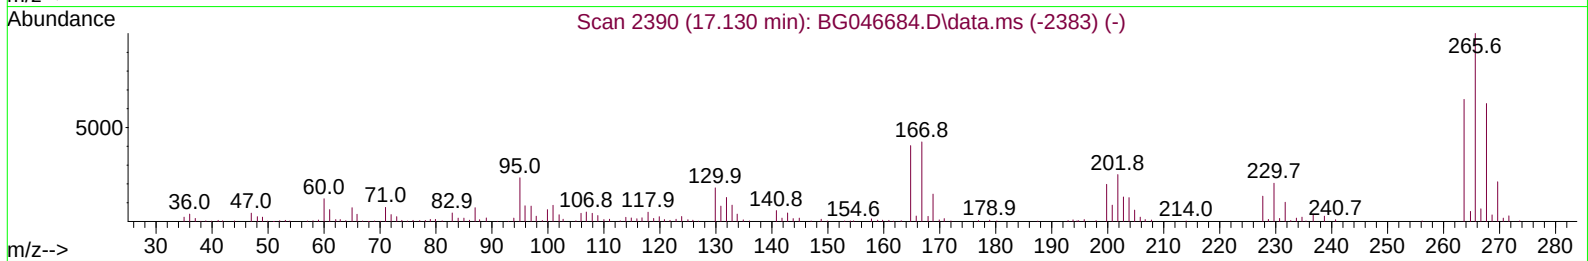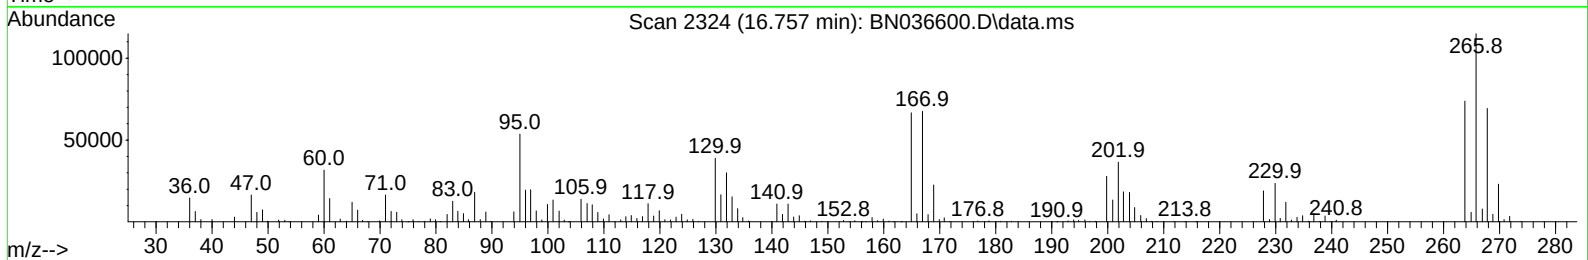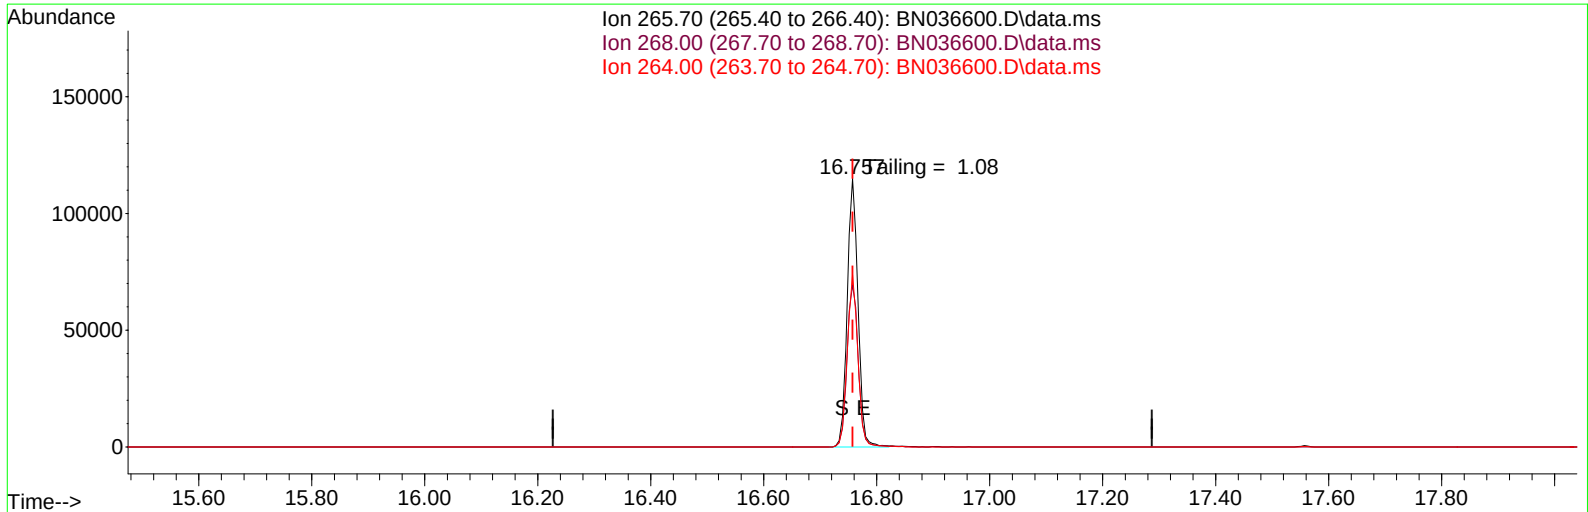

TIC: BN036600.D\data.ms

(70) Pentachlorophenol (C)

16.757min (0.000) 18451.01 ng




response 152618

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.30
264.00	61.60	64.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036600.D
Acq On : 14 Mar 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 15 00:26:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 15 00:26:30 2025
Response via : Initial Calibration

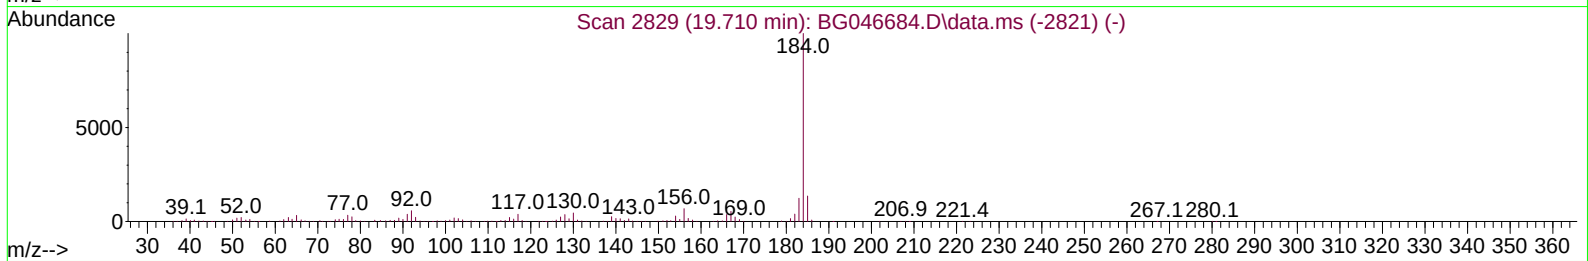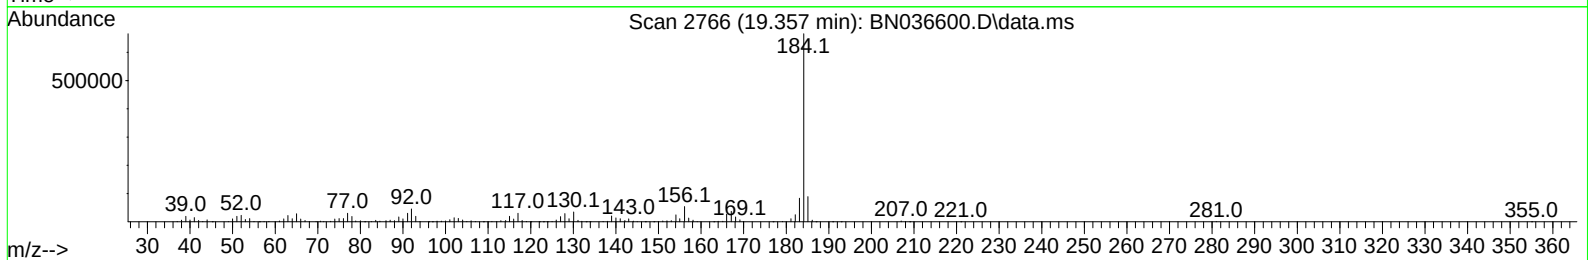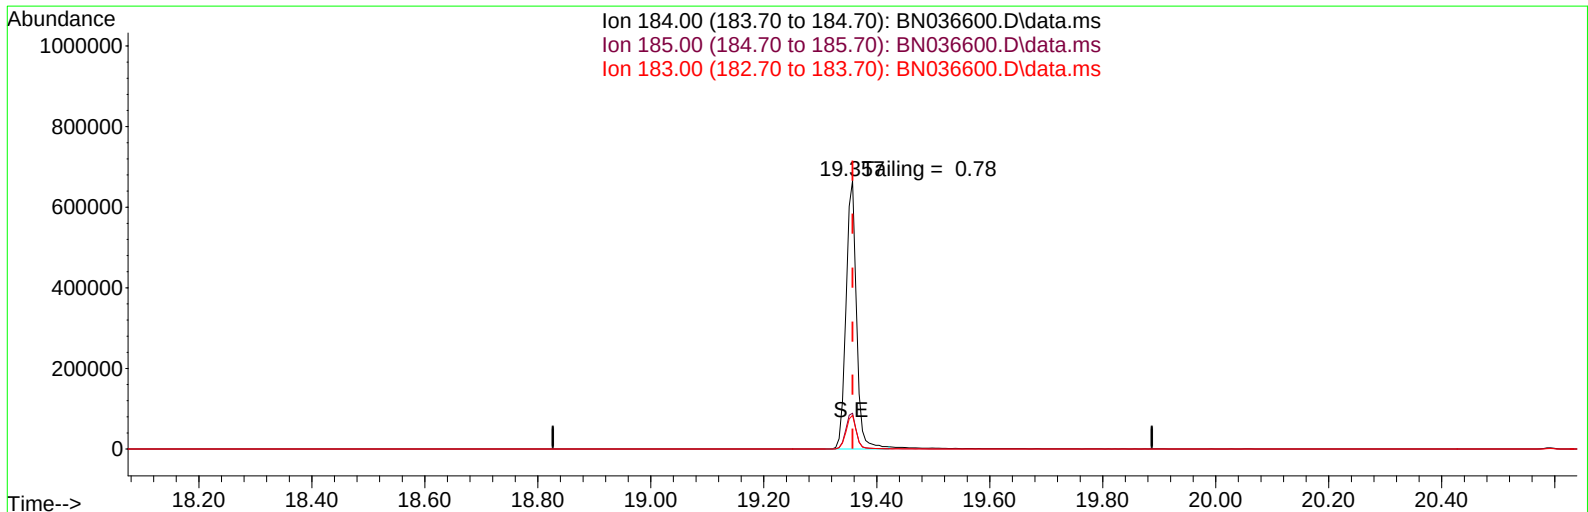

TIC: BN036600.D\data.ms

(77) Benzidine

19.357min (0.000) 0.00 ng

response 868744

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.38
183.00	13.20	12.57
0.00	0.00	0.00