
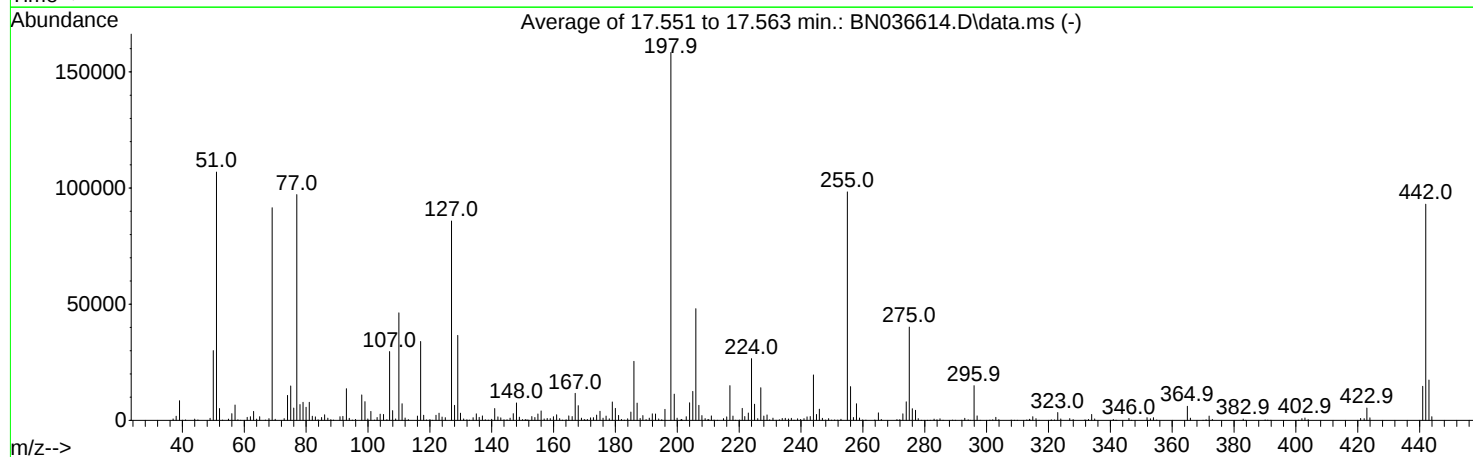


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036614.D
Acq On : 14 Mar 2025 19:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

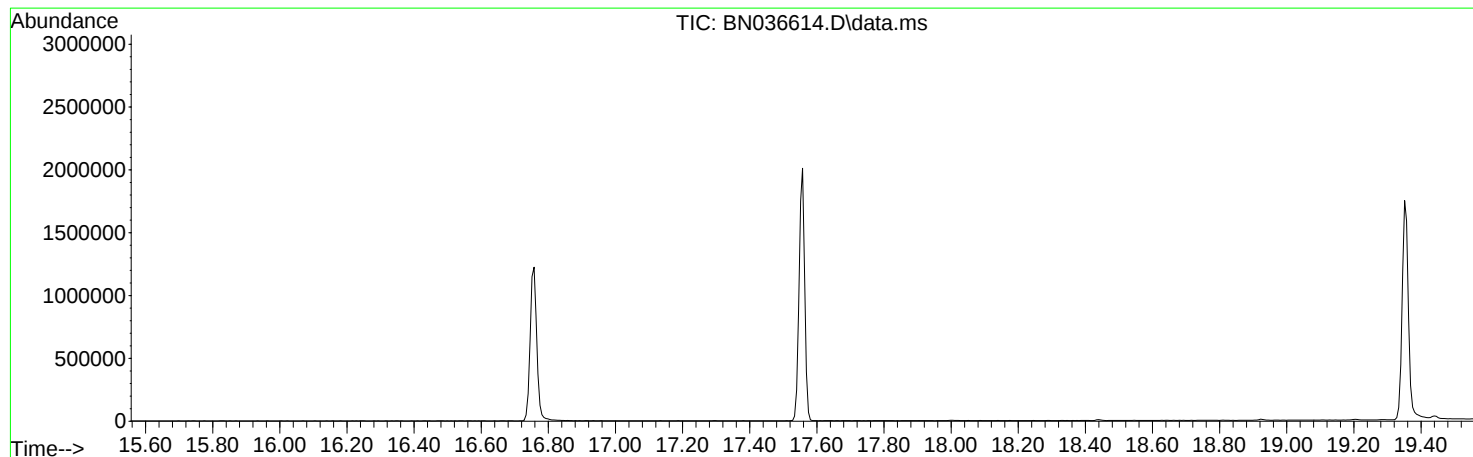

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	67.5	106904	PASS
68	69	0.00	2	0.9	793	PASS
69	198	0.00	100	57.8	91549	PASS
70	69	0.00	2	0.6	519	PASS
127	198	10	80	54.2	85851	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	158365	PASS
199	198	5	9	7.1	11286	PASS
275	198	10	60	25.4	40192	PASS
365	198	1	100	3.8	6077	PASS
441	198	0.01	100	9.3	14651	PASS
442	442	50	100	100.0	93083	PASS
443	442	15	24	18.6	17354	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/14/2025	BNA_N	<u>BN036614.D</u>
Compound Name	Response	Retention Time
DDT	524370	20.592
DDD	5883	20.204
DDE	253	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6136	530506	1.16

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036614.D
Acq On : 14 Mar 2025 19:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 15 00:28:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 15 00:26:30 2025
Response via : Initial Calibration

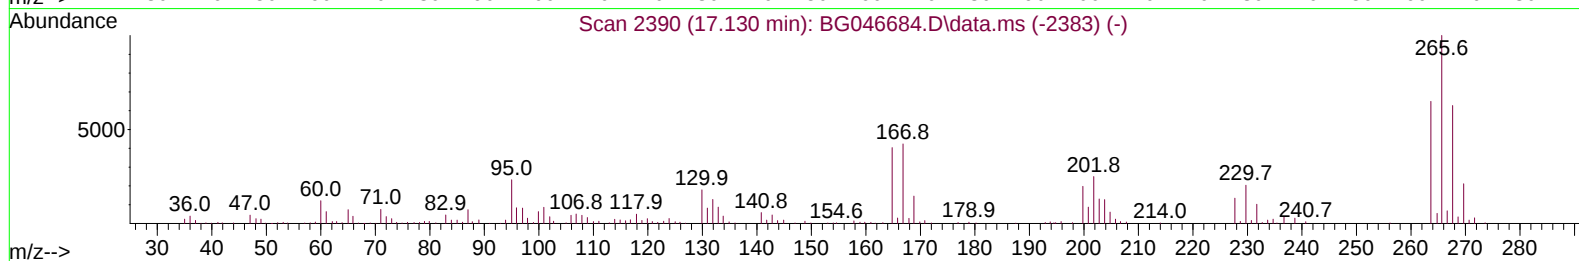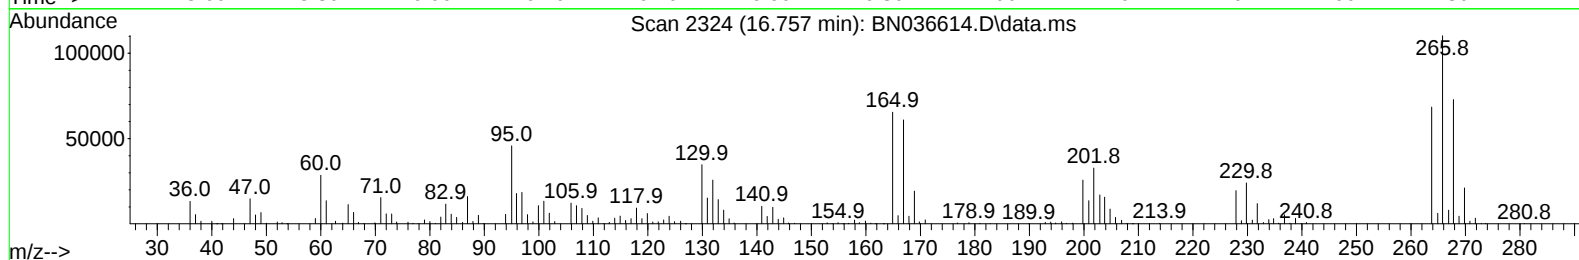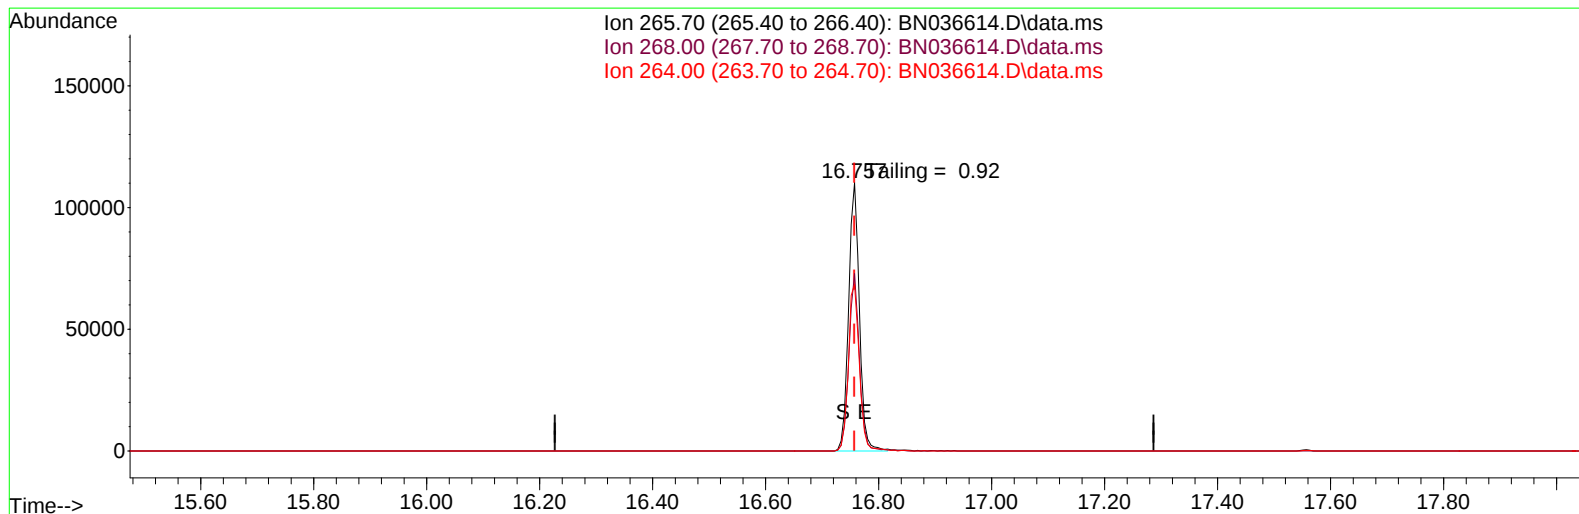

TIC: BN036614.D\data.ms

(70) Pentachlorophenol (C)

16.757min (+ 0.000) 16591.40 ng




response 147262

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.06
264.00	61.60	62.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036614.D
Acq On : 14 Mar 2025 19:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 15 00:28:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 15 00:26:30 2025
Response via : Initial Calibration

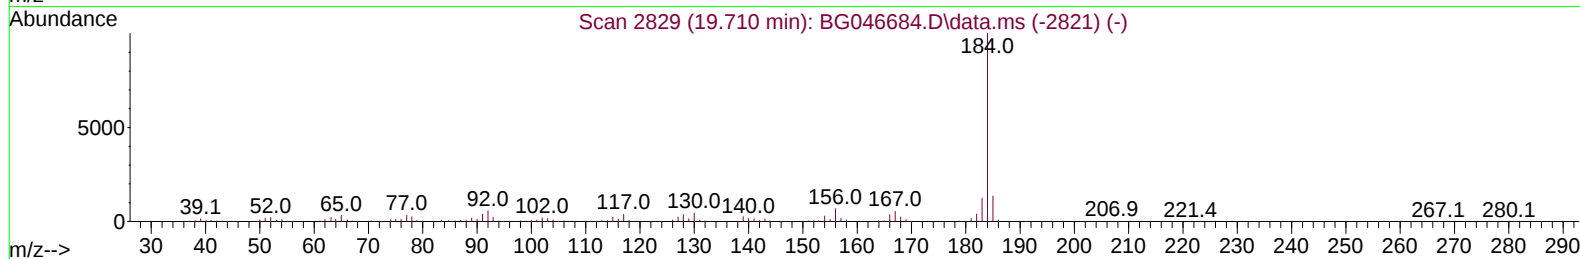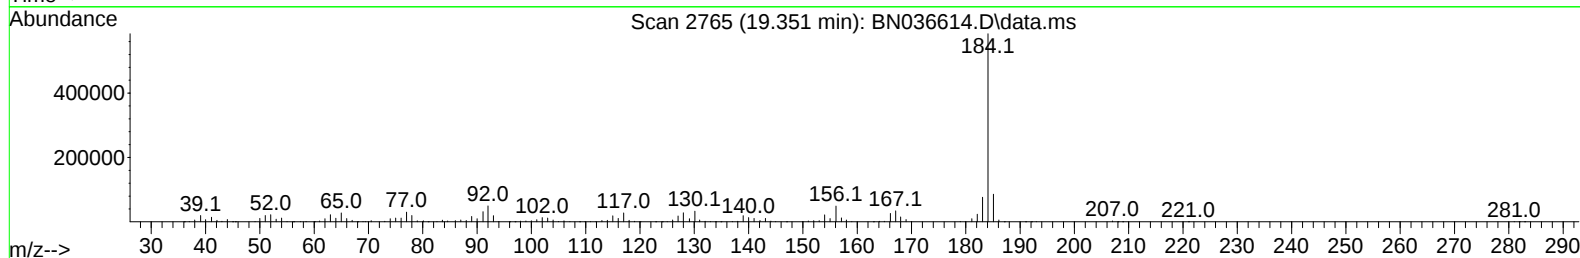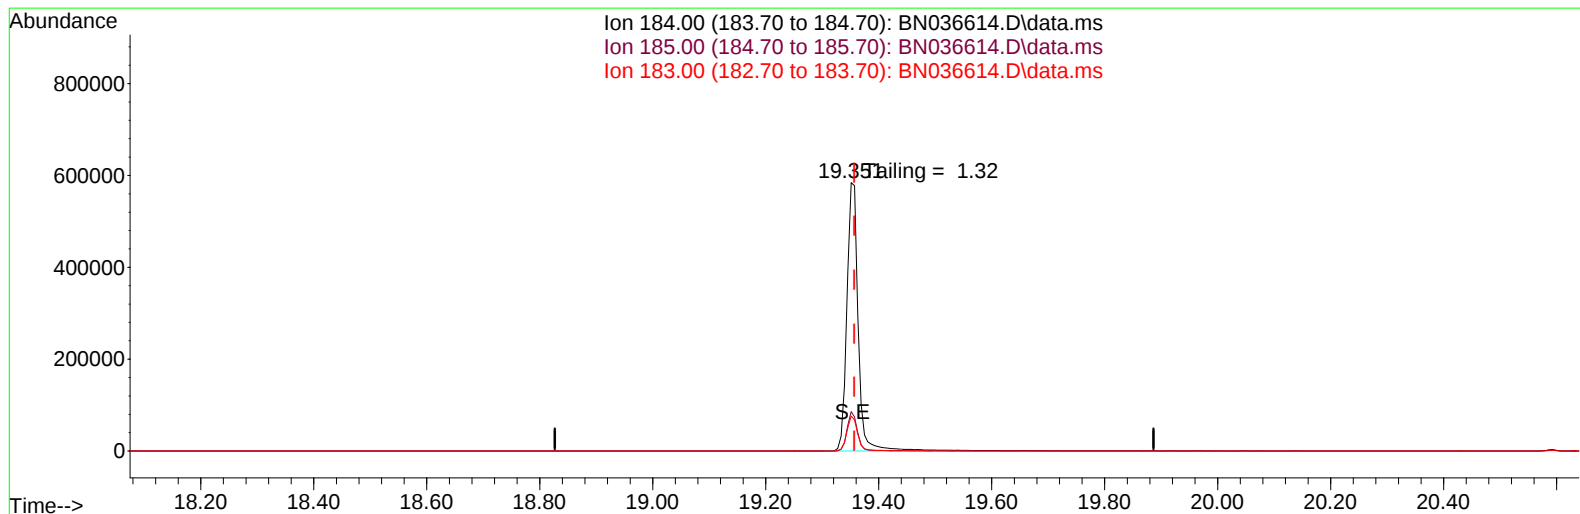

TIC: BN036614.D\data.ms

(77) Benzidine

19.351min (-0.006) 0.00 ng

response 817261

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.66
183.00	13.20	13.06
0.00	0.00	0.00