
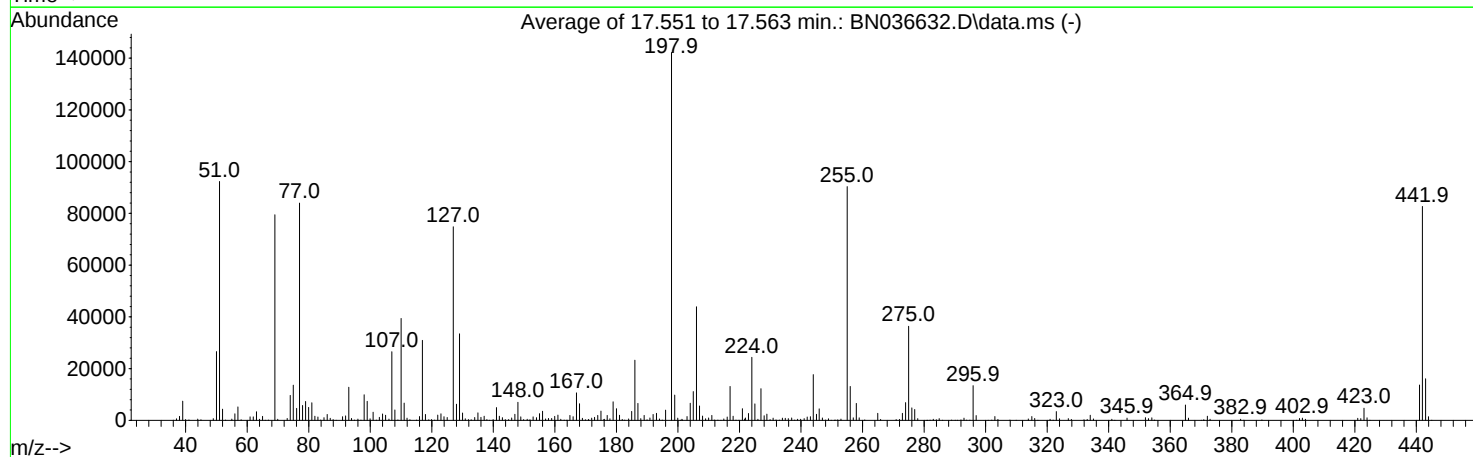


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036632.D
Acq On : 15 Mar 2025 06:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

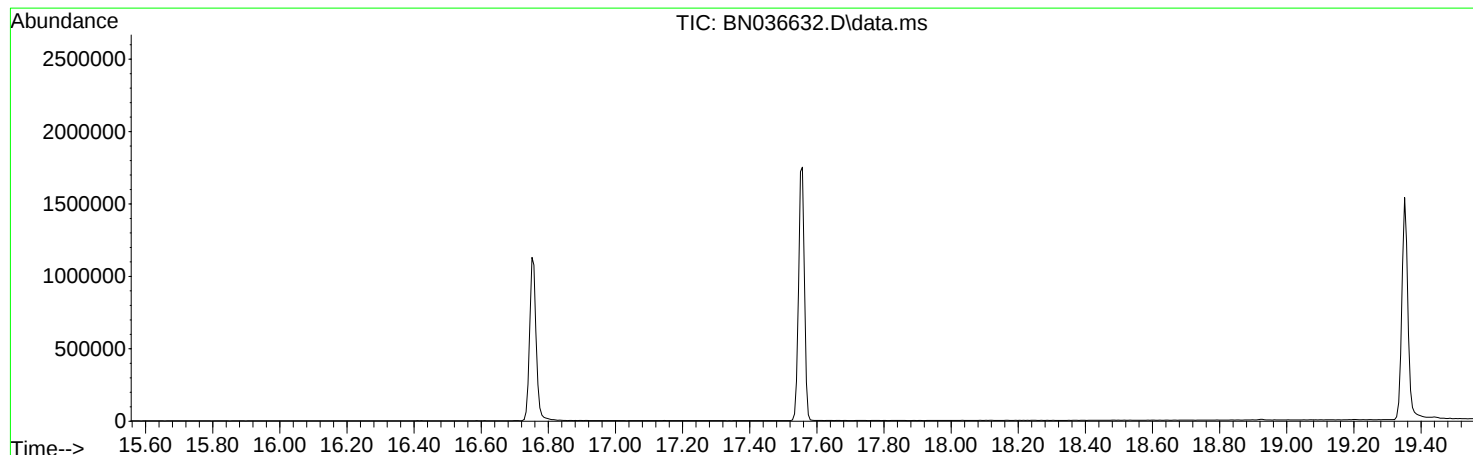

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.9	92315	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	55.9	79448	PASS
70	69	0.00	2	0.5	429	PASS
127	198	10	80	52.7	74864	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	142187	PASS
199	198	5	9	6.9	9755	PASS
275	198	10	60	25.6	36355	PASS
365	198	1	100	4.2	5967	PASS
441	198	0.01	100	9.6	13649	PASS
442	442	50	100	100.0	82675	PASS
443	442	15	24	19.5	16097	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/14/2025	BNA_N	<u>BN036632.D</u>
Compound Name	Response	Retention Time
DDT	477266	20.592
DDD	6330	20.198
DDE	302	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6632	483898	1.37

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031425\
Data File : BN036632.D
Acq On : 15 Mar 2025 06:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 17 01:20:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 17 01:20:13 2025
Response via : Initial Calibration

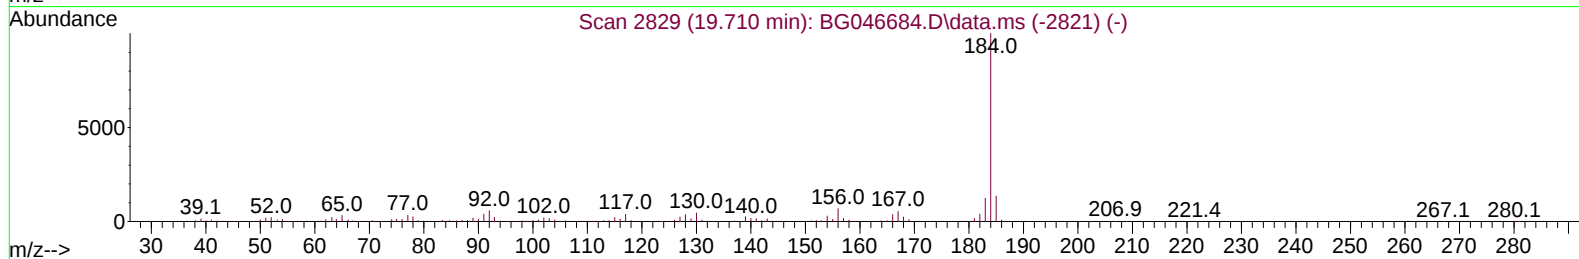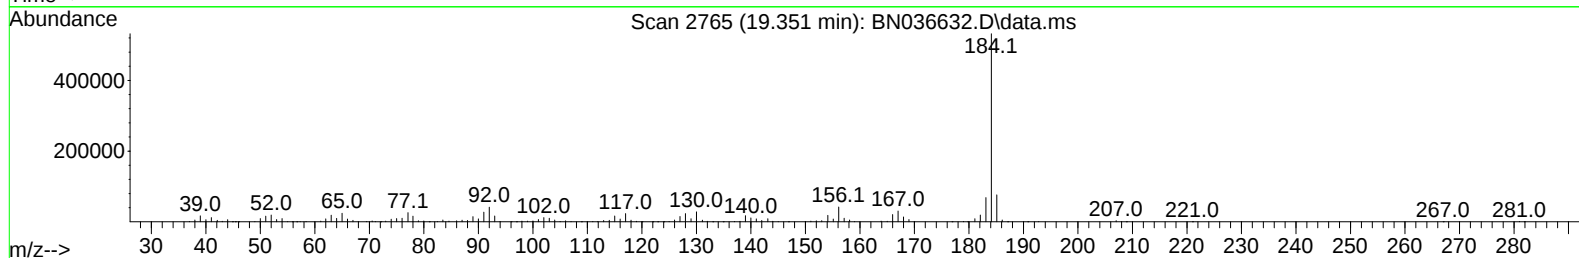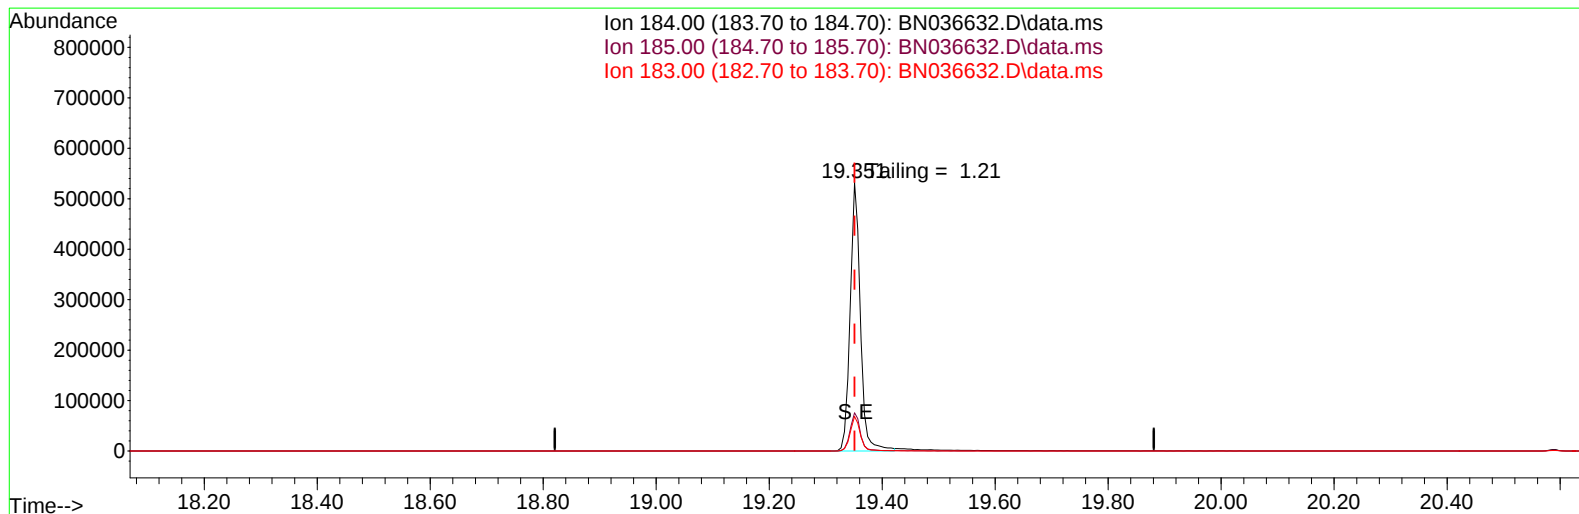

TIC: BN036632.D\data.ms

(77) Benzidine

19.351min (0.000) 0.00 ng

response 681752

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	12.92
0.00	0.00	0.00