
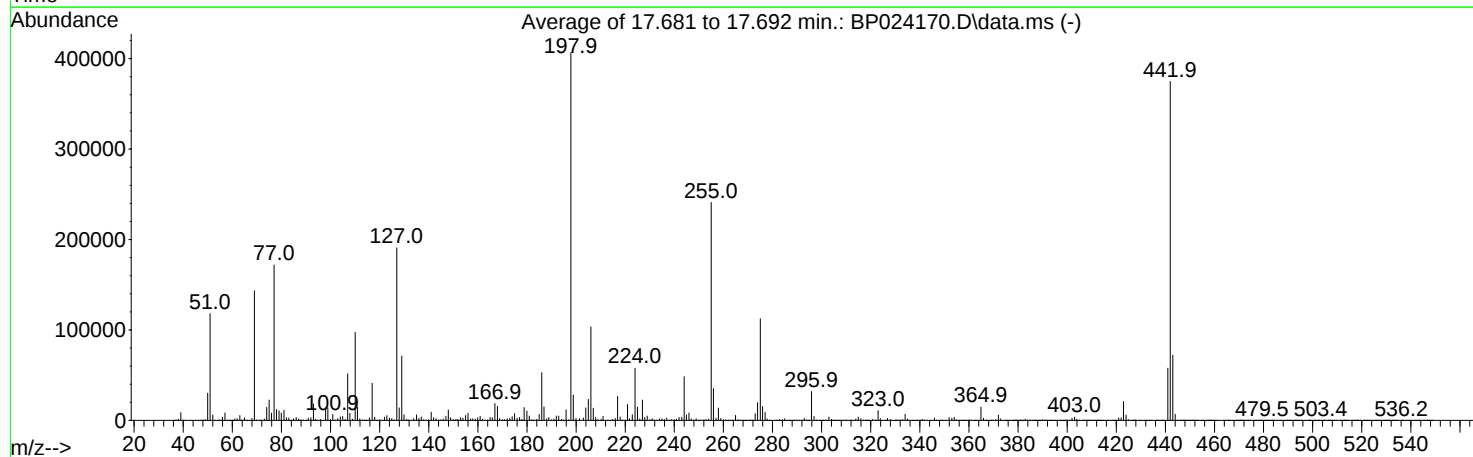


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031325\
Data File : BP024170.D
Acq On : 13 Mar 2025 09:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 13 05:55:58 2025

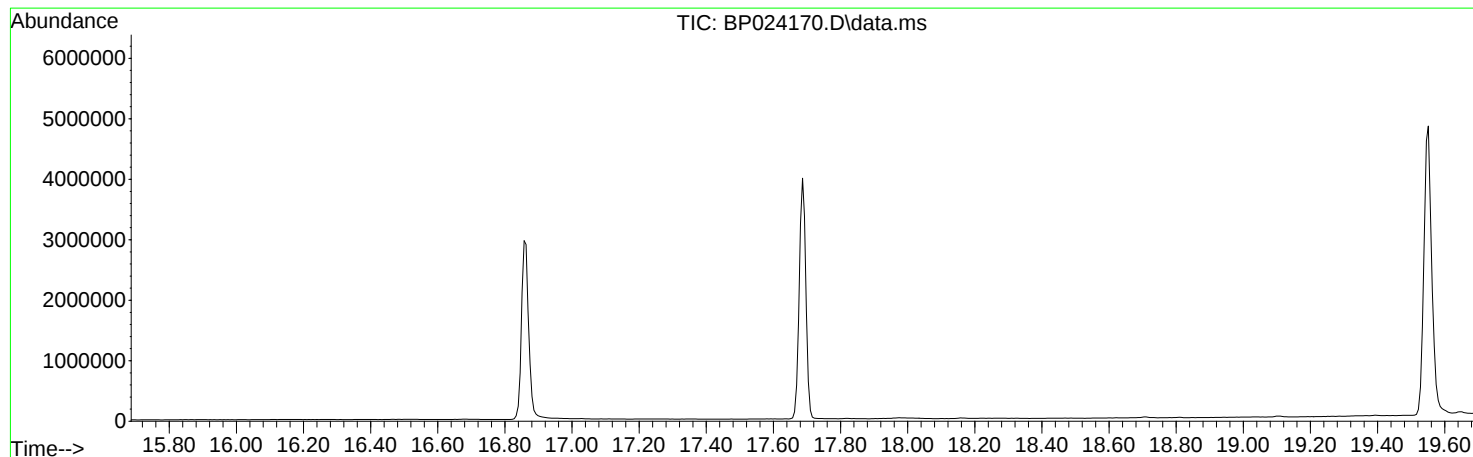



AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	118052	PASS
68	69	0.00	2	1.5	2218	PASS
69	198	0.00	100	35.2	143312	PASS
70	69	0.00	2	0.6	790	PASS
127	198	10	80	46.9	190703	PASS
197	198	0.00	2	0.1	548	PASS
198	198	100	100	100.0	406784	PASS
199	198	5	9	6.9	28034	PASS
275	198	10	60	27.6	112405	PASS
365	198	1	100	3.6	14767	PASS
441	198	0.01	100	14.2	57619	PASS
442	442	100	100	100.0	374803	PASS
443	442	15	24	19.2	71957	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031325\
Data File : BP024170.D
Acq On : 13 Mar 2025 09:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 13 11:49:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

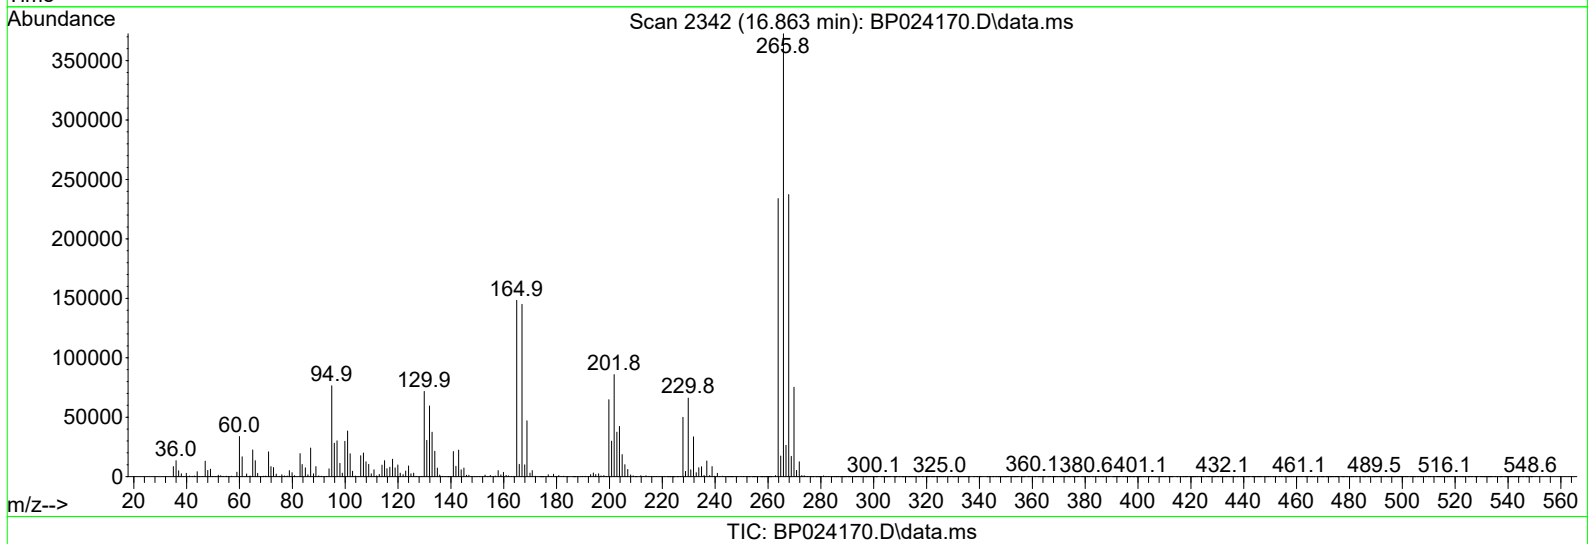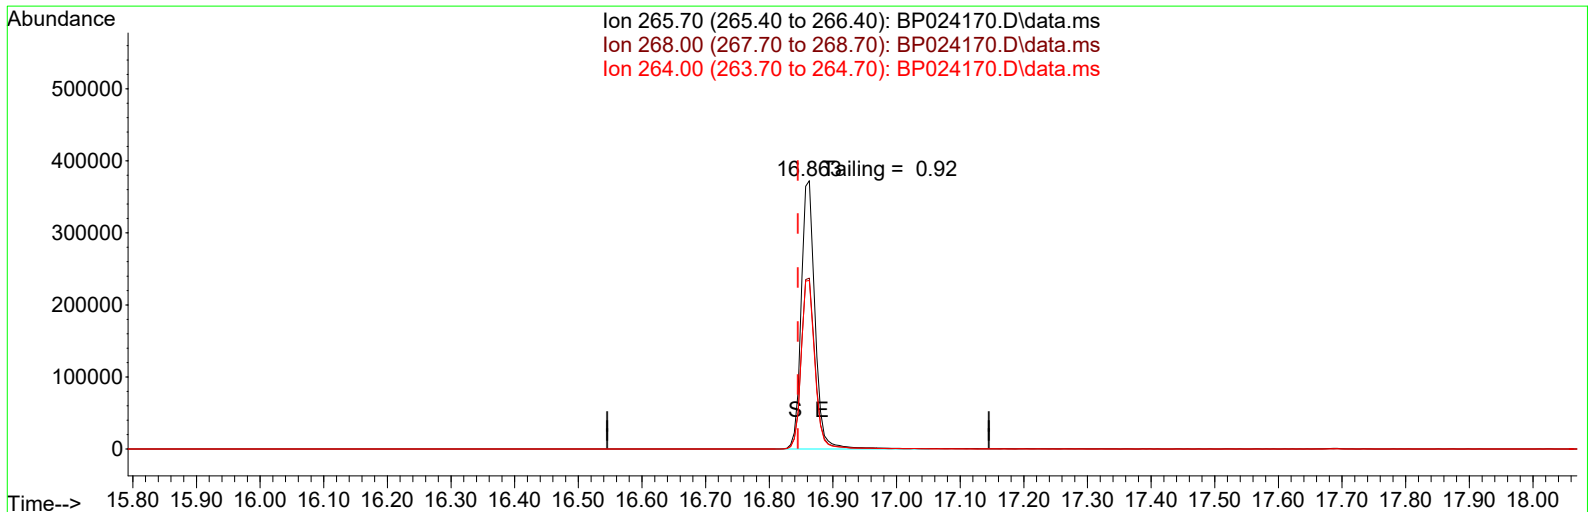

(70) Pentachlorophenol (C)

16.863min (+ 0.018) 604215.30 ng



response 563611

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.70
264.00	63.30	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031325\
Data File : BP024170.D
Acq On : 13 Mar 2025 09:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 13 11:49:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

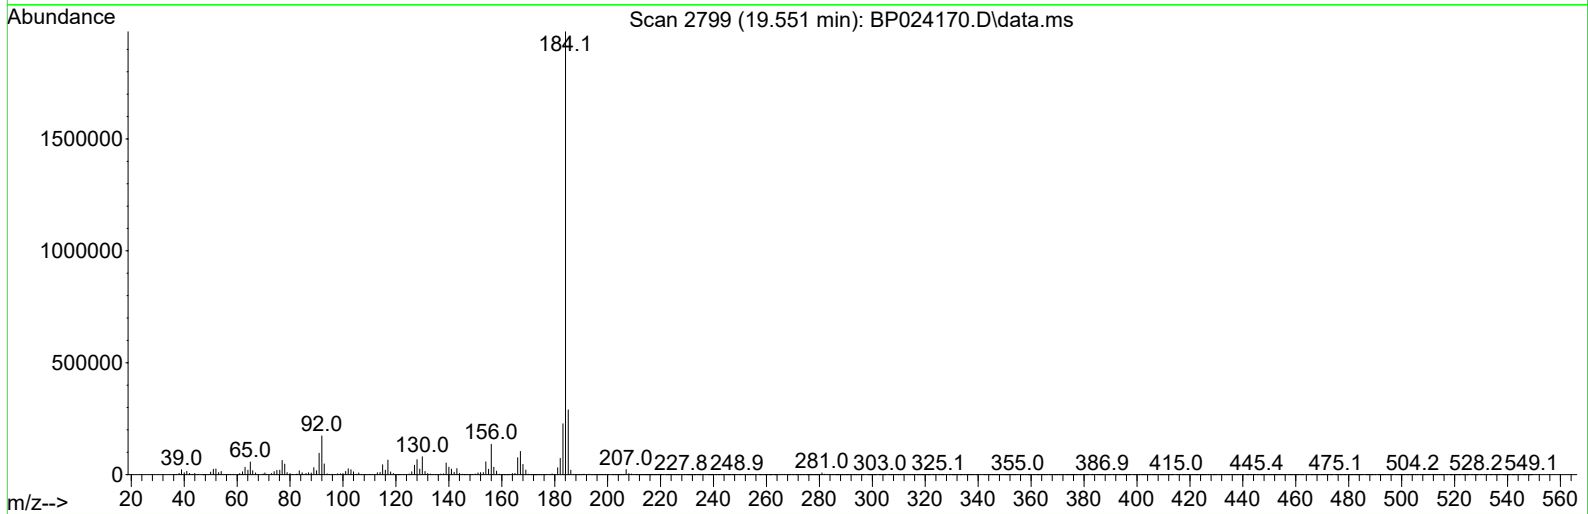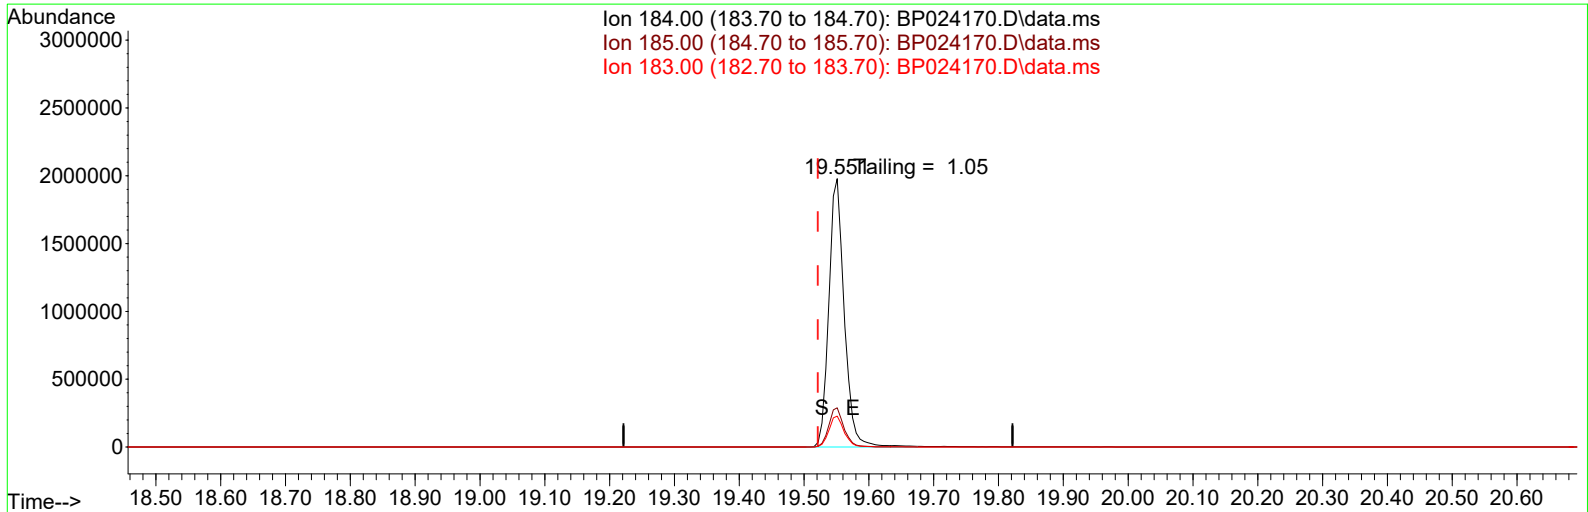

TIC: BP024170.D\data.ms

(77) Benzidine**19.551min (+ 0.029) 3326037.58 ng****response 3272849**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.62
183.00	11.40	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/13/2025	BNA_P	<u>BP024170.D</u>
Compound Name	Response	Retention Time
DDT	1542848	20.851
DDD	21899	20.375
DDE	1202	19.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23101	1565949	1.48

Instrument :
BNA_P
ClientSampleId :
DFTPP