

Cover Page

Order ID : Q1502

Project ID : NJ Waste Water PT

Client : Alliance Technical Group, LLC - Newark

Lab Sample Number

Q1502-01
Q1502-02
Q1502-03
Q1502-04
Q1502-05
Q1502-06
Q1502-07
Q1502-08
Q1502-09
Q1502-10
Q1502-11
Q1502-12
Q1502-13
Q1502-14
Q1502-15
Q1502-16
Q1502-17
Q1502-18
Q1502-19
Q1502-20
Q1502-21
Q1502-22

Client Sample Number

PT-VOA-WP
PT-VOA-WP
PT-BN-WP
PT-BN-WP
PT-BN-WP
PT-ACIDS-WP
PT-ACIDS-WP
PT-ACIDS-WP
PT-PEST-WP
PT-PEST-WP
PT-CHLR-WP
PT-CHLR-WP
PT-TXP-WP
PT-TXP-WP
PT-PCBW-WP
PT-PCBW-WP
PT-HERB-WP
RR-GAS-WP
RR-DIES-WP
RR-8011-WP
RR-PAH-WP
RR-TRIAZINE-WP

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : _____

Date: 3/20/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012



284 Sheffield Street, Mountainside, NJ 07092
Phone: 908 789 8900 Fax: 908 789 8922

CASE NARRATIVE

Alliance Technical Group, LLC - Newark

Project Name: NJ Waste Water PT

Project # N/A

Chemtech Project # Q1502

Test Name: VOCMS Group1

A. Number of Samples and Date of Receipt:

21 Water samples were received on 03/05/2025.

1 Water sample was received on 03/11/2025.

B. Parameters

According to the Chain of Custody document, the following analyses were requested: Diesel Range Organics, Gasoline Range Organics, Herbicide group1, PCB, PESTICIDE Group1, PESTICIDE Group2, PESTICIDE Group3, SVOCMS Group1, SVOCMS Group2, SVOCMS Group3, SVOCMS Group4, SVOCMS Group5, SVOCMS Group6, VOCGC Group 1 and VOCMS Group1. This data package contains results for VOCMS Group1.

C. Analytical Techniques:

The analysis performed on instrument MSVOA_X were done using GC column DB-624UI 20m 0.18mm 1.0 um. Cat#121-1324UIThe analysis of VOCMS Group1 was based on method 624.1,8260D.

D. QA/ QC Samples:

The Holding Times were met for all analysis.

The Surrogate recoveries met the acceptable criteria.

The Internal Standards Areas met the acceptable requirements.

The Retention Times were acceptable for all samples.

The RPD met criteria .

The Blank Spike for {VX0311WBS01} with File ID: VX045214.D met requirements for all samples except for 2,2-Dichloropropane[143%],are failing high but no positive hit in associate samples therefore no corrective action taken.

The Blank Spike Duplicate for {VX0311WBSD01} with File ID: VX045215.D met requirements for all samples except for 2,2-Dichloropropane[136%],are failing high but no positive hit in associate samples therefore no corrective action taken.

The Blank analysis did not indicate the presence of lab contamination.

The Initial Calibration met the requirements .



284 Sheffield Street, Mountainside, NJ 07092
Phone: 908 789 8900 Fax: 908 789 8922

The Continuous Calibration File ID VX045211.D met the requirements except for 2,2-Dichloropropane ,is failing high but no positive hit in associate samples therefore no corrective action taken.

The Tuning criteria met requirements.

E. Additional Comments:

Please use %D calculated based on Avg RF and CCRF for all compounds using Average Response Factor when the %RSD value for a compound is <20% for the Initial Calibration curve and use %D calculated based on Amount added and Calculated amount for all compounds using Linear Regression when the %RSD value for a compound is > 20% for the Initial Calibration curve for SW-846 analysis.

F. Manual Integration Comments:

Please refer to the Manual integration Report included with the Run Logs for information on the manual integrations performed.

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

Signature _____

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following "Results Qualifiers" are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as "12 B".
E	Indicates the analyte 's concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

ALLIANCE 284 Sheffield Street, Mountainside New Jersey 07092

NEW JERSEY LAB ID#: 20012: NEW YORK LAB ID#: 11376

GC/MS VOA CONFORMANCE/NON-CONFORMANCE SUMMARY

CHEMTECH PROJECT NUMBER: Q1502

MATRIX: Water

METHOD: 624.1,8260D

		NA	NO	YES
1.	Chromatograms Labeled/Compounds Identified. (Field samples and Method Blanks)			✓
2.	GC/MS Tuning Specifications BFB Meet Criteria (NOTE THAT THERE ARE DIFFERENT CRITERIA FOR NY ASP CLP, CLP AND NJ)			✓
3.	GC/MS Tuning Frequency - Performed every 24 hours for 600 series and 12 hours for 8000 Series.			✓
4.	GC/MS Calibration - Initial Calibration performed before sample analysis and continuing calibration performed within 24 hours of sample analysis for 600 series and 12 hours for 8000 series.			✓
5.	GC/MS Calibration Requirements. The Initial Calibration met the requirements .			✓
	The Continuous Calibration File ID VX045211.D met the requirements except for 2,2-Dichloropropane ,is failing high but no positive hit in associate samples therefore no corrective action taken.			
6.	Blank Contamination - If yes, list compounds and concentrations in each blank:			✓
7.	Surrogate Recoveries Meet Criteria If not met, list those compounds and their recoveries which fall outside the acceptable ranges.			✓
8.	Matrix Spike/Matrix Spike Duplicate Recoveries Meet Criteria If not met, list those compounds and their recoveries which fall outside the acceptable range.			✓
	The Blank Spike for {VX0311WBS01} with File ID: VX045214.D met requirements for all samples except for 2,2-Dichloropropane[143%],are failing high but no positive hit in associate samples therefore no corrective action taken.			
	The Blank Spike Duplicate for {VX0311WBSD01} with File ID: VX045215.D met requirements for all samples except for 2,2-Dichloropropane[136%],are failing high but no positive hit in associate samples therefore no corrective action taken.			
9.	Internal Standard Area/Retention Time Shift Meet Criteria			✓
	Comments:			
10.	Analysis Holding Time Met If not met, list number of days exceeded for each sample:			✓

ALLIANCE 284 Sheffield Street, Mountainside New Jersey 07092

NEW JERSEY LAB ID#: 20012: NEW YORK LAB ID#: 11376

GC/MS VOA CONFORMANCE/NON-CONFORMANCE SUMMARY (CONTINUED)

NA NO YES

ADDITIONAL COMMENTS:

Please use %D calculated based on Avg RF and CCRF for all compounds using Average Response Factor when the %RSD value for a compound is <20% for the Initial Calibration curve and use %D calculated based on Amount added and Calculated amount for all compounds using Linear Regression when the %RSD value for a compound is > 20% for the Initial Calibration curve for SW-846 analysis.

QA REVIEW

Date

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: Q1502

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication, airbill, sample management lab chronicle, login page) ✓

Check chain-of-custody for proper relinquish/return of samples ✓

Is the chain of custody signed and complete ✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts ✓

Collect information for each project id from server. Were all requirements followed ✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page ✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody ✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results ✓

Do requested analyses on Chain of Custody agree with the log-in page ✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Castody ✓

Were the samples received within hold time ✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle ✓

ANALYTICAL:

Was method requirement followed? ✓

Was client requirement followed? ✓

Does the case narrative summarize all QC failure? ✓

All runlogs and manual integration are reviewed for requirements ✓

All manual calculations and /or hand notations verified ✓

LAB CHRONICLE

OrderID:	Q1502	OrderDate:	3/6/2025 10:04:07 AM					
Client:	Alliance Technical Group, LLC - Newark	Project:	NJ Waste Water PT					
Contact:	Mohammad Ahmed	Location:	QA Office, VOA Lab					
<hr/>								
LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q1502-01	PT-VOA-WP	Water	VOCMS Group1	8260-Low	03/03/25		03/11/25	03/05/25

Hit Summary Sheet
SW-846

SDG No.: Q1502

Client: Alliance Technical Group, LLC - Newark

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
Client ID:	PT-VOA-WP							
Q1502-01	PT-VOA-WP	Water	Bromomethane	61.5	1.40		5.00	ug/L
Q1502-01	PT-VOA-WP	Water	Trichlorofluoromethane	95.4	0.34		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	1,1-Dichloroethene	87.4	0.26		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	Acetone	150	1.40		5.00	ug/L
Q1502-01	PT-VOA-WP	Water	Methyl tert-butyl Ether	54.9	0.16		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	Methylene Chloride	48.8	0.32		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	trans-1,2-Dichloroethene	80.5	0.25		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	2-Butanone	41.2	1.30		5.00	ug/L
Q1502-01	PT-VOA-WP	Water	Carbon Tetrachloride	29.8	0.25		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	cis-1,2-Dichloroethene	110	0.25		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	Chloroform	68.7	0.26		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	Benzene	110	0.16		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	1,2-Dichloroethane	35.7	0.24		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	Trichloroethene	51.9	0.32		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	1,2-Dichloropropane	77.5	0.19		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	Dibromomethane	100	0.23		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	Bromodichloromethane	16.2	0.24		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	4-Methyl-2-Pentanone	120	0.75		5.00	ug/L
Q1502-01	PT-VOA-WP	Water	Toluene	110	0.18		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	t-1,3-Dichloropropene	85.1	0.21		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	cis-1,3-Dichloropropene	61.7	0.18		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	2-Hexanone	140	1.10		5.00	ug/L
Q1502-01	PT-VOA-WP	Water	Tetrachloroethene	120	0.25		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	Chlorobenzene	110	0.13		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	1,1,1,2-Tetrachloroethane	110	0.21		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	Ethyl Benzene	35.4	0.16		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	Total Xylenes	213	0.45		3.00	ug/L
Q1502-01	PT-VOA-WP	Water	m/p-Xylenes	72.6	0.31		2.00	ug/L
Q1502-01	PT-VOA-WP	Water	o-Xylene	140	0.14		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	Styrene	89.6	0.16		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	1,3,5-Trimethylbenzene	92.9	0.18		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	1,3-Dichlorobenzene	48.9	0.24		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	1,2-Dichlorobenzene	120	0.19		1.00	ug/L
Q1502-01	PT-VOA-WP	Water	Naphthalene	86.5	0.59		1.00	ug/L

Total Voc : 2760

Total Concentration: 2760

Hit Summary Sheet
SW-846

SDG No.: Q1502

Client: Alliance Technical Group, LLC - Newark

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------



QC

SUMMARY

Surrogate Summary

SDG No.: Q1502

Client: Alliance Technical Group, LLC - Newark

Analytical Method: SW8260-Low

Lab Sample ID	Client ID	Parameter	Spike	Result	RecoveryQual	Limits	
						Low	High
Q1502-01	PT-VOA-WP	1,2-Dichloroethane-d4	50	48.8	98	74	125
		Dibromofluoromethane	50	49.0	98	75	124
		Toluene-d8	50	49.0	98	86	113
		4-Bromofluorobenzene	50	49.1	98	77	121
VX0311WBL01	VX0311WBL01	1,2-Dichloroethane-d4	50	53.3	107	74	125
		Dibromofluoromethane	50	50.6	101	75	124
		Toluene-d8	50	50.6	101	86	113
		4-Bromofluorobenzene	50	51.4	103	77	121
VX0311WBS01	VX0311WBS01	1,2-Dichloroethane-d4	50	52.0	104	74	125
		Dibromofluoromethane	50	51.9	104	75	124
		Toluene-d8	50	51.2	102	86	113
		4-Bromofluorobenzene	50	52.9	106	77	121
VX0311WBSD0	VX0311WBSD01	1,2-Dichloroethane-d4	50	51.1	102	74	125
		Dibromofluoromethane	50	51.0	102	75	124
		Toluene-d8	50	50.7	101	86	113
		4-Bromofluorobenzene	50	54.4	109	77	121



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:

Q1502

Client:

Alliance Technical Group, LLC - Newark

Analytical Method:

SW8260-Low

Datafile : VX045214.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		
								Low	High	RPD
VX0311WBS01	Dichlorodifluoromethane	20	19.5	ug/L	98			69	116	
	Chloromethane	20	18.8	ug/L	94			65	116	
	Vinyl chloride	20	17.5	ug/L	88			65	117	
	Ethyl Acetate	20	19.1	ug/L	96			75	115	
	Bromomethane	20	18.9	ug/L	95			58	125	
	Chloroethane	20	21.4	ug/L	107			56	128	
	Trichlorodifluoromethane	20	19.1	ug/L	96			73	115	
	1,1,2-Trichlorotrifluoroethane	20	20.8	ug/L	104			80	112	
	1,1-Dichloroethene	20	18.8	ug/L	94			74	110	
	Acrolein	100	83.3	ug/L	83			51	143	
	Acrylonitrile	100	100	ug/L	100			73	113	
	Acetone	100	97.2	ug/L	97			60	125	
	Carbon disulfide	20	16.9	ug/L	85			64	112	
	Methyl tert-butyl Ether	20	19.5	ug/L	98			78	114	
	Methylene Chloride	20	18.6	ug/L	93			72	114	
	trans-1,2-Dichloroethene	20	19.4	ug/L	97			75	108	
	Vinyl Acetate	100	98.7	ug/L	99			76	115	
	1,1-Dichloroethane	20	19.6	ug/L	98			78	112	
	2-Butanone	100	100	ug/L	100			65	122	
	Carbon Tetrachloride	20	19.7	ug/L	99			77	113	
	2,2-Dichloropropane	20	28.6	ug/L	143	*		75	116	
	cis-1,2-Dichloroethene	20	19.2	ug/L	96			77	110	
	Chloroform	20	19.9	ug/L	100			79	113	
	1,1,1-Trichloroethane	20	20.0	ug/L	100			80	108	
	1,1-Dichloropropene	20	18.9	ug/L	95			79	110	
	Benzene	20	19.4	ug/L	97			82	109	
	1,2-Dichloroethane	20	19.8	ug/L	99			80	115	
	Trichloroethene	20	18.9	ug/L	95			77	113	
	1,2-Dichloropropane	20	18.9	ug/L	95			83	111	
	Dibromomethane	20	20.1	ug/L	101			82	110	
	Bromodichloromethane	20	19.6	ug/L	98			83	110	
	4-Methyl-2-Pentanone	100	110	ug/L	110			74	118	
	Toluene	20	20.0	ug/L	100			82	110	
	t-1,3-Dichloropropene	20	20.0	ug/L	100			79	110	
	cis-1,3-Dichloropropene	20	20.6	ug/L	103			82	110	
	1,1,2-Trichloroethane	20	19.5	ug/L	98			83	112	
	1,3-Dichloropropene	20	20.1	ug/L	101			83	111	
	2-Chloroethyl vinyl ether	100	96.2	ug/L	96			75	124	
	2-Hexanone	100	110	ug/L	110			73	117	
	Dibromochloromethane	20	19.5	ug/L	98			82	110	
	1,2-Dibromoethane	20	19.6	ug/L	98			81	110	
	Tetrachloroethene	20	19.5	ug/L	98			67	123	
	Chlorobenzene	20	19.7	ug/L	99			82	109	
	1,1,1,2-Tetrachloroethane	20	19.7	ug/L	99			84	111	
	Ethyl Benzene	20	19.8	ug/L	99			83	109	
	m/p-Xylenes	40	40.1	ug/L	100			82	110	
	o-Xylene	20	19.4	ug/L	97			83	109	
	Styrene	20	20.3	ug/L	102			80	111	



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:

Q1502

Client:

Alliance Technical Group, LLC - Newark

Analytical Method:

SW8260-Low

Datafile : VX045214.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		
								Low	High	RPD
VX0311WBS01	Bromoform	20	20.0	ug/L	100			79	109	
	Isopropylbenzene	20	19.1	ug/L	96			83	112	
	1,1,2,2-Tetrachloroethane	20	19.5	ug/L	98			76	118	
	1,2,3-Trichloropropane	20	19.2	ug/L	96			75	112	
	Bromobenzene	20	18.5	ug/L	93			77	116	
	N-propylbenzene	20	19.2	ug/L	96			83	112	
	2-Chlorotoluene	20	18.4	ug/L	92			83	110	
	1,3,5-Trimethylbenzene	20	19.3	ug/L	97			85	112	
	4-Chlorotoluene	20	19.2	ug/L	96			82	110	
	1,2,4-Trimethylbenzene	20	19.2	ug/L	96			85	111	
	Sec-butylbenzene	20	19.6	ug/L	98			81	114	
	p-Isopropyltoluene	20	19.8	ug/L	99			78	116	
	1,3-Dichlorobenzene	20	19.3	ug/L	97			82	108	
	1,4-Dichlorobenzene	20	18.7	ug/L	94			82	107	
	n-Butylbenzene	20	19.8	ug/L	99			75	115	
	1,2-Dichlorobenzene	20	19.4	ug/L	97			82	109	
	1,2-Dibromo-3-Chloropropane	20	19.1	ug/L	96			68	112	
	1,2,4-Trichlorobenzene	20	18.9	ug/L	95			75	113	
	Hexachlorobutadiene	20	20.1	ug/L	101			81	121	
	Naphthalene	20	18.8	ug/L	94			78	119	
	1,2,3-Trichlorobenzene	20	18.7	ug/L	94			76	114	

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:

Q1502

Client:

Alliance Technical Group, LLC - Newark

Analytical Method:

SW8260-Low

Datafile : VX045215.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		
								Low	High	RPD
VX0311WBSD01	Dichlorodifluoromethane	20	19.4	ug/L	97	1		69	116	20
	Chloromethane	20	17.9	ug/L	90	4		65	116	20
	Vinyl chloride	20	16.9	ug/L	85	3		65	117	20
	Ethyl Acetate	20	18.4	ug/L	92	4		75	115	20
	Bromomethane	20	19.1	ug/L	96	1		58	125	20
	Chloroethane	20	19.7	ug/L	99	8		56	128	20
	Trichlorofluoromethane	20	18.7	ug/L	94	2		73	115	20
	1,1,2-Trichlorotrifluoroethane	20	20.7	ug/L	104	0		80	112	20
	1,1-Dichloroethene	20	18.4	ug/L	92	2		74	110	20
	Acrolein	100	79.1	ug/L	79	5		51	143	20
	Acrylonitrile	100	100	ug/L	100	0		73	113	20
	Acetone	100	96.0	ug/L	96	1		60	125	20
	Carbon disulfide	20	16.4	ug/L	82	4		64	112	20
	Methyl tert-butyl Ether	20	19.3	ug/L	97	1		78	114	20
	Methylene Chloride	20	19.2	ug/L	96	3		72	114	20
	trans-1,2-Dichloroethene	20	19.2	ug/L	96	1		75	108	20
	Vinyl Acetate	100	99.8	ug/L	100	1		76	115	20
	1,1-Dichloroethane	20	19.2	ug/L	96	2		78	112	20
	2-Butanone	100	100	ug/L	100	0		65	122	20
	Carbon Tetrachloride	20	19.4	ug/L	97	2		77	113	20
	2,2-Dichloropropane	20	27.1	ug/L	136	5	*	75	116	20
	cis-1,2-Dichloroethene	20	19.2	ug/L	96	0		77	110	20
	Chloroform	20	19.5	ug/L	98	2		79	113	20
	1,1,1-Trichloroethane	20	19.2	ug/L	96	4		80	108	20
	1,1-Dichloropropene	20	18.9	ug/L	95	0		79	110	20
	Benzene	20	19.2	ug/L	96	1		82	109	20
	1,2-Dichloroethane	20	19.9	ug/L	100	1		80	115	20
	Trichloroethene	20	19.0	ug/L	95	0		77	113	20
	1,2-Dichloropropane	20	19.1	ug/L	96	1		83	111	20
	Dibromomethane	20	19.8	ug/L	99	2		82	110	20
	Bromodichloromethane	20	19.8	ug/L	99	1		83	110	20
	4-Methyl-2-Pentanone	100	110	ug/L	110	0		74	118	20
	Toluene	20	19.8	ug/L	99	1		82	110	20
	t-1,3-Dichloropropene	20	20.1	ug/L	101	1		79	110	20
	cis-1,3-Dichloropropene	20	20.1	ug/L	101	2		82	110	20
	1,1,2-Trichloroethane	20	20.0	ug/L	100	2		83	112	20
	1,3-Dichloropropene	20	20.6	ug/L	103	2		83	111	20
	2-Chloroethyl vinyl ether	100	98.3	ug/L	98	2		75	124	20
	2-Hexanone	100	110	ug/L	110	0		73	117	20
	Dibromochloromethane	20	19.9	ug/L	100	2		82	110	20
	1,2-Dibromoethane	20	20.7	ug/L	104	6		81	110	20
	Tetrachloroethene	20	19.3	ug/L	97	1		67	123	20
	Chlorobenzene	20	19.6	ug/L	98	1		82	109	20
	1,1,1,2-Tetrachloroethane	20	19.0	ug/L	95	4		84	111	20
	Ethyl Benzene	20	19.7	ug/L	99	0		83	109	20
	m/p-Xylenes	40	39.9	ug/L	100	0		82	110	20
	o-Xylene	20	20.2	ug/L	101	4		83	109	20
	Styrene	20	20.5	ug/L	103	1		80	111	20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:

Q1502

Client:

Alliance Technical Group, LLC - Newark

Analytical Method:

SW8260-Low

Datafile : VX045215.D

Lab Sample ID	Parameter	Spike	Result	Unit	Rec	RPD	Qual	Limits		
								Low	High	RPD
VX0311WBSD01	Bromoform	20	20.3	ug/L	102	2		79	109	20
	Isopropylbenzene	20	19.4	ug/L	97	1		83	112	20
	1,1,2,2-Tetrachloroethane	20	19.7	ug/L	99	1		76	118	20
	1,2,3-Trichloropropane	20	19.2	ug/L	96	0		75	112	20
	Bromobenzene	20	19.4	ug/L	97	4		77	116	20
	N-propylbenzene	20	19.9	ug/L	100	4		83	112	20
	2-Chlorotoluene	20	19.3	ug/L	97	5		83	110	20
	1,3,5-Trimethylbenzene	20	20.1	ug/L	101	4		85	112	20
	4-Chlorotoluene	20	20.0	ug/L	100	4		82	110	20
	1,2,4-Trimethylbenzene	20	20.0	ug/L	100	4		85	111	20
	Sec-butylbenzene	20	20.5	ug/L	103	5		81	114	20
	p-Isopropyltoluene	20	20.5	ug/L	103	4		78	116	20
	1,3-Dichlorobenzene	20	19.6	ug/L	98	1		82	108	20
	1,4-Dichlorobenzene	20	19.2	ug/L	96	2		82	107	20
	n-Butylbenzene	20	20.6	ug/L	103	4		75	115	20
	1,2-Dichlorobenzene	20	19.8	ug/L	99	2		82	109	20
	1,2-Dibromo-3-Chloropropane	20	19.4	ug/L	97	1		68	112	20
	1,2,4-Trichlorobenzene	20	19.5	ug/L	98	3		75	113	20
	Hexachlorobutadiene	20	19.9	ug/L	100	1		81	121	20
	Naphthalene	20	19.2	ug/L	96	2		78	119	20
	1,2,3-Trichlorobenzene	20	19.3	ug/L	97	3		76	114	20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE METHOD BLANK SUMMARY

EPA SAMPLE NO.

VX0311WBL01

Lab Name: CHEMTECH

Contract: ALLI03

Lab Code: CHEM Case No.: Q1502

SAS No.: Q1502 SDG NO.: Q1502

Lab File ID: VX045213.D

Lab Sample ID: VX0311WBL01

Date Analyzed: 03/11/2025

Time Analyzed: 10:51

GC Column: DB-624UI ID: 0.18 (mm)

Heated Purge: (Y/N) N

Instrument ID: MSVOA_X

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED
<u>VX0311WBS01</u>	<u>VX0311WBS01</u>	<u>VX045214.D</u>	<u>03/11/2025</u>
<u>VX0311WBSD01</u>	<u>VX0311WBSD01</u>	<u>VX045215.D</u>	<u>03/11/2025</u>
<u>PT-VOA-WP</u>	<u>Q1502-01</u>	<u>VX045216.D</u>	<u>03/11/2025</u>

COMMENTS:



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: CHEMTECH Contract: ALLI03
Lab Code: CHEM Case No.: Q1502 SAS No.: Q1502 SDG NO.: Q1502
Lab File ID: VX045067.D BFB Injection Date: 02/28/2025
Instrument ID: MSVOA_X BFB Injection Time: 01:03
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: Y/N N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	20.7
75	30.0 - 60.0% of mass 95	53.6
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	6.6
173	Less than 2.0% of mass 174	0.7 (1) 1
174	50.0 - 100.0% of mass 95	73.8
175	5.0 - 9.0% of mass 174	5.8 (7.9) 1
176	95.0 - 101.0% of mass 174	70.6 (95.6) 1
177	5.0 - 9.0% of mass 176	4.3 (6.2) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDICC001	VSTDICC001	VX045068.D	02/28/2025	01:27
VSTDICC005	VSTDICC005	VX045069.D	02/28/2025	02:13
VSTDICC020	VSTDICC020	VX045070.D	02/28/2025	02:37
VSTDICCC050	VSTDICCC050	VX045071.D	02/28/2025	03:00
VSTDICC100	VSTDICC100	VX045072.D	02/28/2025	03:23
VSTDICC150	VSTDICC150	VX045073.D	02/28/2025	03:47



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE ORGANIC INSTRUMENT PERFORMANCE CHECK
BROMOFLUOROBENZENE (BFB)

Lab Name: CHEMTECH Contract: ALLI03
Lab Code: CHEM Case No.: Q1502 SAS No.: Q1502 SDG NO.: Q1502
Lab File ID: VX045210.D BFB Injection Date: 03/11/2025
Instrument ID: MSVOA_X BFB Injection Time: 09:30
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: Y/N N

m/e	ION ABUNDANCE CRITERIA	% RELATIVE ABUNDANCE
50	15.0 - 40.0% of mass 95	20.8
75	30.0 - 60.0% of mass 95	54.5
95	Base Peak, 100% relative abundance	100
96	5.0 - 9.0% of mass 95	7
173	Less than 2.0% of mass 174	0.8 (1) 1
174	50.0 - 100.0% of mass 95	76.6
175	5.0 - 9.0% of mass 174	5.8 (7.6) 1
176	95.0 - 101.0% of mass 174	73.2 (95.6) 1
177	5.0 - 9.0% of mass 176	4.8 (6.6) 2

1-Value is % mass 174

2-Value is % mass 176

THIS CHECK APPLIES TO THE FOLLOWING SAMPLES, MS, MSD, BLANKS, AND STANDARDS:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED	TIME ANALYZED
VSTDCCC050	VSTDCCC050	VX045211.D	03/11/2025	09:59
VX0311WBL01	VX0311WBL01	VX045213.D	03/11/2025	10:51
VX0311WBS01	VX0311WBS01	VX045214.D	03/11/2025	11:14
VX0311WBSD01	VX0311WBSD01	VX045215.D	03/11/2025	11:40
PT-VOA-WP	Q1502-01	VX045216.D	03/11/2025	12:03



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH Contract: ALLI03
Lab Code: CHEM Case No.: Q1502 SAS No.: Q1502 SDG No.: Q1502
Lab File ID: VX045211.D Date Analyzed: 03/11/2025
Instrument ID: MSVOA_X Time Analyzed: 09:59
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS1 AREA #	RT #	IS2 AREA #	RT #	IS3 AREA #	RT #
12 HOUR STD	101357	5.54	176548	6.75	153652	10.05
UPPER LIMIT	202714	6.044	353096	7.251	307304	10.549
LOWER LIMIT	50678.5	5.044	88274	6.251	76826	9.549
EPA SAMPLE NO.						
PT-VOA-WP	98273	5.55	178256	6.76	158768	10.06
VX0311WBL01	69956	5.54	139206	6.76	126312	10.06
VX0311WBS01	94786	5.54	172566	6.76	151770	10.06
VX0311WBSD01	92082	5.54	166231	6.76	148942	10.05

IS1 = Pentafluorobenzene

IS2 = 1,4-Difluorobenzene

IS3 = Chlorobenzene-d5

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.

* Values outside of QC limits.



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOLATILE INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: CHEMTECH Contract: ALLI03
Lab Code: CHEM Case No.: Q1502 SAS No.: Q1502 SDG No.: Q1502
Lab File ID: VX045211.D Date Analyzed: 03/11/2025
Instrument ID: MSVOA_X Time Analyzed: 09:59
GC Column: DB-624UI ID: 0.18 (mm) Heated Purge: (Y/N) N

	IS4 AREA #	RT #				
12 HOUR STD	70136	12.018				
	140272	12.518				
	35068	11.518				
EPA SAMPLE NO.						
PT-VOA-WP	68042	12.02				
VX0311WBL01	50068	12.02				
VX0311WBS01	71836	12.02				
VX0311WBSD01	68861	12.02				

IS4 = 1,4-Dichlorobenzene-d4

AREA UPPER LIMIT = +100% of internal standard area

AREA LOWER LIMIT = -50% of internal standard area

RT UPPER LIMIT = +0.50 minutes of internal standard RT

RT LOWER LIMIT = -0.50 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.

* Values outside of QC limits.



SAMPLE

DATA

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:	03/03/25	
Project:	NJ Waste Water PT			Date Received:	03/05/25	
Client Sample ID:	PT-VOA-WP			SDG No.:	Q1502	
Lab Sample ID:	Q1502-01			Matrix:	Water	
Analytical Method:	SW8260			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group1	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045216.D	1		03/11/25 12:03	VX031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-71-8	Dichlorodifluoromethane	0.21	U	0.21	1.00	ug/L
74-87-3	Chloromethane	0.35	U	0.35	1.00	ug/L
75-01-4	Vinyl Chloride	0.34	U	0.34	1.00	ug/L
74-83-9	Bromomethane	61.5		1.40	5.00	ug/L
75-00-3	Chloroethane	0.56	U	0.56	1.00	ug/L
75-69-4	Trichlorofluoromethane	95.4		0.34	1.00	ug/L
75-35-4	1,1-Dichloroethene	87.4		0.26	1.00	ug/L
107-02-8	Acrolein	6.70	U	6.70	25.0	ug/L
107-13-1	Acrylonitrile	0.90	U	0.90	5.00	ug/L
67-64-1	Acetone	150		1.40	5.00	ug/L
75-15-0	Carbon Disulfide	0.32	U	0.32	1.00	ug/L
1634-04-4	Methyl tert-butyl Ether	54.9		0.16	1.00	ug/L
75-09-2	Methylene Chloride	48.8		0.32	1.00	ug/L
156-60-5	trans-1,2-Dichloroethene	80.5		0.25	1.00	ug/L
108-05-4	Vinyl Acetate	0.71	U	0.71	5.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
78-93-3	2-Butanone	41.2		1.30	5.00	ug/L
56-23-5	Carbon Tetrachloride	29.8		0.25	1.00	ug/L
594-20-7	2,2-Dichloropropane	0.31	UQ	0.31	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	110		0.25	1.00	ug/L
74-97-5	Bromochloromethane	0.18	U	0.18	1.00	ug/L
67-66-3	Chloroform	68.7		0.26	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.19	U	0.19	1.00	ug/L
563-58-6	1,1-Dichloropropene	0.18	U	0.18	1.00	ug/L
71-43-2	Benzene	110		0.16	1.00	ug/L
107-06-2	1,2-Dichloroethane	35.7		0.24	1.00	ug/L
79-01-6	Trichloroethene	51.9		0.32	1.00	ug/L
78-87-5	1,2-Dichloropropane	77.5		0.19	1.00	ug/L
74-95-3	Dibromomethane	100		0.23	1.00	ug/L
75-27-4	Bromodichloromethane	16.2		0.24	1.00	ug/L

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:	03/03/25	
Project:	NJ Waste Water PT			Date Received:	03/05/25	
Client Sample ID:	PT-VOA-WP			SDG No.:	Q1502	
Lab Sample ID:	Q1502-01			Matrix:	Water	
Analytical Method:	SW8260			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group1	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045216.D	1		03/11/25 12:03	VX031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
108-10-1	4-Methyl-2-Pentanone	120		0.75	5.00	ug/L
108-88-3	Toluene	110		0.18	1.00	ug/L
10061-02-6	t-1,3-Dichloropropene	85.1		0.21	1.00	ug/L
10061-01-5	cis-1,3-Dichloropropene	61.7		0.18	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
142-28-9	1,3-Dichloropropane	0.17	U	0.17	1.00	ug/L
110-75-8	2-Chloroethyl Vinyl ether	1.80	U	1.80	5.00	ug/L
591-78-6	2-Hexanone	140		1.10	5.00	ug/L
124-48-1	Dibromochloromethane	0.18	U	0.18	1.00	ug/L
106-93-4	1,2-Dibromoethane	0.16	U	0.16	1.00	ug/L
127-18-4	Tetrachloroethene	120		0.25	1.00	ug/L
108-90-7	Chlorobenzene	110		0.13	1.00	ug/L
630-20-6	1,1,1,2-Tetrachloroethane	110		0.21	1.00	ug/L
67-72-1	Hexachloroethane	0	U	0	0	ug/L
100-41-4	Ethyl Benzene	35.4		0.16	1.00	ug/L
179601-23-1	m/p-Xylenes	72.6		0.31	2.00	ug/L
1330-20-7	Total Xylenes	213		0.45	3.00	ug/L
95-47-6	o-Xylene	140		0.14	1.00	ug/L
100-42-5	Styrene	89.6		0.16	1.00	ug/L
75-25-2	Bromoform	0.21	U	0.21	1.00	ug/L
98-82-8	Isopropylbenzene	0.13	U	0.13	1.00	ug/L
79-34-5	1,1,2,2-Tetrachloroethane	0.27	U	0.27	1.00	ug/L
96-18-4	1,2,3-Trichloropropane	0.39	U	0.39	1.00	ug/L
108-86-1	Bromobenzene	0.26	U	0.26	1.00	ug/L
103-65-1	n-propylbenzene	0.14	U	0.14	1.00	ug/L
95-49-8	2-Chlorotoluene	0.16	U	0.16	1.00	ug/L
108-67-8	1,3,5-Trimethylbenzene	92.9		0.18	1.00	ug/L
106-43-4	4-Chlorotoluene	0.18	U	0.18	1.00	ug/L
98-06-6	tert-Butylbenzene	0.17	U	0.17	1.00	ug/L
95-63-6	1,2,4-Trimethylbenzene	0.18	U	0.18	1.00	ug/L
135-98-8	sec-Butylbenzene	0.17	U	0.17	1.00	ug/L

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:	03/03/25	
Project:	NJ Waste Water PT			Date Received:	03/05/25	
Client Sample ID:	PT-VOA-WP			SDG No.:	Q1502	
Lab Sample ID:	Q1502-01			Matrix:	Water	
Analytical Method:	SW8260			% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol:	5000	uL
Soil Aliquot Vol:	uL			Test:	VOCMS Group1	
GC Column:	DB-624UI	ID :	0.18	Level :	LOW	
Prep Method :						

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045216.D	1		03/11/25 12:03	VX031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
99-87-6	p-Isopropyltoluene	0.15	U	0.15	1.00	ug/L
541-73-1	1,3-Dichlorobenzene	48.9		0.24	1.00	ug/L
106-46-7	1,4-Dichlorobenzene	0.27	U	0.27	1.00	ug/L
104-51-8	n-Butylbenzene	0.22	U	0.22	1.00	ug/L
95-50-1	1,2-Dichlorobenzene	120		0.19	1.00	ug/L
96-12-8	1,2-Dibromo-3-Chloropropane	0.46	U	0.46	1.00	ug/L
120-82-1	1,2,4-Trichlorobenzene	0.42	U	0.42	1.00	ug/L
87-68-3	Hexachlorobutadiene	0.31	U	0.31	1.00	ug/L
91-20-3	Naphthalene	86.5		0.59	1.00	ug/L
87-61-6	1,2,3-Trichlorobenzene	0.51	U	0.51	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	48.8		74 - 125	98%	SPK: 50
1868-53-7	Dibromofluoromethane	49.0		75 - 124	98%	SPK: 50
2037-26-5	Toluene-d8	48.9		86 - 113	98%	SPK: 50
460-00-4	4-Bromofluorobenzene	49.1		77 - 121	98%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	98300	5.55			
540-36-3	1,4-Difluorobenzene	178000	6.757			
3114-55-4	Chlorobenzene-d5	159000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	68000	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045216.D
 Acq On : 11 Mar 2025 12:03
 Operator : JC/MD
 Sample : Q1502-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Time: Mar 12 01:45:54 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.550	168	98273	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	178256	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	158768	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	68042	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	76319	48.823	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	97.640%		
35) Dibromofluoromethane	5.385	113	58433	49.023	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	98.040%		
50) Toluene-d8	8.647	98	211517	48.948	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	97.900%		
62) 4-Bromofluorobenzene	11.079	95	70362	49.138	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	98.280%		
Target Compounds						
				Qvalue		
5) Bromomethane	1.593	94	36305	61.496	ug/l	98
7) Trichlorofluoromethane	1.874	101	189623	95.381	ug/l	99
12) 1,1-Dichloroethene	2.313	96	105601	87.449	ug/l	97
16) Acetone	2.386	43	106412	146.721	ug/l	100
19) Methyl tert-butyl Ether	3.117	73	222399	54.895	ug/l	97
20) Methylene Chloride	2.782	84	70051	48.759	ug/l	98
21) trans-1,2-Dichloroethene	3.087	96	96018	80.485	ug/l	96
25) 2-Butanone	4.562	43	44959	41.182	ug/l	99
27) cis-1,2-Dichloroethene	4.483	96	164344	111.594	ug/l	96
30) Chloroform	5.087	83	167331	68.737	ug/l	99
38) Carbon Tetrachloride	5.672	117	49440	29.791	ug/l	98
40) Benzene	6.031	78	580824	112.523	ug/l	99
42) 1,2-Dichloroethane	6.080	62	66393	35.719	ug/l	98
44) Trichloroethene	7.123	130	62917	51.910	ug/l	96
45) 1,2-Dichloropropane	7.428	63	102890	77.527	ug/l	98
46) Dibromomethane	7.580	93	94973	101.245	ug/l	98
47) Bromodichloromethane	7.824	83	29757	16.173	ug/l	98
51) 4-Methyl-2-Pentanone	8.574	43	255054	121.958	ug/l	100
52) Toluene	8.714	92	320220	105.734	ug/l	100
53) t-1,3-Dichloropropene	8.976	75	130835	85.056	ug/l	97
54) cis-1,3-Dichloropropene	8.360	75	110586	61.652	ug/l	95
59) 2-Hexanone	9.427	43	207188	136.734	ug/l	100
64) Tetrachloroethene	9.269	164	117148	115.207	ug/l	98
65) Chlorobenzene	10.080	112	378949	112.799	ug/l	99
66) 1,1,1,2-Tetrachloroethane	10.159	131	119812	107.091	ug/l	99
67) Ethyl Benzene	10.189	91	207014	35.365	ug/l	100
68) m/p-Xylenes	10.299	106	155658	72.639	ug/l	99
69) o-Xylene	10.640	106	304677	140.973	ug/l	98
70) Styrene	10.653	104	313173	89.554	ug/l	92
80) 1,3,5-Trimethylbenzene	11.451	105	398895	92.891	ug/l	100
87) 1,3-Dichlorobenzene	11.969	146	109258	48.877	ug/l	100
91) 1,2-Dichlorobenzene	12.335	146	262915	117.247	ug/l	99
95) Naphthalene	13.774	128	424244	86.479	ug/l	100




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045216.D
 Acq On : 11 Mar 2025 12:03
 Operator : JC/MD
 Sample : Q1502-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

Quant Time: Mar 12 01:45:54 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration


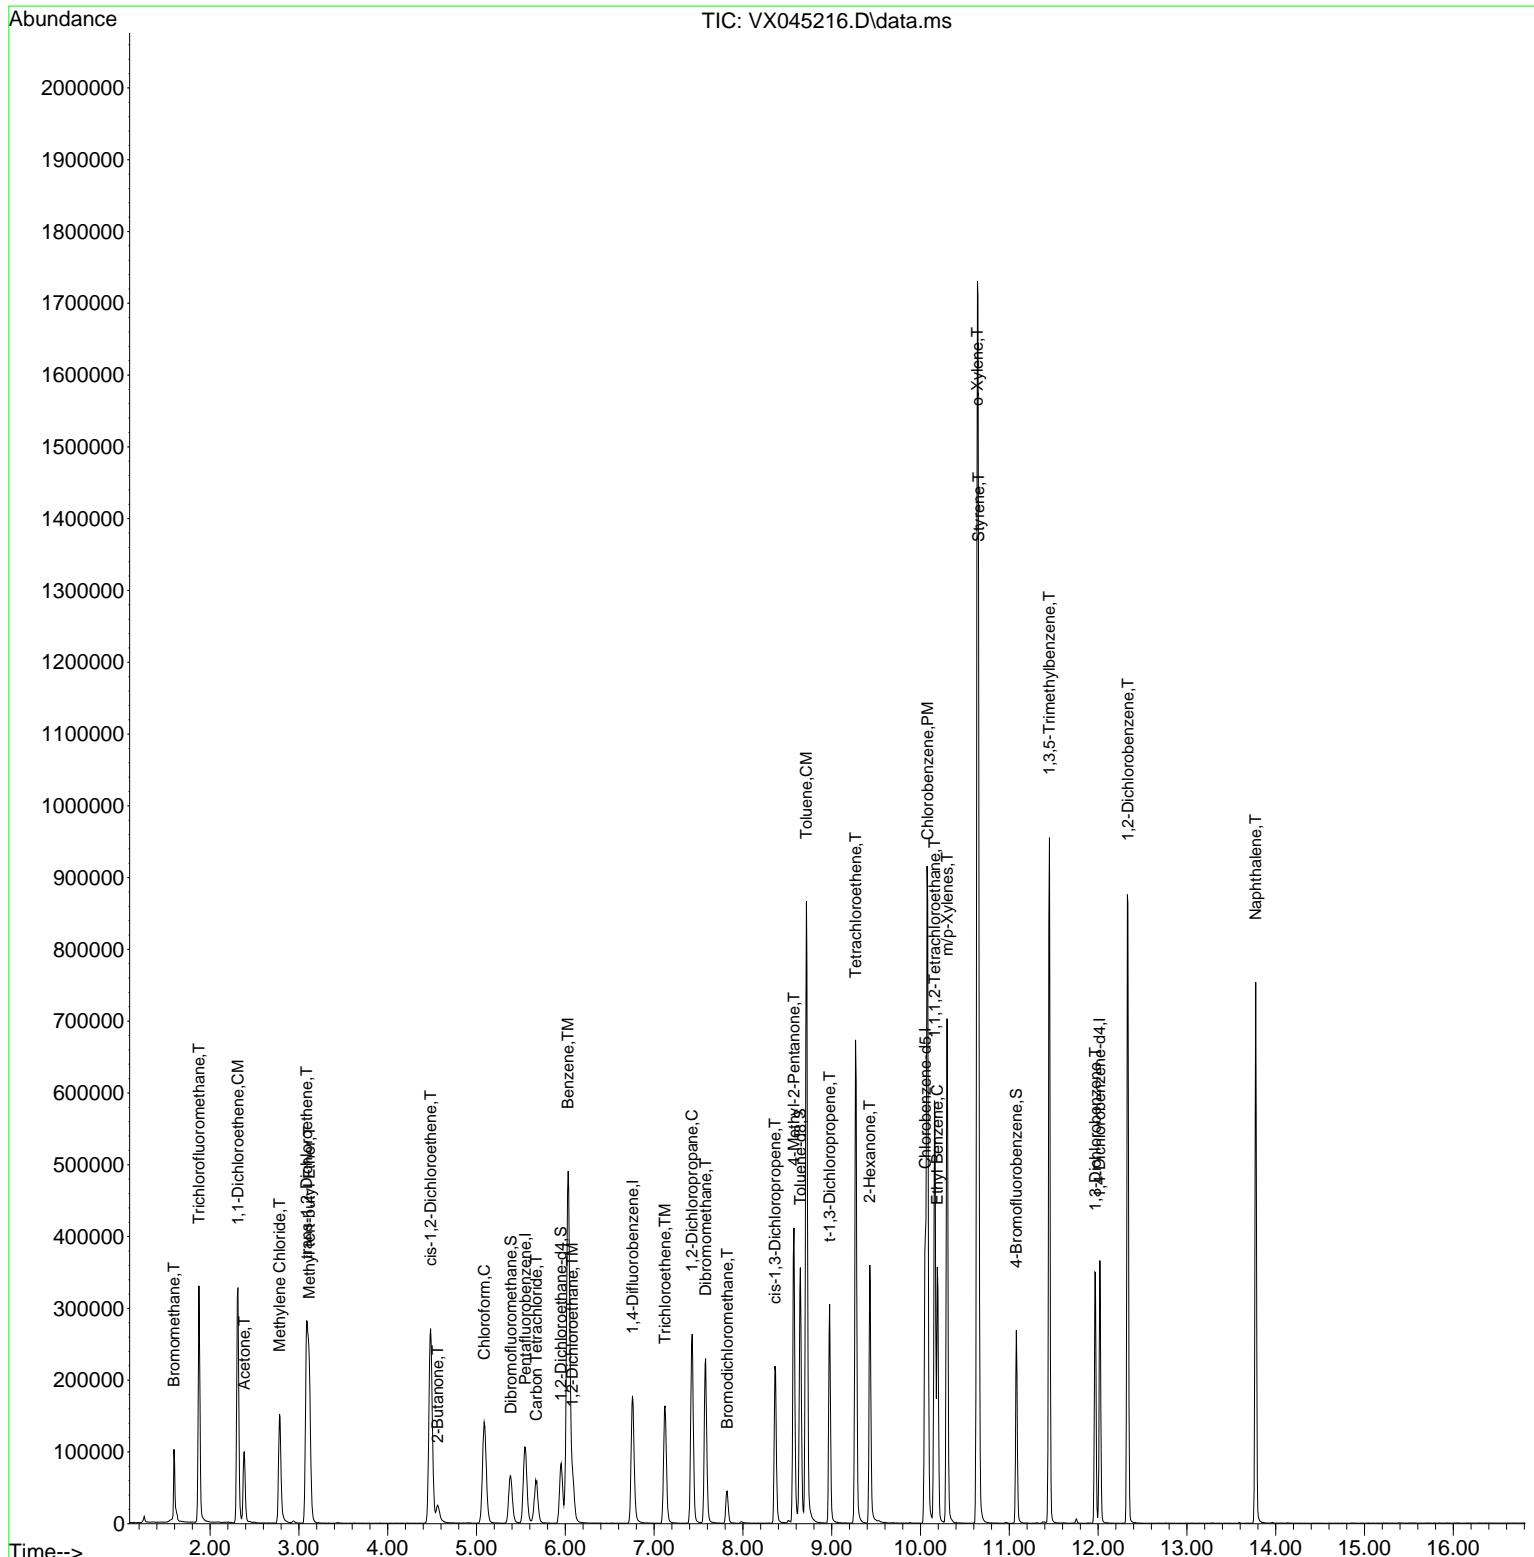


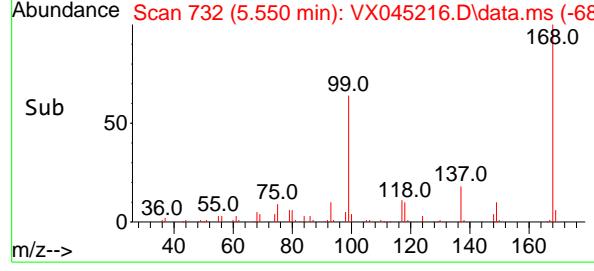

#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.550 min Scan# 7
 Delta R.T. -0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03




Instrument : MSVOA_X
 ClientSampleId : PT-VOA-WP


Tgt Ion:168 Resp: 98273
 Ion Ratio Lower Upper
 168 100
 99 63.7 48.2 72.4

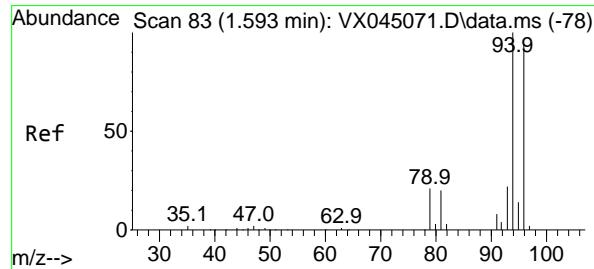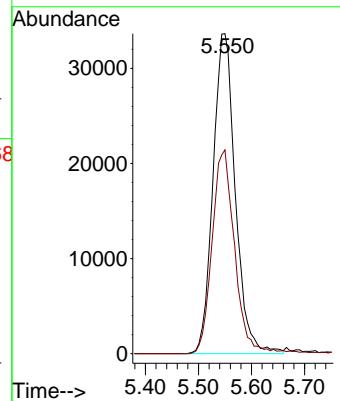

#5
 Bromomethane
 Concen: 61.496 ug/l
 RT: 1.593 min Scan# 83
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03


Tgt Ion: 94 Resp: 36305
 Ion Ratio Lower Upper
 94 100
 96 92.1 75.0 112.4

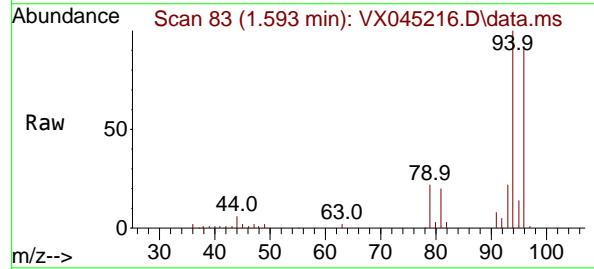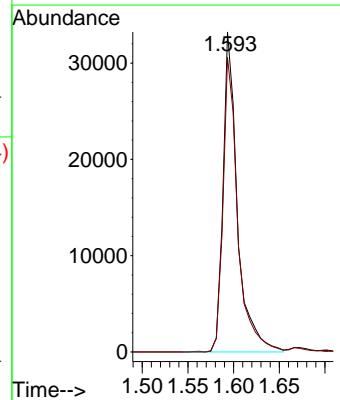






#7
Trichlorofluoromethane
Concen: 95.381 ug/l
RT: 1.874 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03

Instrument : MSVOA_X
ClientSampleId : PT-VOA-WP







Tgt Ion:101 Resp: 189623
Ion Ratio Lower Upper
101 100
103 64.7 52.1 78.1

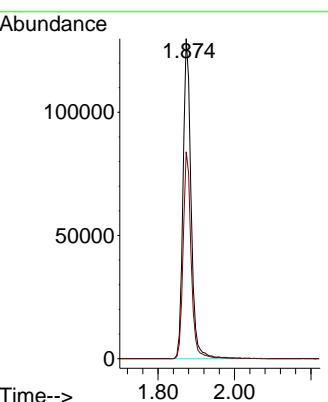


#12
1,1-Dichloroethene
Concen: 87.449 ug/l
RT: 2.313 min Scan# 201
Delta R.T. 0.006 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03

Tgt Ion: 96 Resp: 105601
Ion Ratio Lower Upper
96 100
61 171.5 134.6 202.0
98 67.0 51.0 76.6









#16
Acetone
Concen: 146.721 ug/l
RT: 2.386 min Scan# 2
Instrument : MSVOA_X
Delta R.T. 0.000 min
Lab File: VX045216.D
ClientSampleId : PT-VOA-WP
Acq: 11 Mar 2025 12:03





Tgt Ion: 43 Resp: 106412
Ion Ratio Lower Upper
43 100
58 30.5 24.2 36.4

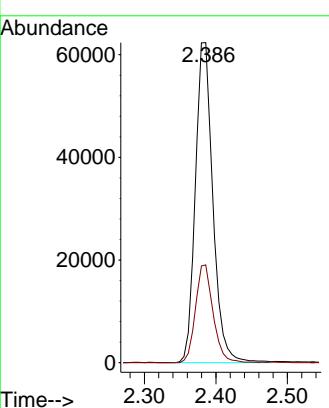


#19
Methyl tert-butyl Ether
Concen: 54.895 ug/l
RT: 3.117 min Scan# 333
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03




Tgt Ion: 73 Resp: 222399
Ion Ratio Lower Upper
73 100
57 21.5 18.5 27.7

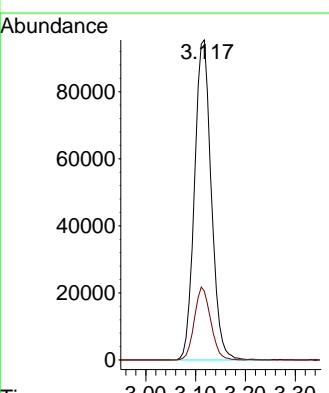





#20
 Methylene Chloride
 Concen: 48.759 ug/l
 RT: 2.782 min Scan# 2
Instrument :
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03
ClientSampleId :
 PT-VOA-WP



Tgt Ion: 84 Resp: 70051

Ion	Ratio	Lower	Upper
84	100		
49	135.4	106.5	159.7
51	40.7	32.1	48.1
86	64.7	50.0	75.0



Abundance

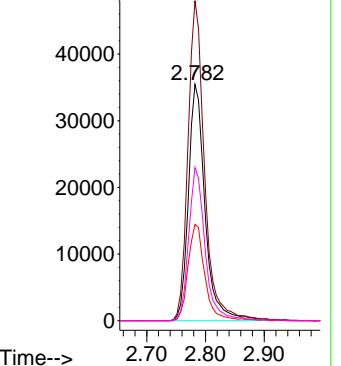

#21
 trans-1,2-Dichloroethene
 Concen: 80.485 ug/l
 RT: 3.087 min Scan# 328
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03

Tgt Ion: 96 Resp: 96018


Ion	Ratio	Lower	Upper
96	100		
61	143.2	117.0	175.4
98	61.8	53.4	80.2

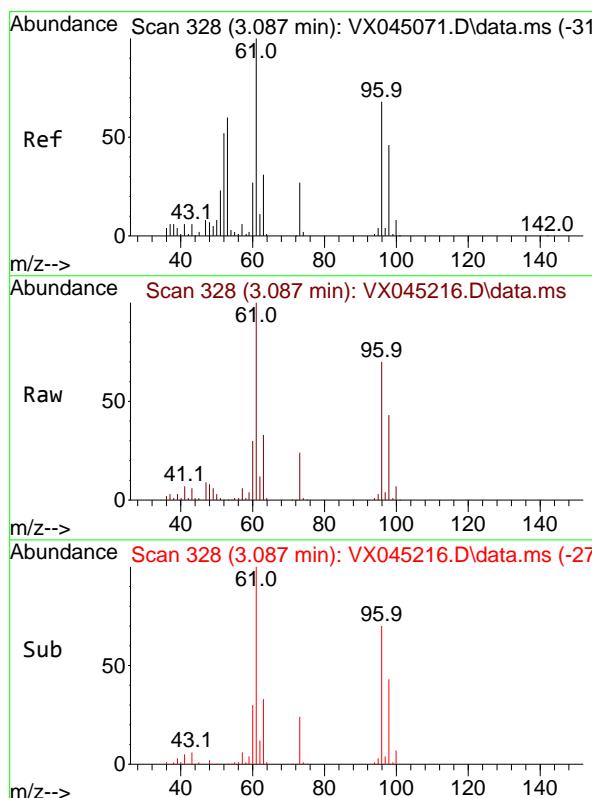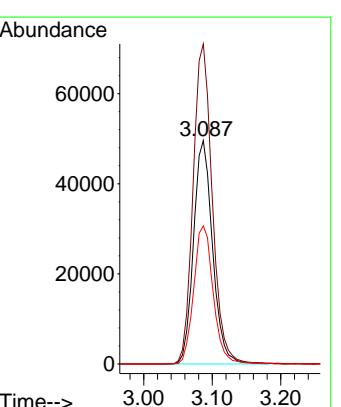

#21
 trans-1,2-Dichloroethene
 Concen: 80.485 ug/l
 RT: 3.087 min Scan# 328
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03


Tgt Ion: 96 Resp: 96018

Ion	Ratio	Lower	Upper
96	100		
61	143.2	117.0	175.4
98	61.8	53.4	80.2



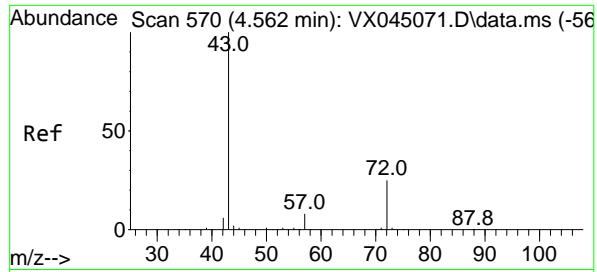


#25
 2-Butanone
 Concen: 41.182 ug/l
 RT: 4.562 min Scan# 5
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03


Instrument : MSVOA_X
 ClientSampleId : PT-VOA-WP

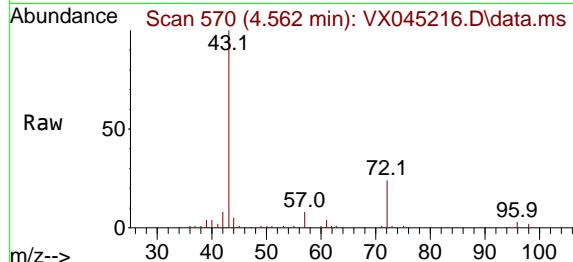



Tgt Ion: 43 Resp: 44959
 Ion Ratio Lower Upper
 43 100
 72 24.4 20.0 30.0

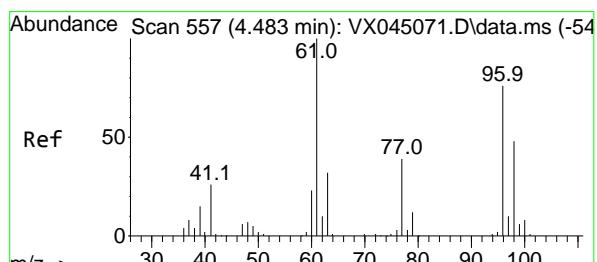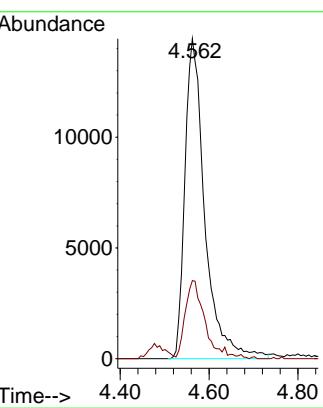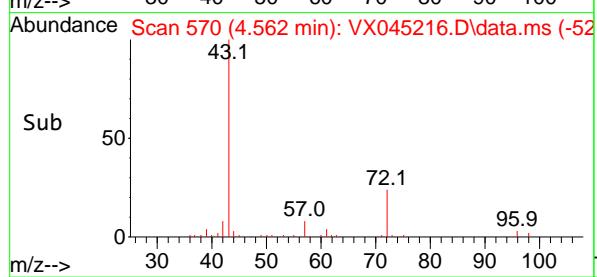


#27
 cis-1,2-Dichloroethene
 Concen: 111.594 ug/l
 RT: 4.483 min Scan# 557
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03

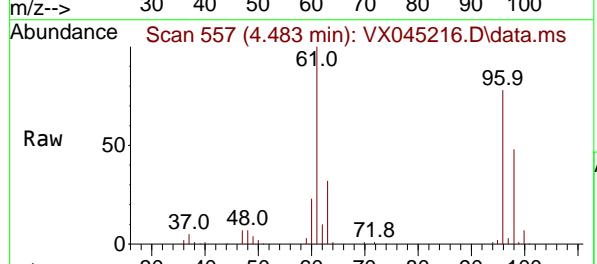


Tgt Ion: 96 Resp: 164344
 Ion Ratio Lower Upper
 96 100
 61 134.1 0.0 283.2
 98 64.0 0.0 128.0

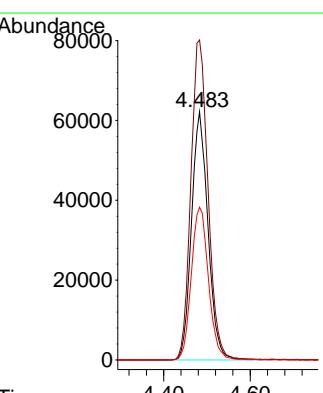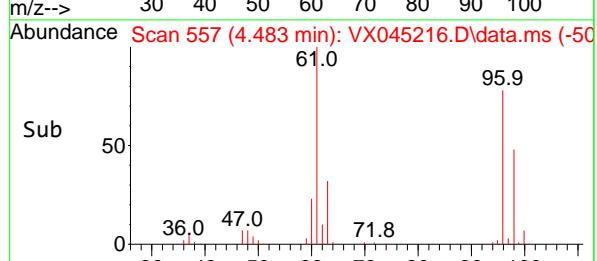


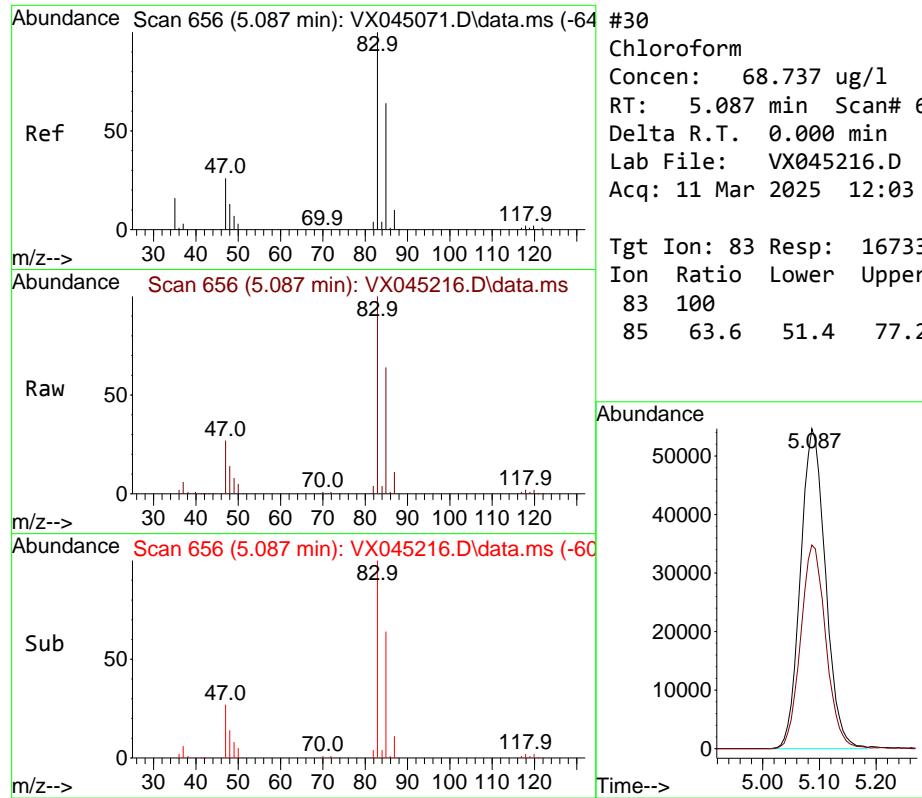

#30
Chloroform
Concen: 68.737 ug/l
RT: 5.087 min Scan# 6
Instrument : MSVOA_X
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03
ClientSampleId : PT-VOA-WP

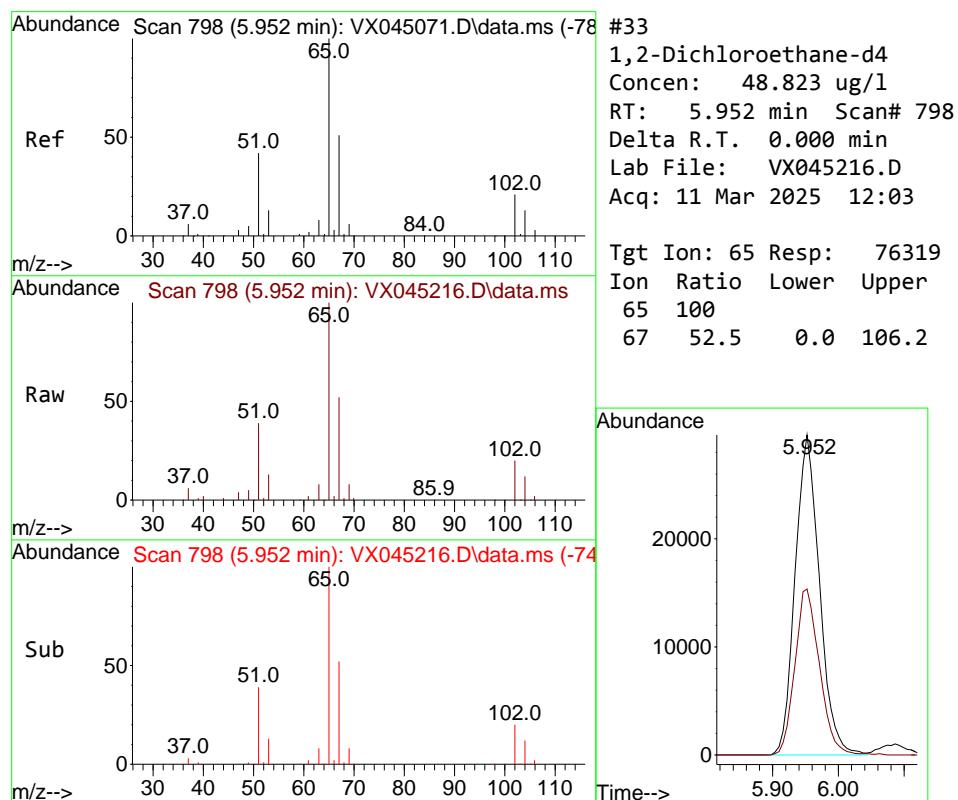



#33
1,2-Dichloroethane-d4
Concen: 48.823 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03

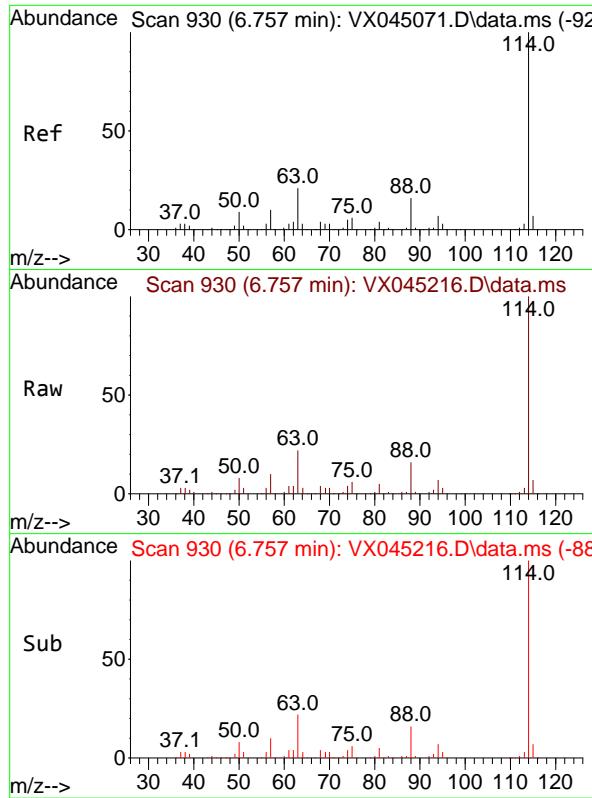

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 9
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03


Instrument : MSVOA_X
 ClientSampleId : PT-VOA-WP


Tgt Ion:114 Resp: 178256
 Ion Ratio Lower Upper
 114 100
 63 21.9 0.0 41.8
 88 15.9 0.0 32.8

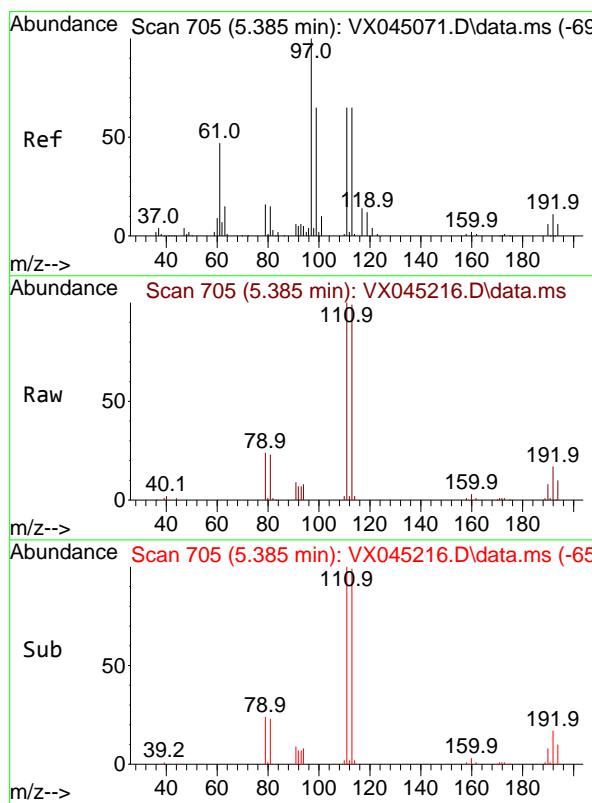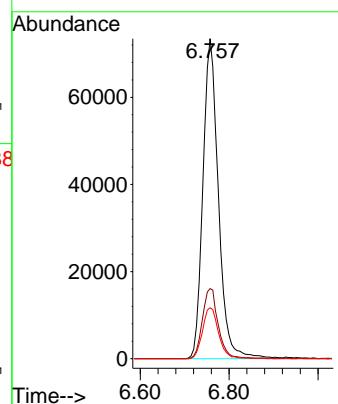

#35
 Dibromofluoromethane
 Concen: 49.023 ug/l
 RT: 5.385 min Scan# 705
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03

Tgt Ion:113 Resp: 58433
 Ion Ratio Lower Upper
 113 100
 111 101.9 81.8 122.6
 192 17.5 14.3 21.5

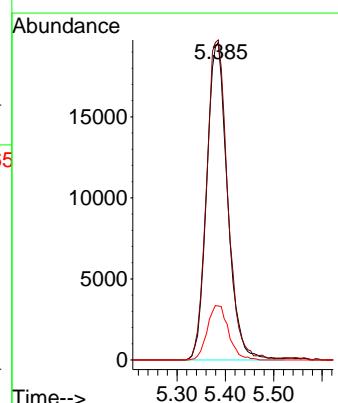


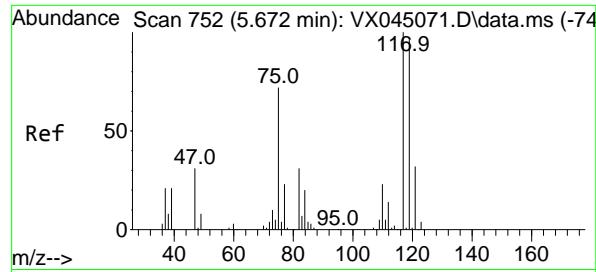




#38

Carbon Tetrachloride
Concen: 29.791 ug/l
RT: 5.672 min Scan# 7
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03


Instrument :
MSVOA_X
ClientSampleId :
PT-VOA-WP

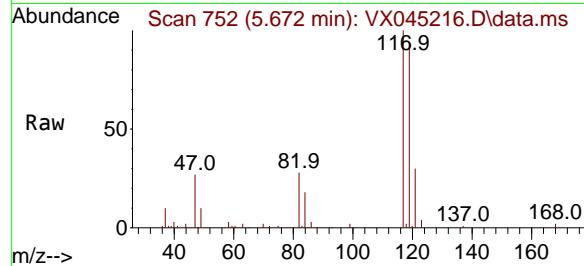



Tgt Ion:117 Resp: 49440
Ion Ratio Lower Upper
117 100
119 93.9 76.7 115.1
121 30.1 25.5 38.3

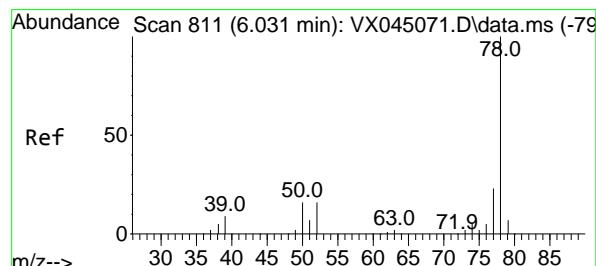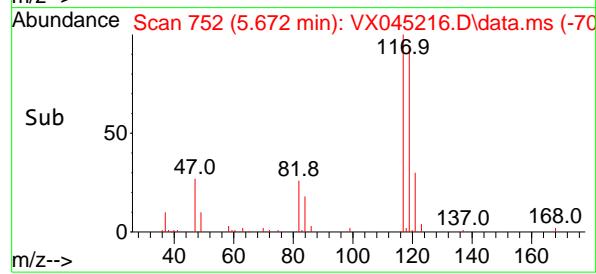


#40
Benzene
Concen: 112.523 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03

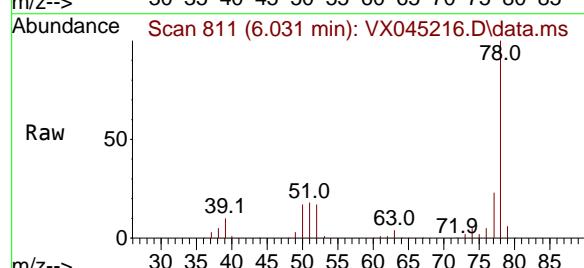


Tgt Ion: 78 Resp: 580824
Ion Ratio Lower Upper
78 100
77 23.1 18.8 28.2



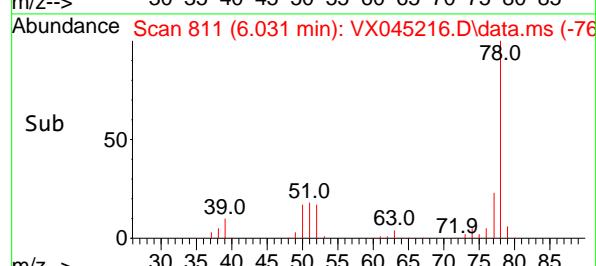





#42
1,2-Dichloroethane
Concen: 35.719 ug/l
RT: 6.080 min Scan# 8
Instrument : MSVOA_X
Delta R.T. 0.000 min
Lab File: VX045216.D
ClientSampleId : PT-VOA-WP
Acq: 11 Mar 2025 12:03





Tgt Ion: 62 Resp: 66393
Ion Ratio Lower Upper
62 100
98 8.4 0.0 18.2




#44
Trichloroethene
Concen: 51.910 ug/l
RT: 7.123 min Scan# 990
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03




Tgt Ion:130 Resp: 62917
Ion Ratio Lower Upper
130 100
95 98.8 0.0 205.0

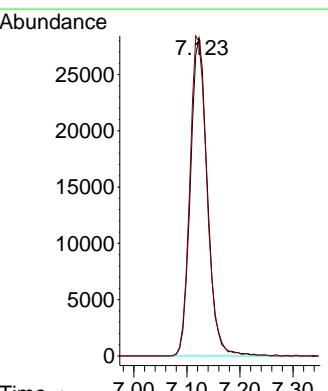






#45
1,2-Dichloropropane
Concen: 77.527 ug/l
RT: 7.428 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03


Instrument : MSVOA_X
ClientSampleId : PT-VOA-WP





Tgt Ion: 63 Resp: 102890
Ion Ratio Lower Upper
63 100
65 31.9 24.7 37.1




#46
Dibromomethane
Concen: 101.245 ug/l
RT: 7.580 min Scan# 1065
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03




Tgt Ion: 93 Resp: 94973
Ion Ratio Lower Upper
93 100
95 82.9 65.8 98.8
174 87.3 72.2 108.2







#47
Bromodichloromethane
Concen: 16.173 ug/l
RT: 7.824 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03

Instrument : MSVOA_X
ClientSampleId : PT-VOA-WP





Tgt Ion: 83 Resp: 29757
Ion Ratio Lower Upper
83 100
85 65.7 51.1 76.7
127 6.5 6.4 9.6




#50
Toluene-d8
Concen: 48.948 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03

Tgt Ion: 98 Resp: 211517
Ion Ratio Lower Upper
98 100
100 64.6 52.0 78.0

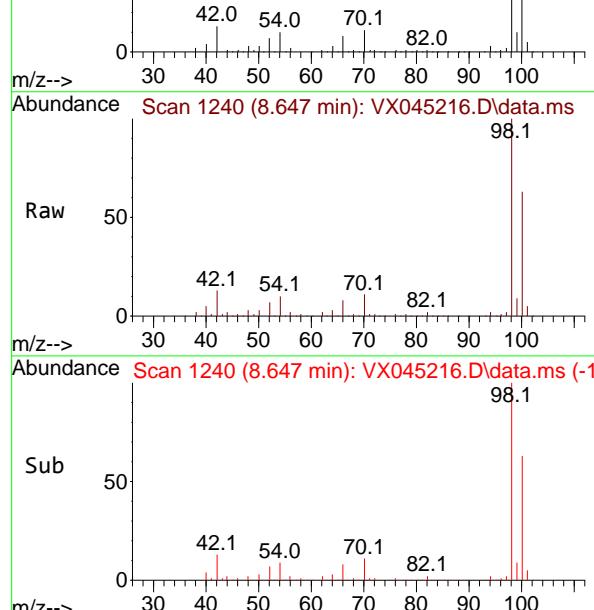


Abundance Scan 1240 (8.647 min): VX045216.D\data.ms (-1)




Abundance Scan 1240 (8.647 min): VX045216.D\data.ms (-1)




#51
4-Methyl-2-Pentanone
Concen: 121.958 ug/l
RT: 8.574 min Scan# 1
Instrument : MSVOA_X
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03
ClientSampleId : PT-VOA-WP





Tgt Ion: 43 Resp: 255054
Ion Ratio Lower Upper
43 100
58 36.2 29.2 43.8

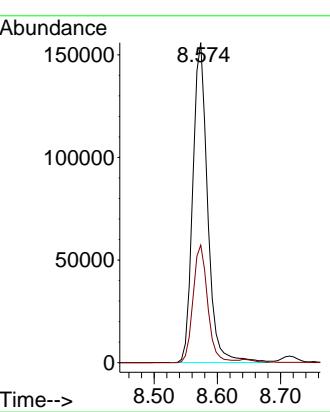


#52
Toluene
Concen: 105.734 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03




Tgt Ion: 92 Resp: 320220
Ion Ratio Lower Upper
92 100
91 173.9 138.9 208.3


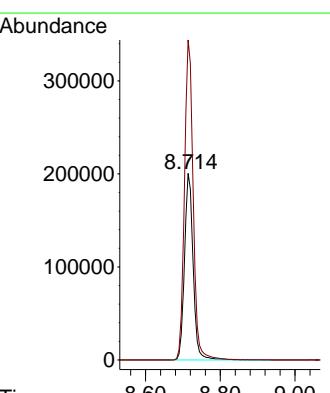
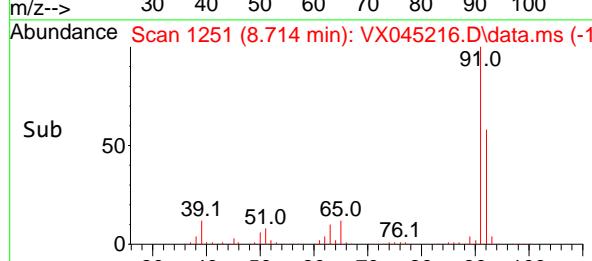





#53
t-1,3-Dichloropropene
Concen: 85.056 ug/l
RT: 8.976 min Scan# 1
Instrument: MSVOA_X
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03
ClientSampleId : PT-VOA-WP

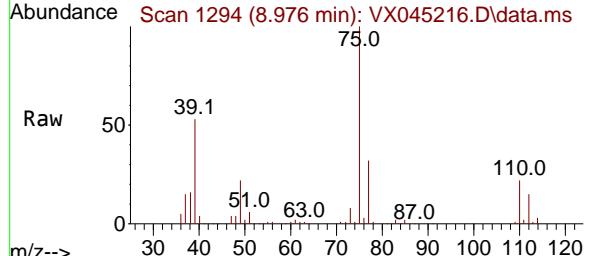



Tgt Ion: 75 Resp: 130835
Ion Ratio Lower Upper
75 100
77 31.5 26.5 39.7

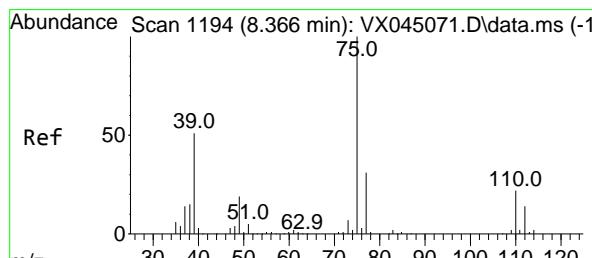


#54
cis-1,3-Dichloropropene
Concen: 61.652 ug/l
RT: 8.360 min Scan# 1193
Delta R.T. -0.006 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03

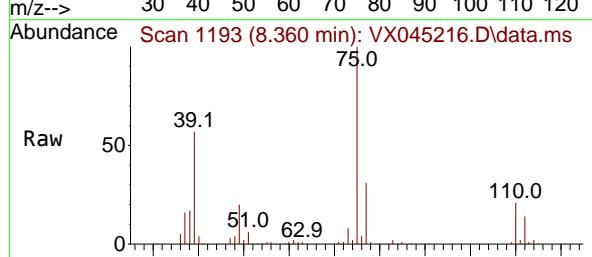


Tgt Ion: 75 Resp: 110586
Ion Ratio Lower Upper
75 100
77 30.6 24.7 37.1
39 56.8 40.7 61.1









#59
2-Hexanone
Concen: 136.734 ug/l
RT: 9.427 min Scan# 1
Instrument : MSVOA_X
Delta R.T. 0.000 min
Lab File: VX045216.D
ClientSampleId : PT-VOA-WP
Acq: 11 Mar 2025 12:03





Tgt Ion: 43 Resp: 207188
Ion Ratio Lower Upper
43 100
58 51.7 25.9 77.6

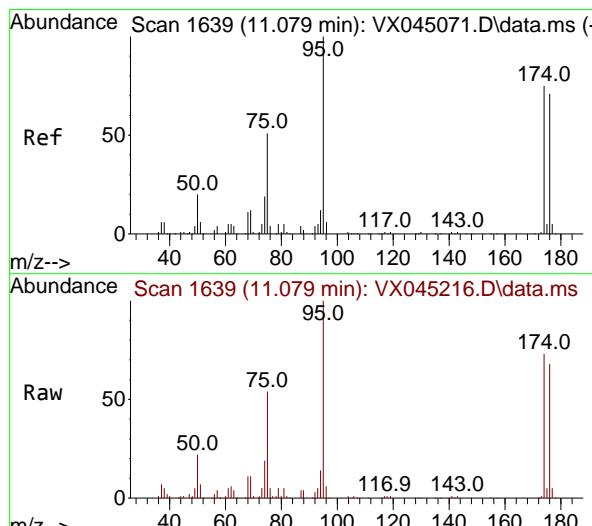


#62
4-Bromofluorobenzene
Concen: 49.138 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03



Tgt Ion: 95 Resp: 70362
Ion Ratio Lower Upper
95 100
174 71.2 0.0 148.2
176 68.4 0.0 141.4





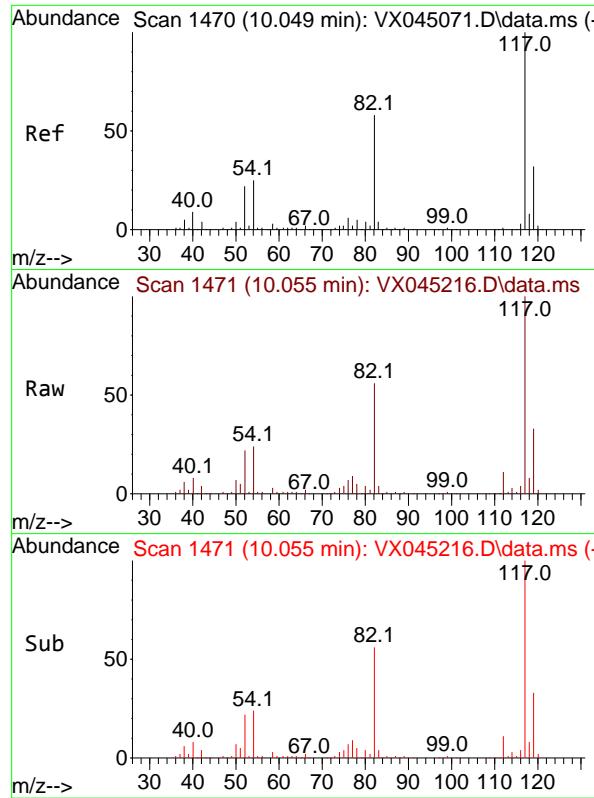

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 10.055 min Scan# 1470
 Delta R.T. 0.006 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03


Instrument : MSVOA_X
 ClientSampleId : PT-VOA-WP


Tgt Ion:117 Resp: 158768
 Ion Ratio Lower Upper
 117 100
 82 55.5 46.3 69.5
 119 32.7 25.7 38.5

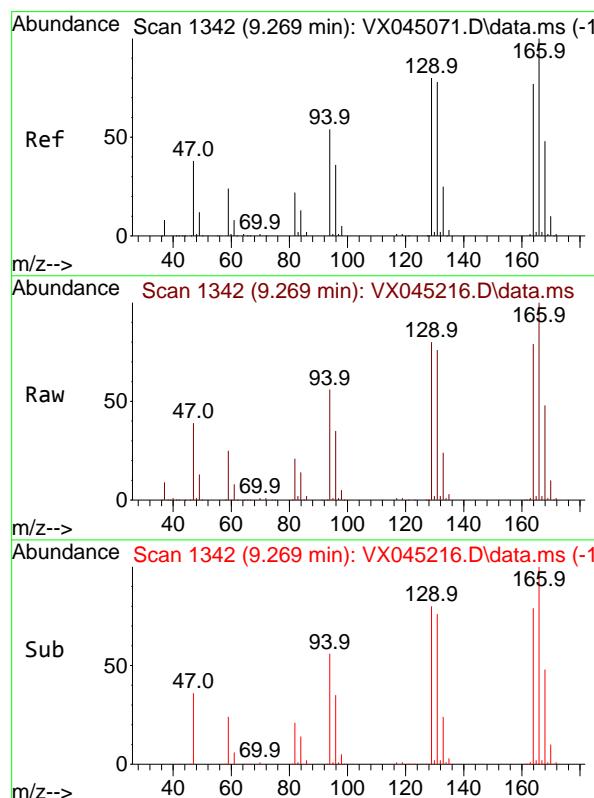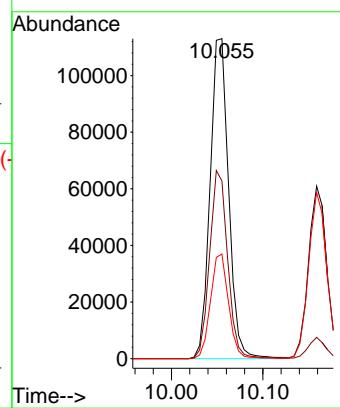

#64
 Tetrachloroethene
 Concen: 115.207 ug/l
 RT: 9.269 min Scan# 1342
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03

Tgt Ion:164 Resp: 117148
 Ion Ratio Lower Upper
 164 100
 166 127.0 103.6 155.4
 129 102.0 82.7 124.1
 131 97.0 80.5 120.7


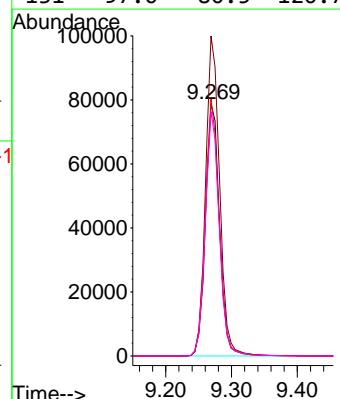


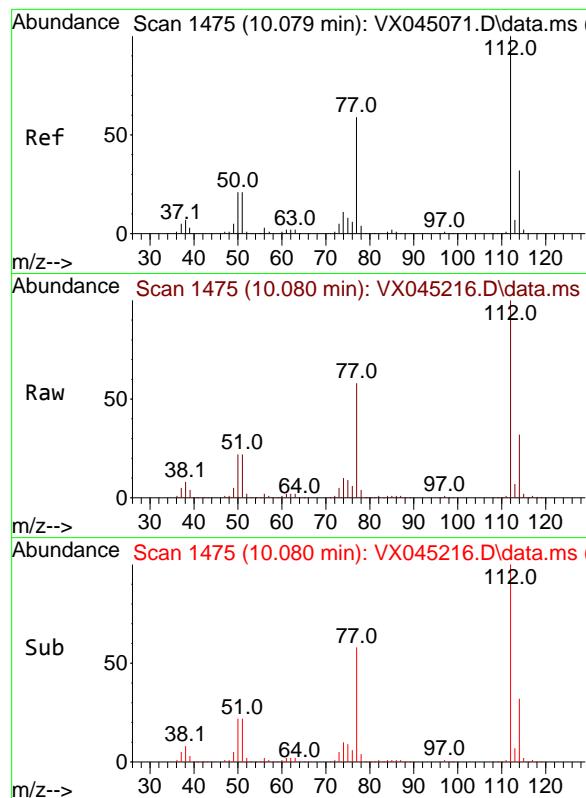

#65
 Chlorobenzene
 Concen: 112.799 ug/l
 RT: 10.080 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03


Instrument : MSVOA_X
 ClientSampleId : PT-VOA-WP


Tgt Ion:112 Resp: 378949
 Ion Ratio Lower Upper
 112 100
 114 31.8 26.0 39.0

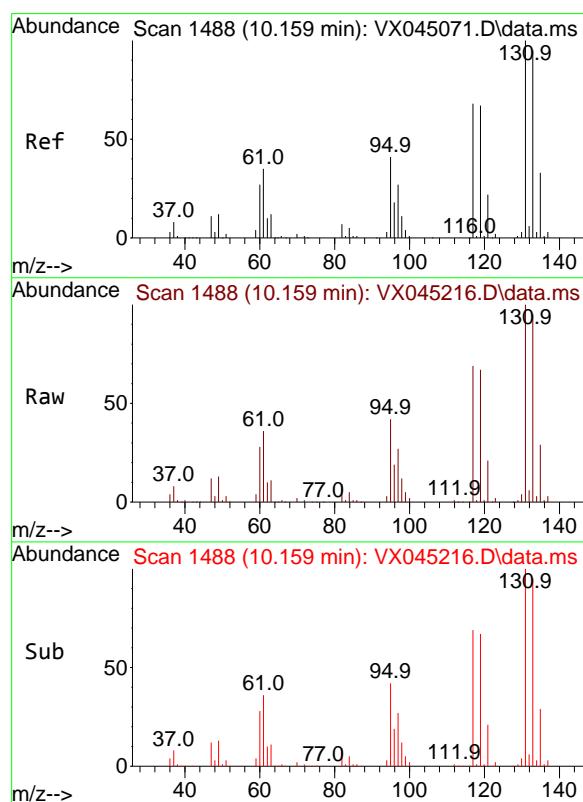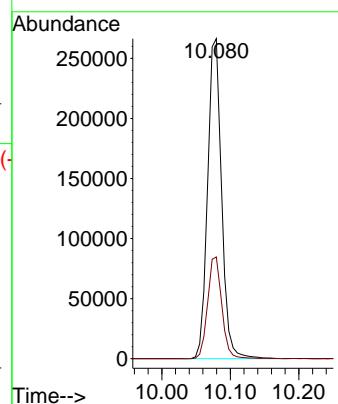

#66
 1,1,1,2-Tetrachloroethane
 Concen: 107.091 ug/l
 RT: 10.159 min Scan# 1488
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03


Tgt Ion:131 Resp: 119812
 Ion Ratio Lower Upper
 131 100
 133 95.3 48.6 145.9
 119 67.3 33.9 101.7

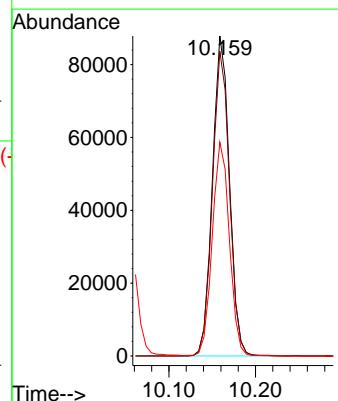





#67
 Ethyl Benzene
 Concen: 35.365 ug/l
 RT: 10.189 min Scan# 1493
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03


Instrument : MSVOA_X
 ClientSampleId : PT-VOA-WP

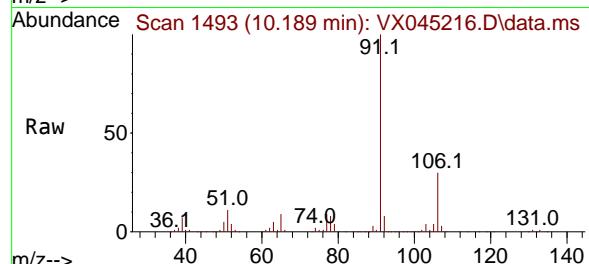


Tgt Ion: 91 Resp: 207014
 Ion Ratio Lower Upper
 91 100
 106 30.0 23.9 35.9

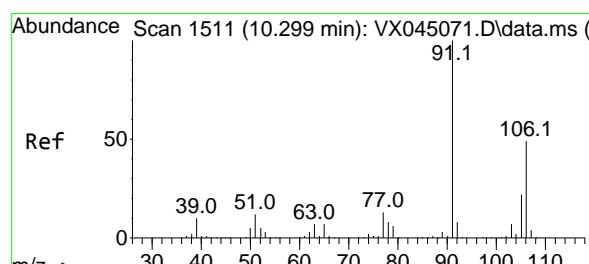


#68
 m/p-Xylenes
 Concen: 72.639 ug/l
 RT: 10.299 min Scan# 1511
 Delta R.T. 0.000 min
 Lab File: VX045216.D
 Acq: 11 Mar 2025 12:03

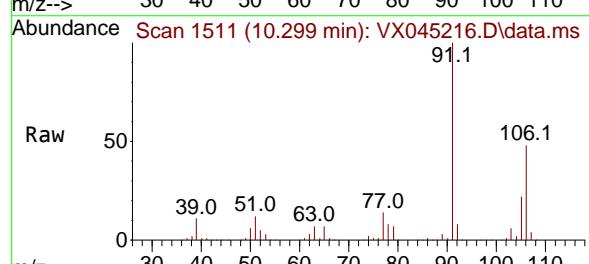



Tgt Ion: 106 Resp: 155658
 Ion Ratio Lower Upper
 106 100
 91 208.7 165.4 248.0



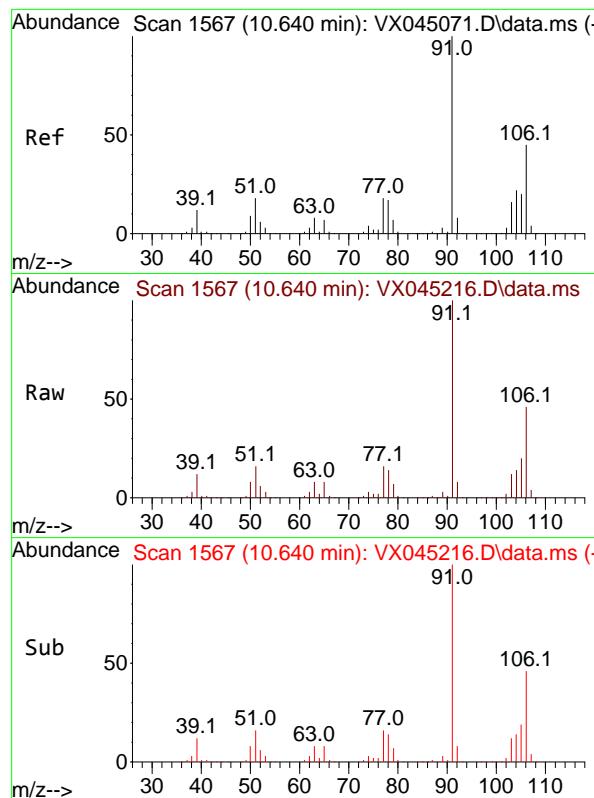


#69
o-Xylene
Concen: 140.973 ug/l
RT: 10.640 min Scan# 1
Instrument : MSVOA_X
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03
ClientSampleId : PT-VOA-WP


Tgt Ion:106 Resp: 304677
Ion Ratio Lower Upper
106 100
91 222.5 109.9 329.6

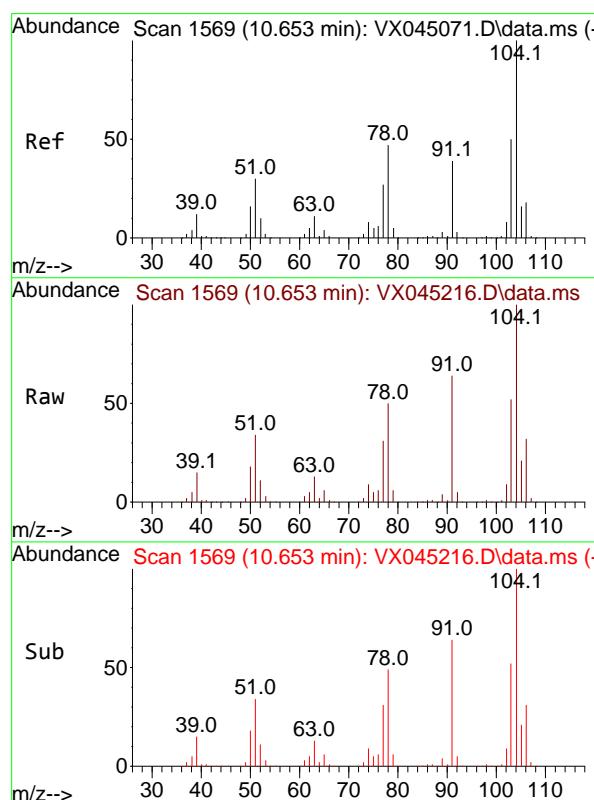

#70
Styrene
Concen: 89.554 ug/l
RT: 10.653 min Scan# 1569
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03



Tgt Ion:104 Resp: 313173
Ion Ratio Lower Upper
104 100
78 59.2 42.2 63.4
103 59.7 43.8 65.8



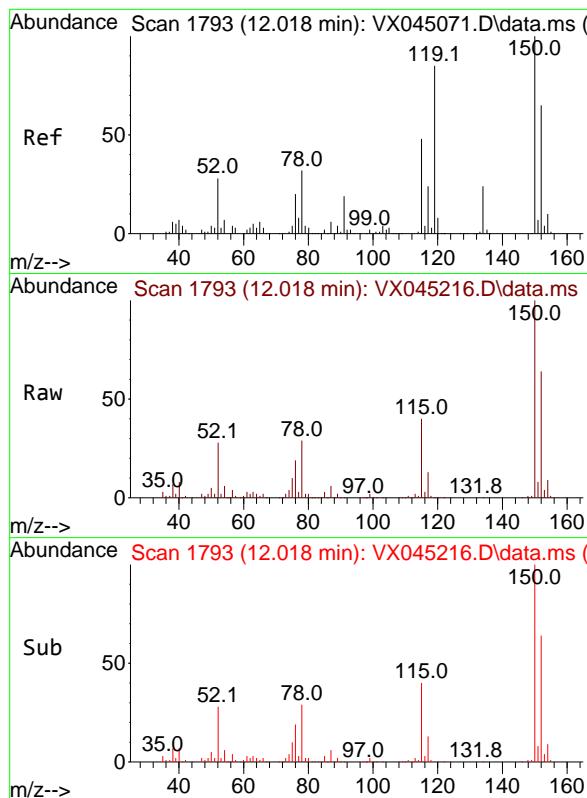


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1
Instrument : MSVOA_X
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03
ClientSampleId : PT-VOA-WP


Tgt Ion:152 Resp: 68042
Ion Ratio Lower Upper
152 100
115 62.8 44.2 132.6
150 156.8 0.0 349.0

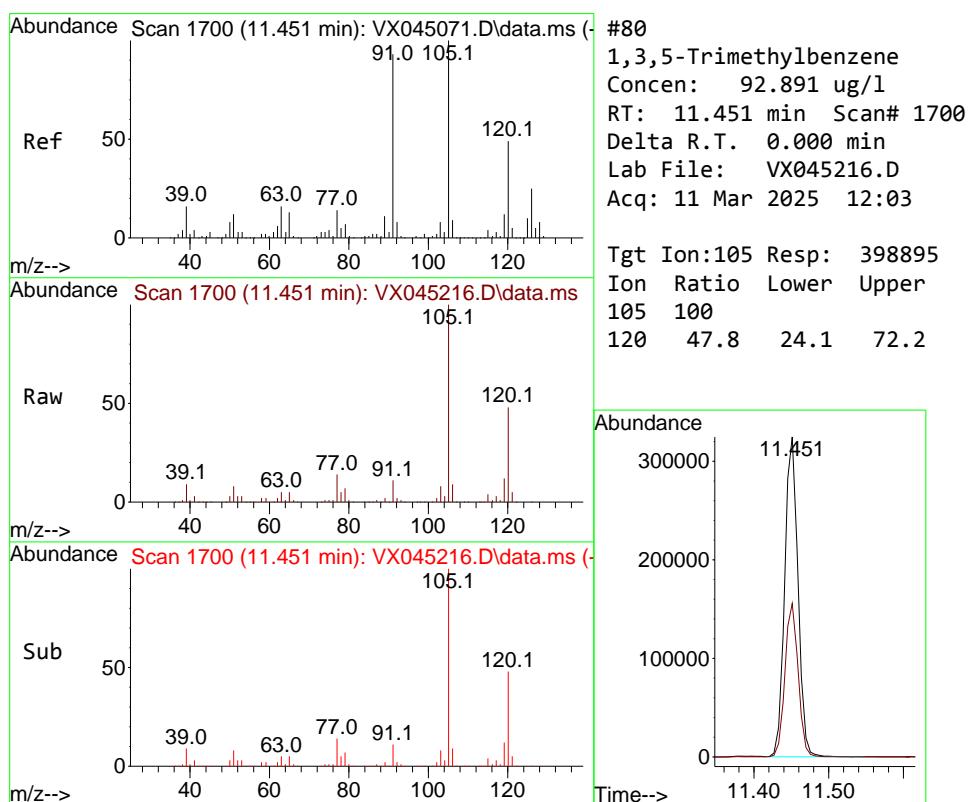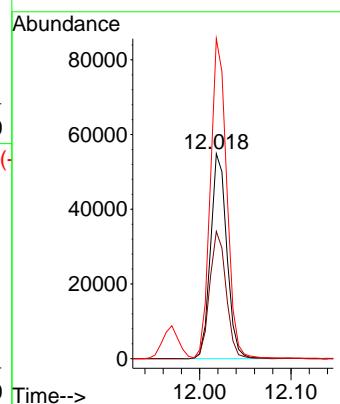

#80
1,3,5-Trimethylbenzene
Concen: 92.891 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03



Tgt Ion:105 Resp: 398895
Ion Ratio Lower Upper
105 100
120 47.8 24.1 72.2

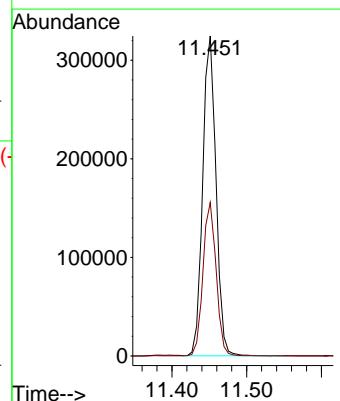

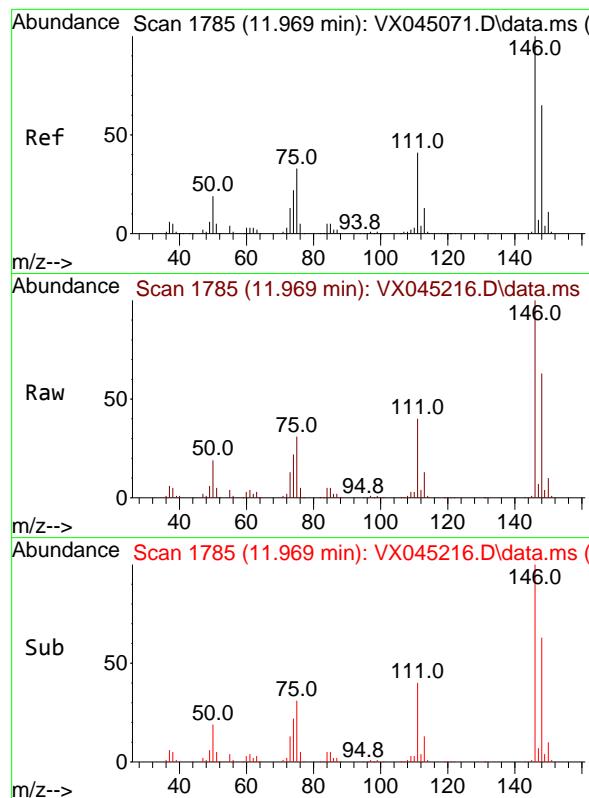


#87
1,3-Dichlorobenzene
Concen: 48.877 ug/l
RT: 11.969 min Scan# 1
Instrument : MSVOA_X
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03
ClientSampleId : PT-VOA-WP


Tgt Ion:146 Resp: 109258
Ion Ratio Lower Upper
146 100
111 42.5 21.1 63.4
148 64.1 31.9 95.7

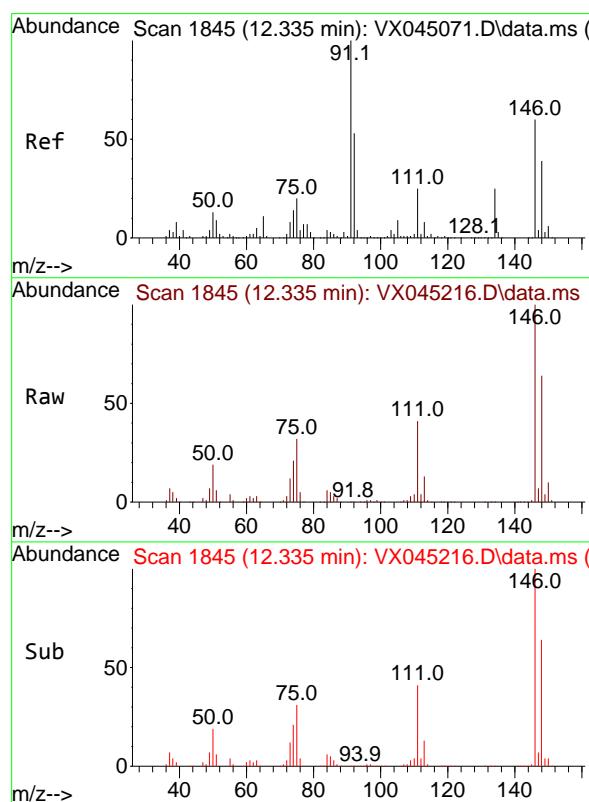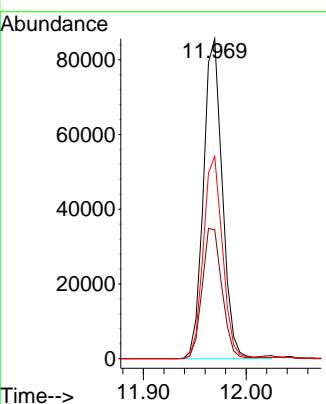

#91
1,2-Dichlorobenzene
Concen: 117.247 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03

Tgt Ion:146 Resp: 262915
Ion Ratio Lower Upper
146 100
111 43.5 21.6 65.0
148 63.3 31.9 95.9

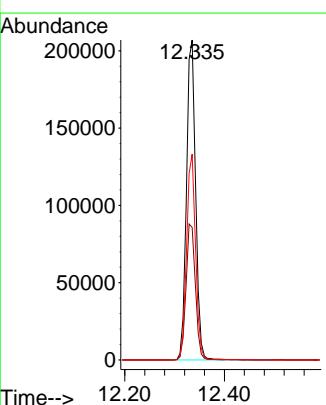


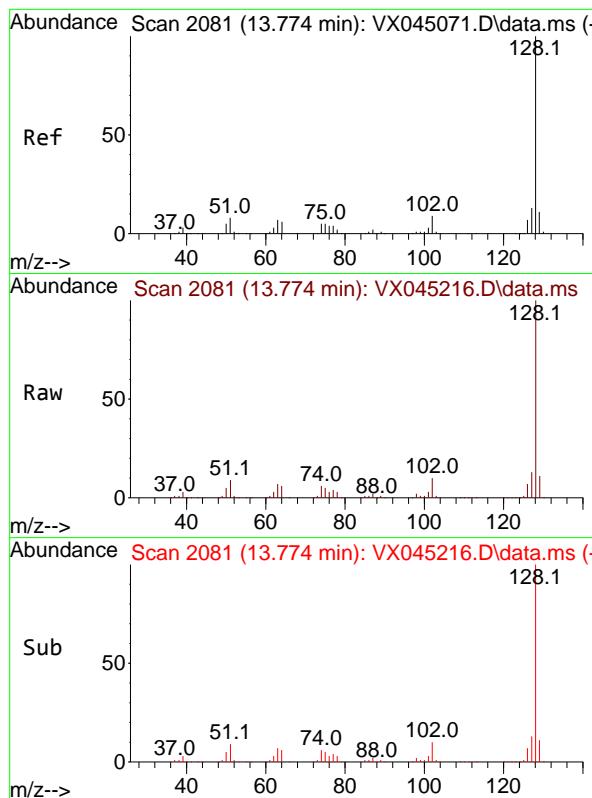

#95
Naphthalene
Concen: 86.479 ug/l
RT: 13.774 min Scan# 2
Delta R.T. 0.000 min
Lab File: VX045216.D
Acq: 11 Mar 2025 12:03

Instrument : MSVOA_X
ClientSampleId : PT-VOA-WP

Tgt Ion:128 Resp: 424244
Ion Ratio Lower Upper
128 100
127 12.8 10.3 15.5
129 11.0 8.7 13.1

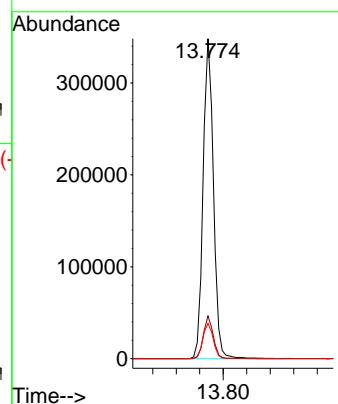



CALIBRATION

SUMMARY

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name:	CHEMTECH	Contract:	ALLI03
Lab Code:	CHEM	Case No.:	Q1502
Instrument ID:	MSVOA_X	Calibration Date(s):	02/28/2025
Heated Purge:	(Y/N) N	Calibration Time(s):	01:27 03:47
GC Column:	DB-624UI	ID:	0.18 (mm)

LAB FILE ID:	RRF001 = VX045068.D	RRF005 = VX045069.D	RRF020 = VX045070.D					
COMPOUND	RRF001	RRF005	RRF020	RRF050	RRF100	RRF150	RRF	% RSD
Dichlorodifluoromethane	0.624	0.646	0.646	0.627	0.626	0.607	0.629	2.4
Chloromethane	0.755	0.821	0.828	0.753	0.721	0.744	0.770	5.7
Vinyl Chloride	0.773	0.755	0.774	0.761	0.765	0.758	0.764	1
Ethyl Acetate	0.589	0.538	0.607	0.606	0.609	0.596	0.591	4.5
Bromomethane		0.337	0.298	0.292	0.284	0.291	0.300	7
Chloroethane	0.373	0.421	0.366	0.373	0.297	0.286	0.352	14.5
Trichlorofluoromethane	0.978	1.061	1.050	1.050	0.982	0.948	1.012	4.7
1,1,2-Trichlorotrifluoroethane	0.526	0.613	0.595	0.594	0.596	0.563	0.581	5.4
1,1-Dichloroethene	0.609	0.620	0.612	0.623	0.620	0.603	0.614	1.3
Acrolein		0.162	0.173	0.174	0.178	0.184	0.174	4.5
Acrylonitrile	0.396	0.398	0.432	0.410	0.387	0.399	0.404	3.9
Acetone	0.414	0.363	0.384	0.351	0.345	0.356	0.369	7
Carbon Disulfide	1.584	1.582	1.587	1.660	1.708	1.698	1.636	3.6
Methyl tert-butyl Ether	1.955	1.913	2.127	2.083	2.132	2.158	2.061	5
Methylene Chloride	0.806	0.730	0.752	0.698	0.694	0.706	0.731	5.8
trans-1,2-Dichloroethene	0.540	0.619	0.603	0.631	0.634	0.616	0.607	5.7
Vinyl Acetate	1.486	1.655	1.961	1.973	2.012	2.049	1.856	12.4
1,1-Dichloroethane	1.200	1.223	1.280	1.242	1.270	1.264	1.247	2.5
2-Butanone	0.476	0.545	0.610	0.579	0.553	0.570	0.555	8.1
Carbon Tetrachloride	0.463	0.463	0.447	0.468	0.489	0.463	0.465	3
2,2-Dichloropropane	0.519	0.562	0.588	0.597	0.617	0.626	0.585	6.7
cis-1,2-Dichloroethene	0.687	0.746	0.765	0.762	0.767	0.769	0.749	4.2
Chloroform	1.206	1.247	1.278	1.246	1.230	1.225	1.239	2
1,1,1-Trichloroethane	0.908	0.992	1.009	1.024	1.044	1.025	1.000	4.8
1,1-Dichloropropene	0.446	0.462	0.444	0.469	0.476	0.455	0.459	2.8
Benzene	1.321	1.459	1.491	1.496	1.497	1.424	1.448	4.7
1,2-Dichloroethane	0.487	0.525	0.545	0.528	0.524	0.520	0.521	3.6
Trichloroethene	0.319	0.351	0.339	0.341	0.354	0.336	0.340	3.7
1,2-Dichloropropane	0.354	0.378	0.382	0.371	0.376	0.373	0.372	2.7
Dibromomethane	0.236	0.265	0.272	0.269	0.269	0.268	0.263	5.1

* Compounds with required minimum RRF and maximum %RSD values.

All other compounds must meet a minimum RRF of 0.010.

RRF of 1,4-Dioxane = Value should be divide by 1000.

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name:	CHEMTECH	Contract:	ALLI03
Lab Code:	CHEM	Case No.:	Q1502
Instrument ID:	MSVOA_X	Calibration Date(s):	02/28/2025
Heated Purge:	(Y/N) N	Calibration Time(s):	01:27 03:47
GC Column:	DB-624UI	ID:	0.18 (mm)

LAB FILE ID:	RRF001 = VX045068.D	RRF005 = VX045069.D	RRF020 = VX045070.D					
COMPOUND	RRF001	RRF005	RRF020	RRF050	RRF100	RRF150	RRF	% RSD
Bromodichloromethane	0.478	0.503	0.536	0.524	0.528	0.528	0.516	4.2
4-Methyl-2-Pentanone	0.535	0.570	0.647	0.610	0.579	0.579	0.587	6.5
Toluene	0.716	0.872	0.892	0.898	0.874	0.845	0.849	8
t-1,3-Dichloropropene	0.304	0.389	0.436	0.469	0.490	0.502	0.431	17.3
cis-1,3-Dichloropropene	0.404	0.463	0.509	0.535	0.555	0.553	0.503	11.8
1,1,2-Trichloroethane	0.346	0.348	0.371	0.356	0.341	0.336	0.350	3.6
1,3-Dichloropropane	0.560	0.623	0.643	0.620	0.597	0.588	0.605	4.9
2-Chloroethyl Vinyl ether	0.218	0.239	0.271	0.284	0.273	0.270	0.259	9.7
2-Hexanone	0.349	0.412	0.476	0.448	0.431	0.436	0.425	10.1
Dibromochloromethane	0.305	0.349	0.390	0.384	0.385	0.380	0.366	9
1,2-Dibromoethane	0.311	0.352	0.371	0.356	0.355	0.350	0.349	5.7
Tetrachloroethene	0.315	0.326	0.319	0.324	0.329	0.309	0.320	2.3
Chlorobenzene	0.968	1.054	1.090	1.092	1.100	1.045	1.058	4.7
1,1,1,2-Tetrachloroethane	0.337	0.331	0.357	0.356	0.372	0.362	0.352	4.4
Ethyl Benzene	1.566	1.794	1.889	1.952	1.972	1.888	1.843	8.1
m/p-Xylenes	0.555	0.672	0.711	0.724	0.715	0.673	0.675	9.3
o-Xylene	0.609	0.689	0.702	0.706	0.707	0.670	0.681	5.5
Styrene	0.879	1.060	1.170	1.181	1.183	1.134	1.101	10.7
Bromoform	0.209	0.234	0.276	0.276	0.300	0.300	0.266	13.9
Isopropylbenzene	3.397	4.034	3.999	4.135	4.006	3.845	3.903	6.8
1,1,2,2-Tetrachloroethane	1.395	1.479	1.513	1.419	1.391	1.396	1.432	3.6
1,2,3-Trichloropropane	1.181	1.201	1.193	1.147	1.131	1.130	1.164	2.7
Bromobenzene	0.899	0.947	0.939	0.939	0.910	0.891	0.921	2.6
n-propylbenzene	3.451	4.375	4.577	4.805	4.696	4.548	4.409	11.1
2-Chlorotoluene	2.788	2.888	2.828	2.869	2.770	2.702	2.808	2.4
1,3,5-Trimethylbenzene	2.611	3.211	3.373	3.384	3.224	3.131	3.156	9
4-Chlorotoluene	2.800	3.015	3.078	3.234	3.140	3.092	3.060	4.8
1,2,4-Trimethylbenzene	2.646	3.202	3.380	3.378	3.258	3.188	3.175	8.6
sec-Butylbenzene	3.000	3.847	4.137	4.215	4.125	3.978	3.884	11.6
p-Isopropyltoluene	2.511	2.986	3.266	3.424	3.369	3.275	3.139	10.9

* Compounds with required minimum RRF and maximum %RSD values.

All other compounds must meet a minimum RRF of 0.010.

RRF of 1,4-Dioxane = Value should be divide by 1000.

VOLATILE ORGANICS INITIAL CALIBRATION DATA

Lab Name:	CHEMTECH		Contract:	ALLI03			
Lab Code:	CHEM	Case No.:	Q1502		SDG No.:	Q1502	
Instrument ID:	MSVOA_X		Calibration Date(s):	02/28/2025		02/28/2025	
Heated Purge:	(Y/N)	N	Calibration Time(s):	01:27		03:47	
GC Column:	DB-624UI	ID:	0.18	(mm)			

LAB FILE ID:	RRF001 = VX045068.D	RRF005 = VX045069.D	RRF020 = VX045070.D					
COMPOUND	RRF001	RRF005	RRF020	RRF050	RRF100	RRF150	RRF	% RSD
1,3-Dichlorobenzene	1.502	1.652	1.710	1.668	1.675	1.649	1.643	4.4
1,4-Dichlorobenzene	1.605	1.702	1.665	1.687	1.669	1.643	1.662	2.1
n-Butylbenzene	1.905	2.359	2.788	3.013	3.099	3.057	2.703	17.7
1,2-Dichlorobenzene	1.479	1.695	1.735	1.668	1.687	1.622	1.648	5.5
1,2-Dibromo-3-Chloropropane	0.237	0.243	0.285	0.289	0.300	0.320	0.279	11.6
1,2,4-Trichlorobenzene	0.668	0.821	0.978	1.009	1.074	1.080	0.938	17.3
Hexachlorobutadiene	0.356	0.369	0.390	0.392	0.406	0.395	0.385	4.8
Naphthalene	2.573	3.115	3.866	3.902	4.091	4.082	3.605	17.2
1,2,3-Trichlorobenzene	0.747	0.897	1.032	1.059	1.107	1.096	0.990	14.2
1,2-Dichloroethane-d4		0.836	0.784	0.757	0.783	0.817	0.795	3.9
Dibromofluoromethane		0.329	0.335	0.329	0.340	0.338	0.334	1.5
Toluene-d8		1.237	1.191	1.210	1.219	1.203	1.212	1.4
4-Bromofluorobenzene		0.383	0.393	0.402	0.410	0.421	0.402	3.7

* Compounds with required minimum RRF and maximum %RSD values.

All other compounds must meet a minimum RRF of 0.010.

RRF of 1,4-Dioxane = Value should be divide by 1000.

Method Path : Z:\voasrv\HPCHEM1\MSVOA_X\Method\

Method File : 82X022825W.M

Title : SW846 8260

Last Update : Fri Feb 28 06:45:16 2025

Response Via : Initial Calibration

Calibration Files

1 =VX045068.D 5 =VX045069.D 20 =VX045070.D 50 =VX045071.D 100 =VX045072.D 150 =VX045073.D

	Compound	1	5	20	50	100	150	Avg	%RSD
<hr/>									
1) I	Pentafluorobenzene	-----	-----	ISTD-----					
2) T	Dichlorodifluo...	0.624	0.646	0.646	0.627	0.626	0.607	0.629	2.38
3) P	Chloromethane	0.755	0.821	0.828	0.753	0.721	0.744	0.770	5.68
4) C	Vinyl Chloride	0.773	0.755	0.774	0.761	0.765	0.758	0.764	1.03#
5) T	Bromomethane	0.337	0.298	0.292	0.284	0.291	0.300	0.300	7.01
6) T	Chloroethane	0.373	0.421	0.366	0.373	0.297	0.286	0.352	14.54
7) T	Trichlorofluor...	0.978	1.061	1.050	1.050	0.982	0.948	1.011	4.73
8) T	Diethyl Ether	0.406	0.402	0.409	0.387	0.387	0.383	0.396	2.83
9) T	1,1,2-Trichlor...	0.526	0.613	0.595	0.594	0.596	0.563	0.581	5.41
10) T	Methyl Iodide	0.607	0.758	0.769	0.758	0.739	0.726	0.726	9.28
11) T	Tert butyl alc...	0.189	0.161	0.134	0.133	0.136	0.151	0.151	16.19
12) CM	1,1-Dichloroet...	0.609	0.620	0.612	0.623	0.620	0.603	0.614	1.27#
13) T	Acrolein	0.162	0.173	0.174	0.178	0.184	0.174	0.174	4.53
14) T	Allyl chloride	1.140	1.047	1.104	1.107	1.091	1.072	1.094	2.92
15) T	Acrylonitrile	0.396	0.398	0.432	0.410	0.387	0.399	0.404	3.90
16) T	Acetone	0.414	0.363	0.384	0.351	0.345	0.356	0.369	7.04
17) T	Carbon Disulfide	1.584	1.582	1.587	1.660	1.708	1.698	1.636	3.62
18) T	Methyl Acetate	0.954	0.835	0.903	0.867	0.869	0.899	0.888	4.59
19) T	Methyl tert-bu...	1.955	1.913	2.127	2.083	2.132	2.158	2.061	4.97
20) T	Methylene Chlo...	0.806	0.730	0.752	0.698	0.694	0.706	0.731	5.84
21) T	trans-1,2-Dich...	0.540	0.619	0.603	0.631	0.634	0.616	0.607	5.73
22) T	Diisopropyl ether	1.959	2.156	2.321	2.291	2.310	2.307	2.224	6.46
23) T	Vinyl Acetate	1.486	1.655	1.961	1.973	2.012	2.049	1.856	12.38
24) P	1,1-Dichloroet...	1.200	1.223	1.280	1.242	1.270	1.264	1.247	2.45
25) T	2-Butanone	0.476	0.545	0.610	0.579	0.553	0.570	0.555	8.09
26) T	2,2-Dichloropr...	0.519	0.562	0.588	0.597	0.617	0.626	0.585	6.74
27) T	cis-1,2-Dichlo...	0.687	0.746	0.765	0.762	0.767	0.769	0.749	4.21
28) T	Bromochloromet...	0.557	0.633	0.613	0.603	0.563	0.596	0.594	4.97
29) T	Tetrahydrofuran	0.362	0.376	0.398	0.373	0.361	0.368	0.373	3.61
30) C	Chloroform	1.206	1.247	1.278	1.246	1.230	1.225	1.239	1.97#
31) T	Cyclohexane	1.021	1.087	1.108	1.142	1.052	1.082	1.082	4.35
32) T	1,1,1-Trichlor...	0.908	0.992	1.009	1.024	1.044	1.025	1.000	4.83
33) S	1,2-Dichloroet...	0.836	0.784	0.757	0.783	0.817	0.795	0.795	3.91
34) I	1,4-Difluorobenzene	-----	-----	ISTD-----					
35) S	Dibromofluorom...	0.329	0.335	0.329	0.340	0.338	0.334	0.334	1.53
36) T	1,1-Dichloropr...	0.446	0.462	0.444	0.469	0.476	0.455	0.459	2.77
37) T	Ethyl Acetate	0.589	0.538	0.607	0.606	0.609	0.596	0.591	4.53
38) T	Carbon Tetrach...	0.463	0.463	0.447	0.468	0.489	0.463	0.465	2.96
39) T	Methylcyclohexane	0.464	0.530	0.560	0.585	0.607	0.550	0.549	9.07
40) TM	Benzene	1.321	1.459	1.491	1.496	1.497	1.424	1.448	4.72
41) T	Methacrylonitrile	0.284	0.293	0.337	0.340	0.332	0.330	0.319	7.59
42) TM	1,2-Dichloroet...	0.487	0.525	0.545	0.528	0.524	0.520	0.521	3.63
43) T	Isopropyl Acetate	0.675	0.800	0.940	0.929	0.935	0.964	0.874	12.98
44) TM	Trichloroethene	0.319	0.351	0.339	0.341	0.354	0.336	0.340	3.72
45) C	1,2-Dichloropr...	0.354	0.378	0.382	0.371	0.376	0.373	0.372	2.68#
46) T	Dibromomethane	0.236	0.265	0.272	0.269	0.269	0.268	0.263	5.10
47) T	Bromodichlorom...	0.478	0.503	0.536	0.524	0.528	0.528	0.516	4.23
48) T	Methyl methacr...	0.352	0.422	0.460	0.463	0.458	0.475	0.438	10.46
49) T	1,4-Dioxane	0.008	0.009	0.010	0.009	0.009	0.009	0.009	6.46
50) S	Toluene-d8	1.237	1.191	1.210	1.219	1.203	1.212	1.212	1.43
51) T	4-Methyl-2-Pen...	0.535	0.570	0.647	0.610	0.579	0.579	0.587	6.52
52) CM	Toluene	0.716	0.872	0.892	0.898	0.874	0.845	0.849	8.03#
53) T	t-1,3-Dichloro...	0.304	0.389	0.436	0.469	0.490	0.502	0.431	17.30
54) T	cis-1,3-Dichlo...	0.404	0.463	0.509	0.535	0.555	0.553	0.503	11.80
55) T	1,1,2-Trichlor...	0.346	0.348	0.371	0.356	0.341	0.336	0.350	3.63
56) T	Ethyl methacry...	0.396	0.500	0.562	0.570	0.577	0.586	0.532	13.74

Method Path : Z:\voasrv\HPCHEM1\MSVOA_X\Method\
 Method File : 82X022825W.M

57) T	1,3-Dichloropr...	0.560	0.623	0.643	0.620	0.597	0.588	0.605	4.90
58) T	2-Chloroethyl ...	0.218	0.239	0.271	0.284	0.273	0.270	0.259	9.71
59) T	2-Hexanone	0.349	0.412	0.476	0.448	0.431	0.436	0.425	10.08
60) T	Dibromochlorom...	0.305	0.349	0.390	0.384	0.385	0.380	0.366	9.01
61) T	1,2-Dibromoethane	0.311	0.352	0.371	0.356	0.355	0.350	0.349	5.73
62) S	4-Bromofluorob...	0.383	0.393	0.402	0.410	0.421	0.402		3.67
63) I	Chlorobenzene-d5	-----ISTD-----							
64) T	Tetrachloroethene	0.315	0.326	0.319	0.324	0.329	0.309	0.320	2.33
65) PM	Chlorobenzene	0.968	1.054	1.090	1.092	1.100	1.045	1.058	4.68
66) T	1,1,1,2-Tetra...	0.337	0.331	0.357	0.356	0.372	0.362	0.352	4.39
67) C	Ethyl Benzene	1.566	1.794	1.889	1.952	1.972	1.888	1.843	8.11#
68) T	m/p-Xylenes	0.555	0.672	0.711	0.724	0.715	0.673	0.675	9.27
69) T	o-Xylene	0.609	0.689	0.702	0.706	0.707	0.670	0.681	5.52
70) T	Styrene	0.879	1.060	1.170	1.181	1.183	1.134	1.101	10.75
71) P	Bromoform	0.209	0.234	0.276	0.276	0.300	0.300	0.266	13.94
72) I	1,4-Dichlorobenzen...	-----ISTD-----							
73) T	Isopropylbenzene	3.397	4.034	3.999	4.135	4.006	3.845	3.903	6.79
74) T	N-amyl acetate	1.349	1.578	1.890	1.977	2.078	2.116	1.831	16.62
75) P	1,1,2,2-Tetra...	1.395	1.479	1.513	1.419	1.391	1.396	1.432	3.60
76) T	1,2,3-Trichlor...	1.181	1.201	1.193	1.147	1.131	1.130	1.164	2.73
77) T	Bromobenzene	0.899	0.947	0.939	0.939	0.910	0.891	0.921	2.57
78) T	n-propylbenzene	3.451	4.375	4.577	4.805	4.696	4.548	4.409	11.14
79) T	2-Chlorotoluene	2.788	2.888	2.828	2.869	2.770	2.702	2.808	2.45
80) T	1,3,5-Trimethyl...	2.611	3.211	3.373	3.384	3.224	3.131	3.156	9.01
81) T	trans-1,4-Dich...	0.268	0.313	0.339	0.376	0.405	0.340		15.78
82) T	4-Chlorotoluene	2.800	3.015	3.078	3.234	3.140	3.092	3.060	4.80
83) T	tert-Butylbenzene	3.029	3.256	3.342	3.375	3.292	3.160	3.242	3.96
84) T	1,2,4-Trimethyl...	2.646	3.202	3.380	3.378	3.258	3.188	3.175	8.57
85) T	sec-Butylbenzene	3.000	3.847	4.137	4.215	4.125	3.978	3.884	11.65
86) T	p-Isopropyltol...	2.511	2.986	3.266	3.424	3.369	3.275	3.139	10.91
87) T	1,3-Dichlorobe...	1.502	1.652	1.710	1.668	1.675	1.649	1.643	4.40
88) T	1,4-Dichlorobe...	1.605	1.702	1.665	1.687	1.669	1.643	1.662	2.06
89) T	n-Butylbenzene	1.905	2.359	2.788	3.013	3.099	3.057	2.703	17.67
90) T	Hexachloroethane	0.470	0.498	0.568	0.605	0.633	0.633	0.568	12.30
91) T	1,2-Dichlorobe...	1.479	1.695	1.735	1.668	1.687	1.622	1.648	5.50
92) T	1,2-Dibromo-3...	0.237	0.243	0.285	0.289	0.300	0.320	0.279	11.64
93) T	1,2,4-Trichlor...	0.668	0.821	0.978	1.009	1.074	1.080	0.938	17.32
94) T	Hexachlorobuta...	0.356	0.369	0.390	0.392	0.406	0.395	0.385	4.77
95) T	Naphthalene	2.573	3.115	3.866	3.902	4.091	4.082	3.605	17.21
96) T	1,2,3-Trichlor...	0.747	0.897	1.032	1.059	1.107	1.096	0.990	14.23

(#) = Out of Range

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045068.D
 Acq On : 28 Feb 2025 01:27
 Operator : JC/MD
 Sample : VSTDICC001
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001

Quant Time: Feb 28 06:28:57 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:18:23 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.550	168	102761	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	188642	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	159886	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	64845	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.000	65	0d	0.000	ug/l	
Spiked Amount 50.000	Range 74 - 125		Recovery	=	0.000%#	
35) Dibromofluoromethane	0.000	113	0d	0.000	ug/l	
Spiked Amount 50.000	Range 75 - 124		Recovery	=	0.000%#	
50) Toluene-d8	0.000	98	0d	0.000	ug/l	
Spiked Amount 50.000	Range 86 - 113		Recovery	=	0.000%#	
62) 4-Bromofluorobenzene	0.000	95	0d	0.000	ug/l	
Spiked Amount 50.000	Range 77 - 121		Recovery	=	0.000%#	
Target Compounds						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	1282	1.007	ug/l	90
3) Chloromethane	1.301	50	1552	0.975	ug/l	91
4) Vinyl Chloride	1.368	62	1588	1.008	ug/l #	85
6) Chloroethane	1.673	64	766m	0.992	ug/l	
7) Trichlorofluoromethane	1.880	101	2011	0.957	ug/l	97
8) Diethyl Ether	2.130	74	835	1.045	ug/l	80
9) 1,1,2-Trichlorotrifluo...	2.319	101	1081	0.884	ug/l	87
12) 1,1-Dichloroethene	2.313	96	1251	0.991	ug/l	92
14) Allyl chloride	2.660	41	2343	1.055	ug/l	93
15) Acrylonitrile	3.075	53	4067	4.931	ug/l	99
16) Acetone	2.380	43	4259	5.635	ug/l	100
17) Carbon Disulfide	2.502	76	3256	0.956	ug/l #	92
18) Methyl Acetate	2.703	43	1960	1.066	ug/l	93
19) Methyl tert-butyl Ether	3.111	73	4017	0.943	ug/l	91
20) Methylene Chloride	2.782	84	1656	1.095	ug/l	98
21) trans-1,2-Dichloroethene	3.093	96	1109	0.869	ug/l	91
22) Diisopropyl ether	3.764	45	4026	0.871	ug/l #	80
23) Vinyl Acetate	3.727	43	15271	3.971	ug/l	97
24) 1,1-Dichloroethane	3.605	63	2467	0.958	ug/l #	83
25) 2-Butanone	4.587	43	4894	4.252	ug/l	96
26) 2,2-Dichloropropane	4.471	77	1066	0.872	ug/l #	56
27) cis-1,2-Dichloroethene	4.501	96	1412	0.902	ug/l #	19
28) Bromochloromethane	4.885	49	1144	0.958	ug/l #	54
29) Tetrahydrofuran	5.032	42	3719	4.809	ug/l #	34
30) Chloroform	5.093	83	2478	0.978	ug/l	92
32) 1,1,1-Trichloroethane	5.373	97	1867	0.893	ug/l #	52
36) 1,1-Dichloropropene	5.690	75	1681	0.967	ug/l #	84
37) Ethyl Acetate	4.739	43	2223m	0.988	ug/l	
38) Carbon Tetrachloride	5.672	117	1747m	0.987	ug/l	
39) Methylcyclohexane	7.385	83	1750	0.831	ug/l	88
40) Benzene	6.031	78	4984	0.907	ug/l	99
41) Methacrylonitrile	4.958	41	1072m	0.879	ug/l	
42) 1,2-Dichloroethane	6.099	62	1837	0.924	ug/l	78
43) Isopropyl Acetate	6.355	43	2545	0.767	ug/l #	95
44) Trichloroethene	7.129	130	1202	0.933	ug/l	65
45) 1,2-Dichloropropane	7.434	63	1334	0.971	ug/l #	82

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045068.D
 Acq On : 28 Feb 2025 01:27
 Operator : JC/MD
 Sample : VSTDICC001
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001

Quant Time: Feb 28 06:28:57 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:18:23 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) Dibromomethane	7.586	93	891	0.897	ug/1	92
47) Bromodichloromethane	7.818	83	1802	0.927	ug/1 #	85
48) Methyl methacrylate	7.714	41	1328m	0.825	ug/1	
49) 1,4-Dioxane	7.684	88	639	18.144	ug/1 #	81
51) 4-Methyl-2-Pentanone	8.574	43	10091	4.567	ug/1	95
52) Toluene	8.720	92	2700	0.841	ug/1	97
53) t-1,3-Dichloropropene	8.994	75	1147	0.700	ug/1 #	85
54) cis-1,3-Dichloropropene	8.373	75	1525	0.804	ug/1 #	90
55) 1,1,2-Trichloroethane	9.153	97	1306	1.004	ug/1 #	90
56) Ethyl methacrylate	9.135	69	1494	0.748	ug/1 #	93
57) 1,3-Dichloropropane	9.311	76	2112	0.920	ug/1	97
58) 2-Chloroethyl Vinyl ether	8.251	63	4115	4.320	ug/1	95
59) 2-Hexanone	9.439	43	6582	4.153	ug/1	96
60) Dibromochloromethane	9.519	129	1152	0.835	ug/1	98
61) 1,2-Dibromoethane	9.610	107	1174	0.890	ug/1	97
64) Tetrachloroethene	9.275	164	1006	0.986	ug/1 #	88
65) Chlorobenzene	10.080	112	3094	0.908	ug/1	90
66) 1,1,1,2-Tetrachloroethane	10.159	131	1078	0.978	ug/1 #	65
67) Ethyl Benzene	10.195	91	5008	0.846	ug/1 #	85
68) m/p-Xylenes	10.305	106	3552	1.630	ug/1	97
69) o-Xylene	10.640	106	1949	0.891	ug/1	95
70) Styrene	10.665	104	2810	0.802	ug/1	97
71) Bromoform	10.799	173	667	0.768	ug/1 #	92
73) Isopropylbenzene	10.964	105	4405	0.858	ug/1	96
74) N-amyl acetate	10.854	43	1750	0.732	ug/1 #	87
75) 1,1,2,2-Tetrachloroethane	11.213	83	1809	0.954	ug/1	88
76) 1,2,3-Trichloropropane	11.244	75	1531m	1.015	ug/1	
77) Bromobenzene	11.201	156	1166	0.972	ug/1	91
78) n-propylbenzene	11.305	91	4475	0.773	ug/1	97
79) 2-Chlorotoluene	11.366	91	3616	0.986	ug/1	98
80) 1,3,5-Trimethylbenzene	11.451	105	3386	0.815	ug/1	94
82) 4-Chlorotoluene	11.457	91	3631	0.904	ug/1	99
83) tert-Butylbenzene	11.713	119	3928	0.929	ug/1	96
84) 1,2,4-Trimethylbenzene	11.756	105	3432	0.827	ug/1	95
85) sec-Butylbenzene	11.890	105	3891	0.752	ug/1	100
86) p-Isopropyltoluene	12.012	119	3257	0.797	ug/1	94
87) 1,3-Dichlorobenzene	11.976	146	1948	0.913	ug/1	96
88) 1,4-Dichlorobenzene	12.043	146	2082m	0.962	ug/1	
89) n-Butylbenzene	12.335	91	2470	0.691	ug/1	93
90) Hexachloroethane	12.536	117	609	0.805	ug/1	94
91) 1,2-Dichlorobenzene	12.335	146	1918	0.890	ug/1	98
92) 1,2-Dibromo-3-Chloropr...	12.945	75	308	0.859	ug/1	82
93) 1,2,4-Trichlorobenzene	13.591	180	866	0.706	ug/1	93
94) Hexachlorobutadiene	13.725	225	462	0.917	ug/1	94
95) Naphthalene	13.780	128	3337	0.707	ug/1 #	94
96) 1,2,3-Trichlorobenzene	13.963	180	969	0.759	ug/1	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045068.D
Acq On : 28 Feb 2025 01:27
Operator : JC/MD
Sample : VSTDIICC001
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

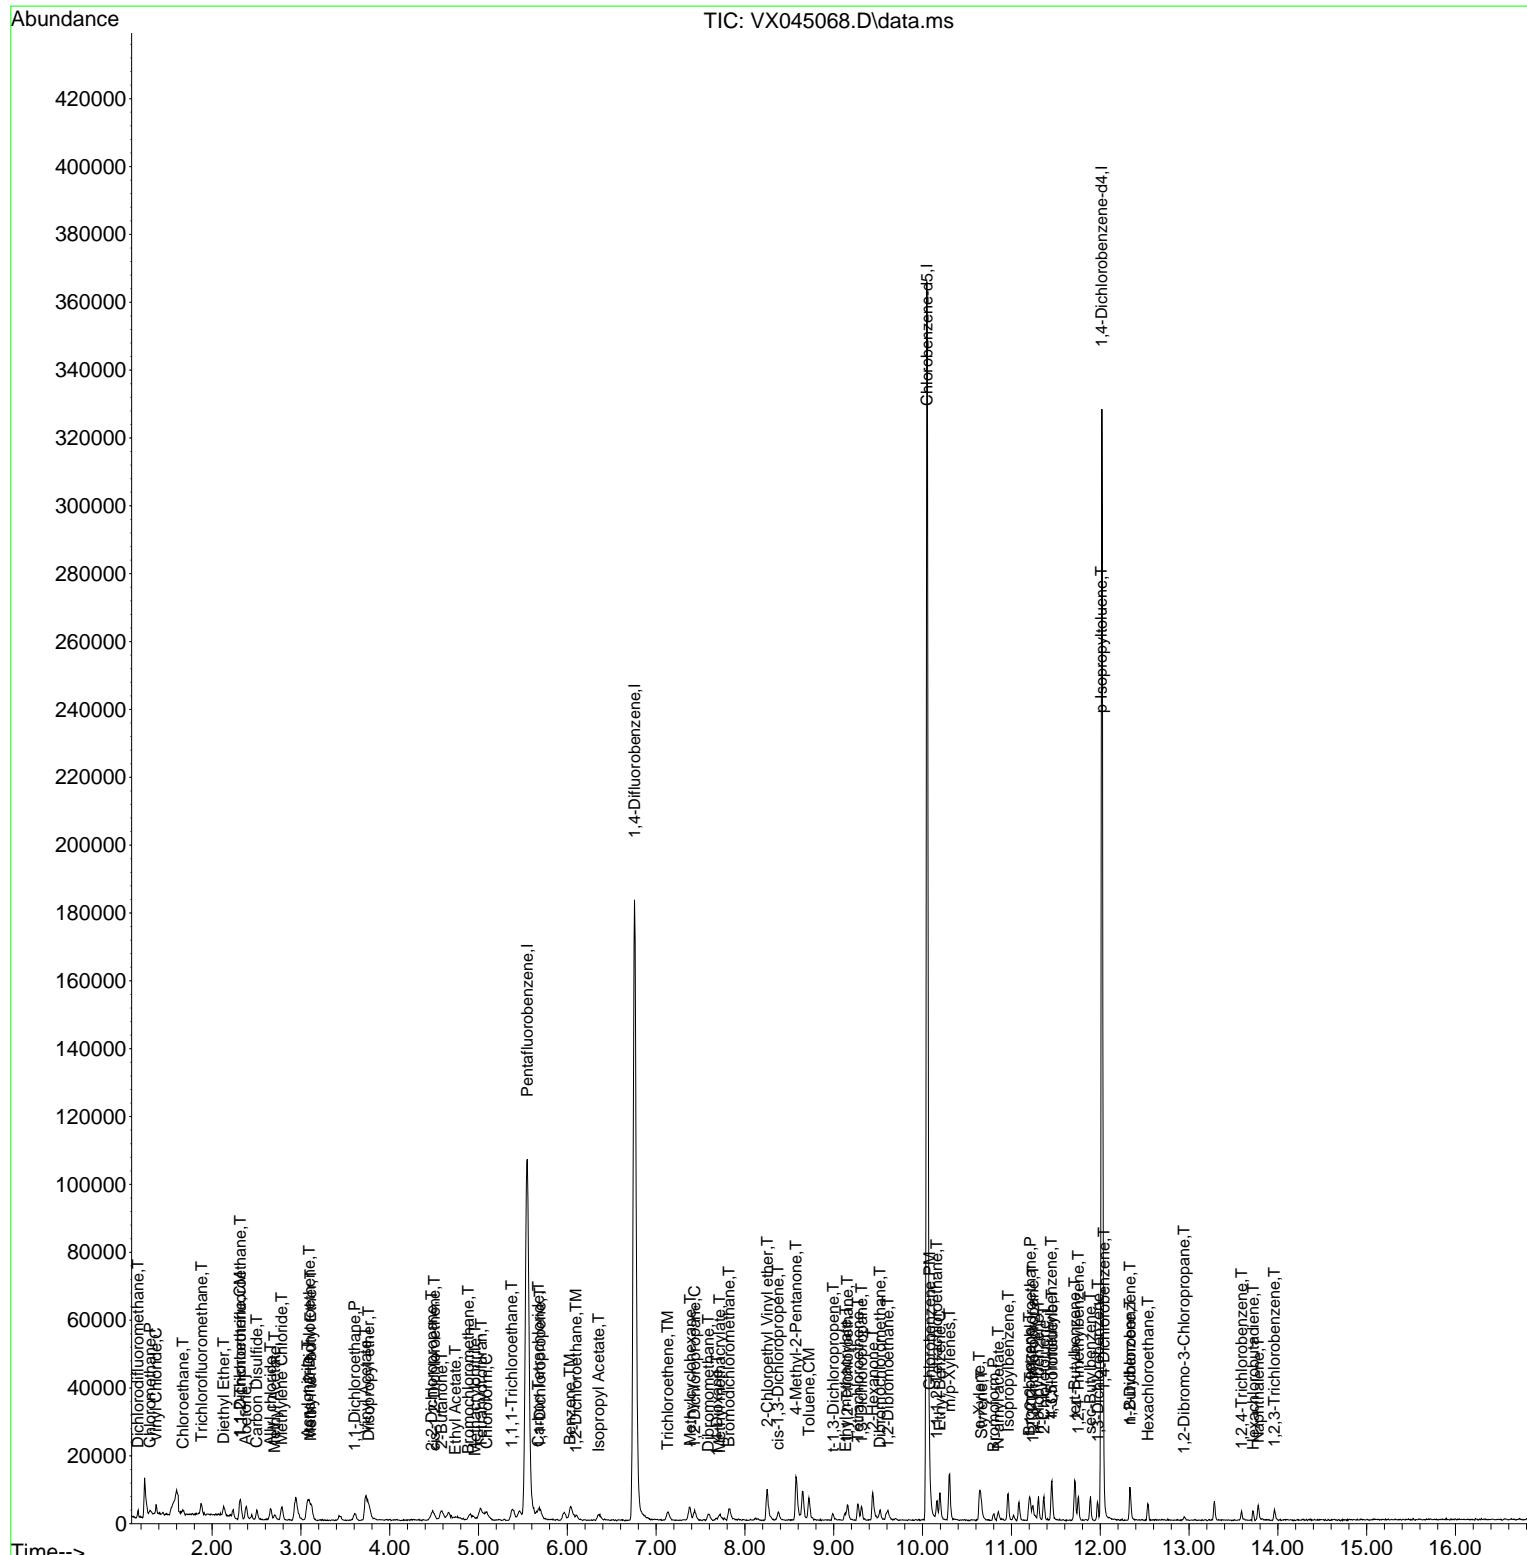



#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.550 min Scan# 7
 Delta R.T. -0.000 min
 Lab File: VX045068.D
 Acq: 28 Feb 2025 01:27



Instrument : MSVOA_X
 ClientSampleId : VSTDICC001




Tgt Ion:168 Resp: 10276
 Ion Ratio Lower Upper
 168 100
 99 59.9 48.2 72.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025




#2
 Dichlorodifluoromethane
 Concen: 1.007 ug/l
 RT: 1.166 min Scan# 13
 Delta R.T. 0.000 min
 Lab File: VX045068.D
 Acq: 28 Feb 2025 01:27




Tgt Ion: 85 Resp: 1282
 Ion Ratio Lower Upper
 85 100
 87 29.2 17.4 52.3





#3
Chloromethane
Concen: 0.975 ug/l
RT: 1.301 min Scan# 3
Delta R.T. -0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001

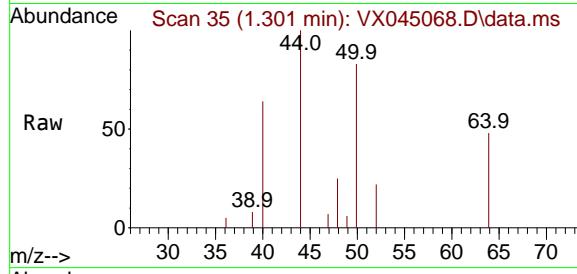


Tgt Ion: 50 Resp: 155:
Ion Ratio Lower Upper
50 100
52 26.3 25.0 37.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

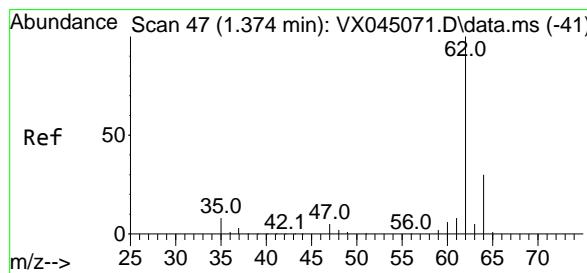


#4
Vinyl Chloride
Concen: 1.008 ug/l
RT: 1.368 min Scan# 46
Delta R.T. -0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

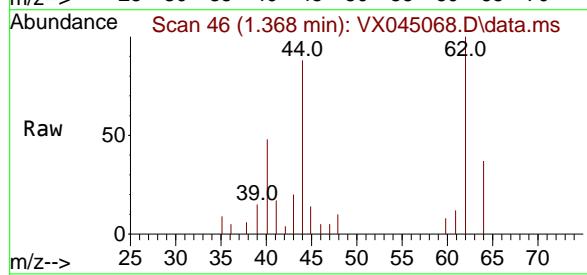


Tgt Ion: 62 Resp: 1588
Ion Ratio Lower Upper
62 100
64 22.0 24.3 36.5#

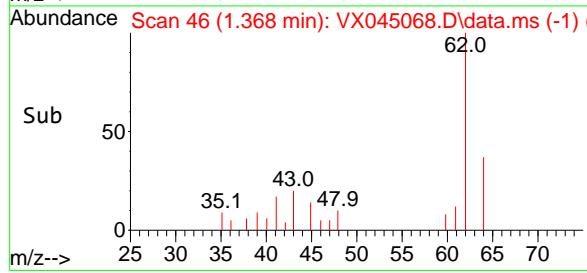

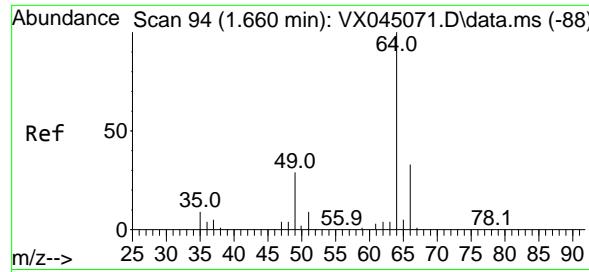

#6
Chloroethane
Concen: 0.992 ug/l m
RT: 1.673 min Scan# 9
Delta R.T. 0.012 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001




Tgt Ion: 64 Resp: 760
Ion Ratio Lower Upper
64 100
66 43.7 26.7 40.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

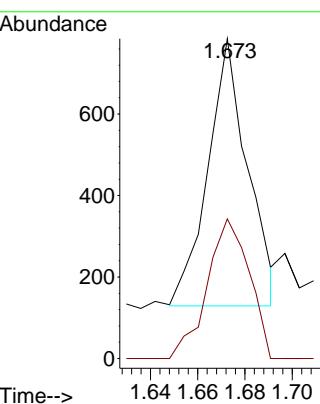


#7
Trichlorofluoromethane
Concen: 0.957 ug/l
RT: 1.880 min Scan# 130
Delta R.T. 0.012 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Tgt Ion:101 Resp: 2011
Ion Ratio Lower Upper
101 100
103 67.8 52.1 78.1

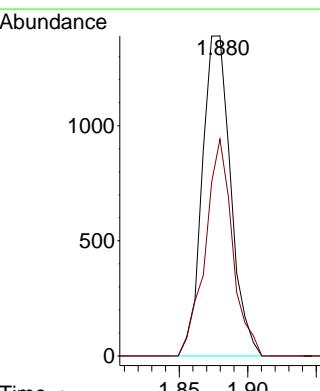



#8
Diethyl Ether
Concen: 1.045 ug/l
RT: 2.130 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001




Tgt Ion: 74 Resp: 839
Ion Ratio Lower Upper
74 100
45 123.5 51.5 154.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

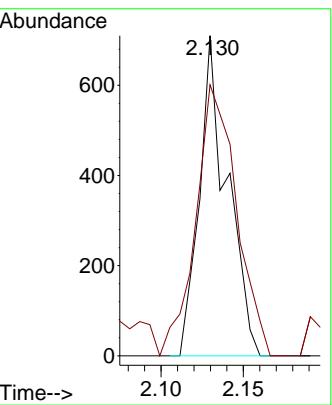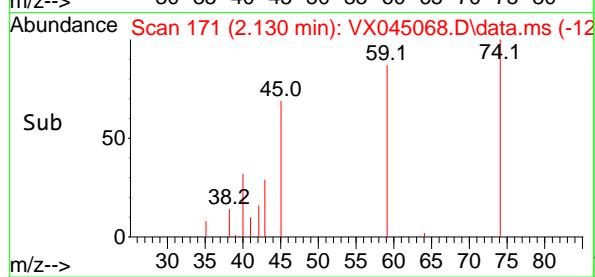


#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.884 ug/l
RT: 2.319 min Scan# 202
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Tgt Ion:101 Resp: 1081
Ion Ratio Lower Upper
101 100
85 53.7 36.2 54.4
151 81.9 56.4 84.6

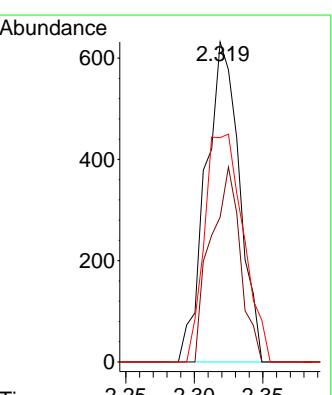



#12
1,1-Dichloroethene
Concen: 0.991 ug/l
RT: 2.313 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001




Tgt Ion: 96 Resp: 125:
Ion Ratio Lower Upper
96 100
61 157.4 134.6 202.0
98 70.0 51.0 76.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#14
Allyl chloride
Concen: 1.055 ug/l
RT: 2.660 min Scan# 258
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Tgt Ion: 41 Resp: 2343
Ion Ratio Lower Upper
41 100
39 62.3 53.8 80.8
76 27.4 25.2 37.8





#15
Acrylonitrile
Concen: 4.931 ug/l
RT: 3.075 min Scan# 31
Delta R.T. 0.012 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Instrument : MSVOA_X
ClientSampleId : VSTDICC001



Tgt Ion: 53 Resp: 4061
Ion Ratio Lower Upper
53 100
52 82.6 66.2 99.2
51 34.6 29.0 43.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#16
Acetone
Concen: 5.635 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27


Tgt Ion: 43 Resp: 4259
Ion Ratio Lower Upper
43 100
58 30.2 24.2 36.4

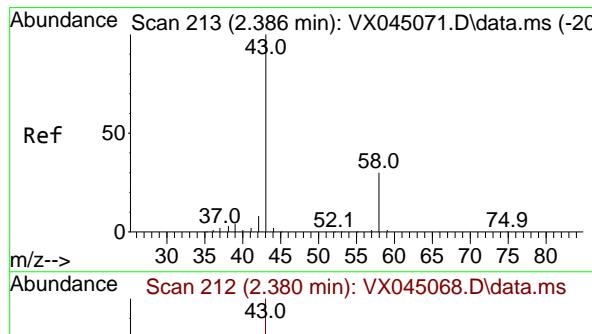



#17
Carbon Disulfide
Concen: 0.956 ug/l
RT: 2.502 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001

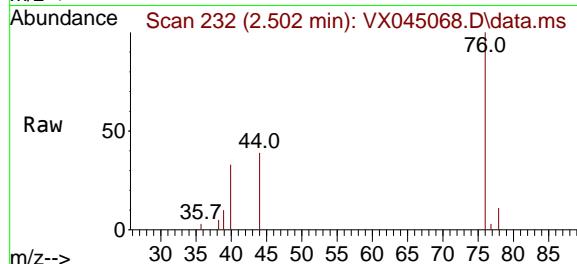


Tgt Ion: 76 Resp: 3250
Ion Ratio Lower Upper
76 100
78 11.2 6.6 9.8

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

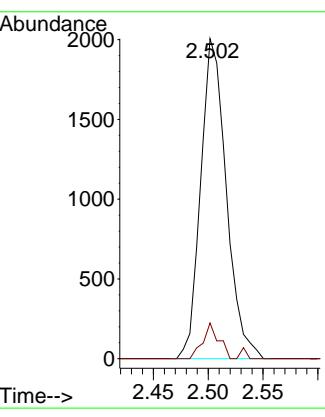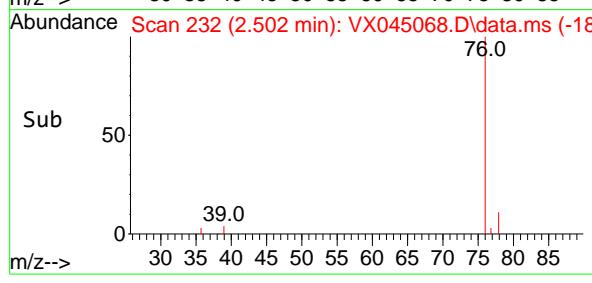


#18
Methyl Acetate
Concen: 1.066 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Tgt Ion: 43 Resp: 1960
Ion Ratio Lower Upper
43 100
74 18.5 17.4 26.2

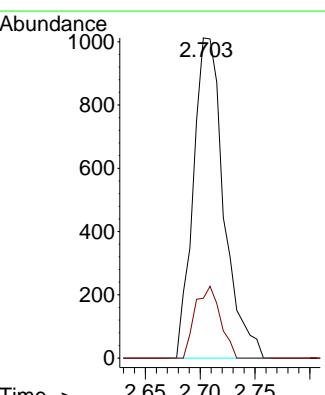



#19
Methyl tert-butyl Ether
Concen: 0.943 ug/l
RT: 3.111 min Scan# 3
Delta R.T. -0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001




Tgt Ion: 73 Resp: 401
Ion Ratio Lower Upper
73 100
57 19.0 18.5 27.7

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

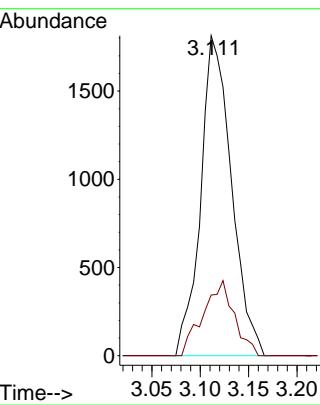


#20
Methylene Chloride
Concen: 1.095 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Tgt Ion: 84 Resp: 1656
Ion Ratio Lower Upper
84 100
49 135.2 106.5 159.7
51 36.6 32.1 48.1
86 63.2 50.0 75.0

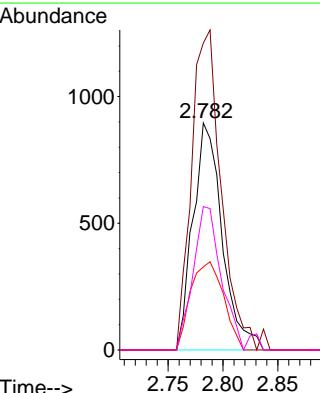



#21
trans-1,2-Dichloroethene
Concen: 0.869 ug/l
RT: 3.093 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001




Tgt Ion: 96 Resp: 1109
Ion Ratio Lower Upper
96 100
61 136.4 117.0 175.4
98 75.6 53.4 80.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

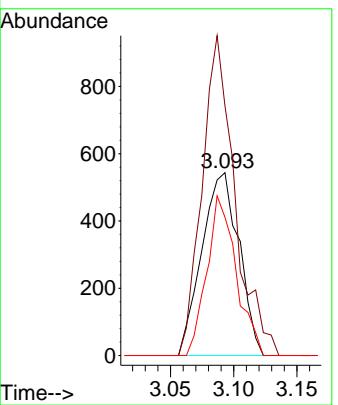


#22
Diisopropyl ether
Concen: 0.871 ug/l
RT: 3.764 min Scan# 439
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Tgt Ion: 45 Resp: 4026
Ion Ratio Lower Upper
45 100
43 91.9 54.9 82.3#
87 25.6 21.0 31.4
59 8.7 8.7 13.1

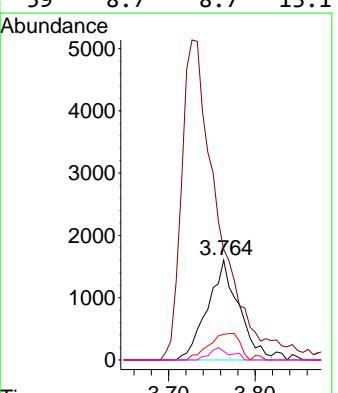



#23
Vinyl Acetate
 Concen: 3.971 ug/l
 RT: 3.727 min Scan# 413
 Delta R.T. 0.006 min
 Lab File: VX045068.D
 Acq: 28 Feb 2025 01:27



Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC001



Tgt Ion: 43 Resp: 1527:
 Ion Ratio Lower Upper
 43 100
 86 11.1 8.1 12.1



Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

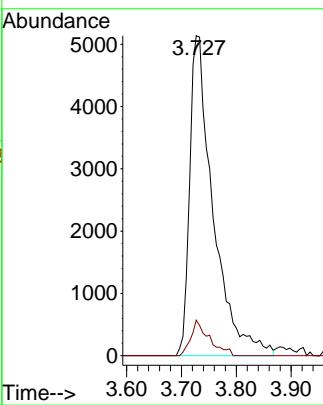



#24
1,1-Dichloroethane
 Concen: 0.958 ug/l
 RT: 3.605 min Scan# 413
 Delta R.T. 0.000 min
 Lab File: VX045068.D
 Acq: 28 Feb 2025 01:27

Tgt Ion: 63 Resp: 2467
 Ion Ratio Lower Upper
 63 100
 98 0.0 3.4 10.2#
 100 0.0 2.1 6.5#

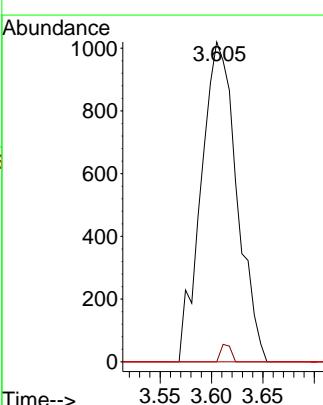


(-36)



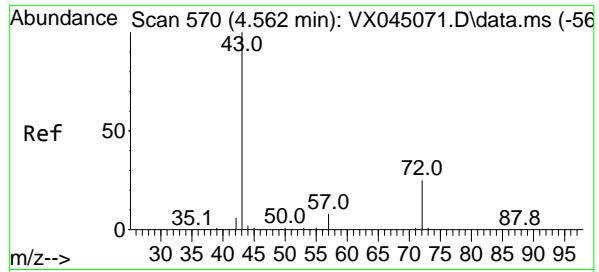

#25
2-Butanone
Concen: 4.252 ug/l
RT: 4.587 min Scan# 51
Delta R.T. 0.024 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001

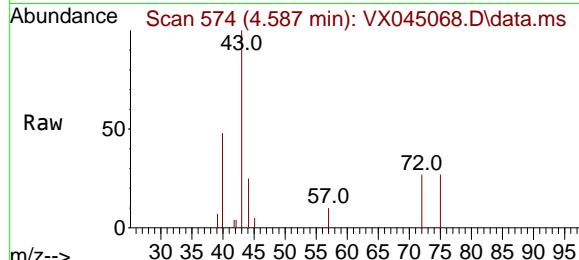


Tgt Ion: 43 Resp: 4894
Ion Ratio Lower Upper
43 100
72 27.2 20.0 30.0

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

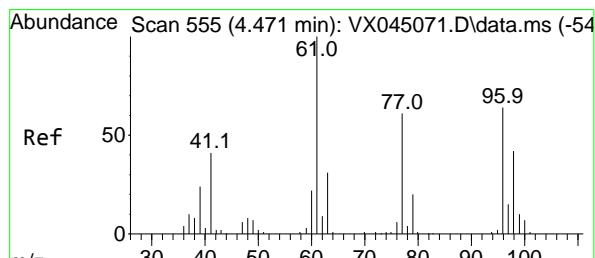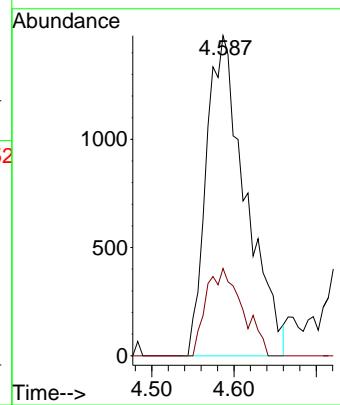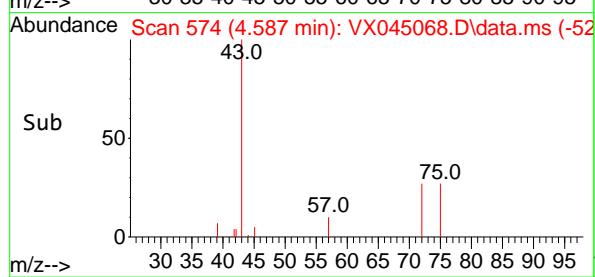


#26
2,2-Dichloropropane
Concen: 0.872 ug/l
RT: 4.471 min Scan# 555
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

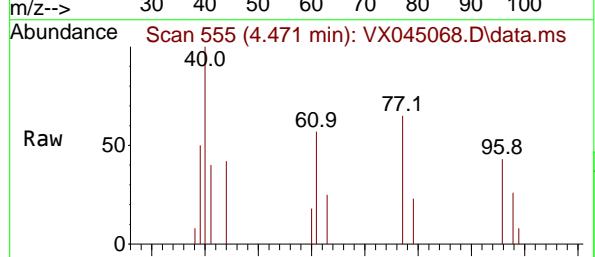


Tgt Ion: 77 Resp: 1066
Ion Ratio Lower Upper
77 100
97 2.5 12.4 37.0#

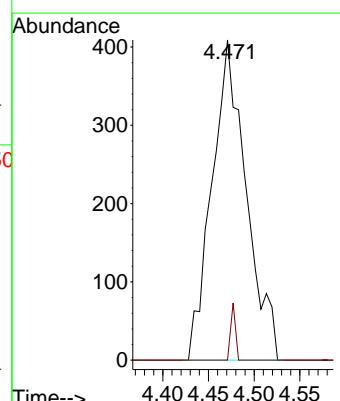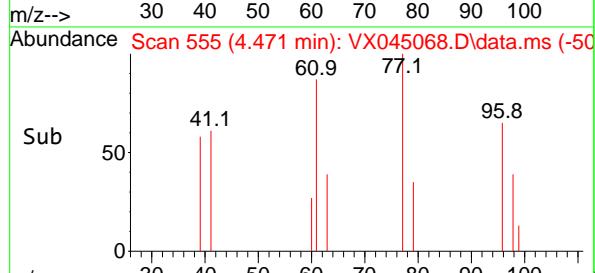





#27
cis-1,2-Dichloroethene
 Concen: 0.902 ug/l
 RT: 4.501 min Scan# 5
 Delta R.T. 0.018 min
 Lab File: VX045068.D
 Acq: 28 Feb 2025 01:27

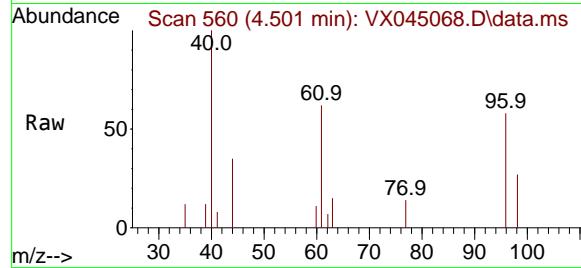


Tgt Ion: 96 Resp: 141:
 Ion Ratio Lower Upper
 96 100
 61 0.0 0.0 283.2
 98 59.1 0.0 128.0

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025




#28
 Bromochloromethane
 Concen: 0.958 ug/l
 RT: 4.885 min Scan# 623
 Delta R.T. -0.012 min
 Lab File: VX045068.D
 Acq: 28 Feb 2025 01:27

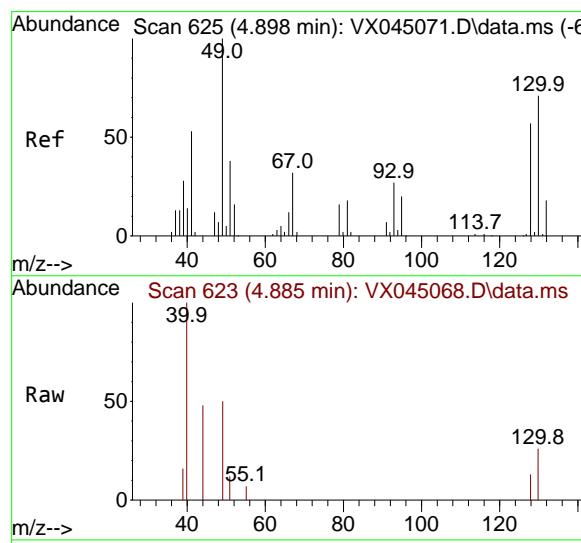

Tgt Ion: 49 Resp: 1144
 Ion Ratio Lower Upper
 49 100
 129 0.0 0.0 3.4
 130 31.5 56.1 84.1#

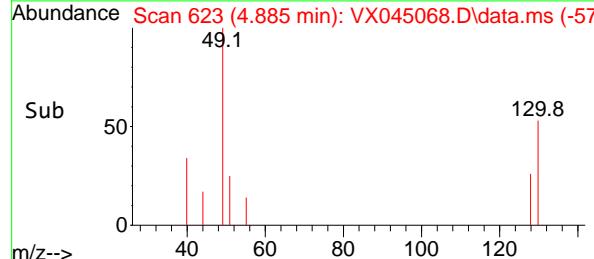



#29

Tetrahydrofuran

Concen: 4.809 ug/l

RT: 5.032 min Scan# 6


Delta R.T. 0.024 min

Lab File: VX045068.D

Acq: 28 Feb 2025 01:27

Instrument : MSVOA_X

ClientSampleId : VSTDICC001



Tgt Ion: 42 Resp: 3719

Ion Ratio Lower Upper

42 100




72 0.0 34.1 51.1

71 0.0 31.4 47.0

Manual Integrations**APPROVED**

Reviewed By :John Carlone 02/28/2025

Supervised By :Mahesh Dadoda 02/28/2025

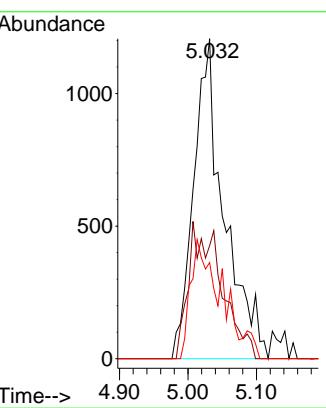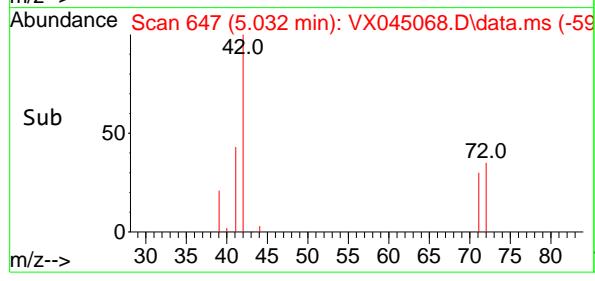

#30

Chloroform

Concen: 0.978 ug/l

RT: 5.093 min Scan# 657

Delta R.T. 0.006 min

Lab File: VX045068.D





Acq: 28 Feb 2025 01:27


Tgt Ion: 83 Resp: 2478

Ion Ratio Lower Upper

83 100


85 58.0 51.4 77.2

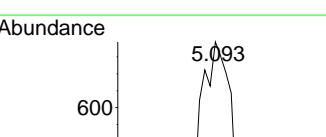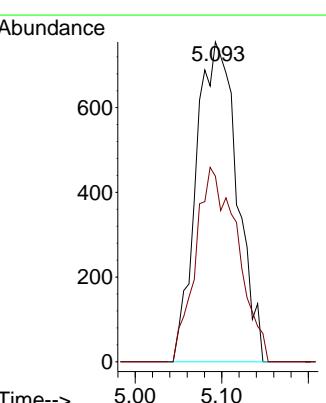



#32
 1,1,1-Trichloroethane
 Concen: 0.893 ug/l
 RT: 5.373 min Scan# 7
 Delta R.T. -0.006 min
 Lab File: VX045068.D
 Acq: 28 Feb 2025 01:27




Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC001



Tgt Ion: 97 Resp: 186
 Ion Ratio Lower Upper
 97 100
 99 0.0 51.6 77.4
 61 50.0 38.4 57.6

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

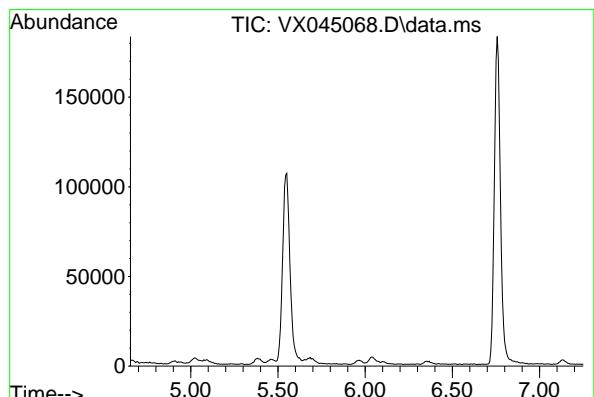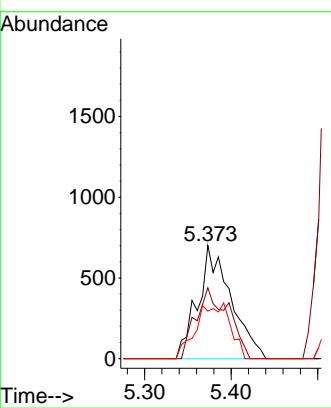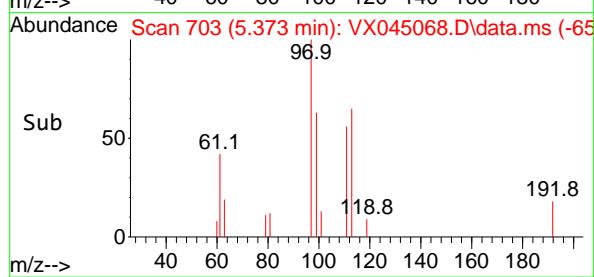


#33
 1,2-Dichloroethane-d4
 Concen: 0.000 ug/l
 Expected RT: 5.95 min


Lab File: VX045068.D
 Acq: 28 Feb 2025 01:27

Tgt Ion: 65
 Sig Exp Ratio
 65 100
 67 53.1

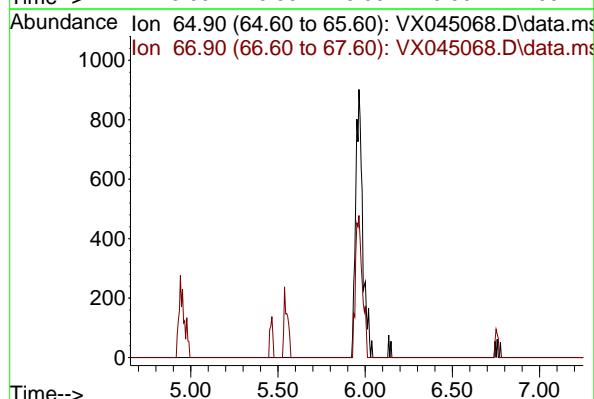






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 9
Instrument : MSVOA_X
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Tgt Ion:114 Resp: 18864
Ion Ratio Lower Upper
114 100
63 21.4 0.0 41.8
88 16.0 0.0 32.8

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

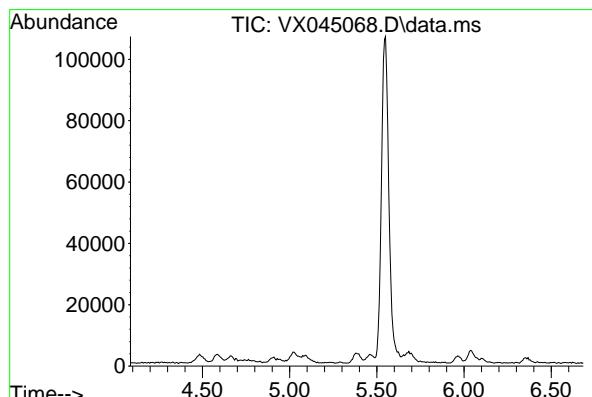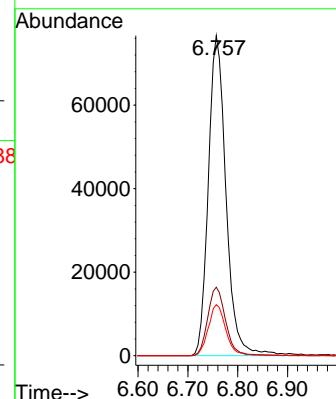


#35
Dibromofluoromethane
Concen: 0.000 ug/l
Expected RT: 5.39 min

Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

Tgt Ion: 113
Sig Exp Ratio
113 100
111 102.2
192 17.9

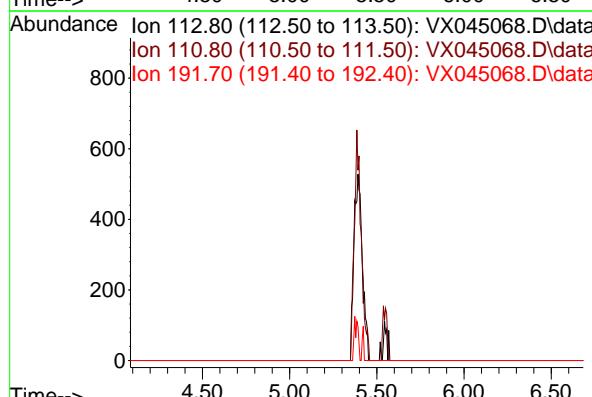



#36

1,1-Dichloropropene



Concen: 0.967 ug/l

RT: 5.690 min Scan# 7

Delta R.T. 0.000 min

Lab File: VX045068.D

Acq: 28 Feb 2025 01:27

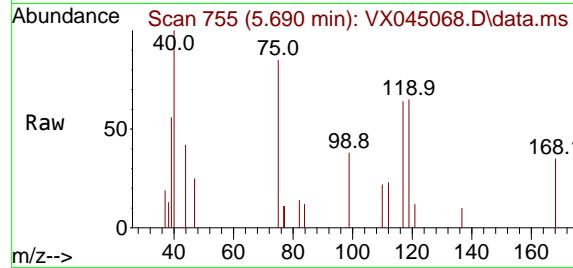

Tgt Ion: 75 Resp: 168

Ion Ratio Lower Upper

75 100



110 29.6 16.9 50.6

77 16.4 24.5 36.7

Manual Integrations**APPROVED**

Reviewed By :John Carlone 02/28/2025

Supervised By :Mahesh Dadoda 02/28/2025

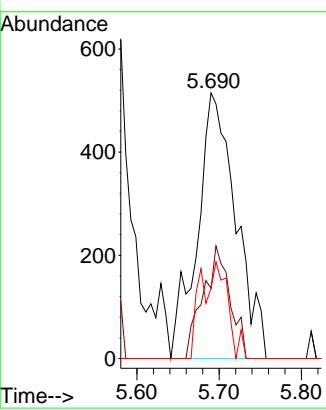

#37

Ethyl Acetate


Concen: 0.988 ug/l m

RT: 4.739 min Scan# 599

Delta R.T. 0.024 min

Lab File: VX045068.D

Acq: 28 Feb 2025 01:27





Tgt Ion: 43 Resp: 2223


Ion Ratio Lower Upper

43 100

61 0.0 10.8 16.2#

70 0.0 7.7 11.5#

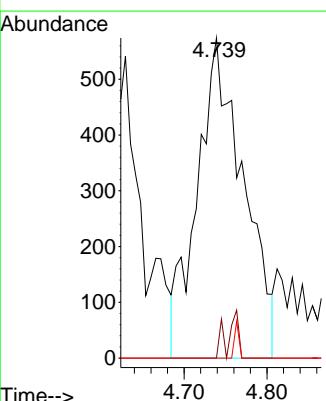




#38

Carbon Tetrachloride
Concen: 0.987 ug/l m
RT: 5.672 min Scan# 7
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001

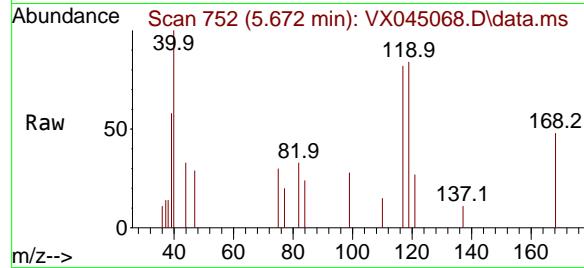


Tgt Ion:117 Resp: 1741
Ion Ratio Lower Upper
117 100
119 103.4 76.7 115.1
121 33.2 25.5 38.3

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

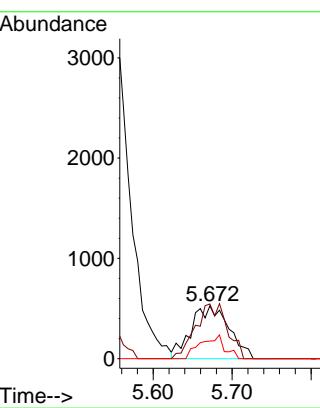


#39
Methylcyclohexane
Concen: 0.831 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. 0.012 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

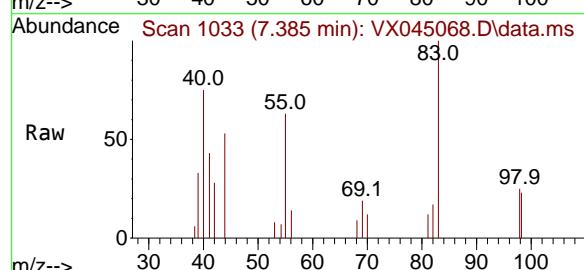


Tgt Ion: 83 Resp: 1750
Ion Ratio Lower Upper
83 100
55 63.0 63.0 94.4
98 47.3 39.7 59.5

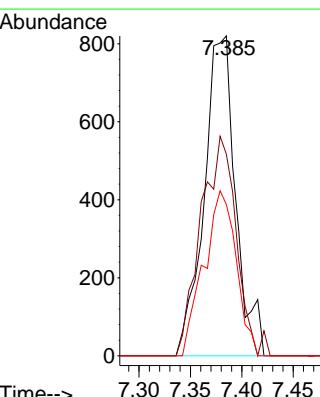



#40
Benzene
Concen: 0.907 ug/l
RT: 6.031 min Scan# 8
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001







Tgt Ion: 78 Resp: 4984
Ion Ratio Lower Upper
78 100
77 23.2 18.8 28.2


Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

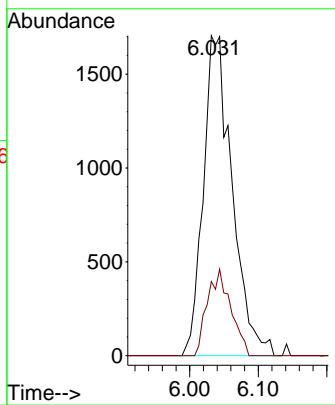


#41
Methacrylonitrile
Concen: 0.879 ug/l m
RT: 4.958 min Scan# 635
Delta R.T. 0.037 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

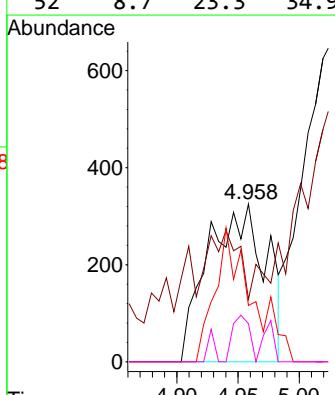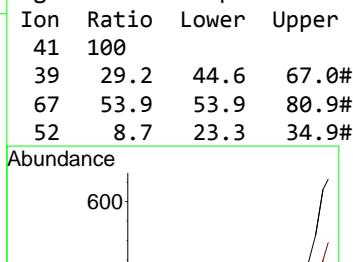



#42
1,2-Dichloroethane
Concen: 0.924 ug/l
RT: 6.099 min Scan# 819
Delta R.T. 0.018 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001

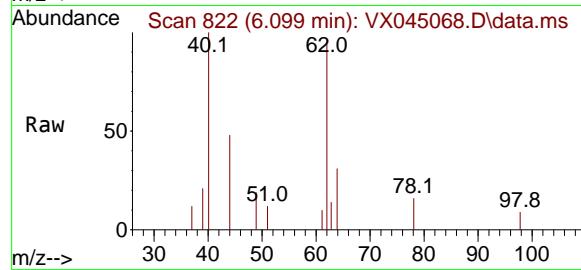


Tgt Ion: 62 Resp: 1831
Ion Ratio Lower Upper
62 100
98 1.2 0.0 18.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

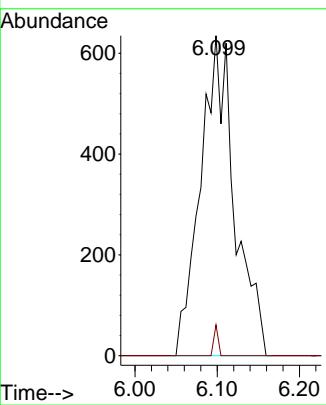


#43
Isopropyl Acetate
Concen: 0.767 ug/l
RT: 6.355 min Scan# 864
Delta R.T. 0.012 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27





Tgt Ion: 43 Resp: 2545
Ion Ratio Lower Upper
43 100
61 17.0 14.9 22.3
87 9.2 9.4 14.2#

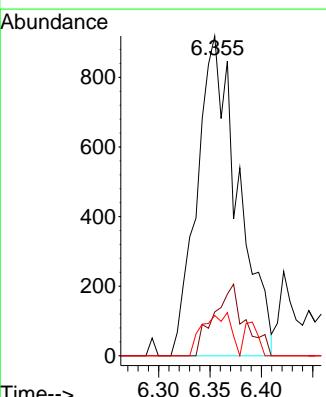



#44
Trichloroethene
Concen: 0.933 ug/l
RT: 7.129 min Scan# 990
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001




Tgt Ion:130 Resp: 1200
Ion Ratio Lower Upper
130 100
95 67.0 0.0 205.0

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#45
1,2-Dichloropropane
Concen: 0.971 ug/l
RT: 7.434 min Scan# 1041
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Tgt Ion: 63 Resp: 1334
Ion Ratio Lower Upper
63 100
65 21.1 24.7 37.1#





#46
Dibromomethane
Concen: 0.897 ug/l
RT: 7.586 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001



Tgt Ion: 93 Resp: 891
Ion Ratio Lower Upper
93 100
95 80.9 65.8 98.8
174 102.8 72.2 108.2




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#47
Bromodichloromethane
Concen: 0.927 ug/l
RT: 7.818 min Scan# 1104
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

Tgt Ion: 83 Resp: 1802
Ion Ratio Lower Upper
83 100
85 50.9 51.1 76.7#
127 6.5 6.4 9.6






#48

Methyl methacrylate
Concen: 0.825 ug/l m
RT: 7.714 min Scan# 1
Delta R.T. 0.024 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001

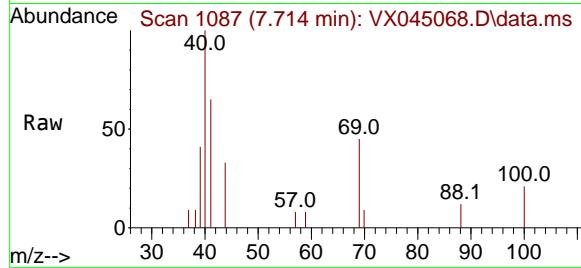


Tgt Ion: 41 Resp: 1322
Ion Ratio Lower Upper
41 100
69 41.4 63.0 94.6#
39 20.7 47.5 71.3#

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

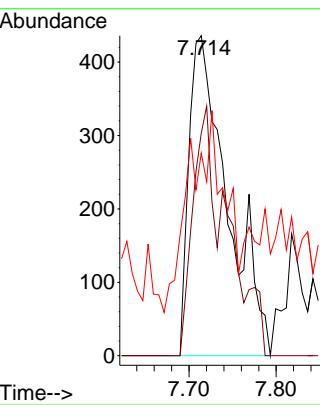


#49
1,4-Dioxane
Concen: 18.144 ug/l
RT: 7.684 min Scan# 1082
Delta R.T. 0.024 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Tgt Ion: 88 Resp: 639
Ion Ratio Lower Upper
88 100
43 17.2 28.7 43.1#
58 59.9 55.8 83.8

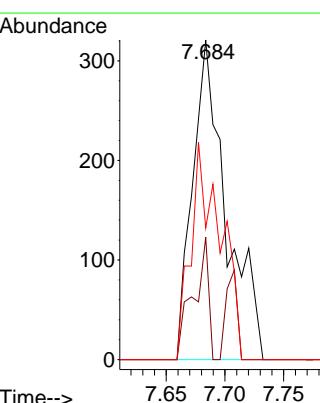

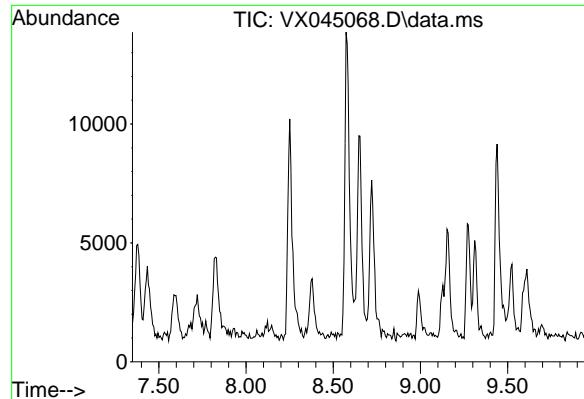

#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 8.65 min


Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001

Tgt Ion: 98
Sig Exp Ratio
98 100
100 65.0



Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

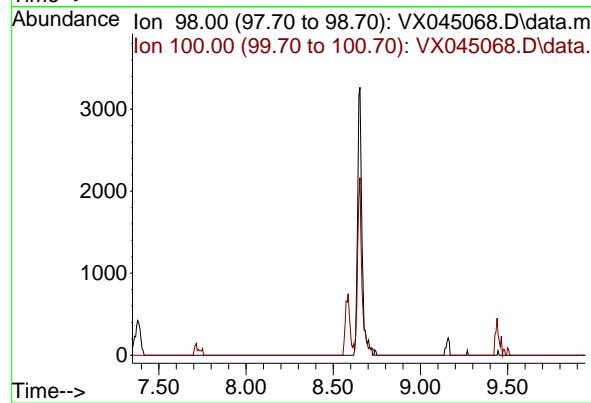

#51
4-Methyl-2-Pentanone
Concen: 4.567 ug/l
RT: 8.574 min Scan# 1228
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27


Tgt Ion: 43 Resp: 10091
Ion Ratio Lower Upper
43 100
58 33.5 29.2 43.8

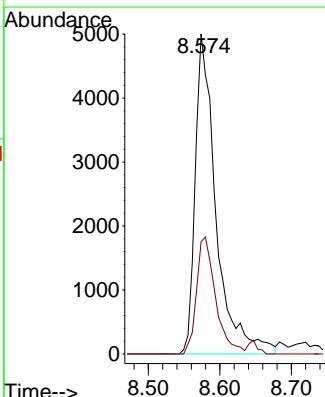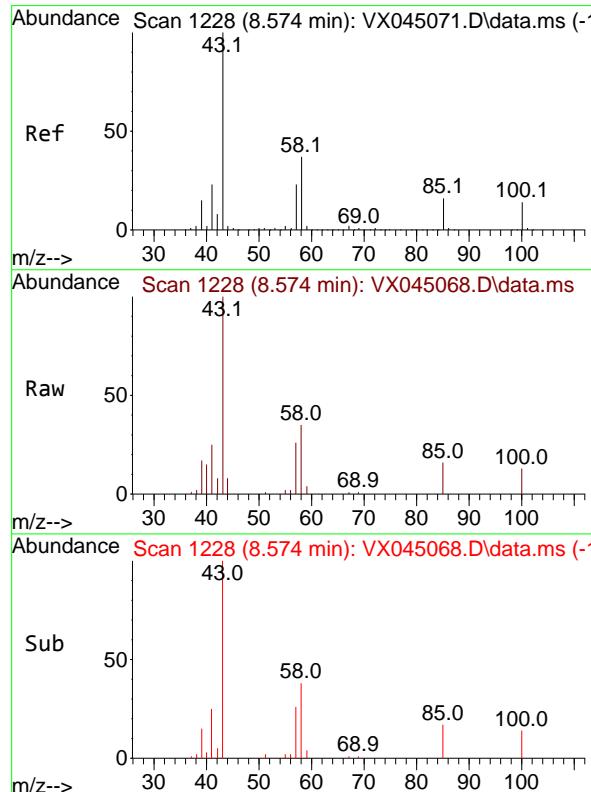



#52
Toluene
Concen: 0.841 ug/l
RT: 8.720 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001




Tgt Ion: 92 Resp: 2700
Ion Ratio Lower Upper
92 100
91 177.7 138.9 208.3

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#53
t-1,3-Dichloropropene
Concen: 0.700 ug/l
RT: 8.994 min Scan# 1297
Delta R.T. 0.018 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Tgt Ion: 75 Resp: 1147
Ion Ratio Lower Upper
75 100
77 41.4 26.5 39.7#





#54
cis-1,3-Dichloropropene
Concen: 0.804 ug/l
RT: 8.373 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001

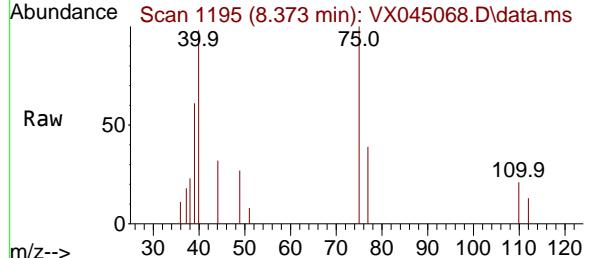


Tgt Ion: 75 Resp: 1525
Ion Ratio Lower Upper
75 100
77 38.6 24.7 37.1
39 45.1 40.7 61.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

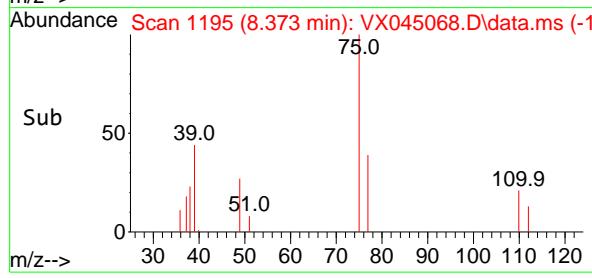


#55
1,1,2-Trichloroethane
Concen: 1.004 ug/l
RT: 9.153 min Scan# 1323
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Tgt Ion: 97 Resp: 1306
Ion Ratio Lower Upper
97 100
83 87.0 69.4 104.2
85 45.8 44.1 66.1
99 79.4 50.7 76.1#





#56
 Ethyl methacrylate
 Concen: 0.748 ug/l
 RT: 9.135 min Scan# 1
 Delta R.T. 0.018 min
 Lab File: VX045068.D
 Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
 ClientSampleId : VSTDICC001



Tgt Ion: 69 Resp: 149.4
 Ion Ratio Lower Upper
 69 100
 41 71.5 57.0 85.4
 39 54.6 34.2 51.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

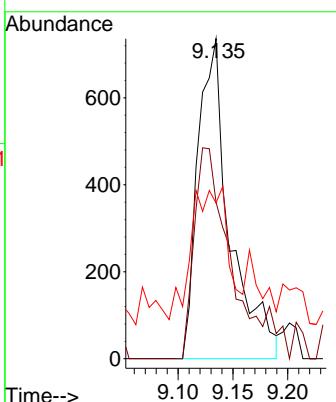

#57
 1,3-Dichloropropane
 Concen: 0.920 ug/l
 RT: 9.311 min Scan# 1349
 Delta R.T. 0.006 min
 Lab File: VX045068.D
 Acq: 28 Feb 2025 01:27


Tgt Ion: 76 Resp: 2112
 Ion Ratio Lower Upper
 76 100
 78 30.1 25.5 38.3

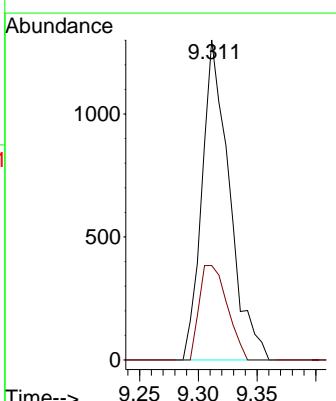



#58
2-Chloroethyl Vinyl ether
Concen: 4.320 ug/l
RT: 8.251 min Scan# 1173
Delta R.T. 0.012 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001

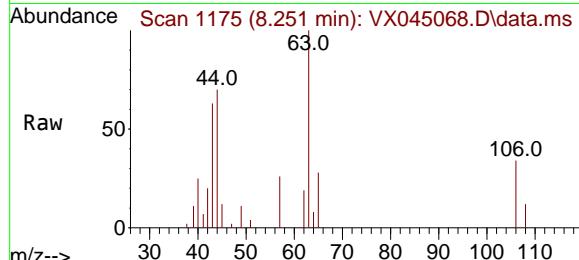

Tgt Ion: 63 Resp: 4119
Ion Ratio Lower Upper
63 100
106 29.2 21.5 32.3




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

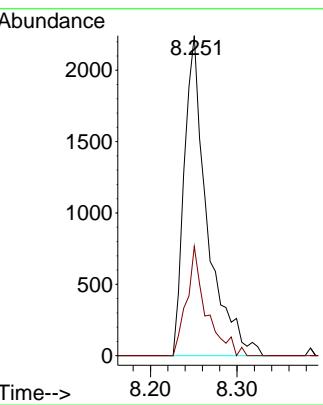

#59
2-Hexanone
Concen: 4.153 ug/l
RT: 9.439 min Scan# 1370
Delta R.T. 0.012 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27


Tgt Ion: 43 Resp: 6582
Ion Ratio Lower Upper
43 100
58 48.7 25.9 77.6

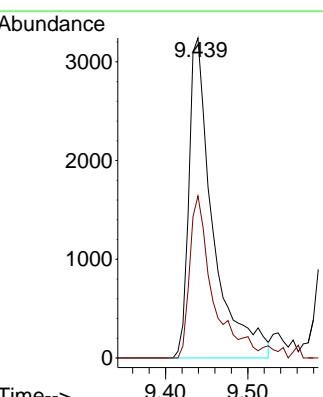



#60
Dibromochloromethane
Concen: 0.835 ug/l
RT: 9.519 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001




Tgt Ion:129 Resp: 1153
Ion Ratio Lower Upper
129 100
127 75.2 38.5 115.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#61
1,2-Dibromoethane
Concen: 0.890 ug/l
RT: 9.610 min Scan# 1398
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Tgt Ion:107 Resp: 1174
Ion Ratio Lower Upper
107 100
109 97.6 76.1 114.1



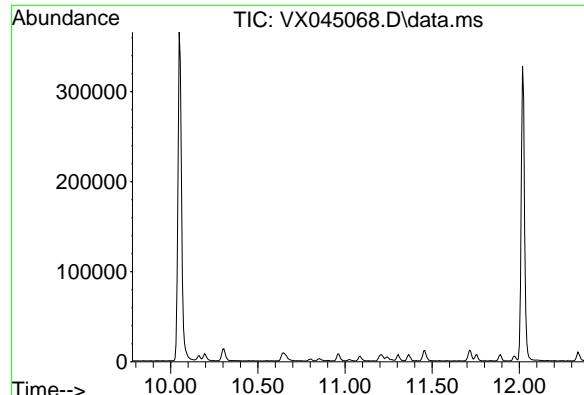

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 11.08 min


Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

Tgt Ion: 95
Sig Exp Ratio
95 100
174 74.1
176 70.7

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001



Manual Integrations
APPROVED


Reviewed By :John Carbone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

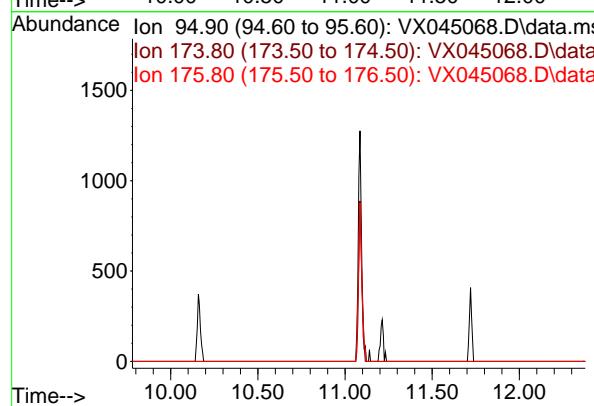

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27


Tgt Ion:117 Resp: 159886
Ion Ratio Lower Upper
117 100
82 59.0 46.3 69.5
119 32.0 25.7 38.5

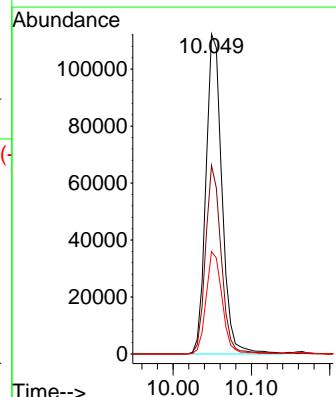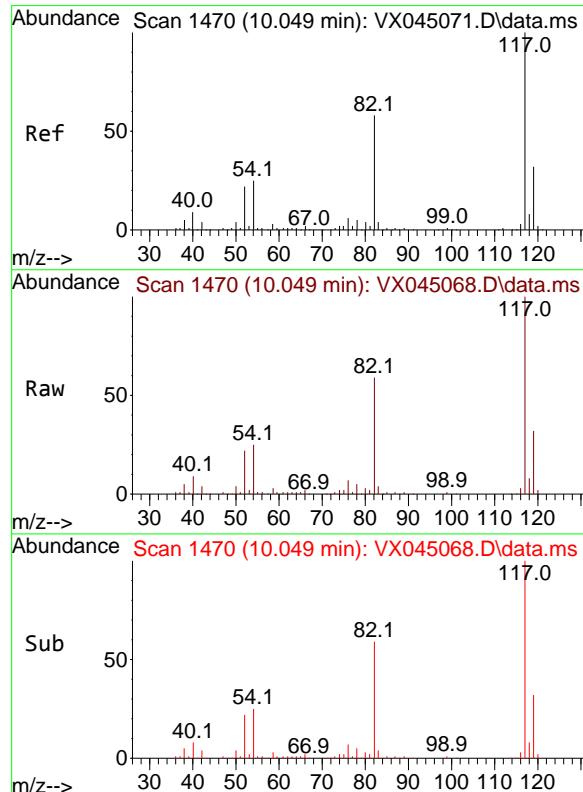



#64
Tetrachloroethene
Concen: 0.986 ug/l
RT: 9.275 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001




Tgt Ion:164 Resp: 1000
Ion Ratio Lower Upper
164 100
166 127.9 103.6 155.4
129 85.8 82.7 124.1
131 80.5 80.5 120.7#

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

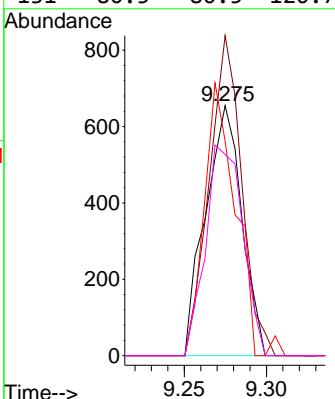


#65
Chlorobenzene
Concen: 0.908 ug/l
RT: 10.080 min Scan# 1475
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Tgt Ion:112 Resp: 3094
Ion Ratio Lower Upper
112 100
114 38.3 26.0 39.0

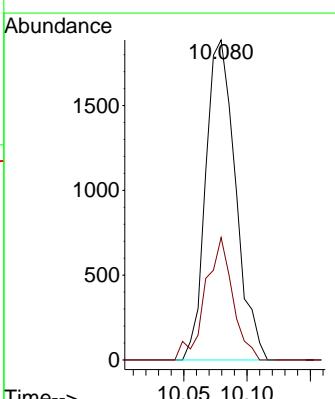

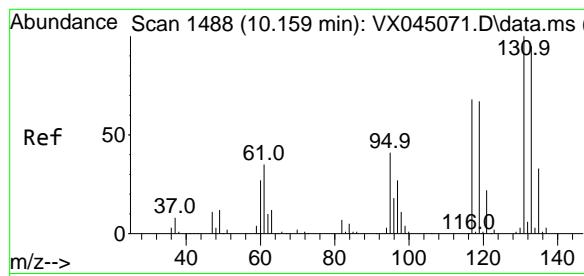




#66
1,1,1,2-Tetrachloroethane
Concen: 0.978 ug/l
RT: 10.159 min Scan# 1488
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Tgt Ion:131 Resp: 1073
Ion Ratio Lower Upper
131 100
133 98.6 48.6 145.9
119 0.0 33.9 101.7

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

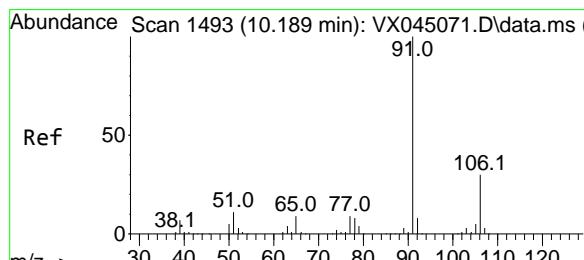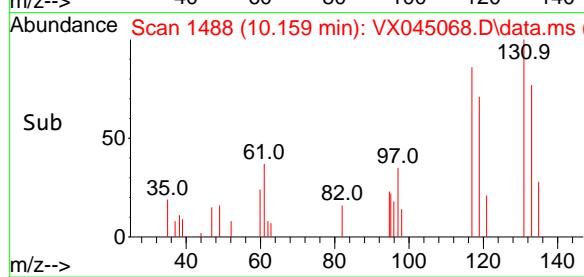


#67
Ethyl Benzene
Concen: 0.846 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Tgt Ion: 91 Resp: 5008
Ion Ratio Lower Upper
91 100
106 38.0 23.9 35.9#

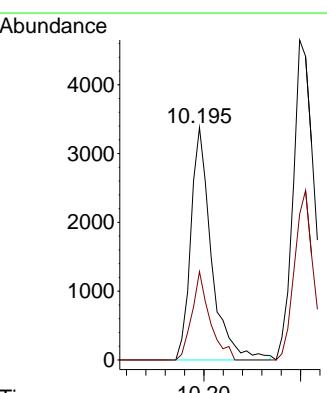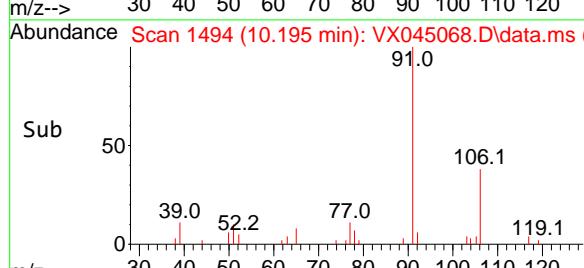


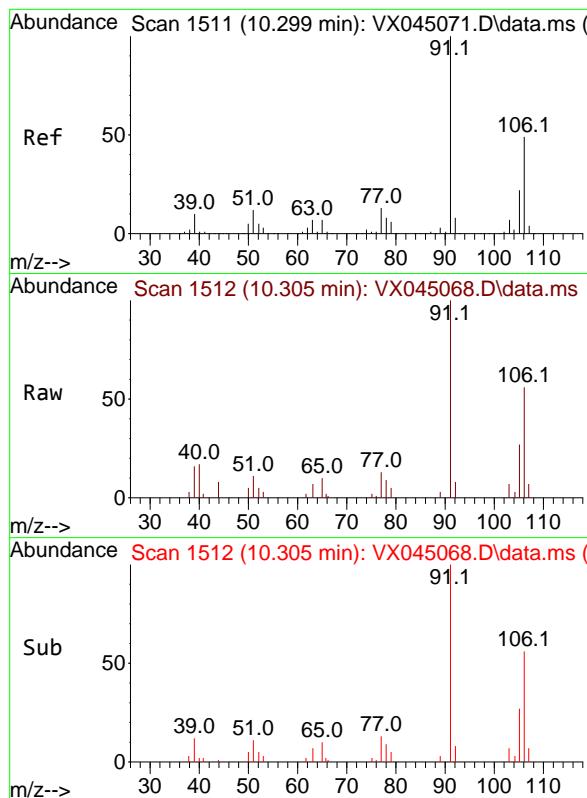


#68
m/p-Xylenes
Concen: 1.630 ug/l
RT: 10.305 min Scan# 1
Instrument : MSVOA_X
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27
ClientSampleId : VSTDICC001

Tgt Ion:106 Resp: 355:
Ion Ratio Lower Upper
106 100
91 211.2 165.4 248.0


Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

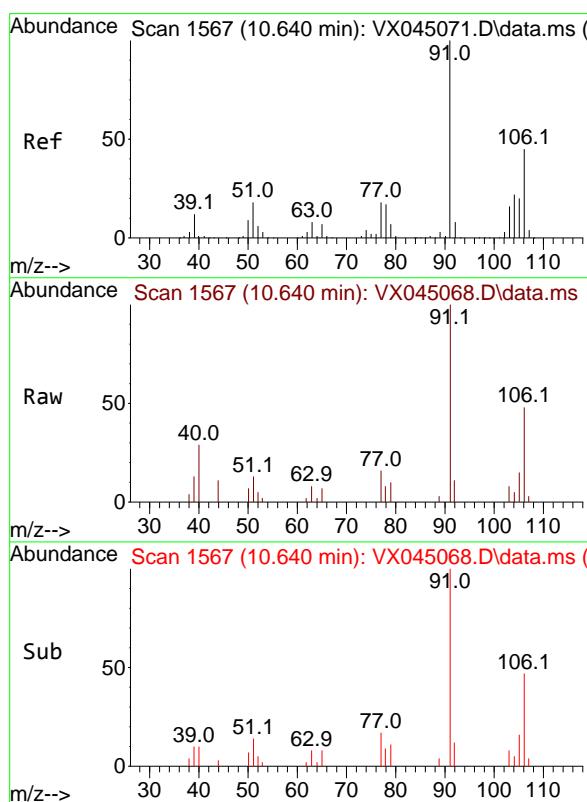

#69
o-Xylene
Concen: 0.891 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27


Tgt Ion:106 Resp: 1949
Ion Ratio Lower Upper
106 100
91 211.0 109.9 329.6

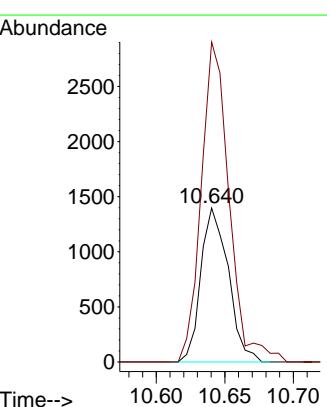



#70
Styrene
Concen: 0.802 ug/l
RT: 10.665 min Scan# 1
Delta R.T. 0.012 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Instrument : MSVOA_X
ClientSampleId : VSTDICC001




Tgt Ion:104 Resp: 2810
Ion Ratio Lower Upper
104 100
78 49.7 42.2 63.4
103 53.6 43.8 65.8

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#71
Bromoform
Concen: 0.768 ug/l
RT: 10.799 min Scan# 1593
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Tgt Ion:173 Resp: 667
Ion Ratio Lower Upper
173 100
175 54.7 24.6 73.6
254 0.0 0.0 0.0




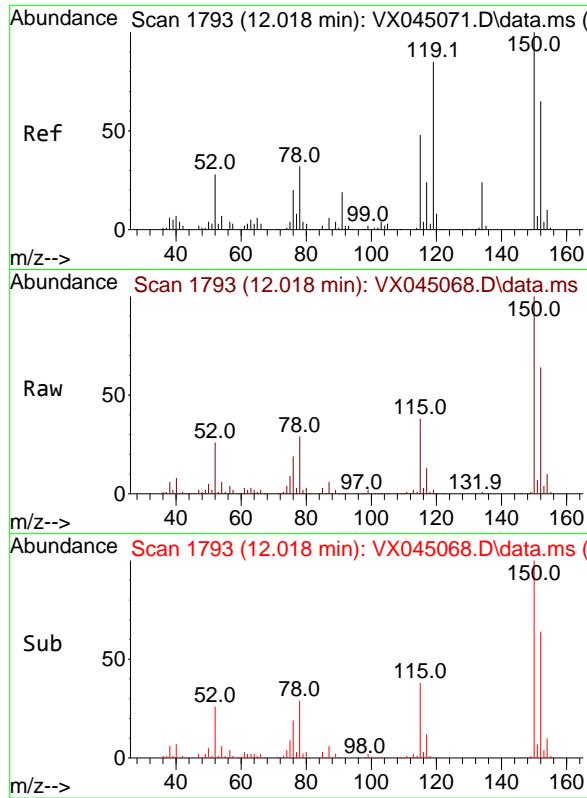


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

Instrument : MSVOA_X
ClientSampleId : VSTDICC001


**Manual Integrations
APPROVED**


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

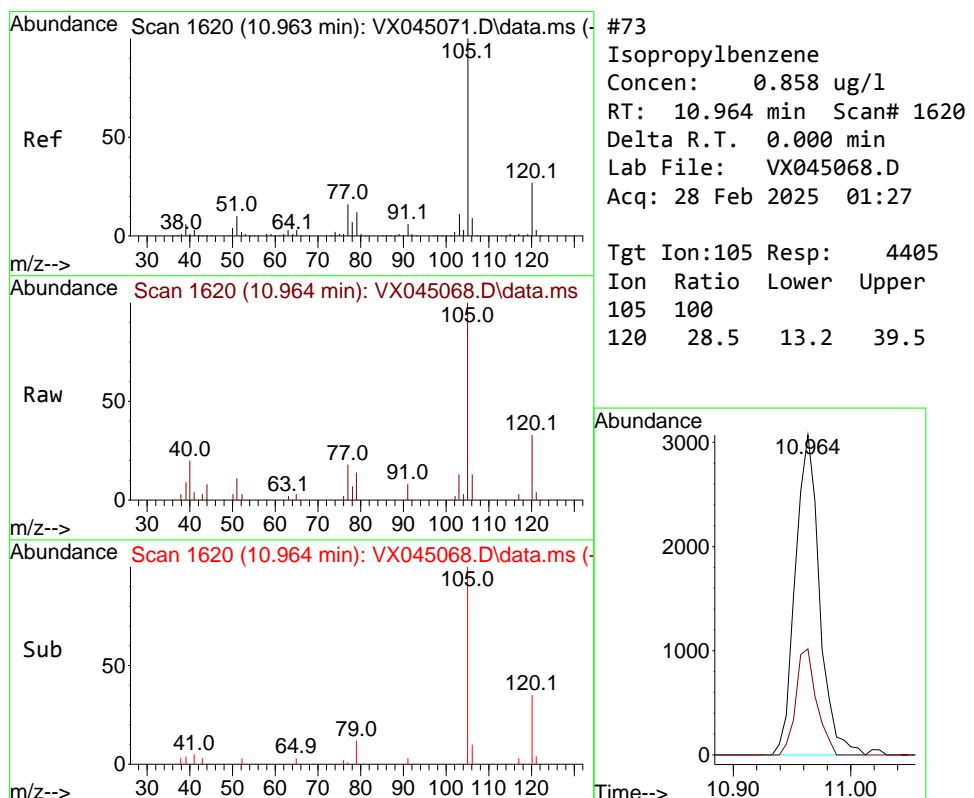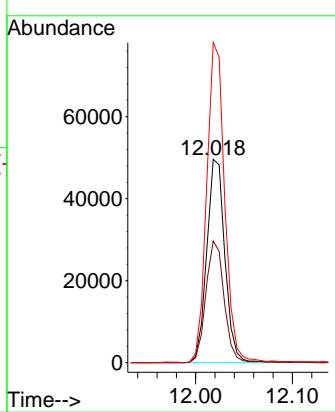

#73
Isopropylbenzene
Concen: 0.858 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

Tgt Ion:105 Resp: 4405
Ion Ratio Lower Upper
105 100
120 28.5 13.2 39.5

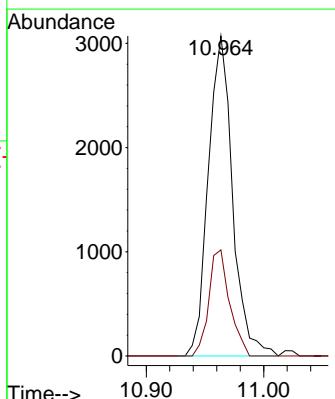

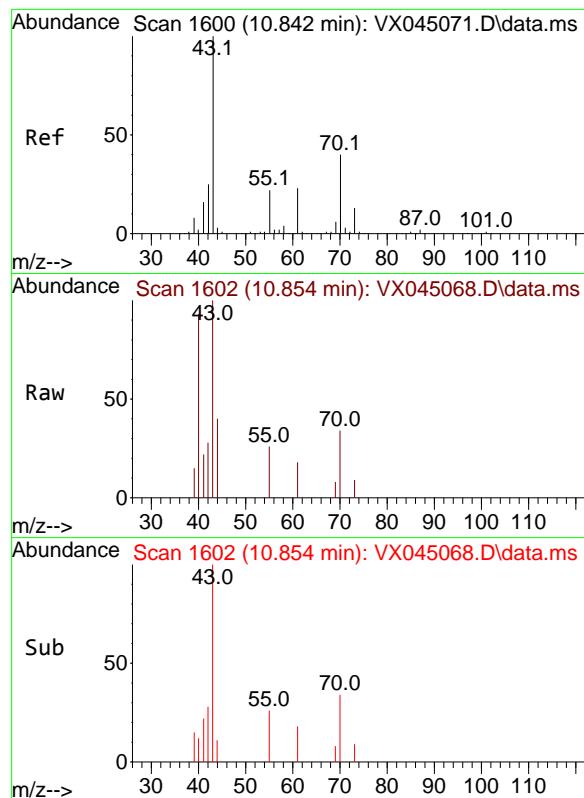

#74
N-amyl acetate
Concen: 0.732 ug/l
RT: 10.854 min Scan# 1
Delta R.T. 0.012 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Instrument : MSVOA_X
ClientSampleId : VSTDICC001

Tgt Ion: 43 Resp: 1750
Ion Ratio Lower Upper

43	100
70	30.1
55	20.9
61	13.7
	18.3
	27.5

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

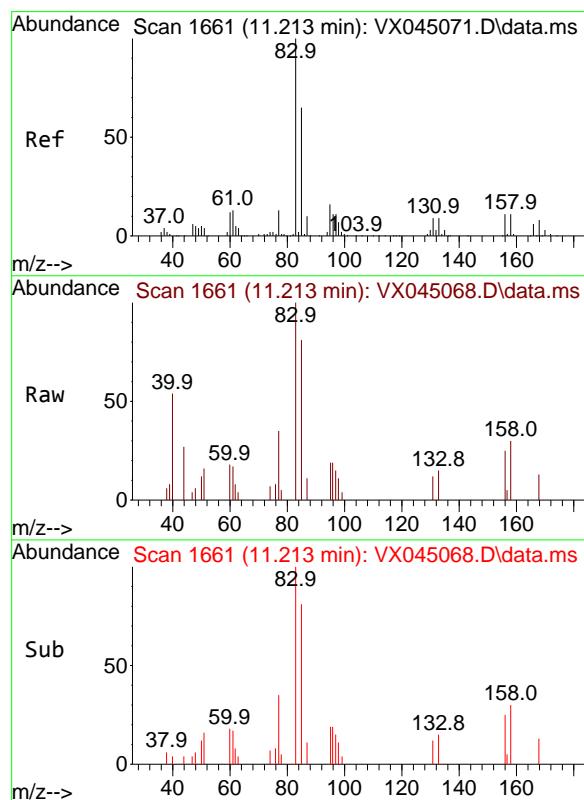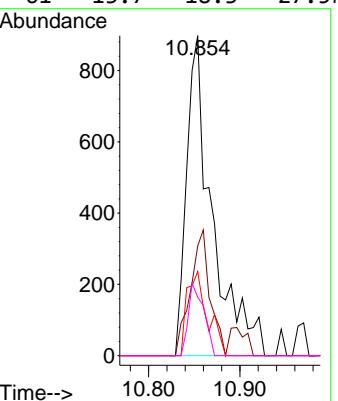


#75
1,1,2,2-Tetrachloroethane
Concen: 0.954 ug/l
RT: 11.213 min Scan# 1661
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

Tgt Ion: 83 Resp: 1809
Ion Ratio Lower Upper


83	100
131	9.2
85	73.7
	4.5
	31.7
	13.4
	95.1





#76
1,2,3-Trichloropropane
Concen: 1.015 ug/l m
RT: 11.244 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001



Tgt Ion: 75 Resp: 153:
Ion Ratio Lower Upper
75 100
77 40.0 20.7 62.1



Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#77
Bromobenzene
Concen: 0.972 ug/l
RT: 11.201 min Scan# 1659
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27


Tgt Ion:156 Resp: 1166
Ion Ratio Lower Upper
156 100
77 159.8 85.8 257.4
158 86.2 48.4 145.2

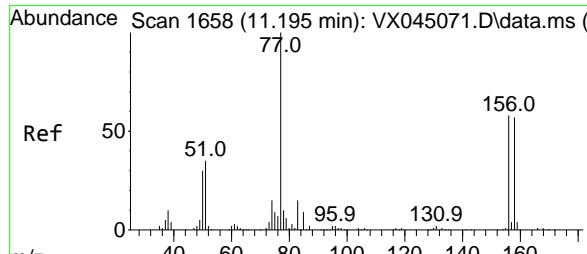


11.201

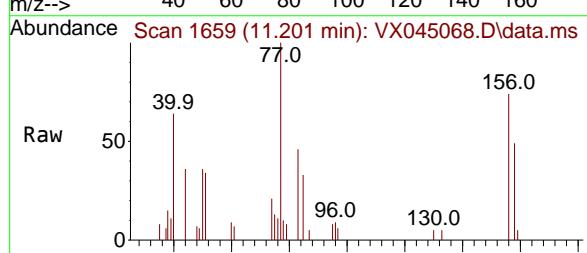


11.201

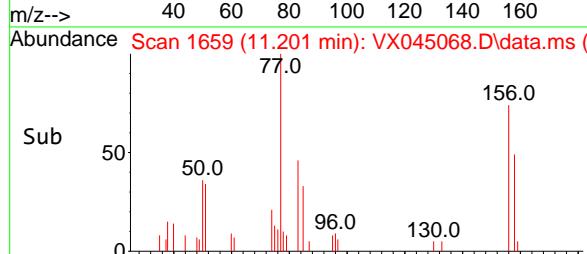



#78
n-propylbenzene
Concen: 0.773 ug/l
RT: 11.305 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001




Tgt Ion: 91 Resp: 4479
Ion Ratio Lower Upper
91 100
120 23.9 11.2 33.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

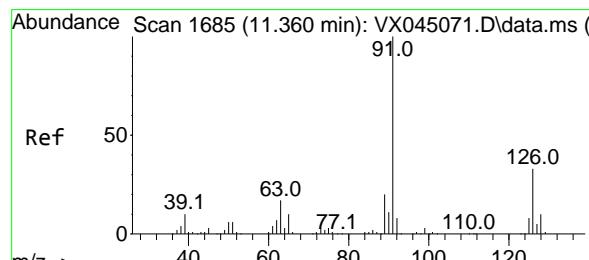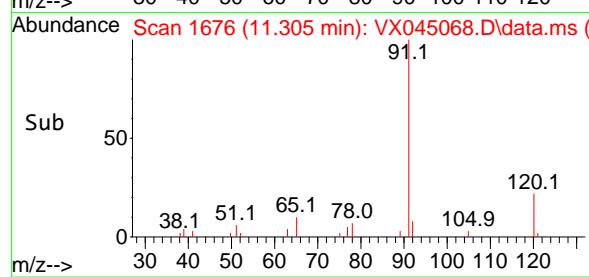


#79
2-Chlorotoluene
Concen: 0.986 ug/l
RT: 11.366 min Scan# 1686
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

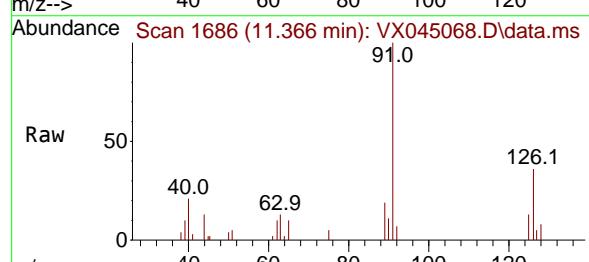


Tgt Ion: 91 Resp: 3616
Ion Ratio Lower Upper
91 100
126 34.2 16.4 49.4

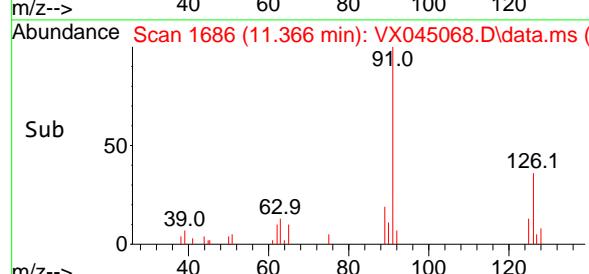



#80
1,3,5-Trimethylbenzene
Concen: 0.815 ug/l
RT: 11.451 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Instrument :
MSVOA_X
ClientSampleId :
VSTDICC001

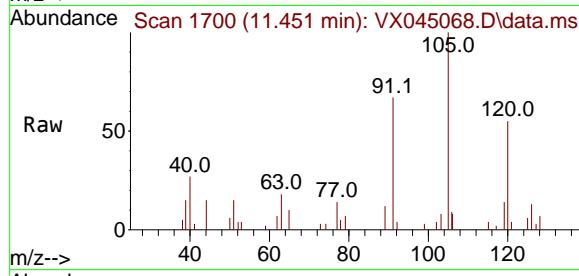

Tgt Ion:105 Resp: 3380
Ion Ratio Lower Upper
105 100
120 52.2 24.1 72.2



Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

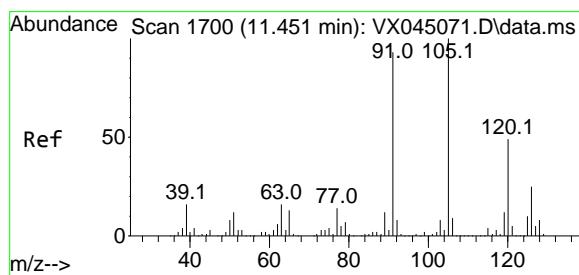





#82
4-Chlorotoluene
Concen: 0.904 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

Tgt Ion: 91 Resp: 3631
Ion Ratio Lower Upper
91 100
126 28.0 14.1 42.4

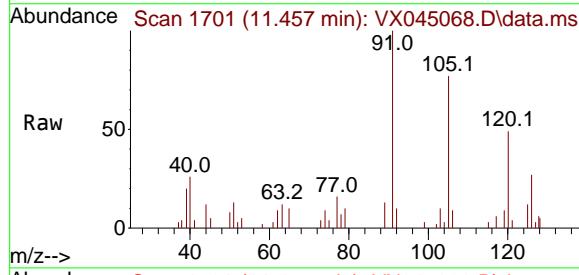

Abundance

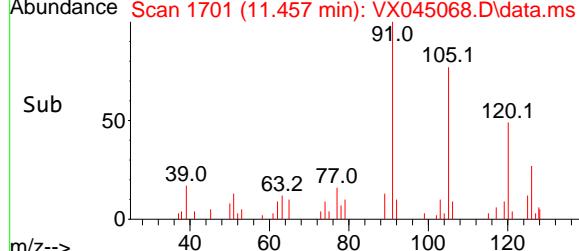



#83

tert-Butylbenzene

Concen: 0.929 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045068.D

Acq: 28 Feb 2025 01:27





Instrument:

MSVOA_X

ClientSampleId :

VSTDICC001

**Manual Integrations
APPROVED**

 Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025


#84

1,2,4-Trimethylbenzene


Concen: 0.827 ug/l


RT: 11.756 min Scan# 1750

Delta R.T. 0.006 min


Lab File: VX045068.D

Acq: 28 Feb 2025 01:27

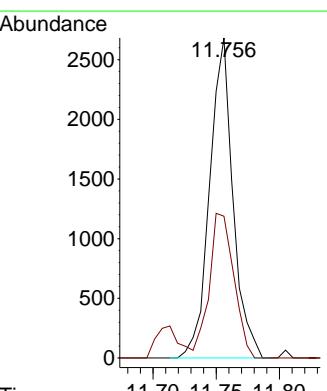 Tgt Ion:105 Resp: 3432
 Ion Ratio Lower Upper
 105 100
 120 47.5 22.1 66.1






#85
sec-Butylbenzene
Concen: 0.752 ug/l
RT: 11.890 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27
Instrument : MSVOA_X
ClientSampleId : VSTDICC001




Tgt Ion:105 Resp: 389:
Ion Ratio Lower Upper
105 100
134 19.5 9.8 29.4

Manual Integrations APPROVED




Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#86
p-Isopropyltoluene
Concen: 0.797 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

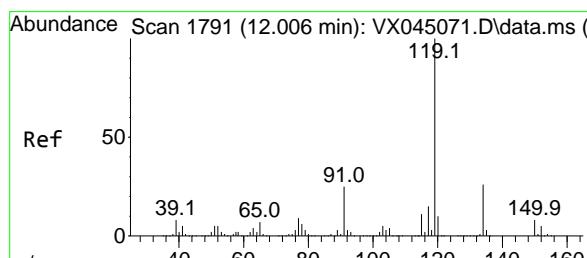

Tgt Ion:119 Resp: 3257
Ion Ratio Lower Upper
119 100
134 25.6 12.9 38.6
91 30.9 12.7 38.0

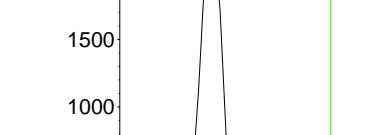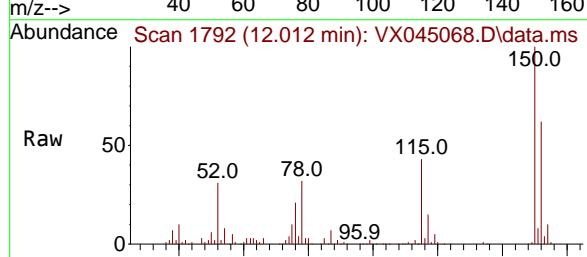


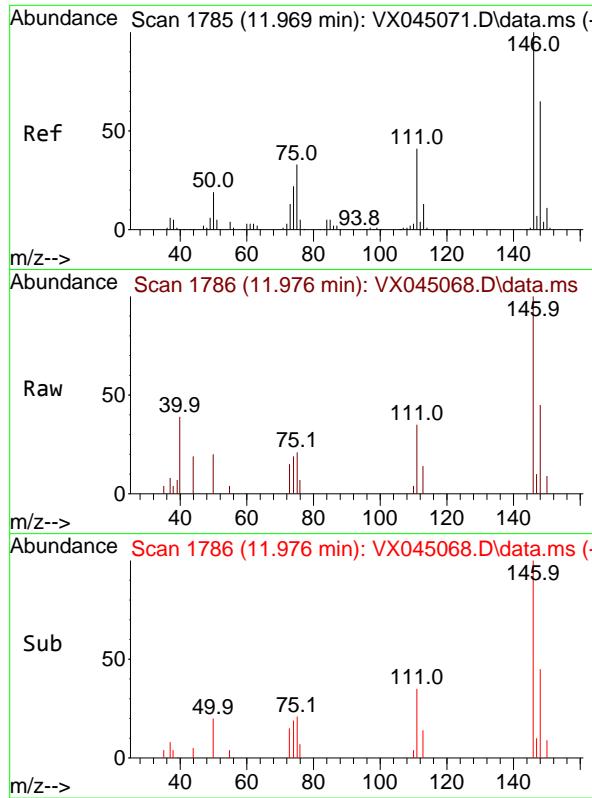


#87
1,3-Dichlorobenzene
Concen: 0.913 ug/l
RT: 11.976 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27

Instrument : MSVOA_X
ClientSampleId : VSTDICC001


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

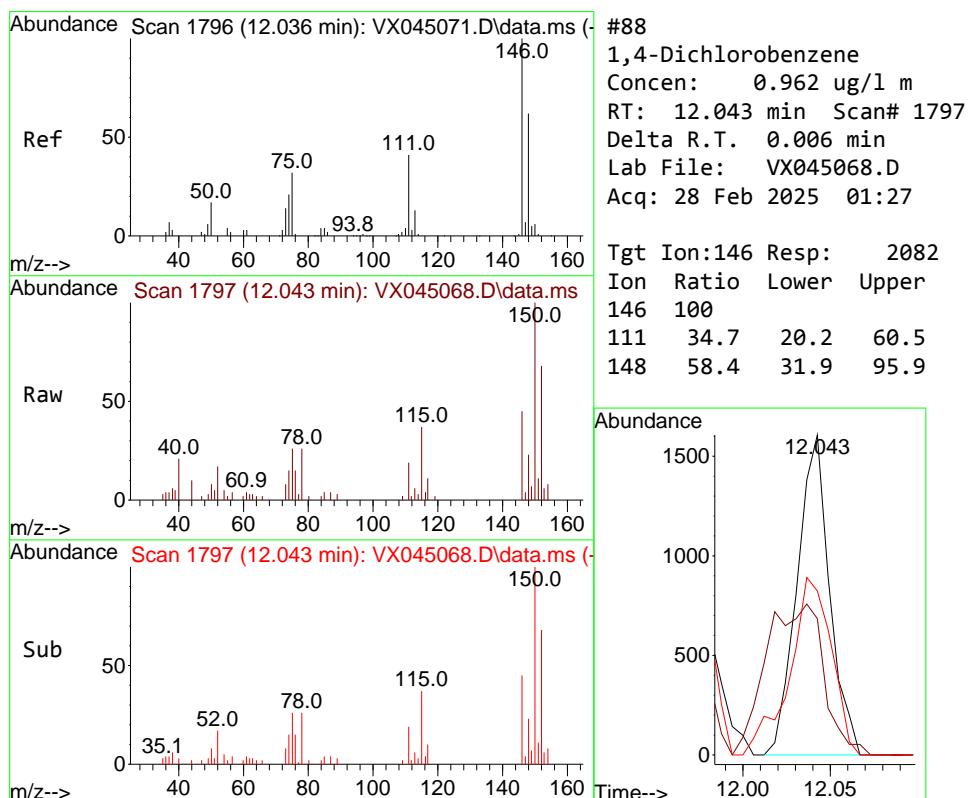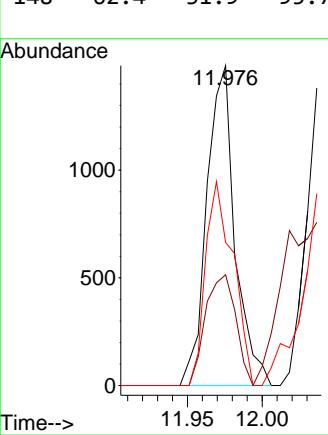

#88
1,4-Dichlorobenzene
Concen: 0.962 ug/l m
RT: 12.043 min Scan# 1797
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27


Tgt Ion:146 Resp: 2082
Ion Ratio Lower Upper
146 100
111 34.7 20.2 60.5
148 58.4 31.9 95.9

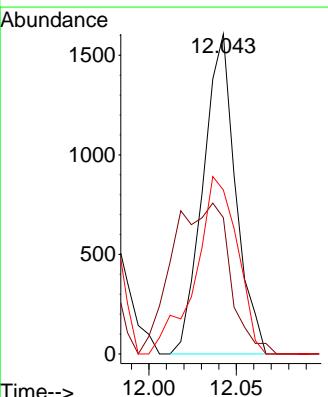



#89
n-Butylbenzene
Concen: 0.691 ug/l
RT: 12.335 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001



Tgt Ion: 91 Resp: 2470
Ion Ratio Lower Upper
91 100
92 48.0 26.7 80.0
134 21.4 12.2 36.6




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

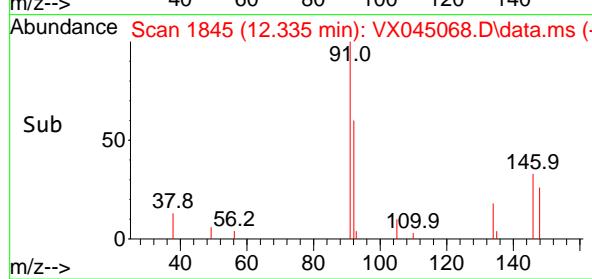

#90
Hexachloroethane
Concen: 0.805 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27


Tgt Ion:117 Resp: 609
Ion Ratio Lower Upper
117 100
201 58.9 31.9 95.9





#91
1,2-Dichlorobenzene
Concen: 0.890 ug/l
RT: 12.335 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument : MSVOA_X
ClientSampleId : VSTDICC001




Tgt Ion:146 Resp: 191:
Ion Ratio Lower Upper
146 100
111 42.0 21.6 65.0
148 66.1 31.9 95.9

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.859 ug/l
RT: 12.945 min Scan# 1945
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Tgt Ion: 75 Resp: 308
Ion Ratio Lower Upper
75 100
155 69.2 39.6 118.7
157 78.6 51.1 153.4




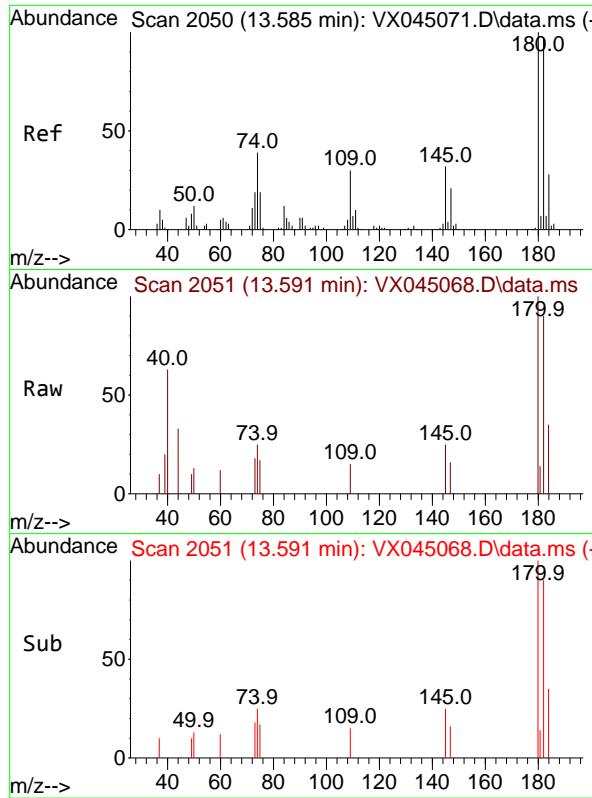


#93
 1,2,4-Trichlorobenzene
 Concen: 0.706 ug/l
 RT: 13.591 min Scan# 2
 Delta R.T. 0.006 min
 Lab File: VX045068.D
 Acq: 28 Feb 2025 01:27

Instrument : MSVOA_X
 ClientSampleId : VSTDICC001


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

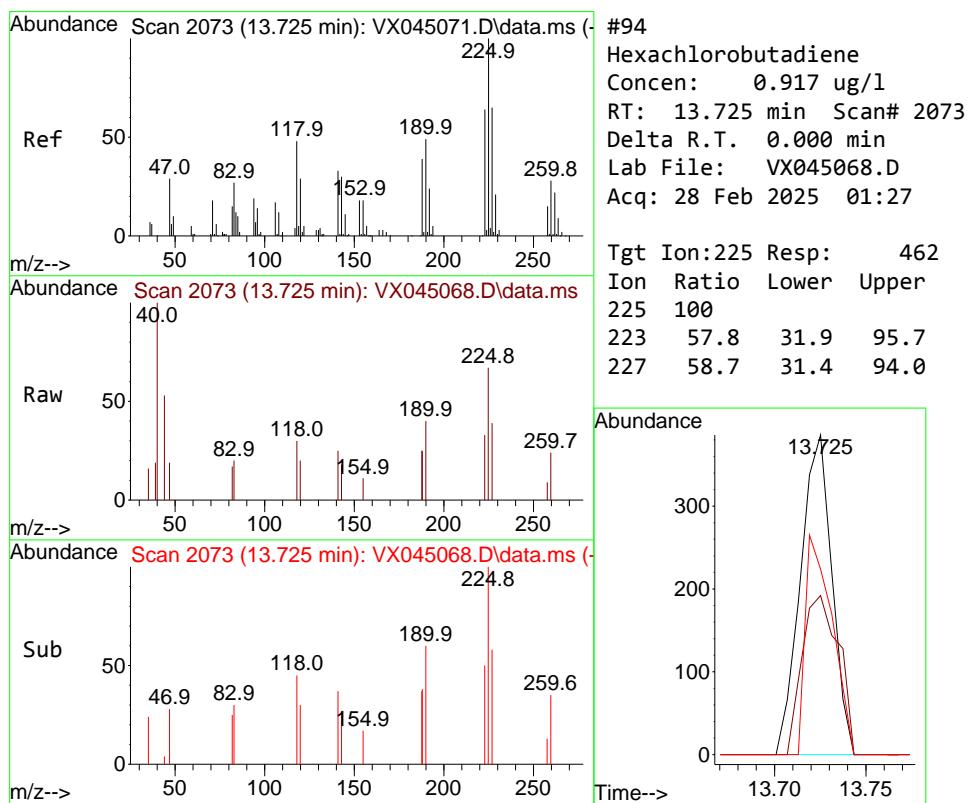

#94
 Hexachlorobutadiene
 Concen: 0.917 ug/l
 RT: 13.725 min Scan# 2073
 Delta R.T. 0.000 min
 Lab File: VX045068.D
 Acq: 28 Feb 2025 01:27


Tgt Ion:225 Resp: 462
 Ion Ratio Lower Upper
 225 100
 223 57.8 31.9 95.7
 227 58.7 31.4 94.0

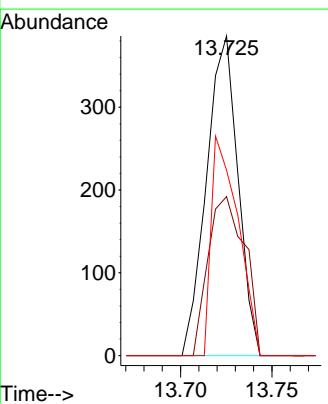

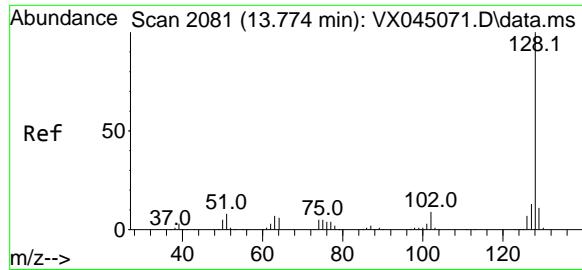

#95
Naphthalene
Concen: 0.707 ug/l
RT: 13.780 min Scan# 2111
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27




Instrument: MSVOA_X
ClientSampleId: VSTDICC001




Tgt Ion:128 Resp: 333
Ion Ratio Lower Upper
128 100
127 10.5 10.3 15.5
129 8.6 8.7 13.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

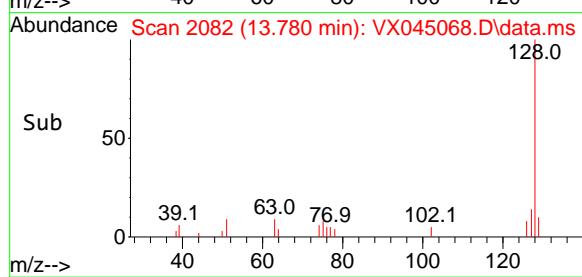

#96
1,2,3-Trichlorobenzene
Concen: 0.759 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.006 min
Lab File: VX045068.D
Acq: 28 Feb 2025 01:27



Tgt Ion:180 Resp: 969
Ion Ratio Lower Upper
180 100
182 102.3 47.5 142.6
145 29.8 17.0 50.9

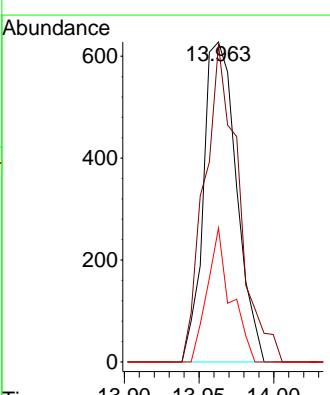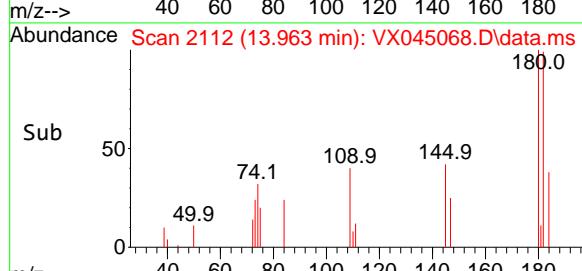

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045069.D
 Acq On : 28 Feb 2025 02:13
 Operator : JC/MD
 Sample : VSTDICC005
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC005

Quant Time: Feb 28 05:32:40 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 05:28:02 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.544	168	107391	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	194243	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	172367	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	73591	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	8978	5.659	ug/l	0.01
Spiked Amount 50.000	Range 74 - 125		Recovery	=	11.320%#	
35) Dibromofluoromethane	5.391	113	6398	5.039	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	10.080%#	
50) Toluene-d8	8.647	98	24037	5.057	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	10.120%#	
62) 4-Bromofluorobenzene	11.079	95	7436	4.685	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	9.360%#	
Target Compounds						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	6941	4.689	ug/l	96
3) Chloromethane	1.307	50	8819	4.896	ug/l	99
4) Vinyl Chloride	1.374	62	8106	4.608	ug/l	94
5) Bromomethane	1.593	94	3620	6.582	ug/l	96
6) Chloroethane	1.660	64	4517	6.746	ug/l	91
7) Trichlorofluoromethane	1.867	101	11392	5.056	ug/l	95
8) Diethyl Ether	2.136	74	4314	5.268	ug/l	99
9) 1,1,2-Trichlorotrifluo...	2.319	101	6586	4.894	ug/l	98
10) Methyl Iodide	2.441	142	6520	3.780	ug/l	95
11) Tert butyl alcohol	2.983	59	10164m	34.976	ug/l	
12) 1,1-Dichloroethene	2.313	96	6658	4.819	ug/l	94
13) Acrolein	2.233	56	8725	27.725	ug/l	97
14) Allyl chloride	2.654	41	11244	4.527	ug/l	96
15) Acrylonitrile	3.068	53	21381	27.072	ug/l	99
16) Acetone	2.386	43	19512	29.891	ug/l	97
17) Carbon Disulfide	2.502	76	16984	4.518	ug/l	99
18) Methyl Acetate	2.703	43	8964	4.559	ug/l	97
19) Methyl tert-butyl Ether	3.117	73	20546	4.651	ug/l	95
20) Methylene Chloride	2.782	84	7835	5.068	ug/l	97
21) trans-1,2-Dichloroethene	3.087	96	6651	4.895	ug/l	94
22) Diisopropyl ether	3.763	45	23151	4.875	ug/l #	82
23) Vinyl Acetate	3.721	43	88852	22.788	ug/l	98
24) 1,1-Dichloroethane	3.605	63	13132	4.949	ug/l	99
25) 2-Butanone	4.574	43	29277	27.819	ug/l	99
26) 2,2-Dichloropropane	4.471	77	6034	3.059	ug/l	97
27) cis-1,2-Dichloroethene	4.483	96	8012	4.892	ug/l	97
28) Bromochloromethane	4.904	49	6797	5.311	ug/l #	96
29) Tetrahydrofuran	5.013	42	20186	28.950	ug/l	99
30) Chloroform	5.093	83	13390	5.159	ug/l	96
31) Cyclohexane	5.464	56	10968	4.504	ug/l	95
32) 1,1,1-Trichloroethane	5.385	97	10654	4.876	ug/l	100
36) 1,1-Dichloropropene	5.690	75	8977	4.917	ug/l #	83
37) Ethyl Acetate	4.727	43	10459	5.035	ug/l	98
38) Carbon Tetrachloride	5.666	117	8997	5.013	ug/l	95
39) Methylcyclohexane	7.379	83	10291	4.414	ug/l	97
40) Benzene	6.037	78	28339	4.966	ug/l	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045069.D
 Acq On : 28 Feb 2025 02:13
 Operator : JC/MD
 Sample : VSTDICC005
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC005

Quant Time: Feb 28 05:32:40 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 05:28:02 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	5700	5.136	ug/1	95
42) 1,2-Dichloroethane	6.092	62	10189	5.510	ug/1	98
43) Isopropyl Acetate	6.348	43	15543	4.700	ug/1	99
44) Trichloroethene	7.129	130	6827	5.234	ug/1	99
45) 1,2-Dichloropropane	7.427	63	7342	5.177	ug/1	95
46) Dibromomethane	7.586	93	5146	5.195	ug/1	97
47) Bromodichloromethane	7.824	83	9773	5.100	ug/1	99
48) Methyl methacrylate	7.696	41	8201	5.224	ug/1	95
49) 1,4-Dioxane	7.665	88	3531	105.826	ug/1	95
51) 4-Methyl-2-Pentanone	8.574	43	55320	27.303	ug/1	99
52) Toluene	8.720	92	16933	4.997	ug/1	99
53) t-1,3-Dichloropropene	8.982	75	7548	3.985	ug/1	94
54) cis-1,3-Dichloropropene	8.366	75	8988	4.244	ug/1	92
55) 1,1,2-Trichloroethane	9.153	97	6759	5.151	ug/1	97
56) Ethyl methacrylate	9.116	69	9712	4.628	ug/1	98
57) 1,3-Dichloropropane	9.305	76	12106	5.289	ug/1	100
58) 2-Chloroethyl Vinyl ether	8.238	63	23212	22.527	ug/1	99
59) 2-Hexanone	9.433	43	39994	27.363	ug/1	99
60) Dibromochloromethane	9.519	129	6785	4.846	ug/1	98
61) 1,2-Dibromoethane	9.610	107	6832	5.161	ug/1	95
64) Tetrachloroethene	9.269	164	5615	5.128	ug/1	93
65) Chlorobenzene	10.079	112	18161	4.908	ug/1	97
66) 1,1,1,2-Tetrachloroethane	10.159	131	5702	4.781	ug/1	96
67) Ethyl Benzene	10.195	91	30918	4.725	ug/1	98
68) m/p-Xylenes	10.299	106	23152	9.608	ug/1	97
69) o-Xylene	10.640	106	11881	4.914	ug/1	95
70) Styrene	10.659	104	18278	4.704	ug/1	99
71) Bromoform	10.799	173	4027	4.541	ug/1 #	98
73) Isopropylbenzene	10.963	105	29685	4.991	ug/1	98
74) N-amyl acetate	10.848	43	11609	4.300	ug/1	97
75) 1,1,2,2-Tetrachloroethane	11.213	83	10881	5.310	ug/1	100
76) 1,2,3-Trichloropropane	11.238	75	8839m	5.384	ug/1	
77) Bromobenzene	11.195	156	6970	5.163	ug/1	96
78) n-propylbenzene	11.305	91	32196	4.694	ug/1	99
79) 2-Chlorotoluene	11.366	91	21253	5.048	ug/1	98
80) 1,3,5-Trimethylbenzene	11.451	105	23627	4.897	ug/1	99
81) trans-1,4-Dichloro-2-b...	11.018	75	1971	3.256	ug/1 #	83
82) 4-Chlorotoluene	11.457	91	22190	4.761	ug/1	98
83) tert-Butylbenzene	11.713	119	23960	4.910	ug/1	97
84) 1,2,4-Trimethylbenzene	11.750	105	23561	4.960	ug/1	99
85) sec-Butylbenzene	11.890	105	28314	4.687	ug/1	99
86) p-Isopropyltoluene	12.006	119	21977	4.532	ug/1	97
87) 1,3-Dichlorobenzene	11.969	146	12157	4.926	ug/1	98
88) 1,4-Dichlorobenzene	12.042	146	12526	5.014	ug/1	96
89) n-Butylbenzene	12.335	91	17358	4.072	ug/1	99
90) Hexachloroethane	12.536	117	3665	4.052	ug/1	96
91) 1,2-Dichlorobenzene	12.335	146	12477	5.138	ug/1	95
92) 1,2-Dibromo-3-Chloropr...	12.945	75	1787	4.712	ug/1	90
93) 1,2,4-Trichlorobenzene	13.591	180	6040	4.114	ug/1	97
94) Hexachlorobutadiene	13.725	225	2716	4.640	ug/1	97
95) Naphthalene	13.780	128	22927	4.287	ug/1	99
96) 1,2,3-Trichlorobenzene	13.963	180	6600	4.437	ug/1	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045069.D
Acq On : 28 Feb 2025 02:13
Operator : JC/MD
Sample : VSTDICC005
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC005

Quant Time: Feb 28 05:32:40 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 05:28:02 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carbone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045069.D
Acq On : 28 Feb 2025 02:13
Operator : JC/MD
Sample : VSTDIICC005
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC005

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

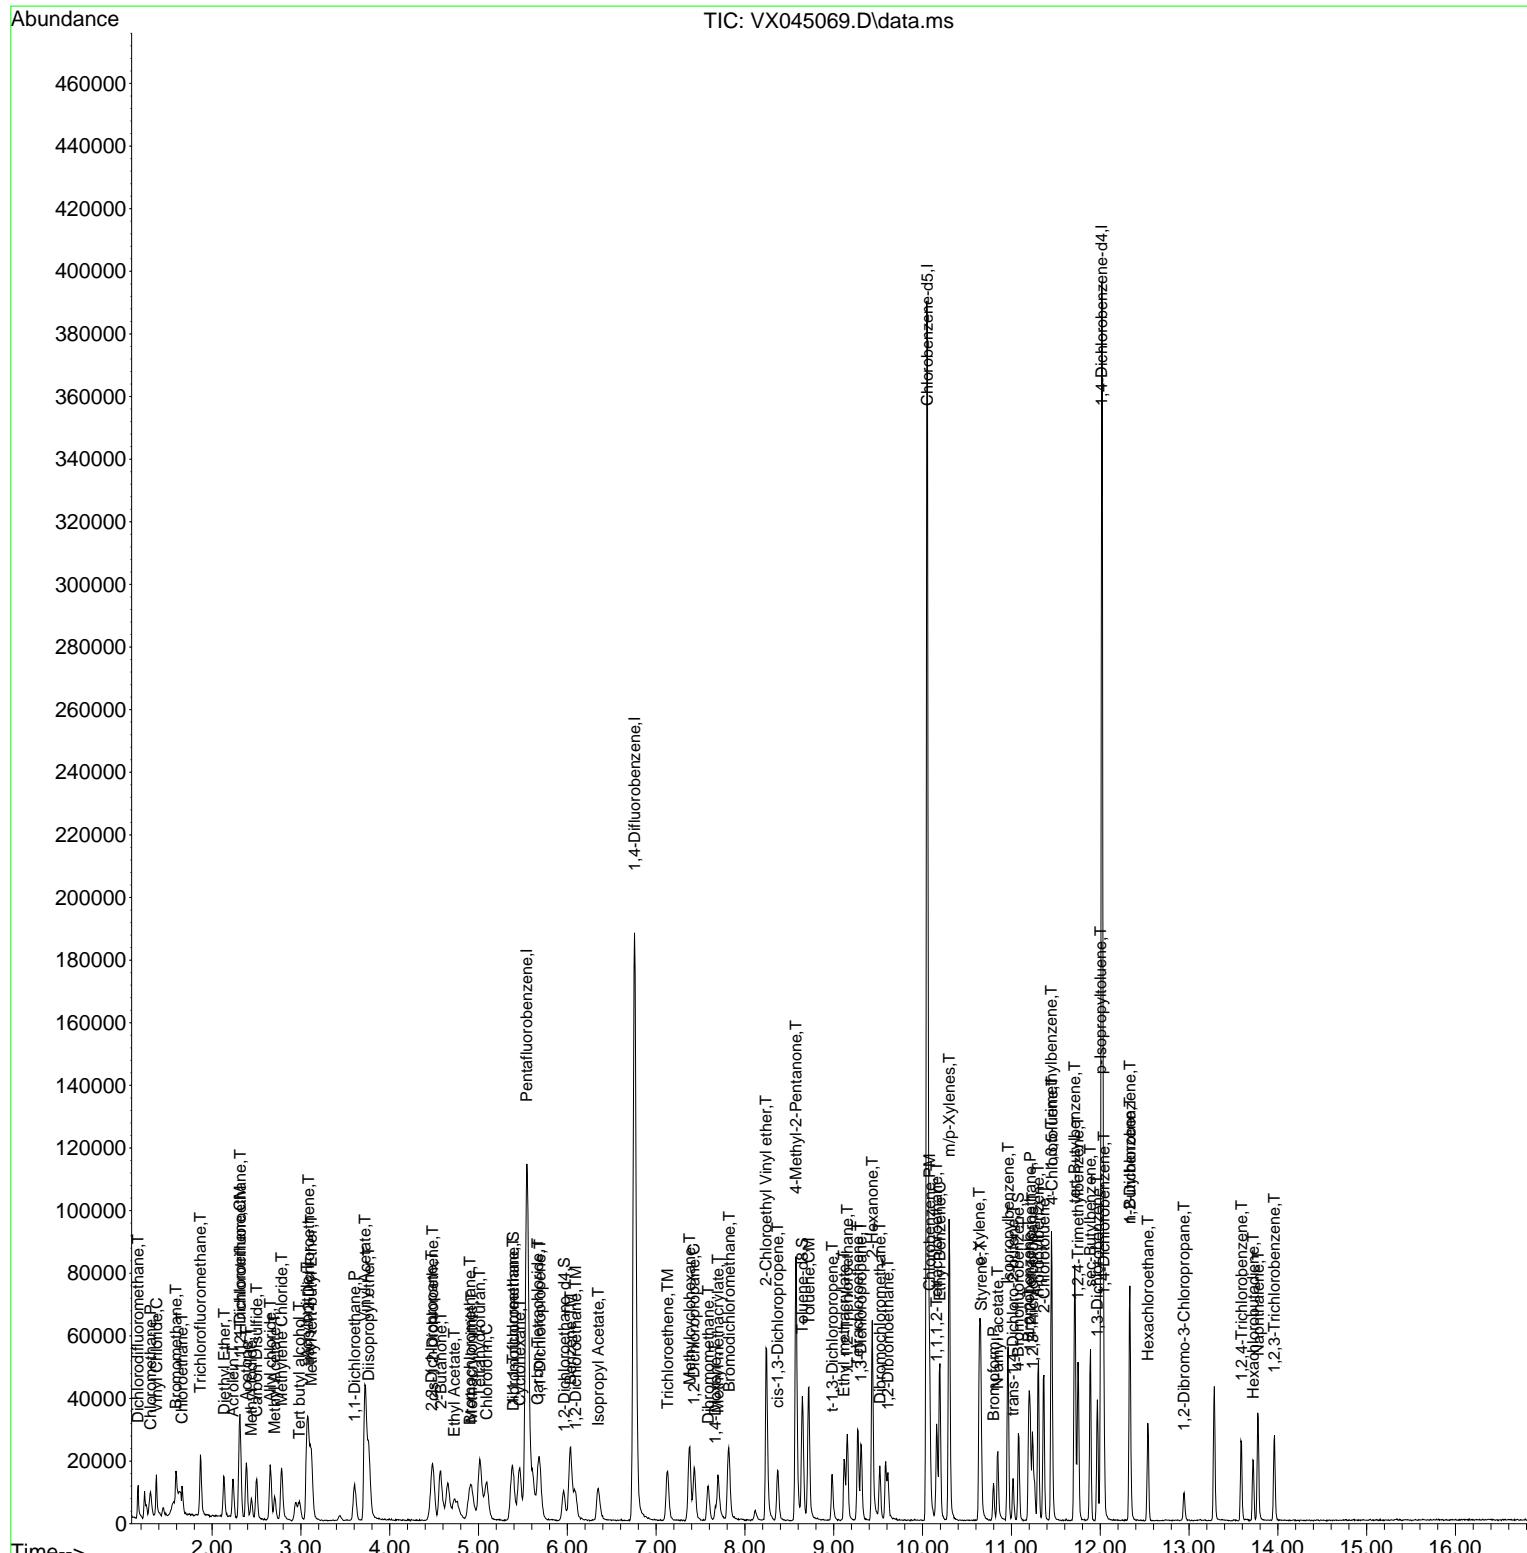



#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.544 min Scan# 7
 Delta R.T. -0.006 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
 ClientSampleId : VSTDICC005




Tgt Ion:168 Resp: 10739
 Ion Ratio Lower Upper
 168 100
 99 61.8 48.2 72.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

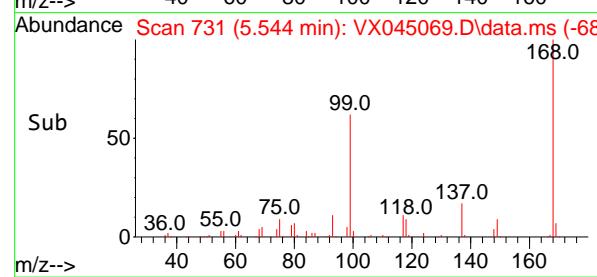


#2
 Dichlorodifluoromethane
 Concen: 4.689 ug/l
 RT: 1.166 min Scan# 13
 Delta R.T. -0.000 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13




Tgt Ion: 85 Resp: 6941
 Ion Ratio Lower Upper
 85 100
 87 32.4 17.4 52.3

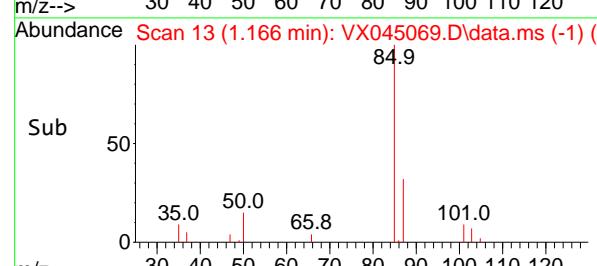



#3
Chloromethane
Concen: 4.896 ug/l
RT: 1.307 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13



Instrument: MSVOA_X
ClientSampleId: VSTDICC005




Tgt Ion: 50 Resp: 8819
Ion Ratio Lower Upper
50 100
52 30.6 25.0 37.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#4
Vinyl Chloride
Concen: 4.608 ug/l
RT: 1.374 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13



Tgt Ion: 62 Resp: 8106
Ion Ratio Lower Upper
62 100
64 33.9 24.3 36.5

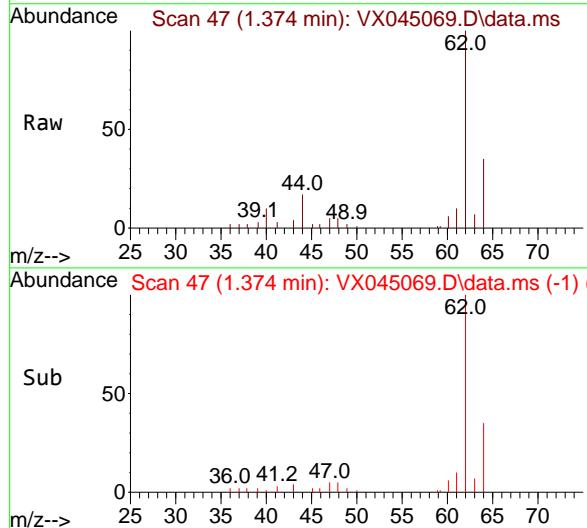


Sub 50
m/z--> 25 30 35 40 45 50 55 60 65 70



#5
Bromomethane
Concen: 6.582 ug/l
RT: 1.593 min Scan# 8
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005




Tgt Ion: 94 Resp: 3620
Ion Ratio Lower Upper
94 100
96 89.5 75.0 112.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

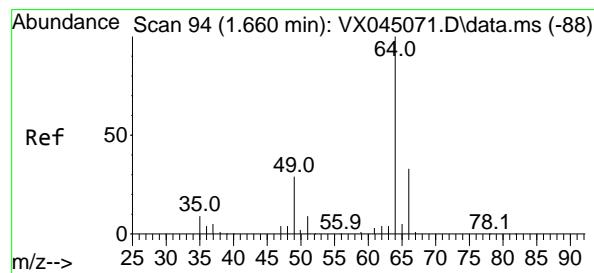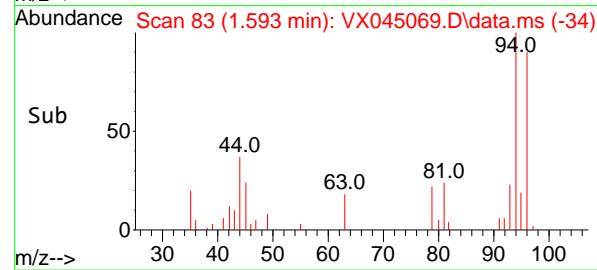


#6
Chloroethane
Concen: 6.746 ug/l
RT: 1.660 min Scan# 94
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

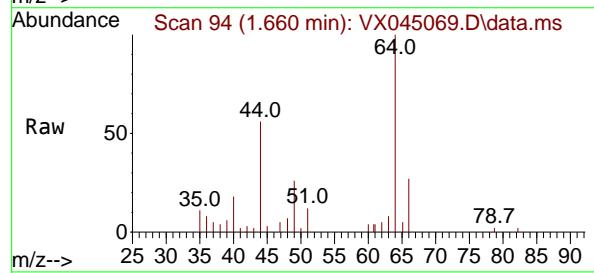


Tgt Ion: 64 Resp: 4517
Ion Ratio Lower Upper
64 100
66 28.1 26.7 40.1

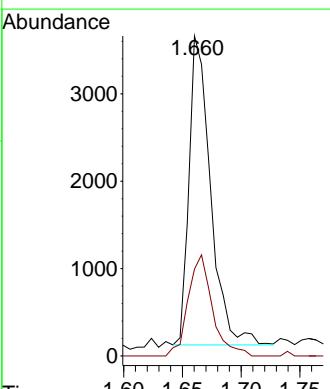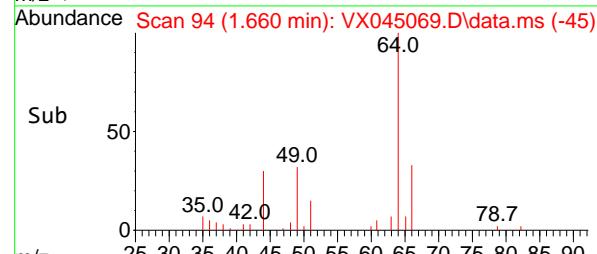



#7
Trichlorofluoromethane
Concen: 5.056 ug/l
RT: 1.867 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005




Tgt Ion: 101 Resp: 1139:
Ion Ratio Lower Upper
101 100
103 60.8 52.1 78.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#8
Diethyl Ether
Concen: 5.268 ug/l
RT: 2.136 min Scan# 172
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13



Tgt Ion: 74 Resp: 4314
Ion Ratio Lower Upper
74 100
45 101.9 51.5 154.5

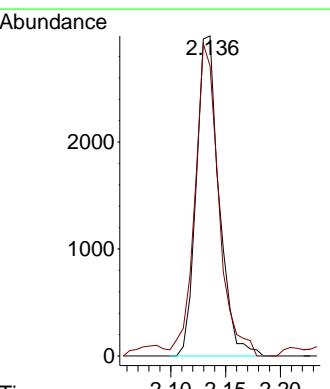


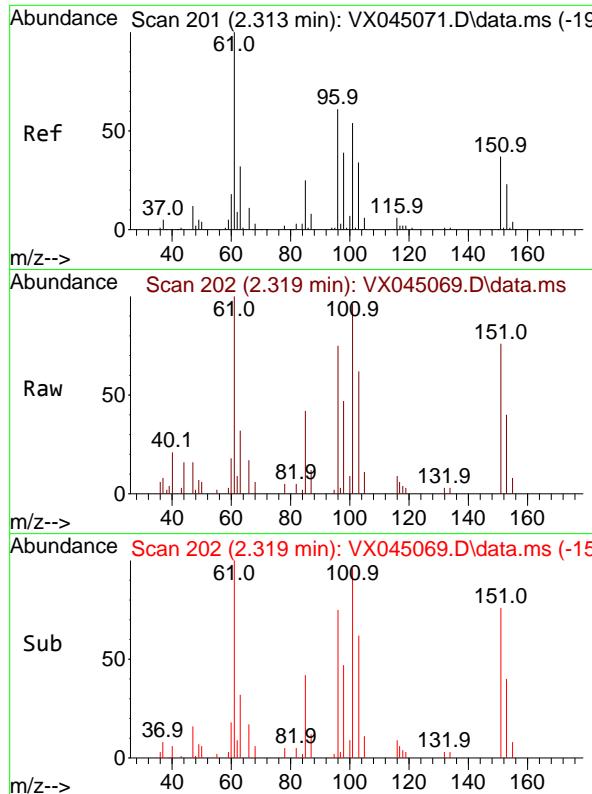


#9
 1,1,2-Trichlorotrifluoroethane
 Concen: 4.894 ug/l
 RT: 2.319 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13

Instrument : MSVOA_X
 ClientSampleId : VSTDICC005


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

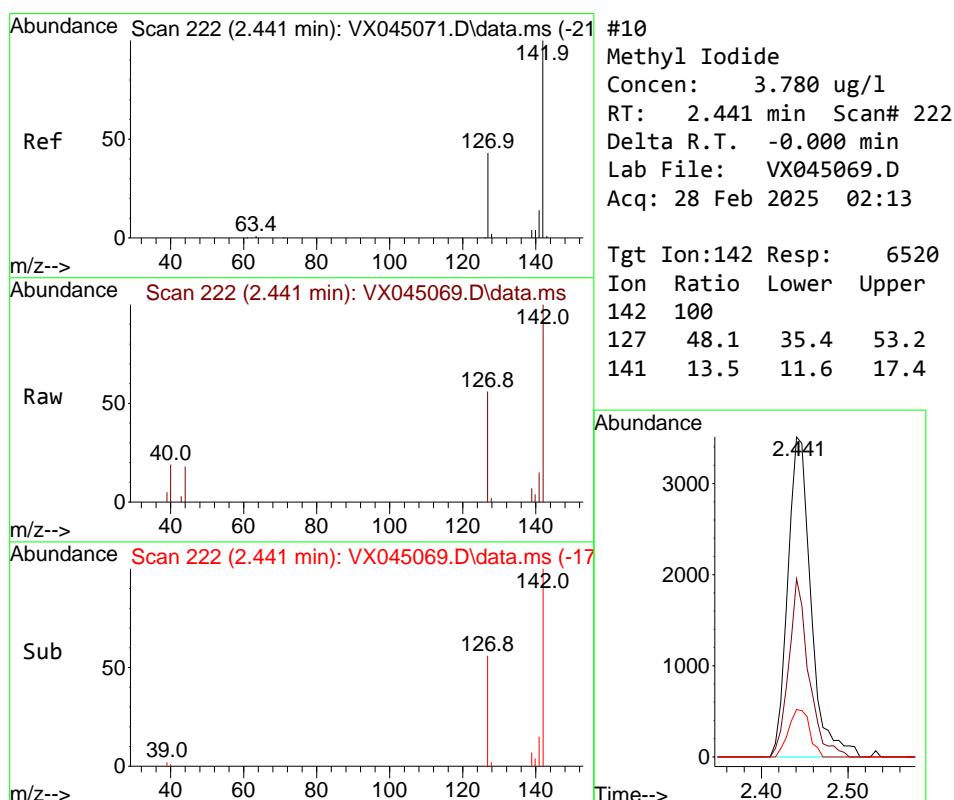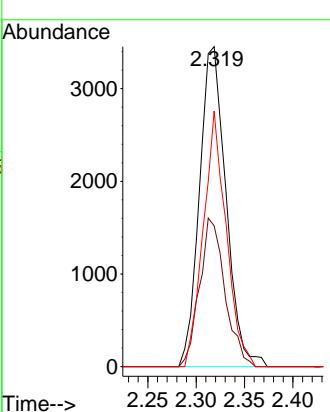

#10
 Methyl Iodide
 Concen: 3.780 ug/l
 RT: 2.441 min Scan# 222
 Delta R.T. -0.000 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13


Tgt Ion:142 Resp: 6520
 Ion Ratio Lower Upper
 142 100
 127 48.1 35.4 53.2
 141 13.5 11.6 17.4

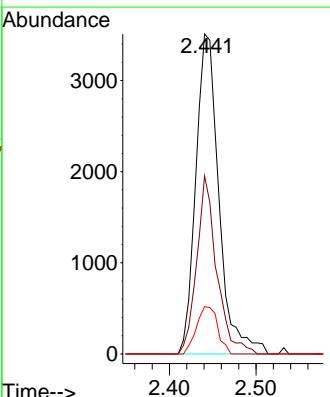



#11
Tert butyl alcohol
Concen: 34.976 ug/l m
RT: 2.983 min Scan# 311
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument: MSVOA_X
ClientSampleId: VSTDICC005




Tgt Ion: 59 Resp: 10164
Ion Ratio Lower Upper
59 100
57 7.2 7.8 11.8

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

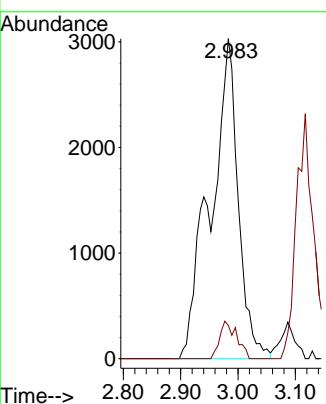


#12
1,1-Dichloroethene
Concen: 4.819 ug/l
RT: 2.313 min Scan# 201
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Tgt Ion: 96 Resp: 6658
Ion Ratio Lower Upper
96 100
61 157.3 134.6 202.0
98 64.3 51.0 76.6

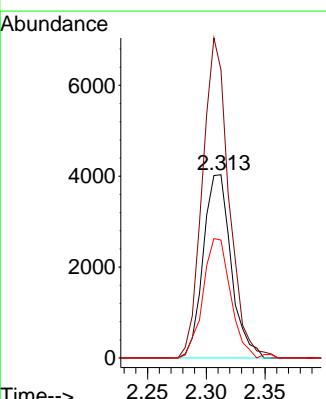

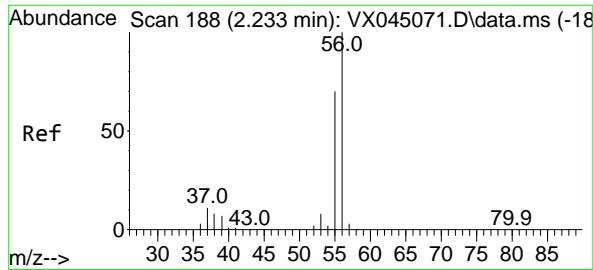




#13
Acrolein
Concen: 27.725 ug/l
RT: 2.233 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13
Instrument : MSVOA_X
ClientSampleId : VSTDICC005

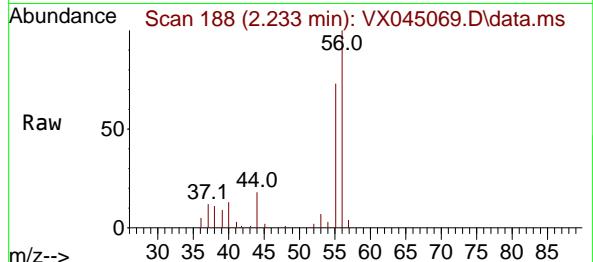


Tgt Ion: 56 Resp: 8725
Ion Ratio Lower Upper
56 100
55 72.4 56.2 84.4

**Manual Integrations
APPROVED**



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

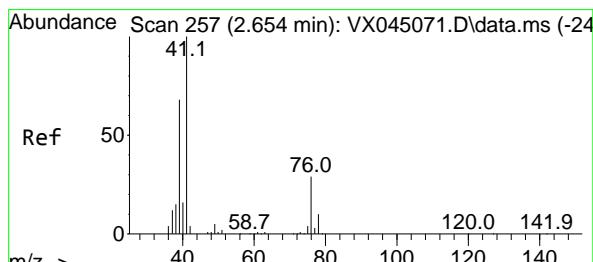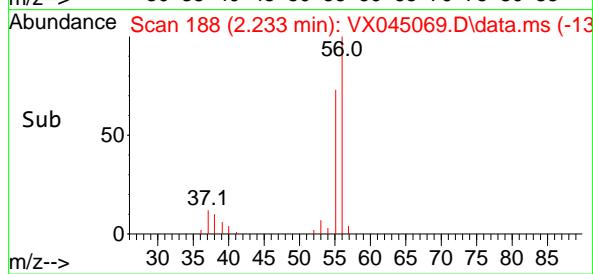


#14
Allyl chloride
Concen: 4.527 ug/l
RT: 2.654 min Scan# 257
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

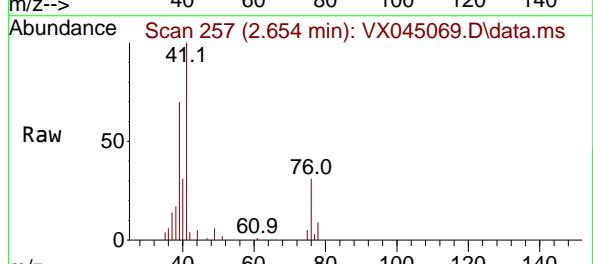


Tgt Ion: 41 Resp: 11244
Ion Ratio Lower Upper
41 100
39 70.8 53.8 80.8
76 30.4 25.2 37.8

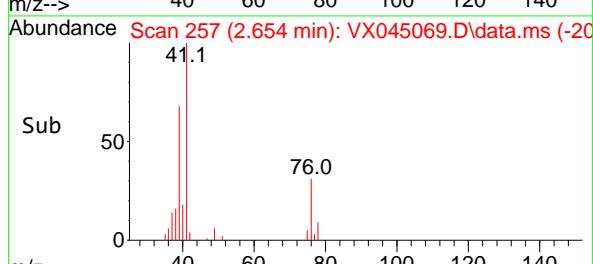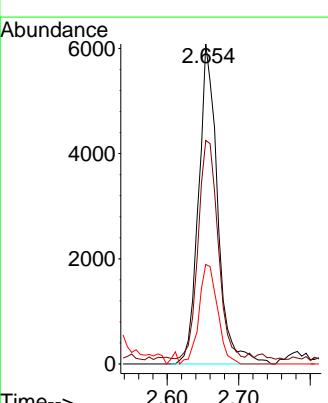



#15
Acrylonitrile
Concen: 27.072 ug/l
RT: 3.068 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13



Instrument : MSVOA_X
ClientSampleId : VSTDICC005




Tgt Ion: 53 Resp: 2138
Ion Ratio Lower Upper
53 100
52 81.1 66.2 99.2
51 36.7 29.0 43.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#16
Acetone
Concen: 29.891 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

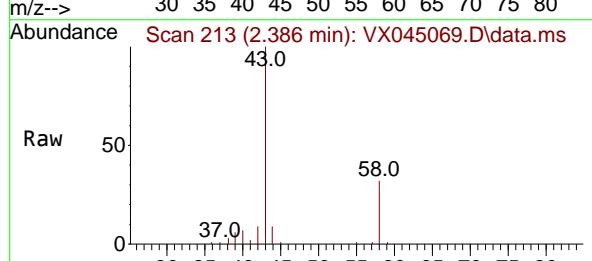


Tgt Ion: 43 Resp: 19512
Ion Ratio Lower Upper
43 100
58 32.1 24.2 36.4

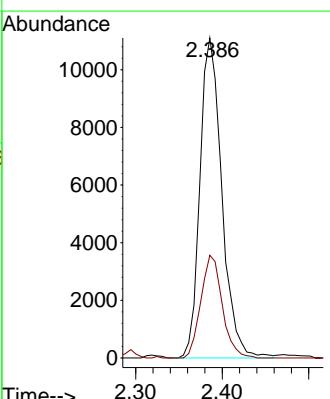



#17
Carbon Disulfide
Concen: 4.518 ug/l
RT: 2.502 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13



Instrument : MSVOA_X
ClientSampleId : VSTDICC005

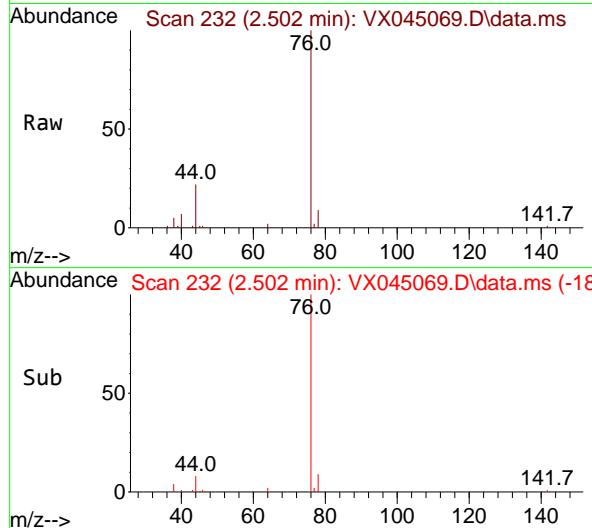

Tgt Ion: 76 Resp: 16984
Ion Ratio Lower Upper
76 100
78 8.5 6.6 9.8




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

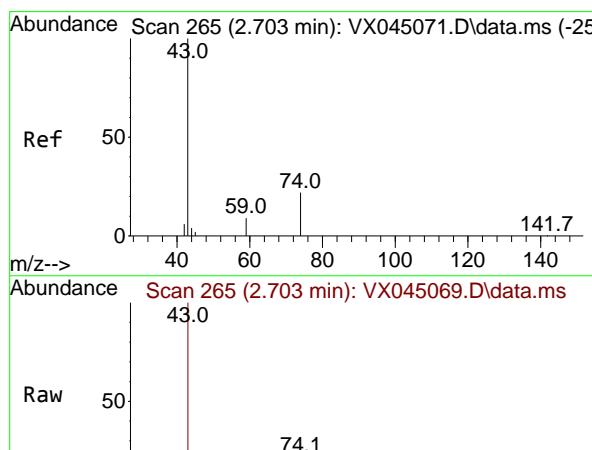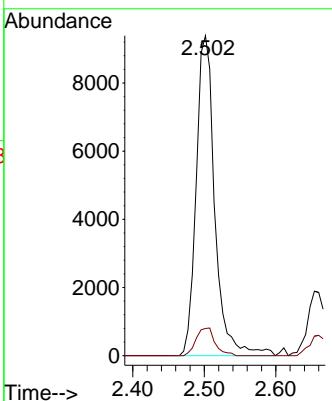

#18
Methyl Acetate
Concen: 4.559 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Tgt Ion: 43 Resp: 8964
Ion Ratio Lower Upper
43 100
74 23.3 17.4 26.2

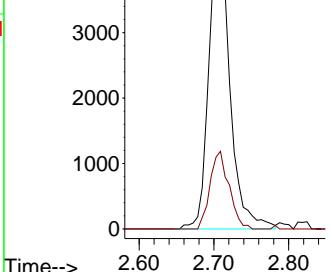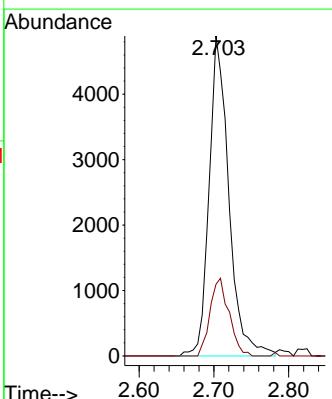


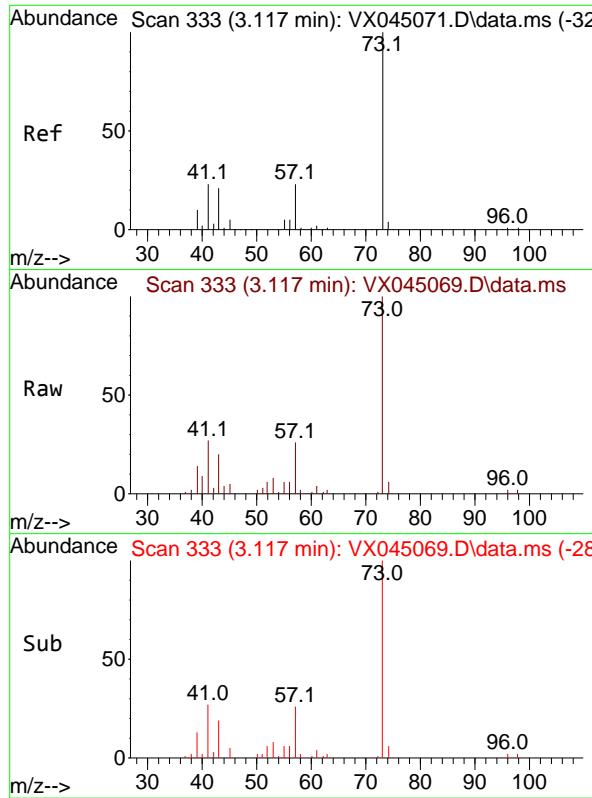


#19
Methyl tert-butyl Ether
Concen: 4.651 ug/l
RT: 3.117 min Scan# 319
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Instrument : MSVOA_X
ClientSampleId : VSTDICC005


Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

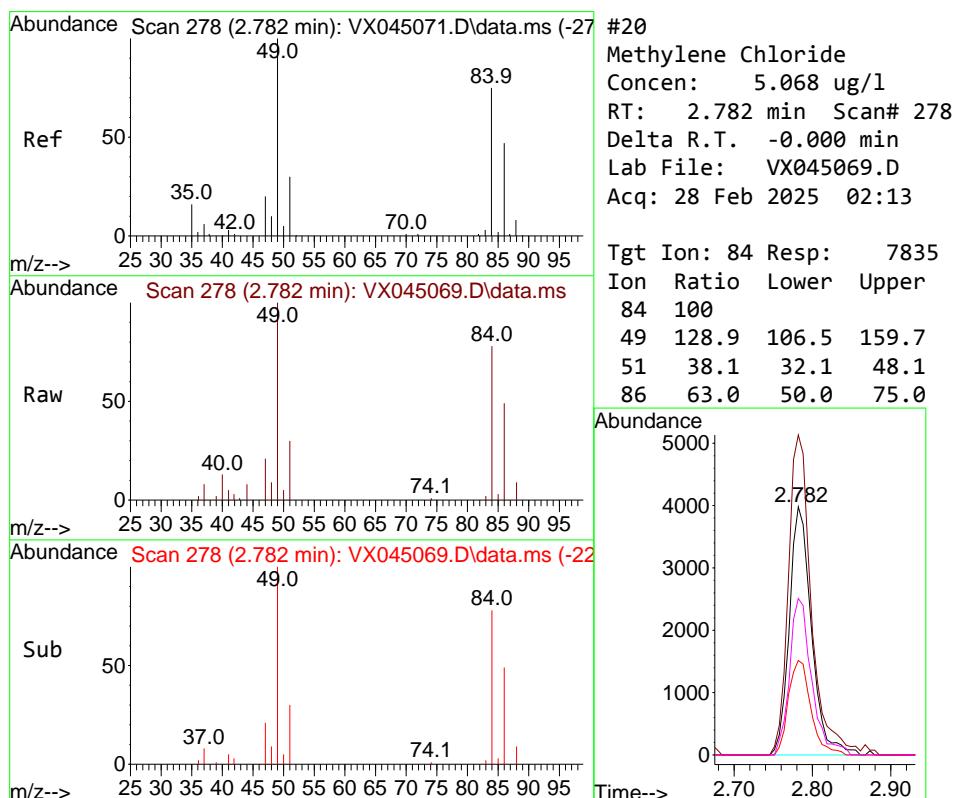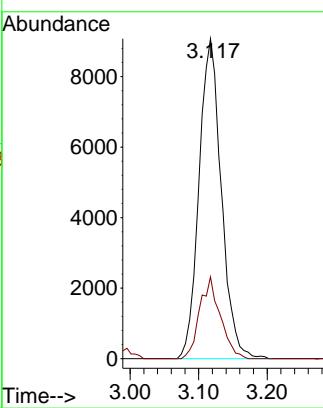

#20
Methylene Chloride
Concen: 5.068 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13


Tgt Ion: 84 Resp: 7835
Ion Ratio Lower Upper
84 100
49 128.9 106.5 159.7
51 38.1 32.1 48.1
86 63.0 50.0 75.0

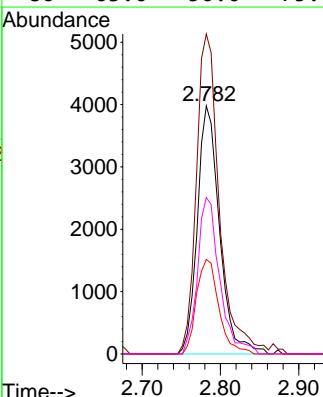



#21
trans-1,2-Dichloroethene
Concen: 4.895 ug/l
RT: 3.087 min Scan# 31
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005




Tgt Ion: 96 Resp: 665:
Ion Ratio Lower Upper
96 100
61 137.2 117.0 175.4
98 64.1 53.4 80.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#22
Diisopropyl ether
Concen: 4.875 ug/l
RT: 3.763 min Scan# 439
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Tgt Ion: 45 Resp: 23151
Ion Ratio Lower Upper
45 100
43 90.2 54.9 82.3#
87 25.1 21.0 31.4
59 10.9 8.7 13.1

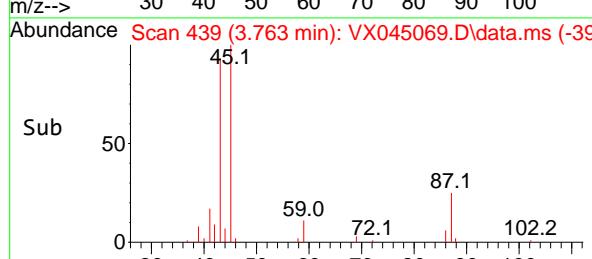






#23
Vinyl Acetate
Concen: 22.788 ug/l
RT: 3.721 min Scan# 413
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13
Instrument: MSVOA_X
ClientSampleId: VSTDICC005




Tgt Ion: 43 Resp: 88852
Ion Ratio Lower Upper
43 100
86 10.7 8.1 12.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#24
1,1-Dichloroethane
Concen: 4.949 ug/l
RT: 3.605 min Scan# 413
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Tgt Ion: 63 Resp: 13132
Ion Ratio Lower Upper
63 100
98 7.0 3.4 10.2
100 5.1 2.1 6.5

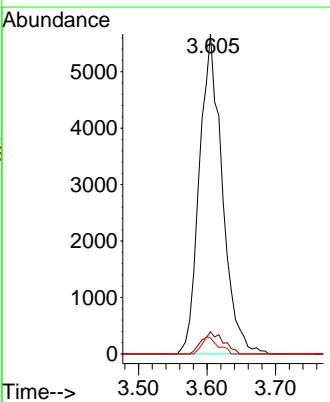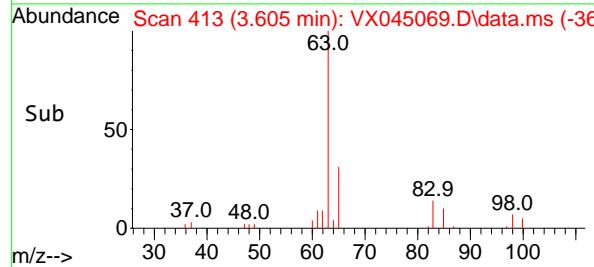

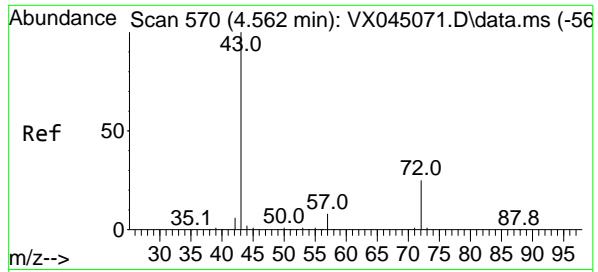

#25
2-Butanone
Concen: 27.819 ug/l
RT: 4.574 min Scan# 5
Delta R.T. 0.012 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC005



Tgt Ion: 43 Resp: 2927
Ion Ratio Lower Upper
43 100
72 25.7 20.0 30.0




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

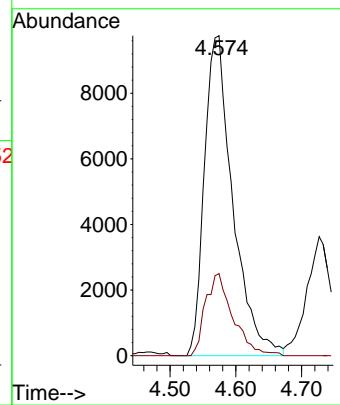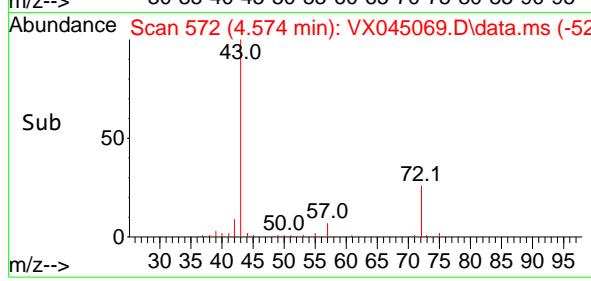


#26
2,2-Dichloropropane
Concen: 3.059 ug/l
RT: 4.471 min Scan# 555
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Tgt Ion: 77 Resp: 6034
Ion Ratio Lower Upper
77 100
97 26.0 12.4 37.0

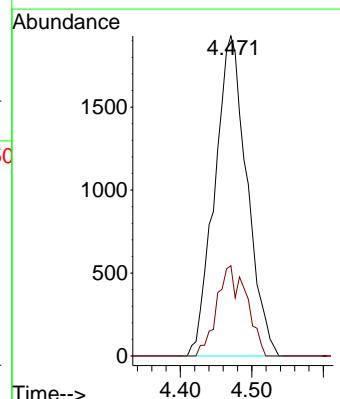



#27
 cis-1,2-Dichloroethene
 Concen: 4.892 ug/l
 RT: 4.483 min Scan# 5
 Delta R.T. -0.000 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13






Tgt Ion: 96 Resp: 801
 Ion Ratio Lower Upper


96	100
61	146.1
98	62.0

Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025



#28
 Bromochloromethane
 Concen: 5.311 ug/l
 RT: 4.904 min Scan# 626
 Delta R.T. 0.006 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13






Tgt Ion: 49 Resp: 6797
 Ion Ratio Lower Upper

49	100
----	-----


129	0.0	0.0	3.4
-----	-----	-----	-----

130	66.5	56.1	84.1
-----	------	------	------








#29
Tetrahydrofuran
Concen: 28.950 ug/l
RT: 5.013 min Scan# 61
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

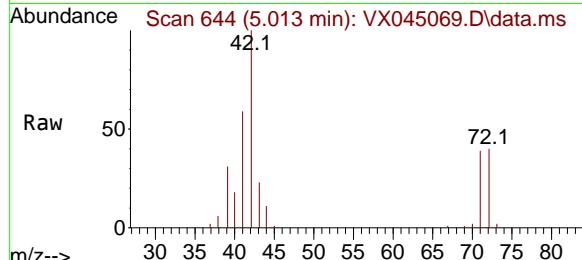


Tgt Ion: 42 Resp: 20180
Ion Ratio Lower Upper
42 100
72 41.2 34.1 51.1
71 39.3 31.4 47.0

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

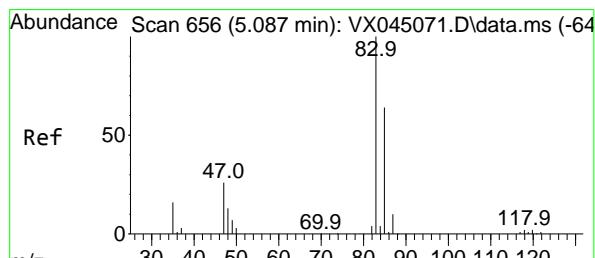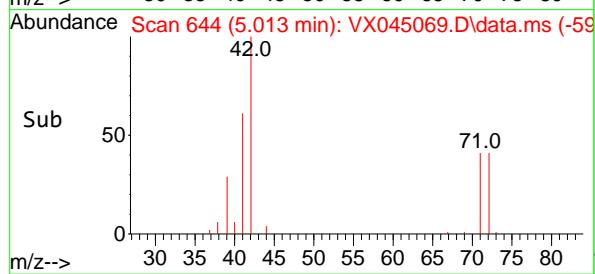


#30
Chloroform
Concen: 5.159 ug/l
RT: 5.093 min Scan# 657
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

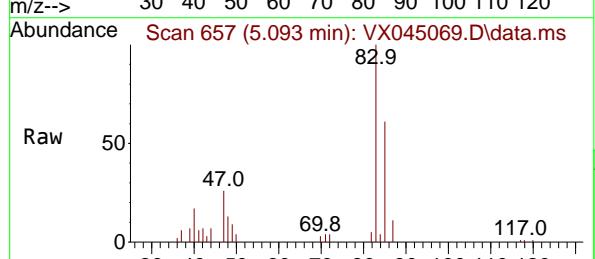


Tgt Ion: 83 Resp: 13390
Ion Ratio Lower Upper
83 100
85 61.5 51.4 77.2

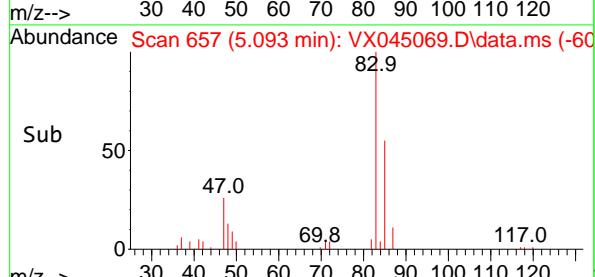






#31
Cyclohexane
Concen: 4.504 ug/l
RT: 5.464 min Scan# 7
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13
Instrument: MSVOA_X
ClientSampleId: VSTDICC005




Tgt Ion: 56 Resp: 10963
Ion Ratio Lower Upper
56 100
69 33.0 23.4 35.2
84 83.1 69.4 104.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

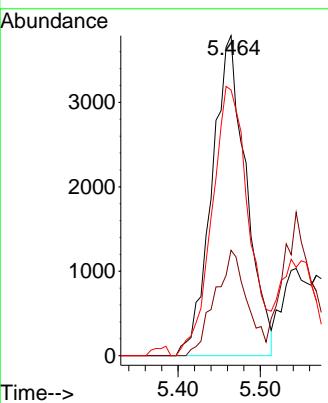


#32
1,1,1-Trichloroethane
Concen: 4.876 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Tgt Ion: 97 Resp: 10654
Ion Ratio Lower Upper
97 100
99 64.5 51.6 77.4
61 48.7 38.4 57.6

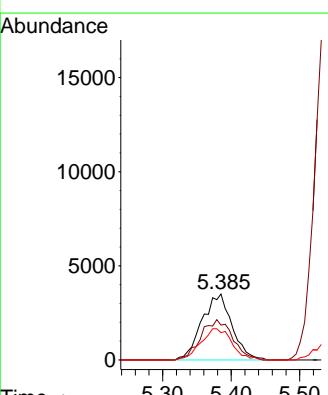



#33
1,2-Dichloroethane-d4
Concen: 5.659 ug/l
RT: 5.964 min Scan# 8
Delta R.T. 0.012 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005




Tgt Ion: 65 Resp: 897:
Ion Ratio Lower Upper
65 100
67 50.5 0.0 106.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

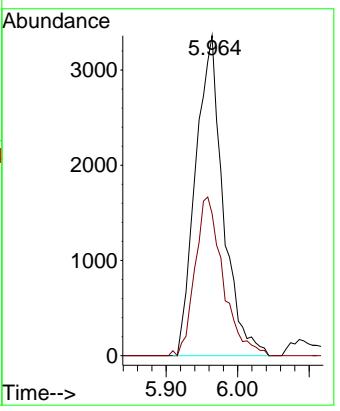


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Tgt Ion:114 Resp: 194243
Ion Ratio Lower Upper
114 100
63 22.1 0.0 41.8
88 16.4 0.0 32.8

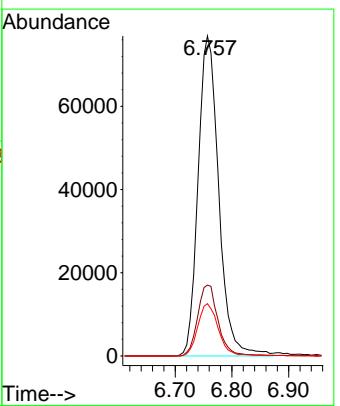



#35
Dibromofluoromethane
Concen: 5.039 ug/l
RT: 5.391 min Scan# 7
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC005

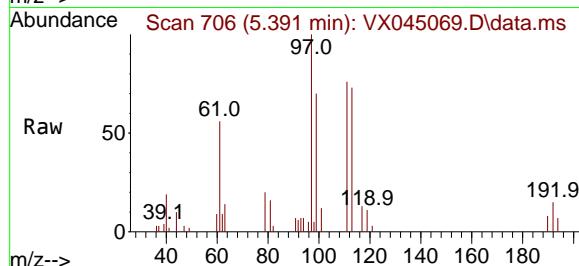


Tgt Ion:113 Resp: 639:
Ion Ratio Lower Upper
113 100
111 103.9 81.8 122.6
192 18.3 14.3 21.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#36
1,1-Dichloropropene
Concen: 4.917 ug/l
RT: 5.690 min Scan# 755
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Tgt Ion: 75 Resp: 8977
Ion Ratio Lower Upper
75 100
110 31.8 16.9 50.6
77 13.2 24.5 36.7#

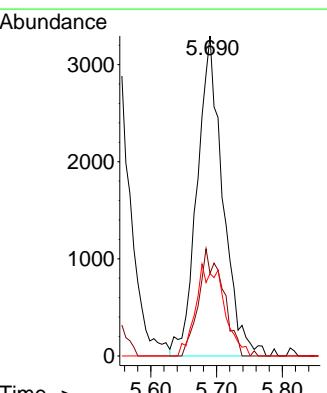

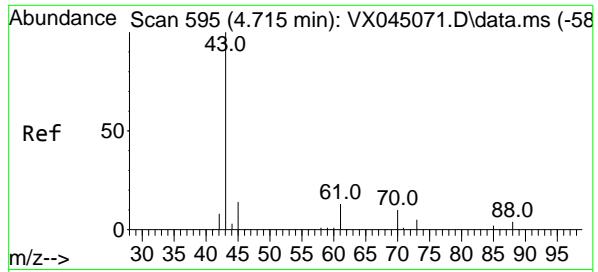

#37
Ethyl Acetate
 Concen: 5.035 ug/l
 RT: 4.727 min Scan# 51
 Delta R.T. 0.012 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
 ClientSampleId : VSTDICC005

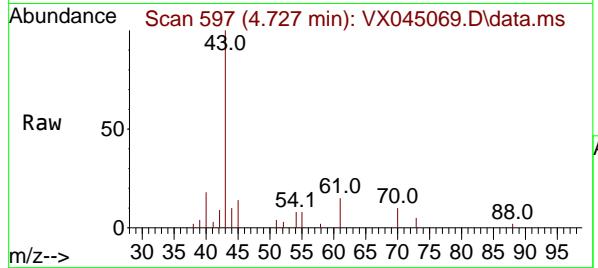

Tgt Ion: 43 Resp: 10459
 Ion Ratio Lower Upper
 43 100
 61 14.4 10.8 16.2
 70 10.2 7.7 11.5




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

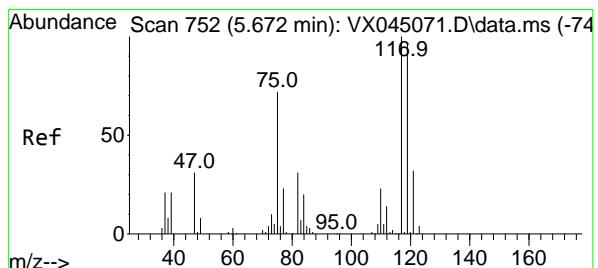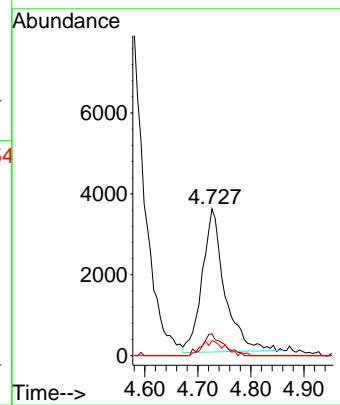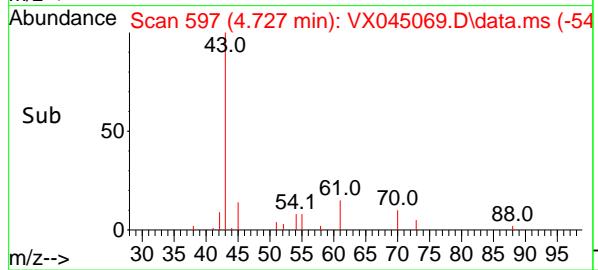

#38
Carbon Tetrachloride
 Concen: 5.013 ug/l
 RT: 5.666 min Scan# 751
 Delta R.T. -0.006 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13

Tgt Ion:117 Resp: 8997
 Ion Ratio Lower Upper
 117 100
 119 92.0 76.7 115.1
 121 27.2 25.5 38.3

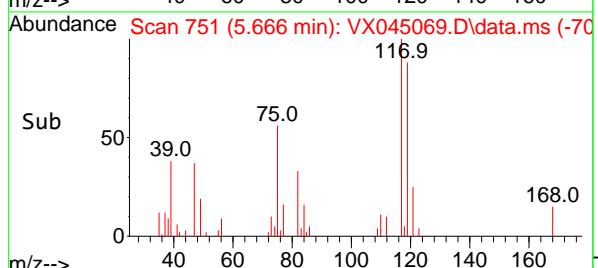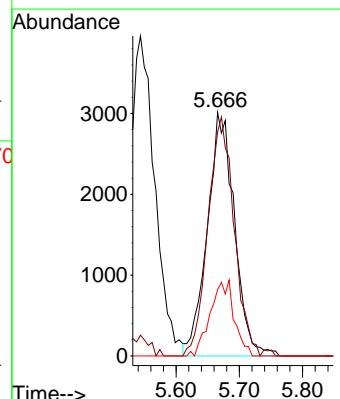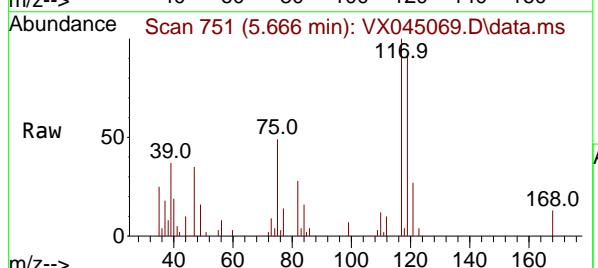







#39
Methylcyclohexane
Concen: 4.414 ug/l
RT: 7.379 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Instrument : MSVOA_X
ClientSampleId : VSTDICC005

Tgt Ion: 83 Resp: 10291
Ion Ratio Lower Upper
83 100
55 76.4 63.0 94.4
98 47.9 39.7 59.5




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#40
Benzene
Concen: 4.966 ug/l
RT: 6.037 min Scan# 812
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13


Tgt Ion: 78 Resp: 28339
Ion Ratio Lower Upper
78 100
77 22.1 18.8 28.2

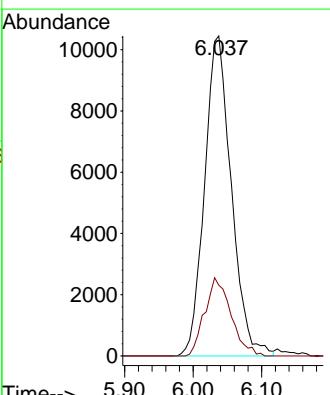



#41
Methacrylonitrile
Concen: 5.136 ug/l
RT: 4.922 min Scan# 61
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005



Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
41	100	5700		
39	53.3	44.6	67.0	
67	73.4	53.9	80.9	
52	30.5	23.3	34.9	




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#42
1,2-Dichloroethane
Concen: 5.510 ug/l
RT: 6.092 min Scan# 821
Delta R.T. 0.012 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13


Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
62	100	10189		
98	8.5	0.0	18.2	





#43
Isopropyl Acetate
Concen: 4.700 ug/l
RT: 6.348 min Scan# 8
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005

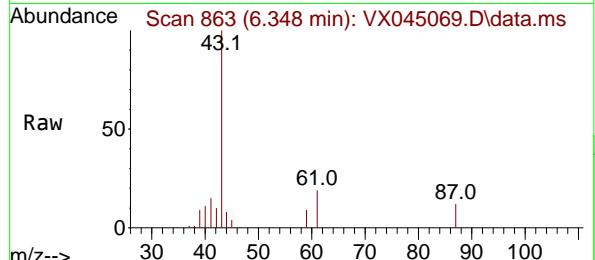


Tgt Ion: 43 Resp: 1554
Ion Ratio Lower Upper
43 100
61 19.0 14.9 22.3
87 12.1 9.4 14.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

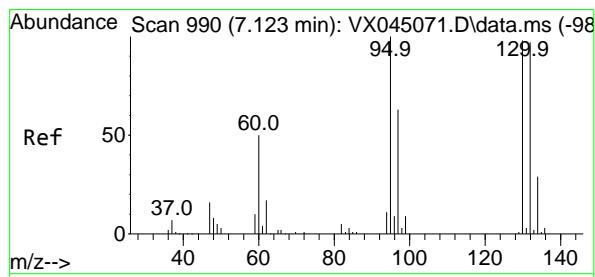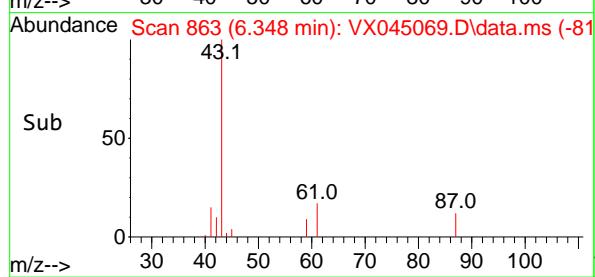


#44
Trichloroethene
Concen: 5.234 ug/l
RT: 7.129 min Scan# 991
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

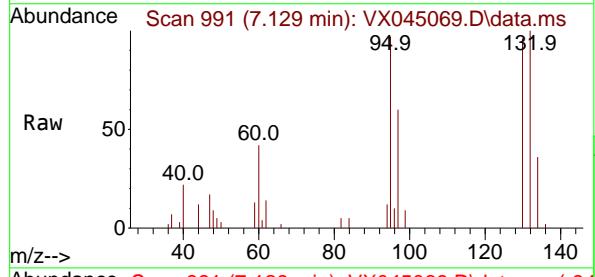


Tgt Ion:130 Resp: 6827
Ion Ratio Lower Upper
130 100
95 101.2 0.0 205.0

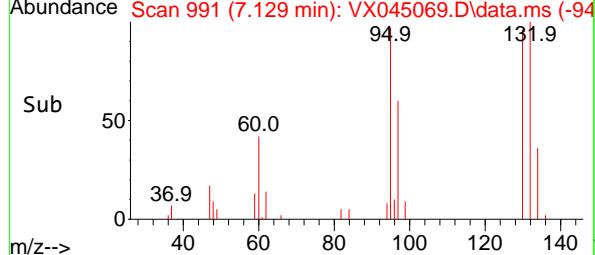



#45
1,2-Dichloropropane
Concen: 5.177 ug/l
RT: 7.427 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC005




Tgt Ion: 63 Resp: 734:
Ion Ratio Lower Upper
63 100
65 33.4 24.7 37.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#46
Dibromomethane
Concen: 5.195 ug/l
RT: 7.586 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Tgt Ion: 93 Resp: 5146
Ion Ratio Lower Upper
93 100
95 86.2 65.8 98.8
174 88.2 72.2 108.2





#47
 Bromodichloromethane
 Concen: 5.100 ug/l
 RT: 7.824 min Scan# 1
 Delta R.T. 0.006 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
 ClientSampleId : VSTDICC005



Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
83	100	977		
85	63.3	51.1	76.7	
127	8.0	6.4	9.6	




Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

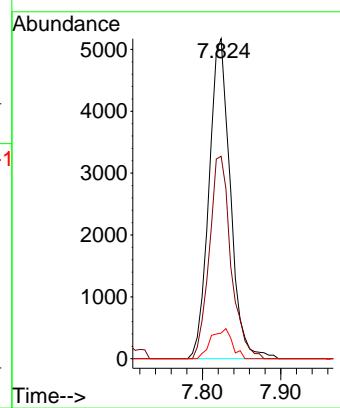

#48
 Methyl methacrylate
 Concen: 5.224 ug/l
 RT: 7.696 min Scan# 1084
 Delta R.T. 0.006 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13


Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
41	100	8201		
69	74.0	63.0	94.6	
39	55.4	47.5	71.3	

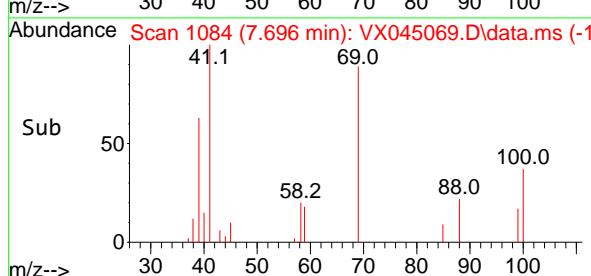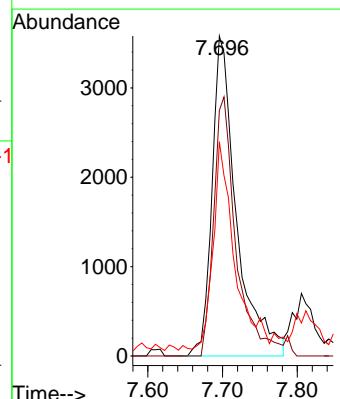



#49
1,4-Dioxane
Concen: 105.826 ug/l
RT: 7.665 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005



Tgt Ion: 88 Resp: 353:
Ion Ratio Lower Upper
88 100
43 35.2 28.7 43.1
58 75.9 55.8 83.8



Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

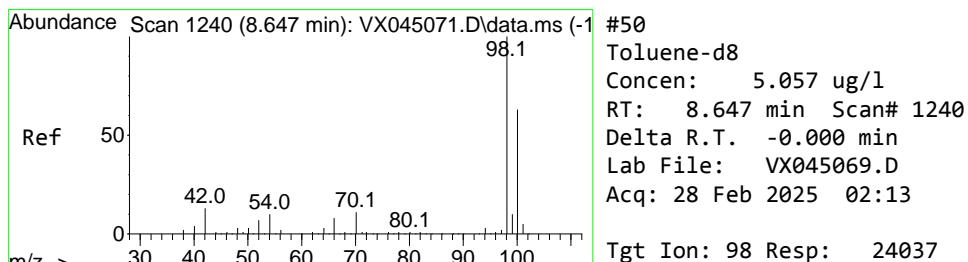

#50
Toluene-d8
Concen: 5.057 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13


Tgt Ion: 98 Resp: 24037
Ion Ratio Lower Upper
98 100
100 64.6 52.0 78.0

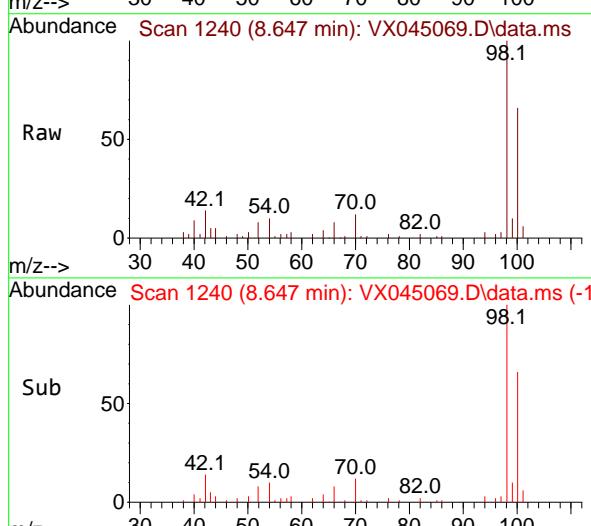



#51
4-Methyl-2-Pentanone
Concen: 27.303 ug/l
RT: 8.574 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005




Tgt Ion: 43 Resp: 55320
Ion Ratio Lower Upper
43 100
58 36.8 29.2 43.8

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#52
Toluene
Concen: 4.997 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Tgt Ion: 92 Resp: 16933
Ion Ratio Lower Upper
92 100
91 172.6 138.9 208.3

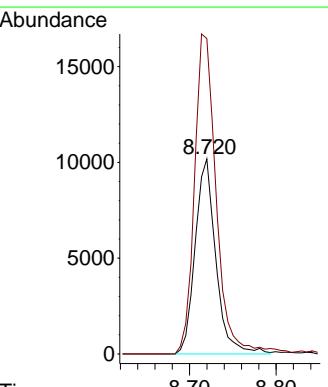

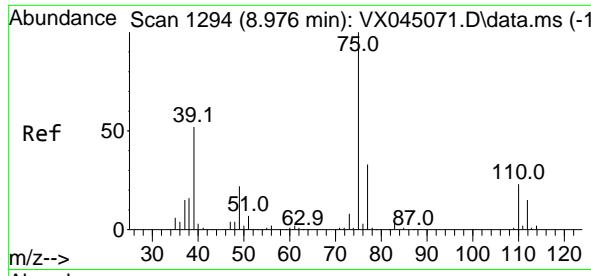

#53
t-1,3-Dichloropropene
Concen: 3.985 ug/l
RT: 8.982 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005




Tgt Ion: 75 Resp: 7543
Ion Ratio Lower Upper
75 100
77 29.6 26.5 39.7

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#54
cis-1,3-Dichloropropene
Concen: 4.244 ug/l
RT: 8.366 min Scan# 1194
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Tgt Ion: 75 Resp: 8988
Ion Ratio Lower Upper
75 100
77 27.0 24.7 37.1
39 57.0 40.7 61.1





#55
1,1,2-Trichloroethane
Concen: 5.151 ug/l
RT: 9.153 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005



Tgt Ion:	Ion Ratio	Resp:	6759
97	100		
83	83.7	Lower	69.4
85	53.6	Upper	104.2
99	61.3		44.1
			66.1
			50.7
			76.1




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

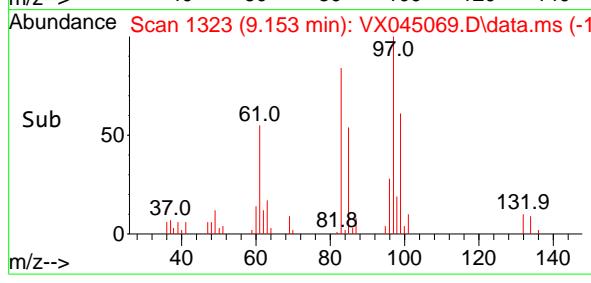

#56
Ethyl methacrylate
Concen: 4.628 ug/l
RT: 9.116 min Scan# 1317
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13


Tgt Ion:	Ion Ratio	Resp:	9712
69	100		
41	71.0	Lower	57.0
39	39.2	Upper	85.4
			34.2
			51.4





#57
1,3-Dichloropropane
Concen: 5.289 ug/l
RT: 9.305 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13



Instrument : MSVOA_X
ClientSampleId : VSTDICC005

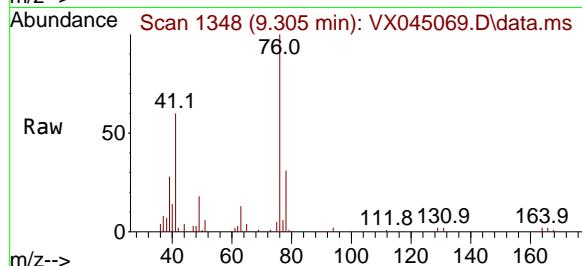

Tgt Ion: 76 Resp: 12100
Ion Ratio Lower Upper
76 100
78 31.9 25.5 38.3



Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#58
2-Chloroethyl Vinyl ether
Concen: 22.527 ug/l
RT: 8.238 min Scan# 1173
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Tgt Ion: 63 Resp: 23212
Ion Ratio Lower Upper
63 100
106 27.4 21.5 32.3

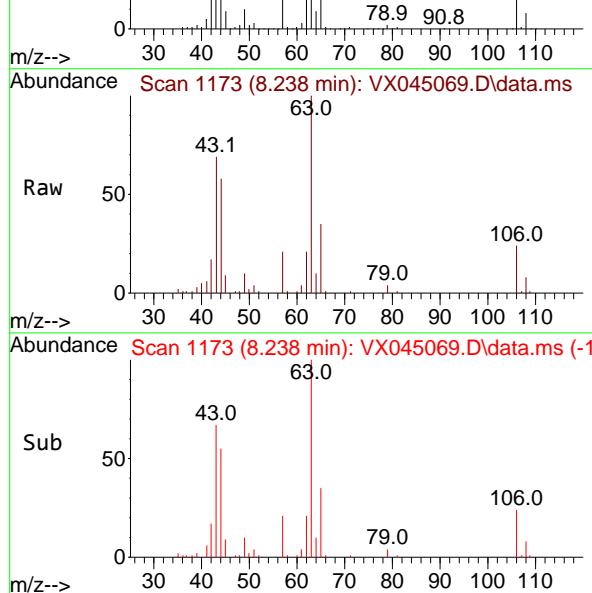


Abundance Scan 1173 (8.238 min): VX045069.D\data.ms (-1)

m/z-->

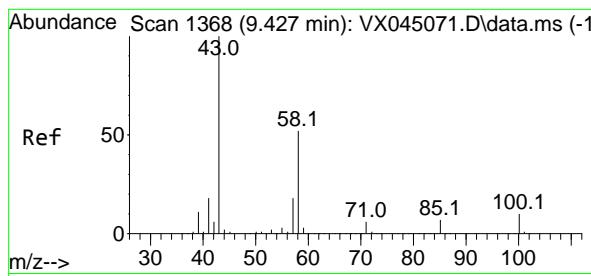

#59
2-Hexanone
Concen: 27.363 ug/l
RT: 9.433 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005




Tgt Ion: 43 Resp: 3999.
Ion Ratio Lower Upper
43 100
58 50.7 25.9 77.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

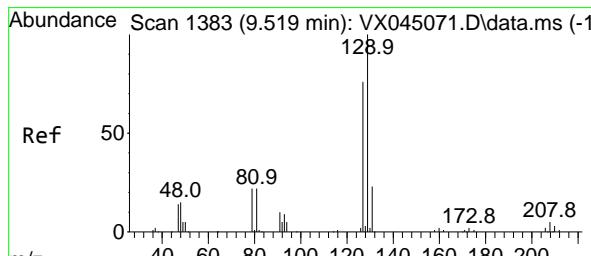


#60
Dibromochloromethane
Concen: 4.846 ug/l
RT: 9.519 min Scan# 1383
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

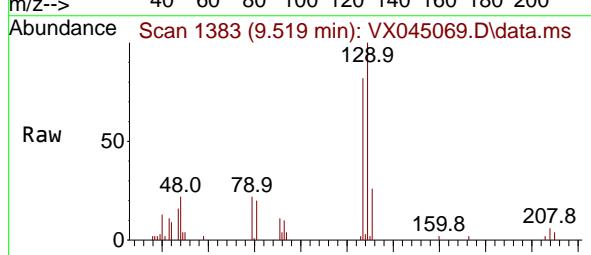



Tgt Ion:129 Resp: 6785
Ion Ratio Lower Upper
129 100
127 79.0 38.5 115.5

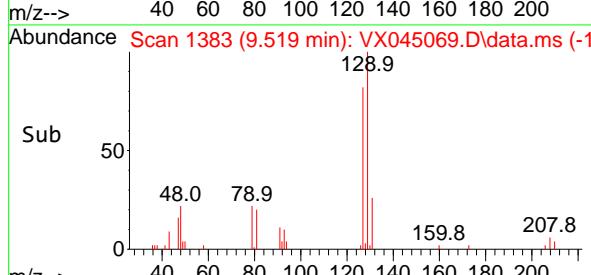



#61
1,2-Dibromoethane
Concen: 5.161 ug/l
RT: 9.610 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13



Instrument : MSVOA_X
ClientSampleId : VSTDICC005

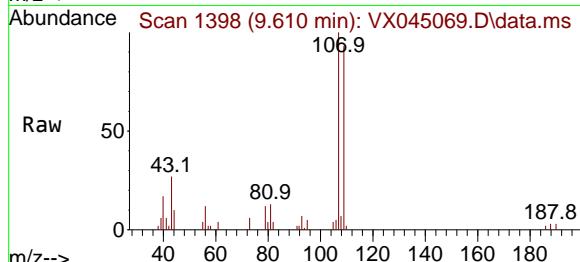


Tgt Ion:107 Resp: 683
Ion Ratio Lower Upper
107 100
109 90.7 76.1 114.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#62
4-Bromofluorobenzene
Concen: 4.685 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13



Tgt Ion: 95 Resp: 7436
Ion Ratio Lower Upper
95 100
174 76.5 0.0 148.2
176 76.3 0.0 141.4




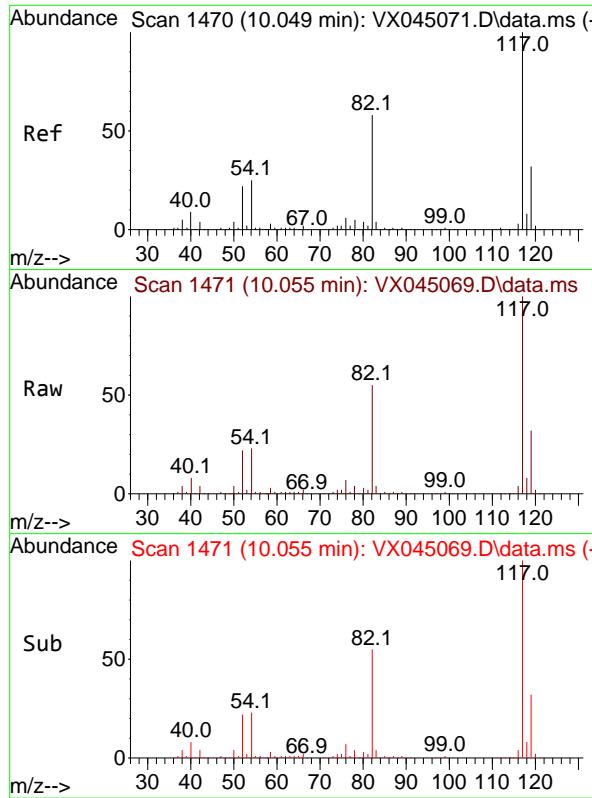


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1470
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Instrument : MSVOA_X
ClientSampleId : VSTDICC005


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

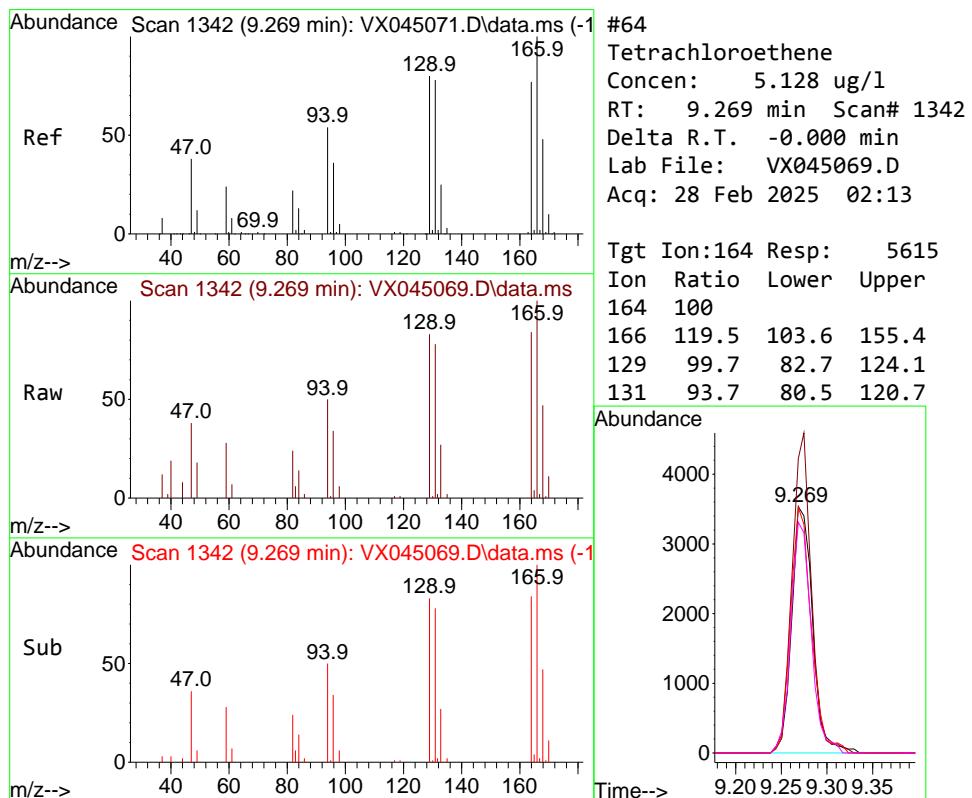

#64
Tetrachloroethene
Concen: 5.128 ug/l
RT: 9.269 min Scan# 1342
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Tgt Ion:164 Resp: 5615
Ion Ratio Lower Upper
164 100
166 119.5 103.6 155.4
129 99.7 82.7 124.1
131 93.7 80.5 120.7




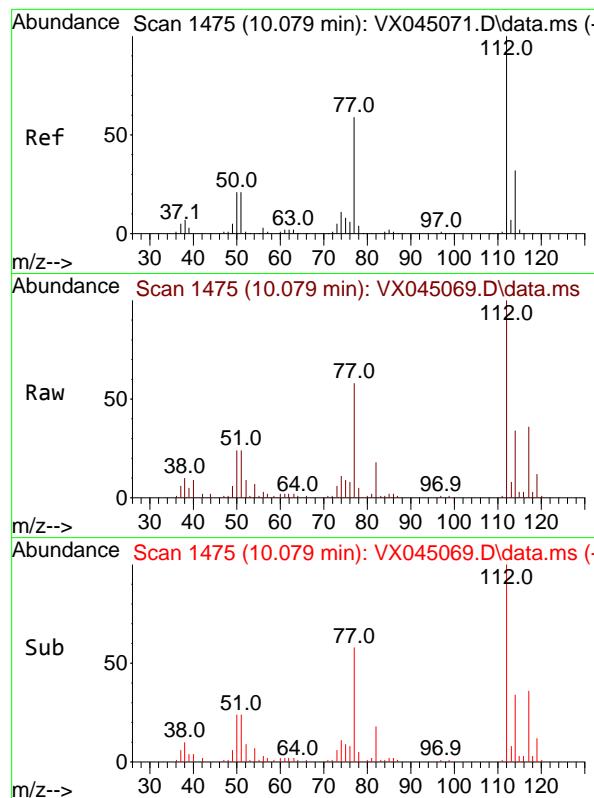


#65
Chlorobenzene
Concen: 4.908 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Instrument : MSVOA_X
ClientSampleId : VSTDICC005


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

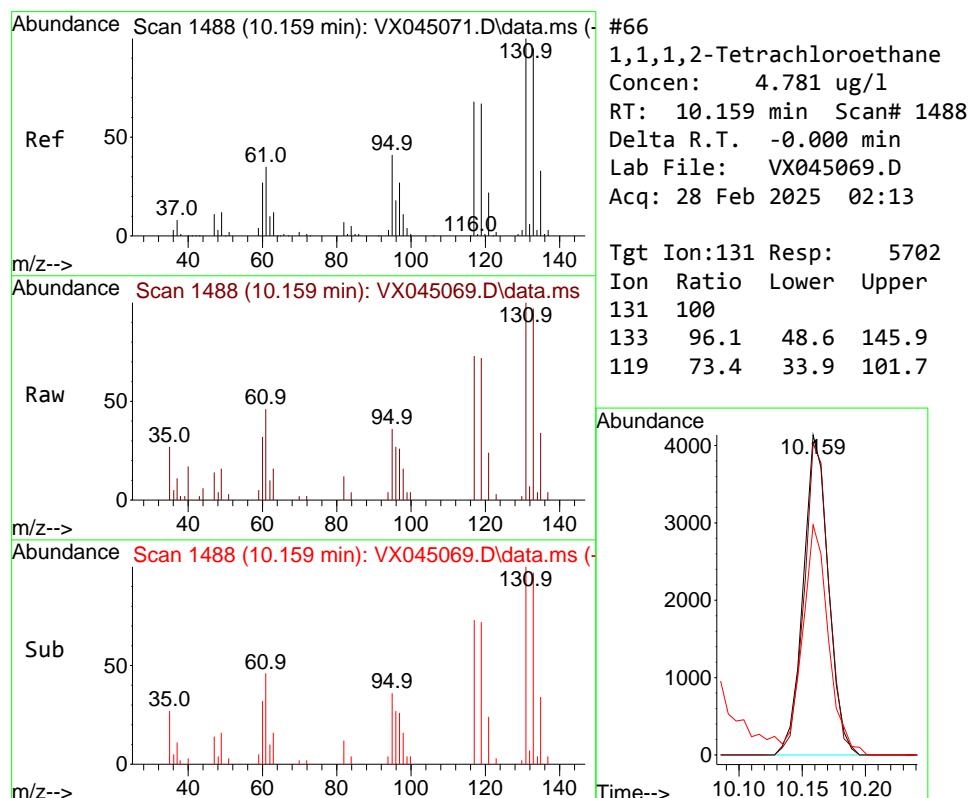


#66
1,1,1,2-Tetrachloroethane
Concen: 4.781 ug/l
RT: 10.159 min Scan# 1488
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Tgt Ion:131 Resp: 5702
Ion Ratio Lower Upper
131 100
133 96.1 48.6 145.9
119 73.4 33.9 101.7



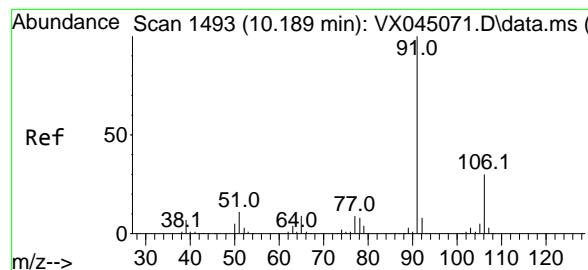




#67
Ethyl Benzene
Concen: 4.725 ug/l
RT: 10.195 min Scan# 1493
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13
Instrument: MSVOA_X
ClientSampleId: VSTDICC005

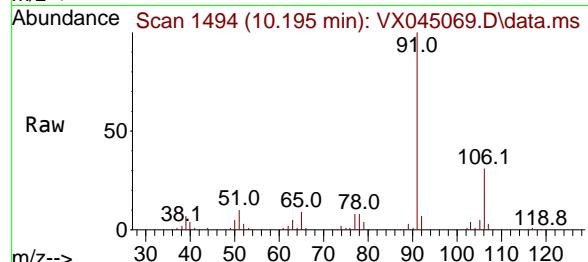


Tgt Ion: 91 Resp: 30913
Ion Ratio Lower Upper
91 100
106 30.8 23.9 35.9

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

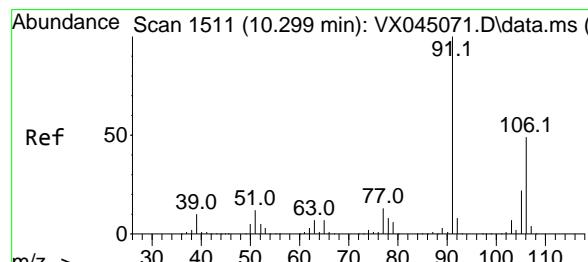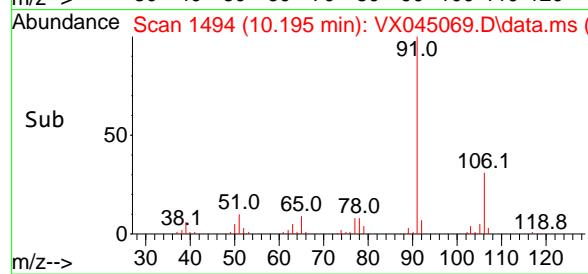


#68
m/p-Xylenes
Concen: 9.608 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

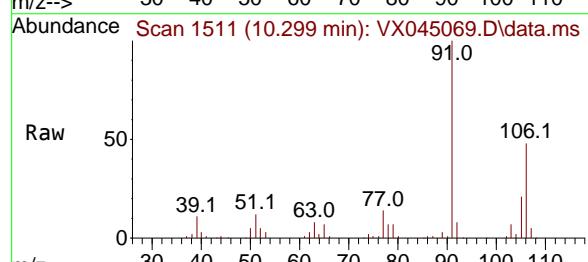

Tgt Ion:106 Resp: 23152
Ion Ratio Lower Upper
106 100
91 202.7 165.4 248.0

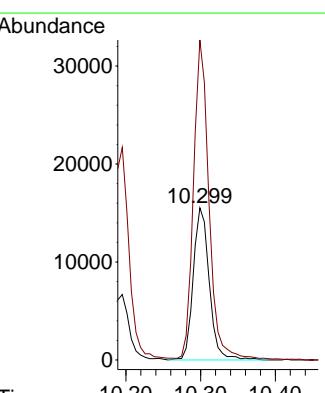


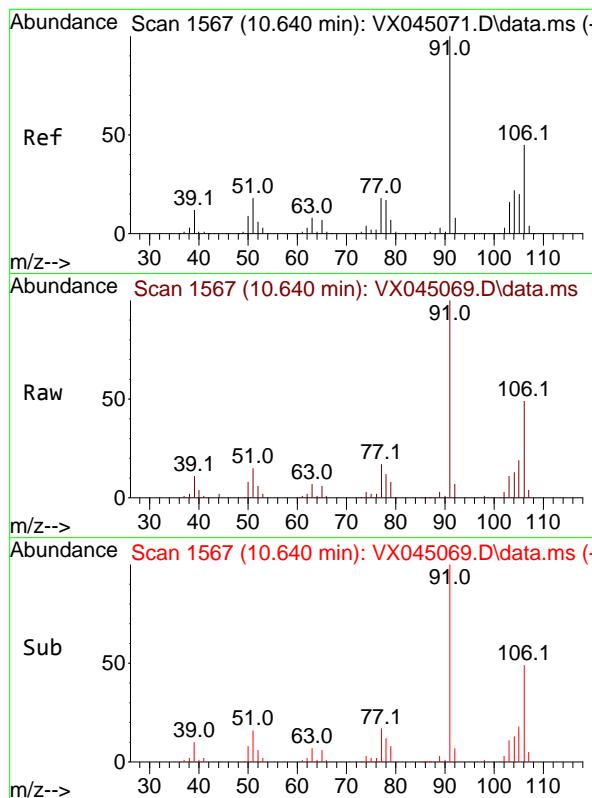


#69
o-Xylene
Concen: 4.914 ug/l
RT: 10.640 min Scan# 1
Instrument : MSVOA_X
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13
ClientSampleId : VSTDICC005

Tgt Ion:106 Resp: 1188:
Ion Ratio Lower Upper
106 100
91 211.7 109.9 329.6


Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

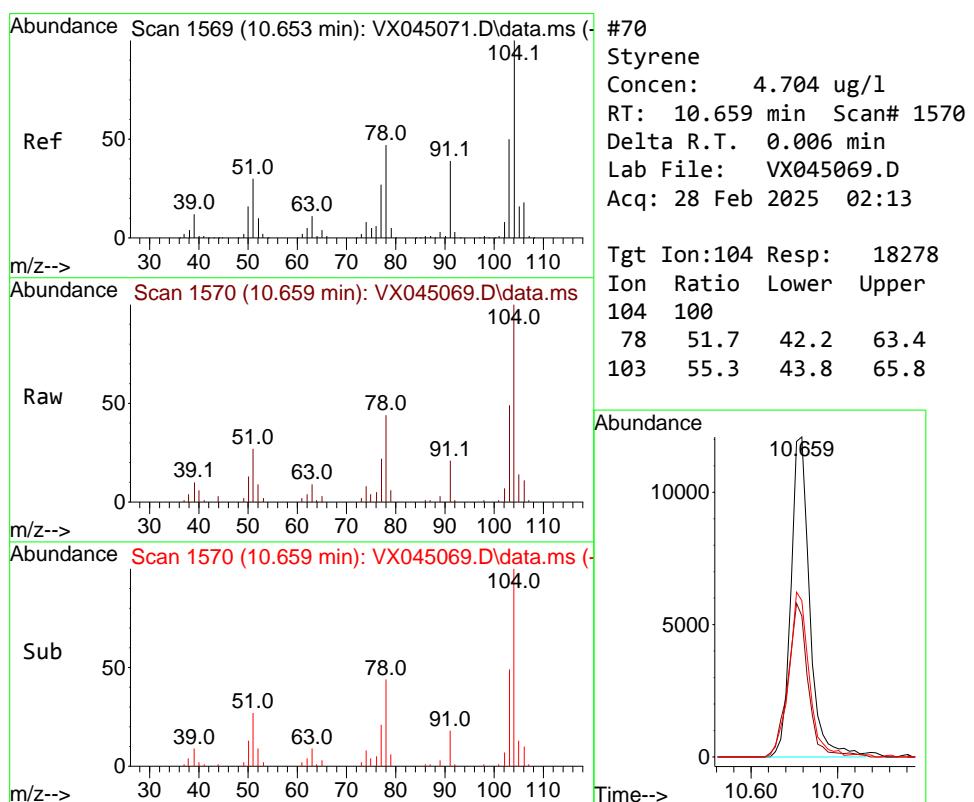


#70
Styrene
Concen: 4.704 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Tgt Ion:104 Resp: 18278
Ion Ratio Lower Upper
104 100
78 51.7 42.2 63.4
103 55.3 43.8 65.8







#71
 Bromoform
 Concen: 4.541 ug/l
 RT: 10.799 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13
Instrument: MSVOA_X
ClientSampleId: VSTDICC005



Tgt	Ion:173	Resp:	402
	Ion Ratio	Lower	Upper
173	100		
175	50.1	24.6	73.6
254	0.0	0.0	0.0




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

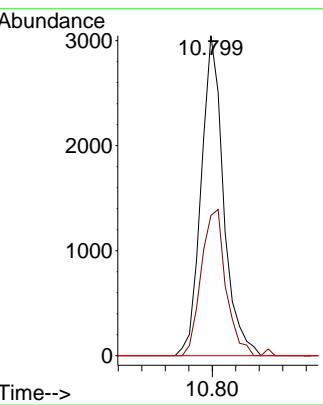

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.018 min Scan# 1793
 Delta R.T. -0.000 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13

Tgt	Ion:152	Resp:	73591
	Ion Ratio	Lower	Upper
152	100		
115	62.6	44.2	132.6
150	156.2	0.0	349.0

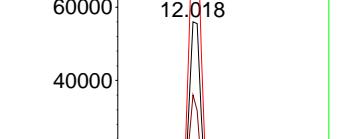
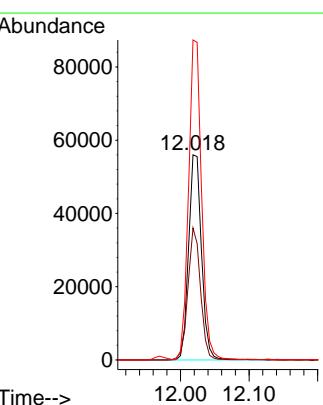


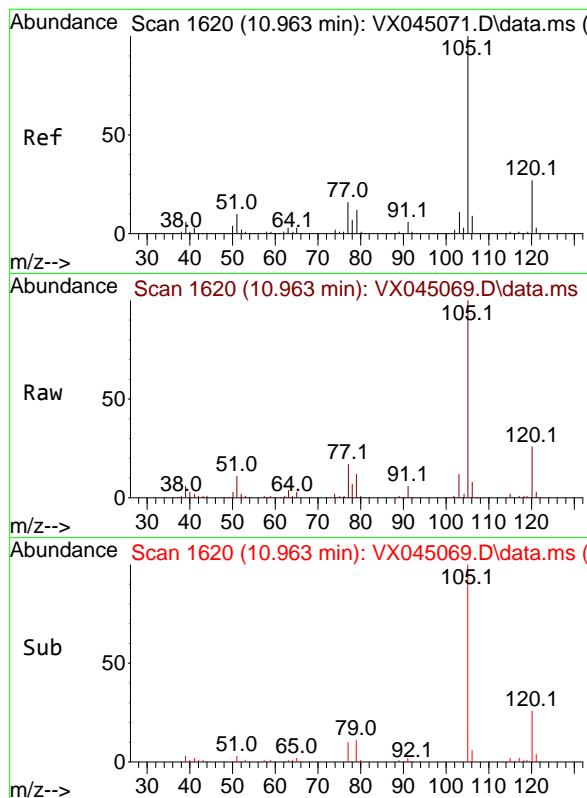

#73
Isopropylbenzene
Concen: 4.991 ug/l
RT: 10.963 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13
Instrument: MSVOA_X
ClientSampleId: VSTDICC005


Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

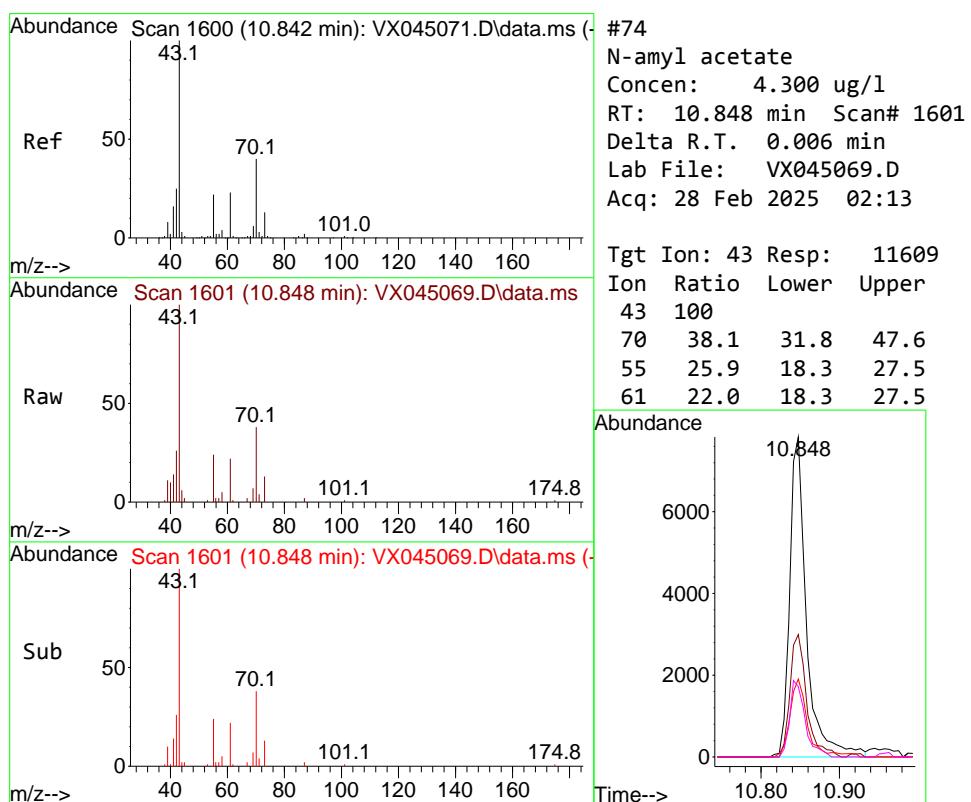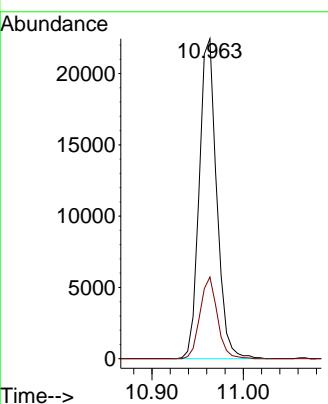

#74
N-amyl acetate
Concen: 4.300 ug/l
RT: 10.848 min Scan# 1601
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Tgt Ion: 43 Resp: 11609
Ion Ratio Lower Upper
43 100
70 38.1 31.8 47.6
55 25.9 18.3 27.5
61 22.0 18.3 27.5



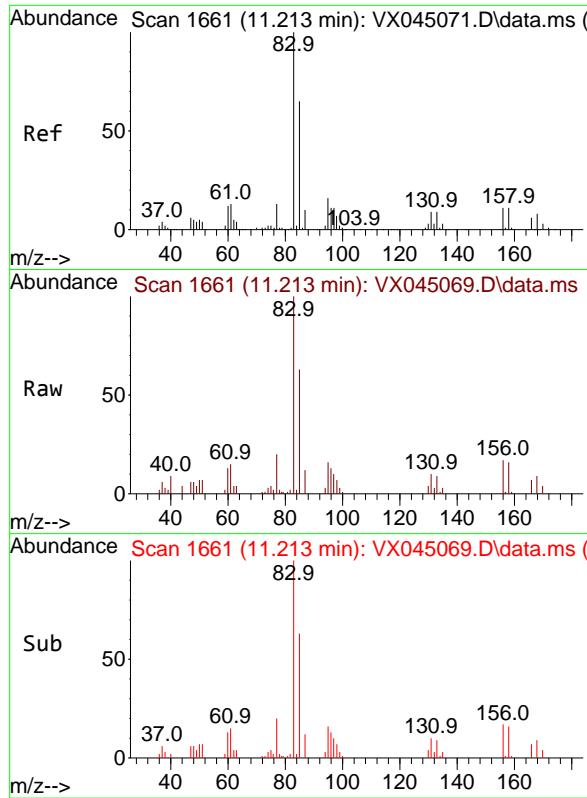



#75
1,1,2,2-Tetrachloroethane
Concen: 5.310 ug/l
RT: 11.213 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Instrument : MSVOA_X
ClientSampleId : VSTDICC005

Tgt Ion: 83 Resp: 1088:
Ion Ratio Lower Upper
83 100
131 9.2 4.5 13.4
85 63.1 31.7 95.1


Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

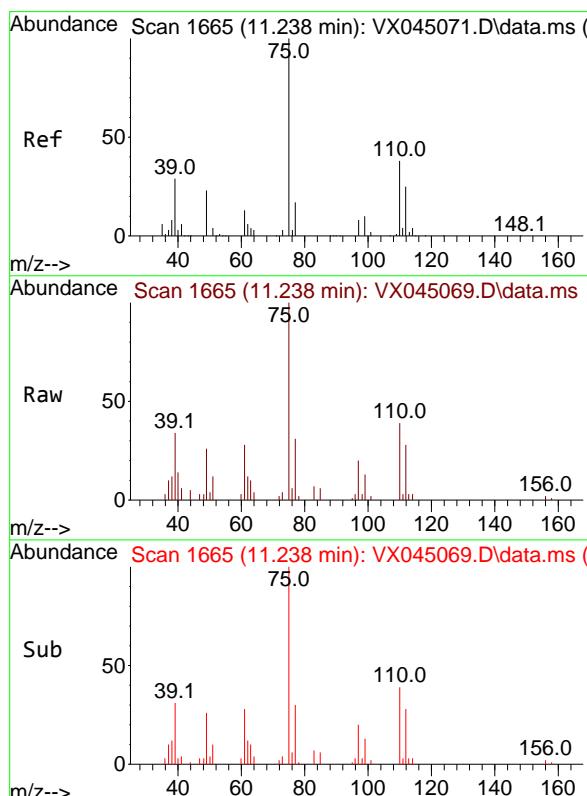


#76
1,2,3-Trichloropropane
Concen: 5.384 ug/l
RT: 11.238 min Scan# 1665
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Tgt Ion: 75 Resp: 8839
Ion Ratio Lower Upper
75 100
77 39.8 20.7 62.1

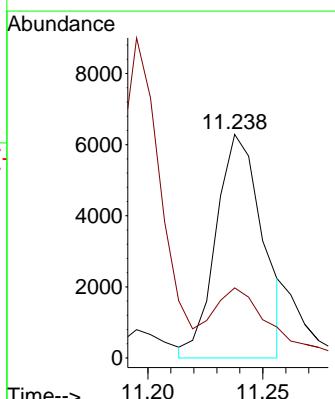






#77
Bromobenzene
Concen: 5.163 ug/l
RT: 11.195 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13
Instrument :
MSVOA_X
ClientSampleId :
VSTDICC005




Tgt Ion:156 Resp: 6970
Ion Ratio Lower Upper
156 100
77 163.3 85.8 257.4
158 97.8 48.4 145.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#78
n-propylbenzene
Concen: 4.694 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Tgt Ion: 91 Resp: 32196
Ion Ratio Lower Upper
91 100
120 21.7 11.2 33.6









#79
2-Chlorotoluene
Concen: 5.048 ug/l
RT: 11.366 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13
Instrument: MSVOA_X
ClientSampleId: VSTDICC005





Tgt Ion: 91 Resp: 21251
Ion Ratio Lower Upper
91 100
126 32.0 16.4 49.4
Manual Integrations APPROVED
Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

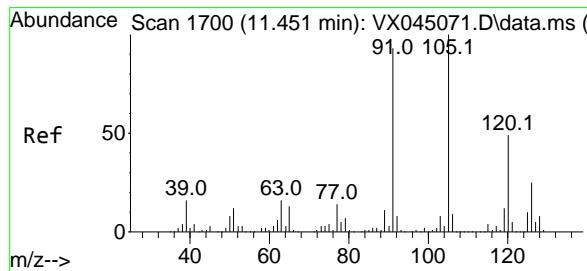


#80
1,3,5-Trimethylbenzene
Concen: 4.897 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Tgt Ion:105 Resp: 23627
Ion Ratio Lower Upper
105 100
120 47.6 24.1 72.2

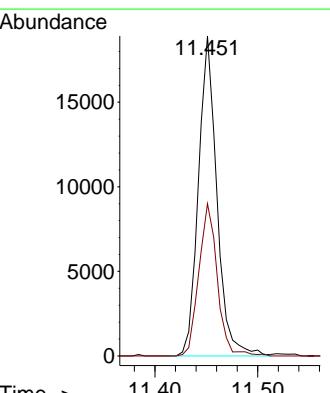






#81
trans-1,4-Dichloro-2-butene
Concen: 3.256 ug/l
RT: 11.018 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

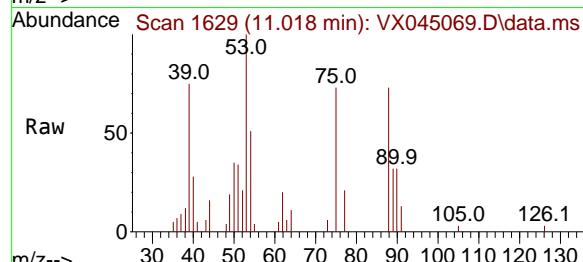


Tgt Ion: 75 Resp: 197:
Ion Ratio Lower Upper
75 100
53 134.1 88.5 132.7
89 43.4 36.2 54.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

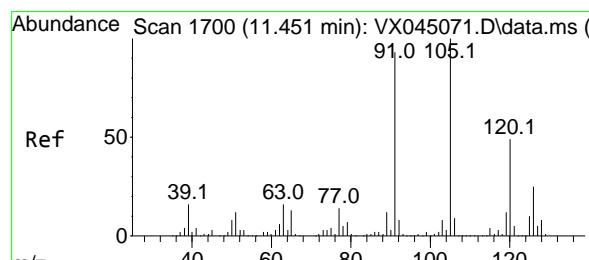

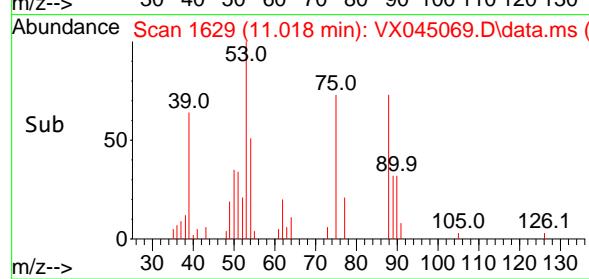


#82
4-Chlorotoluene
Concen: 4.761 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

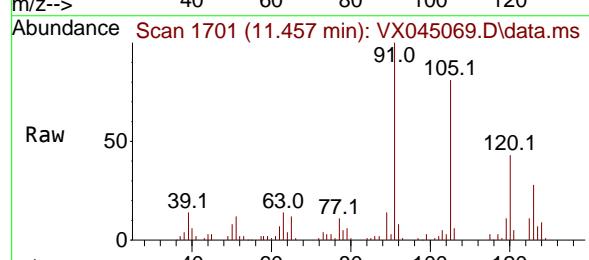

Tgt Ion: 91 Resp: 22190
Ion Ratio Lower Upper
91 100
126 27.3 14.1 42.4

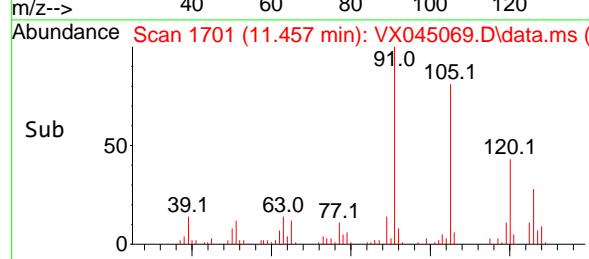



#83

tert-Butylbenzene

Concen: 4.910 ug/l

RT: 11.713 min Scan# 1743

Delta R.T. -0.000 min

Lab File: VX045069.D

Acq: 28 Feb 2025 02:13




Instrument:

MSVOA_X

ClientSampleId :

VSTDICC005

**Manual Integrations
APPROVED**

 Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025


#84

1,2,4-Trimethylbenzene

Concen: 4.960 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX045069.D


Acq: 28 Feb 2025 02:13


Tgt Ion:105 Resp: 23561

Ion Ratio Lower Upper

105 100


120 43.4 22.1 66.1





#85
sec-Butylbenzene
Concen: 4.687 ug/l
RT: 11.890 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13



Instrument : MSVOA_X
ClientSampleId : VSTDICC005




Tgt Ion:105 Resp: 2831
Ion Ratio Lower Upper
105 100
134 19.3 9.8 29.4

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#86
p-Isopropyltoluene
Concen: 4.532 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13



Tgt Ion:119 Resp: 21977
Ion Ratio Lower Upper
119 100
134 27.9 12.9 38.6
91 26.1 12.7 38.0



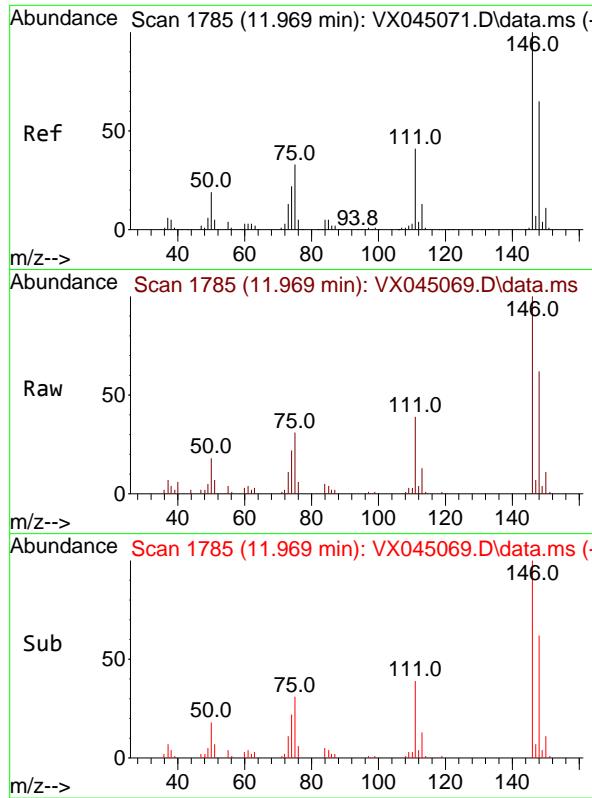



#87
 1,3-Dichlorobenzene
 Concen: 4.926 ug/l
 RT: 11.969 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13

Instrument : MSVOA_X
 ClientSampleId : VSTDICC005

Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025


Tgt	Ion:146	Resp:	1215
Ion	Ratio	Lower	Upper
146	100		
111	40.5	21.1	63.4
148	62.9	31.9	95.7

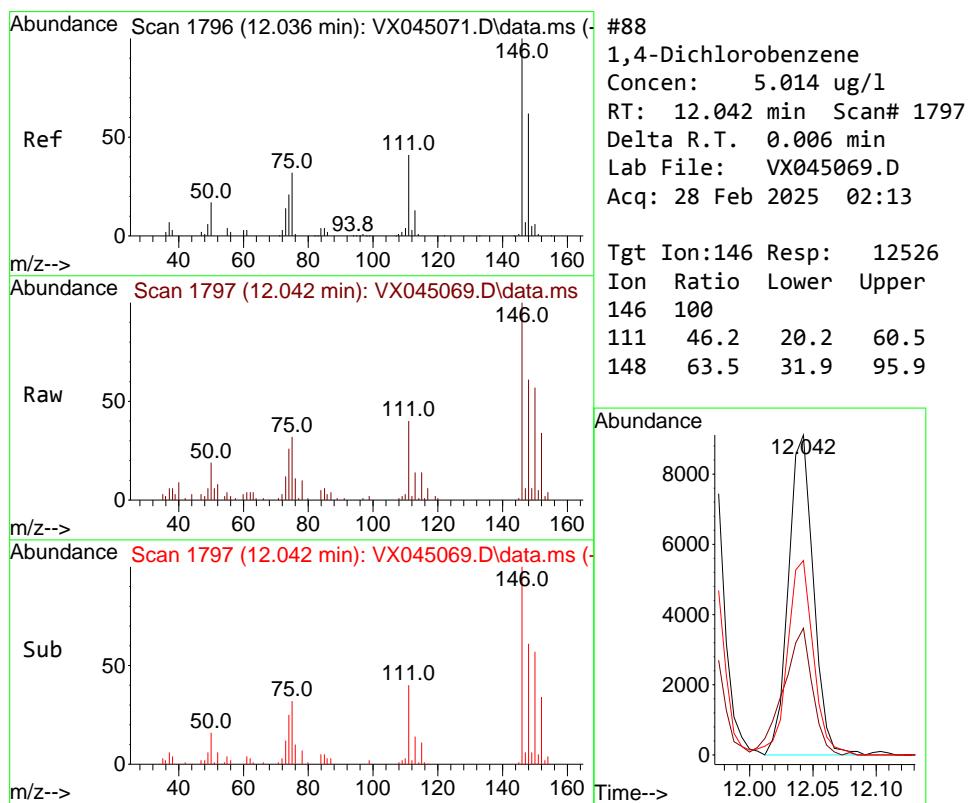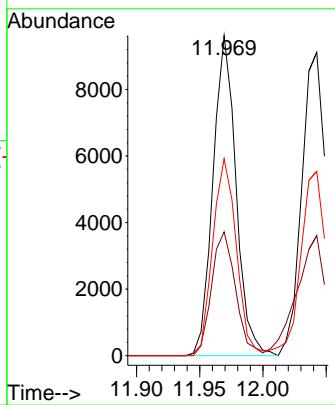

#88
 1,4-Dichlorobenzene
 Concen: 5.014 ug/l
 RT: 12.042 min Scan# 1797
 Delta R.T. 0.006 min
 Lab File: VX045069.D
 Acq: 28 Feb 2025 02:13


Tgt	Ion:146	Resp:	12526
Ion	Ratio	Lower	Upper
146	100		
111	46.2	20.2	60.5
148	63.5	31.9	95.9

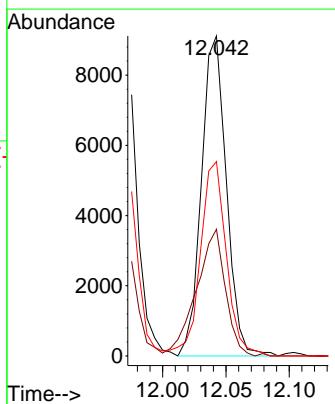



#89
n-Butylbenzene
Concen: 4.072 ug/l
RT: 12.335 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005




Tgt Ion: 91 Resp: 1735:
Ion Ratio Lower Upper
91 100
92 53.9 26.7 80.0
134 24.4 12.2 36.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#90
Hexachloroethane
Concen: 4.052 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Tgt Ion:117 Resp: 3665
Ion Ratio Lower Upper
117 100
201 67.1 31.9 95.9

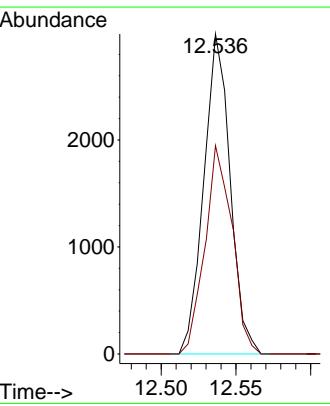



#91
1,2-Dichlorobenzene
Concen: 5.138 ug/l
RT: 12.335 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005




Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
146	100		1247		
111	41.2	21.6		65.0	
148	59.4	31.9		95.9	

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#92
1,2-Dibromo-3-Chloropropane
Concen: 4.712 ug/l
RT: 12.945 min Scan# 1945
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13



Tgt	Ion	Ion Ratio	Resp:	Lower	Upper
75	100		1787		
155	83.8	39.6		118.7	
157	115.4	51.1		153.4	




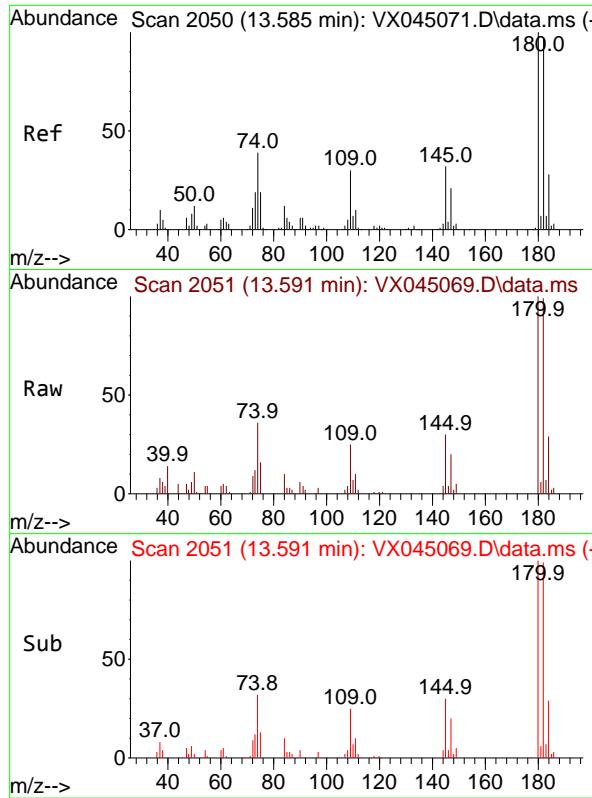


#93
1,2,4-Trichlorobenzene
Concen: 4.114 ug/l
RT: 13.591 min Scan# 2
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13

Instrument : MSVOA_X
ClientSampleId : VSTDICC005


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

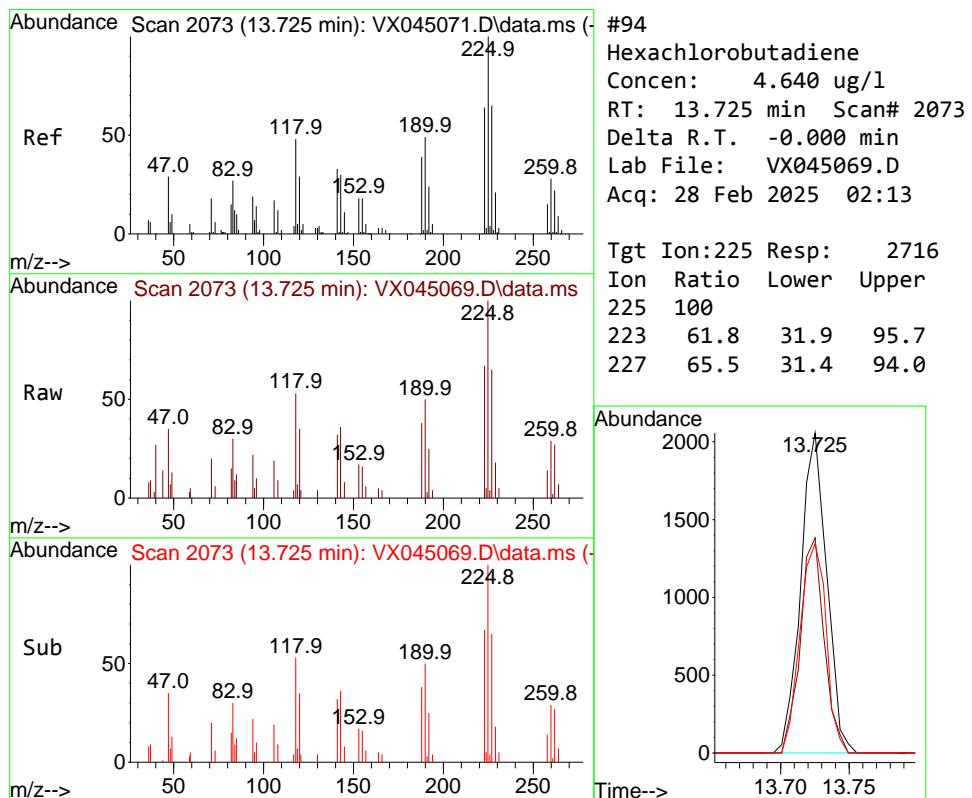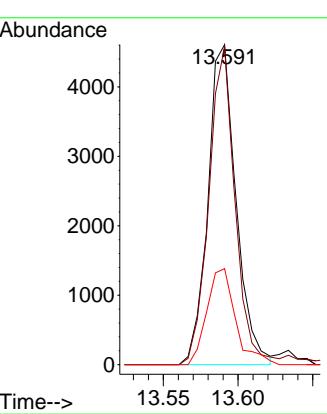

#94
Hexachlorobutadiene
Concen: 4.640 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. -0.000 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13


Tgt Ion:225 Resp: 2716
Ion Ratio Lower Upper
225 100
223 61.8 31.9 95.7
227 65.5 31.4 94.0





#95
Naphthalene
Concen: 4.287 ug/l
RT: 13.780 min Scan# 2111
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13




Instrument : MSVOA_X
ClientSampleId : VSTDICC005




Tgt Ion:128 Resp: 2292
Ion Ratio Lower Upper
128 100
127 12.6 10.3 15.5
129 10.6 8.7 13.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#96
1,2,3-Trichlorobenzene
Concen: 4.437 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.006 min
Lab File: VX045069.D
Acq: 28 Feb 2025 02:13



Tgt Ion:180 Resp: 6600
Ion Ratio Lower Upper
180 100
182 93.3 47.5 142.6
145 32.6 17.0 50.9



Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045070.D
 Acq On : 28 Feb 2025 02:37
 Operator : JC/MD
 Sample : VSTDICC020
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020

Quant Time: Feb 28 05:33:34 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 05:28:02 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.543	168	97338	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	177403	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	157714	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	70072	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	30514	21.221	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 42.440%#			
35) Dibromofluoromethane	5.385	113	23739	20.473	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 40.940%#			
50) Toluene-d8	8.646	98	84516	19.469	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 38.940%#			
62) 4-Bromofluorobenzene	11.079	95	27856	19.215	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 38.420%#			
Target Compounds						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	25155	18.750	ug/l	95
3) Chloromethane	1.306	50	32219	19.736	ug/l	99
4) Vinyl Chloride	1.373	62	30134	18.899	ug/l	97
5) Bromomethane	1.593	94	11584	23.239	ug/l	99
6) Chloroethane	1.660	64	14237	23.457	ug/l	99
7) Trichlorofluoromethane	1.867	101	40880	20.015	ug/l	99
8) Diethyl Ether	2.135	74	15911	21.437	ug/l	98
9) 1,1,2-Trichlorotrifluo...	2.312	101	23154	18.984	ug/l	98
10) Methyl Iodide	2.440	142	29500	18.867	ug/l	100
11) Tert butyl alcohol	2.983	59	31246	118.627	ug/l	98
12) 1,1-Dichloroethene	2.306	96	23810	19.014	ug/l	97
13) Acrolein	2.239	56	33586	117.747	ug/l	99
14) Allyl chloride	2.654	41	42993	19.096	ug/l	100
15) Acrylonitrile	3.068	53	84182	117.598	ug/l	100
16) Acetone	2.385	43	74701	126.257	ug/l	99
17) Carbon Disulfide	2.501	76	61802	18.139	ug/l	99
18) Methyl Acetate	2.709	43	35157	19.729	ug/l	99
19) Methyl tert-butyl Ether	3.117	73	82833	20.689	ug/l	96
20) Methylene Chloride	2.782	84	29281	20.895	ug/l	94
21) trans-1,2-Dichloroethene	3.080	96	23471	19.057	ug/l	97
22) Diisopropyl ether	3.763	45	90378	20.995	ug/l	93
23) Vinyl Acetate	3.721	43	381808	108.038	ug/l	99
24) 1,1-Dichloroethane	3.605	63	49826	20.716	ug/l	99
25) 2-Butanone	4.562	43	118713	124.449	ug/l	97
26) 2,2-Dichloropropane	4.470	77	22886	12.799	ug/l	99
27) cis-1,2-Dichloroethene	4.483	96	29788	20.065	ug/l	99
28) Bromochloromethane	4.891	49	23869	20.579	ug/l	99
29) Tetrahydrofuran	5.007	42	77433	122.519	ug/l	99
30) Chloroform	5.086	83	49751	21.147	ug/l	97
31) Cyclohexane	5.464	56	42340	19.181	ug/l	98
32) 1,1,1-Trichloroethane	5.373	97	39276	19.831	ug/l	99
36) 1,1-Dichloropropene	5.684	75	31519	18.903	ug/l	99
37) Ethyl Acetate	4.714	43	43097	22.714	ug/l	99
38) Carbon Tetrachloride	5.671	117	31694	19.334	ug/l	97
39) Methylcyclohexane	7.372	83	39769	18.676	ug/l	97
40) Benzene	6.031	78	105787	20.298	ug/l	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045070.D
 Acq On : 28 Feb 2025 02:37
 Operator : JC/MD
 Sample : VSTDICC020
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020

Quant Time: Feb 28 05:33:34 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 05:28:02 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.928	41	23924	23.605	ug/1	97
42) 1,2-Dichloroethane	6.086	62	38653	22.886	ug/1	99
43) Isopropyl Acetate	6.348	43	66727	22.094	ug/1	99
44) Trichloroethene	7.122	130	24052	20.191	ug/1	98
45) 1,2-Dichloropropane	7.427	63	27128	20.945	ug/1	99
46) Dibromomethane	7.580	93	19323	21.357	ug/1	97
47) Bromodichloromethane	7.817	83	38038	21.732	ug/1	97
48) Methyl methacrylate	7.695	41	32627	22.757	ug/1	98
49) 1,4-Dioxane	7.665	88	14602	479.170	ug/1	97
51) 4-Methyl-2-Pentanone	8.573	43	229615	124.081	ug/1	98
52) Toluene	8.714	92	63326	20.463	ug/1	100
53) t-1,3-Dichloropropene	8.976	75	30917	17.871	ug/1	97
54) cis-1,3-Dichloropropene	8.366	75	36118	18.675	ug/1	97
55) 1,1,2-Trichloroethane	9.152	97	26358	21.992	ug/1	99
56) Ethyl methacrylate	9.116	69	39850	20.791	ug/1	97
57) 1,3-Dichloropropane	9.305	76	45644	21.836	ug/1	100
58) 2-Chloroethyl Vinyl ether	8.238	63	96311	102.342	ug/1	99
59) 2-Hexanone	9.433	43	168768	126.428	ug/1	100
60) Dibromochloromethane	9.518	129	27705	21.668	ug/1	99
61) 1,2-Dibromoethane	9.610	107	26311	21.764	ug/1	98
64) Tetrachloroethene	9.268	164	20140	20.102	ug/1	97
65) Chlorobenzene	10.079	112	68777	20.316	ug/1	98
66) 1,1,1,2-Tetrachloroethane	10.158	131	22508	20.627	ug/1	97
67) Ethyl Benzene	10.189	91	119165	19.905	ug/1	100
68) m/p-Xylenes	10.299	106	89735	40.699	ug/1	98
69) o-Xylene	10.640	106	44281	20.018	ug/1	98
70) Styrene	10.652	104	73832	20.767	ug/1	98
71) Bromoform	10.799	173	17403	21.449	ug/1 #	99
73) Isopropylbenzene	10.963	105	112099	19.794	ug/1	99
74) N-amyl acetate	10.841	43	52972	20.606	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	42413	21.738	ug/1	100
76) 1,2,3-Trichloropropane	11.237	75	33440m	21.394	ug/1	
77) Bromobenzene	11.195	156	26310	20.466	ug/1	99
78) n-propylbenzene	11.305	91	128284	19.641	ug/1	100
79) 2-Chlorotoluene	11.359	91	79275	19.775	ug/1	100
80) 1,3,5-Trimethylbenzene	11.451	105	94545	20.581	ug/1	98
81) trans-1,4-Dichloro-2-b...	11.018	75	8759	15.196	ug/1	96
82) 4-Chlorotoluene	11.451	91	86281	19.443	ug/1	98
83) tert-Butylbenzene	11.713	119	93670	20.159	ug/1	99
84) 1,2,4-Trimethylbenzene	11.750	105	94734	20.943	ug/1	100
85) sec-Butylbenzene	11.890	105	115953	20.160	ug/1	100
86) p-Isopropyltoluene	12.006	119	91554	19.827	ug/1	99
87) 1,3-Dichlorobenzene	11.969	146	47934	20.400	ug/1	97
88) 1,4-Dichlorobenzene	12.042	146	46657	19.615	ug/1	99
89) n-Butylbenzene	12.329	91	78135	19.249	ug/1	100
90) Hexachloroethane	12.536	117	15919	18.483	ug/1	98
91) 1,2-Dichlorobenzene	12.335	146	48632	21.031	ug/1	98
92) 1,2-Dibromo-3-Chloropr...	12.944	75	7987	22.119	ug/1	99
93) 1,2,4-Trichlorobenzene	13.585	180	27424	19.617	ug/1	99
94) Hexachlorobutadiene	13.725	225	10934	19.616	ug/1	99
95) Naphthalene	13.774	128	108350	21.279	ug/1	100
96) 1,2,3-Trichlorobenzene	13.963	180	28937	20.432	ug/1	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045070.D
Acq On : 28 Feb 2025 02:37
Operator : JC/MD
Sample : VSTDICC020
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020

Quant Time: Feb 28 05:33:34 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 05:28:02 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carbone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045070.D
Acq On : 28 Feb 2025 02:37
Operator : JC/MD
Sample : VSTDIICC020
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

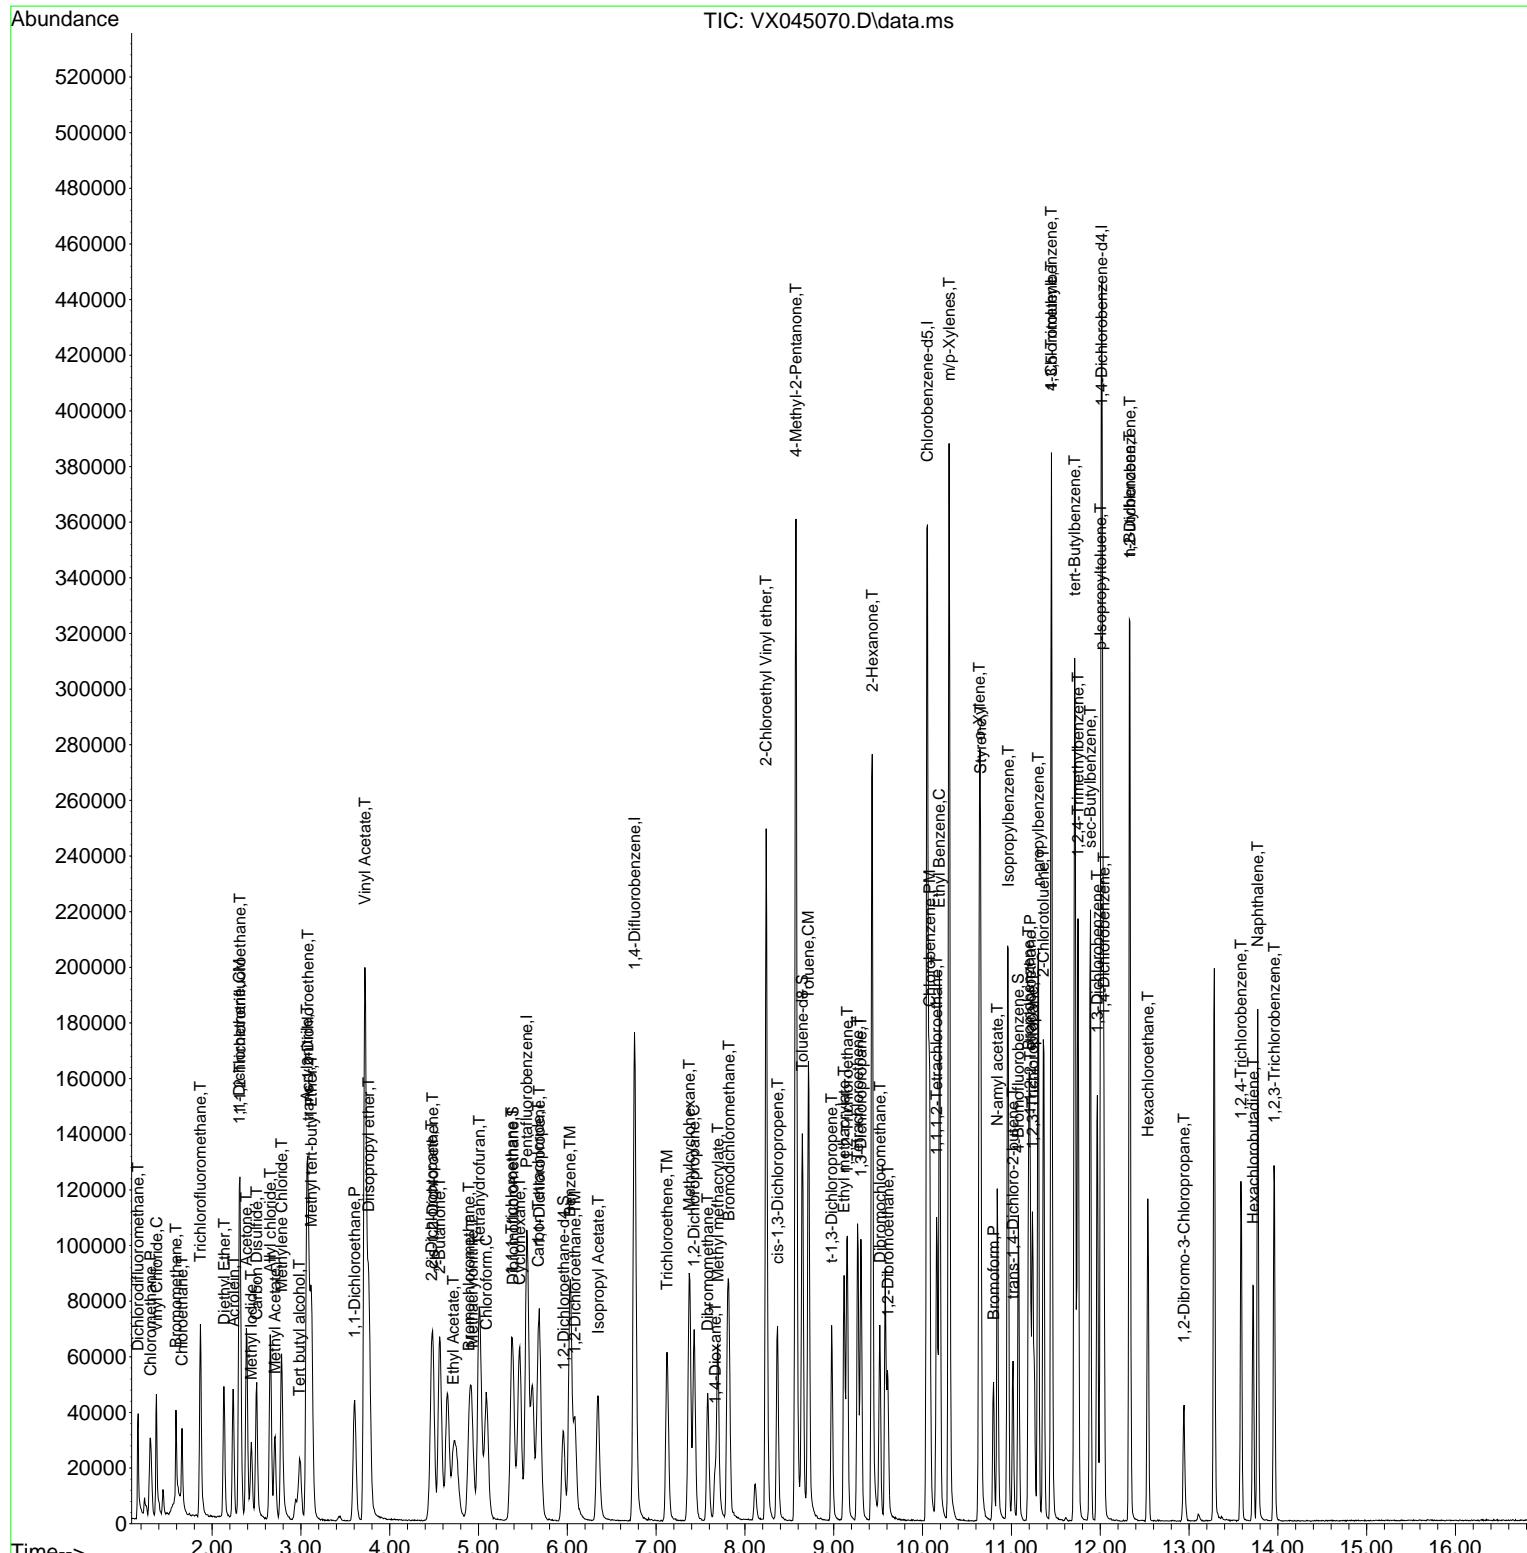



#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.543 min Scan# 7
 Delta R.T. -0.007 min
 Lab File: VX045070.D
 Acq: 28 Feb 2025 02:37



Instrument : MSVOA_X
 ClientSampleId : VSTDICC020




Tgt Ion:168 Resp: 9733
 Ion Ratio Lower Upper
 168 100
 99 59.4 48.2 72.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025




#2
 Dichlorodifluoromethane
 Concen: 18.750 ug/l
 RT: 1.166 min Scan# 13
 Delta R.T. -0.000 min
 Lab File: VX045070.D
 Acq: 28 Feb 2025 02:37




Tgt Ion: 85 Resp: 25155
 Ion Ratio Lower Upper
 85 100
 87 31.9 17.4 52.3

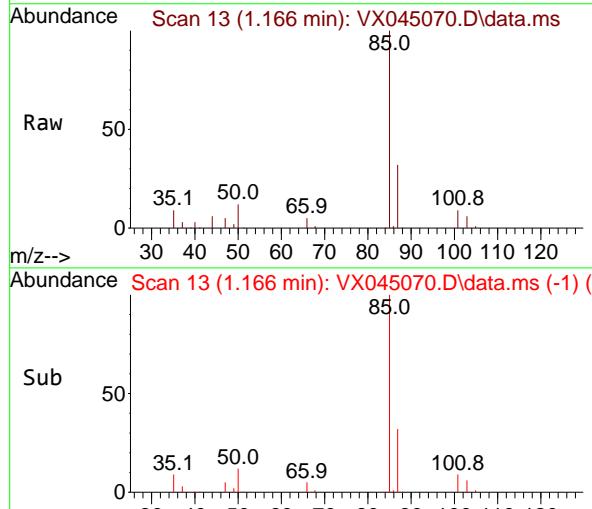



#3
Chloromethane
Concen: 19.736 ug/l
RT: 1.306 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument: MSVOA_X
ClientSampleId: VSTDICC020




Tgt Ion: 50 Resp: 32219
Ion Ratio Lower Upper
50 100
52 31.7 25.0 37.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

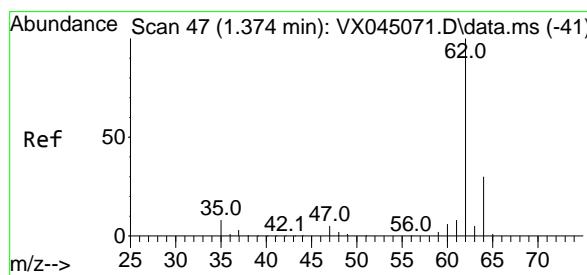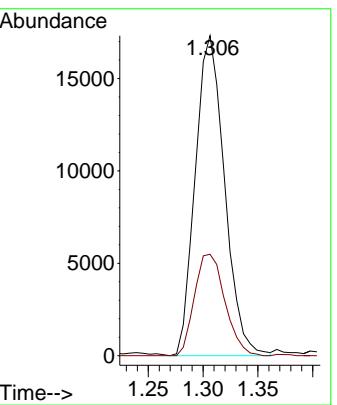


#4
Vinyl Chloride
Concen: 18.899 ug/l
RT: 1.373 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

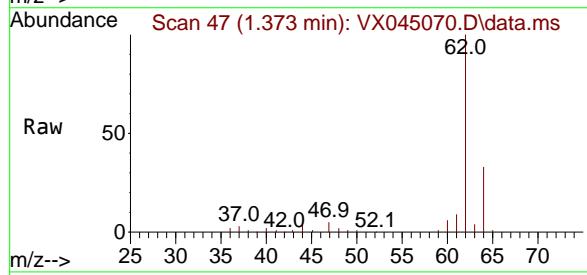


Tgt Ion: 62 Resp: 30134
Ion Ratio Lower Upper
62 100
64 32.0 24.3 36.5

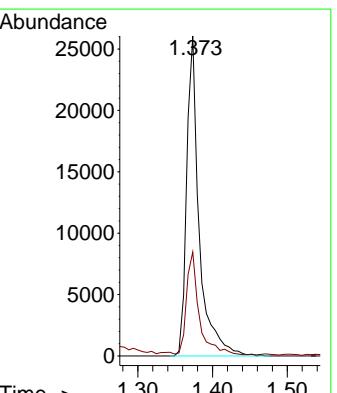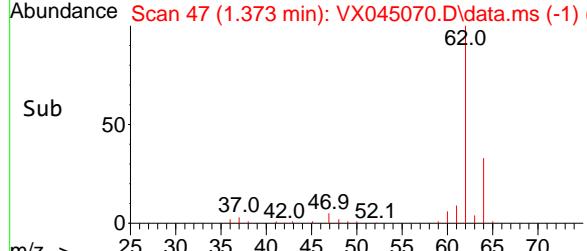



#5
Bromomethane
Concen: 23.239 ug/l
RT: 1.593 min Scan# 8
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37



Instrument : MSVOA_X
ClientSampleId : VSTDICC020




Tgt Ion: 94 Resp: 11584
Ion Ratio Lower Upper
94 100
96 92.4 75.0 112.4

**Manual Integrations
APPROVED**



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

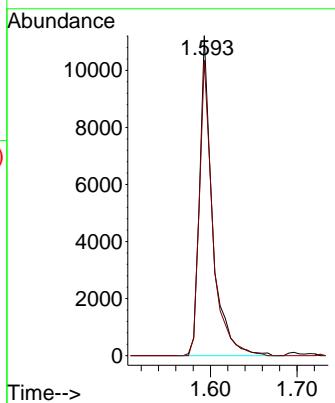


#6
Chloroethane
Concen: 23.457 ug/l
RT: 1.660 min Scan# 94
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion: 64 Resp: 14237
Ion Ratio Lower Upper
64 100
66 32.6 26.7 40.1

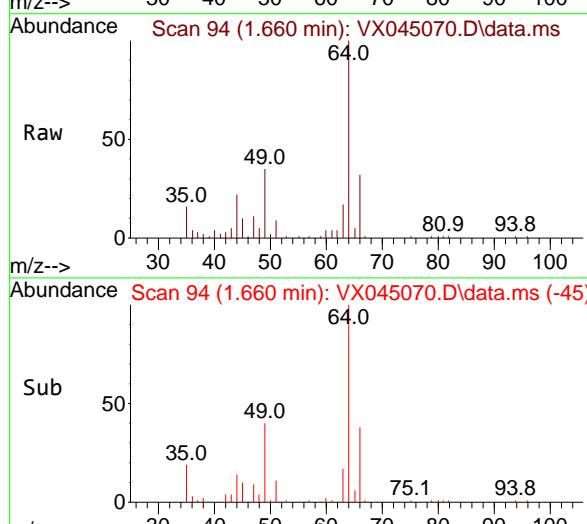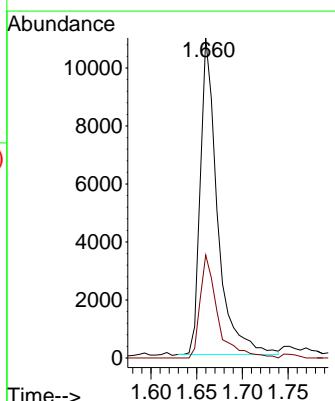


Abundance Scan 94 (1.660 min): VX045070.D\data.ms (-45)

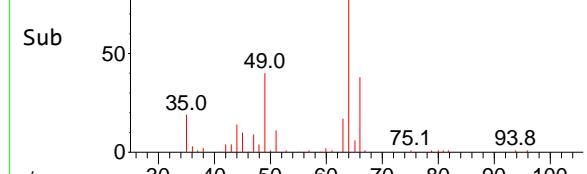



#7
Trichlorofluoromethane
Concen: 20.015 ug/l
RT: 1.867 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
ClientSampleId : VSTDICC020



Tgt Ion: 101 Resp: 40880
Ion Ratio Lower Upper
101 100
103 64.0 52.1 78.1




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

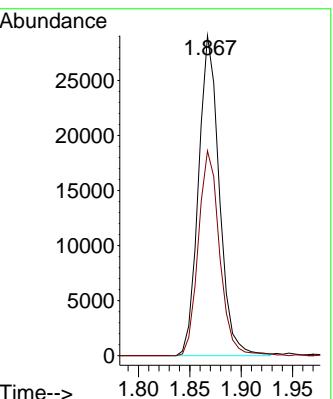

#8
Diethyl Ether
Concen: 21.437 ug/l
RT: 2.135 min Scan# 172
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion: 74 Resp: 15911
Ion Ratio Lower Upper
74 100
45 105.3 51.5 154.5

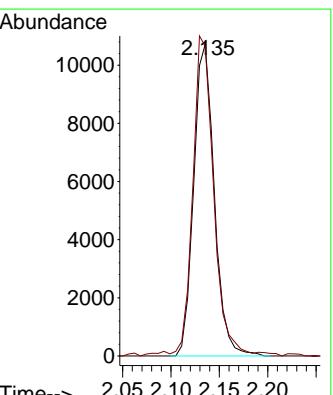



#9
1,1,2-Trichlorotrifluoroethane
Concen: 18.984 ug/l
RT: 2.312 min Scan# 2315
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020




Tgt Ion:101 Resp: 23154
Ion Ratio Lower Upper
101 100
85 46.5 36.2 54.4
151 71.8 56.4 84.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#10
Methyl Iodide
Concen: 18.867 ug/l
RT: 2.440 min Scan# 222
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion:142 Resp: 29500
Ion Ratio Lower Upper
142 100
127 44.2 35.4 53.2
141 14.3 11.6 17.4





#11
Tert butyl alcohol
Concen: 118.627 ug/l
RT: 2.983 min Scan# 311
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
ClientSampleId : VSTDICC020



Tgt Ion: 59 Resp: 31240
Ion Ratio Lower Upper
59 100
57 8.9 7.8 11.8




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

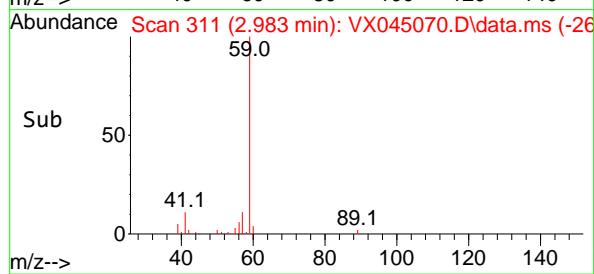

#12
1,1-Dichloroethene
Concen: 19.014 ug/l
RT: 2.306 min Scan# 200
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion: 96 Resp: 23810
Ion Ratio Lower Upper
96 100
61 172.8 134.6 202.0
98 64.1 51.0 76.6





#13
Acrolein
Concen: 117.747 ug/l
RT: 2.239 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020



Tgt Ion: 56 Resp: 33580
Ion Ratio Lower Upper
56 100
55 71.4 56.2 84.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#14
Allyl chloride
Concen: 19.096 ug/l
RT: 2.654 min Scan# 257
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion: 41 Resp: 42993
Ion Ratio Lower Upper
41 100
39 67.4 53.8 80.8
76 32.1 25.2 37.8

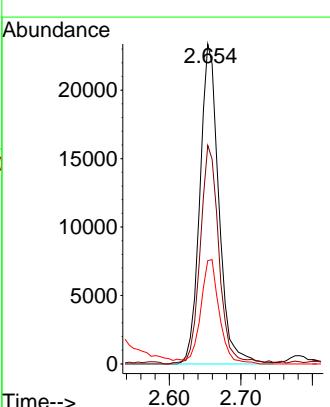



#15
Acrylonitrile
 Concen: 117.598 ug/l
 RT: 3.068 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VX045070.D
 Acq: 28 Feb 2025 02:37



Instrument : MSVOA_X
 ClientSampleId : VSTDICC020



Tgt Ion: 53 Resp: 84183
 Ion Ratio Lower Upper
 53 100
 52 82.8 66.2 99.2
 51 36.0 29.0 43.4





Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025



#16
Acetone
 Concen: 126.257 ug/l
 RT: 2.385 min Scan# 213
 Delta R.T. -0.000 min
 Lab File: VX045070.D
 Acq: 28 Feb 2025 02:37


Tgt Ion: 43 Resp: 74701
 Ion Ratio Lower Upper
 43 100
 58 30.7 24.2 36.4





#17
Carbon Disulfide
Concen: 18.139 ug/l
RT: 2.501 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020




Tgt Ion: 76 Resp: 6180
Ion Ratio Lower Upper
76 100
78 8.5 6.6 9.8

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

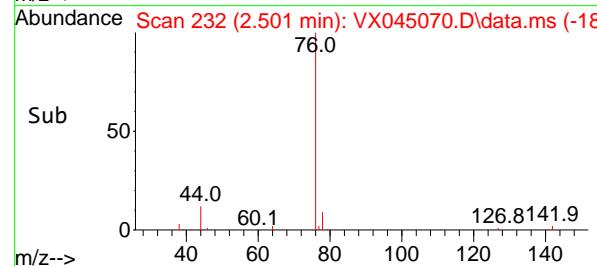


#18
Methyl Acetate
Concen: 19.729 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion: 43 Resp: 35157
Ion Ratio Lower Upper
43 100
74 22.2 17.4 26.2

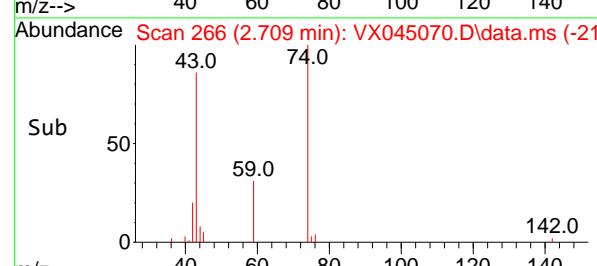



#19
Methyl tert-butyl Ether
Concen: 20.689 ug/l
RT: 3.117 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
ClientSampleId : VSTDICC020




Tgt Ion: 73 Resp: 8283
Ion Ratio Lower Upper
73 100
57 21.1 18.5 27.7

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

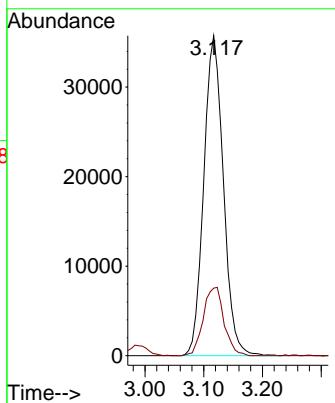


#20
Methylene Chloride
Concen: 20.895 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion: 84 Resp: 29281
Ion Ratio Lower Upper
84 100
49 122.9 106.5 159.7
51 38.9 32.1 48.1
86 60.1 50.0 75.0

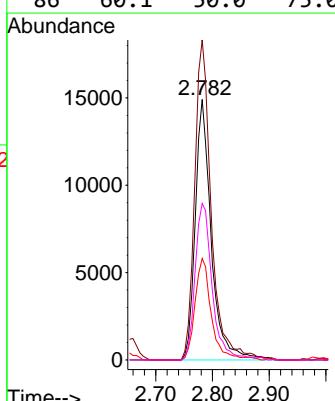



#21
trans-1,2-Dichloroethene
Concen: 19.057 ug/l
RT: 3.080 min Scan# 3
Delta R.T. -0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37



Instrument : MSVOA_X
ClientSampleId : VSTDICC020



Tgt Ion: 96 Resp: 2347
Ion Ratio Lower Upper
96 100
61 150.3 117.0 175.4
98 67.5 53.4 80.2



Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#22
Diisopropyl ether
Concen: 20.995 ug/l
RT: 3.763 min Scan# 439
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion: 45 Resp: 90378
Ion Ratio Lower Upper
45 100
43 76.4 54.9 82.3
87 24.7 21.0 31.4
59 11.6 8.7 13.1




Diisopropyl ether
Concen: 20.995 ug/l
RT: 3.763 min Scan# 439
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37



Tgt Ion: 45 Resp: 90378
Ion Ratio Lower Upper
45 100
43 76.4 54.9 82.3
87 24.7 21.0 31.4
59 11.6 8.7 13.1





#23

Vinyl Acetate

Concen: 108.038 ug/l

RT: 3.721 min Scan# 413

Delta R.T. -0.000 min

Lab File: VX045070.D


Acq: 28 Feb 2025 02:37

Instrument:

MSVOA_X

ClientSampleId :

VSTDICC020

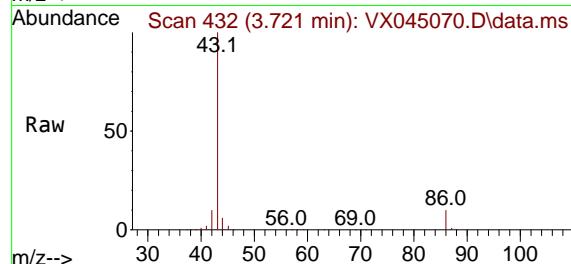

Tgt Ion: 43 Resp: 38180

Ion Ratio Lower Upper

43 100







86 9.9 8.1 12.1


Manual Integrations

APPROVED

Reviewed By :John Carlone 02/28/2025


Supervised By :Mahesh Dadoda 02/28/2025
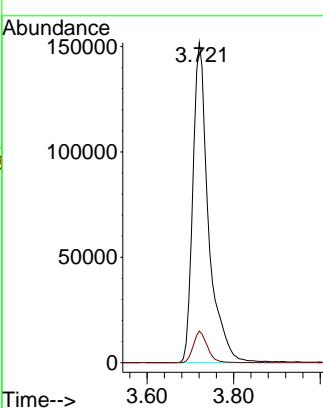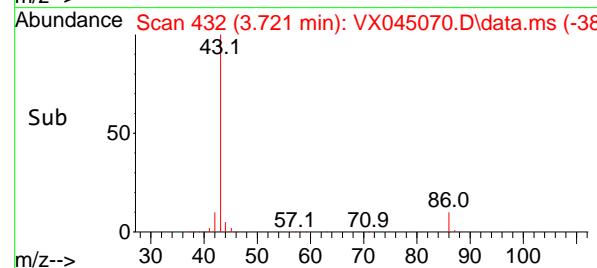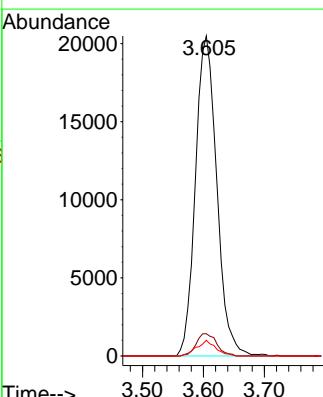
#24
1,1-Dichloroethane
Concen: 20.716 ug/l
RT: 3.605 min Scan# 413
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37Tgt Ion: 63 Resp: 49826
Ion Ratio Lower Upper
63 100
98 7.0 3.4 10.2
100 4.9 2.1 6.5

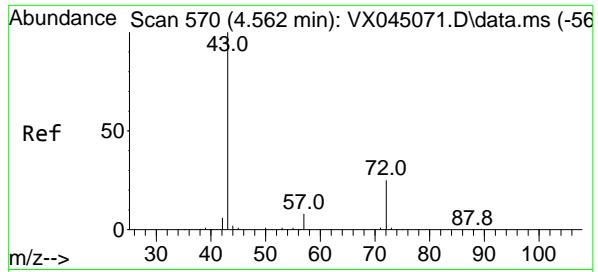

#25
2-Butanone
Concen: 124.449 ug/l
RT: 4.562 min Scan# 51
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020

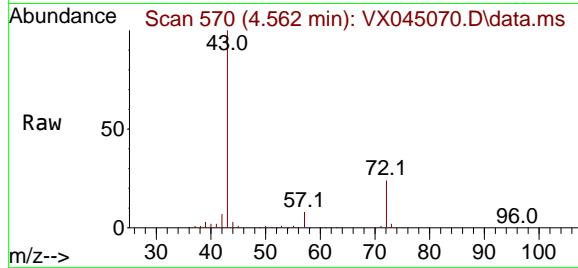


Tgt Ion: 43 Resp: 11871
Ion Ratio Lower Upper
43 100
72 23.5 20.0 30.0

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

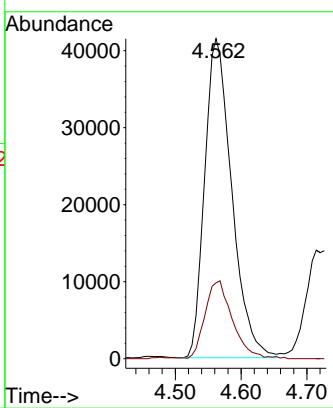


#26
2,2-Dichloropropane
Concen: 12.799 ug/l
RT: 4.470 min Scan# 555
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion: 77 Resp: 22886
Ion Ratio Lower Upper
77 100
97 24.2 12.4 37.0

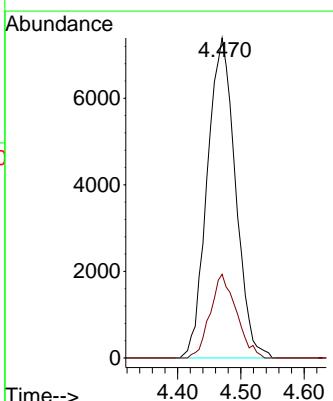

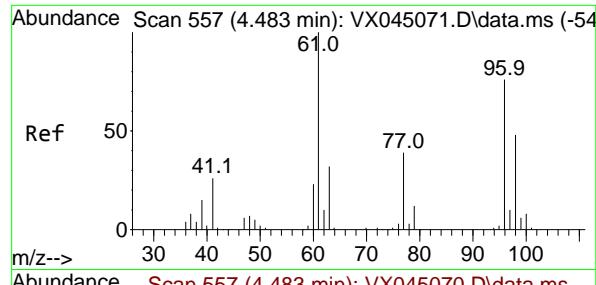



#27
cis-1,2-Dichloroethene
 Concen: 20.065 ug/l
 RT: 4.483 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: VX045070.D
 Acq: 28 Feb 2025 02:37

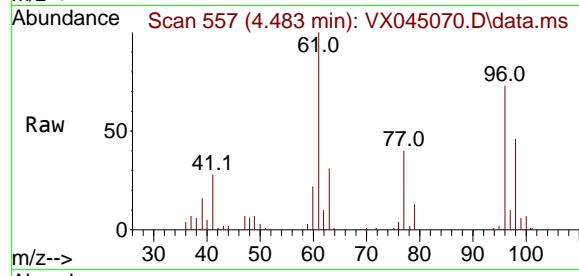


Tgt Ion: 96 Resp: 29788
 Ion Ratio Lower Upper
 96 100
 61 142.7 0.0 283.2
 98 65.6 0.0 128.0

Manual Integrations APPROVED




Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

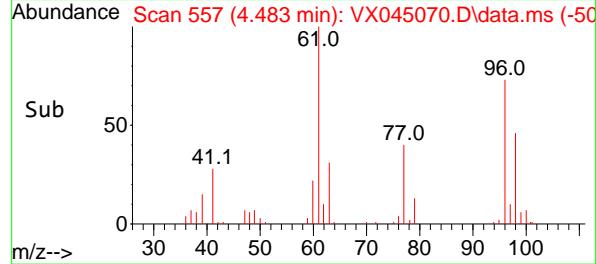


#28
 Bromochloromethane
 Concen: 20.579 ug/l
 RT: 4.891 min Scan# 624
 Delta R.T. -0.006 min
 Lab File: VX045070.D
 Acq: 28 Feb 2025 02:37

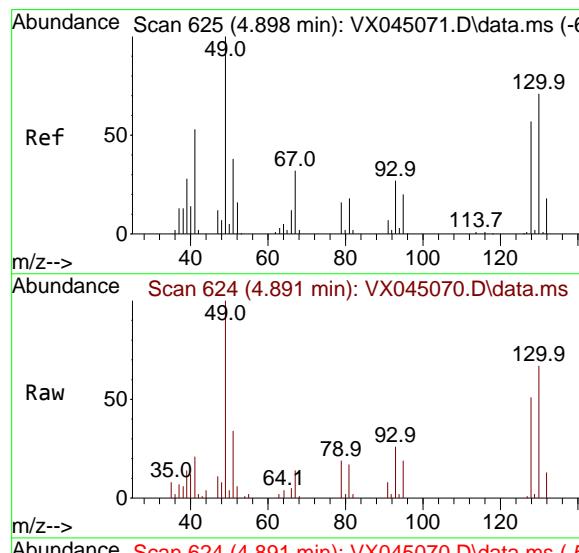

Tgt Ion: 49 Resp: 23869
 Ion Ratio Lower Upper
 49 100
 129 2.0 0.0 3.4
 130 70.6 56.1 84.1

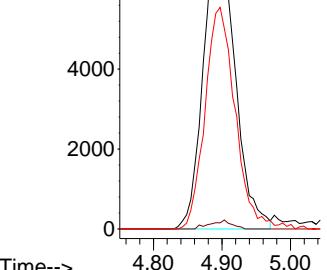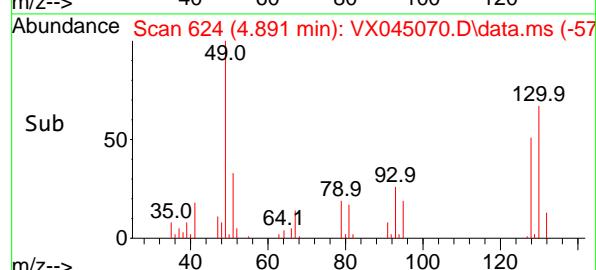



#29

Tetrahydrofuran

Concen: 122.519 ug/l

RT: 5.007 min Scan# 6

Delta R.T. -0.000 min

Lab File: VX045070.D


Acq: 28 Feb 2025 02:37

Instrument :

MSVOA_X

ClientSampleId :



VSTDICC020




Tgt Ion:	Ion Ratio	Resp:	7743
42	100		
72	41.0	Lower	51.1
71	39.0	Upper	47.0

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#30
Chloroform
Concen: 21.147 ug/l
RT: 5.086 min Scan# 656
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion:	Ion Ratio	Resp:	49751
83	100		
85	62.3	Lower	77.2

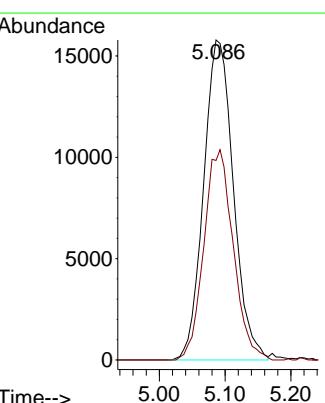






#31
Cyclohexane
Concen: 19.181 ug/l
RT: 5.464 min Scan# 718
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37
Instrument: MSVOA_X
ClientSampleId: VSTDICC020




Tgt Ion: 56 Resp: 42340
Ion Ratio Lower Upper
56 100
69 29.0 23.4 35.2
84 84.2 69.4 104.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

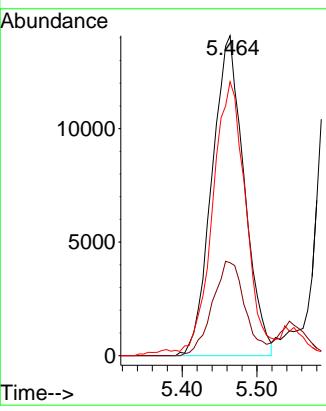


#32
1,1,1-Trichloroethane
Concen: 19.831 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion: 97 Resp: 39276
Ion Ratio Lower Upper
97 100
99 65.2 51.6 77.4
61 48.9 38.4 57.6

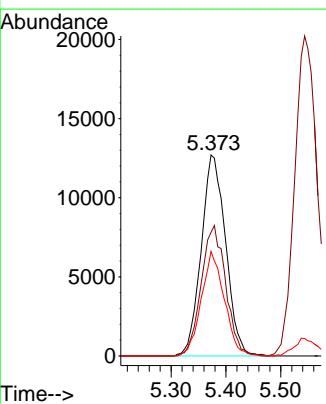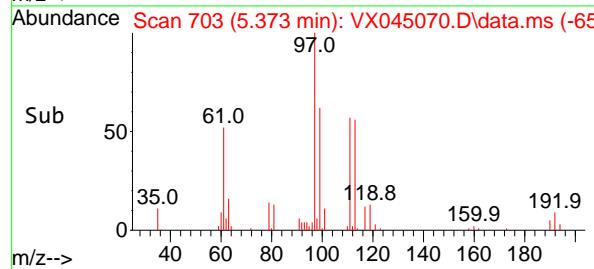



#33
1,2-Dichloroethane-d4
Concen: 21.221 ug/l
RT: 5.958 min Scan# 798
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020




Tgt Ion: 65 Resp: 30514
Ion Ratio Lower Upper
65 100
67 53.2 0.0 106.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

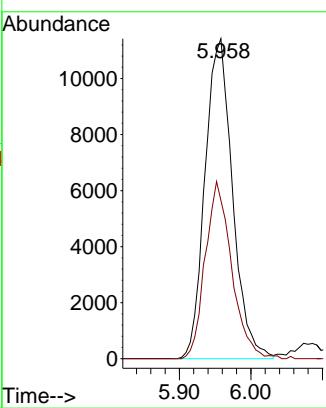


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion:114 Resp: 177403
Ion Ratio Lower Upper
114 100
63 21.3 0.0 41.8
88 16.6 0.0 32.8

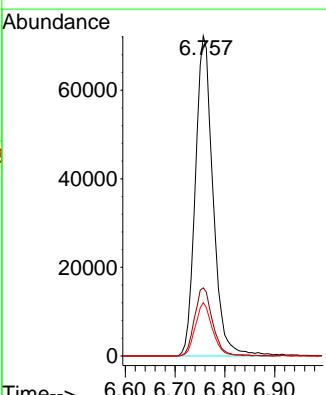






#35
Dibromofluoromethane
Concen: 20.473 ug/l
RT: 5.385 min Scan# 7
Instrument : MSVOA_X
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion:113 Resp: 23739
Ion Ratio Lower Upper
113 100
111 102.7 81.8 122.6
192 17.2 14.3 21.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

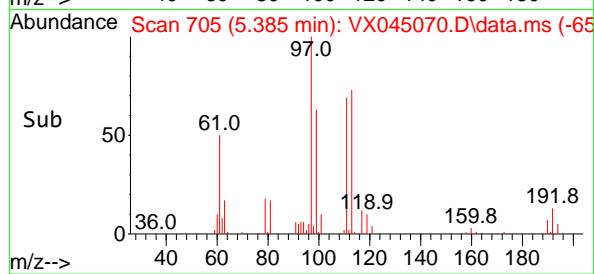


#36
1,1-Dichloropropene
Concen: 18.903 ug/l
RT: 5.684 min Scan# 754
Delta R.T. -0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion: 75 Resp: 31519
Ion Ratio Lower Upper
75 100
110 34.4 16.9 50.6
77 30.3 24.5 36.7





#37
Ethyl Acetate
 Concen: 22.714 ug/l
 RT: 4.714 min Scan# 595
 Delta R.T. -0.000 min
 Lab File: VX045070.D
 Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
 ClientSampleId : VSTDICC020




Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
43	100	4309		
61	13.4		10.8	16.2
70	10.1		7.7	11.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

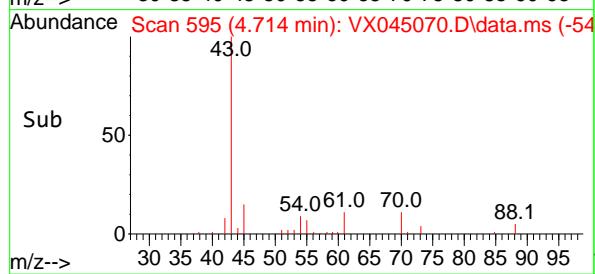


#38
Carbon Tetrachloride
 Concen: 19.334 ug/l
 RT: 5.671 min Scan# 752
 Delta R.T. -0.000 min
 Lab File: VX045070.D
 Acq: 28 Feb 2025 02:37




Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
117	100	31694		
119	98.7		76.7	115.1
121	30.7		25.5	38.3

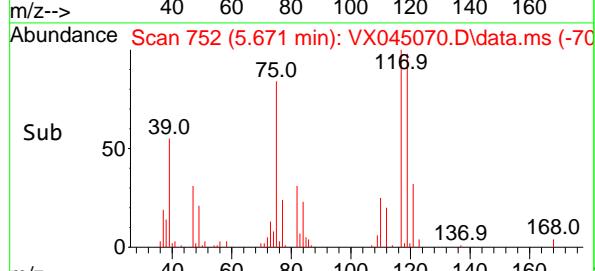



#39
Methylcyclohexane
Concen: 18.676 ug/l
RT: 7.372 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37



Instrument : MSVOA_X
ClientSampleId : VSTDICC020




Tgt Ion: 83 Resp: 39769
Ion Ratio Lower Upper
83 100
55 74.6 63.0 94.4
98 48.7 39.7 59.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#40
Benzene
Concen: 20.298 ug/l
RT: 6.031 min Scan# 811
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion: 78 Resp: 105787
Ion Ratio Lower Upper
78 100
77 24.3 18.8 28.2

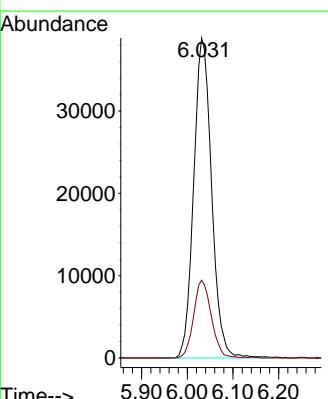



#41
Methacrylonitrile
Concen: 23.605 ug/l
RT: 4.928 min Scan# 6
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
ClientSampleId : VSTDICC020



Tgt Ion: 41 Resp: 23924
Ion Ratio Lower Upper
41 100
39 55.3 44.6 67.0
67 71.6 53.9 80.9
52 30.7 23.3 34.9




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

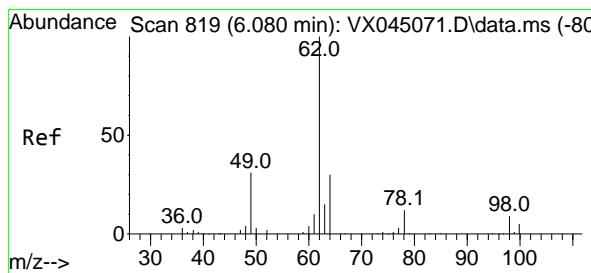

#42
1,2-Dichloroethane
Concen: 22.886 ug/l
RT: 6.086 min Scan# 820
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion: 62 Resp: 38653
Ion Ratio Lower Upper
62 100
98 8.8 0.0 18.2

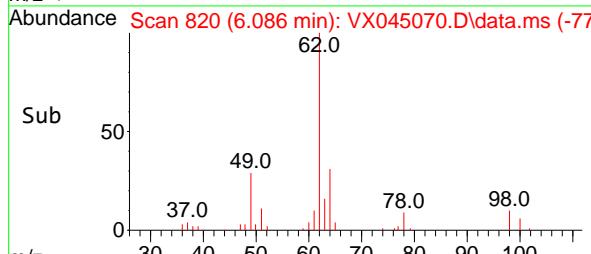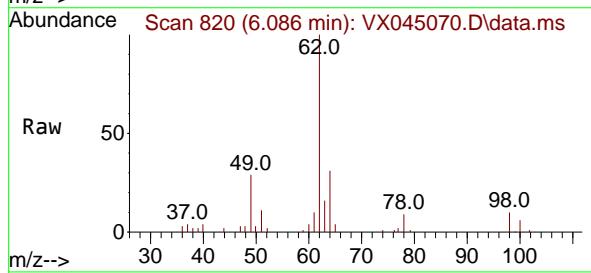



#43
Isopropyl Acetate
Concen: 22.094 ug/l
RT: 6.348 min Scan# 8
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
ClientSampleId : VSTDICC020




Tgt Ion: 43 Resp: 6672
Ion Ratio Lower Upper
43 100
61 17.8 14.9 22.3
87 11.5 9.4 14.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

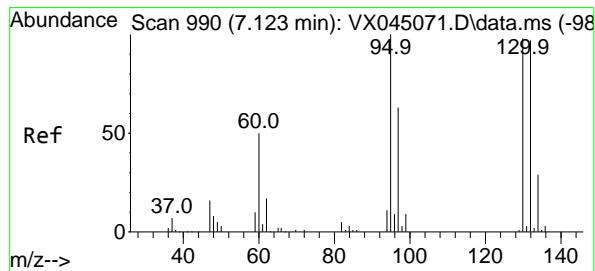


#44
Trichloroethene
Concen: 20.191 ug/l
RT: 7.122 min Scan# 990
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion:130 Resp: 24052
Ion Ratio Lower Upper
130 100
95 100.3 0.0 205.0

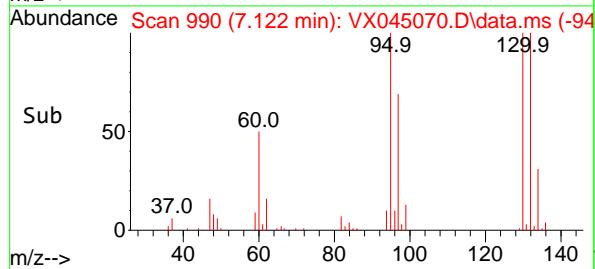



#45
1,2-Dichloropropane
Concen: 20.945 ug/l
RT: 7.427 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020



Tgt Ion: 63 Resp: 27123
Ion Ratio Lower Upper
63 100
65 30.1 24.7 37.1




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#46
Dibromomethane
Concen: 21.357 ug/l
RT: 7.580 min Scan# 1065
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion: 93 Resp: 19323
Ion Ratio Lower Upper
93 100
95 86.4 65.8 98.8
174 89.6 72.2 108.2

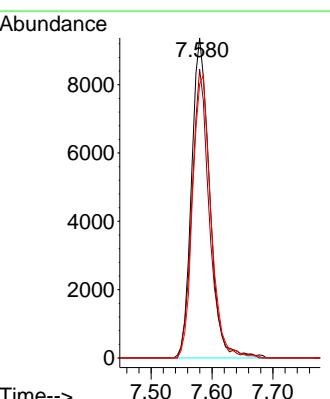



#47
 Bromodichloromethane
 Concen: 21.732 ug/l
 RT: 7.817 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX045070.D
 Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
 ClientSampleId : VSTDICC020




Tgt Ion: 83 Resp: 3803
 Ion Ratio Lower Upper
 83 100
 85 61.3 51.1 76.7
 127 7.8 6.4 9.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025




#48
 Methyl methacrylate
 Concen: 22.757 ug/l
 RT: 7.695 min Scan# 1084
 Delta R.T. 0.006 min
 Lab File: VX045070.D
 Acq: 28 Feb 2025 02:37




Tgt Ion: 41 Resp: 32627
 Ion Ratio Lower Upper
 41 100
 69 81.2 63.0 94.6
 39 59.8 47.5 71.3

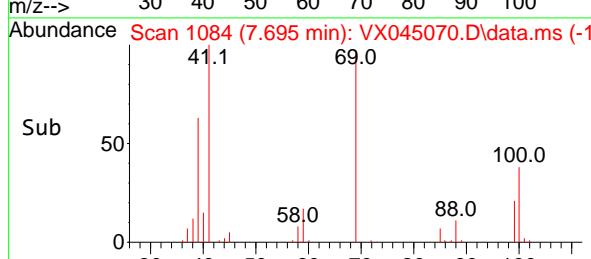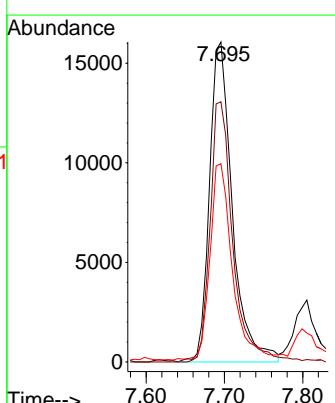



#49
1,4-Dioxane
Concen: 479.170 ug/l
RT: 7.665 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
ClientSampleId : VSTDICC020




Tgt Ion: 88 Resp: 1460:
Ion Ratio Lower Upper
88 100
43 38.7 28.7 43.1
58 68.3 55.8 83.8

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#50
Toluene-d8
Concen: 19.469 ug/l
RT: 8.646 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion: 98 Resp: 84516
Ion Ratio Lower Upper
98 100
100 67.2 52.0 78.0

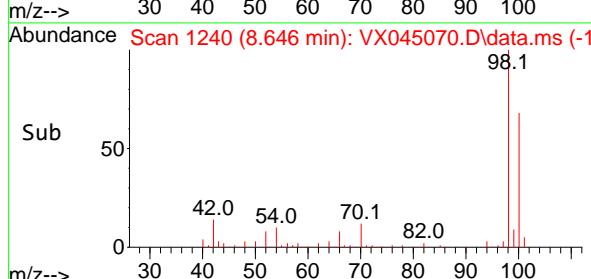



#51
4-Methyl-2-Pentanone
Concen: 124.081 ug/l
RT: 8.573 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
ClientSampleId : VSTDICC020



Tgt Ion: 43 Resp: 22961
Ion Ratio Lower Upper
43 100
58 37.5 29.2 43.8



Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#52
Toluene
Concen: 20.463 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion: 92 Resp: 63326
Ion Ratio Lower Upper
92 100
91 173.7 138.9 208.3



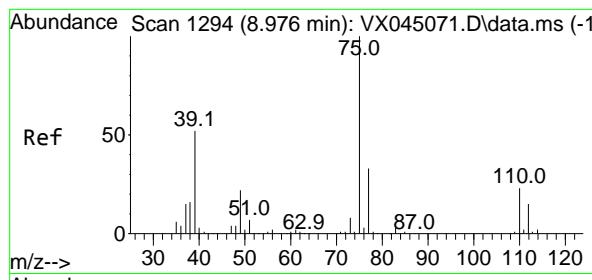

#53
t-1,3-Dichloropropene
Concen: 17.871 ug/l
RT: 8.976 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
ClientSampleId : VSTDICC020



Tgt Ion: 75 Resp: 30911
Ion Ratio Lower Upper
75 100
77 31.5 26.5 39.7




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

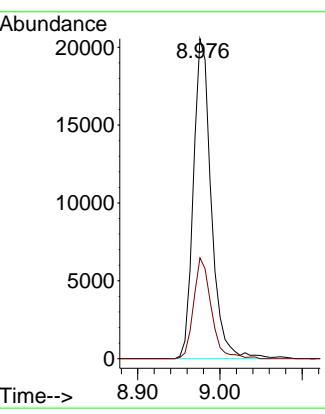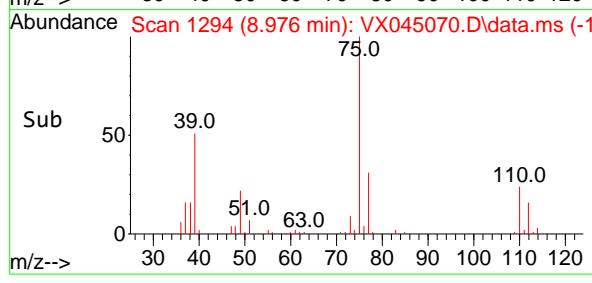

#54
cis-1,3-Dichloropropene
Concen: 18.675 ug/l
RT: 8.366 min Scan# 1194
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion: 75 Resp: 36118
Ion Ratio Lower Upper
75 100
77 29.9 24.7 37.1
39 53.5 40.7 61.1

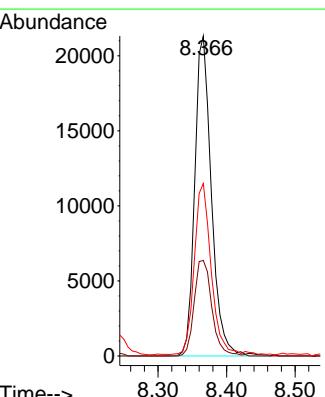



#55
1,1,2-Trichloroethane
Concen: 21.992 ug/l
RT: 9.152 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37



Instrument : MSVOA_X
ClientSampleId : VSTDICC020

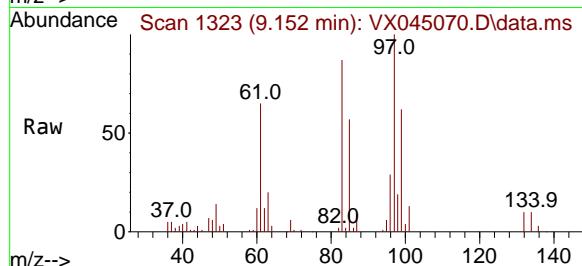

Tgt Ion: 97 Resp: 2635:
Ion Ratio Lower Upper
97 100
83 86.7 69.4 104.2
85 57.3 44.1 66.1
99 62.1 50.7 76.1





Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#56
Ethyl methacrylate
Concen: 20.791 ug/l
RT: 9.116 min Scan# 1317
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion: 69 Resp: 39850
Ion Ratio Lower Upper
69 100
41 73.6 57.0 85.4
39 40.6 34.2 51.4

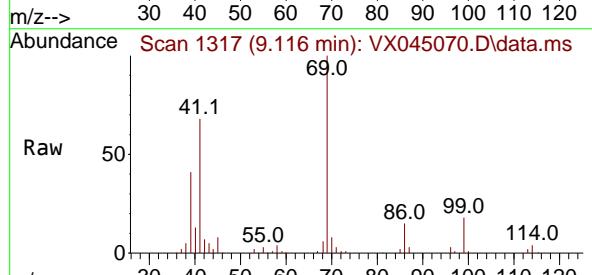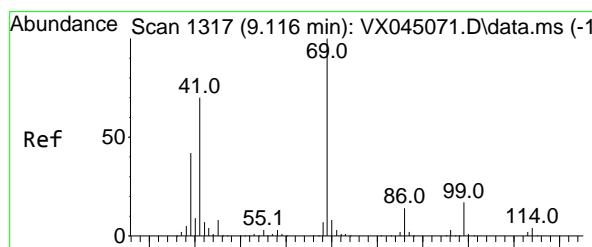



#57
1,3-Dichloropropane
Concen: 21.836 ug/l
RT: 9.305 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
ClientSampleId : VSTDICC020



Tgt Ion: 76 Resp: 4564
Ion Ratio Lower Upper
76 100
78 31.9 25.5 38.3




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

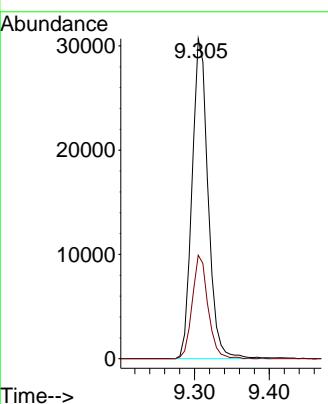

#58
2-Chloroethyl Vinyl ether
Concen: 102.342 ug/l
RT: 8.238 min Scan# 1173
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion: 63 Resp: 96311
Ion Ratio Lower Upper
63 100
106 26.4 21.5 32.3

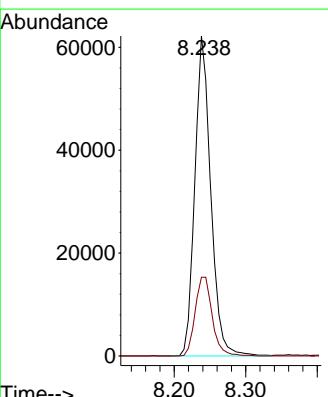



#59
2-Hexanone
Concen: 126.428 ug/l
RT: 9.433 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020



Tgt Ion: 43 Resp: 16876
Ion Ratio Lower Upper
43 100
58 51.6 25.9 77.6




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

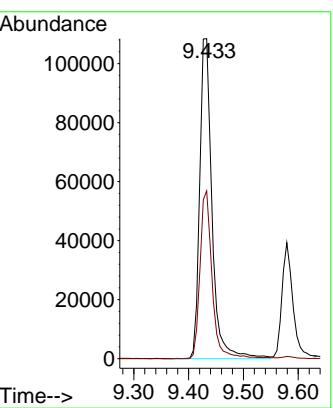

#60
Dibromochloromethane
Concen: 21.668 ug/l
RT: 9.518 min Scan# 1383
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion:129 Resp: 27705
Ion Ratio Lower Upper
129 100
127 77.8 38.5 115.5

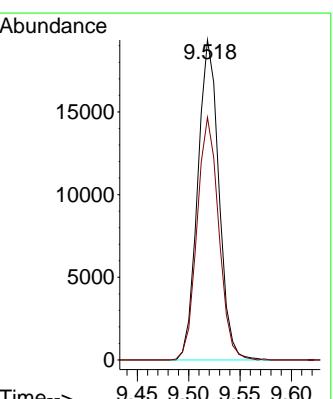



#61
1,2-Dibromoethane
Concen: 21.764 ug/l
RT: 9.610 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
ClientSampleId : VSTDICC020



Tgt Ion:107 Resp: 2631:
Ion Ratio Lower Upper
107 100
109 93.3 76.1 114.1




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

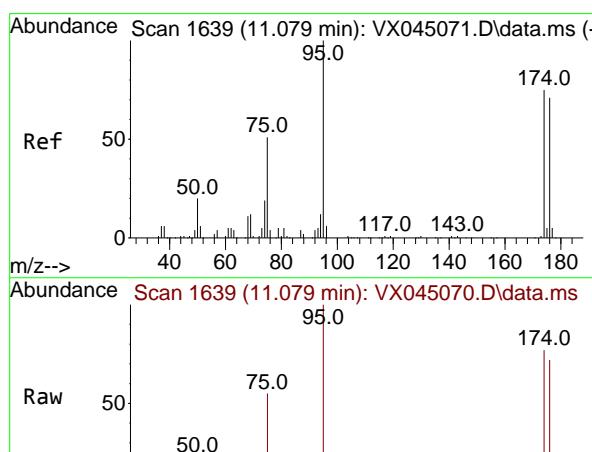

#62
4-Bromofluorobenzene
Concen: 19.215 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

Tgt Ion: 95 Resp: 27856
Ion Ratio Lower Upper
95 100
174 76.1 0.0 148.2
176 72.8 0.0 141.4




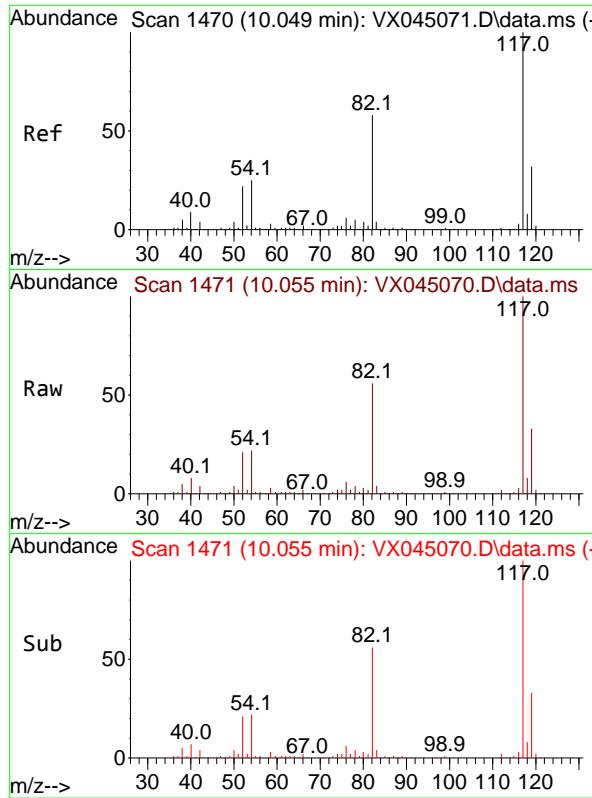


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1470
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

Instrument : MSVOA_X
ClientSampleId : VSTDICC020


Manual Integrations
APPROVED


Reviewed By :John Carbone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

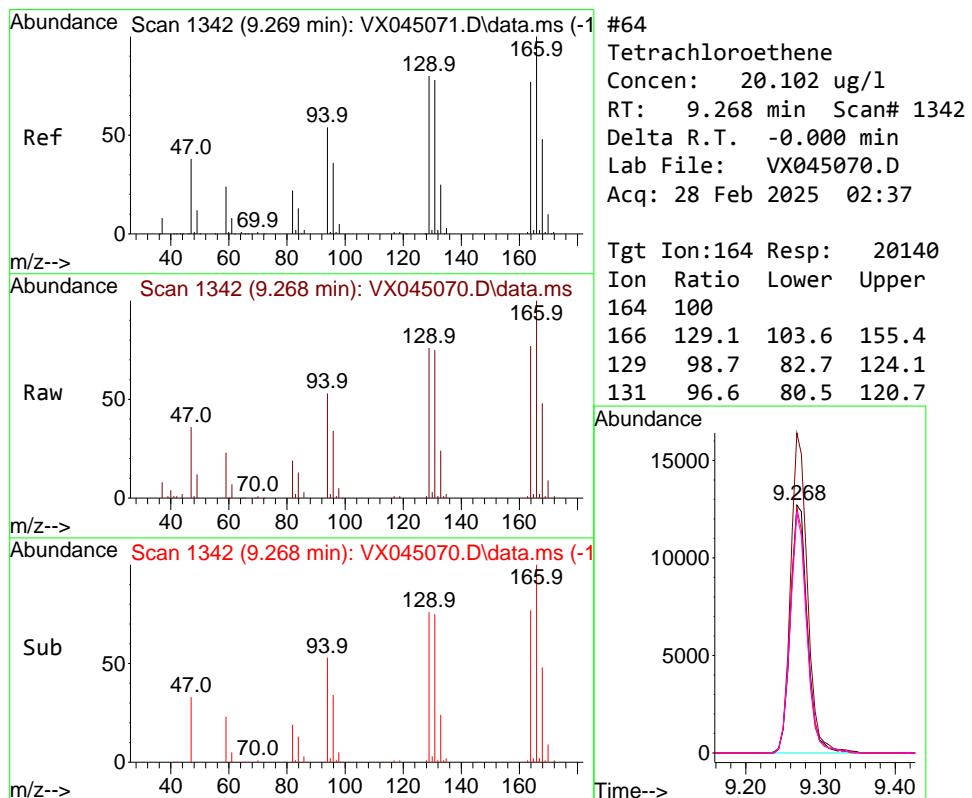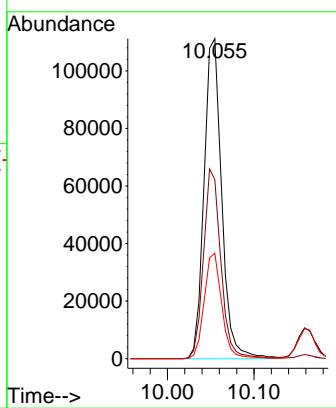


#64
Tetrachloroethene
Concen: 20.102 ug/l
RT: 9.268 min Scan# 1342
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

Tgt Ion:164 Resp: 20140
Ion Ratio Lower Upper
164 100
166 129.1 103.6 155.4
129 98.7 82.7 124.1
131 96.6 80.5 120.7

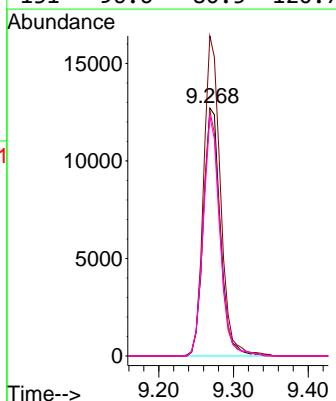

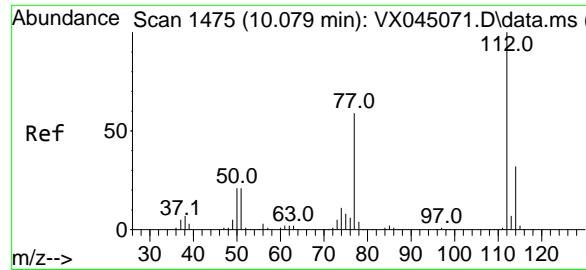



#65
Chlorobenzene
Concen: 20.316 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37
Instrument:
MSVOA_X
ClientSampleId :
VSTDICC020

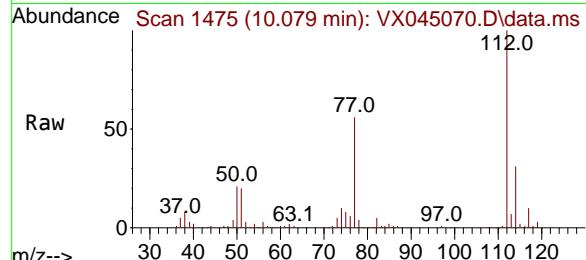


Tgt Ion:112 Resp: 6877
Ion Ratio Lower Upper
112 100
114 31.3 26.0 39.0

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

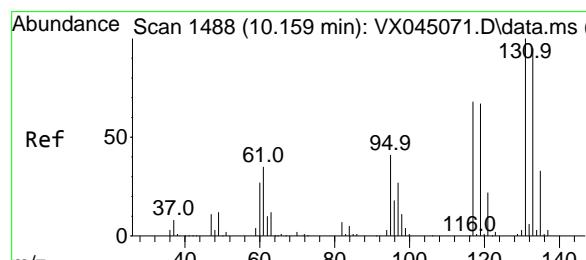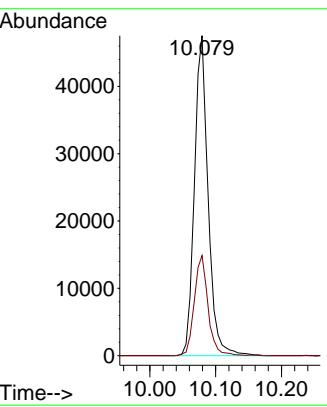


#66
1,1,1,2-Tetrachloroethane
Concen: 20.627 ug/l
RT: 10.158 min Scan# 1488
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

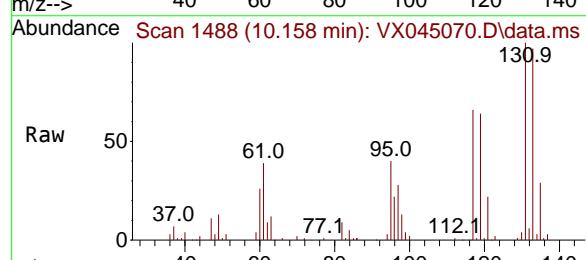

Tgt Ion:131 Resp: 22508
Ion Ratio Lower Upper
131 100
133 94.6 48.6 145.9
119 65.4 33.9 101.7





#67

Ethyl Benzene

Concen: 19.905 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. -0.000 min

Lab File: VX045070.D


Acq: 28 Feb 2025 02:37

Instrument :

MSVOA_X

ClientSampleId :

VSTDICC020


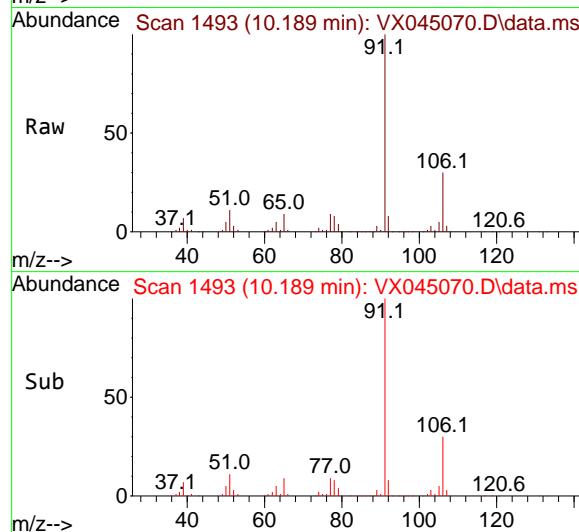


Tgt Ion: 91 Resp: 119161

Ion	Ratio	Lower	Upper
91	100		
106	29.9	23.9	35.9

Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

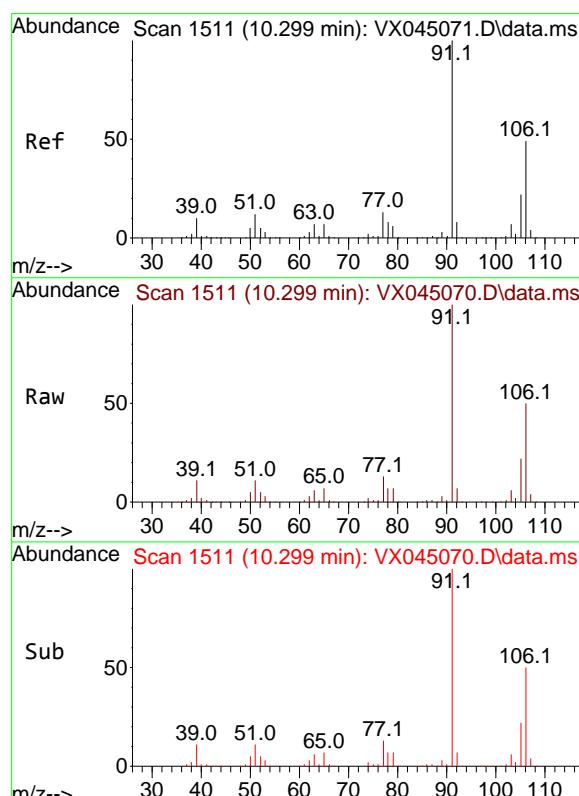

#68

m/p-Xylenes

Concen: 40.699 ug/l

RT: 10.299 min Scan# 1511


Delta R.T. -0.000 min


Lab File: VX045070.D

Acq: 28 Feb 2025 02:37


Tgt Ion:106 Resp: 89735

Ion	Ratio	Lower	Upper
106	100		
91	204.2	165.4	248.0

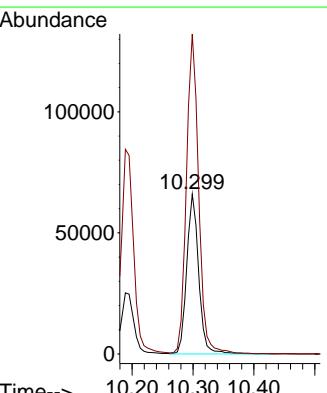






#69
o-Xylene
Concen: 20.018 ug/l
RT: 10.640 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37
Instrument: MSVOA_X
ClientSampleId: VSTDICC020




Tgt Ion:106 Resp: 4428
Ion Ratio Lower Upper
106 100
91 216.8 109.9 329.6

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

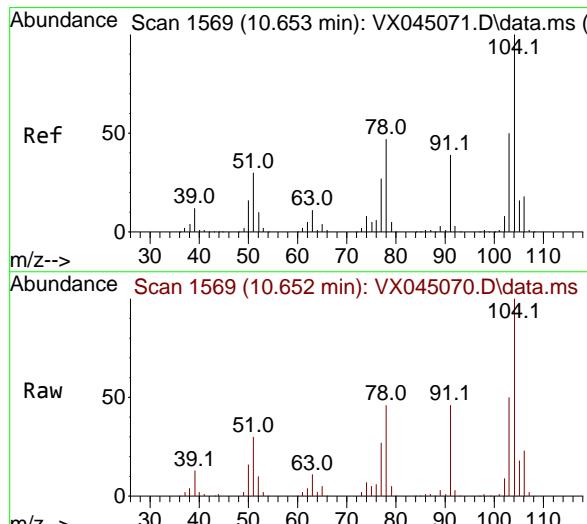


#70
Styrene
Concen: 20.767 ug/l
RT: 10.652 min Scan# 1569
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

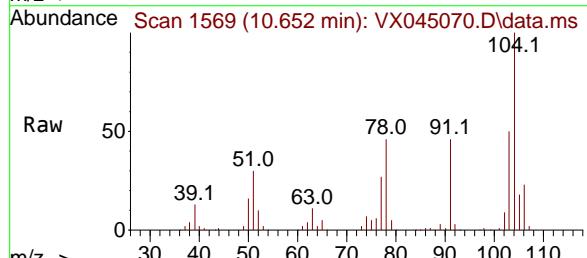


Tgt Ion:104 Resp: 73832
Ion Ratio Lower Upper
104 100
78 50.9 42.2 63.4
103 54.1 43.8 65.8





#71
Bromoform
Concen: 21.449 ug/l
RT: 10.799 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020



Tgt Ion:173 Resp: 17400
Ion Ratio Lower Upper
173 100
175 49.7 24.6 73.6
254 0.0 0.0 0.0





Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

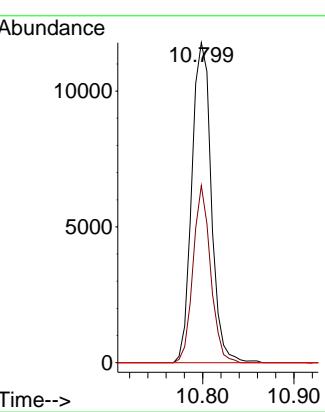

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion:152 Resp: 70072
Ion Ratio Lower Upper
152 100
115 70.9 44.2 132.6
150 163.4 0.0 349.0

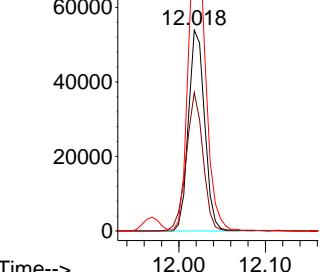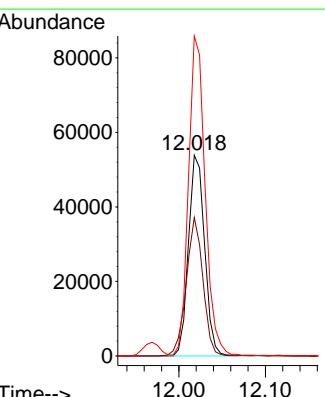



#73
Isopropylbenzene
Concen: 19.794 ug/l
RT: 10.963 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020




Tgt Ion:105 Resp: 112095
Ion Ratio Lower Upper
105 100
120 26.7 13.2 39.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#74
N-amyl acetate
Concen: 20.606 ug/l
RT: 10.841 min Scan# 1600
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37



Tgt Ion: 43 Resp: 52972
Ion Ratio Lower Upper
43 100
70 40.0 31.8 47.6
55 23.0 18.3 27.5
61 21.7 18.3 27.5




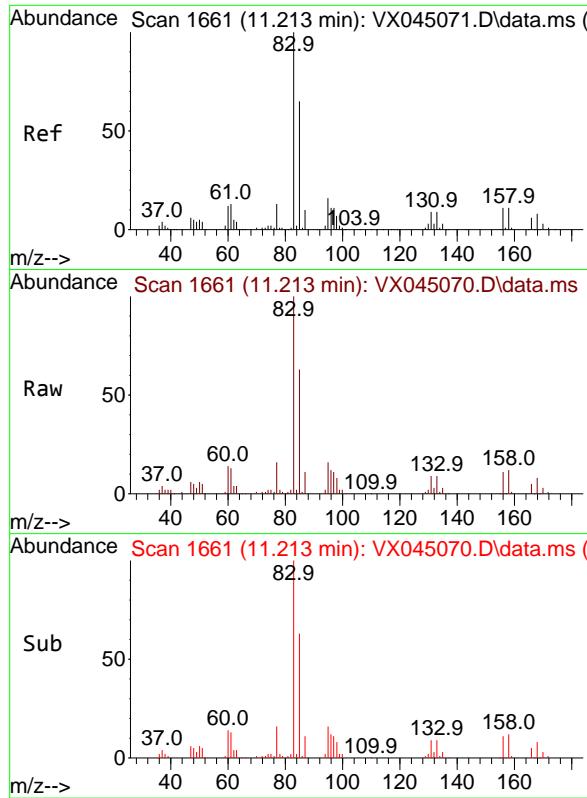


#75
1,1,2,2-Tetrachloroethane
Concen: 21.738 ug/l
RT: 11.213 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

Instrument : MSVOA_X
ClientSampleId : VSTDICC020


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

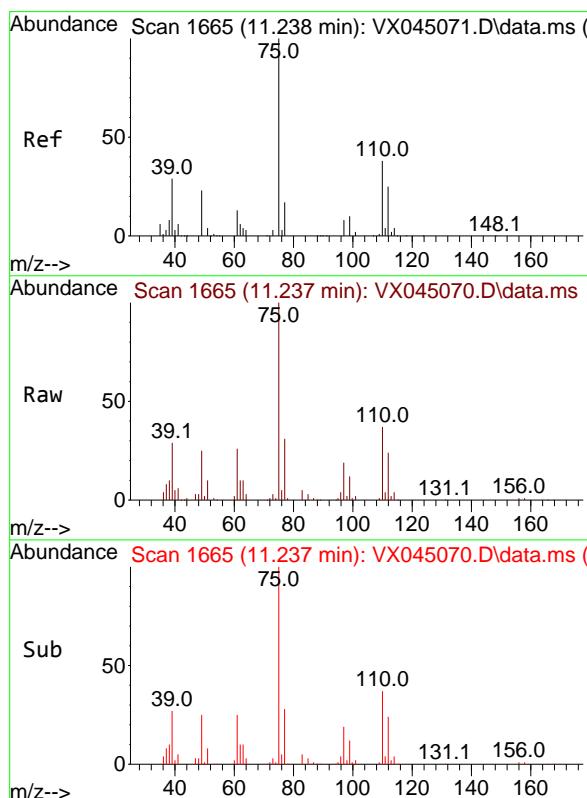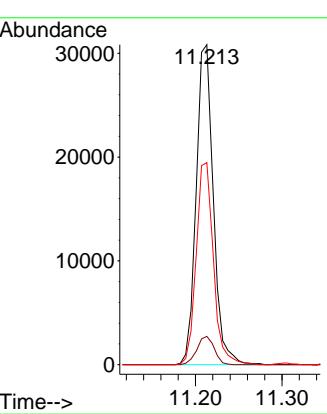

#76
1,2,3-Trichloropropane
Concen: 21.394 ug/l
RT: 11.237 min Scan# 1665
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion: 75 Resp: 33440
Ion Ratio Lower Upper
75 100
77 40.6 20.7 62.1





#77
Bromobenzene
Concen: 20.466 ug/l
RT: 11.195 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37



Instrument : MSVOA_X
ClientSampleId : VSTDICC020




Tgt Ion:156 Resp: 26310
Ion Ratio Lower Upper
156 100
77 170.2 85.8 257.4
158 95.9 48.4 145.2

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#78
n-propylbenzene
Concen: 19.641 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Tgt Ion: 91 Resp: 128284
Ion Ratio Lower Upper
91 100
120 22.3 11.2 33.6





#79
2-Chlorotoluene
Concen: 19.775 ug/l
RT: 11.359 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020



Tgt Ion: 91 Resp: 7927
Ion Ratio Lower Upper
91 100
126 33.1 16.4 49.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

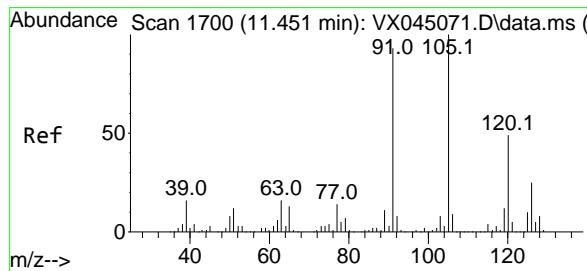

#80
1,3,5-Trimethylbenzene
Concen: 20.581 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

Tgt Ion:105 Resp: 94545
Ion Ratio Lower Upper
105 100
120 46.8 24.1 72.2

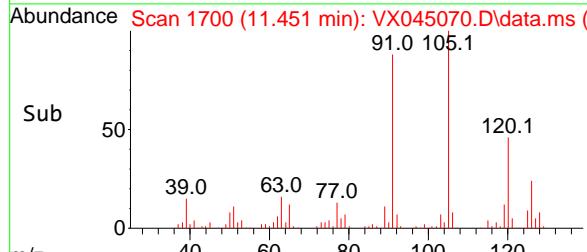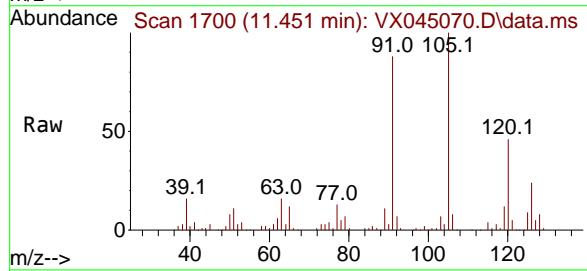


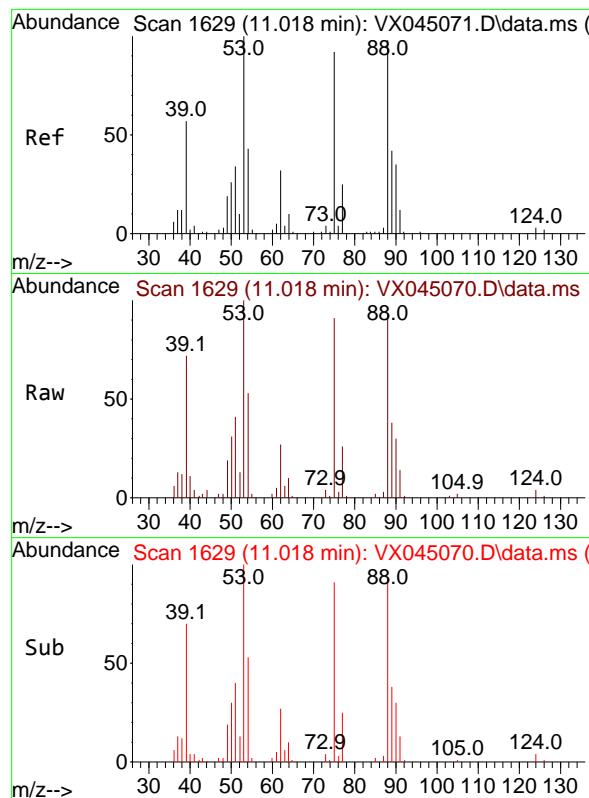


#81
trans-1,4-Dichloro-2-butene
Concen: 15.196 ug/l
RT: 11.018 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC020


Manual Integrations APPROVED




Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

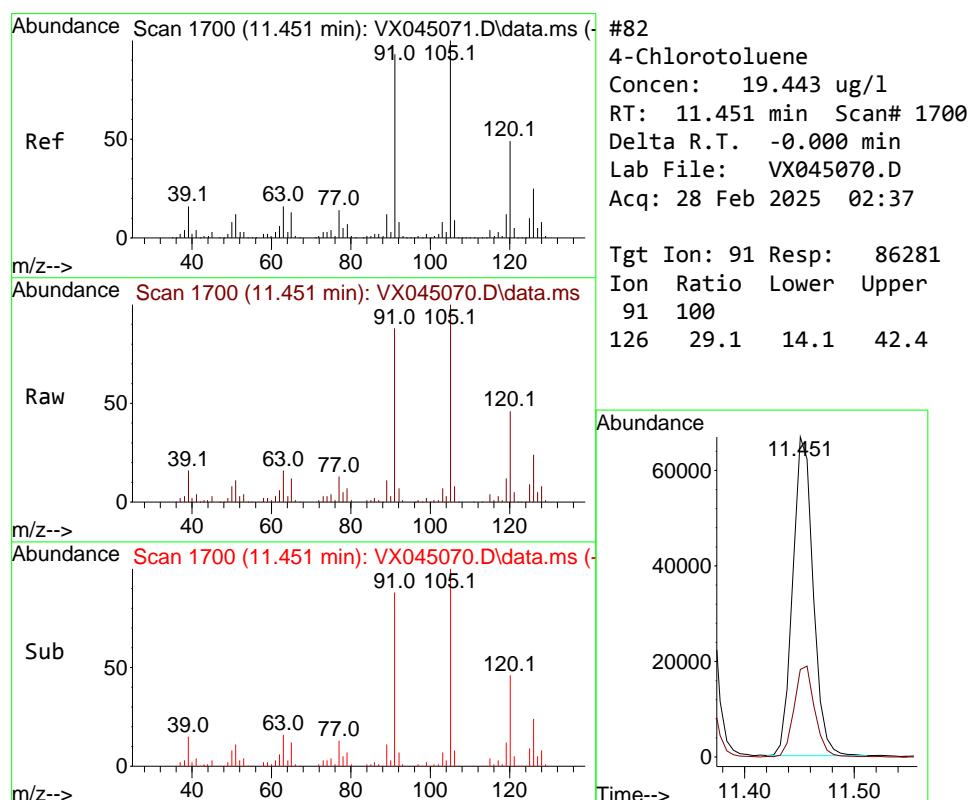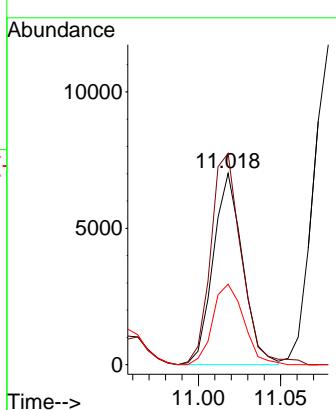

#82
4-Chlorotoluene
Concen: 19.443 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

Tgt Ion: 91 Resp: 86281
Ion Ratio Lower Upper
91 100
126 29.1 14.1 42.4

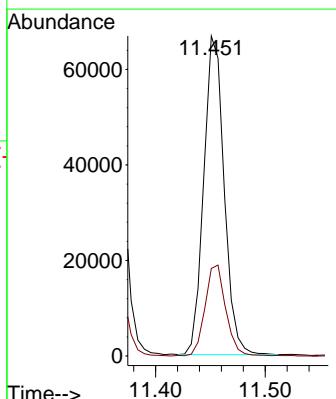

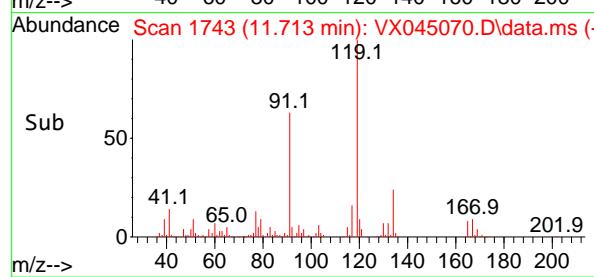

#83

tert-Butylbenzene

Concen: 20.159 ug/l

RT: 11.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045070.D

Acq: 28 Feb 2025 02:37





Instrument:

MSVOA_X

ClientSampleId :

VSTDICC020

**Manual Integrations
APPROVED**

 Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025


#84

1,2,4-Trimethylbenzene

Concen: 20.943 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX045070.D


Acq: 28 Feb 2025 02:37


Tgt Ion:105 Resp: 94734

Ion Ratio Lower Upper


105 100

120 44.3 22.1 66.1

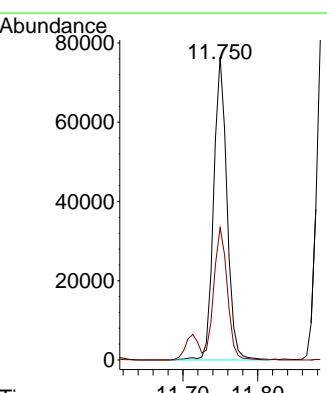

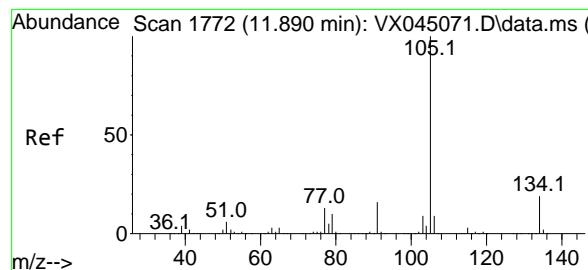



#85
sec-Butylbenzene
Concen: 20.160 ug/l
RT: 11.890 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37
Instrument: MSVOA_X
ClientSampleId: VSTDICC020




Tgt Ion:105 Resp: 115951
Ion Ratio Lower Upper
105 100
134 19.6 9.8 29.4

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#86
p-Isopropyltoluene
Concen: 19.827 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37



Tgt Ion:119 Resp: 91554
Ion Ratio Lower Upper
119 100
134 26.8 12.9 38.6
91 25.6 12.7 38.0

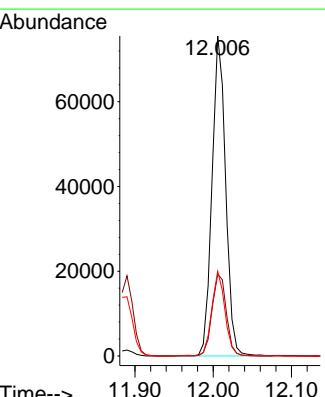

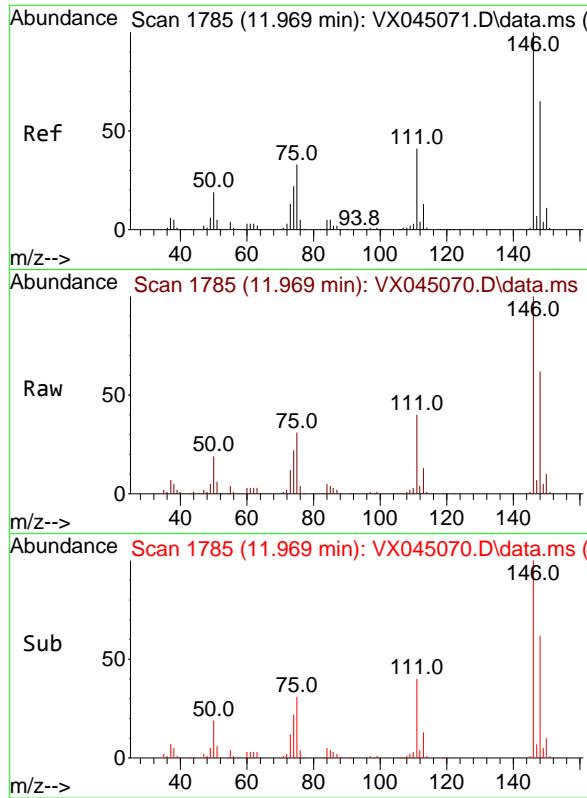



#87
1,3-Dichlorobenzene
Concen: 20.400 ug/l
RT: 11.969 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

Instrument : MSVOA_X
ClientSampleId : VSTDICC020

**Manual Integrations
APPROVED**


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025


Tgt Ion:146 Resp: 47934
Ion Ratio Lower Upper
146 100
111 40.2 21.1 63.4
148 61.6 31.9 95.7

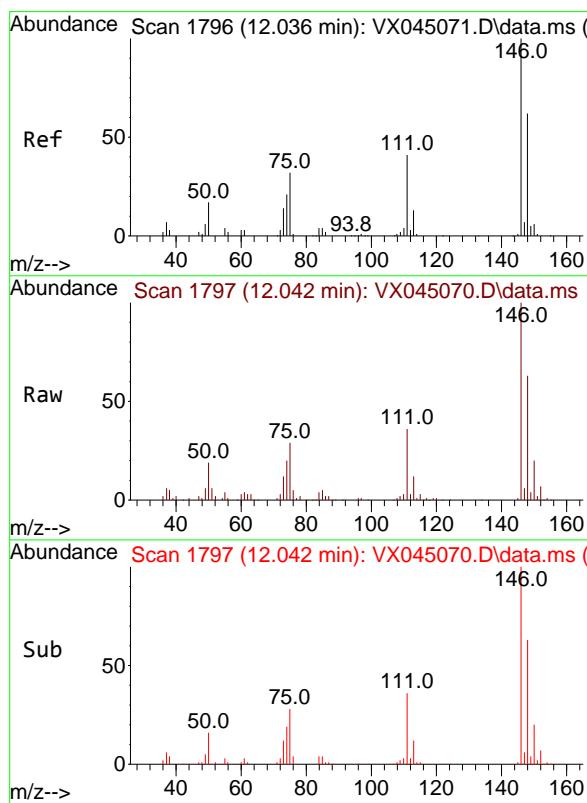

#88
1,4-Dichlorobenzene
Concen: 19.615 ug/l
RT: 12.042 min Scan# 1797
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37


Tgt Ion:146 Resp: 46657
Ion Ratio Lower Upper
146 100
111 41.4 20.2 60.5
148 63.8 31.9 95.9

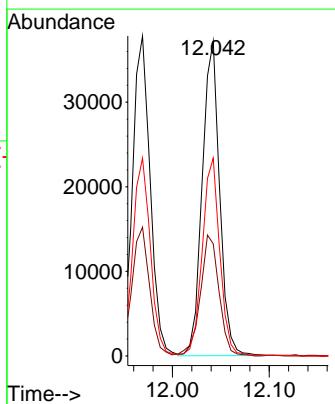



#89
n-Butylbenzene
Concen: 19.249 ug/l
RT: 12.329 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37



Instrument : MSVOA_X
ClientSampleId : VSTDICC020



Tgt Ion: 91 Resp: 78139
Ion Ratio Lower Upper
91 100
92 52.9 26.7 80.0
134 24.3 12.2 36.6



Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#90
Hexachloroethane
Concen: 18.483 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

Tgt Ion:117 Resp: 15919
Ion Ratio Lower Upper
117 100
201 65.6 31.9 95.9

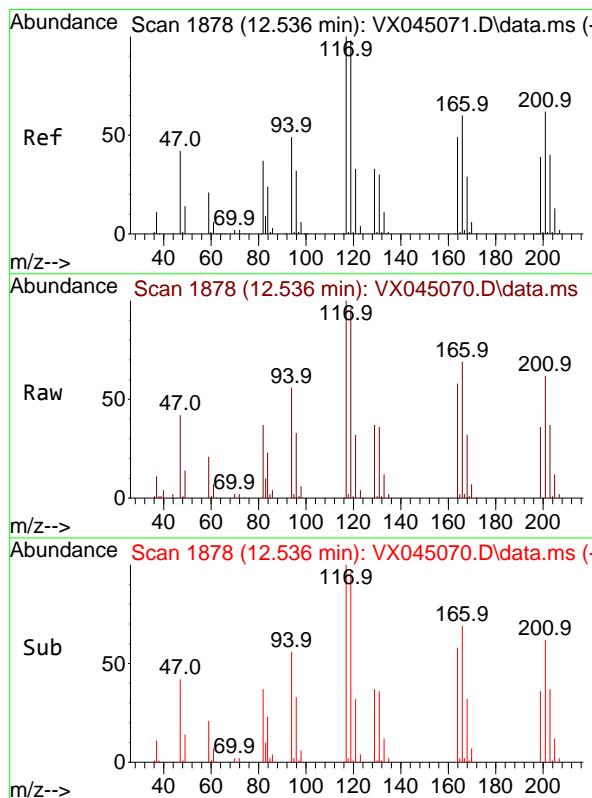


Sub



#91
1,2-Dichlorobenzene
Concen: 21.031 ug/l
RT: 12.335 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument : MSVOA_X
ClientSampleId : VSTDICC020




Tgt Ion:146 Resp: 4863
Ion Ratio Lower Upper
146 100
111 42.6 21.6 65.0
148 62.1 31.9 95.9

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

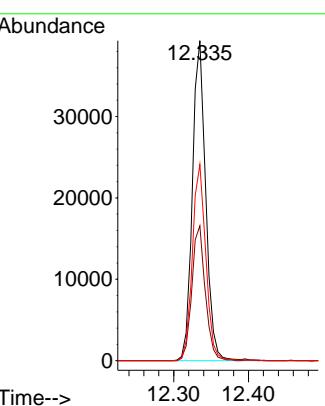


#92
1,2-Dibromo-3-Chloropropane
Concen: 22.119 ug/l
RT: 12.944 min Scan# 1945
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37



Tgt Ion: 75 Resp: 7987
Ion Ratio Lower Upper
75 100
155 78.7 39.6 118.7
157 103.3 51.1 153.4




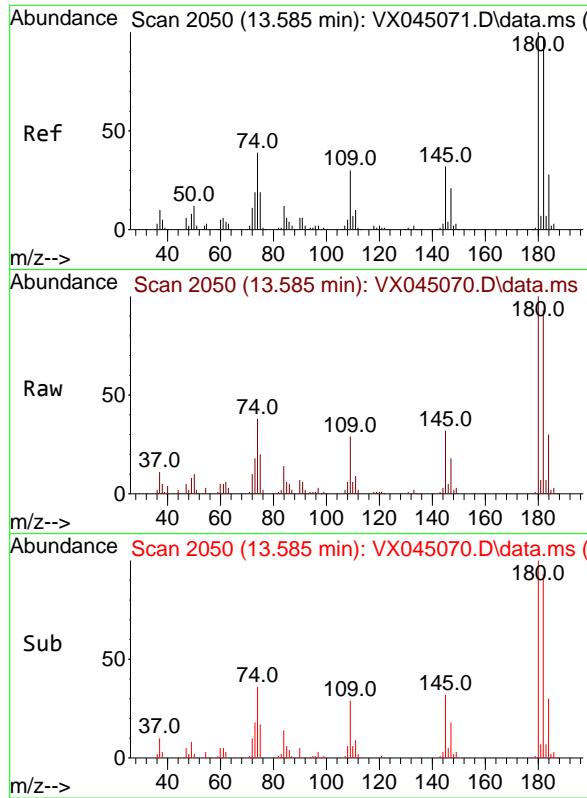


#93
 1,2,4-Trichlorobenzene
 Concen: 19.617 ug/l
 RT: 13.585 min Scan# 2
 Delta R.T. -0.000 min
 Lab File: VX045070.D
 Acq: 28 Feb 2025 02:37

Instrument : MSVOA_X
 ClientSampleId : VSTDICC020


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

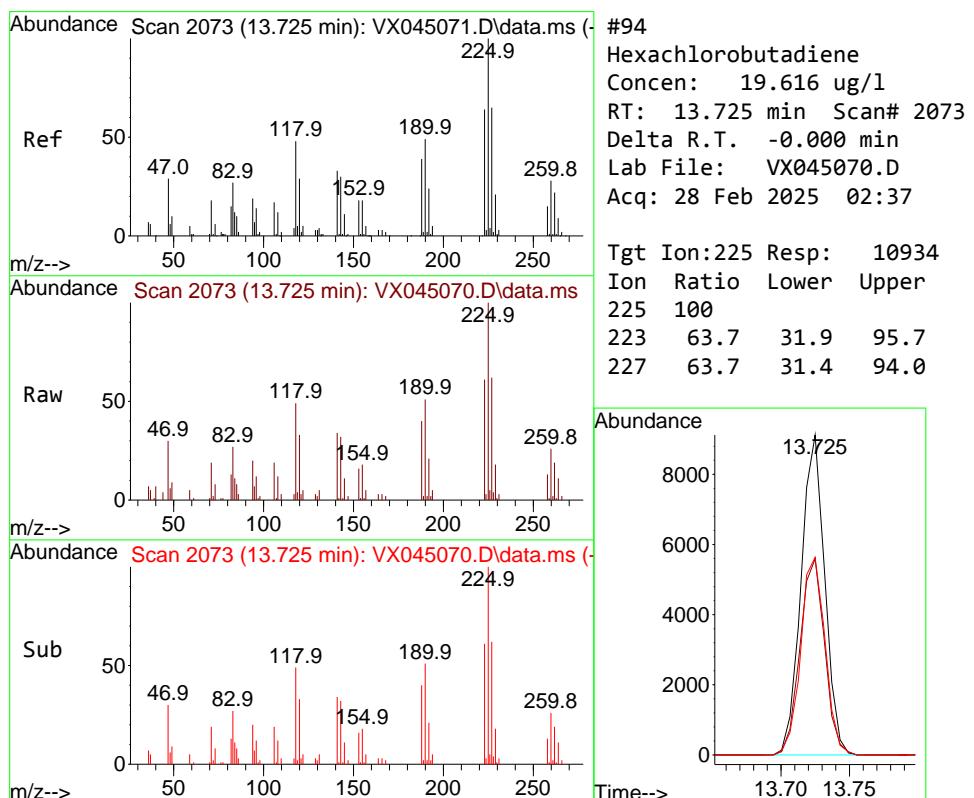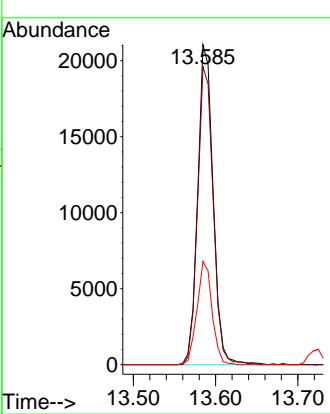

#94
 Hexachlorobutadiene
 Concen: 19.616 ug/l
 RT: 13.725 min Scan# 2073
 Delta R.T. -0.000 min
 Lab File: VX045070.D
 Acq: 28 Feb 2025 02:37


Tgt Ion:225 Resp: 10934
 Ion Ratio Lower Upper
 225 100
 223 63.7 31.9 95.7
 227 63.7 31.4 94.0

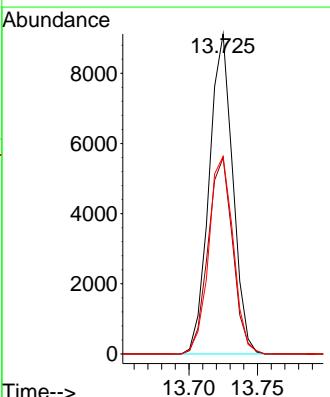

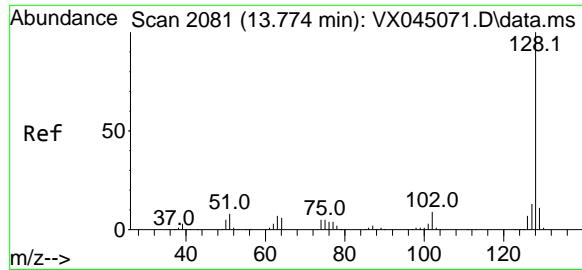

#95
Naphthalene
Concen: 21.279 ug/l
RT: 13.774 min Scan# 2111
Delta R.T. -0.000 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37




Instrument: MSVOA_X
ClientSampleId: VSTDICC020

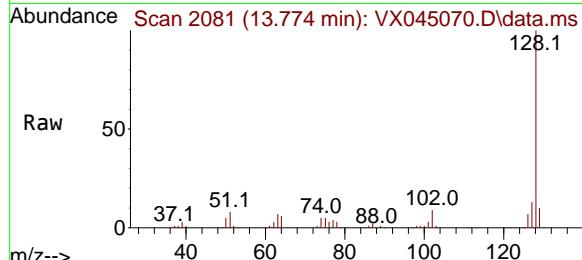


Tgt Ion:128 Resp: 108350
Ion Ratio Lower Upper
128 100
127 12.7 10.3 15.5
129 10.8 8.7 13.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

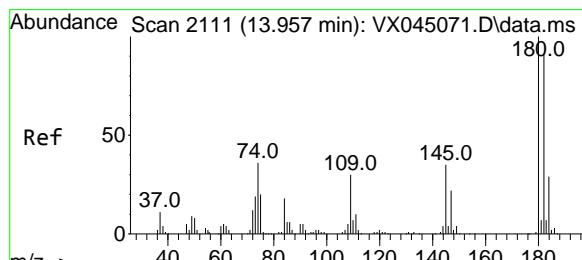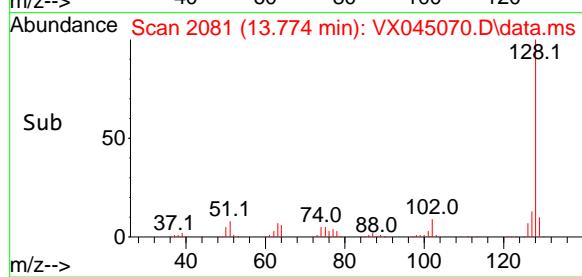

#96
1,2,3-Trichlorobenzene
Concen: 20.432 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.006 min
Lab File: VX045070.D
Acq: 28 Feb 2025 02:37

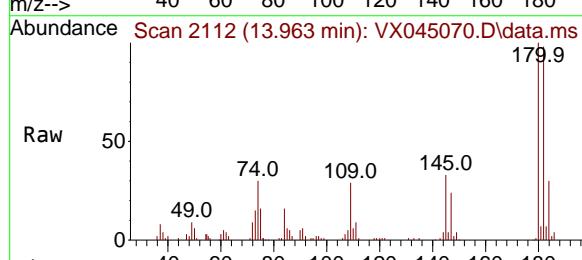

Tgt Ion:180 Resp: 28937
Ion Ratio Lower Upper
180 100
182 97.0 47.5 142.6
145 33.7 17.0 50.9

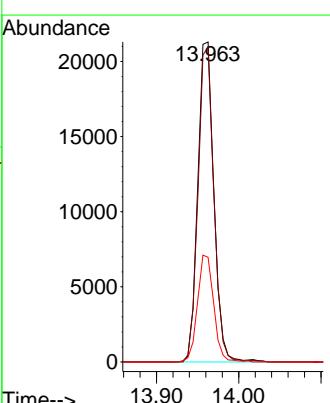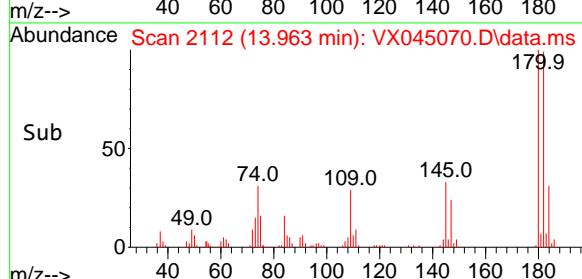

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045071.D
 Acq On : 28 Feb 2025 03:00
 Operator : JC/MD
 Sample : VSTDICCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICCC050

Quant Time: Feb 28 05:34:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 05:28:02 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.550	168	103235	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	186358	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	162079	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	71264	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	78159	51.250	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125			Recovery	=	102.500%
35) Dibromofluoromethane	5.385	113	61323	50.346	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124			Recovery	=	100.700%
50) Toluene-d8	8.647	98	225493	49.449	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113			Recovery	=	98.900%
62) 4-Bromofluorobenzene	11.079	95	74945	49.212	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121			Recovery	=	98.420%
Target Compounds						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	64743	45.502	ug/l	100
3) Chloromethane	1.307	50	77729	44.894	ug/l	100
4) Vinyl Chloride	1.374	62	78524	46.434	ug/l	100
5) Bromomethane	1.593	94	30169	57.066	ug/l	100
6) Chloroethane	1.660	64	38461	59.750	ug/l	100
7) Trichlorofluoromethane	1.868	101	108411	50.047	ug/l	100
8) Diethyl Ether	2.136	74	40001	50.814	ug/l	100
9) 1,1,2-Trichlorotrifluo...	2.313	101	61312	47.399	ug/l	100
10) Methyl Iodide	2.441	142	79357	47.854	ug/l	100
11) Tert butyl alcohol	2.983	59	69139	247.496	ug/l	100
12) 1,1-Dichloroethene	2.307	96	64327	48.434	ug/l	100
13) Acrolein	2.233	56	89603	296.189	ug/l	100
14) Allyl chloride	2.654	41	114313	47.875	ug/l	100
15) Acrylonitrile	3.062	53	211455	278.519	ug/l	100
16) Acetone	2.386	43	181429	289.130	ug/l	100
17) Carbon Disulfide	2.502	76	171353	47.419	ug/l	100
18) Methyl Acetate	2.703	43	89508	47.359	ug/l	100
19) Methyl tert-butyl Ether	3.117	73	215043	50.642	ug/l	100
20) Methylene Chloride	2.782	84	72081	48.500	ug/l	100
21) trans-1,2-Dichloroethene	3.087	96	65093	49.832	ug/l	100
22) Diisopropyl ether	3.764	45	236563	51.816	ug/l	100
23) Vinyl Acetate	3.721	43	1018631	271.773	ug/l	100
24) 1,1-Dichloroethane	3.605	63	128235	50.270	ug/l	100
25) 2-Butanone	4.562	43	298785	295.330	ug/l	100
26) 2,2-Dichloropropane	4.471	77	61631	32.498	ug/l	100
27) cis-1,2-Dichloroethene	4.483	96	78657	49.955	ug/l	100
28) Bromochloromethane	4.898	49	62299	50.643	ug/l	100
29) Tetrahydrofuran	5.007	42	192607	287.345	ug/l	100
30) Chloroform	5.087	83	128581	51.532	ug/l	100
31) Cyclohexane	5.464	56	114333	48.836	ug/l	100
32) 1,1,1-Trichloroethane	5.379	97	105671	50.306	ug/l	100
36) 1,1-Dichloropropene	5.690	75	87338	49.861	ug/l	100
37) Ethyl Acetate	4.715	43	112892	56.641	ug/l	100
38) Carbon Tetrachloride	5.672	117	87123	50.593	ug/l	100
39) Methylcyclohexane	7.373	83	108974	48.715	ug/l	100
40) Benzene	6.031	78	278802	50.925	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045071.D
 Acq On : 28 Feb 2025 03:00
 Operator : JC/MD
 Sample : VSTDICCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICCC050

Quant Time: Feb 28 05:34:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 05:28:02 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	63454	59.598	ug/1	100
42) 1,2-Dichloroethane	6.080	62	98340	55.428	ug/1	100
43) Isopropyl Acetate	6.342	43	173045	54.544	ug/1	100
44) Trichloroethene	7.123	130	63513	50.756	ug/1	100
45) 1,2-Dichloropropane	7.428	63	69128	50.808	ug/1	100
46) Dibromomethane	7.580	93	50143	52.757	ug/1	100
47) Bromodichloromethane	7.818	83	97729	53.153	ug/1	100
48) Methyl methacrylate	7.690	41	86231	57.256	ug/1	100
49) 1,4-Dioxane	7.659	88	35053	1095.003	ug/1	100
51) 4-Methyl-2-Pentanone	8.574	43	568737	292.570	ug/1	100
52) Toluene	8.714	92	167431	51.505	ug/1	100
53) t-1,3-Dichloropropene	8.976	75	87373	48.078	ug/1	100
54) cis-1,3-Dichloropropene	8.366	75	99713	49.079	ug/1	100
55) 1,1,2-Trichloroethane	9.147	97	66379	52.724	ug/1	100
56) Ethyl methacrylate	9.116	69	106157	52.724	ug/1	100
57) 1,3-Dichloropropane	9.305	76	115488	52.594	ug/1	100
58) 2-Chloroethyl Vinyl ether	8.238	63	264555	267.612	ug/1	100
59) 2-Hexanone	9.427	43	416984	297.362	ug/1	100
60) Dibromochloromethane	9.519	129	71569	53.284	ug/1	100
61) 1,2-Dibromoethane	9.604	107	66312	52.217	ug/1	100
64) Tetrachloroethene	9.269	164	52531	51.021	ug/1	100
65) Chlorobenzene	10.079	112	176922	50.853	ug/1	100
66) 1,1,1,2-Tetrachloroethane	10.159	131	57642	51.402	ug/1	100
67) Ethyl Benzene	10.189	91	316427	51.431	ug/1	100
68) m/p-Xylenes	10.299	106	234554	103.515	ug/1	100
69) o-Xylene	10.640	106	114440	50.341	ug/1	100
70) Styrene	10.653	104	191406	52.387	ug/1	100
71) Bromoform	10.799	173	44730	53.645	ug/1 #	100
73) Isopropylbenzene	10.963	105	294694	51.167	ug/1	100
74) N-amyl acetate	10.842	43	140869	53.881	ug/1	100
75) 1,1,2,2-Tetrachloroethane	11.213	83	101089	50.945	ug/1	100
76) 1,2,3-Trichloropropane	11.238	75	81743m	51.421	ug/1	
77) Bromobenzene	11.195	156	66904	51.173	ug/1	100
78) n-propylbenzene	11.305	91	342399	51.546	ug/1	100
79) 2-Chlorotoluene	11.360	91	204484	50.154	ug/1	100
80) 1,3,5-Trimethylbenzene	11.451	105	241129	51.613	ug/1	100
81) trans-1,4-Dichloro-2-b...	11.018	75	24135	41.172	ug/1	100
82) 4-Chlorotoluene	11.451	91	230493	51.072	ug/1	100
83) tert-Butylbenzene	11.713	119	240510	50.895	ug/1	100
84) 1,2,4-Trimethylbenzene	11.750	105	240719	52.326	ug/1	100
85) sec-Butylbenzene	11.890	105	300393	51.353	ug/1	100
86) p-Isopropyltoluene	12.006	119	244031	51.964	ug/1	100
87) 1,3-Dichlorobenzene	11.969	146	118879	49.747	ug/1	100
88) 1,4-Dichlorobenzene	12.036	146	120217	49.694	ug/1	100
89) n-Butylbenzene	12.329	91	214685	52.006	ug/1	100
90) Hexachloroethane	12.536	117	43086	49.188	ug/1	100
91) 1,2-Dichlorobenzene	12.335	146	118896	50.557	ug/1	100
92) 1,2-Dibromo-3-Chloropr...	12.939	75	20610	56.123	ug/1	100
93) 1,2,4-Trichlorobenzene	13.585	180	71897	50.571	ug/1	100
94) Hexachlorobutadiene	13.725	225	27916	49.245	ug/1	100
95) Naphthalene	13.774	128	278086	53.700	ug/1	100
96) 1,2,3-Trichlorobenzene	13.957	180	75482	52.406	ug/1	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045071.D
Acq On : 28 Feb 2025 03:00
Operator : JC/MD
Sample : VSTDICCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICCC050

Quant Time: Feb 28 05:34:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 05:28:02 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carbone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045071.D
Acq On : 28 Feb 2025 03:00
Operator : JC/MD
Sample : VSTDICCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICCC050

Manual Integrations APPROVED

Reviewed By :John Carbone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

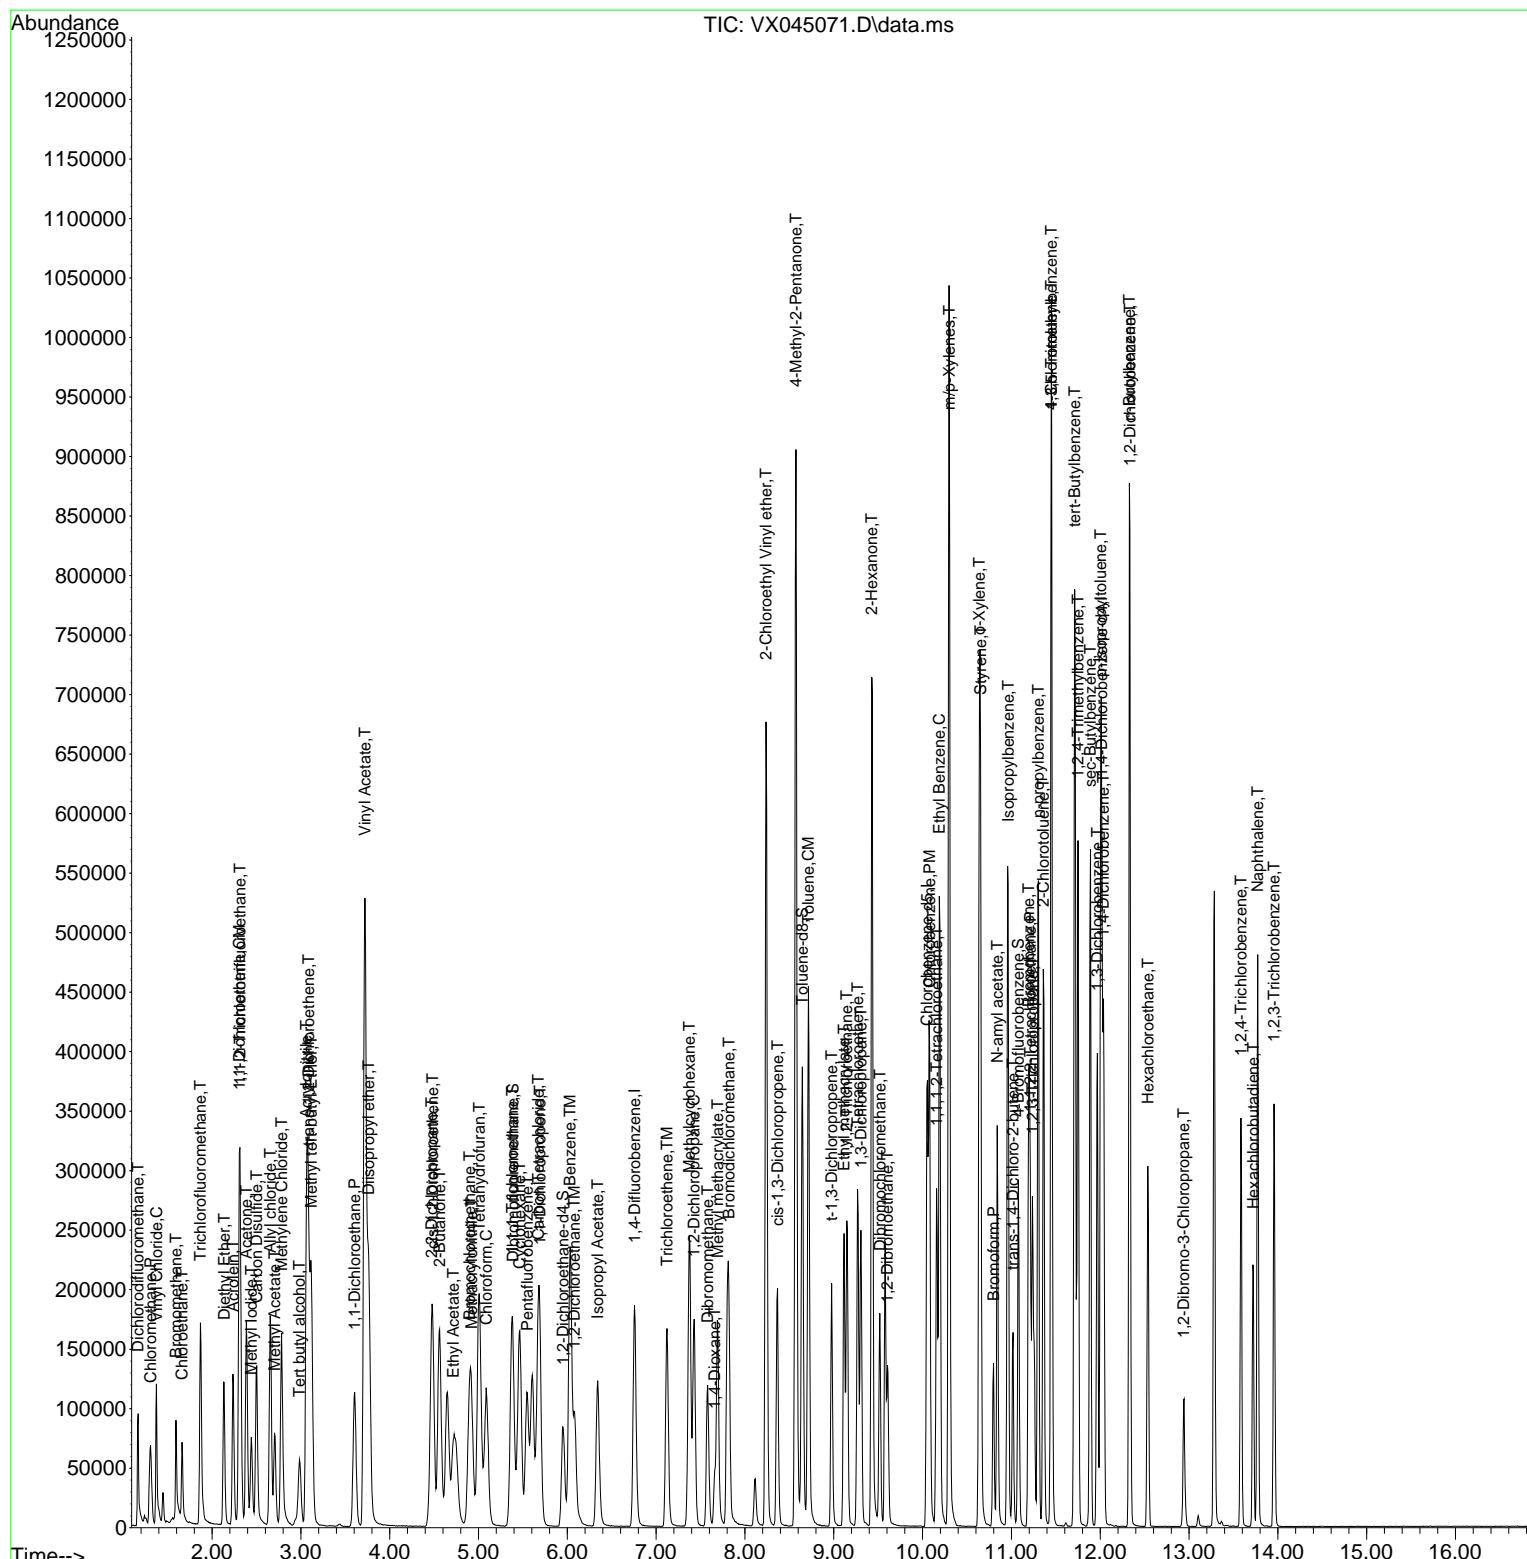

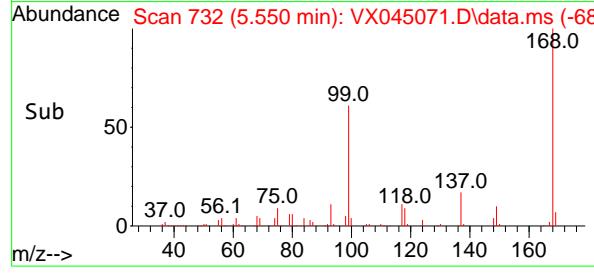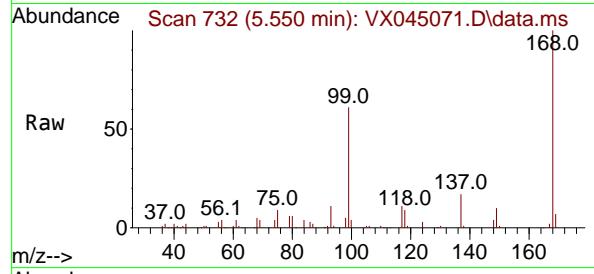
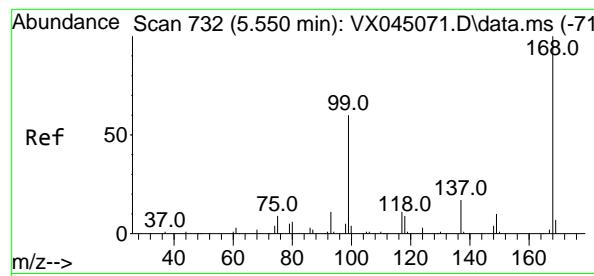


#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.550 min Scan# 7
 Delta R.T. -0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICCC050



**Manual Integrations
APPROVED**

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

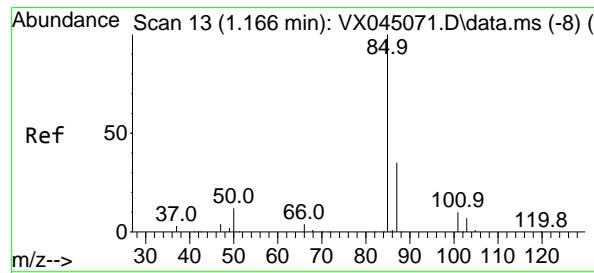



#2
 Dichlorodifluoromethane
 Concen: 45.502 ug/l
 RT: 1.166 min Scan# 13
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00

Tgt Ion: 85 Resp: 64743
 Ion Ratio Lower Upper
 85 100
 87 34.9 17.4 52.3

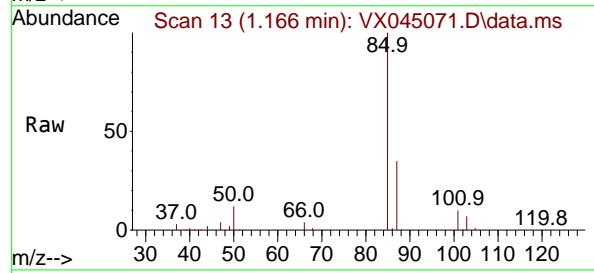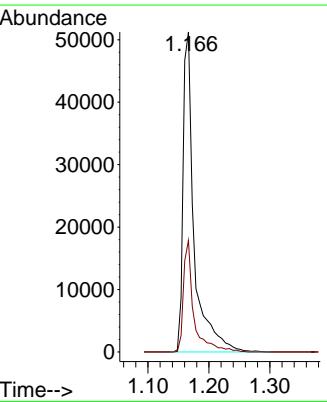

Scan 13 (1.166 min): VX045071.D\data.ms (-1)

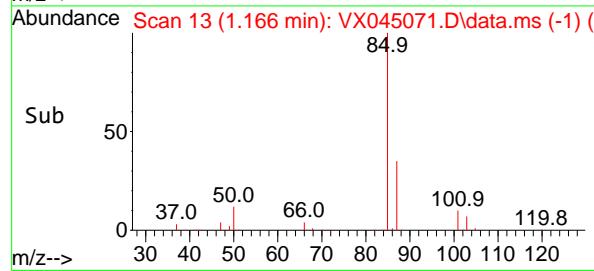







#3
Chloromethane
Concen: 44.894 ug/l
RT: 1.307 min Scan# 3
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Instrument : MSVOA_X
ClientSampleId : VSTDICCC050

Tgt Ion: 50 Resp: 77729
Ion Ratio Lower Upper
50 100
52 31.2 25.0 37.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

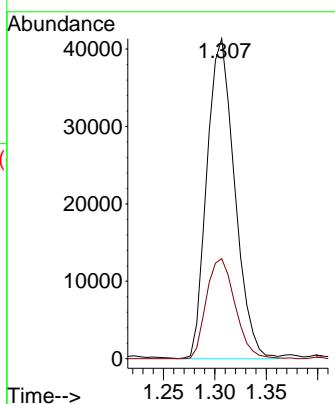

#4
Vinyl Chloride
Concen: 46.434 ug/l
RT: 1.374 min Scan# 47
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00


Tgt Ion: 62 Resp: 78524
Ion Ratio Lower Upper
62 100
64 30.4 24.3 36.5

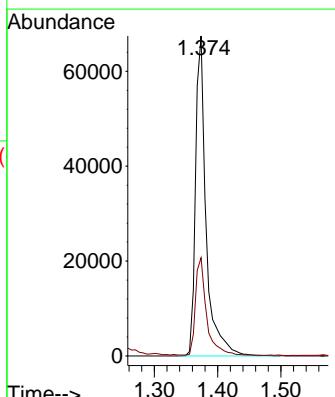



#5
 Bromomethane
 Concen: 57.066 ug/l
 RT: 1.593 min Scan# 8
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00



Instrument : MSVOA_X
 ClientSampleId : VSTDICCC050




Tgt Ion: 94 Resp: 30169
 Ion Ratio Lower Upper
 94 100
 96 93.7 75.0 112.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025




#6
 Chloroethane
 Concen: 59.750 ug/l
 RT: 1.660 min Scan# 94
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00




Tgt Ion: 64 Resp: 38461
 Ion Ratio Lower Upper
 64 100
 66 33.4 26.7 40.1





#7
Trichlorofluoromethane
Concen: 50.047 ug/l
RT: 1.868 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050




Tgt Ion: 101 Resp: 10841
Ion Ratio Lower Upper
101 100
103 65.1 52.1 78.1

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#8
Diethyl Ether
Concen: 50.814 ug/l
RT: 2.136 min Scan# 172
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Tgt Ion: 74 Resp: 40001
Ion Ratio Lower Upper
74 100
45 103.0 51.5 154.5





#9
1,1,2-Trichlorotrifluoroethane
Concen: 47.399 ug/l
RT: 2.313 min Scan# 2
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050




Tgt Ion:101 Resp: 6131:
Ion Ratio Lower Upper
101 100
85 45.3 36.2 54.4
151 70.5 56.4 84.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#10
Methyl Iodide
Concen: 47.854 ug/l
RT: 2.441 min Scan# 222
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00



Tgt Ion:142 Resp: 79357
Ion Ratio Lower Upper
142 100
127 44.3 35.4 53.2
141 14.5 11.6 17.4









#11
 Tert butyl alcohol
 Concen: 247.496 ug/l
 RT: 2.983 min Scan# 311
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00

Instrument : MSVOA_X
 ClientSampleId : VSTDICCC050

Tgt Ion: 59 Resp: 69139
 Ion Ratio Lower Upper
 59 100
 57 9.8 7.8 11.8




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

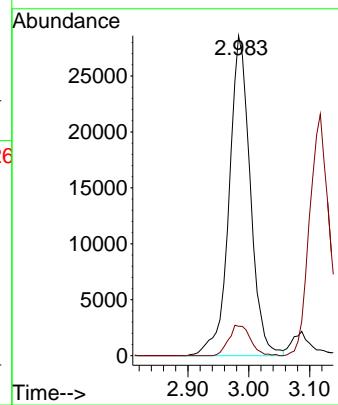

#12
 1,1-Dichloroethene
 Concen: 48.434 ug/l
 RT: 2.307 min Scan# 200
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00


Tgt Ion: 96 Resp: 64327
 Ion Ratio Lower Upper
 96 100
 61 168.3 134.6 202.0
 98 63.8 51.0 76.6

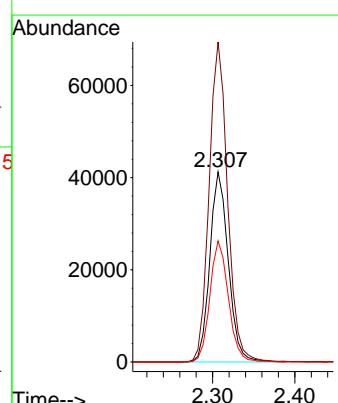



#13
Acrolein
Concen: 296.189 ug/l
RT: 2.233 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050

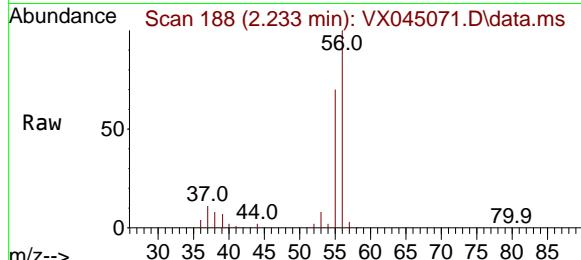

Tgt Ion: 56 Resp: 8960
Ion Ratio Lower Upper
56 100
55 70.3 56.2 84.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

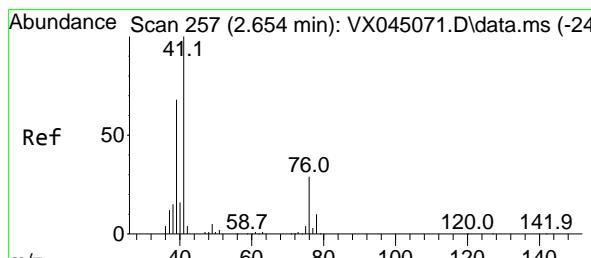

#14
Allyl chloride
Concen: 47.875 ug/l
RT: 2.654 min Scan# 257
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00


Tgt Ion: 41 Resp: 114313
Ion Ratio Lower Upper
41 100
39 67.3 53.8 80.8
76 31.5 25.2 37.8

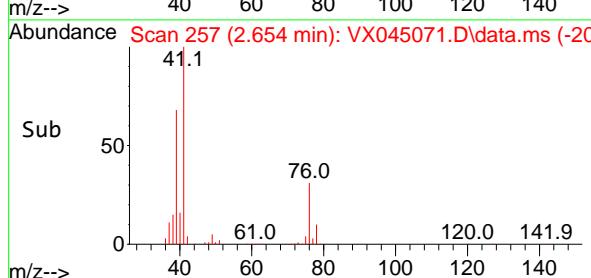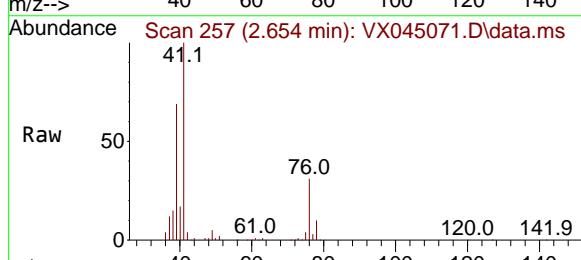



#15
Acrylonitrile
Concen: 278.519 ug/l
RT: 3.062 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00



Instrument : MSVOA_X
ClientSampleId : VSTDICCC050



Tgt Ion:	Ion Ratio	Lower	Upper
53	100		
52	82.7	66.2	99.2
51	36.2	29.0	43.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#16
Acetone
Concen: 289.130 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00


Tgt Ion:	Ion Ratio	Lower	Upper
43	100		
58	30.3	24.2	36.4

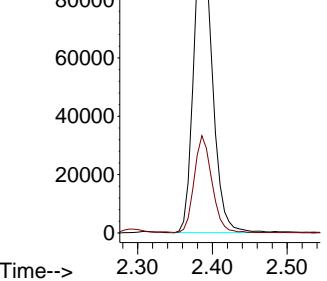



#17
Carbon Disulfide
Concen: 47.419 ug/l
RT: 2.502 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00



Instrument : MSVOA_X
ClientSampleId : VSTDICCC050

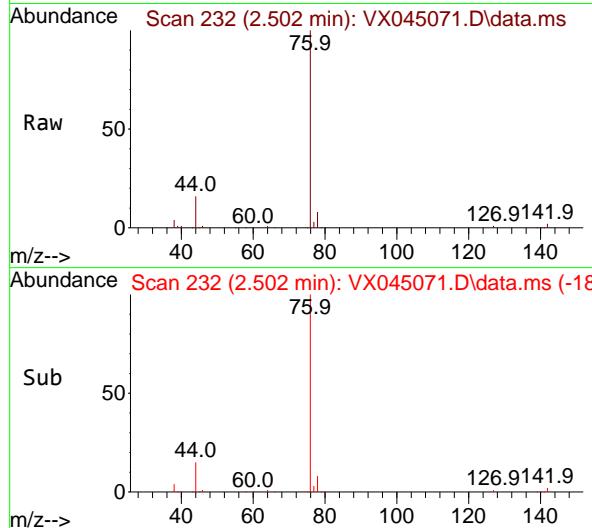

Tgt Ion: 76 Resp: 17135
Ion Ratio Lower Upper
76 100
78 8.2 6.6 9.8


Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

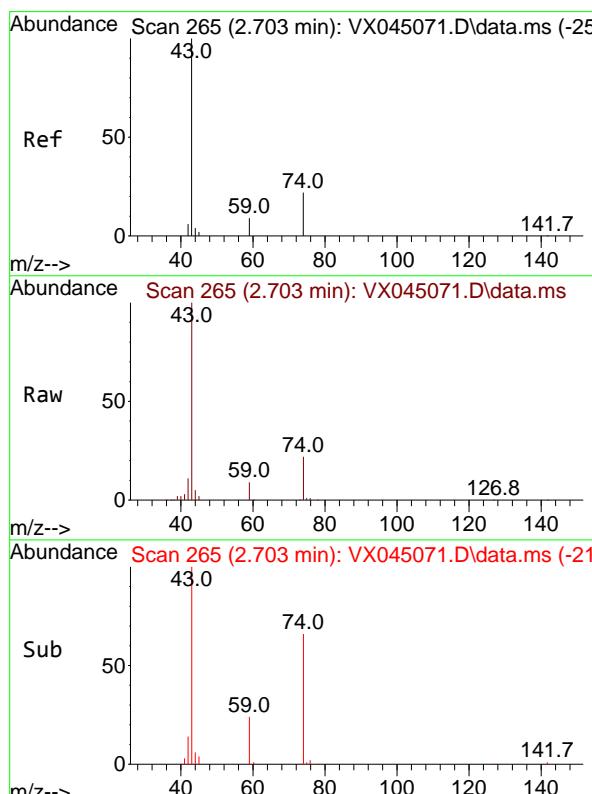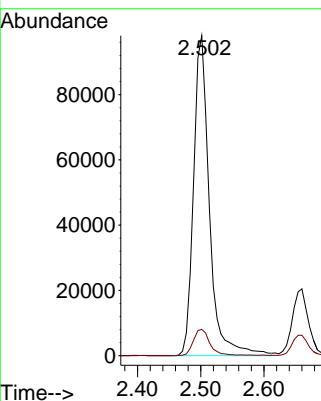

#18
Methyl Acetate
Concen: 47.359 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00


Tgt Ion: 43 Resp: 89508
Ion Ratio Lower Upper
43 100
74 21.8 17.4 26.2

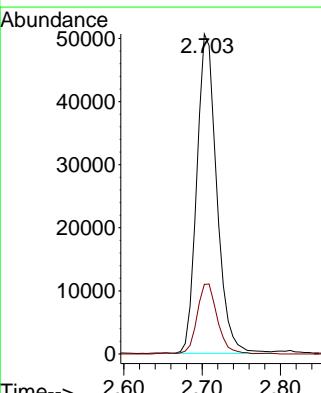



#19
Methyl tert-butyl Ether
Concen: 50.642 ug/l
RT: 3.117 min Scan# 3
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050



Tgt Ion: 73 Resp: 21504
Ion Ratio Lower Upper
73 100
57 23.1 18.5 27.7




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

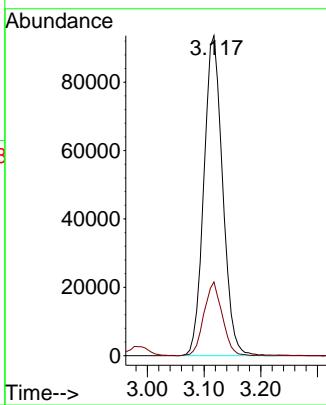

#20
Methylene Chloride
Concen: 48.500 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00


Tgt Ion: 84 Resp: 72081
Ion Ratio Lower Upper
84 100
49 133.1 106.5 159.7
51 40.1 32.1 48.1
86 62.5 50.0 75.0

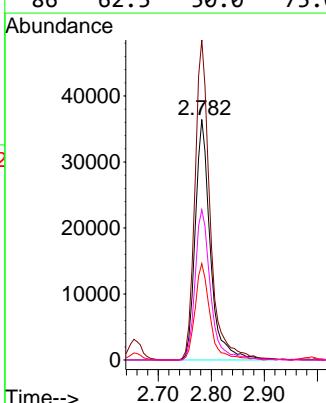



#21
trans-1,2-Dichloroethene
Concen: 49.832 ug/l
RT: 3.087 min Scan# 328
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050




Tgt Ion: 96 Resp: 6509
Ion Ratio Lower Upper
96 100
61 146.2 117.0 175.4
98 66.8 53.4 80.2

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

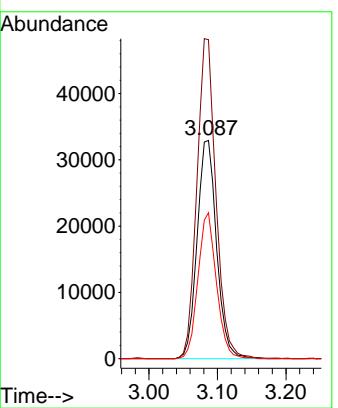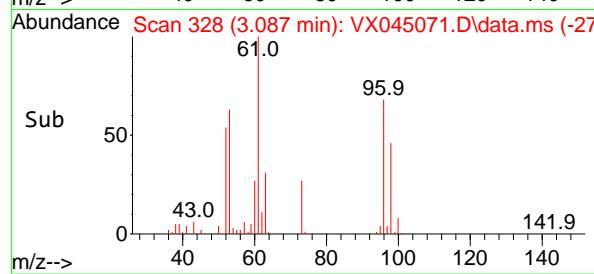


#22
Diisopropyl ether
Concen: 51.816 ug/l
RT: 3.764 min Scan# 439
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Tgt Ion: 45 Resp: 236563
Ion Ratio Lower Upper
45 100
43 68.6 54.9 82.3
87 26.2 21.0 31.4
59 10.9 8.7 13.1

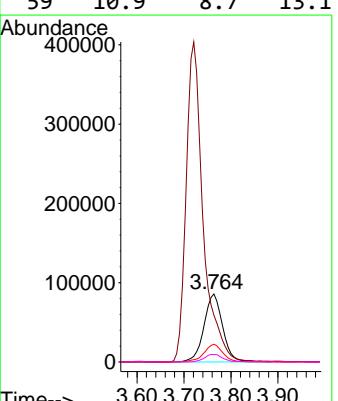



#23
Vinyl Acetate
 Concen: 271.773 ug/l
 RT: 3.721 min Scan# 413
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00



Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICCC050



Tgt Ion: 43 Resp: 101863
 Ion Ratio Lower Upper
 43 100
 86 10.1 8.1 12.1



Manual Integrations
APPROVED

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

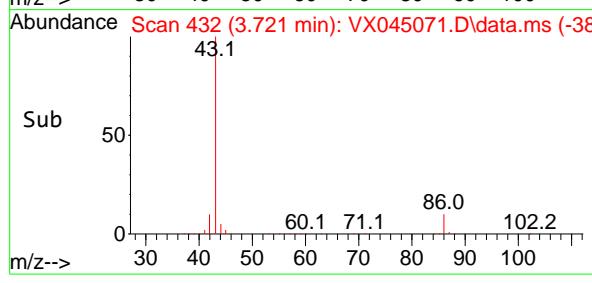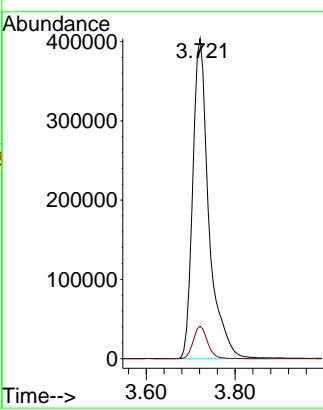

#24
1,1-Dichloroethane
 Concen: 50.270 ug/l
 RT: 3.605 min Scan# 413
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00

Tgt Ion: 63 Resp: 128235
 Ion Ratio Lower Upper
 63 100
 98 6.8 3.4 10.2
 100 4.3 2.1 6.5

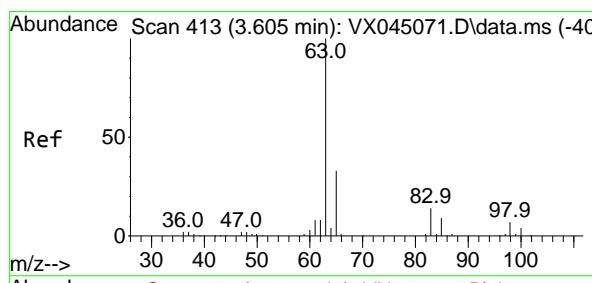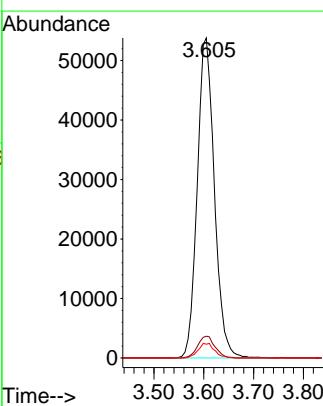



Abundance Scan 413 (3.605 min): VX045071.D\data.ms

Raw 50

m/z--> 0 30 40 50 60 70 80 90 100


63.0 36.0 47.0 82.9 97.9

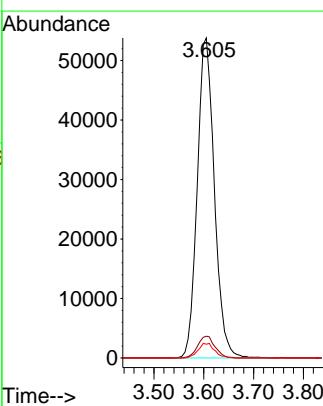

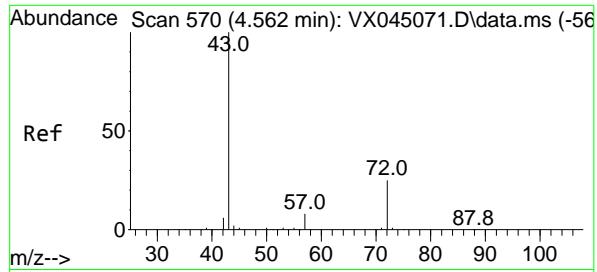

#25
2-Butanone
Concen: 295.330 ug/l
RT: 4.562 min Scan# 51
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050



Tgt Ion: 43 Resp: 29878
Ion Ratio Lower Upper
43 100
72 25.0 20.0 30.0



Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

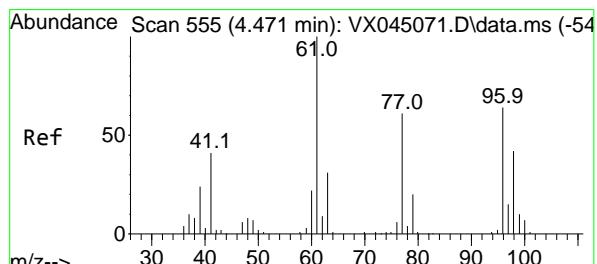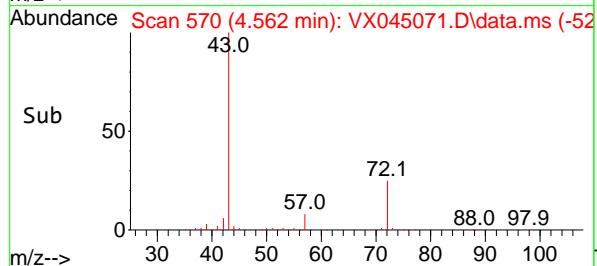

#26
2,2-Dichloropropane
Concen: 32.498 ug/l
RT: 4.471 min Scan# 555
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00


Tgt Ion: 77 Resp: 61631
Ion Ratio Lower Upper
77 100
97 24.7 12.4 37.0

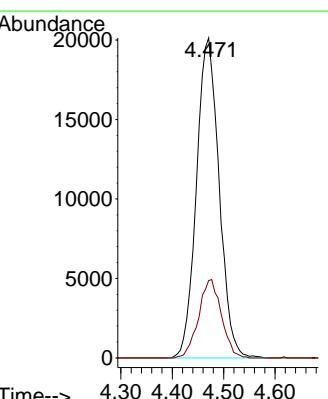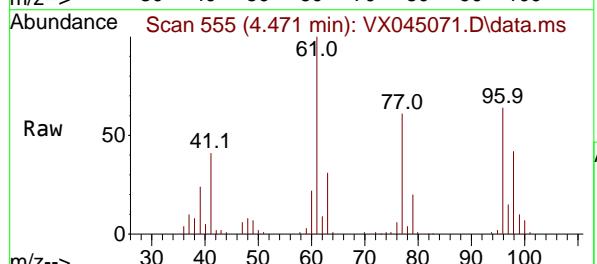

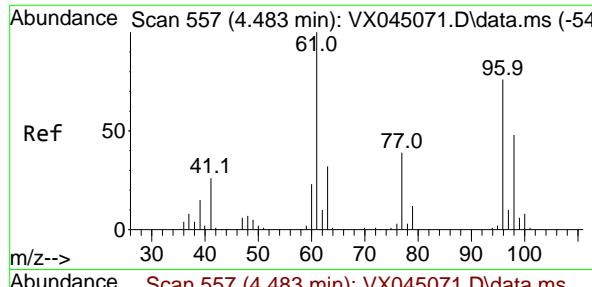

#27
cis-1,2-Dichloroethene
Concen: 49.955 ug/l
RT: 4.483 min Scan# 5
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050

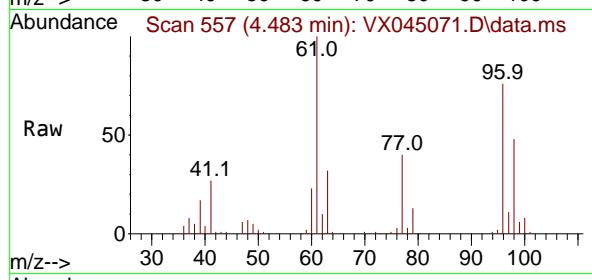

Tgt Ion: 96 Resp: 78655
Ion Ratio Lower Upper
96 100
61 141.6 0.0 283.2
98 64.0 0.0 128.0




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#28
Bromochloromethane
Concen: 50.643 ug/l
RT: 4.898 min Scan# 625
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Tgt Ion: 49 Resp: 62299
Ion Ratio Lower Upper
49 100
129 1.7 0.0 3.4
130 70.1 56.1 84.1

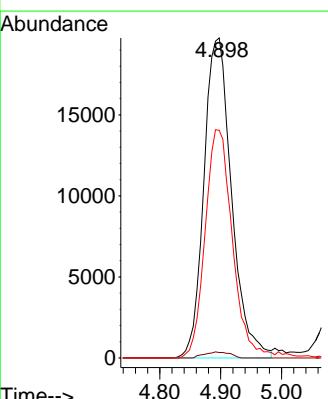



#29

Tetrahydrofuran

Concen: 287.345 ug/l

RT: 5.007 min Scan# 6


Delta R.T. 0.000 min

Lab File: VX045071.D

Acq: 28 Feb 2025 03:00

Instrument : MSVOA_X



ClientSampleId : VSTDICCC050

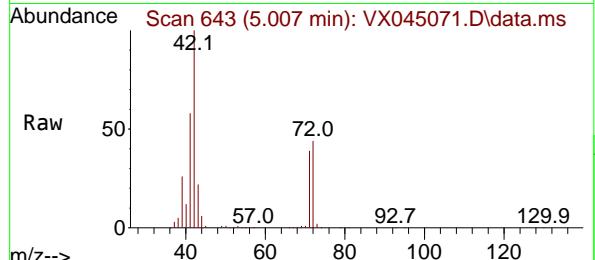

Tgt	Ion:	42	Ion Ratio	100	Resp:	19260
		42		42.6	Lower	
		72		34.1	Upper	
		71		39.2	31.4	47.0


Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

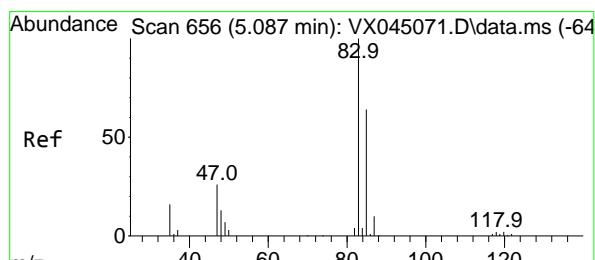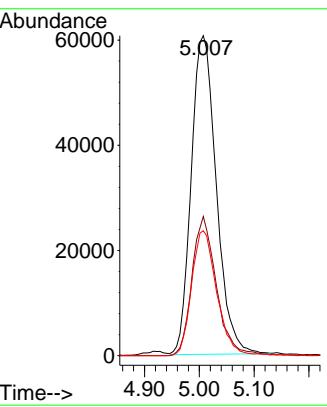


#30
Chloroform
Concen: 51.532 ug/l
RT: 5.087 min Scan# 656
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00


Tgt	Ion:	83	Ion Ratio	100	Resp:	128581
		83		64.3	Lower	
		85		51.4	Upper	




Abundance Scan 656 (5.087 min): VX045071.D\data.ms (-60)

Sub

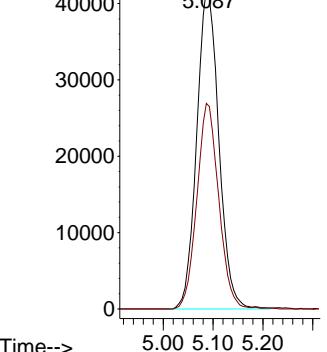






#31
Cyclohexane
Concen: 48.836 ug/l
RT: 5.464 min Scan# 718
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00
Instrument: MSVOA_X
ClientSampleId: VSTDICCC050




Tgt Ion: 56 Resp: 114331
Ion Ratio Lower Upper
56 100
69 29.3 23.4 35.2
84 86.8 69.4 104.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#32
1,1,1-Trichloroethane
Concen: 50.306 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Tgt Ion: 97 Resp: 105671
Ion Ratio Lower Upper
97 100
99 64.5 51.6 77.4
61 48.0 38.4 57.6





#33
1,2-Dichloroethane-d4
Concen: 51.250 ug/l
RT: 5.952 min Scan# 78159
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument :
MSVOA_X
ClientSampleId :
VSTDICCC050




Tgt Ion: 65 Resp: 78159
Ion Ratio Lower Upper
65 100
67 53.1 0.0 106.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

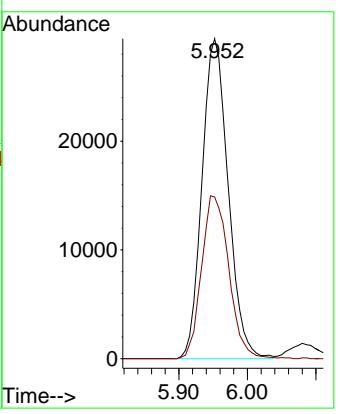


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Tgt Ion:114 Resp: 186358
Ion Ratio Lower Upper
114 100
63 20.9 0.0 41.8
88 16.4 0.0 32.8

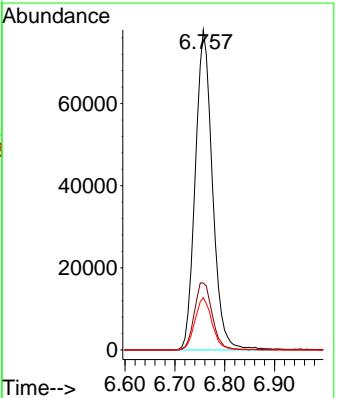



#35
Dibromofluoromethane
Concen: 50.346 ug/l
RT: 5.385 min Scan# 7
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument :
MSVOA_X
ClientSampleId :
VSTDICCC050




Tgt Ion:113 Resp: 61322
Ion Ratio Lower Upper
113 100
111 102.2 81.8 122.6
192 17.9 14.3 21.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#36
1,1-Dichloropropene
Concen: 49.861 ug/l
RT: 5.690 min Scan# 755
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Tgt Ion: 75 Resp: 87338
Ion Ratio Lower Upper
75 100
110 33.7 16.9 50.6
77 30.6 24.5 36.7



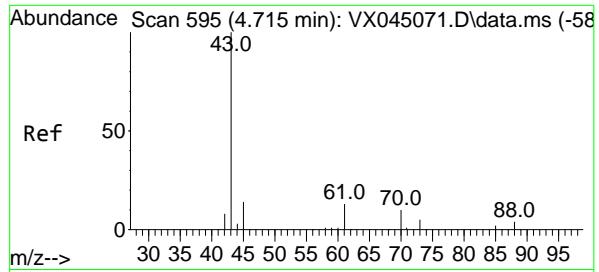

#37
Ethyl Acetate
 Concen: 56.641 ug/l
 RT: 4.715 min Scan# 5
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
 ClientSampleId : VSTDICCC050



Tgt Ion: 43 Resp: 11289
 Ion Ratio Lower Upper
 43 100
 61 13.5 10.8 16.2
 70 9.6 7.7 11.5




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

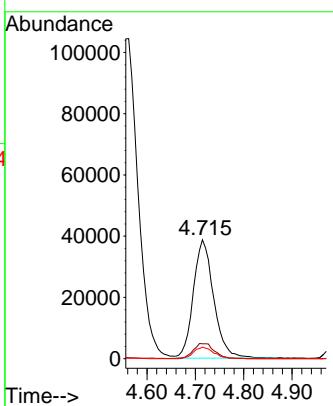

#38
Carbon Tetrachloride
 Concen: 50.593 ug/l
 RT: 5.672 min Scan# 752
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00


Tgt Ion:117 Resp: 87123
 Ion Ratio Lower Upper
 117 100
 119 95.9 76.7 115.1
 121 31.9 25.5 38.3

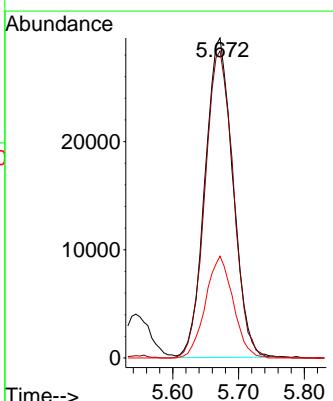



#39
Methylcyclohexane
Concen: 48.715 ug/l
RT: 7.373 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00



Instrument : MSVOA_X
ClientSampleId : VSTDICCC050




Tgt Ion: 83 Resp: 108974
Ion Ratio Lower Upper
83 100
55 78.7 63.0 94.4
98 49.6 39.7 59.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

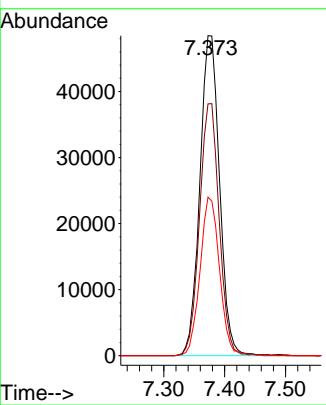


#40
Benzene
Concen: 50.925 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Tgt Ion: 78 Resp: 278802
Ion Ratio Lower Upper
78 100
77 23.5 18.8 28.2

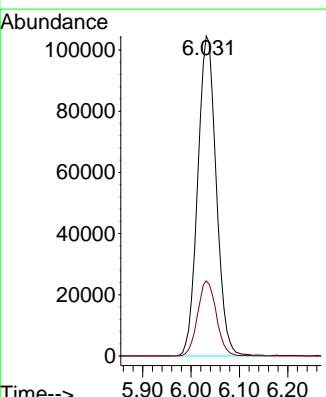



#41
Methacrylonitrile
Concen: 59.598 ug/l
RT: 4.922 min Scan# 61
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050

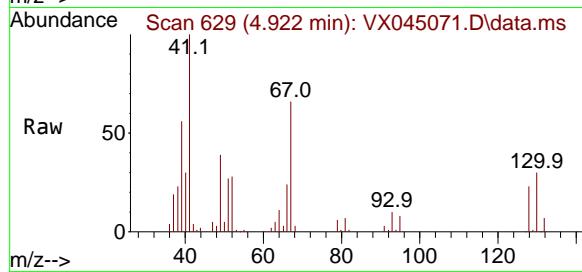


Tgt Ion: 41 Resp: 63454
Ion Ratio Lower Upper
41 100
39 55.8 44.6 67.0
67 67.4 53.9 80.9
52 29.1 23.3 34.9

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#42
1,2-Dichloroethane
Concen: 55.428 ug/l
RT: 6.080 min Scan# 819
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Tgt Ion: 62 Resp: 98340
Ion Ratio Lower Upper
62 100
98 9.1 0.0 18.2

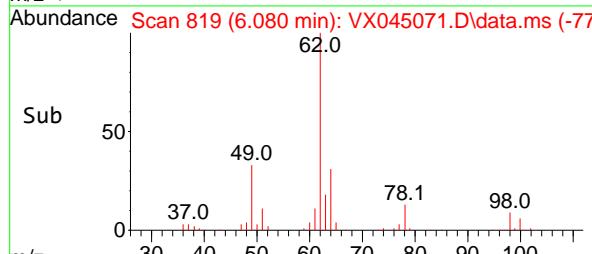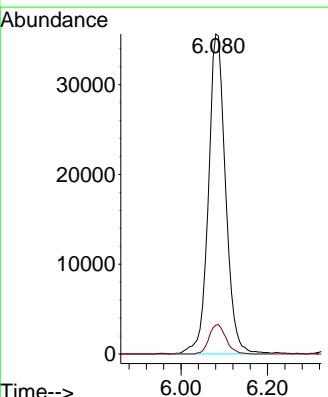



#43
Isopropyl Acetate
Concen: 54.544 ug/l
RT: 6.342 min Scan# 8
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050




Tgt Ion: 43 Resp: 17304
Ion Ratio Lower Upper
43 100
61 18.6 14.9 22.3
87 11.8 9.4 14.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#44
Trichloroethene
Concen: 50.756 ug/l
RT: 7.123 min Scan# 990
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Tgt Ion:130 Resp: 63513
Ion Ratio Lower Upper
130 100
95 102.5 0.0 205.0





#45
1,2-Dichloropropane
Concen: 50.808 ug/l
RT: 7.428 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050




Tgt Ion: 63 Resp: 69123
Ion Ratio Lower Upper
63 100
65 30.9 24.7 37.1

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

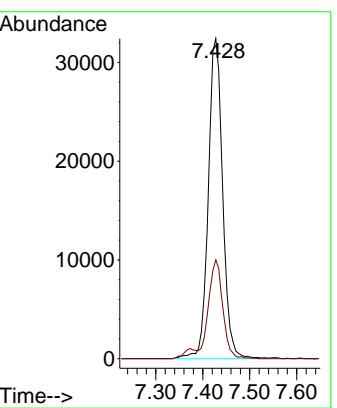


#46
Dibromomethane
Concen: 52.757 ug/l
RT: 7.580 min Scan# 1065
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

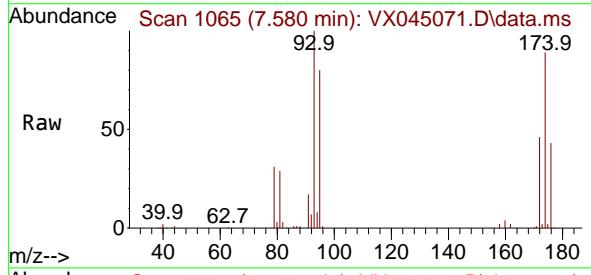

Tgt Ion: 93 Resp: 50143
Ion Ratio Lower Upper
93 100
95 82.3 65.8 98.8
174 90.2 72.2 108.2

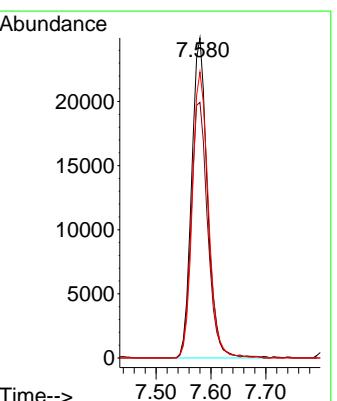

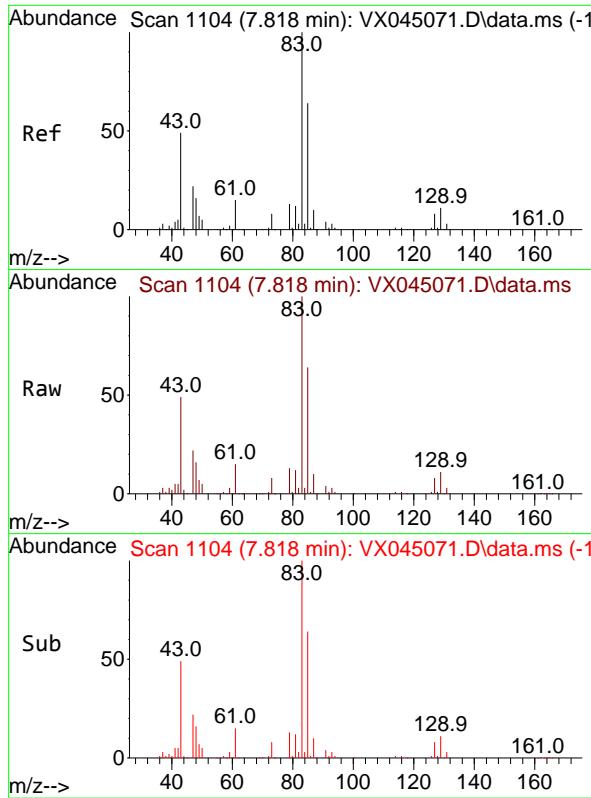

#47

Bromodichloromethane

Concen: 53.153 ug/l

RT: 7.818 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045071.D

Acq: 28 Feb 2025 03:00

Instrument:

MSVOA_X

ClientSampleId :

VSTDICCC050

Tgt Ion: 83 Resp: 97729

Ion Ratio Lower Upper

83 100



85 63.9 51.1 76.7

127 8.0 6.4 9.6

Manual Integrations**APPROVED**

Reviewed By :John Carlone 02/28/2025

Supervised By :Mahesh Dadoda 02/28/2025

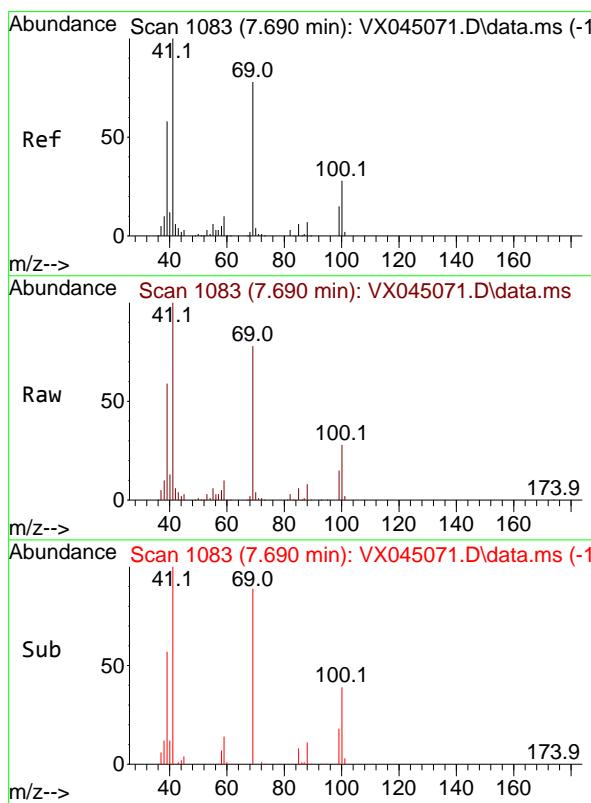

#48

Methyl methacrylate

Concen: 57.256 ug/l

RT: 7.690 min Scan# 1083

Delta R.T. 0.000 min

Lab File: VX045071.D

Acq: 28 Feb 2025 03:00


Tgt Ion: 41 Resp: 86231


Ion Ratio Lower Upper

41 100

69 78.8 63.0 94.6


39 59.4 47.5 71.3





#49
1,4-Dioxane
Concen: 1095.003 ug/l
RT: 7.659 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050




Tgt Ion: 88 Resp: 35051
Ion Ratio Lower Upper
88 100
43 35.9 28.7 43.1
58 69.8 55.8 83.8

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#50
Toluene-d8
Concen: 49.449 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Tgt Ion: 98 Resp: 225493
Ion Ratio Lower Upper
98 100
100 65.0 52.0 78.0

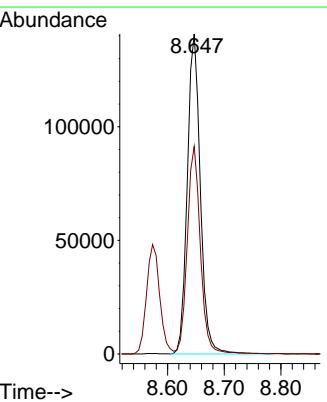



#51
4-Methyl-2-Pentanone
Concen: 292.570 ug/l
RT: 8.574 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050



Tgt Ion: 43 Resp: 56873
Ion Ratio Lower Upper
43 100
58 36.5 29.2 43.8




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

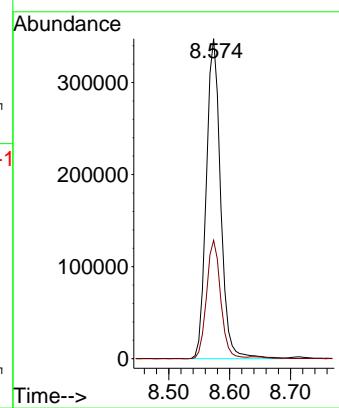

#52
Toluene
Concen: 51.505 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00


Tgt Ion: 92 Resp: 167431
Ion Ratio Lower Upper
92 100
91 173.6 138.9 208.3

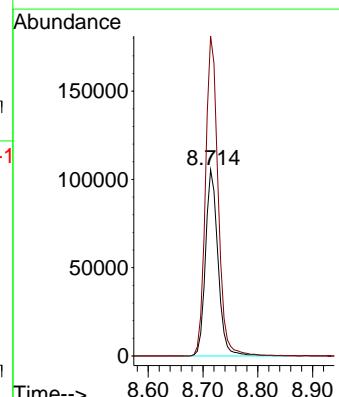

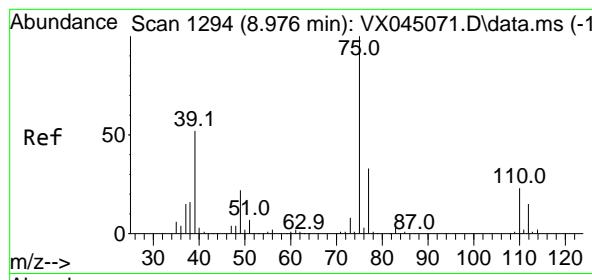

#53
t-1,3-Dichloropropene
Concen: 48.078 ug/l
RT: 8.976 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050



Tgt Ion: 75 Resp: 8737
Ion Ratio Lower Upper
75 100
77 33.1 26.5 39.7




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

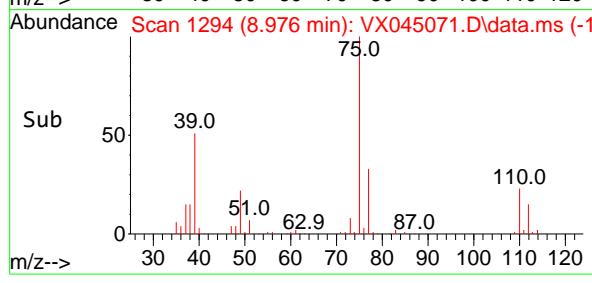

#54
cis-1,3-Dichloropropene
Concen: 49.079 ug/l
RT: 8.366 min Scan# 1194
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00


Tgt Ion: 75 Resp: 99713
Ion Ratio Lower Upper
75 100
77 30.9 24.7 37.1
39 50.9 40.7 61.1

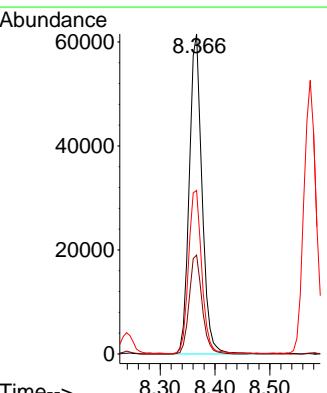



#55
1,1,2-Trichloroethane
Concen: 52.724 ug/l
RT: 9.147 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050




Tgt Ion: 97 Resp: 66379
Ion Ratio Lower Upper
97 100
83 86.8 69.4 104.2
85 55.1 44.1 66.1
99 63.4 50.7 76.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

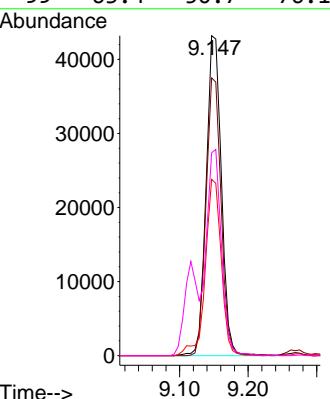


#56
Ethyl methacrylate
Concen: 52.724 ug/l
RT: 9.116 min Scan# 1317
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00



Tgt Ion: 69 Resp: 106157
Ion Ratio Lower Upper
69 100
41 71.2 57.0 85.4
39 42.8 34.2 51.4

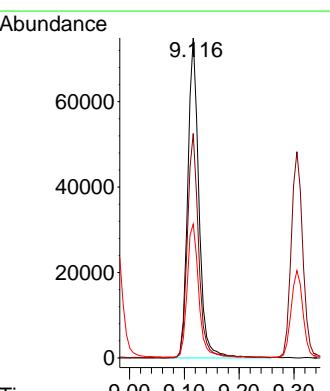


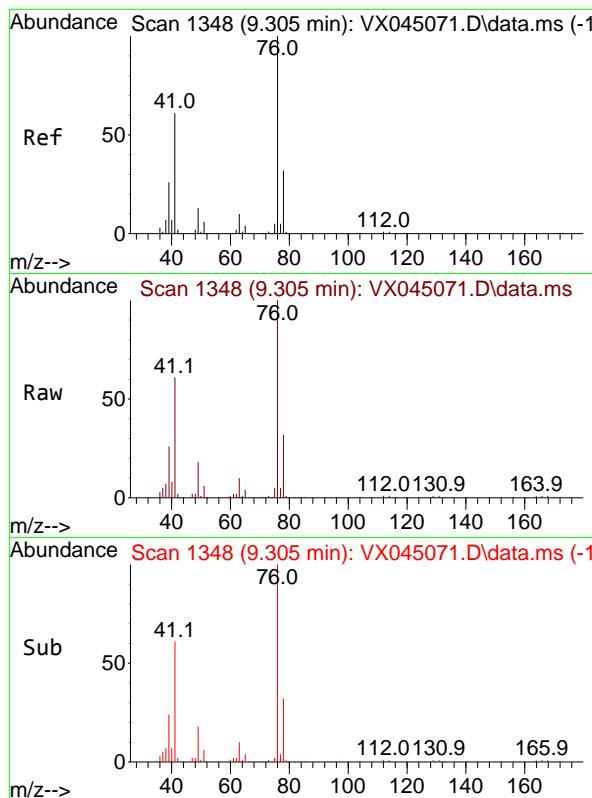


#57
1,3-Dichloropropane
Concen: 52.594 ug/l
RT: 9.305 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Instrument : MSVOA_X
ClientSampleId : VSTDICCC050


**Manual Integrations
APPROVED**


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

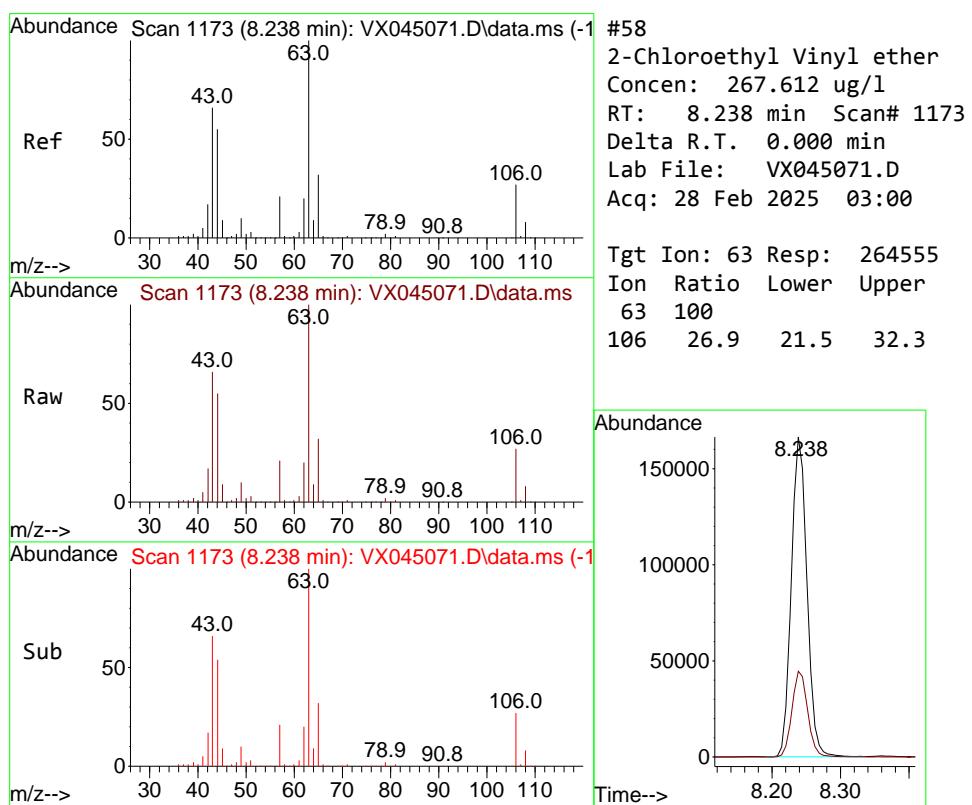

#58
2-Chloroethyl Vinyl ether
Concen: 267.612 ug/l
RT: 8.238 min Scan# 1173
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00


Tgt Ion: 63 Resp: 264555
Ion Ratio Lower Upper
63 100
106 26.9 21.5 32.3

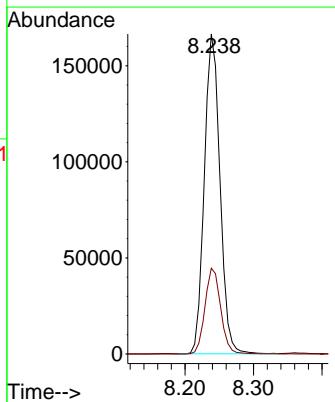



#59
2-Hexanone
Concen: 297.362 ug/l
RT: 9.427 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050



Tgt Ion: 43 Resp: 416984
Ion Ratio Lower Upper
43 100
58 51.7 25.9 77.6




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#60
Dibromochloromethane
Concen: 53.284 ug/l
RT: 9.519 min Scan# 1383
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00


Tgt Ion:129 Resp: 71569
Ion Ratio Lower Upper
129 100
127 77.0 38.5 115.5





#61
1,2-Dibromoethane
Concen: 52.217 ug/l
RT: 9.604 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050

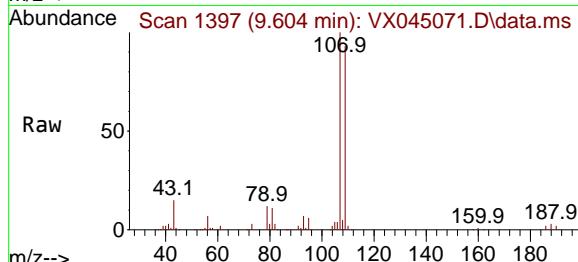


Tgt Ion:107 Resp: 6631
Ion Ratio Lower Upper
107 100
109 95.1 76.1 114.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#62
4-Bromofluorobenzene
Concen: 49.212 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00



Tgt Ion: 95 Resp: 74945
Ion Ratio Lower Upper
95 100
174 74.1 0.0 148.2
176 70.7 0.0 141.4




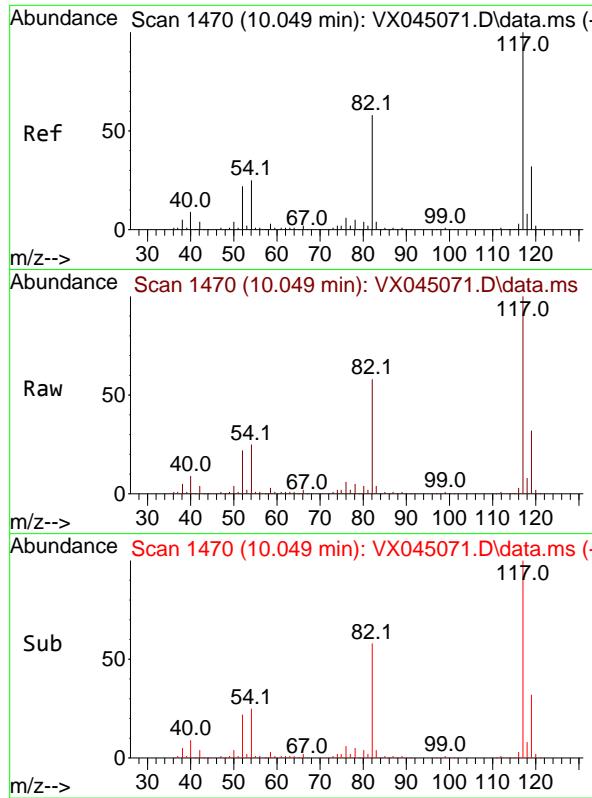


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 162079
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Instrument : MSVOA_X
ClientSampleId : VSTDICCC050


**Manual Integrations
APPROVED**


Reviewed By :John Carbone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

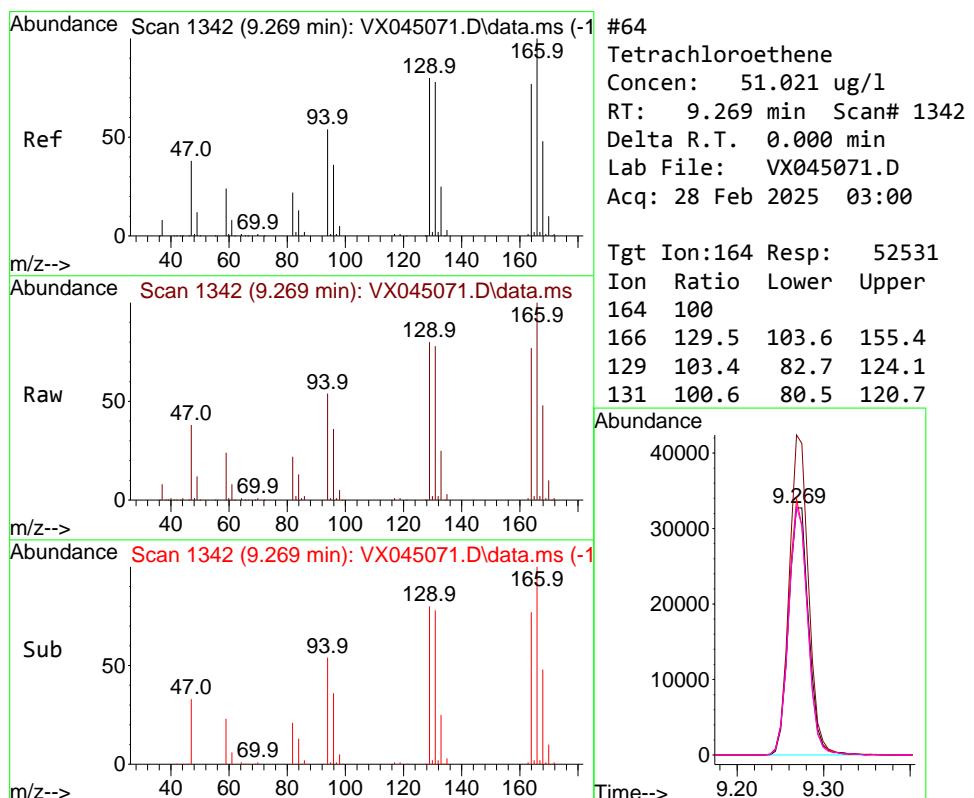

#64
Tetrachloroethene
Concen: 51.021 ug/l
RT: 9.269 min Scan# 1342
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Tgt Ion:164 Resp: 52531
Ion Ratio Lower Upper
164 100
166 129.5 103.6 155.4
129 103.4 82.7 124.1
131 100.6 80.5 120.7




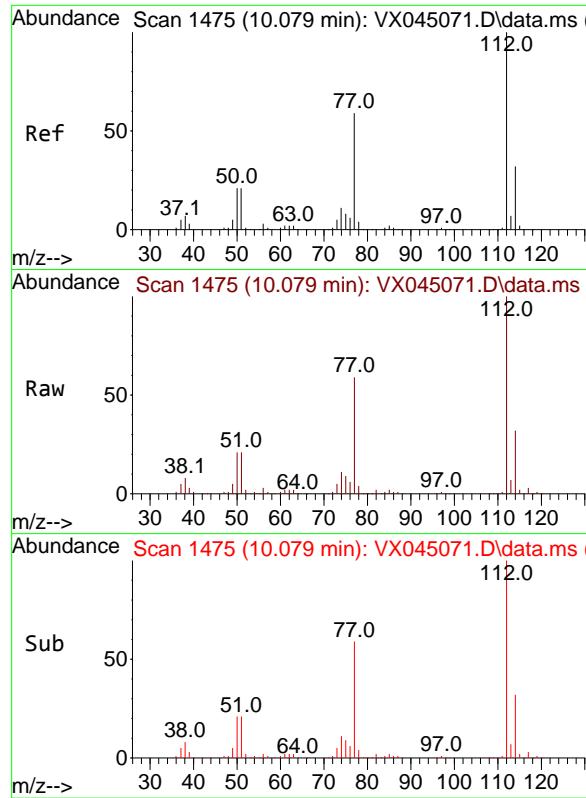


#65
Chlorobenzene
Concen: 50.853 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Instrument : MSVOA_X
ClientSampleId : VSTDICCC050


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

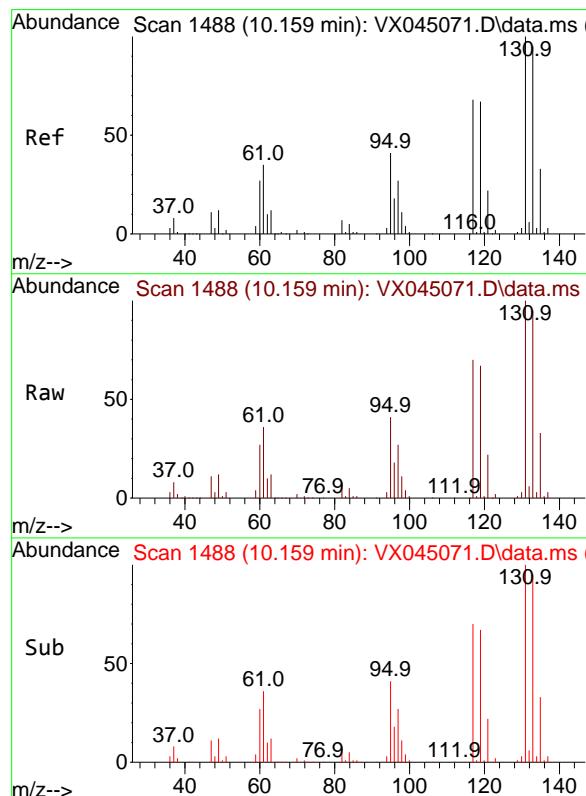


#66
1,1,1,2-Tetrachloroethane
Concen: 51.402 ug/l
RT: 10.159 min Scan# 1488
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Tgt Ion:131 Resp: 57642
Ion Ratio Lower Upper
131 100
133 97.3 48.6 145.9
119 67.8 33.9 101.7







#67
Ethyl Benzene
 Concen: 51.431 ug/l
 RT: 10.189 min Scan# 1493
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00
Instrument: MSVOA_X
ClientSampleId : VSTDICCC050

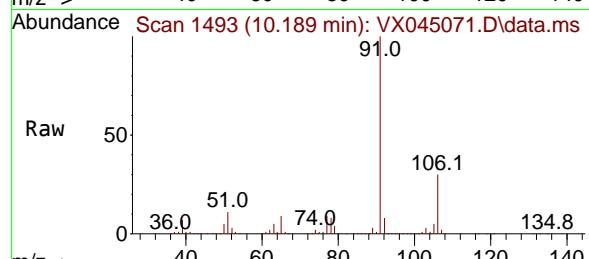


Tgt Ion: 91 Resp: 316421
 Ion Ratio Lower Upper
 91 100
 106 29.9 23.9 35.9

Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

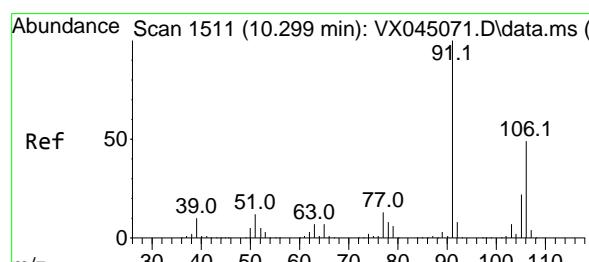


#68
m/p-Xylenes
 Concen: 103.515 ug/l
 RT: 10.299 min Scan# 1511
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00

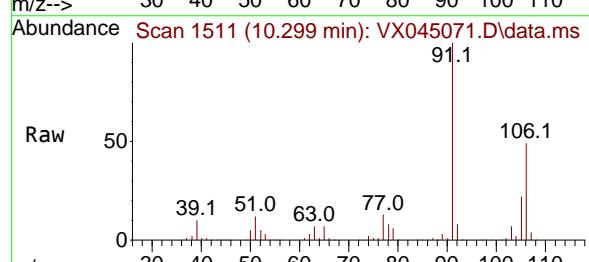

Tgt Ion:106 Resp: 234554
 Ion Ratio Lower Upper
 106 100
 91 206.7 165.4 248.0




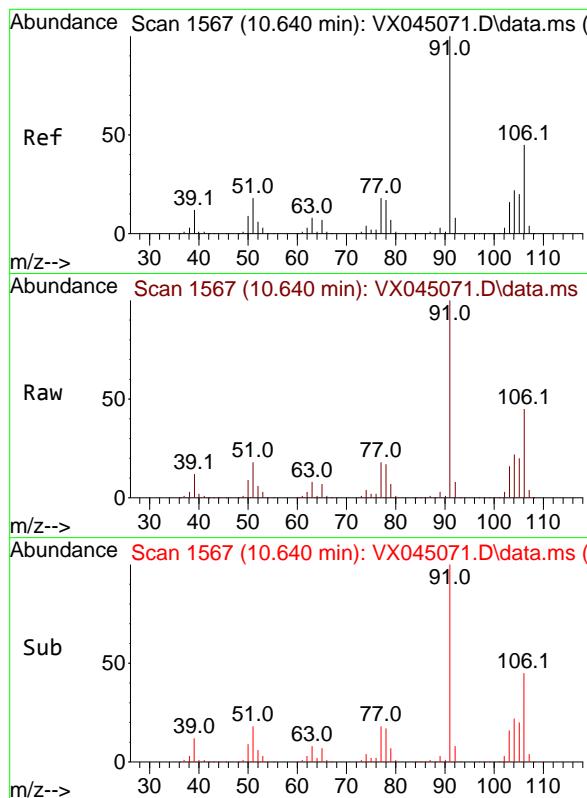


#69
o-Xylene
Concen: 50.341 ug/l
RT: 10.640 min Scan# 1
Instrument : MSVOA_X
Delta R.T. 0.000 min
Lab File: VX045071.D
ClientSampleId : VSTDICCC050
Acq: 28 Feb 2025 03:00

Tgt Ion:106 Resp: 114440
Ion Ratio Lower Upper
106 100
91 219.7 109.9 329.6


Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

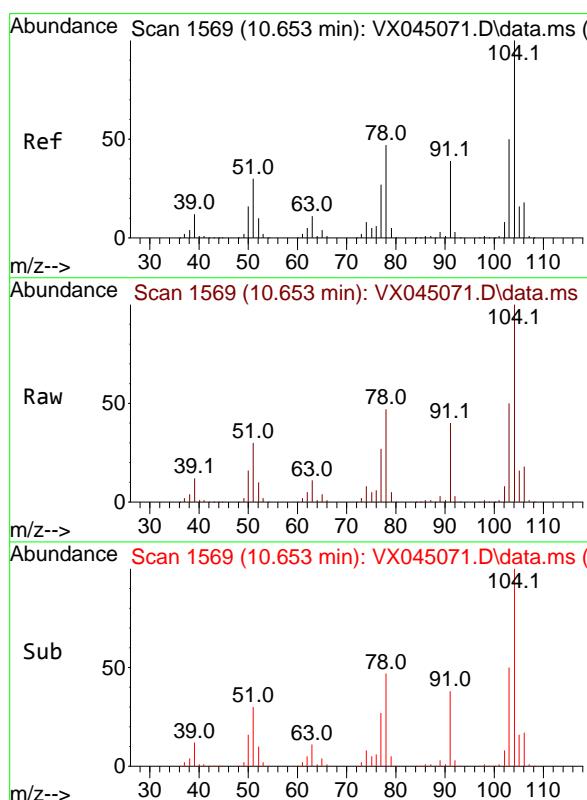

#70
Styrene
Concen: 52.387 ug/l
RT: 10.653 min Scan# 1569
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00


Tgt Ion:104 Resp: 191406
Ion Ratio Lower Upper
104 100
78 52.8 42.2 63.4
103 54.8 43.8 65.8





#71
Bromoform
Concen: 53.645 ug/l
RT: 10.799 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050



Tgt	Ion:173	Resp:	44730
Ion	Ratio	Lower	Upper
173	100		
175	49.1	24.6	73.6
254	0.0	0.0	0.0




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

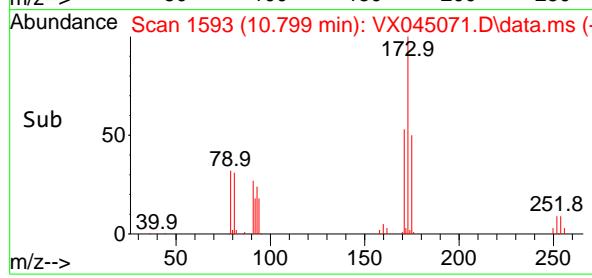

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Tgt	Ion:152	Resp:	71264
Ion	Ratio	Lower	Upper
152	100		
115	88.4	44.2	132.6
150	174.5	0.0	349.0

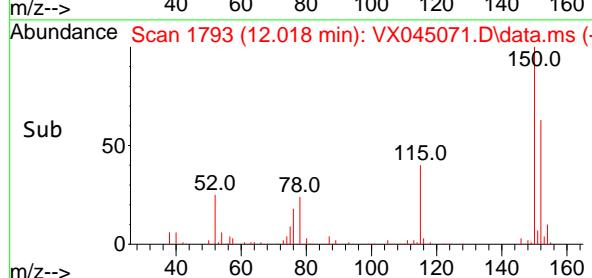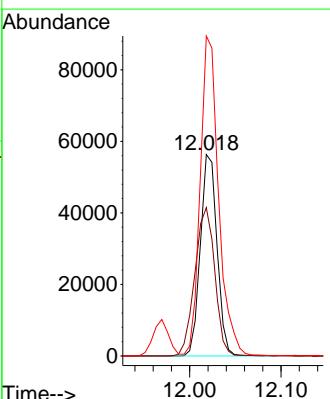


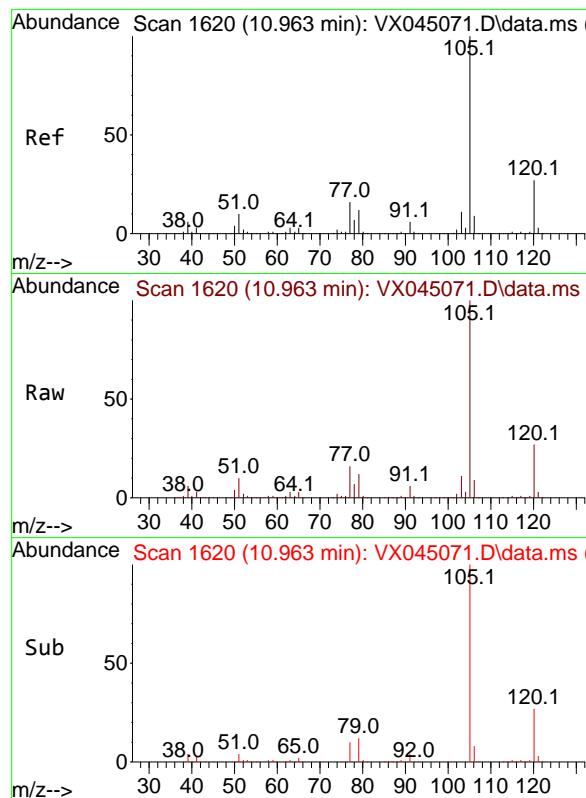


#73
Isopropylbenzene
Concen: 51.167 ug/l
RT: 10.963 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Instrument :
MSVOA_X
ClientSampleId :
VSTDICCC050


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

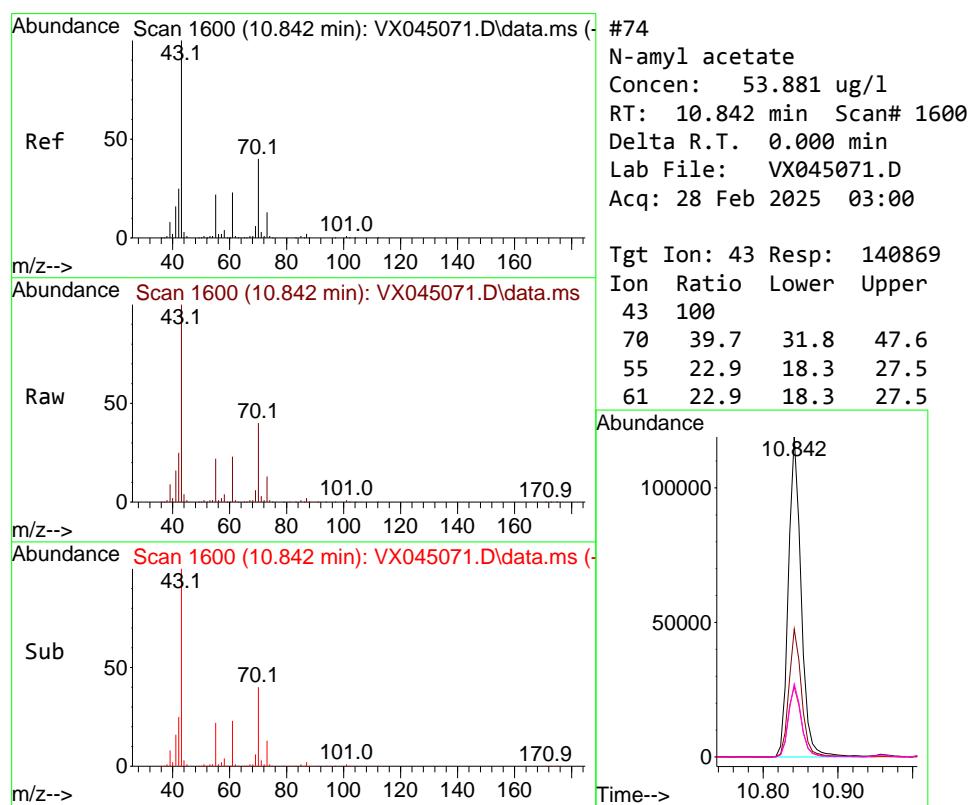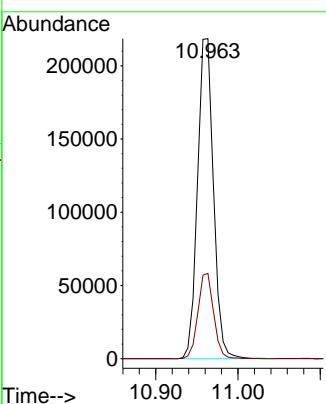

#74
N-amyl acetate
Concen: 53.881 ug/l
RT: 10.842 min Scan# 1600
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Tgt Ion: 43 Resp: 140869
Ion Ratio Lower Upper
43 100
70 39.7 31.8 47.6
55 22.9 18.3 27.5
61 22.9 18.3 27.5

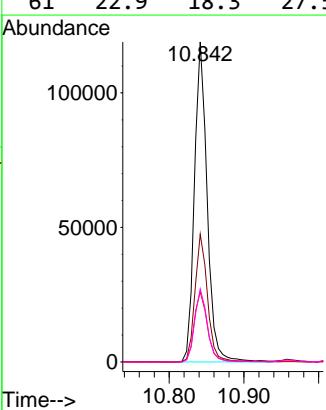

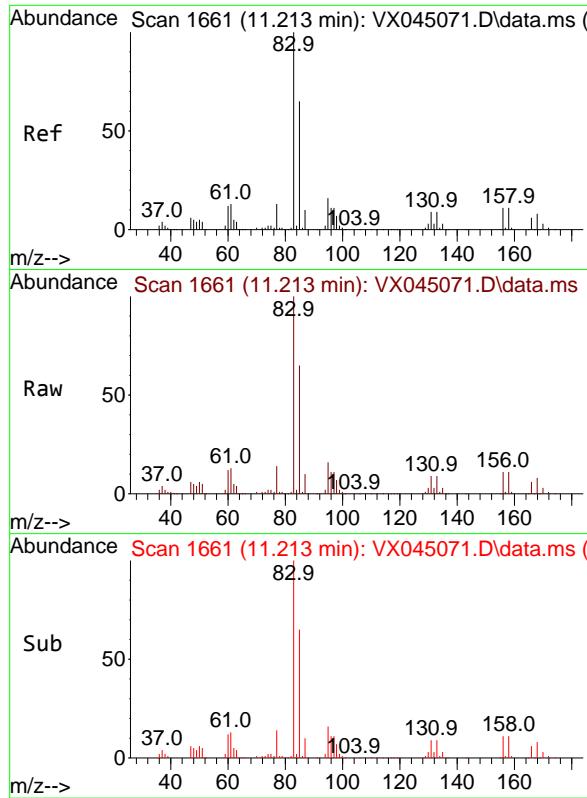


#75
1,1,2,2-Tetrachloroethane
Concen: 50.945 ug/l
RT: 11.213 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Instrument : MSVOA_X
ClientSampleId : VSTDICCC050

Tgt Ion: 83 Resp: 101089
Ion Ratio Lower Upper
83 100
131 8.9 4.5 13.4
85 63.4 31.7 95.1


Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

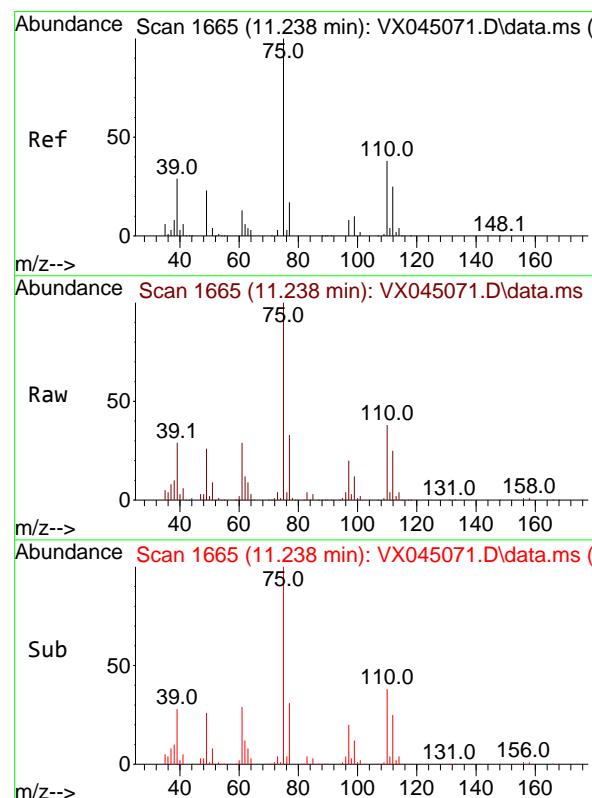

#76
1,2,3-Trichloropropane
Concen: 51.421 ug/l m
RT: 11.238 min Scan# 1665
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00



Tgt Ion: 75 Resp: 81743
Ion Ratio Lower Upper
75 100
77 41.4 20.7 62.1

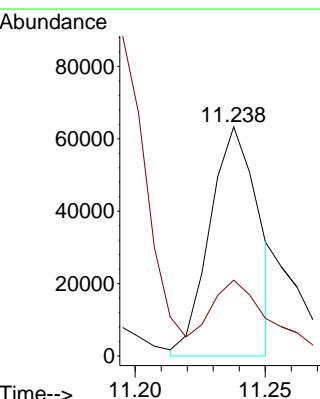



#77
Bromobenzene
Concen: 51.173 ug/l
RT: 11.195 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00



Instrument : MSVOA_X
ClientSampleId : VSTDICCC050

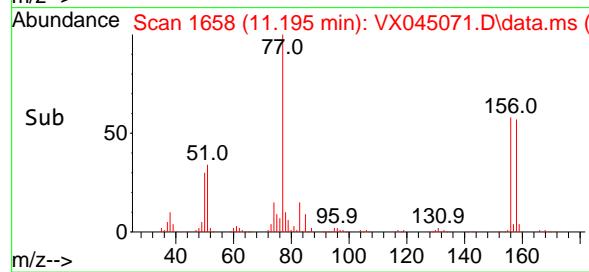


Tgt Ion:156 Resp: 6690
Ion Ratio Lower Upper
156 100
77 171.6 85.8 257.4
158 96.8 48.4 145.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#78
n-propylbenzene
Concen: 51.546 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Tgt Ion: 91 Resp: 342399
Ion Ratio Lower Upper
91 100
120 22.4 11.2 33.6





#79
2-Chlorotoluene
Concen: 50.154 ug/l
RT: 11.360 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument :
MSVOA_X
ClientSampleId :
VSTDICCC050



Tgt Ion: 91 Resp: 204484
Ion Ratio Lower Upper
91 100
126 32.9 16.4 49.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

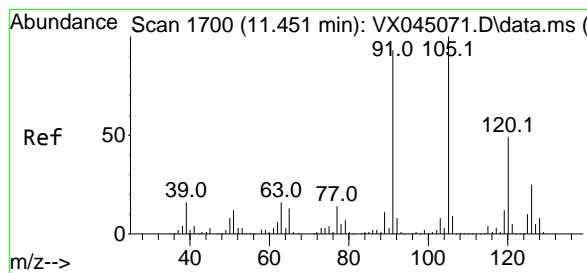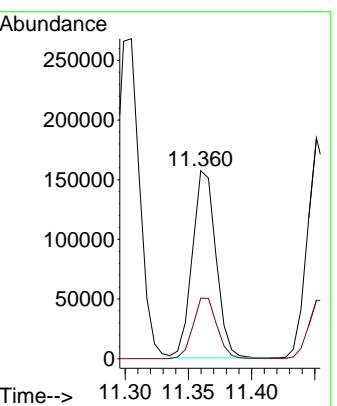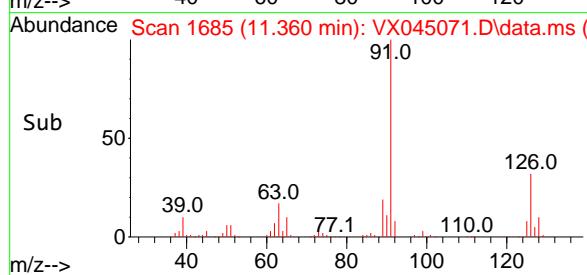

#80
1,3,5-Trimethylbenzene
Concen: 51.613 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Tgt Ion:105 Resp: 241129
Ion Ratio Lower Upper
105 100
120 48.1 24.1 72.2

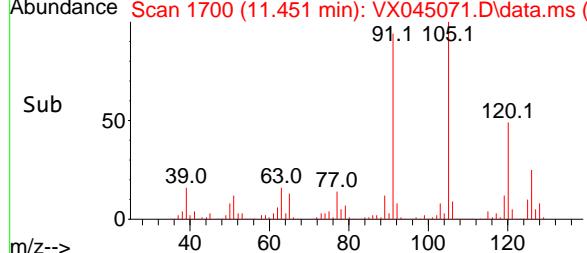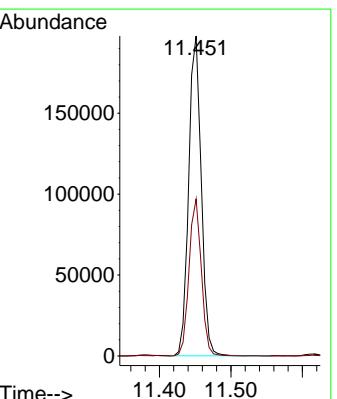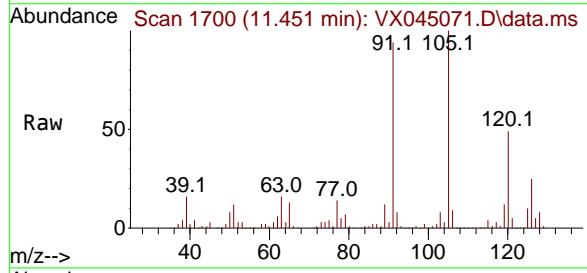


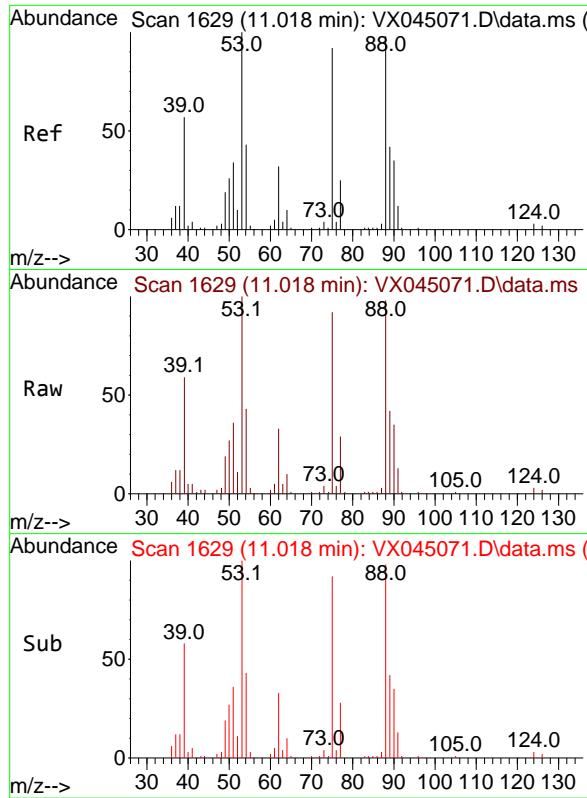


#81
trans-1,4-Dichloro-2-butene
Concen: 41.172 ug/l
RT: 11.018 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Instrument : MSVOA_X
ClientSampleId : VSTDICCC050


Manual Integrations APPROVED




Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

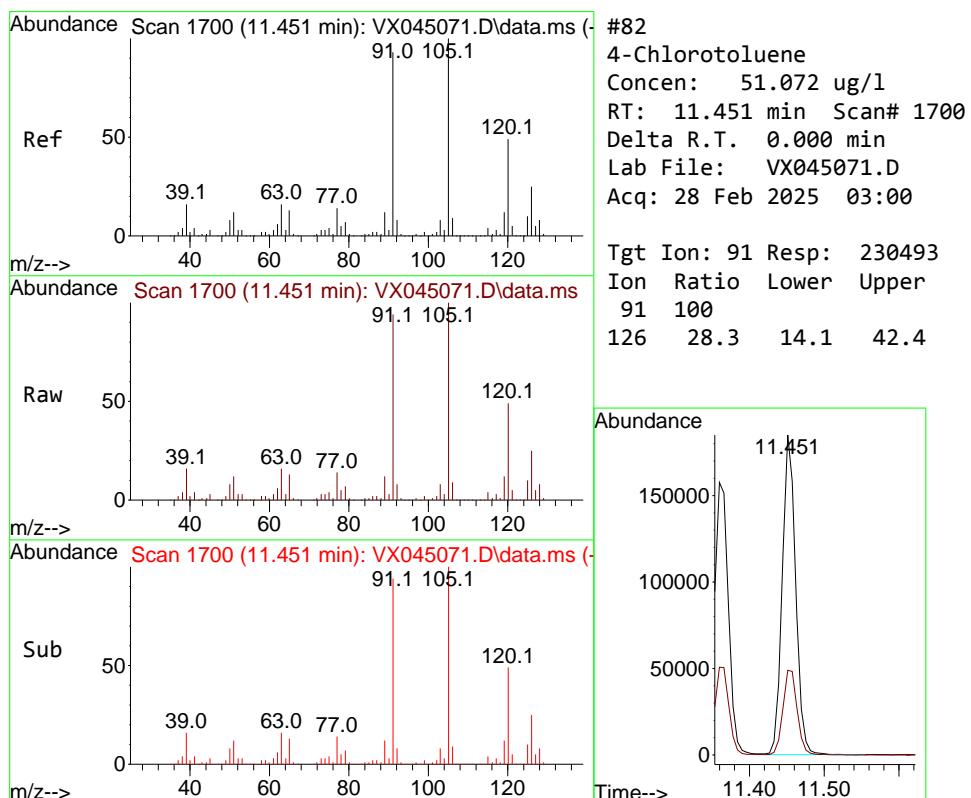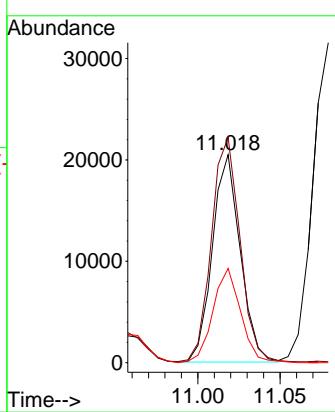

#82
4-Chlorotoluene
Concen: 51.072 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Tgt Ion: 91 Resp: 230493
Ion Ratio Lower Upper
91 100
126 28.3 14.1 42.4

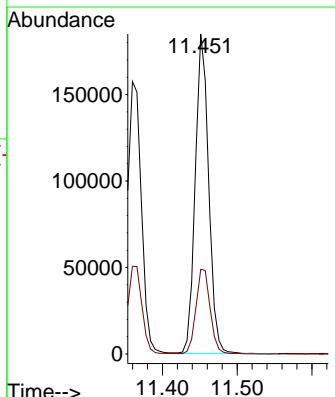



#83

tert-Butylbenzene

Concen: 50.895 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045071.D

Acq: 28 Feb 2025 03:00




Instrument:

MSVOA_X

ClientSampleId :

VSTDICCC050

**Manual Integrations
APPROVED**

 Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025


#84

1,2,4-Trimethylbenzene


Concen: 52.326 ug/l


RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX045071.D


Acq: 28 Feb 2025 03:00

 Tgt Ion:105 Resp: 240719
 Ion Ratio Lower Upper
 105 100
 120 44.1 22.1 66.1




#85
sec-Butylbenzene
Concen: 51.353 ug/l
RT: 11.890 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00



Instrument : MSVOA_X
ClientSampleId : VSTDICCC050

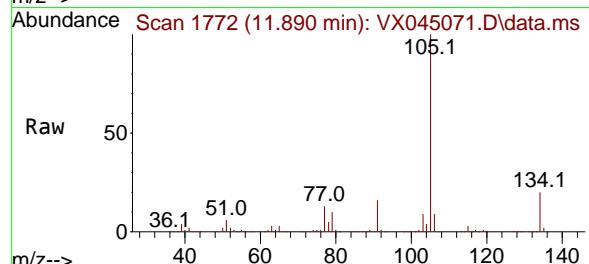


Tgt Ion:105 Resp: 300391
Ion Ratio Lower Upper
105 100
134 19.6 9.8 29.4

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

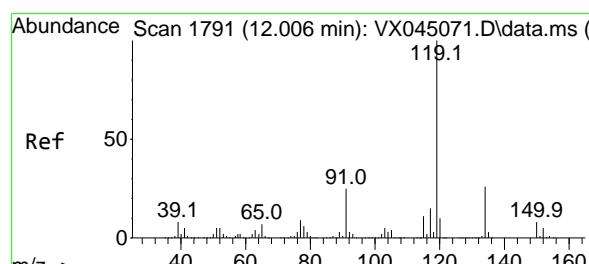


#86
p-Isopropyltoluene
Concen: 51.964 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

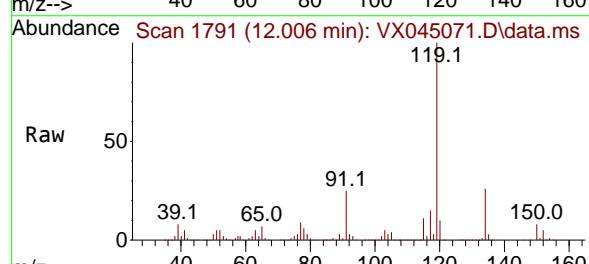

Tgt Ion:119 Resp: 244031
Ion Ratio Lower Upper
119 100
134 25.7 12.9 38.6
91 25.3 12.7 38.0




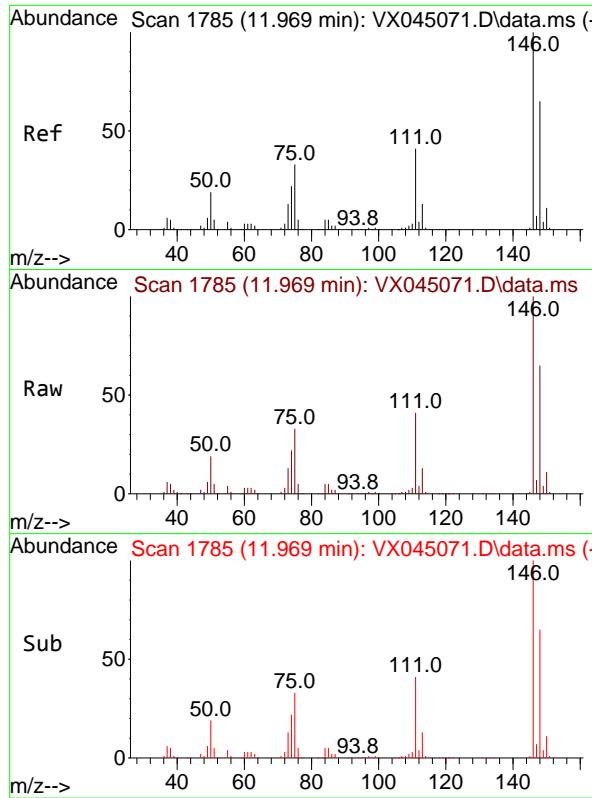


#87
 1,3-Dichlorobenzene
 Concen: 49.747 ug/l
 RT: 11.969 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00

Instrument : MSVOA_X
 ClientSampleId : VSTDICCC050


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

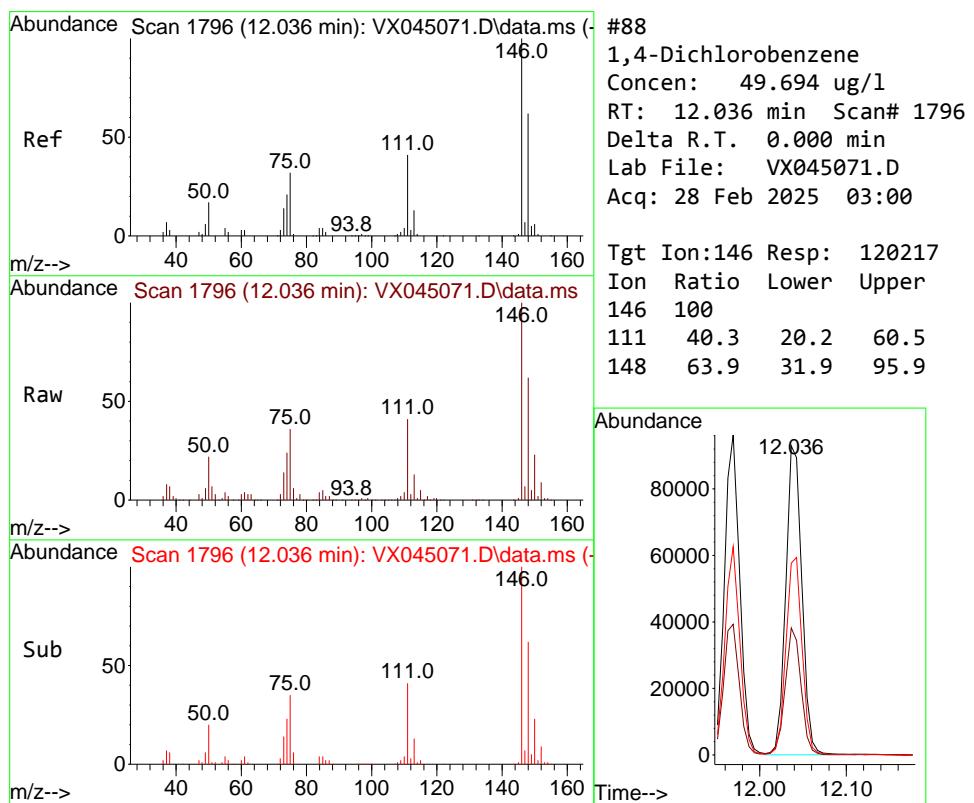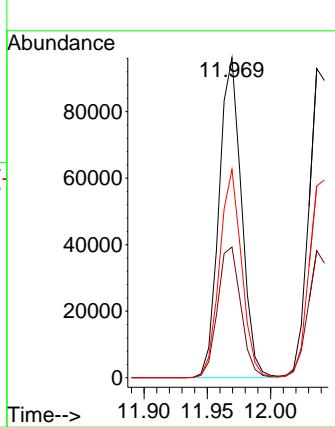

#88
 1,4-Dichlorobenzene
 Concen: 49.694 ug/l
 RT: 12.036 min Scan# 1796
 Delta R.T. 0.000 min
 Lab File: VX045071.D
 Acq: 28 Feb 2025 03:00


Tgt Ion:146 Resp: 120217
 Ion Ratio Lower Upper
 146 100
 111 40.3 20.2 60.5
 148 63.9 31.9 95.9





#89
n-Butylbenzene
Concen: 52.006 ug/l
RT: 12.329 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050




Tgt Ion: 91 Resp: 21468
Ion Ratio Lower Upper
91 100
92 53.3 26.7 80.0
134 24.4 12.2 36.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

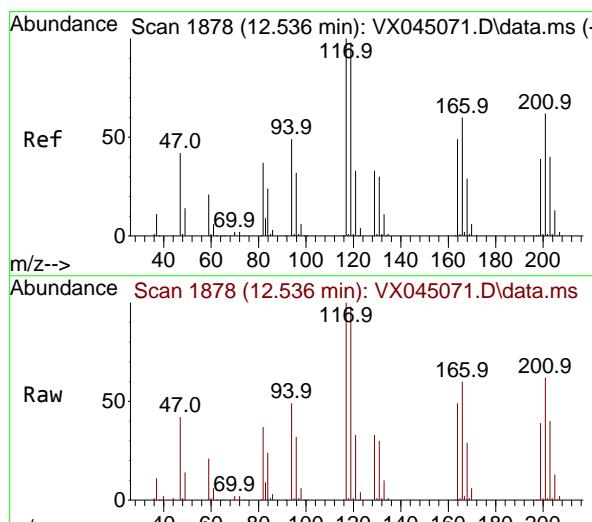


#90
Hexachloroethane
Concen: 49.188 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Tgt Ion:117 Resp: 43086
Ion Ratio Lower Upper
117 100
201 63.9 31.9 95.9





#91
1,2-Dichlorobenzene
Concen: 50.557 ug/l
RT: 12.335 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00




Instrument : MSVOA_X
ClientSampleId : VSTDICCC050



Tgt Ion:146 Resp: 118890
Ion Ratio Lower Upper
146 100
111 43.3 21.6 65.0
148 63.9 31.9 95.9



Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#92
1,2-Dibromo-3-Chloropropane
Concen: 56.123 ug/l
RT: 12.939 min Scan# 1944
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Tgt Ion: 75 Resp: 20610
Ion Ratio Lower Upper
75 100
155 79.1 39.6 118.7
157 102.3 51.1 153.4




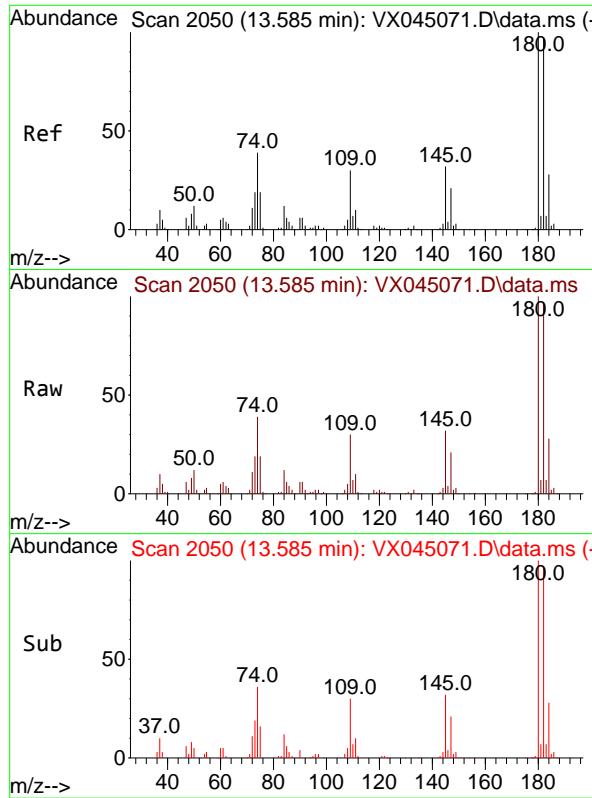


#93
1,2,4-Trichlorobenzene
Concen: 50.571 ug/l
RT: 13.585 min Scan# 2
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Instrument : MSVOA_X
ClientSampleId : VSTDICCC050


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

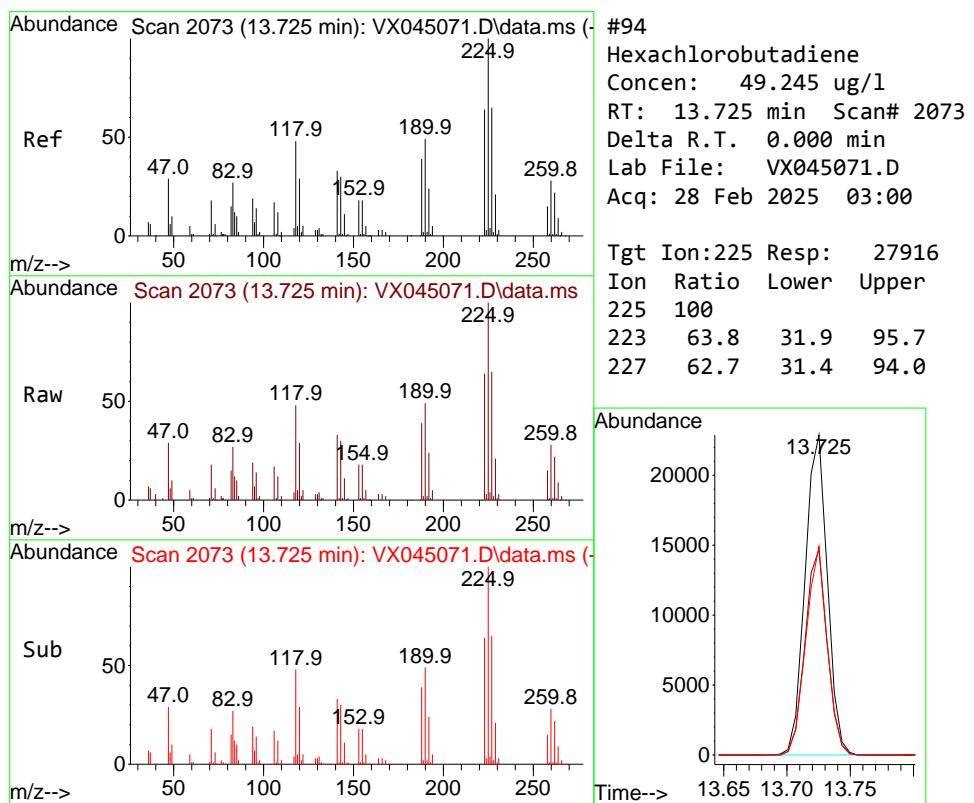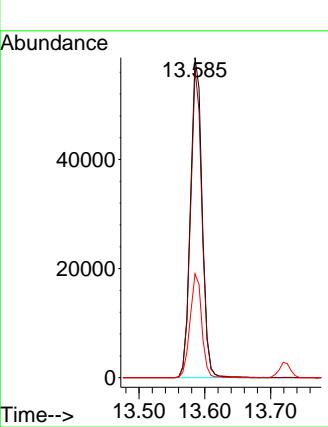

#94
Hexachlorobutadiene
Concen: 49.245 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Tgt Ion:225 Resp: 27916
Ion Ratio Lower Upper
225 100
223 63.8 31.9 95.7
227 62.7 31.4 94.0

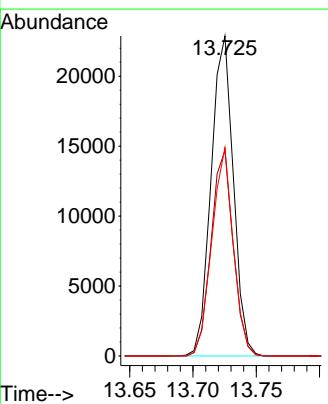

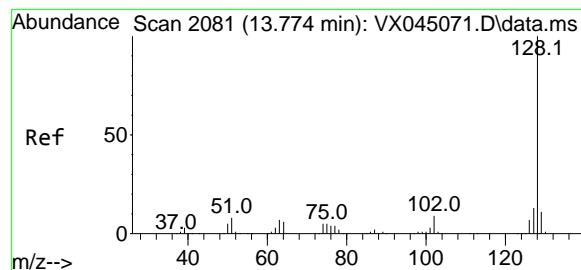





#95
Naphthalene
Concen: 53.700 ug/l
RT: 13.774 min Scan# 20
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Instrument :
MSVOA_X
ClientSampleId :
VSTDICCC050

Manual Integrations




APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

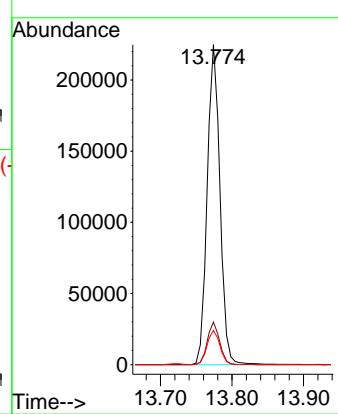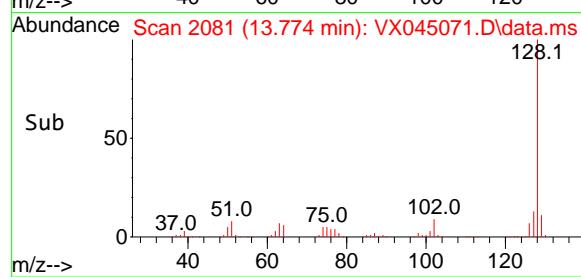

#96
1,2,3-Trichlorobenzene
Concen: 52.406 ug/l
RT: 13.957 min Scan# 2111
Delta R.T. 0.000 min
Lab File: VX045071.D
Acq: 28 Feb 2025 03:00

Tgt	Ion:180	Resp:	75482
Ion	Ratio	Lower	Upper
180	100		
182	95.1	47.5	142.6
145	33.9	17.0	50.9

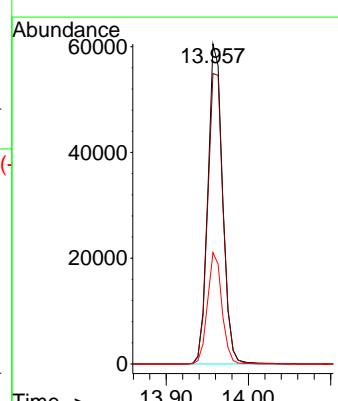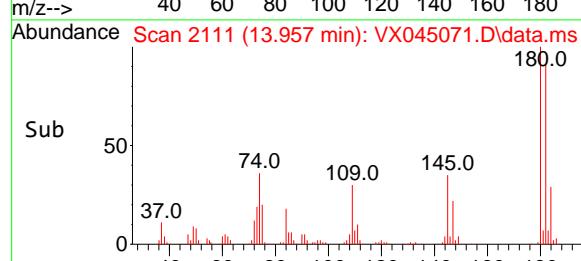

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045072.D
 Acq On : 28 Feb 2025 03:23
 Operator : JC/MD
 Sample : VSTDICC100
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

Quant Time: Feb 28 05:35:19 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 05:28:02 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.550	168	101178	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	181031	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	151175	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	69086	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	158452	106.011	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 212.020%	#	
35) Dibromofluoromethane	5.385	113	123185	104.110	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 208.220%	#	
50) Toluene-d8	8.647	98	441188	99.595	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 199.200%	#	
62) 4-Bromofluorobenzene	11.079	95	148476	100.365	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	= 200.720%	#	
Target Compounds						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	126718	90.869	ug/l	95
3) Chloromethane	1.306	50	145825	85.936	ug/l	98
4) Vinyl Chloride	1.373	62	154734	93.360	ug/l	96
5) Bromomethane	1.593	94	57503	110.980	ug/l	97
6) Chloroethane	1.660	64	60155	95.351	ug/l	97
7) Trichlorofluoromethane	1.861	101	198701	93.594	ug/l	99
8) Diethyl Ether	2.135	74	78263	101.441	ug/l	100
9) 1,1,2-Trichlorotrifluo...	2.312	101	120518	95.064	ug/l	98
10) Methyl Iodide	2.440	142	153466	94.425	ug/l	99
11) Tert butyl alcohol	3.001	59	135016	493.141	ug/l	98
12) 1,1-Dichloroethene	2.306	96	125436	96.366	ug/l	98
13) Acrolein	2.239	56	180411	608.485	ug/l	99
14) Allyl chloride	2.654	41	220783	94.344	ug/l	98
15) Acrylonitrile	3.068	53	391946	526.749	ug/l	100
16) Acetone	2.392	43	348698	566.991	ug/l	99
17) Carbon Disulfide	2.495	76	345572	97.574	ug/l	98
18) Methyl Acetate	2.709	43	175784	94.899	ug/l	98
19) Methyl tert-butyl Ether	3.117	73	431413	103.661	ug/l	100
20) Methylene Chloride	2.782	84	140388	96.381	ug/l	98
21) trans-1,2-Dichloroethene	3.080	96	128232	100.164	ug/l	98
22) Diisopropyl ether	3.763	45	467534	104.489	ug/l	98
23) Vinyl Acetate	3.721	43	2035880	554.219	ug/l	99
24) 1,1-Dichloroethane	3.605	63	257023	102.805	ug/l	100
25) 2-Butanone	4.562	43	559182	563.952	ug/l	99
26) 2,2-Dichloropropane	4.470	77	124805	67.148	ug/l	100
27) cis-1,2-Dichloroethene	4.483	96	155193	100.568	ug/l	99
28) Bromochloromethane	4.897	49	113848	94.428	ug/l	98
29) Tetrahydrofuran	5.007	42	365565	556.465	ug/l	100
30) Chloroform	5.092	83	248978	101.814	ug/l	97
31) Cyclohexane	5.464	56	231082	100.711	ug/l	97
32) 1,1,1-Trichloroethane	5.379	97	211302	102.638	ug/l	99
36) 1,1-Dichloropropene	5.690	75	172295	101.258	ug/l	99
37) Ethyl Acetate	4.720	43	220327	113.796	ug/l	99
38) Carbon Tetrachloride	5.671	117	177219	105.940	ug/l	97
39) Methylcyclohexane	7.372	83	219856	101.175	ug/l	99
40) Benzene	6.031	78	541974	101.908	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045072.D
 Acq On : 28 Feb 2025 03:23
 Operator : JC/MD
 Sample : VSTDICC100
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

Quant Time: Feb 28 05:35:19 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 05:28:02 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	120186	116.205	ug/1	98
42) 1,2-Dichloroethane	6.086	62	189857	110.158	ug/1	99
43) Isopropyl Acetate	6.342	43	338414	109.806	ug/1	99
44) Trichloroethene	7.122	130	128124	105.402	ug/1	96
45) 1,2-Dichloropropane	7.427	63	135997	102.898	ug/1	100
46) Dibromomethane	7.580	93	97248	105.329	ug/1	99
47) Bromodichloromethane	7.817	83	191016	106.947	ug/1	97
48) Methyl methacrylate	7.695	41	165825	113.344	ug/1	99
49) 1,4-Dioxane	7.665	88	66308	2132.314	ug/1	99
51) 4-Methyl-2-Pentanone	8.573	43	1048140	555.050	ug/1	99
52) Toluene	8.714	92	316349	100.178	ug/1	100
53) t-1,3-Dichloropropene	8.976	75	177352	100.462	ug/1	97
54) cis-1,3-Dichloropropene	8.366	75	200943	101.815	ug/1	98
55) 1,1,2-Trichloroethane	9.146	97	123426	100.920	ug/1	99
56) Ethyl methacrylate	9.116	69	208782	106.744	ug/1	100
57) 1,3-Dichloropropane	9.305	76	216267	101.387	ug/1	100
58) 2-Chloroethyl Vinyl ether	8.238	63	494551	514.987	ug/1	99
59) 2-Hexanone	9.433	43	779492	572.233	ug/1	99
60) Dibromochloromethane	9.518	129	139245	106.719	ug/1	99
61) 1,2-Dibromoethane	9.610	107	128617	104.259	ug/1	99
64) Tetrachloroethene	9.268	164	99386	103.491	ug/1	98
65) Chlorobenzene	10.079	112	332473	102.456	ug/1	100
66) 1,1,1,2-Tetrachloroethane	10.158	131	112451	107.511	ug/1	96
67) Ethyl Benzene	10.189	91	596257	103.905	ug/1	100
68) m/p-Xylenes	10.299	106	432214	204.507	ug/1	99
69) o-Xylene	10.640	106	213835	100.849	ug/1	99
70) Styrene	10.652	104	357649	104.948	ug/1	99
71) Bromoform	10.799	173	90800	116.751	ug/1 #	99
73) Isopropylbenzene	10.963	105	553533	99.138	ug/1	99
74) N-amyl acetate	10.841	43	287104	113.277	ug/1	100
75) 1,1,2,2-Tetrachloroethane	11.213	83	192217	99.923	ug/1	98
76) 1,2,3-Trichloropropane	11.238	75	156259m	101.395	ug/1	
77) Bromobenzene	11.195	156	125700	99.175	ug/1	97
78) n-propylbenzene	11.305	91	648835	100.758	ug/1	99
79) 2-Chlorotoluene	11.359	91	382703	96.825	ug/1	100
80) 1,3,5-Trimethylbenzene	11.451	105	445466	98.356	ug/1	99
81) trans-1,4-Dichloro-2-b...	11.018	75	51975	91.460	ug/1	99
82) 4-Chlorotoluene	11.451	91	433881	99.168	ug/1	100
83) tert-Butylbenzene	11.713	119	454859	99.288	ug/1	99
84) 1,2,4-Trimethylbenzene	11.750	105	450108	100.926	ug/1	99
85) sec-Butylbenzene	11.890	105	570006	100.517	ug/1	100
86) p-Isopropyltoluene	12.006	119	465512	102.252	ug/1	100
87) 1,3-Dichlorobenzene	11.969	146	231440	99.903	ug/1	100
88) 1,4-Dichlorobenzene	12.042	146	230663	98.355	ug/1	99
89) n-Butylbenzene	12.329	91	428209	107.000	ug/1	99
90) Hexachloroethane	12.536	117	87448	102.980	ug/1	99
91) 1,2-Dichlorobenzene	12.335	146	233125	102.254	ug/1	99
92) 1,2-Dibromo-3-Chloropr...	12.938	75	41402	116.296	ug/1	99
93) 1,2,4-Trichlorobenzene	13.585	180	148368	107.648	ug/1	99
94) Hexachlorobutadiene	13.725	225	56065	102.019	ug/1	99
95) Naphthalene	13.774	128	565250	112.593	ug/1	100
96) 1,2,3-Trichlorobenzene	13.963	180	152970	109.554	ug/1	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045072.D
Acq On : 28 Feb 2025 03:23
Operator : JC/MD
Sample : VSTDICC100
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

Quant Time: Feb 28 05:35:19 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 05:28:02 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carbone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045072.D
Acq On : 28 Feb 2025 03:23
Operator : JC/MD
Sample : VSTDIICC100
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

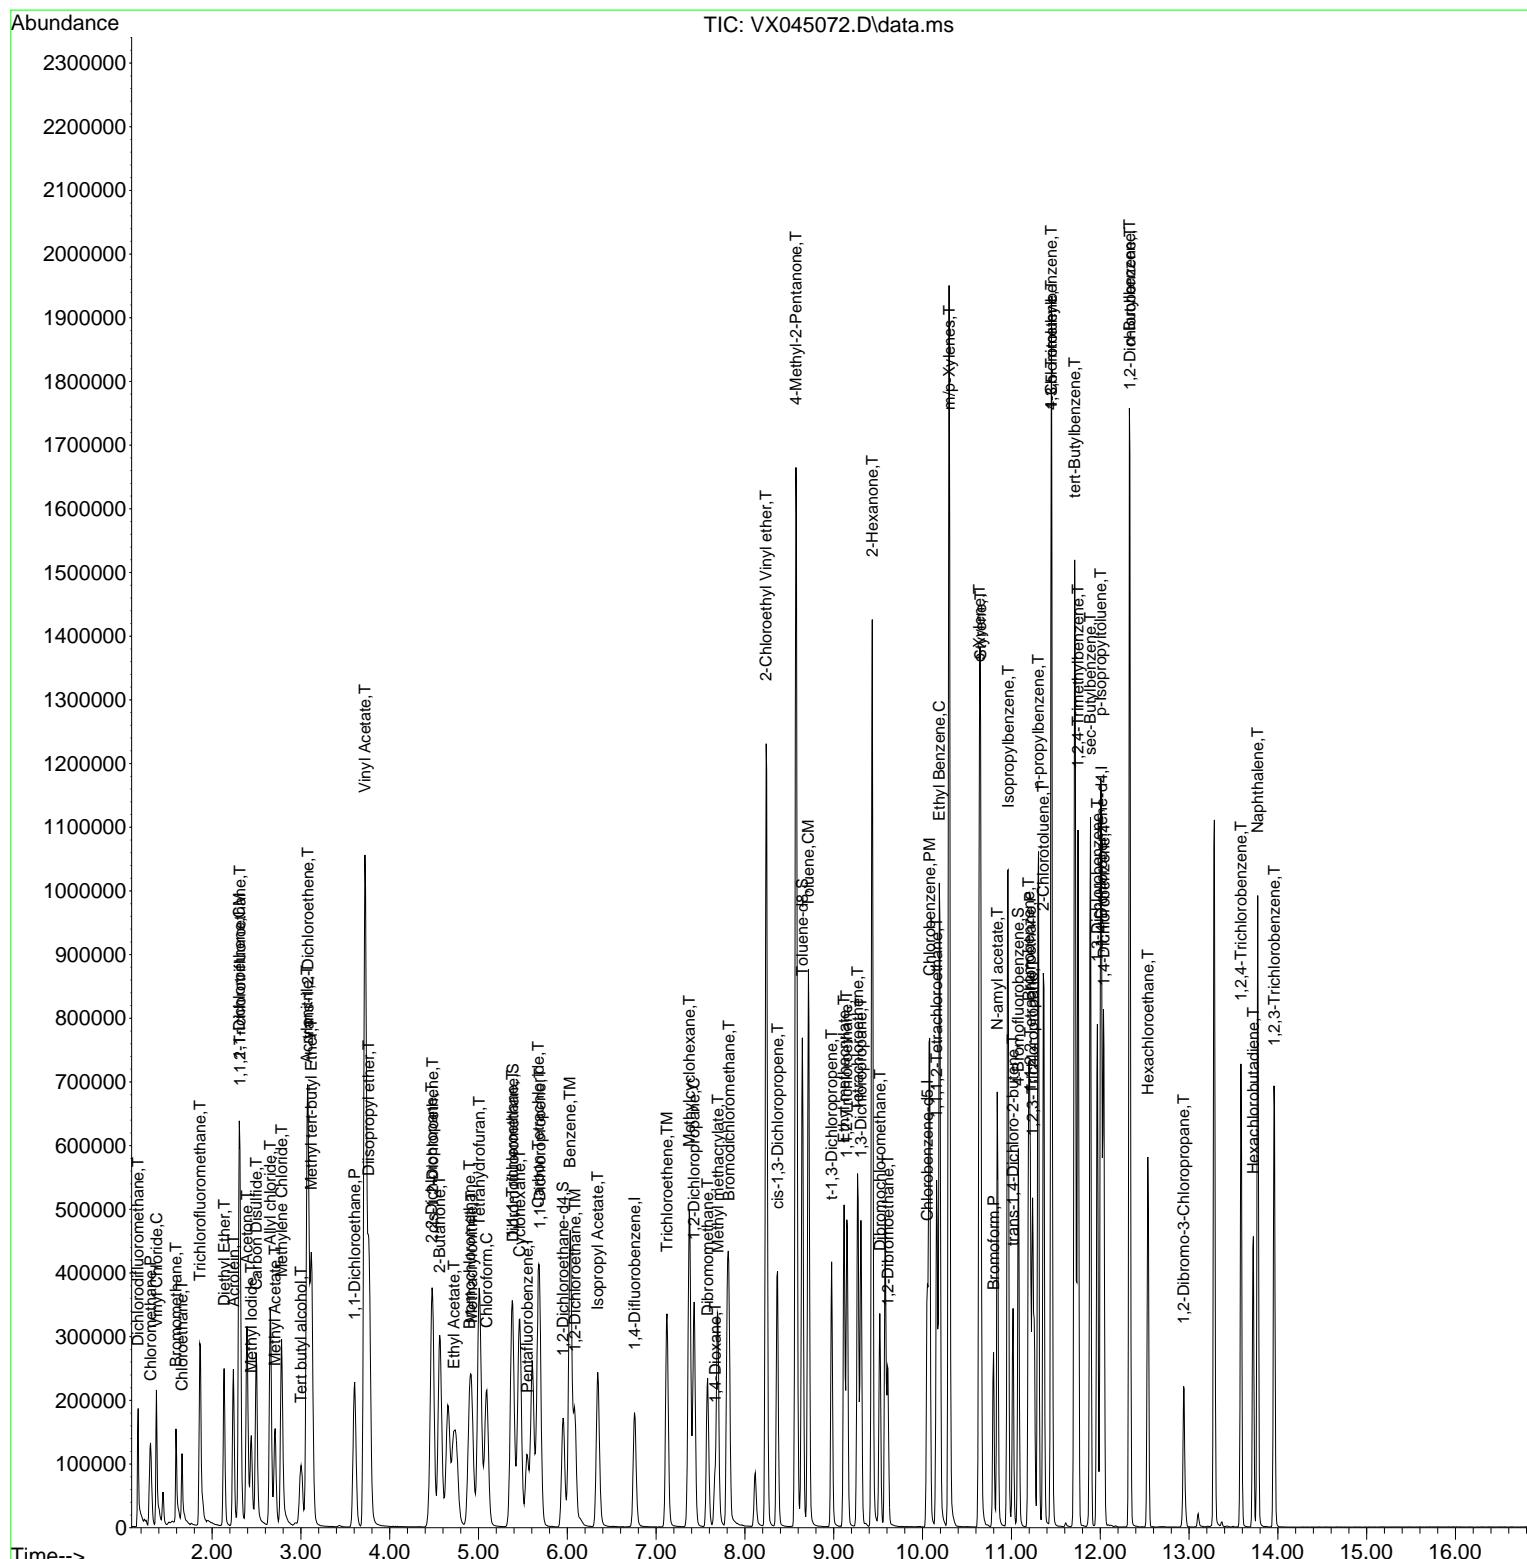



#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.550 min Scan# 7
 Delta R.T. -0.000 min
 Lab File: VX045072.D
 Acq: 28 Feb 2025 03:23



Instrument : MSVOA_X
 ClientSampleId : VSTDICC100



Tgt Ion:168 Resp: 101173
 Ion Ratio Lower Upper
 168 100
 99 60.2 48.2 72.4



Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025



#2
 Dichlorodifluoromethane
 Concen: 90.869 ug/l
 RT: 1.166 min Scan# 13
 Delta R.T. -0.000 min
 Lab File: VX045072.D
 Acq: 28 Feb 2025 03:23


Tgt Ion: 85 Resp: 126718
 Ion Ratio Lower Upper
 85 100
 87 32.1 17.4 52.3




Abundance Scan 13 (1.166 min): VX045072.D\data.ms

Raw


m/z	Relative Abundance (approx)
37.0	10
50.0	15
66.0	15
85.0	100
100.9	20
121.8	20





#3
Chloromethane
Concen: 85.936 ug/l
RT: 1.306 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23



Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion: 50 Resp: 14582
Ion Ratio Lower Upper
50 100
52 32.5 25.0 37.4

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



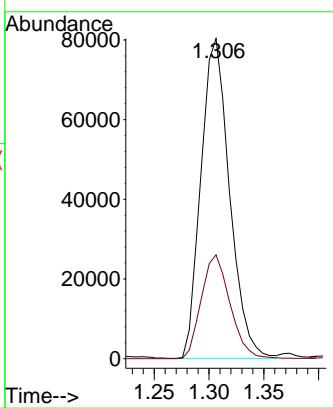


#4
Vinyl Chloride
Concen: 93.360 ug/l
RT: 1.373 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

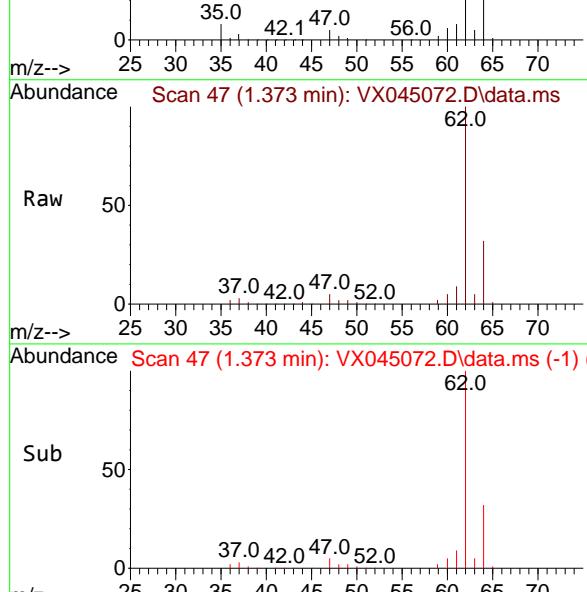

Tgt Ion: 62 Resp: 154734
Ion Ratio Lower Upper
62 100
64 32.4 24.3 36.5

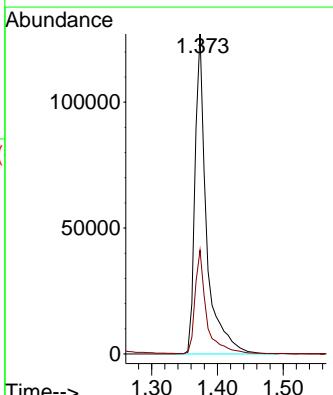







#5
 Bromomethane
 Concen: 110.980 ug/l
 RT: 1.593 min Scan# 8
 Delta R.T. -0.000 min
 Lab File: VX045072.D
 Acq: 28 Feb 2025 03:23

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC100


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

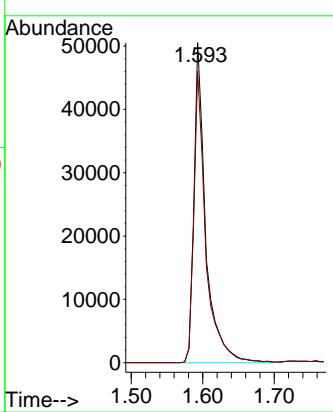


#6
 Chloroethane
 Concen: 95.351 ug/l
 RT: 1.660 min Scan# 94
 Delta R.T. -0.000 min
 Lab File: VX045072.D
 Acq: 28 Feb 2025 03:23

Tgt Ion: 64 Resp: 60155
 Ion Ratio Lower Upper
 64 100
 66 31.7 26.7 40.1

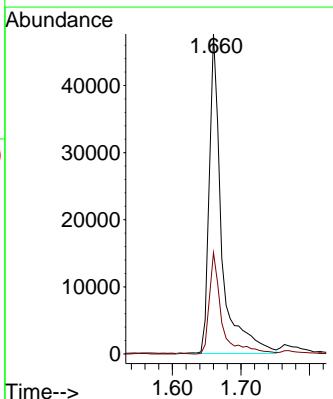






#7
Trichlorofluoromethane
Concen: 93.594 ug/l
RT: 1.861 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

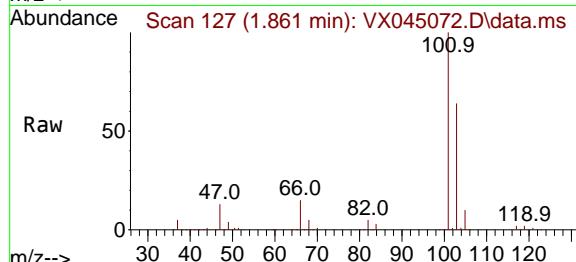


Tgt Ion: 101 Resp: 19870
Ion Ratio Lower Upper
101 100
103 64.2 52.1 78.1

**Manual Integrations
APPROVED**



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

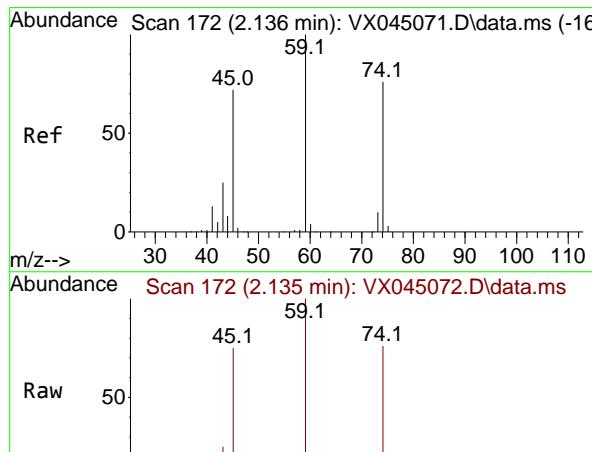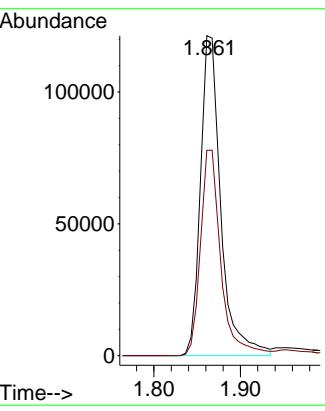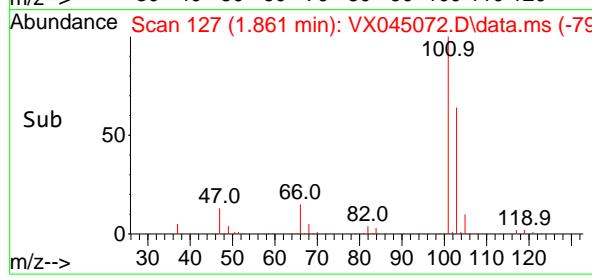


#8
Diethyl Ether
Concen: 101.441 ug/l
RT: 2.135 min Scan# 172
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 74 Resp: 78263
Ion Ratio Lower Upper
74 100
45 102.7 51.5 154.5

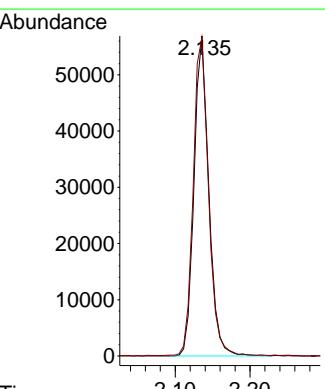



#9
1,1,2-Trichlorotrifluoroethane
Concen: 95.064 ug/l
RT: 2.312 min Scan# 2
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

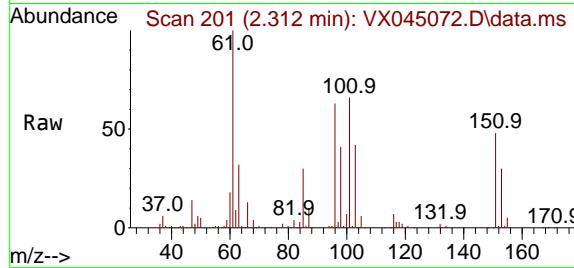


Tgt Ion:101 Resp: 12051:
Ion Ratio Lower Upper
101 100
85 46.5 36.2 54.4
151 72.4 56.4 84.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

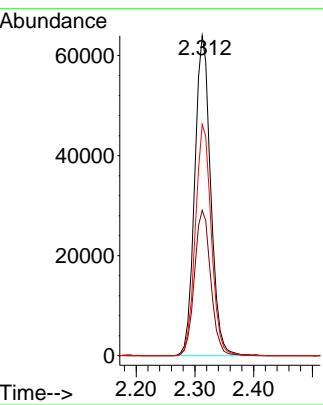


#10
Methyl Iodide
Concen: 94.425 ug/l
RT: 2.440 min Scan# 222
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion:142 Resp: 153466
Ion Ratio Lower Upper
142 100
127 45.0 35.4 53.2
141 14.4 11.6 17.4

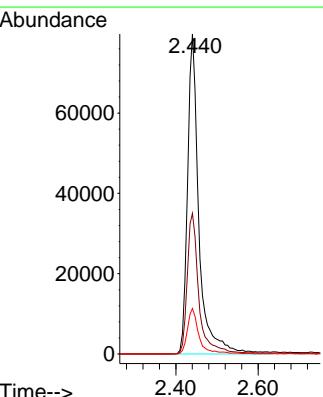



#11
Tert butyl alcohol
Concen: 493.141 ug/l
RT: 3.001 min Scan# 311
Delta R.T. 0.018 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion: 59 Resp: 135010
Ion Ratio Lower Upper
59 100
57 10.4 7.8 11.8

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

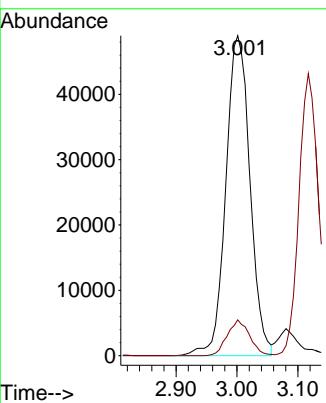


#12
1,1-Dichloroethene
Concen: 96.366 ug/l
RT: 2.306 min Scan# 200
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 96 Resp: 125436
Ion Ratio Lower Upper
96 100
61 165.4 134.6 202.0
98 63.7 51.0 76.6

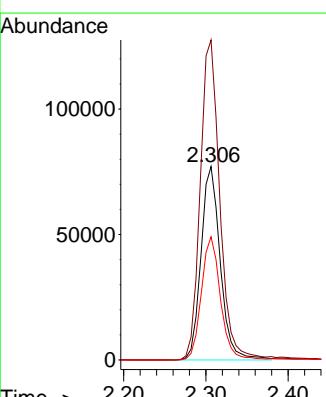



#13
Acrolein
Concen: 608.485 ug/l
RT: 2.239 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument : MSVOA_X
ClientSampleId : VSTDICC100

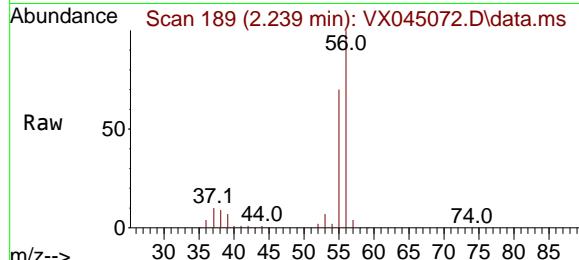


Tgt Ion: 56 Resp: 18041:
Ion Ratio Lower Upper
56 100
55 69.8 56.2 84.4

**Manual Integrations
APPROVED**



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#14
Allyl chloride
Concen: 94.344 ug/l
RT: 2.654 min Scan# 257
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 41 Resp: 220783
Ion Ratio Lower Upper
41 100
39 68.4 53.8 80.8
76 32.6 25.2 37.8

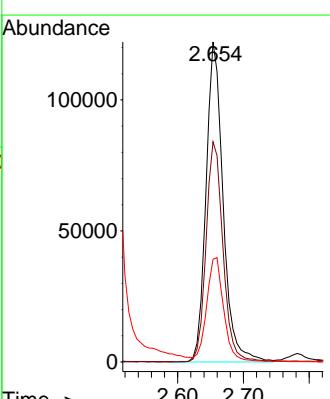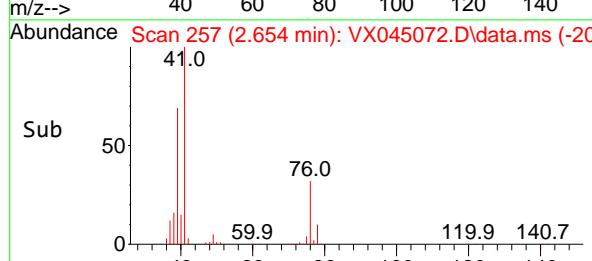



#15
Acrylonitrile
Concen: 526.749 ug/l
RT: 3.068 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23



Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion: 53 Resp: 391940
Ion Ratio Lower Upper
53 100
52 82.9 66.2 99.2
51 36.6 29.0 43.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#16
Acetone
Concen: 566.991 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 43 Resp: 348698
Ion Ratio Lower Upper
43 100
58 29.7 24.2 36.4





#17
Carbon Disulfide
Concen: 97.574 ug/l
RT: 2.495 min Scan# 2
Delta R.T. -0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100




Tgt Ion: 76 Resp: 34557
Ion Ratio Lower Upper
76 100
78 8.7 6.6 9.8

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

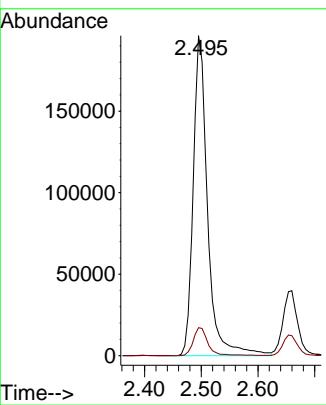


#18
Methyl Acetate
Concen: 94.899 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 43 Resp: 175784
Ion Ratio Lower Upper
43 100
74 22.7 17.4 26.2

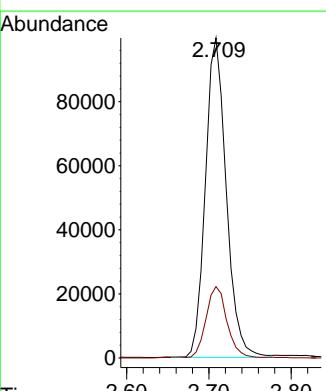



#19
Methyl tert-butyl Ether
Concen: 103.661 ug/l
RT: 3.117 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion: 73 Resp: 43141
Ion Ratio Lower Upper
73 100
57 23.0 18.5 27.7

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

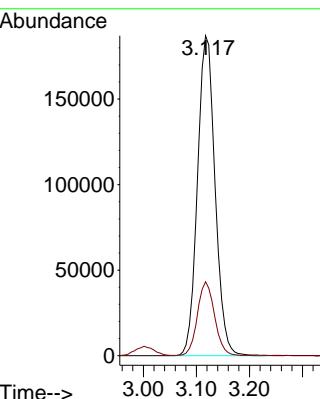


#20
Methylene Chloride
Concen: 96.381 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 84 Resp: 140388
Ion Ratio Lower Upper
84 100
49 131.2 106.5 159.7
51 41.2 32.1 48.1
86 64.4 50.0 75.0

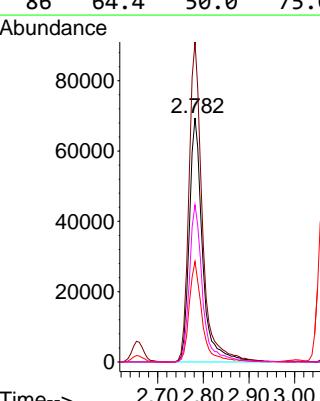






#21
trans-1,2-Dichloroethene
Concen: 100.164 ug/l
RT: 3.080 min Scan# 31
Delta R.T. -0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 96 Resp: 128233
Ion Ratio Lower Upper
96 100
61 147.3 117.0 175.4
98 63.0 53.4 80.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

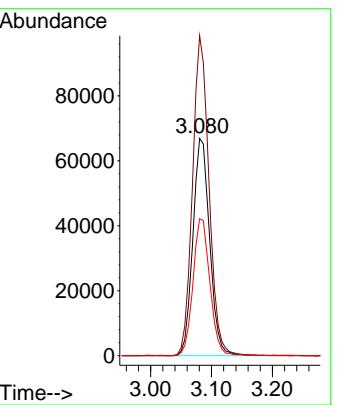


#22
Diisopropyl ether
Concen: 104.489 ug/l
RT: 3.763 min Scan# 439
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 45 Resp: 467534
Ion Ratio Lower Upper
45 100
43 70.4 54.9 82.3
87 26.0 21.0 31.4
59 11.7 8.7 13.1

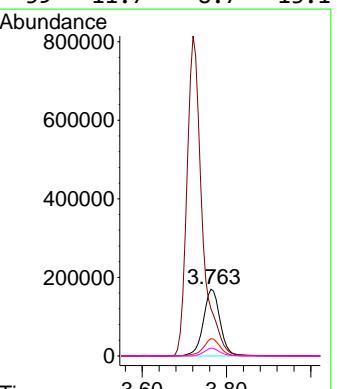



#23
Vinyl Acetate
Concen: 554.219 ug/l
RT: 3.721 min Scan# 413
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument: MSVOA_X
ClientSampleId: VSTDICC100

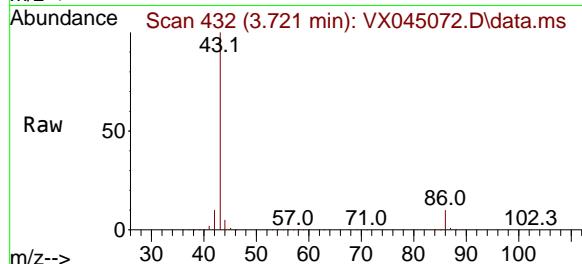


Tgt Ion: 43 Resp: 2035880
Ion Ratio Lower Upper
43 100
86 9.9 8.1 12.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#24
1,1-Dichloroethane
Concen: 102.805 ug/l
RT: 3.605 min Scan# 413
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 63 Resp: 257023
Ion Ratio Lower Upper
63 100
98 6.8 3.4 10.2
100 4.6 2.1 6.5



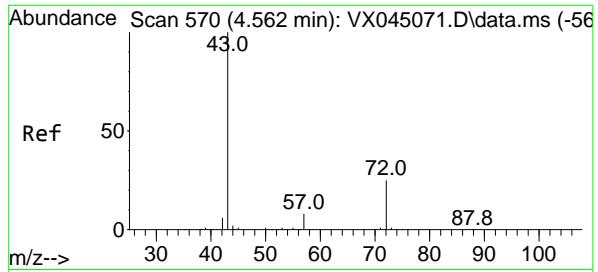

#25
2-Butanone
Concen: 563.952 ug/l
RT: 4.562 min Scan# 51
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

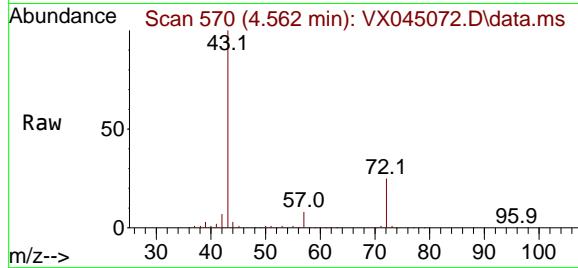

Tgt Ion: 43 Resp: 55918:
Ion Ratio Lower Upper
43 100
72 24.6 20.0 30.0



Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

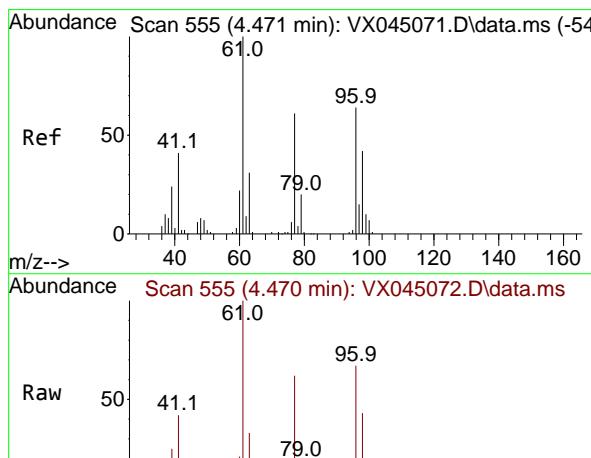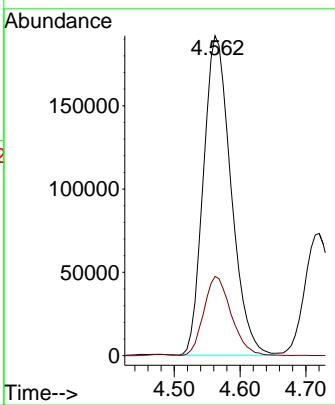


#26
2,2-Dichloropropane
Concen: 67.148 ug/l
RT: 4.470 min Scan# 555
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

Tgt Ion: 77 Resp: 124805
Ion Ratio Lower Upper
77 100
97 24.6 12.4 37.0

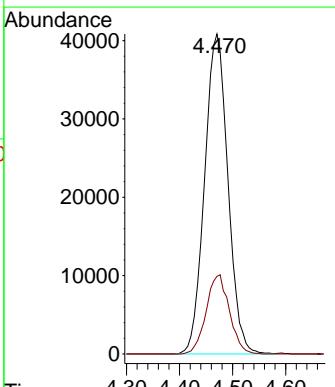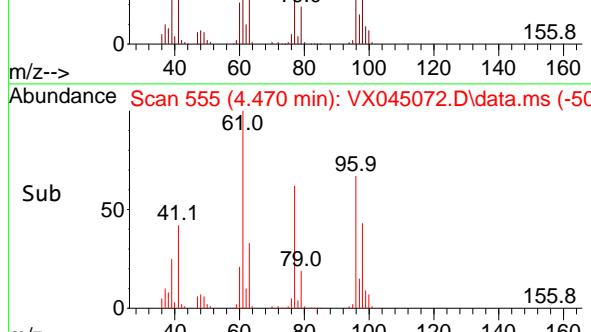

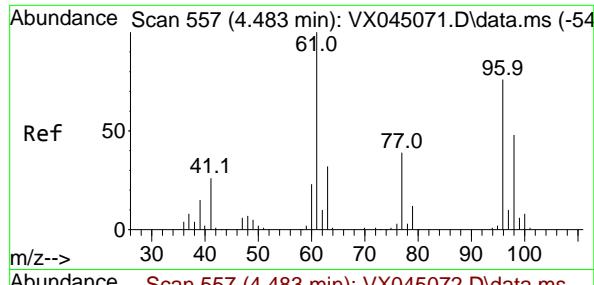

#27
cis-1,2-Dichloroethene
 Concen: 100.568 ug/l
 RT: 4.483 min Scan# 5
 Delta R.T. -0.000 min
 Lab File: VX045072.D
 Acq: 28 Feb 2025 03:23


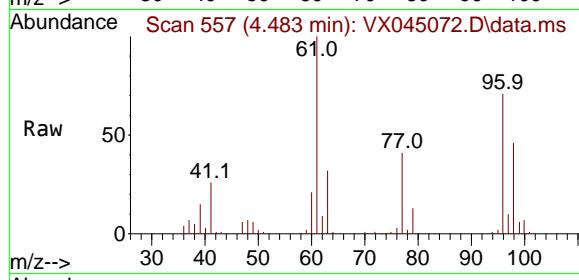


Tgt Ion: 96 Resp: 155195


Ion	Ratio	Lower	Upper
96	100		
61	143.8	0.0	283.2
98	64.3	0.0	128.0

Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025






#28
 Bromochloromethane
 Concen: 94.428 ug/l
 RT: 4.897 min Scan# 625
 Delta R.T. -0.000 min
 Lab File: VX045072.D
 Acq: 28 Feb 2025 03:23

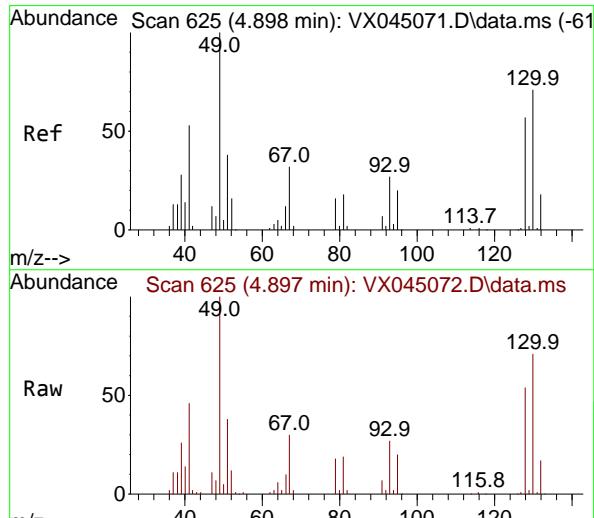

Tgt Ion: 49 Resp: 113848


Ion	Ratio	Lower	Upper
49	100		
129	1.8	0.0	3.4
130	72.2	56.1	84.1

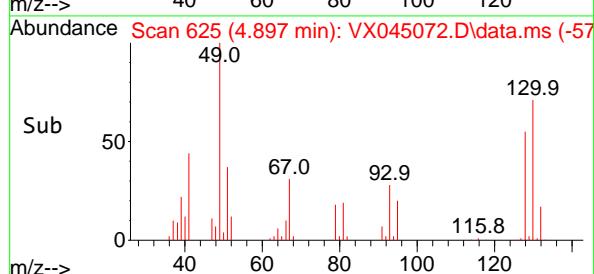



#29
Tetrahydrofuran
Concen: 556.465 ug/l
RT: 5.007 min Scan# 6
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument : MSVOA_X
ClientSampleId : VSTDICC100

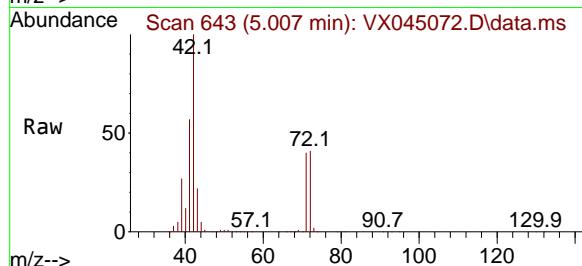


Tgt Ion: 42 Resp: 36556
Ion Ratio Lower Upper
42 100
72 42.1 34.1 51.1
71 39.2 31.4 47.0

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

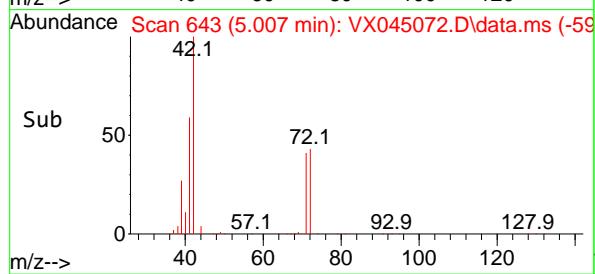


#30
Chloroform
Concen: 101.814 ug/l
RT: 5.092 min Scan# 657
Delta R.T. 0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 83 Resp: 248978
Ion Ratio Lower Upper
83 100
85 66.9 51.4 77.2







#31
Cyclohexane
Concen: 100.711 ug/l
RT: 5.464 min Scan# 718
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23
Instrument: MSVOA_X
ClientSampleId: VSTDICC100




Tgt Ion: 56 Resp: 231082
Ion Ratio Lower Upper
56 100
69 29.1 23.4 35.2
84 83.3 69.4 104.2

Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

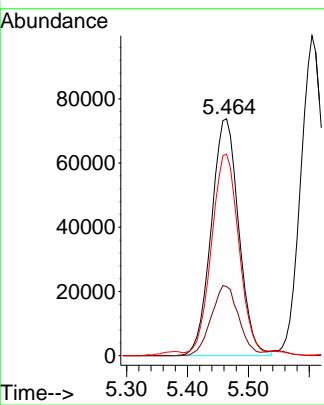


#32
1,1,1-Trichloroethane
Concen: 102.638 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 97 Resp: 211302
Ion Ratio Lower Upper
97 100
99 64.7 51.6 77.4
61 47.3 38.4 57.6

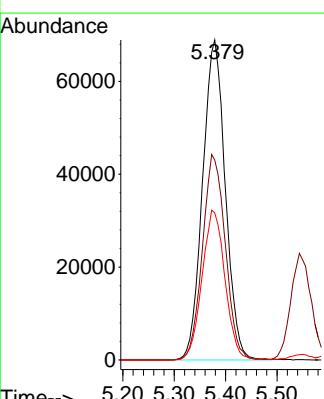



#33
1,2-Dichloroethane-d4
Concen: 106.011 ug/l
RT: 5.952 min Scan# 7
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100




Tgt Ion: 65 Resp: 15845:
Ion Ratio Lower Upper
65 100
67 52.5 0.0 106.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

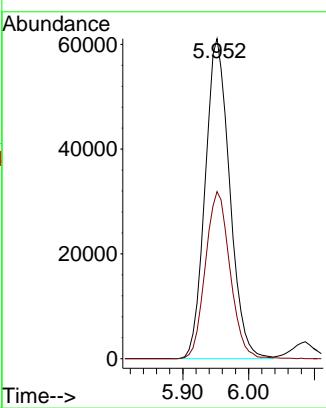


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion:114 Resp: 181031
Ion Ratio Lower Upper
114 100
63 22.5 0.0 41.8
88 15.1 0.0 32.8

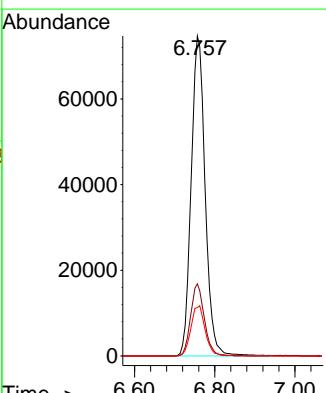






#35
Dibromofluoromethane
Concen: 104.110 ug/l
RT: 5.385 min Scan# 7
Instrument : MSVOA_X
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

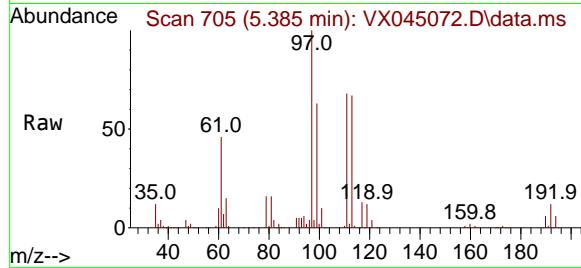


Tgt Ion:113 Resp: 123189
Ion Ratio Lower Upper
113 100
111 102.1 81.8 122.6
192 17.5 14.3 21.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#36
1,1-Dichloropropene
Concen: 101.258 ug/l
RT: 5.690 min Scan# 755
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 75 Resp: 172295
Ion Ratio Lower Upper
75 100
110 34.4 16.9 50.6
77 31.0 24.5 36.7



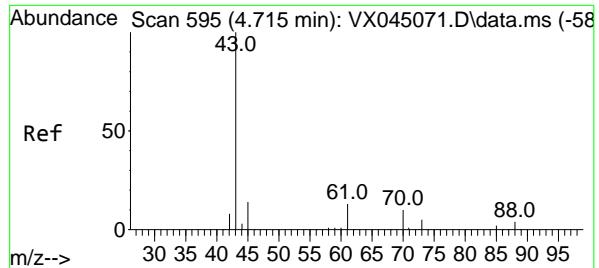

#37
Ethyl Acetate
 Concen: 113.796 ug/l
 RT: 4.720 min Scan# 51
 Delta R.T. 0.006 min
 Lab File: VX045072.D
 Acq: 28 Feb 2025 03:23




Instrument : MSVOA_X
 ClientSampleId : VSTDICC100




Tgt Ion: 43 Resp: 22032
 Ion Ratio Lower Upper
 43 100
 61 12.6 10.8 16.2
 70 9.6 7.7 11.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025


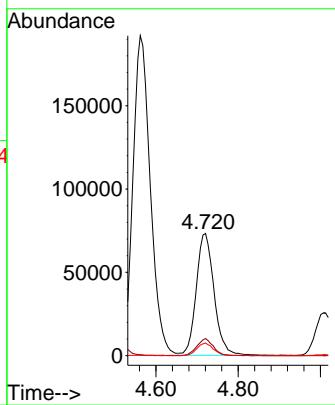
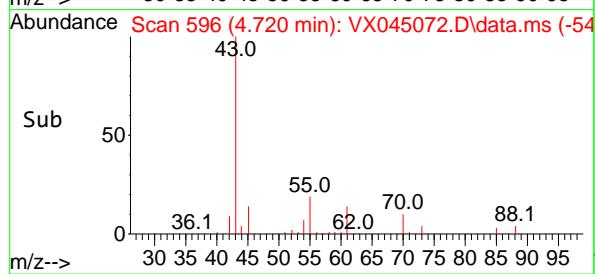


#38
Carbon Tetrachloride
 Concen: 105.940 ug/l
 RT: 5.671 min Scan# 752
 Delta R.T. -0.000 min
 Lab File: VX045072.D
 Acq: 28 Feb 2025 03:23



Tgt Ion:117 Resp: 177219
 Ion Ratio Lower Upper
 117 100
 119 93.0 76.7 115.1
 121 30.4 25.5 38.3

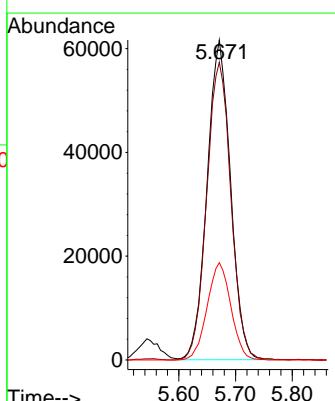

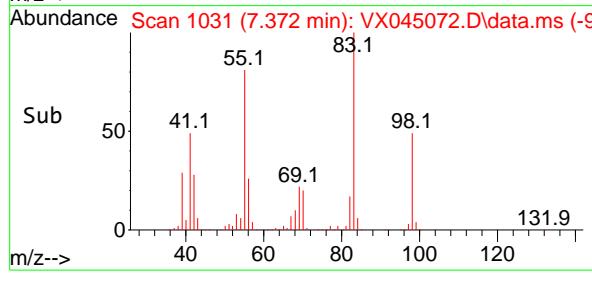

#39

Methylcyclohexane

Concen: 101.175 ug/l

RT: 7.372 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045072.D

Acq: 28 Feb 2025 03:23





Instrument:

MSVOA_X

ClientSampleId :

VSTDICC100

**Manual Integrations
APPROVED**

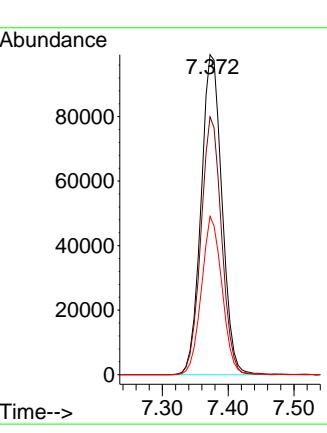 Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025


#40

Benzene


Concen: 101.908 ug/l


RT: 6.031 min Scan# 811

Delta R.T. -0.000 min


Lab File: VX045072.D

Acq: 28 Feb 2025 03:23

 Tgt Ion: 78 Resp: 541974
 Ion Ratio Lower Upper
 78 100
 77 23.4 18.8 28.2




#41
Methacrylonitrile
Concen: 116.205 ug/l
RT: 4.922 min Scan# 61
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23






Tgt Ion: 41 Resp: 120180
Ion Ratio Lower Upper

41	100
39	54.3
67	68.3
52	29.9


Lower	Upper
44.6	67.0
53.9	80.9
23.3	34.9

Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

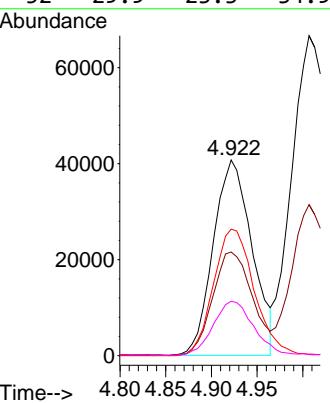



#42
1,2-Dichloroethane
Concen: 110.158 ug/l
RT: 6.086 min Scan# 820
Delta R.T. 0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 62 Resp: 189857
Ion Ratio Lower Upper

62	100
98	8.8


0.0	18.2
-----	------

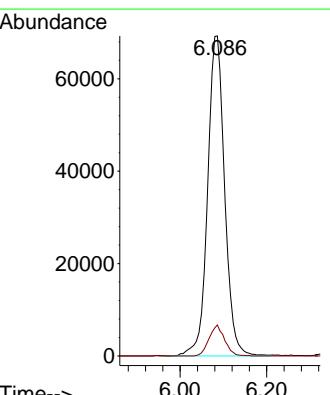



#43
Isopropyl Acetate
Concen: 109.806 ug/l
RT: 6.342 min Scan# 8
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23



Instrument : MSVOA_X
ClientSampleId : VSTDICC100

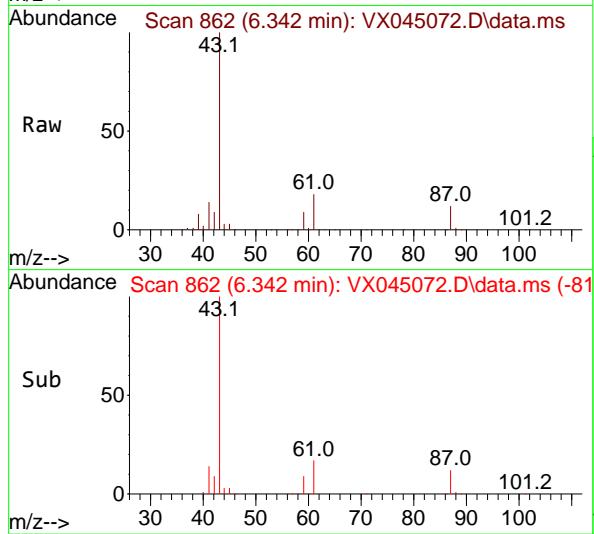

Tgt Ion: 43 Resp: 33841
Ion Ratio Lower Upper
43 100
61 18.9 14.9 22.3
87 12.3 9.4 14.2



Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

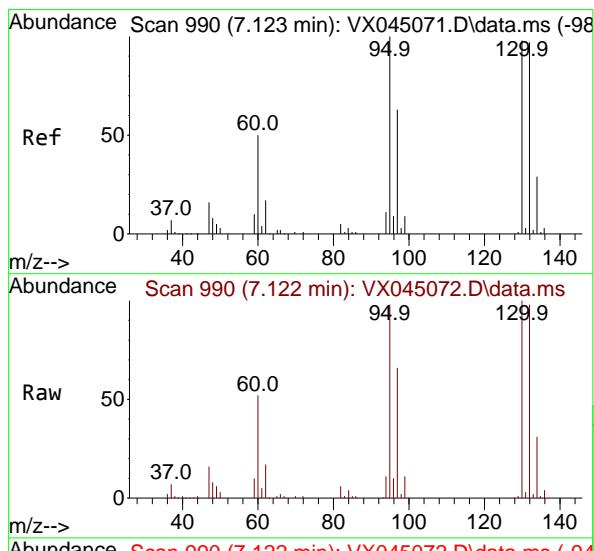

#44
Trichloroethene
Concen: 105.402 ug/l
RT: 7.122 min Scan# 990
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23


Tgt Ion:130 Resp: 128124
Ion Ratio Lower Upper
130 100
95 98.1 0.0 205.0

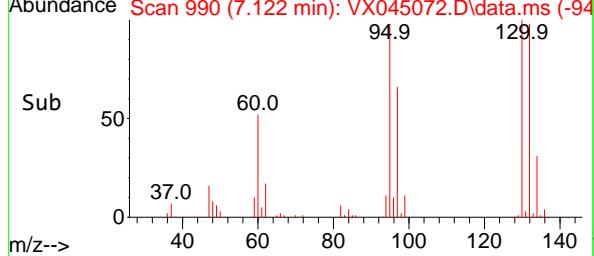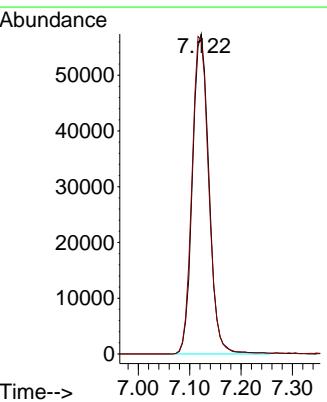



#45
1,2-Dichloropropane
Concen: 102.898 ug/l
RT: 7.427 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100



Tgt Ion: 63 Resp: 135991
Ion Ratio Lower Upper
63 100
65 30.7 24.7 37.1




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#46
Dibromomethane
Concen: 105.329 ug/l
RT: 7.580 min Scan# 1065
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23


Tgt Ion: 93 Resp: 97248
Ion Ratio Lower Upper
93 100
95 83.3 65.8 98.8
174 89.0 72.2 108.2

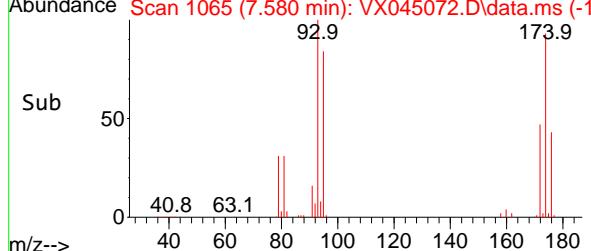



#47
 Bromodichloromethane
 Concen: 106.947 ug/l
 RT: 7.817 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX045072.D
 Acq: 28 Feb 2025 03:23




Instrument : MSVOA_X
 ClientSampleId : VSTDICC100



Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
83	100			
85	66.4	191010	51.1	76.7
127	7.9		6.4	9.6




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

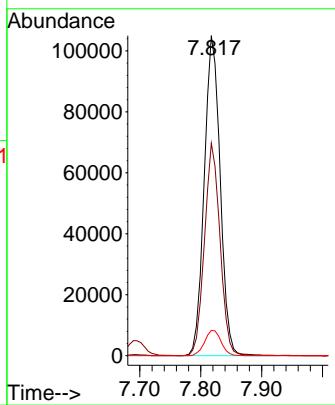

#48
 Methyl methacrylate
 Concen: 113.344 ug/l
 RT: 7.695 min Scan# 1084
 Delta R.T. 0.006 min
 Lab File: VX045072.D
 Acq: 28 Feb 2025 03:23


Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
41	100			
69	78.5	165825	63.0	94.6
39	60.9		47.5	71.3

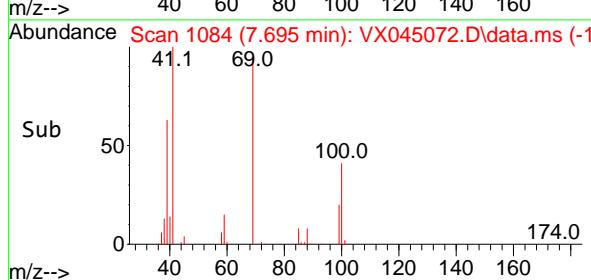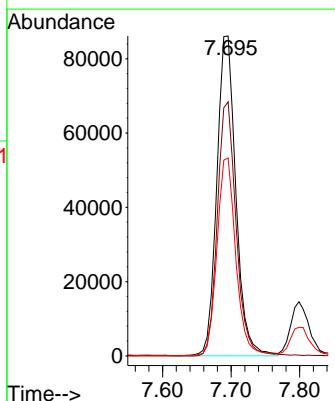



#49
1,4-Dioxane
Concen: 2132.314 ug/l
RT: 7.665 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion: 88 Resp: 66308
Ion Ratio Lower Upper
88 100
43 35.6 28.7 43.1
58 70.5 55.8 83.8

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#50
Toluene-d8
Concen: 99.595 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 98 Resp: 441188
Ion Ratio Lower Upper
98 100
100 65.3 52.0 78.0





#51
4-Methyl-2-Pentanone
Concen: 555.050 ug/l
RT: 8.573 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion: 43 Resp: 1048140
Ion Ratio Lower Upper
43 100
58 37.4 29.2 43.8

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

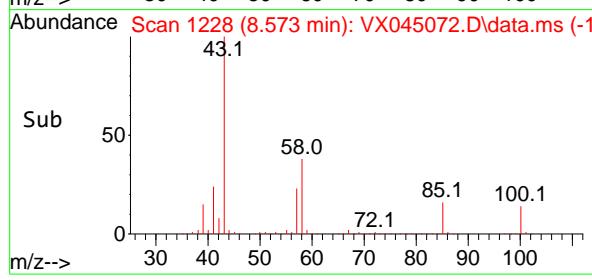


#52
Toluene
Concen: 100.178 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 92 Resp: 316349
Ion Ratio Lower Upper
92 100
91 173.2 138.9 208.3

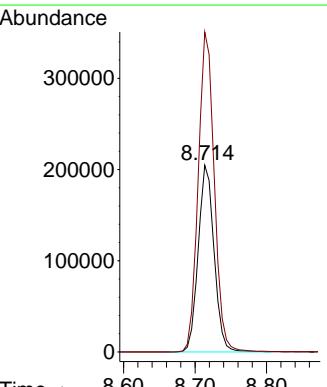



#53
t-1,3-Dichloropropene
Concen: 100.462 ug/l
RT: 8.976 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

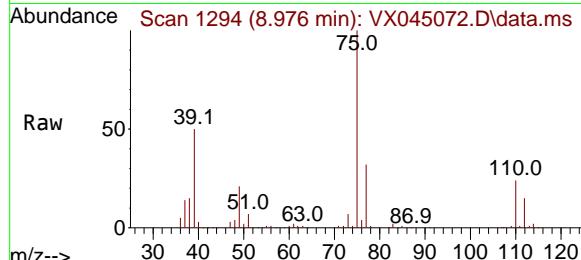


Tgt Ion: 75 Resp: 17735
Ion Ratio Lower Upper
75 100
77 31.6 26.5 39.7

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

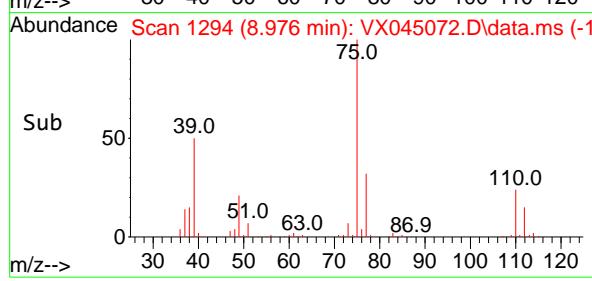


#54
cis-1,3-Dichloropropene
Concen: 101.815 ug/l
RT: 8.366 min Scan# 1194
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 75 Resp: 200943
Ion Ratio Lower Upper
75 100
77 32.2 24.7 37.1
39 51.6 40.7 61.1

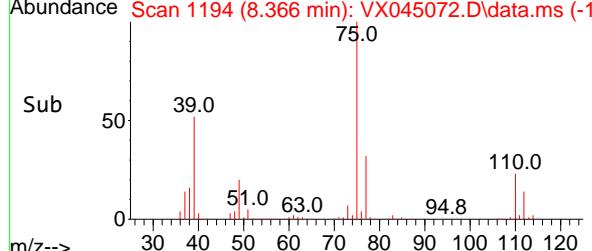



#55
1,1,2-Trichloroethane
Concen: 100.920 ug/l
RT: 9.146 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23



Instrument : MSVOA_X
ClientSampleId : VSTDICC100

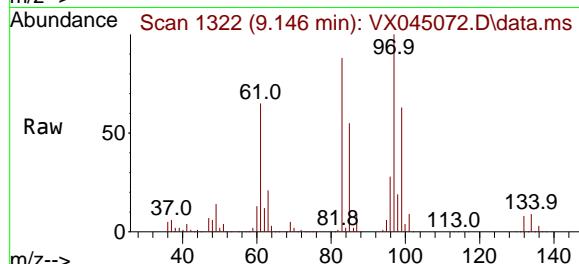

Tgt Ion: 97 Resp: 123420
Ion Ratio Lower Upper
97 100
83 88.0 69.4 104.2
85 55.1 44.1 66.1
99 63.0 50.7 76.1





Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#56
Ethyl methacrylate
Concen: 106.744 ug/l
RT: 9.116 min Scan# 1317
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23


Tgt Ion: 69 Resp: 208782
Ion Ratio Lower Upper
69 100
41 71.3 57.0 85.4
39 43.0 34.2 51.4

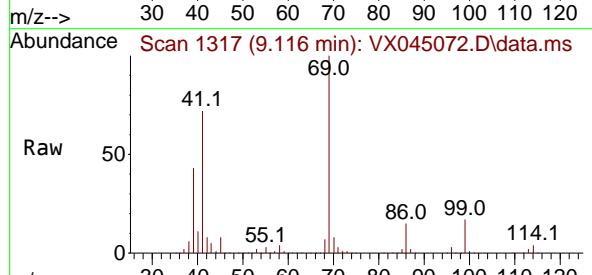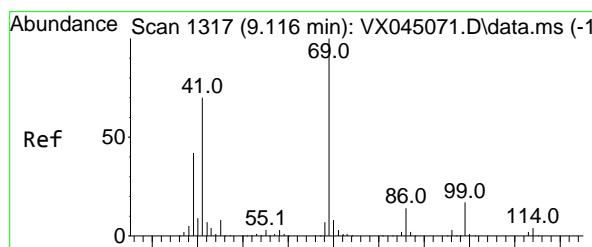



#57
1,3-Dichloropropane
Concen: 101.387 ug/l
RT: 9.305 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument : MSVOA_X
ClientSampleId : VSTDICC100

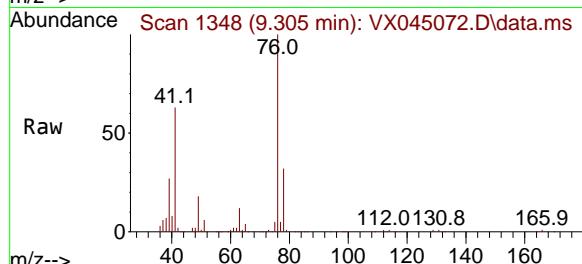

Tgt Ion: 76 Resp: 21626
Ion Ratio Lower Upper
76 100
78 31.8 25.5 38.3



Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#58
2-Chloroethyl Vinyl ether
Concen: 514.987 ug/l
RT: 8.238 min Scan# 1173
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23


Tgt Ion: 63 Resp: 494551
Ion Ratio Lower Upper
63 100
106 26.1 21.5 32.3





#59
2-Hexanone
Concen: 572.233 ug/l
RT: 9.433 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion: 43 Resp: 77949
Ion Ratio Lower Upper
43 100
58 52.2 25.9 77.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#60
Dibromochloromethane
Concen: 106.719 ug/l
RT: 9.518 min Scan# 1383
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion:129 Resp: 139245
Ion Ratio Lower Upper
129 100
127 76.3 38.5 115.5

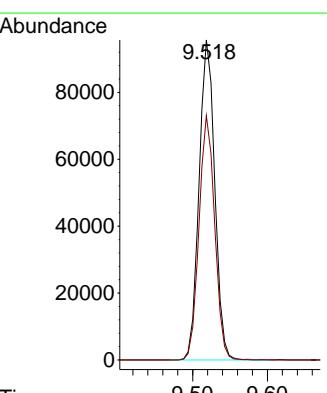



#61
1,2-Dibromoethane
Concen: 104.259 ug/l
RT: 9.610 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument : MSVOA_X
ClientSampleId : VSTDICC100

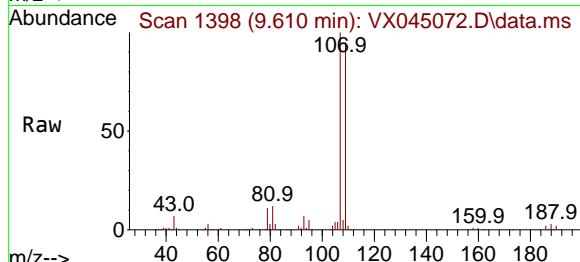

Tgt Ion:107 Resp: 12861
Ion Ratio Lower Upper
107 100
109 94.3 76.1 114.1



Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

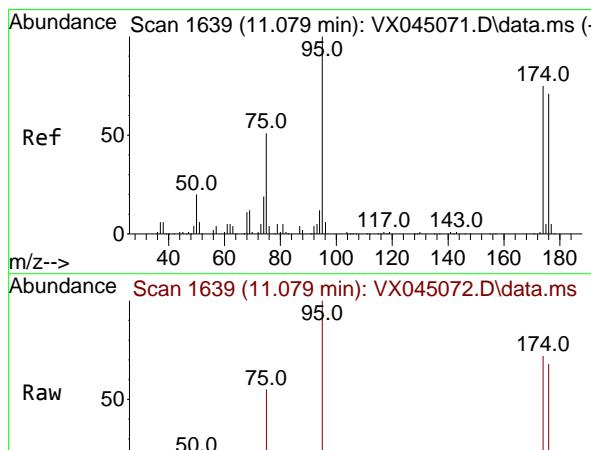

#62
4-Bromofluorobenzene
Concen: 100.365 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

Tgt Ion: 95 Resp: 148476
Ion Ratio Lower Upper
95 100
174 73.0 0.0 148.2
176 69.2 0.0 141.4

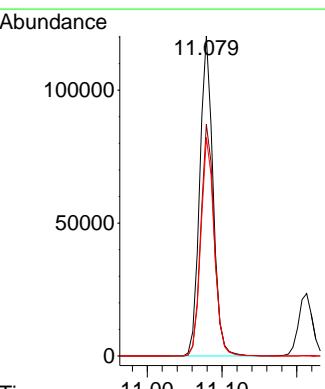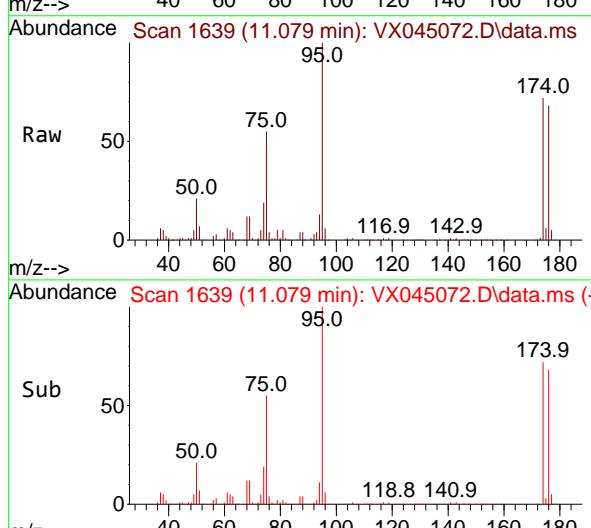


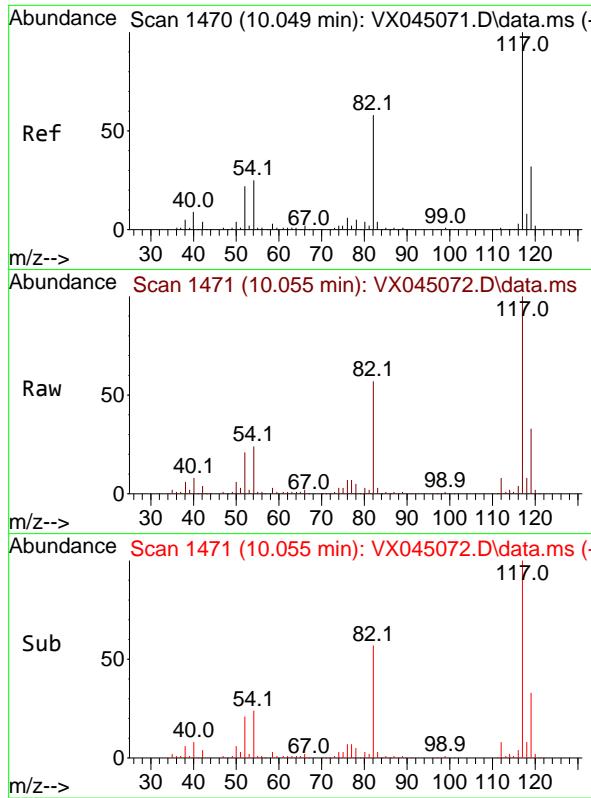


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

Instrument : MSVOA_X
ClientSampleId : VSTDICC100


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

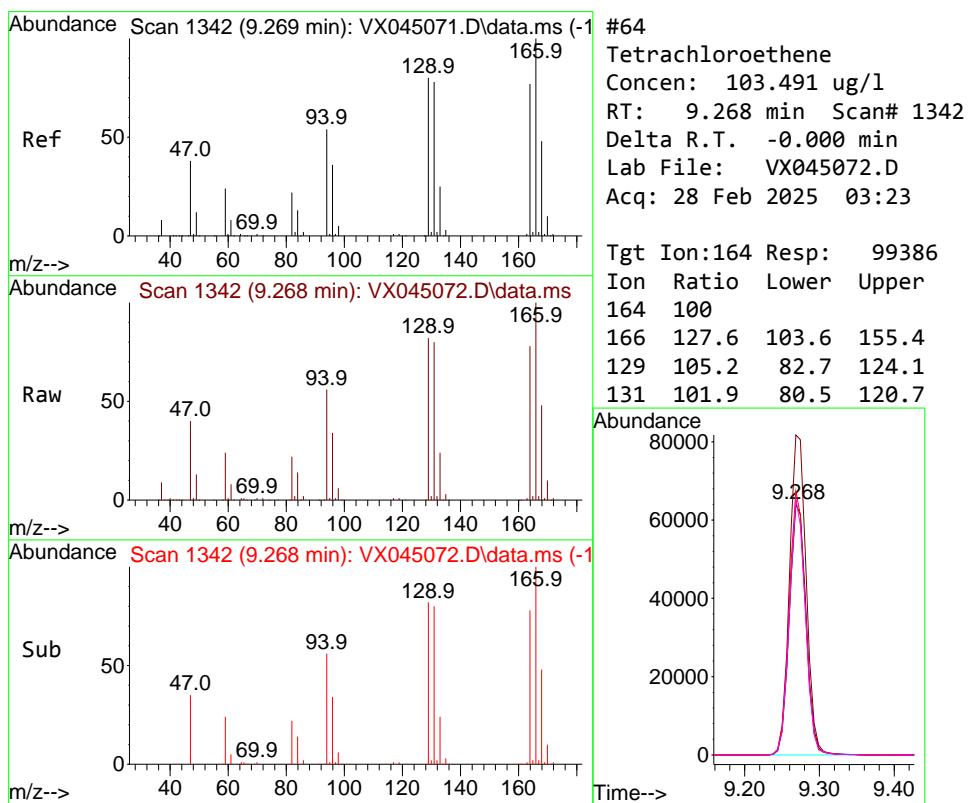

#64
Tetrachloroethene
Concen: 103.491 ug/l
RT: 9.268 min Scan# 1342
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

Tgt Ion:164 Resp: 99386
Ion Ratio Lower Upper
164 100
166 127.6 103.6 155.4
129 105.2 82.7 124.1
131 101.9 80.5 120.7

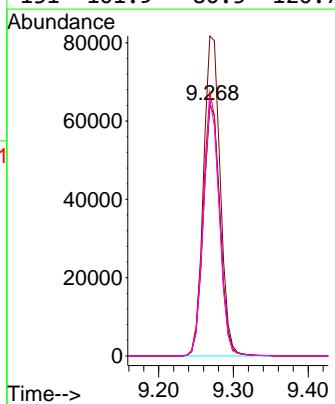


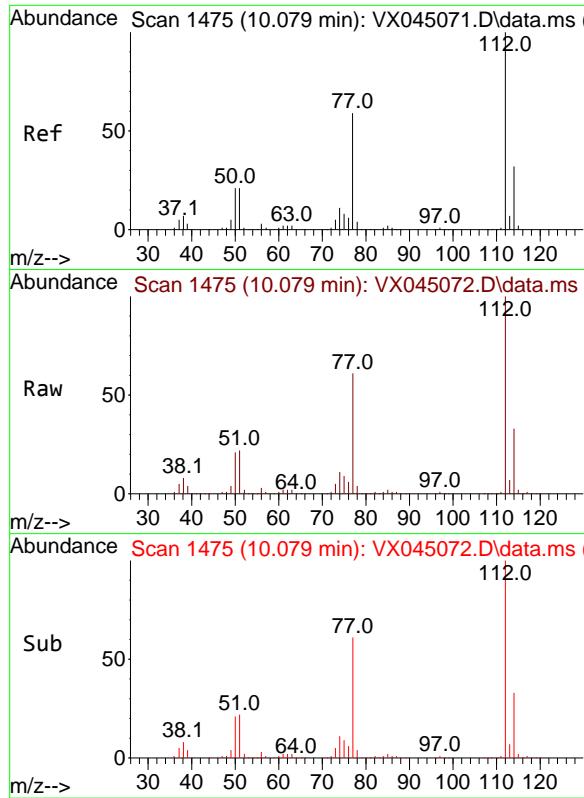


#65
Chlorobenzene
Concen: 102.456 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

Instrument : MSVOA_X
ClientSampleId : VSTDICC100


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

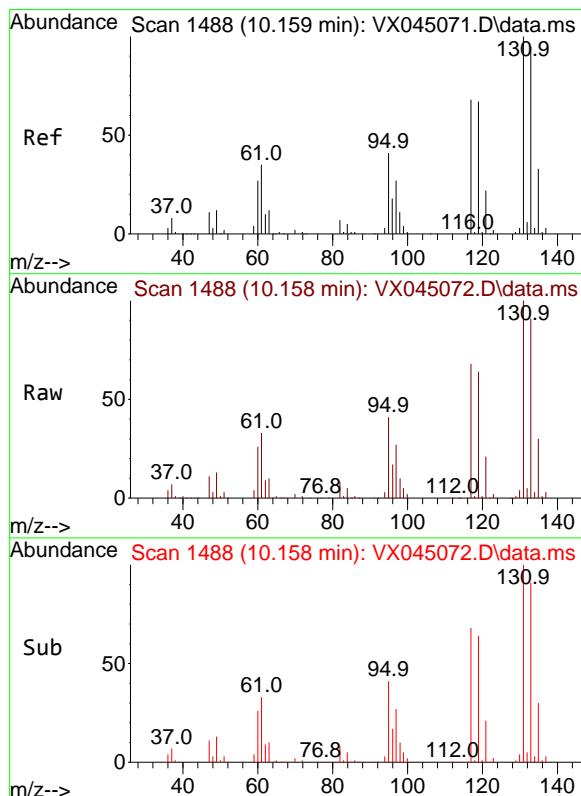

#66
1,1,1,2-Tetrachloroethane
Concen: 107.511 ug/l
RT: 10.158 min Scan# 1488
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23


Tgt Ion:131 Resp: 112451
Ion Ratio Lower Upper
131 100
133 93.1 48.6 145.9
119 65.8 33.9 101.7



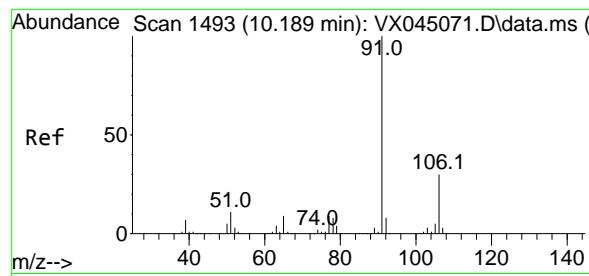

#67
Ethyl Benzene
Concen: 103.905 ug/l
RT: 10.189 min Scan# 1493
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23



Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion: 91 Resp: 596251
Ion Ratio Lower Upper
91 100
106 30.1 23.9 35.9

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

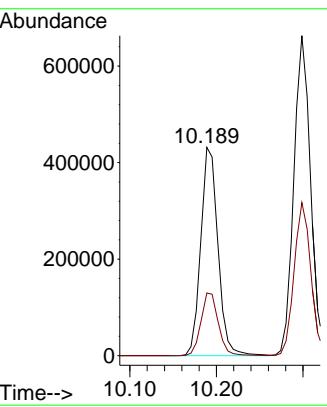


#68
m/p-Xylenes
Concen: 204.507 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23



Tgt Ion:106 Resp: 432214
Ion Ratio Lower Upper
106 100
91 208.9 165.4 248.0




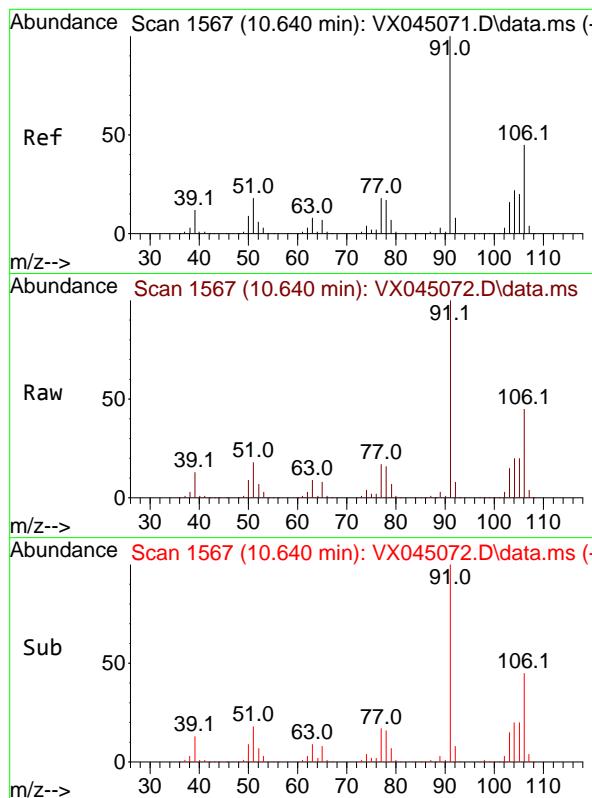


#69
o-Xylene
Concen: 100.849 ug/l
RT: 10.640 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

Instrument : MSVOA_X
ClientSampleId : VSTDICC100


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

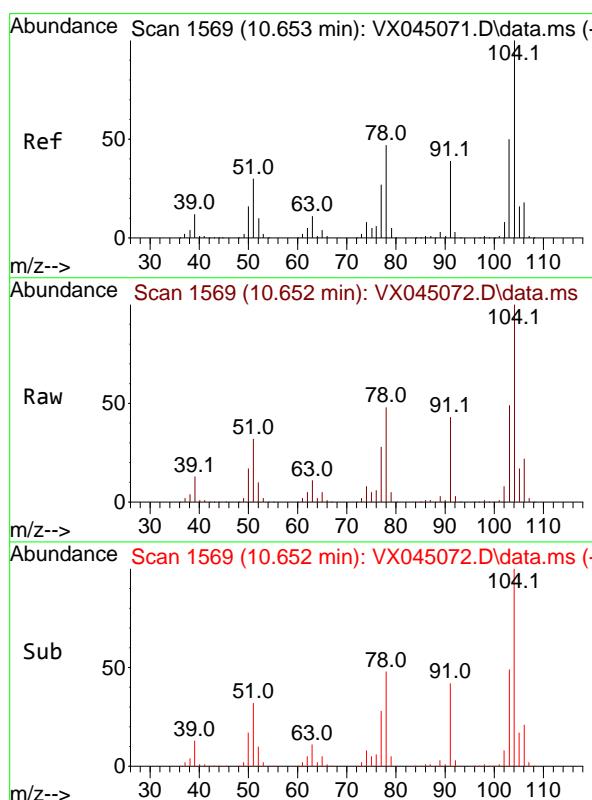

#70
Styrene
Concen: 104.948 ug/l
RT: 10.652 min Scan# 1569
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23


Tgt Ion:104 Resp: 357649
Ion Ratio Lower Upper
104 100
78 53.7 42.2 63.4
103 54.3 43.8 65.8





#71
Bromoform
Concen: 116.751 ug/l
RT: 10.799 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100



Tgt Ion:173 Resp: 90800
Ion Ratio Lower Upper
173 100
175 48.3 24.6 73.6
254 0.0 0.0 0.0




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

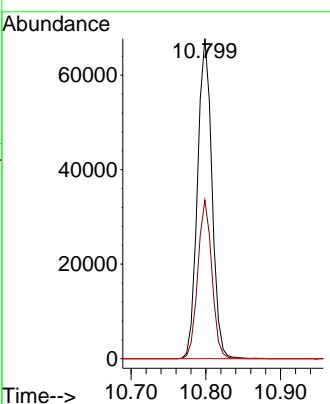


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

Tgt Ion:152 Resp: 69086
Ion Ratio Lower Upper
152 100
115 114.1 44.2 132.6
150 190.7 0.0 349.0



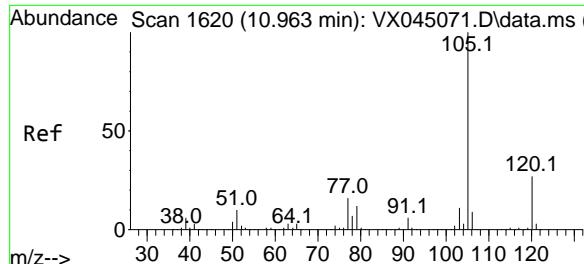




#73
Isopropylbenzene
Concen: 99.138 ug/l
RT: 10.963 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23
Instrument: MSVOA_X
ClientSampleId: VSTDICC100




Tgt Ion:105 Resp: 55353
Ion Ratio Lower Upper
105 100
120 26.0 13.2 39.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

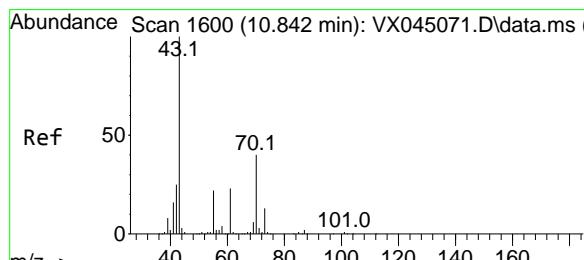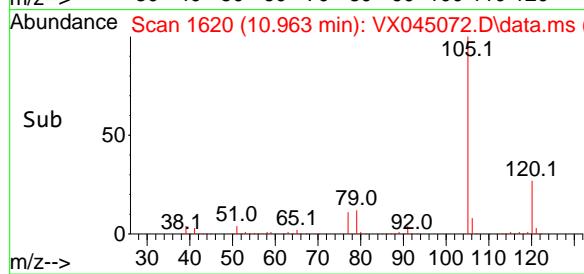


#74
N-amyl acetate
Concen: 113.277 ug/l
RT: 10.841 min Scan# 1600
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 43 Resp: 287104
Ion Ratio Lower Upper
43 100
70 39.6 31.8 47.6
55 22.3 18.3 27.5
61 23.0 18.3 27.5

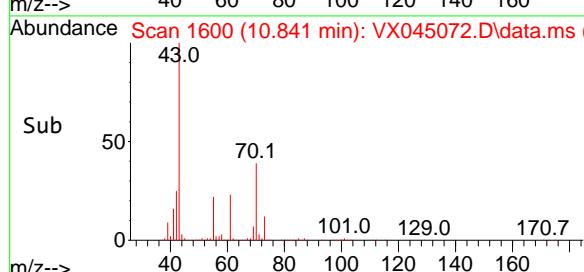

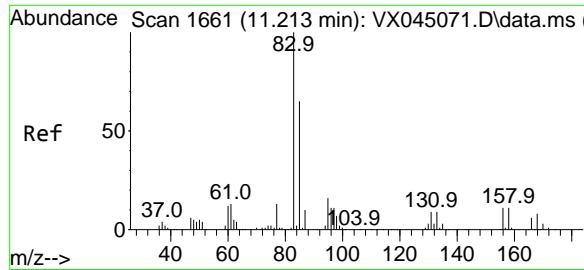

#75
1,1,2,2-Tetrachloroethane
Concen: 99.923 ug/l
RT: 11.213 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

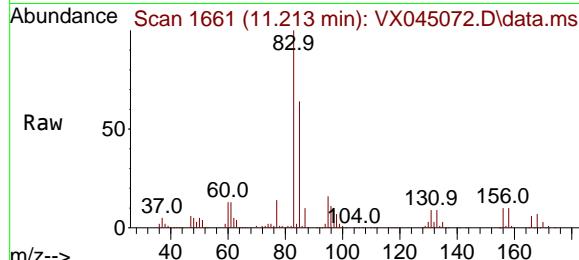


Tgt Ion: 83 Resp: 19221
Ion Ratio Lower Upper
83 100
131 9.4 4.5 13.4
85 64.7 31.7 95.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

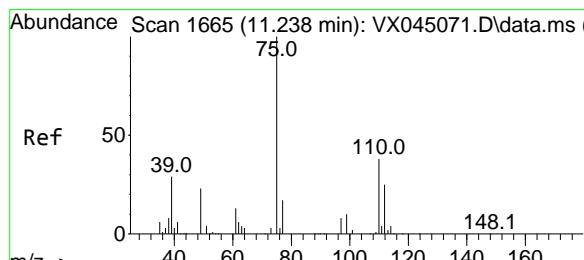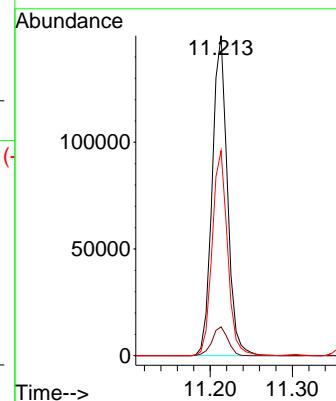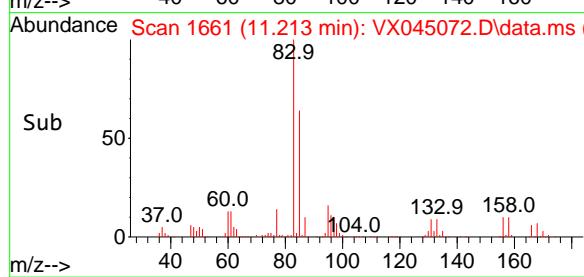


#76
1,2,3-Trichloropropane
Concen: 101.395 ug/l
RT: 11.238 min Scan# 1665
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

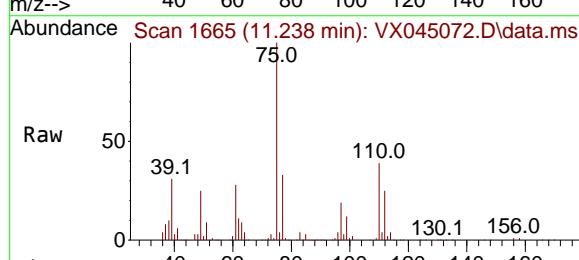


Tgt Ion: 75 Resp: 156259
Ion Ratio Lower Upper
75 100
77 42.7 20.7 62.1

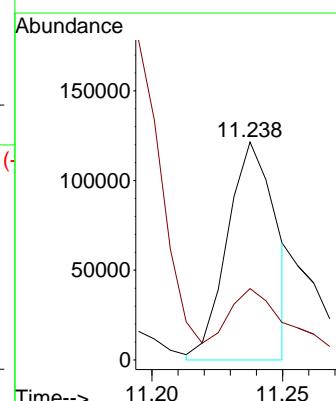



#77
Bromobenzene
Concen: 99.175 ug/l
RT: 11.195 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23



Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion:156 Resp: 125700
Ion Ratio Lower Upper
156 100
77 177.3 85.8 257.4
158 95.9 48.4 145.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#78
n-propylbenzene
Concen: 100.758 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 91 Resp: 648835
Ion Ratio Lower Upper
91 100
120 21.8 11.2 33.6





#79
2-Chlorotoluene
Concen: 96.825 ug/l
RT: 11.359 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion: 91 Resp: 38270
Ion Ratio Lower Upper
91 100
126 32.7 16.4 49.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

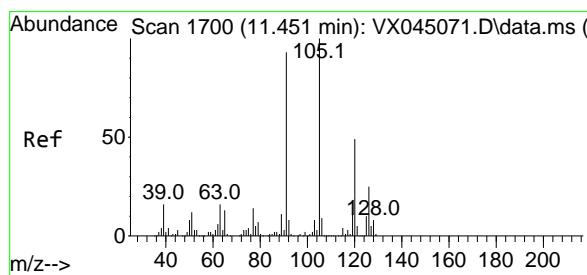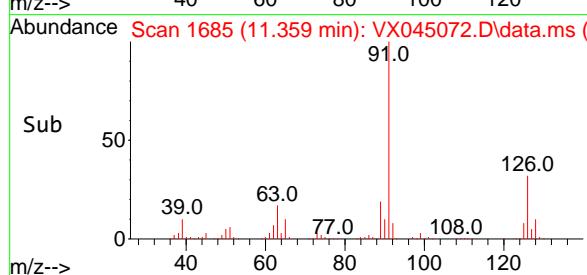


#80
1,3,5-Trimethylbenzene
Concen: 98.356 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23



Tgt Ion:105 Resp: 445466
Ion Ratio Lower Upper
105 100
120 47.1 24.1 72.2




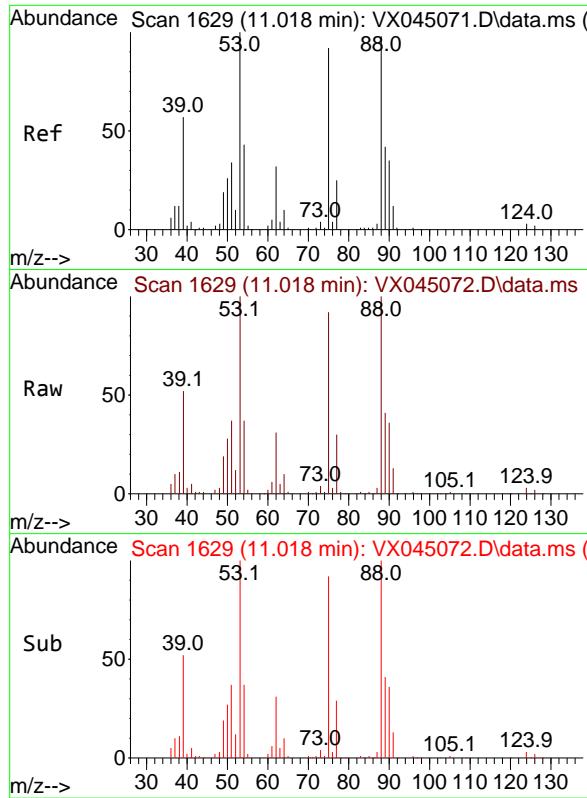


#81
trans-1,4-Dichloro-2-butene
Concen: 91.460 ug/l
RT: 11.018 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100


Manual Integrations
APPROVED




Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

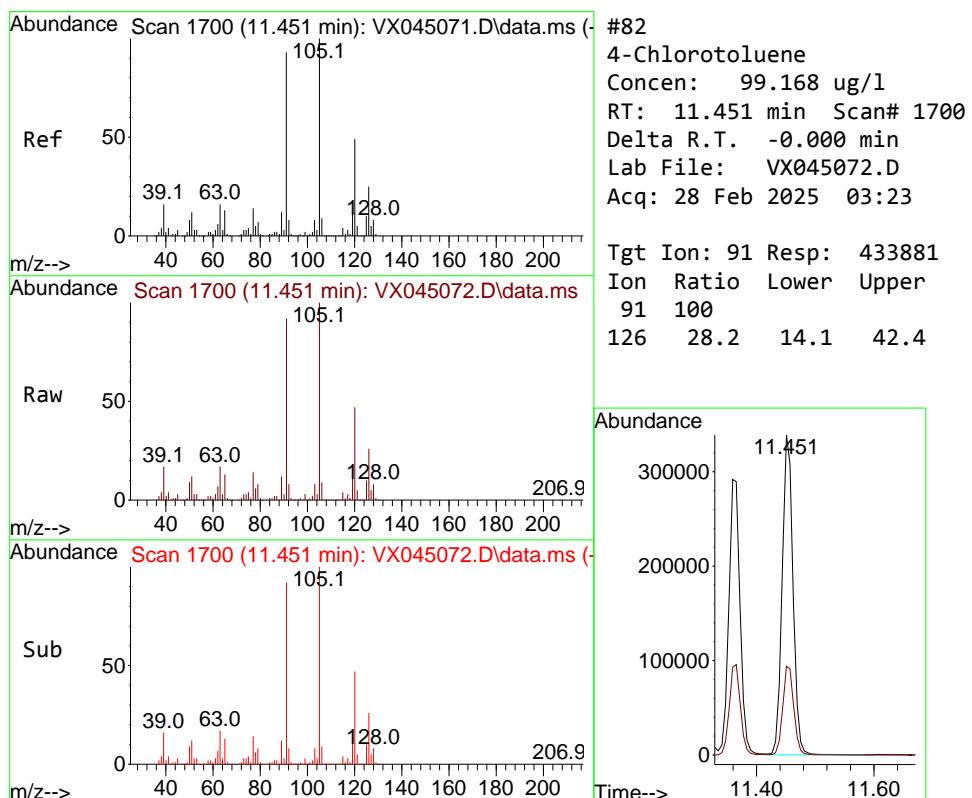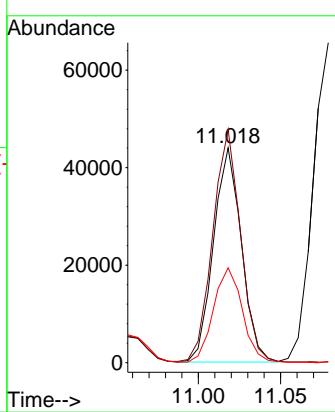

#82
4-Chlorotoluene
Concen: 99.168 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

Tgt Ion: 91 Resp: 433881
Ion Ratio Lower Upper
91 100
126 28.2 14.1 42.4

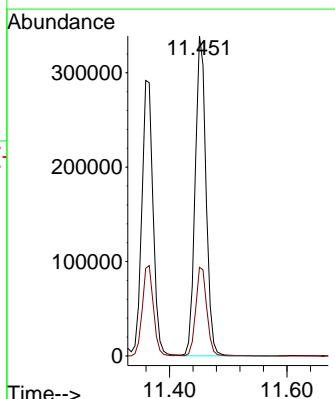



#83

tert-Butylbenzene

Concen: 99.288 ug/l

RT: 11.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045072.D

Acq: 28 Feb 2025 03:23




Instrument:

MSVOA_X

ClientSampleId :

VSTDICC100

**Manual Integrations
APPROVED**

 Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025


#84

1,2,4-Trimethylbenzene


Concen: 100.926 ug/l


RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX045072.D


Acq: 28 Feb 2025 03:23

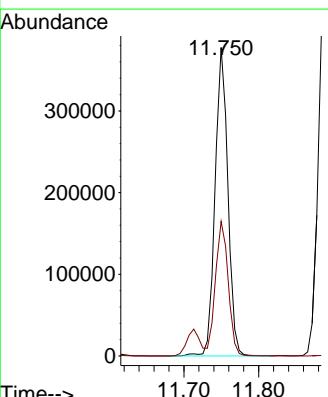 Tgt Ion:105 Resp: 450108
 Ion Ratio Lower Upper
 105 100
 120 43.4 22.1 66.1

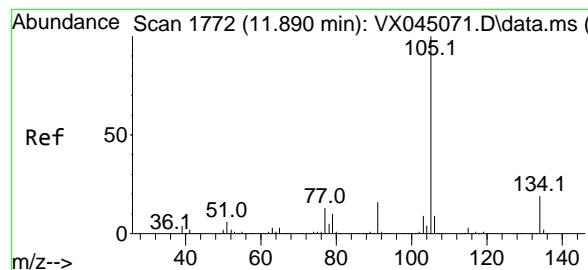


#85
sec-Butylbenzene
Concen: 100.517 ug/l
RT: 11.890 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23



Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion:105 Resp: 570000
Ion Ratio Lower Upper
105 100
134 19.6 9.8 29.4

**Manual Integrations
APPROVED**


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

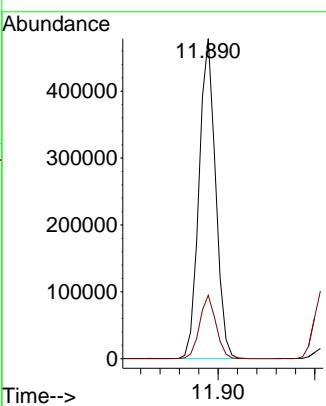


#86
p-Isopropyltoluene
Concen: 102.252 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion:119 Resp: 465512
Ion Ratio Lower Upper
119 100
134 26.0 12.9 38.6
91 25.3 12.7 38.0

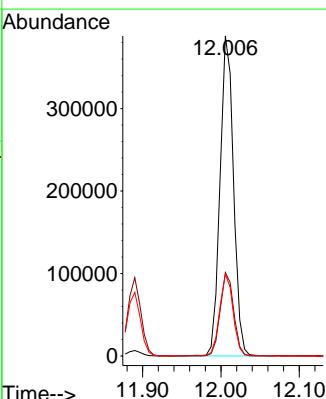



#87
1,3-Dichlorobenzene
Concen: 99.903 ug/l
RT: 11.969 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100




Tgt Ion:146 Resp: 231440
Ion Ratio Lower Upper
146 100
111 42.6 21.1 63.4
148 64.1 31.9 95.7

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#88
1,4-Dichlorobenzene
Concen: 98.355 ug/l
RT: 12.042 min Scan# 1797
Delta R.T. 0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion:146 Resp: 230663
Ion Ratio Lower Upper
146 100
111 41.5 20.2 60.5
148 63.9 31.9 95.9

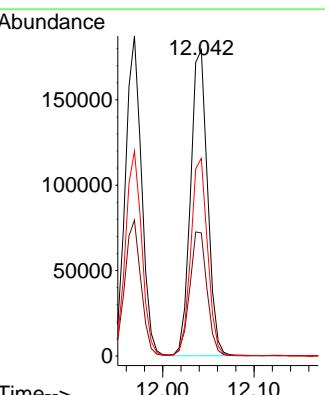



#89
n-Butylbenzene
Concen: 107.000 ug/l
RT: 12.329 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23



Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion: 91 Resp: 428209
Ion Ratio Lower Upper
91 100
92 54.4 26.7 80.0
134 24.2 12.2 36.6

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#90
Hexachloroethane
Concen: 102.980 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion:117 Resp: 87448
Ion Ratio Lower Upper
117 100
201 63.4 31.9 95.9








#91
1,2-Dichlorobenzene
Concen: 102.254 ug/l
RT: 12.335 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23
Instrument : MSVOA_X
ClientSampleId : VSTDICC100




Tgt Ion:146 Resp: 233125
Ion Ratio Lower Upper
146 100
111 43.7 21.6 65.0
148 63.2 31.9 95.9

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

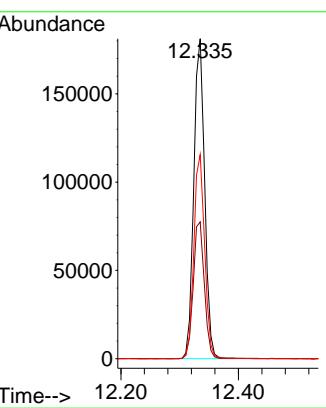


#92
1,2-Dibromo-3-Chloropropane
Concen: 116.296 ug/l
RT: 12.938 min Scan# 1944
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion: 75 Resp: 41402
Ion Ratio Lower Upper
75 100
155 80.6 39.6 118.7
157 101.8 51.1 153.4

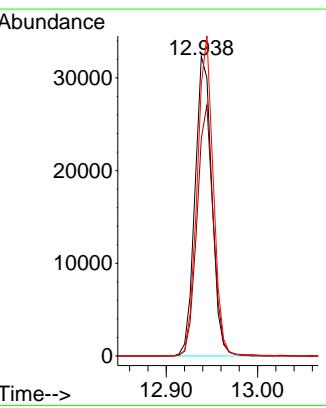






#93
1,2,4-Trichlorobenzene
Concen: 107.648 ug/l
RT: 13.585 min Scan# 2
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion:180 Resp: 148363
Ion Ratio Lower Upper
180 100
182 95.1 47.3 141.9
145 33.6 16.3 48.9

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

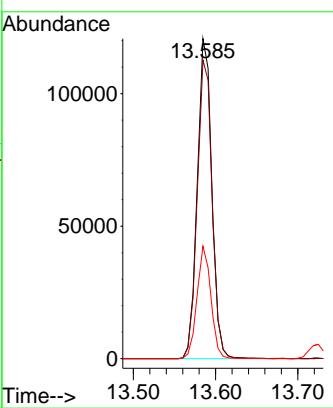


#94
Hexachlorobutadiene
Concen: 102.019 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Tgt Ion:225 Resp: 56065
Ion Ratio Lower Upper
225 100
223 64.1 31.9 95.7
227 64.4 31.4 94.0

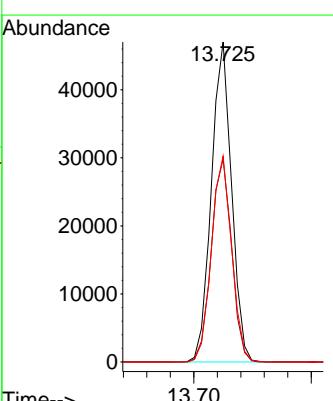

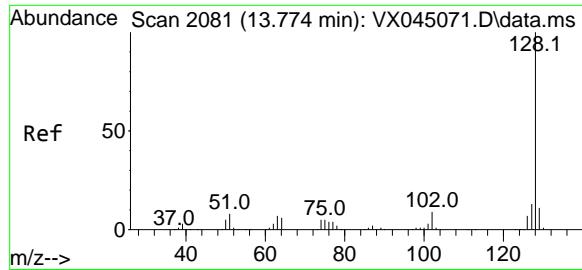

#95
Naphthalene
Concen: 112.593 ug/l
RT: 13.774 min Scan# 2111
Delta R.T. -0.000 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC100

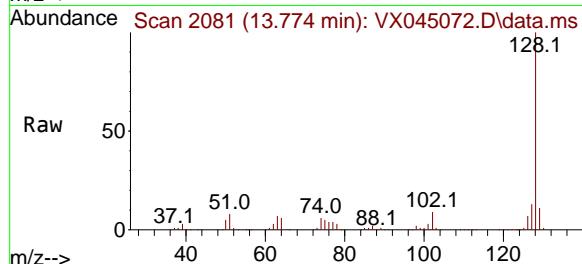


Tgt Ion:128 Resp: 565250
Ion Ratio Lower Upper
128 100
127 12.6 10.3 15.5
129 10.9 8.7 13.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

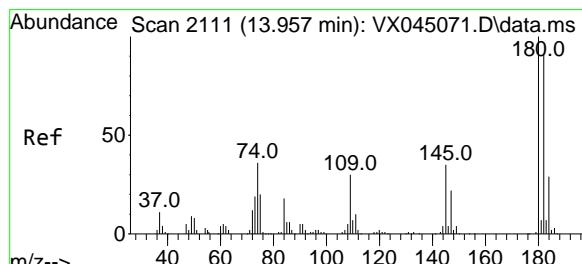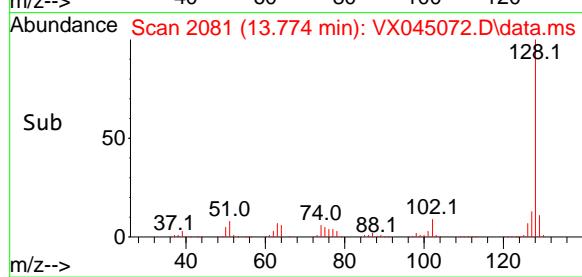

#96
1,2,3-Trichlorobenzene
Concen: 109.554 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.006 min
Lab File: VX045072.D
Acq: 28 Feb 2025 03:23

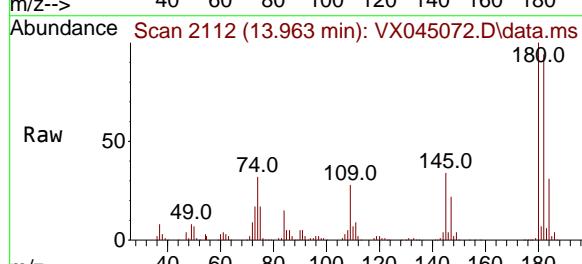

Tgt Ion:180 Resp: 152970
Ion Ratio Lower Upper
180 100
182 95.2 47.5 142.6
145 34.5 17.0 50.9

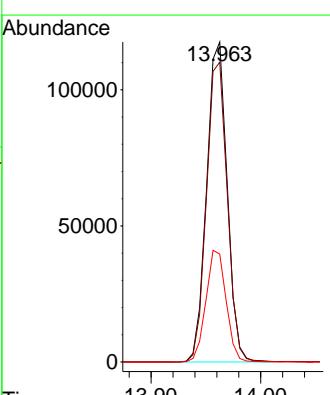

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045073.D
 Acq On : 28 Feb 2025 03:47
 Operator : JC/MD
 Sample : VSTDICC150
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150

Quant Time: Feb 28 05:36:17 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 05:28:02 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.544	168	95754	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	176991	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	150547	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	67685	50.000	ug/l	# 0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	234624	165.865	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 331.740%	#	
35) Dibromofluoromethane	5.379	113	179722	155.359	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 310.720%	#	
50) Toluene-d8	8.647	98	638979	147.538	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 295.080%	#	
62) 4-Bromofluorobenzene	11.079	95	223346	154.420	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	= 308.840%	#	
Target Compounds						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	174297	132.067	ug/l	96
3) Chloromethane	1.307	50	213704	133.072	ug/l	97
4) Vinyl Chloride	1.374	62	217672	138.774	ug/l	97
5) Bromomethane	1.593	94	83547	170.379	ug/l	98
6) Chloroethane	1.660	64	82101	137.509	ug/l	95
7) Trichlorofluoromethane	1.861	101	272235	135.494	ug/l	98
8) Diethyl Ether	2.136	74	110005	150.660	ug/l	98
9) 1,1,2-Trichlorotrifluo...	2.313	101	161825	134.877	ug/l	99
10) Methyl Iodide	2.441	142	212355	138.059	ug/l	99
11) Tert butyl alcohol	3.014	59	195415	754.176	ug/l	97
12) 1,1-Dichloroethene	2.300	96	173271	140.655	ug/l	96
13) Acrolein	2.239	56	263999	940.846	ug/l	98
14) Allyl chloride	2.654	41	308018	139.077	ug/l	98
15) Acrylonitrile	3.069	53	573208	813.990	ug/l	99
16) Acetone	2.392	43	511828	879.387	ug/l	100
17) Carbon Disulfide	2.495	76	487720	145.511	ug/l	98
18) Methyl Acetate	2.709	43	258303	147.347	ug/l	100
19) Methyl tert-butyl Ether	3.117	73	619778	157.358	ug/l	99
20) Methylene Chloride	2.782	84	202913	147.198	ug/l	99
21) trans-1,2-Dichloroethene	3.081	96	176924	146.027	ug/l	98
22) Diisopropyl ether	3.764	45	662828	156.526	ug/l	98
23) Vinyl Acetate	3.721	43	2943150	846.586	ug/l	99
24) 1,1-Dichloroethane	3.605	63	363081	153.453	ug/l	99
25) 2-Butanone	4.568	43	818497	872.239	ug/l	99
26) 2,2-Dichloropropane	4.465	77	179826	102.231	ug/l	99
27) cis-1,2-Dichloroethene	4.483	96	220826	151.205	ug/l	98
28) Bromochloromethane	4.891	49	171273	150.105	ug/l	100
29) Tetrahydrofuran	5.007	42	528574	850.174	ug/l	99
30) Chloroform	5.093	83	351934	152.067	ug/l	97
31) Cyclohexane	5.458	56	302215	139.174	ug/l	96
32) 1,1,1-Trichloroethane	5.379	97	294434	151.120	ug/l	100
36) 1,1-Dichloropropene	5.684	75	241405	145.112	ug/l	100
37) Ethyl Acetate	4.721	43	316250	167.067	ug/l	99
38) Carbon Tetrachloride	5.672	117	245917	150.363	ug/l	99
39) Methylcyclohexane	7.373	83	292216	137.544	ug/l	97
40) Benzene	6.031	78	755854	145.368	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045073.D
 Acq On : 28 Feb 2025 03:47
 Operator : JC/MD
 Sample : VSTDICC150
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150

Quant Time: Feb 28 05:36:17 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 05:28:02 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.928	41	175023	173.088	ug/l	99
42) 1,2-Dichloroethane	6.080	62	276129	163.872	ug/l	99
43) Isopropyl Acetate	6.342	43	511643	169.804	ug/l	99
44) Trichloroethene	7.123	130	178483	150.181	ug/l	97
45) 1,2-Dichloropropane	7.428	63	198135	153.334	ug/l	100
46) Dibromomethane	7.580	93	142119	157.443	ug/l	99
47) Bromodichloromethane	7.818	83	280255	160.492	ug/l	99
48) Methyl methacrylate	7.696	41	252275	176.370	ug/l	99
49) 1,4-Dioxane	7.665	88	96268	3166.423	ug/l	99
51) 4-Methyl-2-Pentanone	8.580	43	1536157	832.051	ug/l	99
52) Toluene	8.714	92	448664	145.321	ug/l	99
53) t-1,3-Dichloropropene	8.976	75	266444	154.373	ug/l	96
54) cis-1,3-Dichloropropene	8.366	75	293521	152.117	ug/l	96
55) 1,1,2-Trichloroethane	9.147	97	178217	149.046	ug/l	98
56) Ethyl methacrylate	9.116	69	310992	162.631	ug/l	98
57) 1,3-Dichloropropane	9.305	76	312196	149.699	ug/l	100
58) 2-Chloroethyl Vinyl ether	8.238	63	717328	764.019	ug/l	99
59) 2-Hexanone	9.433	43	1156653	868.492	ug/l	100
60) Dibromochloromethane	9.519	129	201906	158.276	ug/l	99
61) 1,2-Dibromoethane	9.610	107	185828	154.074	ug/l	100
64) Tetrachloroethene	9.269	164	139536	145.906	ug/l	94
65) Chlorobenzene	10.079	112	472117	146.096	ug/l	99
66) 1,1,1,2-Tetrachloroethane	10.159	131	163370	156.845	ug/l	97
67) Ethyl Benzene	10.189	91	852575	149.191	ug/l	99
68) m/p-Xylenes	10.299	106	607523	288.655	ug/l	97
69) o-Xylene	10.640	106	302495	143.259	ug/l	99
70) Styrene	10.653	104	512379	150.979	ug/l	99
71) Bromoform	10.799	173	135388	174.808	ug/l #	99
73) Isopropylbenzene	10.963	105	780706	142.719	ug/l	99
74) N-amyl acetate	10.842	43	429686	173.042	ug/l	100
75) 1,1,2,2-Tetrachloroethane	11.213	83	283558	150.458	ug/l	99
76) 1,2,3-Trichloropropane	11.238	75	229435m	151.960	ug/l	
77) Bromobenzene	11.195	156	180997	145.760	ug/l	96
78) n-propylbenzene	11.305	91	923593	146.395	ug/l	99
79) 2-Chlorotoluene	11.366	91	548695	141.695	ug/l	99
80) 1,3,5-Trimethylbenzene	11.451	105	635832	143.293	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.018	75	82267	147.761	ug/l	98
82) 4-Chlorotoluene	11.451	91	627816	146.464	ug/l	99
83) tert-Butylbenzene	11.713	119	641713	142.974	ug/l	99
84) 1,2,4-Trimethylbenzene	11.750	105	647248	148.135	ug/l	100
85) sec-Butylbenzene	11.890	105	807713	145.383	ug/l	100
86) p-Isopropyltoluene	12.006	119	664916	149.075	ug/l	100
87) 1,3-Dichlorobenzene	11.969	146	334751	147.488	ug/l	100
88) 1,4-Dichlorobenzene	12.043	146	333594	145.189	ug/l	99
89) n-Butylbenzene	12.329	91	620757	158.324	ug/l	99
90) Hexachloroethane	12.536	117	128582	154.554	ug/l	100
91) 1,2-Dichlorobenzene	12.335	146	329318	147.436	ug/l	99
92) 1,2-Dibromo-3-Chloropr...	12.939	75	64958	186.240	ug/l	98
93) 1,2,4-Trichlorobenzene	13.585	180	219313	162.416	ug/l	99
94) Hexachlorobutadiene	13.725	225	80241	149.034	ug/l	99
95) Naphthalene	13.774	128	828949	168.538	ug/l	100
96) 1,2,3-Trichlorobenzene	13.957	180	222608	162.727	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045073.D
Acq On : 28 Feb 2025 03:47
Operator : JC/MD
Sample : VSTDICC150
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150

Quant Time: Feb 28 05:36:17 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 05:28:02 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carbone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045073.D
 Acq On : 28 Feb 2025 03:47
 Operator : JC/MD
 Sample : VSTDICC150
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1


Instrument :
 MSVOA_X
ClientSampleId :
 VSTDICC150

Quant Time: Feb 28 05:36:17 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 05:28:02 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :John Carbone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

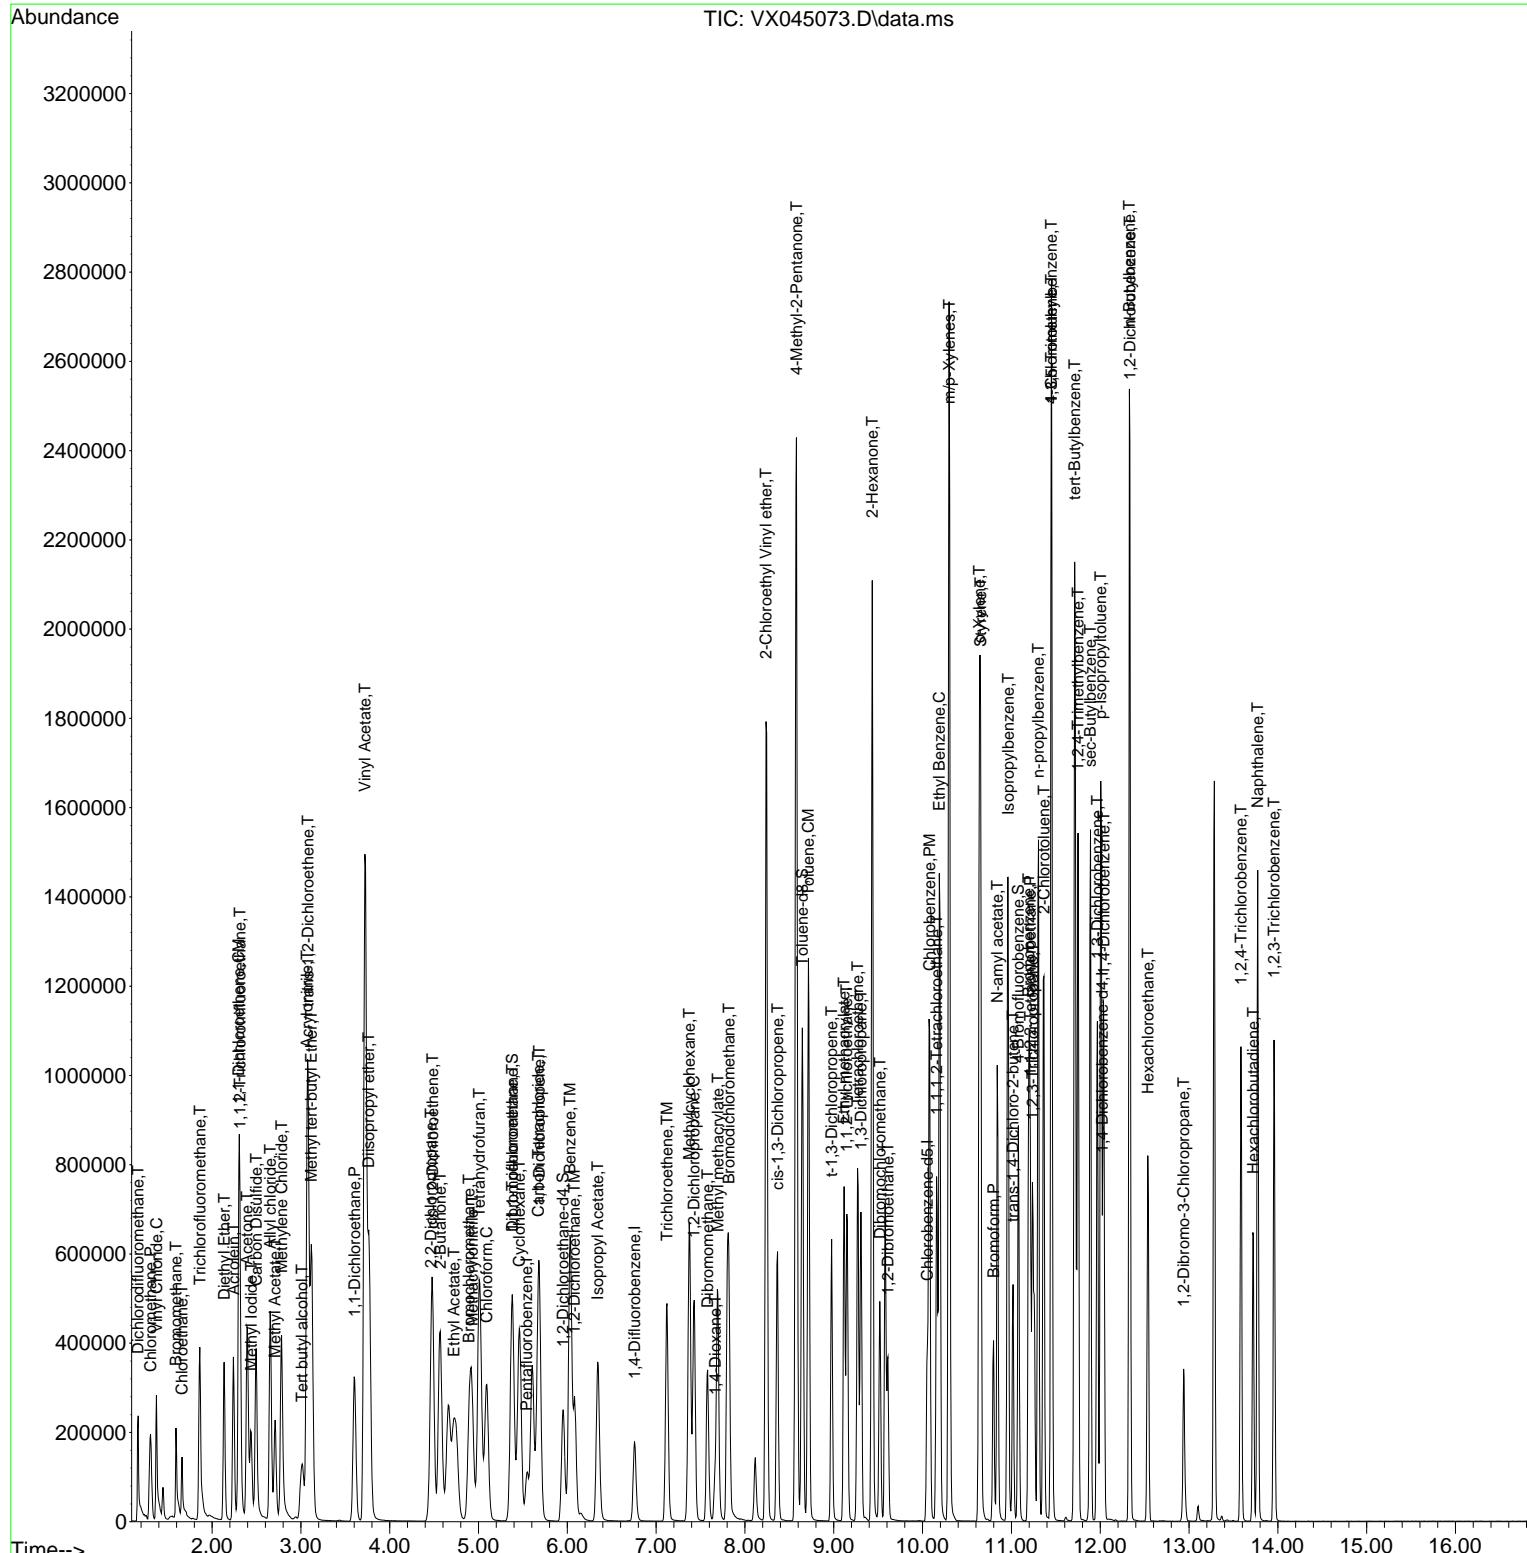



#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.544 min Scan# 7
 Delta R.T. -0.006 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47



Instrument : MSVOA_X
 ClientSampleId : VSTDICC150




Tgt Ion:168 Resp: 95754
 Ion Ratio Lower Upper
 168 100
 99 64.8 48.2 72.4

Manual Integrations APPROVED




Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025




#2
 Dichlorodifluoromethane
 Concen: 132.067 ug/l
 RT: 1.166 min Scan# 13
 Delta R.T. -0.000 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47



Tgt Ion: 85 Resp: 174297
 Ion Ratio Lower Upper
 85 100
 87 32.5 17.4 52.3

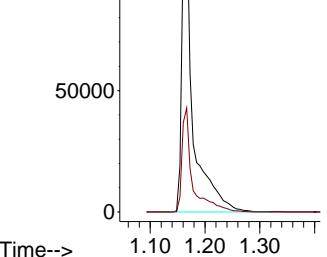







#3
Chloromethane
Concen: 133.072 ug/l
RT: 1.307 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Instrument : MSVOA_X
ClientSampleId : VSTDICC150

Tgt Ion: 50 Resp: 21370
Ion Ratio Lower Upper
50 100
52 32.7 25.0 37.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

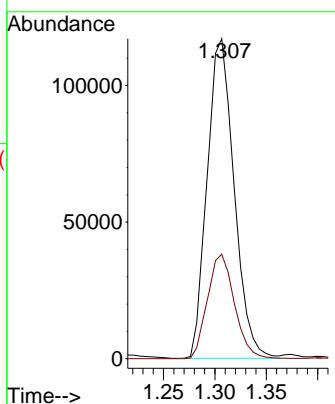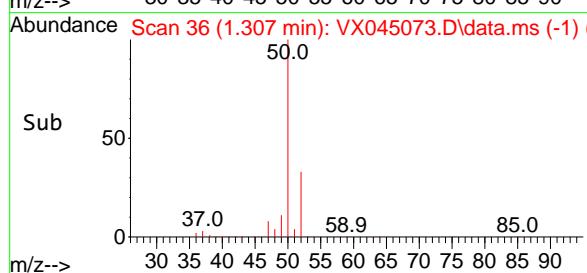


#4
Vinyl Chloride
Concen: 138.774 ug/l
RT: 1.374 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Tgt Ion: 62 Resp: 217672
Ion Ratio Lower Upper
62 100
64 31.8 24.3 36.5

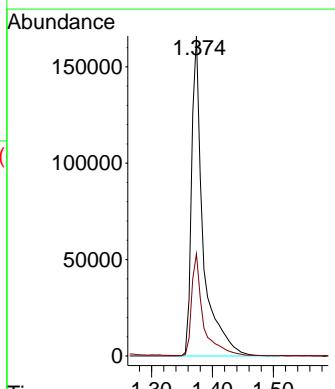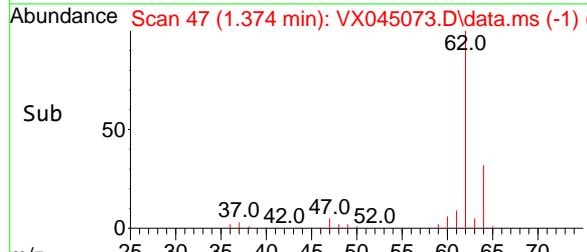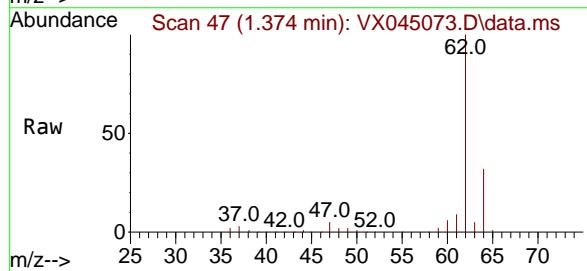






#5
Bromomethane
Concen: 170.379 ug/l
RT: 1.593 min Scan# 8
Instrument : MSVOA_X
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion: 94 Resp: 8354
Ion Ratio Lower Upper
94 100
96 92.2 75.0 112.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

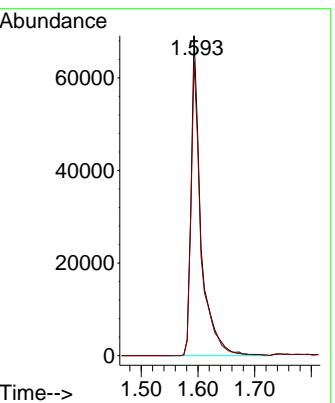


#6
Chloroethane
Concen: 137.509 ug/l
RT: 1.660 min Scan# 94
Instrument : MSVOA_X
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion: 64 Resp: 82101
Ion Ratio Lower Upper
64 100
66 30.8 26.7 40.1

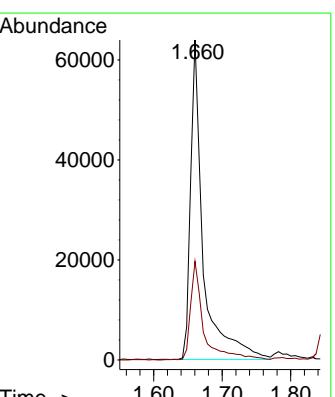



#7
Trichlorofluoromethane
Concen: 135.494 ug/l
RT: 1.861 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150

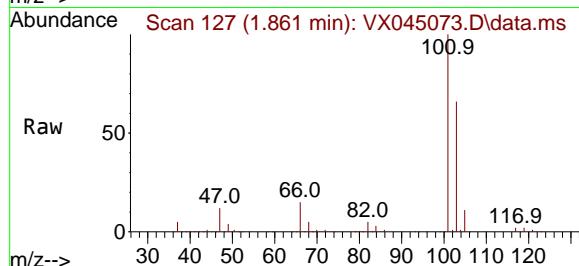


Tgt Ion:101 Resp: 272239
Ion Ratio Lower Upper
101 100
103 66.4 52.1 78.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

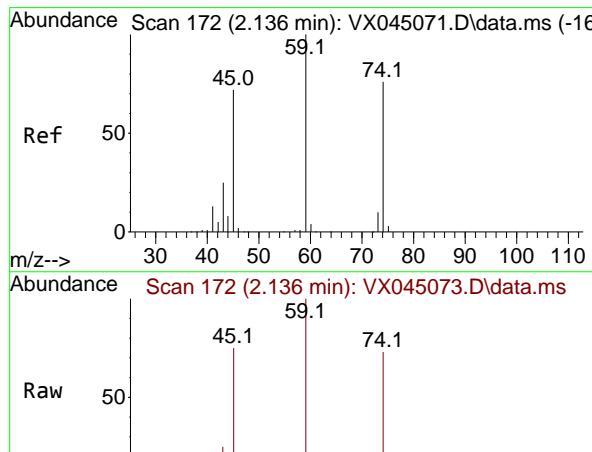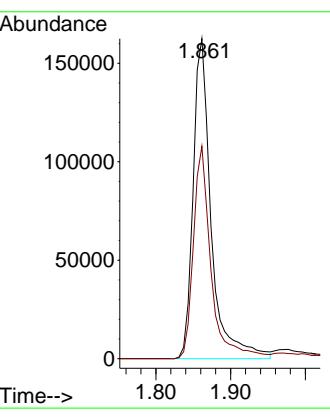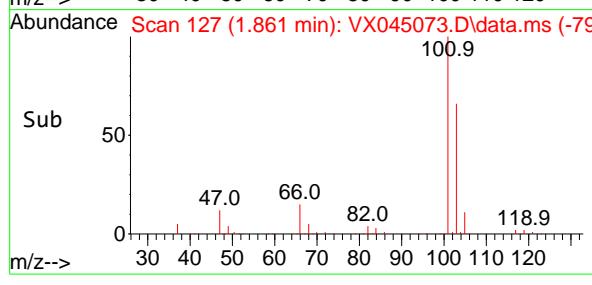


#8
Diethyl Ether
Concen: 150.660 ug/l
RT: 2.136 min Scan# 172
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion: 74 Resp: 110005
Ion Ratio Lower Upper
74 100
45 104.9 51.5 154.5

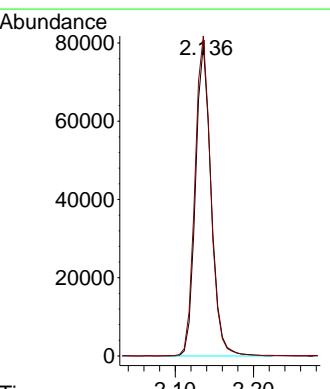



#9
1,1,2-Trichlorotrifluoroethane
Concen: 134.877 ug/l
RT: 2.313 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150




Tgt Ion:101 Resp: 16182
Ion Ratio Lower Upper
101 100
85 45.8 36.2 54.4
151 70.8 56.4 84.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

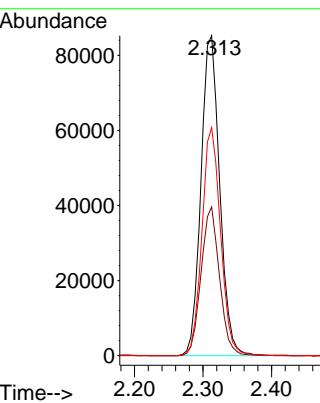


#10
Methyl Iodide
Concen: 138.059 ug/l
RT: 2.441 min Scan# 222
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion:142 Resp: 212355
Ion Ratio Lower Upper
142 100
127 45.2 35.4 53.2
141 14.3 11.6 17.4

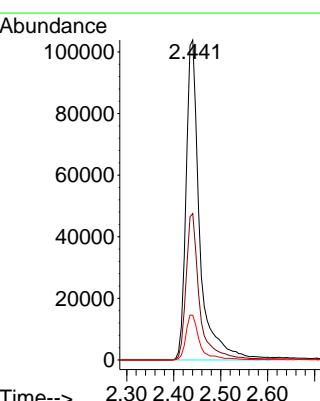



#11
Tert butyl alcohol
Concen: 754.176 ug/l
RT: 3.014 min Scan# 311
Delta R.T. 0.030 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150




Tgt Ion: 59 Resp: 195411
Ion Ratio Lower Upper
59 100
57 10.9 7.8 11.8

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

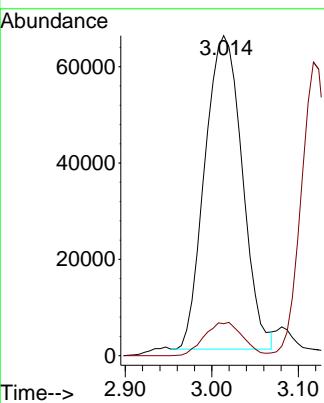


#12
1,1-Dichloroethene
Concen: 140.655 ug/l
RT: 2.300 min Scan# 199
Delta R.T. -0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion: 96 Resp: 173271
Ion Ratio Lower Upper
96 100
61 174.5 134.6 202.0
98 65.6 51.0 76.6

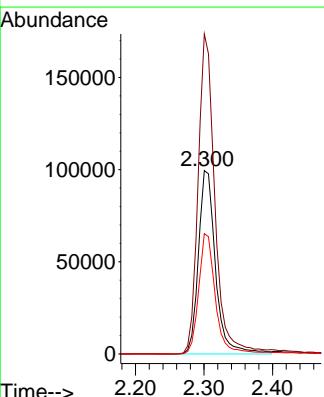



#13
Acrolein
Concen: 940.846 ug/l
RT: 2.239 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150

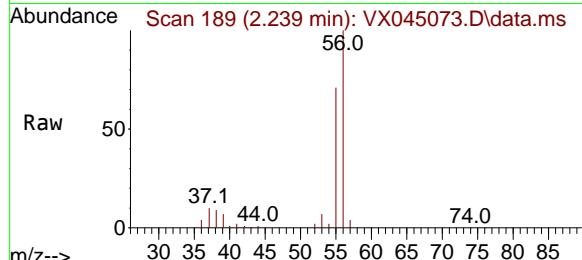

Tgt Ion: 56 Resp: 263999
Ion Ratio Lower Upper
56 100
55 71.6 56.2 84.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#14
Allyl chloride
Concen: 139.077 ug/l
RT: 2.654 min Scan# 257
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47


Tgt Ion: 41 Resp: 308018
Ion Ratio Lower Upper
41 100
39 67.9 53.8 80.8
76 33.8 25.2 37.8

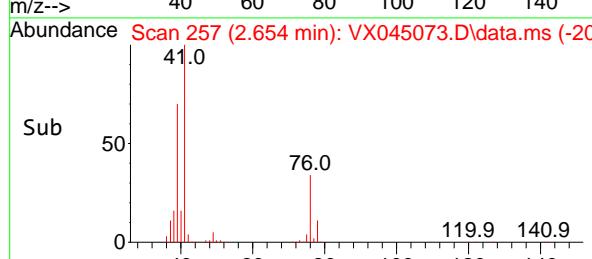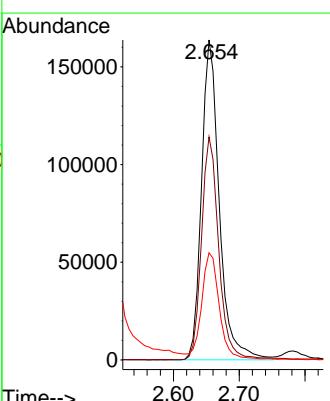



#15
Acrylonitrile
Concen: 813.990 ug/l
RT: 3.069 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150




Tgt Ion: 53 Resp: 573208
Ion Ratio Lower Upper
53 100
52 83.3 66.2 99.2
51 37.0 29.0 43.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#16
Acetone
Concen: 879.387 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion: 43 Resp: 511828
Ion Ratio Lower Upper
43 100
58 30.3 24.2 36.4





#17
Carbon Disulfide
Concen: 145.511 ug/l
RT: 2.495 min Scan# 2
Delta R.T. -0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150

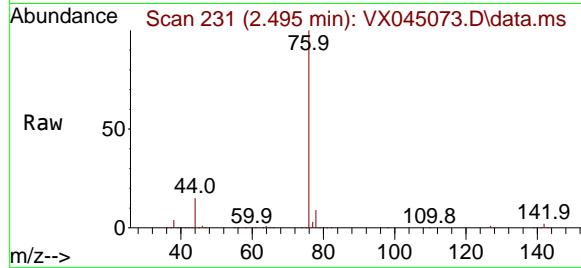

Tgt Ion: 76 Resp: 487720
Ion Ratio Lower Upper
76 100
78 8.8 6.6 9.8




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#18
Methyl Acetate
Concen: 147.347 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47


Tgt Ion: 43 Resp: 258303
Ion Ratio Lower Upper
43 100
74 22.0 17.4 26.2

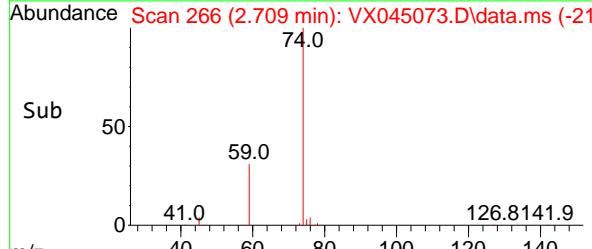



#19
Methyl tert-butyl Ether
Concen: 157.358 ug/l
RT: 3.117 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150




Tgt Ion: 73 Resp: 61977
Ion Ratio Lower Upper
73 100
57 22.4 18.5 27.7

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

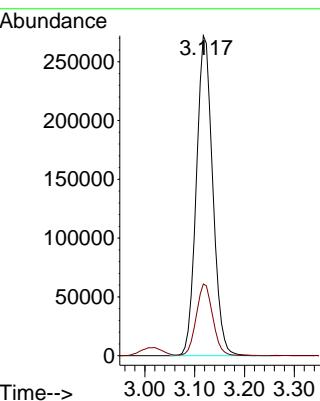


#20
Methylene Chloride
Concen: 147.198 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion: 84 Resp: 202913
Ion Ratio Lower Upper
84 100
49 133.6 106.5 159.7
51 40.9 32.1 48.1
86 64.8 50.0 75.0

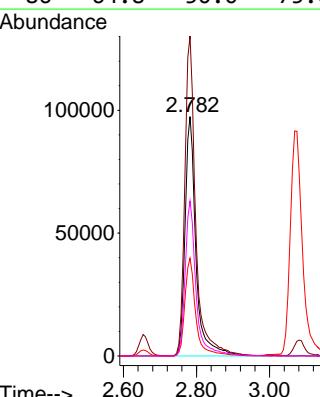



#21
trans-1,2-Dichloroethene
Concen: 146.027 ug/l
RT: 3.081 min Scan# 3
Delta R.T. -0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150



Tgt Ion: 96 Resp: 17692
Ion Ratio Lower Upper
96 100
61 147.0 117.0 175.4
98 63.6 53.4 80.2



Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

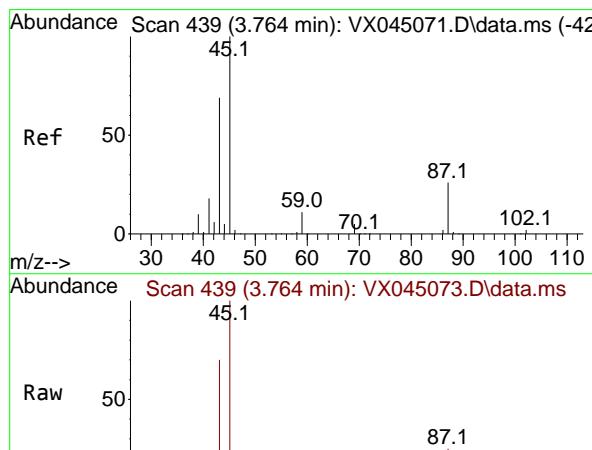

#22
Diisopropyl ether
Concen: 156.526 ug/l
RT: 3.764 min Scan# 439
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47


Tgt Ion: 45 Resp: 662828
Ion Ratio Lower Upper
45 100
43 70.0 54.9 82.3
87 25.2 21.0 31.4
59 10.9 8.7 13.1

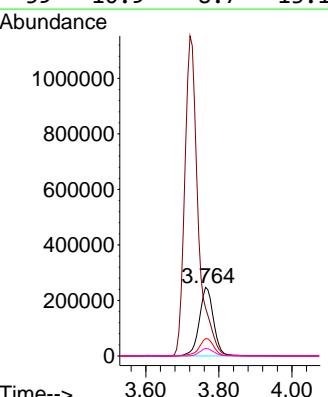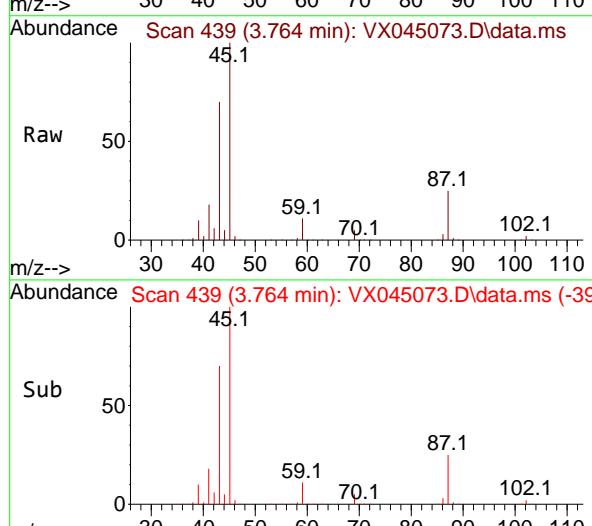



#23
Vinyl Acetate
Concen: 846.586 ug/l
RT: 3.721 min Scan# 413
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument: MSVOA_X
ClientSampleId: VSTDICC150




Tgt Ion: 43 Resp: 2943150
Ion Ratio Lower Upper
43 100
86 9.8 8.1 12.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

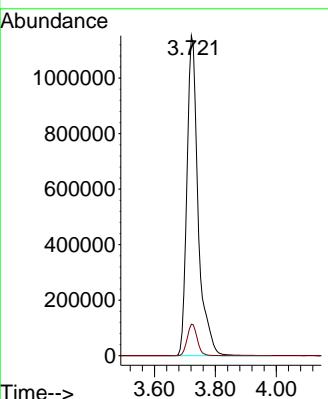


#24
1,1-Dichloroethane
Concen: 153.453 ug/l
RT: 3.605 min Scan# 413
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion: 63 Resp: 363081
Ion Ratio Lower Upper
63 100
98 7.1 3.4 10.2
100 4.4 2.1 6.5



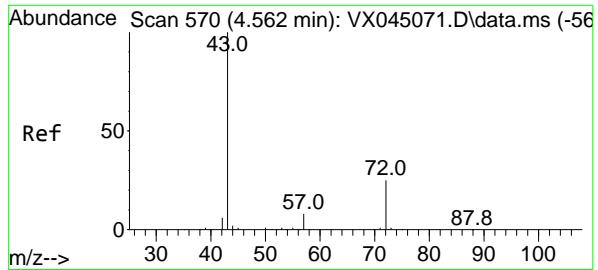

#25
2-Butanone
Concen: 872.239 ug/l
RT: 4.568 min Scan# 51
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150

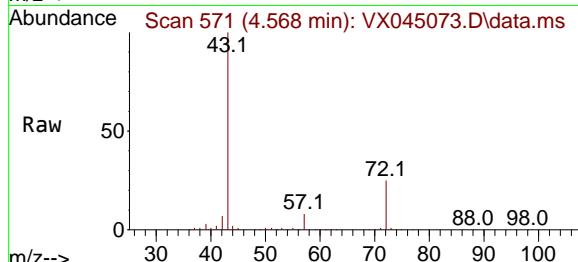


Tgt Ion: 43 Resp: 81849
Ion Ratio Lower Upper
43 100
72 24.7 20.0 30.0

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

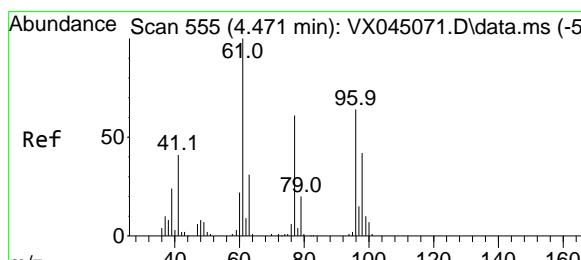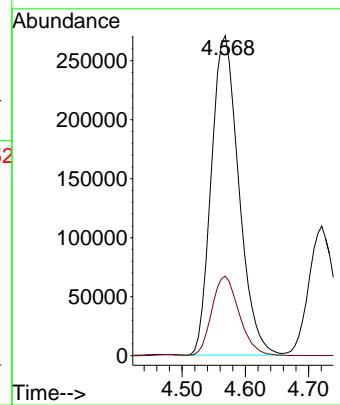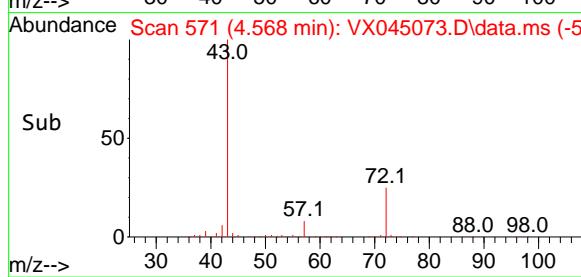


#26
2,2-Dichloropropane
Concen: 102.231 ug/l
RT: 4.465 min Scan# 554
Delta R.T. -0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

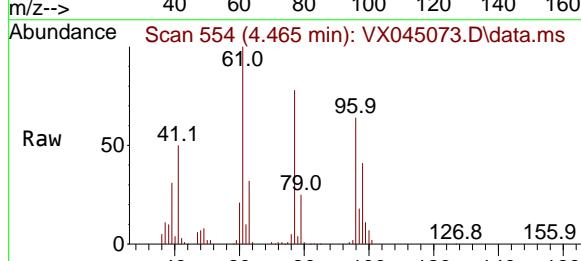


Tgt Ion: 77 Resp: 179826
Ion Ratio Lower Upper
77 100
97 24.1 12.4 37.0

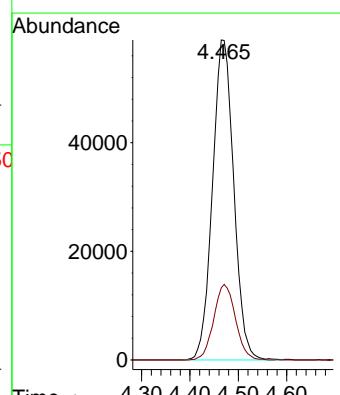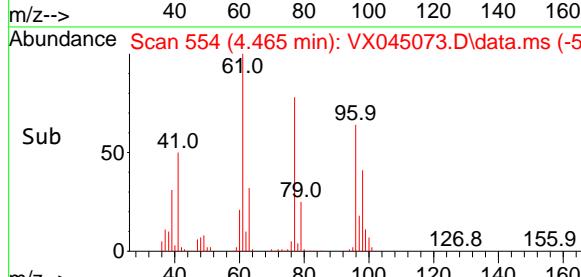



#27
cis-1,2-Dichloroethene
Concen: 151.205 ug/l
RT: 4.483 min Scan# 51
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150




Tgt Ion: 96 Resp: 220820
Ion Ratio Lower Upper
96 100
61 144.2 0.0 283.2
98 64.3 0.0 128.0

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

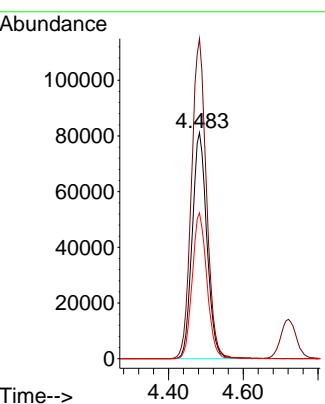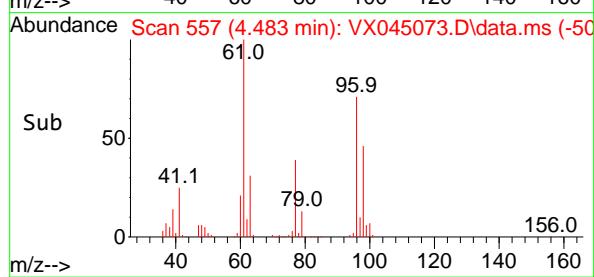


#28
Bromochloromethane
Concen: 150.105 ug/l
RT: 4.891 min Scan# 624
Delta R.T. -0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion: 49 Resp: 171273
Ion Ratio Lower Upper
49 100
129 1.7 0.0 3.4
130 70.3 56.1 84.1





#29
Tetrahydrofuran
Concen: 850.174 ug/l
RT: 5.007 min Scan# 6
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150

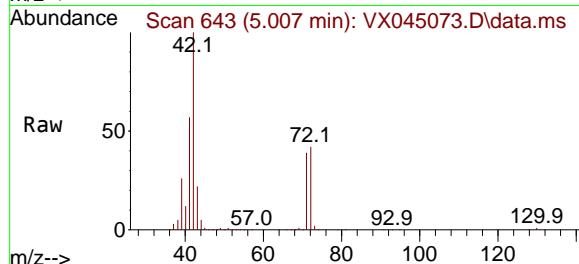

Tgt Ion: 42 Resp: 528574
Ion Ratio Lower Upper
42 100
72 42.8 34.1 51.1
71 39.7 31.4 47.0




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

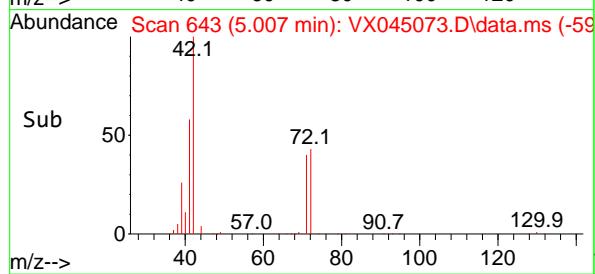


#30
Chloroform
Concen: 152.067 ug/l
RT: 5.093 min Scan# 657
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Tgt Ion: 83 Resp: 351934
Ion Ratio Lower Upper
83 100
85 66.9 51.4 77.2








#31
Cyclohexane
Concen: 139.174 ug/l
RT: 5.458 min Scan# 7
Instrument : MSVOA_X
Delta R.T. -0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

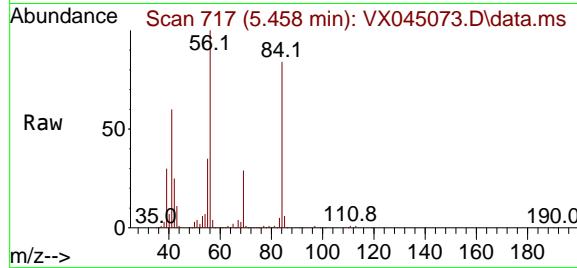


Tgt Ion: 56 Resp: 30221
Ion Ratio Lower Upper
56 100
69 28.8 23.4 35.2
84 82.2 69.4 104.2

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

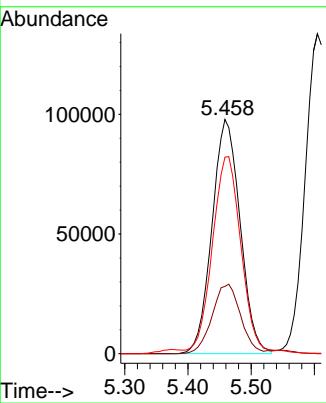


#32
1,1,1-Trichloroethane
Concen: 151.120 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion: 97 Resp: 294434
Ion Ratio Lower Upper
97 100
99 64.7 51.6 77.4
61 48.1 38.4 57.6

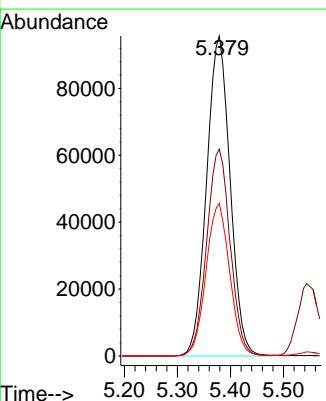



#33
1,2-Dichloroethane-d4
Concen: 165.865 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150




Tgt Ion: 65 Resp: 234624
Ion Ratio Lower Upper
65 100
67 52.7 0.0 106.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

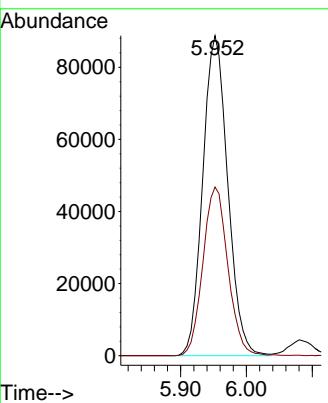


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion:114 Resp: 176991
Ion Ratio Lower Upper
114 100
63 22.8 0.0 41.8
88 16.4 0.0 32.8

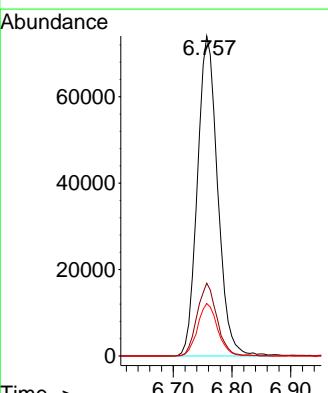



#35
Dibromofluoromethane
Concen: 155.359 ug/l
RT: 5.379 min Scan# 7
Delta R.T. -0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150

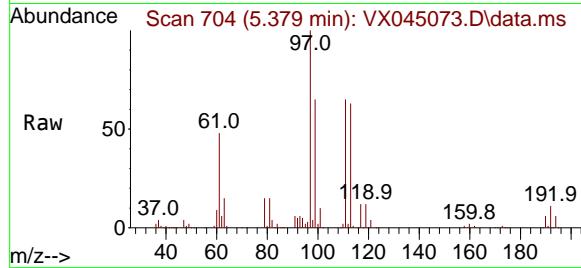


Tgt Ion:113 Resp: 17972
Ion Ratio Lower Upper
113 100
111 102.7 81.8 122.6
192 17.5 14.3 21.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#36
1,1-Dichloropropene
Concen: 145.112 ug/l
RT: 5.684 min Scan# 754
Delta R.T. -0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion: 75 Resp: 241405
Ion Ratio Lower Upper
75 100
110 33.7 16.9 50.6
77 30.5 24.5 36.7



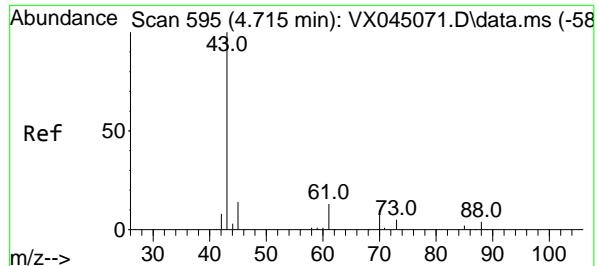

#37
Ethyl Acetate
 Concen: 167.067 ug/l
 RT: 4.721 min Scan# 51
 Delta R.T. 0.006 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
 ClientSampleId : VSTDICC150



Tgt Ion: 43 Resp: 316250
 Ion Ratio Lower Upper
 43 100
 61 13.2 10.8 16.2
 70 10.1 7.7 11.5




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

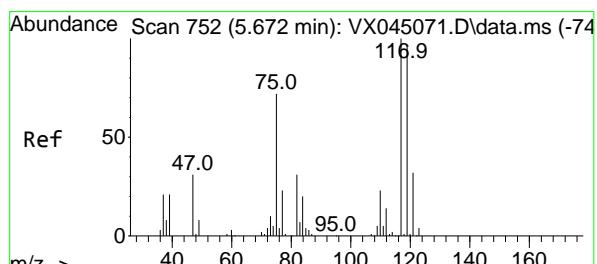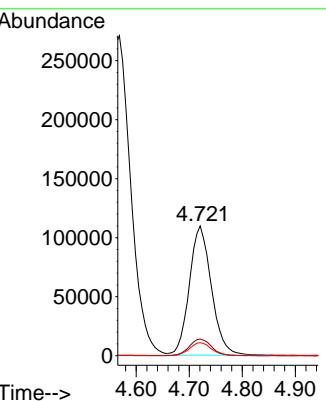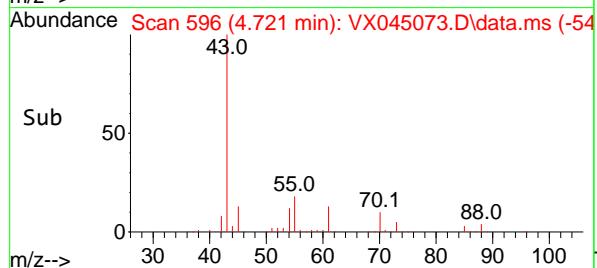

#38
Carbon Tetrachloride
 Concen: 150.363 ug/l
 RT: 5.672 min Scan# 752
 Delta R.T. -0.000 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47


Tgt Ion:117 Resp: 245917
 Ion Ratio Lower Upper
 117 100
 119 95.9 76.7 115.1
 121 30.7 25.5 38.3

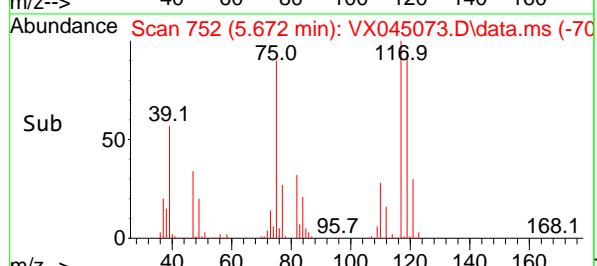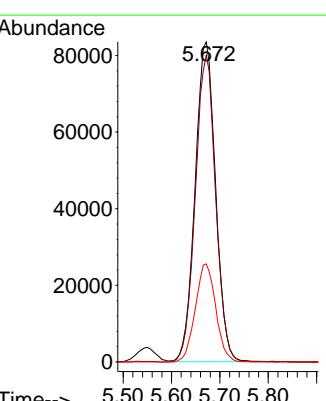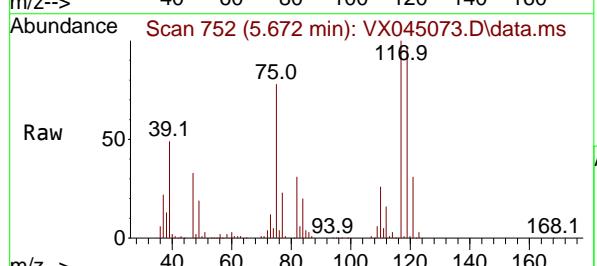



#39
Methylcyclohexane
Concen: 137.544 ug/l
RT: 7.373 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150




Tgt Ion: 83 Resp: 292210
Ion Ratio Lower Upper
83 100
55 81.7 63.0 94.4
98 47.4 39.7 59.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025






#40
Benzene
Concen: 145.368 ug/l
RT: 6.031 min Scan# 811
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47



Tgt Ion: 78 Resp: 755854
Ion Ratio Lower Upper
78 100
77 23.7 18.8 28.2



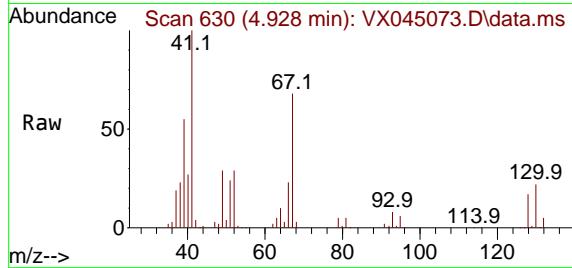

#41

Methacrylonitrile

Concen: 173.088 ug/l

RT: 4.928 min Scan# 6

Delta R.T. 0.006 min

Lab File: VX045073.D

Acq: 28 Feb 2025 03:47

Instrument :

MSVOA_X




ClientSampleId :

VSTDICC150

Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025

Supervised By :Mahesh Dadoda 02/28/2025



#42

1,2-Dichloroethane

Concen: 163.872 ug/l

RT: 6.080 min Scan# 819

Delta R.T. -0.000 min

Lab File: VX045073.D


Acq: 28 Feb 2025 03:47


Tgt Ion: 62 Resp: 276129

Ion Ratio Lower Upper

62 100


98 8.8 0.0 18.2

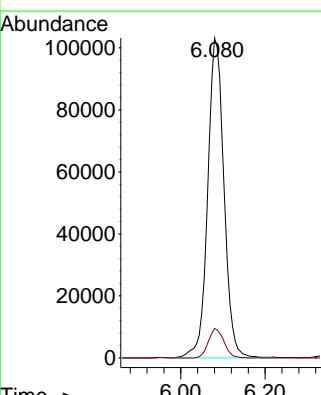



#43
Isopropyl Acetate
Concen: 169.804 ug/l
RT: 6.342 min Scan# 8
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47



Instrument : MSVOA_X
ClientSampleId : VSTDICC150

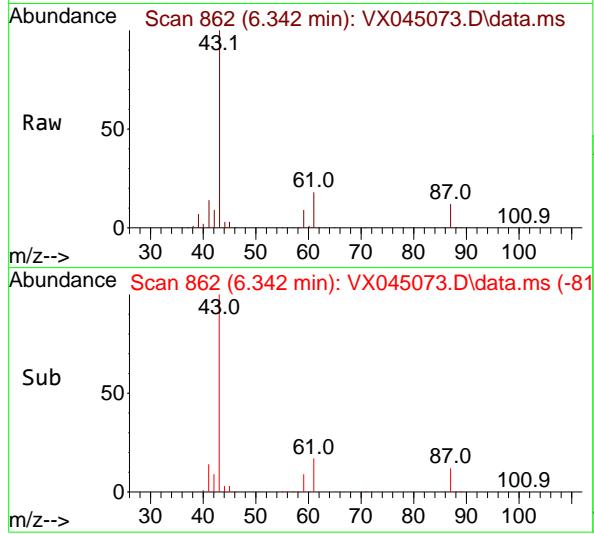

Tgt Ion: 43 Resp: 51164
Ion Ratio Lower Upper
43 100
61 18.7 14.9 22.3
87 12.1 9.4 14.2



Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

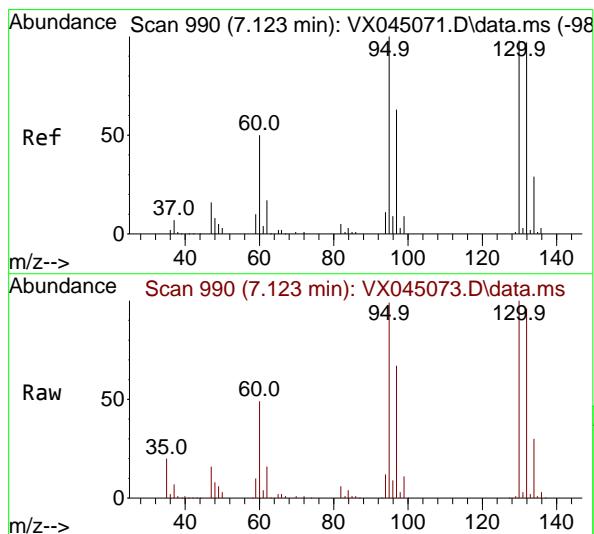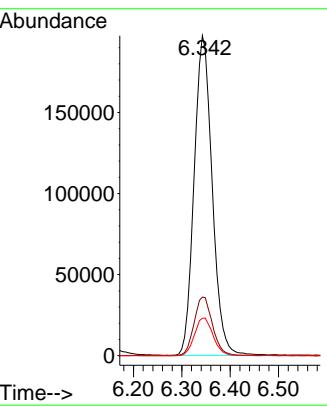

#44
Trichloroethene
Concen: 150.181 ug/l
RT: 7.123 min Scan# 990
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47


Tgt Ion:130 Resp: 178483
Ion Ratio Lower Upper
130 100
95 99.3 0.0 205.0





#45
1,2-Dichloropropane
Concen: 153.334 ug/l
RT: 7.428 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150




Tgt Ion: 63 Resp: 198139
Ion Ratio Lower Upper
63 100
65 30.8 24.7 37.1

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#46
Dibromomethane
Concen: 157.443 ug/l
RT: 7.580 min Scan# 1065
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion: 93 Resp: 142119
Ion Ratio Lower Upper
93 100
95 82.6 65.8 98.8
174 88.2 72.2 108.2

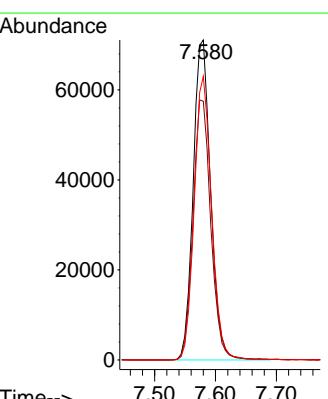



#47
 Bromodichloromethane
 Concen: 160.492 ug/l
 RT: 7.818 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
 ClientSampleId : VSTDICC150




Tgt Ion: 83 Resp: 280255
 Ion Ratio Lower Upper
 83 100
 85 64.9 51.1 76.7
 127 7.8 6.4 9.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

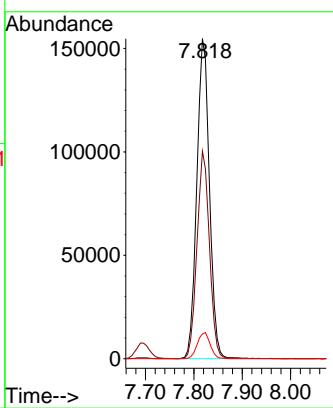


#48
 Methyl methacrylate
 Concen: 176.370 ug/l
 RT: 7.696 min Scan# 1084
 Delta R.T. 0.006 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47




Tgt Ion: 41 Resp: 252275
 Ion Ratio Lower Upper
 41 100
 69 78.1 63.0 94.6
 39 61.1 47.5 71.3

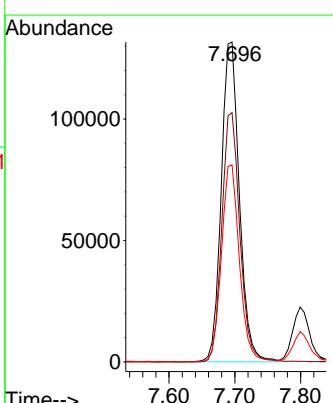



#49
1,4-Dioxane
Concen: 3166.423 ug/l
RT: 7.665 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150




Tgt Ion: 88 Resp: 96263
Ion Ratio Lower Upper
88 100
43 37.0 28.7 43.1
58 70.8 55.8 83.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

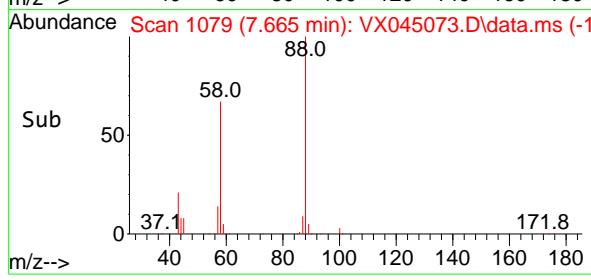


#50
Toluene-d8
Concen: 147.538 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion: 98 Resp: 638979
Ion Ratio Lower Upper
98 100
100 65.4 52.0 78.0





#51
4-Methyl-2-Pentanone
Concen: 832.051 ug/l
RT: 8.580 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150



Tgt Ion: 43 Resp: 153615
Ion Ratio Lower Upper
43 100
58 37.1 29.2 43.8




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#52
Toluene
Concen: 145.321 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47


Tgt Ion: 92 Resp: 448664
Ion Ratio Lower Upper
92 100
91 172.3 138.9 208.3





#53
t-1,3-Dichloropropene
Concen: 154.373 ug/l
RT: 8.976 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150




Tgt Ion: 75 Resp: 266444
Ion Ratio Lower Upper
75 100
77 30.9 26.5 39.7

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

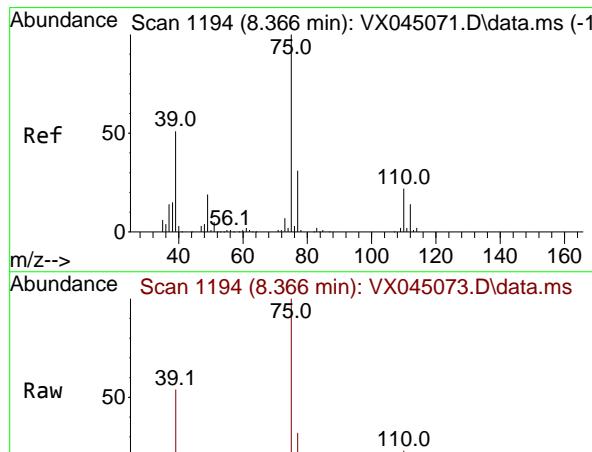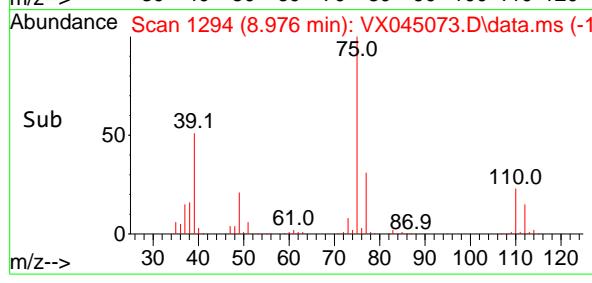


#54
cis-1,3-Dichloropropene
Concen: 152.117 ug/l
RT: 8.366 min Scan# 1194
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

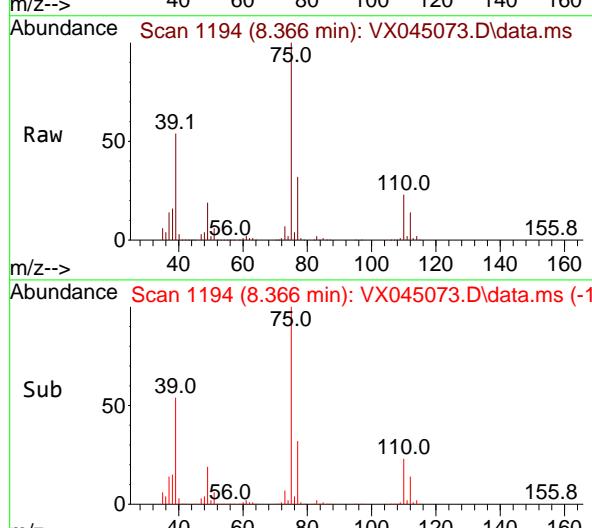


Tgt Ion: 75 Resp: 293521
Ion Ratio Lower Upper
75 100
77 32.3 24.7 37.1
39 54.0 40.7 61.1





#55
1,1,2-Trichloroethane
Concen: 149.046 ug/l
RT: 9.147 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150

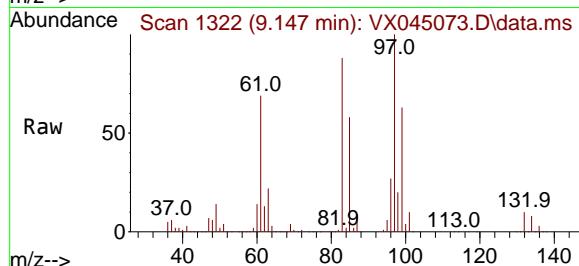


Tgt Ion: 97 Resp: 17821
Ion Ratio Lower Upper
97 100
83 87.8 69.4 104.2
85 57.8 44.1 66.1
99 63.1 50.7 76.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#56
Ethyl methacrylate
Concen: 162.631 ug/l
RT: 9.116 min Scan# 1317
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47



Tgt Ion: 69 Resp: 310992
Ion Ratio Lower Upper
69 100
41 72.6 57.0 85.4
39 44.2 34.2 51.4




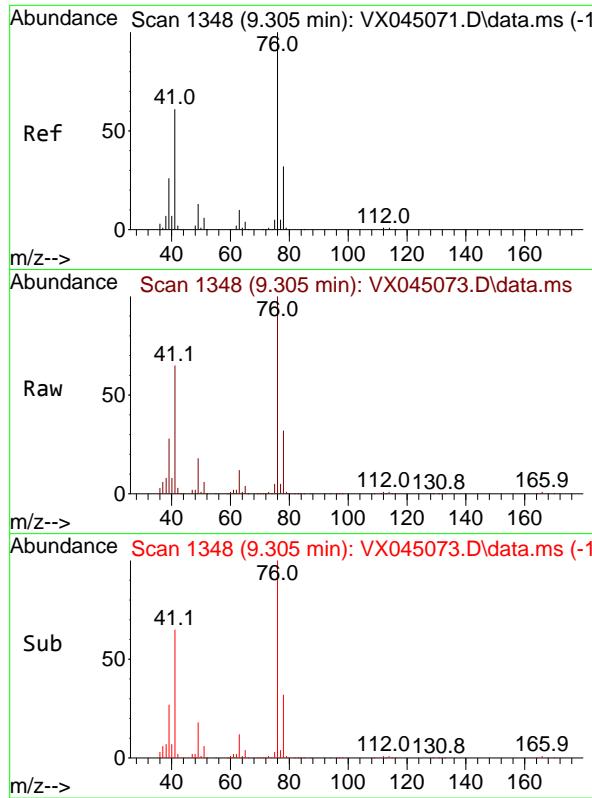


#57
 1,3-Dichloropropane
 Concen: 149.699 ug/l
 RT: 9.305 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47

Instrument : MSVOA_X
 ClientSampleId : VSTDICC150


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

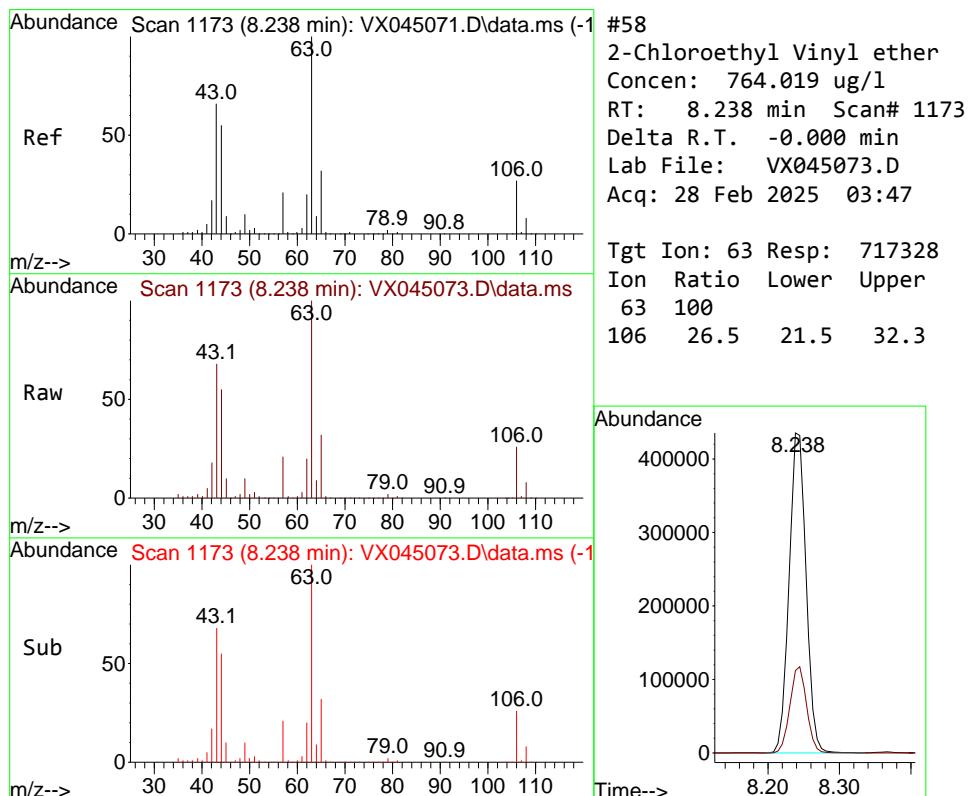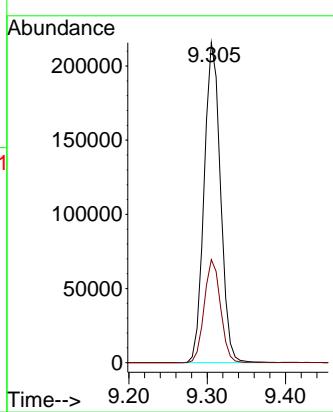

#58
 2-Chloroethyl Vinyl ether
 Concen: 764.019 ug/l
 RT: 8.238 min Scan# 1173
 Delta R.T. -0.000 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47


Tgt Ion: 63 Resp: 717328
 Ion Ratio Lower Upper
 63 100
 106 26.5 21.5 32.3

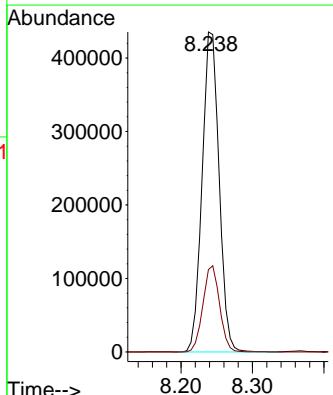



#59
2-Hexanone
Concen: 868.492 ug/l
RT: 9.433 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150




Tgt Ion: 43 Resp: 115665
Ion Ratio Lower Upper
43 100
58 51.6 25.9 77.6

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#60
Dibromochloromethane
Concen: 158.276 ug/l
RT: 9.519 min Scan# 1383
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion:129 Resp: 201906
Ion Ratio Lower Upper
129 100
127 77.9 38.5 115.5

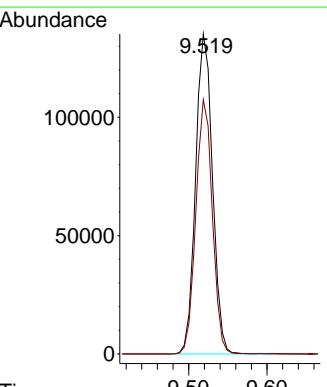



#61
1,2-Dibromoethane
Concen: 154.074 ug/l
RT: 9.610 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150




Tgt Ion:107 Resp: 185823
Ion Ratio Lower Upper
107 100
109 95.2 76.1 114.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

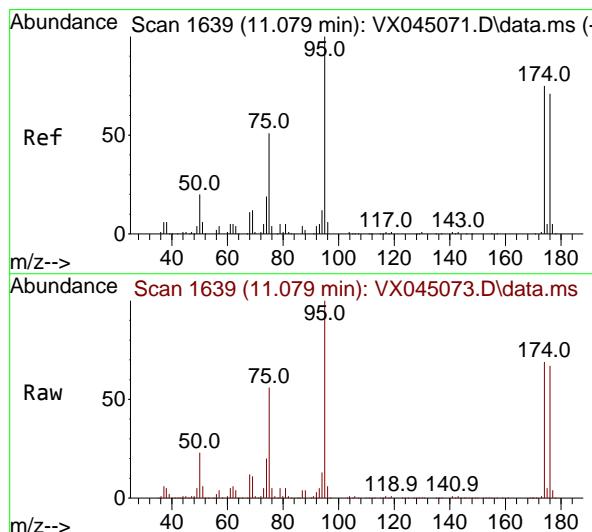


#62
4-Bromofluorobenzene
Concen: 154.420 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47



Tgt Ion: 95 Resp: 223346
Ion Ratio Lower Upper
95 100
174 70.4 0.0 148.2
176 69.4 0.0 141.4

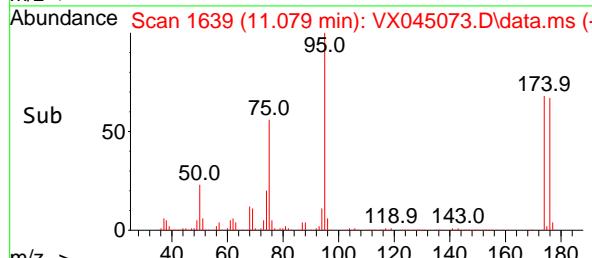


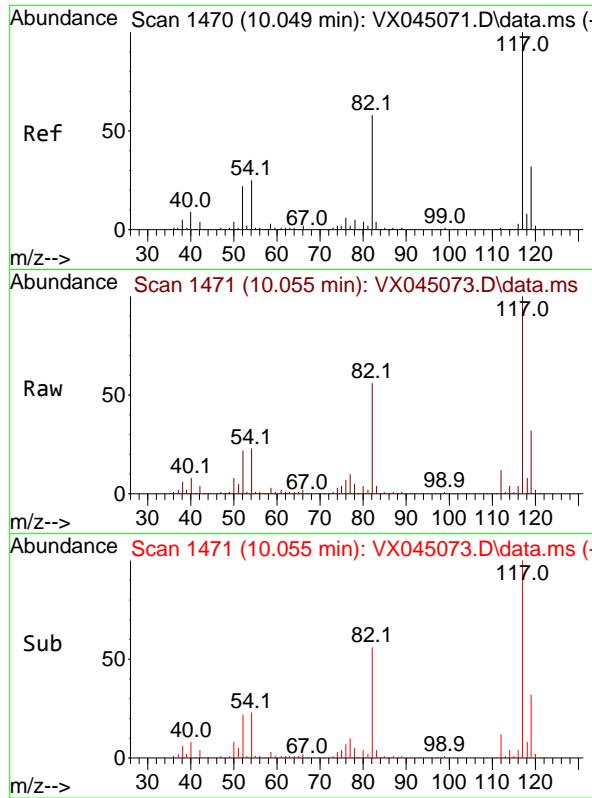


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Instrument : MSVOA_X
ClientSampleId : VSTDICC150


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

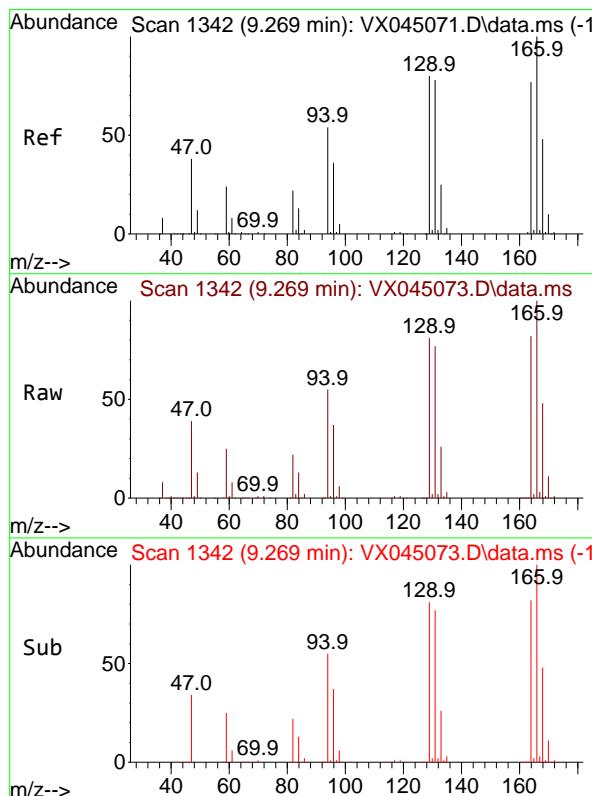

#64
Tetrachloroethene
Concen: 145.906 ug/l
RT: 9.269 min Scan# 1342
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Tgt Ion:164 Resp: 139536
Ion Ratio Lower Upper
164 100
166 121.6 103.6 155.4
129 99.0 82.7 124.1
131 93.6 80.5 120.7




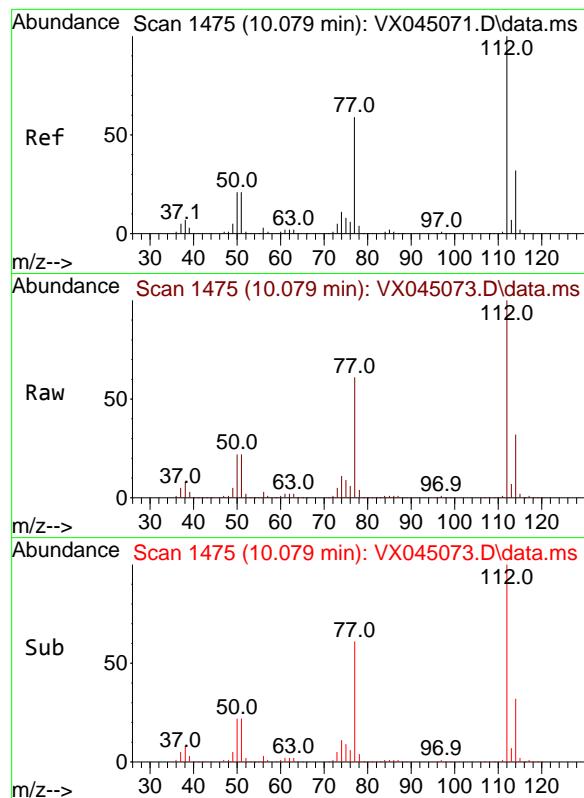


#65
Chlorobenzene
Concen: 146.096 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Instrument : MSVOA_X
ClientSampleId : VSTDICC150


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

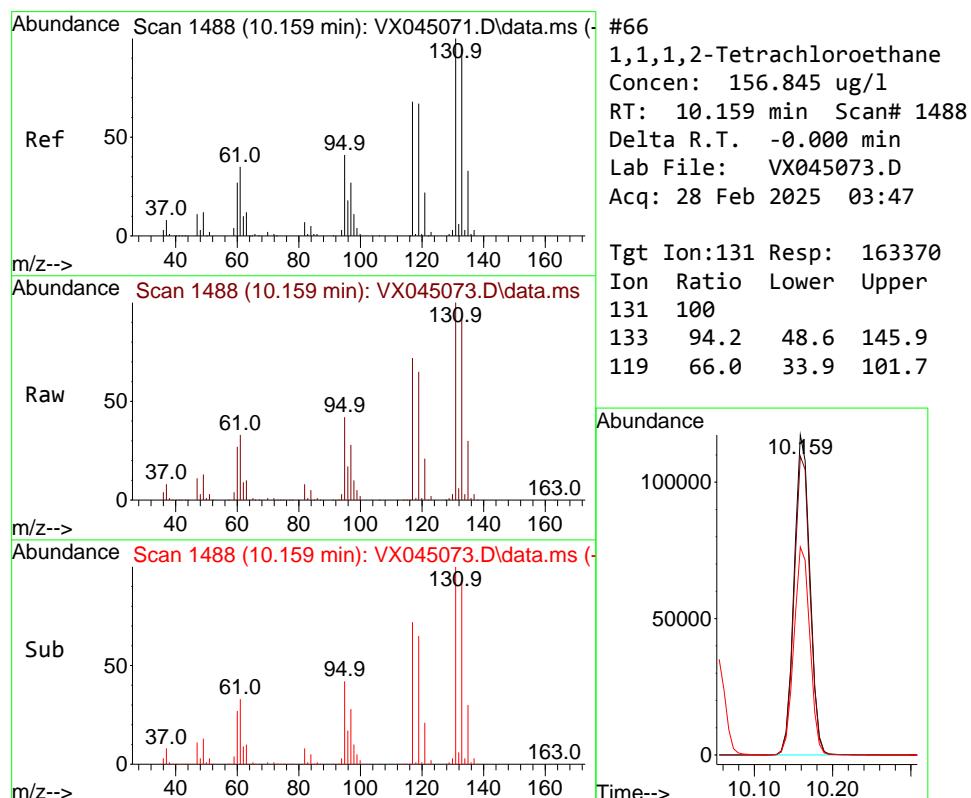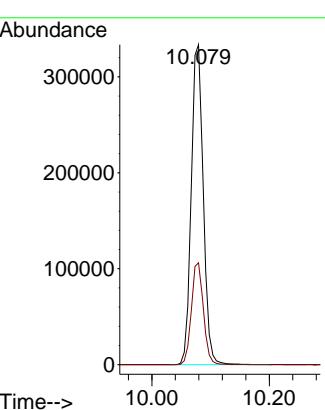


#66
1,1,1,2-Tetrachloroethane
Concen: 156.845 ug/l
RT: 10.159 min Scan# 1488
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Tgt Ion:131 Resp: 163370
Ion Ratio Lower Upper
131 100
133 94.2 48.6 145.9
119 66.0 33.9 101.7

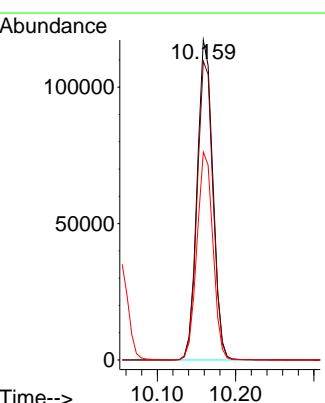

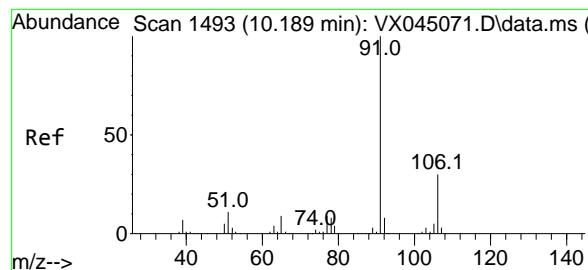



#67
 Ethyl Benzene
 Concen: 149.191 ug/l
 RT: 10.189 min Scan# 1493
 Delta R.T. -0.000 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47
Instrument: MSVOA_X
ClientSampleId: VSTDICC150




Tgt Ion: 91 Resp: 852571
 Ion Ratio Lower Upper
 91 100
 106 29.5 23.9 35.9

Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025




#68
 m/p-Xylenes
 Concen: 288.655 ug/l
 RT: 10.299 min Scan# 1511
 Delta R.T. -0.000 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47



Tgt Ion:106 Resp: 607523
 Ion Ratio Lower Upper
 106 100
 91 211.2 165.4 248.0




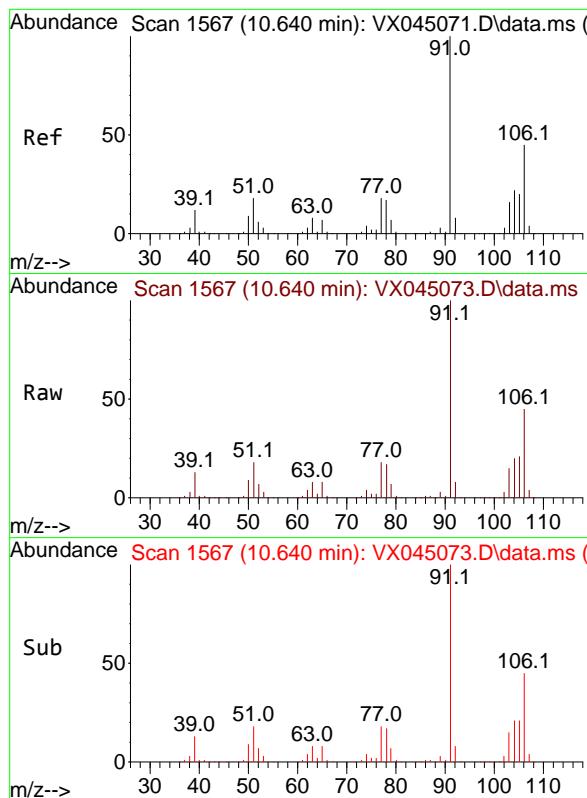


#69
o-Xylene
Concen: 143.259 ug/l
RT: 10.640 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Instrument : MSVOA_X
ClientSampleId : VSTDICC150

Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

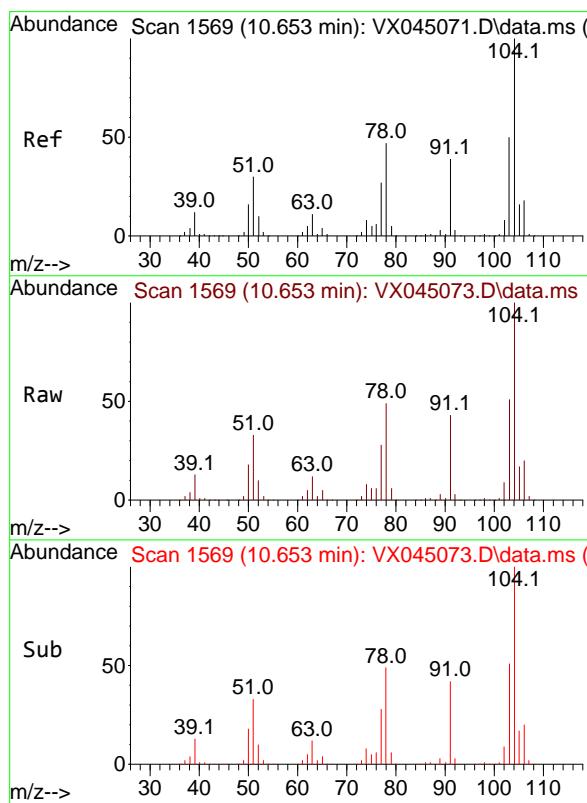


#70
Styrene
Concen: 150.979 ug/l
RT: 10.653 min Scan# 1569
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Abundance

Time-->






#71
Bromoform
Concen: 174.808 ug/l
RT: 10.799 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47
Instrument: MSVOA_X
ClientSampleId: VSTDICC150




Tgt Ion:173 Resp: 135388
Ion Ratio Lower Upper
173 100
175 48.3 24.6 73.6#
254 0.1 0.0 0.0#

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

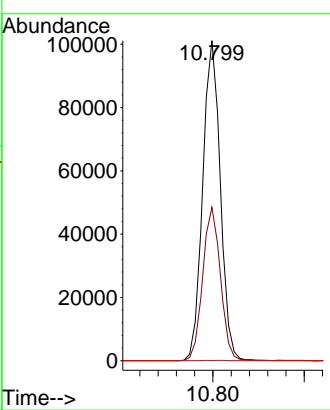


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

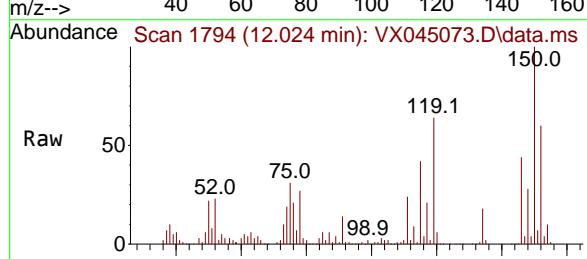

Tgt Ion:152 Resp: 67685
Ion Ratio Lower Upper
152 100
115 138.4 44.2 132.6#
150 208.8 0.0 349.0

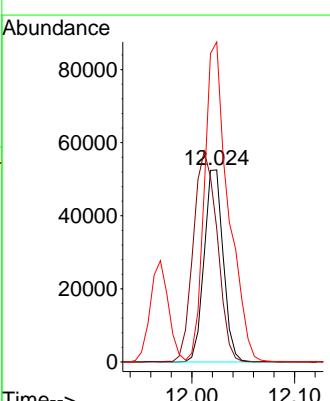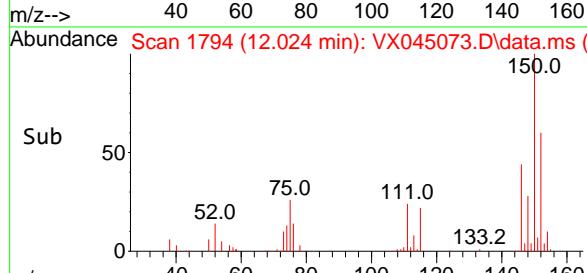


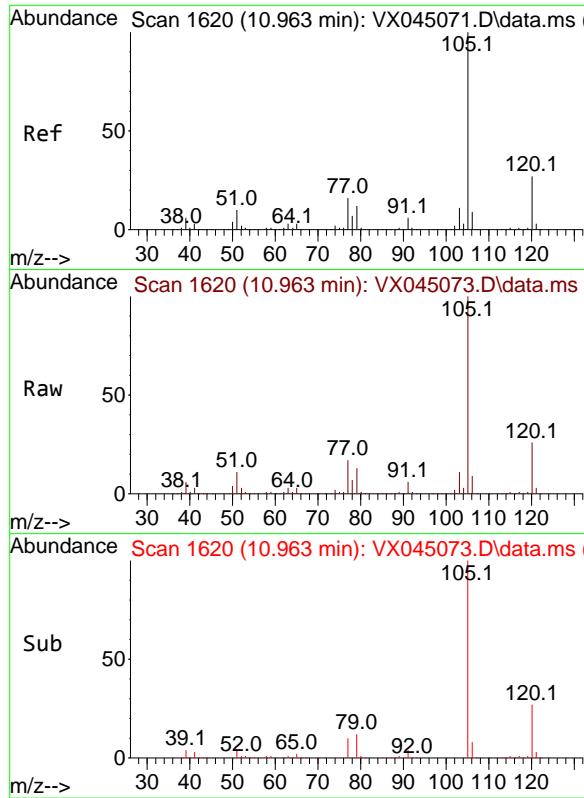


#73
Isopropylbenzene
Concen: 142.719 ug/l
RT: 10.963 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Instrument : MSVOA_X
ClientSampleId : VSTDICC150


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

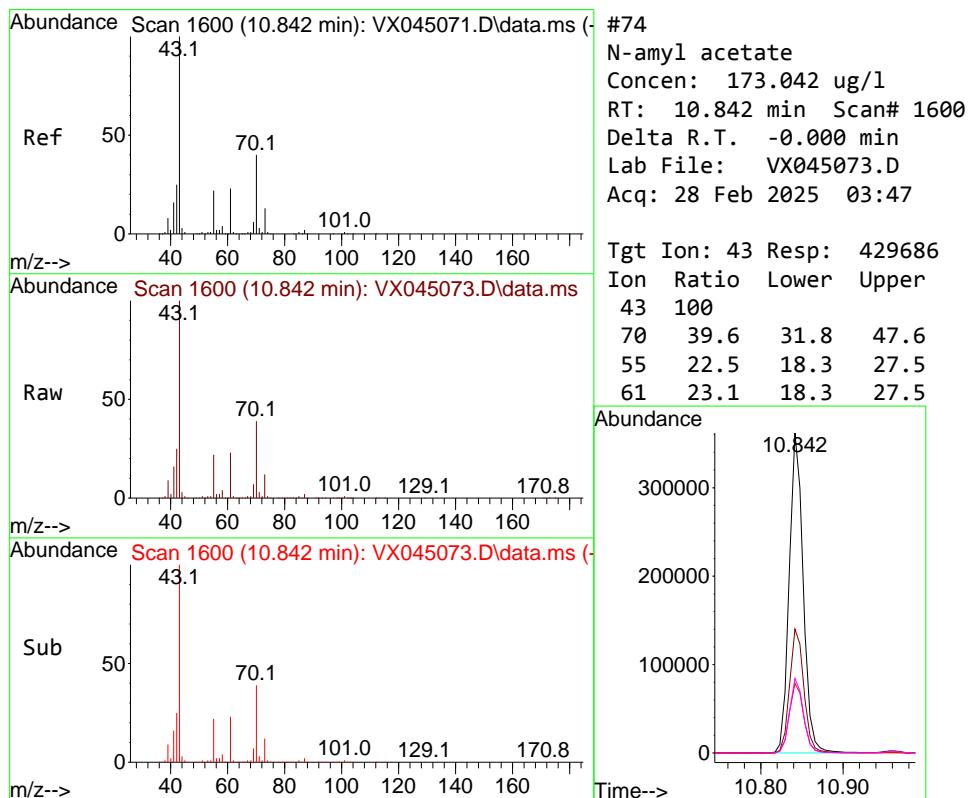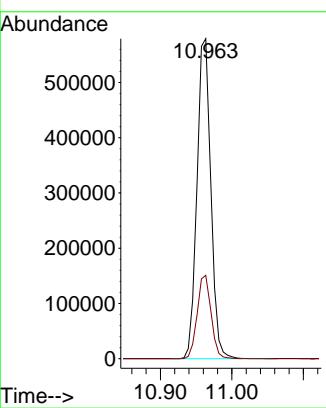

#74
N-amyl acetate
Concen: 173.042 ug/l
RT: 10.842 min Scan# 1600
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Tgt Ion: 43 Resp: 429686
Ion Ratio Lower Upper
43 100
70 39.6 31.8 47.6
55 22.5 18.3 27.5
61 23.1 18.3 27.5

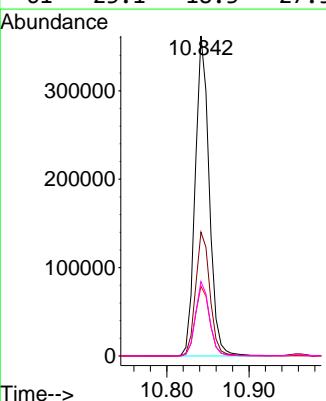


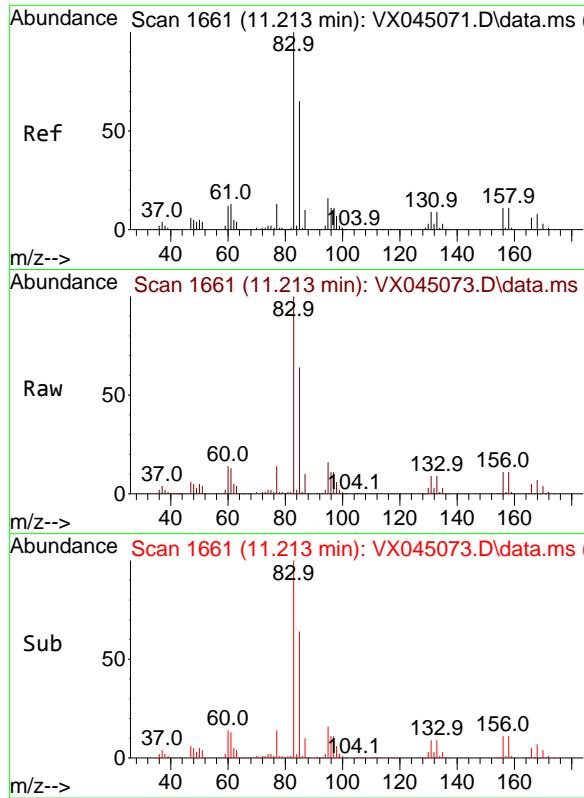


#75
1,1,2,2-Tetrachloroethane
Concen: 150.458 ug/l
RT: 11.213 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150


Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

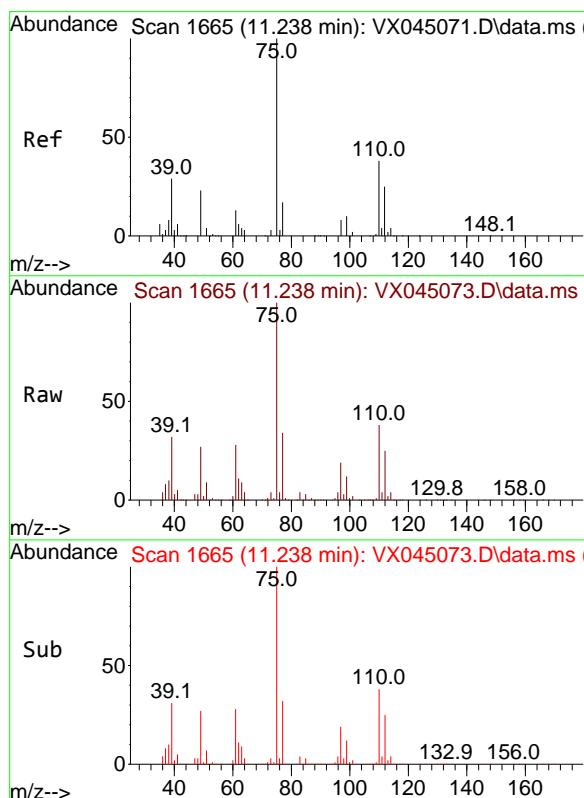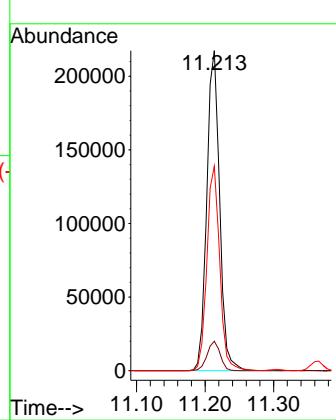

#76
1,2,3-Trichloropropane
Concen: 151.960 ug/l
RT: 11.238 min Scan# 1665
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47


Tgt Ion: 75 Resp: 229435
Ion Ratio Lower Upper
75 100
77 43.2 20.7 62.1

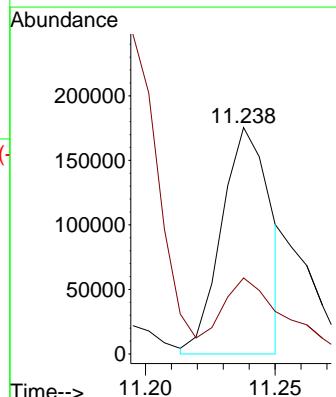

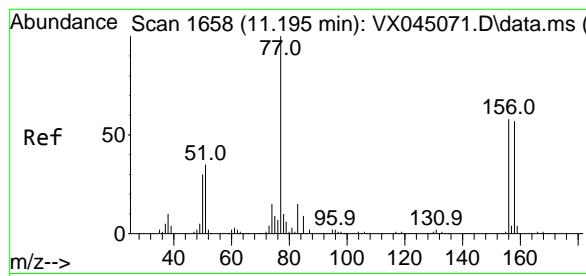

#77
Bromobenzene
Concen: 145.760 ug/l
RT: 11.195 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150

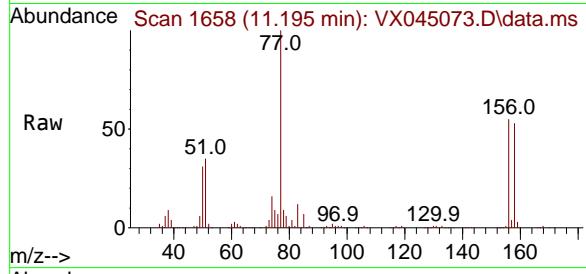


Tgt Ion:156 Resp: 180991
Ion Ratio Lower Upper
156 100
77 179.4 85.8 257.4
158 97.1 48.4 145.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

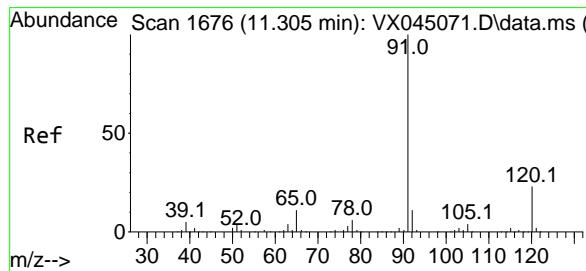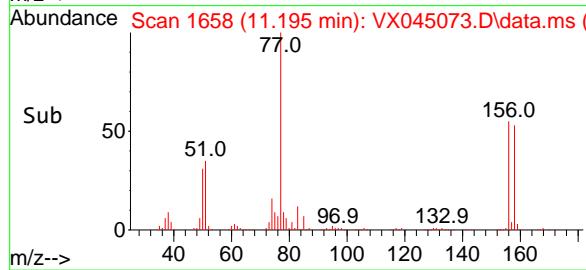


#78
n-propylbenzene
Concen: 146.395 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

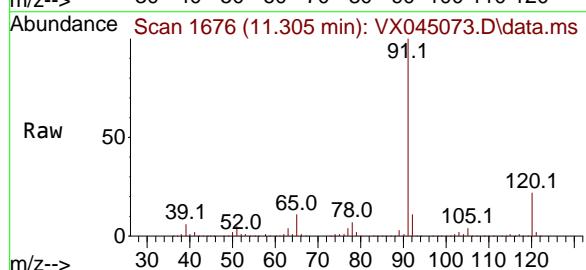


Tgt Ion: 91 Resp: 923593
Ion Ratio Lower Upper
91 100
120 21.8 11.2 33.6

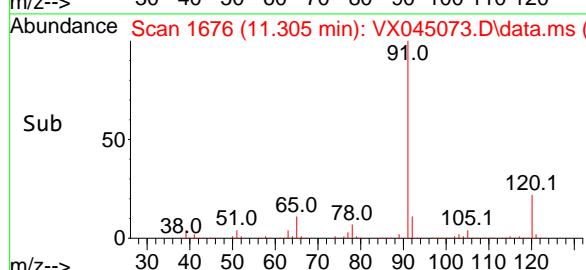

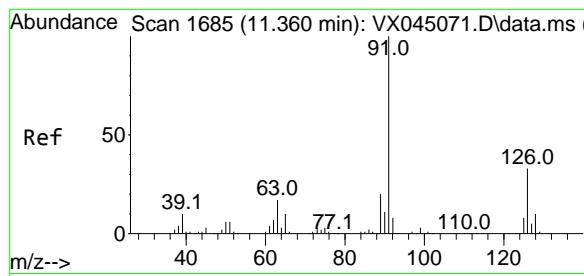

#79
2-Chlorotoluene
Concen: 141.695 ug/l
RT: 11.366 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150

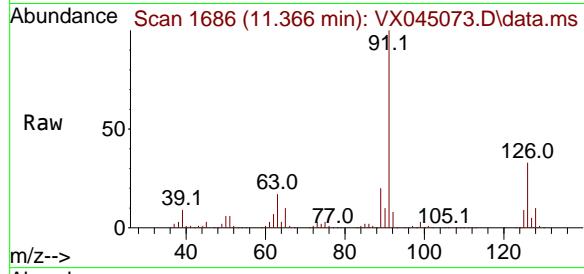


Tgt Ion: 91 Resp: 54869
Ion Ratio Lower Upper
91 100
126 32.4 16.4 49.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

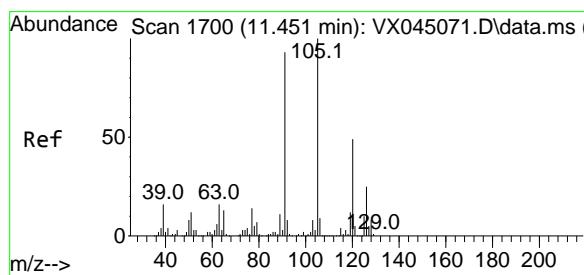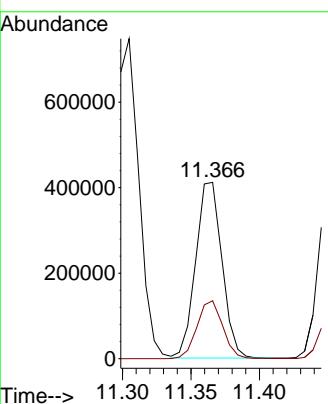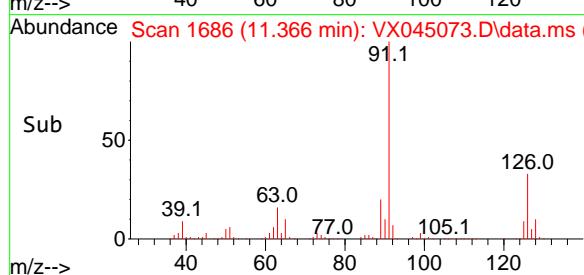


#80
1,3,5-Trimethylbenzene
Concen: 143.293 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

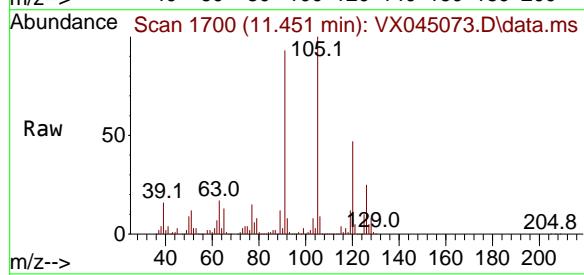

Tgt Ion:105 Resp: 635832
Ion Ratio Lower Upper
105 100
120 46.7 24.1 72.2

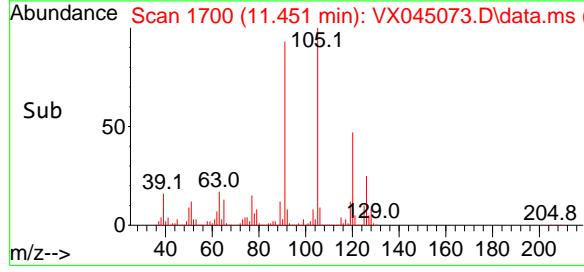


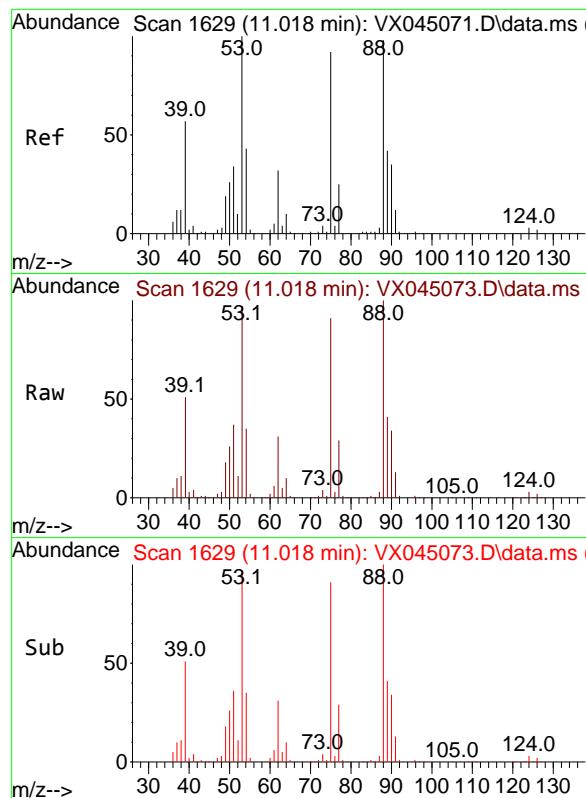


#81
trans-1,4-Dichloro-2-butene
Concen: 147.761 ug/l
RT: 11.018 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Instrument :
MSVOA_X
ClientSampleId :
VSTDICC150


Manual Integrations APPROVED




Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

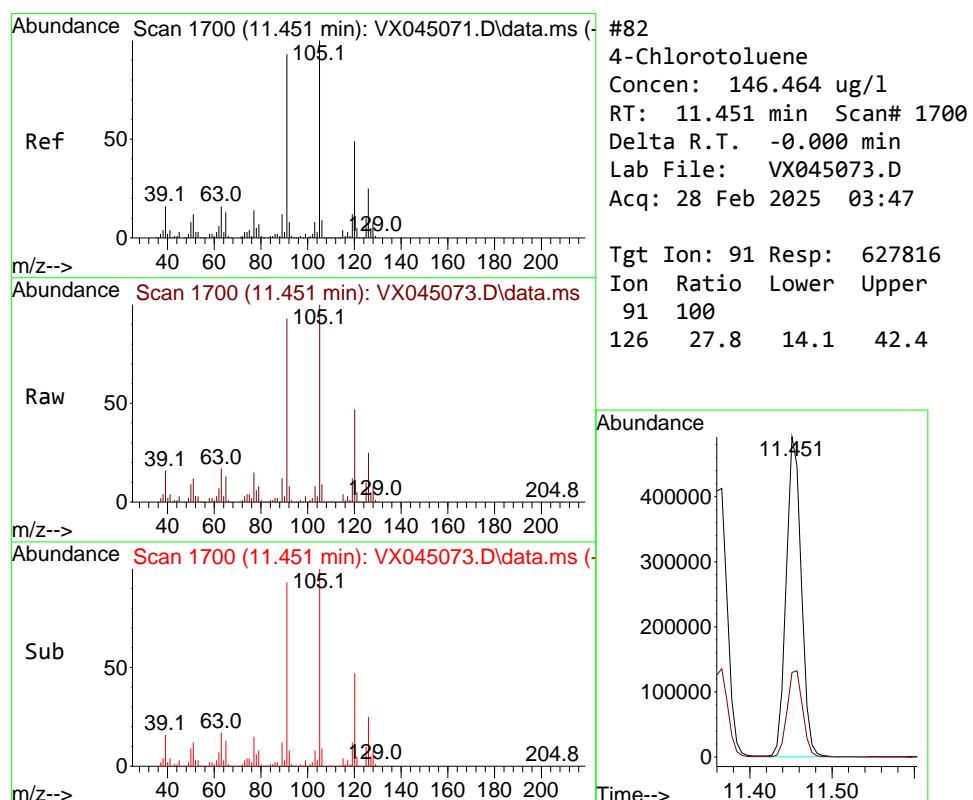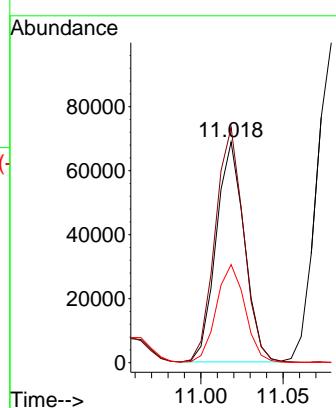

#82
4-Chlorotoluene
Concen: 146.464 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Tgt Ion: 91 Resp: 627816
Ion Ratio Lower Upper
91 100
126 27.8 14.1 42.4

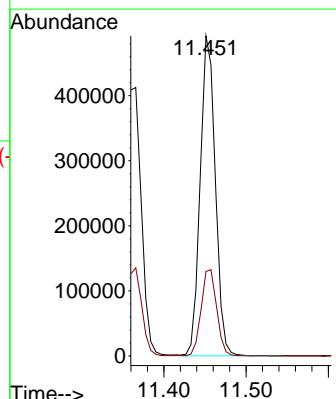



#83

tert-Butylbenzene

Concen: 142.974 ug/l

RT: 11.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045073.D

Acq: 28 Feb 2025 03:47





Instrument:

MSVOA_X

ClientSampleId :

VSTDICC150

**Manual Integrations
APPROVED**

 Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025


#84

1,2,4-Trimethylbenzene


Concen: 148.135 ug/l


RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX045073.D


Acq: 28 Feb 2025 03:47

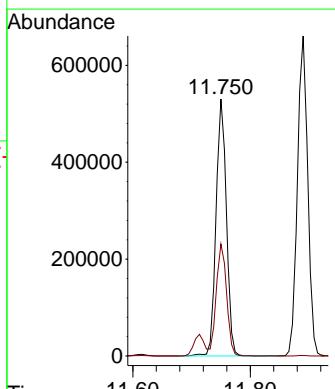 Tgt Ion:105 Resp: 647248
 Ion Ratio Lower Upper
 105 100
 120 43.8 22.1 66.1

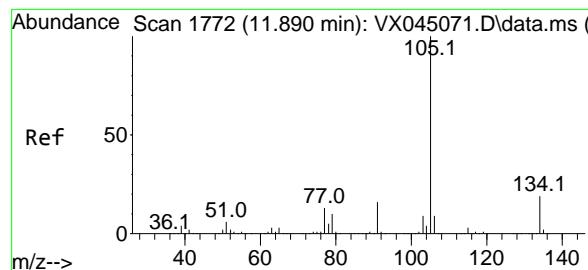


#85
sec-Butylbenzene
Concen: 145.383 ug/l
RT: 11.890 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47



Instrument : MSVOA_X
ClientSampleId : VSTDICC150

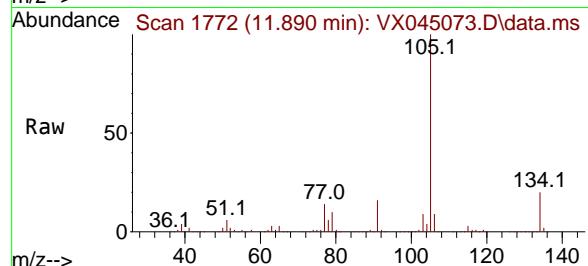


Tgt Ion:105 Resp: 80771
Ion Ratio Lower Upper
105 100
134 19.4 9.8 29.4

**Manual Integrations
APPROVED**


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

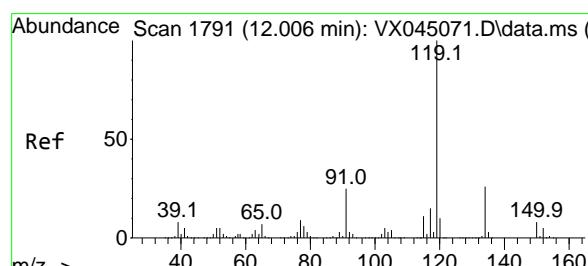


#86
p-Isopropyltoluene
Concen: 149.075 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

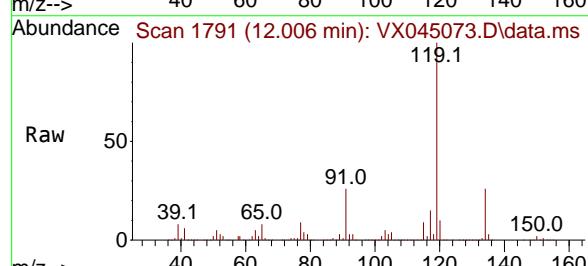

Tgt Ion:119 Resp: 664916
Ion Ratio Lower Upper
119 100
134 25.7 12.9 38.6
91 25.8 12.7 38.0




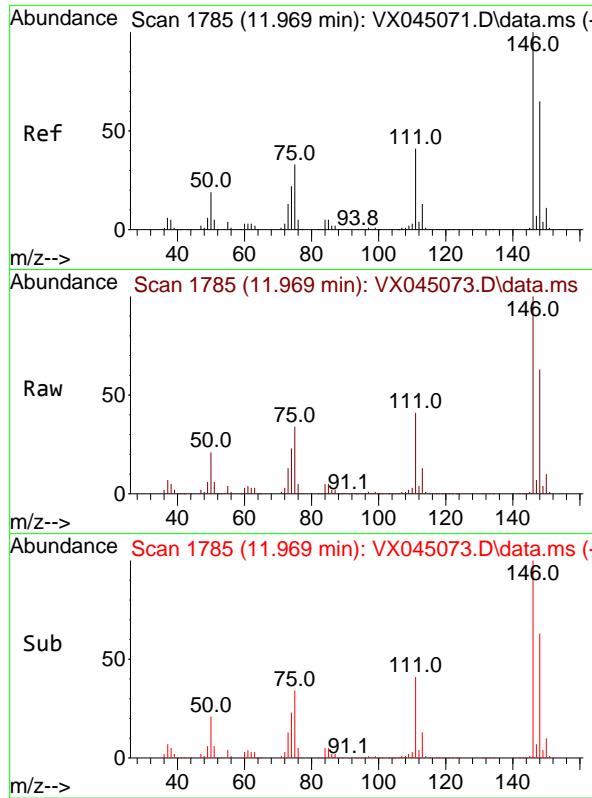


#87
1,3-Dichlorobenzene
Concen: 147.488 ug/l
RT: 11.969 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Instrument : MSVOA_X
ClientSampleId : VSTDICC150


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

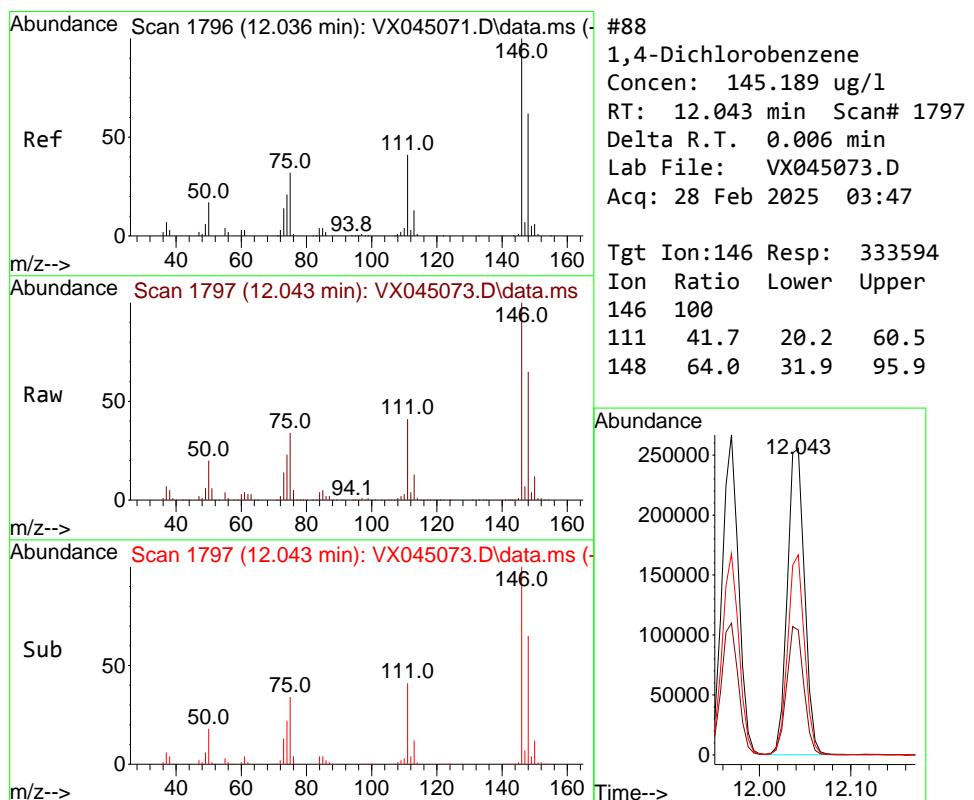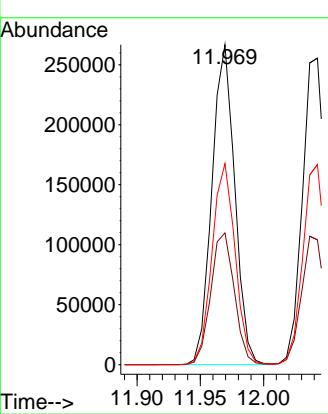

#88
1,4-Dichlorobenzene
Concen: 145.189 ug/l
RT: 12.043 min Scan# 1797
Delta R.T. 0.006 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47


Tgt Ion:146 Resp: 333594
Ion Ratio Lower Upper
146 100
111 41.7 20.2 60.5
148 64.0 31.9 95.9

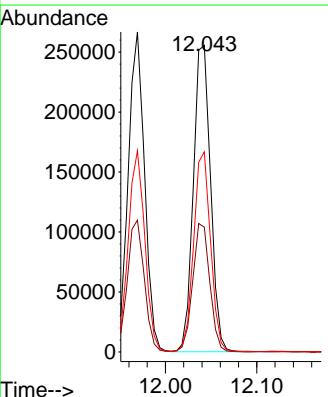



#89
n-Butylbenzene
Concen: 158.324 ug/l
RT: 12.329 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150




Tgt Ion: 91 Resp: 620751
Ion Ratio Lower Upper
91 100
92 53.9 26.7 80.0
134 23.6 12.2 36.6

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

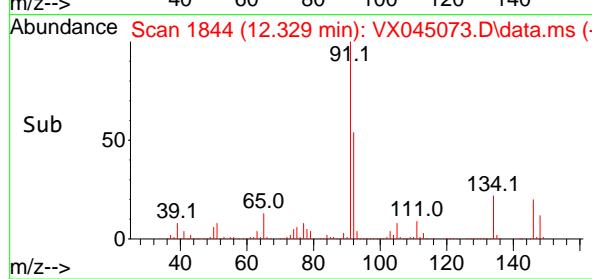


#90
Hexachloroethane
Concen: 154.554 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Tgt Ion:117 Resp: 128582
Ion Ratio Lower Upper
117 100
201 64.2 31.9 95.9

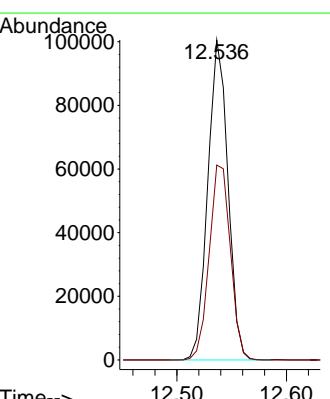



#91
1,2-Dichlorobenzene
Concen: 147.436 ug/l
RT: 12.335 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47




Instrument : MSVOA_X
ClientSampleId : VSTDICC150



Tgt Ion:146 Resp: 32931:
Ion Ratio Lower Upper
146 100
111 44.9 21.6 65.0
148 63.4 31.9 95.9




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

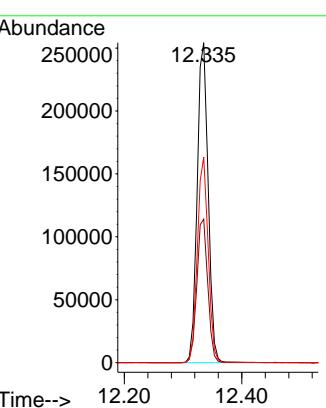

#92
1,2-Dibromo-3-Chloropropane
Concen: 186.240 ug/l
RT: 12.939 min Scan# 1944
Delta R.T. -0.000 min
Lab File: VX045073.D
Acq: 28 Feb 2025 03:47

Tgt Ion: 75 Resp: 64958
Ion Ratio Lower Upper
75 100
155 77.9 39.6 118.7
157 100.1 51.1 153.4

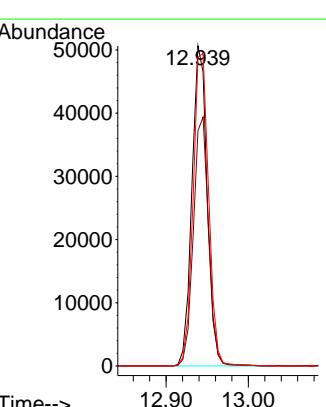


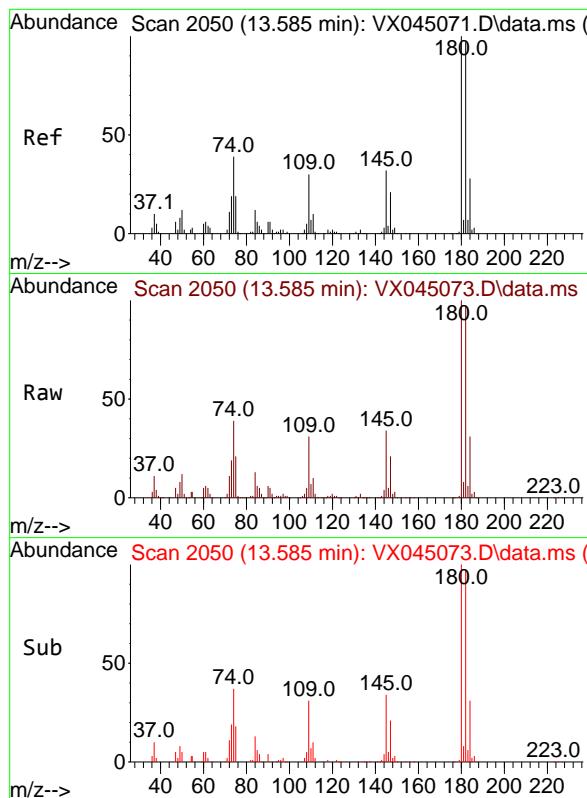


#93
 1,2,4-Trichlorobenzene
 Concen: 162.416 ug/l
 RT: 13.585 min Scan# 21931
 Delta R.T. -0.000 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDICC150


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

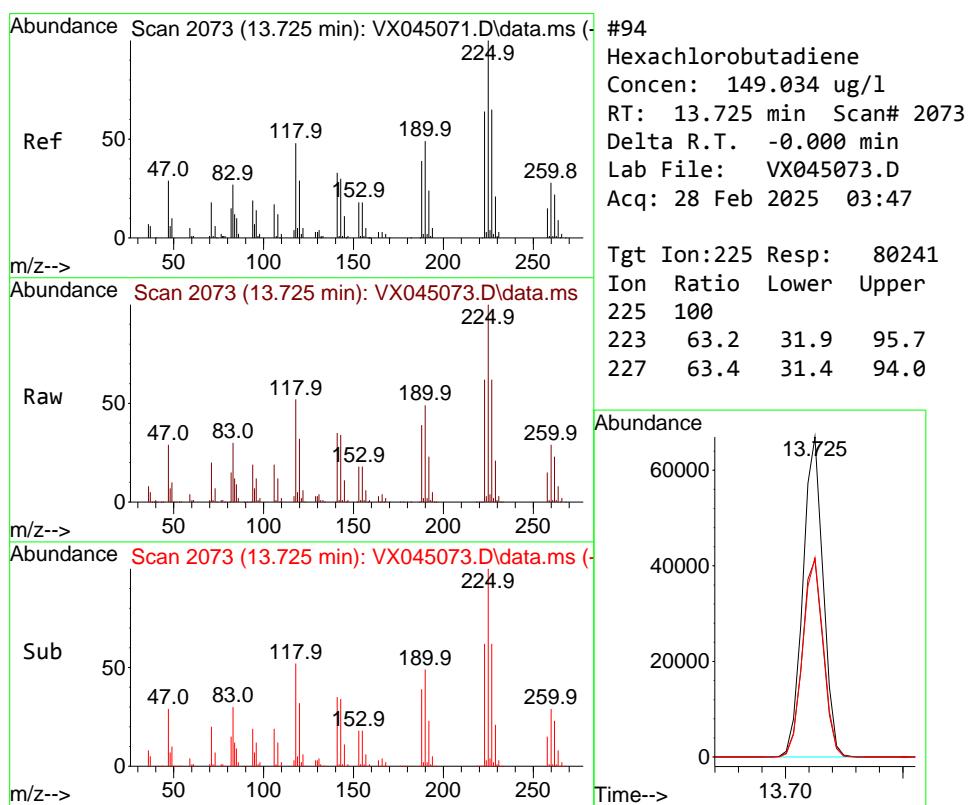

#94
 Hexachlorobutadiene
 Concen: 149.034 ug/l
 RT: 13.725 min Scan# 2073
 Delta R.T. -0.000 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47

Tgt Ion:225 Resp: 80241
 Ion Ratio Lower Upper
 225 100
 223 63.2 31.9 95.7
 227 63.4 31.4 94.0

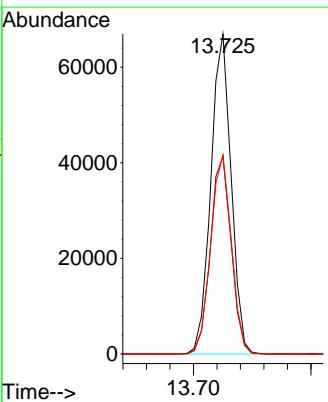


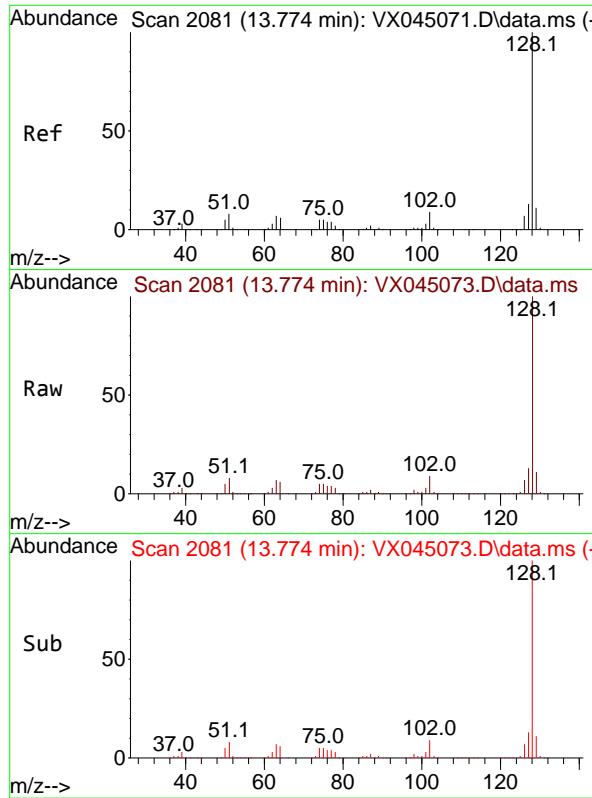


#95
 Naphthalene
 Concen: 168.538 ug/l
 RT: 13.774 min Scan# 2
 Delta R.T. -0.000 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47

Instrument : MSVOA_X
 ClientSampleId : VSTDICC150


Manual Integrations
APPROVED

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

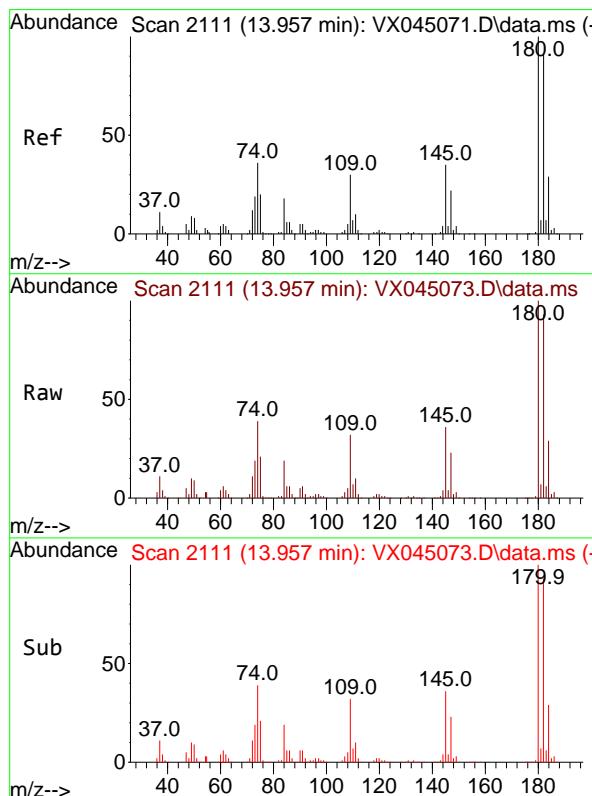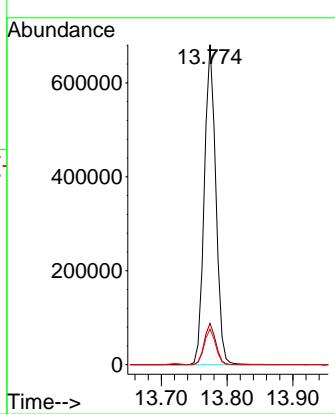

#96
 1,2,3-Trichlorobenzene
 Concen: 162.727 ug/l
 RT: 13.957 min Scan# 2111
 Delta R.T. -0.000 min
 Lab File: VX045073.D
 Acq: 28 Feb 2025 03:47

Tgt Ion:180 Resp: 222608
 Ion Ratio Lower Upper
 180 100
 182 95.7 47.5 142.6
 145 35.5 17.0 50.9

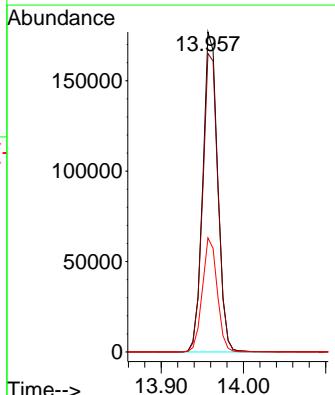

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045075.D
 Acq On : 28 Feb 2025 04:33
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

Quant Time: Feb 28 06:55:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.550	168	101603	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	184964	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	157797	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	69357	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	81288	50.297	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	100.600%	
35) Dibromofluoromethane	5.385	113	62880	50.841	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	101.680%	
50) Toluene-d8	8.647	98	225823	50.364	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	100.720%	
62) 4-Bromofluorobenzene	11.079	95	73162	49.240	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	98.480%	
Target Compounds						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	61303	47.933	ug/l	95
3) Chloromethane	1.306	50	76216	48.696	ug/l	94
4) Vinyl Chloride	1.373	62	76901	49.529	ug/l	97
5) Bromomethane	1.593	94	28193	46.190	ug/l	97
6) Chloroethane	1.660	64	30042	41.948	ug/l	99
7) Trichlorofluoromethane	1.867	101	101886	49.569	ug/l	98
8) Diethyl Ether	2.136	74	39113	48.651	ug/l	96
9) 1,1,2-Trichlorotrifluo...	2.312	101	59477	50.367	ug/l	100
10) Methyl Iodide	2.440	142	74585	50.541	ug/l	98
11) Tert butyl alcohol	2.989	59	73034	238.577	ug/l	98
12) 1,1-Dichloroethene	2.306	96	61885	49.568	ug/l	98
13) Acrolein	2.239	56	95989	271.255	ug/l	99
14) Allyl chloride	2.654	41	114875	51.691	ug/l	98
15) Acrylonitrile	3.068	53	209607	255.479	ug/l	99
16) Acetone	2.392	43	182119	242.877	ug/l	100
17) Carbon Disulfide	2.501	76	166105	49.952	ug/l	97
18) Methyl Acetate	2.709	43	90756	50.312	ug/l	99
19) Methyl tert-butyl Ether	3.117	73	222475	53.114	ug/l	99
20) Methylene Chloride	2.782	84	73731	49.639	ug/l	98
21) trans-1,2-Dichloroethene	3.081	96	63117	51.172	ug/l	98
22) Diisopropyl ether	3.763	45	243860	53.955	ug/l	97
23) Vinyl Acetate	3.721	43	1064817	282.313	ug/l	100
24) 1,1-Dichloroethane	3.605	63	129666	51.190	ug/l	100
25) 2-Butanone	4.562	43	298021	264.040	ug/l	98
26) 2,2-Dichloropropane	4.471	77	58694	49.401	ug/l	99
27) cis-1,2-Dichloroethene	4.483	96	78576	51.606	ug/l	100
28) Bromochloromethane	4.891	49	60849	50.399	ug/l	100
29) Tetrahydrofuran	5.007	42	195768	258.277	ug/l	99
30) Chloroform	5.086	83	126437	50.236	ug/l	98
31) Cyclohexane	5.464	56	110288	50.158	ug/l	98
32) 1,1,1-Trichloroethane	5.373	97	103546	50.939	ug/l	99
36) 1,1-Dichloropropene	5.684	75	82722	48.770	ug/l	99
37) Ethyl Acetate	4.714	43	112768	51.596	ug/l	99
38) Carbon Tetrachloride	5.672	117	85110	49.425	ug/l	99
39) Methylcyclohexane	7.372	83	103996	51.169	ug/l	98
40) Benzene	6.031	78	274206	51.195	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045075.D
 Acq On : 28 Feb 2025 04:33
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

Quant Time: Feb 28 06:55:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	63051	53.352	ug/l	99
42) 1,2-Dichloroethane	6.080	62	97821	50.718	ug/l	100
43) Isopropyl Acetate	6.342	43	175982	54.452	ug/l	100
44) Trichloroethene	7.122	130	61530	48.924	ug/l	99
45) 1,2-Dichloropropane	7.427	63	70350	51.086	ug/l	97
46) Dibromomethane	7.580	93	50284	51.661	ug/l	99
47) Bromodichloromethane	7.817	83	97236	50.930	ug/l	99
48) Methyl methacrylate	7.689	41	87582	54.016	ug/l	100
49) 1,4-Dioxane	7.665	88	35878	1049.007	ug/l	98
51) 4-Methyl-2-Pentanone	8.573	43	564197	259.995	ug/l	99
52) Toluene	8.714	92	160331	51.020	ug/l	99
53) t-1,3-Dichloropropene	8.976	75	86584	54.247	ug/l	99
54) cis-1,3-Dichloropropene	8.366	75	98146	52.732	ug/l	95
55) 1,1,2-Trichloroethane	9.146	97	64985	50.232	ug/l	99
56) Ethyl methacrylate	9.116	69	106405	54.109	ug/l	100
57) 1,3-Dichloropropane	9.305	76	114880	51.312	ug/l	99
58) 2-Chloroethyl Vinyl ether	8.238	63	264335	275.557	ug/l	99
59) 2-Hexanone	9.427	43	416731	265.049	ug/l	99
60) Dibromochloromethane	9.518	129	69492	51.374	ug/l	98
61) 1,2-Dibromoethane	9.610	107	66501	51.492	ug/l	99
64) Tetrachloroethene	9.268	164	50659	50.126	ug/l	96
65) Chlorobenzene	10.079	112	168885	50.580	ug/l	99
66) 1,1,1,2-Tetrachloroethane	10.159	131	56822	51.102	ug/l	98
67) Ethyl Benzene	10.189	91	300324	51.621	ug/l	100
68) m/p-Xylenes	10.299	106	220335	103.454	ug/l	99
69) o-Xylene	10.640	106	108836	50.668	ug/l	100
70) Styrene	10.652	104	181349	52.177	ug/l	100
71) Bromoform	10.799	173	44135	52.636	ug/l #	100
73) Isopropylbenzene	10.957	105	279278	51.589	ug/l	99
74) N-amyl acetate	10.841	43	144412	56.851	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	100800	50.741	ug/l	99
76) 1,2,3-Trichloropropane	11.238	75	80618m	49.940	ug/l	
77) Bromobenzene	11.195	156	64324	50.360	ug/l	100
78) n-propylbenzene	11.305	91	319235	52.203	ug/l	99
79) 2-Chlorotoluene	11.360	91	192150	49.338	ug/l	100
80) 1,3,5-Trimethylbenzene	11.451	105	225622	51.544	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.018	75	23943	50.757	ug/l	99
82) 4-Chlorotoluene	11.451	91	216511	51.009	ug/l	100
83) tert-Butylbenzene	11.713	119	227357	50.552	ug/l	100
84) 1,2,4-Trimethylbenzene	11.750	105	228729	51.932	ug/l	100
85) sec-Butylbenzene	11.890	105	283931	52.703	ug/l	100
86) p-Isopropyltoluene	12.006	119	229894	52.803	ug/l	100
87) 1,3-Dichlorobenzene	11.969	146	114778	50.372	ug/l	100
88) 1,4-Dichlorobenzene	12.036	146	115486	50.097	ug/l	99
89) n-Butylbenzene	12.329	91	204972	54.662	ug/l	99
90) Hexachloroethane	12.536	117	40844	51.866	ug/l	99
91) 1,2-Dichlorobenzene	12.335	146	116343	50.899	ug/l	100
92) 1,2-Dibromo-3-Chloropr...	12.938	75	20589	53.199	ug/l	99
93) 1,2,4-Trichlorobenzene	13.585	180	71368	54.834	ug/l	98
94) Hexachlorobutadiene	13.725	225	26697	50.032	ug/l	99
95) Naphthalene	13.774	128	275844	55.163	ug/l	100
96) 1,2,3-Trichlorobenzene	13.957	180	74211	54.049	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045075.D
Acq On : 28 Feb 2025 04:33
Operator : JC/MD
Sample : VSTDICV050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

Quant Time: Feb 28 06:55:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carbone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045075.D
Acq On : 28 Feb 2025 04:33
Operator : JC/MD
Sample : VSTDICV050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

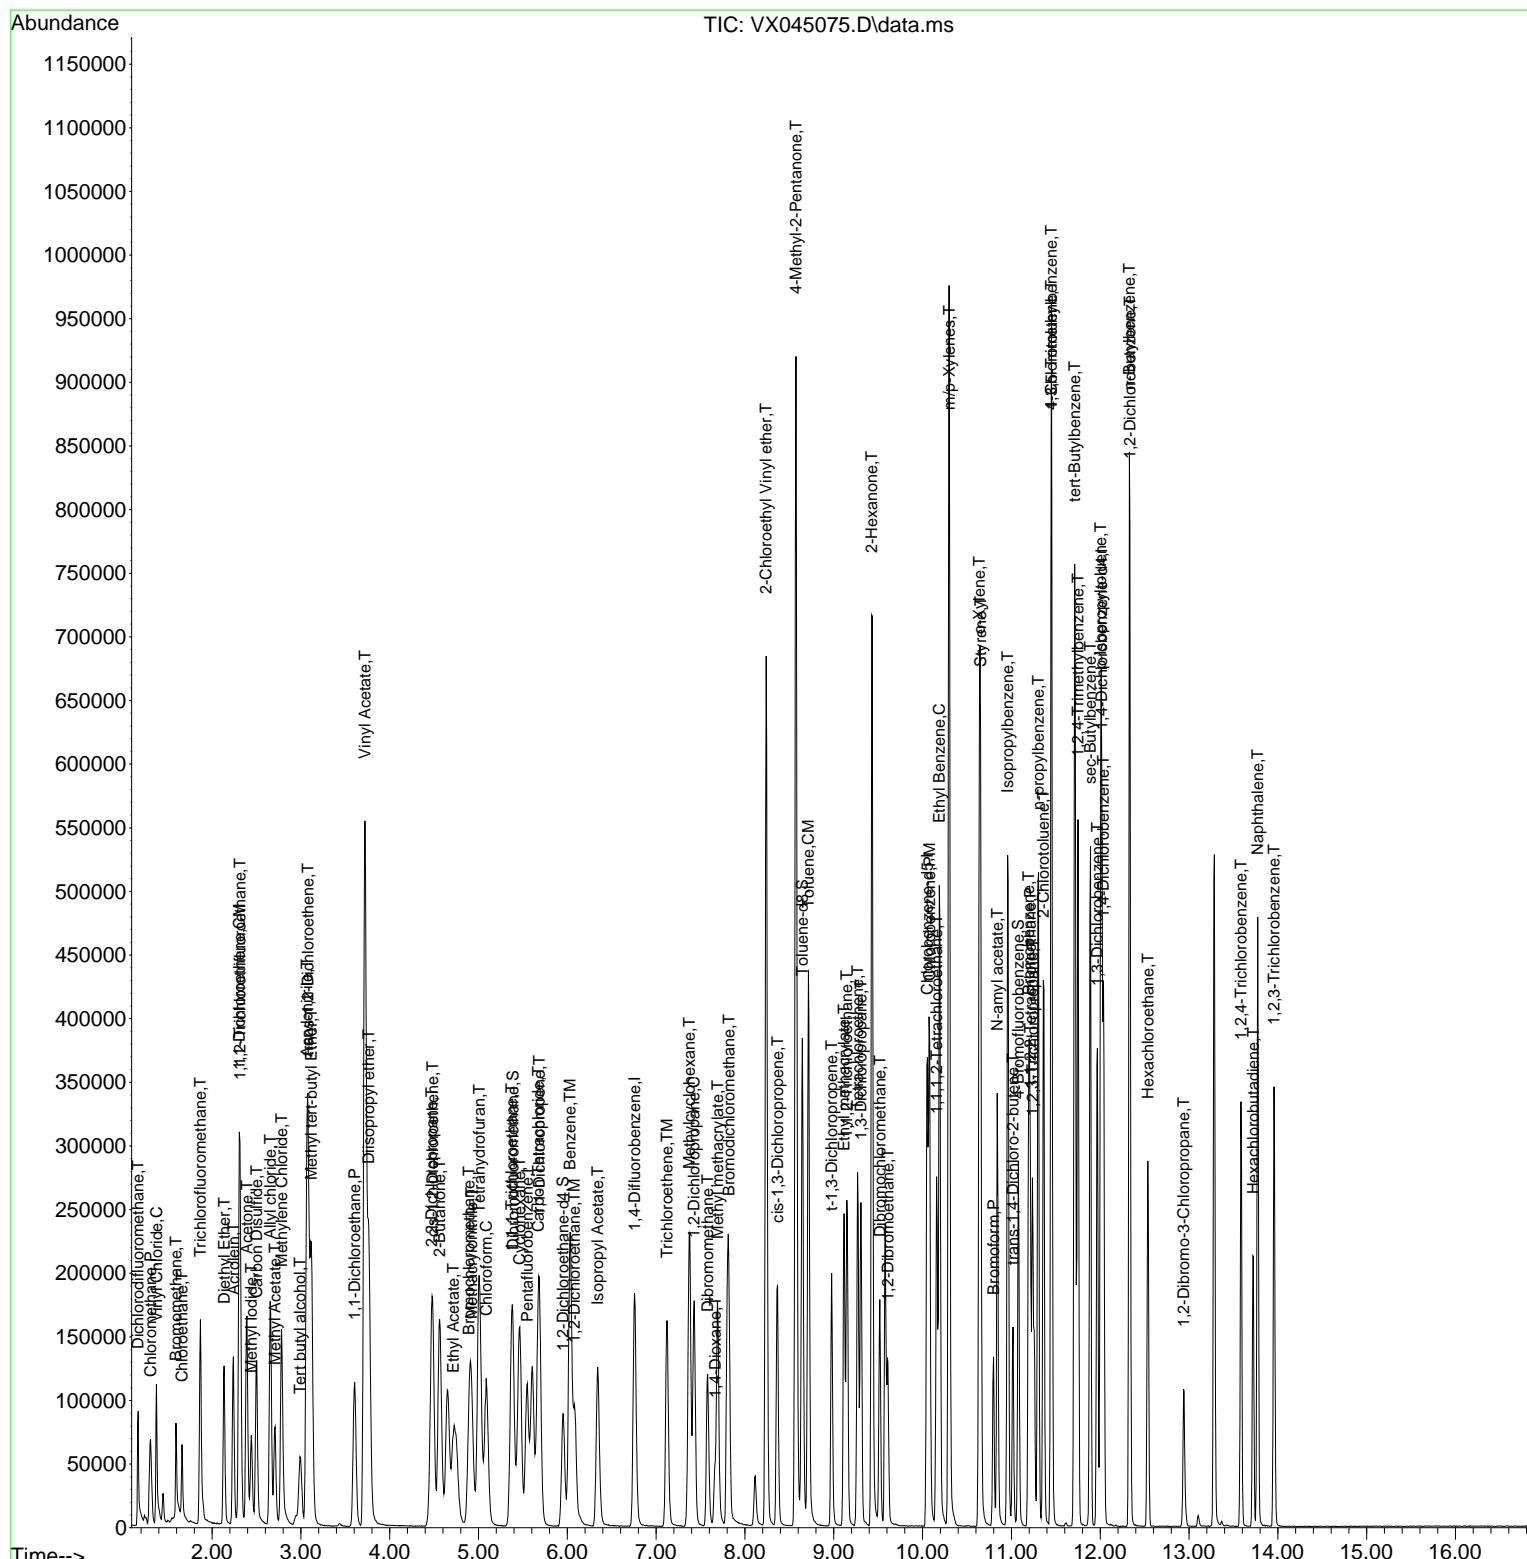







#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.550 min Scan# 7
 Delta R.T. -0.000 min
 Lab File: VX045075.D
 Acq: 28 Feb 2025 04:33

Instrument :
 MSVOA_X
 ClientSampleId :
 ICVX022825


Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

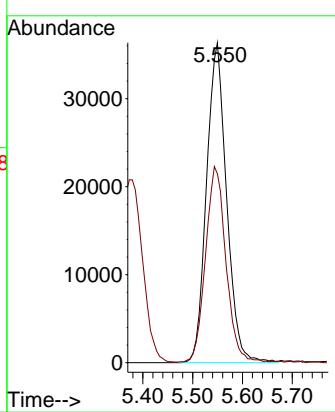

#2
 Dichlorodifluoromethane
 Concen: 47.933 ug/l
 RT: 1.166 min Scan# 13
 Delta R.T. -0.000 min
 Lab File: VX045075.D
 Acq: 28 Feb 2025 04:33


Tgt Ion: 85 Resp: 61303
 Ion Ratio Lower Upper
 85 100
 87 31.8 17.4 52.3

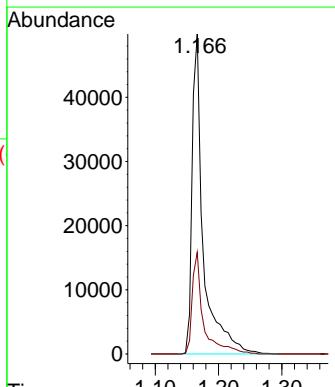



#3
Chloromethane
Concen: 48.696 ug/l
RT: 1.306 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825




Tgt Ion: 50 Resp: 76210
Ion Ratio Lower Upper
50 100
52 34.3 25.0 37.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#4
Vinyl Chloride
Concen: 49.529 ug/l
RT: 1.373 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion: 62 Resp: 76901
Ion Ratio Lower Upper
62 100
64 32.2 24.3 36.5



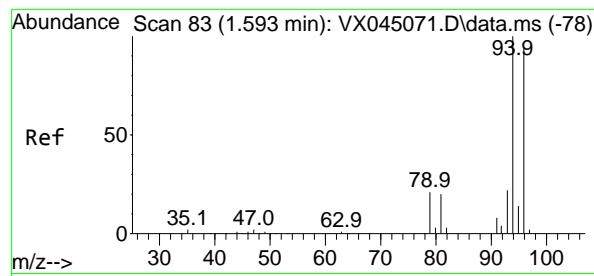

#5
Bromomethane
Concen: 46.190 ug/l
RT: 1.593 min Scan# 8
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825



Tgt Ion: 94 Resp: 28192
Ion Ratio Lower Upper
94 100
96 90.5 75.0 112.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

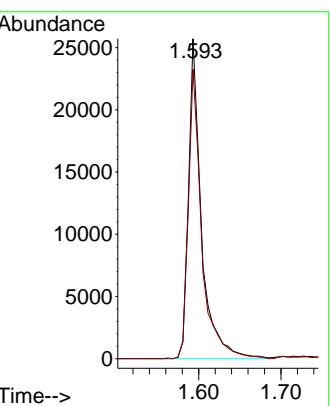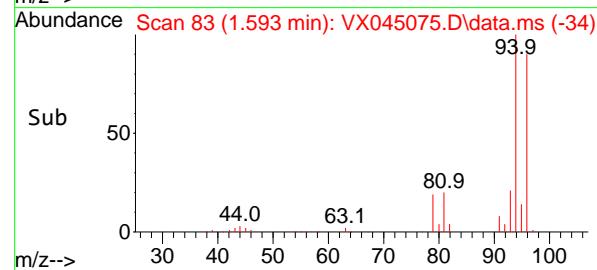

#6
Chloroethane
Concen: 41.948 ug/l
RT: 1.660 min Scan# 94
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Tgt Ion: 64 Resp: 30042
Ion Ratio Lower Upper
64 100
66 32.6 26.7 40.1

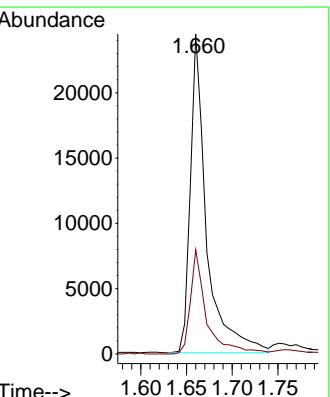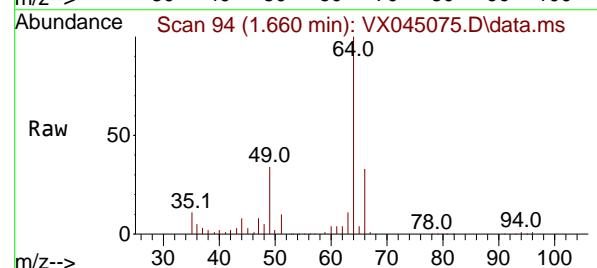



#7
Trichlorofluoromethane
Concen: 49.569 ug/l
RT: 1.867 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825



Tgt Ion: 101 Resp: 101880
Ion Ratio Lower Upper
101 100
103 66.4 52.1 78.1




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#8
Diethyl Ether
Concen: 48.651 ug/l
RT: 2.136 min Scan# 172
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Tgt Ion: 74 Resp: 39113
Ion Ratio Lower Upper
74 100
45 107.2 51.5 154.5

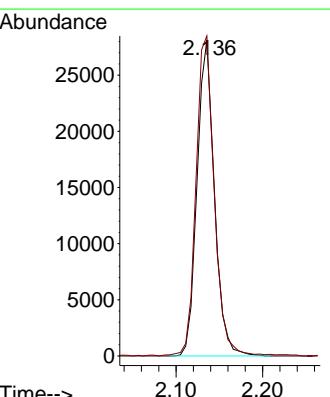



#9
1,1,2-Trichlorotrifluoroethane
Concen: 50.367 ug/l
RT: 2.312 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

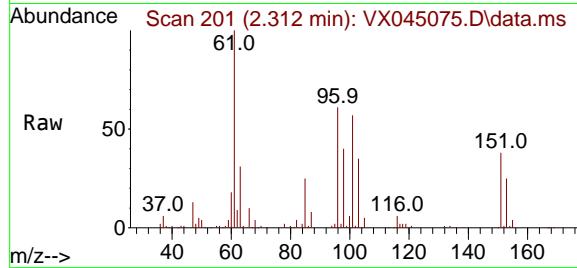

Tgt Ion:101 Resp: 5947
Ion Ratio Lower Upper
101 100
85 45.4 36.2 54.4
151 70.2 56.4 84.6




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

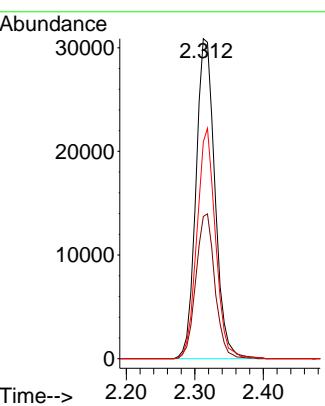

#10
Methyl Iodide
Concen: 50.541 ug/l
RT: 2.440 min Scan# 222
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Tgt Ion:142 Resp: 74585
Ion Ratio Lower Upper
142 100
127 46.3 35.4 53.2
141 14.3 11.6 17.4





#11
Tert butyl alcohol
Concen: 238.577 ug/l
RT: 2.989 min Scan# 3
Delta R.T. 0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVX022825



Tgt Ion: 59 Resp: 73034
Ion Ratio Lower Upper
59 100
57 10.4 7.8 11.8




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

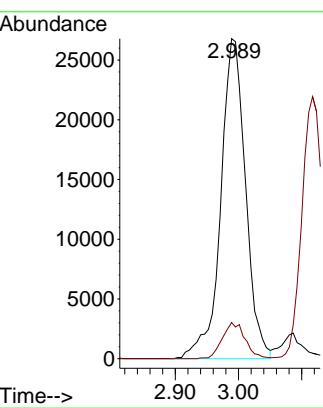

#12
1,1-Dichloroethene
Concen: 49.568 ug/l
RT: 2.306 min Scan# 200
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Tgt Ion: 96 Resp: 61885
Ion Ratio Lower Upper
96 100
61 171.3 134.6 202.0
98 63.2 51.0 76.6

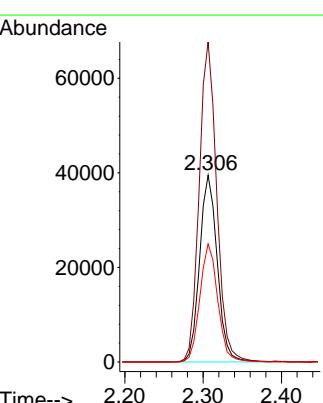



#13
Acrolein
Concen: 271.255 ug/l
RT: 2.239 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825



Tgt Ion: 56 Resp: 95989
Ion Ratio Lower Upper
56 100
55 69.5 56.2 84.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

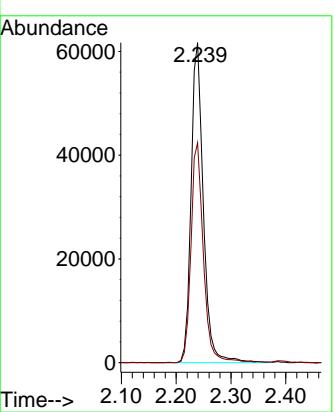

#14
Allyl chloride
Concen: 51.691 ug/l
RT: 2.654 min Scan# 257
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Tgt Ion: 41 Resp: 114875
Ion Ratio Lower Upper
41 100
39 66.3 53.8 80.8
76 33.0 25.2 37.8

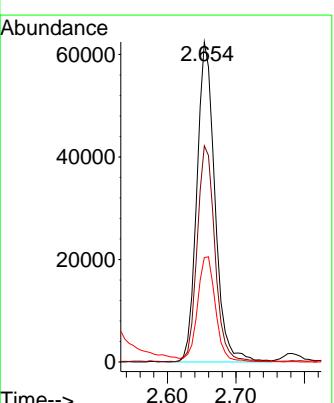



#15
Acrylonitrile
Concen: 255.479 ug/l
RT: 3.068 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33



Instrument : MSVOA_X
ClientSampleId : ICVVX022825




Tgt Ion: 53 Resp: 209601
Ion Ratio Lower Upper
53 100
52 83.8 66.2 99.2
51 35.8 29.0 43.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#16
Acetone
Concen: 242.877 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion: 43 Resp: 182119
Ion Ratio Lower Upper
43 100
58 30.5 24.2 36.4

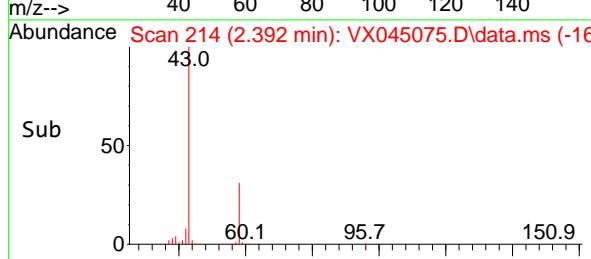



#17
Carbon Disulfide
Concen: 49.952 ug/l
RT: 2.501 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33



Instrument : MSVOA_X
ClientSampleId : ICVVX022825

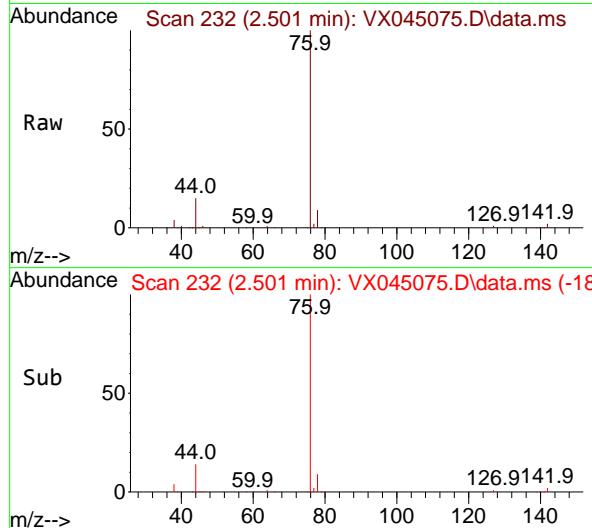

Tgt Ion: 76 Resp: 16610
Ion Ratio Lower Upper
76 100
78 9.3 6.6 9.8


Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

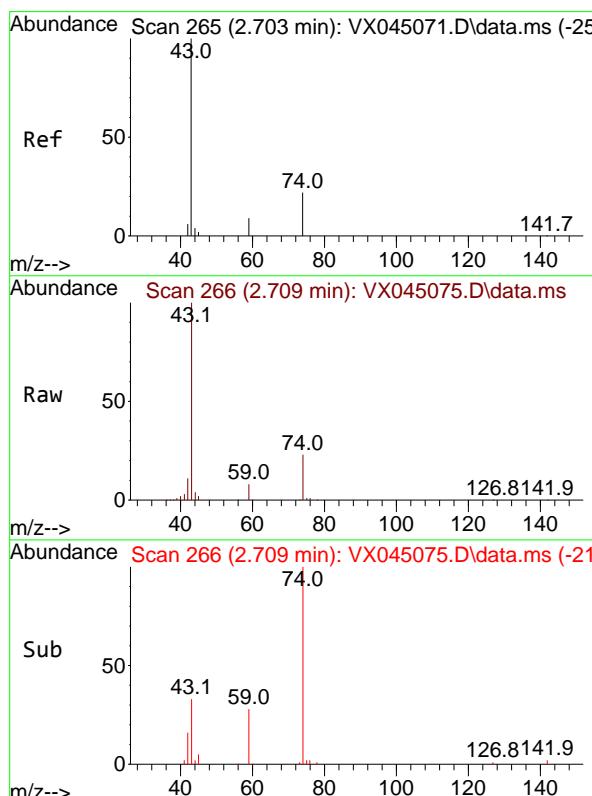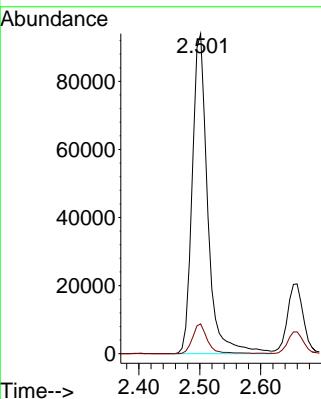

#18
Methyl Acetate
Concen: 50.312 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Tgt Ion: 43 Resp: 90756
Ion Ratio Lower Upper
43 100
74 22.1 17.4 26.2

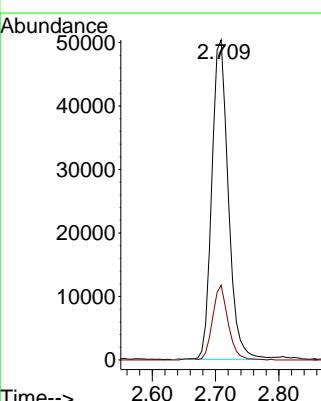



#19
Methyl tert-butyl Ether
Concen: 53.114 ug/l
RT: 3.117 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825




Tgt Ion: 73 Resp: 22247
Ion Ratio Lower Upper
73 100
57 22.7 18.5 27.7

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

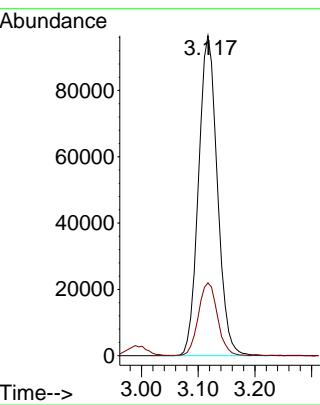


#20
Methylene Chloride
Concen: 49.639 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion: 84 Resp: 73731
Ion Ratio Lower Upper
84 100
49 129.3 106.5 159.7
51 39.1 32.1 48.1
86 61.7 50.0 75.0

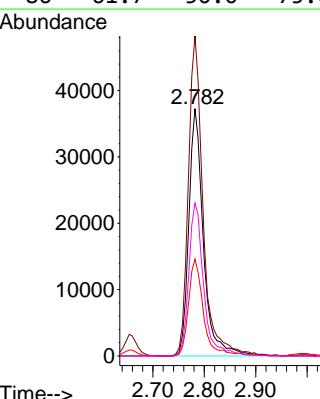



#21
trans-1,2-Dichloroethene
Concen: 51.172 ug/l
RT: 3.081 min Scan# 3
Delta R.T. -0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825




Tgt Ion: 96 Resp: 6311
Ion Ratio Lower Upper
96 100
61 145.2 117.0 175.4
98 64.4 53.4 80.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

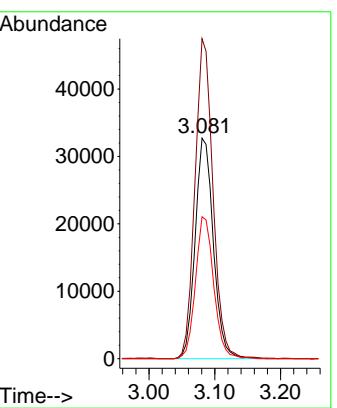


#22
Diisopropyl ether
Concen: 53.955 ug/l
RT: 3.763 min Scan# 439
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33



Tgt Ion: 45 Resp: 243860
Ion Ratio Lower Upper
45 100
43 71.9 54.9 82.3
87 25.8 21.0 31.4
59 11.6 8.7 13.1

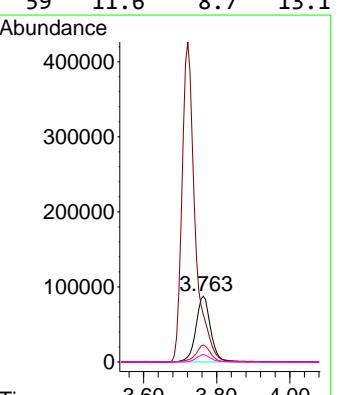



#23

Vinyl Acetate

Concen: 282.313 ug/l

RT: 3.721 min Scan# 413

Delta R.T. -0.000 min

Lab File: VX045075.D



Acq: 28 Feb 2025 04:33

Instrument:

MSVOA_X

ClientSampleId :



ICVVX022825

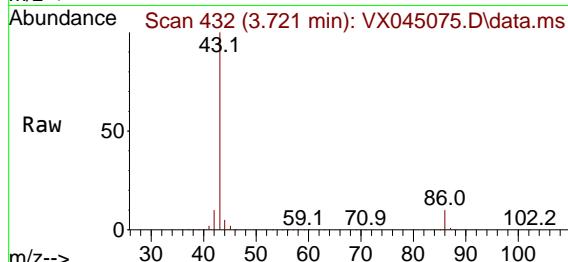


Tgt Ion: 43 Resp: 106481
 Ion Ratio Lower Upper
 43 100
 86 10.0 8.1 12.1

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

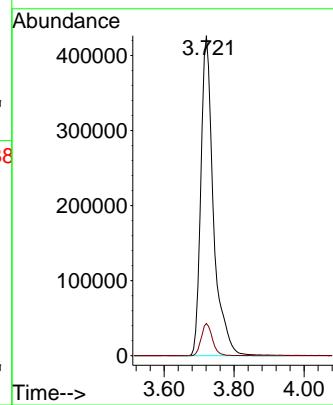


#24
 1,1-Dichloroethane
 Concen: 51.190 ug/l
 RT: 3.605 min Scan# 413
 Delta R.T. -0.000 min
 Lab File: VX045075.D
 Acq: 28 Feb 2025 04:33

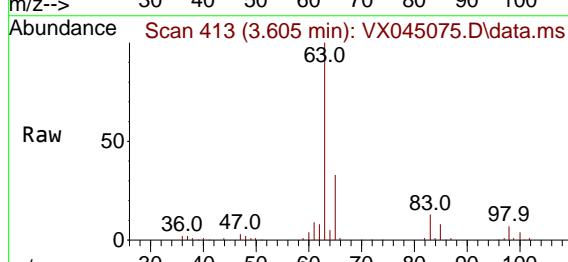


Tgt Ion: 63 Resp: 129666
 Ion Ratio Lower Upper
 63 100
 98 6.8 3.4 10.2
 100 4.1 2.1 6.5

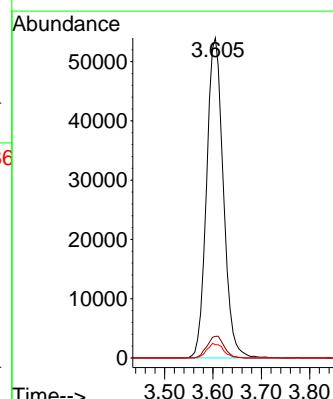

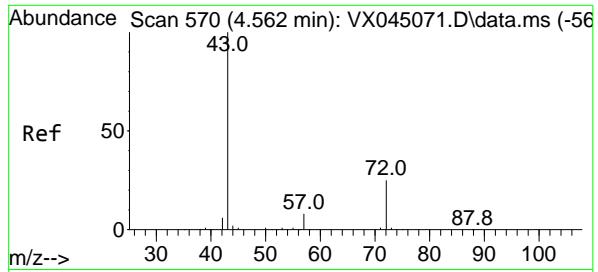

#25
2-Butanone
Concen: 264.040 ug/l
RT: 4.562 min Scan# 51
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

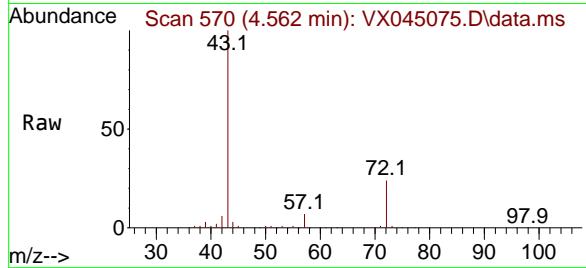

Tgt Ion: 43 Resp: 29802
Ion Ratio Lower Upper
43 100
72 24.1 20.0 30.0



Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#26
2,2-Dichloropropane
Concen: 49.401 ug/l
RT: 4.471 min Scan# 555
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Tgt Ion: 77 Resp: 58694
Ion Ratio Lower Upper
77 100
97 24.2 12.4 37.0

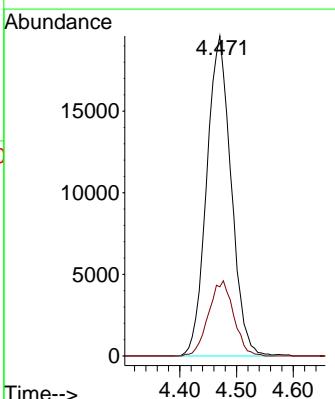



#27
cis-1,2-Dichloroethene
Concen: 51.606 ug/l
RT: 4.483 min Scan# 51
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825




Tgt Ion: 96 Resp: 78570
Ion Ratio Lower Upper
96 100
61 141.2 0.0 283.2
98 63.8 0.0 128.0

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

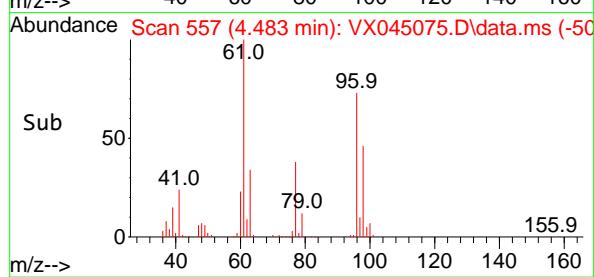


#28
Bromochloromethane
Concen: 50.399 ug/l
RT: 4.891 min Scan# 624
Delta R.T. -0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion: 49 Resp: 60849
Ion Ratio Lower Upper
49 100
129 1.7 0.0 3.4
130 70.0 56.1 84.1





#29
Tetrahydrofuran
Concen: 258.277 ug/l
RT: 5.007 min Scan# 6
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVX022825




Tgt Ion: 42 Resp: 19576
Ion Ratio Lower Upper
42 100
72 42.0 34.1 51.1
71 38.9 31.4 47.0

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#30
Chloroform
Concen: 50.236 ug/l
RT: 5.086 min Scan# 656
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion: 83 Resp: 126437
Ion Ratio Lower Upper
83 100
85 62.4 51.4 77.2



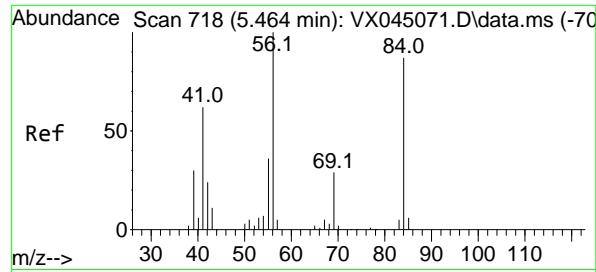




#31
Cyclohexane
Concen: 50.158 ug/l
RT: 5.464 min Scan# 718
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33
Instrument: MSVOA_X
ClientSampleId : ICVX022825




Tgt Ion: 56 Resp: 110288
Ion Ratio Lower Upper
56 100
69 28.8 23.4 35.2
84 84.6 69.4 104.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

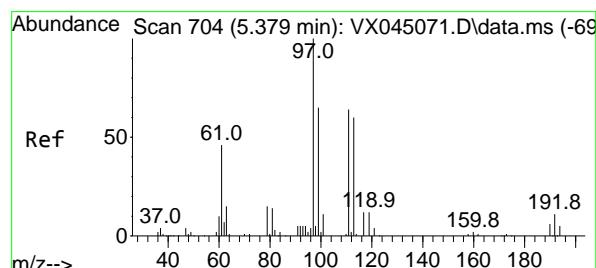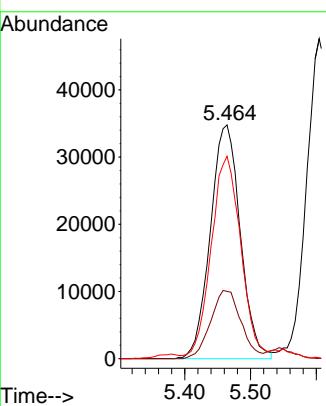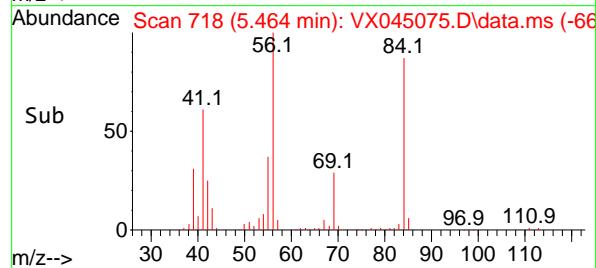


#32
1,1,1-Trichloroethane
Concen: 50.939 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion: 97 Resp: 103546
Ion Ratio Lower Upper
97 100
99 64.0 51.6 77.4
61 46.7 38.4 57.6

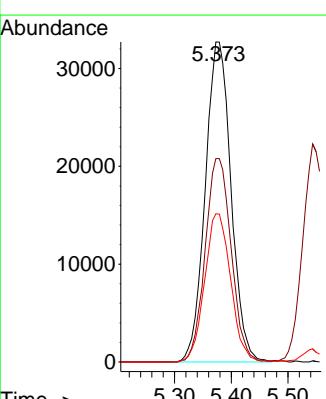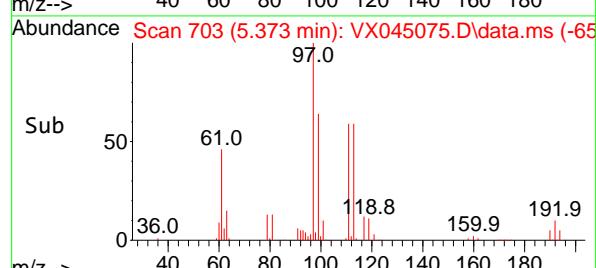



#33
1,2-Dichloroethane-d4
Concen: 50.297 ug/l
RT: 5.952 min Scan# 7
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825




Tgt Ion: 65 Resp: 81288
Ion Ratio Lower Upper
65 100
67 53.1 0.0 106.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

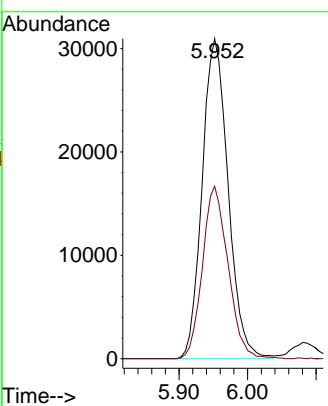


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion:114 Resp: 184964
Ion Ratio Lower Upper
114 100
63 22.7 0.0 41.8
88 16.3 0.0 32.8

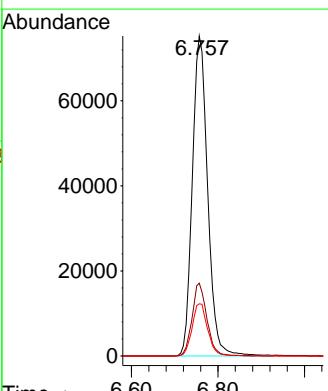






#35
Dibromofluoromethane
Concen: 50.841 ug/l
RT: 5.385 min Scan# 7
Instrument : MSVOA_X
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion:113 Resp: 62880
Ion Ratio Lower Upper
113 100
111 102.6 81.8 122.6
192 17.8 14.3 21.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

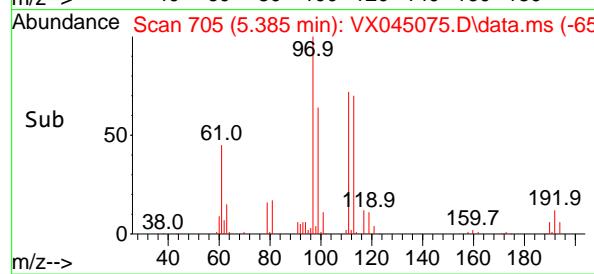


#36
1,1-Dichloropropene
Concen: 48.770 ug/l
RT: 5.684 min Scan# 754
Delta R.T. -0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33



Tgt Ion: 75 Resp: 82722
Ion Ratio Lower Upper
75 100
110 34.3 16.9 50.6
77 31.2 24.5 36.7



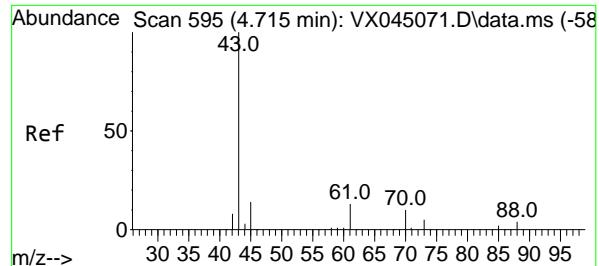

#37

Ethyl Acetate


Concen: 51.596 ug/l

RT: 4.714 min Scan# 5

Delta R.T. -0.000 min

Lab File: VX045075.D

Acq: 28 Feb 2025 04:33

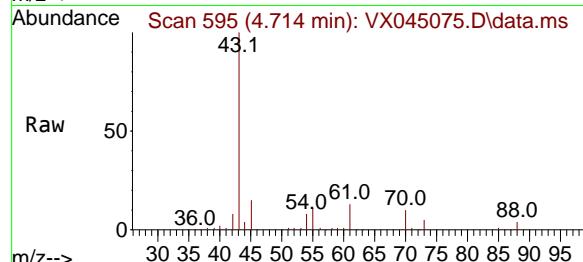

Tgt Ion: 43 Resp: 112763

Ion Ratio Lower Upper

43 100

61 13.3 10.8 16.2

70 10.1 7.7 11.5

Instrument:

MSVOA_X




ClientSampleId :

ICVVX022825


Manual Integrations**APPROVED**

Reviewed By :John Carlone 02/28/2025



Supervised By :Mahesh Dadoda 02/28/2025

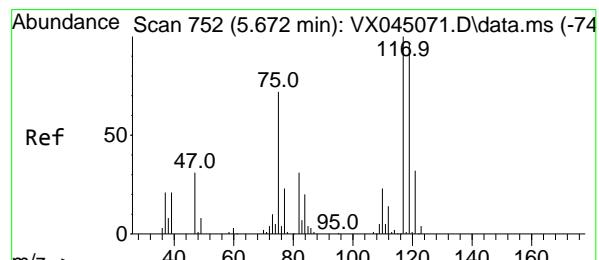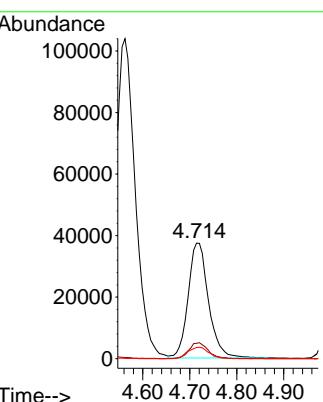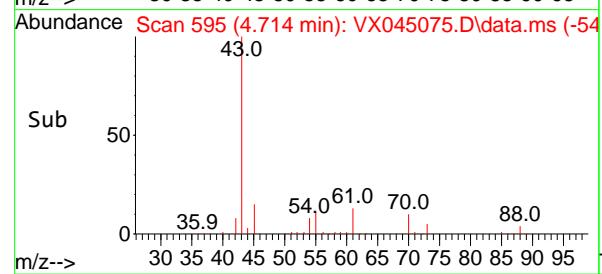


#38
Carbon Tetrachloride
Concen: 49.425 ug/l
RT: 5.672 min Scan# 752
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

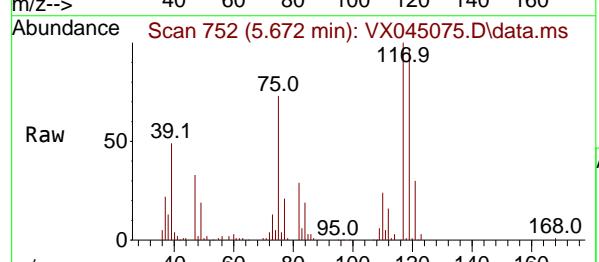


Tgt Ion:117 Resp: 85110
Ion Ratio Lower Upper
117 100
119 95.6 76.7 115.1
121 29.5 25.5 38.3

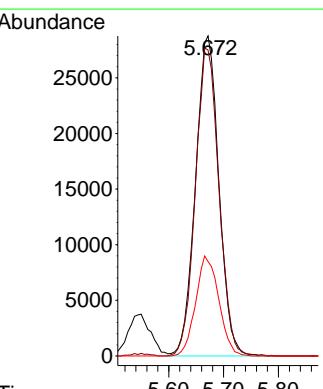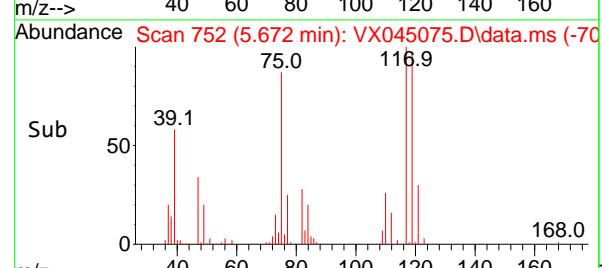



#39
Methylcyclohexane
Concen: 51.169 ug/l
RT: 7.372 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33



Instrument : MSVOA_X
ClientSampleId : ICVVX022825

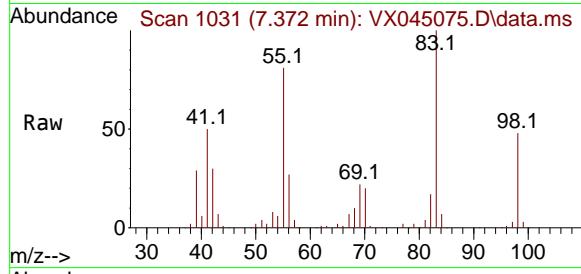


Tgt Ion: 83 Resp: 103990
Ion Ratio Lower Upper
83 100
55 80.7 63.0 94.4
98 47.9 39.7 59.5

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

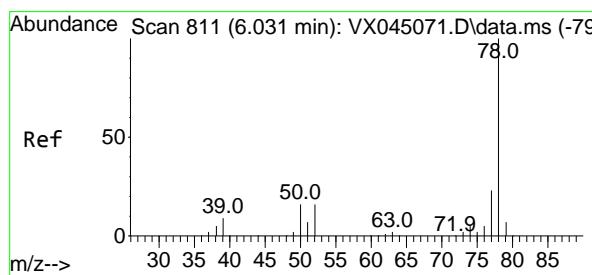


#40
Benzene
Concen: 51.195 ug/l
RT: 6.031 min Scan# 811
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

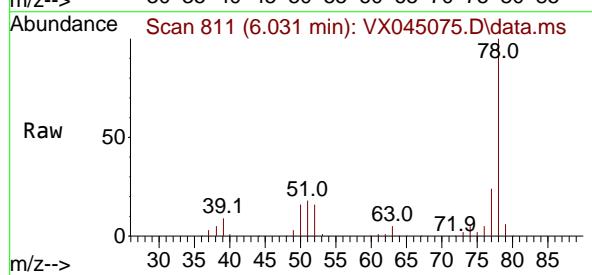


Tgt Ion: 78 Resp: 274206
Ion Ratio Lower Upper
78 100
77 24.0 18.8 28.2

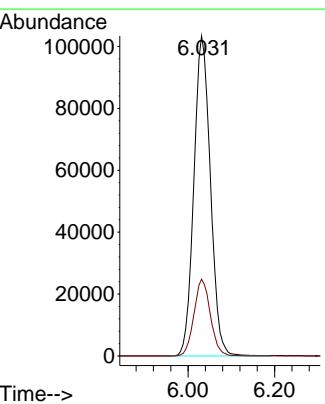



#41
Methacrylonitrile
Concen: 53.352 ug/l
RT: 4.922 min Scan# 63051
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825

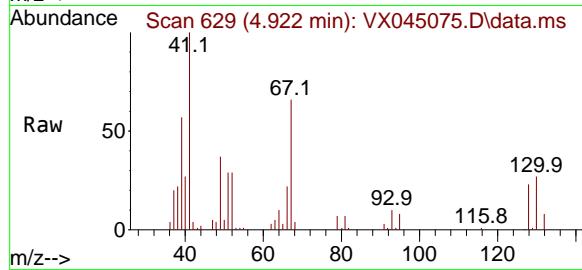

Tgt Ion: 41 Resp: 63051
Ion Ratio Lower Upper
41 100
39 55.0 44.6 67.0
67 68.1 53.9 80.9
52 30.0 23.3 34.9




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#42
1,2-Dichloroethane
Concen: 50.718 ug/l
RT: 6.080 min Scan# 819
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Tgt Ion: 62 Resp: 97821
Ion Ratio Lower Upper
62 100
98 9.1 0.0 18.2





#43
Isopropyl Acetate
Concen: 54.452 ug/l
RT: 6.342 min Scan# 8
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825




Tgt Ion: 43 Resp: 17598
Ion Ratio Lower Upper
43 100
61 18.5 14.9 22.3
87 11.8 9.4 14.2

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#44
Trichloroethene
Concen: 48.924 ug/l
RT: 7.122 min Scan# 990
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion:130 Resp: 61530
Ion Ratio Lower Upper
130 100
95 101.1 0.0 205.0





#45
1,2-Dichloropropane
Concen: 51.086 ug/l
RT: 7.427 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825




Tgt Ion: 63 Resp: 70350
Ion Ratio Lower Upper
63 100
65 29.2 24.7 37.1

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#46
Dibromomethane
Concen: 51.661 ug/l
RT: 7.580 min Scan# 1065
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion: 93 Resp: 50284
Ion Ratio Lower Upper
93 100
95 82.8 65.8 98.8
174 89.4 72.2 108.2





#47
 Bromodichloromethane
 Concen: 50.930 ug/l
 RT: 7.817 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX045075.D
 Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
 ClientSampleId : ICVVX022825



Tgt Ion: 83 Resp: 97230
 Ion Ratio Lower Upper
 83 100
 85 63.0 51.1 76.7
 127 7.4 6.4 9.6




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

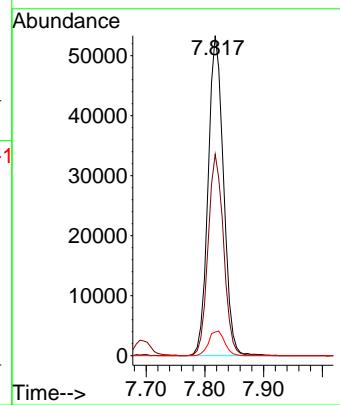

#48
 Methyl methacrylate
 Concen: 54.016 ug/l
 RT: 7.689 min Scan# 1083
 Delta R.T. -0.000 min
 Lab File: VX045075.D
 Acq: 28 Feb 2025 04:33


Tgt Ion: 41 Resp: 87582
 Ion Ratio Lower Upper
 41 100
 69 78.5 63.0 94.6
 39 59.4 47.5 71.3

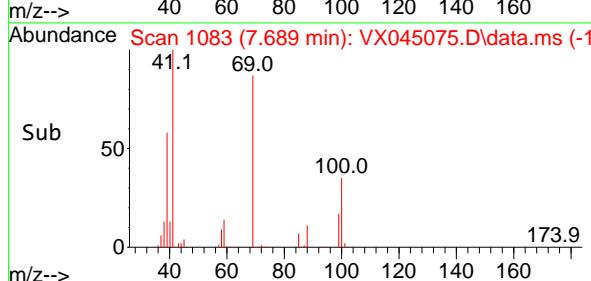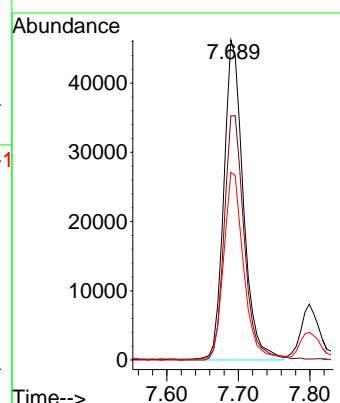



#49
1,4-Dioxane
Concen: 1049.007 ug/l
RT: 7.665 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825




Tgt Ion: 88 Resp: 35873
Ion Ratio Lower Upper
88 100
43 34.3 28.7 43.1
58 70.8 55.8 83.8

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

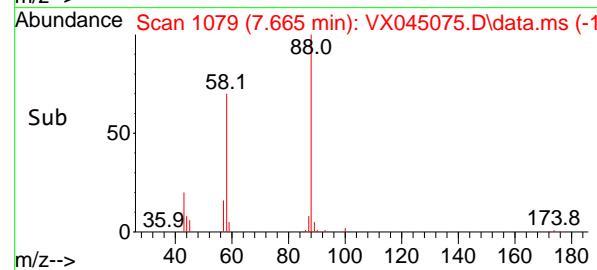


#50
Toluene-d8
Concen: 50.364 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion: 98 Resp: 225823
Ion Ratio Lower Upper
98 100
100 65.6 52.0 78.0

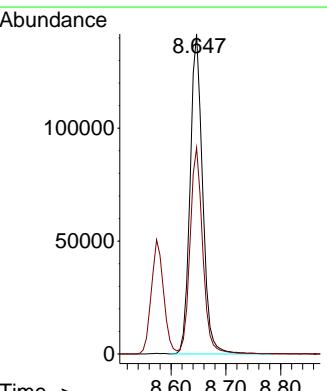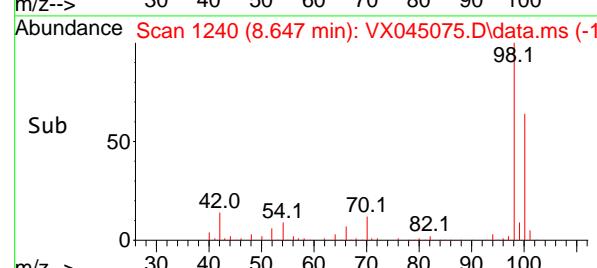



#51
4-Methyl-2-Pentanone
Concen: 259.995 ug/l
RT: 8.573 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825



Tgt Ion: 43 Resp: 56419
Ion Ratio Lower Upper
43 100
58 37.3 29.2 43.8




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#52
Toluene
Concen: 51.020 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Tgt Ion: 92 Resp: 160331
Ion Ratio Lower Upper
92 100
91 175.1 138.9 208.3









#53
t-1,3-Dichloropropene
Concen: 54.247 ug/l
RT: 8.976 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Instrument : MSVOA_X
ClientSampleId : ICVVX022825

Tgt Ion: 75 Resp: 86584
Ion Ratio Lower Upper
75 100
77 32.7 26.5 39.7




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

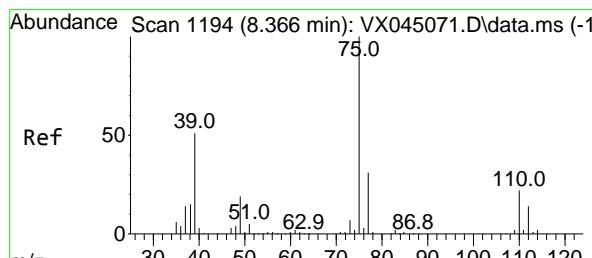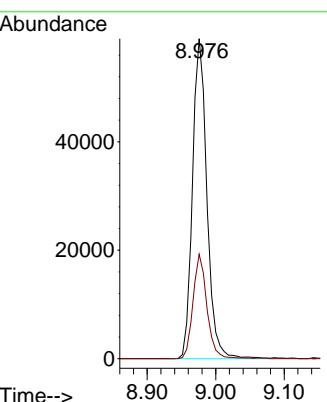

#54
cis-1,3-Dichloropropene
Concen: 52.732 ug/l
RT: 8.366 min Scan# 1194
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Tgt Ion: 75 Resp: 98146
Ion Ratio Lower Upper
75 100
77 32.2 24.7 37.1
39 56.0 40.7 61.1

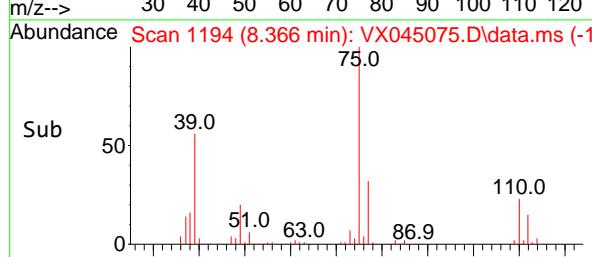



#55
1,1,2-Trichloroethane
Concen: 50.232 ug/l
RT: 9.146 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825




Tgt Ion: 97 Resp: 64989
Ion Ratio Lower Upper
97 100
83 87.8 69.4 104.2
85 55.6 44.1 66.1
99 62.1 50.7 76.1

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

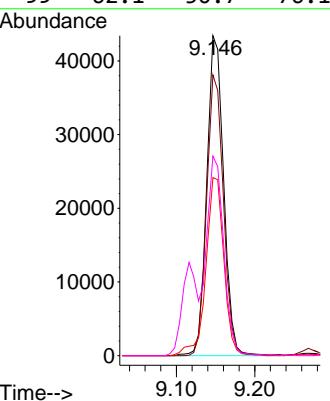


#56
Ethyl methacrylate
Concen: 54.109 ug/l
RT: 9.116 min Scan# 1317
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion: 69 Resp: 106405
Ion Ratio Lower Upper
69 100
41 71.5 57.0 85.4
39 43.2 34.2 51.4

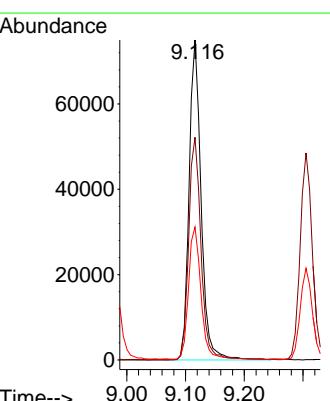



#57
1,3-Dichloropropane
Concen: 51.312 ug/l
RT: 9.305 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825



Tgt Ion: 76 Resp: 114880
Ion Ratio Lower Upper
76 100
78 32.5 25.5 38.3



Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

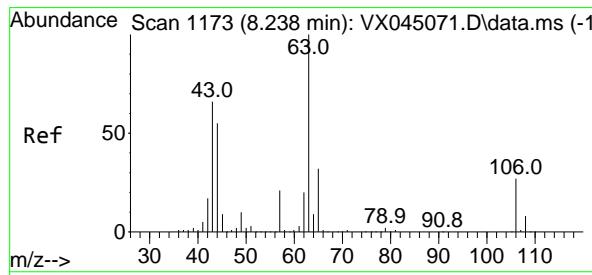

#58
2-Chloroethyl Vinyl ether
Concen: 275.557 ug/l
RT: 8.238 min Scan# 1173
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Tgt Ion: 63 Resp: 264335
Ion Ratio Lower Upper
63 100
106 26.5 21.5 32.3

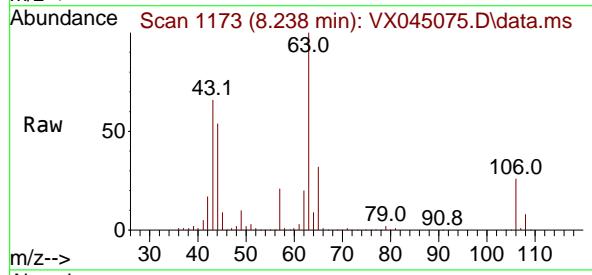



#59
2-Hexanone
Concen: 265.049 ug/l
RT: 9.427 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument : MSVOA_X
ClientSampleId : ICVVX022825

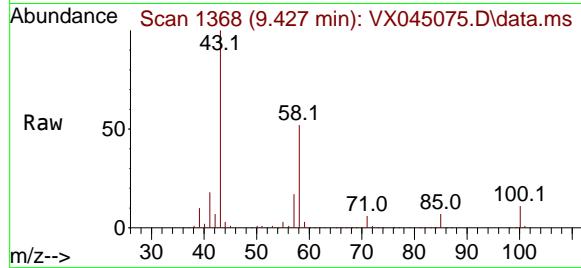

Tgt Ion: 43 Resp: 41673
Ion Ratio Lower Upper
43 100
58 52.2 25.9 77.6




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#60
Dibromochloromethane
Concen: 51.374 ug/l
RT: 9.518 min Scan# 1383
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Tgt Ion:129 Resp: 69492
Ion Ratio Lower Upper
129 100
127 78.6 38.5 115.5





#61
1,2-Dibromoethane
Concen: 51.492 ug/l
RT: 9.610 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33



Instrument : MSVOA_X
ClientSampleId : ICVVX022825



Tgt Ion:107 Resp: 6650
Ion Ratio Lower Upper
107 100
109 93.8 76.1 114.1



Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025





#62
4-Bromofluorobenzene
Concen: 49.240 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Tgt Ion: 95 Resp: 73162
Ion Ratio Lower Upper
95 100
174 74.0 0.0 148.2
176 71.3 0.0 141.4

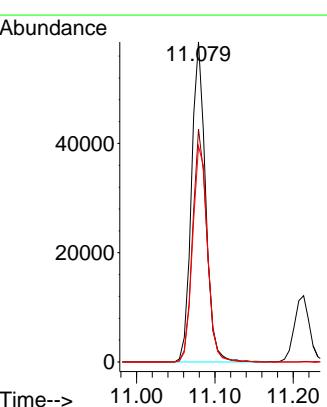

Abundance Scan 1639 (11.079 min): VX045075.D\data.ms (-1)

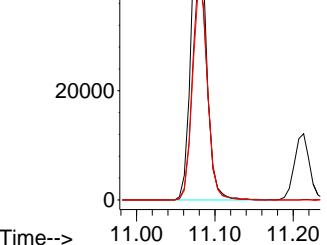


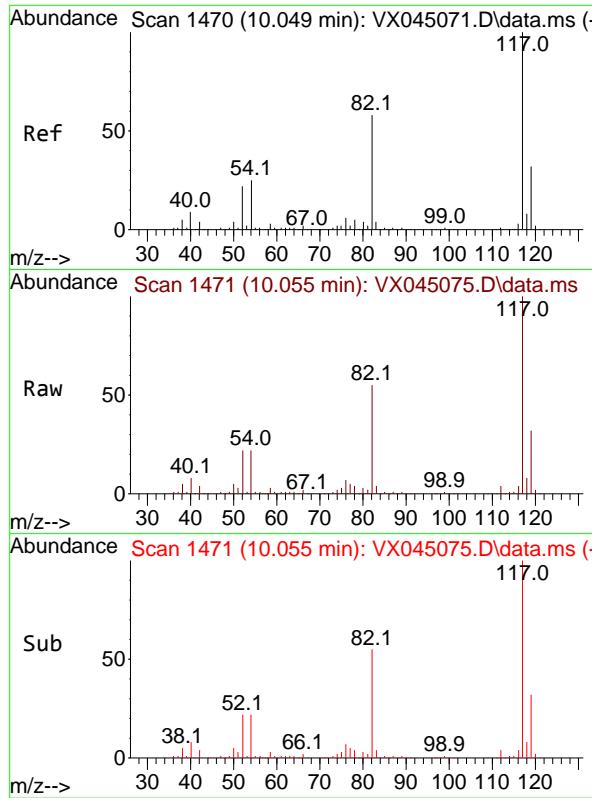


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Instrument : MSVOA_X
ClientSampleId : ICVVX022825


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

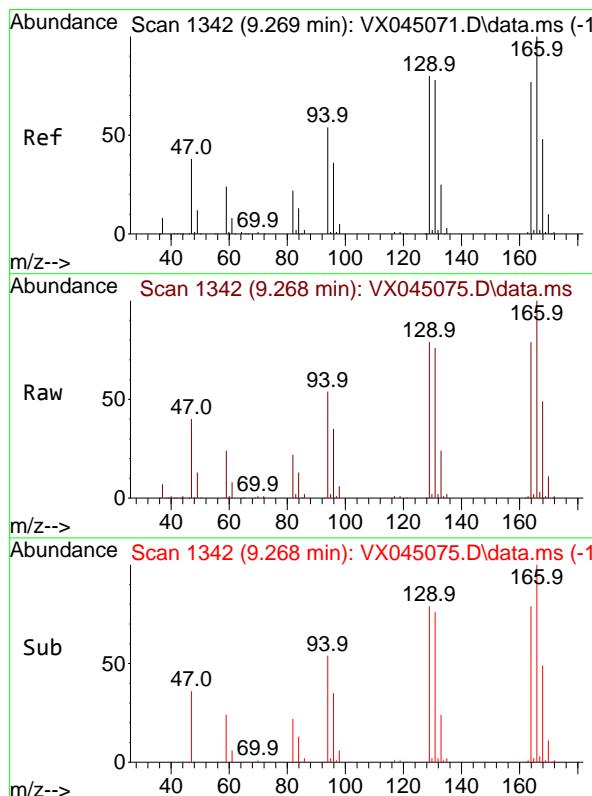

#64
Tetrachloroethene
Concen: 50.126 ug/l
RT: 9.268 min Scan# 1342
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Tgt Ion:164 Resp: 50659
Ion Ratio Lower Upper
164 100
166 126.0 103.6 155.4
129 99.0 82.7 124.1
131 95.9 80.5 120.7




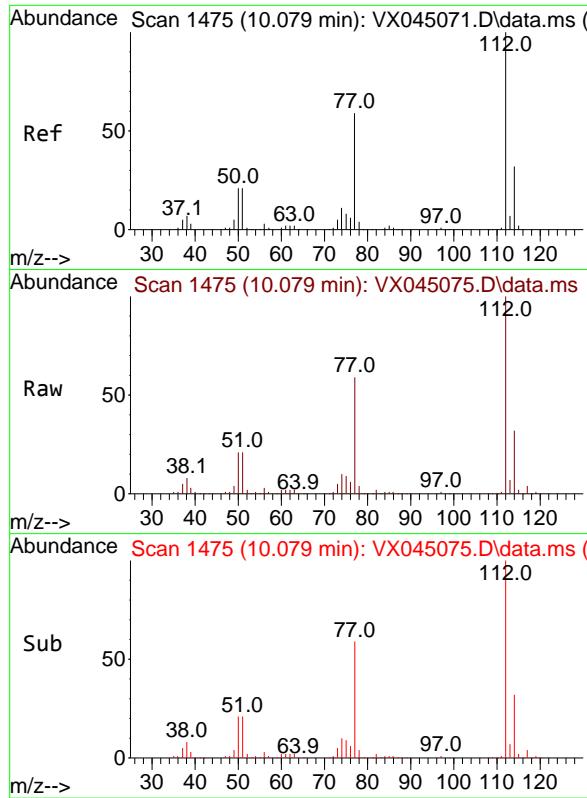


#65
Chlorobenzene
Concen: 50.580 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Instrument : MSVOA_X
ClientSampleId : ICVVX022825


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

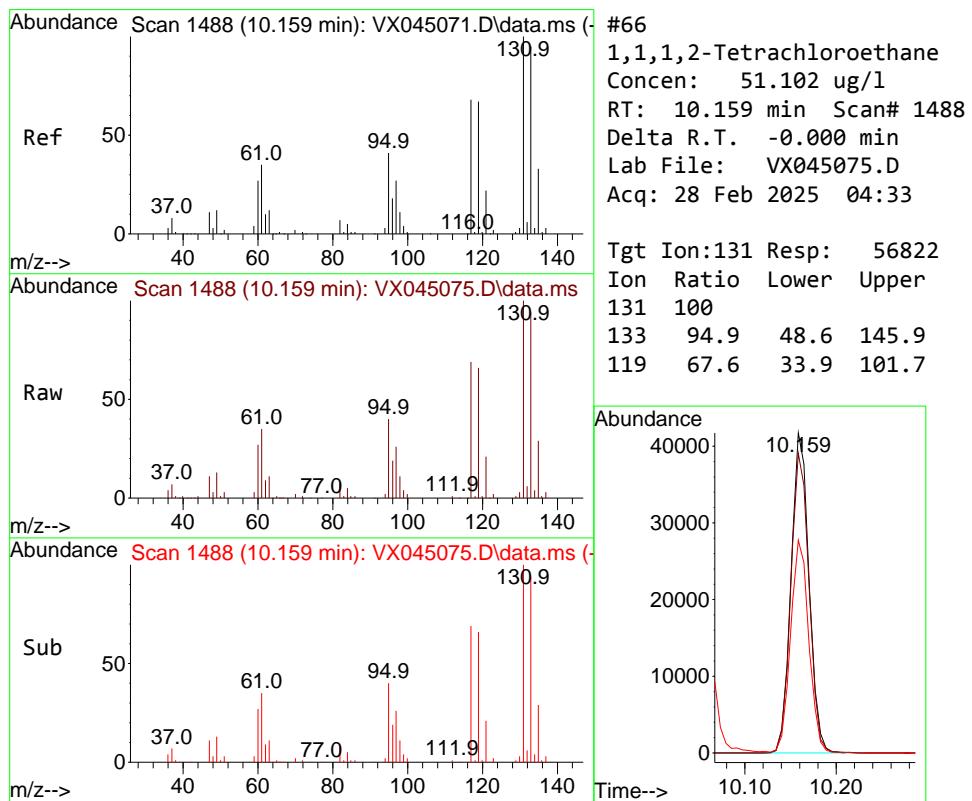



#66
1,1,1,2-Tetrachloroethane
Concen: 51.102 ug/l
RT: 10.159 min Scan# 1488
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Tgt Ion:131 Resp: 56822
Ion Ratio Lower Upper
131 100
133 94.9 48.6 145.9
119 67.6 33.9 101.7







#67
 Ethyl Benzene
 Concen: 51.621 ug/l
 RT: 10.189 min Scan# 1493
 Delta R.T. -0.000 min
 Lab File: VX045075.D
 Acq: 28 Feb 2025 04:33
Instrument: MSVOA_X
ClientSampleId : ICVVX022825

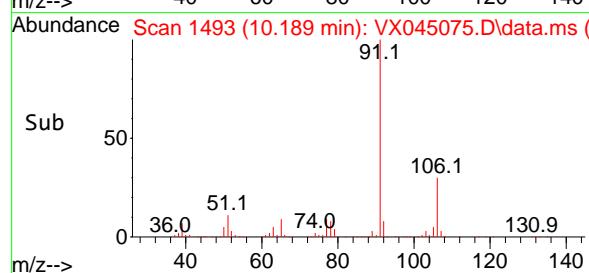


Tgt Ion: 91 Resp: 300324
 Ion Ratio Lower Upper
 91 100
 106 30.0 23.9 35.9

Manual Integrations
APPROVED



Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025




#68
 m/p-Xylenes
 Concen: 103.454 ug/l
 RT: 10.299 min Scan# 1511
 Delta R.T. -0.000 min
 Lab File: VX045075.D
 Acq: 28 Feb 2025 04:33




Tgt Ion:106 Resp: 220335
 Ion Ratio Lower Upper
 106 100
 91 207.8 165.4 248.0








#69
o-Xylene
Concen: 50.668 ug/l
RT: 10.640 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33
Instrument : MSVOA_X
ClientSampleId : ICVVX022825




Tgt Ion:106 Resp: 108830
Ion Ratio Lower Upper
106 100
91 220.5 109.9 329.6

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#70
Styrene
Concen: 52.177 ug/l
RT: 10.652 min Scan# 1569
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion:104 Resp: 181349
Ion Ratio Lower Upper
104 100
78 52.8 42.2 63.4
103 55.1 43.8 65.8





#71
Bromoform
Concen: 52.636 ug/l
RT: 10.799 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825



Tgt Ion:173 Resp: 44139
Ion Ratio Lower Upper
173 100
175 49.3 24.6 73.6
254 0.0 0.0 0.0



Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Tgt Ion:152 Resp: 69357
Ion Ratio Lower Upper
152 100
115 86.9 44.2 132.6
150 174.3 0.0 349.0







Abundance



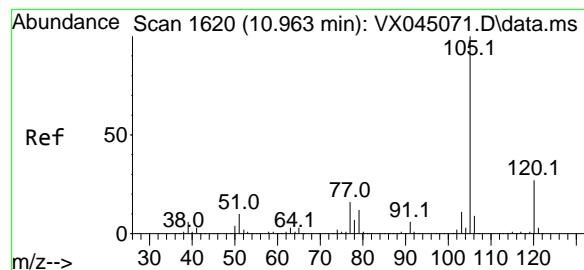


#73
Isopropylbenzene
Concen: 51.589 ug/l
RT: 10.957 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

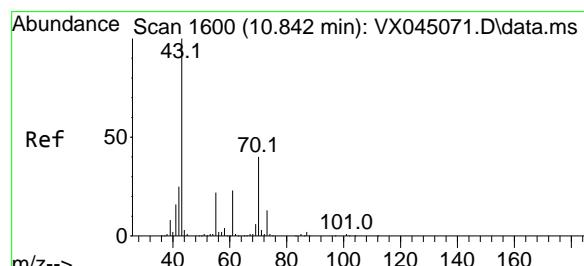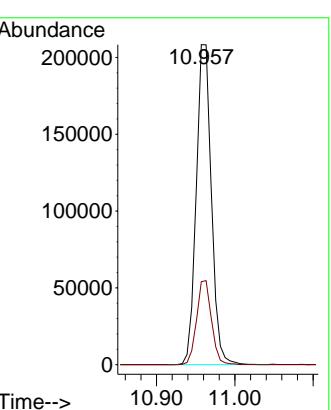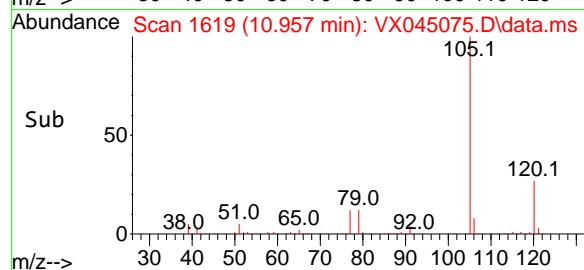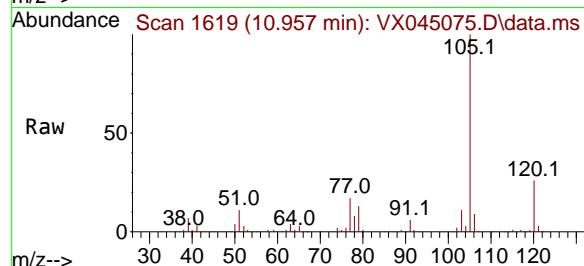


#74
N-amyl acetate
Concen: 56.851 ug/l
RT: 10.841 min Scan# 1600
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


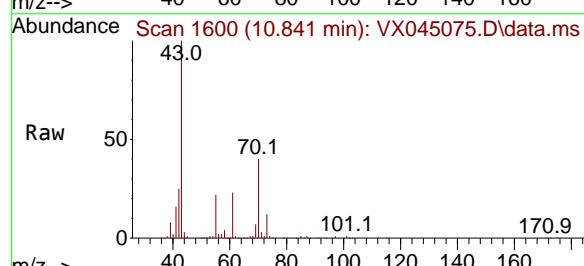


Tgt Ion: 43 Resp: 144412
Ion Ratio Lower Upper
43 100
70 39.5 31.8 47.6
55 22.3 18.3 27.5
61 23.0 18.3 27.5

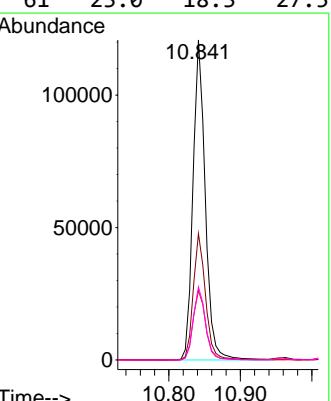

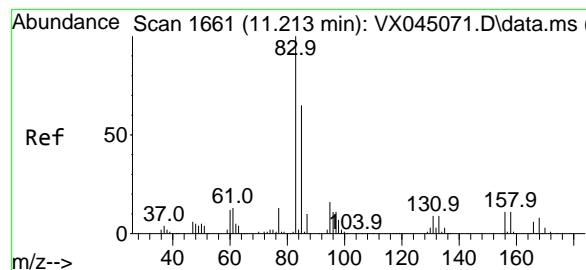



#75
1,1,2,2-Tetrachloroethane
Concen: 50.741 ug/l
RT: 11.213 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

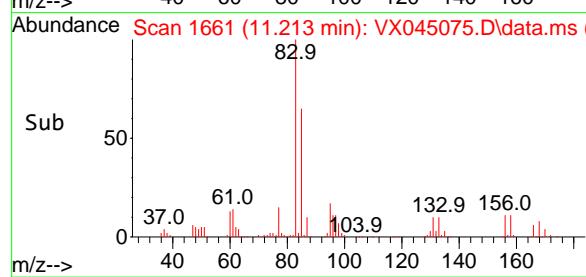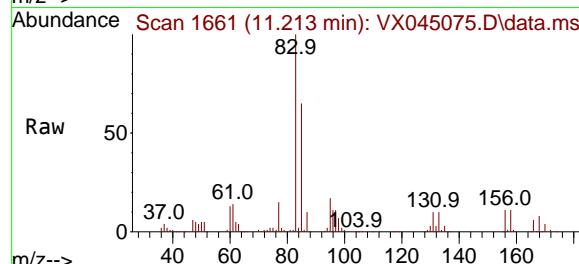


Tgt Ion: 83 Resp: 100800
Ion Ratio Lower Upper
83 100
131 9.4 4.5 13.4
85 64.0 31.7 95.1

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

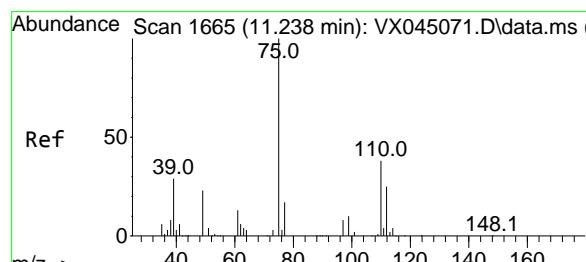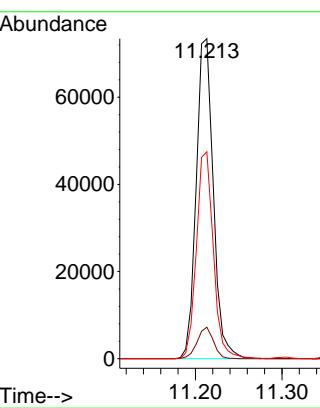


#76
1,2,3-Trichloropropane
Concen: 49.940 ug/l m
RT: 11.238 min Scan# 1665
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

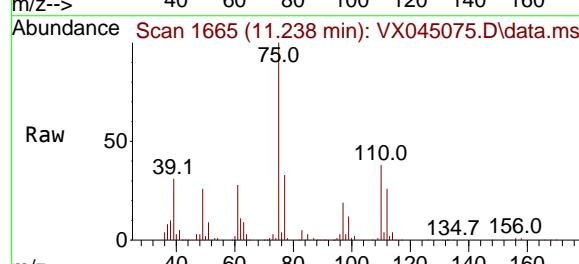


Tgt Ion: 75 Resp: 80618
Ion Ratio Lower Upper
75 100
77 42.5 20.7 62.1

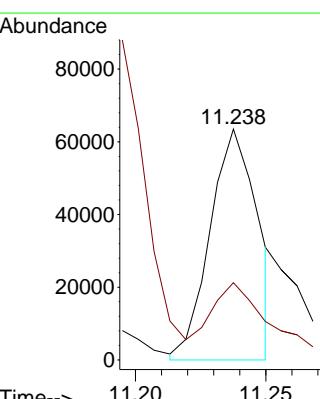

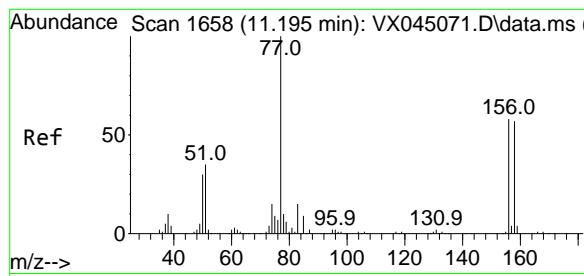

#77
Bromobenzene
Concen: 50.360 ug/l
RT: 11.195 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33



Instrument : MSVOA_X
ClientSampleId : ICVVX022825



Tgt Ion:156 Resp: 64324
Ion Ratio Lower Upper
156 100
77 172.1 85.8 257.4
158 96.5 48.4 145.2



Manual Integrations APPROVED

Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025





#78
n-propylbenzene
Concen: 52.203 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Tgt Ion: 91 Resp: 319235
Ion Ratio Lower Upper
91 100
120 22.2 11.2 33.6




Abundance





#79
2-Chlorotoluene
Concen: 49.338 ug/l
RT: 11.360 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825



Tgt Ion: 91 Resp: 192150
Ion Ratio Lower Upper
91 100
126 33.1 16.4 49.4




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

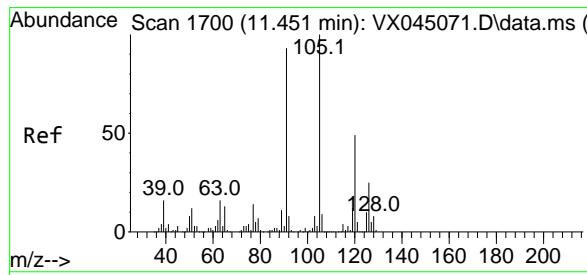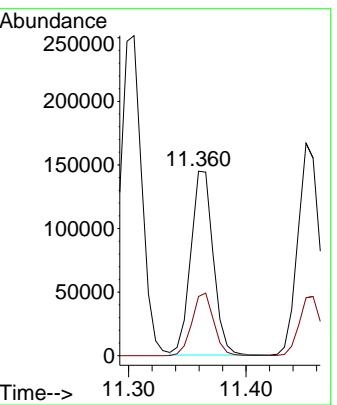


#80
1,3,5-Trimethylbenzene
Concen: 51.544 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Tgt Ion: 105 Resp: 225622
Ion Ratio Lower Upper
105 100
120 48.0 24.1 72.2

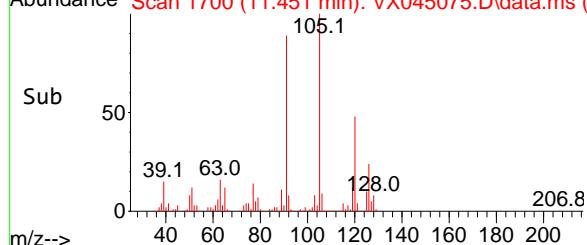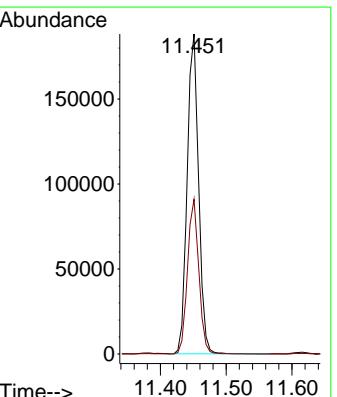

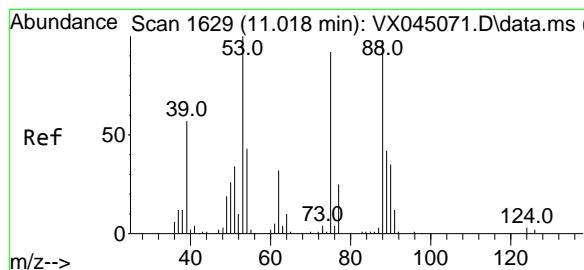




#81
trans-1,4-Dichloro-2-butene
Concen: 50.757 ug/l
RT: 11.018 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

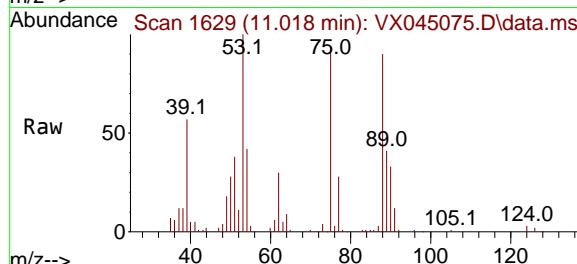


Tgt Ion: 75 Resp: 23941
Ion Ratio Lower Upper
75 100
53 111.4 88.5 132.7
89 45.8 36.2 54.4

Manual Integrations APPROVED



Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



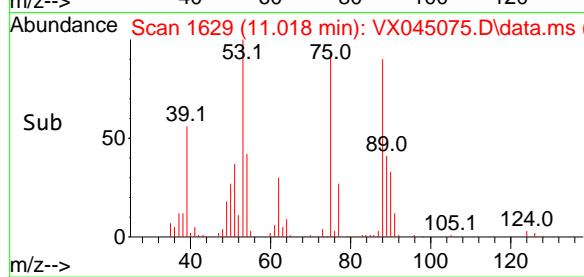


#82
4-Chlorotoluene
Concen: 51.009 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33



Tgt Ion: 91 Resp: 216511
Ion Ratio Lower Upper
91 100
126 28.3 14.1 42.4

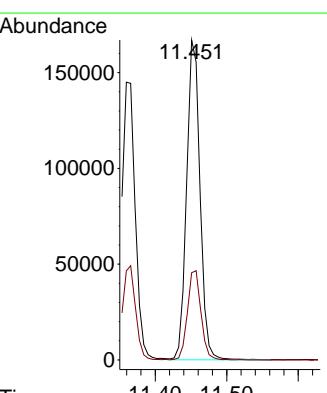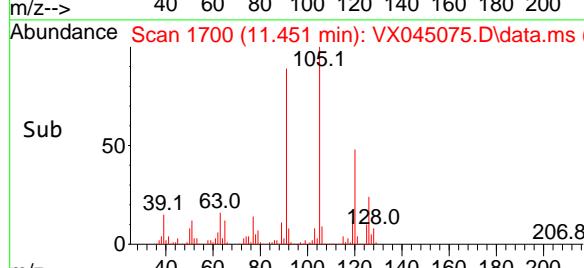



#83

tert-Butylbenzene

Concen: 50.552 ug/l

RT: 11.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045075.D

Acq: 28 Feb 2025 04:33




Instrument:


MSVOA_X


ClientSampleId :

ICVVX022825


**Manual Integrations
APPROVED**

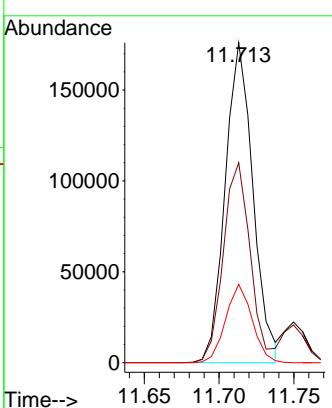 Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

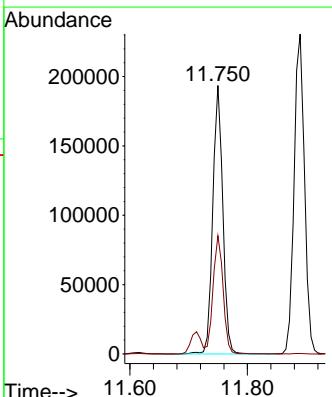 #84
 1,2,4-Trimethylbenzene
 Concen: 51.932 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. -0.000 min
 Lab File: VX045075.D
 Acq: 28 Feb 2025 04:33

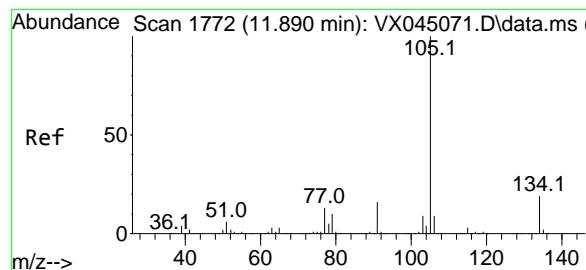 Tgt Ion:105 Resp: 228729
 Ion Ratio Lower Upper
 105 100
 120 44.3 22.1 66.1

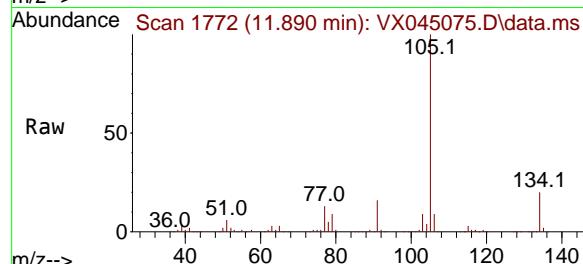


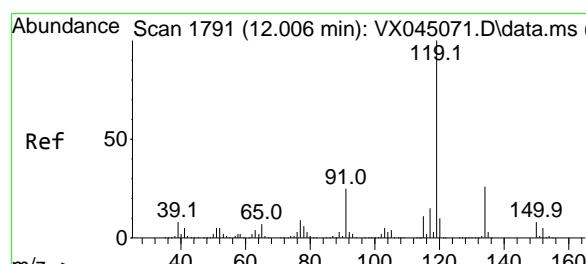

#85
sec-Butylbenzene
Concen: 52.703 ug/l
RT: 11.890 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33
Instrument: MSVOA_X
ClientSampleId : ICVVX022825




Tgt Ion:105 Resp: 28393
Ion Ratio Lower Upper
105 100
134 19.6 9.8 29.4

Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#86
p-Isopropyltoluene
Concen: 52.803 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

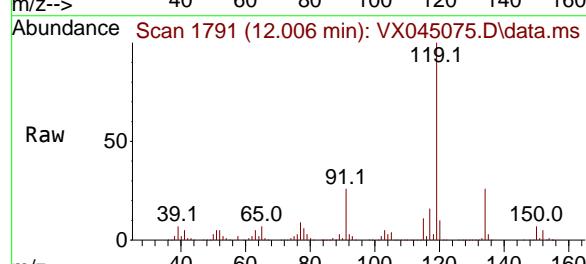

Tgt Ion:119 Resp: 229894
Ion Ratio Lower Upper
119 100
134 25.9 12.9 38.6
91 25.3 12.7 38.0




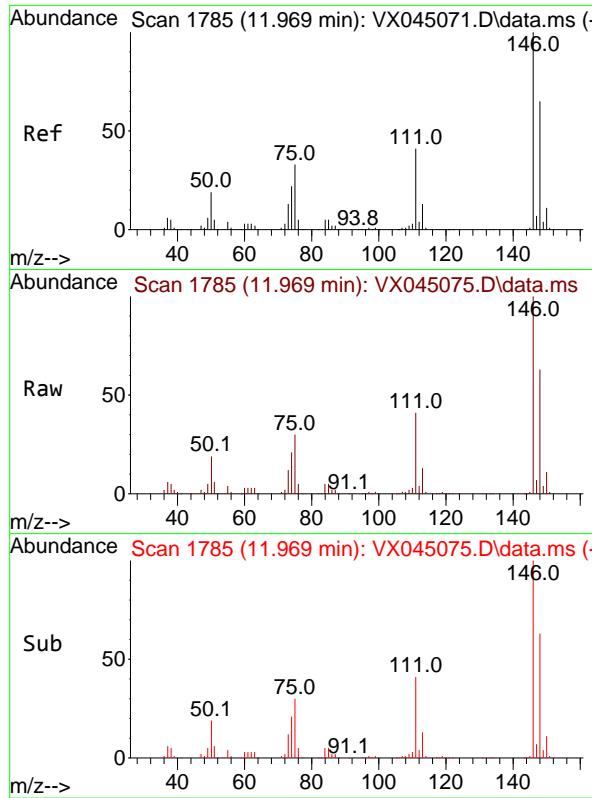


#87
1,3-Dichlorobenzene
Concen: 50.372 ug/l
RT: 11.969 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Instrument : MSVOA_X
ClientSampleId : ICVVX022825


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

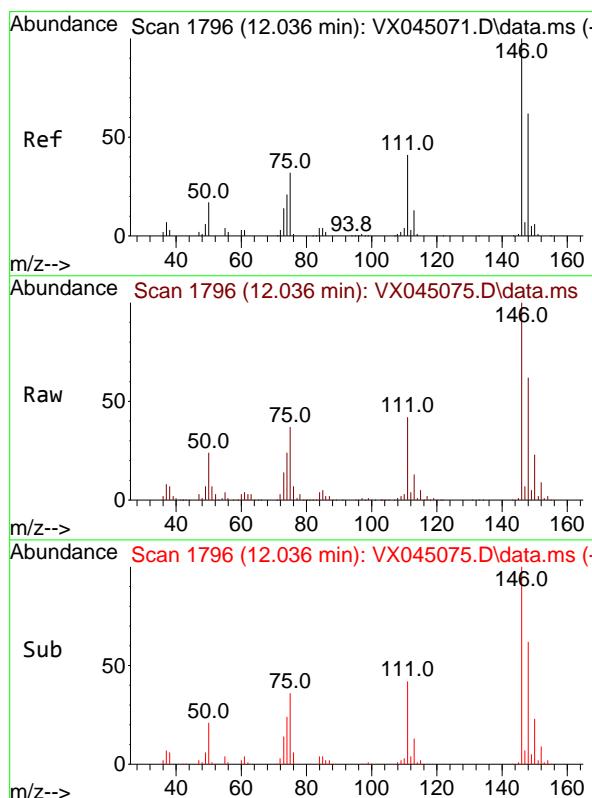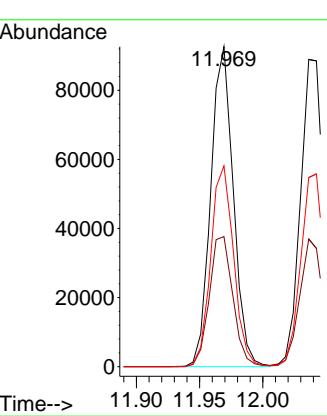

#88
1,4-Dichlorobenzene
Concen: 50.097 ug/l
RT: 12.036 min Scan# 1796
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Tgt Ion:146 Resp: 115486
Ion Ratio Lower Upper
146 100
111 41.0 20.2 60.5
148 63.0 31.9 95.9









#89
n-Butylbenzene
Concen: 54.662 ug/l
RT: 12.329 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Instrument : MSVOA_X
ClientSampleId : ICVX022825

Tgt Ion: 91 Resp: 20497:
Ion Ratio Lower Upper
91 100
92 53.8 26.7 80.0
134 23.9 12.2 36.6




Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025



#90
Hexachloroethane
Concen: 51.866 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33


Tgt Ion:117 Resp: 40844
Ion Ratio Lower Upper
117 100
201 64.7 31.9 95.9








#91
1,2-Dichlorobenzene
Concen: 50.899 ug/l
RT: 12.335 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

Instrument : MSVOA_X
ClientSampleId : ICVVX022825




Tgt	Ion	Ion Ratio	Resp:	11634
			Lower	Upper
146	100			
111	43.2	21.6	65.0	
148	63.9	31.9	95.9	



Manual Integrations APPROVED
Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025




#92
1,2-Dibromo-3-Chloropropane
Concen: 53.199 ug/l
RT: 12.938 min Scan# 1944
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33

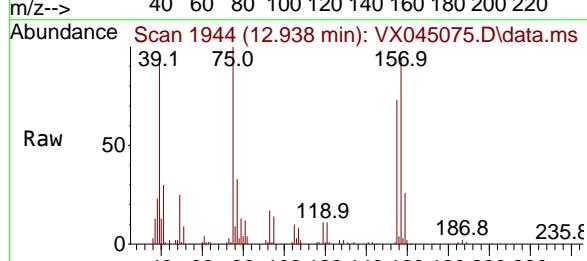

Tgt	Ion	Ion Ratio	Resp:	20589
			Lower	Upper
75	100			
155	79.8	39.6	118.7	
157	101.7	51.1	153.4	

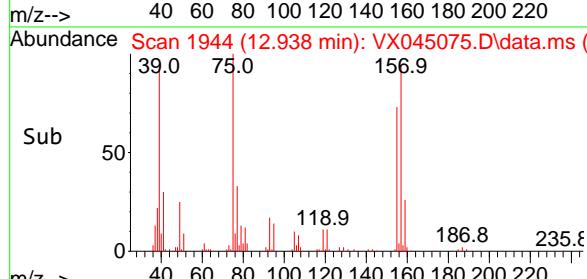


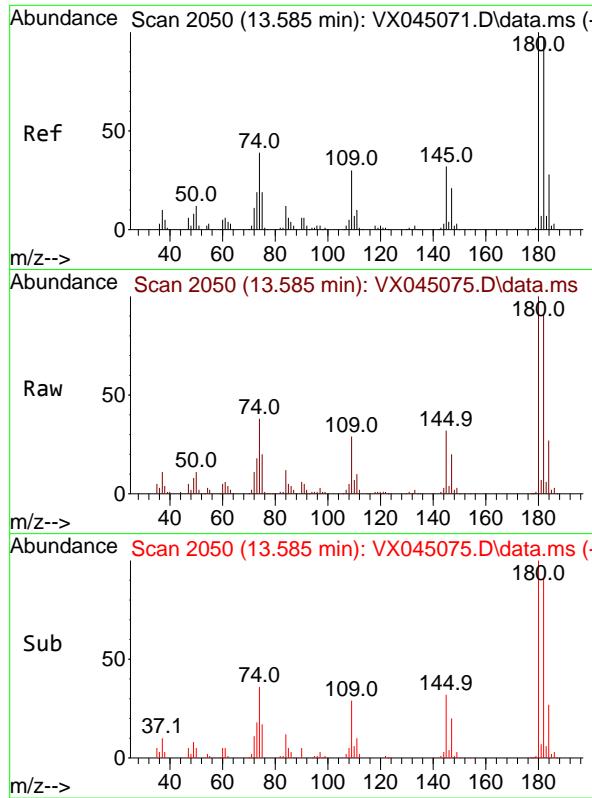


#93
 1,2,4-Trichlorobenzene
 Concen: 54.834 ug/l
 RT: 13.585 min Scan# 2
 Delta R.T. -0.000 min
 Lab File: VX045075.D
 Acq: 28 Feb 2025 04:33

Instrument : MSVOA_X
 ClientSampleId : ICVVX022825


Manual Integrations
APPROVED


Reviewed By :John Carlone 02/28/2025
 Supervised By :Mahesh Dadoda 02/28/2025

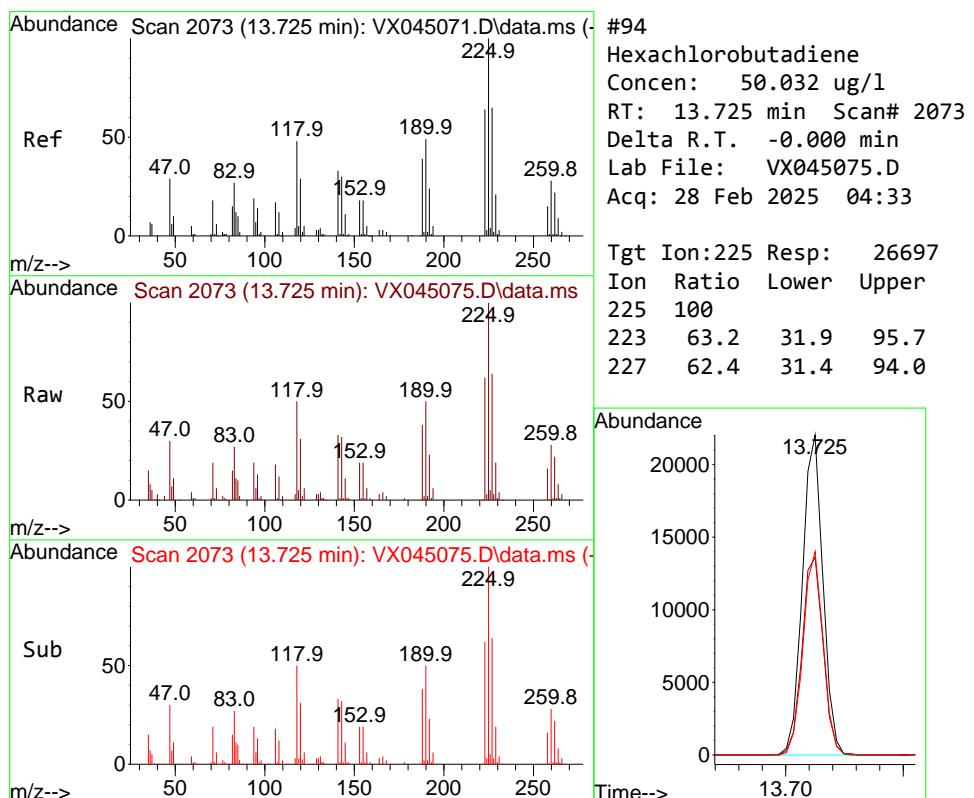


#94
 Hexachlorobutadiene
 Concen: 50.032 ug/l
 RT: 13.725 min Scan# 2073
 Delta R.T. -0.000 min
 Lab File: VX045075.D
 Acq: 28 Feb 2025 04:33

Tgt Ion:225 Resp: 26697
 Ion Ratio Lower Upper
 225 100
 223 63.2 31.9 95.7
 227 62.4 31.4 94.0



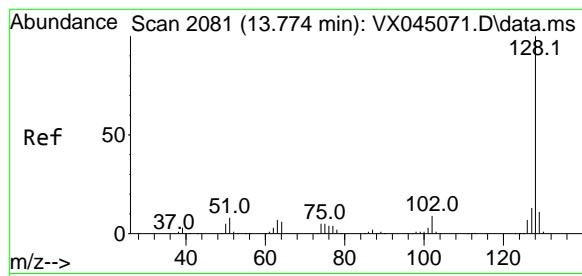



#95
Naphthalene
Concen: 55.163 ug/l
RT: 13.774 min Scan# 2
Instrument : MSVOA_X
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33




Tgt Ion:128 Resp: 27584
Ion Ratio Lower Upper
128 100
127 12.8 10.3 15.5
129 10.9 8.7 13.1

Manual Integrations APPROVED


Reviewed By :John Carlone 02/28/2025
Supervised By :Mahesh Dadoda 02/28/2025

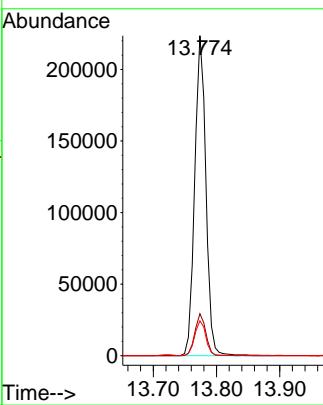

#96
1,2,3-Trichlorobenzene
Concen: 54.049 ug/l
RT: 13.957 min Scan# 2111
Instrument : MSVOA_X
Delta R.T. -0.000 min
Lab File: VX045075.D
Acq: 28 Feb 2025 04:33



Tgt Ion:180 Resp: 74211
Ion Ratio Lower Upper
180 100
182 94.5 47.5 142.6
145 33.9 17.0 50.9

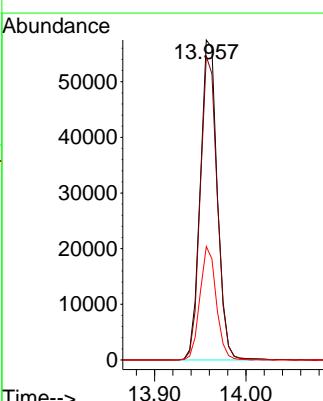

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045075.D
 Acq On : 28 Feb 2025 04:33
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

Quant Time: Feb 28 06:55:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	98	0.00
2 T	Dichlorodifluoromethane	0.629	0.603	4.1	95	0.00
3 P	Chloromethane	0.770	0.750	2.6	98	0.00
4 C	Vinyl Chloride	0.764	0.757	0.9#	98	0.00
5 T	Bromomethane	0.300	0.277	7.7	93	0.00
6 T	Chloroethane	0.352	0.296	15.9	78	0.00
7 T	Trichlorofluoromethane	1.011	1.003	0.8	94	0.00
8 T	Diethyl Ether	0.396	0.385	2.8	98	0.00
9 T	1,1,2-Trichlorotrifluoroeth	0.581	0.585	-0.7	97	0.00
10 T	Methyl Iodide	0.726	0.734	-1.1	94	0.00
11 T	Tert butyl alcohol	0.151	0.144	4.6	106	0.00
12 CM	1,1-Dichloroethene	0.614	0.609	0.8#	96	0.00
13 T	Acrolein	0.174	0.189	-8.6	107	0.00
14 T	Allyl chloride	1.094	1.131	-3.4	100	0.00
15 T	Acrylonitrile	0.404	0.413	-2.2	99	0.00
16 T	Acetone	0.369	0.358	3.0	100	0.00
17 T	Carbon Disulfide	1.636	1.635	0.1	97	0.00
18 T	Methyl Acetate	0.888	0.893	-0.6	101	0.00
19 T	Methyl tert-butyl Ether	2.061	2.190	-6.3	103	0.00
20 T	Methylene Chloride	0.731	0.726	0.7	102	0.00
21 T	trans-1,2-Dichloroethene	0.607	0.621	-2.3	97	0.00
22 T	Diisopropyl ether	2.224	2.400	-7.9	103	0.00
23 T	Vinyl Acetate	1.856	2.096	-12.9	105	0.00
24 P	1,1-Dichloroethane	1.247	1.276	-2.3	101	0.00
25 T	2-Butanone	0.555	0.587	-5.8	100	0.00
26 T	2,2-Dichloropropane	0.585	0.578	1.2	95	0.00
27 T	cis-1,2-Dichloroethene	0.749	0.773	-3.2	100	0.00
28 T	Bromochloromethane	0.594	0.599	-0.8	98	0.00
29 T	Tetrahydrofuran	0.373	0.385	-3.2	102	0.00
30 C	Chloroform	1.239	1.244	-0.4#	98	0.00
31 T	Cyclohexane	1.082	1.085	-0.3	96	0.00
32 T	1,1,1-Trichloroethane	1.000	1.019	-1.9	98	0.00
33 S	1,2-Dichloroethane-d4	0.795	0.800	-0.6	104	0.00
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	99	0.00
35 S	Dibromofluoromethane	0.334	0.340	-1.8	103	0.00
36 T	1,1-Dichloropropene	0.459	0.447	2.6	95	0.00
37 T	Ethyl Acetate	0.591	0.610	-3.2	100	0.00
38 T	Carbon Tetrachloride	0.465	0.460	1.1	98	0.00
39 T	Methylcyclohexane	0.549	0.562	-2.4	95	0.00
40 TM	Benzene	1.448	1.482	-2.3	98	0.00
41 T	Methacrylonitrile	0.319	0.341	-6.9	99	0.00
42 TM	1,2-Dichloroethane	0.521	0.529	-1.5	99	0.00
43 T	Isopropyl Acetate	0.874	0.951	-8.8	102	0.00
44 TM	Trichloroethene	0.340	0.333	2.1	97	0.00
45 C	1,2-Dichloropropane	0.372	0.380	-2.2#	102	0.00
46 T	Dibromomethane	0.263	0.272	-3.4	100	0.00
47 T	Bromodichloromethane	0.516	0.526	-1.9	99	0.00
48 T	Methyl methacrylate	0.438	0.474	-8.2	102	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045075.D
 Acq On : 28 Feb 2025 04:33
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

Quant Time: Feb 28 06:55:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.009	0.010	-11.1	102	0.00
50 S	Toluene-d8	1.212	1.221	-0.7	100	0.00
51 T	4-Methyl-2-Pentanone	0.587	0.610	-3.9	99	0.00
52 CM	Toluene	0.849	0.867	-2.1#	96	0.00
53 T	t-1,3-Dichloropropene	0.431	0.468	-8.6	99	0.00
54 T	cis-1,3-Dichloropropene	0.503	0.531	-5.6	98	0.00
55 T	1,1,2-Trichloroethane	0.350	0.351	-0.3	98	0.00
56 T	Ethyl methacrylate	0.532	0.575	-8.1	100	0.00
57 T	1,3-Dichloropropane	0.605	0.621	-2.6	99	0.00
58 T	2-Chloroethyl Vinyl ether	0.259	0.286	-10.4	100	0.00
59 T	2-Hexanone	0.425	0.451	-6.1	100	0.00
60 T	Dibromochloromethane	0.366	0.376	-2.7	97	0.00
61 T	1,2-Dibromoethane	0.349	0.360	-3.2	100	0.00
62 S	4-Bromofluorobenzene	0.402	0.396	1.5	98	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	97	0.00
64 T	Tetrachloroethene	0.320	0.321	-0.3	96	0.00
65 PM	Chlorobenzene	1.058	1.070	-1.1	95	0.00
66 T	1,1,1,2-Tetrachloroethane	0.352	0.360	-2.3	99	0.00
67 C	Ethyl Benzene	1.843	1.903	-3.3#	95	0.00
68 T	m/p-Xylenes	0.675	0.698	-3.4	94	0.00
69 T	o-Xylene	0.681	0.690	-1.3	95	0.00
70 T	Styrene	1.101	1.149	-4.4	95	0.00
71 P	Bromoform	0.266	0.280	-5.3	99	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	97	0.00
73 T	Isopropylbenzene	3.903	4.027	-3.2	95	0.00
74 T	N-amyl acetate	1.831	2.082	-13.7	103	0.00
75 P	1,1,2,2-Tetrachloroethane	1.432	1.453	-1.5	100	0.00
76 T	1,2,3-Trichloropropane	1.164	1.162	0.2	99	0.00
77 T	Bromobenzene	0.921	0.927	-0.7	96	0.00
78 T	n-propylbenzene	4.409	4.603	-4.4	93	0.00
79 T	2-Chlorotoluene	2.808	2.770	1.4	94	0.00
80 T	1,3,5-Trimethylbenzene	3.156	3.253	-3.1	94	0.00
81 T	trans-1,4-Dichloro-2-butene	0.340	0.345	-1.5	99	0.00
82 T	4-Chlorotoluene	3.060	3.122	-2.0	94	0.00
83 T	tert-Butylbenzene	3.242	3.278	-1.1	95	0.00
84 T	1,2,4-Trimethylbenzene	3.175	3.298	-3.9	95	0.00
85 T	sec-Butylbenzene	3.884	4.094	-5.4	95	0.00
86 T	p-Isopropyltoluene	3.139	3.315	-5.6	94	0.00
87 T	1,3-Dichlorobenzene	1.643	1.655	-0.7	97	0.00
88 T	1,4-Dichlorobenzene	1.662	1.665	-0.2	96	0.00
89 T	n-Butylbenzene	2.703	2.955	-9.3	95	0.00
90 T	Hexachloroethane	0.568	0.589	-3.7	95	0.00
91 T	1,2-Dichlorobenzene	1.648	1.677	-1.8	98	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.279	0.297	-6.5	100	0.00
93 T	1,2,4-Trichlorobenzene	0.938	1.029	-9.7	99	0.00
94 T	Hexachlorobutadiene	0.385	0.385	0.0	96	0.00
95 T	Naphthalene	3.605	3.977	-10.3	99	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045075.D
Acq On : 28 Feb 2025 04:33
Operator : JC/MD
Sample : VSTDICV050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

Quant Time: Feb 28 06:55:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T 1,2,3-Trichlorobenzene	0.990	1.070	-8.1	98	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045075.D
 Acq On : 28 Feb 2025 04:33
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

Quant Time: Feb 28 06:55:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	98	0.00
2 T	Dichlorodifluoromethane	50.000	47.933	4.1	95	0.00
3 P	Chloromethane	50.000	48.696	2.6	98	0.00
4 C	Vinyl Chloride	50.000	49.529	0.9#	98	0.00
5 T	Bromomethane	50.000	46.190	7.6	93	0.00
6 T	Chloroethane	50.000	41.948	16.1	78	0.00
7 T	Trichlorofluoromethane	50.000	49.569	0.9	94	0.00
8 T	Diethyl Ether	50.000	48.651	2.7	98	0.00
9 T	1,1,2-Trichlorotrifluoroeth	50.000	50.367	-0.7	97	0.00
10 T	Methyl Iodide	50.000	50.541	-1.1	94	0.00
11 T	Tert butyl alcohol	250.000	238.577	4.6	106	0.00
12 CM	1,1-Dichloroethene	50.000	49.568	0.9#	96	0.00
13 T	Acrolein	250.000	271.255	-8.5	107	0.00
14 T	Allyl chloride	50.000	51.691	-3.4	100	0.00
15 T	Acrylonitrile	250.000	255.479	-2.2	99	0.00
16 T	Acetone	250.000	242.877	2.8	100	0.00
17 T	Carbon Disulfide	50.000	49.952	0.1	97	0.00
18 T	Methyl Acetate	50.000	50.312	-0.6	101	0.00
19 T	Methyl tert-butyl Ether	50.000	53.114	-6.2	103	0.00
20 T	Methylene Chloride	50.000	49.639	0.7	102	0.00
21 T	trans-1,2-Dichloroethene	50.000	51.172	-2.3	97	0.00
22 T	Diisopropyl ether	50.000	53.955	-7.9	103	0.00
23 T	Vinyl Acetate	250.000	282.313	-12.9	105	0.00
24 P	1,1-Dichloroethane	50.000	51.190	-2.4	101	0.00
25 T	2-Butanone	250.000	264.040	-5.6	100	0.00
26 T	2,2-Dichloropropane	50.000	49.401	1.2	95	0.00
27 T	cis-1,2-Dichloroethene	50.000	51.606	-3.2	100	0.00
28 T	Bromochloromethane	50.000	50.399	-0.8	98	0.00
29 T	Tetrahydrofuran	250.000	258.277	-3.3	102	0.00
30 C	Chloroform	50.000	50.236	-0.5#	98	0.00
31 T	Cyclohexane	50.000	50.158	-0.3	96	0.00
32 T	1,1,1-Trichloroethane	50.000	50.939	-1.9	98	0.00
33 S	1,2-Dichloroethane-d4	50.000	50.297	-0.6	104	0.00
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	99	0.00
35 S	Dibromofluoromethane	50.000	50.841	-1.7	103	0.00
36 T	1,1-Dichloropropene	50.000	48.770	2.5	95	0.00
37 T	Ethyl Acetate	50.000	51.596	-3.2	100	0.00
38 T	Carbon Tetrachloride	50.000	49.425	1.2	98	0.00
39 T	Methylcyclohexane	50.000	51.169	-2.3	95	0.00
40 TM	Benzene	50.000	51.195	-2.4	98	0.00
41 T	Methacrylonitrile	50.000	53.352	-6.7	99	0.00
42 TM	1,2-Dichloroethane	50.000	50.718	-1.4	99	0.00
43 T	Isopropyl Acetate	50.000	54.452	-8.9	102	0.00
44 TM	Trichloroethene	50.000	48.924	2.2	97	0.00
45 C	1,2-Dichloropropane	50.000	51.086	-2.2#	102	0.00
46 T	Dibromomethane	50.000	51.661	-3.3	100	0.00
47 T	Bromodichloromethane	50.000	50.930	-1.9	99	0.00
48 T	Methyl methacrylate	50.000	54.016	-8.0	102	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045075.D
 Acq On : 28 Feb 2025 04:33
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

Quant Time: Feb 28 06:55:08 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	1049.007	-4.9	102	0.00
50 S	Toluene-d8	50.000	50.364	-0.7	100	0.00
51 T	4-Methyl-2-Pentanone	250.000	259.995	-4.0	99	0.00
52 CM	Toluene	50.000	51.020	-2.0#	96	0.00
53 T	t-1,3-Dichloropropene	50.000	54.247	-8.5	99	0.00
54 T	cis-1,3-Dichloropropene	50.000	52.732	-5.5	98	0.00
55 T	1,1,2-Trichloroethane	50.000	50.232	-0.5	98	0.00
56 T	Ethyl methacrylate	50.000	54.109	-8.2	100	0.00
57 T	1,3-Dichloropropane	50.000	51.312	-2.6	99	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	275.557	-10.2	100	0.00
59 T	2-Hexanone	250.000	265.049	-6.0	100	0.00
60 T	Dibromochloromethane	50.000	51.374	-2.7	97	0.00
61 T	1,2-Dibromoethane	50.000	51.492	-3.0	100	0.00
62 S	4-Bromofluorobenzene	50.000	49.240	1.5	98	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	97	0.00
64 T	Tetrachloroethene	50.000	50.126	-0.3	96	0.00
65 PM	Chlorobenzene	50.000	50.580	-1.2	95	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	51.102	-2.2	99	0.00
67 C	Ethyl Benzene	50.000	51.621	-3.2#	95	0.00
68 T	m/p-Xylenes	100.000	103.454	-3.5	94	0.00
69 T	o-Xylene	50.000	50.668	-1.3	95	0.00
70 T	Styrene	50.000	52.177	-4.4	95	0.00
71 P	Bromoform	50.000	52.636	-5.3	99	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	97	0.00
73 T	Isopropylbenzene	50.000	51.589	-3.2	95	0.00
74 T	N-amyl acetate	50.000	56.851	-13.7	103	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	50.741	-1.5	100	0.00
76 T	1,2,3-Trichloropropane	50.000	49.940	0.1	99	0.00
77 T	Bromobenzene	50.000	50.360	-0.7	96	0.00
78 T	n-propylbenzene	50.000	52.203	-4.4	93	0.00
79 T	2-Chlorotoluene	50.000	49.338	1.3	94	0.00
80 T	1,3,5-Trimethylbenzene	50.000	51.544	-3.1	94	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	50.757	-1.5	99	0.00
82 T	4-Chlorotoluene	50.000	51.009	-2.0	94	0.00
83 T	tert-Butylbenzene	50.000	50.552	-1.1	95	0.00
84 T	1,2,4-Trimethylbenzene	50.000	51.932	-3.9	95	0.00
85 T	sec-Butylbenzene	50.000	52.703	-5.4	95	0.00
86 T	p-Isopropyltoluene	50.000	52.803	-5.6	94	0.00
87 T	1,3-Dichlorobenzene	50.000	50.372	-0.7	97	0.00
88 T	1,4-Dichlorobenzene	50.000	50.097	-0.2	96	0.00
89 T	n-Butylbenzene	50.000	54.662	-9.3	95	0.00
90 T	Hexachloroethane	50.000	51.866	-3.7	95	0.00
91 T	1,2-Dichlorobenzene	50.000	50.899	-1.8	98	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	53.199	-6.4	100	0.00
93 T	1,2,4-Trichlorobenzene	50.000	54.834	-9.7	99	0.00
94 T	Hexachlorobutadiene	50.000	50.032	-0.1	96	0.00
95 T	Naphthalene	50.000	55.163	-10.3	99	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
Data File : VX045075.D
Acq On : 28 Feb 2025 04:33
Operator : JC/MD
Sample : VSTDICV050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX022825

Quant Time: Feb 28 06:55:08 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	Amount	Calc.	%Dev	Area%	Dev(min)
96 T 1,2,3-Trichlorobenzene	50.000	54.049	-8.1	98	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	CHEMTECH	Contract:	ALLI03				
Lab Code:	CHEM	Case No.:	Q1502	SAS No.:	Q1502	SDG No.:	Q1502
Instrument ID:	MSVOA_X	Calibration Date/Time: 03/11/2025 09:59					
Lab File ID:	VX045211.D	Init. Calib. Date(s): 02/28/2025 02/28/2025					
Heated Purge:	(Y/N) N	Init. Calib. Time(s): 01:27 03:47					
GC Column:	DB-624UI	ID:	0.18	(mm)			

COMPOUND	RRF	RRF050	MIN RRF	%D	MAX%D
Dichlorodifluoromethane	0.629	0.659		4.77	20
Chloromethane	0.770	0.731	0.1	-5.07	20
Vinyl Chloride	0.764	0.723		-5.37	20
Ethyl Acetate	0.591	0.613		3.72	20
Bromomethane	0.300	0.303		1	20
Chloroethane	0.352	0.386		9.66	20
Trichlorofluoromethane	1.012	1.035		2.27	20
1,1,2-Trichlorotrifluoroethane	0.581	0.644		10.84	20
1,1-Dichloroethene	0.614	0.615		0.16	20
Acrolein	0.174	0.153		-12.07	20
Acrylonitrile	0.404	0.413		2.23	20
Acetone	0.369	0.381		3.25	20
Carbon Disulfide	1.636	1.547		-5.44	20
Methyl tert-butyl Ether	2.061	2.061		0	20
Methylene Chloride	0.731	0.714		-2.33	20
trans-1,2-Dichloroethene	0.607	0.616		1.48	20
Vinyl Acetate	1.856	1.965		5.87	20
1,1-Dichloroethane	1.247	1.245	0.1	-0.16	20
2-Butanone	0.555	0.581		4.68	20
Carbon Tetrachloride	0.465	0.493		6.02	20
2,2-Dichloropropane	0.585	0.905		54.7	20
cis-1,2-Dichloroethene	0.749	0.755		0.8	20
Chloroform	1.239	1.234		-0.4	20
1,1,1-Trichloroethane	1.000	1.017		1.7	20
1,1-Dichloropropene	0.459	0.476		3.7	20
Benzene	1.448	1.486		2.62	20
1,2-Dichloroethane	0.521	0.546		4.8	20
Trichloroethene	0.340	0.354		4.12	20
1,2-Dichloropropane	0.372	0.380		2.15	20
Dibromomethane	0.263	0.278		5.7	20
Bromodichloromethane	0.516	0.557		7.95	20
4-Methyl-2-Pentanone	0.587	0.636		8.35	20
Toluene	0.849	0.900		6.01	20
t-1,3-Dichloropropene	0.431	0.514		19.26	20
cis-1,3-Dichloropropene	0.503	0.580		15.31	20
1,1,2-Trichloroethane	0.350	0.361		3.14	20
1,3-Dichloropropane	0.605	0.631		4.3	20
2-Chloroethyl Vinyl ether	0.259	0.302		16.6	20

All other compounds must meet a minimum RRF of 0.010.

RRF of 1,4-Dioxane = Value should be divide by 1000.

VOLATILE CONTINUING CALIBRATION CHECK

Lab Name:	CHEMTECH	Contract:	ALLI03				
Lab Code:	CHEM	Case No.:	Q1502	SAS No.:	Q1502	SDG No.:	Q1502
Instrument ID:	MSVOA_X	Calibration Date/Time:				03/11/2025	09:59
Lab File ID:	VX045211.D	Init. Calib. Date(s):				02/28/2025	02/28/2025
Heated Purge:	(Y/N) N	Init. Calib. Time(s):				01:27	03:47
GC Column:	DB-624UI	ID:	0.18	(mm)			

COMPOUND	RRF	RRF050	MIN RRF	%D	MAX%D
2-Hexanone	0.425	0.458		7.76	20
Dibromochloromethane	0.366	0.404		10.38	20
1,2-Dibromoethane	0.349	0.373		6.88	20
Tetrachloroethene	0.320	0.336		5	20
Chlorobenzene	1.058	1.120	0.3	5.86	20
1,1,1,2-Tetrachloroethane	0.352	0.372		5.68	20
Ethyl Benzene	1.843	1.996		8.3	20
m/p-Xylenes	0.675	0.738		9.33	20
o-Xylene	0.681	0.724		6.31	20
Styrene	1.101	1.222		10.99	20
Bromoform	0.266	0.306	0.1	15.04	20
Isopropylbenzene	3.903	4.178		7.05	20
1,1,2,2-Tetrachloroethane	1.432	1.392	0.3	-2.79	20
1,2,3-Trichloropropane	1.164	1.182		1.55	20
Bromobenzene	0.921	0.953		3.47	20
n-propylbenzene	4.409	4.921		11.61	20
2-Chlorotoluene	2.808	2.904		3.42	20
1,3,5-Trimethylbenzene	3.156	3.410		8.05	20
4-Chlorotoluene	3.060	3.281		7.22	20
1,2,4-Trimethylbenzene	3.175	3.431		8.06	20
sec-Butylbenzene	3.884	4.364		12.36	20
p-Isopropyltoluene	3.139	3.522		12.2	20
1,3-Dichlorobenzene	1.643	1.694		3.1	20
1,4-Dichlorobenzene	1.662	1.696		2.05	20
n-Butylbenzene	2.703	3.210		18.76	20
1,2-Dichlorobenzene	1.648	1.671		1.4	20
1,2-Dibromo-3-Chloropropane	0.279	0.293		5.02	20
1,2,4-Trichlorobenzene	0.938	1.037		10.55	20
Hexachlorobutadiene	0.385	0.438		13.77	20
Naphthalene	3.605	3.723		3.27	20
1,2,3-Trichlorobenzene	0.990	1.037		4.75	20
1,2-Dichloroethane-d4	0.795	0.792		-0.38	20
Dibromofluoromethane	0.334	0.355		6.29	20
Toluene-d8	1.212	1.251		3.22	20
4-Bromofluorobenzene	0.402	0.446		10.94	20

All other compounds must meet a minimum RRF of 0.010.
RRF of 1,4-Dioxane = Value should be divide by 1000.

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045211.D
 Acq On : 11 Mar 2025 09:59
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050

Quant Time: Mar 12 01:41:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.544	168	101357	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	176548	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	153652	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	70136	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	80318	49.818	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	99.640%	
35) Dibromofluoromethane	5.373	113	62691	53.104	ug/l	-0.01
Spiked Amount 50.000	Range 75 - 124		Recovery	=	106.200%	
50) Toluene-d8	8.641	98	220779	51.586	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	103.180%	
62) 4-Bromofluorobenzene	11.079	95	78726	55.511	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	111.020%	
Target Compounds						
				Qvalue		
2) Dichlorodifluoromethane	1.167	85	66819	52.372	ug/l	97
3) Chloromethane	1.301	50	74121	47.472	ug/l	97
4) Vinyl Chloride	1.374	62	73280	47.311	ug/l	97
5) Bromomethane	1.593	94	30682	50.390	ug/l	99
6) Chloroethane	1.660	64	39147	54.794	ug/l	100
7) Trichlorofluoromethane	1.874	101	104874	51.147	ug/l	99
8) Diethyl Ether	2.130	74	37439	46.681	ug/l	100
9) 1,1,2-Trichlorotrifluo...	2.319	101	65226	55.369	ug/l	99
10) Methyl Iodide	2.441	142	77939	52.942	ug/l	98
11) Tert butyl alcohol	2.977	59	59389	194.474	ug/l	97
12) 1,1-Dichloroethene	2.307	96	62298	50.020	ug/l	99
13) Acrolein	2.233	56	77625	219.893	ug/l	100
14) Allyl chloride	2.654	41	118042	53.245	ug/l	99
15) Acrylonitrile	3.063	53	209132	255.519	ug/l	99
16) Acetone	2.380	43	192994	258.004	ug/l	99
17) Carbon Disulfide	2.502	76	156835	47.279	ug/l	96
18) Methyl Acetate	2.703	43	101610	56.465	ug/l	99
19) Methyl tert-butyl Ether	3.111	73	208892	49.992	ug/l	100
20) Methylene Chloride	2.782	84	72325	48.811	ug/l	97
21) trans-1,2-Dichloroethene	3.081	96	62483	50.781	ug/l	96
22) Diisopropyl ether	3.758	45	233037	51.685	ug/l	96
23) Vinyl Acetate	3.715	43	995766	264.646	ug/l	98
24) 1,1-Dichloroethane	3.599	63	126144	49.921	ug/l	99
25) 2-Butanone	4.550	43	294568	261.614	ug/l	99
26) 2,2-Dichloropropane	4.465	77	91726	77.390	ug/l	95
27) cis-1,2-Dichloroethene	4.477	96	76526	50.382	ug/l	96
28) Bromochloromethane	4.891	49	58687	48.726	ug/l	99
29) Tetrahydrofuran	5.001	42	185916	245.874	ug/l	99
30) Chloroform	5.087	83	125081	49.818	ug/l	100
31) Cyclohexane	5.458	56	112624	51.345	ug/l	97
32) 1,1,1-Trichloroethane	5.373	97	103045	50.816	ug/l	98
36) 1,1-Dichloropropene	5.684	75	83960	51.860	ug/l	100
37) Ethyl Acetate	4.709	43	108170	51.851	ug/l	99
38) Carbon Tetrachloride	5.666	117	87028	52.948	ug/l	98
39) Methylcyclohexane	7.373	83	109872	56.638	ug/l	99
40) Benzene	6.025	78	262366	51.320	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045211.D
 Acq On : 11 Mar 2025 09:59
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050

Quant Time: Mar 12 01:41:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.916	41	60141	53.315	ug/1	98
42) 1,2-Dichloroethane	6.080	62	96385	52.356	ug/1	99
43) Isopropyl Acetate	6.336	43	168322	54.564	ug/1	99
44) Trichloroethene	7.117	130	62473	52.042	ug/1	100
45) 1,2-Dichloropropane	7.422	63	67025	50.991	ug/1	99
46) Dibromomethane	7.574	93	49158	52.911	ug/1	98
47) Bromodichloromethane	7.818	83	98381	53.986	ug/1	99
48) Methyl methacrylate	7.690	41	83051	53.663	ug/1	97
49) 1,4-Dioxane	7.659	88	29383	900.059	ug/1	99
51) 4-Methyl-2-Pentanone	8.568	43	561413	271.045	ug/1	100
52) Toluene	8.714	92	158892	52.972	ug/1	100
53) t-1,3-Dichloropropene	8.976	75	90808	59.606	ug/1	97
54) cis-1,3-Dichloropropene	8.360	75	102314	57.592	ug/1	97
55) 1,1,2-Trichloroethane	9.147	97	63793	51.661	ug/1	97
56) Ethyl methacrylate	9.116	69	104915	55.894	ug/1	99
57) 1,3-Dichloropropane	9.305	76	111402	52.131	ug/1	100
58) 2-Chloroethyl Vinyl ether	8.238	63	266994	291.597	ug/1	99
59) 2-Hexanone	9.427	43	404272	269.382	ug/1	100
60) Dibromochloromethane	9.519	129	71357	55.267	ug/1	99
61) 1,2-Dibromoethane	9.604	107	65874	53.438	ug/1	97
64) Tetrachloroethene	9.269	164	51638	52.473	ug/1	94
65) Chlorobenzene	10.073	112	172081	52.928	ug/1	99
66) 1,1,1,2-Tetrachloroethane	10.159	131	57191	52.821	ug/1	99
67) Ethyl Benzene	10.189	91	306683	54.136	ug/1	98
68) m/p-Xylenes	10.299	106	226899	109.410	ug/1	99
69) o-Xylene	10.640	106	111278	53.202	ug/1	98
70) Styrene	10.653	104	187697	55.460	ug/1	99
71) Bromoform	10.799	173	46985	57.546	ug/1 #	98
73) Isopropylbenzene	10.957	105	293007	53.524	ug/1	99
74) N-amyl acetate	10.842	43	137353	53.471	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.207	83	97628	48.598	ug/1	99
76) 1,2,3-Trichloropropane	11.238	75	82866m	50.763	ug/1	
77) Bromobenzene	11.195	156	66839	51.748	ug/1	99
78) n-propylbenzene	11.299	91	345156	55.815	ug/1	99
79) 2-Chlorotoluene	11.360	91	203667	51.714	ug/1	99
80) 1,3,5-Trimethylbenzene	11.445	105	239185	54.036	ug/1	99
81) trans-1,4-Dichloro-2-b...	11.018	75	28423	59.586	ug/1	97
82) 4-Chlorotoluene	11.451	91	230104	53.609	ug/1	100
83) tert-Butylbenzene	11.713	119	240128	52.798	ug/1	99
84) 1,2,4-Trimethylbenzene	11.750	105	240636	54.029	ug/1	100
85) sec-Butylbenzene	11.890	105	306106	56.188	ug/1	99
86) p-Isopropyltoluene	12.006	119	247047	56.113	ug/1	100
87) 1,3-Dichlorobenzene	11.969	146	118813	51.564	ug/1	99
88) 1,4-Dichlorobenzene	12.037	146	118921	51.014	ug/1	98
89) n-Butylbenzene	12.329	91	225130	59.371	ug/1	100
90) Hexachloroethane	12.536	117	43824	55.032	ug/1	100
91) 1,2-Dichlorobenzene	12.335	146	117166	50.690	ug/1	98
92) 1,2-Dibromo-3-Chloropr...	12.939	75	20560	52.534	ug/1	96
93) 1,2,4-Trichlorobenzene	13.585	180	72696	55.234	ug/1	99
94) Hexachlorobutadiene	13.725	225	30733	56.956	ug/1	98
95) Naphthalene	13.774	128	261123	51.639	ug/1	100
96) 1,2,3-Trichlorobenzene	13.963	180	72754	52.399	ug/1	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
Data File : VX045211.D
Acq On : 11 Mar 2025 09:59
Operator : JC/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050

Manual Integrations
APPROVED

Reviewed By :John Carbone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

Quant Time: Mar 12 01:41:38 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
Data File : VX045211.D
Acq On : 11 Mar 2025 09:59
Operator : JC/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050

Manual Integrations APPROVED


Reviewed By :John Caralone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

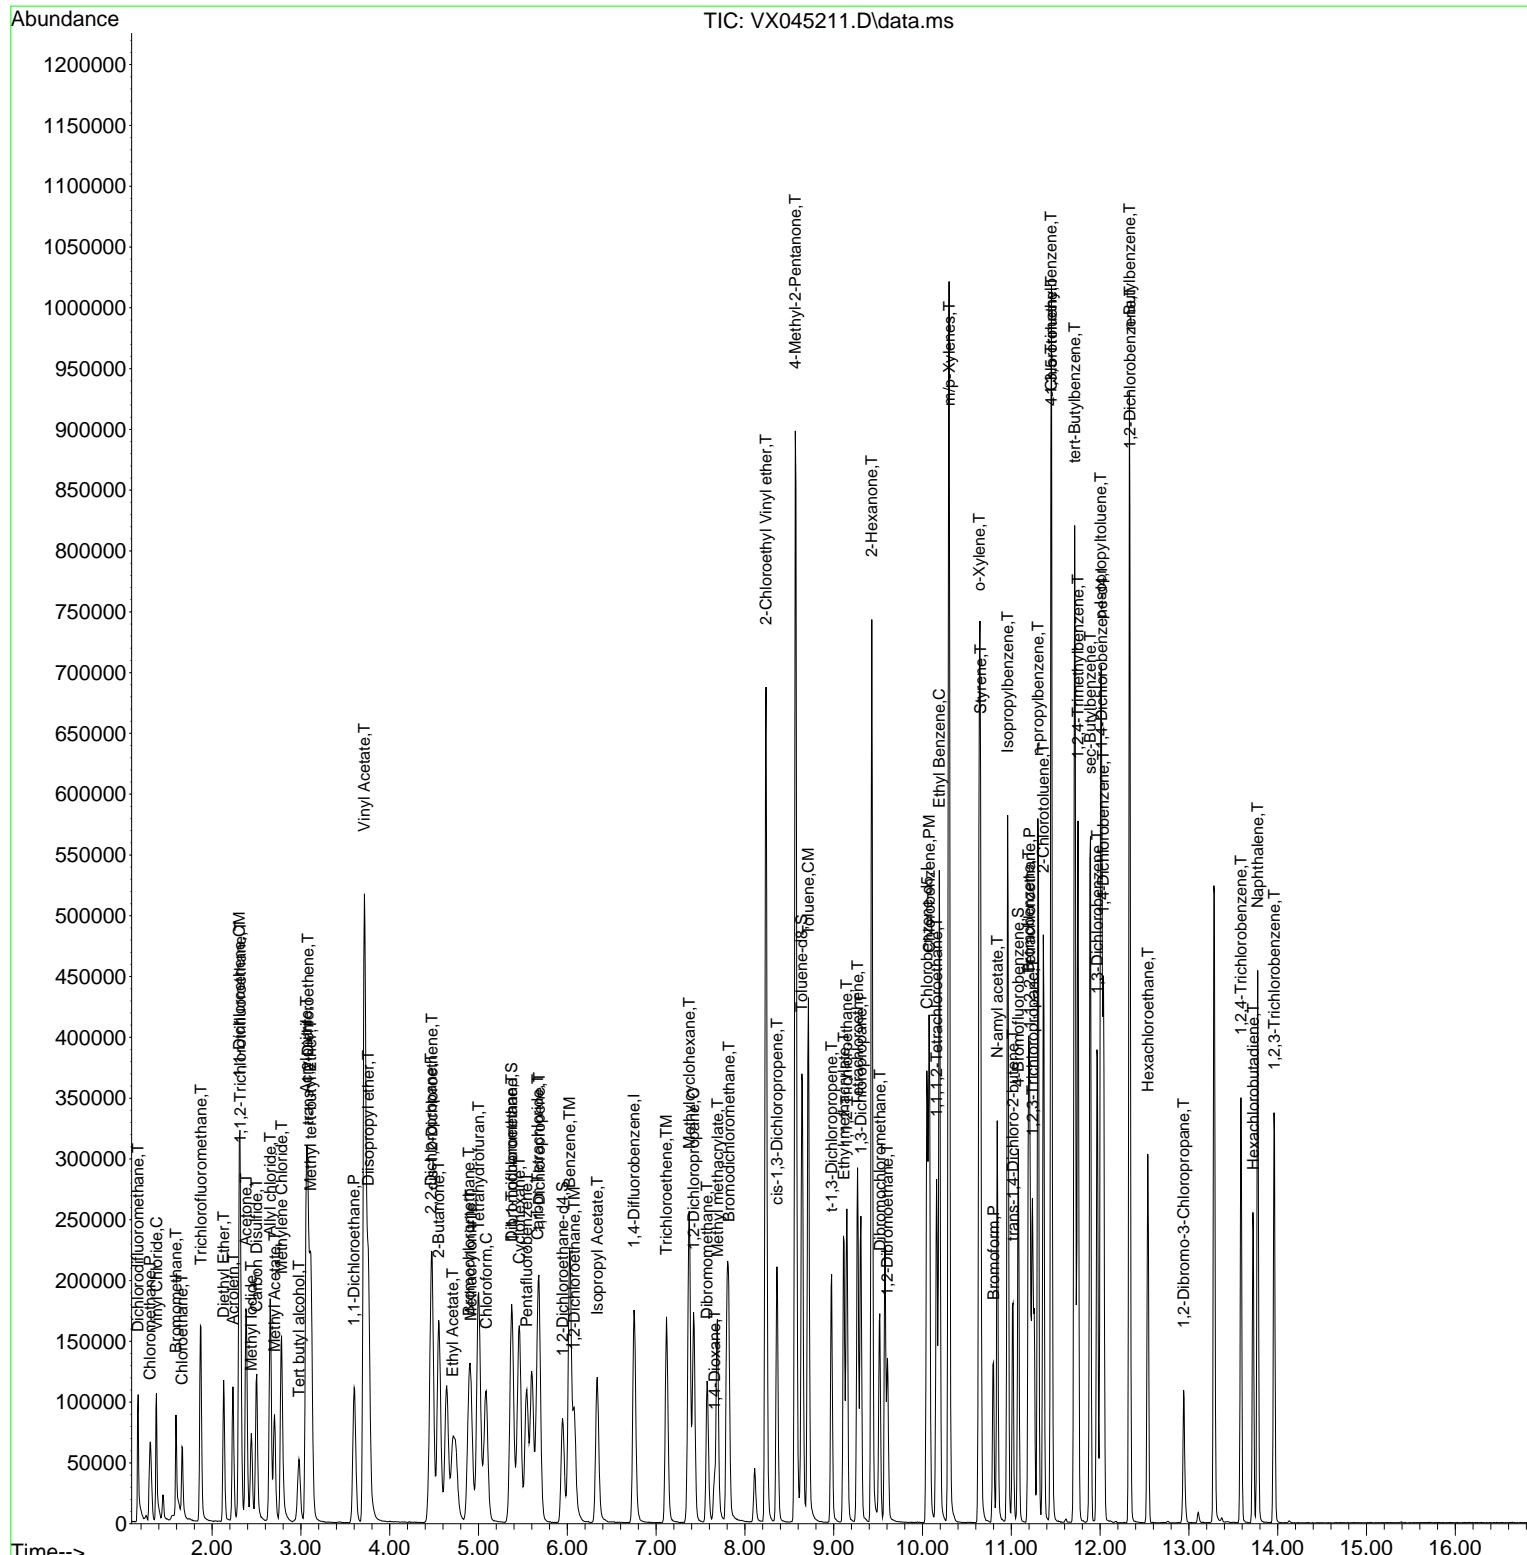



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 7
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050



Tgt Ion:168 Resp: 101357
Ion Ratio Lower Upper
168 100
99 60.3 48.2 72.4




Manual Integrations APPROVED


Reviewed By :John Carbone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#2
Dichlorodifluoromethane
Concen: 52.372 ug/l
RT: 1.167 min Scan# 13
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion: 85 Resp: 66819
Ion Ratio Lower Upper
85 100
87 33.4 17.4 52.3

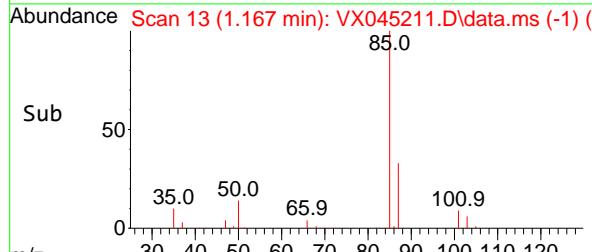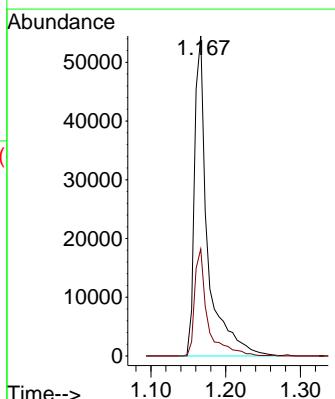



#3
Chloromethane
Concen: 47.472 ug/l
RT: 1.301 min Scan# 3
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050




Tgt Ion: 50 Resp: 7412
Ion Ratio Lower Upper
50 100
52 32.7 25.0 37.4

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

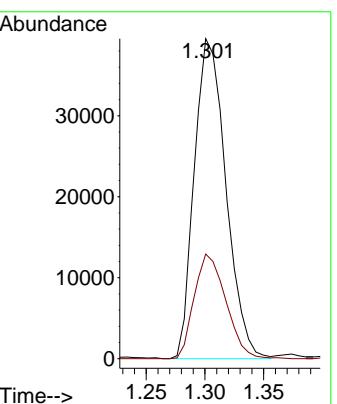


#4
Vinyl Chloride
Concen: 47.311 ug/l
RT: 1.374 min Scan# 47
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Tgt Ion: 62 Resp: 73280
Ion Ratio Lower Upper
62 100
64 32.0 24.3 36.5

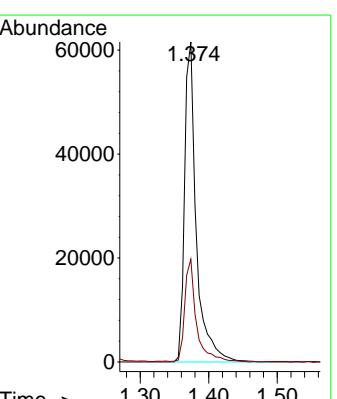



#5
Bromomethane
Concen: 50.390 ug/l
RT: 1.593 min Scan# 8
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050




Tgt Ion: 94 Resp: 3068
Ion Ratio Lower Upper
94 100
96 94.3 75.0 112.4

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

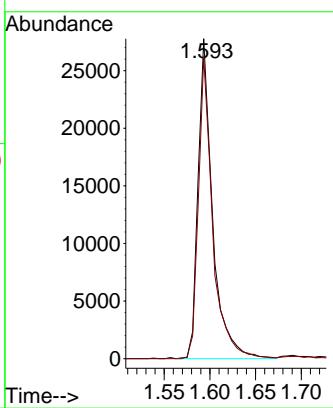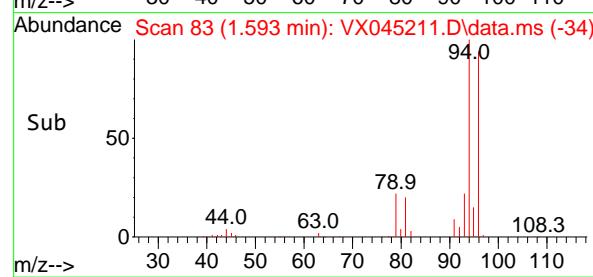


#6
Chloroethane
Concen: 54.794 ug/l
RT: 1.660 min Scan# 94
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Tgt Ion: 64 Resp: 39147
Ion Ratio Lower Upper
64 100
66 33.3 26.7 40.1

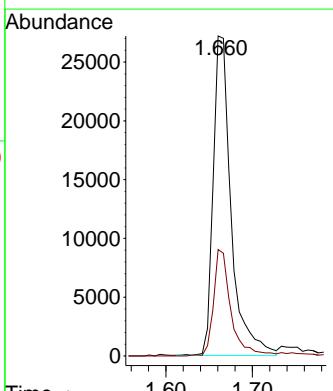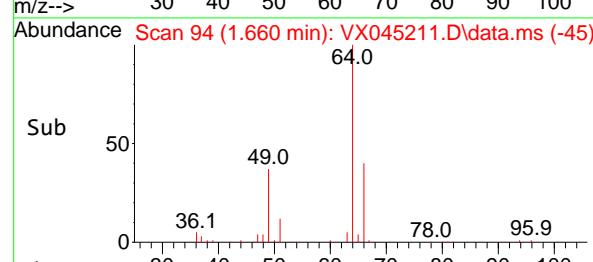



#7
Trichlorofluoromethane
Concen: 51.147 ug/l
RT: 1.874 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050

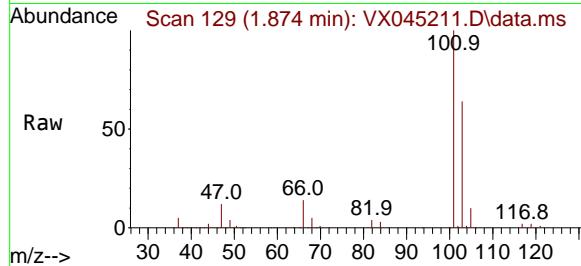


Tgt Ion: 101 Resp: 104874
Ion Ratio Lower Upper
101 100
103 64.4 52.1 78.1

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#8
Diethyl Ether
Concen: 46.681 ug/l
RT: 2.130 min Scan# 171
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Tgt Ion: 74 Resp: 37439
Ion Ratio Lower Upper
74 100
45 103.5 51.5 154.5





#9
1,1,2-Trichlorotrifluoroethane
Concen: 55.369 ug/l
RT: 2.319 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59



Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050

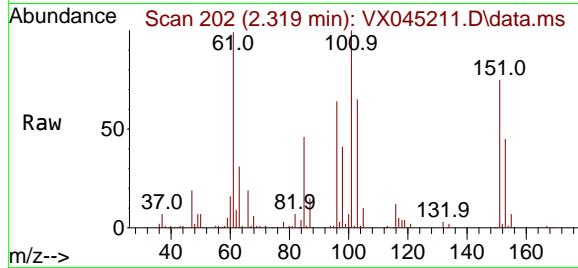

Tgt	Ion:101	Resp:	65220
	Ion Ratio	Lower	Upper
101	100		
85	46.5	36.2	54.4
151	71.0	56.4	84.6



Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#10
Methyl Iodide
Concen: 52.942 ug/l
RT: 2.441 min Scan# 222
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt	Ion:142	Resp:	77939
	Ion Ratio	Lower	Upper
142	100		
127	46.0	35.4	53.2
141	14.3	11.6	17.4

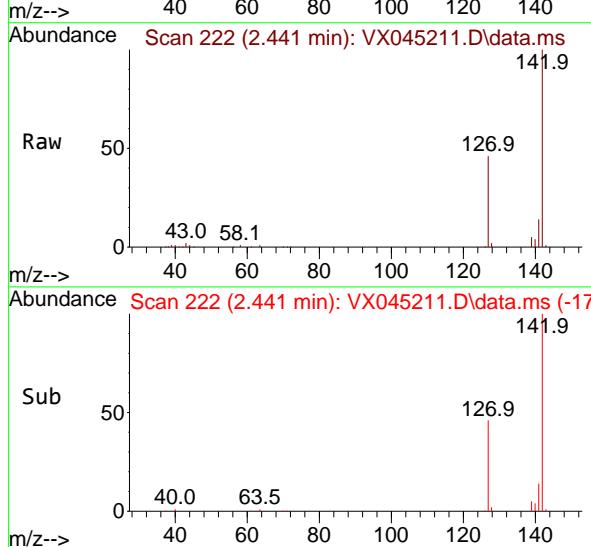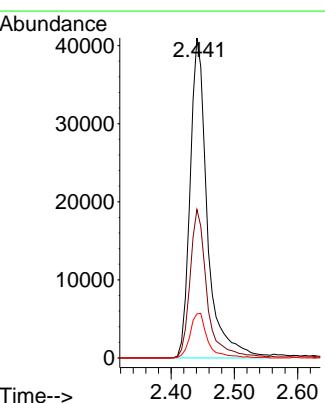



#11
Tert butyl alcohol
Concen: 194.474 ug/l
RT: 2.977 min Scan# 3
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050



Tgt Ion: 59 Resp: 59389
Ion Ratio Lower Upper
59 100
57 11.0 7.8 11.8




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#12
1,1-Dichloroethene
Concen: 50.020 ug/l
RT: 2.307 min Scan# 200
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion: 96 Resp: 62298
Ion Ratio Lower Upper
96 100
61 167.1 134.6 202.0
98 64.3 51.0 76.6





#13
Acrolein
Concen: 219.893 ug/l
RT: 2.233 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59



Instrument : MSVOA_X
ClientSampleId : VSTDCCC050

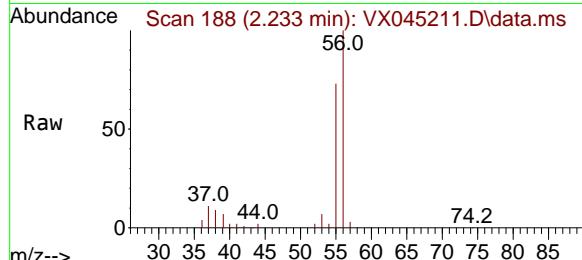

Tgt Ion: 56 Resp: 7762
Ion Ratio Lower Upper
56 100
55 70.2 56.2 84.4




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

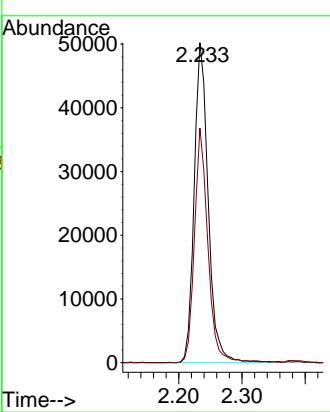

#14
Allyl chloride
Concen: 53.245 ug/l
RT: 2.654 min Scan# 257
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion: 41 Resp: 118042
Ion Ratio Lower Upper
41 100
39 68.3 53.8 80.8
76 31.7 25.2 37.8

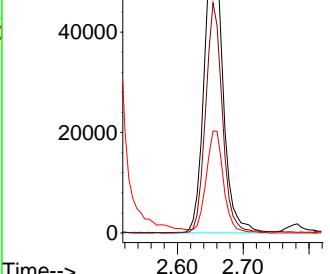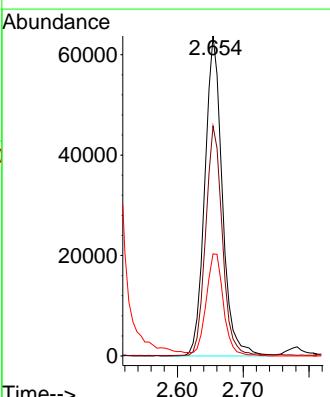



#15
Acrylonitrile
Concen: 255.519 ug/l
RT: 3.063 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59



Instrument : MSVOA_X
ClientSampleId : VSTDCCC050



Tgt Ion: 53 Resp: 209133
Ion Ratio Lower Upper
53 100
52 83.6 66.2 99.2
51 36.8 29.0 43.4





Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#16
Acetone
Concen: 258.004 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion: 43 Resp: 192994
Ion Ratio Lower Upper
43 100
58 29.5 24.2 36.4

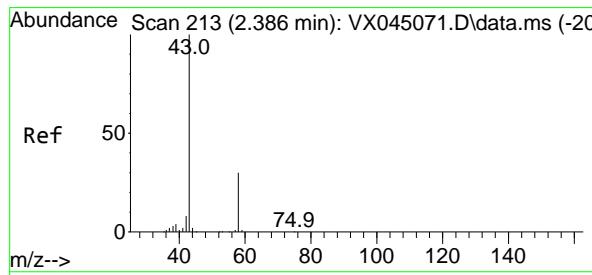



#17
Carbon Disulfide
Concen: 47.279 ug/l
RT: 2.502 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59



Instrument : MSVOA_X
ClientSampleId : VSTDCCC050



Tgt Ion: 76 Resp: 15683
Ion Ratio Lower Upper
76 100
78 9.5 6.6 9.8



Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#18
Methyl Acetate
Concen: 56.465 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion: 43 Resp: 101610
Ion Ratio Lower Upper
43 100
74 22.4 17.4 26.2

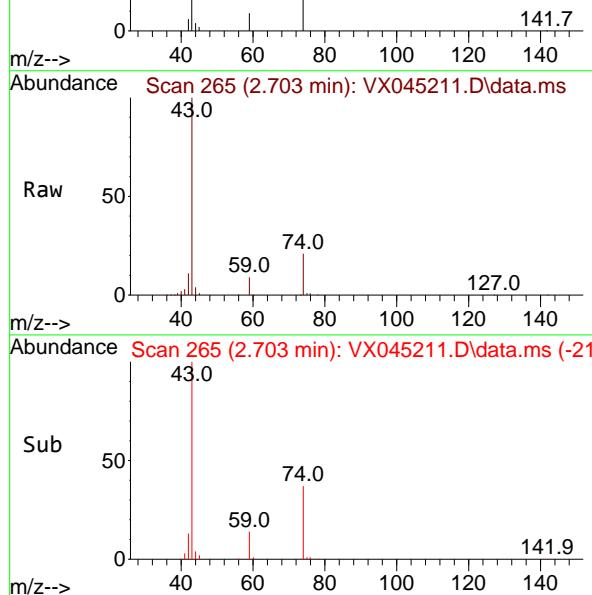



#19
Methyl tert-butyl Ether
Concen: 49.992 ug/l
RT: 3.111 min Scan# 3
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050

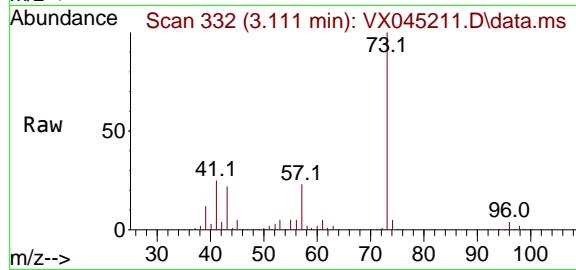


Tgt Ion: 73 Resp: 20889
Ion Ratio Lower Upper
73 100
57 23.0 18.5 27.7

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

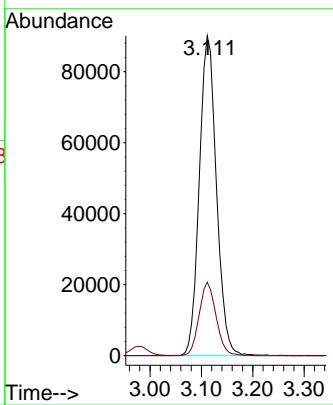


#20
Methylene Chloride
Concen: 48.811 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Tgt Ion: 84 Resp: 72325
Ion Ratio Lower Upper
84 100
49 128.7 106.5 159.7
51 37.0 32.1 48.1
86 64.0 50.0 75.0

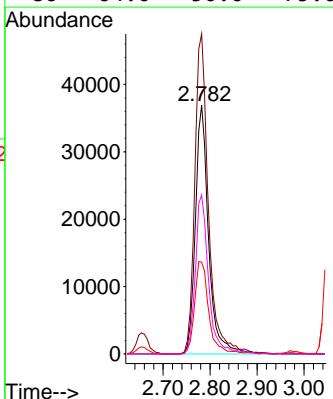



#21
trans-1,2-Dichloroethene
Concen: 50.781 ug/l
RT: 3.081 min Scan# 31
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59



Instrument : MSVOA_X
ClientSampleId : VSTDCCC050



Tgt Ion: 96 Resp: 62481
Ion Ratio Lower Upper
96 100
61 143.0 117.0 175.4
98 62.2 53.4 80.2





Manual Integrations APPROVED


Reviewed By :John Carbone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

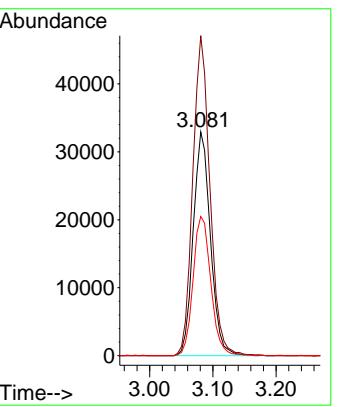

#22
Diisopropyl ether
Concen: 51.685 ug/l
RT: 3.758 min Scan# 438
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

Tgt Ion: 45 Resp: 233037
Ion Ratio Lower Upper
45 100
43 73.5 54.9 82.3
87 25.3 21.0 31.4
59 10.8 8.7 13.1

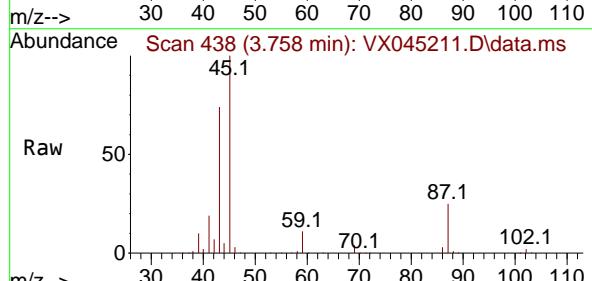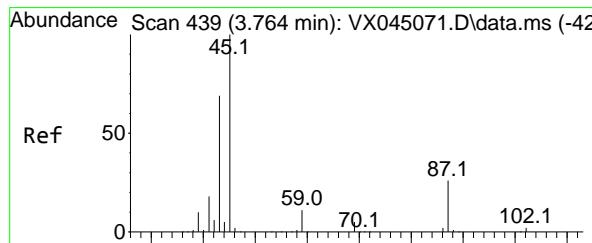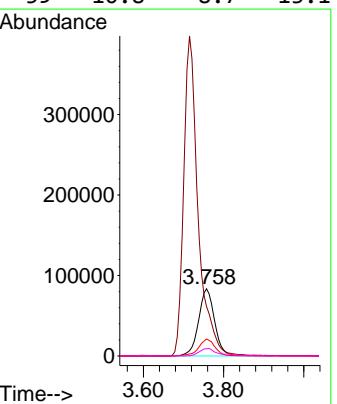

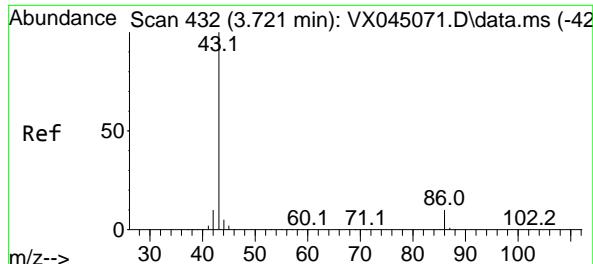

#23

Vinyl Acetate

Concen: 264.646 ug/l

RT: 3.715 min Scan# 412

Delta R.T. -0.006 min

Lab File: VX045211.D

Acq: 11 Mar 2025 09:59

Instrument:

MSVOA_X

ClientSampleId :

VSTDCCC050






Tgt Ion: 43 Resp: 995760

Ion Ratio Lower Upper

43 100

86 9.5 8.1 12.1

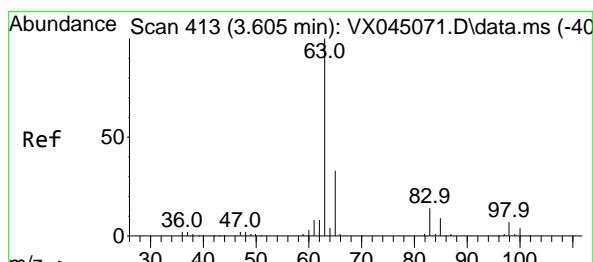**Manual Integrations
APPROVED**
Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

#24

1,1-Dichloroethane


Concen: 49.921 ug/l

RT: 3.599 min Scan# 412

Delta R.T. -0.006 min

Lab File: VX045211.D

Acq: 11 Mar 2025 09:59





Tgt Ion: 63 Resp: 126144


Ion Ratio Lower Upper

63 100

98 7.3 3.4 10.2


100 4.1 2.1 6.5





#25
2-Butanone
Concen: 261.614 ug/l
RT: 4.550 min Scan# 5
Delta R.T. -0.012 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050




Tgt Ion: 43 Resp: 29456
Ion Ratio Lower Upper
43 100
72 24.3 20.0 30.0

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

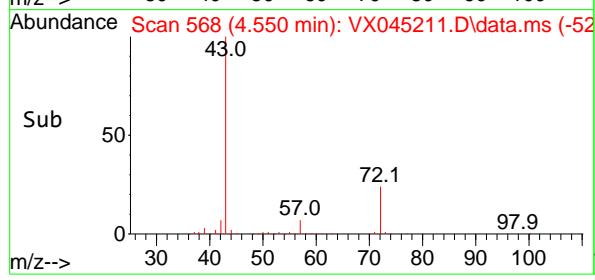


#26
2,2-Dichloropropane
Concen: 77.390 ug/l
RT: 4.465 min Scan# 554
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Tgt Ion: 77 Resp: 91726
Ion Ratio Lower Upper
77 100
97 22.3 12.4 37.0

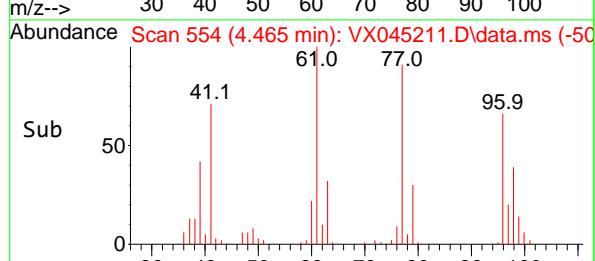

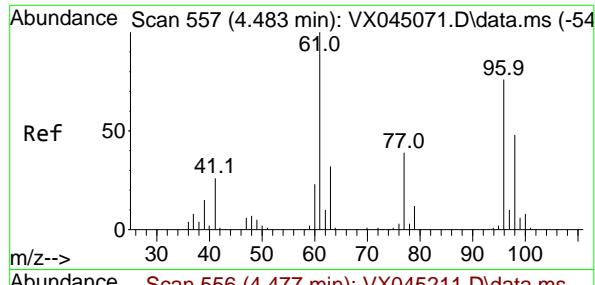

#27
cis-1,2-Dichloroethene
 Concen: 50.382 ug/l
 RT: 4.477 min Scan# 51
 Delta R.T. -0.006 min
 Lab File: VX045211.D
 Acq: 11 Mar 2025 09:59


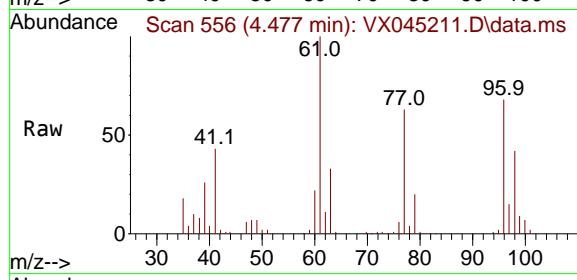


Tgt Ion: 96 Resp: 76520


Ion	Ratio	Lower	Upper
96	100		
61	148.9	0.0	283.2
98	63.1	0.0	128.0

Manual Integrations APPROVED

Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025







#28
 Bromochloromethane
 Concen: 48.726 ug/l
 RT: 4.891 min Scan# 624
 Delta R.T. -0.006 min
 Lab File: VX045211.D
 Acq: 11 Mar 2025 09:59



Tgt Ion: 49 Resp: 58687

Ion	Ratio	Lower	Upper
49	100		
129	1.7	0.0	3.4
130	69.2	56.1	84.1

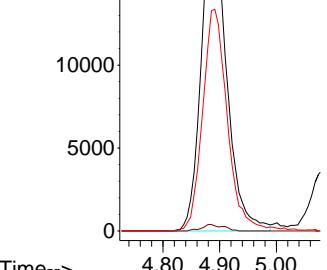



#29

Tetrahydrofuran

Concen: 245.874 ug/l

RT: 5.001 min Scan# 6

Delta R.T. -0.006 min


Lab File: VX045211.D

Acq: 11 Mar 2025 09:59

Instrument : MSVOA_X

ClientSampleId :



VSTDCCC050




Tgt	Ion:	42	Ion Ratio	100	Resp:	185910
		42		42.0	Lower	34.1
		71		39.0	Upper	51.1
				31.4		47.0

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#30
Chloroform
Concen: 49.818 ug/l
RT: 5.087 min Scan# 656
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Tgt	Ion:	83	Ion Ratio	100	Resp:	125081
		83		64.5	Lower	51.4
		85			Upper	77.2

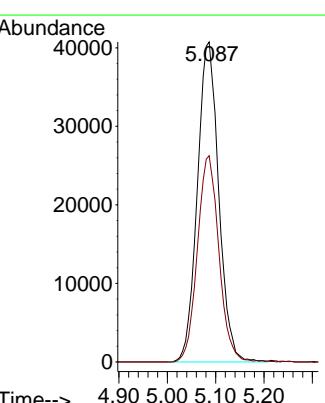






#31
Cyclohexane
Concen: 51.345 ug/l
RT: 5.458 min Scan# 7
Instrument : MSVOA_X
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59
ClientSampleId : VSTDCCC050




Tgt Ion: 56 Resp: 112624
Ion Ratio Lower Upper
56 100
69 29.7 23.4 35.2
84 83.4 69.4 104.2

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

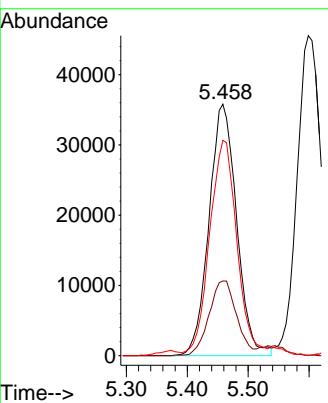


#32
1,1,1-Trichloroethane
Concen: 50.816 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59





Tgt Ion: 97 Resp: 103045
Ion Ratio Lower Upper
97 100
99 64.7 51.6 77.4
61 50.2 38.4 57.6

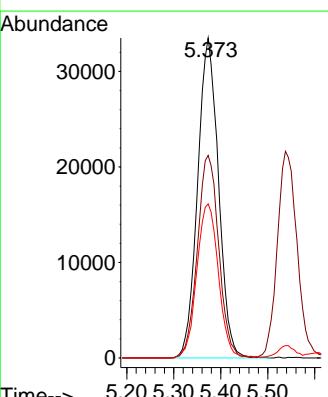





#33
1,2-Dichloroethane-d4
Concen: 49.818 ug/l
RT: 5.946 min Scan# 7
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

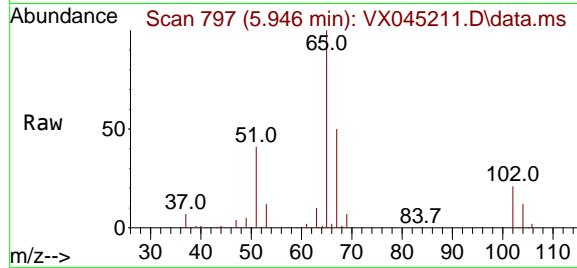


Tgt Ion: 65 Resp: 8031:
Ion Ratio Lower Upper
65 100
67 52.3 0.0 106.2

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

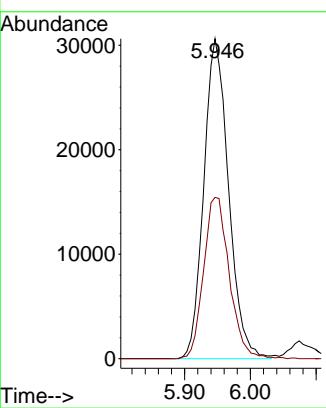


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 929
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

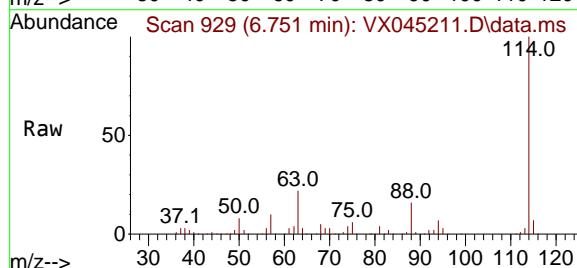


Tgt Ion:114 Resp: 176548
Ion Ratio Lower Upper
114 100
63 21.9 0.0 41.8
88 16.1 0.0 32.8

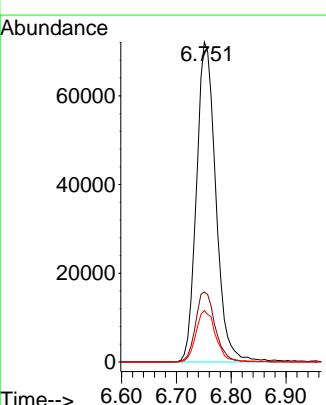



#35
 Dibromofluoromethane
 Concen: 53.104 ug/l
 RT: 5.373 min Scan# 7
 Delta R.T. -0.012 min
 Lab File: VX045211.D
 Acq: 11 Mar 2025 09:59




Instrument :
 MSVOA_X
 ClientSampleId :
 VSTDCCC050




Tgt Ion:113 Resp: 6269
 Ion Ratio Lower Upper
 113 100
 111 102.0 81.8 122.6
 192 17.4 14.3 21.5

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

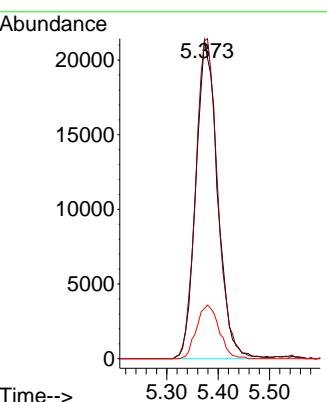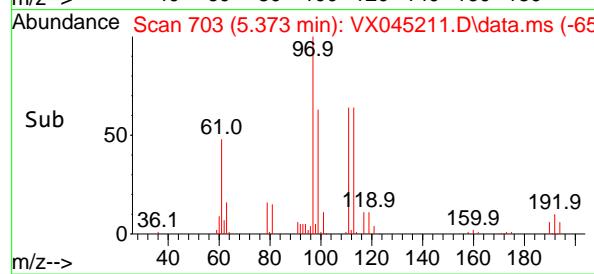


#36
 1,1-Dichloropropene
 Concen: 51.860 ug/l
 RT: 5.684 min Scan# 754
 Delta R.T. -0.006 min
 Lab File: VX045211.D
 Acq: 11 Mar 2025 09:59




Tgt Ion: 75 Resp: 83960
 Ion Ratio Lower Upper
 75 100
 110 33.7 16.9 50.6
 77 30.3 24.5 36.7



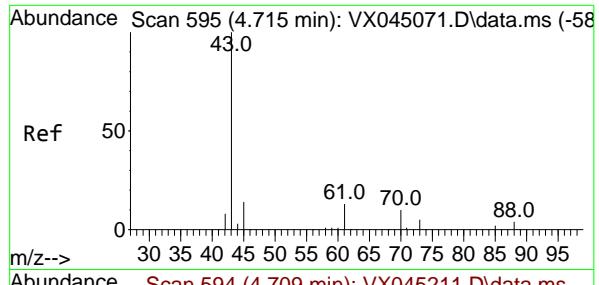

#37
Ethyl Acetate
Concen: 51.851 ug/l
RT: 4.709 min Scan# 51
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050

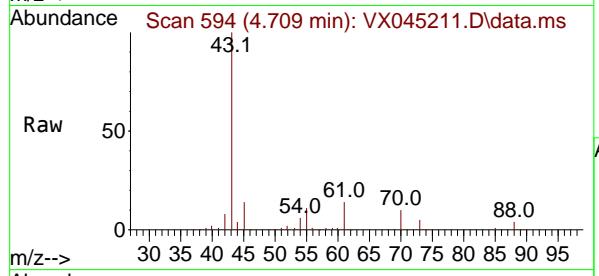

Tgt Ion: 43 Resp: 108170
Ion Ratio Lower Upper
43 100
61 12.8 10.8 16.2
70 10.0 7.7 11.5




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

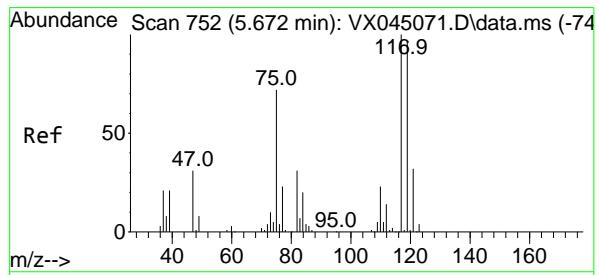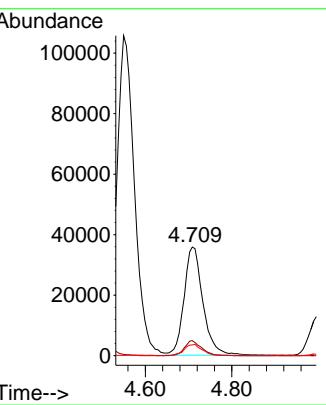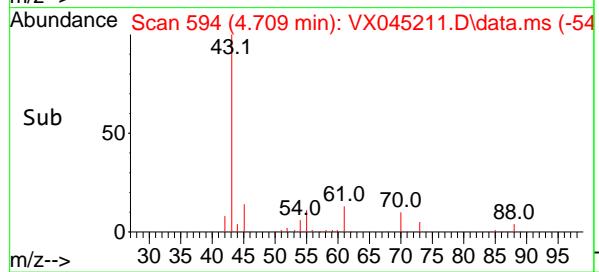

#38
Carbon Tetrachloride
Concen: 52.948 ug/l
RT: 5.666 min Scan# 751
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion:117 Resp: 87028
Ion Ratio Lower Upper
117 100
119 94.5 76.7 115.1
121 29.6 25.5 38.3

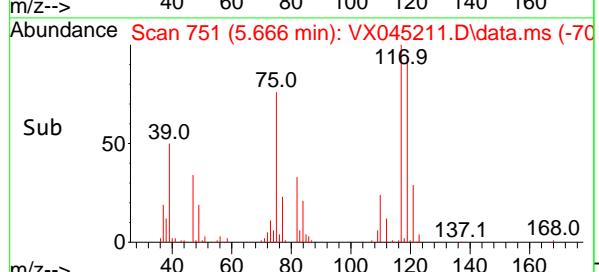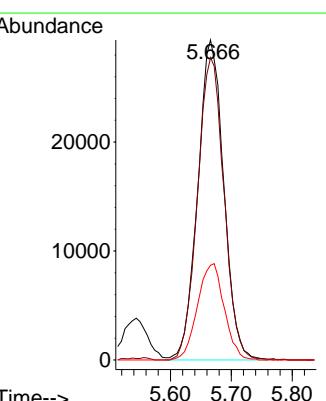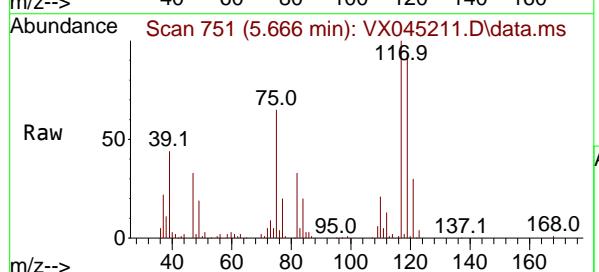



#39
Methylcyclohexane
Concen: 56.638 ug/l
RT: 7.373 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050

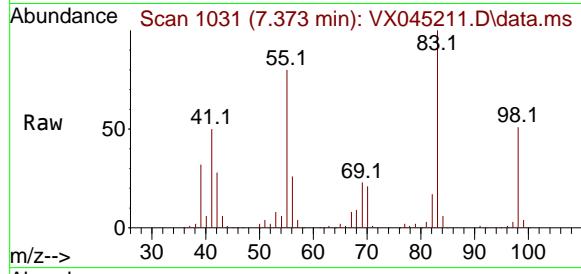


Tgt Ion: 83 Resp: 10987:
Ion Ratio Lower Upper
83 100
55 79.8 63.0 94.4
98 50.7 39.7 59.5

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

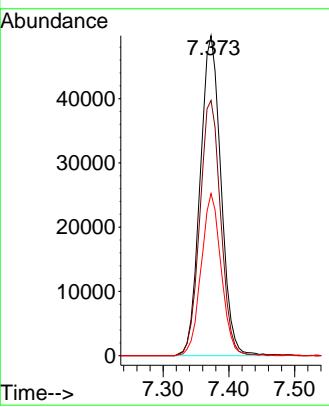


#40
Benzene
Concen: 51.320 ug/l
RT: 6.025 min Scan# 810
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

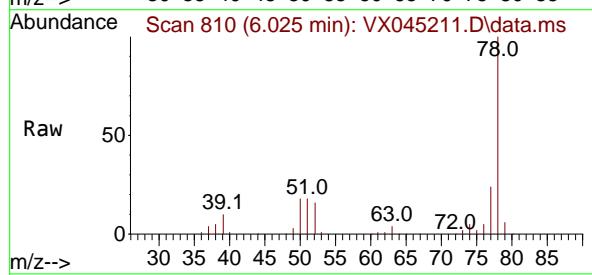


Tgt Ion: 78 Resp: 262366
Ion Ratio Lower Upper
78 100
77 24.0 18.8 28.2

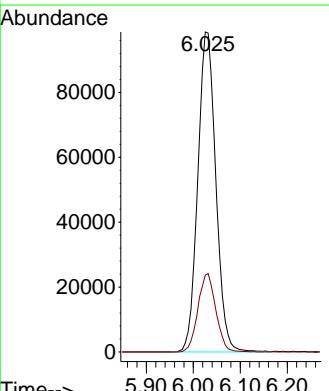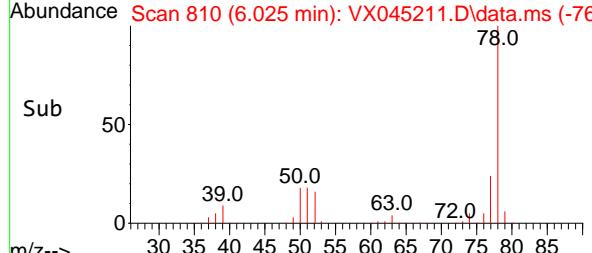



#41
Methacrylonitrile
Concen: 53.315 ug/l
RT: 4.916 min Scan# 61
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050




Tgt Ion: 41 Resp: 6014:
Ion Ratio Lower Upper
41 100
39 56.5 44.6 67.0
67 69.3 53.9 80.9
52 30.5 23.3 34.9

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#42
1,2-Dichloroethane
Concen: 52.356 ug/l
RT: 6.080 min Scan# 819
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Tgt Ion: 62 Resp: 96385
Ion Ratio Lower Upper
62 100
98 8.9 0.0 18.2





#43
Isopropyl Acetate
Concen: 54.564 ug/l
RT: 6.336 min Scan# 8
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050




Tgt Ion: 43 Resp: 16832
Ion Ratio Lower Upper
43 100
61 17.7 14.9 22.3
87 11.9 9.4 14.2

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

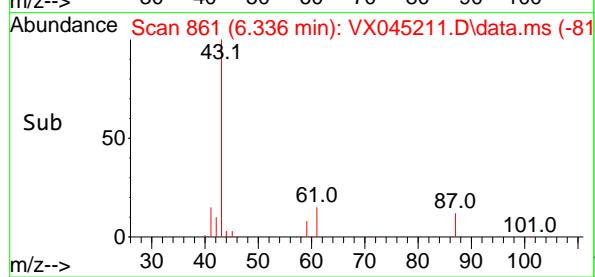


#44
Trichloroethene
Concen: 52.042 ug/l
RT: 7.117 min Scan# 989
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Tgt Ion:130 Resp: 62473
Ion Ratio Lower Upper
130 100
95 102.1 0.0 205.0

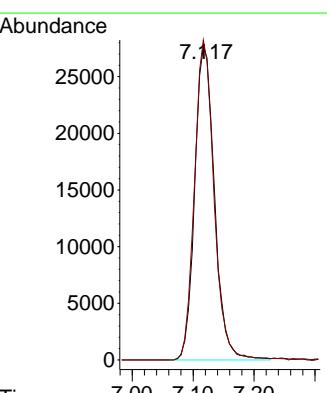



#45
1,2-Dichloropropane
Concen: 50.991 ug/l
RT: 7.422 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050



Tgt Ion: 63 Resp: 6702
Ion Ratio Lower Upper
63 100
65 31.4 24.7 37.1




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#46
Dibromomethane
Concen: 52.911 ug/l
RT: 7.574 min Scan# 1064
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion: 93 Resp: 49158
Ion Ratio Lower Upper
93 100
95 82.7 65.8 98.8
174 87.6 72.2 108.2

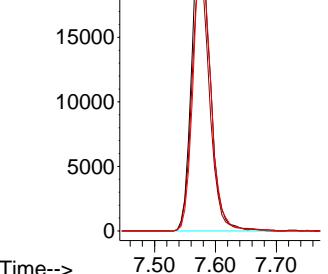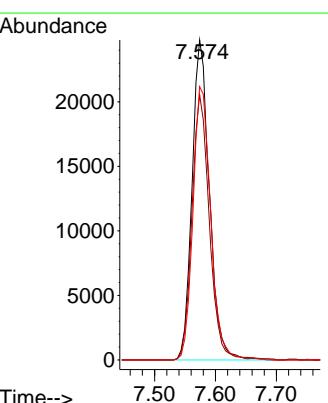



#47
Bromodichloromethane
Concen: 53.986 ug/l
RT: 7.818 min Scan# 1104
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050




Tgt Ion:	83	Resp:	9838
Ion Ratio		Lower	Upper
83	100		
85	64.3	51.1	76.7
127	8.4	6.4	9.6

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#48
Methyl methacrylate
Concen: 53.663 ug/l
RT: 7.690 min Scan# 1083
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59



Tgt Ion:	41	Resp:	83051
Ion Ratio		Lower	Upper
41	100		
69	78.6	63.0	94.6
39	63.7	47.5	71.3

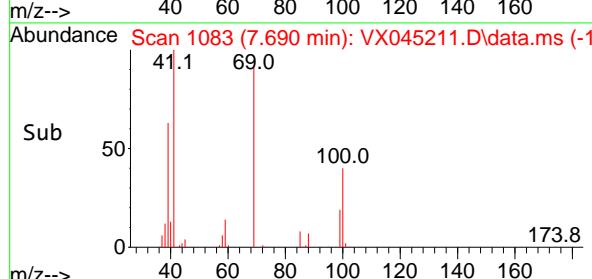







#49
1,4-Dioxane
Concen: 900.059 ug/l
RT: 7.659 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

Instrument : MSVOA_X
ClientSampleId : VSTDCCC050

Tgt Ion: 88 Resp: 29381
Ion Ratio Lower Upper
88 100
43 38.0 28.7 43.1
58 70.1 55.8 83.8




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

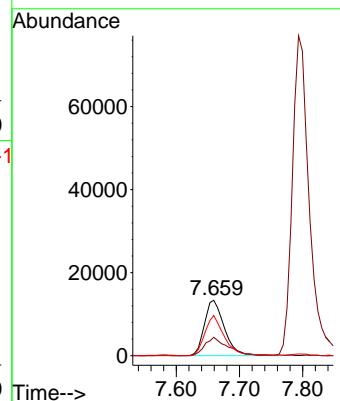

#50
Toluene-d8
Concen: 51.586 ug/l
RT: 8.641 min Scan# 1239
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion: 98 Resp: 220779
Ion Ratio Lower Upper
98 100
100 66.2 52.0 78.0

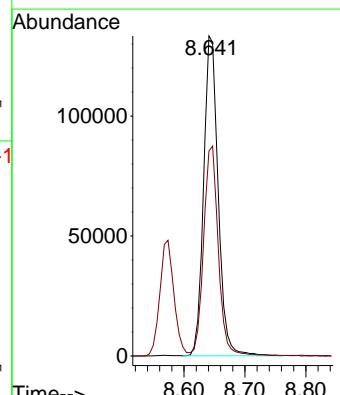



#51
4-Methyl-2-Pentanone
Concen: 271.045 ug/l
RT: 8.568 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050



Tgt Ion: 43 Resp: 56141
Ion Ratio Lower Upper
43 100
58 36.6 29.2 43.8




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

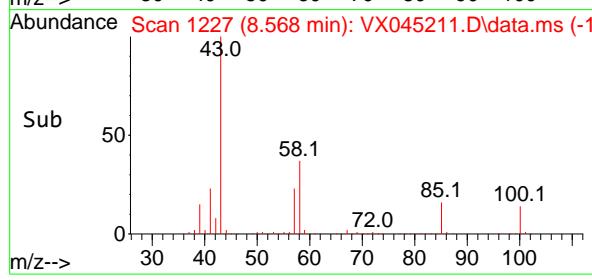

#52
Toluene
Concen: 52.972 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion: 92 Resp: 158892
Ion Ratio Lower Upper
92 100
91 173.6 138.9 208.3





#53
t-1,3-Dichloropropene
Concen: 59.606 ug/l
RT: 8.976 min Scan# 1193
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050




Tgt Ion: 75 Resp: 9080
Ion Ratio Lower Upper
75 100
77 31.4 26.5 39.7

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

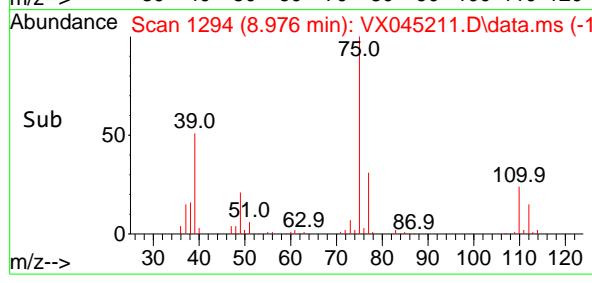


#54
cis-1,3-Dichloropropene
Concen: 57.592 ug/l
RT: 8.360 min Scan# 1193
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Tgt Ion: 75 Resp: 102314
Ion Ratio Lower Upper
75 100
77 31.4 24.7 37.1
39 53.4 40.7 61.1





#55
1,1,2-Trichloroethane
Concen: 51.661 ug/l
RT: 9.147 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59



Instrument : MSVOA_X
ClientSampleId : VSTDCCC050



Tgt Ion: 97 Resp: 63791
Ion Ratio Lower Upper
97 100
83 90.9 69.4 104.2
85 57.2 44.1 66.1
99 64.1 50.7 76.1





Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#56
Ethyl methacrylate
Concen: 55.894 ug/l
RT: 9.116 min Scan# 1317
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion: 69 Resp: 104915
Ion Ratio Lower Upper
69 100
41 71.9 57.0 85.4
39 44.3 34.2 51.4

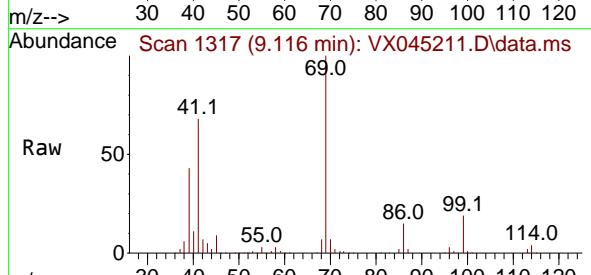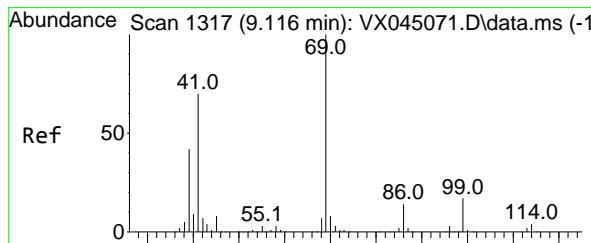



#57
1,3-Dichloropropane
Concen: 52.131 ug/l
RT: 9.305 min Scan# 11140
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050

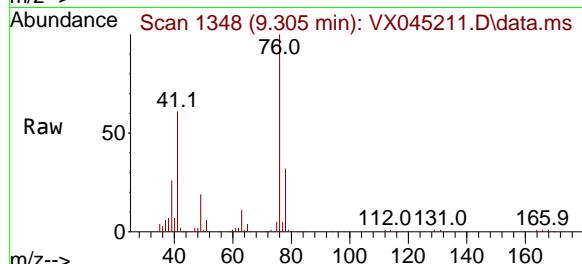

Tgt Ion: 76 Resp: 11140
Ion Ratio Lower Upper
76 100
78 32.2 25.5 38.3




Manual Integrations APPROVED


Reviewed By :John Carbone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

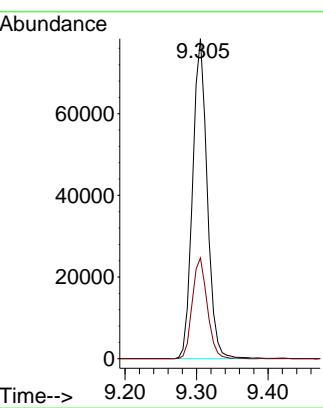

#58
2-Chloroethyl Vinyl ether
Concen: 291.597 ug/l
RT: 8.238 min Scan# 1173
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion: 63 Resp: 266994
Ion Ratio Lower Upper
63 100
106 26.2 21.5 32.3

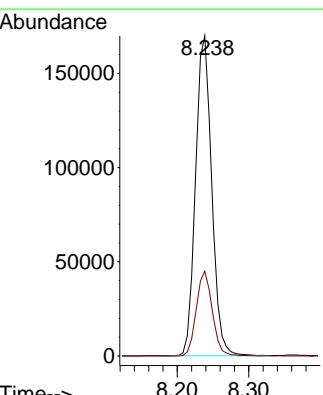



#59
2-Hexanone
Concen: 269.382 ug/l
RT: 9.427 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050



Tgt Ion: 43 Resp: 40427:
Ion Ratio Lower Upper
43 100
58 51.9 25.9 77.6




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#60
Dibromochloromethane
Concen: 55.267 ug/l
RT: 9.519 min Scan# 1383
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion:129 Resp: 71357
Ion Ratio Lower Upper
129 100
127 77.6 38.5 115.5

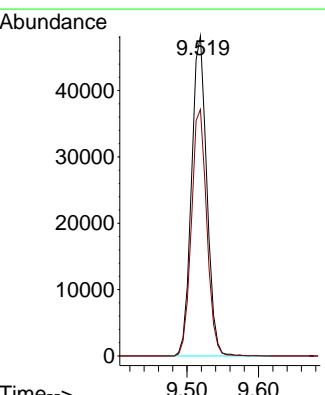



#61
1,2-Dibromoethane
Concen: 53.438 ug/l
RT: 9.604 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050



Tgt Ion:107 Resp: 6587
Ion Ratio Lower Upper
107 100
109 92.1 76.1 114.1




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#62
4-Bromofluorobenzene
Concen: 55.511 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

Tgt Ion: 95 Resp: 78726
Ion Ratio Lower Upper
95 100
174 72.2 0.0 148.2
176 70.8 0.0 141.4




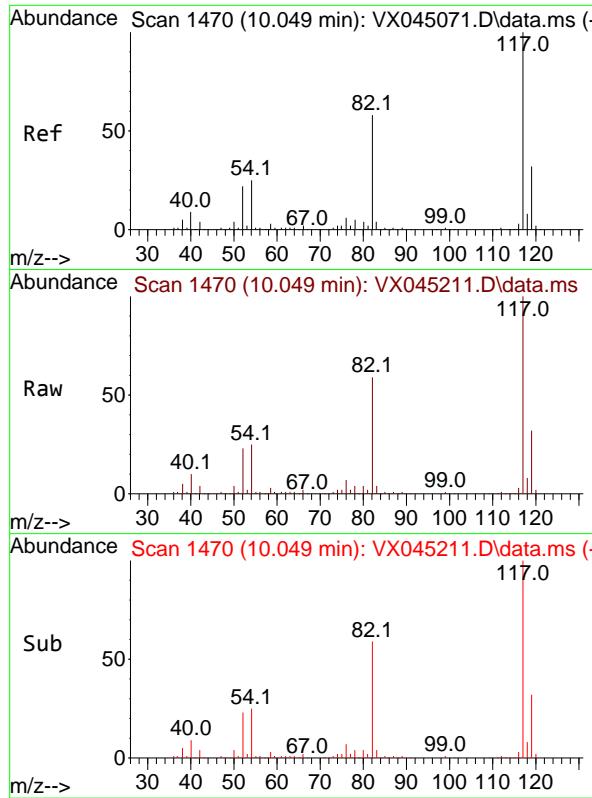


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

Instrument : MSVOA_X
ClientSampleId : VSTDCCC050


Manual Integrations
APPROVED


Reviewed By :John Carbone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

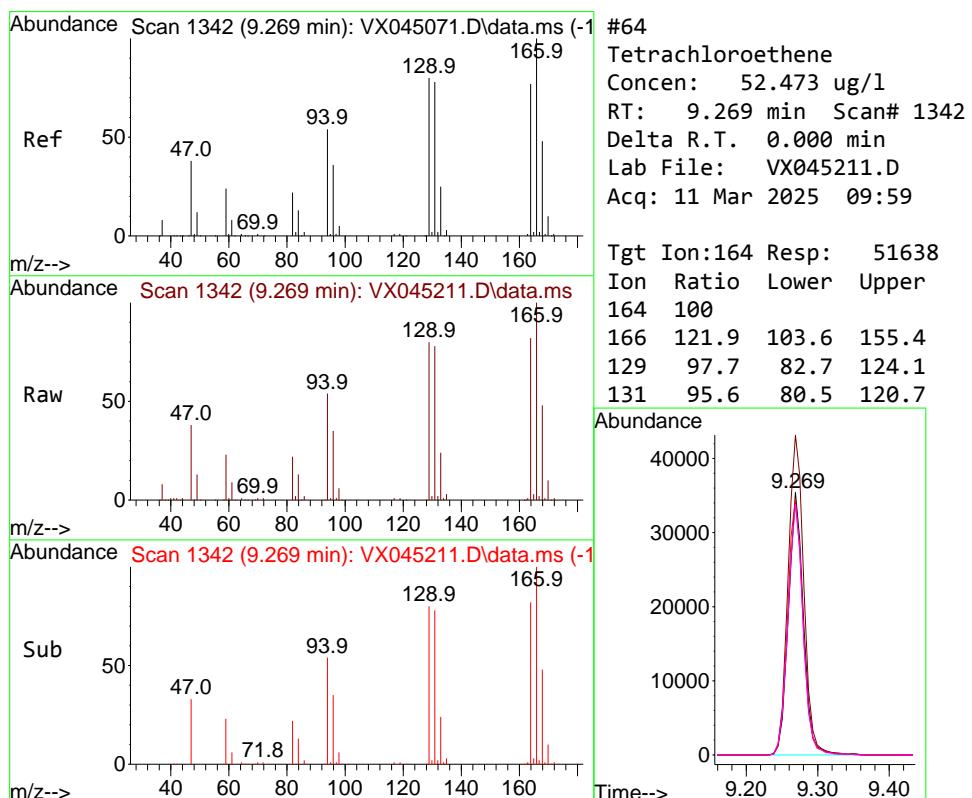

#64
Tetrachloroethene
Concen: 52.473 ug/l
RT: 9.269 min Scan# 1342
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion:164 Resp: 51638
Ion Ratio Lower Upper
164 100
166 121.9 103.6 155.4
129 97.7 82.7 124.1
131 95.6 80.5 120.7



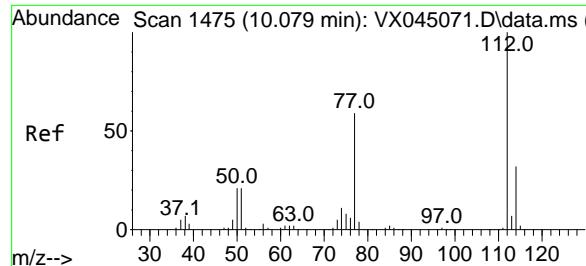

#65
Chlorobenzene
Concen: 52.928 ug/l
RT: 10.073 min Scan# 1474
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050

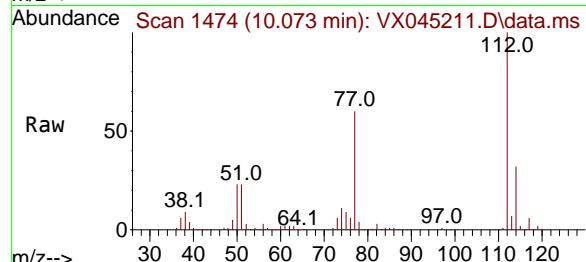

Tgt Ion:112 Resp: 17208
Ion Ratio Lower Upper
112 100
114 32.0 26.0 39.0




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

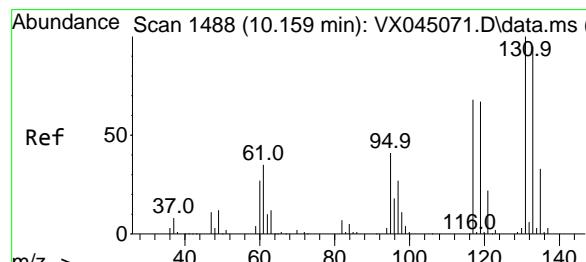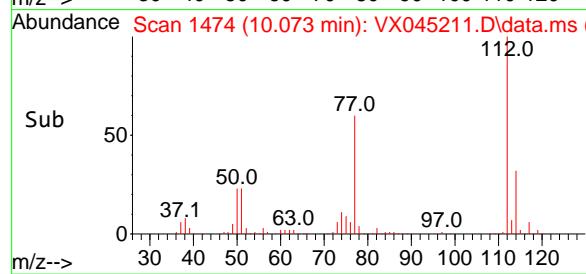


#66
1,1,1,2-Tetrachloroethane
Concen: 52.821 ug/l
RT: 10.159 min Scan# 1488
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

Tgt Ion:131 Resp: 57191
Ion Ratio Lower Upper
131 100
133 95.4 48.6 145.9
119 67.1 33.9 101.7

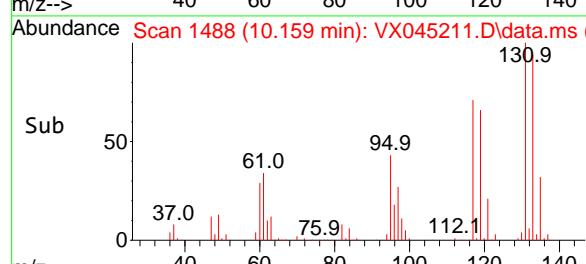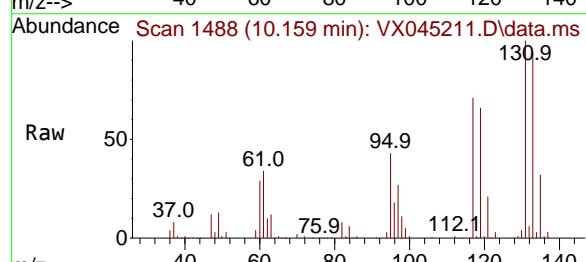





#67
 Ethyl Benzene
 Concen: 54.136 ug/l
 RT: 10.189 min Scan# 1493
 Delta R.T. 0.000 min
 Lab File: VX045211.D
 Acq: 11 Mar 2025 09:59
Instrument: MSVOA_X
ClientSampleId: VSTDCCC050




Tgt Ion: 91 Resp: 306681
 Ion Ratio Lower Upper
 91 100
 106 30.8 23.9 35.9


Manual Integrations APPROVED
 Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025




#68
 m/p-Xylenes
 Concen: 109.410 ug/l
 RT: 10.299 min Scan# 1511
 Delta R.T. 0.000 min
 Lab File: VX045211.D
 Acq: 11 Mar 2025 09:59




Tgt Ion:106 Resp: 226899
 Ion Ratio Lower Upper
 106 100
 91 208.7 165.4 248.0





#69
o-Xylene
Concen: 53.202 ug/l
RT: 10.640 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050




Tgt Ion:106 Resp: 111273
Ion Ratio Lower Upper
106 100
91 222.9 109.9 329.6

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

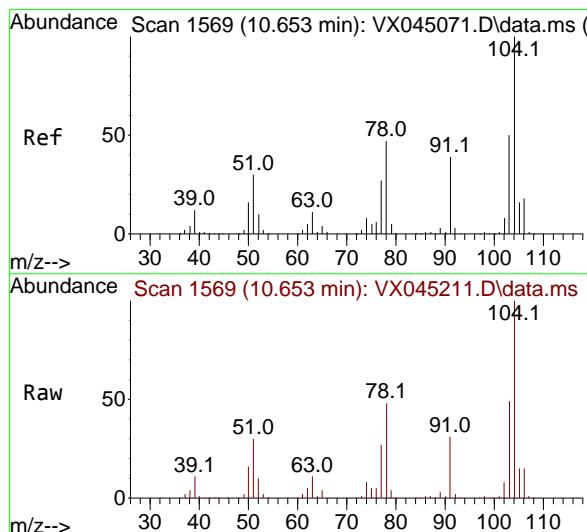


#70
Styrene
Concen: 55.460 ug/l
RT: 10.653 min Scan# 1569
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Tgt Ion:104 Resp: 187697
Ion Ratio Lower Upper
104 100
78 54.1 42.2 63.4
103 54.7 43.8 65.8








#71
Bromoform
Concen: 57.546 ug/l
RT: 10.799 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

Instrument : MSVOA_X
ClientSampleId : VSTDCCC050




Tgt	Ion:173	Resp:	4698
	Ion Ratio	Lower	Upper
173	100		
175	48.1	24.6	73.6
254	0.1	0.0	0.0



Manual Integrations APPROVED
Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

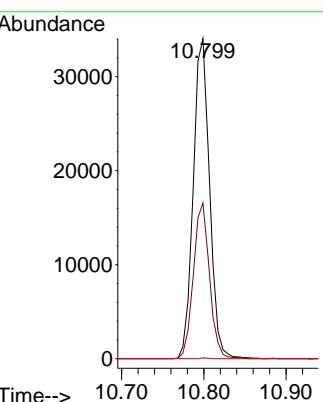


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

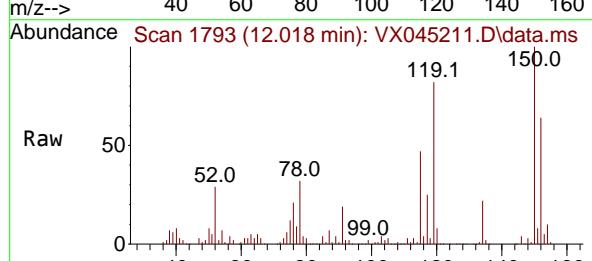


Tgt	Ion:152	Resp:	70136
	Ion Ratio	Lower	Upper
152	100		
115	89.7	44.2	132.6
150	172.9	0.0	349.0

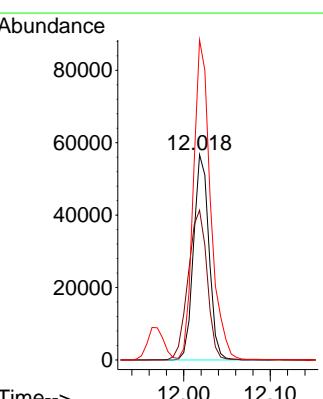



#73
Isopropylbenzene
Concen: 53.524 ug/l
RT: 10.957 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050




Tgt Ion:105 Resp: 29300
Ion Ratio Lower Upper
105 100
120 25.8 13.2 39.5

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#74
N-amyl acetate
Concen: 53.471 ug/l
RT: 10.842 min Scan# 1600
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Tgt Ion: 43 Resp: 137353
Ion Ratio Lower Upper
43 100
70 39.2 31.8 47.6
55 22.8 18.3 27.5
61 22.7 18.3 27.5



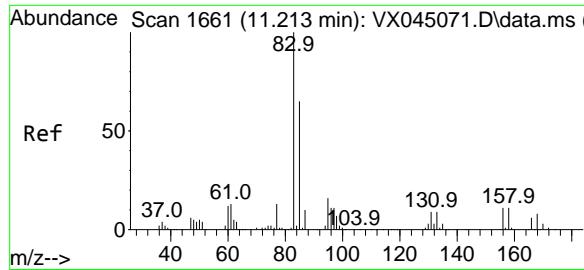

#75
1,1,2,2-Tetrachloroethane
Concen: 48.598 ug/l
RT: 11.207 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050

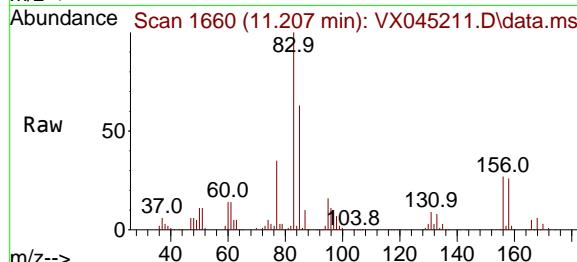


Tgt Ion: 83 Resp: 9762
Ion Ratio Lower Upper
83 100
131 9.5 4.5 13.4
85 64.3 31.7 95.1

Manual Integrations APPROVED



Reviewed By :John Carbone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

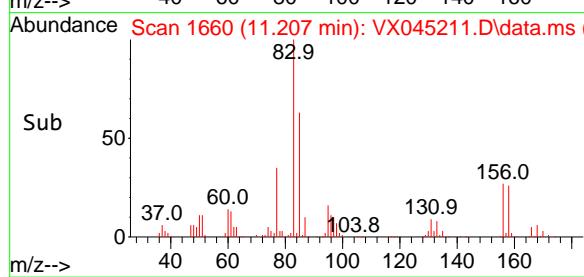


#76
1,2,3-Trichloropropane
Concen: 50.763 ug/l
RT: 11.238 min Scan# 1665
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Tgt Ion: 75 Resp: 82866
Ion Ratio Lower Upper
75 100
77 40.3 20.7 62.1

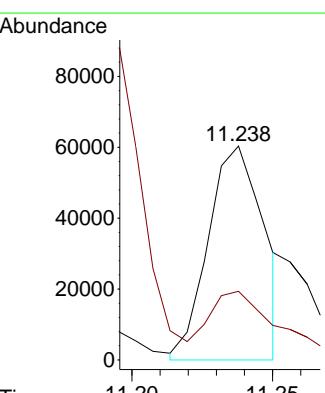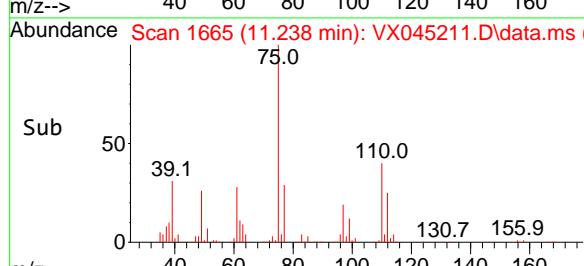



#77
Bromobenzene
Concen: 51.748 ug/l
RT: 11.195 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59



Instrument : MSVOA_X
ClientSampleId : VSTDCCC050



Tgt Ion:156 Resp: 66839
Ion Ratio Lower Upper
156 100
77 173.3 85.8 257.4
158 96.2 48.4 145.2




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

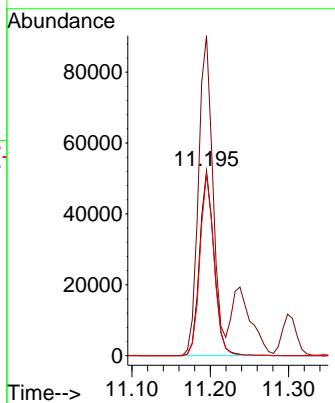

#78
n-propylbenzene
Concen: 55.815 ug/l
RT: 11.299 min Scan# 1675
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion: 91 Resp: 345156
Ion Ratio Lower Upper
91 100
120 22.0 11.2 33.6

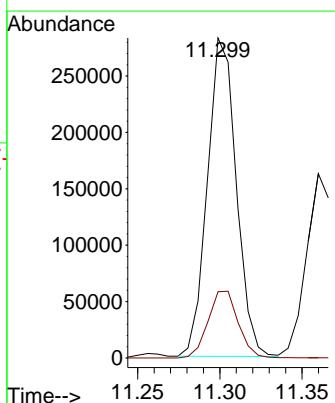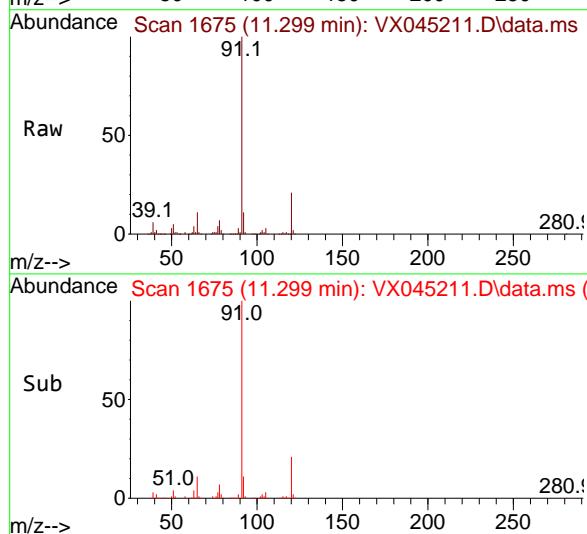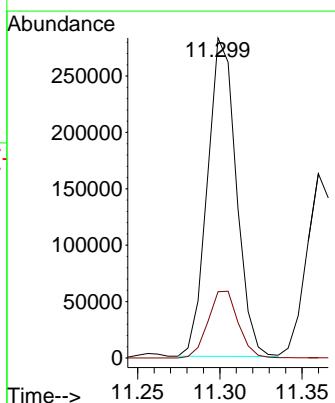



#79
2-Chlorotoluene
Concen: 51.714 ug/l
RT: 11.360 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050




Tgt Ion: 91 Resp: 20366
Ion Ratio Lower Upper
91 100
126 32.2 16.4 49.4

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

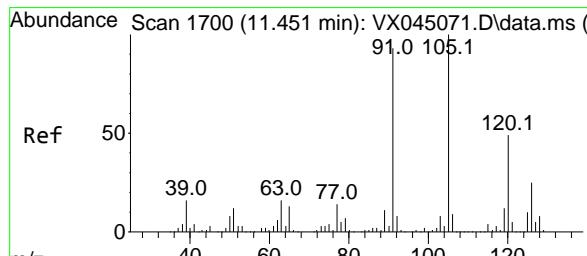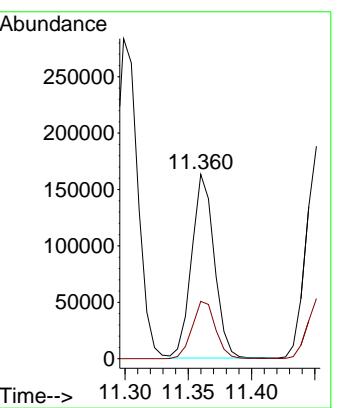


#80
1,3,5-Trimethylbenzene
Concen: 54.036 ug/l
RT: 11.445 min Scan# 1699
Delta R.T. -0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

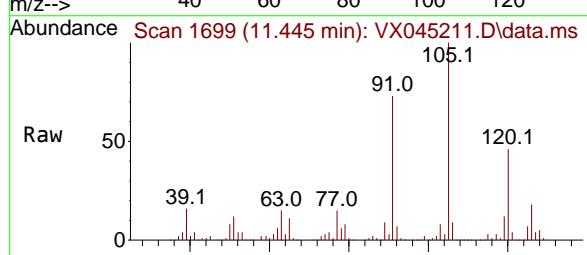

Tgt Ion:105 Resp: 239185
Ion Ratio Lower Upper
105 100
120 47.2 24.1 72.2

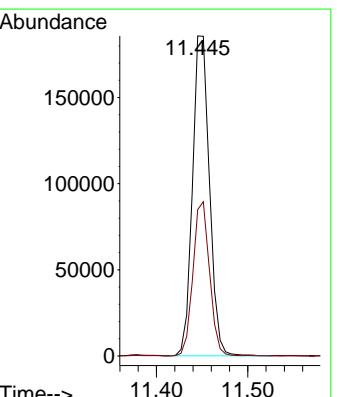


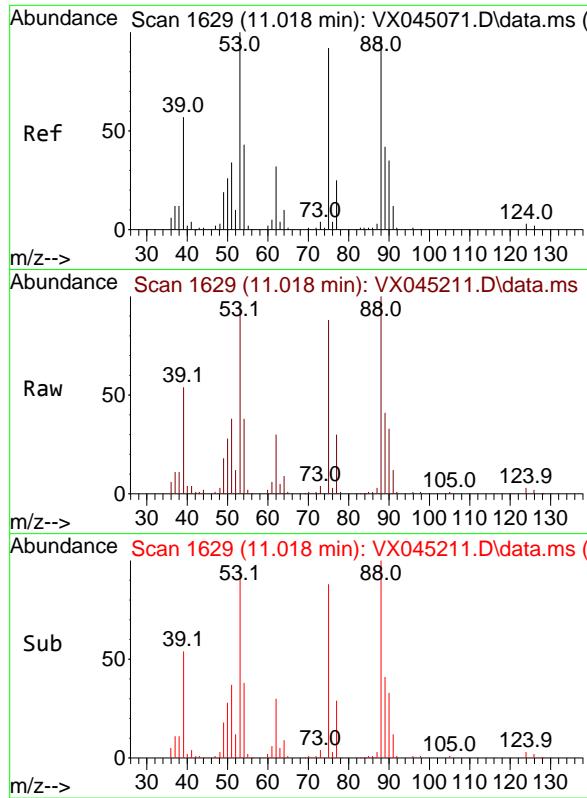


#81
trans-1,4-Dichloro-2-butene
Concen: 59.586 ug/l
RT: 11.018 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

Instrument : MSVOA_X
ClientSampleId : VSTDCCC050


**Manual Integrations
APPROVED**




Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

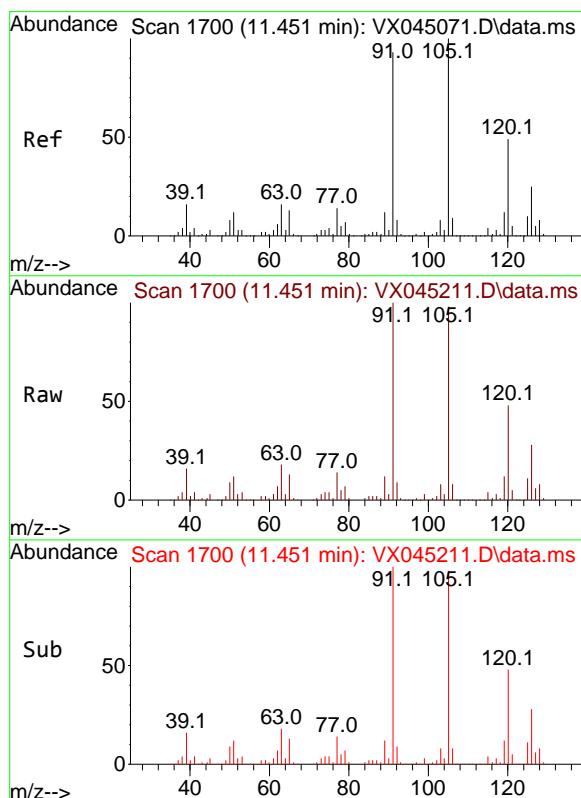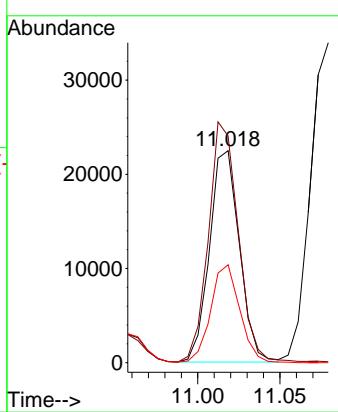

#82
4-Chlorotoluene
Concen: 53.609 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

Tgt Ion: 91 Resp: 230104
Ion Ratio Lower Upper
91 100
126 28.4 14.1 42.4

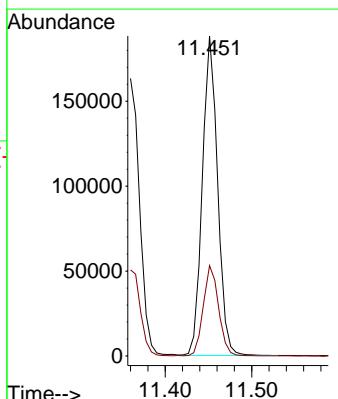



#83

tert-Butylbenzene

Concen: 52.798 ug/l

RT: 11.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX045211.D

Acq: 11 Mar 2025 09:59




Instrument:

MSVOA_X

ClientSampleId :

VSTDCCC050

**Manual Integrations
APPROVED**

 Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025


#84

1,2,4-Trimethylbenzene


Concen: 54.029 ug/l


RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX045211.D


Acq: 11 Mar 2025 09:59

 Tgt Ion:105 Resp: 240636
 Ion Ratio Lower Upper
 105 100
 120 43.9 22.1 66.1




#85
sec-Butylbenzene
Concen: 56.188 ug/l
RT: 11.890 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument :
MSVOA_X
ClientSampleId :
VSTDCCC050




Tgt Ion:105 Resp: 306100
Ion Ratio Lower Upper
105 100
134 19.3 9.8 29.4

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#86
p-Isopropyltoluene
Concen: 56.113 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59



Tgt Ion:119 Resp: 247047
Ion Ratio Lower Upper
119 100
134 25.7 12.9 38.6
91 25.6 12.7 38.0




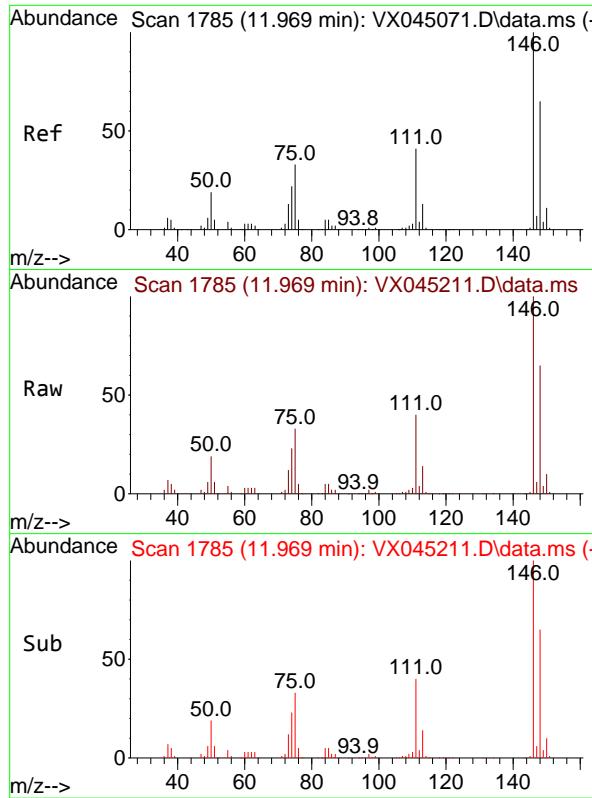


#87
1,3-Dichlorobenzene
Concen: 51.564 ug/l
RT: 11.969 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59

Instrument : MSVOA_X
ClientSampleId : VSTDCCC050


Manual Integrations
APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

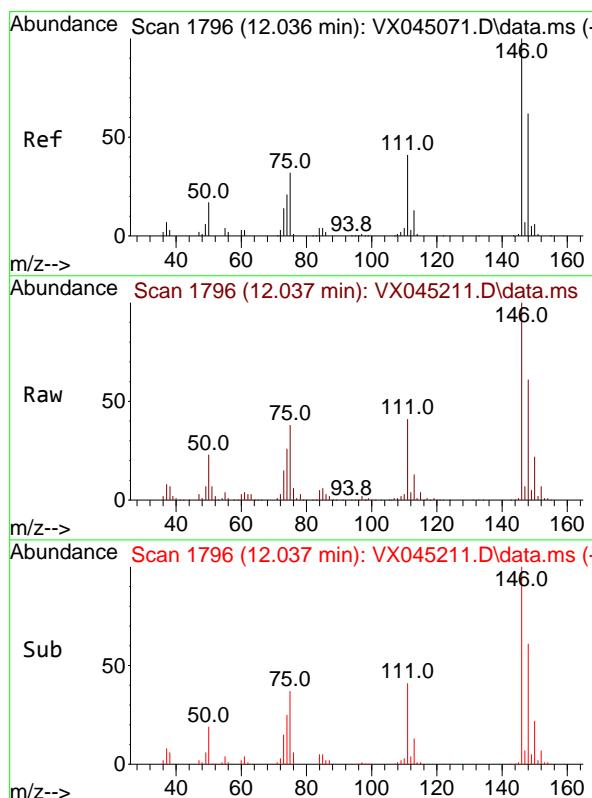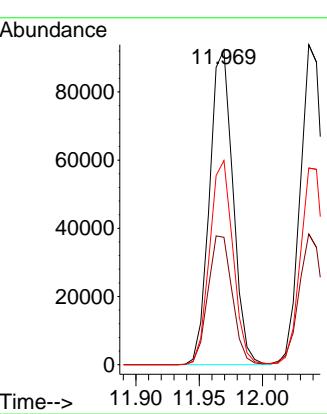

#88
1,4-Dichlorobenzene
Concen: 51.014 ug/l
RT: 12.037 min Scan# 1796
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion:146 Resp: 118921
Ion Ratio Lower Upper
146 100
111 41.6 20.2 60.5
148 63.0 31.9 95.9





#89
n-Butylbenzene
Concen: 59.371 ug/l
RT: 12.329 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050



Tgt Ion: 91 Resp: 225130
Ion Ratio Lower Upper
91 100
92 53.3 26.7 80.0
134 24.1 12.2 36.6



Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

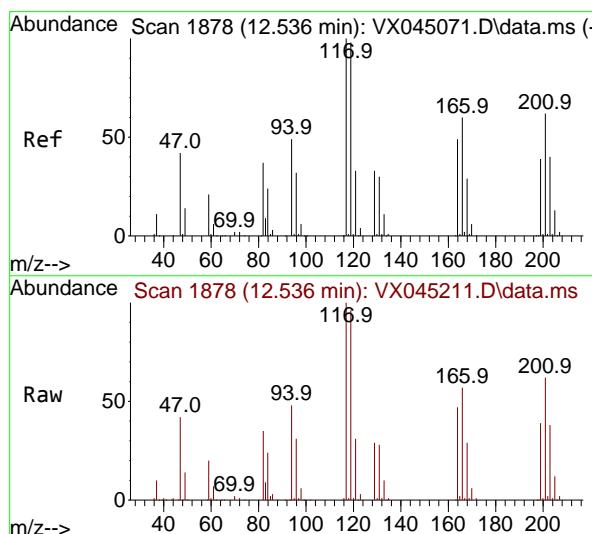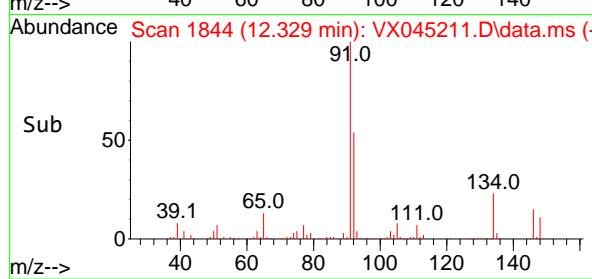

#90
Hexachloroethane
Concen: 55.032 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59


Tgt Ion:117 Resp: 43824
Ion Ratio Lower Upper
117 100
201 63.6 31.9 95.9

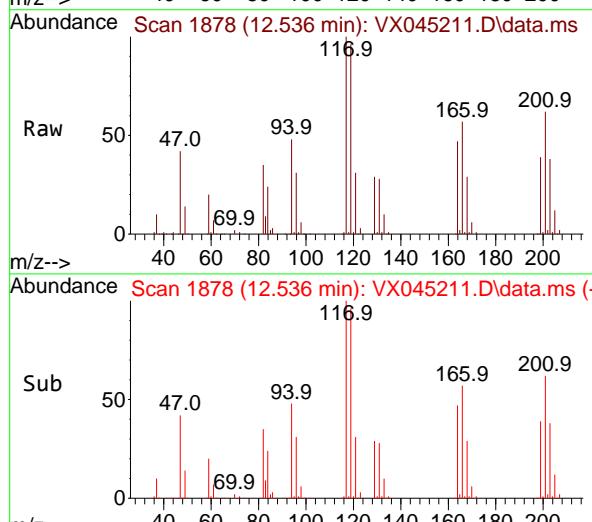



#91
1,2-Dichlorobenzene
Concen: 50.690 ug/l
RT: 12.335 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument : MSVOA_X
ClientSampleId : VSTDCCC050




Tgt Ion:146 Resp: 117160
Ion Ratio Lower Upper
146 100
111 44.3 21.6 65.0
148 65.5 31.9 95.9

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

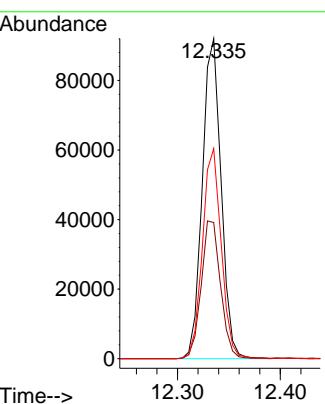


#92
1,2-Dibromo-3-Chloropropane
Concen: 52.534 ug/l
RT: 12.939 min Scan# 1944
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59



Tgt Ion: 75 Resp: 20560
Ion Ratio Lower Upper
75 100
155 76.0 39.6 118.7
157 98.2 51.1 153.4




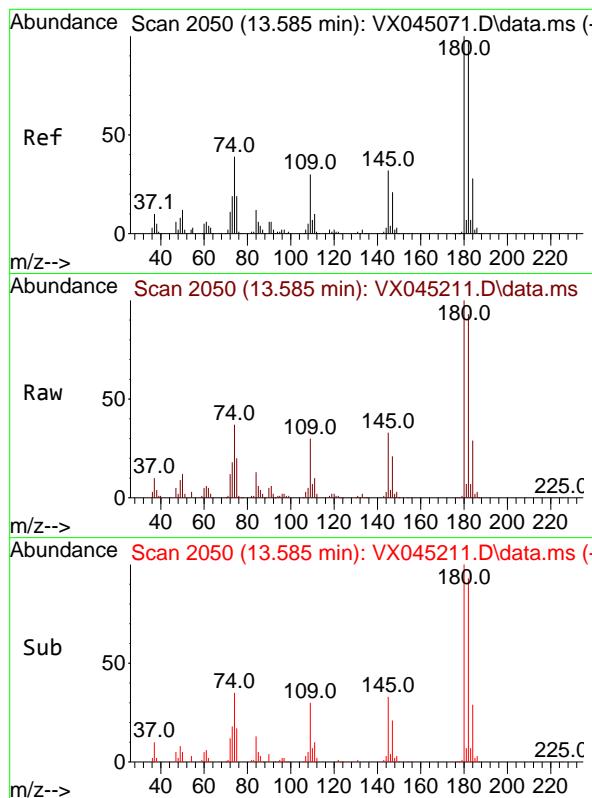


#93
 1,2,4-Trichlorobenzene
 Concen: 55.234 ug/l
 RT: 13.585 min Scan# 2
 Delta R.T. 0.000 min
 Lab File: VX045211.D
 Acq: 11 Mar 2025 09:59

Instrument : MSVOA_X
 ClientSampleId : VSTDCCC050


Manual Integrations
APPROVED


Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

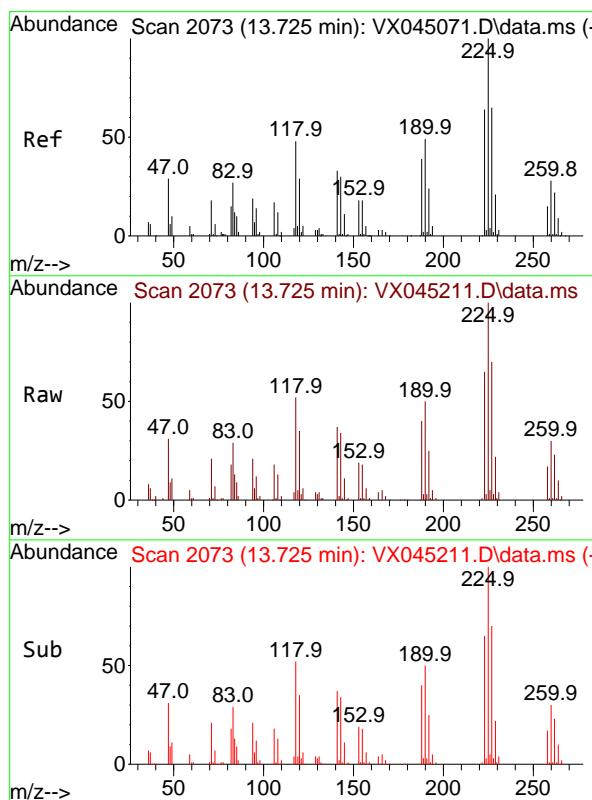

#94
 Hexachlorobutadiene
 Concen: 56.956 ug/l
 RT: 13.725 min Scan# 2073
 Delta R.T. 0.000 min
 Lab File: VX045211.D
 Acq: 11 Mar 2025 09:59


Tgt Ion:225 Resp: 30733
 Ion Ratio Lower Upper
 225 100
 223 61.6 31.9 95.7
 227 63.1 31.4 94.0



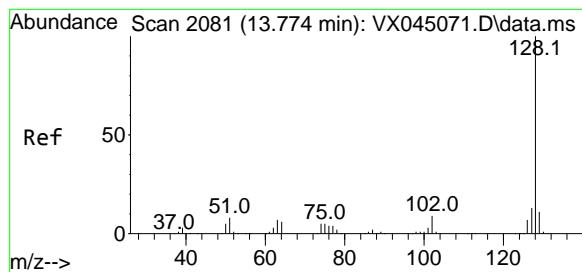

#95
Naphthalene
Concen: 51.639 ug/l
RT: 13.774 min Scan# 2112
Delta R.T. 0.000 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59




Instrument: MSVOA_X
ClientSampleId: VSTDCCC050




Tgt Ion:128 Resp: 26112
Ion Ratio Lower Upper
128 100
127 12.8 10.3 15.5
129 11.1 8.7 13.1

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

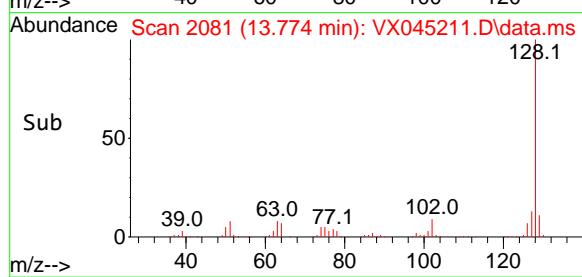

#96
1,2,3-Trichlorobenzene
Concen: 52.399 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.006 min
Lab File: VX045211.D
Acq: 11 Mar 2025 09:59



Tgt Ion:180 Resp: 72754
Ion Ratio Lower Upper
180 100
182 95.8 47.5 142.6
145 34.9 17.0 50.9

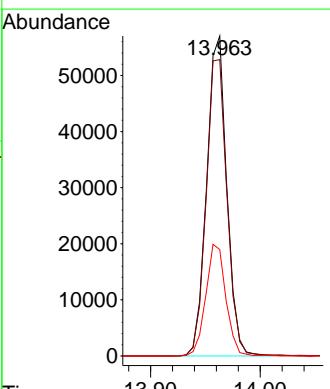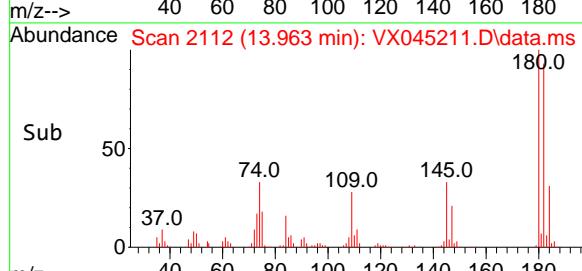

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045211.D
 Acq On : 11 Mar 2025 09:59
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
VSTDCCC050

Quant Time: Mar 12 01:41:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	1.000	1.000	0.0	98	0.00
2 T	Dichlorodifluoromethane	0.629	0.659	-4.8	103	0.00
3 P	Chloromethane	0.770	0.731	5.1	95	0.00
4 C	Vinyl Chloride	0.764	0.723	5.4#	93	0.00
5 T	Bromomethane	0.300	0.303	-1.0	102	0.00
6 T	Chloroethane	0.352	0.386	-9.7	102	0.00
7 T	Trichlorofluoromethane	1.011	1.035	-2.4	97	0.00
8 T	Diethyl Ether	0.396	0.369	6.8	94	0.00
9 T	1,1,2-Trichlorotrifluoroeth	0.581	0.644	-10.8	106	0.00
10 T	Methyl Iodide	0.726	0.769	-5.9	98	0.00
11 T	Tert butyl alcohol	0.151	0.117	22.5	86	0.00
12 CM	1,1-Dichloroethene	0.614	0.615	-0.2#	97	0.00
13 T	Acrolein	0.174	0.153	12.1	87	0.00
14 T	Allyl chloride	1.094	1.165	-6.5	103	0.00
15 T	Acrylonitrile	0.404	0.413	-2.2	99	0.00
16 T	Acetone	0.369	0.381	-3.3	106	0.00
17 T	Carbon Disulfide	1.636	1.547	5.4	92	0.00
18 T	Methyl Acetate	0.888	1.002	-12.8	114	0.00
19 T	Methyl tert-butyl Ether	2.061	2.061	0.0	97	0.00
20 T	Methylene Chloride	0.731	0.714	2.3	100	0.00
21 T	trans-1,2-Dichloroethene	0.607	0.616	-1.5	96	0.00
22 T	Diisopropyl ether	2.224	2.299	-3.4	99	0.00
23 T	Vinyl Acetate	1.856	1.965	-5.9	98	0.00
24 P	1,1-Dichloroethane	1.247	1.245	0.2	98	0.00
25 T	2-Butanone	0.555	0.581	-4.7	99	-0.01
26 T	2,2-Dichloropropane	0.585	0.905	-54.7#	149	0.00
27 T	cis-1,2-Dichloroethene	0.749	0.755	-0.8	97	0.00
28 T	Bromochloromethane	0.594	0.579	2.5	94	0.00
29 T	Tetrahydrofuran	0.373	0.367	1.6	97	0.00
30 C	Chloroform	1.239	1.234	0.4#	97	0.00
31 T	Cyclohexane	1.082	1.111	-2.7	99	0.00
32 T	1,1,1-Trichloroethane	1.000	1.017	-1.7	98	0.00
33 S	1,2-Dichloroethane-d4	0.795	0.792	0.4	103	0.00
34 I	1,4-Difluorobenzene	1.000	1.000	0.0	95	0.00
35 S	Dibromofluoromethane	0.334	0.355	-6.3	102	-0.01
36 T	1,1-Dichloropropene	0.459	0.476	-3.7	96	0.00
37 T	Ethyl Acetate	0.591	0.613	-3.7	96	0.00
38 T	Carbon Tetrachloride	0.465	0.493	-6.0	100	0.00
39 T	Methylcyclohexane	0.549	0.622	-13.3	101	0.00
40 TM	Benzene	1.448	1.486	-2.6	94	0.00
41 T	Methacrylonitrile	0.319	0.341	-6.9	95	0.00
42 TM	1,2-Dichloroethane	0.521	0.546	-4.8	98	0.00
43 T	Isopropyl Acetate	0.874	0.953	-9.0	97	0.00
44 TM	Trichloroethene	0.340	0.354	-4.1	98	0.00
45 C	1,2-Dichloropropane	0.372	0.380	-2.2#	97	0.00
46 T	Dibromomethane	0.263	0.278	-5.7	98	0.00
47 T	Bromodichloromethane	0.516	0.557	-7.9	101	0.00
48 T	Methyl methacrylate	0.438	0.470	-7.3	96	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045211.D
 Acq On : 11 Mar 2025 09:59
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
VSTDCCC050

Quant Time: Mar 12 01:41:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	0.009	0.008	11.1	84	0.00
50 S	Toluene-d8	1.212	1.251	-3.2	98	0.00
51 T	4-Methyl-2-Pentanone	0.587	0.636	-8.3	99	0.00
52 CM	Toluene	0.849	0.900	-6.0#	95	0.00
53 T	t-1,3-Dichloropropene	0.431	0.514	-19.3	104	0.00
54 T	cis-1,3-Dichloropropene	0.503	0.580	-15.3	103	0.00
55 T	1,1,2-Trichloroethane	0.350	0.361	-3.1	96	0.00
56 T	Ethyl methacrylate	0.532	0.594	-11.7	99	0.00
57 T	1,3-Dichloropropane	0.605	0.631	-4.3	96	0.00
58 T	2-Chloroethyl Vinyl ether	0.259	0.302	-16.6	101	0.00
59 T	2-Hexanone	0.425	0.458	-7.8	97	0.00
60 T	Dibromochloromethane	0.366	0.404	-10.4	100	0.00
61 T	1,2-Dibromoethane	0.349	0.373	-6.9	99	0.00
62 S	4-Bromofluorobenzene	0.402	0.446	-10.9	105	0.00
63 I	Chlorobenzene-d5	1.000	1.000	0.0	95	0.00
64 T	Tetrachloroethene	0.320	0.336	-5.0	98	0.00
65 PM	Chlorobenzene	1.058	1.120	-5.9	97	0.00
66 T	1,1,1,2-Tetrachloroethane	0.352	0.372	-5.7	99	0.00
67 C	Ethyl Benzene	1.843	1.996	-8.3#	97	0.00
68 T	m/p-Xylenes	0.675	0.738	-9.3	97	0.00
69 T	o-Xylene	0.681	0.724	-6.3	97	0.00
70 T	Styrene	1.101	1.222	-11.0	98	0.00
71 P	Bromoform	0.266	0.306	-15.0	105	0.00
72 I	1,4-Dichlorobenzene-d4	1.000	1.000	0.0	98	0.00
73 T	Isopropylbenzene	3.903	4.178	-7.0	99	0.00
74 T	N-amyl acetate	1.831	1.958	-6.9	98	0.00
75 P	1,1,2,2-Tetrachloroethane	1.432	1.392	2.8	97	0.00
76 T	1,2,3-Trichloropropane	1.164	1.182	-1.5	101	0.00
77 T	Bromobenzene	0.921	0.953	-3.5	100	0.00
78 T	n-propylbenzene	4.409	4.921	-11.6	101	0.00
79 T	2-Chlorotoluene	2.808	2.904	-3.4	100	0.00
80 T	1,3,5-Trimethylbenzene	3.156	3.410	-8.0	99	0.00
81 T	trans-1,4-Dichloro-2-butene	0.340	0.405	-19.1	118	0.00
82 T	4-Chlorotoluene	3.060	3.281	-7.2	100	0.00
83 T	tert-Butylbenzene	3.242	3.424	-5.6	100	0.00
84 T	1,2,4-Trimethylbenzene	3.175	3.431	-8.1	100	0.00
85 T	sec-Butylbenzene	3.884	4.364	-12.4	102	0.00
86 T	p-Isopropyltoluene	3.139	3.522	-12.2	101	0.00
87 T	1,3-Dichlorobenzene	1.643	1.694	-3.1	100	0.00
88 T	1,4-Dichlorobenzene	1.662	1.696	-2.0	99	0.00
89 T	n-Butylbenzene	2.703	3.210	-18.8	105	0.00
90 T	Hexachloroethane	0.568	0.625	-10.0	102	0.00
91 T	1,2-Dichlorobenzene	1.648	1.671	-1.4	99	0.00
92 T	1,2-Dibromo-3-Chloropropane	0.279	0.293	-5.0	100	0.00
93 T	1,2,4-Trichlorobenzene	0.938	1.037	-10.6	101	0.00
94 T	Hexachlorobutadiene	0.385	0.438	-13.8	110	0.00
95 T	Naphthalene	3.605	3.723	-3.3	94	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
Data File : VX045211.D
Acq On : 11 Mar 2025 09:59
Operator : JC/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
VSTDCCC050

Quant Time: Mar 12 01:41:38 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	AvgRF	CCRF	%Dev	Area%	Dev(min)
96 T 1,2,3-Trichlorobenzene	0.990	1.037	-4.7	96	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045211.D
 Acq On : 11 Mar 2025 09:59
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
VSTDCCC050

Quant Time: Mar 12 01:41:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
1 I	Pentafluorobenzene	50.000	50.000	0.0	98	0.00
2 T	Dichlorodifluoromethane	50.000	52.372	-4.7	103	0.00
3 P	Chloromethane	50.000	47.472	5.1	95	0.00
4 C	Vinyl Chloride	50.000	47.311	5.4#	93	0.00
5 T	Bromomethane	50.000	50.390	-0.8	102	0.00
6 T	Chloroethane	50.000	54.794	-9.6	102	0.00
7 T	Trichlorofluoromethane	50.000	51.147	-2.3	97	0.00
8 T	Diethyl Ether	50.000	46.681	6.6	94	0.00
9 T	1,1,2-Trichlorotrifluoroeth	50.000	55.369	-10.7	106	0.00
10 T	Methyl Iodide	50.000	52.942	-5.9	98	0.00
11 T	Tert butyl alcohol	250.000	194.474	22.2	86	0.00
12 CM	1,1-Dichloroethene	50.000	50.020	-0.0#	97	0.00
13 T	Acrolein	250.000	219.893	12.0	87	0.00
14 T	Allyl chloride	50.000	53.245	-6.5	103	0.00
15 T	Acrylonitrile	250.000	255.519	-2.2	99	0.00
16 T	Acetone	250.000	258.004	-3.2	106	0.00
17 T	Carbon Disulfide	50.000	47.279	5.4	92	0.00
18 T	Methyl Acetate	50.000	56.465	-12.9	114	0.00
19 T	Methyl tert-butyl Ether	50.000	49.992	0.0	97	0.00
20 T	Methylene Chloride	50.000	48.811	2.4	100	0.00
21 T	trans-1,2-Dichloroethene	50.000	50.781	-1.6	96	0.00
22 T	Diisopropyl ether	50.000	51.685	-3.4	99	0.00
23 T	Vinyl Acetate	250.000	264.646	-5.9	98	0.00
24 P	1,1-Dichloroethane	50.000	49.921	0.2	98	0.00
25 T	2-Butanone	250.000	261.614	-4.6	99	-0.01
26 T	2,2-Dichloropropane	50.000	77.390	-54.8#	149	0.00
27 T	cis-1,2-Dichloroethene	50.000	50.382	-0.8	97	0.00
28 T	Bromochloromethane	50.000	48.726	2.5	94	0.00
29 T	Tetrahydrofuran	250.000	245.874	1.7	97	0.00
30 C	Chloroform	50.000	49.818	0.4#	97	0.00
31 T	Cyclohexane	50.000	51.345	-2.7	99	0.00
32 T	1,1,1-Trichloroethane	50.000	50.816	-1.6	98	0.00
33 S	1,2-Dichloroethane-d4	50.000	49.818	0.4	103	0.00
34 I	1,4-Difluorobenzene	50.000	50.000	0.0	95	0.00
35 S	Dibromofluoromethane	50.000	53.104	-6.2	102	-0.01
36 T	1,1-Dichloropropene	50.000	51.860	-3.7	96	0.00
37 T	Ethyl Acetate	50.000	51.851	-3.7	96	0.00
38 T	Carbon Tetrachloride	50.000	52.948	-5.9	100	0.00
39 T	Methylcyclohexane	50.000	56.638	-13.3	101	0.00
40 TM	Benzene	50.000	51.320	-2.6	94	0.00
41 T	Methacrylonitrile	50.000	53.315	-6.6	95	0.00
42 TM	1,2-Dichloroethane	50.000	52.356	-4.7	98	0.00
43 T	Isopropyl Acetate	50.000	54.564	-9.1	97	0.00
44 TM	Trichloroethene	50.000	52.042	-4.1	98	0.00
45 C	1,2-Dichloropropane	50.000	50.991	-2.0#	97	0.00
46 T	Dibromomethane	50.000	52.911	-5.8	98	0.00
47 T	Bromodichloromethane	50.000	53.986	-8.0	101	0.00
48 T	Methyl methacrylate	50.000	53.663	-7.3	96	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045211.D
 Acq On : 11 Mar 2025 09:59
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
VSTDCCC050

Quant Time: Mar 12 01:41:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
 Max. RRF Dev : 25% Max. Rel. Area : 150%

	Compound	Amount	Calc.	%Dev	Area%	Dev(min)
49 T	1,4-Dioxane	1000.000	900.059	10.0	84	0.00
50 S	Toluene-d8	50.000	51.586	-3.2	98	0.00
51 T	4-Methyl-2-Pentanone	250.000	271.045	-8.4	99	0.00
52 CM	Toluene	50.000	52.972	-5.9#	95	0.00
53 T	t-1,3-Dichloropropene	50.000	59.606	-19.2	104	0.00
54 T	cis-1,3-Dichloropropene	50.000	57.592	-15.2	103	0.00
55 T	1,1,2-Trichloroethane	50.000	51.661	-3.3	96	0.00
56 T	Ethyl methacrylate	50.000	55.894	-11.8	99	0.00
57 T	1,3-Dichloropropane	50.000	52.131	-4.3	96	0.00
58 T	2-Chloroethyl Vinyl ether	250.000	291.597	-16.6	101	0.00
59 T	2-Hexanone	250.000	269.382	-7.8	97	0.00
60 T	Dibromochloromethane	50.000	55.267	-10.5	100	0.00
61 T	1,2-Dibromoethane	50.000	53.438	-6.9	99	0.00
62 S	4-Bromofluorobenzene	50.000	55.511	-11.0	105	0.00
63 I	Chlorobenzene-d5	50.000	50.000	0.0	95	0.00
64 T	Tetrachloroethene	50.000	52.473	-4.9	98	0.00
65 PM	Chlorobenzene	50.000	52.928	-5.9	97	0.00
66 T	1,1,1,2-Tetrachloroethane	50.000	52.821	-5.6	99	0.00
67 C	Ethyl Benzene	50.000	54.136	-8.3#	97	0.00
68 T	m/p-Xylenes	100.000	109.410	-9.4	97	0.00
69 T	o-Xylene	50.000	53.202	-6.4	97	0.00
70 T	Styrene	50.000	55.460	-10.9	98	0.00
71 P	Bromoform	50.000	57.546	-15.1	105	0.00
72 I	1,4-Dichlorobenzene-d4	50.000	50.000	0.0	98	0.00
73 T	Isopropylbenzene	50.000	53.524	-7.0	99	0.00
74 T	N-amyl acetate	50.000	53.471	-6.9	98	0.00
75 P	1,1,2,2-Tetrachloroethane	50.000	48.598	2.8	97	0.00
76 T	1,2,3-Trichloropropane	50.000	50.763	-1.5	101	0.00
77 T	Bromobenzene	50.000	51.748	-3.5	100	0.00
78 T	n-propylbenzene	50.000	55.815	-11.6	101	0.00
79 T	2-Chlorotoluene	50.000	51.714	-3.4	100	0.00
80 T	1,3,5-Trimethylbenzene	50.000	54.036	-8.1	99	0.00
81 T	trans-1,4-Dichloro-2-butene	50.000	59.586	-19.2	118	0.00
82 T	4-Chlorotoluene	50.000	53.609	-7.2	100	0.00
83 T	tert-Butylbenzene	50.000	52.798	-5.6	100	0.00
84 T	1,2,4-Trimethylbenzene	50.000	54.029	-8.1	100	0.00
85 T	sec-Butylbenzene	50.000	56.188	-12.4	102	0.00
86 T	p-Isopropyltoluene	50.000	56.113	-12.2	101	0.00
87 T	1,3-Dichlorobenzene	50.000	51.564	-3.1	100	0.00
88 T	1,4-Dichlorobenzene	50.000	51.014	-2.0	99	0.00
89 T	n-Butylbenzene	50.000	59.371	-18.7	105	0.00
90 T	Hexachloroethane	50.000	55.032	-10.1	102	0.00
91 T	1,2-Dichlorobenzene	50.000	50.690	-1.4	99	0.00
92 T	1,2-Dibromo-3-Chloropropane	50.000	52.534	-5.1	100	0.00
93 T	1,2,4-Trichlorobenzene	50.000	55.234	-10.5	101	0.00
94 T	Hexachlorobutadiene	50.000	56.956	-13.9	110	0.00
95 T	Naphthalene	50.000	51.639	-3.3	94	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
Data File : VX045211.D
Acq On : 11 Mar 2025 09:59
Operator : JC/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
VSTDCCC050

Quant Time: Mar 12 01:41:38 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration

Min. RRF : 0.000 Min. Rel. Area : 50% Max. R.T. Dev 0.50min
Max. RRF Dev : 25% Max. Rel. Area : 150%

Compound	Amount	Calc.	%Dev	Area%	Dev(min)
96 T 1,2,3-Trichlorobenzene	50.000	52.399	-4.8	96	0.00

(#) = Out of Range SPCC's out = 0 CCC's out = 6



QC SAMPLE

DATA

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022825\
 Data File : VX045067.D
 Acq On : 28 Feb 2025 01:03
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M

Title : SW846 8260

Last Update : Fri Feb 28 06:45:16 2025

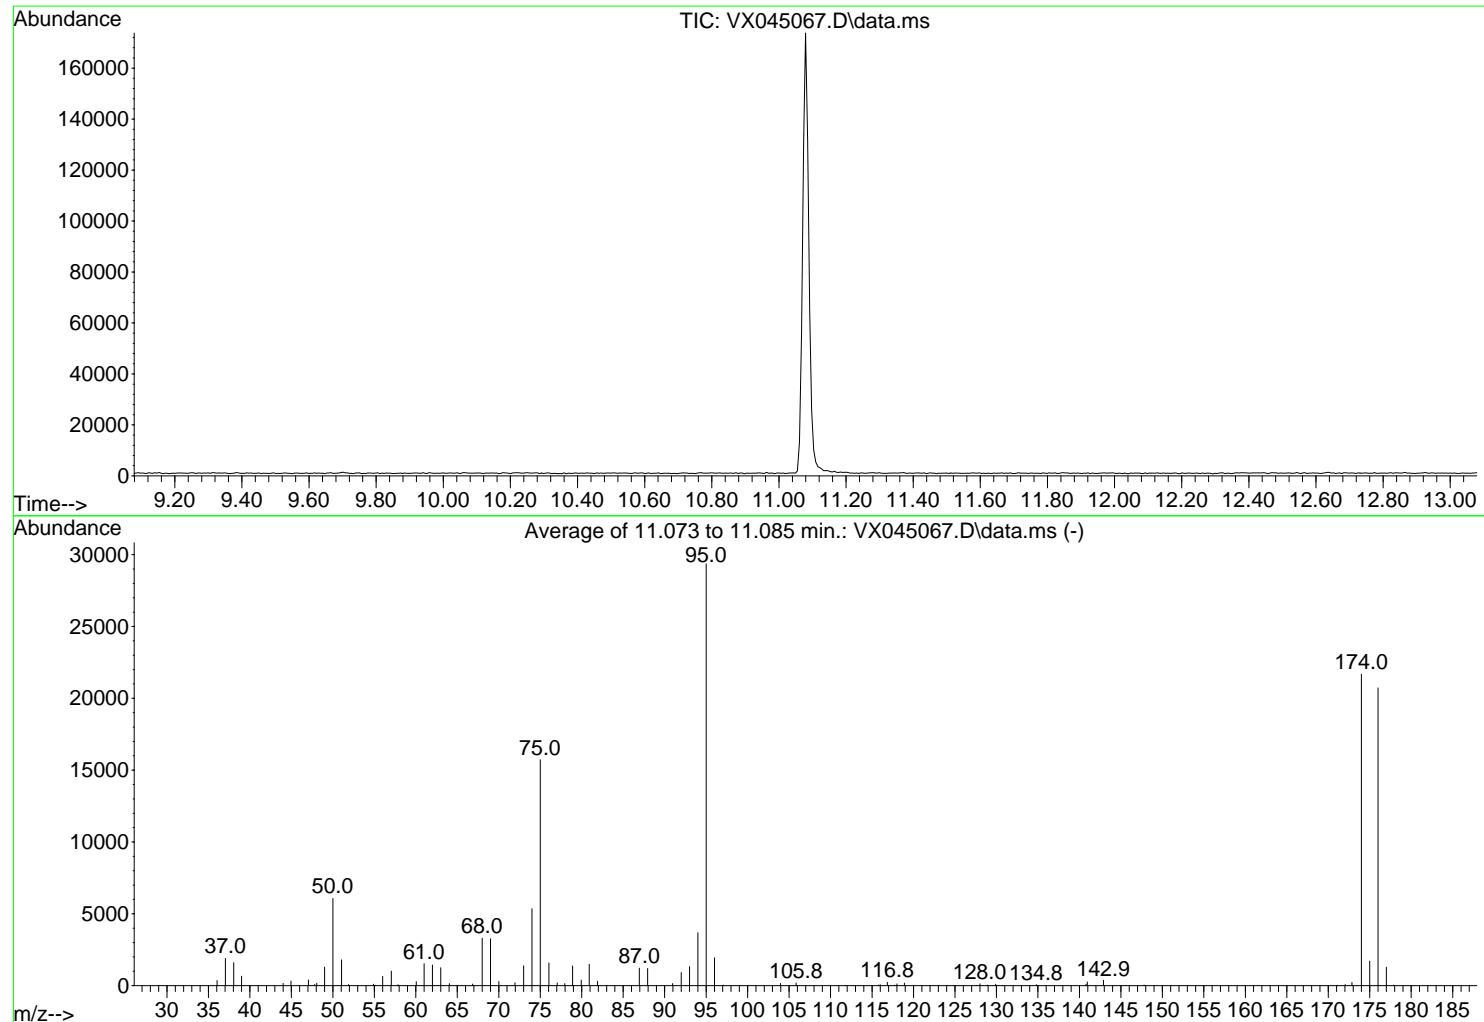

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	6072	PASS
75	95	30	60	53.6	15726	PASS
95	95	100	100	100.0	29360	PASS
96	95	5	9	6.6	1942	PASS
173	174	0.00	2	1.0	219	PASS
174	95	50	100	73.8	21677	PASS
175	174	5	9	7.9	1702	PASS
176	174	95	101	95.6	20723	PASS
177	176	5	9	6.2	1277	PASS

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045210.D
 Acq On : 11 Mar 2025 09:30
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M

Title : SW846 8260

Last Update : Fri Feb 28 06:45:16 2025

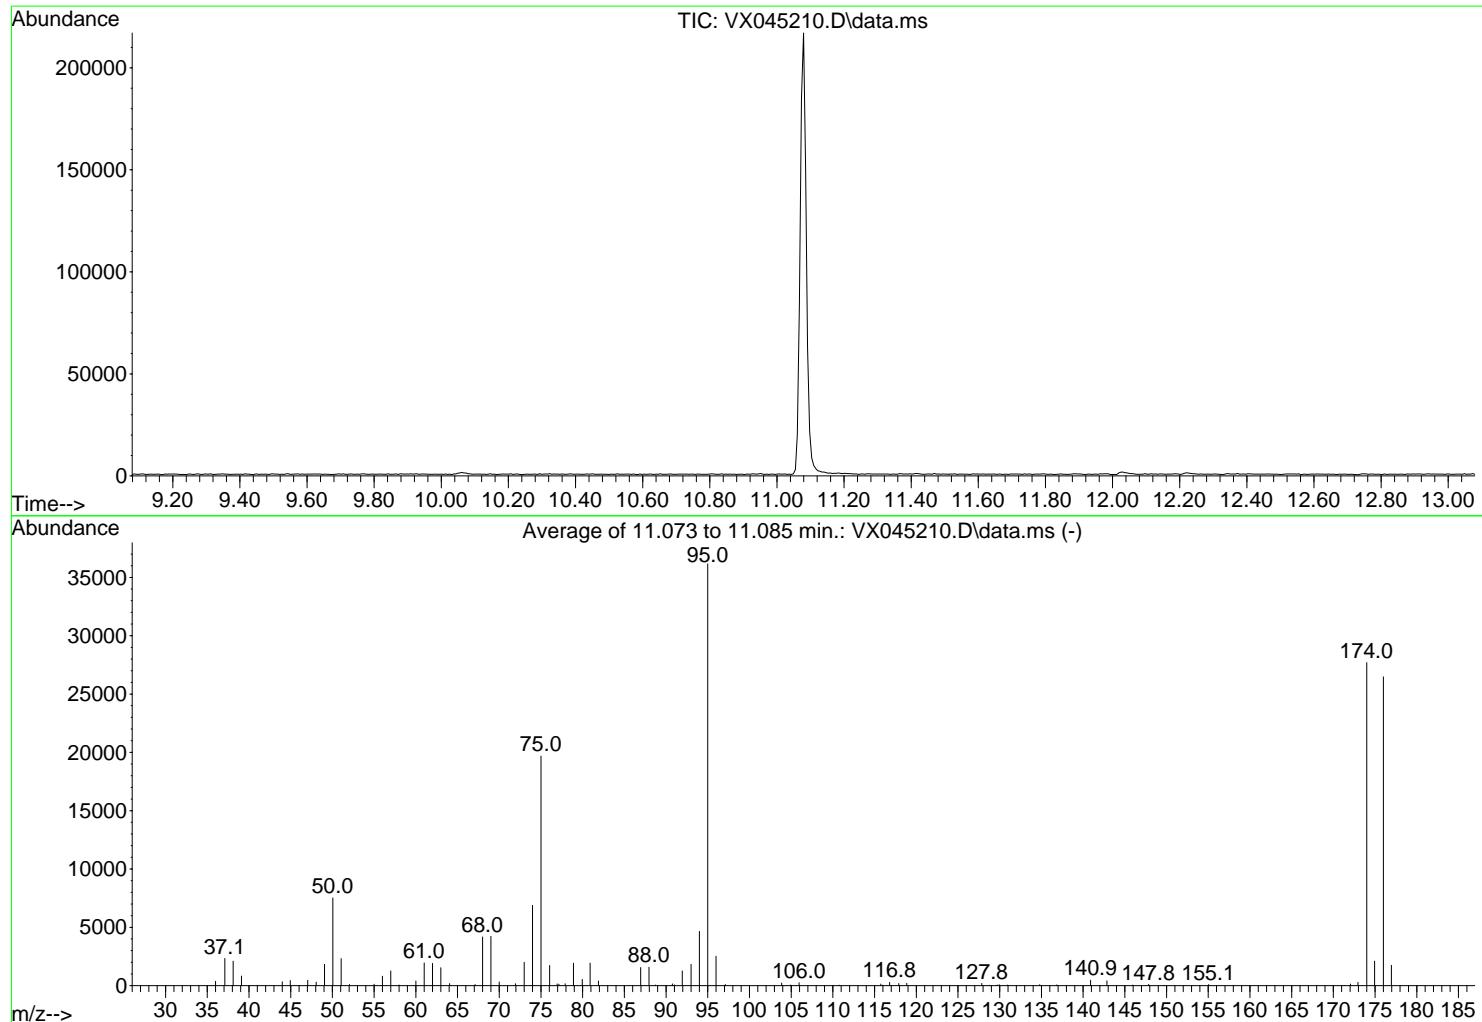

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	7524	PASS
75	95	30	60	54.5	19691	PASS
95	95	100	100	100.0	36163	PASS
96	95	5	9	7.0	2523	PASS
173	174	0.00	2	1.0	284	PASS
174	95	50	100	76.6	27691	PASS
175	174	5	9	7.6	2094	PASS
176	174	95	101	95.6	26483	PASS
177	176	5	9	6.6	1736	PASS

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Waste Water PT			Date Received:
Client Sample ID:	VX0311WBL01		SDG No.:	Q1502
Lab Sample ID:	VX0311WBL01		Matrix:	Water
Analytical Method:	SW8260		% Solid:	0
Sample Wt/Vol:	5	Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045213.D	1		03/11/25 10:51	VX031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-71-8	Dichlorodifluoromethane	0.21	U	0.21	1.00	ug/L
74-87-3	Chloromethane	0.35	U	0.35	1.00	ug/L
75-01-4	Vinyl Chloride	0.34	U	0.34	1.00	ug/L
74-83-9	Bromomethane	1.40	U	1.40	5.00	ug/L
75-00-3	Chloroethane	0.56	U	0.56	1.00	ug/L
75-69-4	Trichlorofluoromethane	0.34	U	0.34	1.00	ug/L
75-35-4	1,1-Dichloroethene	0.26	U	0.26	1.00	ug/L
107-02-8	Acrolein	6.70	U	6.70	25.0	ug/L
107-13-1	Acrylonitrile	0.90	U	0.90	5.00	ug/L
67-64-1	Acetone	1.40	U	1.40	5.00	ug/L
75-15-0	Carbon Disulfide	0.32	U	0.32	1.00	ug/L
1634-04-4	Methyl tert-butyl Ether	0.16	U	0.16	1.00	ug/L
75-09-2	Methylene Chloride	0.32	U	0.32	1.00	ug/L
156-60-5	trans-1,2-Dichloroethene	0.25	U	0.25	1.00	ug/L
108-05-4	Vinyl Acetate	0.71	U	0.71	5.00	ug/L
75-34-3	1,1-Dichloroethane	0.23	U	0.23	1.00	ug/L
78-93-3	2-Butanone	1.30	U	1.30	5.00	ug/L
56-23-5	Carbon Tetrachloride	0.25	U	0.25	1.00	ug/L
594-20-7	2,2-Dichloropropane	0.31	U	0.31	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	0.25	U	0.25	1.00	ug/L
74-97-5	Bromochloromethane	0.18	U	0.18	1.00	ug/L
67-66-3	Chloroform	0.26	U	0.26	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	0.19	U	0.19	1.00	ug/L
563-58-6	1,1-Dichloropropene	0.18	U	0.18	1.00	ug/L
71-43-2	Benzene	0.16	U	0.16	1.00	ug/L
107-06-2	1,2-Dichloroethane	0.24	U	0.24	1.00	ug/L
79-01-6	Trichloroethene	0.32	U	0.32	1.00	ug/L
78-87-5	1,2-Dichloropropane	0.19	U	0.19	1.00	ug/L
74-95-3	Dibromomethane	0.23	U	0.23	1.00	ug/L
75-27-4	Bromodichloromethane	0.24	U	0.24	1.00	ug/L

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Waste Water PT			Date Received:
Client Sample ID:	VX0311WBL01		SDG No.:	Q1502
Lab Sample ID:	VX0311WBL01		Matrix:	Water
Analytical Method:	SW8260		% Solid:	0
Sample Wt/Vol:	5	Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045213.D	1		03/11/25 10:51	VX031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
108-10-1	4-Methyl-2-Pentanone	0.75	U	0.75	5.00	ug/L
108-88-3	Toluene	0.18	U	0.18	1.00	ug/L
10061-02-6	t-1,3-Dichloropropene	0.21	U	0.21	1.00	ug/L
10061-01-5	cis-1,3-Dichloropropene	0.18	U	0.18	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	0.21	U	0.21	1.00	ug/L
142-28-9	1,3-Dichloropropane	0.17	U	0.17	1.00	ug/L
110-75-8	2-Chloroethyl Vinyl ether	1.80	U	1.80	5.00	ug/L
591-78-6	2-Hexanone	1.10	U	1.10	5.00	ug/L
124-48-1	Dibromochloromethane	0.18	U	0.18	1.00	ug/L
106-93-4	1,2-Dibromoethane	0.16	U	0.16	1.00	ug/L
127-18-4	Tetrachloroethene	0.25	U	0.25	1.00	ug/L
108-90-7	Chlorobenzene	0.13	U	0.13	1.00	ug/L
630-20-6	1,1,1,2-Tetrachloroethane	0.21	U	0.21	1.00	ug/L
67-72-1	Hexachloroethane	0	U	0	0	ug/L
100-41-4	Ethyl Benzene	0.16	U	0.16	1.00	ug/L
179601-23-1	m/p-Xylenes	0.31	U	0.31	2.00	ug/L
1330-20-7	Total Xylenes	0.45	U	0.45	3.00	ug/L
95-47-6	o-Xylene	0.14	U	0.14	1.00	ug/L
100-42-5	Styrene	0.16	U	0.16	1.00	ug/L
75-25-2	Bromoform	0.21	U	0.21	1.00	ug/L
98-82-8	Isopropylbenzene	0.13	U	0.13	1.00	ug/L
79-34-5	1,1,2,2-Tetrachloroethane	0.27	U	0.27	1.00	ug/L
96-18-4	1,2,3-Trichloropropane	0.39	U	0.39	1.00	ug/L
108-86-1	Bromobenzene	0.26	U	0.26	1.00	ug/L
103-65-1	n-propylbenzene	0.14	U	0.14	1.00	ug/L
95-49-8	2-Chlorotoluene	0.16	U	0.16	1.00	ug/L
108-67-8	1,3,5-Trimethylbenzene	0.18	U	0.18	1.00	ug/L
106-43-4	4-Chlorotoluene	0.18	U	0.18	1.00	ug/L
98-06-6	tert-Butylbenzene	0.17	U	0.17	1.00	ug/L
95-63-6	1,2,4-Trimethylbenzene	0.18	U	0.18	1.00	ug/L
135-98-8	sec-Butylbenzene	0.17	U	0.17	1.00	ug/L

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Waste Water PT			Date Received:
Client Sample ID:	VX0311WBL01		SDG No.:	Q1502
Lab Sample ID:	VX0311WBL01		Matrix:	Water
Analytical Method:	SW8260		% Solid:	0
Sample Wt/Vol:	5	Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045213.D	1		03/11/25 10:51	VX031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
99-87-6	p-Isopropyltoluene	0.15	U	0.15	1.00	ug/L
541-73-1	1,3-Dichlorobenzene	0.24	U	0.24	1.00	ug/L
106-46-7	1,4-Dichlorobenzene	0.27	U	0.27	1.00	ug/L
104-51-8	n-Butylbenzene	0.22	U	0.22	1.00	ug/L
95-50-1	1,2-Dichlorobenzene	0.19	U	0.19	1.00	ug/L
96-12-8	1,2-Dibromo-3-Chloropropane	0.46	U	0.46	1.00	ug/L
120-82-1	1,2,4-Trichlorobenzene	0.42	U	0.42	1.00	ug/L
87-68-3	Hexachlorobutadiene	0.31	U	0.31	1.00	ug/L
91-20-3	Naphthalene	0.59	U	0.59	1.00	ug/L
87-61-6	1,2,3-Trichlorobenzene	0.51	U	0.51	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	53.3		74 - 125	107%	SPK: 50
1868-53-7	Dibromofluoromethane	50.7		75 - 124	101%	SPK: 50
2037-26-5	Toluene-d8	50.6		86 - 113	101%	SPK: 50
460-00-4	4-Bromofluorobenzene	51.4		77 - 121	103%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	70000	5.544			
540-36-3	1,4-Difluorobenzene	139000	6.757			
3114-55-4	Chlorobenzene-d5	126000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	50100	12.024			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045213.D
 Acq On : 11 Mar 2025 10:51
 Operator : JC/MD
 Sample : VX0311WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0311WBL01

Quant Time: Mar 12 01:43:18 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.544	168	69956	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	139206	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	126312	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	50068	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	59358	53.343	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	106.680%	
35) Dibromofluoromethane	5.385	113	47150	50.653	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	101.300%	
50) Toluene-d8	8.647	98	170914	50.647	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	101.300%	
62) 4-Bromofluorobenzene	11.079	95	57517	51.435	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	=	102.880%	




Target Compounds	Qvalue
(#= qualifier out of range (m) = manual integration (+) = signals summed	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
Data File : VX045213.D
Acq On : 11 Mar 2025 10:51
Operator : JC/MD
Sample : VX0311WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0311WBL01




Quant Time: Mar 12 01:43:18 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration

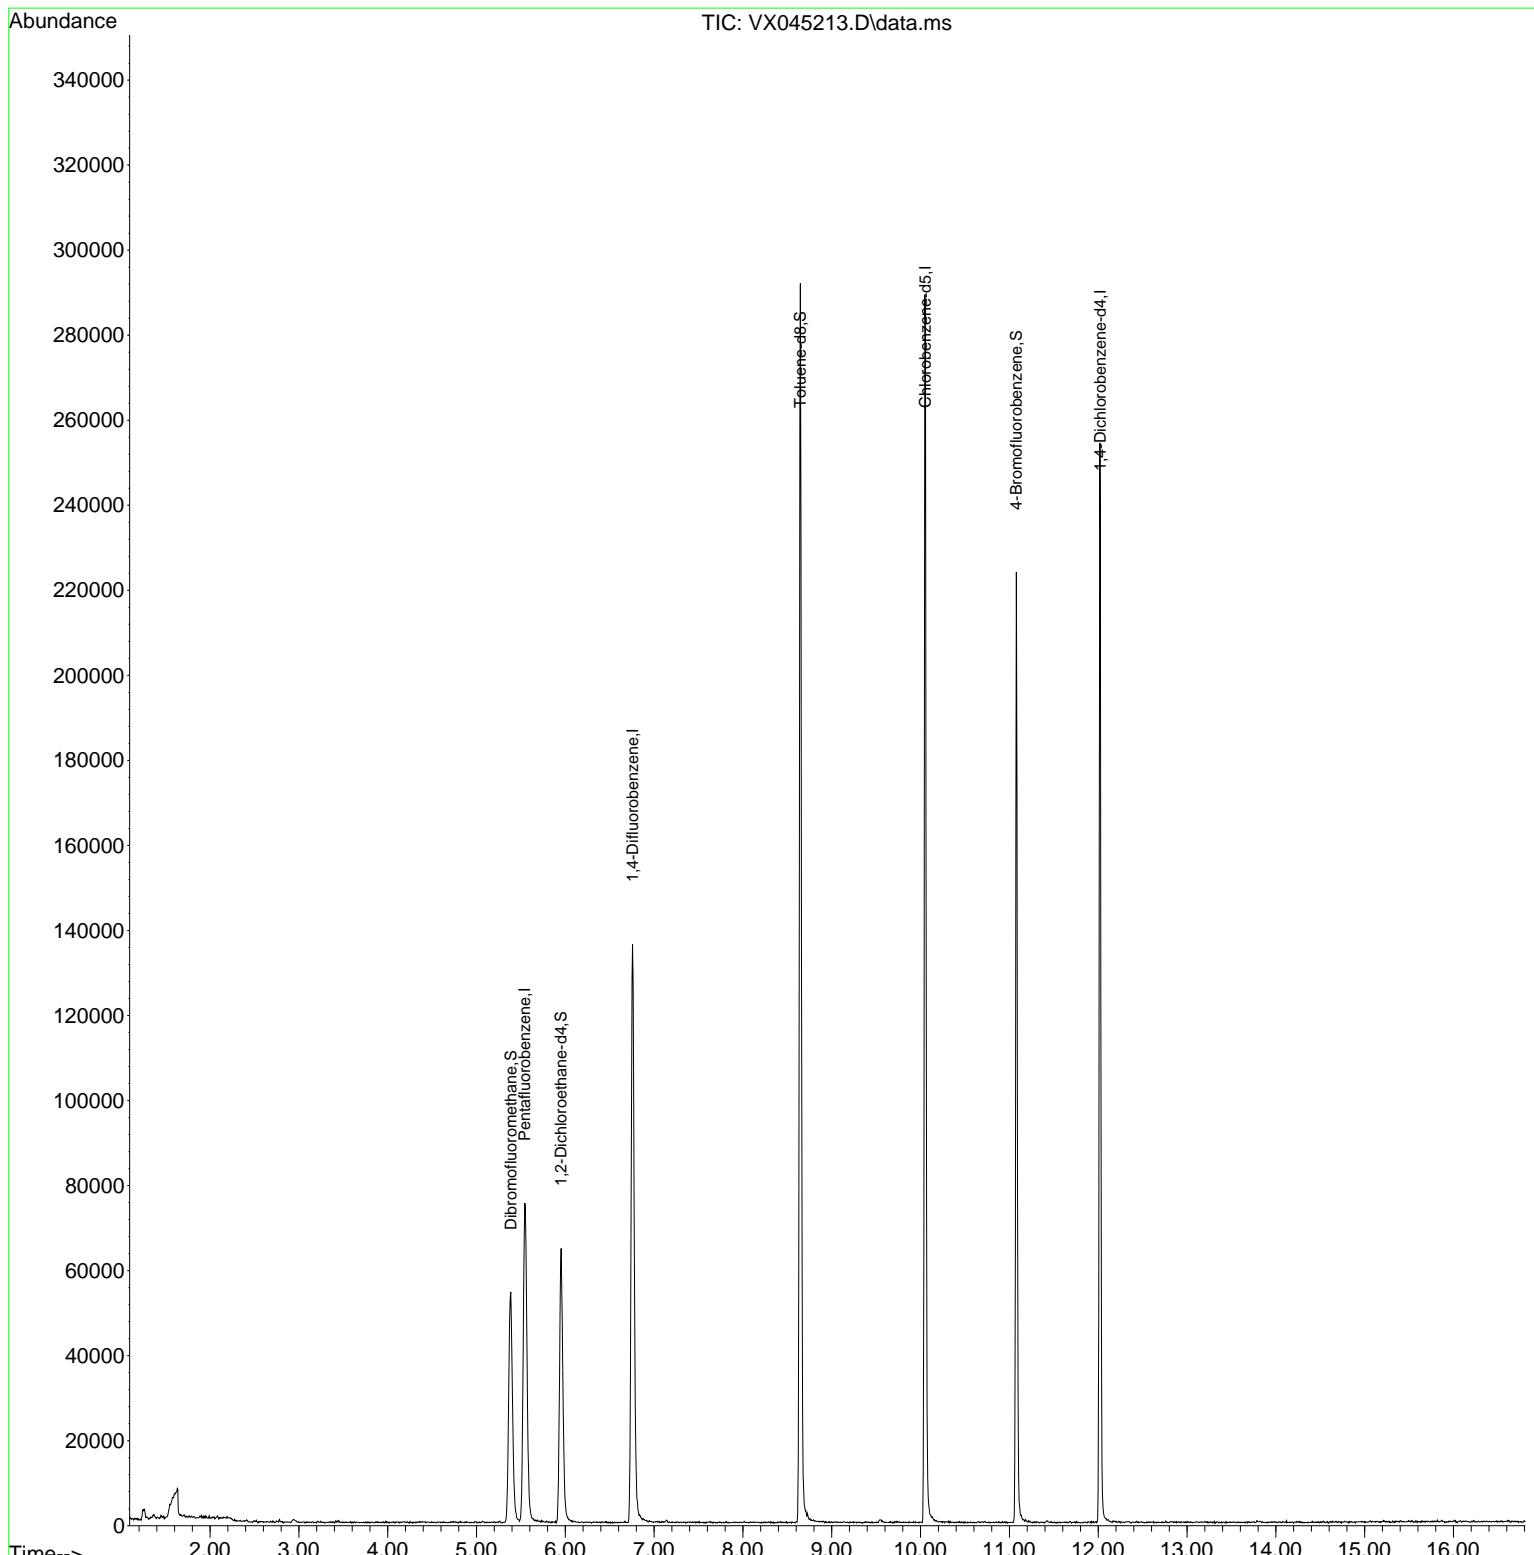




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 7
Instrument : MSVOA_X
Delta R.T. -0.006 min
Lab File: VX045213.D
Acq: 11 Mar 2025 10:51
ClientSampleId : VX0311WBL01


Tgt Ion:168 Resp: 69956
Ion Ratio Lower Upper
168 100
99 65.0 48.2 72.4

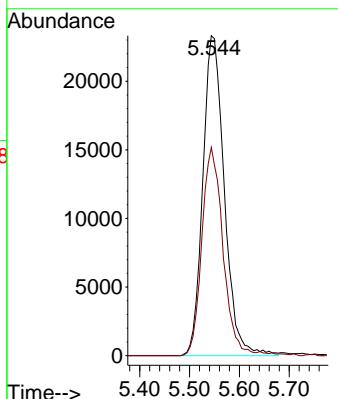

#33
1,2-Dichloroethane-d4
Concen: 53.343 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX045213.D
Acq: 11 Mar 2025 10:51

Tgt Ion: 65 Resp: 59358
Ion Ratio Lower Upper
65 100
67 51.3 0.0 106.2


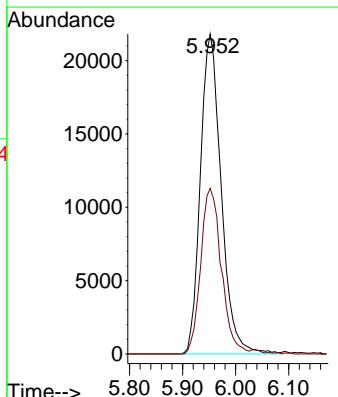


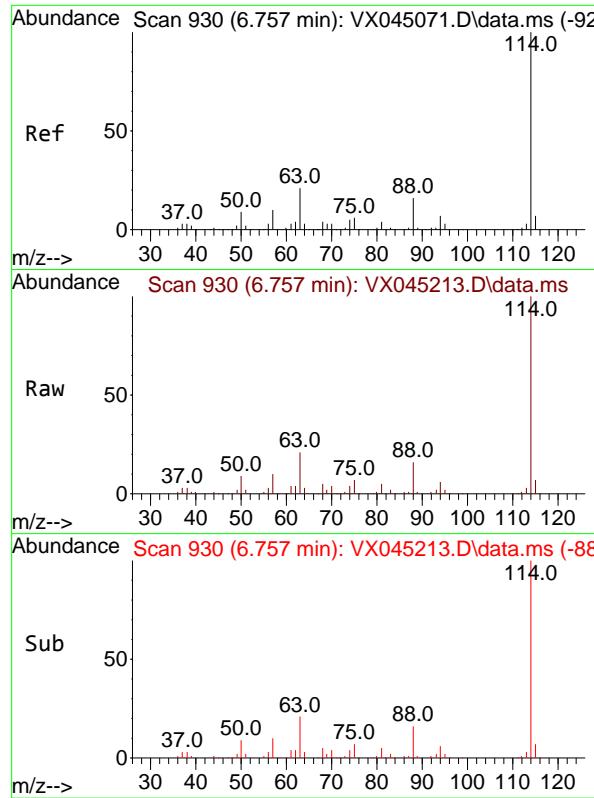

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 9
 Delta R.T. -0.000 min
 Lab File: VX045213.D
 Acq: 11 Mar 2025 10:51


Instrument : MSVOA_X
 ClientSampleId : VX0311WBL01


Tgt Ion:114 Resp: 139206
 Ion Ratio Lower Upper
 114 100
 63 21.0 0.0 41.8
 88 16.1 0.0 32.8

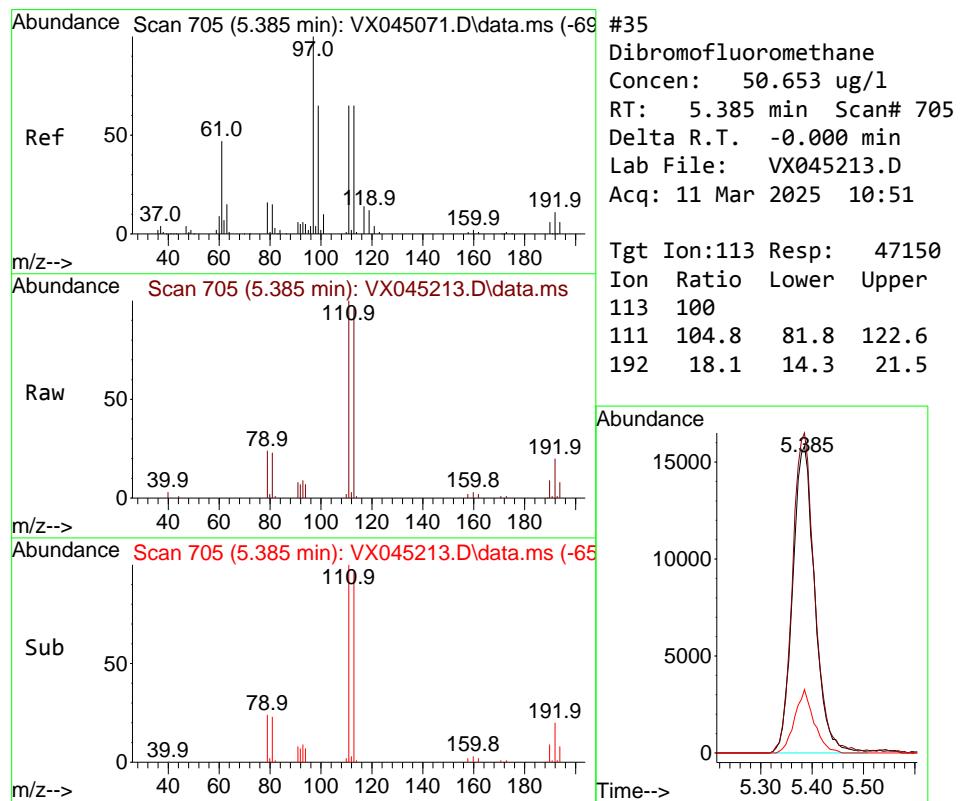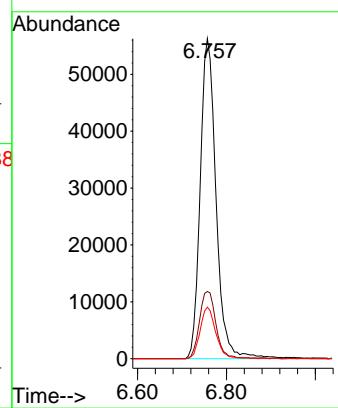

#35
 Dibromofluoromethane
 Concen: 50.653 ug/l
 RT: 5.385 min Scan# 705
 Delta R.T. -0.000 min
 Lab File: VX045213.D
 Acq: 11 Mar 2025 10:51


Tgt Ion:113 Resp: 47150
 Ion Ratio Lower Upper
 113 100
 111 104.8 81.8 122.6
 192 18.1 14.3 21.5

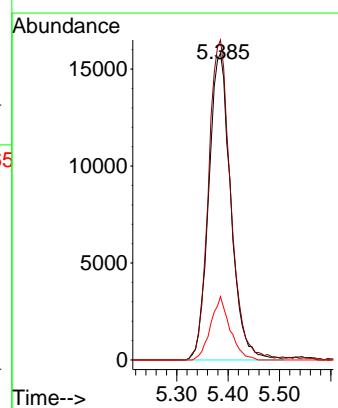






#50
Toluene-d8
Concen: 50.647 ug/l
RT: 8.647 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045213.D
Acq: 11 Mar 2025 10:51


Instrument : MSVOA_X
ClientSampleId : VX0311WBL01





Tgt Ion: 98 Resp: 170914
Ion Ratio Lower Upper
98 100
100 65.5 52.0 78.0




#62
4-Bromofluorobenzene
Concen: 51.435 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045213.D
Acq: 11 Mar 2025 10:51



Tgt Ion: 95 Resp: 57517
Ion Ratio Lower Upper
95 100
174 73.1 0.0 148.2
176 71.2 0.0 141.4

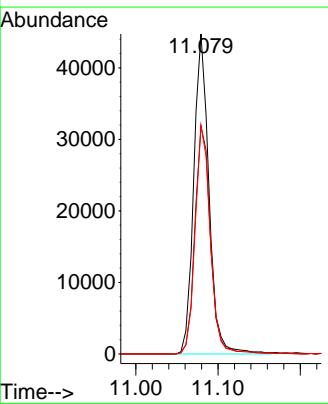



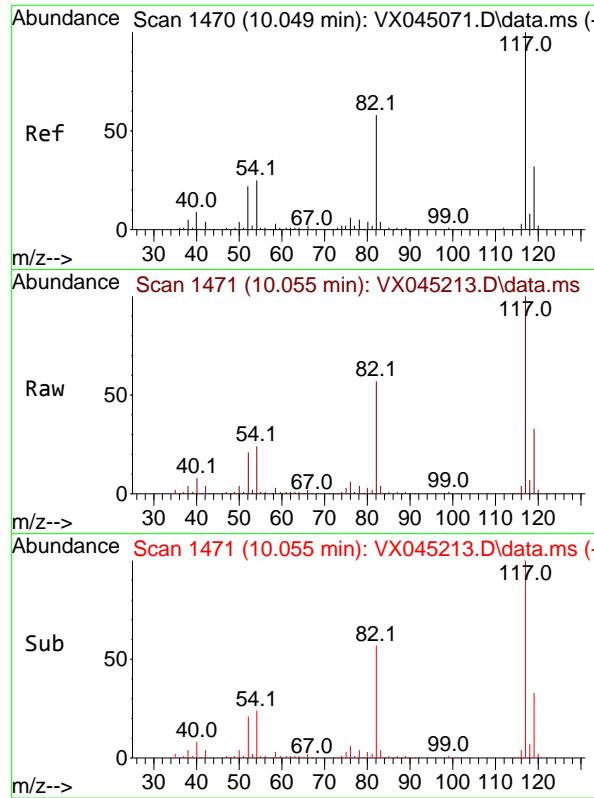

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 10.055 min Scan# 1
 Delta R.T. 0.006 min
 Lab File: VX045213.D
 Acq: 11 Mar 2025 10:51


Instrument : MSVOA_X
 ClientSampleId : VX0311WBL01

Tgt Ion:117 Resp: 126312
 Ion Ratio Lower Upper
 117 100
 82 56.6 46.3 69.5
 119 33.4 25.7 38.5

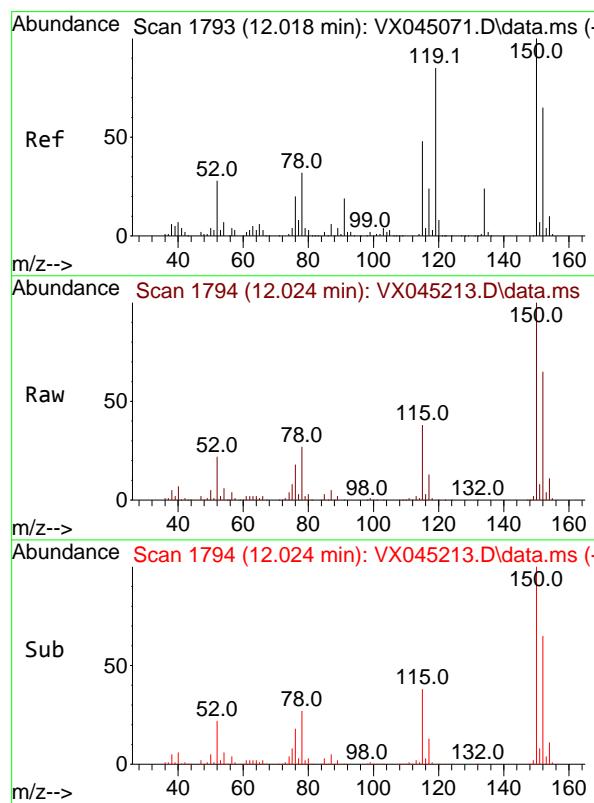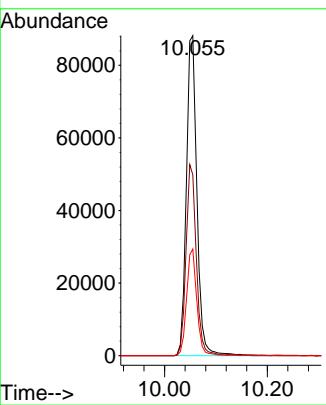

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1794
 Delta R.T. 0.006 min
 Lab File: VX045213.D
 Acq: 11 Mar 2025 10:51

Tgt Ion:152 Resp: 50068
 Ion Ratio Lower Upper
 152 100
 115 62.2 44.2 132.6
 150 156.6 0.0 349.0

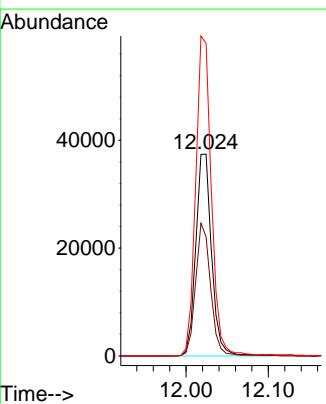

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Waste Water PT			Date Received:
Client Sample ID:	VX0311WBS01	SDG No.:	Q1502	
Lab Sample ID:	VX0311WBS01	Matrix:	Water	
Analytical Method:	SW8260	% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol: 5000 uL
Soil Aliquot Vol:		uL		Test: VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level : LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045214.D	1		03/11/25 11:14	VX031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-71-8	Dichlorodifluoromethane	19.5	0.21		1.00	ug/L
74-87-3	Chloromethane	18.8	0.35		1.00	ug/L
75-01-4	Vinyl Chloride	17.5	0.34		1.00	ug/L
74-83-9	Bromomethane	18.9	1.40		5.00	ug/L
75-00-3	Chloroethane	21.4	0.56		1.00	ug/L
75-69-4	Trichlorofluoromethane	19.1	0.34		1.00	ug/L
75-35-4	1,1-Dichloroethene	18.8	0.26		1.00	ug/L
107-02-8	Acrolein	83.3	6.70		25.0	ug/L
107-13-1	Acrylonitrile	100	0.90		5.00	ug/L
67-64-1	Acetone	97.2	1.40		5.00	ug/L
75-15-0	Carbon Disulfide	16.9	0.32		1.00	ug/L
1634-04-4	Methyl tert-butyl Ether	19.5	0.16		1.00	ug/L
75-09-2	Methylene Chloride	18.6	0.32		1.00	ug/L
156-60-5	trans-1,2-Dichloroethene	19.4	0.25		1.00	ug/L
108-05-4	Vinyl Acetate	98.7	0.71		5.00	ug/L
75-34-3	1,1-Dichloroethane	19.6	0.23		1.00	ug/L
78-93-3	2-Butanone	100	1.30		5.00	ug/L
56-23-5	Carbon Tetrachloride	19.7	0.25		1.00	ug/L
594-20-7	2,2-Dichloropropane	28.6	0.31		1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	19.2	0.25		1.00	ug/L
74-97-5	Bromoform	20.4	0.18		1.00	ug/L
67-66-3	Chloroform	19.9	0.26		1.00	ug/L
71-55-6	1,1,1-Trichloroethane	20.0	0.19		1.00	ug/L
563-58-6	1,1-Dichloropropene	18.9	0.18		1.00	ug/L
71-43-2	Benzene	19.4	0.16		1.00	ug/L
107-06-2	1,2-Dichloroethane	19.8	0.24		1.00	ug/L
79-01-6	Trichloroethene	18.9	0.32		1.00	ug/L
78-87-5	1,2-Dichloropropane	18.9	0.19		1.00	ug/L
74-95-3	Dibromomethane	20.1	0.23		1.00	ug/L
75-27-4	Bromodichloromethane	19.6	0.24		1.00	ug/L

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Waste Water PT			Date Received:
Client Sample ID:	VX0311WBS01	SDG No.:	Q1502	
Lab Sample ID:	VX0311WBS01	Matrix:	Water	
Analytical Method:	SW8260	% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol: 5000 uL
Soil Aliquot Vol:		uL		Test: VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level : LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045214.D	1		03/11/25 11:14	VX031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
108-10-1	4-Methyl-2-Pentanone	110		0.75	5.00	ug/L
108-88-3	Toluene	20.0		0.18	1.00	ug/L
10061-02-6	t-1,3-Dichloropropene	20.0		0.21	1.00	ug/L
10061-01-5	cis-1,3-Dichloropropene	20.6		0.18	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	19.5		0.21	1.00	ug/L
142-28-9	1,3-Dichloropropane	20.1		0.17	1.00	ug/L
110-75-8	2-Chloroethyl Vinyl ether	96.2		1.80	5.00	ug/L
591-78-6	2-Hexanone	110		1.10	5.00	ug/L
124-48-1	Dibromochloromethane	19.5		0.18	1.00	ug/L
106-93-4	1,2-Dibromoethane	19.6		0.16	1.00	ug/L
127-18-4	Tetrachloroethene	19.5		0.25	1.00	ug/L
108-90-7	Chlorobenzene	19.7		0.13	1.00	ug/L
630-20-6	1,1,1,2-Tetrachloroethane	19.7		0.21	1.00	ug/L
67-72-1	Hexachloroethane	17.5		0	0	ug/L
100-41-4	Ethyl Benzene	19.8		0.16	1.00	ug/L
179601-23-1	m/p-Xylenes	40.1		0.31	2.00	ug/L
1330-20-7	Total Xylenes	59.5		0.45	3.00	ug/L
95-47-6	o-Xylene	19.4		0.14	1.00	ug/L
100-42-5	Styrene	20.3		0.16	1.00	ug/L
75-25-2	Bromoform	20.0		0.21	1.00	ug/L
98-82-8	Isopropylbenzene	19.1		0.13	1.00	ug/L
79-34-5	1,1,2,2-Tetrachloroethane	19.5		0.27	1.00	ug/L
96-18-4	1,2,3-Trichloropropane	19.2		0.39	1.00	ug/L
108-86-1	Bromobenzene	18.5		0.26	1.00	ug/L
103-65-1	n-propylbenzene	19.2		0.14	1.00	ug/L
95-49-8	2-Chlorotoluene	18.4		0.16	1.00	ug/L
108-67-8	1,3,5-Trimethylbenzene	19.3		0.18	1.00	ug/L
106-43-4	4-Chlorotoluene	19.2		0.18	1.00	ug/L
98-06-6	tert-Butylbenzene	18.8		0.17	1.00	ug/L
95-63-6	1,2,4-Trimethylbenzene	19.2		0.18	1.00	ug/L
135-98-8	sec-Butylbenzene	19.6		0.17	1.00	ug/L

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Waste Water PT			Date Received:
Client Sample ID:	VX0311WBS01	SDG No.:	Q1502	
Lab Sample ID:	VX0311WBS01	Matrix:	Water	
Analytical Method:	SW8260	% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol: 5000 uL
Soil Aliquot Vol:		uL		Test: VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level : LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045214.D	1		03/11/25 11:14	VX031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
99-87-6	p-Isopropyltoluene	19.8		0.15	1.00	ug/L
541-73-1	1,3-Dichlorobenzene	19.3		0.24	1.00	ug/L
106-46-7	1,4-Dichlorobenzene	18.7		0.27	1.00	ug/L
104-51-8	n-Butylbenzene	19.8		0.22	1.00	ug/L
95-50-1	1,2-Dichlorobenzene	19.4		0.19	1.00	ug/L
96-12-8	1,2-Dibromo-3-Chloropropane	19.1		0.46	1.00	ug/L
120-82-1	1,2,4-Trichlorobenzene	18.9		0.42	1.00	ug/L
87-68-3	Hexachlorobutadiene	20.1		0.31	1.00	ug/L
91-20-3	Naphthalene	18.8		0.59	1.00	ug/L
87-61-6	1,2,3-Trichlorobenzene	18.7		0.51	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	52.0		74 - 125	104%	SPK: 50
1868-53-7	Dibromofluoromethane	51.8		75 - 124	104%	SPK: 50
2037-26-5	Toluene-d8	51.2		86 - 113	102%	SPK: 50
460-00-4	4-Bromofluorobenzene	52.9		77 - 121	106%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	94800	5.544			
540-36-3	1,4-Difluorobenzene	173000	6.757			
3114-55-4	Chlorobenzene-d5	152000	10.055			
3855-82-1	1,4-Dichlorobenzene-d4	71800	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045214.D
 Acq On : 11 Mar 2025 11:14
 Operator : JC/MD
 Sample : VX0311WBS01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0311WBS01

Quant Time: Mar 12 01:43:44 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.544	168	94786	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	172566	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	151770	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	71836	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	78434	52.022	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125			Recovery =	104.040%	
35) Dibromofluoromethane	5.385	113	59827	51.847	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124			Recovery =	103.700%	
50) Toluene-d8	8.647	98	214187	51.200	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113			Recovery =	102.400%	
62) 4-Bromofluorobenzene	11.079	95	73373	52.930	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121			Recovery =	105.860%	
Target Compounds						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	23221	19.462	ug/l	93
3) Chloromethane	1.307	50	27497	18.832	ug/l	98
4) Vinyl Chloride	1.374	62	25371	17.516	ug/l	100
5) Bromomethane	1.593	94	10762	18.900	ug/l	99
6) Chloroethane	1.666	64	14288	21.385	ug/l	99
7) Trichlorofluoromethane	1.873	101	36662	19.119	ug/l	98
8) Diethyl Ether	2.130	74	13336	17.781	ug/l	98
9) 1,1,2-Trichlorotrifluo...	2.318	101	22963	20.844	ug/l	98
10) Methyl Iodide	2.440	142	26241	19.060	ug/l	98
11) Tert butyl alcohol	2.977	59	23827	83.432	ug/l	99
12) 1,1-Dichloroethene	2.306	96	21892	18.796	ug/l	96
13) Acrolein	2.233	56	27498	83.295	ug/l	98
14) Allyl chloride	2.654	41	42402	20.452	ug/l	97
15) Acrylonitrile	3.062	53	76815	100.359	ug/l	98
16) Acetone	2.379	43	68022	97.239	ug/l	100
17) Carbon Disulfide	2.501	76	52443	16.905	ug/l	99
18) Methyl Acetate	2.703	43	38406	22.822	ug/l	98
19) Methyl tert-butyl Ether	3.111	73	76028	19.456	ug/l	97
20) Methylene Chloride	2.782	84	25706	18.551	ug/l	95
21) trans-1,2-Dichloroethene	3.087	96	22379	19.449	ug/l	96
22) Diisopropyl ether	3.763	45	82227	19.501	ug/l	92
23) Vinyl Acetate	3.721	43	347170	98.664	ug/l	100
24) 1,1-Dichloroethane	3.605	63	46401	19.636	ug/l	100
25) 2-Butanone	4.556	43	108494	103.036	ug/l	98
26) 2,2-Dichloropropane	4.471	77	31745	28.640	ug/l	97
27) cis-1,2-Dichloroethene	4.483	96	27319	19.233	ug/l	93
28) Bromochloromethane	4.891	49	23024	20.441	ug/l	98
29) Tetrahydrofuran	5.007	42	69813	98.728	ug/l	99
30) Chloroform	5.092	83	46678	19.880	ug/l	96
31) Cyclohexane	5.458	56	40348	19.670	ug/l	92
32) 1,1,1-Trichloroethane	5.373	97	37908	19.990	ug/l	98
36) 1,1-Dichloropropene	5.684	75	29907	18.899	ug/l	99
37) Ethyl Acetate	4.714	43	38853	19.054	ug/l	100
38) Carbon Tetrachloride	5.665	117	31723	19.746	ug/l	94
39) Methylcyclohexane	7.372	83	37800	19.935	ug/l	96
40) Benzene	6.031	78	96762	19.364	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045214.D
 Acq On : 11 Mar 2025 11:14
 Operator : JC/MD
 Sample : VX0311WBS01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0311WBS01

Quant Time: Mar 12 01:43:44 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.922	41	22316	20.240	ug/1	96
42) 1,2-Dichloroethane	6.086	62	35693	19.836	ug/1	100
43) Isopropyl Acetate	6.342	43	60338	20.011	ug/1	98
44) Trichloroethene	7.123	130	22228	18.944	ug/1	100
45) 1,2-Dichloropropane	7.421	63	24329	18.936	ug/1	92
46) Dibromomethane	7.580	93	18282	20.132	ug/1	97
47) Bromodichloromethane	7.818	83	34860	19.571	ug/1	100
48) Methyl methacrylate	7.696	41	30110	19.905	ug/1	96
49) 1,4-Dioxane	7.665	88	12029	376.974	ug/1	92
51) 4-Methyl-2-Pentanone	8.573	43	214467	105.932	ug/1	99
52) Toluene	8.714	92	58726	20.030	ug/1	99
53) t-1,3-Dichloropropene	8.976	75	29814	20.021	ug/1	96
54) cis-1,3-Dichloropropene	8.366	75	35732	20.578	ug/1	97
55) 1,1,2-Trichloroethane	9.153	97	23516	19.483	ug/1	98
56) Ethyl methacrylate	9.116	69	35989	19.616	ug/1	95
57) 1,3-Dichloropropane	9.305	76	42034	20.124	ug/1	100
58) 2-Chloroethyl Vinyl ether	8.238	63	86098	96.201	ug/1	98
59) 2-Hexanone	9.427	43	159240	108.556	ug/1	100
60) Dibromochloromethane	9.518	129	24640	19.524	ug/1	99
61) 1,2-Dibromoethane	9.610	107	23673	19.647	ug/1	98
64) Tetrachloroethene	9.268	164	18990	19.537	ug/1	94
65) Chlorobenzene	10.079	112	63389	19.739	ug/1	96
66) 1,1,1,2-Tetrachloroethane	10.159	131	21025	19.659	ug/1	97
67) Ethyl Benzene	10.189	91	110625	19.770	ug/1	97
68) m/p-Xylenes	10.299	106	82080	40.069	ug/1	100
69) o-Xylene	10.640	106	40108	19.413	ug/1	99
70) Styrene	10.652	104	67728	20.260	ug/1	100
71) Bromoform	10.799	173	16153	20.029	ug/1 #	96
73) Isopropylbenzene	10.963	105	107006	19.084	ug/1	99
74) N-amyl acetate	10.841	43	50165	19.067	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	40119	19.498	ug/1	100
76) 1,2,3-Trichloropropane	11.238	75	32153m	19.230	ug/1	
77) Bromobenzene	11.195	156	24515	18.531	ug/1	99
78) n-propylbenzene	11.305	91	121782	19.227	ug/1	99
79) 2-Chlorotoluene	11.360	91	74331	18.427	ug/1	99
80) 1,3,5-Trimethylbenzene	11.451	105	87665	19.336	ug/1	98
81) trans-1,4-Dichloro-2-b...	11.018	75	8908	18.233	ug/1	92
82) 4-Chlorotoluene	11.451	91	84393	19.196	ug/1	99
83) tert-Butylbenzene	11.713	119	87407	18.764	ug/1	99
84) 1,2,4-Trimethylbenzene	11.750	105	87408	19.161	ug/1	99
85) sec-Butylbenzene	11.890	105	109340	19.595	ug/1	100
86) p-Isopropyltoluene	12.006	119	89213	19.784	ug/1	100
87) 1,3-Dichlorobenzene	11.969	146	45456	19.261	ug/1	97
88) 1,4-Dichlorobenzene	12.042	146	44731	18.734	ug/1	99
89) n-Butylbenzene	12.329	91	77043	19.837	ug/1	99
90) Hexachloroethane	12.536	117	14295	17.526	ug/1	98
91) 1,2-Dichlorobenzene	12.335	146	45966	19.416	ug/1	100
92) 1,2-Dibromo-3-Chloropr...	12.945	75	7663	19.117	ug/1	96
93) 1,2,4-Trichlorobenzene	13.585	180	25441	18.873	ug/1	99
94) Hexachlorobutadiene	13.725	225	11095	20.075	ug/1	96
95) Naphthalene	13.774	128	97611	18.846	ug/1	100
96) 1,2,3-Trichlorobenzene	13.963	180	26572	18.685	ug/1	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
Data File : VX045214.D
Acq On : 11 Mar 2025 11:14
Operator : JC/MD
Sample : VX0311WBS01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0311WBS01

Manual Integrations
APPROVED

Reviewed By :John Carbone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

Quant Time: Mar 12 01:43:44 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045214.D
 Acq On : 11 Mar 2025 11:14
 Operator : JC/MD
 Sample : VX0311WBS01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
VX0311WBS01

Quant Time: Mar 12 01:43:44 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :John Carlane 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

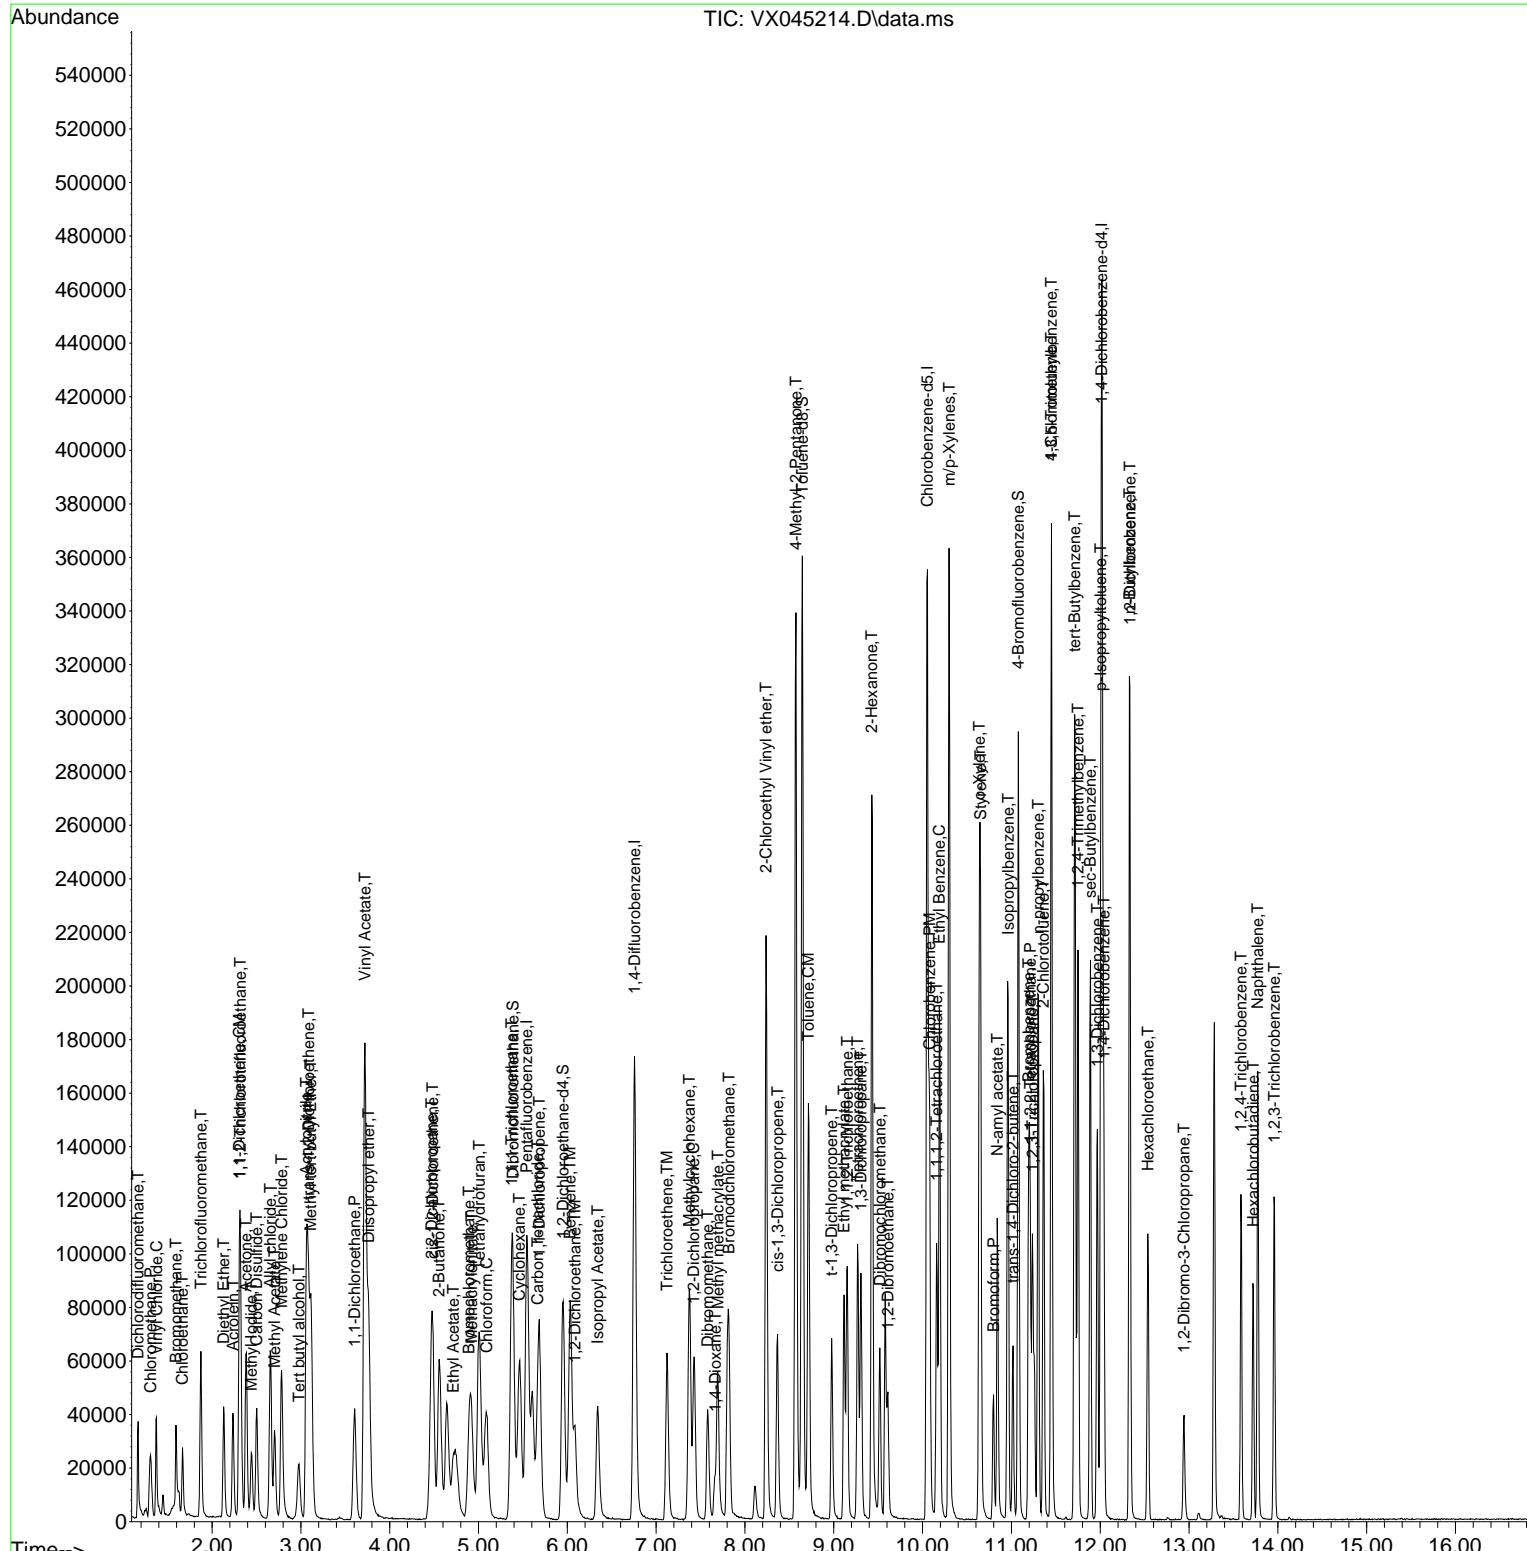



#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.544 min Scan# 7
 Delta R.T. -0.006 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
 ClientSampleId : VX0311WBS01




Tgt Ion:168 Resp: 94780
 Ion Ratio Lower Upper
 168 100
 99 65.0 48.2 72.4

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025




#2
 Dichlorodifluoromethane
 Concen: 19.462 ug/l
 RT: 1.166 min Scan# 13
 Delta R.T. -0.000 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14

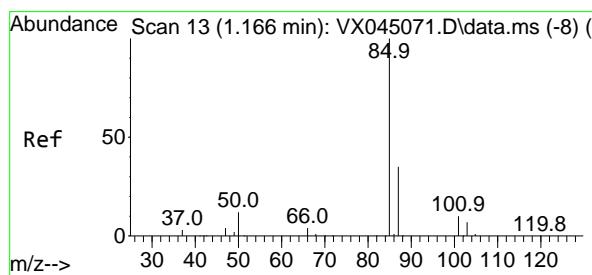


Tgt Ion: 85 Resp: 23221
 Ion Ratio Lower Upper
 85 100
 87 31.0 17.4 52.3

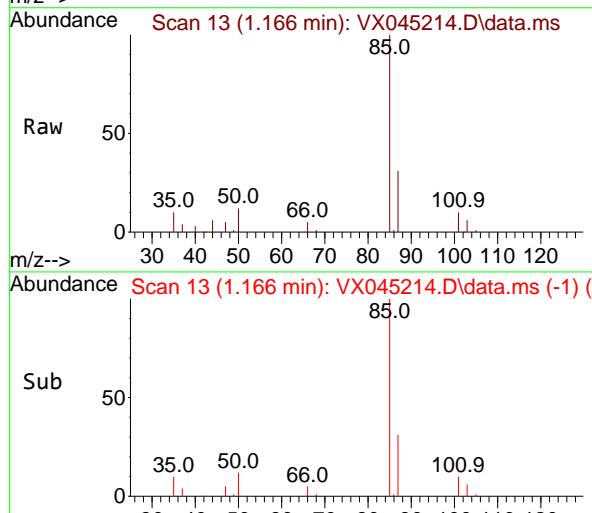



#3
Chloromethane
Concen: 18.832 ug/l
RT: 1.307 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument :
MSVOA_X
ClientSampleId :
VX0311WBS01




Tgt Ion: 50 Resp: 27491
Ion Ratio Lower Upper
50 100
52 30.2 25.0 37.4

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

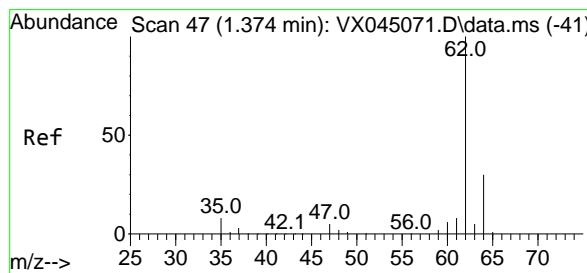


#4
Vinyl Chloride
Concen: 17.516 ug/l
RT: 1.374 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion: 62 Resp: 25371
Ion Ratio Lower Upper
62 100
64 30.2 24.3 36.5

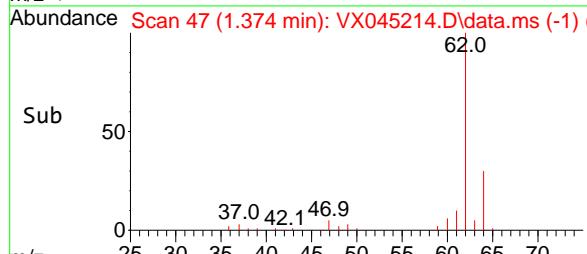



#5
Bromomethane
Concen: 18.900 ug/l
RT: 1.593 min Scan# 8
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01



Tgt Ion: 94 Resp: 1076
Ion Ratio Lower Upper
94 100
96 93.1 75.0 112.4




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#6
Chloroethane
Concen: 21.385 ug/l
RT: 1.666 min Scan# 95
Delta R.T. 0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14


Tgt Ion: 64 Resp: 14288
Ion Ratio Lower Upper
64 100
66 32.7 26.7 40.1

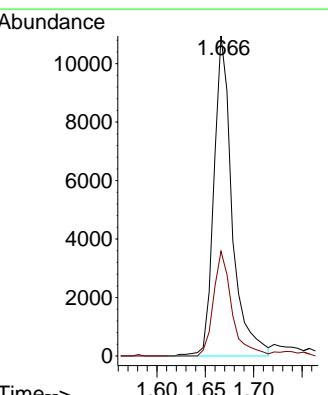



#7
Trichlorofluoromethane
Concen: 19.119 ug/l
RT: 1.873 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01




Tgt Ion:101 Resp: 3666
Ion Ratio Lower Upper
101 100
103 66.9 52.1 78.1

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#8
Diethyl Ether
Concen: 17.781 ug/l
RT: 2.130 min Scan# 171
Delta R.T. -0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion: 74 Resp: 13336
Ion Ratio Lower Upper
74 100
45 104.8 51.5 154.5

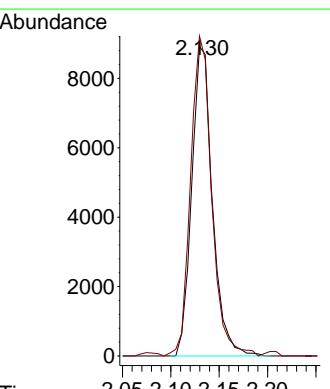



#9
1,1,2-Trichlorotrifluoroethane
Concen: 20.844 ug/l
RT: 2.318 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
ClientSampleId : VX0311WBS01



Tgt	Ion:101	Resp:	2296
	Ion Ratio	Lower	Upper
101	100		
85	47.1	36.2	54.4
151	72.4	56.4	84.6



Manual Integrations APPROVED

Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

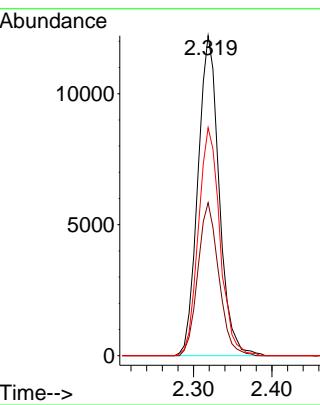


#10
Methyl Iodide
Concen: 19.060 ug/l
RT: 2.440 min Scan# 222
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

Tgt	Ion:142	Resp:	26241
	Ion Ratio	Lower	Upper
142	100		
127	45.6	35.4	53.2
141	14.7	11.6	17.4

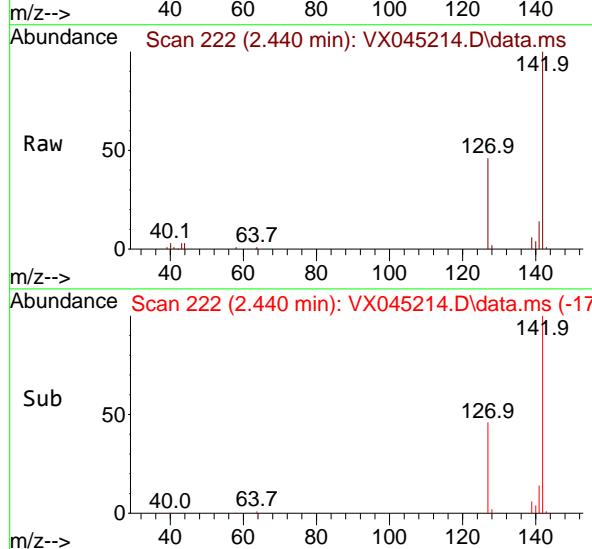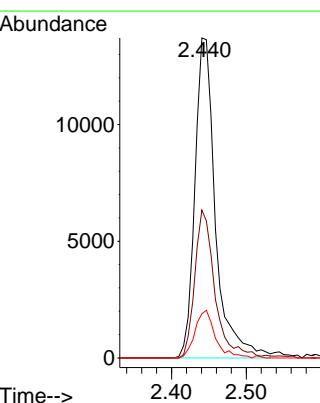


Abundance Scan 222 (2.440 min): VX045214.D\data.ms (-17)

m/z-->



#11
 Tert butyl alcohol
 Concen: 83.432 ug/l
 RT: 2.977 min Scan# 3
 Delta R.T. -0.006 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
 ClientSampleId : VX0311WBS01

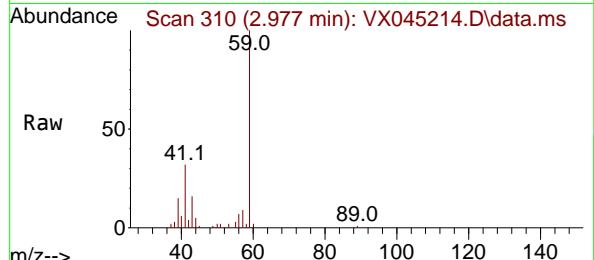

Tgt Ion: 59 Resp: 2382
 Ion Ratio Lower Upper
 59 100
 57 10.3 7.8 11.8




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

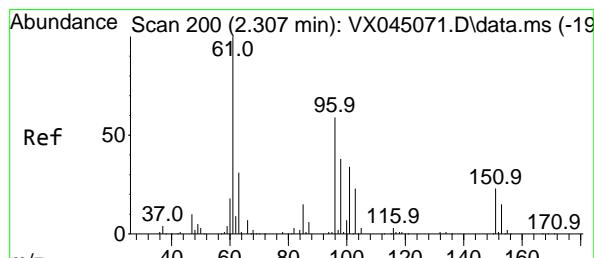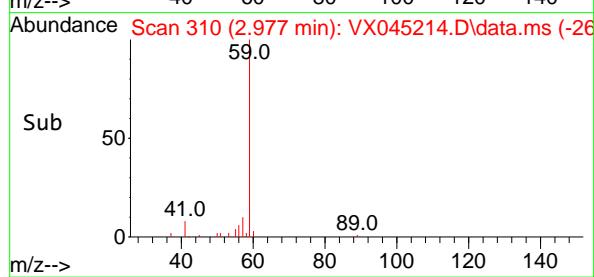

#12
 1,1-Dichloroethene
 Concen: 18.796 ug/l
 RT: 2.306 min Scan# 200
 Delta R.T. -0.000 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14


Tgt Ion: 96 Resp: 21892
 Ion Ratio Lower Upper
 96 100
 61 174.2 134.6 202.0
 98 62.7 51.0 76.6

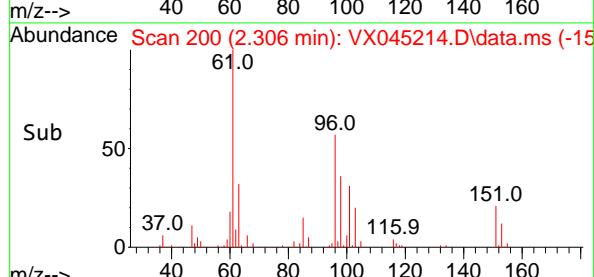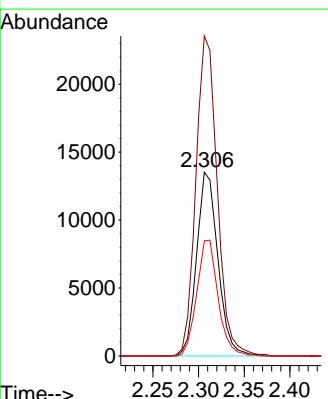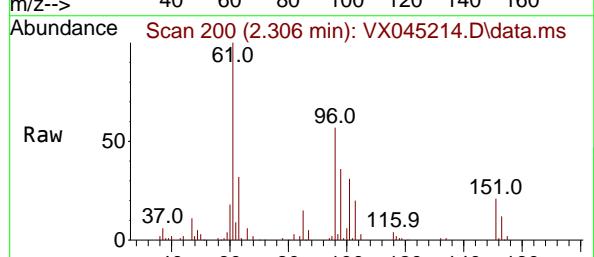



#13
Acrolein
Concen: 83.295 ug/l
RT: 2.233 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

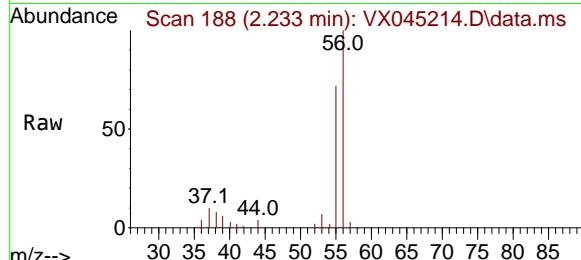

Tgt Ion: 56 Resp: 27498
Ion Ratio Lower Upper
56 100
55 72.3 56.2 84.4



Manual Integrations APPROVED

Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

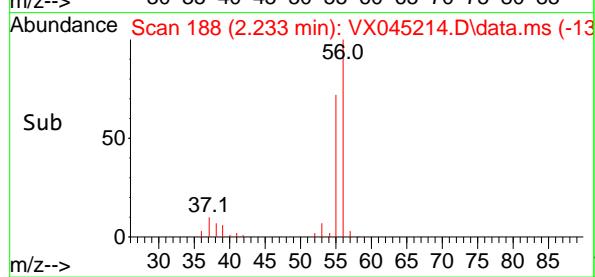


#14
Allyl chloride
Concen: 20.452 ug/l
RT: 2.654 min Scan# 257
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14


Tgt Ion: 41 Resp: 42402
Ion Ratio Lower Upper
41 100
39 70.5 53.8 80.8
76 30.2 25.2 37.8

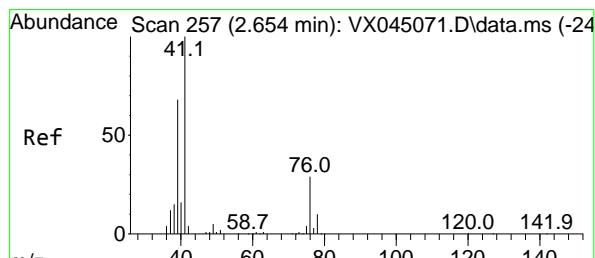


#14
Allyl chloride
Concen: 20.452 ug/l
RT: 2.654 min Scan# 257
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion: 41 Resp: 42402
Ion Ratio Lower Upper
41 100
39 70.5 53.8 80.8
76 30.2 25.2 37.8

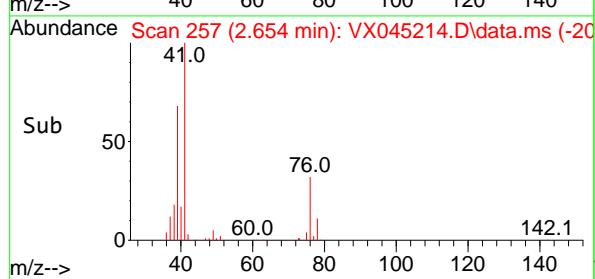



#15
Acrylonitrile
Concen: 100.359 ug/l
RT: 3.062 min Scan# 31
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
ClientSampleId : VX0311WBS01




Tgt Ion: 53 Resp: 7681
Ion Ratio Lower Upper
53 100
52 84.1 66.2 99.2
51 37.1 29.0 43.4

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#16
Acetone
Concen: 97.239 ug/l
RT: 2.379 min Scan# 212
Delta R.T. -0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion: 43 Resp: 68022
Ion Ratio Lower Upper
43 100
58 30.3 24.2 36.4





#17
Carbon Disulfide
Concen: 16.905 ug/l
RT: 2.501 min Scan# 2
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

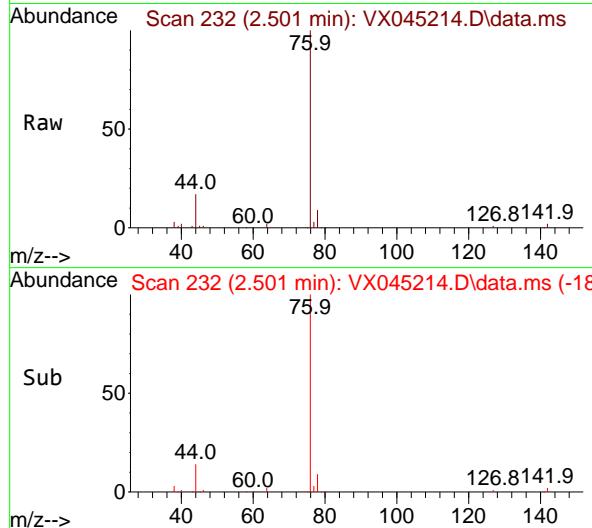

Tgt Ion: 76 Resp: 5244
Ion Ratio Lower Upper
76 100
78 8.7 6.6 9.8


Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

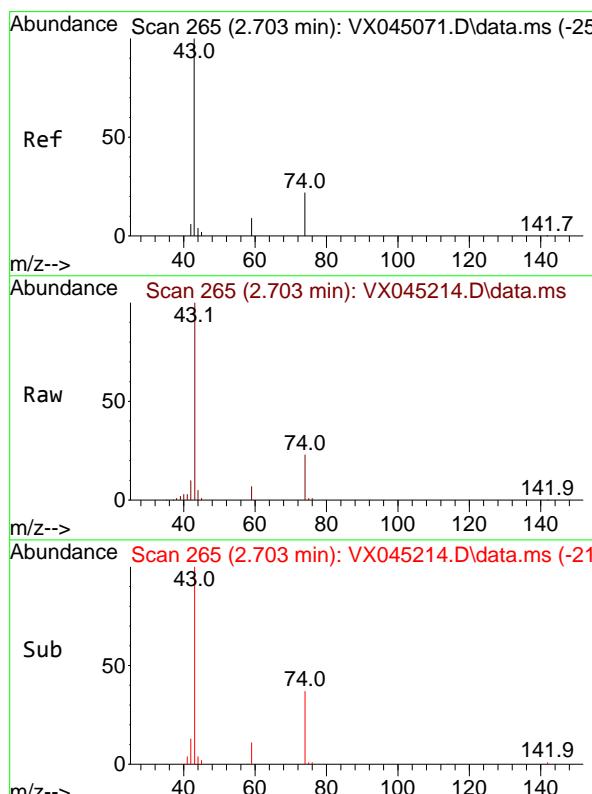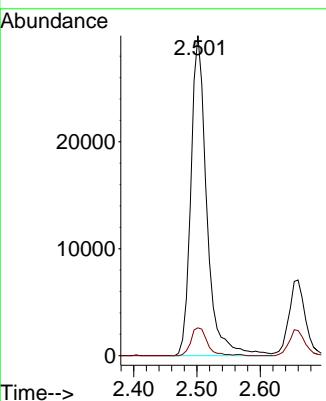


#18
Methyl Acetate
Concen: 22.822 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

Tgt Ion: 43 Resp: 38406
Ion Ratio Lower Upper
43 100
74 22.6 17.4 26.2

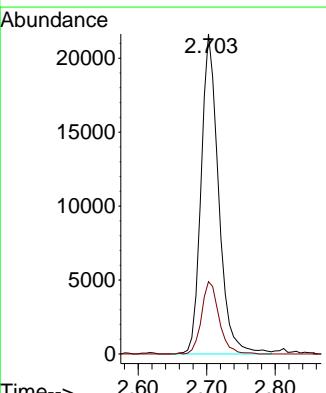





#19
Methyl tert-butyl Ether
Concen: 19.456 ug/l
RT: 3.111 min Scan# 3
Delta R.T. -0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

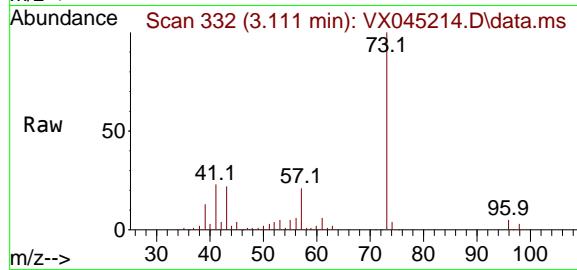


Tgt Ion: 73 Resp: 7602
Ion Ratio Lower Upper
73 100
57 21.4 18.5 27.7

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

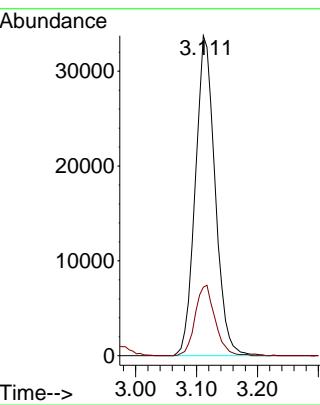


#20
Methylene Chloride
Concen: 18.551 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

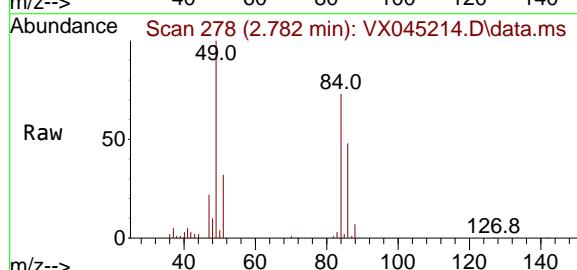


Tgt Ion: 84 Resp: 25706
Ion Ratio Lower Upper
84 100
49 137.6 106.5 159.7
51 44.1 32.1 48.1
86 66.3 50.0 75.0

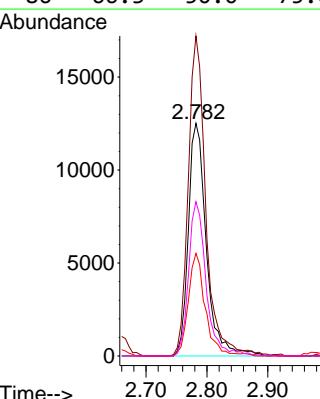



#21
trans-1,2-Dichloroethene
Concen: 19.449 ug/l
RT: 3.087 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
ClientSampleId : VX0311WBS01



Tgt Ion: 96 Resp: 22379
Ion Ratio Lower Upper
96 100
61 139.5 117.0 175.4
98 64.8 53.4 80.2



Manual Integrations APPROVED

Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#22
Diisopropyl ether
Concen: 19.501 ug/l
RT: 3.763 min Scan# 439
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

Tgt Ion: 45 Resp: 82227
Ion Ratio Lower Upper
45 100
43 78.2 54.9 82.3
87 25.1 21.0 31.4
59 10.4 8.7 13.1




45.1

87.1

59.0

70.1

102.1




45.1

87.1

59.0

70.0

102.0




45.1

87.1

59.0

70.0

102.0



#23

Vinyl Acetate

Concen: 98.664 ug/l

RT: 3.721 min Scan# 413

Delta R.T. -0.000 min

Lab File: VX045214.D


Acq: 11 Mar 2025 11:14

Instrument :

MSVOA_X

ClientSampleId :

VX0311WBS01



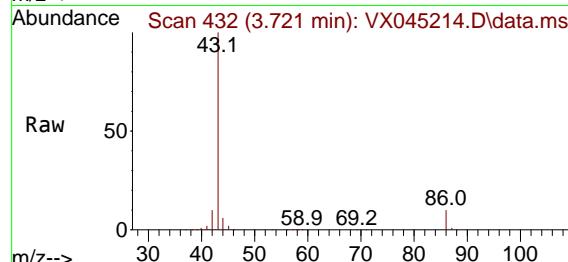


Tgt Ion: 43 Resp: 347170


Ion Ratio	Lower	Upper
43	100	
86	10.2	8.1
		12.1

**Manual Integrations
APPROVED**

Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

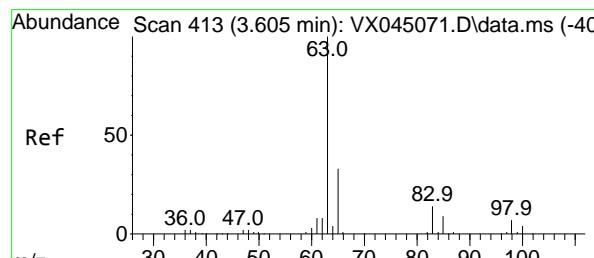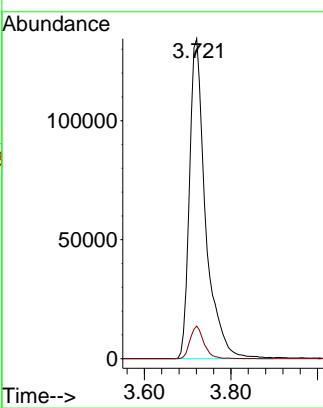
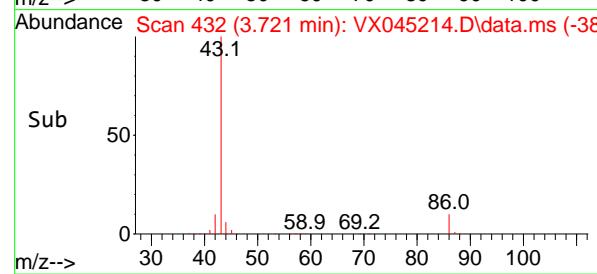



#24
1,1-Dichloroethane
Concen: 19.636 ug/l
RT: 3.605 min Scan# 413
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

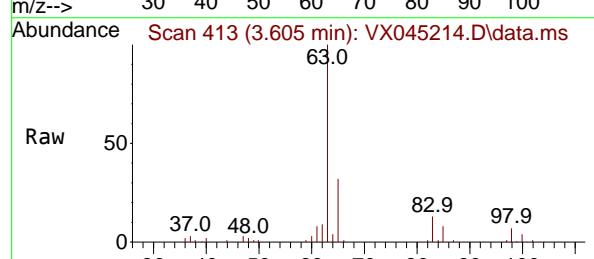

Tgt Ion: 63 Resp: 46401


Ion Ratio	Lower	Upper
63	100	
98	6.9	3.4
100	4.4	2.1
		6.5

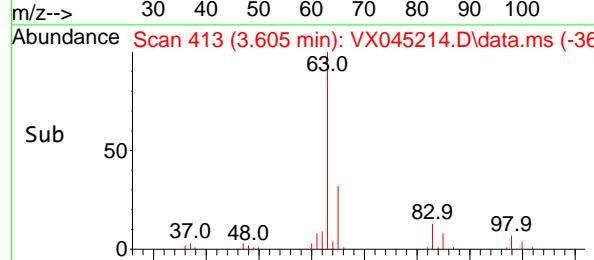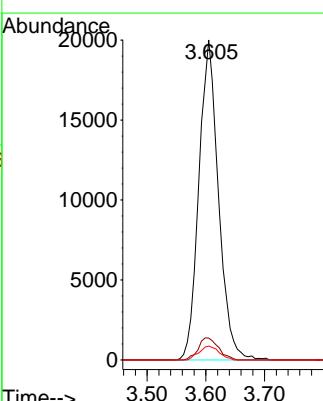

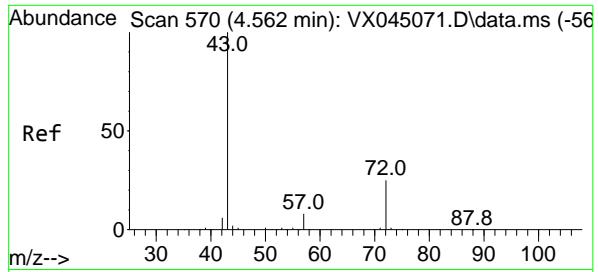

#25
2-Butanone
Concen: 103.036 ug/l
RT: 4.556 min Scan# 5
Delta R.T. -0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

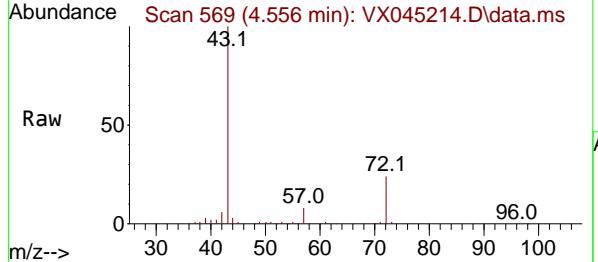

Tgt Ion: 43 Resp: 108494
Ion Ratio Lower Upper
43 100
72 24.0 20.0 30.0




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

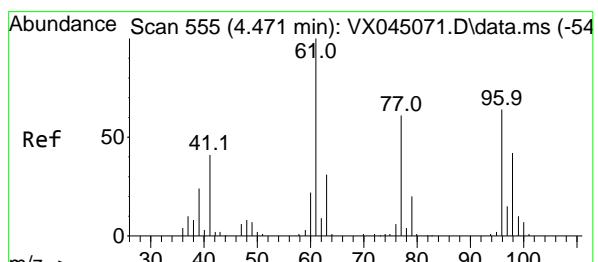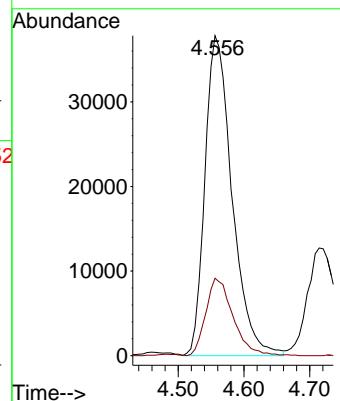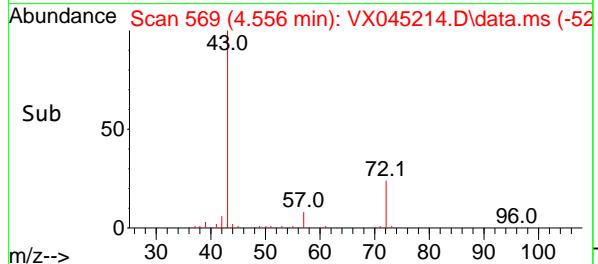


#26
2,2-Dichloropropane
Concen: 28.640 ug/l
RT: 4.471 min Scan# 555
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

Tgt Ion: 77 Resp: 31745
Ion Ratio Lower Upper
77 100
97 23.1 12.4 37.0

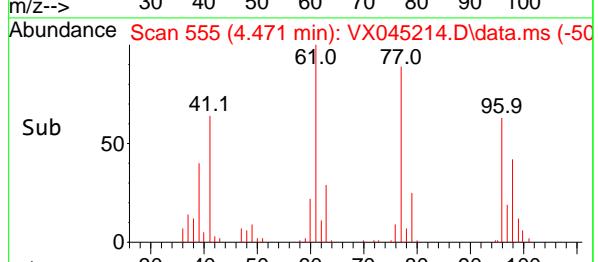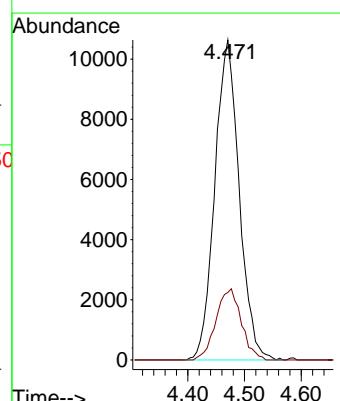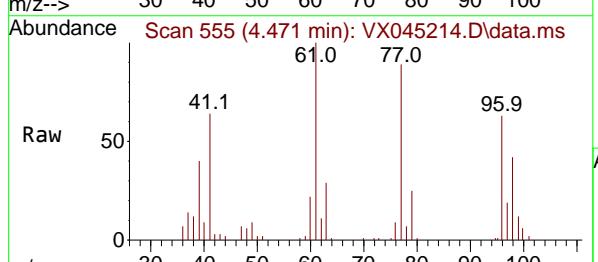

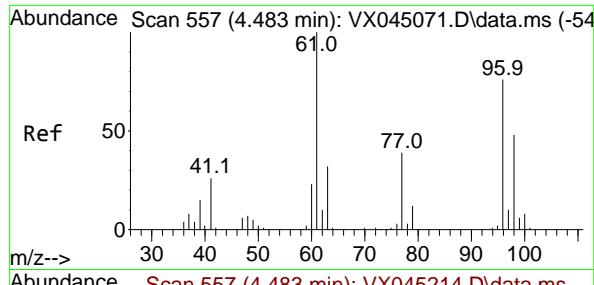



#27
cis-1,2-Dichloroethene
 Concen: 19.233 ug/l
 RT: 4.483 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14

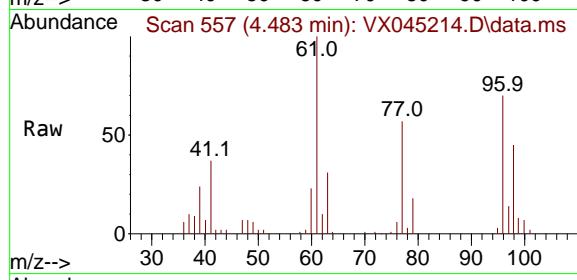


Tgt Ion: 96 Resp: 27319
 Ion Ratio Lower Upper
 96 100
 61 154.7 0.0 283.2
 98 64.3 0.0 128.0

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

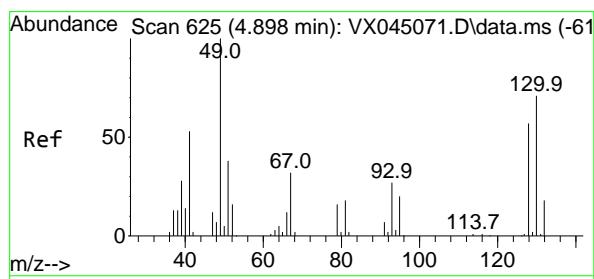


#28
 Bromochloromethane
 Concen: 20.441 ug/l
 RT: 4.891 min Scan# 624
 Delta R.T. -0.006 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14

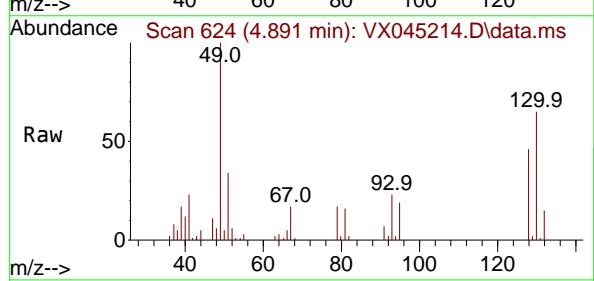


Tgt Ion: 49 Resp: 23024
 Ion Ratio Lower Upper
 49 100
 129 1.7 0.0 3.4
 130 68.8 56.1 84.1





#29
Tetrahydrofuran
Concen: 98.728 ug/l
RT: 5.007 min Scan# 6
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

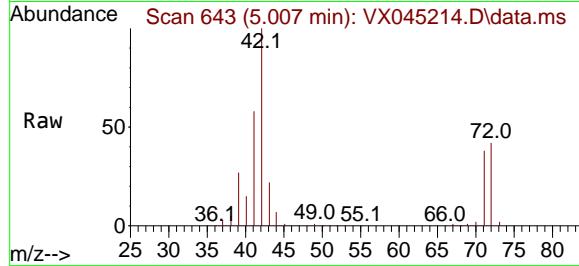


Tgt Ion: 42 Resp: 6981
Ion Ratio Lower Upper
42 100
72 42.0 34.1 51.1
71 38.7 31.4 47.0

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

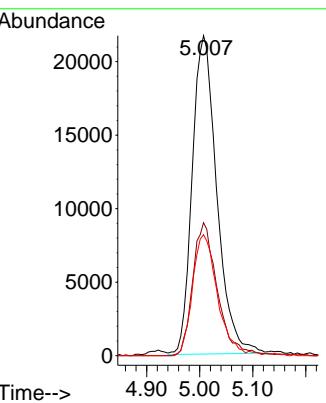


#30
Chloroform
Concen: 19.880 ug/l
RT: 5.092 min Scan# 657
Delta R.T. 0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion: 83 Resp: 46678
Ion Ratio Lower Upper
83 100
85 60.8 51.4 77.2

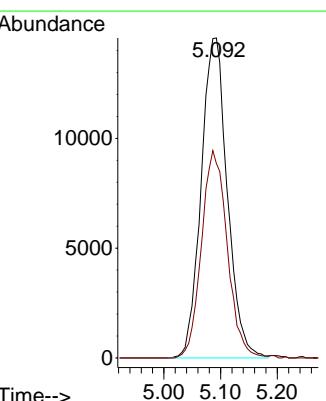



#31
Cyclohexane
Concen: 19.670 ug/l
RT: 5.458 min Scan# 7
Delta R.T. -0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
ClientSampleId : VX0311WBS01




Tgt Ion: 56 Resp: 40343
Ion Ratio Lower Upper
56 100
69 31.5 23.4 35.2
84 78.8 69.4 104.2

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#32
1,1,1-Trichloroethane
Concen: 19.990 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion: 97 Resp: 37908
Ion Ratio Lower Upper
97 100
99 63.3 51.6 77.4
61 49.1 38.4 57.6





#33
1,2-Dichloroethane-d4
Concen: 52.022 ug/l
RT: 5.952 min Scan# 7
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument :
MSVOA_X
ClientSampleId :
VX0311WBS01




Tgt Ion: 65 Resp: 78434
Ion Ratio Lower Upper
65 100
67 52.1 0.0 106.2

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion:114 Resp: 172566
Ion Ratio Lower Upper
114 100
63 22.5 0.0 41.8
88 16.2 0.0 32.8








#35
Dibromofluoromethane
Concen: 51.847 ug/l
RT: 5.385 min Scan# 7
Instrument : MSVOA_X
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion:113 Resp: 5982
Ion Ratio Lower Upper
113 100
111 102.5 81.8 122.6
192 17.4 14.3 21.5

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#36
1,1-Dichloropropene
Concen: 18.899 ug/l
RT: 5.684 min Scan# 754
Delta R.T. -0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion: 75 Resp: 29907
Ion Ratio Lower Upper
75 100
110 34.4 16.9 50.6
77 31.1 24.5 36.7



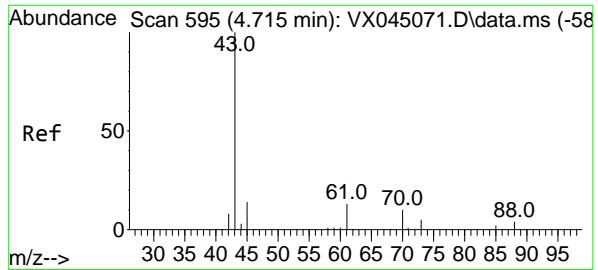

#37
Ethyl Acetate
 Concen: 19.054 ug/l
 RT: 4.714 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
 ClientSampleId : VX0311WBS01




Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
43	100			
61	13.2	3885	10.8	16.2
70	9.7		7.7	11.5

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

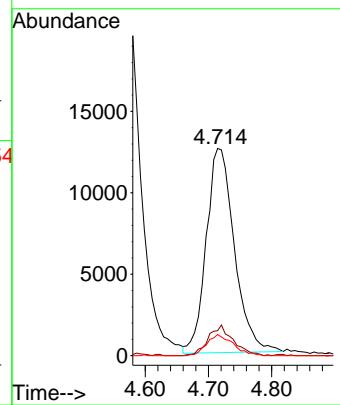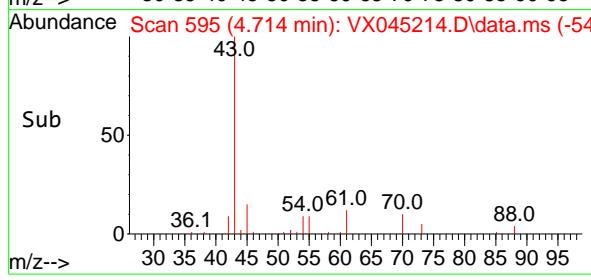


#38
Carbon Tetrachloride
 Concen: 19.746 ug/l
 RT: 5.665 min Scan# 751
 Delta R.T. -0.006 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14




Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
117	100			
119	89.6	31723	76.7	115.1
121	28.9		25.5	38.3

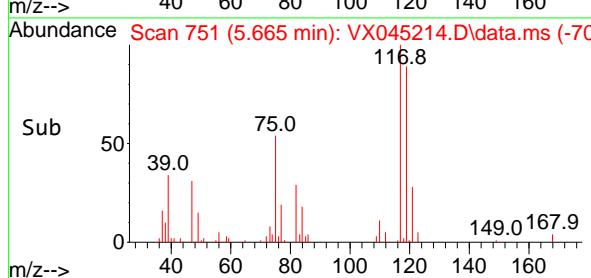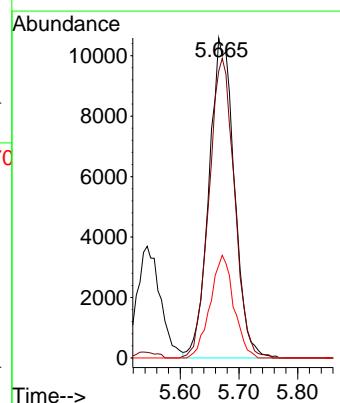



#39
Methylcyclohexane
Concen: 19.935 ug/l
RT: 7.372 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

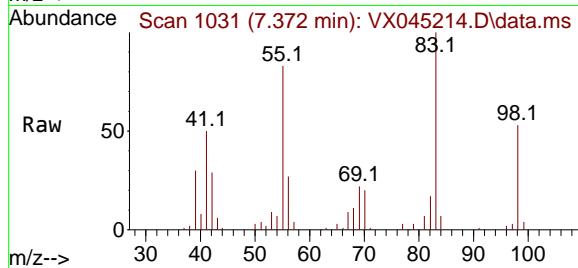


Tgt Ion: 83 Resp: 37800
Ion Ratio Lower Upper
83 100
55 82.7 63.0 94.4
98 52.6 39.7 59.5

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#40
Benzene
Concen: 19.364 ug/l
RT: 6.031 min Scan# 811
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion: 78 Resp: 96762
Ion Ratio Lower Upper
78 100
77 23.5 18.8 28.2





#41
Methacrylonitrile
Concen: 20.240 ug/l
RT: 4.922 min Scan# 61
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

Instrument : MSVOA_X
ClientSampleId : VX0311WBS01






Tgt Ion: 41 Resp: 22310
Ion Ratio Lower Upper

41	100
39	57.4
67	71.1
52	32.2

Lower	Upper
44.6	67.0
53.9	80.9
23.3	34.9

Manual Integrations APPROVED

Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025


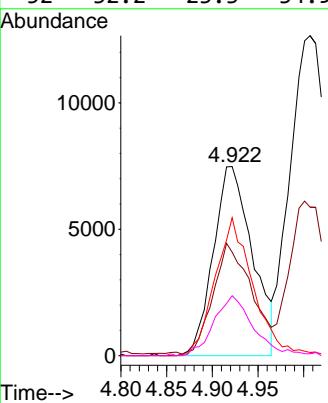




#42
1,2-Dichloroethane
Concen: 19.836 ug/l
RT: 6.086 min Scan# 820
Delta R.T. 0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

Tgt Ion: 62 Resp: 35693
Ion Ratio Lower Upper

62	100
98	9.0


0.0	18.2
-----	------

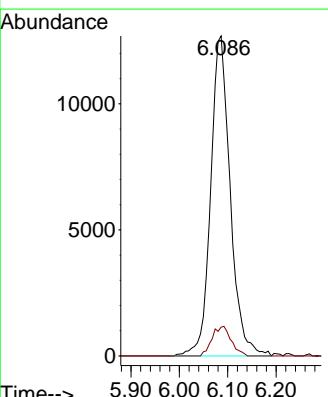



#43
Isopropyl Acetate
Concen: 20.011 ug/l
RT: 6.342 min Scan# 8
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01




Tgt Ion: 43 Resp: 60338
Ion Ratio Lower Upper
43 100
61 17.1 14.9 22.3
87 12.0 9.4 14.2

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#44
Trichloroethene
Concen: 18.944 ug/l
RT: 7.123 min Scan# 990
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion:130 Resp: 22228
Ion Ratio Lower Upper
130 100
95 102.1 0.0 205.0





#45
1,2-Dichloropropane
Concen: 18.936 ug/l
RT: 7.421 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01




Tgt Ion: 63 Resp: 24329
Ion Ratio Lower Upper
63 100
65 26.6 24.7 37.1

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

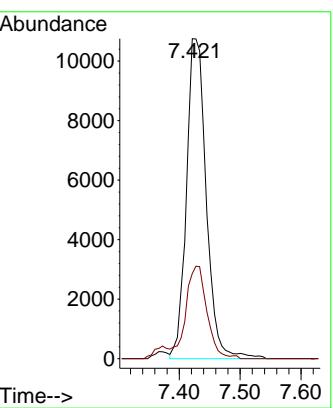


#46
Dibromomethane
Concen: 20.132 ug/l
RT: 7.580 min Scan# 1065
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion: 93 Resp: 18282
Ion Ratio Lower Upper
93 100
95 79.8 65.8 98.8
174 87.9 72.2 108.2

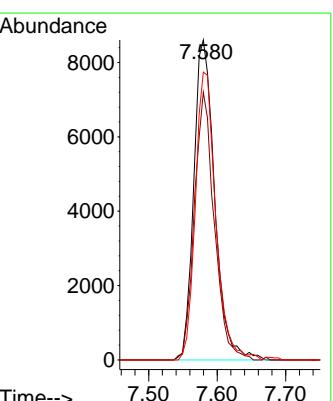



#47
 Bromodichloromethane
 Concen: 19.571 ug/l
 RT: 7.818 min Scan# 1104
 Delta R.T. -0.000 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
 ClientSampleId : VX0311WBS01




Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
83	100	34860		
85	64.2		51.1	76.7
127	8.3		6.4	9.6

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

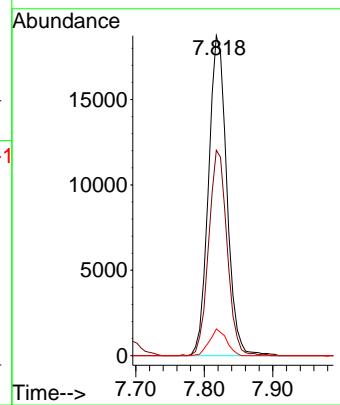


#48
 Methyl methacrylate
 Concen: 19.905 ug/l
 RT: 7.696 min Scan# 1084
 Delta R.T. 0.006 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14



Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
41	100	30110		
69	73.9		63.0	94.6
39	61.1		47.5	71.3

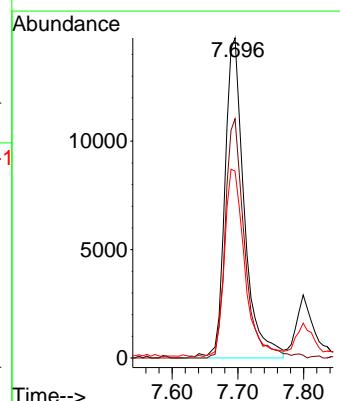






#49
1,4-Dioxane
Concen: 376.974 ug/l
RT: 7.665 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

Tgt Ion:	88	Resp:	12029
Ion Ratio	100	Lower	Upper
88	100		
43	40.5	28.7	43.1
58	76.0	55.8	83.8





Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

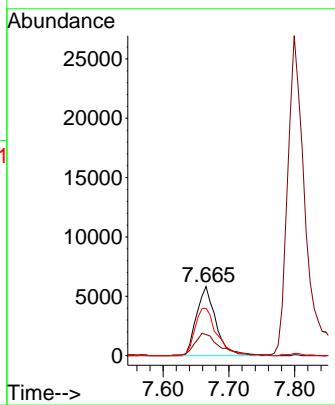

#50
Toluene-d8
Concen: 51.200 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14


Tgt Ion:	98	Resp:	214187
Ion Ratio	100	Lower	Upper
98	100		
100	65.0	52.0	78.0

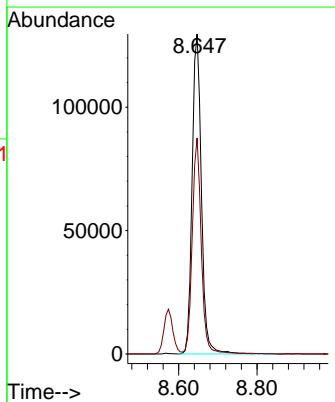



#51
4-Methyl-2-Pentanone
Concen: 105.932 ug/l
RT: 8.573 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

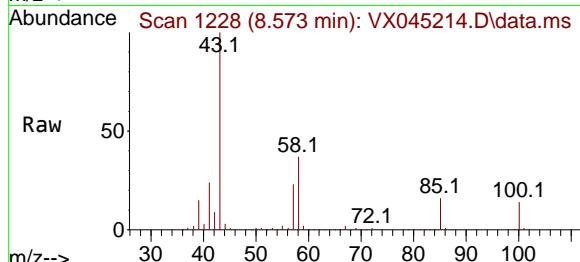


Tgt Ion: 43 Resp: 21446
Ion Ratio Lower Upper
43 100
58 35.7 29.2 43.8

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

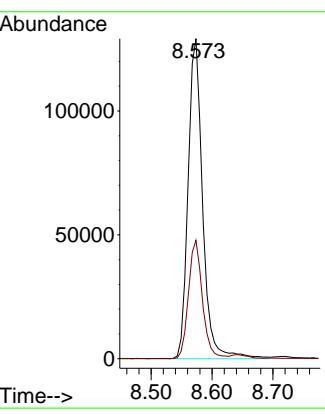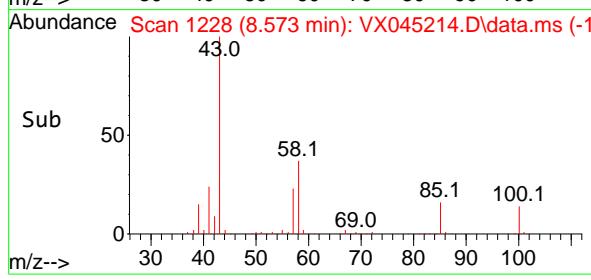


#52
Toluene
Concen: 20.030 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion: 92 Resp: 58726
Ion Ratio Lower Upper
92 100
91 174.6 138.9 208.3

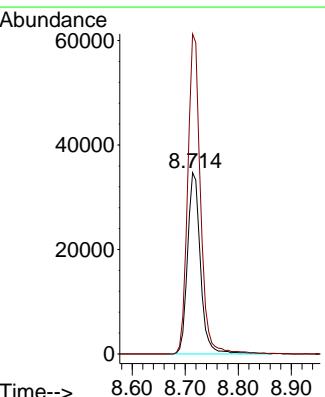

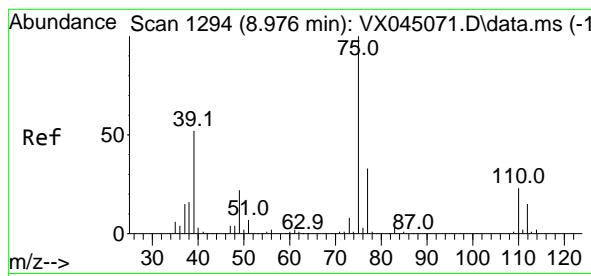

#53
t-1,3-Dichloropropene
Concen: 20.021 ug/l
RT: 8.976 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01



Tgt Ion: 75 Resp: 29814
Ion Ratio Lower Upper
75 100
77 30.8 26.5 39.7




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#54
cis-1,3-Dichloropropene
Concen: 20.578 ug/l
RT: 8.366 min Scan# 1194
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14


Tgt Ion: 75 Resp: 35732
Ion Ratio Lower Upper
75 100
77 33.5 24.7 37.1
39 51.8 40.7 61.1

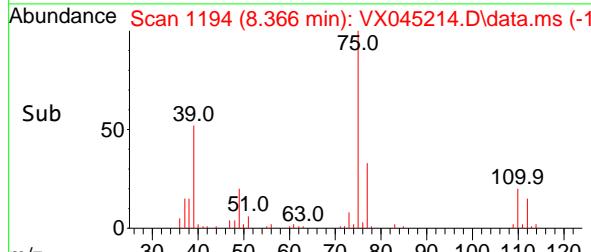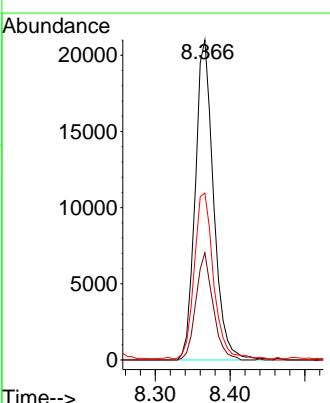



#55
1,1,2-Trichloroethane
Concen: 19.483 ug/l
RT: 9.153 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

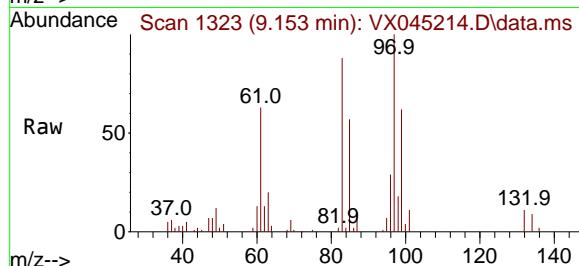


Tgt Ion: 97 Resp: 23510
Ion Ratio Lower Upper
97 100
83 88.5 69.4 104.2
85 56.6 44.1 66.1
99 61.6 50.7 76.1

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#56
Ethyl methacrylate
Concen: 19.616 ug/l
RT: 9.116 min Scan# 1317
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion: 69 Resp: 35989
Ion Ratio Lower Upper
69 100
41 74.9 57.0 85.4
39 45.8 34.2 51.4





#57
1,3-Dichloropropane
Concen: 20.124 ug/l
RT: 9.305 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01



Tgt Ion: 76 Resp: 42034
Ion Ratio Lower Upper
76 100
78 31.9 25.5 38.3




Manual Integrations APPROVED


Reviewed By :John Carbone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#58
2-Chloroethyl Vinyl ether
Concen: 96.201 ug/l
RT: 8.238 min Scan# 1173
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14


Tgt Ion: 63 Resp: 86098
Ion Ratio Lower Upper
63 100
106 25.6 21.5 32.3





#59
2-Hexanone
Concen: 108.556 ug/l
RT: 9.427 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01



Tgt Ion: 43 Resp: 159240
Ion Ratio Lower Upper
43 100
58 51.5 25.9 77.6




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#60
Dibromochloromethane
Concen: 19.524 ug/l
RT: 9.518 min Scan# 1383
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14


Tgt Ion:129 Resp: 24640
Ion Ratio Lower Upper
129 100
127 78.0 38.5 115.5





#61
1,2-Dibromoethane
Concen: 19.647 ug/l
RT: 9.610 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01



Tgt Ion:107 Resp: 2367
Ion Ratio Lower Upper
107 100
109 92.7 76.1 114.1



Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

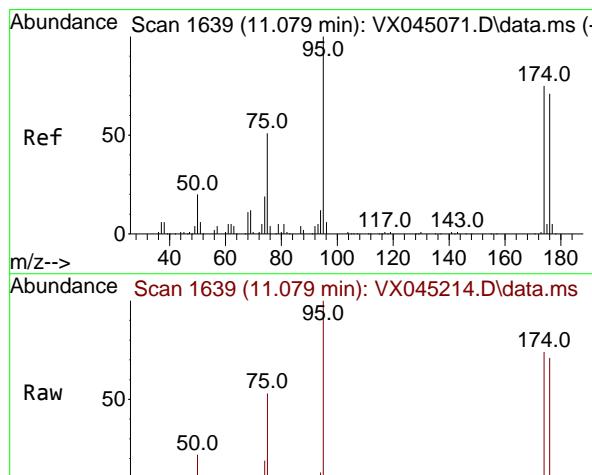

#62
4-Bromofluorobenzene
Concen: 52.930 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

Tgt Ion: 95 Resp: 73373
Ion Ratio Lower Upper
95 100
174 72.7 0.0 148.2
176 70.8 0.0 141.4

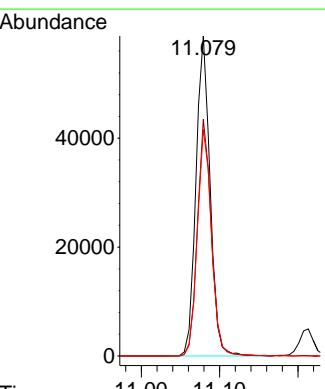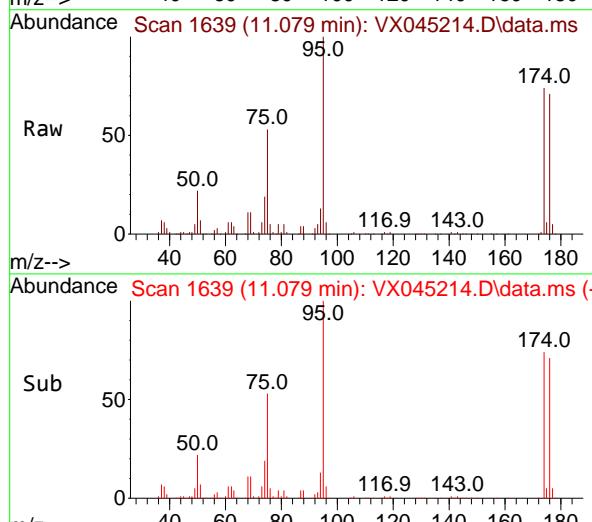


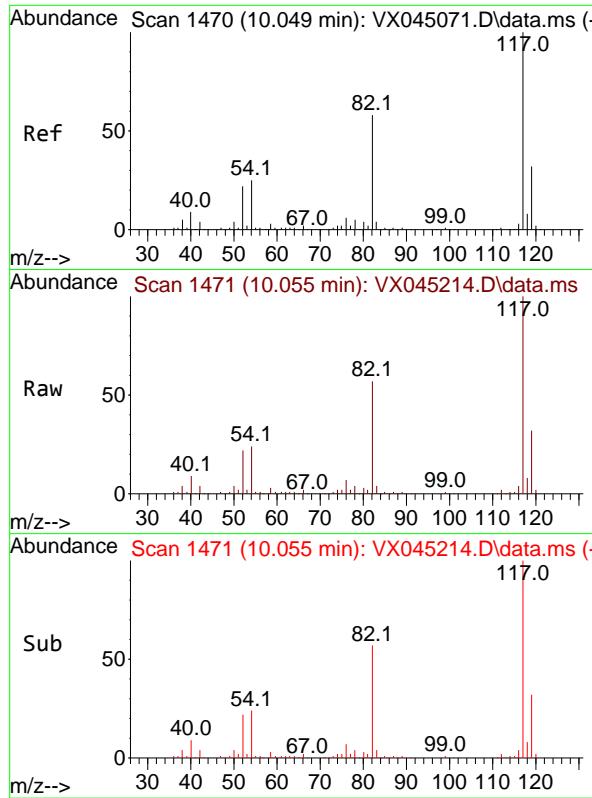


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1470
Delta R.T. 0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

Instrument : MSVOA_X
ClientSampleId : VX0311WBS01


Manual Integrations
APPROVED


Reviewed By :John Carbone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

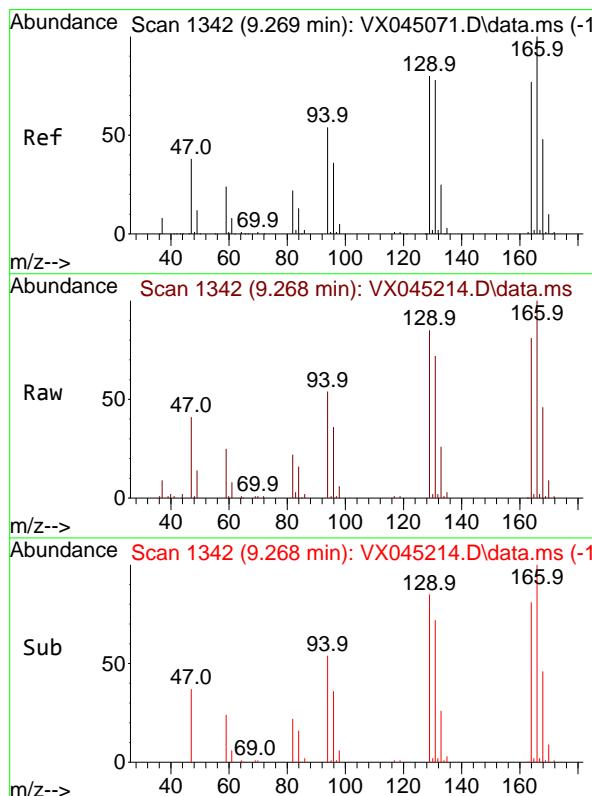

#64
Tetrachloroethene
Concen: 19.537 ug/l
RT: 9.268 min Scan# 1342
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14


Tgt Ion:164 Resp: 18990
Ion Ratio Lower Upper
164 100
166 123.4 103.6 155.4
129 105.2 82.7 124.1
131 88.4 80.5 120.7



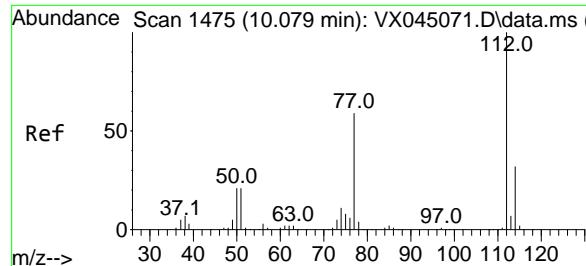

#65
Chlorobenzene
Concen: 19.739 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

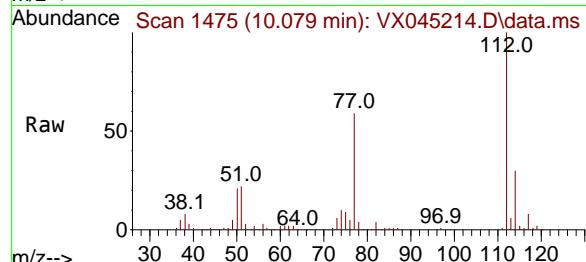

Tgt Ion:112 Resp: 63389
Ion Ratio Lower Upper
112 100
114 30.3 26.0 39.0





Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

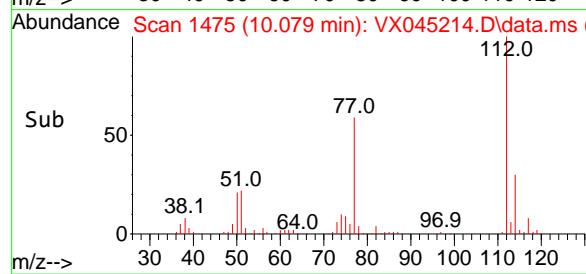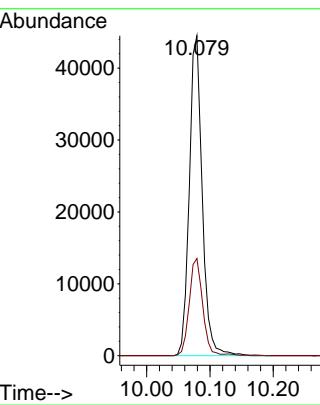

#66
1,1,1,2-Tetrachloroethane
Concen: 19.659 ug/l
RT: 10.159 min Scan# 1488
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

Tgt Ion:131 Resp: 21025
Ion Ratio Lower Upper
131 100
133 93.4 48.6 145.9
119 66.2 33.9 101.7

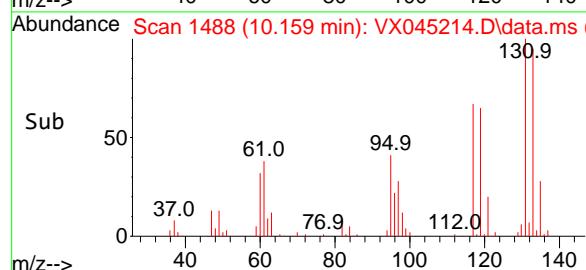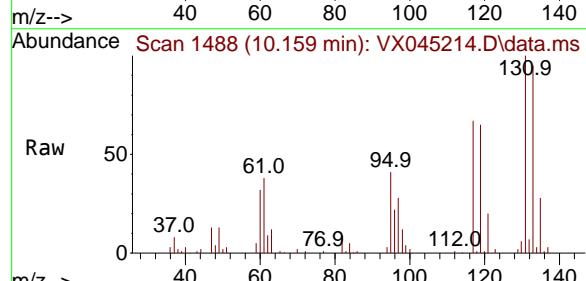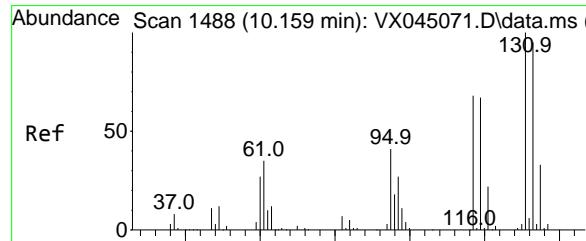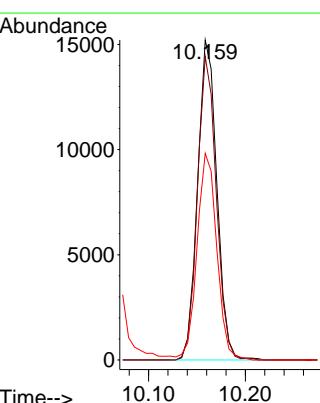



#67

Ethyl Benzene



Concen: 19.770 ug/l

RT: 10.189 min Scan# 1493

Delta R.T. -0.000 min

Lab File: VX045214.D

Acq: 11 Mar 2025 11:14

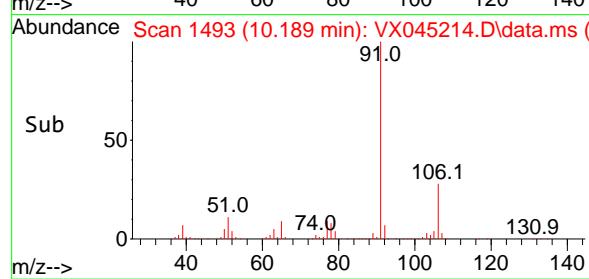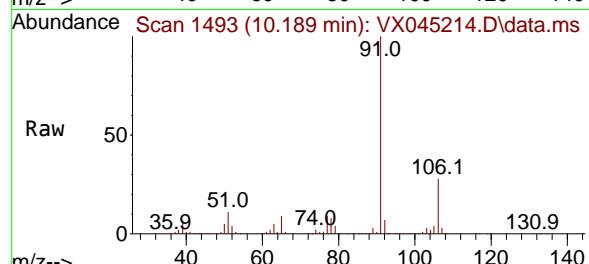

Tgt Ion: 91 Resp: 11062



Ion Ratio Lower Upper

91 100

106 28.4 23.9 35.9

Manual Integrations APPROVED

Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

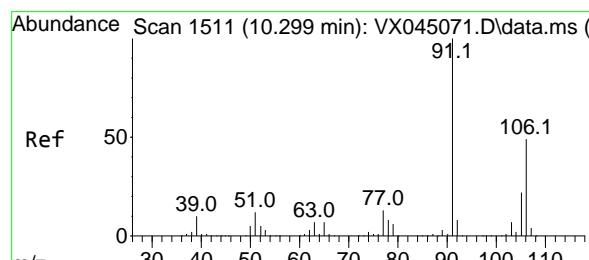

#68

m/p-Xylenes


Concen: 40.069 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX045214.D

Acq: 11 Mar 2025 11:14


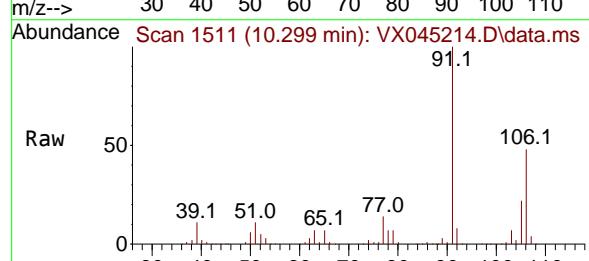



Tgt Ion:106 Resp: 82080

Ion Ratio Lower Upper

106 100


91 206.1 165.4 248.0

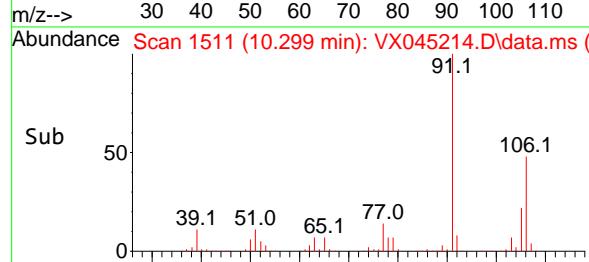



#69
o-Xylene
Concen: 19.413 ug/l
RT: 10.640 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument :
MSVOA_X
ClientSampleId :
VX0311WBS01




Tgt Ion:106 Resp: 40103
Ion Ratio Lower Upper
106 100
91 221.5 109.9 329.6

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#70
Styrene
Concen: 20.260 ug/l
RT: 10.652 min Scan# 1569
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion:104 Resp: 67728
Ion Ratio Lower Upper
104 100
78 53.0 42.2 63.4
103 54.3 43.8 65.8





#71
Bromoform
Concen: 20.029 ug/l
RT: 10.799 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01



Tgt	Ion:173	Resp:	16153
	Ion Ratio	Lower	Upper
173	100		
175	46.6	24.6	73.6
254	0.0	0.0	0.0




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14


Tgt	Ion:152	Resp:	71836
	Ion Ratio	Lower	Upper
152	100		
115	69.9	44.2	132.6
150	159.1	0.0	349.0

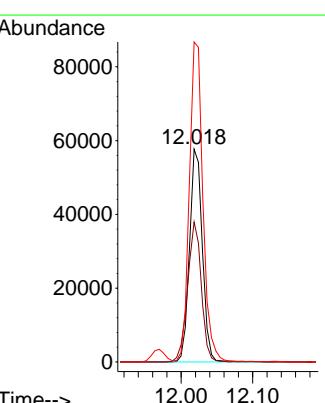

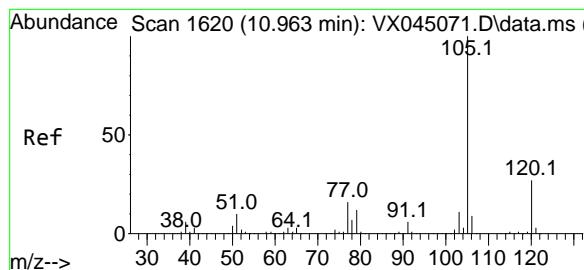

#73
Isopropylbenzene
Concen: 19.084 ug/l
RT: 10.963 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

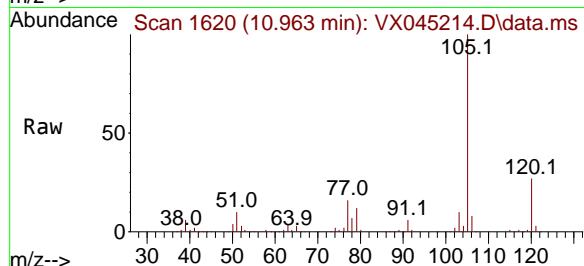


Tgt Ion:105 Resp: 10700
Ion Ratio Lower Upper
105 100
120 25.6 13.2 39.5

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

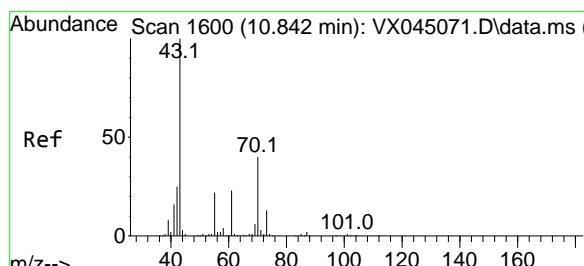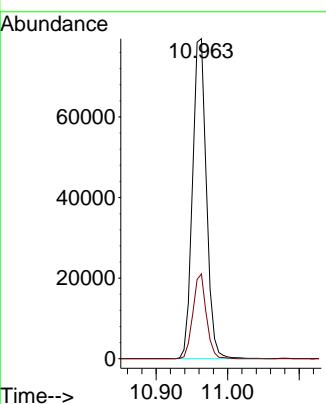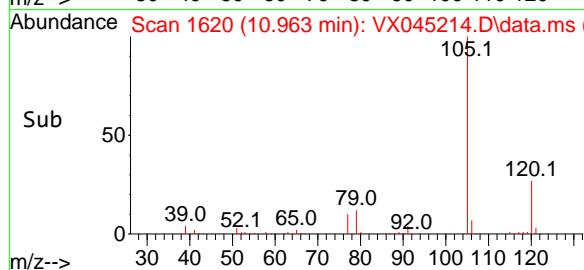


#74
N-amyl acetate
Concen: 19.067 ug/l
RT: 10.841 min Scan# 1600
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

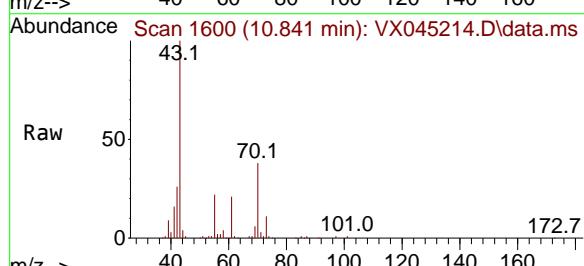


Tgt Ion: 43 Resp: 50165
Ion Ratio Lower Upper
43 100
70 40.0 31.8 47.6
55 23.5 18.3 27.5
61 22.0 18.3 27.5

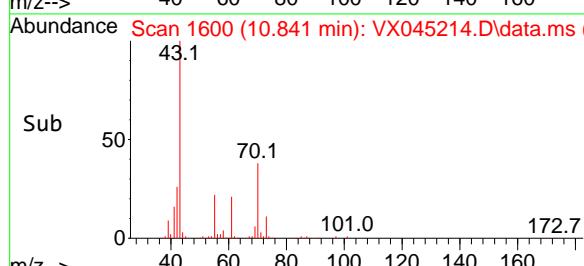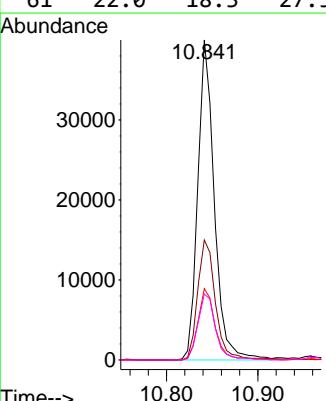



#75
1,1,2,2-Tetrachloroethane
Concen: 19.498 ug/l
RT: 11.213 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

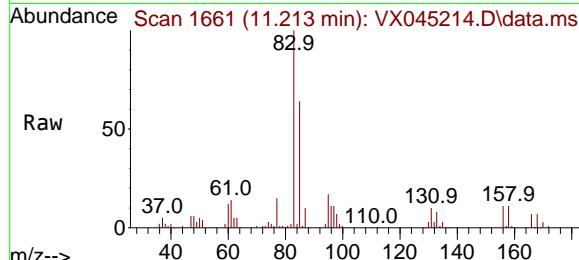


Tgt Ion: 83 Resp: 40119
Ion Ratio Lower Upper
83 100
131 9.6 4.5 13.4
85 63.2 31.7 95.1

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#76
1,2,3-Trichloropropane
Concen: 19.230 ug/l
RT: 11.238 min Scan# 1665
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion: 75 Resp: 32153
Ion Ratio Lower Upper
75 100
77 41.9 20.7 62.1

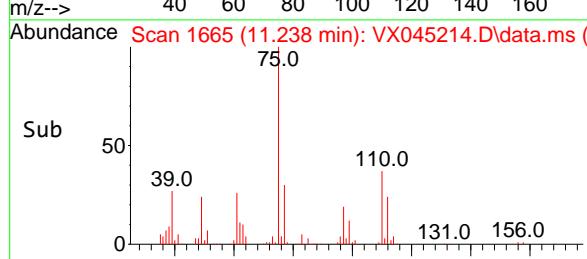



#77
Bromobenzene
Concen: 18.531 ug/l
RT: 11.195 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
ClientSampleId : VX0311WBS01



Tgt Ion:156 Resp: 24519
Ion Ratio Lower Upper
156 100
77 170.4 85.8 257.4
158 95.0 48.4 145.2




Manual Integrations
APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#78
n-propylbenzene
Concen: 19.227 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14


Tgt Ion: 91 Resp: 121782
Ion Ratio Lower Upper
91 100
120 22.2 11.2 33.6

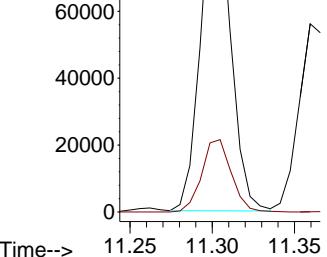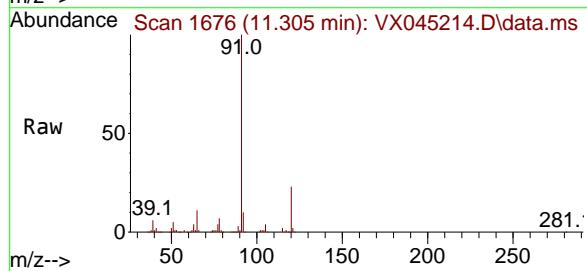



#79
2-Chlorotoluene
Concen: 18.427 ug/l
RT: 11.360 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument :
MSVOA_X
ClientSampleId :
VX0311WBS01




Tgt Ion: 91 Resp: 7433
Ion Ratio Lower Upper
91 100
126 32.2 16.4 49.4

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

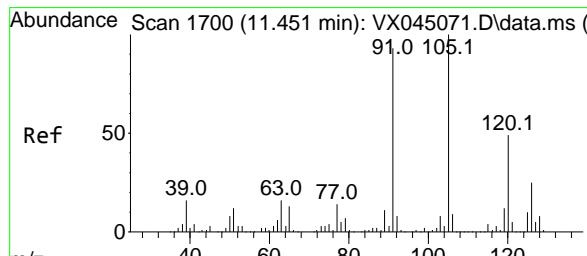


#80
1,3,5-Trimethylbenzene
Concen: 19.336 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

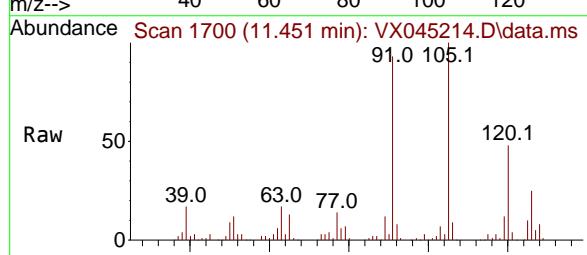


Tgt Ion:105 Resp: 87665
Ion Ratio Lower Upper
105 100
120 47.0 24.1 72.2





#81
trans-1,4-Dichloro-2-butene
Concen: 18.233 ug/l
RT: 11.018 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

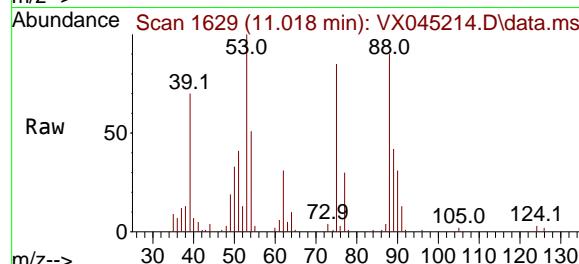

Tgt Ion: 75 Resp: 8903
Ion Ratio Lower Upper
75 100
53 120.4 88.5 132.7
89 49.0 36.2 54.4




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

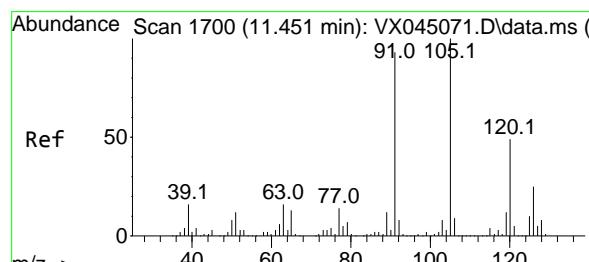

#82
4-Chlorotoluene
Concen: 19.196 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14


Tgt Ion: 91 Resp: 84393
Ion Ratio Lower Upper
91 100
126 27.6 14.1 42.4





#83
 tert-Butylbenzene
 Concen: 18.764 ug/l
 RT: 11.713 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
 ClientSampleId : VX0311WBS01



Tgt Ion:119 Resp: 87401
 Ion Ratio Lower Upper
 119 100
 91 61.8 30.7 92.1
 134 23.7 11.7 35.0



Manual Integrations APPROVED

Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025







#84
 1,2,4-Trimethylbenzene
 Concen: 19.161 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. -0.000 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14

Tgt Ion:105 Resp: 87408
 Ion Ratio Lower Upper
 105 100
 120 43.7 22.1 66.1




#84
 1,2,4-Trimethylbenzene
 Concen: 19.161 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. -0.000 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14

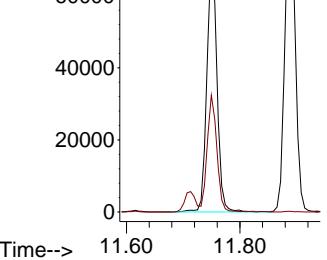



#85
sec-Butylbenzene
Concen: 19.595 ug/l
RT: 11.890 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
ClientSampleId : VX0311WBS01




Tgt Ion:105 Resp: 109340
Ion Ratio Lower Upper
105 100
134 19.6 9.8 29.4

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#86
p-Isopropyltoluene
Concen: 19.784 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Tgt Ion:119 Resp: 89213
Ion Ratio Lower Upper
119 100
134 25.5 12.9 38.6
91 25.5 12.7 38.0





#87
1,3-Dichlorobenzene
Concen: 19.261 ug/l
RT: 11.969 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument :
MSVOA_X
ClientSampleId :
VX0311WBS01



Tgt	Ion:146	Resp:	45450
Ion Ratio		Lower	Upper
146	100		
111	41.1	21.1	63.4
148	61.0	31.9	95.7


Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#88
1,4-Dichlorobenzene
Concen: 18.734 ug/l
RT: 12.042 min Scan# 1797
Delta R.T. 0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14


Tgt	Ion:146	Resp:	44731
Ion Ratio		Lower	Upper
146	100		
111	42.0	20.2	60.5
148	63.7	31.9	95.9

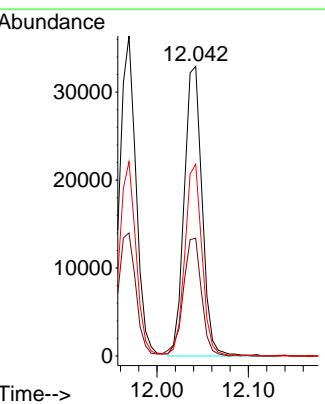



#89
n-Butylbenzene
Concen: 19.837 ug/l
RT: 12.329 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
ClientSampleId : VX0311WBS01

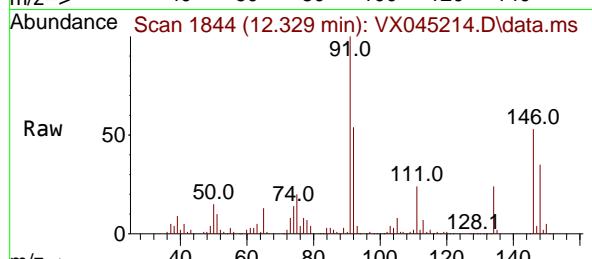


Tgt Ion: 91 Resp: 7704
Ion Ratio Lower Upper
91 100
92 52.4 26.7 80.0
134 23.8 12.2 36.6

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

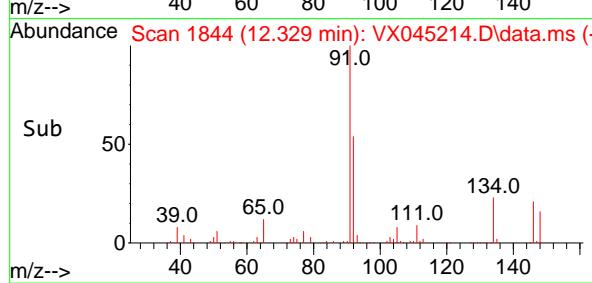

#90
Hexachloroethane
Concen: 17.526 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14

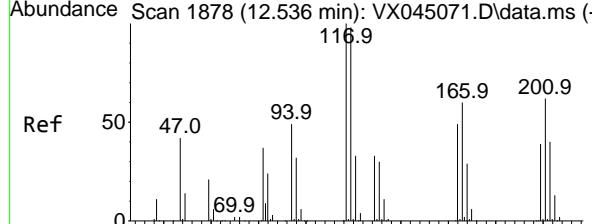


Tgt Ion:117 Resp: 14295
Ion Ratio Lower Upper
117 100
201 65.6 31.9 95.9

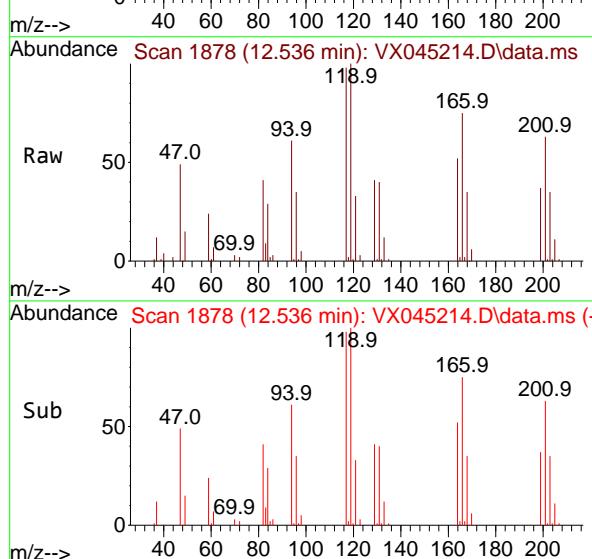

Sub


m/z-->

m/z	Relative Abundance (approx)
47.0	10
69.9	10
93.9	10
118.9	100
165.9	30
200.9	30



#91
1,2-Dichlorobenzene
Concen: 19.416 ug/l
RT: 12.335 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14




Instrument : MSVOA_X
ClientSampleId : VX0311WBS01




Tgt Ion:146 Resp: 45960
Ion Ratio Lower Upper
146 100
111 43.2 21.6 65.0
148 63.8 31.9 95.9

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

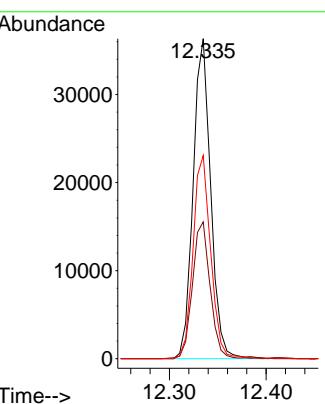


#92
1,2-Dibromo-3-Chloropropane
Concen: 19.117 ug/l
RT: 12.945 min Scan# 1945
Delta R.T. 0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Tgt Ion: 75 Resp: 7663
Ion Ratio Lower Upper
75 100
155 75.0 39.6 118.7
157 99.5 51.1 153.4




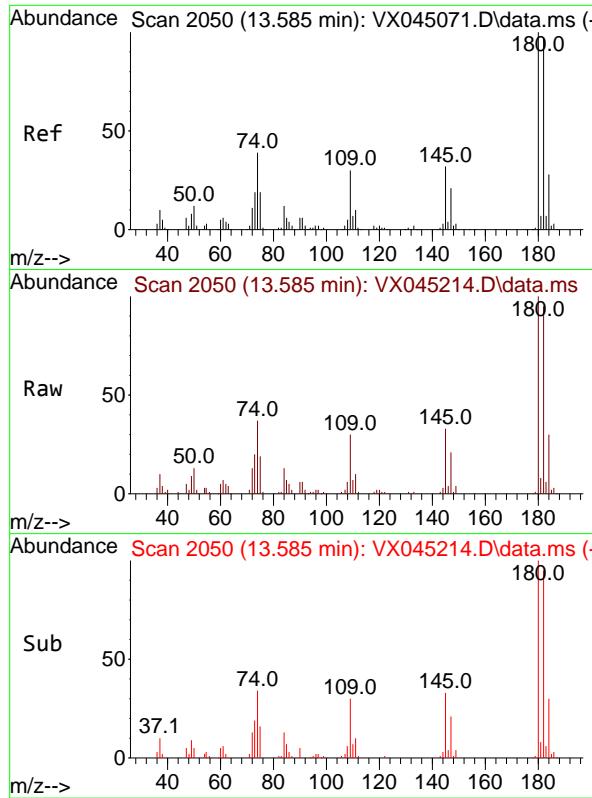


#93
 1,2,4-Trichlorobenzene
 Concen: 18.873 ug/l
 RT: 13.585 min Scan# 2
 Delta R.T. -0.000 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14

Instrument : MSVOA_X
 ClientSampleId : VX0311WBS01


Manual Integrations
APPROVED


Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

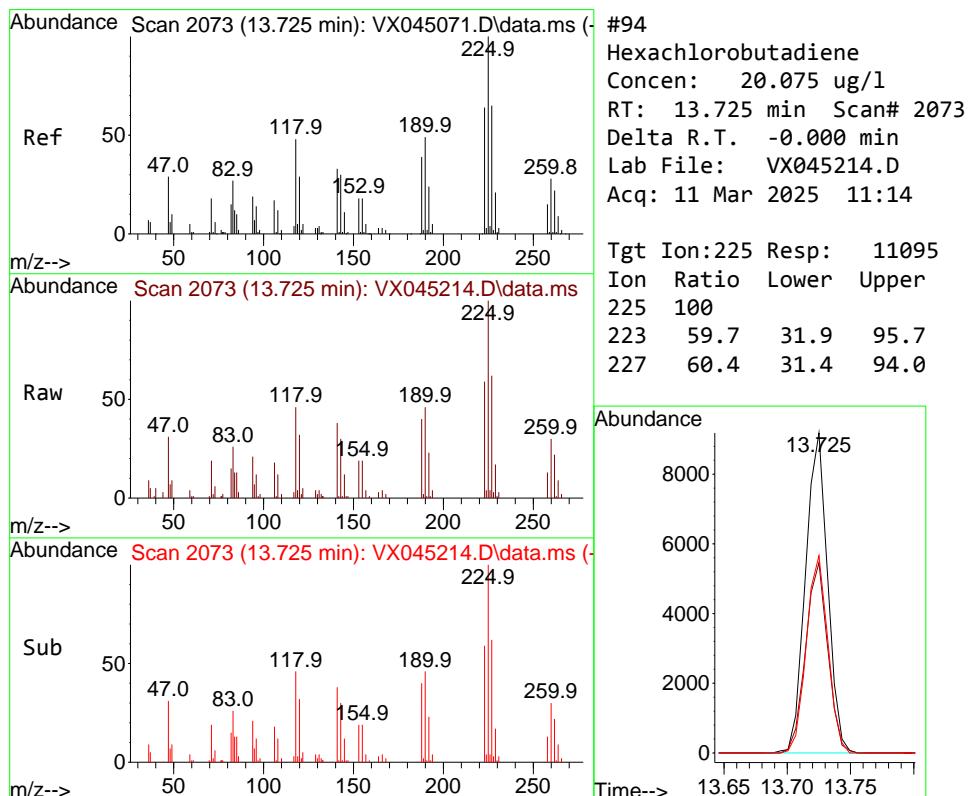

#94
 Hexachlorobutadiene
 Concen: 20.075 ug/l
 RT: 13.725 min Scan# 2073
 Delta R.T. -0.000 min
 Lab File: VX045214.D
 Acq: 11 Mar 2025 11:14


Tgt Ion:225 Resp: 11095
 Ion Ratio Lower Upper
 225 100
 223 59.7 31.9 95.7
 227 60.4 31.4 94.0





#95
Naphthalene
Concen: 18.846 ug/l
RT: 13.774 min Scan# 2
Delta R.T. -0.000 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Instrument : MSVOA_X
ClientSampleId : VX0311WBS01




Tgt Ion:128 Resp: 9761
Ion Ratio Lower Upper
128 100
127 12.8 10.3 15.5
129 10.8 8.7 13.1

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#96
1,2,3-Trichlorobenzene
Concen: 18.685 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.006 min
Lab File: VX045214.D
Acq: 11 Mar 2025 11:14



Tgt Ion:180 Resp: 26572
Ion Ratio Lower Upper
180 100
182 94.4 47.5 142.6
145 34.2 17.0 50.9

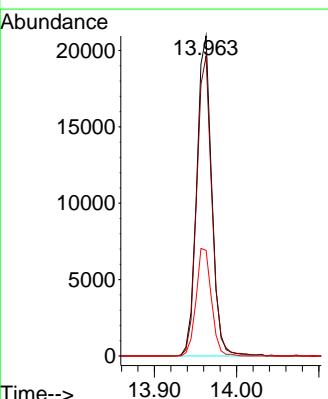

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Waste Water PT			Date Received:
Client Sample ID:	VX0311WBSD01	SDG No.:	Q1502	
Lab Sample ID:	VX0311WBSD01	Matrix:	Water	
Analytical Method:	SW8260	% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol: 5000 uL
Soil Aliquot Vol:		uL		Test: VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level : LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045215.D	1		03/11/25 11:40	VX031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
75-71-8	Dichlorodifluoromethane	19.4		0.21	1.00	ug/L
74-87-3	Chloromethane	17.9		0.35	1.00	ug/L
75-01-4	Vinyl Chloride	16.9		0.34	1.00	ug/L
74-83-9	Bromomethane	19.1		1.40	5.00	ug/L
75-00-3	Chloroethane	19.7		0.56	1.00	ug/L
75-69-4	Trichlorofluoromethane	18.7		0.34	1.00	ug/L
75-35-4	1,1-Dichloroethene	18.4		0.26	1.00	ug/L
107-02-8	Acrolein	79.1		6.70	25.0	ug/L
107-13-1	Acrylonitrile	100		0.90	5.00	ug/L
67-64-1	Acetone	96.0		1.40	5.00	ug/L
75-15-0	Carbon Disulfide	16.4		0.32	1.00	ug/L
1634-04-4	Methyl tert-butyl Ether	19.3		0.16	1.00	ug/L
75-09-2	Methylene Chloride	19.2		0.32	1.00	ug/L
156-60-5	trans-1,2-Dichloroethene	19.2		0.25	1.00	ug/L
108-05-4	Vinyl Acetate	99.8		0.71	5.00	ug/L
75-34-3	1,1-Dichloroethane	19.2		0.23	1.00	ug/L
78-93-3	2-Butanone	100		1.30	5.00	ug/L
56-23-5	Carbon Tetrachloride	19.4		0.25	1.00	ug/L
594-20-7	2,2-Dichloropropane	27.1		0.31	1.00	ug/L
156-59-2	cis-1,2-Dichloroethene	19.2		0.25	1.00	ug/L
74-97-5	Bromoform	19.9		0.18	1.00	ug/L
67-66-3	Chloroform	19.5		0.26	1.00	ug/L
71-55-6	1,1,1-Trichloroethane	19.2		0.19	1.00	ug/L
563-58-6	1,1-Dichloropropene	18.9		0.18	1.00	ug/L
71-43-2	Benzene	19.2		0.16	1.00	ug/L
107-06-2	1,2-Dichloroethane	19.9		0.24	1.00	ug/L
79-01-6	Trichloroethene	19.0		0.32	1.00	ug/L
78-87-5	1,2-Dichloropropane	19.1		0.19	1.00	ug/L
74-95-3	Dibromomethane	19.8		0.23	1.00	ug/L
75-27-4	Bromodichloromethane	19.8		0.24	1.00	ug/L

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Waste Water PT			Date Received:
Client Sample ID:	VX0311WBSD01	SDG No.:	Q1502	
Lab Sample ID:	VX0311WBSD01	Matrix:	Water	
Analytical Method:	SW8260	% Solid:	0	
Sample Wt/Vol:	5	Units:	mL	Final Vol: 5000 uL
Soil Aliquot Vol:		uL		Test: VOCMS Group1
GC Column:	DB-624UI	ID :	0.18	Level : LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045215.D	1		03/11/25 11:40	VX031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
108-10-1	4-Methyl-2-Pentanone	110		0.75	5.00	ug/L
108-88-3	Toluene	19.8		0.18	1.00	ug/L
10061-02-6	t-1,3-Dichloropropene	20.1		0.21	1.00	ug/L
10061-01-5	cis-1,3-Dichloropropene	20.1		0.18	1.00	ug/L
79-00-5	1,1,2-Trichloroethane	20.0		0.21	1.00	ug/L
142-28-9	1,3-Dichloropropane	20.6		0.17	1.00	ug/L
110-75-8	2-Chloroethyl Vinyl ether	98.3		1.80	5.00	ug/L
591-78-6	2-Hexanone	110		1.10	5.00	ug/L
124-48-1	Dibromochloromethane	19.9		0.18	1.00	ug/L
106-93-4	1,2-Dibromoethane	20.7		0.16	1.00	ug/L
127-18-4	Tetrachloroethene	19.3		0.25	1.00	ug/L
108-90-7	Chlorobenzene	19.6		0.13	1.00	ug/L
630-20-6	1,1,1,2-Tetrachloroethane	19.0		0.21	1.00	ug/L
67-72-1	Hexachloroethane	18.3		0	0	ug/L
100-41-4	Ethyl Benzene	19.7		0.16	1.00	ug/L
179601-23-1	m/p-Xylenes	39.9		0.31	2.00	ug/L
1330-20-7	Total Xylenes	60.1		0.45	3.00	ug/L
95-47-6	o-Xylene	20.2		0.14	1.00	ug/L
100-42-5	Styrene	20.5		0.16	1.00	ug/L
75-25-2	Bromoform	20.3		0.21	1.00	ug/L
98-82-8	Isopropylbenzene	19.4		0.13	1.00	ug/L
79-34-5	1,1,2,2-Tetrachloroethane	19.7		0.27	1.00	ug/L
96-18-4	1,2,3-Trichloropropane	19.2		0.39	1.00	ug/L
108-86-1	Bromobenzene	19.4		0.26	1.00	ug/L
103-65-1	n-propylbenzene	19.9		0.14	1.00	ug/L
95-49-8	2-Chlorotoluene	19.3		0.16	1.00	ug/L
108-67-8	1,3,5-Trimethylbenzene	20.1		0.18	1.00	ug/L
106-43-4	4-Chlorotoluene	20.0		0.18	1.00	ug/L
98-06-6	tert-Butylbenzene	19.3		0.17	1.00	ug/L
95-63-6	1,2,4-Trimethylbenzene	20.0		0.18	1.00	ug/L
135-98-8	sec-Butylbenzene	20.5		0.17	1.00	ug/L

Report of Analysis

Client:	Alliance Technical Group, LLC - Newark			Date Collected:
Project:	NJ Waste Water PT			Date Received:
Client Sample ID:	VX0311WBSD01		SDG No.:	Q1502
Lab Sample ID:	VX0311WBSD01		Matrix:	Water
Analytical Method:	SW8260		% Solid:	0
Sample Wt/Vol:	5	Units: mL	Final Vol:	5000 uL
Soil Aliquot Vol:		uL	Test:	VOCMS Group1
GC Column:	DB-624UI	ID : 0.18	Level :	LOW
Prep Method :				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
VX045215.D	1		03/11/25 11:40	VX031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
99-87-6	p-Isopropyltoluene	20.5		0.15	1.00	ug/L
541-73-1	1,3-Dichlorobenzene	19.6		0.24	1.00	ug/L
106-46-7	1,4-Dichlorobenzene	19.2		0.27	1.00	ug/L
104-51-8	n-Butylbenzene	20.6		0.22	1.00	ug/L
95-50-1	1,2-Dichlorobenzene	19.8		0.19	1.00	ug/L
96-12-8	1,2-Dibromo-3-Chloropropane	19.4		0.46	1.00	ug/L
120-82-1	1,2,4-Trichlorobenzene	19.5		0.42	1.00	ug/L
87-68-3	Hexachlorobutadiene	19.9		0.31	1.00	ug/L
91-20-3	Naphthalene	19.2		0.59	1.00	ug/L
87-61-6	1,2,3-Trichlorobenzene	19.3		0.51	1.00	ug/L
SURROGATES						
17060-07-0	1,2-Dichloroethane-d4	51.1		74 - 125	102%	SPK: 50
1868-53-7	Dibromofluoromethane	51.0		75 - 124	102%	SPK: 50
2037-26-5	Toluene-d8	50.7		86 - 113	101%	SPK: 50
460-00-4	4-Bromofluorobenzene	54.4		77 - 121	109%	SPK: 50
INTERNAL STANDARDS						
363-72-4	Pentafluorobenzene	92100	5.544			
540-36-3	1,4-Difluorobenzene	166000	6.757			
3114-55-4	Chlorobenzene-d5	149000	10.049			
3855-82-1	1,4-Dichlorobenzene-d4	68900	12.018			

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

() = Laboratory InHouse Limit

A = Aldol-Condensation Reaction Products

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045215.D
 Acq On : 11 Mar 2025 11:40
 Operator : JC/MD
 Sample : VX0311WBSD01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0311WBSD01

Quant Time: Mar 12 01:44:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.544	168	92082	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	166231	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	148942	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	68861	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	74856	51.107	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 102.220%		
35) Dibromofluoromethane	5.379	113	56645	50.961	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 101.920%		
50) Toluene-d8	8.647	98	204141	50.659	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 101.320%		
62) 4-Bromofluorobenzene	11.079	95	72695	54.440	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery	= 108.880%		
Target Compounds						
				Qvalue		
2) Dichlorodifluoromethane	1.166	85	22434	19.355	ug/l	93
3) Chloromethane	1.307	50	25404	17.909	ug/l	98
4) Vinyl Chloride	1.374	62	23820	16.928	ug/l	95
5) Bromomethane	1.593	94	10572	19.112	ug/l	100
6) Chloroethane	1.666	64	12761	19.661	ug/l	88
7) Trichlorofluoromethane	1.867	101	34778	18.670	ug/l	96
8) Diethyl Ether	2.130	74	12910	17.718	ug/l	99
9) 1,1,2-Trichlorotrifluo...	2.312	101	22149	20.696	ug/l	99
10) Methyl Iodide	2.440	142	25294	18.912	ug/l	96
11) Tert butyl alcohol	2.977	59	23337	84.116	ug/l	100
12) 1,1-Dichloroethene	2.306	96	20823	18.403	ug/l	98
13) Acrolein	2.233	56	25369	79.103	ug/l	99
14) Allyl chloride	2.654	41	39210	19.468	ug/l	98
15) Acrylonitrile	3.062	53	75766	101.896	ug/l	100
16) Acetone	2.386	43	65266	96.039	ug/l	98
17) Carbon Disulfide	2.501	76	49556	16.444	ug/l	99
18) Methyl Acetate	2.703	43	37547	22.967	ug/l	99
19) Methyl tert-butyl Ether	3.117	73	73152	19.270	ug/l	100
20) Methylene Chloride	2.782	84	25802	19.167	ug/l	97
21) trans-1,2-Dichloroethene	3.081	96	21427	19.168	ug/l	93
22) Diisopropyl ether	3.757	45	79872	19.499	ug/l #	81
23) Vinyl Acetate	3.721	43	341251	99.830	ug/l	100
24) 1,1-Dichloroethane	3.605	63	43990	19.162	ug/l	97
25) 2-Butanone	4.556	43	105263	102.904	ug/l	98
26) 2,2-Dichloropropane	4.465	77	29182	27.101	ug/l	96
27) cis-1,2-Dichloroethene	4.483	96	26511	19.212	ug/l	96
28) Bromochloromethane	4.897	49	21801	19.924	ug/l	98
29) Tetrahydrofuran	5.007	42	67355	98.050	ug/l	99
30) Chloroform	5.086	83	44426	19.477	ug/l	98
31) Cyclohexane	5.458	56	37985	19.062	ug/l	98
32) 1,1,1-Trichloroethane	5.379	97	35413	19.223	ug/l	98
36) 1,1-Dichloropropene	5.684	75	28849	18.925	ug/l	99
37) Ethyl Acetate	4.714	43	36207	18.433	ug/l	98
38) Carbon Tetrachloride	5.672	117	29989	19.378	ug/l	94
39) Methylcyclohexane	7.373	83	36647	20.064	ug/l	97
40) Benzene	6.031	78	92458	19.208	ug/l	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045215.D
 Acq On : 11 Mar 2025 11:40
 Operator : JC/MD
 Sample : VX0311WBSD01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0311WBSD01

Quant Time: Mar 12 01:44:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :John Carlane 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
41) Methacrylonitrile	4.916	41	21766	20.493	ug/1	98
42) 1,2-Dichloroethane	6.086	62	34432	19.864	ug/1	100
43) Isopropyl Acetate	6.342	43	57873	19.925	ug/1	100
44) Trichloroethene	7.123	130	21499	19.021	ug/1	100
45) 1,2-Dichloropropane	7.427	63	23603	19.071	ug/1	93
46) Dibromomethane	7.580	93	17341	19.824	ug/1	99
47) Bromodichloromethane	7.818	83	33921	19.769	ug/1	99
48) Methyl methacrylate	7.696	41	29960	20.560	ug/1	98
49) 1,4-Dioxane	7.665	88	11450	372.504	ug/1	97
51) 4-Methyl-2-Pentanone	8.574	43	212449	108.934	ug/1	99
52) Toluene	8.714	92	56008	19.831	ug/1	99
53) t-1,3-Dichloropropene	8.976	75	28894	20.143	ug/1	100
54) cis-1,3-Dichloropropene	8.366	75	33564	20.066	ug/1	95
55) 1,1,2-Trichloroethane	9.153	97	23281	20.024	ug/1	99
56) Ethyl methacrylate	9.116	69	37256	21.080	ug/1	98
57) 1,3-Dichloropropane	9.305	76	41547	20.649	ug/1	99
58) 2-Chloroethyl Vinyl ether	8.238	63	84737	98.289	ug/1	99
59) 2-Hexanone	9.427	43	154662	109.453	ug/1	99
60) Dibromochloromethane	9.518	129	24209	19.914	ug/1	99
61) 1,2-Dibromoethane	9.610	107	23982	20.662	ug/1	98
64) Tetrachloroethene	9.269	164	18450	19.341	ug/1	94
65) Chlorobenzene	10.079	112	61875	19.633	ug/1	96
66) 1,1,1,2-Tetrachloroethane	10.159	131	19978	19.035	ug/1	97
67) Ethyl Benzene	10.189	91	108234	19.710	ug/1	98
68) m/p-Xylenes	10.299	106	80292	39.941	ug/1	97
69) o-Xylene	10.640	106	40924	20.185	ug/1	98
70) Styrene	10.652	104	67151	20.469	ug/1	99
71) Bromoform	10.799	173	16098	20.340	ug/1 #	99
73) Isopropylbenzene	10.957	105	104215	19.390	ug/1	99
74) N-amyl acetate	10.841	43	49701	19.707	ug/1	99
75) 1,1,2,2-Tetrachloroethane	11.213	83	38763	19.653	ug/1	100
76) 1,2,3-Trichloropropane	11.238	75	30828m	19.234	ug/1	
77) Bromobenzene	11.195	156	24637	19.428	ug/1	97
78) n-propylbenzene	11.305	91	121031	19.934	ug/1	99
79) 2-Chlorotoluene	11.360	91	74800	19.344	ug/1	99
80) 1,3,5-Trimethylbenzene	11.451	105	87336	20.096	ug/1	99
81) trans-1,4-Dichloro-2-b...	11.018	75	8951	19.112	ug/1	92
82) 4-Chlorotoluene	11.451	91	84411	20.030	ug/1	100
83) tert-Butylbenzene	11.713	119	86368	19.342	ug/1	99
84) 1,2,4-Trimethylbenzene	11.750	105	87556	20.023	ug/1	100
85) sec-Butylbenzene	11.890	105	109529	20.477	ug/1	99
86) p-Isopropyltoluene	12.006	119	88543	20.483	ug/1	99
87) 1,3-Dichlorobenzene	11.969	146	44375	19.615	ug/1	99
88) 1,4-Dichlorobenzene	12.042	146	43983	19.217	ug/1	98
89) n-Butylbenzene	12.329	91	76829	20.636	ug/1	99
90) Hexachloroethane	12.536	117	14287	18.273	ug/1	99
91) 1,2-Dichlorobenzene	12.335	146	44841	19.759	ug/1	99
92) 1,2-Dibromo-3-Chloropr...	12.945	75	7436	19.352	ug/1	98
93) 1,2,4-Trichlorobenzene	13.591	180	25138	19.453	ug/1	97
94) Hexachlorobutadiene	13.725	225	10532	19.880	ug/1	98
95) Naphthalene	13.774	128	95200	19.175	ug/1	100
96) 1,2,3-Trichlorobenzene	13.963	180	26292	19.287	ug/1	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
Data File : VX045215.D
Acq On : 11 Mar 2025 11:40
Operator : JC/MD
Sample : VX0311WBSD01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0311WBSD01

Manual Integrations
APPROVED

Reviewed By :John Carbone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

Quant Time: Mar 12 01:44:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 28 06:45:16 2025
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX031125\
 Data File : VX045215.D
 Acq On : 11 Mar 2025 11:40
 Operator : JC/MD
 Sample : VX0311WBSD01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1


Instrument :
 MSVOA_X
ClientSampleId :
 VX0311WBSD01

Quant Time: Mar 12 01:44:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X022825W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 28 06:45:16 2025
 Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :John Carlane 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

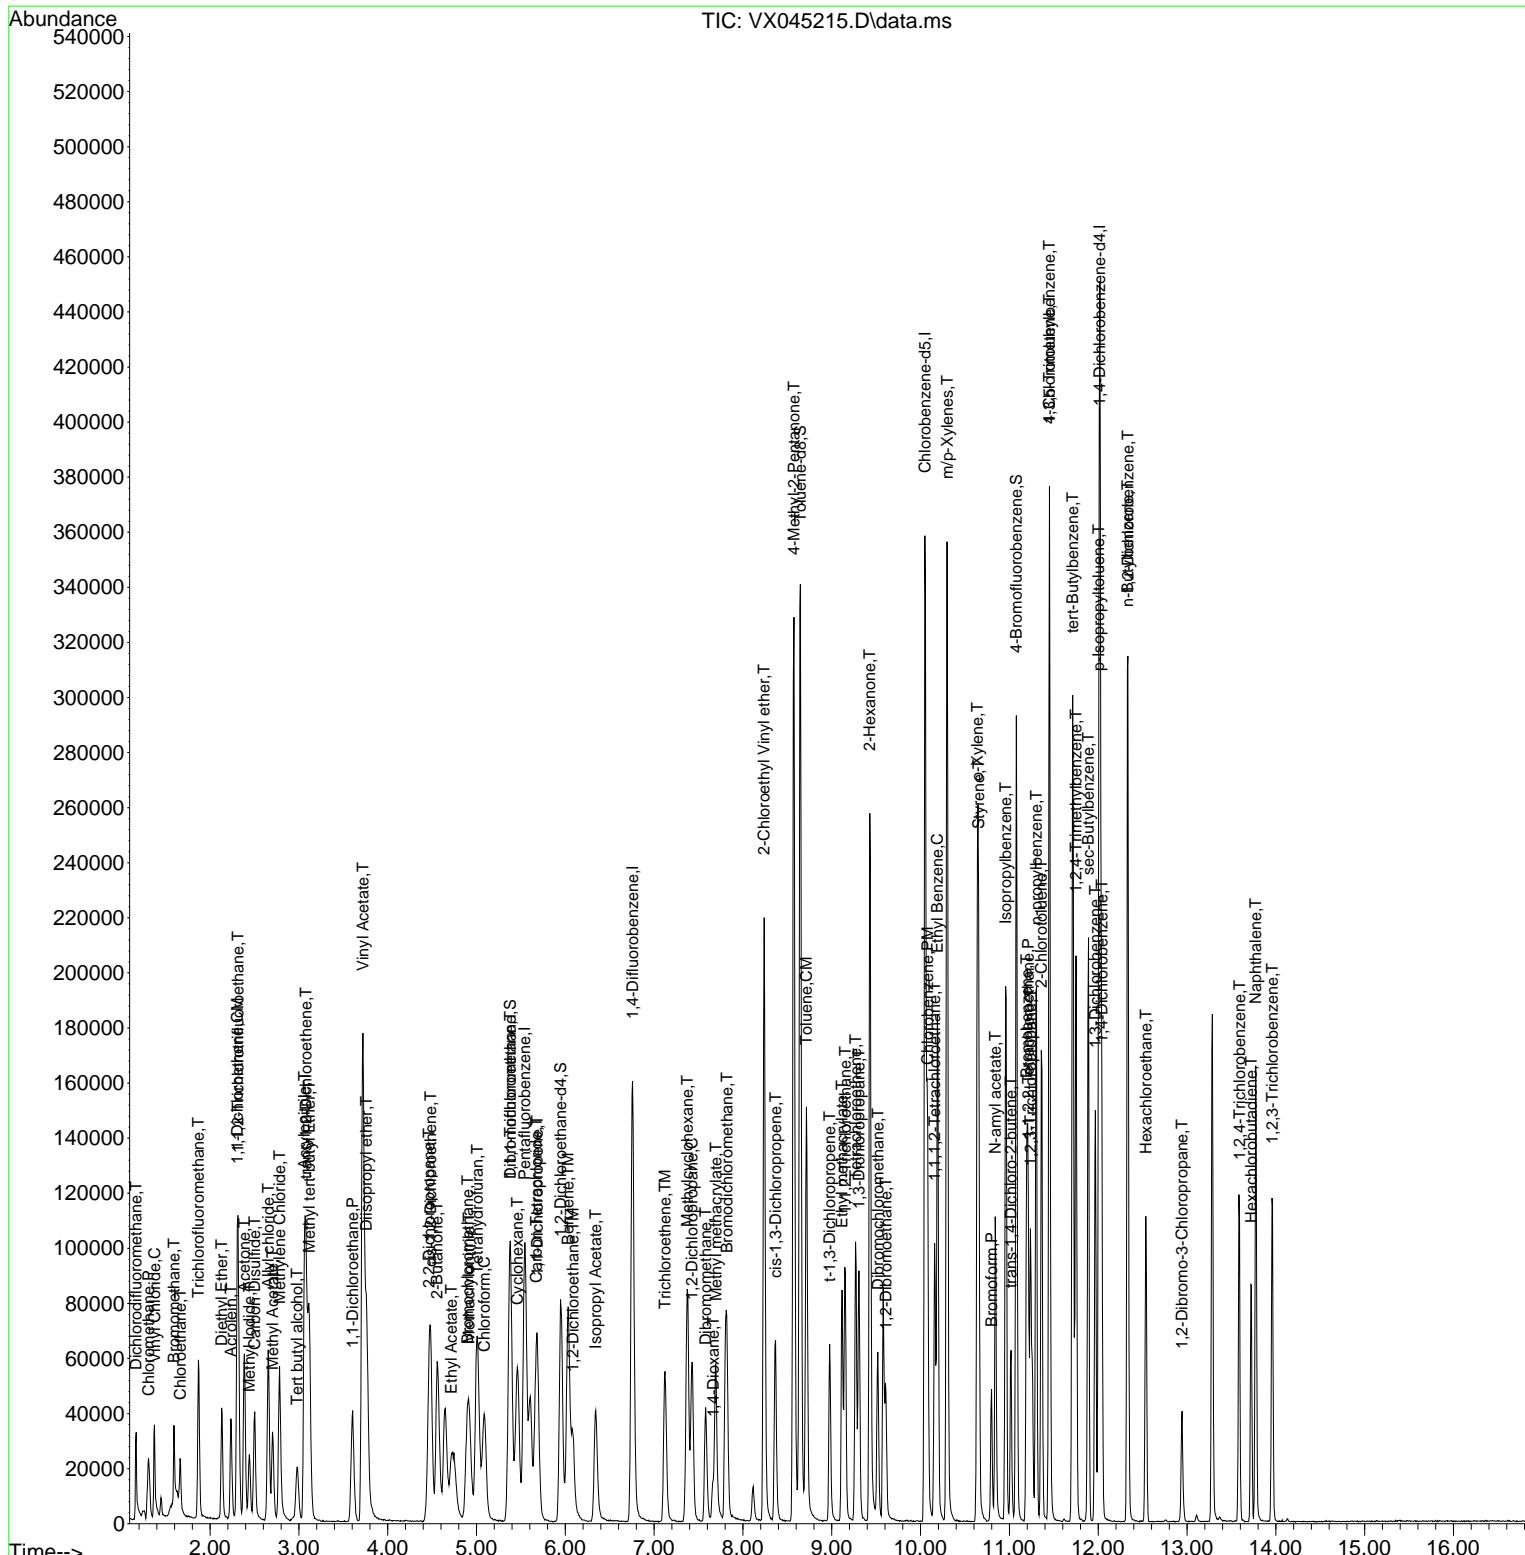



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 7
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt Ion:168 Resp: 9208
Ion Ratio Lower Upper
168 100
99 66.5 48.2 72.4




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

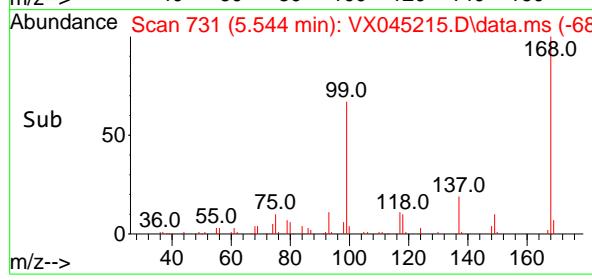

#2
Dichlorodifluoromethane
Concen: 19.355 ug/l
RT: 1.166 min Scan# 13
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion: 85 Resp: 22434
Ion Ratio Lower Upper
85 100
87 31.1 17.4 52.3

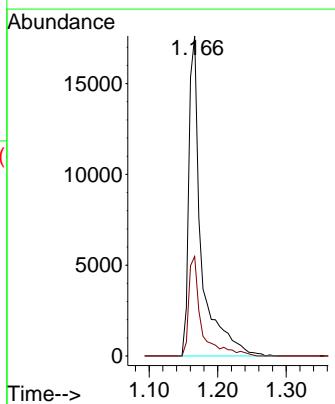



#3
Chloromethane
Concen: 17.909 ug/l
RT: 1.307 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt Ion: 50 Resp: 2540
Ion Ratio Lower Upper
50 100
52 32.3 25.0 37.4




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#4
Vinyl Chloride
Concen: 16.928 ug/l
RT: 1.374 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion: 62 Resp: 23820
Ion Ratio Lower Upper
62 100
64 33.4 24.3 36.5





#5
Bromomethane
Concen: 19.112 ug/l
RT: 1.593 min Scan# 8
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion: 94 Resp: 1057:
Ion Ratio Lower Upper
94 100
96 93.8 75.0 112.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#6
Chloroethane
Concen: 19.661 ug/l
RT: 1.666 min Scan# 95
Delta R.T. 0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

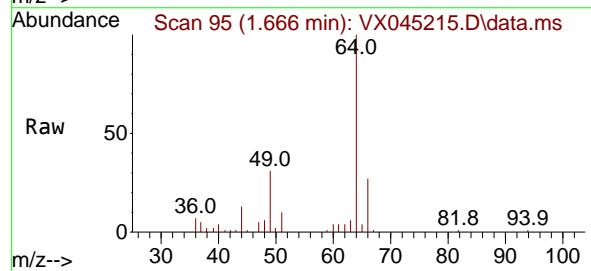


Tgt Ion: 64 Resp: 12761
Ion Ratio Lower Upper
64 100
66 26.8 26.7 40.1

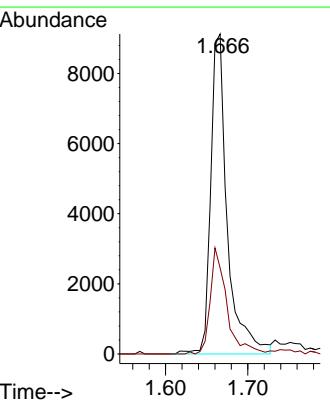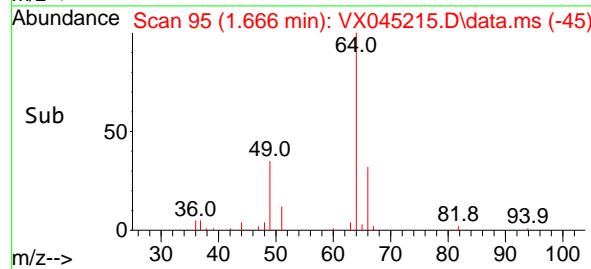



#7
Trichlorofluoromethane
Concen: 18.670 ug/l
RT: 1.867 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion:101 Resp: 34773
Ion Ratio Lower Upper
101 100
103 62.3 52.1 78.1

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

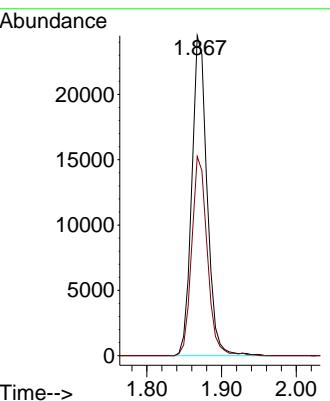


#8
Diethyl Ether
Concen: 17.718 ug/l
RT: 2.130 min Scan# 171
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion: 74 Resp: 12910
Ion Ratio Lower Upper
74 100
45 104.1 51.5 154.5

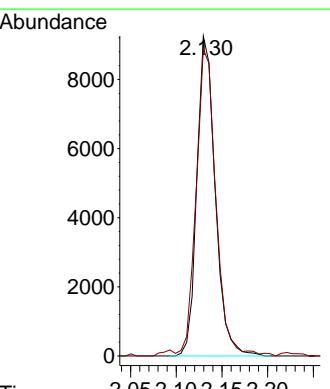






#9
1,1,2-Trichlorotrifluoroethane
Concen: 20.696 ug/l
RT: 2.312 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion:101 Resp: 22149
Ion Ratio Lower Upper
101 100
85 45.0 36.2 54.4
151 71.9 56.4 84.6

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#10
Methyl Iodide
Concen: 18.912 ug/l
RT: 2.440 min Scan# 222
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion:142 Resp: 25294
Ion Ratio Lower Upper
142 100
127 47.6 35.4 53.2
141 13.9 11.6 17.4





#11
Tert butyl alcohol
Concen: 84.116 ug/l
RT: 2.977 min Scan# 3
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt Ion: 59 Resp: 2333
Ion Ratio Lower Upper
59 100
57 9.9 7.8 11.8




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#12
1,1-Dichloroethene
Concen: 18.403 ug/l
RT: 2.306 min Scan# 200
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion: 96 Resp: 20823
Ion Ratio Lower Upper
96 100
61 172.1 134.6 202.0
98 64.4 51.0 76.6

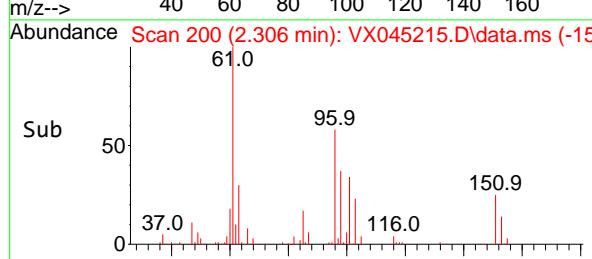



#13
Acrolein
Concen: 79.103 ug/l
RT: 2.233 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion: 56 Resp: 25369
Ion Ratio Lower Upper
56 100
55 71.3 56.2 84.4

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

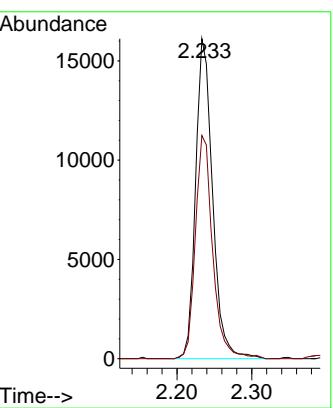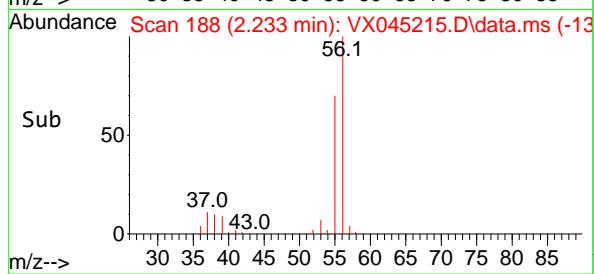


#14
Allyl chloride
Concen: 19.468 ug/l
RT: 2.654 min Scan# 257
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion: 41 Resp: 39210
Ion Ratio Lower Upper
41 100
39 68.5 53.8 80.8
76 32.6 25.2 37.8

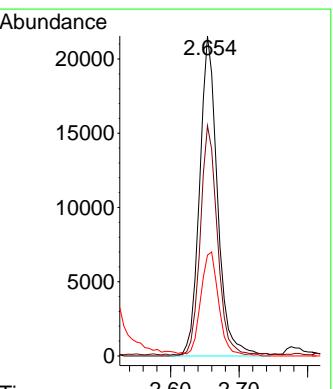



#15
Acrylonitrile
Concen: 101.896 ug/l
RT: 3.062 min Scan# 31
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40



Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion: 53 Resp: 75760
Ion Ratio Lower Upper
53 100
52 82.4 66.2 99.2
51 36.4 29.0 43.4

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#16
Acetone
Concen: 96.039 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

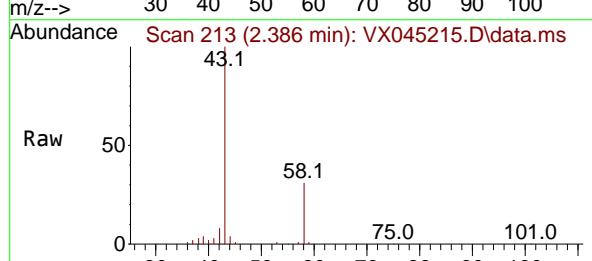


Tgt Ion: 43 Resp: 65266
Ion Ratio Lower Upper
43 100
58 31.4 24.2 36.4





#17
Carbon Disulfide
Concen: 16.444 ug/l
RT: 2.501 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40



Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01

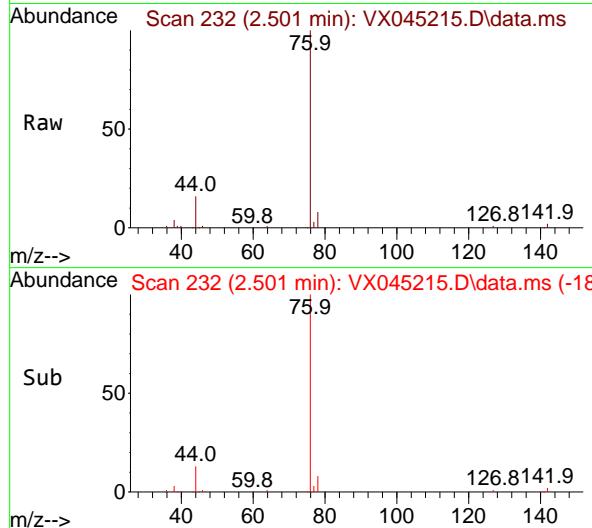

Tgt Ion: 76 Resp: 49550
Ion Ratio Lower Upper
76 100
78 8.4 6.6 9.8


Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

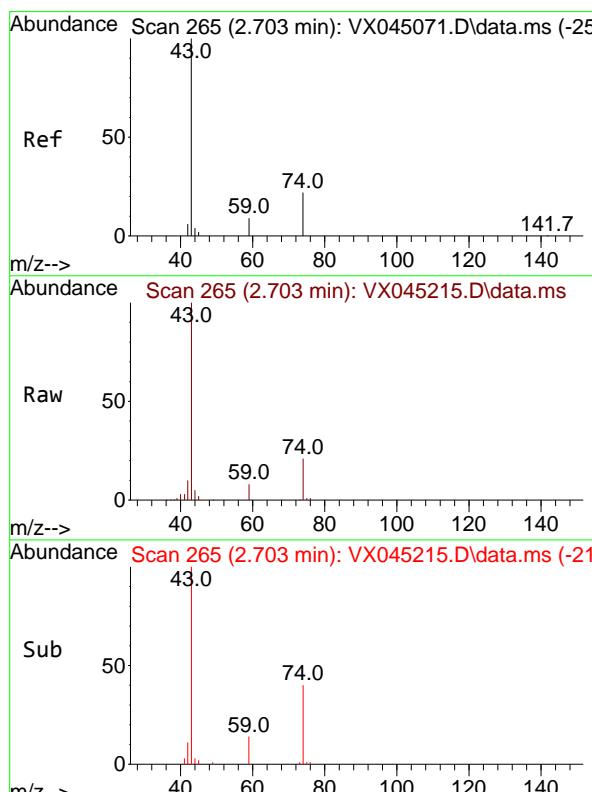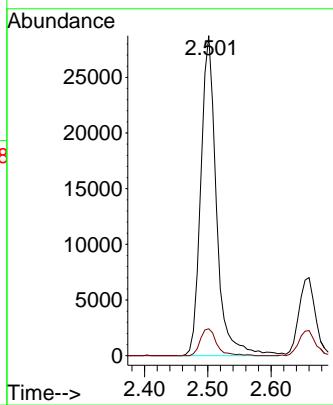

#18
Methyl Acetate
Concen: 22.967 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion: 43 Resp: 37547
Ion Ratio Lower Upper
43 100
74 21.3 17.4 26.2

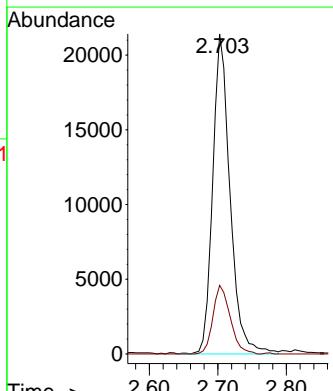



#19
Methyl tert-butyl Ether
Concen: 19.270 ug/l
RT: 3.117 min Scan# 3
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01

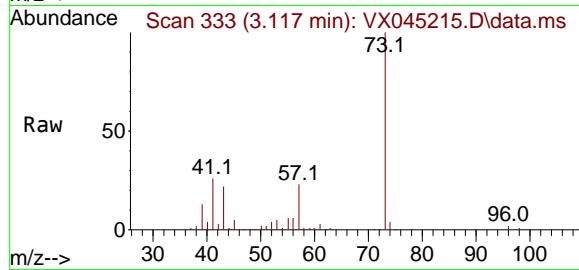


Tgt Ion: 73 Resp: 7315
Ion Ratio Lower Upper
73 100
57 23.3 18.5 27.7

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

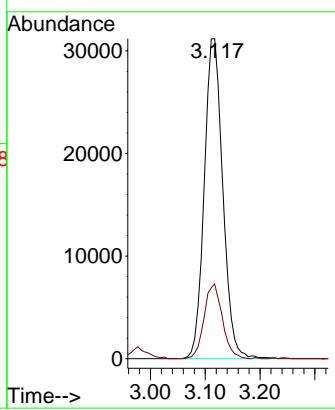


#20
Methylene Chloride
Concen: 19.167 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion: 84 Resp: 25802
Ion Ratio Lower Upper
84 100
49 128.8 106.5 159.7
51 37.7 32.1 48.1
86 60.3 50.0 75.0

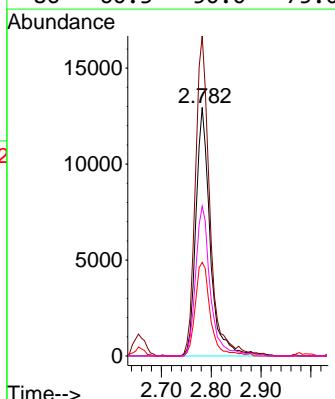



#21
trans-1,2-Dichloroethene
Concen: 19.168 ug/l
RT: 3.081 min Scan# 31
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40



Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt Ion: 96 Resp: 2142
Ion Ratio Lower Upper
96 100
61 137.3 117.0 175.4
98 62.7 53.4 80.2



Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#22
Diisopropyl ether
Concen: 19.499 ug/l
RT: 3.757 min Scan# 438
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

Tgt Ion: 45 Resp: 79872
Ion Ratio Lower Upper
45 100
43 91.5 54.9 82.3#
87 24.5 21.0 31.4
59 9.9 8.7 13.1

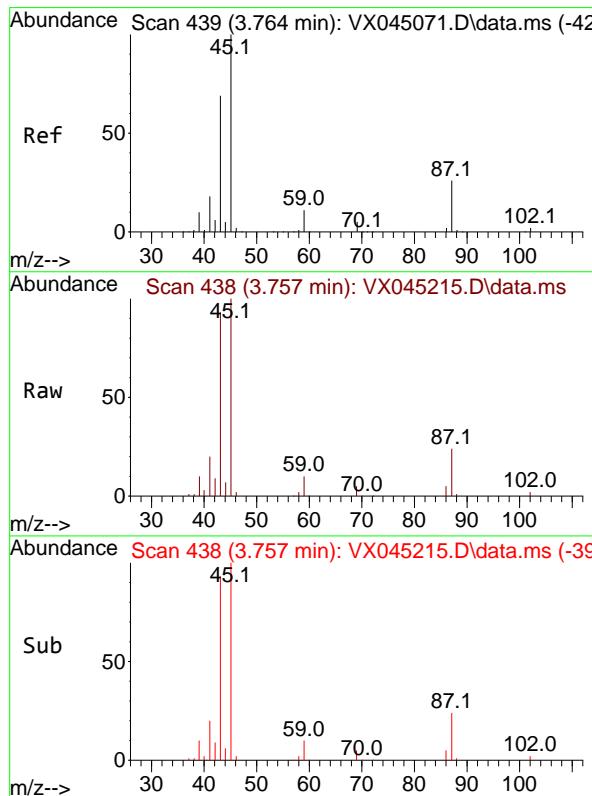



#23

Vinyl Acetate

Concen: 99.830 ug/l

RT: 3.721 min Scan# 4125

Delta R.T. -0.000 min

Lab File: VX045215.D


Acq: 11 Mar 2025 11:40

Instrument:

MSVOA_X

ClientSampleId :

VX0311WBSD01





Tgt Ion: 43 Resp: 34125

Ion Ratio Lower Upper

43 100

86 10.0 8.1 12.1

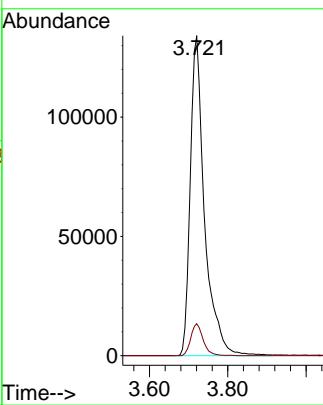**Manual Integrations
APPROVED**
Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

#24

1,1-Dichloroethane


Concen: 19.162 ug/l

RT: 3.605 min Scan# 413

Delta R.T. -0.000 min

Lab File: VX045215.D

Acq: 11 Mar 2025 11:40




Tgt Ion: 63 Resp: 43990


Ion Ratio Lower Upper

63 100


98 7.8 3.4 10.2

100 5.5 2.1 6.5

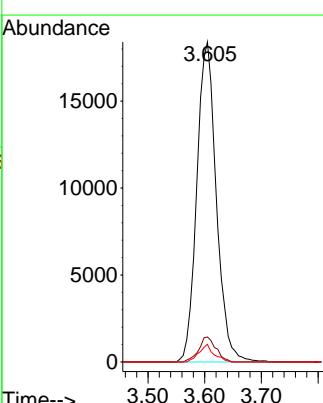

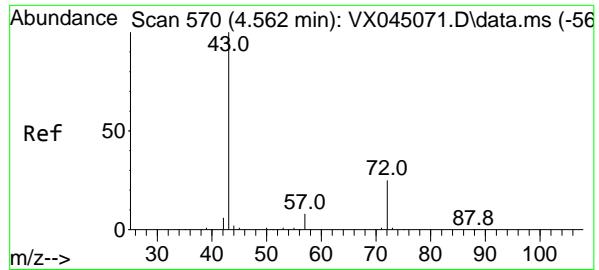




#25
2-Butanone
Concen: 102.904 ug/l
RT: 4.556 min Scan# 5
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

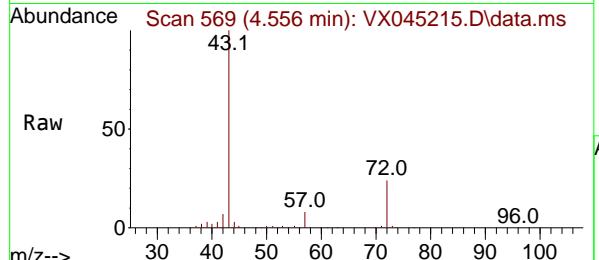


Tgt Ion: 43 Resp: 10526
Ion Ratio Lower Upper
43 100
72 24.2 20.0 30.0

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

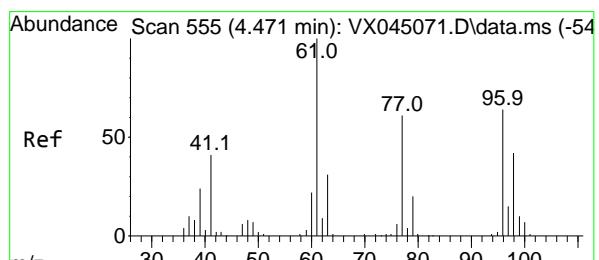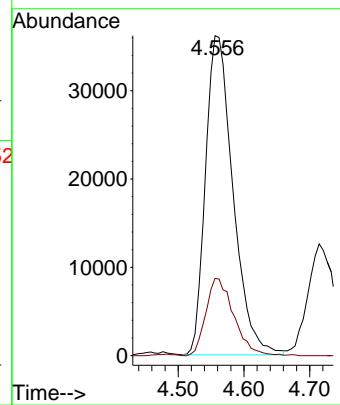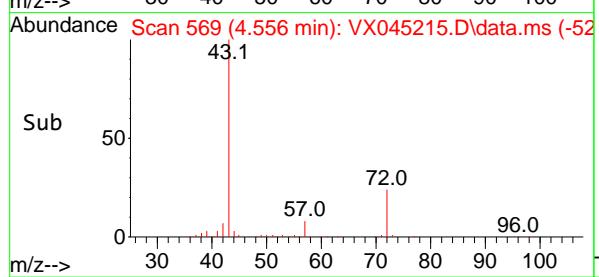


#26
2,2-Dichloropropane
Concen: 27.101 ug/l
RT: 4.465 min Scan# 554
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

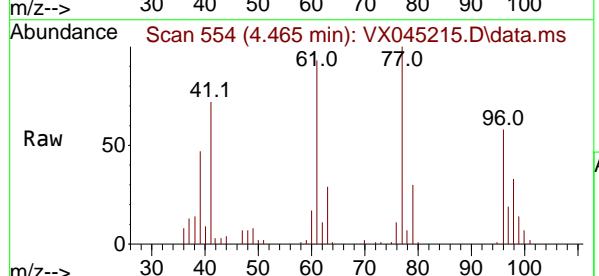


Tgt Ion: 77 Resp: 29182
Ion Ratio Lower Upper
77 100
97 22.8 12.4 37.0

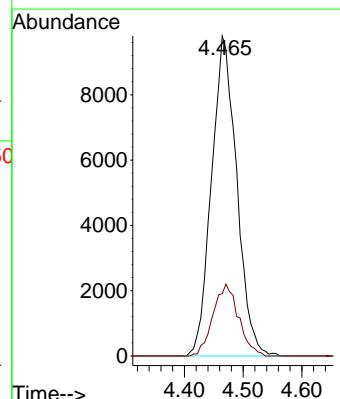

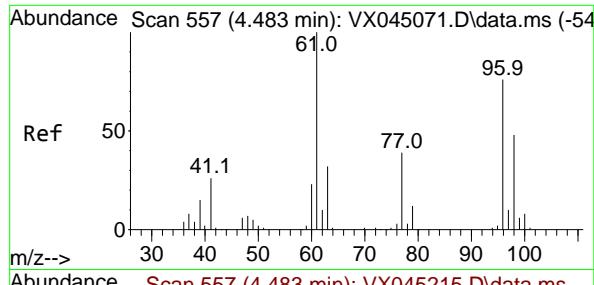



#27
cis-1,2-Dichloroethene
 Concen: 19.212 ug/l
 RT: 4.483 min Scan# 5
 Delta R.T. -0.000 min
 Lab File: VX045215.D
 Acq: 11 Mar 2025 11:40

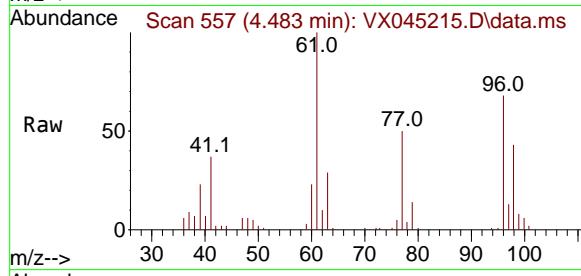


Tgt Ion: 96 Resp: 2651
 Ion Ratio Lower Upper
 96 100
 61 148.6 0.0 283.2
 98 63.4 0.0 128.0

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

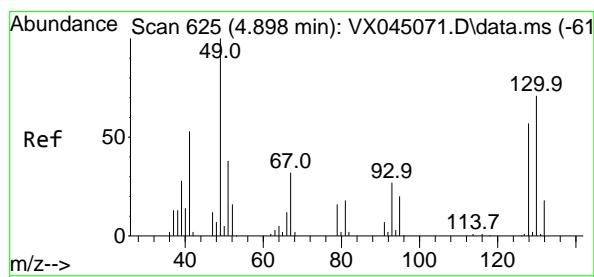


#28
 Bromochloromethane
 Concen: 19.924 ug/l
 RT: 4.897 min Scan# 625
 Delta R.T. -0.000 min
 Lab File: VX045215.D
 Acq: 11 Mar 2025 11:40

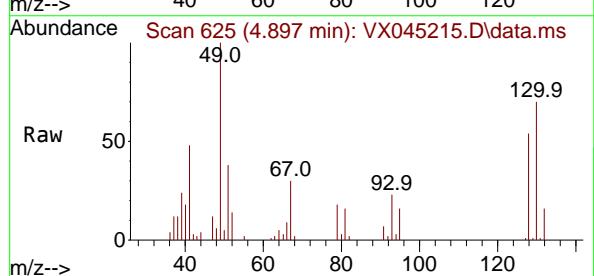

Tgt Ion: 49 Resp: 21801
 Ion Ratio Lower Upper
 49 100
 129 1.4 0.0 3.4
 130 71.4 56.1 84.1





#29

Tetrahydrofuran

Concen: 98.050 ug/l

RT: 5.007 min Scan# 6

Delta R.T. -0.000 min

Lab File: VX045215.D


Acq: 11 Mar 2025 11:40

Instrument :

MSVOA_X

ClientSampleId :


VX0311WBSD01

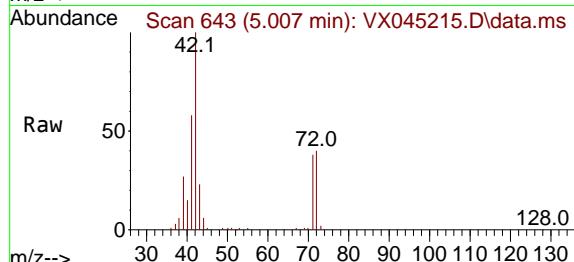

Tgt	Ion:	42	Ion Ratio	100	Resp:	6735
			Lower		Upper	
		42	100			
		72	43.1	34.1	51.1	
		71	38.5	31.4	47.0	


Manual Integrations APPROVED

Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

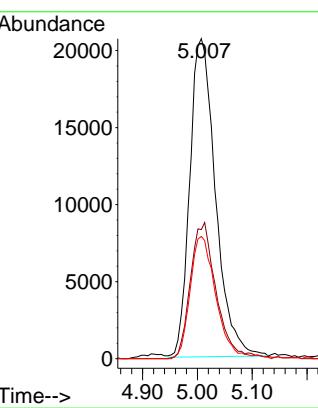


Time-->

5.007

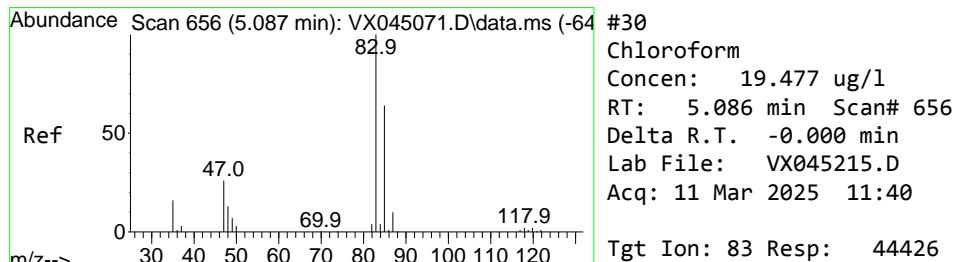
#30
Chloroform
Concen: 19.477 ug/l
RT: 5.086 min Scan# 656
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

Tgt	Ion:	83	Ion Ratio	100	Resp:	44426
			Lower		Upper	
		83	100			
		85	63.1	51.4	77.2	

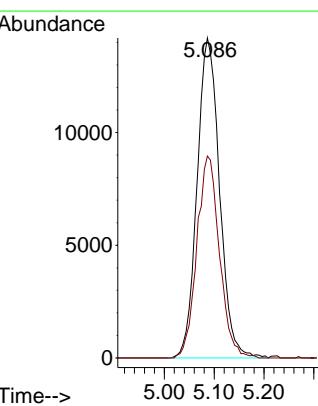


Time-->

5.086



#31
Cyclohexane
Concen: 19.062 ug/l
RT: 5.458 min Scan# 7
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt Ion: 56 Resp: 37989
Ion Ratio Lower Upper
56 100
69 27.9 23.4 35.2
84 88.9 69.4 104.2




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#32
1,1,1-Trichloroethane
Concen: 19.223 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion: 97 Resp: 35413
Ion Ratio Lower Upper
97 100
99 63.7 51.6 77.4
61 49.7 38.4 57.6





#33
1,2-Dichloroethane-d4
Concen: 51.107 ug/l
RT: 5.946 min Scan# 7
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40



Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion: 65 Resp: 74850
Ion Ratio Lower Upper
65 100
67 52.0 0.0 106.2

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

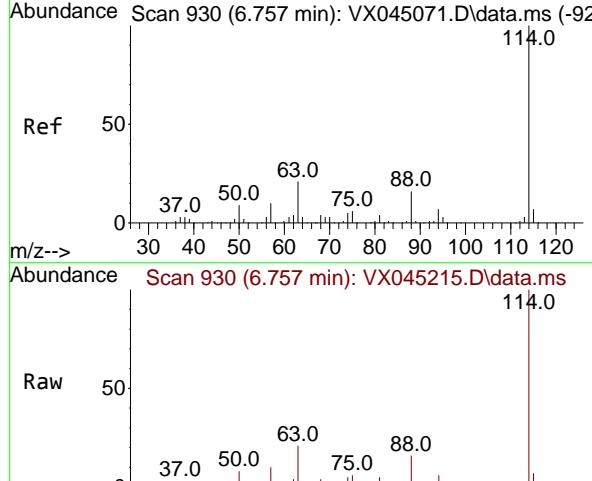


Tgt Ion:114 Resp: 166231
Ion Ratio Lower Upper
114 100
63 21.2 0.0 41.8
88 15.8 0.0 32.8

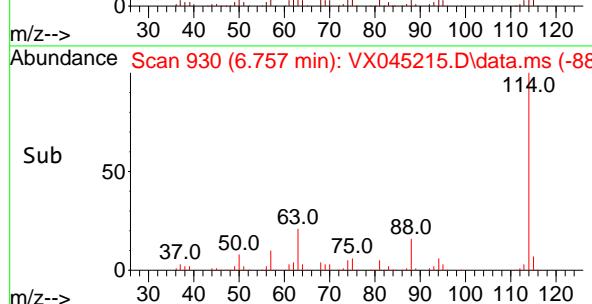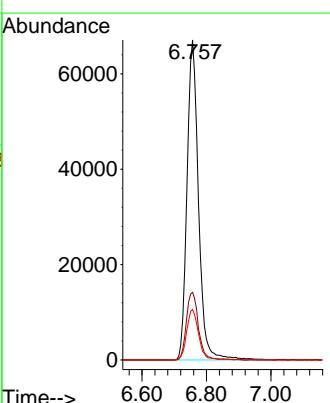



#35
Dibromofluoromethane
Concen: 50.961 ug/l
RT: 5.379 min Scan# 7
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01

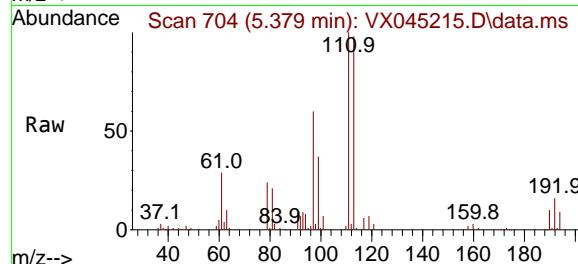


Tgt Ion:113 Resp: 5664
Ion Ratio Lower Upper
113 100
111 103.1 81.8 122.6
192 17.5 14.3 21.5

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#36
1,1-Dichloropropene
Concen: 18.925 ug/l
RT: 5.684 min Scan# 754
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion: 75 Resp: 28849
Ion Ratio Lower Upper
75 100
110 33.4 16.9 50.6
77 31.4 24.5 36.7








#37
Ethyl Acetate
 Concen: 18.433 ug/l
 RT: 4.714 min Scan# 595
 Delta R.T. -0.000 min
 Lab File: VX045215.D
 Acq: 11 Mar 2025 11:40




Tgt Ion: 43 Resp: 3620
 Ion Ratio Lower Upper
 43 100
 61 14.4 10.8 16.2
 70 10.2 7.7 11.5

Manual Integrations APPROVED



Reviewed By :John Carbone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025




#38
Carbon Tetrachloride
 Concen: 19.378 ug/l
 RT: 5.672 min Scan# 752
 Delta R.T. -0.000 min
 Lab File: VX045215.D
 Acq: 11 Mar 2025 11:40



Tgt Ion:117 Resp: 29989
 Ion Ratio Lower Upper
 117 100
 119 89.4 76.7 115.1
 121 28.9 25.5 38.3





#39

Methylcyclohexane

Concen: 20.064 ug/l

RT: 7.373 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045215.D


Acq: 11 Mar 2025 11:40

Instrument :

MSVOA_X

ClientSampleId :



VX0311WBSD01




Tgt Ion:	83	Ion Ratio	100	Resp:	3664
	55	82.0	63.0	Lower	94.4
	98	48.1	39.7	Upper	59.5

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#40
Benzene
Concen: 19.208 ug/l
RT: 6.031 min Scan# 811
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

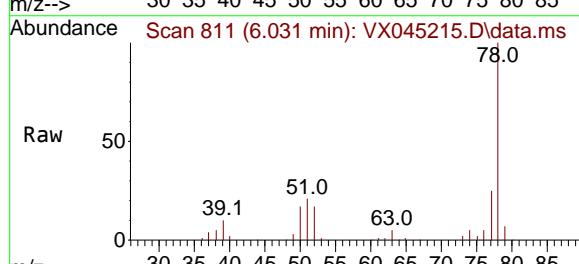


Tgt Ion:	78	Ion Ratio	100	Resp:	92458
	77	25.3	18.8	Lower	28.2

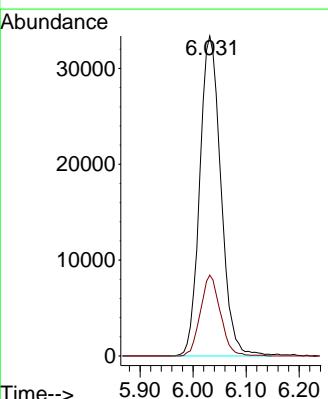



#41
Methacrylonitrile
Concen: 20.493 ug/l
RT: 4.916 min Scan# 61
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt Ion: 41 Resp: 21760
Ion Ratio Lower Upper
41 100
39 57.7 44.6 67.0
67 68.5 53.9 80.9
52 30.3 23.3 34.9




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

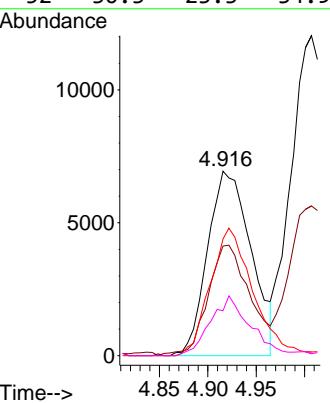

#42
1,2-Dichloroethane
Concen: 19.864 ug/l
RT: 6.086 min Scan# 820
Delta R.T. 0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion: 62 Resp: 34432
Ion Ratio Lower Upper
62 100
98 9.2 0.0 18.2

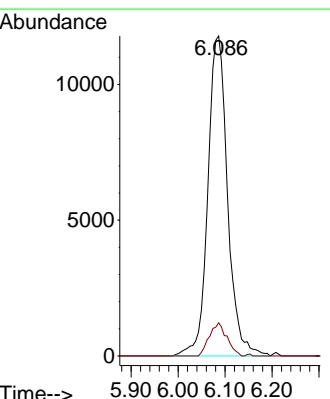



#43
Isopropyl Acetate
Concen: 19.925 ug/l
RT: 6.342 min Scan# 8
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01

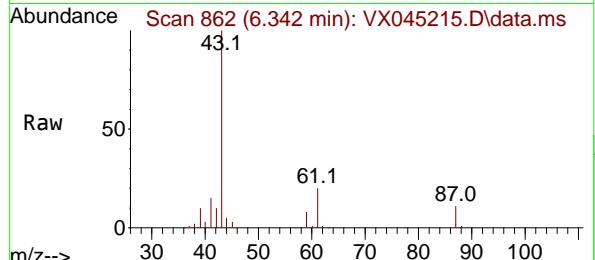


Tgt Ion: 43 Resp: 5787
Ion Ratio Lower Upper
43 100
61 18.4 14.9 22.3
87 11.9 9.4 14.2

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

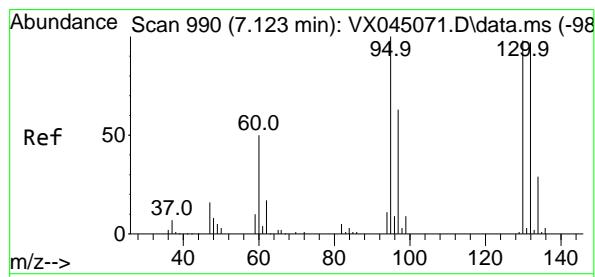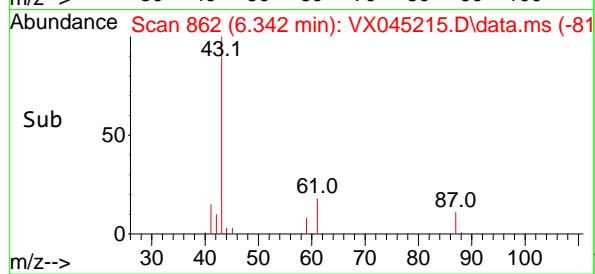


#44
Trichloroethene
Concen: 19.021 ug/l
RT: 7.123 min Scan# 990
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

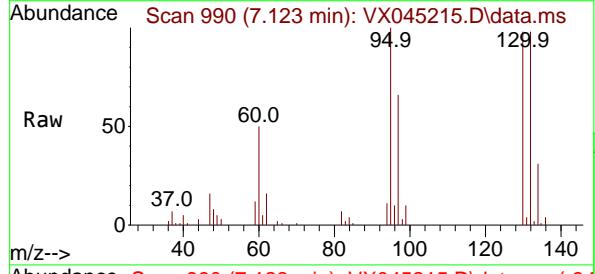


Tgt Ion:130 Resp: 21499
Ion Ratio Lower Upper
130 100
95 102.4 0.0 205.0

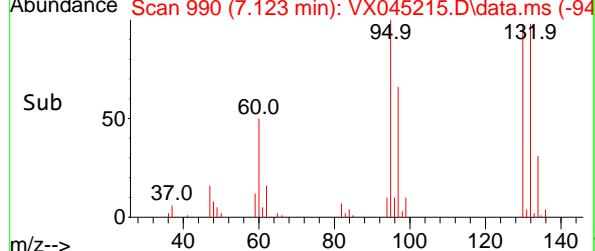



#45
1,2-Dichloropropane
Concen: 19.071 ug/l
RT: 7.427 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt Ion: 63 Resp: 2360
Ion Ratio Lower Upper
63 100
65 26.8 24.7 37.1




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#46
Dibromomethane
Concen: 19.824 ug/l
RT: 7.580 min Scan# 1065
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion: 93 Resp: 17341
Ion Ratio Lower Upper
93 100
95 83.6 65.8 98.8
174 89.0 72.2 108.2





#47
 Bromodichloromethane
 Concen: 19.769 ug/l
 RT: 7.818 min Scan# 1104
 Delta R.T. -0.000 min
 Lab File: VX045215.D
 Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
 ClientSampleId : VX0311WBSD01

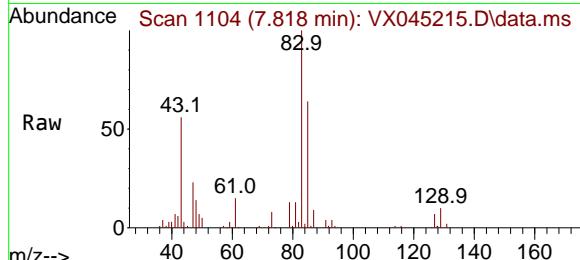


Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
83	100	3392		
85	64.1		51.1	76.7
127	6.8		6.4	9.6

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

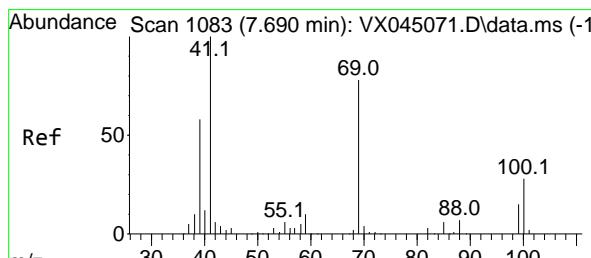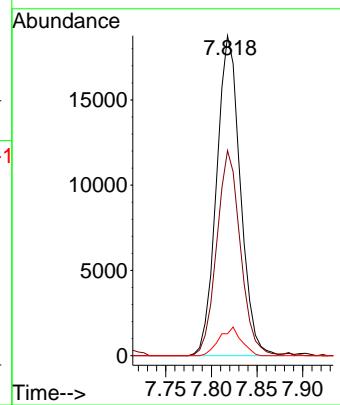


#48
 Methyl methacrylate
 Concen: 20.560 ug/l
 RT: 7.696 min Scan# 1084
 Delta R.T. 0.006 min
 Lab File: VX045215.D
 Acq: 11 Mar 2025 11:40




Tgt Ion:	Ion Ratio	Resp:	Lower	Upper
41	100	29960		
69	76.1		63.0	94.6
39	60.6		47.5	71.3

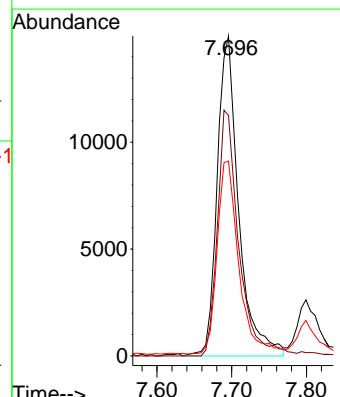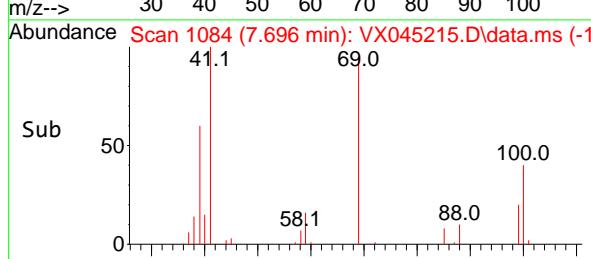



#49
1,4-Dioxane
Concen: 372.504 ug/l
RT: 7.665 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01

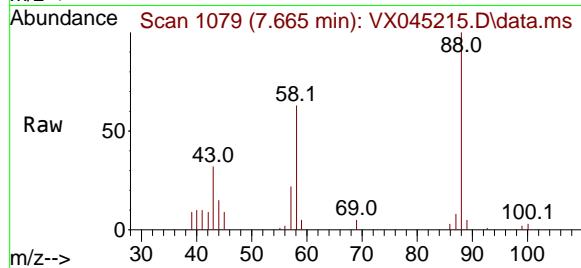


Tgt Ion: 88 Resp: 11450
Ion Ratio Lower Upper
88 100
43 39.7 28.7 43.1
58 69.0 55.8 83.8

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

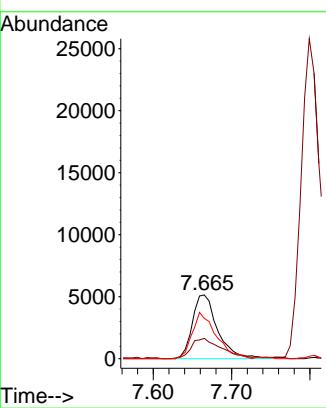


#50
Toluene-d8
Concen: 50.659 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion: 98 Resp: 204141
Ion Ratio Lower Upper
98 100
100 65.3 52.0 78.0

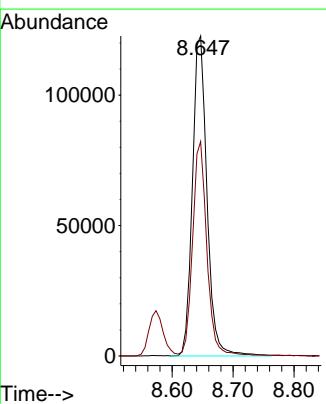



#51
4-Methyl-2-Pentanone
Concen: 108.934 ug/l
RT: 8.574 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion: 43 Resp: 212449
Ion Ratio Lower Upper
43 100
58 36.1 29.2 43.8

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

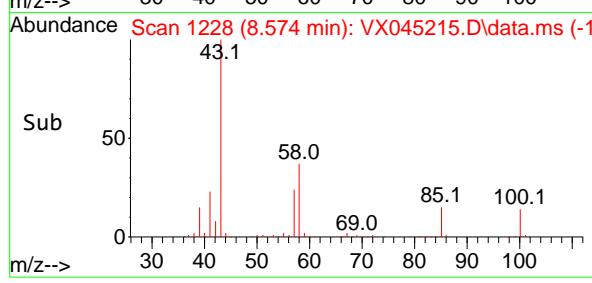


#52
Toluene
Concen: 19.831 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion: 92 Resp: 56008
Ion Ratio Lower Upper
92 100
91 174.5 138.9 208.3

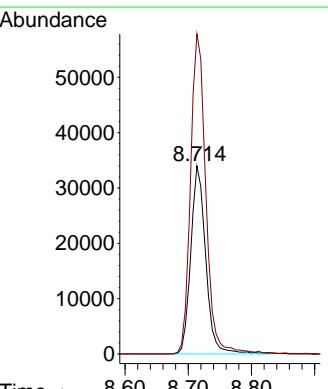

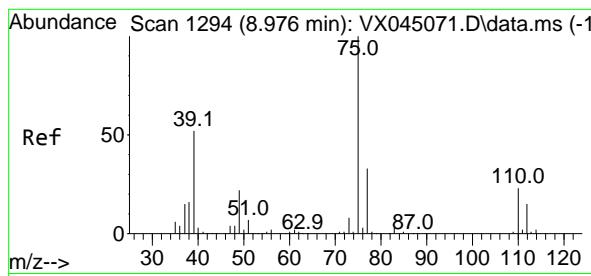

#53
t-1,3-Dichloropropene
Concen: 20.143 ug/l
RT: 8.976 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion: 75 Resp: 28894
Ion Ratio Lower Upper
75 100
77 33.0 26.5 39.7

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#54
cis-1,3-Dichloropropene
Concen: 20.066 ug/l
RT: 8.366 min Scan# 1194
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion: 75 Resp: 33564
Ion Ratio Lower Upper
75 100
77 30.8 24.7 37.1
39 56.0 40.7 61.1





#55
1,1,2-Trichloroethane
Concen: 20.024 ug/l
RT: 9.153 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion: 97 Resp: 2328
Ion Ratio Lower Upper
97 100
83 87.1 69.4 104.2
85 56.5 44.1 66.1
99 64.0 50.7 76.1

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#56
Ethyl methacrylate
Concen: 21.080 ug/l
RT: 9.116 min Scan# 1317
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion: 69 Resp: 37256
Ion Ratio Lower Upper
69 100
41 73.2 57.0 85.4
39 43.5 34.2 51.4





#57
1,3-Dichloropropane
Concen: 20.649 ug/l
RT: 9.305 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt Ion: 76 Resp: 4154
Ion Ratio Lower Upper
76 100
78 31.6 25.5 38.3




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#58
2-Chloroethyl Vinyl ether
Concen: 98.289 ug/l
RT: 8.238 min Scan# 1173
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion: 63 Resp: 84737
Ion Ratio Lower Upper
63 100
106 26.2 21.5 32.3





#59
2-Hexanone
Concen: 109.453 ug/l
RT: 9.427 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt Ion: 43 Resp: 15466
Ion Ratio Lower Upper
43 100
58 51.2 25.9 77.6




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

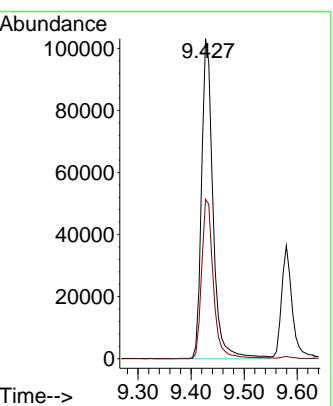

#60
Dibromochloromethane
Concen: 19.914 ug/l
RT: 9.518 min Scan# 1383
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion:129 Resp: 24209
Ion Ratio Lower Upper
129 100
127 78.0 38.5 115.5

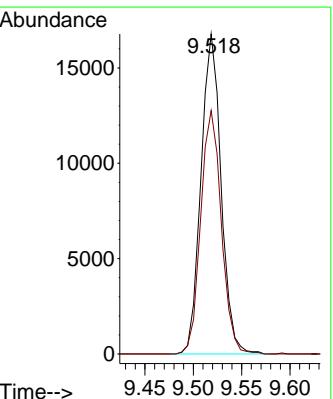



#61
1,2-Dibromoethane
Concen: 20.662 ug/l
RT: 9.610 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt Ion:107 Resp: 2398:
Ion Ratio Lower Upper
107 100
109 93.5 76.1 114.1



Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

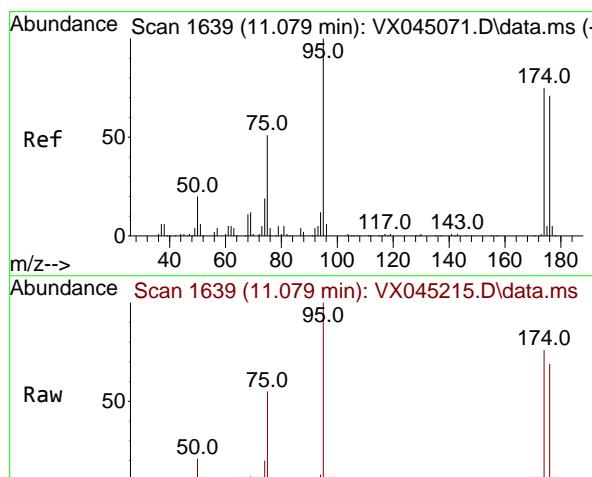

#62
4-Bromofluorobenzene
Concen: 54.440 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

Tgt Ion: 95 Resp: 72695
Ion Ratio Lower Upper
95 100
174 75.0 0.0 148.2
176 70.5 0.0 141.4

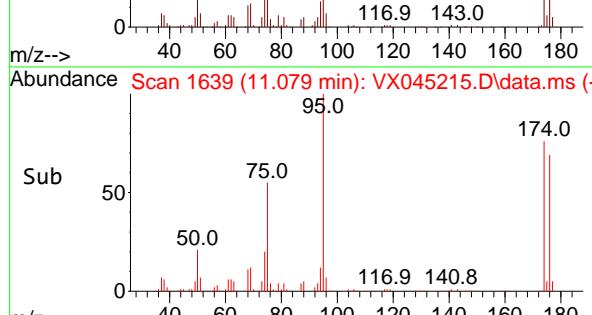

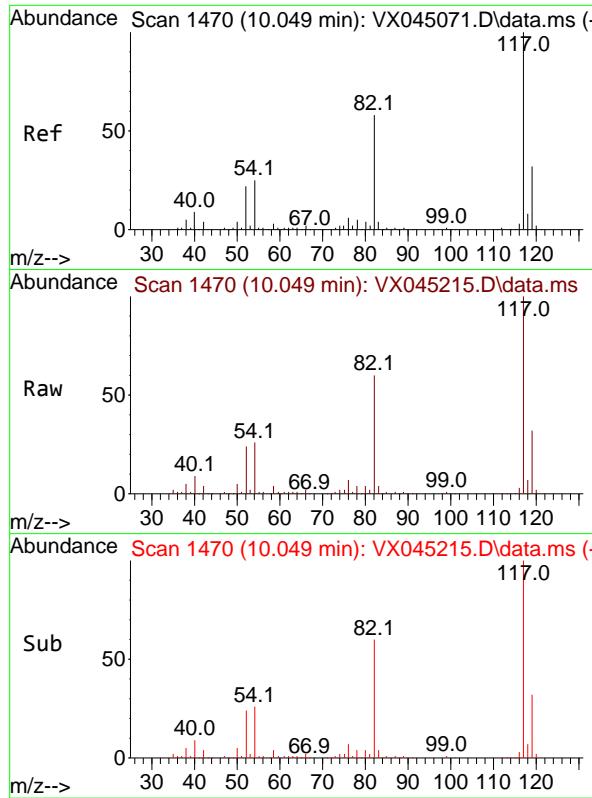



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01

Tgt Ion:117 Resp: 14894
Ion Ratio Lower Upper
117 100
82 60.3 46.3 69.5
119 31.9 25.7 38.5


Manual Integrations APPROVED


Reviewed By :John Carbone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

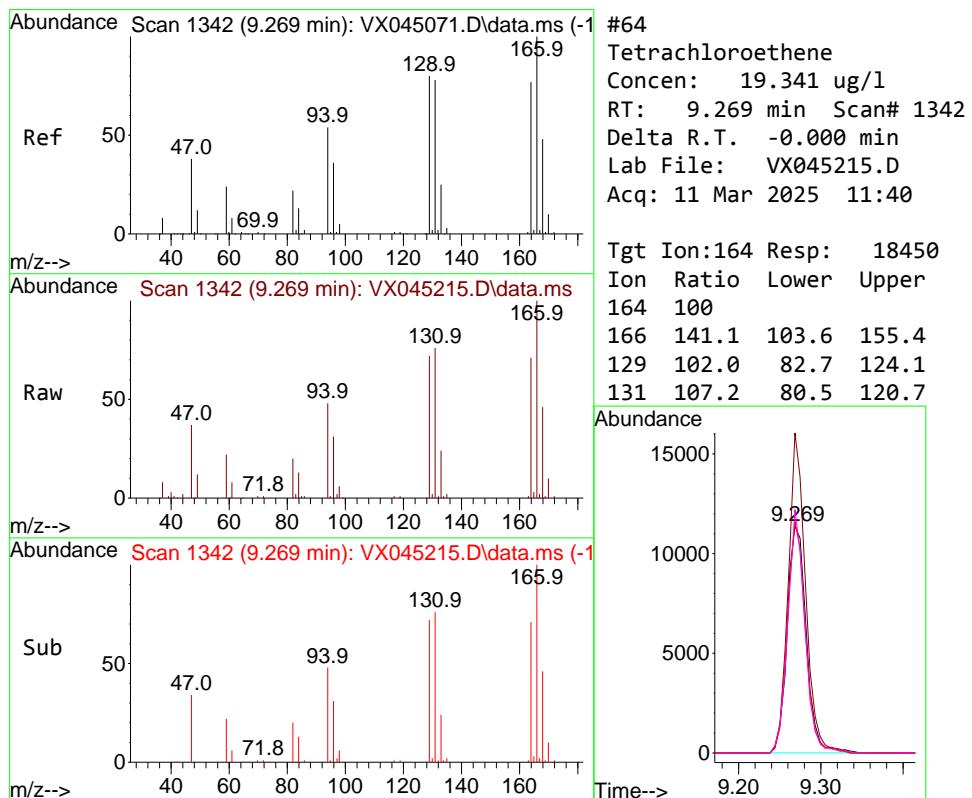

#64
Tetrachloroethene
Concen: 19.341 ug/l
RT: 9.269 min Scan# 1342
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion:164 Resp: 18450
Ion Ratio Lower Upper
164 100
166 141.1 103.6 155.4
129 102.0 82.7 124.1
131 107.2 80.5 120.7

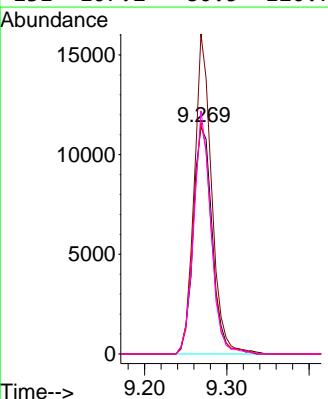



#65
Chlorobenzene
Concen: 19.633 ug/l
RT: 10.079 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt Ion:112 Resp: 6187
Ion Ratio Lower Upper
112 100
114 30.3 26.0 39.0




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#66
1,1,1,2-Tetrachloroethane
Concen: 19.035 ug/l
RT: 10.159 min Scan# 1488
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion:131 Resp: 19978
Ion Ratio Lower Upper
131 100
133 92.8 48.6 145.9
119 67.9 33.9 101.7

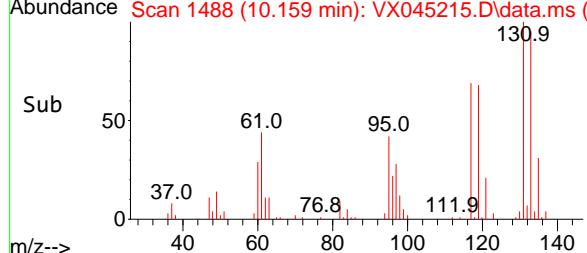



#67
Ethyl Benzene
Concen: 19.710 ug/l
RT: 10.189 min Scan# 1493
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt Ion: 91 Resp: 108234
Ion Ratio Lower Upper
91 100
106 29.1 23.9 35.9




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#68
m/p-Xylenes
Concen: 39.941 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion: 106 Resp: 80292
Ion Ratio Lower Upper
106 100
91 211.5 165.4 248.0





#69
o-Xylene
Concen: 20.185 ug/l
RT: 10.640 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument :
MSVOA_X
ClientSampleId :
VX0311WBSD01




Tgt Ion:106 Resp: 4092
Ion Ratio Lower Upper
106 100
91 215.9 109.9 329.6

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

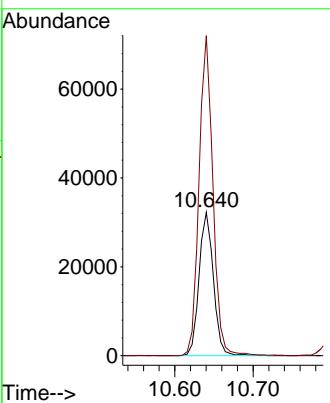


#70
Styrene
Concen: 20.469 ug/l
RT: 10.652 min Scan# 1569
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion:104 Resp: 67151
Ion Ratio Lower Upper
104 100
78 53.5 42.2 63.4
103 56.2 43.8 65.8

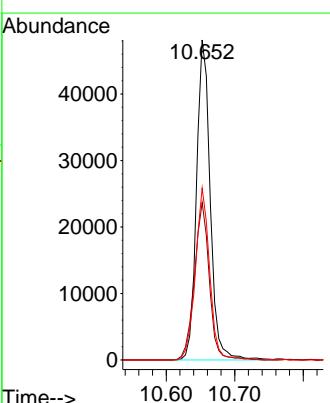



#71
Bromoform
Concen: 20.340 ug/l
RT: 10.799 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01



Tgt	Ion:173	Resp:	16093
	Ion Ratio	Lower	Upper
173	100		
175	48.8	24.6	73.6
254	0.0	0.0	0.0




Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

Tgt	Ion:152	Resp:	68861
	Ion Ratio	Lower	Upper
152	100		
115	73.8	44.2	132.6
150	161.8	0.0	349.0




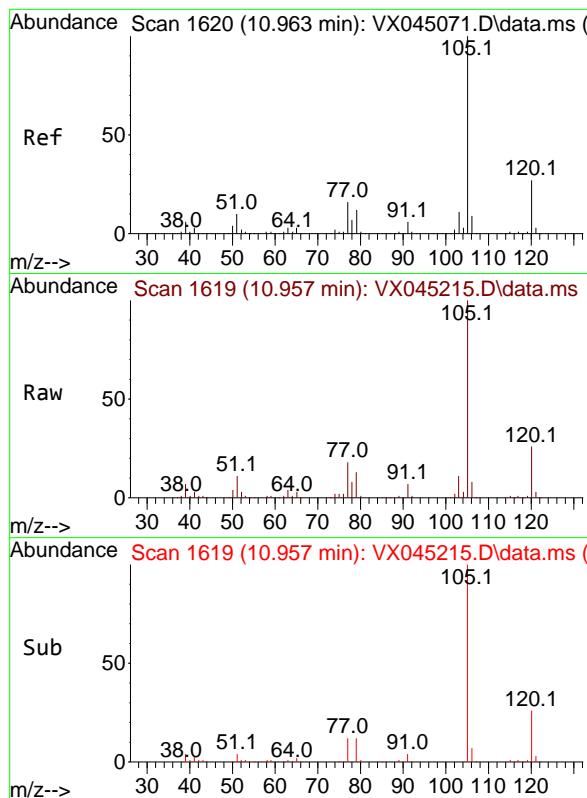


#73
Isopropylbenzene
Concen: 19.390 ug/l
RT: 10.957 min Scan# 1
Delta R.T. -0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01


Manual Integrations
APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

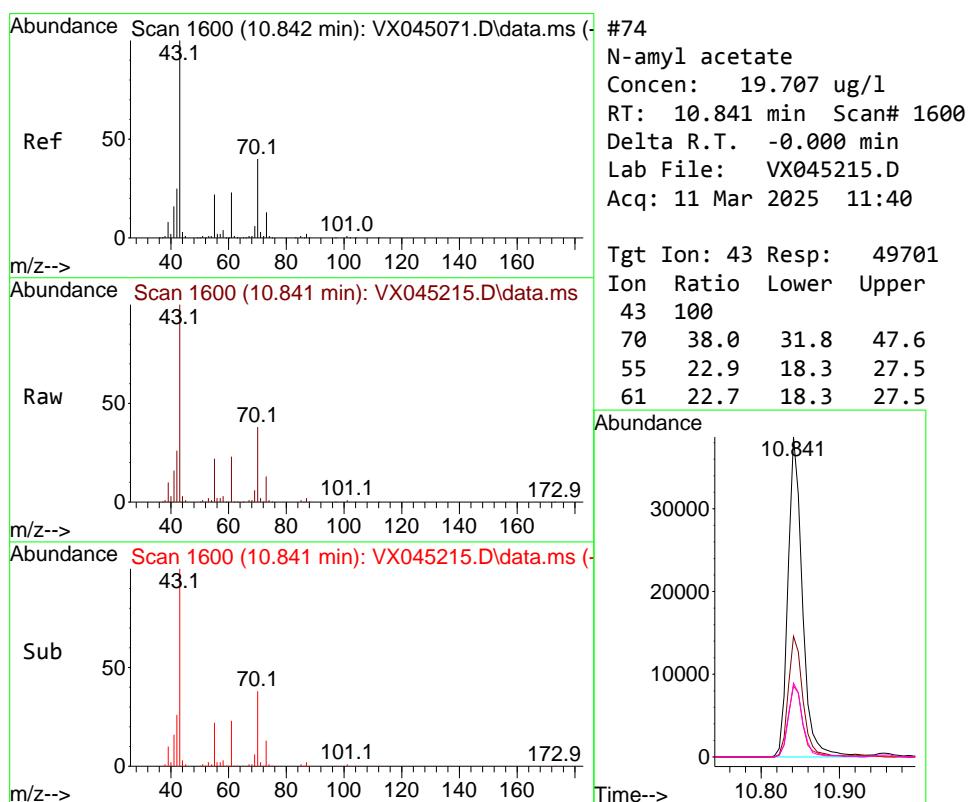

#74
N-amyl acetate
Concen: 19.707 ug/l
RT: 10.841 min Scan# 1600
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion: 43 Resp: 49701
Ion Ratio Lower Upper
43 100
70 38.0 31.8 47.6
55 22.9 18.3 27.5
61 22.7 18.3 27.5





#75
1,1,2,2-Tetrachloroethane
Concen: 19.653 ug/l
RT: 11.213 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion: 83 Resp: 3876
Ion Ratio Lower Upper
83 100
131 8.9 4.5 13.4
85 63.4 31.7 95.1

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

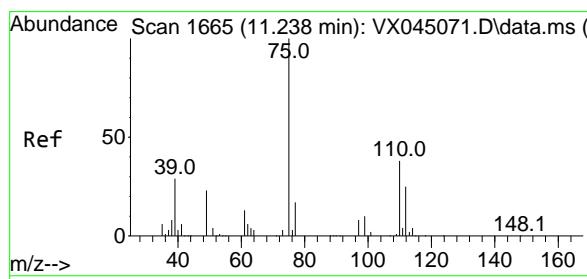


#76
1,2,3-Trichloropropane
Concen: 19.234 ug/l
RT: 11.238 min Scan# 1665
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion: 75 Resp: 30828
Ion Ratio Lower Upper
75 100
77 42.8 20.7 62.1

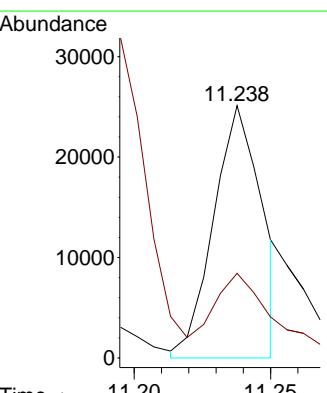



#77
Bromobenzene
Concen: 19.428 ug/l
RT: 11.195 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion:156 Resp: 2463
Ion Ratio Lower Upper
156 100
77 167.5 85.8 257.4
158 93.7 48.4 145.2

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

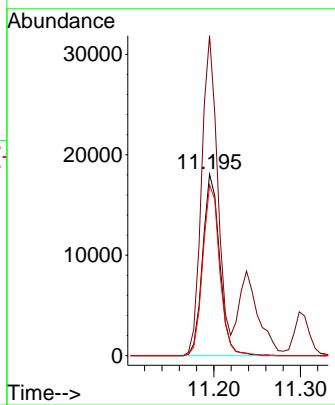


#78
n-propylbenzene
Concen: 19.934 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion: 91 Resp: 121031
Ion Ratio Lower Upper
91 100
120 21.8 11.2 33.6

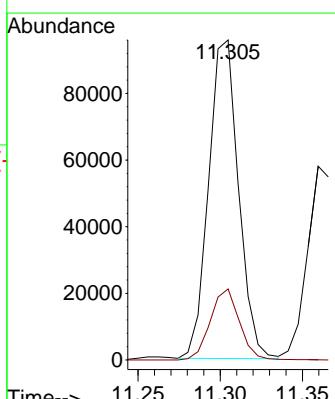



#79
2-Chlorotoluene
Concen: 19.344 ug/l
RT: 11.360 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion: 91 Resp: 74800
Ion Ratio Lower Upper
91 100
126 32.1 16.4 49.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#80
1,3,5-Trimethylbenzene
Concen: 20.096 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion:105 Resp: 87336
Ion Ratio Lower Upper
105 100
120 47.2 24.1 72.2







#81
trans-1,4-Dichloro-2-butene
Concen: 19.112 ug/l
RT: 11.018 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion: 75 Resp: 895:
Ion Ratio Lower Upper
75 100
53 123.0 88.5 132.7
89 45.2 36.2 54.4

Manual Integrations APPROVED



Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

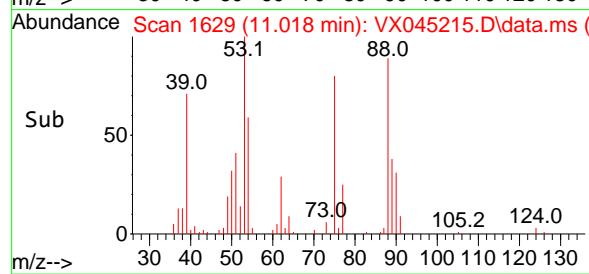


#82
4-Chlorotoluene
Concen: 20.030 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

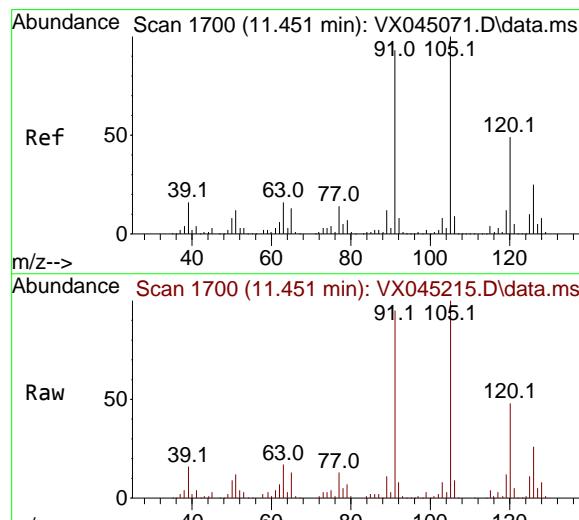


Tgt Ion: 91 Resp: 84411
Ion Ratio Lower Upper
91 100
126 28.5 14.1 42.4

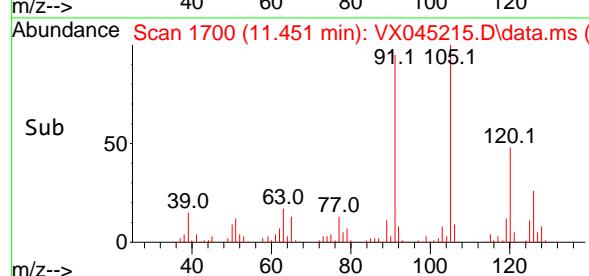

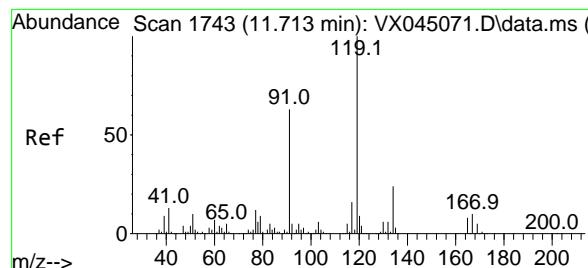

#83
 tert-Butylbenzene
 Concen: 19.342 ug/l
 RT: 11.713 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX045215.D
 Acq: 11 Mar 2025 11:40



Instrument : MSVOA_X
 ClientSampleId : VX0311WBSD01

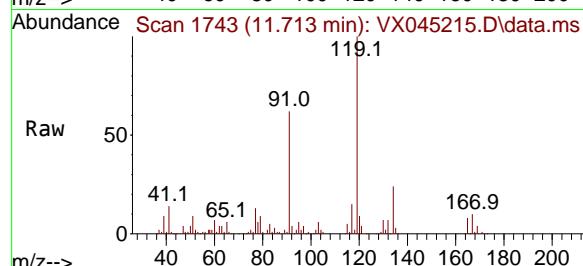

Tgt Ion:119 Resp: 86363
 Ion Ratio Lower Upper
 119 100
 91 62.2 30.7 92.1
 134 23.3 11.7 35.0





Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

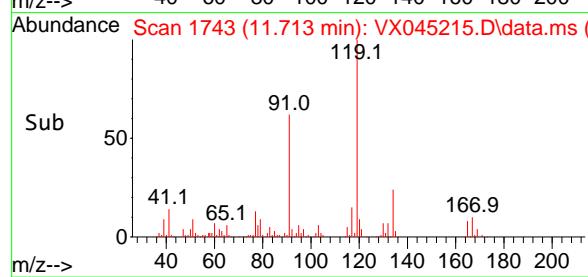

#84
 1,2,4-Trimethylbenzene
 Concen: 20.023 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. -0.000 min
 Lab File: VX045215.D
 Acq: 11 Mar 2025 11:40

Tgt Ion:105 Resp: 87556
 Ion Ratio Lower Upper
 105 100
 120 44.3 22.1 66.1

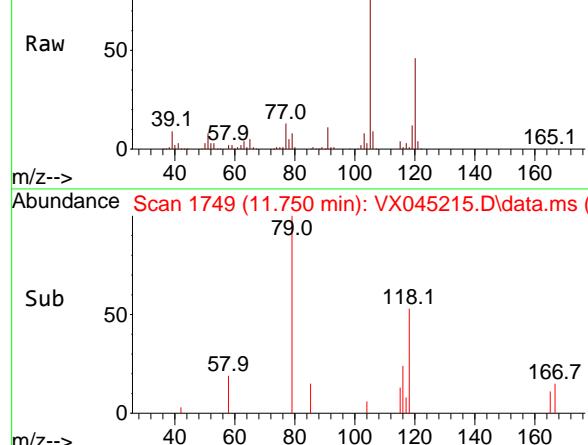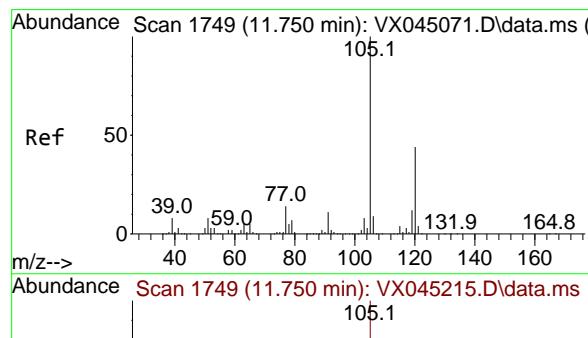






#85
sec-Butylbenzene
Concen: 20.477 ug/l
RT: 11.890 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01

Tgt Ion:105 Resp: 109529
Ion Ratio Lower Upper
105 100
134 19.9 9.8 29.4





Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

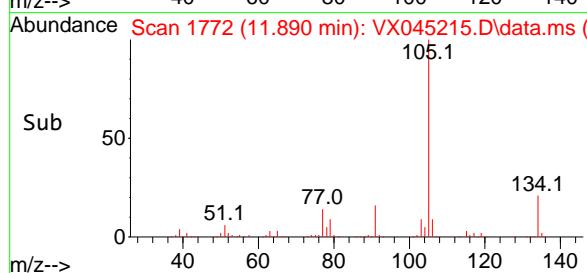

#86
p-Isopropyltoluene
Concen: 20.483 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

Tgt Ion:119 Resp: 88543
Ion Ratio Lower Upper
119 100
134 25.2 12.9 38.6
91 25.4 12.7 38.0

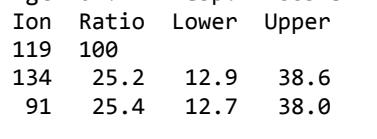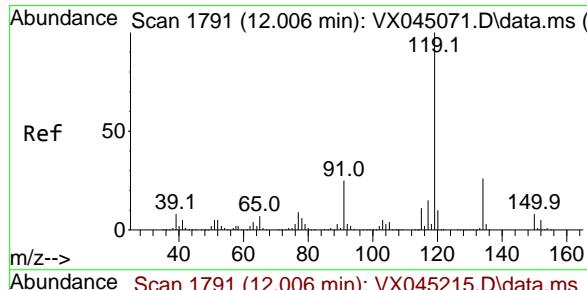


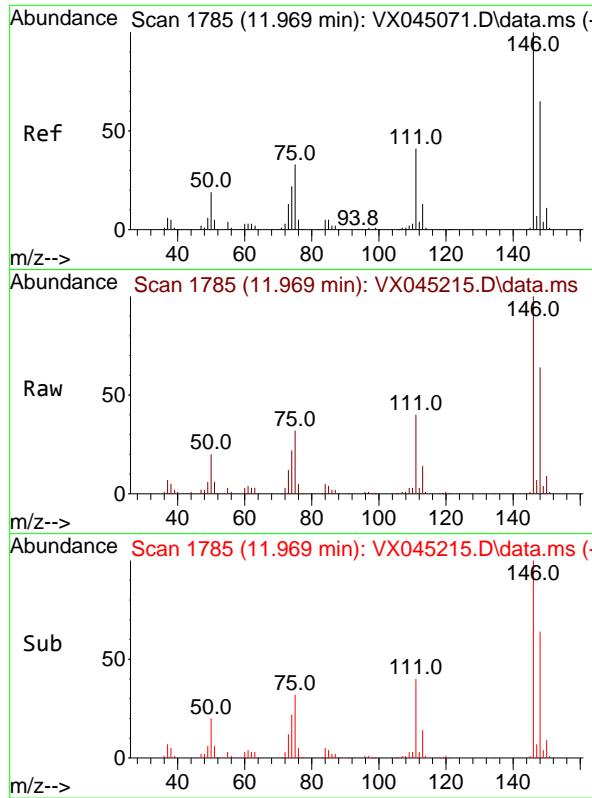


#87
 1,3-Dichlorobenzene
 Concen: 19.615 ug/l
 RT: 11.969 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX045215.D
 Acq: 11 Mar 2025 11:40

Instrument : MSVOA_X
 ClientSampleId : VX0311WBSD01


Manual Integrations
APPROVED


Reviewed By :John Carlone 03/12/2025
 Supervised By :Mahesh Dadoda 03/12/2025

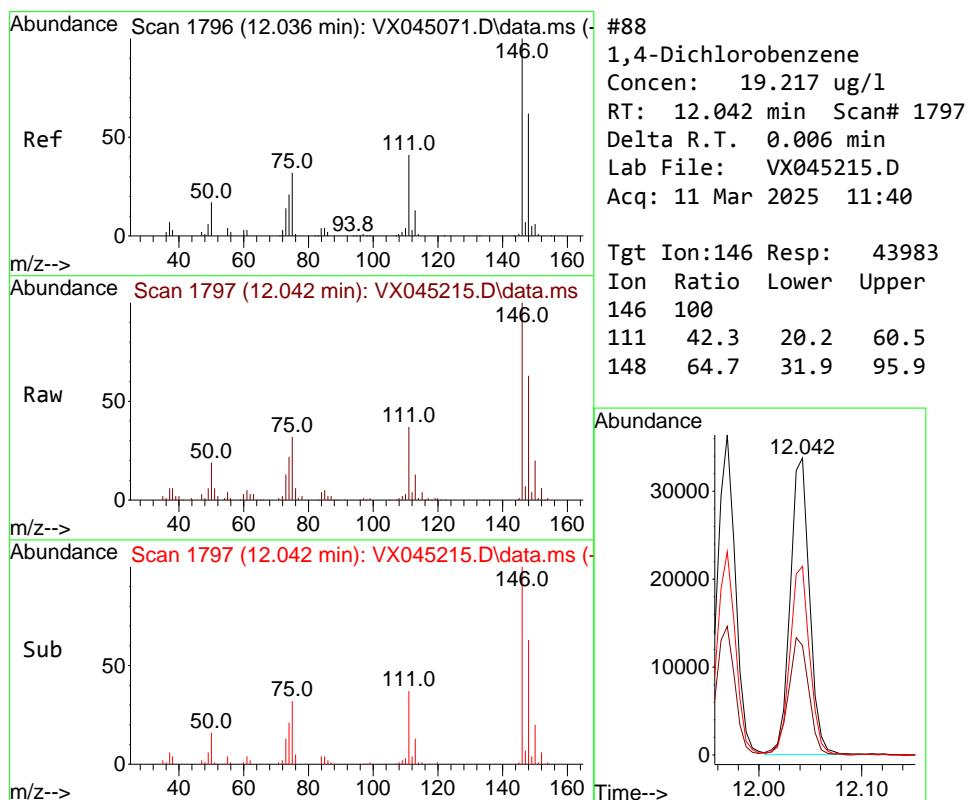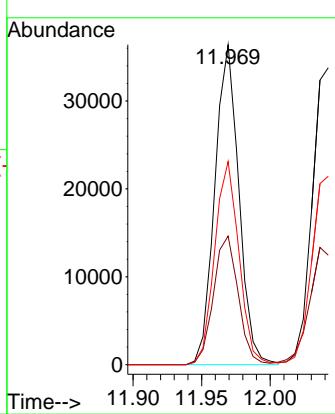

#88
 1,4-Dichlorobenzene
 Concen: 19.217 ug/l
 RT: 12.042 min Scan# 1797
 Delta R.T. 0.006 min
 Lab File: VX045215.D
 Acq: 11 Mar 2025 11:40


Tgt Ion:146 Resp: 43983
 Ion Ratio Lower Upper
 146 100
 111 42.3 20.2 60.5
 148 64.7 31.9 95.9

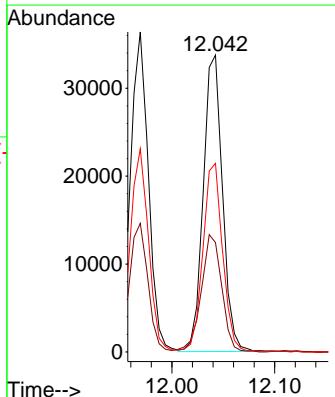



#89
n-Butylbenzene
Concen: 20.636 ug/l
RT: 12.329 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40



Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion: 91 Resp: 76829
Ion Ratio Lower Upper
91 100
92 54.0 26.7 80.0
134 23.6 12.2 36.6

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#90
Hexachloroethane
Concen: 18.273 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Tgt Ion:117 Resp: 14287
Ion Ratio Lower Upper
117 100
201 63.3 31.9 95.9





#91
1,2-Dichlorobenzene
Concen: 19.759 ug/l
RT: 12.335 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40




Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01




Tgt Ion:146 Resp: 4484:
Ion Ratio Lower Upper
146 100
111 42.4 21.6 65.0
148 63.9 31.9 95.9

Manual Integrations APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025




#92
1,2-Dibromo-3-Chloropropane
Concen: 19.352 ug/l
RT: 12.945 min Scan# 1945
Delta R.T. 0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40



Tgt Ion: 75 Resp: 7436
Ion Ratio Lower Upper
75 100
155 76.2 39.6 118.7
157 100.8 51.1 153.4




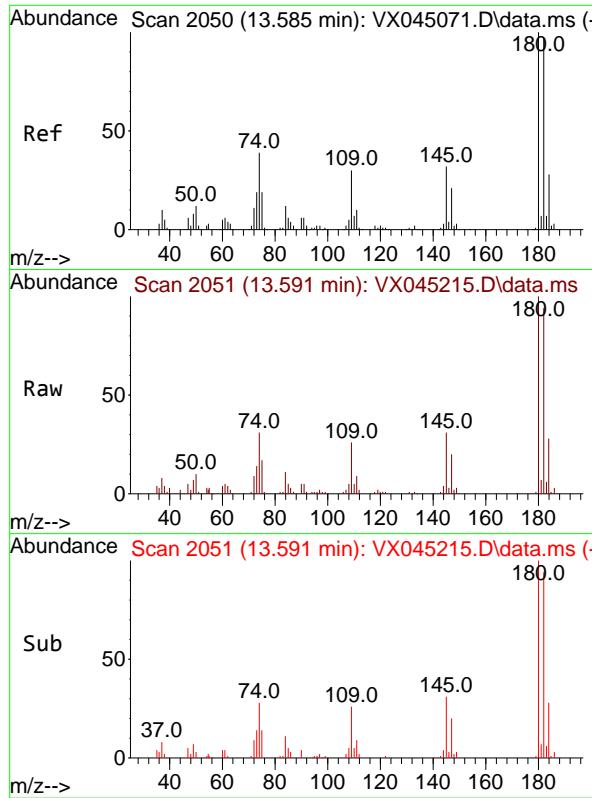


#93
1,2,4-Trichlorobenzene
Concen: 19.453 ug/l
RT: 13.591 min Scan# 2
Delta R.T. 0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

Instrument : MSVOA_X
ClientSampleId : VX0311WBSD01


Manual Integrations
APPROVED


Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

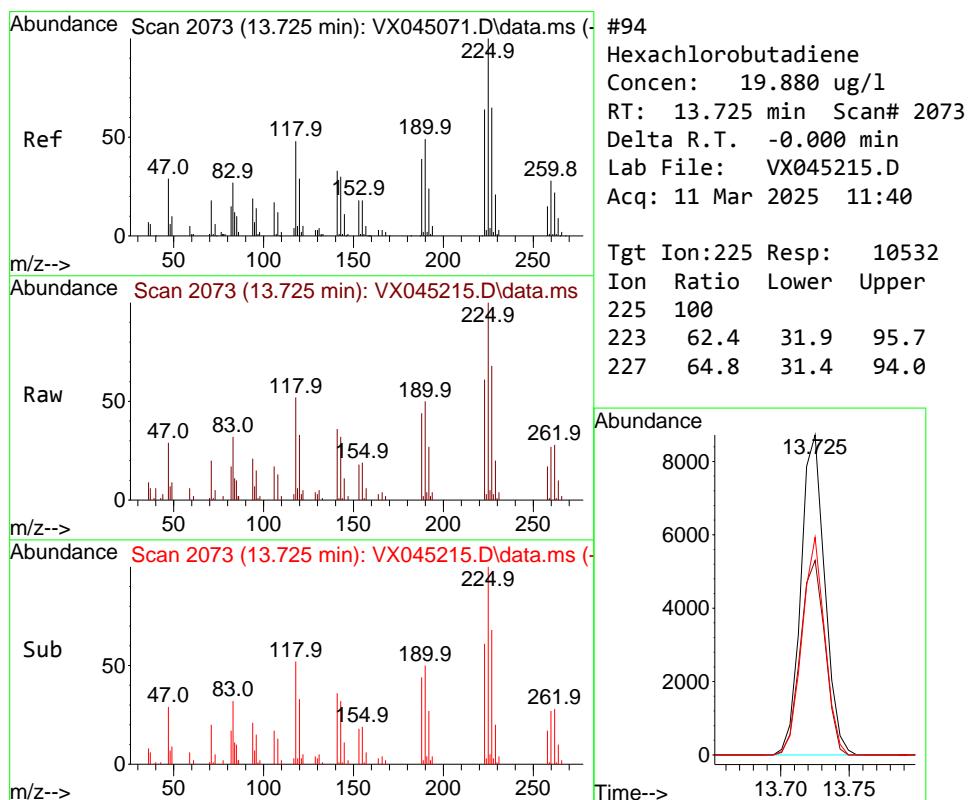

#94
Hexachlorobutadiene
Concen: 19.880 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40


Tgt Ion:225 Resp: 10532
Ion Ratio Lower Upper
225 100
223 62.4 31.9 95.7
227 64.8 31.4 94.0



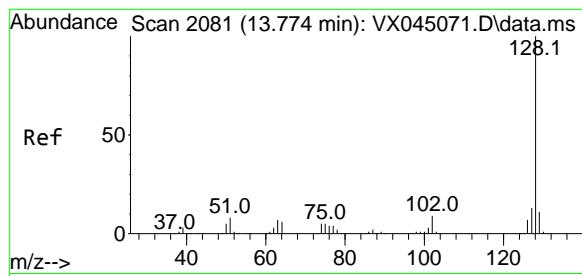




#95
Naphthalene
Concen: 19.175 ug/l
RT: 13.774 min Scan# 2111
Delta R.T. -0.000 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40

Instrument: MSVOA_X
ClientSampleId: VX0311WBSD01




Tgt	Ion:128	Resp:	95200
	Ion Ratio	Lower	Upper
128	100		
127	13.0	10.3	15.5
129	10.8	8.7	13.1



Manual Integrations APPROVED
Reviewed By :John Carlone 03/12/2025
Supervised By :Mahesh Dadoda 03/12/2025

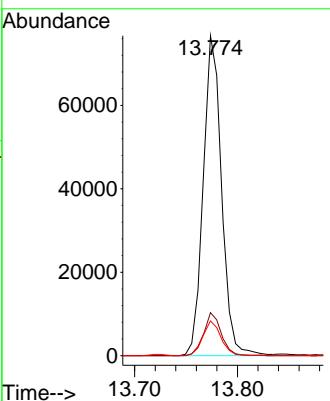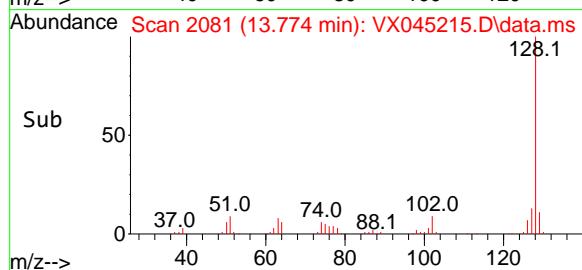

#96
1,2,3-Trichlorobenzene
Concen: 19.287 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.006 min
Lab File: VX045215.D
Acq: 11 Mar 2025 11:40



Tgt	Ion:180	Resp:	26292
	Ion Ratio	Lower	Upper
180	100		
182	93.3	47.5	142.6
145	33.8	17.0	50.9

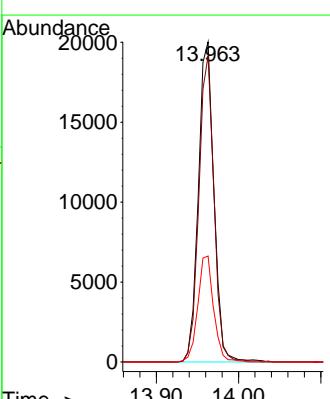



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:	VX022825	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDICC001	VX045068.D	1,2,3-Trichloropropane	JOHN	2/28/2025 10:05:09 AM	MMDadoda	2/28/2025 11:09:31 AM	Peak Integrated by Software
VSTDICC001	VX045068.D	1,4-Dichlorobenzene	JOHN	2/28/2025 10:05:09 AM	MMDadoda	2/28/2025 11:09:31 AM	Peak Integrated by Software
VSTDICC001	VX045068.D	Carbon Tetrachloride	JOHN	2/28/2025 10:05:09 AM	MMDadoda	2/28/2025 11:09:31 AM	Peak Integrated by Software
VSTDICC001	VX045068.D	Chloroethane	JOHN	2/28/2025 10:05:09 AM	MMDadoda	2/28/2025 11:09:31 AM	Peak Integrated by Software
VSTDICC001	VX045068.D	Ethyl Acetate	JOHN	2/28/2025 10:05:09 AM	MMDadoda	2/28/2025 11:09:31 AM	Peak Integrated by Software
VSTDICC001	VX045068.D	Methacrylonitrile	JOHN	2/28/2025 10:05:09 AM	MMDadoda	2/28/2025 11:09:31 AM	Peak Integrated by Software
VSTDICC001	VX045068.D	Methyl methacrylate	JOHN	2/28/2025 10:05:09 AM	MMDadoda	2/28/2025 11:09:31 AM	Peak Integrated by Software
VSTDICC005	VX045069.D	1,2,3-Trichloropropane	JOHN	2/28/2025 10:05:14 AM	MMDadoda	2/28/2025 11:09:31 AM	Peak Integrated by Software
VSTDICC005	VX045069.D	Tert butyl alcohol	JOHN	2/28/2025 10:05:14 AM	MMDadoda	2/28/2025 11:09:31 AM	Peak Integrated by Software
VSTDICC020	VX045070.D	1,2,3-Trichloropropane	JOHN	2/28/2025 10:05:21 AM	MMDadoda	2/28/2025 11:09:33 AM	Peak Integrated by Software
VSTDICCC050	VX045071.D	1,2,3-Trichloropropane	JOHN	2/28/2025 10:05:25 AM	MMDadoda	2/28/2025 11:09:35 AM	Peak Integrated by Software
VSTDICC100	VX045072.D	1,2,3-Trichloropropane	JOHN	2/28/2025 10:05:30 AM	MMDadoda	2/28/2025 11:09:37 AM	Peak Integrated by Software
VSTDICC150	VX045073.D	1,2,3-Trichloropropane	JOHN	2/28/2025 10:05:33 AM	MMDadoda	2/28/2025 11:09:42 AM	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:	VX022825	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDICV050	VX045075.D	1,2,3-Trichloropropane	JOHN	2/28/2025 10:05:38 AM	MMDadoda	2/28/2025 11:09:44 AM	Peak Integrated by Software
VSTDCCC050	VX045077.D	1,2,3-Trichloropropane	JOHN	3/3/2025 8:20:45 AM	MMDadoda	3/3/2025 1:49:43 PM	Peak Integrated by Software
VSTDCCC050	VX045077.D	Tert butyl alcohol	JOHN	3/3/2025 8:20:45 AM	MMDadoda	3/3/2025 1:49:43 PM	Peak Integrated by Software
VSTDCCC050	VX045098.D	1,2,3-Trichloropropane	JOHN	3/3/2025 8:20:59 AM	MMDadoda	3/3/2025 1:49:50 PM	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:	VX031125	Instrument	MSVOA_x
-----------	----------	------------	---------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
VSTDCCC050	VX045211.D	1,2,3-Trichloropropane	JOHN	3/12/2025 9:52:29 AM	MMDadoda	3/12/2025 3:17:16 PM	Peak Integrated by Software
VX0311WBS01	VX045214.D	1,2,3-Trichloropropane	JOHN	3/12/2025 9:52:33 AM	MMDadoda	3/12/2025 3:17:16 PM	Peak Integrated by Software
VX0311WBSD01	VX045215.D	1,2,3-Trichloropropane	JOHN	3/12/2025 9:52:37 AM	MMDadoda	3/12/2025 3:17:18 PM	Peak Integrated by Software
VSTDCCC050	VX045236.D	1,2,3-Trichloropropane	JOHN	3/12/2025 9:53:00 AM	MMDadoda	3/12/2025 3:17:20 PM	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QCBatch ID # VX022825

Review By	Mahesh Dadoda	Review On	2/28/2025 11:09:50 AM
Supervise By	Semsettin Yesilyurt	Supervise On	2/28/2025 11:11:09 AM
SubDirectory	VX022825	HP Acquire Method	HP Processing Method 82X022825W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133187,VP133189 VP133194,VP133195,VP133196,VP133197,VP133198,VP133199 VP133188,VP133190 VP133200		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VX045067.D	28 Feb 2025 01:03	JC/MD	Ok
2	VSTDICC001	VX045068.D	28 Feb 2025 01:27	JC/MD	Ok,M
3	VSTDICC005	VX045069.D	28 Feb 2025 02:13	JC/MD	Ok,M
4	VSTDICC020	VX045070.D	28 Feb 2025 02:37	JC/MD	Ok,M
5	VSTDICCC050	VX045071.D	28 Feb 2025 03:00	JC/MD	Ok,M
6	VSTDICC100	VX045072.D	28 Feb 2025 03:23	JC/MD	Ok,M
7	VSTDICC150	VX045073.D	28 Feb 2025 03:47	JC/MD	Ok,M
8	IBLK	VX045074.D	28 Feb 2025 04:10	JC/MD	Ok
9	VSTDICV050	VX045075.D	28 Feb 2025 04:33	JC/MD	Ok,M
10	BFB	VX045076.D	28 Feb 2025 10:03	JC/MD	Ok
11	VSTDCCCC050	VX045077.D	28 Feb 2025 10:32	JC/MD	Ok,M
12	VX0228MBL01	VX045078.D	28 Feb 2025 11:00	JC/MD	Ok
13	VX0228WBL01	VX045079.D	28 Feb 2025 11:23	JC/MD	Ok
14	VX0228WBS01	VX045080.D	28 Feb 2025 11:46	JC/MD	Ok,M
15	VX0228WBSD01	VX045081.D	28 Feb 2025 12:13	JC/MD	Ok,M
16	Q1401-03	VX045082.D	28 Feb 2025 12:37	JC/MD	Ok
17	Q1401-06	VX045083.D	28 Feb 2025 13:00	JC/MD	Ok
18	Q1423-01	VX045084.D	28 Feb 2025 13:23	JC/MD	Ok
19	Q1423-03	VX045085.D	28 Feb 2025 13:47	JC/MD	Ok
20	Q1403-01	VX045086.D	28 Feb 2025 14:10	JC/MD	Ok
21	Q1403-02	VX045087.D	28 Feb 2025 14:33	JC/MD	Ok

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QCBatch ID # VX022825

Review By	Mahesh Dadoda	Review On	2/28/2025 11:09:50 AM		
Supervise By	Semsettin Yesilyurt	Supervise On	2/28/2025 11:11:09 AM		
SubDirectory	VX022825	HP Acquire Method		HP Processing Method	82X022825W.M
STD. NAME	STD REF.#				
Tune/Reschk Initial Calibration Stds	VP133187,VP133189 VP133194,VP133195,VP133196,VP133197,VP133198,VP133199				
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133188,VP133190 VP133200				

22	Q1435-01	VX045088.D	28 Feb 2025 14:57	JC/MD	Ok
23	Q1403-04	VX045089.D	28 Feb 2025 15:20	JC/MD	Ok
24	Q1462-02	VX045090.D	28 Feb 2025 15:44	JC/MD	Ok
25	Q1469-01	VX045091.D	28 Feb 2025 16:07	JC/MD	Ok
26	Q1469-02	VX045092.D	28 Feb 2025 16:31	JC/MD	Ok
27	Q1469-03	VX045093.D	28 Feb 2025 16:54	JC/MD	Ok
28	Q1469-04	VX045094.D	28 Feb 2025 17:17	JC/MD	Ok
29	Q1403-03	VX045095.D	28 Feb 2025 17:41	JC/MD	Ok
30	Q1462-01	VX045096.D	28 Feb 2025 18:04	JC/MD	Ok,M
31	IBLK	VX045097.D	28 Feb 2025 18:27	JC/MD	Ok
32	VSTDCCC050	VX045098.D	28 Feb 2025 18:50	JC/MD	Ok,M

M : Manual Integration



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QCBatch ID # VX031125

Review By	John Carfone	Review On	3/12/2025 10:04:41 AM
Supervise By	Mahesh Dadoda	Supervise On	3/12/2025 3:17:22 PM
SubDirectory	VX031125	HP Acquire Method	HP Processing Method 82X022825W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP133244		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133245,VP133246		

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VX045210.D	11 Mar 2025 09:30	JC/MD	Ok
2	VSTDCCC050	VX045211.D	11 Mar 2025 09:59	JC/MD	Ok,M
3	VX0311MBL01	VX045212.D	11 Mar 2025 10:27	JC/MD	Ok
4	VX0311WBL01	VX045213.D	11 Mar 2025 10:51	JC/MD	Ok
5	VX0311WBS01	VX045214.D	11 Mar 2025 11:14	JC/MD	Ok,M
6	VX0311WBSD01	VX045215.D	11 Mar 2025 11:40	JC/MD	Ok,M
7	Q1502-01	VX045216.D	11 Mar 2025 12:03	JC/MD	Ok
8	IBLK	VX045217.D	11 Mar 2025 12:27	JC/MD	Ok
9	Q1500-07DL	VX045218.D	11 Mar 2025 12:50	JC/MD	Ok
10	Q1531-16DL	VX045219.D	11 Mar 2025 13:13	JC/MD	Ok
11	Q1500-04DL	VX045220.D	11 Mar 2025 13:36	JC/MD	Ok
12	Q1531-03DL	VX045221.D	11 Mar 2025 14:00	JC/MD	Ok
13	Q1531-05DL	VX045222.D	11 Mar 2025 14:23	JC/MD	Ok
14	Q1531-11DL	VX045223.D	11 Mar 2025 14:46	JC/MD	Ok
15	Q1531-17DL	VX045224.D	11 Mar 2025 15:09	JC/MD	Ok
16	Q1531-07DL	VX045225.D	11 Mar 2025 15:33	JC/MD	Ok
17	Q1531-18	VX045226.D	11 Mar 2025 15:56	JC/MD	Ok
18	Q1531-21	VX045227.D	11 Mar 2025 16:19	JC/MD	Ok
19	Q1531-02	VX045228.D	11 Mar 2025 16:43	JC/MD	Ok
20	Q1541-01	VX045229.D	11 Mar 2025 17:06	JC/MD	Ok
21	Q1531-19	VX045230.D	11 Mar 2025 17:29	JC/MD	Dilution



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QCBatch ID # VX031125

Review By	John Carfone	Review On	3/12/2025 10:04:41 AM
Supervise By	Mahesh Dadoda	Supervise On	3/12/2025 3:17:22 PM
SubDirectory	VX031125	HP Acquire Method	HP Processing Method 82X022825W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP133244		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133245,VP133246		

22	Q1531-20	VX045231.D	11 Mar 2025 17:52	JC/MD	ReRun
23	Q1531-12	VX045232.D	11 Mar 2025 18:16	JC/MD	Dilution
24	Q1531-15	VX045233.D	11 Mar 2025 18:39	JC/MD	Dilution
25	Q1531-06	VX045234.D	11 Mar 2025 19:02	JC/MD	Not Ok
26	Q1525-01	VX045235.D	11 Mar 2025 19:25	JC/MD	Ok,M
27	VSTDCCC050	VX045236.D	11 Mar 2025 19:49	JC/MD	Ok,M

M : Manual Integration



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QCBatch ID # VX022825

Review By	Mahesh Dadoda	Review On	2/28/2025 11:09:50 AM
Supervise By	Semsettin Yesilyurt	Supervise On	2/28/2025 11:11:09 AM
SubDirectory	VX022825	HP Acquire Method	HP Processing Method 82X022825W.M
STD. NAME	STD REF.#		
Tune/Reschk	VP133187,VP133189		
Initial Calibration Stds	VP133194,VP133195,VP133196,VP133197,VP133198,VP133199		
CCC	VP133188,VP133190		
Internal Standard/PEM	VP133200		
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VX045067.D	28 Feb 2025 01:03		JC/MD	Ok
2	VSTDICCC001	VSTDICCC001	VX045068.D	28 Feb 2025 01:27		JC/MD	Ok,M
3	VSTDICCC005	VSTDICCC005	VX045069.D	28 Feb 2025 02:13		JC/MD	Ok,M
4	VSTDICCC020	VSTDICCC020	VX045070.D	28 Feb 2025 02:37		JC/MD	Ok,M
5	VSTDICCC050	VSTDICCC050	VX045071.D	28 Feb 2025 03:00		JC/MD	Ok,M
6	VSTDICCC100	VSTDICCC100	VX045072.D	28 Feb 2025 03:23		JC/MD	Ok,M
7	VSTDICCC150	VSTDICCC150	VX045073.D	28 Feb 2025 03:47		JC/MD	Ok,M
8	IBLK	IBLK	VX045074.D	28 Feb 2025 04:10		JC/MD	Ok
9	VSTDICCV050	ICVVX022825	VX045075.D	28 Feb 2025 04:33		JC/MD	Ok,M
10	BFB	BFB	VX045076.D	28 Feb 2025 10:03		JC/MD	Ok
11	VSTDCCC050	VSTDCCC050	VX045077.D	28 Feb 2025 10:32	V12668	JC/MD	Ok,M
12	VX0228MBL01	VX0228MBL01	VX045078.D	28 Feb 2025 11:00		JC/MD	Ok
13	VX0228WBL01	VX0228WBL01	VX045079.D	28 Feb 2025 11:23		JC/MD	Ok
14	VX0228WBS01	VX0228WBS01	VX045080.D	28 Feb 2025 11:46		JC/MD	Ok,M
15	VX0228WBSD01	VX0228WBSD01	VX045081.D	28 Feb 2025 12:13		JC/MD	Ok,M
16	Q1401-03	BP-VPB-192-GW-840-8	VX045082.D	28 Feb 2025 12:37	vial B pH<2	JC/MD	Ok
17	Q1401-06	BP-VPB-192-GW-900-9	VX045083.D	28 Feb 2025 13:00	vial B pH<2	JC/MD	Ok
18	Q1423-01	BP-VPB-192-TB-20250	VX045084.D	28 Feb 2025 13:23	vial B pH<2 TB	JC/MD	Ok



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QCBatch ID # VX022825

Review By	Mahesh Dadoda	Review On	2/28/2025 11:09:50 AM
Supervise By	Semsettin Yesilyurt	Supervise On	2/28/2025 11:11:09 AM
SubDirectory	VX022825	HP Acquire Method	HP Processing Method 82X022825W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP133187,VP133189 VP133194,VP133195,VP133196,VP133197,VP133198,VP133199		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133188,VP133190 VP133200		

19	Q1423-03	BP-VPB-192-EB-20250	VX045085.D	28 Feb 2025 13:47	vial B pH<2 EB	JC/MD	Ok
20	Q1403-01	Storage-Blank-SOIL-RE	VX045086.D	28 Feb 2025 14:10	vial B pH<2	JC/MD	Ok
21	Q1403-02	Storage-Blank-WATER-	VX045087.D	28 Feb 2025 14:33	vial B pH<2	JC/MD	Ok
22	Q1435-01	286107	VX045088.D	28 Feb 2025 14:57	vial A pH<2	JC/MD	Ok
23	Q1403-04	Storage-Blank-SAMPLE	VX045089.D	28 Feb 2025 15:20	vial B pH<2	JC/MD	Ok
24	Q1462-02	FB	VX045090.D	28 Feb 2025 15:44	vial A pH<2 FB	JC/MD	Ok
25	Q1469-01	Storage-Blank-SOIL-RE	VX045091.D	28 Feb 2025 16:07	vial A pH<2	JC/MD	Ok
26	Q1469-02	Storage-Blank-WATER-	VX045092.D	28 Feb 2025 16:31	vial A pH<2	JC/MD	Ok
27	Q1469-03	Storage-Blank-WATER-	VX045093.D	28 Feb 2025 16:54	vial A pH<2	JC/MD	Ok
28	Q1469-04	Storage-Blank-SAMPLE	VX045094.D	28 Feb 2025 17:17	vial A pH<2	JC/MD	Ok
29	Q1403-03	Storage-Blank-WATER-	VX045095.D	28 Feb 2025 17:41	vial B pH<2	JC/MD	Ok
30	Q1462-01	MW2	VX045096.D	28 Feb 2025 18:04	vial A pH<2	JC/MD	Ok,M
31	IBLK	IBLK	VX045097.D	28 Feb 2025 18:27		JC/MD	Ok
32	VSTDCCC050	VSTDCCC050EC	VX045098.D	28 Feb 2025 18:50		JC/MD	Ok,M

M : Manual Integration



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QCBatch ID # VX031125

Review By	John Carlone	Review On	3/12/2025 10:04:41 AM
Supervise By	Mahesh Dadoda	Supervise On	3/12/2025 3:17:22 PM
SubDirectory	VX031125	HP Acquire Method	HP Processing Method 82X022825W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	VP133244		
CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133245,VP133246		

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	BFB	BFB	VX045210.D	11 Mar 2025 09:30		JC/MD	Ok
2	VSTDCCC050	VSTDCCC050	VX045211.D	11 Mar 2025 09:59	CCAL failed low for comp. #11	JC/MD	Ok,M
3	VX0311MBL01	VX0311MBL01	VX045212.D	11 Mar 2025 10:27		JC/MD	Ok
4	VX0311WBL01	VX0311WBL01	VX045213.D	11 Mar 2025 10:51		JC/MD	Ok
5	VX0311WBS01	VX0311WBS01	VX045214.D	11 Mar 2025 11:14		JC/MD	Ok,M
6	VX0311WBSD01	VX0311WBSD01	VX045215.D	11 Mar 2025 11:40		JC/MD	Ok,M
7	Q1502-01	PT-VOA-WP	VX045216.D	11 Mar 2025 12:03	PT-VOA-WP (8260)	JC/MD	Ok
8	IBLK	IBLK	VX045217.D	11 Mar 2025 12:27		JC/MD	Ok
9	Q1500-07DL	MW179D-20250305DL	VX045218.D	11 Mar 2025 12:50	vial B pH<2	JC/MD	Ok
10	Q1531-16DL	RE125D1-20250307DL	VX045219.D	11 Mar 2025 13:13	vial B pH<2	JC/MD	Ok
11	Q1500-04DL	MW178I1-20250305DL	VX045220.D	11 Mar 2025 13:36	vial B pH<2	JC/MD	Ok
12	Q1531-03DL	RE122D1-20250305DL	VX045221.D	11 Mar 2025 14:00	vial B pH<2	JC/MD	Ok
13	Q1531-05DL	RE126D2-20250306DL	VX045222.D	11 Mar 2025 14:23	vial B pH<2	JC/MD	Ok
14	Q1531-11DL	RE103D2-20250306DL	VX045223.D	11 Mar 2025 14:46	vial B pH<2	JC/MD	Ok
15	Q1531-17DL	RE125D2-20250307DL	VX045224.D	11 Mar 2025 15:09	vial B pH<2	JC/MD	Ok
16	Q1531-07DL	RE103D1-20250306DL	VX045225.D	11 Mar 2025 15:33	vial B pH<2	JC/MD	Ok
17	Q1531-18	FB01	VX045226.D	11 Mar 2025 15:56	vial A pH<2 FB	JC/MD	Ok
18	Q1531-21	TB	VX045227.D	11 Mar 2025 16:19	vial A pH<2 TB	JC/MD	Ok



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Instrument ID: MSVOA_X

Daily Analysis Runlog For Sequence/QCBatch ID # VX031125

Review By	John Carbone	Review On	3/12/2025 10:04:41 AM
Supervise By	Mahesh Dadoda	Supervise On	3/12/2025 3:17:22 PM
SubDirectory	VX031125	HP Acquire Method	HP Processing Method 82X022825W.M
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard	VP133244 VP133245,VP133246		

19	Q1531-02	RE122D3-20250305	VX045228.D	11 Mar 2025 16:43	vial B pH<2	JC/MD	Ok
20	Q1541-01	205703	VX045229.D	11 Mar 2025 17:06	vial A pH<2	JC/MD	Ok
21	Q1531-19	RE104D2-20250307	VX045230.D	11 Mar 2025 17:29	vial A pH<2 Need 10X	JC/MD	Dilution
22	Q1531-20	RE104D3-20250307	VX045231.D	11 Mar 2025 17:52	vial A pH<2 E flage in previous sample	JC/MD	ReRun
23	Q1531-12	RE108D2-20250306	VX045232.D	11 Mar 2025 18:16	vial A pH<2 Need 40X	JC/MD	Dilution
24	Q1531-15	RE105D2-20250306	VX045233.D	11 Mar 2025 18:39	vial A pH<2 Need 40X	JC/MD	Dilution
25	Q1531-06	DUP01-20250306	VX045234.D	11 Mar 2025 19:02	run straight	JC/MD	Not Ok
26	Q1525-01	MW10	VX045235.D	11 Mar 2025 19:25	vial B pH<2	JC/MD	Ok,M
27	VSTDCCC050	VSTDCCC050EC	VX045236.D	11 Mar 2025 19:49		JC/MD	Ok,M

M : Manual Integration

Prep Standard - Chemical Standard Summary

Order ID : Q1502

Test : VOCMS Group1

Prepbatch ID :

Sequence ID/Qc Batch ID: VX031125,

Standard ID :

VP131746,VP131767,VP132035,VP132096,VP133036,VP133174,VP133178,VP133244,VP133245,VP133246,

Chemical ID :

V13391,V13457,V13460,V13465,V13466,V13706,V14154,V14175,V14176,V14289,V14433,V14439,V14521,V14522,V14613,V14614,V14624,V14630,V14631,V14632,V14633,V14722,V14723,V14724,V14744,V14754,V14809,V14814,V14842,V14872,V14873,V14874,V14875,W3112,



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
247	8260 Internal Standard, 250PPM	VP131746	11/22/2024	05/18/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 11/23/2024

FROM 0.50000ml of V14289 + 49.50000ml of V14154 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
218	BFB, 25PPM	VP131767	11/22/2024	05/18/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 11/27/2024

FROM 0.50000ml of V13391 + 49.50000ml of V14154 = Final Quantity: 50.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1810	8260 Working Std(2-CVE)-800ppm	VP132035	12/10/2024	06/10/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 12/12/2024

FROM 1.00000ml of V14630 + 1.00000ml of V14631 + 1.00000ml of V14632 + 1.00000ml of V14633 + 46.00000ml of V14614 = Final
Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
719	8260 Working STD (BCM)-First source, 400PPM	VP132096	12/12/2024	06/10/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 12/19/2024

FROM 1.00000ml of V13465 + 1.00000ml of V13466 + 1.50000ml of V13457 + 1.50000ml of V13460 + 20.00000ml of V14614 = Final
Quantity: 25.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
51	8260 Working STD (Acrolein) -first source, 800PPM	VP133036	02/14/2025	03/13/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 02/18/2025

FROM 1.00000ml of V14872 + 1.00000ml of V14873 + 1.00000ml of V14874 + 1.00000ml of V14875 + 21.00000ml of V14624 = Final
Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
617	8260 Surrogate, 400PPM	VP133174	02/27/2025	08/27/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 03/04/2025

FROM 0.40000ml of V13706 + 24.60000ml of V14613 = Final Quantity: 25.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
257	8260 Calibration Working STD Mix-First source, 160PPM	VP133178	02/27/2025	03/31/2025	Semsettin Yesilyurt	None	None	Mahesh Dadoda 03/04/2025

FROM 0.40000ml of V14842 + 1.00000ml of V14175 + 1.00000ml of V14176 + 1.00000ml of V14433 + 1.00000ml of V14439 + 1.00000ml of V14521 + 1.00000ml of V14522 + 1.00000ml of V14724 + 1.00000ml of V14744 + 1.00000ml of V14754 + 1.00000ml of V14809 + 1.00000ml of V14814 + 1.50000ml of V14722 + 1.50000ml of V14723 + 10.60000ml of V14613 = Final
Quantity: 25.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
589	BFB TUNE CHECK	VP133244	03/11/2025	03/12/2025	John Carlone	None	None	Romaben Patel 03/11/2025

FROM 39.98400ml of W3112 + 0.01600ml of VP131767 = Final Quantity: 40.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

VOC STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
620	50 PPB CCC, 8260-Water	VP133245	03/11/2025	03/12/2025	John Carlone	None	None	Romaben Patel 03/11/2025

FROM 39.94450ml of W3112 + 0.00500ml of VP132096 + 0.00500ml of VP133174 + 0.00800ml of VP131746 + 0.01250ml of VP132035 + 0.01250ml of VP133036 + 0.01250ml of VP133178 = Final Quantity: 40.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
620	50 PPB CCC, 8260-Water	VP133246	03/11/2025	03/12/2025	John Carlone	None	None	Romaben Patel 03/11/2025

FROM 39.94450ml of W3112 + 0.00500ml of VP132096 + 0.00500ml of VP133174 + 0.00800ml of VP131746 + 0.01250ml of VP132035 + 0.01250ml of VP133036 + 0.01250ml of VP133178 = Final Quantity: 40.000 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30067 / BFB tuneing solution	A0191805	11/22/2025	11/22/2024 / SAM	01/13/2023 / SAM	V13391
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0193071	06/12/2025	12/12/2024 / SAM	01/27/2023 / SAM	V13457
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0193071	06/12/2025	12/12/2024 / SAM	01/27/2023 / SAM	V13460
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0193071	06/12/2025	12/12/2024 / SAM	01/27/2023 / SAM	V13465
Restek	30225 / VOA Mix, bromochloromethane, 2000ug/mL, P&TM, 1mL/ampul	A0193071	06/12/2025	12/12/2024 / SAM	01/27/2023 / SAM	V13466
Restek	555582 / Custom Mixture, 8260 A/B Surrogate Mix [CS 5179-2]	A0196865	02/27/2026	02/27/2025 / SAM	04/12/2023 / SAM	V13706



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	05/18/2025	11/18/2024 / pedro	02/06/2024 / SAM	V14154
Absolute Standards, Inc.	95317 / Universal VOA Mega Mix (Min order = 5)	021624	07/10/2025	01/10/2025 / SAM	02/20/2024 / SAM	V14175
Absolute Standards, Inc.	95317 / Universal VOA Mega Mix (Min order = 5)	021624	07/10/2025	01/10/2025 / SAM	02/20/2024 / SAM	V14176
Restek	555581 / Custom Standard, 8260 Internal Std [CS 5179-1]	A0210184	11/22/2025	11/22/2024 / SAM	04/15/2024 / SAM	V14289
Restek	30489 / VOA Mix, 8260B Acetates Mix, P&TM, 1mL	A0209618	07/10/2025	01/10/2025 / SAM	08/15/2024 / SAM	V14433
Restek	30489 / VOA Mix, 8260B Acetates Mix, P&TM, 1mL	A0209618	07/10/2025	01/10/2025 / SAM	08/15/2024 / SAM	V14439



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95319 / Revised Additions Mix (Min = 5)	091724	07/10/2025	01/10/2025 / SAM	09/18/2024 / SAM	V14521
Absolute Standards, Inc.	95319 / Revised Additions Mix (Min = 5)	091724	07/10/2025	01/10/2025 / SAM	09/18/2024 / SAM	V14522
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	08/27/2025	02/27/2025 / SAM	11/26/2024 / SAM	V14613
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22L0562016	06/10/2025	12/10/2024 / SAM	11/26/2024 / SAM	V14614
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	23I0762004	07/13/2025	01/13/2025 / SAM	11/26/2024 / SAM	V14624
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	06/10/2025	12/10/2024 / SAM	12/06/2024 / SAM	V14630



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	06/10/2025	12/10/2024 / SAM	12/06/2024 / SAM	V14631
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	06/10/2025	12/10/2024 / SAM	12/06/2024 / SAM	V14632
Absolute Standards, Inc.	/ 2-Chloroethyl vinyl ether	120524	06/10/2025	12/10/2024 / SAM	12/06/2024 / SAM	V14633
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000ug/ml, PTM, 1ml	A02110618	07/10/2025	01/10/2025 / SAM	12/17/2024 / SAM	V14722
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000ug/ml, PTM, 1ml	A02110618	07/10/2025	01/10/2025 / SAM	12/17/2024 / SAM	V14723
Restek	30006 / VOA Mix, CLP method Calibration Std #1 ketones 5000ug/ml, PTM, 1ml	A02110618	07/10/2025	01/10/2025 / SAM	12/17/2024 / SAM	V14724



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30042 / VOA Mix,500 series method 502.2 Calibration Std #1 gases, 2000uq/ml, PTM, 1ml	A0216826	08/27/2025	02/27/2025 / SAM	12/17/2024 / SAM	V14744
Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30042 / VOA Mix,500 series method 502.2 Calibration Std #1 gases, 2000uq/ml, PTM, 1ml	A0216826	05/31/2031	01/10/2025 / SAM	12/17/2024 / SAM	V14754
Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555408 / Custom Standard, Vinyl Acetate Standard w/ Grav [CS 5066-6] TWO SEPARATE LOTS	A0220471	07/10/2025	01/10/2025 / SAM	01/08/2025 / SAM	V14809
Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	555408 / Custom Standard, Vinyl Acetate Standard w/ Grav [CS 5066-6] TWO SEPARATE LOTS	A0220471	07/10/2025	01/10/2025 / SAM	01/08/2025 / SAM	V14814
Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30470 / VOA Stock Solution, tert-butanol std, 1mL, P&TM	A0217535	08/27/2025	02/27/2025 / SAM	01/21/2025 / SAM	V14842
Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	021325	03/13/2025	02/14/2025 / SAM	02/14/2025 / SAM	V14872



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	021325	03/13/2025	02/14/2025 / SAM	02/14/2025 / SAM	V14873
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	021325	03/13/2025	02/14/2025 / SAM	02/14/2025 / SAM	V14874
Absolute Standards, Inc.	91980 / Acrolin Std (Min = 5)	021325	03/13/2025	02/14/2025 / SAM	02/14/2025 / SAM	V14875
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis



Material No.: 9077-02
Batch No.: 23I0762004
Manufactured Date: 2023-08-11
Expiration Date: 2026-08-10
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.5 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.01
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms


For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

A handwritten signature in black ink.

Ken Koehnlein
Sr. Manager, Quality Assurance

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis

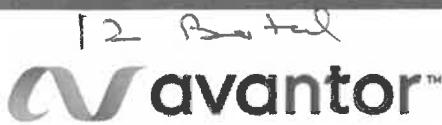

Material No.: 9077-02
Batch No.: 22L0562016
Manufactured Date: 2022-10-26
Expiration Date: 2025-10-25
Revision No.: 0

Certificate of Analysis


Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Ethier
Vice President Global Quality

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis

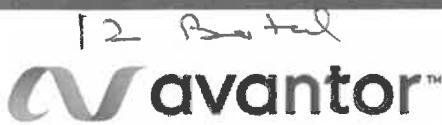

Material No.: 9077-02
Batch No.: 22L0562016
Manufactured Date: 2022-10-26
Expiration Date: 2025-10-25
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titrable Acid (μeq/g)	≤ 0.3	0.2
Titrable Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Ethier
Vice President Global Quality



5/14



CERTIFIED WEIGHT REPORT

Part Number: 91980
Lot Number: 021325
Description: Acrolein

Solvent(s): Water Lot# 072324Q

V14872 +
V14876

Expiration Date: 031325
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration ($\mu\text{g/mL}$): 5000
NIST Test ID#: 6UTB


5E-05 Balance Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0 0.001 Flask Uncertainty

<i>[Signature]</i>	021325
Formulated By:	Anthony Mahoney
<i>[Signature]</i>	021325
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information (Solvent Safety Info. On Attached pg.)		
										CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05178	5011.8	52.6	107-02-8	0.1 ppm	orl-rat 46mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Column: Vocol (60m X 0.25mm ID X 1.5 μm film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C (Time 2 = 8.75 min.) Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately Long term storage is not recommended. Please contact our technical department if further information is required.

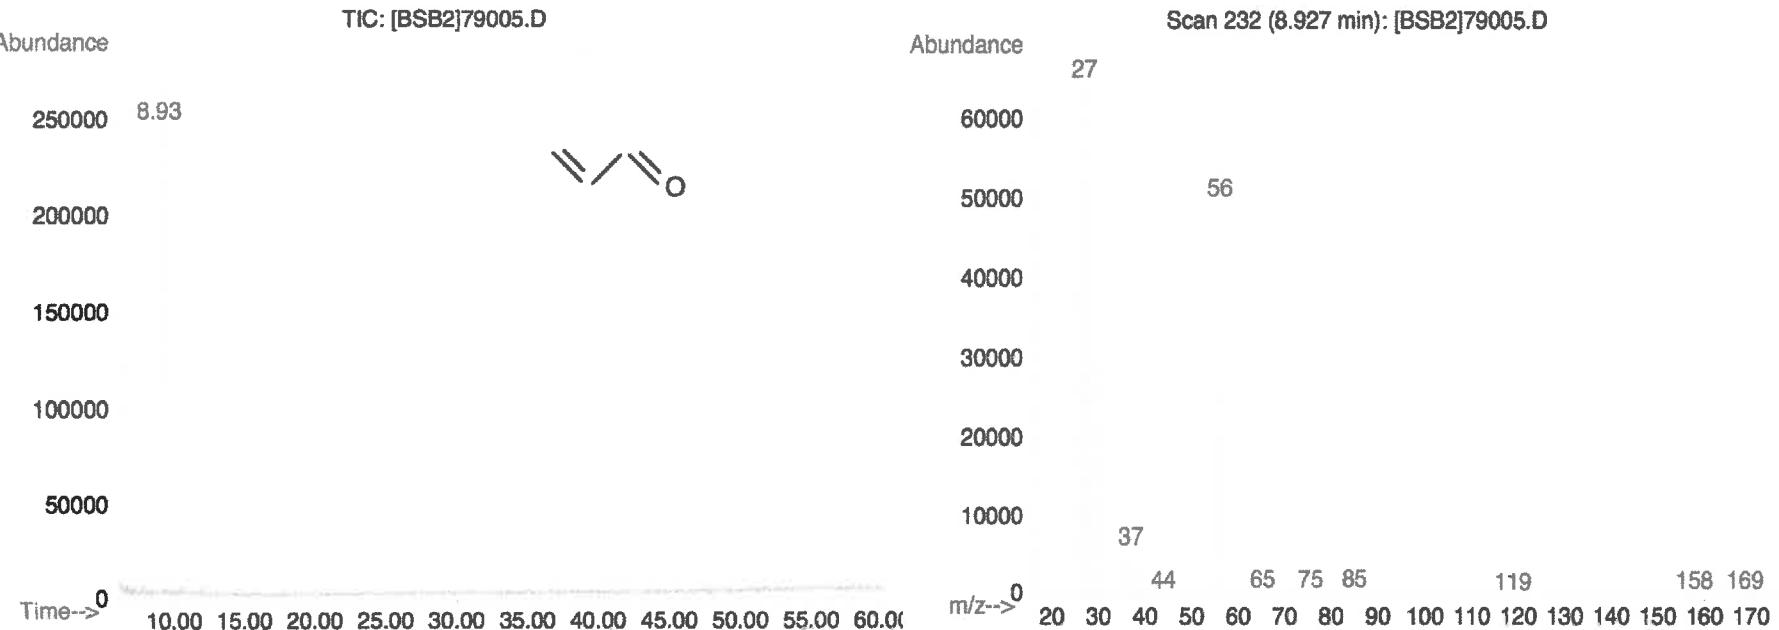

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS) GHS/OSHA Compliant**Section I Product and Company Identification****IDENTITY ANALYTICAL STANDARD DISSOLVED IN WATER**

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International	1-352-323-3500
		Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification**GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)**

P271	Use in ventilated area	H315	Causes skin and eye irritation.
P302,332	If on skin, wash with soap and water	P280	Use gloves, eye protection/face shield
		P305,351,338	If in eyes, remove contacts, rinse with water

**Signal Word: DANGER****Section III - Composition**

Components (Specific Chemical Identity; Common Name(s))	CAS#: 7732-18-5	% (optional) > 97
Water		

See Certified Weight Report For Other Analytes Present At Trace Quantities.**INTENDED USE: REFERENCE MATERIAL****Section IV. FIRST AID MEASURES**

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.
Hazardous Decomposition products	Carbon oxides

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Water	CAS#: 7732-18-5	TWA: 500 ppm
-------	-----------------	--------------

Personal protective equipment	Respiratory protection	Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.		

Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS

Boiling Point	100°C	Specific Gravity (H ₂ O = 1)	1
Vapor Pressure (mm Hg)		Melting Point	

Vapor Density (AIR = 1)	NA	Evaporation rate (Butyl Acetate = 1)	0°C
Solubility in Water	Completely miscible		NA

Appearance and Odor CLEAR, COLORLESS LIQUID WITH SLIGHT CHEMICAL ODOR.

Section X. STABILITY AND REACTIVITY

Chemical stability Stable under recommended storage conditions.
 Possibility of hazardous reactions NA
 Conditions to avoid NA
 Materials to avoid NA
 Hazardous decomposition products - No data available

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - Rat NA
 LC50 Inhalation - Rat NA
 LD50 Dermal - Guinea pig NA
 Causes skin irritation.
 Eye irritation

Section XII. ECOLOGICAL INFORMATION

LC50 NA
 EC50 NA

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US) Not dangerous goods Proper shipping name: Water	IATA Not dangerous goods Proper shipping name: Water
--	--

Section XV. REGULATORY INFORMATION

SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



5/14



CERTIFIED WEIGHT REPORT

Part Number: 91980
Lot Number: 021325
Description: Acrolein

Solvent(s): Water Lot# 072324Q

V14872 +
V14876

Expiration Date: 031325
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration ($\mu\text{g/mL}$): 5000
NIST Test ID#: 6UTB


5E-05 Balance Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0 0.001 Flask Uncertainty

<i>[Signature]</i>	021325
Formulated By:	Anthony Mahoney
<i>[Signature]</i>	021325
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information (Solvent Safety Info. On Attached pg.)		
										CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05178	5011.8	52.6	107-02-8	0.1 ppm	orl-rat 46mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Column: Vocol (60m X 0.25mm ID X 1.5 μm film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C (Time 2 = 8.75 min.) Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately Long term storage is not recommended. Please contact our technical department if further information is required.

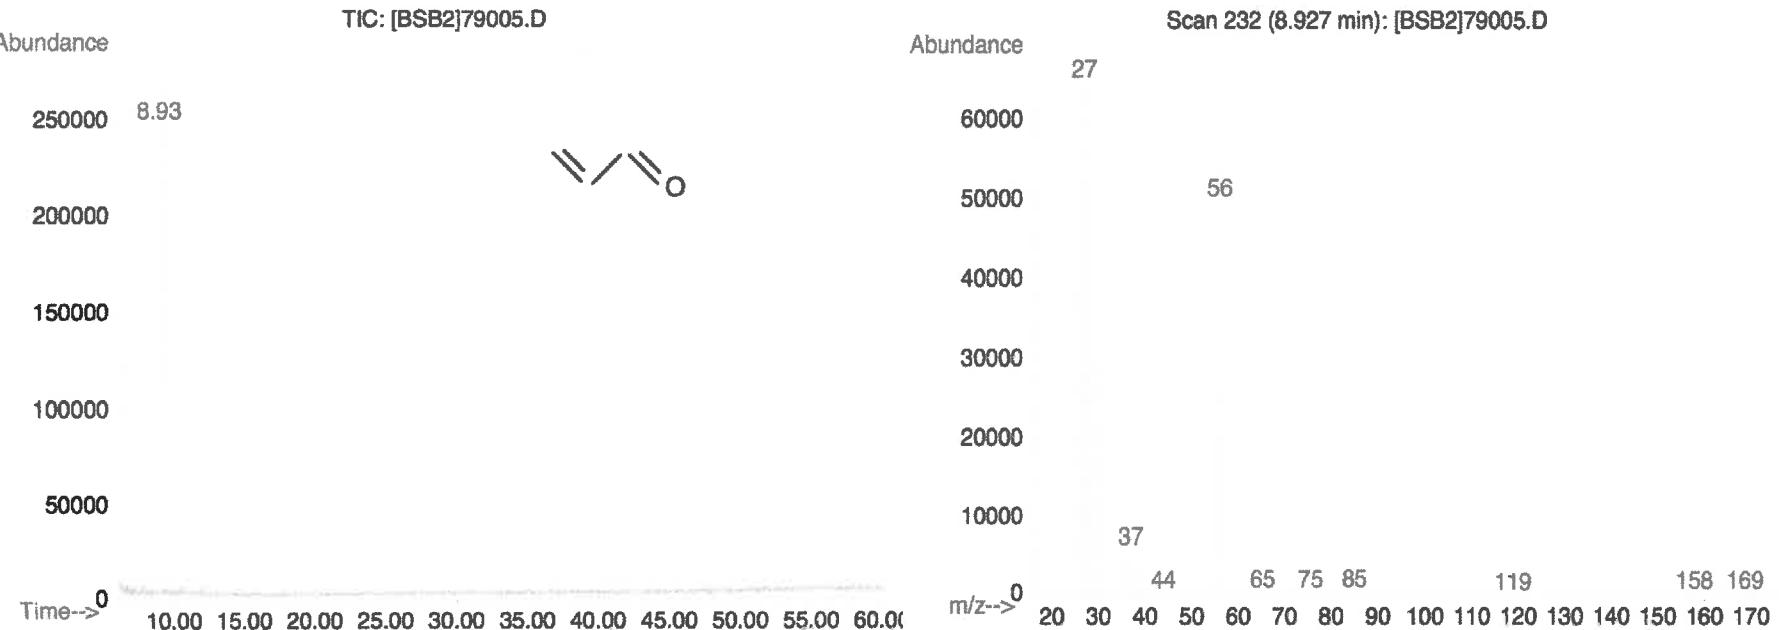

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS) GHS/OSHA Compliant**Section I Product and Company Identification****IDENTITY ANALYTICAL STANDARD DISSOLVED IN WATER**

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International	1-352-323-3500
		Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification**GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)**

P271	Use in ventilated area	H315	Causes skin and eye irritation.
P302,332	If on skin, wash with soap and water	P280	Use gloves, eye protection/face shield
		P305,351,338	If in eyes, remove contacts, rinse with water

**Signal Word: DANGER****Section III - Composition**

Components (Specific Chemical Identity; Common Name(s))	CAS#: 7732-18-5	% (optional) > 97
Water		

See Certified Weight Report For Other Analytes Present At Trace Quantities.**INTENDED USE: REFERENCE MATERIAL****Section IV. FIRST AID MEASURES**

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.
Hazardous Decomposition products	Carbon oxides

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Water	CAS#: 7732-18-5	TWA: 500 ppm
-------	-----------------	--------------

Personal protective equipment	Respiratory protection	Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.		

Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS

Boiling Point	100°C	Specific Gravity (H ₂ O = 1)	1
Vapor Pressure (mm Hg)		Melting Point	

Vapor Density (AIR = 1)	NA	Evaporation rate (Butyl Acetate = 1)	0°C
Solubility in Water	Completely miscible		NA

Appearance and Odor CLEAR, COLORLESS LIQUID WITH SLIGHT CHEMICAL ODOR.

Section X. STABILITY AND REACTIVITY

Chemical stability Stable under recommended storage conditions.
 Possibility of hazardous reactions NA
 Conditions to avoid NA
 Materials to avoid NA
 Hazardous decomposition products - No data available

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - Rat NA
 LC50 Inhalation - Rat NA
 LD50 Dermal - Guinea pig NA
 Causes skin irritation.
 Eye irritation

Section XII. ECOLOGICAL INFORMATION

LC50 NA
 EC50 NA

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US) Not dangerous goods Proper shipping name: Water	IATA Not dangerous goods Proper shipping name: Water
--	--

Section XV. REGULATORY INFORMATION

SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



5/14



CERTIFIED WEIGHT REPORT

Part Number: 91980
Lot Number: 021325
Description: Acrolein

Solvent(s): Water Lot# 072324Q

V14872 +
V14876

Expiration Date: 031325
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration ($\mu\text{g/mL}$): 5000
NIST Test ID#: 6UTB


5E-05 Balance Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0 0.001 Flask Uncertainty

<i>[Signature]</i>	021325
Formulated By:	Anthony Mahoney
<i>[Signature]</i>	021325
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information (Solvent Safety Info. On Attached pg.)		
										CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05178	5011.8	52.6	107-02-8	0.1 ppm	orl-rat 46mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Column: Vocol (60m X 0.25mm ID X 1.5 μm film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C (Time 2 = 8.75 min.) Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately Long term storage is not recommended. Please contact our technical department if further information is required.

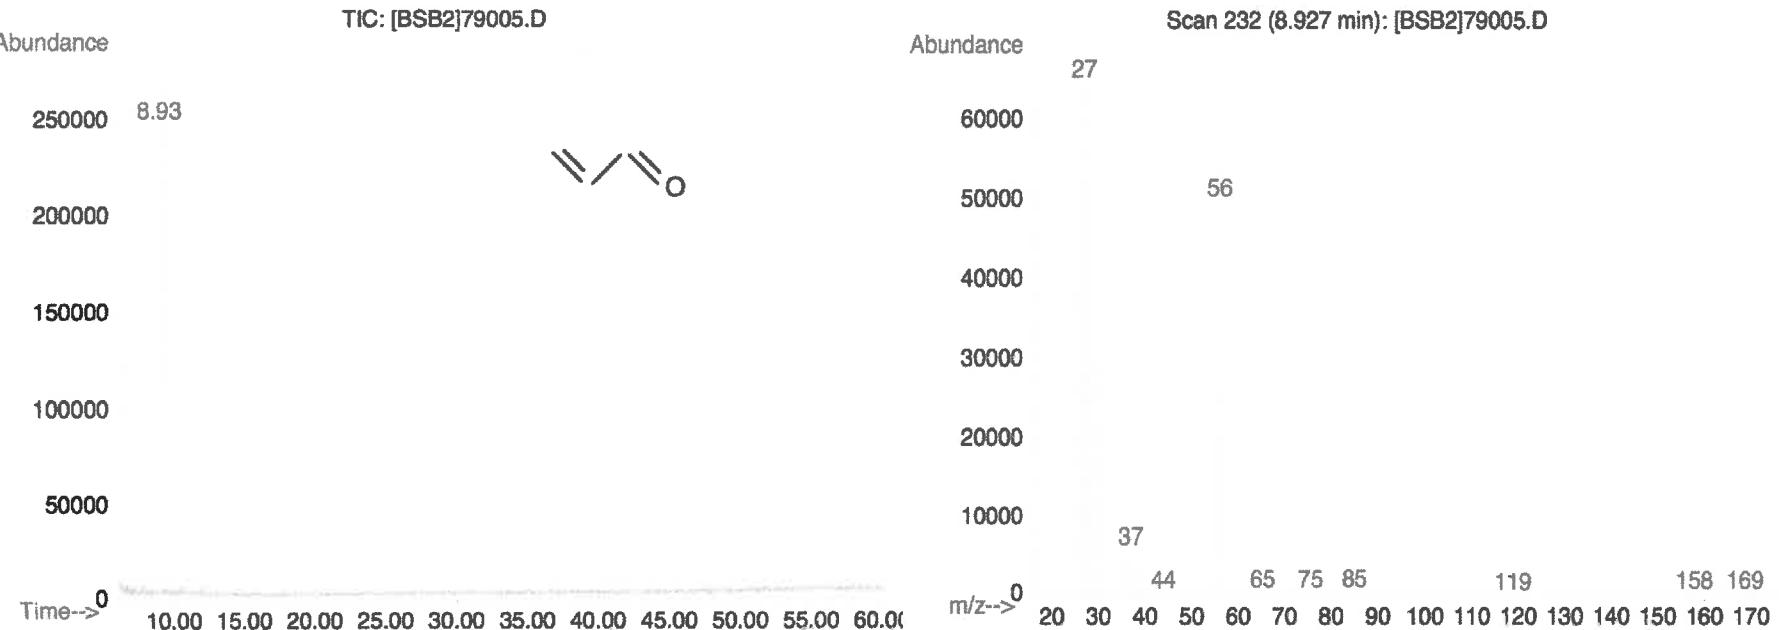

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS) GHS/OSHA Compliant**Section I Product and Company Identification****IDENTITY ANALYTICAL STANDARD DISSOLVED IN WATER**

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International	1-352-323-3500
		Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification**GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)**

P271	Use in ventilated area	H315	Causes skin and eye irritation.
P302,332	If on skin, wash with soap and water	P280	Use gloves, eye protection/face shield
		P305,351,338	If in eyes, remove contacts, rinse with water

**Signal Word: DANGER****Section III - Composition**

Components (Specific Chemical Identity; Common Name(s))	CAS#: 7732-18-5	% (optional) > 97
Water		

See Certified Weight Report For Other Analytes Present At Trace Quantities.**INTENDED USE: REFERENCE MATERIAL****Section IV. FIRST AID MEASURES**

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.
Hazardous Decomposition products	Carbon oxides

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Water	CAS#: 7732-18-5	TWA: 500 ppm
-------	-----------------	--------------

Personal protective equipment	Respiratory protection	Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.		

Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS

Boiling Point	100°C	Specific Gravity (H ₂ O = 1)	1
Vapor Pressure (mm Hg)		Melting Point	

Vapor Density (AIR = 1)	NA	Evaporation rate (Butyl Acetate = 1)	0°C
Solubility in Water	Completely miscible		NA

Appearance and Odor CLEAR, COLORLESS LIQUID WITH SLIGHT CHEMICAL ODOR.

Section X. STABILITY AND REACTIVITY

Chemical stability Stable under recommended storage conditions.
 Possibility of hazardous reactions NA
 Conditions to avoid NA
 Materials to avoid NA
 Hazardous decomposition products - No data available

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - Rat NA
 LC50 Inhalation - Rat NA
 LD50 Dermal - Guinea pig NA
 Causes skin irritation.
 Eye irritation

Section XII. ECOLOGICAL INFORMATION

LC50 NA
 EC50 NA

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US) Not dangerous goods Proper shipping name: Water	IATA Not dangerous goods Proper shipping name: Water
--	--

Section XV. REGULATORY INFORMATION

SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



5/14



CERTIFIED WEIGHT REPORT

Part Number: 91980
Lot Number: 021325
Description: Acrolein

Solvent(s): Water Lot# 072324Q

V14872 +
V14876

Expiration Date: 031325
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration ($\mu\text{g/mL}$): 5000
NIST Test ID#: 6UTB


5E-05 Balance Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0 0.001 Flask Uncertainty

<i>[Signature]</i>	021325
Formulated By: <u>Anthony Mahoney</u>	DATE
<i>[Signature]</i>	021325
Reviewed By: <u>Pedro L. Rentas</u>	DATE

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information (Solvent Safety Info. On Attached pg.)		
										CAS#	OSHA PEL (TWA)	LD50
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05178	5011.8	52.6	107-02-8	0.1 ppm	orl-rat 46mg/kg

Method: GC6MSD-1. Detector: Mass Selective Detector (Scan mode). Column: Vocol (60m X 0.25mm ID X 1.5 μm film thickness). Oven Profile: Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C (Time 2 = 8.75 min.) Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. Analyst: Pedro Rentas. NOTE: Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately Long term storage is not recommended. Please contact our technical department if further information is required.

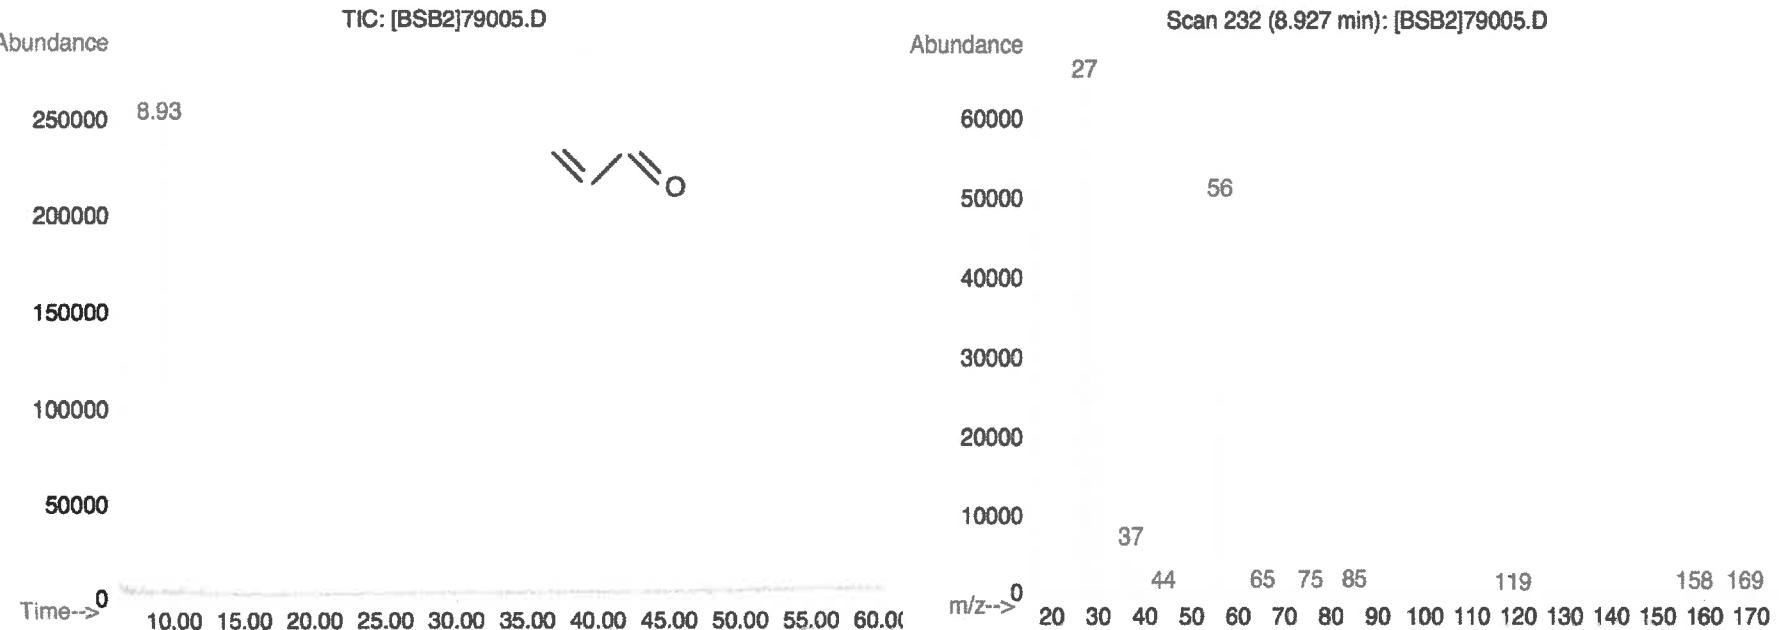

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS) GHS/OSHA Compliant**Section I Product and Company Identification****IDENTITY ANALYTICAL STANDARD DISSOLVED IN WATER**

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International	1-352-323-3500
		Date Prepared/Revised	January 1, 2024

Section II - Hazards Identification**GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)**

P271	Use in ventilated area	H315	Causes skin and eye irritation.
P302,332	If on skin, wash with soap and water	P280	Use gloves, eye protection/face shield
		P305,351,338	If in eyes, remove contacts, rinse with water

**Signal Word: DANGER****Section III - Composition**

Components (Specific Chemical Identity; Common Name(s))	CAS#: 7732-18-5	% (optional) > 97
Water		

See Certified Weight Report For Other Analytes Present At Trace Quantities.**INTENDED USE: REFERENCE MATERIAL****Section IV. FIRST AID MEASURES**

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Suitable extinguishing media	Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire	Wear self contained breathing apparatus for fire fighting if necessary.
Hazardous Decomposition products	Carbon oxides

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Water	CAS#: 7732-18-5	TWA: 500 ppm
-------	-----------------	--------------

Personal protective equipment	Respiratory protection	Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.		

Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS

Boiling Point	100°C	Specific Gravity (H ₂ O = 1)	1
Vapor Pressure (mm Hg)		Melting Point	

Vapor Density (AIR = 1)	NA	Evaporation rate (Butyl Acetate = 1)	0°C
Solubility in Water	Completely miscible		NA

Appearance and Odor CLEAR, COLORLESS LIQUID WITH SLIGHT CHEMICAL ODOR.

Section X. STABILITY AND REACTIVITY

Chemical stability Stable under recommended storage conditions.
 Possibility of hazardous reactions NA
 Conditions to avoid NA
 Materials to avoid NA
 Hazardous decomposition products - No data available

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - Rat NA
 LC50 Inhalation - Rat NA
 LD50 Dermal - Guinea pig NA
 Causes skin irritation.
 Eye irritation

Section XII. ECOLOGICAL INFORMATION

LC50 NA
 EC50 NA

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US) Not dangerous goods Proper shipping name: Water	IATA Not dangerous goods Proper shipping name: Water
--	--

Section XV. REGULATORY INFORMATION

SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



CERTIFIED WEIGHT REPORT

Part Number: 95317
 Lot Number: 021624
 Description: Universal VOA Megamix

69 components

Expiration Date: 021627

Recommended Storage: Freezer (0 °C)

Nominal Concentration (µg/mL): 2000

NIST Test ID#: 8UTB

5E-05 Balance Uncertainty

Weight(s) shown below were combined and diluted to (mL):

100.0

0.021

Flask Uncertainty

Solvent(s): Lot#
 Methanol EG359-USQ12

P. Chauhan 021624
 Formulated By: Prashant Chauhan DATE

P. L. Rentas 021624

Reviewed By: Pedro L. Rentas DATE

Compound	(RM#)	Lot Number	Dil. Factor	Initial Vol. (mL)	Initial Conc.(µg/mL)	Nominal Conc. (µg/mL)	Purity (%)	Purity Uncertainty	Pipette (mL.)	Target Weight(g)	Actual Weight(g)	Actual Conc. (µg/mL)	Expanded Uncertainty (±) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)
	Part Number													CAS# OSHA PEL (TWA) LD50
1. Acetonitrile	(0324)	021644	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20020	2001.3	8.1	75-05-8 40 ppm (70mg/m³/8H) or-lab 2460mg/kg
2. Allyl chloride (3-Chloropropene)	(0325)	102395	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	107-05-1 1 ppm (3mg/m³/8H) or-lab 700mg/kg
3. Carbon disulphide	(0460)	MKCBR0581	NA	NA	NA	2000	99.99	0.2	NA	0.20007	0.20023	2001.6	8.1	75-15-0 4 ppm (12mg/m³/8H)(skin) or-lab 1200mg/kg
4. cis-1,4-Dichloro-2-butene	(1168)	14718EF	NA	NA	NA	2000	95	0.2	NA	0.21058	0.21069	2001.1	8.5	1478-11-5 N/A N/A
5. trans-1,4-Dichloro-2-butene	(0488)	MKCBP041V	NA	NA	NA	2000	96.5	0.2	NA	0.20731	0.20748	2001.7	8.4	110-57-6 N/A N/A
6. Diethyl ether	(0153)	HK10CAS000C	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	60-29-7 N/A N/A
7. Ethyl methacrylate	(0361)	06128PX	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20230	2002.3	8.2	97-63-2 N/A or-lab 14800mg/kg
8. Iodomethane	(0489)	SHSF8718V	NA	NA	NA	2000	99.5	0.2	NA	0.20106	0.20121	2001.5	8.2	74-88-4 5 ppm (28mg/m³/8H)(skin) or-lab 76mg/kg
9. 2-Methyl-1-propanol	(0445)	15241EB	NA	NA	NA	2000	98.5	0.2	NA	0.20106	0.20120	2001.4	8.1	78-83-1 60 ppm (15mg/m³/8H) or-lab 240mg/kg
10. Methylacrylonitrile	(0442)	00427ET	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	126-98-7 1 ppm (3mg/m³/8H)(skin) or-lab 120mg/kg
11. Methyl acrylate	(1075)	SHBK0679	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20040	2001.5	8.1	96-33-3 10 ppm (35mg/m³/8H)(skin) or-lab 277mg/kg
12. Methyl methacrylate	(0404)	MKBW5137V	NA	NA	NA	2000	99.9	0.2	NA	0.20025	0.20041	2001.6	8.1	60-62-6 100 ppm (610mg/m³/8H) or-lab 7873mg/kg
13. Nitrobenzene	(0228)	01213TV	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20220	2001.3	8.2	66-95-3 1 ppm (3mg/m³/8H)(skin) or-lab 780mg/kg
14. 2-Nitropropane	(0461)	14002JX	NA	NA	NA	2000	97.3	0.2	NA	0.20560	0.20577	2001.6	8.3	79-46-9 10 ppm (35mg/m³/8H) or-lab 720mg/kg
15. Pentachloroethane	(0450)	HGA01	NA	NA	NA	2000	98	0.2	NA	0.20413	0.20430	2001.8	8.3	76-01-7 N/A N/A
16. 1,1,2-Trichlorotrifluoroethane	(0474)	18930	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20225	2001.8	8.2	76-13-1 1000 ppm (7800mg/m³/8H) or-lab 43kg/kg
17. Bromodichloromethane	35171	101623	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1998.6	22.9	75-27-4 50 ppm (28mg/m³/8H) or-lab 70mg/kg
18. Dibromochloromethane	35171	101823	0.05	6.00	40002.1	2000	NA	NA	0.017	NA	NA	1999.6	23.0	124-48-1 N/A or-lab 84mg/kg
19. cis-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	158-59-2 N/A N/A
20. trans-1,2-Dichloroethene	35171	101623	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.6	22.9	75-09-2 500 ppm or-lab 820mg/kg
21. Methylene chloride	35171	101623	0.05	5.00	40002.8	2000	NA	NA	0.017	NA	NA	1999.6	23.0	158-90-5 N/A or-lab 1235mg/kg
22. 1,1-Dichloroethene	32251	102023	0.10	10.00	20001.6	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-25-2 1 ppm (4mg/m³/8H)(skin) or-lab 200mg/kg
23. Bromform	95321	020724	0.10	10.00	20003.2	2000	NA	NA	0.042	NA	NA	1999.8	20.4	58-23-5 0.5 ppm (5mg/m³/8H)(skin) or-lab 933mg/kg
24. Carbon tetrachloride	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	594-20-7 2 ppm (12.5mg/m³/8H) or-lab 2550mg/kg
25. Chlorform	95321	020724	0.10	10.00	20024.0	2000	NA	NA	0.042	NA	NA	2001.9	20.5	87-88-3 50 ppm (240mg/m³/8H) or-lab 908mg/kg
26. Dibromomethane	95321	020724	0.10	10.00	20002.8	2000	NA	NA	0.042	NA	NA	1999.8	20.5	74-95-3 N/A or-lab 108mg/kg
27. 1,1-Dichloroethane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	107-08-2 50 ppm (8mg/m³/8H) or-lab 870mg/kg
28. 2,2-Dichloropropane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	126-95-5 100 ppm or-lab 725mg/kg
29. Tetrachloroethene	95321	020724	0.10	10.00	20201.1	2000	NA	NA	0.042	NA	NA	2019.6	20.6	127-18-4 26 ppm (170mg/m³/8H)(final) or-lab 2639mg/kg
30. 1,1,1-Trichloroethane	95321	020724	0.10	10.00	20003.0	2000	NA	NA	0.042	NA	NA	1999.8	20.5	71-55-6 350 ppm (1900mg/m³/8H) or-lab 10300mg/kg
31. 1,2-Dibromo-3-chloropropane	35181	112322	0.05	5.00	40165.5	2000	NA	NA	0.017	NA	NA	2000.3	22.9	96-12-8 0.001 ppm or-lab 170mg/kg
32. 1,2-Dimethoxyethane	35181	112322	0.05	5.00	40024.8	2000	NA	NA	0.017	NA	NA	2000.7	22.9	106-93-4 20 ppm (8H) or-lab 108mg/kg
33. 1,2-Dichloroethane	35181	112322	0.05	5.00	4018.0	2000	NA	NA	0.017	NA	NA	2000.4	22.9	107-08-2 50 ppm (8H) or-lab 870mg/kg
34. 1,2-Dichloropropane	35181	112322	0.05	5.00	40051.0	2000	NA	NA	0.017	NA	NA	2002.0	22.9	78-87-5 75 ppm (350mg/m³/8H)(skin) or-lab 1947mg/kg
35. 1,3-Dichloropropane	35181	112322	0.05	5.00	40005.9	2000	NA	NA	0.017	NA	NA	1999.8	22.8	142-28-9 N/A or-lab 3500mg/kg
36. 1,1-Dichloropropene	35181	112322	0.05	5.00	40012.1	2000	NA	NA	0.017	NA	NA	2000.1	29.7	563-58-6 N/A N/A
37. cis-1,3-Dichloropropene	35181	112322	0.05	5.00	40101.0	2000	NA	NA	0.017	NA	NA	2000.0	23.0	10081-01-5 N/A N/A
38. trans-1,3-Dichloropropene	35181	112322	0.05	5.00	40017.8	2000	NA	NA	0.017	NA	NA	2000.4	23.0	10081-02-6 N/A N/A
39. Hexachloro-1,3-butadiene	35181	112322	0.05	5.00	40219.1	2000	NA	NA	0.017	NA	NA	2000.6	29.7	87-68-3 0.02 ppm (0.24mg/m³/8H) or-lab 82mg/kg
40. 1,1,2-Tetrachloroethane	35181	112322	0.05	5.00	40011.9	2000	NA	NA	0.017	NA	NA	2000.1	22.9	630-20-6 N/A or-lab 870mg/kg
41. 1,1,2-Tetrachloroethane	35181	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	1999.9	22.9	79-34-5 5 ppm (35mg/m³/8H)(skin) or-lab 800mg/kg
42. 1,1,2-Trichloroethane	35181	112322	0.05	5.00	40006.6	2000	NA	NA	0.017	NA	NA	1999.6	23.0	79-00-5 10 ppm (460mg/m³/8H)(skin) or-lab 870mg/kg
43. Trichloroethene	35181	112322	0.05	5.00	40029.0	2000	NA	NA	0.017	NA	NA	2000.9	22.9	79-01-6 50 ppm (270mg/m³/8H) or-lab 240mg/kg
44. 1,2,3-Trichloropropane	35181	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	1999.9	22.9	98-18-4 10 ppm (60mg/m³/8H) or-lab 149mg/kg
45. Benzene	35182	050823	0.05	5.00	40005.0	2000	NA	NA	0.017	NA	NA	1999.7	22.9	71-43-2 1 ppm or-lab 494mg/kg
46. Bromobenzene	35182	050823	0.05	5.00	40006.9	2000	NA	NA	0.017	NA	NA	1999.8	22.9	109-88-1 N/A or-lab 2100mg/kg
47. n-Butyl benzene	35182	050823	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	104-51-8 N/A N/A
48. Ethyl benzene	35182	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-41-4 100 ppm (435mg/m³/8H) or-lab >2000mg/kg
49. p-Isopropyl toluene	35182	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	89-87-6 N/A or-lab 4750mg/kg
50. Naphthalene	35182	050823	0.05	5.00	40006.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	91-20-3 10 ppm (50mg/m³/8H) or-lab 400mg/kg
51. Styrene	35182	050823	0.05	5.00	40004.6	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-42-5 100 ppm or-lab 5000mg/kg
52. Toluene	35182	050823	0.05	5.00	40006.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-88-3 200 ppm or-lab 5000mg/kg
53. 1,2,3-Trichlorobenzene	35182	050823	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	87-81-6 N/A or-lab 1360mg/kg
54. 1,2,4-Trichlorobenzene	35182	050823	0.05	5.00	40006.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	120-82-1 5 ppm (CL) (40mg/m³) or-lab 750mg/kg
55. 1,2,4-Trimethylbenzene	35182	050823	0.05	5.00	40001.8	2000	NA	NA	0.017	NA	NA	1999.8	23.0	95-63-6 N/A or-lab 5kg
56. 1,3,5-Trimethylbenzene	35182	050823	0.05	5.00	40006.7	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-57-8 N/A or-lab 5000mg/kg
57. m-Xylene	35182	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-38-3 100 ppm (435mg/m³/8H) or-lab 5kg
58. <i>tert</i> -Butyl benzene	35183	101923	0.05	5.00	40001.2	2000	NA	NA	0.017	NA	NA	1999.8	22.8	88-06-8 N/A or-lab 5kg
59. <i>sec</i> -Butyl benzene	35183	101923	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.6	22.8	135-98-8 N/A or-lab 5kg
60. Chlorobenzene	35183	101923	0.05	5.00	40003.8	2000	NA	NA	0.017					



Run 16, "P95317 L021624 [2000µg/mL in MeOH]"

Run Length: 60.00 min, 35998 points at 10 points/second.

Created: Sat, Feb 17, 2024 at 8:56:46 AM.

Sampled: Sequence "021624-GC5M1", Method "GC5-M1".

Analyzed using Method "GC5-M1".

Comments

GC5-M1 Analysis by Candice Warren

Column ID SPB-Vocel 105 meter X 0.53mm X 3.0µm film thickness

Flow rates: Total flow=290mL/min., Helium (carrier)=10mL/min.,


Helium(make-up)=10mL/min., Hydrogen(make-up)=40mL/min., Air(make-up)=230mL/min.

Oven Profile: Temp. 1=35°C (Time 1=10 min.), Temp 2=200°C (Time 2=8.75 min.).

Rate = 4°C/min., Total run time=60 min. Injector temp.=200°C, FID Temp.=200°C.

FID Signal = Edaq Channel 1

Standard injection = 0.5µL, Range=3

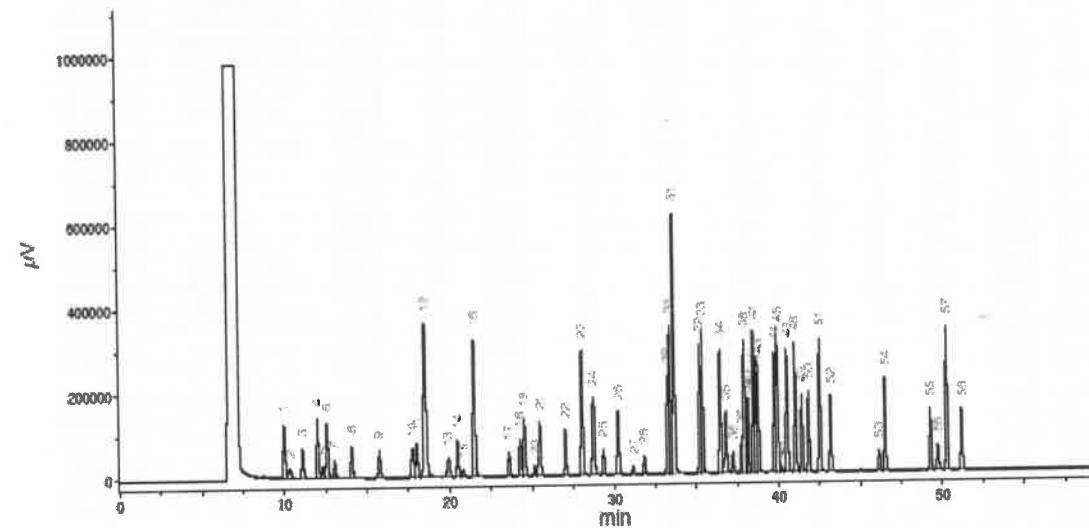

Peak #	Name	FID RT (min.)
1	Ether	0.07
2	1,1,2-Trichloro-1,2-difluoroethane	10.33
3	1,1-Dichloroethane	11.10
4	Acrylonitrile	12.40
5	Iodomethane	12.31
6	Allyl chloride	12.56
7	Carbon disulfide/Methylene chloride	13.04
8	trans-1,2-Dichloroethene	14.07
9	1,1-Dichloroethane	15.74
10	2,2-Dichloropropane	17.74
11	cis-1,2-Dichloroethane	18.00
12	Methyl acrylate/Methyl acrylate/Chloroform	18.49
13	Isobutane/1,1,1-Trifluoroethane	19.01
14	1,1-Dichloropropane	20.46
15	Carbon tetrachloride	20.79
16	Benzene/1,2-Dichloroethane	21.49
17	Trichloroethene	23.59
18	1,2-Dichloropropene	24.28
19	Methyl methacrylate	24.53
20	Bromoethane/bromethane	25.11
21	Dibromomethane/2-Nitropropane	25.46
22	cis-1,3-Dichloropropene	27.03
23	Toluene	28.05
24	Ethylnitropropane/trans-1,2-Dichloropropene	28.73
25	1,1,2-Trichloroethane	29.24
26	Tetrahydroethene/1,3-Dichloropropene	30.24
27	Dibromochloromethane	31.16
28	1,2-Dibromoethane	31.84
29	Chlorobenzene	33.26
30	Ethylbenzene/1,1,1,2-Tetrachloroethane	33.40
31	m-Xylene/p-Xylene	33.86
32	o-Xylene	35.22
33	Styrene	35.39
34	Isopropylbenzene/Bromoform	36.18
35	cis-1,4-Dichloro-2-butene	36.80
36	1,1,2,2-Tetrachloroethane	37.23
37	1,2,3-Trichloropropene	37.77
38	n-Propylbenzene	37.93
39	trans-1,4-Dichloro-3-butene	38.05
40	Bromobenzene	38.14
41	1,2,5-Trimethylbenzene	38.80
42	2-Chlorotoluene	38.83
43	4-Chlorotoluene	38.77
44	tert-Butylbenzene	39.76
45	1,2,4-Trimethylbenzene	39.91
46	Perfumebenzene	40.17
47	sec-Butylbenzene	40.57
48	p-Isopropylbenzene	41.02
49	1,3-Dichlorobenzene	41.83
50	1,4-Dichlorobenzene	42.53
51	n-Butylbenzene	43.18
52	1,2-Dichlorobenzene	43.18
53	1,2-Dibromo-3-chloropropane	46.12
54	Acrylonitrile	46.46
55	1,2,4-Trichlorobenzene	49.26
56	Hexachlorobutadiene	49.72
57	Naphthalene	50.26
58	1,2,3-Trichlorobenzenes	51.16

Safety Data Sheet (SDS) GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2023

Section II - Hazards Identification

GHS Classification In accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, Inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302+332	If on skin, wash with soap and water	P305+351+338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact Wash with soap and water. Consult a physician.
In case of eye contact Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol 67-56-1 TWA 200 ppm
Skin notation TWA 200 ppm
Potential for skin absorption , ingestion and inhalation.
Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6

Solubility in Water COMPLETE

Appearance and Odor CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.

Section X. STABILITY AND REACTIVITY

Chemical stability Stable under recommended storage conditions.
 Possibility of hazardous reactions Vapours may form explosive mixture with air.
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
 LC50 Inhalation - rat - 4 h - 64000 ppm
 LD50 Dermal - rabbit - 15,800 mg/kg
 Toxic if absorbed through skin. Causes skin irritation.
 Eye damage/eye irritation
 Toxic if inhaled. Causes respiratory tract irritation.
 Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
 EC50 24,500.00 mg/l - 48 h
 EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)
 UN number: 1230 Class: 3 Packing group: II
 Proper shipping name: Methanol

IATA	UN number: 1230 Class: 3 Packing group: II
Proper shipping name:	Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



CERTIFIED WEIGHT REPORT

Part Number: 95317
 Lot Number: 021624
 Description: Universal VOA Megamix

69 components

Expiration Date: 021627

Recommended Storage: Freezer (0 °C)

Nominal Concentration (µg/mL): 2000

NIST Test ID#: 8UTB

Weight(s) shown below were combined and diluted to (mL):

100.0 0.021 Flask Uncertainty

Solvent(s): Lot#
 Methanol EG359-USQ12

P. Chauhan 021624
 Formulated By: Prashant Chauhan DATE

P. L. Rentas 021624

Reviewed By: Pedro L. Rentas DATE

Compound	(R#)	Lot	Dil.	Initial Vol. (mL)	Initial Conc.(µg/mL)	Nominal Conc. (µg/mL)	Purity (%)	Purity Uncertainty	Pipette (mL.)	Target Weight(g)	Actual Weight(g)	Actual Conc. (µg/mL)	Expanded Uncertainty (±) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)
	Part Number	Number	Factor											CAS# OSHA PEL (TWA) LD50
1. Acetonitrile	(0324)	021644	NA	NA	NA	2000	98.99	0.2	NA	0.20007	0.20020	2001.3	8.1	75-05-8 40 ppm (70mg/m³/8H) orl-rat 2460mg/kg
2. Allyl chloride (3-Chloropropene)	(0325)	102395	NA	NA	NA	2000	98	0.2	NA	0.20207	0.20221	2001.4	8.2	107-05-1 1 ppm (3mg/m³/8H) orl-rat 700mg/kg
3. Carbon disulphide	(0460)	MKCBR0581	NA	NA	NA	2000	98.99	0.2	NA	0.20007	0.20023	2001.6	8.1	75-15-0 4 ppm (12mg/m³/8H) (skin) orl-rat 1200mg/kg
4. cis-1,4-Dichloro-2-butene	(1168)	14718EF	NA	NA	NA	2000	95	0.2	NA	0.21058	0.21069	2001.1	8.5	1478-11-5 N/A N/A
5. trans-1,4-Dichloro-2-butene	(0488)	MKCBP041V	NA	NA	NA	2000	96.5	0.2	NA	0.20731	0.20748	2001.7	8.4	110-57-6 N/A N/A
6. Diethyl ether	(0153)	HK10CAS000C	NA	NA	NA	2000	98.9	0.2	NA	0.20025	0.20040	2001.5	8.1	60-29-7 N/A N/A
7. Ethyl methacrylate	(0361)	06128PX	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20230	2002.3	8.2	97-63-2 N/A orl-rat 14800mg/kg
8. Iodomethane	(0489)	SHSF8718V	NA	NA	NA	2000	99.5	0.2	NA	0.20106	0.20121	2001.5	8.2	74-88-4 5 ppm (28mg/m³/8H) (skin) orl-rat 76mg/kg
9. 2-Methyl-1-propanol	(0445)	15241EB	NA	NA	NA	2000	98.5	0.2	NA	0.20106	0.20120	2001.4	8.1	78-83-1 60 ppm (15mg/m³/8H) orl-rat 240mg/kg
10. Methylacrylonitrile	(0442)	00427ET	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20221	2001.4	8.2	126-98-7 1 ppm (3mg/m³/8H) (skin) orl-rat 120mg/kg
11. Methyl acrylate	(1075)	SHBK0679	NA	NA	NA	2000	98.9	0.2	NA	0.20025	0.20040	2001.5	8.1	96-33-3 10 ppm (35mg/m³/8H) (skin) orl-rat 277mg/kg
12. Methyl methacrylate	(0404)	MKBW5137V	NA	NA	NA	2000	98.9	0.2	NA	0.20025	0.20041	2001.6	8.1	60-62-6 100 ppm (610mg/m³/8H) orl-rat 787mg/kg
13. Nitrobenzene	(0228)	01213TV	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20220	2001.3	8.2	66-95-3 1 ppm (5mg/m³/8H) (skin) orl-rat 780mg/kg
14. 2-Nitropropane	(0461)	14002JX	NA	NA	NA	2000	97.3	0.2	NA	0.20560	0.20577	2001.6	8.3	79-46-9 10 ppm (35mg/m³/8H) orl-rat 720mg/kg
15. Pentachloroethane	(0450)	HGA01	NA	NA	NA	2000	98	0.2	NA	0.20413	0.20430	2001.8	8.3	76-01-7 N/A N/A
16. 1,1,2-Trichlorotrifluoroethane	(0474)	18930	NA	NA	NA	2000	99	0.2	NA	0.20207	0.20225	2001.8	8.2	76-13-1 1000 ppm (7800mg/m³/8H) orl-rat 43kg/kg
17. Bromodichloromethane	35171	101623	0.05	5.00	40001.7	2000	NA	NA	0.017	NA	NA	1986.6	22.9	75-27-4 N/A orl-rat 916mg/kg
18. Dibromochloromethane	35171	101823	0.05	6.00	40002.1	2000	NA	NA	0.017	NA	NA	1999.6	23.0	124-48-1 N/A orl-rat 848mg/kg
19. cis-1,2-Dichloroethene	35171	101623	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	158-59-2 N/A N/A
20. trans-1,2-Dichloroethene	35171	101623	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.6	22.9	75-09-2 500 ppm orl-rat 820mg/kg
21. Methylene chloride	35171	101623	0.05	5.00	40002.8	2000	NA	NA	0.017	NA	NA	1999.6	23.0	158-90-5 N/A orl-rat 1235mg/kg
22. 1,1-Dichloroethene	32251	102023	0.10	10.00	20001.6	2000	NA	NA	0.042	NA	NA	1999.8	20.5	75-25-2 1 ppm (4mg/m³/8H) (skin) orl-rat 200mg/kg
23. Bromform	95321	020724	0.10	10.00	20003.2	2000	NA	NA	0.042	NA	NA	1999.8	20.4	58-23-5 0.5 ppm (5mg/m³/8H) (skin) orl-rat 933mg/kg
24. Carbon tetrachloride	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.4	594-20-7 2 ppm (12.5mg/m³/8H) orl-rat 250mg/kg
25. Chlorform	95321	020724	0.10	10.00	20024.0	2000	NA	NA	0.042	NA	NA	2001.9	20.5	87-88-3 50 ppm (240mg/m³/8H) (CL) orl-rat 908mg/kg
26. Dibromomethane	95321	020724	0.10	10.00	20002.8	2000	NA	NA	0.042	NA	NA	1999.8	20.5	74-95-3 N/A orl-rat 108mg/kg
27. 1,1-Dichloroethane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	107-08-2 50 ppm (8mg/m³/8H) orl-rat 870mg/kg
28. 2,2-Dichloropropane	95321	020724	0.10	10.00	20003.4	2000	NA	NA	0.042	NA	NA	1999.8	20.5	126-95-5 100 ppm orl-rat 725mg/kg
29. Tetrachloroethene	95321	020724	0.10	10.00	20201.1	2000	NA	NA	0.042	NA	NA	2019.6	20.6	127-18-4 26 ppm (170mg/m³/8H) (final) orl-rat 2629mg/kg
30. 1,1,1-Trichloroethane	95321	020724	0.10	10.00	20003.0	2000	NA	NA	0.042	NA	NA	1999.8	20.5	71-55-6 350 ppm (1900mg/m³/8H) orl-rat 10300mg/kg
31. 1,2-Dibromo-3-chloropropane	35181	112322	0.05	5.00	40165.5	2000	NA	NA	0.017	NA	NA	2000.3	22.9	96-12-8 0.001 ppm orl-rat 170mg/kg
32. 1,2-Dichloroethane	35181	112322	0.05	5.00	40024.8	2000	NA	NA	0.017	NA	NA	2000.7	22.9	106-93-4 20 ppm (8H) orl-rat 108mg/kg
33. 1,2-Dichloroethane	35181	112322	0.05	5.00	4018.0	2000	NA	NA	0.017	NA	NA	2000.4	22.9	107-08-2 50 ppm (8H) orl-rat 870mg/kg
34. 1,2-Dichloropropane	35181	112322	0.05	5.00	40051.0	2000	NA	NA	0.017	NA	NA	2002.0	22.9	78-87-5 75 ppm (35mg/m³/8H) (skin) orl-rat 1947mg/kg
35. 1,3-Dichloropropane	35181	112322	0.05	5.00	40005.9	2000	NA	NA	0.017	NA	NA	1999.8	22.8	142-28-9 N/A un-rms 3500mg/kg
36. 1,1-Dichloropropene	35181	112322	0.05	5.00	40012.1	2000	NA	NA	0.017	NA	NA	2000.1	29.7	563-58-6 N/A N/A
37. cis-1,3-Dichloropropene	35181	112322	0.05	5.00	40101.0	2000	NA	NA	0.017	NA	NA	2000.0	23.0	10081-01-5 N/A N/A
38. trans-1,3-Dichloropropene	35181	112322	0.05	5.00	40017.8	2000	NA	NA	0.017	NA	NA	2000.4	23.0	10081-02-6 N/A N/A
39. Hexachloro-1,3-butadiene	35181	112322	0.05	5.00	40021.9	2000	NA	NA	0.017	NA	NA	2000.6	29.7	87-68-3 0.02 ppm (0.24mg/m³/8H) orl-rat 82mg/kg
40. 1,1,2-Tetrachloroethane	35181	112322	0.05	5.00	40011.9	2000	NA	NA	0.017	NA	NA	2000.1	22.9	630-20-6 N/A orl-rat 870mg/kg
41. 1,1,2-Tetrachloroethane	35181	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	1999.9	22.9	79-34-5 5 ppm (35mg/m³/8H) (skin) orl-rat 800mg/kg
42. 1,1,2-Trichloroethane	35181	112322	0.05	5.00	40006.6	2000	NA	NA	0.017	NA	NA	1999.6	23.0	79-00-5 10 ppm (46mg/m³/8H) (skin) orl-rat 830mg/kg
43. Trichloroethene	35181	112322	0.05	5.00	40029.0	2000	NA	NA	0.017	NA	NA	2000.9	22.9	79-01-6 50 ppm (270mg/m³/8H) orl-rms 240mg/kg
44. 1,2,3-Trichloropropane	35181	112322	0.05	5.00	40007.5	2000	NA	NA	0.017	NA	NA	1999.9	22.9	98-18-4 10 ppm (60mg/m³/8H) orl-rat 149mg/kg
45. Benzene	35182	050823	0.05	5.00	40005.0	2000	NA	NA	0.017	NA	NA	1999.7	22.9	71-43-2 1 ppm orl-rat 469mg/kg
46. Bromobenzene	35182	050823	0.05	5.00	40006.9	2000	NA	NA	0.017	NA	NA	1999.8	22.9	109-98-1 N/A orl-rat 210mg/kg
47. n-Butyl benzene	35182	050823	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	104-51-8 N/A N/A
48. Ethyl benzene	35182	050823	0.05	5.00	40004.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	99-41-4 100 ppm (435mg/m³/8H) orl-rat >2000mg/kg
49. p-Isopropyl toluene	35182	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	89-87-6 N/A orl-rat 4750mg/kg
50. Naphthalene	35182	050823	0.05	5.00	40006.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	91-20-3 10 ppm (50mg/m³/8H) orl-rat 400mg/kg
51. Styrene	35182	050823	0.05	5.00	40004.6	2000	NA	NA	0.017	NA	NA	1999.7	22.9	100-42-5 100 ppm orl-rat 5000mg/kg
52. Toluene	35182	050823	0.05	5.00	40006.2	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-88-3 200 ppm orl-rat 5000mg/kg
53. 1,2,3-Trichlorobenzene	35182	050823	0.05	5.00	40003.1	2000	NA	NA	0.017	NA	NA	1999.7	22.9	87-81-6 N/A ipr-mus 1360mg/kg
54. 1,2,4-Trichlorobenzene	35182	050823	0.05	5.00	40006.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	120-82-1 5 ppm (CL) (40mg/m³) orl-rat 750mg/kg
55. 1,2,4-Trimethylbenzene	35182	050823	0.05	5.00	40001.8	2000	NA	NA	0.017	NA	NA	1999.8	23.0	95-63-6 N/A orl-rat 5kg/kg
56. 1,3,5-Trimethylbenzene	35182	050823	0.05	5.00	40006.7	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-57-8 N/A orl-rat 5000mg/kg
57. m-Xylene	35182	050823	0.05	5.00	40005.8	2000	NA	NA	0.017	NA	NA	1999.8	22.9	108-39-3 100 ppm (435mg/m³/8H) orl-rat 5kg/kg
58. <i>tert</i> -Butyl benzene	35183	101923	0.05	5.00	40001.2	2000	NA	NA	0.017	NA	NA	1999.8	22.8	88-06-8 N/A orl-rat 5kg/kg
59. <i>sec</i> -Butyl benzene	35183	101923	0.05	5.00	40002.4	2000	NA	NA	0.017	NA	NA	1999.6	22.8	135-98-8 N/A orl-rat 5kg/kg
60. Chlorobenzene	35183	101923	0.05	5.00	40003.8	2000	NA	NA	0.017	NA	NA	1999.7	22.9	106



Run 16, "P95317 L021624 [2000µg/mL in MeOH]"

Run Length: 60.00 min, 35998 points at 10 points/second.

Created: Sat, Feb 17, 2024 at 8:56:46 AM.

Sampled: Sequence "021624-GC5M1", Method "GC5-M1".

Analyzed using Method "GC5-M1".

Comments

GC5-M1 Analysis by Candice Warren

Column ID SPB-Vocel 105 meter X 0.53mm X 3.0µm film thickness

Flow rates: Total flow=290mL/min., Helium (carrier)=10mL/min.,


Helium(make-up)=10mL/min., Hydrogen(make-up)=40mL/min., Air(make-up)=230mL/min.

Oven Profile: Temp. 1=35°C (Time 1=10 min.), Temp 2=200°C (Time 2=8.75 min.).

Rate = 4°C/min., Total run time=60 min. Injector temp.=200°C, FID Temp.=200°C.

FID Signal = Edaq Channel 1

Standard injection = 0.5µL, Range=3

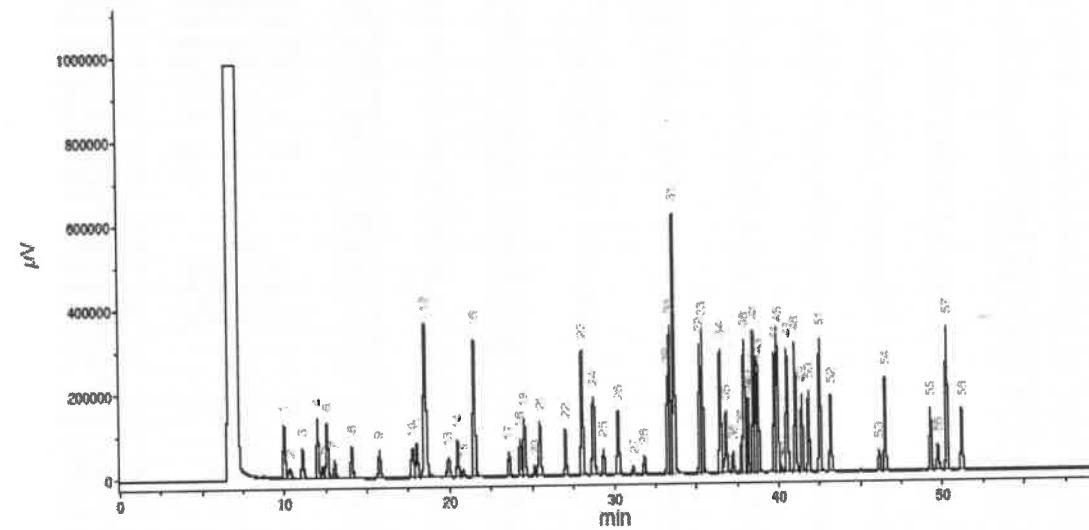

Peak #	Name	FID RT (min.)
1	Ether	0.07
2	1,1,2-Trichloro-1,2-difluoroethane	10.33
3	1,1-Dichloroethane	11.10
4	Acrylonitrile	12.40
5	Iodomethane	12.31
6	Allyl chloride	12.56
7	Carbon disulfide/Methylene chloride	13.04
8	trans-1,2-Dichloroethene	14.07
9	1,1-Dichloroethane	15.74
10	2,2-Dichloropropane	17.74
11	cis-1,2-Dichloroethane	18.00
12	Methyl acrylate/Methyl acrylate/Chloroform	18.49
13	Isobutane/1,1,1-Trifluoroethane	19.01
14	1,1-Dichloropropane	20.46
15	Carbon tetrachloride	20.79
16	Benzene/1,2-Dichloroethane	21.49
17	Trichloroethene	23.59
18	1,2-Dichloropropene	24.28
19	Methyl methacrylate	24.53
20	Bromoethane/bromethane	25.11
21	Dibromomethane/2-Nitropropane	25.46
22	cis-1,3-Dichloropropene	27.03
23	Toluene	28.05
24	Ethylnitropropane/trans-1,2-Dichloropropene	28.73
25	1,1,2-Trichloroethane	29.24
26	Tetrahydroethene/1,3-Dichloropropene	30.24
27	Dibromochloromethane	31.16
28	1,2-Dibromoethane	31.84
29	Chlorobenzene	33.26
30	Ethylbenzene/1,1,1,2-Tetrachloroethane	33.40
31	m-Xylene/p-Xylene	33.86
32	o-Xylene	35.22
33	Styrene	35.39
34	Isopropylbenzene/Bromoform	36.18
35	cis-1,4-Dichloro-2-butene	36.80
36	1,1,2,2-Tetrachloroethane	37.23
37	1,2,3-Trichloropropene	37.77
38	n-Propylbenzene	37.93
39	trans-1,4-Dichloro-3-butene	38.05
40	Bromobenzene	38.14
41	1,2,5-Trimethylbenzene	38.80
42	2-Chlorotoluene	38.83
43	4-Chlorotoluene	38.77
44	tert-Butylbenzene	39.76
45	1,2,4-Trimethylbenzene	39.91
46	Perfumebenzene	40.17
47	sec-Butylbenzene	40.57
48	p-Tropylbenzene	41.02
49	1,3-Dichlorobenzene	41.83
50	1,4-Dichlorobenzene	42.53
51	n-Butylbenzene	43.18
52	1,2-Dichlorobenzene	43.18
53	1,2-Dibromo-3-chloropropane	46.12
54	Acrylonitrile	46.46
55	1,2,4-Trichlorobenzene	49.26
56	Hexachlorobutadiene	49.72
57	Naphthalene	50.26
58	1,2,3-Trichlorobenzenes	51.16

Safety Data Sheet (SDS) GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2023

Section II - Hazards Identification

GHS Classification In accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, Inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302+332	If on skin, wash with soap and water	P305+351+338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol 67-56-1 TWA 200 ppm
Skin notation TWA 200 ppm
Potential for skin absorption , ingestion and inhalation.
Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

Section IX - Physical/Chemical Characteristics

Boiling Point	65°C	Specific Gravity (H ₂ O = 1)	0.79
Vapor Pressure (mm Hg)	96	Melting Point	-98°C
Vapor Density (AIR = 1)	1.11	Evaporation rate (Butyl Acetate = 1)	4.6

Solubility in Water COMPLETE

Appearance and Odor CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.

Section X. STABILITY AND REACTIVITY

Chemical stability Stable under recommended storage conditions.
 Possibility of hazardous reactions Vapours may form explosive mixture with air.
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
 LC50 Inhalation - rat - 4 h - 64000 ppm
 LD50 Dermal - rabbit - 15,800 mg/kg
 Toxic if absorbed through skin. Causes skin irritation.
 Eye damage/eye irritation
 Toxic if inhaled. Causes respiratory tract irritation.
 Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
 EC50 24,500.00 mg/l - 48 h
 EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US)
 UN number: 1230 Class: 3 Packing group: II
 Proper shipping name: Methanol

IATA
 UN number: 1230 Class: 3 Packing group: II
 Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Dec 09/17/24

2 Uvof

CERTIFIED WEIGHT REPORT

Part Number: 91980
 Lot Number: 091424
 Description: Acrolein


 Expiration Date: 101424
 Recommended Storage: Refrigerate (4 °C)
 Nominal Concentration ($\mu\text{g/mL}$): 5000
 NIST Test ID#: 6UTB
 Weight(s) shown below were combined and diluted to (mL): 10.0

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

091424	DATE
Formulated By: Justin Dippold	
091424	DATE
Reviewed By: Pedro L. Rentas	

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information		
										(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05175	5008.9	52.5	107-02-8	0.1 ppm	orl-rat 46mg/kg

Method: GC6MSD-1. **Detector:** Mass Selective Detector (Scan mode). **Column:** Vocol (60m X 0.25mm ID X 1.5 μm film thickness). **Oven Profile:** Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C (Time 2 = 8.75 min.).
 Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. **Analyst:** Pedro Rentas. **NOTE:** Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately.
 Long term storage is not recommended. Please contact our technical department if further information is required.

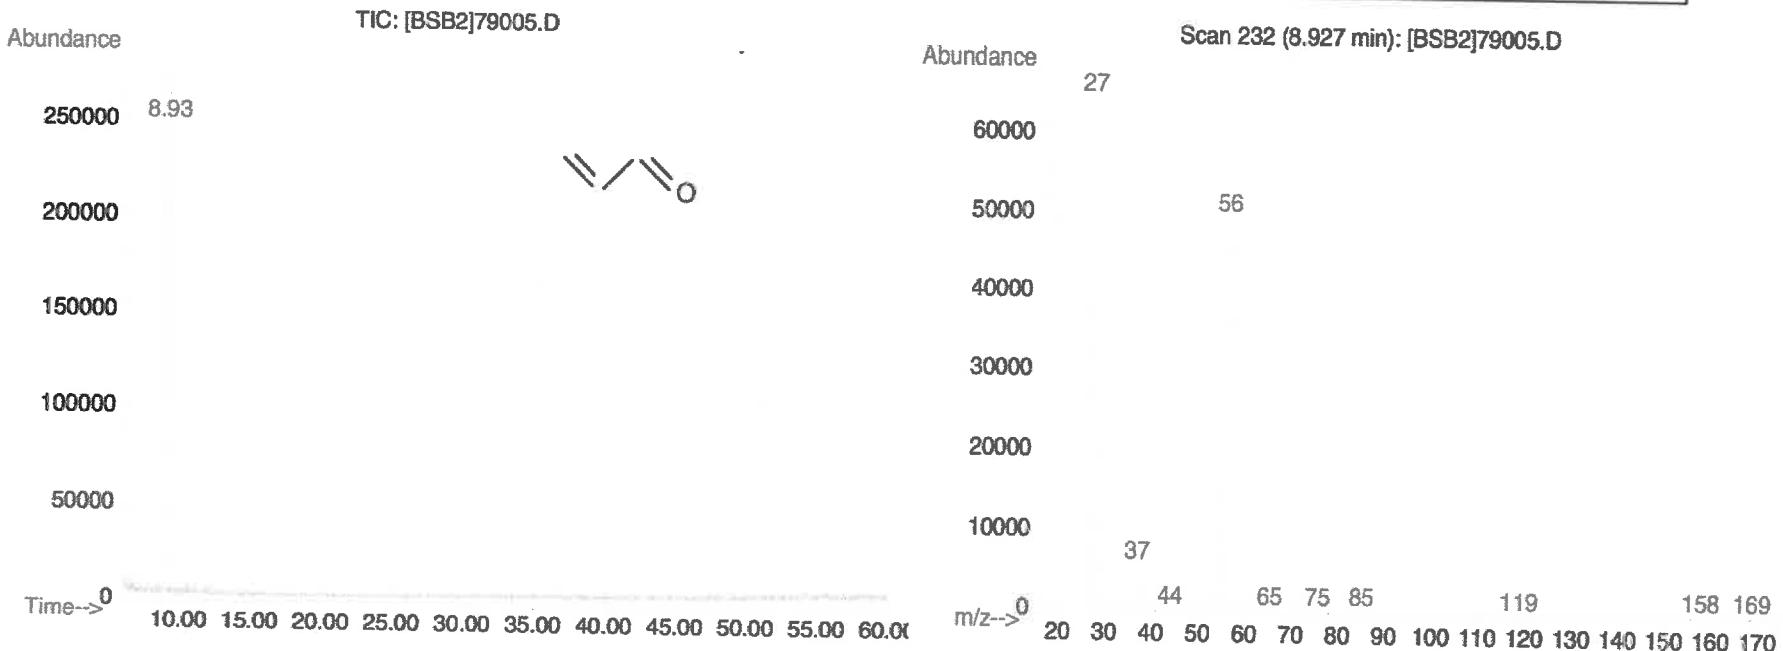

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5 % of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Dec 09/17/24

2 Uvof

CERTIFIED WEIGHT REPORT

Part Number: 91980
 Lot Number: 091424
 Description: Acrolein


 Expiration Date: 101424
 Recommended Storage: Refrigerate (4 °C)
 Nominal Concentration ($\mu\text{g/mL}$): 5000
 NIST Test ID#: 6UTB
 Weight(s) shown below were combined and diluted to (mL): 10.0

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

091424	DATE
Formulated By: Justin Dippold	
091424	DATE
Reviewed By: Pedro L. Rentas	

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight(g)	Actual Weight(g)	Actual Conc ($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information		
										(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)
1. Acrolein	5	103755V10F	5000	97	0.5	0.05166	0.05175	5008.9	52.5	107-02-8	0.1 ppm	orl-rat 46mg/kg

Method: GC6MSD-1. **Detector:** Mass Selective Detector (Scan mode). **Column:** Vocol (60m X 0.25mm ID X 1.5 μm film thickness). **Oven Profile:** Temp. 1 = 35°C (Time 1 = 10min.), Temp. 2=200°C (Time 2 = 8.75 min.).
 Rate = 4°C/min., Injector Temp. = 200°C, Detector Temp. = 220°C. **Analyst:** Pedro Rentas. **NOTE:** Due to the instability of acrolein in solution, all solutions of acrolein, and any dilutions thereof, should be used immediately.
 Long term storage is not recommended. Please contact our technical department if further information is required.

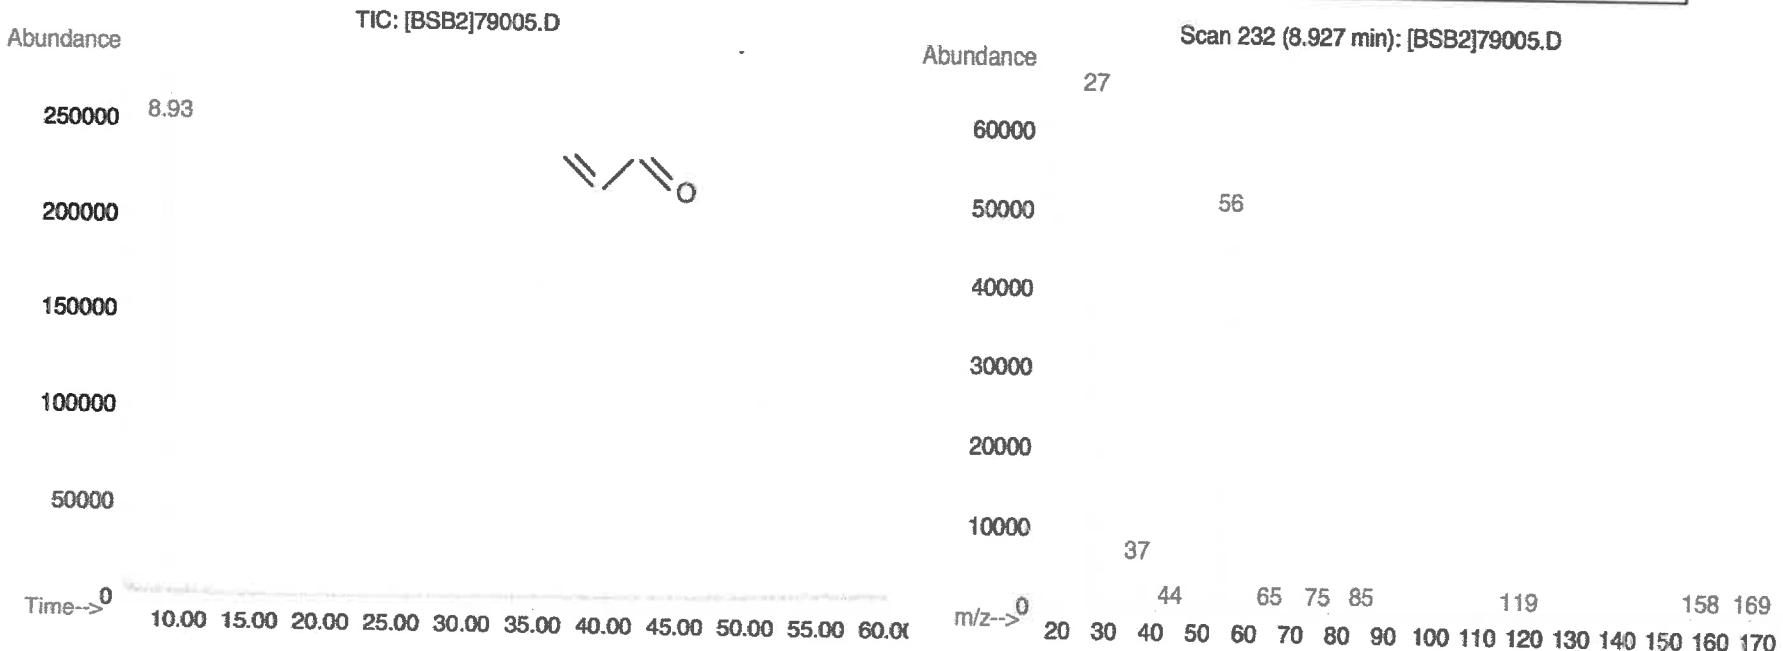

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5 % of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Rec 12/16/24

20 vial



CERTIFIED WEIGHT REPORT

Part Number: 95318
 Lot Number: 120524
 Description: 2-Chloroethyl vinyl ether

Solvent(s): Methanol
 Lot# EJ143-US

Expiration Date: 120527
 Recommended Storage: Refrigerate (4 °C)
 Nominal Concentration ($\mu\text{g/mL}$): 10000
 NIST Test ID#: 6UTB




V14630 to
V14649

Weight(s) shown below were combined and diluted to (mL): 50.0 Balance Uncertainty 5E-05
 Flask Uncertainty 0.001

<i>Prashant Chauhan</i>	120524
Formulated By:	Prashant Chauhan
<i>Pedro L. Rentas</i>	120524
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information			
										CAS#	Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	oral-rat 250mg/kg	

Method: GC6MSD-1.M. **Detector:** MSD. **Column:** (60m X 0.25mm X 1.5 μm). **Oven Profile:** Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min., Injector B Temp.= 200°C, Detector B Temp. = 220°C. **Analyst:** Candice Warren.

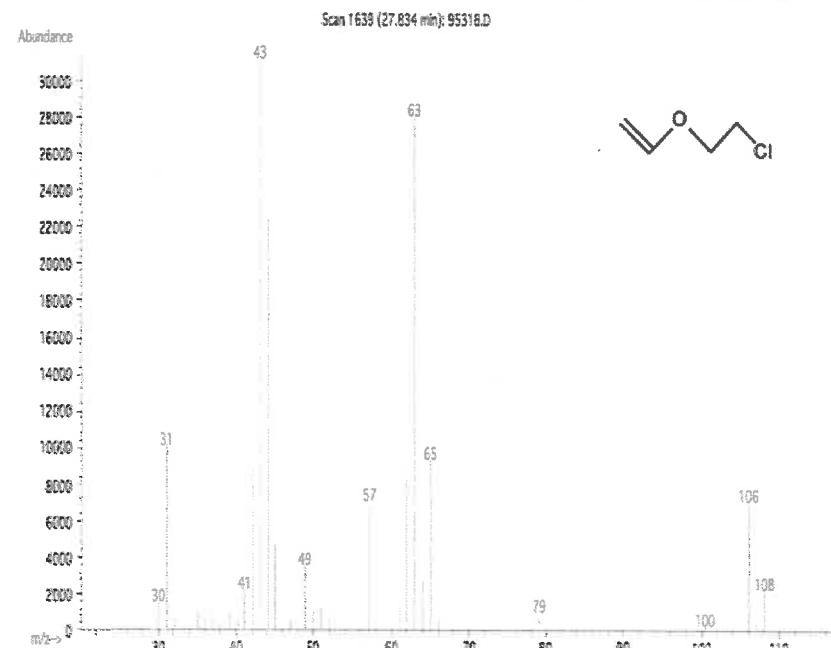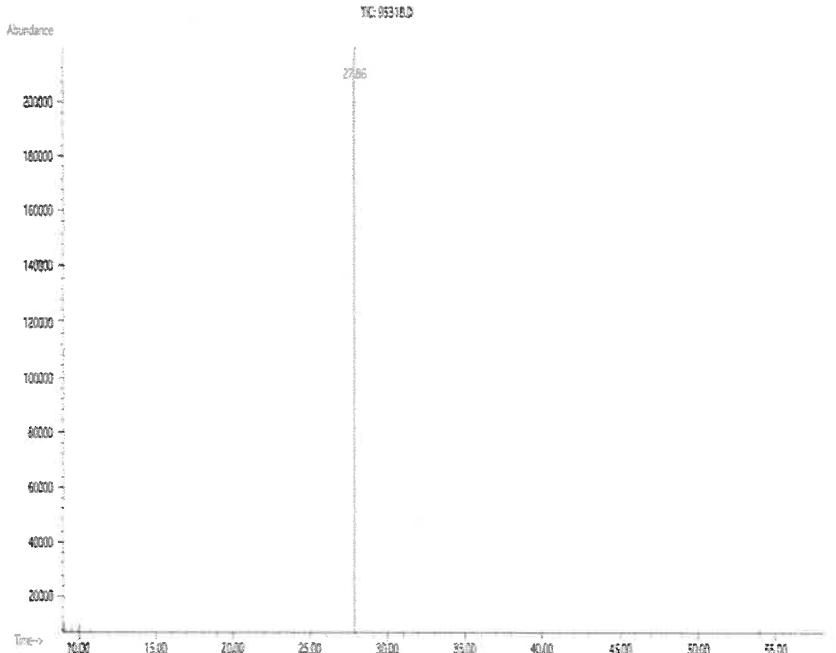

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified ($\pm 0.5\%$ of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS) GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

CAS#: 67-56-1

% (optional)
 > 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact Wash with soap and water. Consult a physician.
In case of eye contact Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol 67-56-1 TWA 200 ppm
Skin notation TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.
Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection. Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

Section IX - Physical/Chemical Characteristics

Boiling Point		Specific Gravity (H ₂ O = 1)	
Vapor Pressure (mm Hg)	65°C	Melting Point	0.79
Vapor Density (AIR = 1)	96	Evaporation rate (Butyl Acetate = 1)	-98°C
Solubility in Water	1.11		4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability Stable under recommended storage conditions.
 Possibility of hazardous reactions Vapours may form explosive mixture with air.
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
 LC50 Inhalation - rat - 4 h - 64000 ppm
 LD50 Dermal - rabbit - 15,800 mg/kg
 Toxic if absorbed through skin. Causes skin irritation.
 Eye damage/eye irritation
 Toxic if inhaled. Causes respiratory tract irritation.
 Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
 EC50 24,500.00 mg/l - 48 h
 EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US) IATA
 UN number: 1230 Class: 3 Packing group: II
 Proper shipping name: Methanol
 UN number: 1230 Class: 3 Packing group: II
 Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Rec 12/16/24

20 vial



CERTIFIED WEIGHT REPORT

Part Number: 95318
 Lot Number: 120524
 Description: 2-Chloroethyl vinyl ether

Solvent(s): Methanol
 Lot# EJ143-US

Expiration Date: 120527
 Recommended Storage: Refrigerate (4 °C)
 Nominal Concentration ($\mu\text{g/mL}$): 10000
 NIST Test ID#: 6UTB




V14630 to
V14649

Weight(s) shown below were combined and diluted to (mL): 50.0 Balance Uncertainty 5E-05
 Flask Uncertainty 0.001

<i>Prashant Chauhan</i>	120524
Formulated By:	Prashant Chauhan
<i>Pedro L. Rentas</i>	120524
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information			
										CAS#	Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	oral-rat 250mg/kg	

Method: GC6MSD-1.M. **Detector:** MSD. **Column:** (60m X 0.25mm X 1.5 μm). **Oven Profile:** Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min., Injector B Temp.= 200°C, Detector B Temp. = 220°C. **Analyst:** Candice Warren.

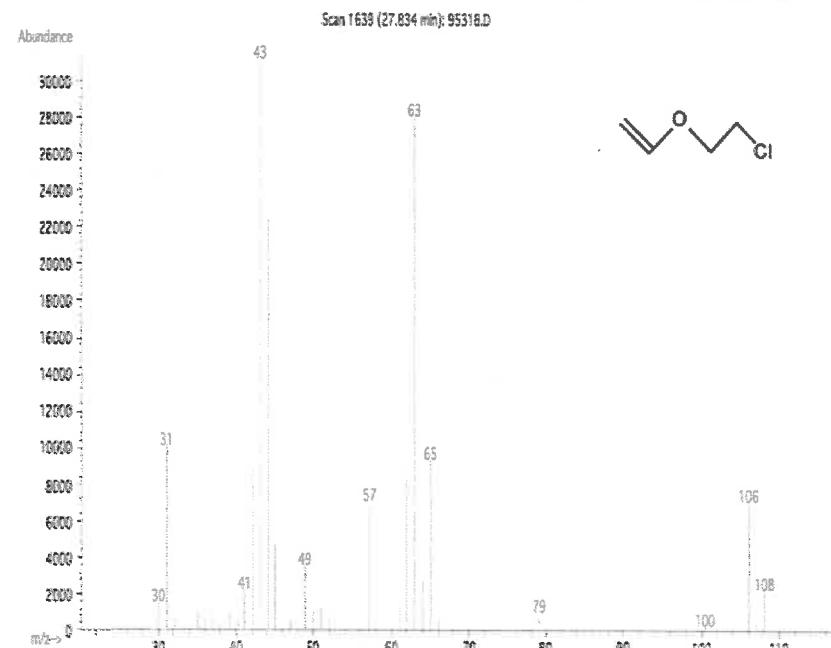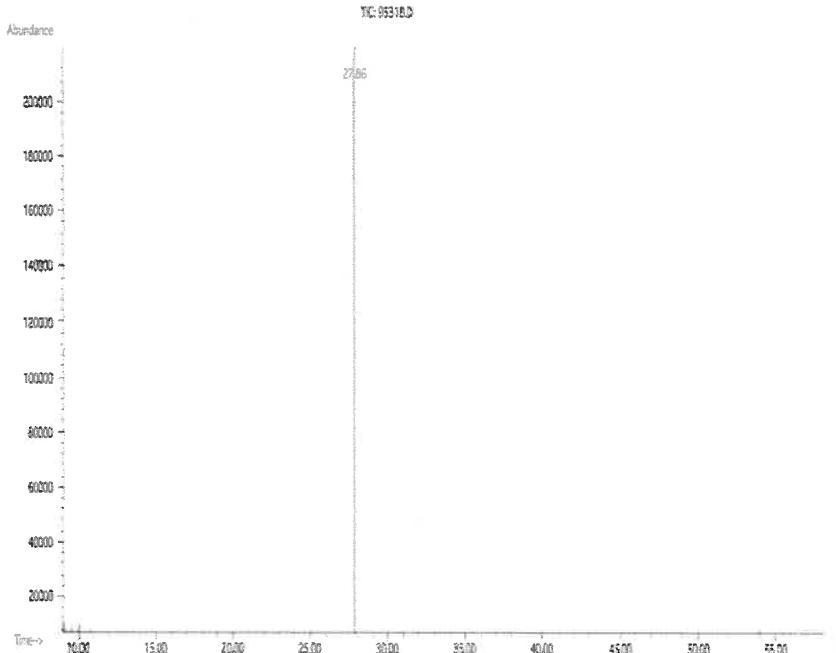

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified ($\pm 0.5\%$ of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS) GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

CAS#: 67-56-1

% (optional)
 > 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice	Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled	If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact	Wash with soap and water. Consult a physician.
In case of eye contact	Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed	Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol 67-56-1 TWA 200 ppm
Skin notation TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.
Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection. Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

Section IX - Physical/Chemical Characteristics

Boiling Point		Specific Gravity (H ₂ O = 1)	
Vapor Pressure (mm Hg)	65°C	Melting Point	0.79
Vapor Density (AIR = 1)	96	Evaporation rate (Butyl Acetate = 1)	-98°C
Solubility in Water	1.11		4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability: Stable under recommended storage conditions.
 Possibility of hazardous reactions: Vapours may form explosive mixture with air.
 Conditions to avoid: Heat, flames, sparks, extreme temperature and sunlight.
 Materials to avoid: Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
 LC50 Inhalation - rat - 4 h - 64000 ppm
 LD50 Dermal - rabbit - 15,800 mg/kg
 Toxic if absorbed through skin. Causes skin irritation.
 Eye damage/eye irritation
 Toxic if inhaled. Causes respiratory tract irritation.
 Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
 EC50 24,500.00 mg/l - 48 h
 EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US) IATA
 UN number: 1230 Class: 3 Packing group: II
 Proper shipping name: Methanol
 UN number: 1230 Class: 3 Packing group: II
 Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Rec 12/16/24

20 vial



CERTIFIED WEIGHT REPORT

Part Number: 95318
 Lot Number: 120524
 Description: 2-Chloroethyl vinyl ether

Solvent(s): Methanol
 Lot# EJ143-US

Expiration Date: 120527
 Recommended Storage: Refrigerate (4 °C)
 Nominal Concentration ($\mu\text{g/mL}$): 10000
 NIST Test ID#: 6UTB




V14630 to
V14649

Weight(s) shown below were combined and diluted to (mL): 50.0 Balance Uncertainty 5E-05
 Flask Uncertainty 0.001

<i>Prashant Chauhan</i>	120524
Formulated By:	Prashant Chauhan
<i>Pedro L. Rentas</i>	120524
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information			
										CAS#	Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	oral-rat 250mg/kg	

Method: GC6MSD-1.M. **Detector:** MSD. **Column:** (60m X 0.25mm X 1.5 μm). **Oven Profile:** Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min., Injector B Temp.= 200°C, Detector B Temp. = 220°C. **Analyst:** Candice Warren.

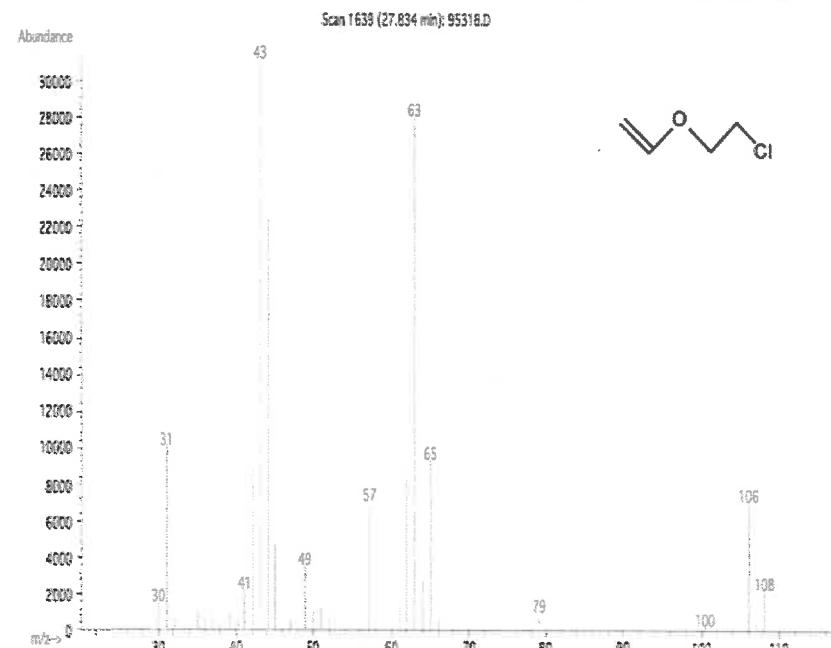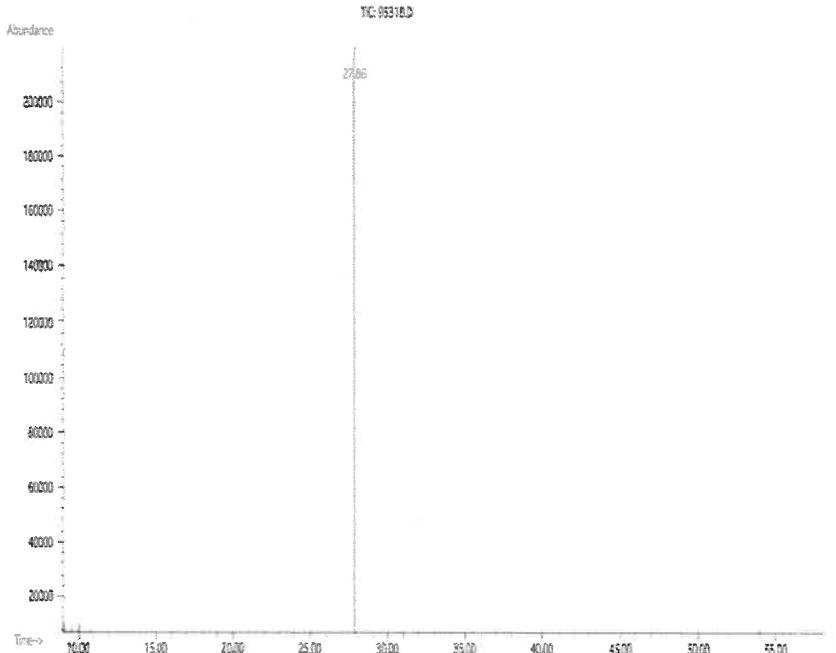

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified ($\pm 0.5\%$ of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS) GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

Components (Specific Chemical Identity; Common Name(s))
Methanol METHYL ALCOHOL

CAS#: 67-56-1

% (optional)
 > 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact Wash with soap and water. Consult a physician.
In case of eye contact Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol 67-56-1 TWA 200 ppm
Skin notation TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.
Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection. Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

Section IX - Physical/Chemical Characteristics

Boiling Point		Specific Gravity (H ₂ O = 1)	
Vapor Pressure (mm Hg)	65°C	Melting Point	0.79
Vapor Density (AIR = 1)	96	Evaporation rate (Butyl Acetate = 1)	-98°C
Solubility in Water	1.11		4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability Stable under recommended storage conditions.
 Possibility of hazardous reactions Vapours may form explosive mixture with air.
 Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.
 Materials to avoid Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
 LC50 Inhalation - rat - 4 h - 64000 ppm
 LD50 Dermal - rabbit - 15,800 mg/kg
 Toxic if absorbed through skin. Causes skin irritation.
 Eye damage/eye irritation
 Toxic if inhaled. Causes respiratory tract irritation.
 Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
 EC50 24,500.00 mg/l - 48 h
 EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US) IATA
 UN number: 1230 Class: 3 Packing group: II
 Proper shipping name: Methanol
 UN number: 1230 Class: 3 Packing group: II
 Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



Rec 12/16/24

20 vial



CERTIFIED WEIGHT REPORT

Part Number: 95318
 Lot Number: 120524
 Description: 2-Chloroethyl vinyl ether

Solvent(s): Methanol
 Lot# EJ143-US

Expiration Date: 120527
 Recommended Storage: Refrigerate (4 °C)
 Nominal Concentration ($\mu\text{g/mL}$): 10000
 NIST Test ID#: 6UTB




V14630 to
V14649

Weight(s) shown below were combined and diluted to (mL): 50.0 Balance Uncertainty 5E-05
 Flask Uncertainty 0.001

<i>Prashant Chauhan</i>	120524
Formulated By:	Prashant Chauhan
<i>Pedro L. Rentas</i>	120524
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc($\mu\text{g/mL}$)	Expanded Uncertainty (+/-) ($\mu\text{g/mL}$)	SDS Information			
										CAS#	Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50
1. 2-Chloroethyl vinyl ether	74	MKCD0033	10000	99	0.2	0.50536	0.50550	10002.9	40.5	110-75-8	N/A	oral-rat 250mg/kg	

Method: GC6MSD-1.M. **Detector:** MSD. **Column:** (60m X 0.25mm X 1.5 μm). **Oven Profile:** Temp 1 = 35°C (Time 1=10min.), Temp 2 = 200°C (Time 2=8.75 min.), Rate = 4°C/min., Injector B Temp.= 200°C, Detector B Temp. = 220°C. **Analyst:** Candice Warren.

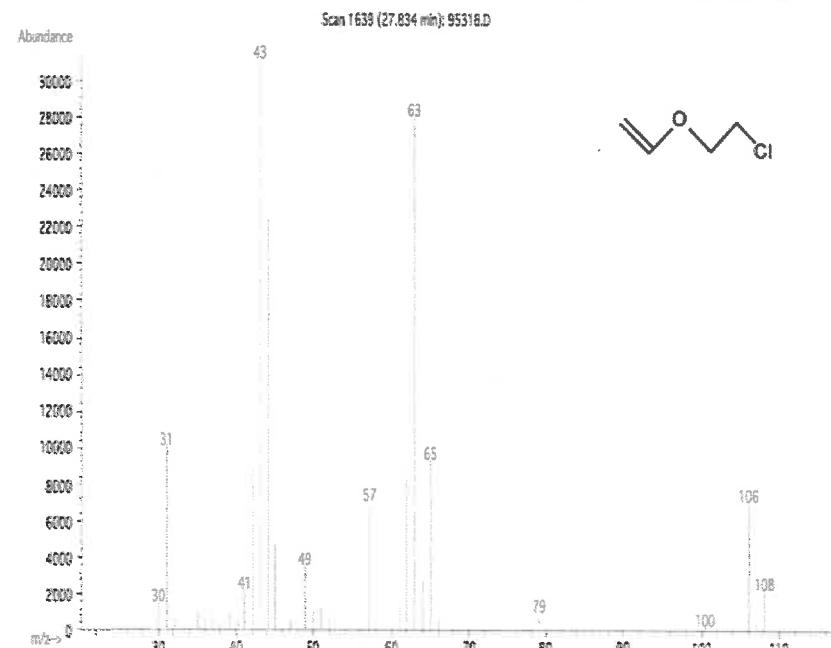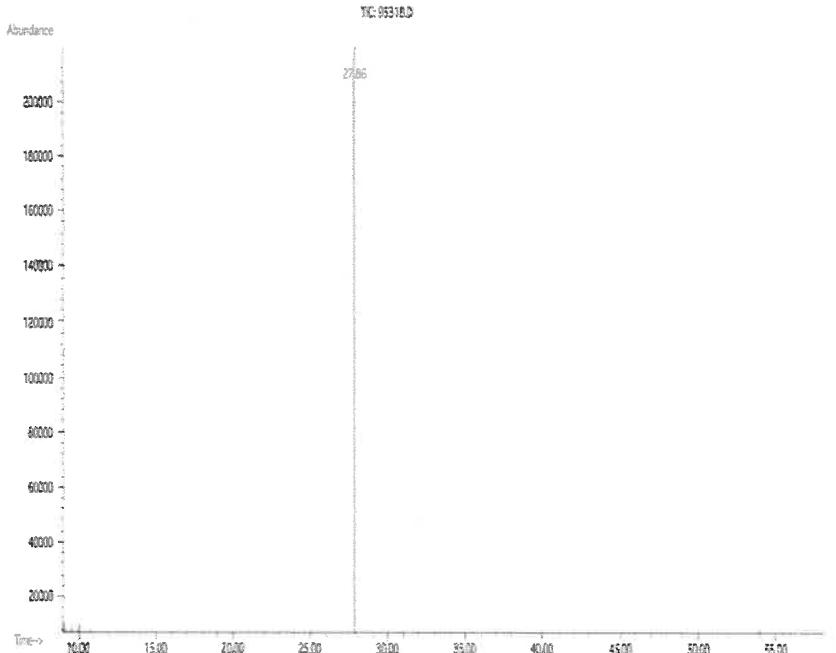

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified ($\pm 0.5\%$ of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS) GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHANOL

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rossotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2024

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H225	Highly Flammable Liquid and Vapor	H301, 311, 331	Toxic if swallowed, skin contact, inhaled
H370	Cause damage to organs	H351	Suspected of causing cancer
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: DANGER

Section III - Composition

CAS#: 67-56-1

% (optional)
 > 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.

INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact Wash with soap and water. Consult a physician.
In case of eye contact Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Flammability Flammable in the presence of a source of ignition when the temperature is above the flash point. Keep away from heat/sparks/open flame/hot surface. No smoking.
Suitable extinguishing media Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions	Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions	Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up	Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling	Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Storage Conditions	Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methanol 67-56-1 TWA 200 ppm
Skin notation TWA 200 ppm
Potential for skin absorption, ingestion and inhalation.
Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection. Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

Section IX - Physical/Chemical Characteristics

Boiling Point		Specific Gravity (H ₂ O = 1)	
Vapor Pressure (mm Hg)	65°C	Melting Point	0.79
Vapor Density (AIR = 1)	96	Evaporation rate (Butyl Acetate = 1)	-98°C
Solubility in Water	1.11		4.6
Solubility in Water	COMPLETE		
Appearance and Odor	CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.		

Section X. STABILITY AND REACTIVITY

Chemical stability: Stable under recommended storage conditions.
 Possibility of hazardous reactions: Vapours may form explosive mixture with air.
 Conditions to avoid: Heat, flames, sparks, extreme temperature and sunlight.
 Materials to avoid: Acid chlorides, Acid anhydrides, Oxidizing agents, Alkali metals, Reducing agents, Acids
 Hazardous decomposition products formed under fire conditions. - Carbon oxides

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - rat - 5,628 mg/kg
 LC50 Inhalation - rat - 4 h - 64000 ppm
 LD50 Dermal - rabbit - 15,800 mg/kg
 Toxic if absorbed through skin. Causes skin irritation.
 Eye damage/eye irritation
 Toxic if inhaled. Causes respiratory tract irritation.
 Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 5000 lbs.

LC50 15,400 mg/l - 96 h
 EC50 24,500.00 mg/l - 48 h
 EC100 10,000.00 mg/l - 24 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US) IATA
 UN number: 1230 Class: 3 Packing group: II
 Proper shipping name: Methanol
 UN number: 1230 Class: 3 Packing group: II
 Proper shipping name: Methanol

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
 SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



ILAC-MRA
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ILAC-MRA
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

Certificate of Analysis *chromatographic plus*

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30067

Lot No.: A0191805

Description : 4-Bromofluorobenzene Standard

4-Bromofluorobenzene Standard 2,500 μ g/mL, P&T Methanol,
1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : November 30, 2027

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1-Bromo-4-fluorobenzene (BFB)	460-00-4	184975	99%	2,483.9 μ g/mL	+/- 139.5488

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol


1 μ l

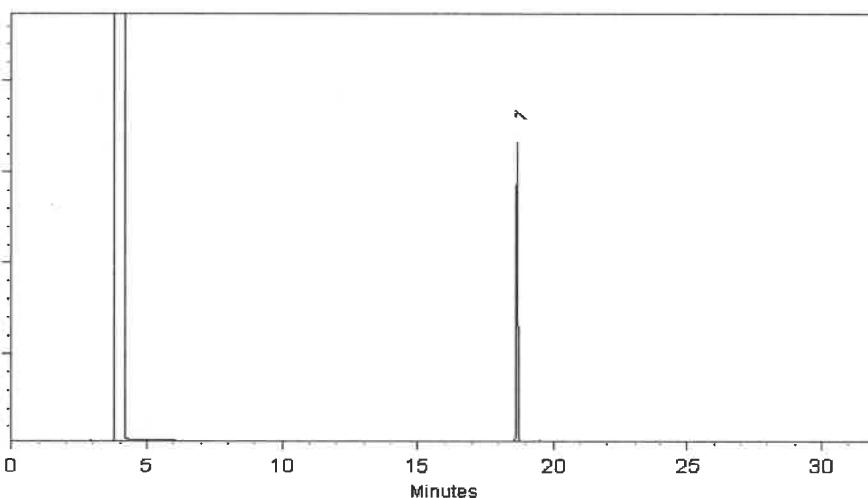

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Alicia Leathers - Operation Technician I

Date Mixed: 17-Nov-2022 Balance Serial #: B251644995


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 21-Nov-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/pECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309
www.restek.com

CERTIFIED REFERENCE MATERIAL



Certificate of Analysis

chromatographic plus

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 30225 **Lot No.:** A0193071
Description : Bromochloromethane Standard

Bromochloromethane 2000 μ g/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : December 31, 2027 **Storage:** 0°C or colder
Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	00008541	99%	2,018.0 μ g/mL	+/- 113.3890

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1 μ l

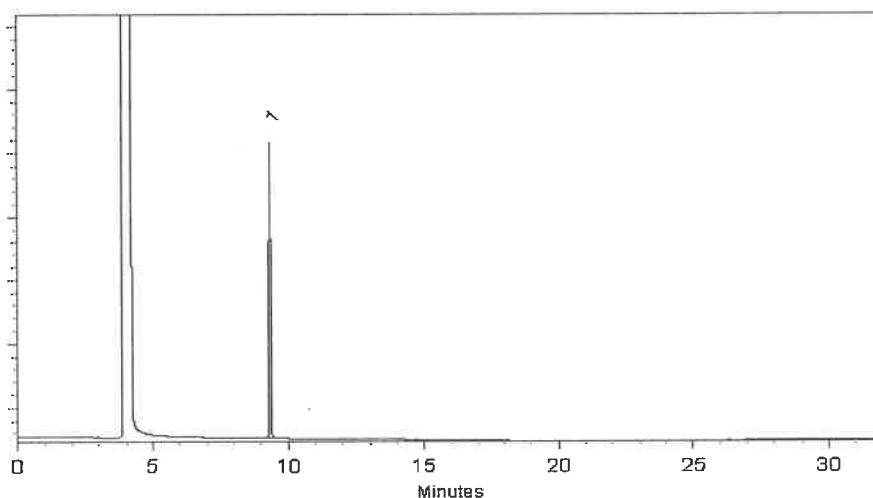

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Tom Suckar - Mix Technician

Date Mixed: 29-Dec-2022 Balance Serial #: B707717271


Christie Mills - Operations Tech II - ARM QC

Date Passed: 03-Jan-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309
www.restek.com

CERTIFIED REFERENCE MATERIAL



Certificate of Analysis

chromatographic plus

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 30225 **Lot No.:** A0193071

Description : Bromochloromethane Standard
Bromochloromethane 2000 μ g/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : December 31, 2027 **Storage:** 0°C or colder
Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	00008541	99%	2,018.0 μ g/mL	+/- 113.3890

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1 μ l

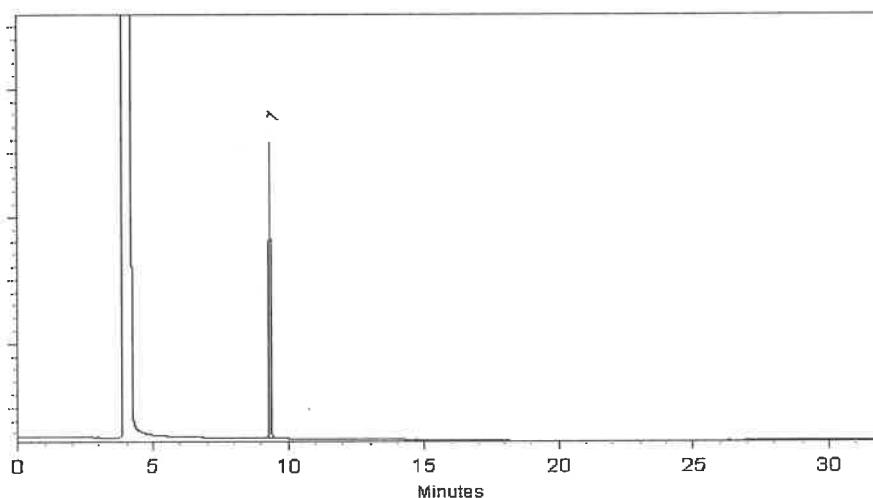

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Tom Suckar - Mix Technician

Date Mixed: 29-Dec-2022 Balance Serial #: B707717271


Christie Mills - Operations Tech II - ARM QC

Date Passed: 03-Jan-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309
www.restek.com

CERTIFIED REFERENCE MATERIAL



Certificate of Analysis

chromatographic plus

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 30225 **Lot No.:** A0193071
Description : Bromochloromethane Standard

Bromochloromethane 2000 μ g/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : December 31, 2027 **Storage:** 0°C or colder
Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	00008541	99%	2,018.0 μ g/mL	+/- 113.3890

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1 μ l

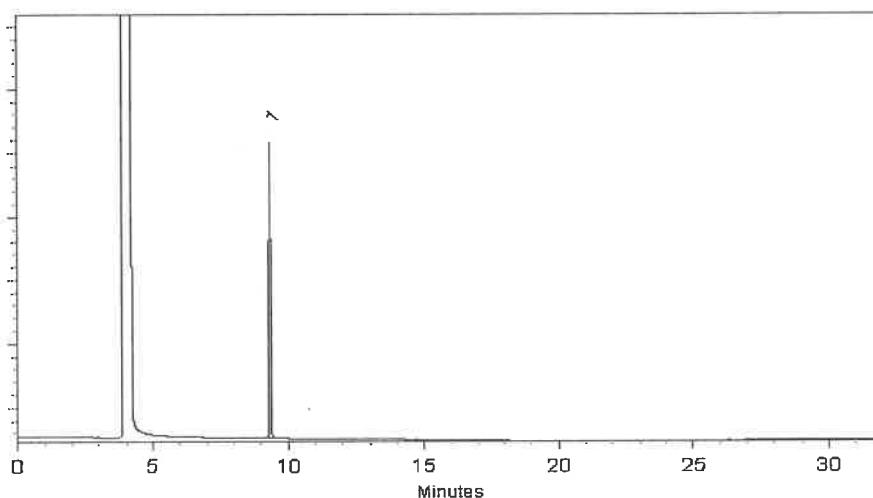

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Tom Suckar - Mix Technician

Date Mixed: 29-Dec-2022 Balance Serial #: B707717271


Christie Mills - Operations Tech II - ARM QC

Date Passed: 03-Jan-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309
www.restek.com

CERTIFIED REFERENCE MATERIAL



Certificate of Analysis

chromatographic plus

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 30225 **Lot No.:** A0193071

Description : Bromochloromethane Standard
Bromochloromethane 2000µg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : December 31, 2027 **Storage:** 0°C or colder
Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Bromochloromethane	74-97-5	00008541	99%	2,018.0 µg/mL	+/- 113.3890

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1 μ l

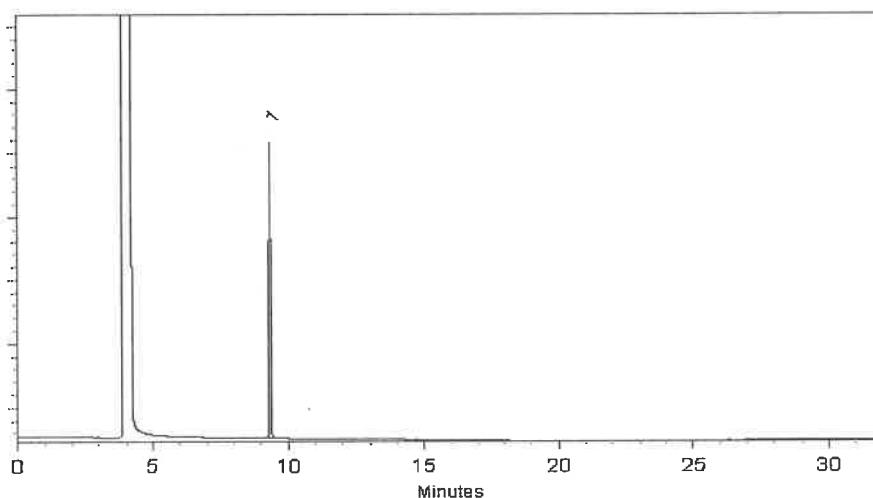

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Tom Suckar - Mix Technician

Date Mixed: 29-Dec-2022 Balance Serial #: B707717271


Christie Mills - Operations Tech II - ARM QC

Date Passed: 03-Jan-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis *gravimetric*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 555582

Lot No.: A0196865

Description : Custom 8260A/B Surrogate Mix

Custom 8260A/B Surrogate Mix 25,000 μ g/mL, P&T Methanol,
1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : April 30, 2026


Storage: 10°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,2-Dichloroethane-d4	17060-07-0	PR-32845	99%	25,036.0 μ g/mL	+/- 1,417.9179
2	1-Bromo-4-fluorobenzene (BFB)	460-00-4	184975	99%	25,132.0 μ g/mL	+/- 1,423.3549
3	Dibromofluoromethane	1868-53-7	022013	99%	25,040.0 μ g/mL	+/- 1,418.1445
4	Toluene-d8	2037-26-5	PR-33397	99%	25,028.0 μ g/mL	+/- 1,417.4648

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%


Russ Bookhamer - Operations Technician

Date Mixed: 11-Apr-2023 Balance: 1127510105

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



21
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



21
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30489

Lot No.: A0209618

Description : 8260B Acetates Mix

8260B Acetates Mix 2,000 µg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : September 30, 2025

Storage: -20°C or colder

Handling: This product is photosensitive.

Ship: On Ice

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Methyl acetate	79-20-9	SHBP3100	99%	2,019.3 µg/mL	+/- 69.7974
2	Vinyl acetate	108-05-4	RP231030CTH	98%	2,016.8 µg/mL	+/- 69.7112
3	Ethyl acetate	141-78-6	SHBQ9682	99%	2,010.7 µg/mL	+/- 69.4979
4	Isopropyl acetate	108-21-4	BCCG7069	99%	2,016.0 µg/mL	+/- 69.6822
5	Propyl acetate	109-60-4	P8XLN	99%	2,008.0 µg/mL	+/- 69.4057
6	Butyl acetate	123-86-4	SHBP6314	99%	2,007.3 µg/mL	+/- 69.3826
7	Amyl acetate	628-63-7	41325/1	97%	2,004.7 µg/mL	+/- 69.2905

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this

reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1 μ l

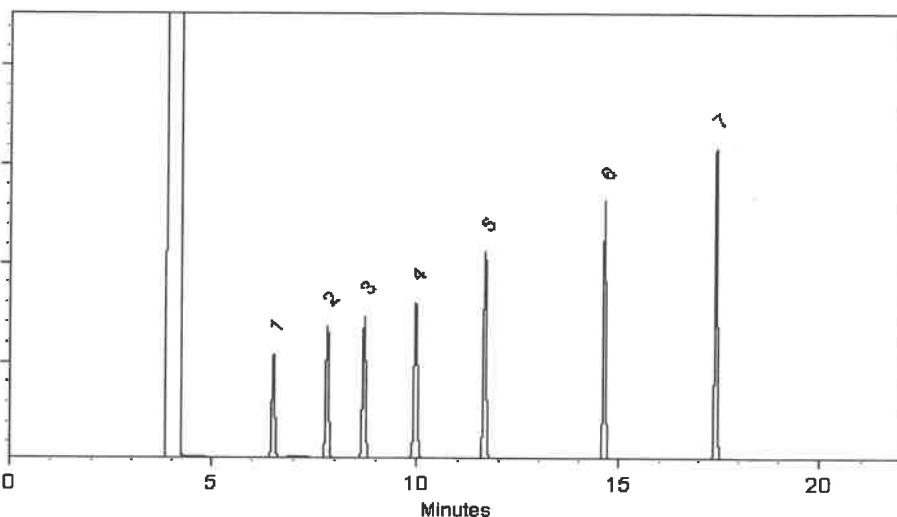

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Samuel Moodier
Sam Moodier - Operations Tech I

Date Mixed: 28-Mar-2024 Balance Serial #: B707717271

Dillan Murphy
Dillan Murphy - Operations Technician |

Date Passed: 01-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



21
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



21
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30489

Lot No.: A0209618

Description : 8260B Acetates Mix

8260B Acetates Mix 2,000 µg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : September 30, 2025

Storage: -20°C or colder

Handling: This product is photosensitive.

Ship: On Ice

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Methyl acetate	79-20-9	SHBP3100	99%	2,019.3 µg/mL	+/- 69.7974
2	Vinyl acetate	108-05-4	RP231030CTH	98%	2,016.8 µg/mL	+/- 69.7112
3	Ethyl acetate	141-78-6	SHBQ9682	99%	2,010.7 µg/mL	+/- 69.4979
4	Isopropyl acetate	108-21-4	BCCG7069	99%	2,016.0 µg/mL	+/- 69.6822
5	Propyl acetate	109-60-4	P8XLN	99%	2,008.0 µg/mL	+/- 69.4057
6	Butyl acetate	123-86-4	SHBP6314	99%	2,007.3 µg/mL	+/- 69.3826
7	Amyl acetate	628-63-7	41325/1	97%	2,004.7 µg/mL	+/- 69.2905

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this

reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1 μ l

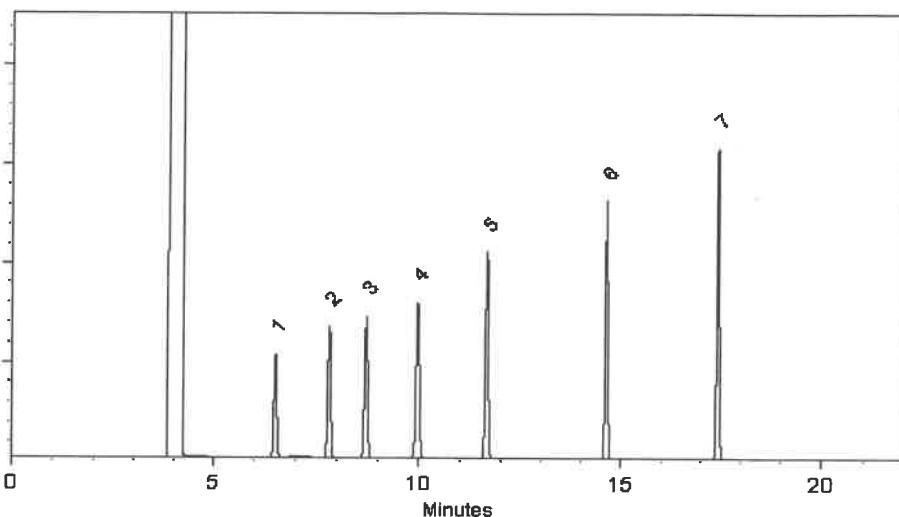

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Samuel Moodier
Sam Moodier - Operations Tech I

Date Mixed: 28-Mar-2024 Balance Serial #: B707717271

Dillan Murphy
Dillan Murphy - Operations Technician |

Date Passed: 01-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis *gravimetric*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555581

Lot No.: A0210184

Description : Custom 8260 Internal Standard Mix

Custom 8260 Internal Standard Mix 25,000 μ g/mL, P&T Methanol,
1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : April 30, 2027


Storage: 10°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Component #	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	1,4-Dichlorobenzene-d4	3855-82-1	PR-30447	99%	25,212.0 μ g/mL	+/- 1,427.8857
2	1,4-Difluorobenzene	540-36-3	MKCS8657	99%	25,220.0 μ g/mL	+/- 1,428.3388
3	Chlorobenzene-d5	3114-55-4	PR-31132	99%	25,116.0 μ g/mL	+/- 1,422.4487
4	Pentafluorobenzene	363-72-4	MKCR9383	99%	25,180.0 μ g/mL	+/- 1,426.0734

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%


John Friedline - Operations Technician I

Date Mixed: 11-Apr-2024

Balance: 1127510105

APPROVED
By Analyst Name: [Redacted] Date: [Redacted]

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Dec 12 (17) 24

30 v14

Certificate of Analysis

chromatographic plus

V14697-to-14726



ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30006

Lot No.: A0210618

Description : VOA Calibration Mix #1

VOA Calibration Mix #1 5,000 μ g/mL, P&T Methanol/Water(90:10),
1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : July 31, 2027

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 μ g/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 μ g/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 μ g/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 μ g/mL	+/- 173.2261

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol/Water (90:10)

CAS # 67-56-1/7732-18-5

Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol


1 μ l

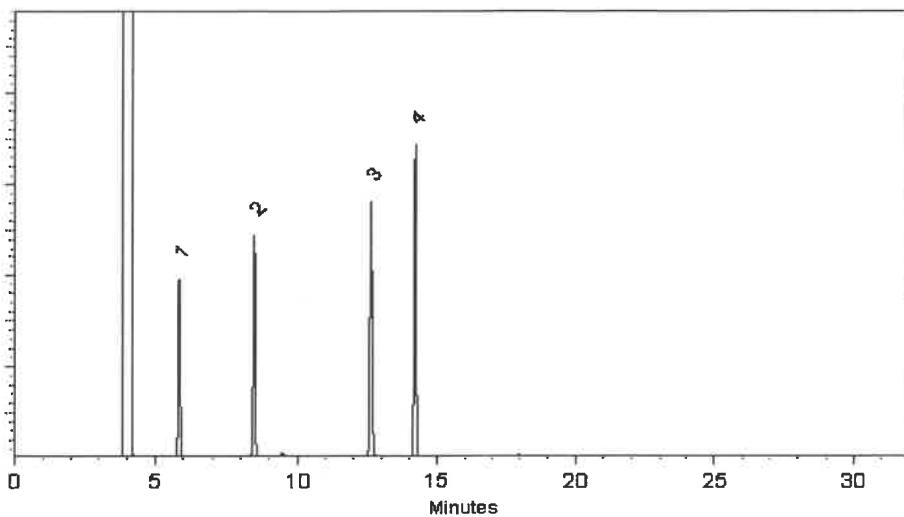

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I.

Date Mixed: 22-Apr-2024 Balance Serial #: B707717271


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Dec 12 (17) 24

30 v14

Certificate of Analysis

chromatographic plus

V14697-to-14726



ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30006

Lot No.: A0210618

Description : VOA Calibration Mix #1

VOA Calibration Mix #1 5,000 μ g/mL, P&T Methanol/Water(90:10),
1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : July 31, 2027

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 μ g/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 μ g/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 μ g/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 μ g/mL	+/- 173.2261

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol/Water (90:10)

CAS # 67-56-1/7732-18-5

Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol


1 μ l

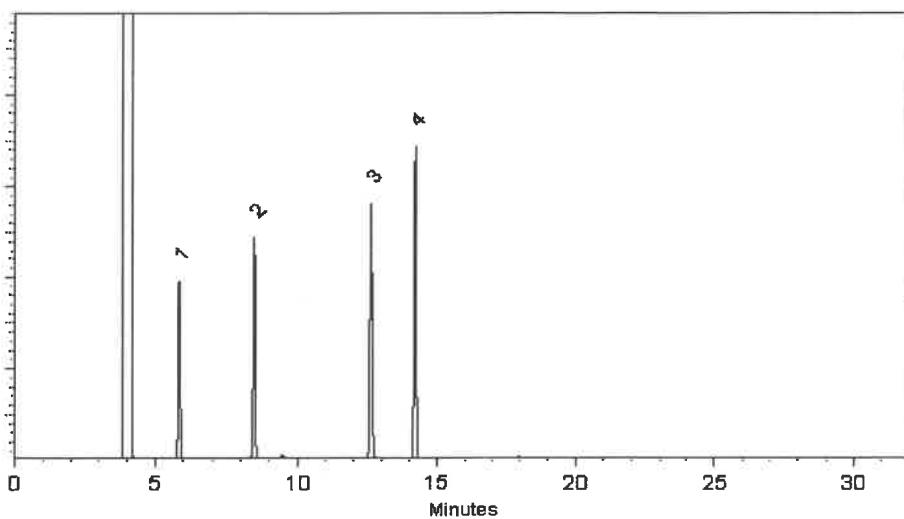

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

 Dakota Parson - Operations Technician I.

Date Mixed: 22-Apr-2024 Balance Serial #: B707717271

 Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Dec 12 (17) 24

30 v14

Certificate of Analysis

chromatographic plus

V14697-to-14726



ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30006

Lot No.: A0210618

Description : VOA Calibration Mix #1

VOA Calibration Mix #1 5,000 μ g/mL, P&T Methanol/Water(90:10),
1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : July 31, 2027

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Acetone	67-64-1	SHBQ8504	99%	5,014.8 μ g/mL	+/- 173.2883
2	2-Butanone (MEK)	78-93-3	SHBQ4704	99%	5,012.4 μ g/mL	+/- 173.2054
3	4-Methyl-2-pentanone (MIBK)	108-10-1	SHBP9200	99%	5,011.6 μ g/mL	+/- 173.1777
4	2-Hexanone	591-78-6	MKCQ6663	99%	5,013.0 μ g/mL	+/- 173.2261

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol/Water (90:10)

CAS # 67-56-1/7732-18-5

Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol


1 μ l

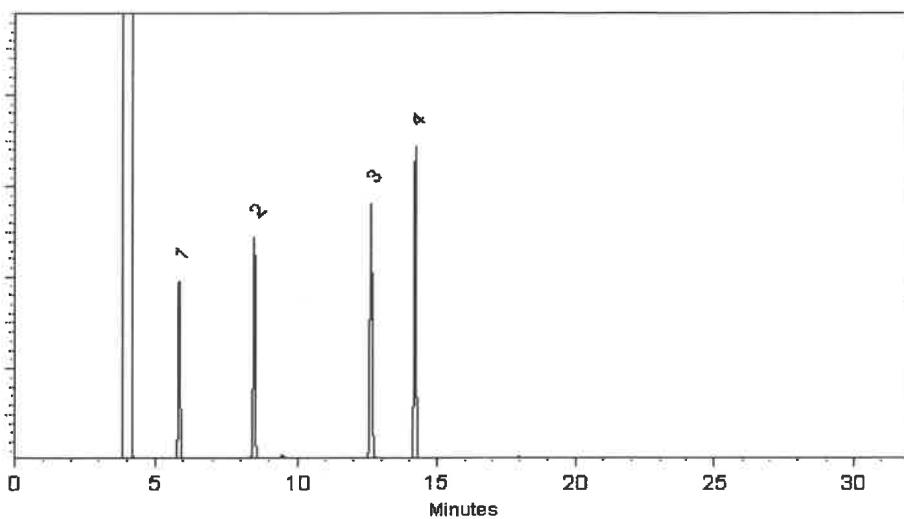

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I.

Date Mixed: 22-Apr-2024 Balance Serial #: B707717271


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

Rev 12/17/24
CERTIFIED REFERENCE MATERIAL
30 μL

Certificate of Analysis
chromatographic plus

*V14727 +
V14756*



ILAC-MRA
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222-01



ILAC-MRA
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222-02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 30042

Lot No.: A0216826

Description : 502.2 Calibration Mix #1

502.2 Calibration Mix #1 2,000μg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : May 31, 2031

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dichlorodifluoromethane (CFC-12)	75-71-8	00022922	99%	2,000.9 μg/mL	+/- 112.4144
2	Chloromethane (methyl chloride)	74-87-3	00022694	99%	2,000.7 μg/mL	+/- 112.3998
3	Vinyl chloride	75-01-4	00015559	99%	2,000.3 μg/mL	+/- 112.3779
4	Bromomethane (methyl bromide)	74-83-9	00017022	99%	2,001.8 μg/mL	+/- 112.4650
5	Chloroethane (ethyl chloride)	75-00-3	107-401039114-1	99%	2,000.1 μg/mL	+/- 112.3700
6	Trichlorofluoromethane (CFC-11)	75-69-4	MKCJ8658	99%	2,000.7 μg/mL	+/- 112.3992

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol

CAS # 67-56-1

Purity 99%

Quality Confirmation Test

Column:

60m x 0.25mm x 1.4 μ m
Rtx-502.2 (cat.#10916)

Carrier Gas:

helium-constant flow 2.0 mL/min.

Temp. Program:

40°C (hold 6 min.) to 100°C
@ 6°C/min.

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


MSD

Split Vent:

Split ratio 10:1

Inj. Vol

1 μ l

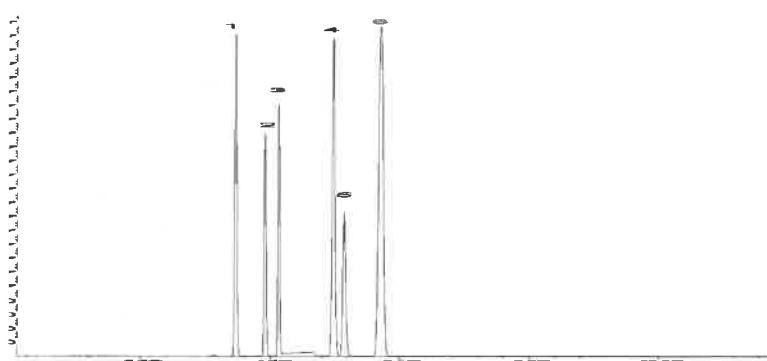

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar Mix Technician

Date Mixed: 23-Sep-2024 Balance Serial #: B707717271

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 04-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

Rec 12/17/24
CERTIFIED REFERENCE MATERIAL

30 mL



ILAC
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222-01



ILAC
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222-02

Certificate of Analysis
chromatographic plus

*V14727 +
V14756*

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 30042

Lot No.: A0216826

Description : 502.2 Calibration Mix #1

502.2 Calibration Mix #1 2,000µg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : May 31, 2031

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dichlorodifluoromethane (CFC-12)	75-71-8	00022922	99%	2,000.9 µg/mL	+/- 112.4144
2	Chloromethane (methyl chloride)	74-87-3	00022694	99%	2,000.7 µg/mL	+/- 112.3998
3	Vinyl chloride	75-01-4	00015559	99%	2,000.3 µg/mL	+/- 112.3779
4	Bromomethane (methyl bromide)	74-83-9	00017022	99%	2,001.8 µg/mL	+/- 112.4650
5	Chloroethane (ethyl chloride)	75-00-3	107-401039114-1	99%	2,000.1 µg/mL	+/- 112.3700
6	Trichlorofluoromethane (CFC-11)	75-69-4	MKCJ8658	99%	2,000.7 µg/mL	+/- 112.3992

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol

CAS # 67-56-1

Purity 99%

Quality Confirmation Test

Column:

60m x 0.25mm x 1.4 μ m
Rtx-502.2 (cat.#10916)

Carrier Gas:

helium-constant flow 2.0 mL/min.

Temp. Program:

40°C (hold 6 min.) to 100°C
@ 6°C/min.

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


MSD

Split Vent:

Split ratio 10:1

Inj. Vol

1 μ l

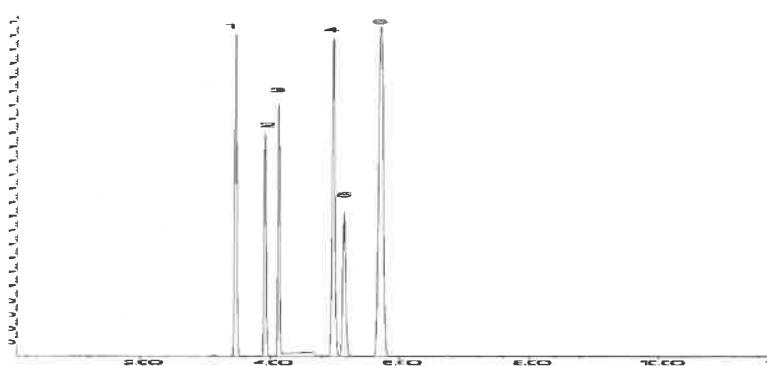

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar Mix Technician

Date Mixed: 23-Sep-2024 Balance Serial #: B707717271

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 04-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus

✓ 14842 to 14846



ILAC-MRA
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ILAC-MRA
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 30470

Lot No.: A0217535

Description : tert-Butanol Standard

tert-Butanol Std 50,000 μ g/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : October 31, 2027

Storage: 0°C or colder

Ship: Ambient

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	tert-Butanol (TBA)	75-65-0	SHBQ8002-1	99%	50,007.5 μ g/mL	+/- 717.6137

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1 μ l

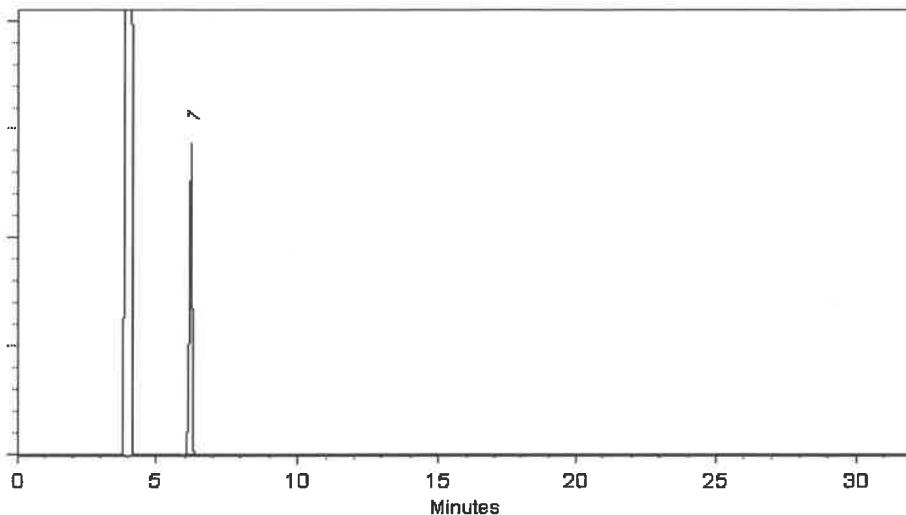

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A.O.EF
Aaron Enyart - Operations Tech I

Date Mixed: 07-Oct-2024 Balance Serial #: B251644995

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 09-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

2014 Dec 01 (08/21)



ILAC
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ILAC
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

Certificate of Analysis

chromatographic

J14803 - J14822

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555408-SL

Lot No.: A0220471

Description : Custom Vinyl Acetate Standard

Custom Vinyl Acetate Standard 8,000 μ g/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : June 30, 2026

Storage: -20°C or colder

Handling: This product is photosensitive.

Ship: On Ice

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Vinyl acetate	108-05-4	RD240423RSR	99%	8,066.0 μ g/mL	+/- 278.7979

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol

CAS # 67-56-1

Purity 99%

Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1 μ l

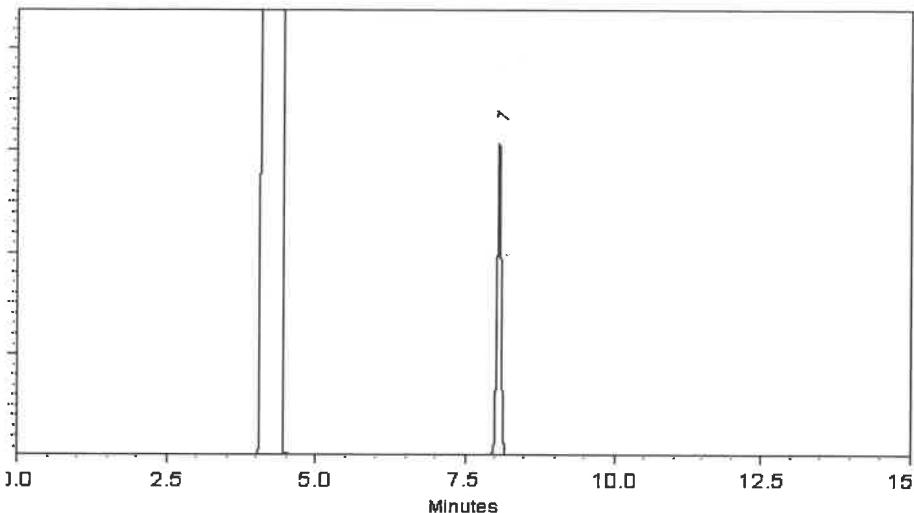

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ethan Winiarski - Operations Tech I

Date Mixed: 24-Dec-2024 Balance Serial #: 1127510105

REVIEWED
By Jennifer Polson at 7:17 am, Jan 05, 2025

Dillon Murphy - Operations Technician I

Date Passed: 02-Jan-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

2014 Dec 01 (08/21)



ILAC
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ILAC
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

Certificate of Analysis

chromatographic

J14803 - J14822

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 555408-SL

Lot No.: A0220471

Description : Custom Vinyl Acetate Standard

Custom Vinyl Acetate Standard 8,000 μ g/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : June 30, 2026

Storage: -20°C or colder

Handling: This product is photosensitive.

Ship: On Ice

C E R T I F I E D V A L U E S

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Vinyl acetate	108-05-4	RD240423RSR	99%	8,066.0 μ g/mL	+/- 278.7979

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: P&T Methanol

CAS # 67-56-1

Purity 99%

Tech Tips:

Vinyl acetate is a volatile organic ester included in the target lists of several US EPA and other methods. Under acidic conditions, esters react with alcohols to form new esters (transesterification). Methanol-based mixes containing halogenated compounds are slightly acidic, so it is important to minimize exposure of vinyl acetate to mixes of halogenated compounds in methanol. For this reason, we offer vinyl acetate in individual solution, and suggest that it be introduced into the working level calibration solution immediately before use. This will minimize problems and ensure more consistent results.

Quality Confirmation Test

Column:

105m x 0.53mm x 3.0 μ m
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:

200°C

Det. Temp:

250°C

Det. Type:


FID

Split Vent:

40 ml/min

Inj. Vol

1 μ l

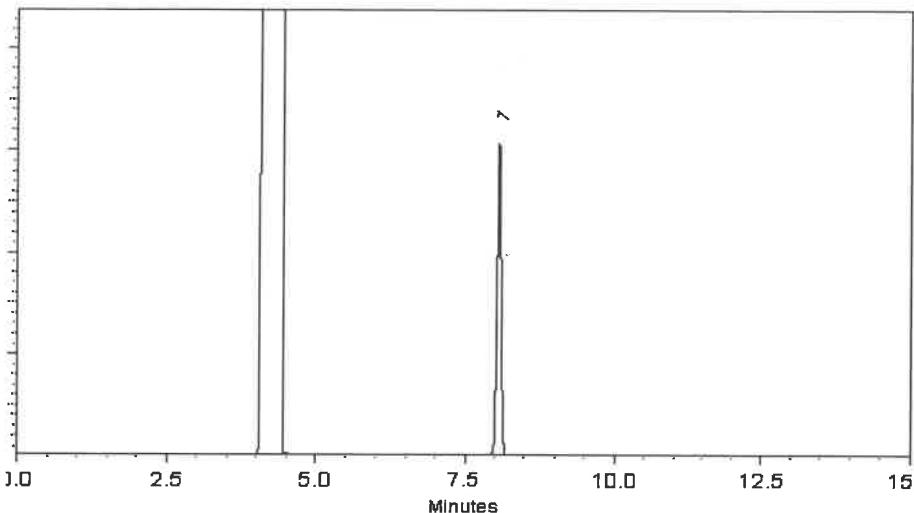

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Ethan Winiarski - Operations Tech I

Date Mixed: 24-Dec-2024 Balance Serial #: 1127510105

REVIEWED
By Jennifer Polson at 7:17 am, Jan 05, 2025

Dillon Murphy - Operations Technician I

Date Passed: 02-Jan-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis




Material No.: 9077-02
Batch No.: 22L0562016
Manufactured Date: 2022-10-26
Expiration Date: 2025-10-25
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH_3OH) (by GC, corrected for water)	$\geq 99.9 \%$	100.0 %
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.2 ppm
Titrable Acid ($\mu\text{eq/g}$)	≤ 0.3	0.2
Titrable Base ($\mu\text{eq/g}$)	≤ 0.10	0.03
Water (by KF, coulometric)	$\leq 0.08 \%$	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

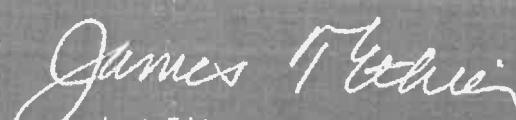
Jamie Ethier
Vice President Global Quality



SHIPPING DOCUMENTS



A Phenomenex®
Company

6390 Joyce Dr., #100
Golden, CO 80403

Tel: +1-303-940-0033
Fax: +1-303-940-0043
info@phenova.com
www.phenova.com

For terms and conditions of your order, please visit:
www.phenova.com/home/termsofsale

Packing List

Date	Order #
03/03/2025	333289



Ship To

Alliance Tech Group - Newark
ATTN: Sohil Jodhani
284 Sheffield St., #1
Mountainside, NJ 07092
USA

Received by: SJ

3/5/2025 14:30

Customer PO #	Terms	PT Acct #	Customer #	Ship Via	F.O.B.
PO2-1517	Net 30	ZCM-100	1500470	FedEx 2nd Day	Golden, CO

Qty Ordered	Qty Shipped	Qty Backorder	Part Number	Part Description	Study Number	Lot Number
			PT-TMSET-WP	WP Trace Metals Set : (TM1, HG and SNTI)		
1	1	0	PT-TM1-WP	WP Trace Metals 1	WP0325	8264-04
1	1	0	PT-HG-WP	WP Mercury	WP0325	8264-05
1	1	0	PT-SNTI-WP	WP Tin & Titanium	WP0325	8264-38
1	1	0	PT-CR6-WP	WP Hexavalent Chromium	WP0325	8264-06
1	1	0	PT-DEM-WP	WP Demand	WP0325	8264-07
			PT-MINSET-WP	WP Minerals Set : (MIN1, MIN2 and COND)		
1	1	0	PT-MIN1-WP	WP Minerals 1 Only	WP0325	8264-08
1	1	0	PT-MIN2-WP	WP Minerals 2 Only	WP0325	8264-102
1	1	0	PT-COND-WP	WP Conductivity Only	WP0325	8264-72
1	1	0	PT-SOL-WP	WP Solids	WP0325	8264-09
			PT-NUTSET-WP	WP Nutrients Set : (NUT1, NUT2 and NUT3)		
1	1	0	PT-NUT1-WP	WP NUT1 Simple Nutrients Only	WP0325	8264-10
1	1	0	PT-NUT2-WP	WP NUT2 - Complex Nutrients	WP0325	8264-11
1	1	0	PT-NUT3-WP	WP NUT3 - Nitrite Only	WP0325	8264-69
1	1	0	PT-OGR1L-WP	WP Oil and Grease 1L	WP0325	8264-103
1	1	0	PT-CL-WP	WP Residual Chlorine	WP0325	8264-13
1	1	0	PT-PH-WP	WP pH	WP0325	8264-15
1	1	0	PT-CN-WP	WP Cyanide	WP0325	8264-14
1	1	0	PT-PHEN-WP	WP Phenolics	WP0325	8264-16



A Phenomenex®
Company

6390 Joyce Dr., #100
Golden, CO 80403

Tel: +1-303-940-0033
Fax: +1-303-940-0043
info@phenova.com
www.phenova.com

For terms and conditions of your order, please visit:
www.phenova.com/home/termsofsale

Packing List

Date	Order #
03/03/2025	333289



Ship To

Alliance Tech Group - Newark
ATTN: Sohil Jodhani
284 Sheffield St., #1
Mountainside, NJ 07092
USA

Received by: SJ

3/5/2025 14:30

Customer PO #	Terms	PT Acct #	Customer #	Ship Via	F.O.B.
PO2-1517	Net 30	ZCM-100	1500470	FedEx 2nd Day	Golden, CO

Qty Ordered	Qty Shipped	Qty Backorder	Part Number	Part Description	Study Number	Lot Number
1	1	0	PT-S2-WP	WP Sulfide	WP0325	8264-22
1	1	0	PT-SSOL-WP	WP Settleable Solids	WP0325	8264-17
1	1	0	PT-TURB-WP	WP Turbidity	WP0325	8264-20
1	1	0	PT-VOA-WP	WP Volatiles	WP0325	8264-26
1	1	0	PT-BN-WP	WP Base Neutrals	WP0325	8264-27
1	1	0	PT-ACIDS-WP	WP Acids	WP0325	8264-28
1	1	0	PT-PEST-WP	WP Pesticides	WP0325	8264-29
1	1	0	PT-CHLR-WP	WP Chlordane	WP0325	8264-30
1	1	0	PT-TXP-WP	WP Toxaphene	WP0325	8264-31
1	1	0	PT-PCBW-WP	WP PCBs in Water	WP0325	8264-32
1	1	0	PT-HERB-WP	WP Herbicides	WP0325	8264-36
1	1	0	RR-TPH1L-WP	WP TPH 1L	R40367	R40367-104
1	1	0	RR-VSOL-WP	WP Volatile Solids	R40367	R40367-18
1	1	0	RR-SIO2-WP	WP Silica	R40367	R40367-21
1	1	0	RR-COL-WP	WP Color	R40367	R40367-51
1	1	0	RR-GAS-WP	WP Gasoline Range Organics	R40367	R40367-62
1	1	0	RR-DIES-WP	WP Diesel Range Organics	R40367	R40367-63
1	1	0	RR-8011-WP	WP EDB/DBCP/TCP	R40367	R40367-98
1	1	0	RR-PAH-WP	WP PAH-Low Level	R40433	R40433-37



A Phenomenex®
Company

6390 Joyce Dr., #100
Golden, CO 80403

Tel: +1-303-940-0033
Fax: +1-303-940-0043
info@phenova.com
www.phenova.com

For terms and conditions of your order, please visit:
www.phenova.com/home/termsofsale

Packing List

Date	Order #
03/07/2025	335989



Ship To

Alliance Tech Group - Newark
ATTN: Sohil Jodhani
284 Sheffield St., #1
Mountainside, NJ 07092

USA Received by: SJ

3/11/2025 9:55

Customer PO #	Terms	PT Acct #	Customer #	Ship Via	F.O.B.
Email: Sohil Jodhani	Net 30	ZCM-100	1500470	FedEx 2nd Day	Golden, CO

Qty Ordered	Qty Shipped	Qty Backorder	Part Number	Part Description	Study Number	Lot Number
1	1	0	RR-TRIAZINE-WP	WP Triazine Pesticides	R40480	R40480-108

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488