
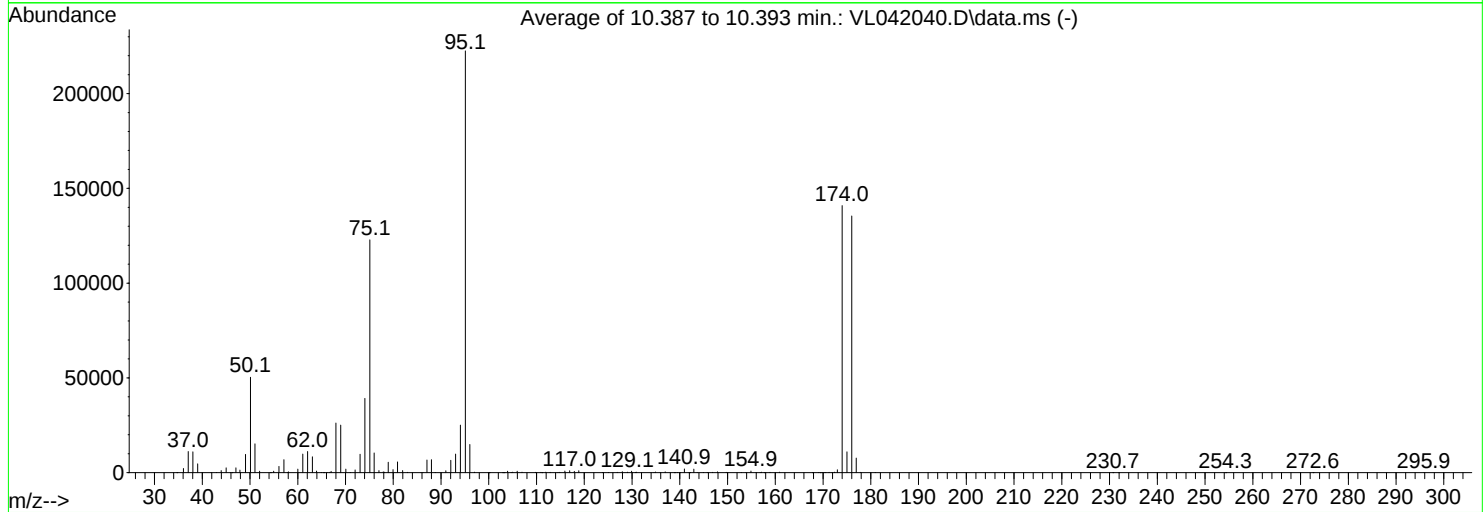


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL022525\
 Data File : VL042040.D
 Acq On : 25 Feb 2025 07:56
 Operator : SY/MD
 Sample : BFB
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL022525AIR.M
 Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 Last Update : Wed Feb 26 01:08:36 2025

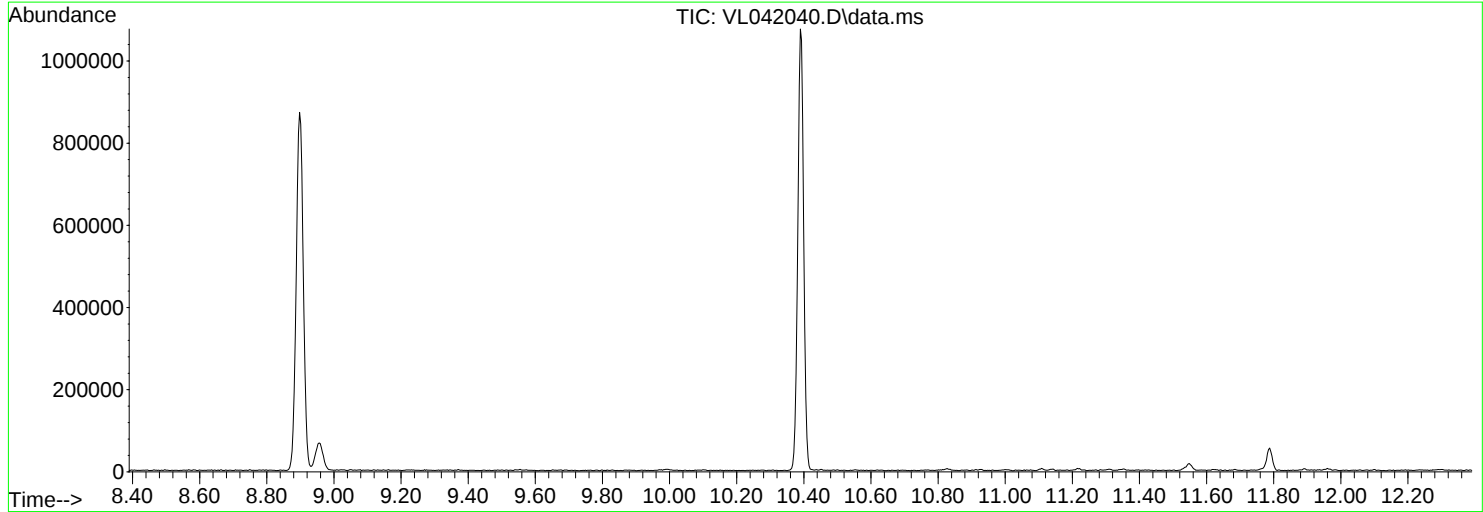

AutoFind: Scans 3182, 3183, 3184; Background Corrected with Scan 3168

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	22.6	50320	PASS
75	95	30	66	55.2	122859	PASS
95	95	100	100	100.0	222571	PASS
96	95	5	9	6.7	14875	PASS
173	174	0.00	2	1.1	1534	PASS
174	95	50	120	63.3	140957	PASS
175	174	4	9	7.8	11014	PASS
176	174	93	101	96.1	135437	PASS
177	176	5	9	5.7	7676	PASS

Average of 10.387 to 10.393 min.: VL042040.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
34.70	28	47.05	2526	58.05	414	68.00	2618
36.05	2223	47.90	1374	60.00	1900	69.00	2505
37.05	11140	49.05	9623	61.05	9827	70.05	185
38.05	10945	50.10	50320	62.05	11140	71.00	6
39.05	4647	51.05	15242	63.05	8365	72.00	1450
41.85	112	52.00	740	63.95	890	73.05	9731
43.00	126	54.30	17	64.95	122	74.05	39184
43.95	1131	54.95	752	65.40	22	75.10	122859
45.00	2511	56.05	3327	66.10	82	76.00	10406
45.90	77	57.10	6812	66.70	141	77.00	1084
46.20	45	57.90	131	67.00	689	77.90	437

Average of 10.387 to 10.393 min.: VL042040.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.10	265	91.00	978	103.95	765	114.85	144
78.95	5465	92.05	6469	104.70	49	115.95	842
79.95	1631	93.05	9774	105.00	247	116.95	1016
80.90	5642	94.05	25088	105.95	752	117.90	687
81.95	1083	95.10	222571	106.95	295	118.85	1016
82.95	188	96.05	14875	109.80	139	123.80	72
85.80	135	97.00	284	110.90	160	124.00	81
86.20	121	99.90	37	111.10	25	125.10	63
87.05	6697	100.10	27	111.95	220	126.90	143
88.00	6841	102.90	35	112.85	148	127.95	520
88.80	63	103.20	35	114.50	51	129.05	303

Average of 10.387 to 10.393 min.: VL042040.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
129.90	788	140.95	1984	150.00	105	167.80	25
130.70	187	141.90	37	152.90	126	169.10	103
130.95	248	142.05	44	153.85	131	169.40	46
134.60	83	142.95	1834	154.90	850	169.95	64
134.95	371	143.65	110	156.00	119	170.40	64
135.90	48	144.95	99	156.85	134	170.60	88
136.95	394	145.75	130	157.10	226	171.25	175
138.90	30	146.00	95	157.70	18	171.90	106
139.50	84	146.85	213	158.00	51	172.40	228
139.90	68	147.90	442	158.90	147	173.00	1534
140.10	99	149.70	178	160.90	256	174.00	140957

Average of 10.387 to 10.393 min.: VL042040.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.00	11014						
176.00	135437						
176.95	7676						
177.90	161						
180.95	55						
230.70	27						
231.90	20						
254.30	36						
272.60	20						
295.85	67						

Instrument :

MSVOA_L

ClientSampleId :

BFB