
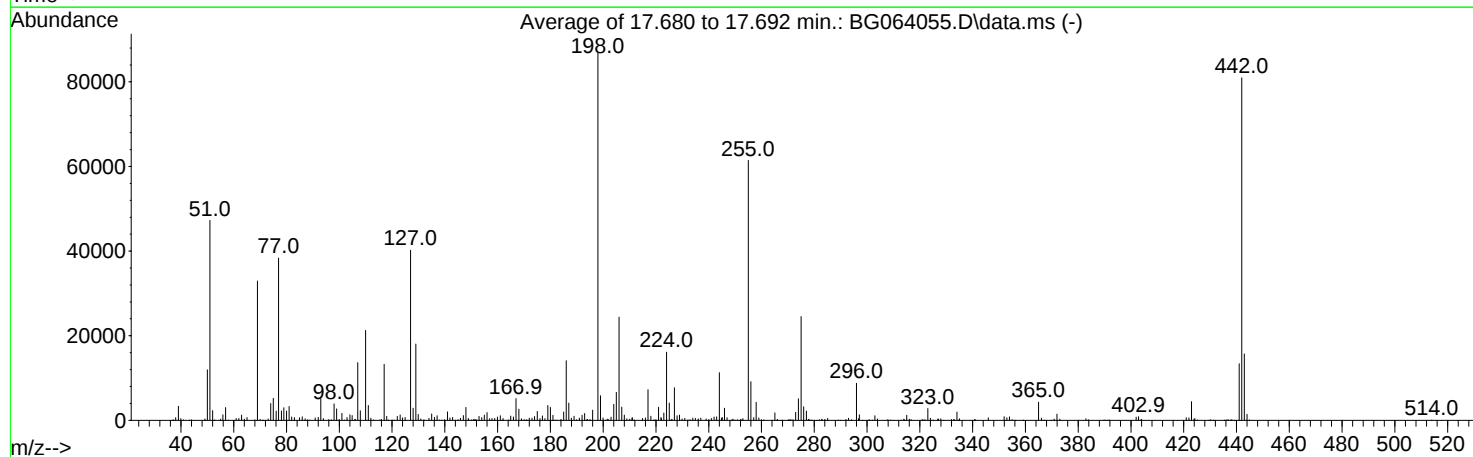


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030725\
Data File : BG064055.D
Acq On : 7 Mar 2025 12:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 05 15:39:19 2025

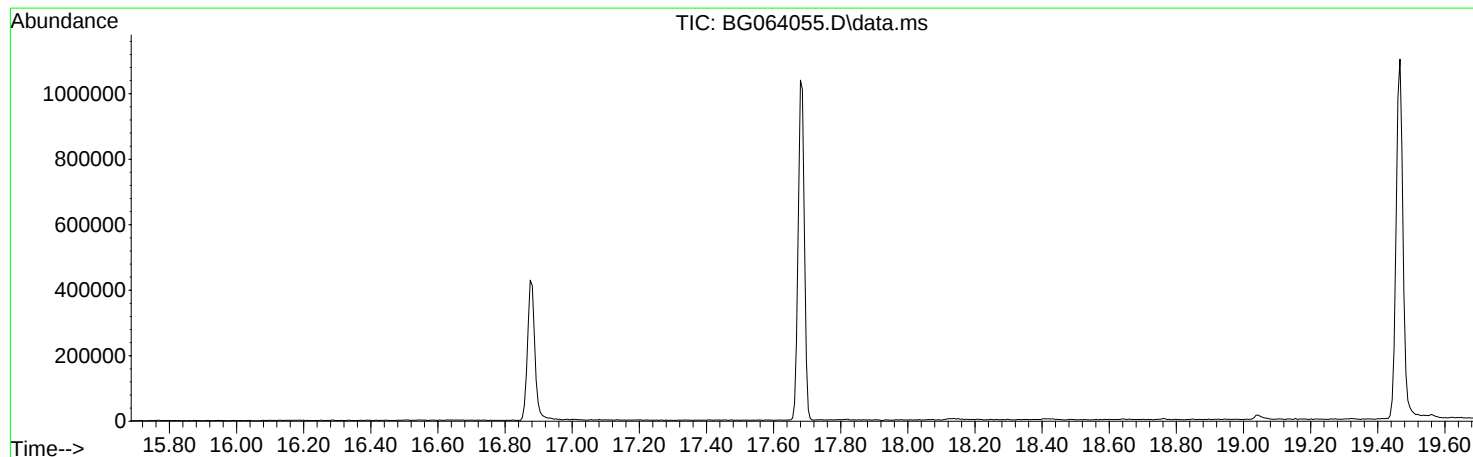

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.4	47256	PASS
68	69	0.00	2	0.4	135	PASS
69	198	0.00	100	37.9	32949	PASS
70	69	0.00	2	0.7	228	PASS
127	198	10	80	46.2	40187	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	86939	PASS
199	198	5	9	6.7	5811	PASS
275	198	10	60	28.2	24555	PASS
365	198	1	100	4.9	4267	PASS
441	198	0.01	100	15.4	13386	PASS
442	442	50	100	100.0	80960	PASS
443	442	15	24	19.4	15696	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/7/2025	BNA_G	<u>BG064055.D</u>
Compound Name	Response	Retention Time
DDT	224456	20.7
DDD	6821	20.259
DDE	122	19.754
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6943	231399	3.00

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030725\
Data File : BG064055.D
Acq On : 7 Mar 2025 12:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 07 14:17:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

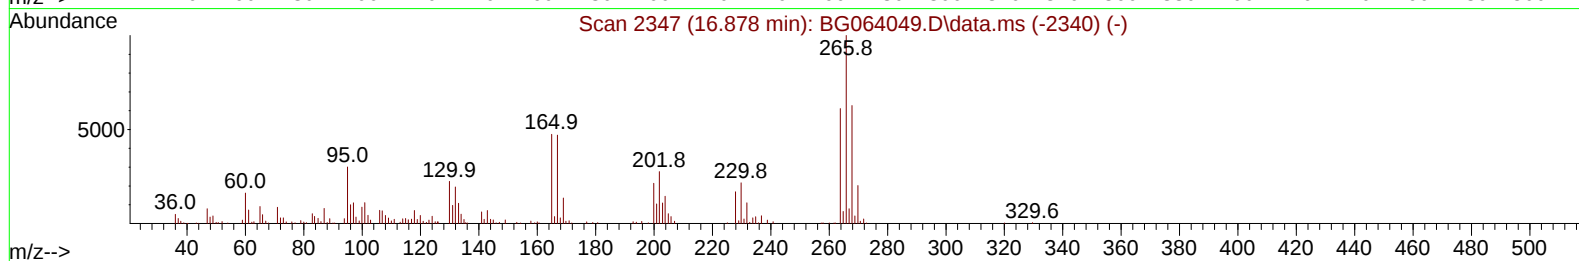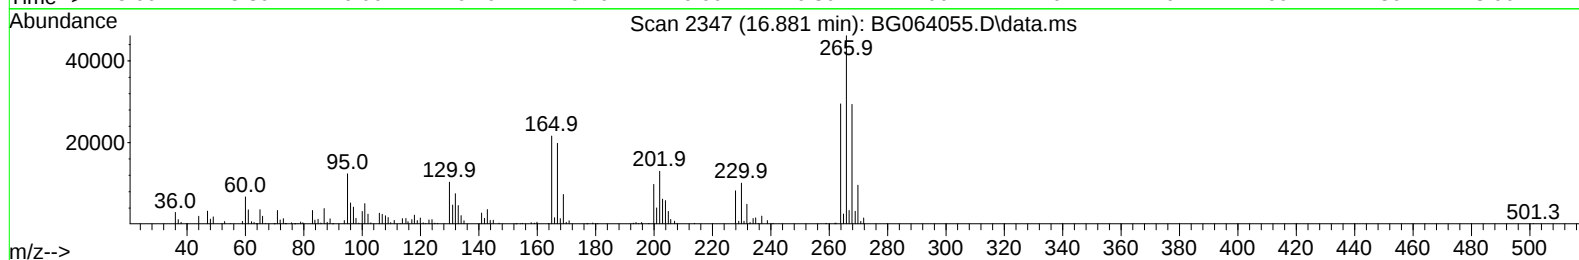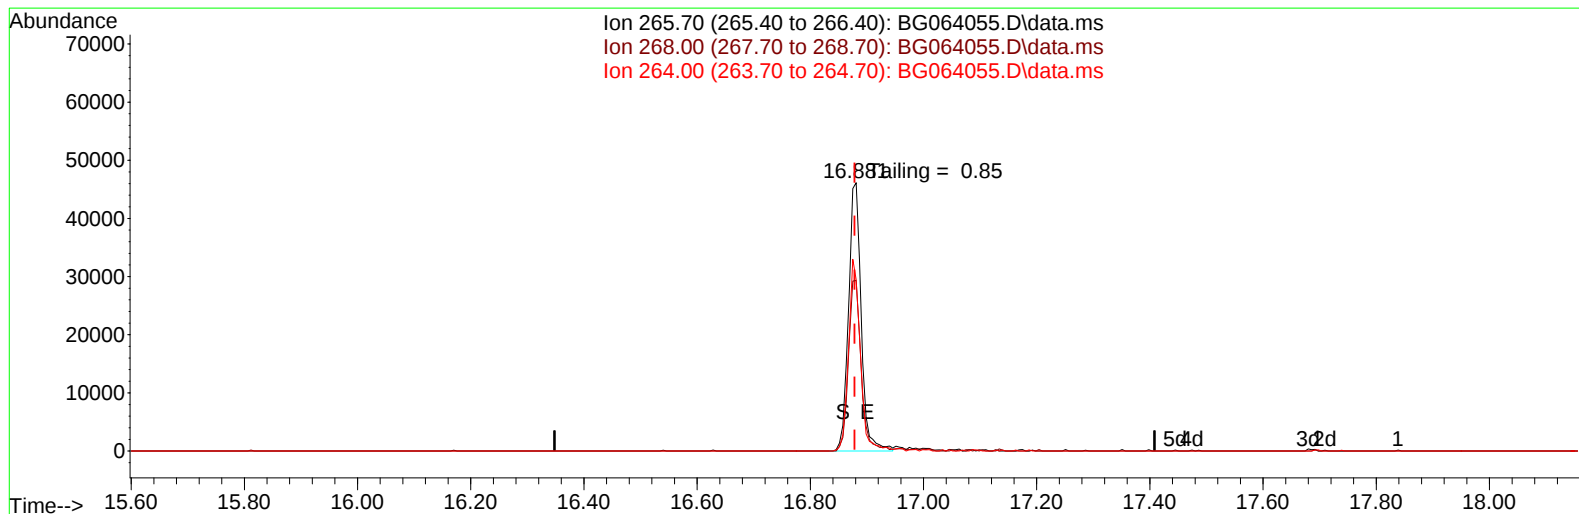

TIC: BG064055.D\data.ms

(70) Pentachlorophenol (C)

16.881min (+ 0.003) 140577.90 ng m




response 74060

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	63.59
264.00	61.10	63.88
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030725\  
Data File : BG064055.D  
Acq On    : 7 Mar 2025 12:15  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 07 14:17:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

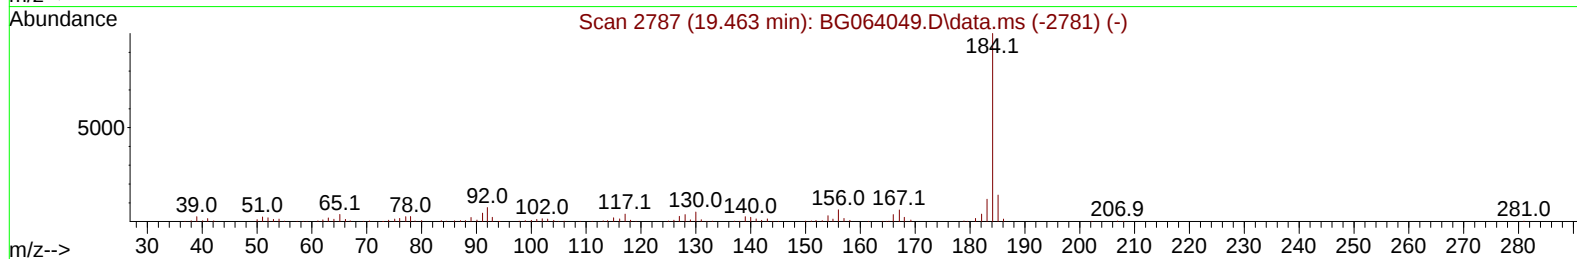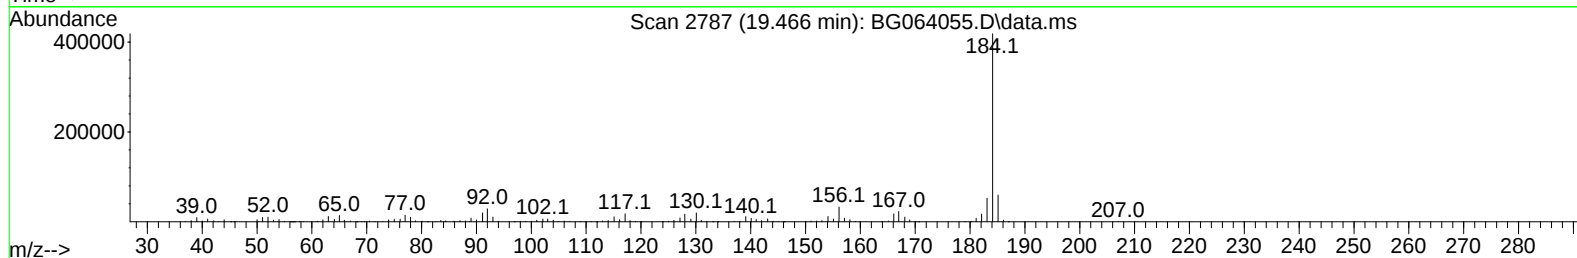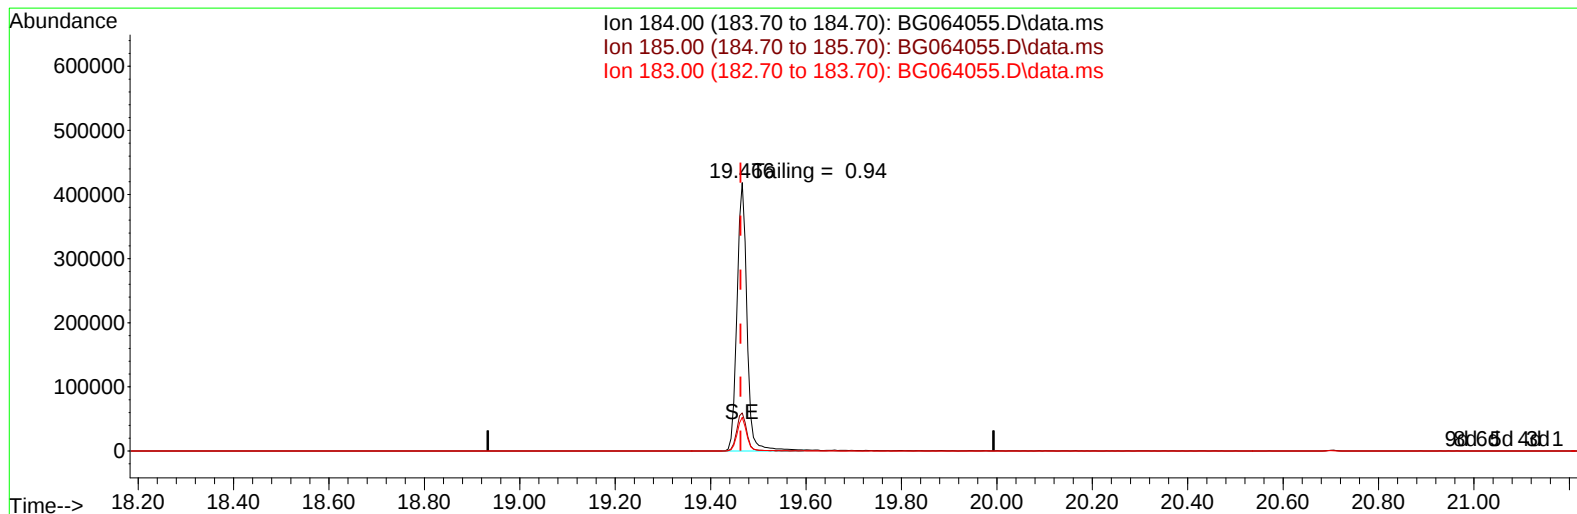

TIC: BG064055.D\data.ms

(77) Benzidine

19.466min (+ 0.003) 780316.23 ng m

response **626699**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.22
183.00	11.90	12.55
0.00	0.00	0.00