
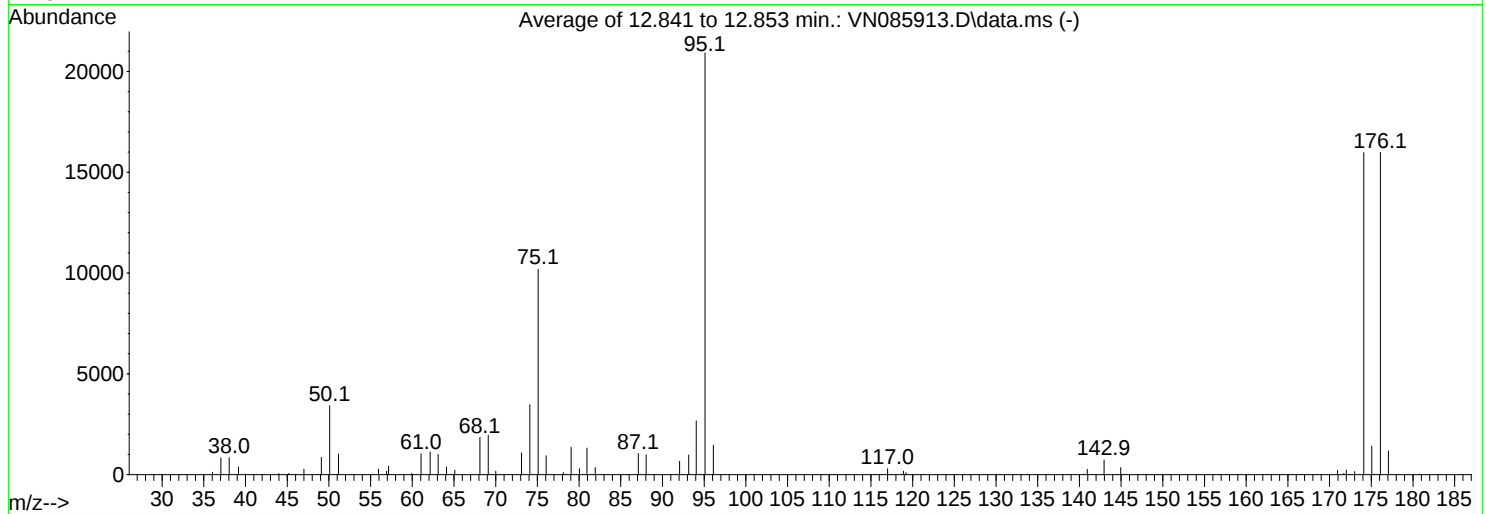


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN031025\
Data File : VN085913.D
Acq On : 10 Mar 2025 10:54
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

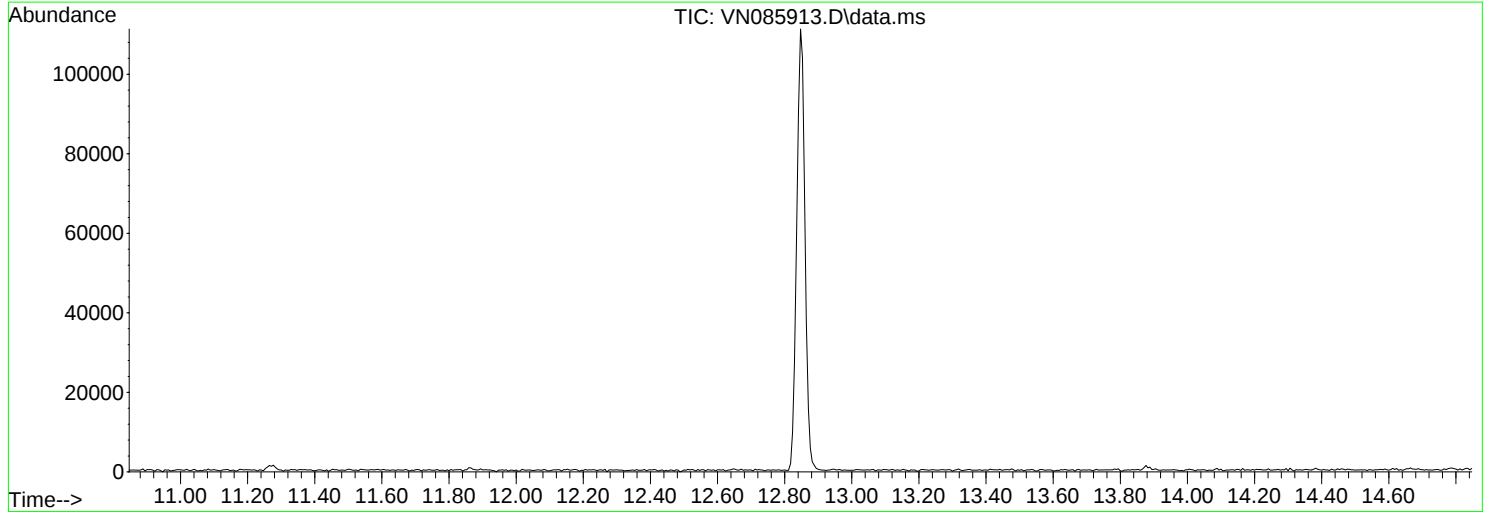

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	3418	PASS
75	95	30	60	48.7	10194	PASS
95	95	100	100	100.0	20923	PASS
96	95	5	9	7.0	1459	PASS
173	174	0.00	2	1.0	154	PASS
174	95	50	100	76.4	15975	PASS
175	174	5	9	8.8	1412	PASS
176	174	95	101	100.1	15983	PASS
177	176	5	9	7.4	1178	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	116	55.95	279	70.00	177	88.05	981
37.05	836	56.90	168	73.10	1077	92.05	651
38.05	842	57.15	413	74.10	3467	93.15	971
39.15	385	59.90	59	75.10	10194	94.05	2669
40.00	29	61.05	1036	76.05	933	95.10	20923
44.00	50	62.15	1129	78.10	105	96.10	1459
45.20	60	63.10	1000	79.05	1363	117.00	294
47.00	273	64.10	382	80.05	296	118.90	174
49.10	860	65.10	223	80.95	1319	119.20	98
50.10	3418	68.10	1849	81.95	350	140.95	260
51.15	1028	69.10	1952	87.10	1046	142.95	727

Average of 12.841 to 12.853 min.: VN085913.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
144.95	349						
170.95	210						
171.70	56						
172.00	226						
173.00	154						
174.10	15975						
175.05	1412						
176.10	15983						
177.05	1178						