
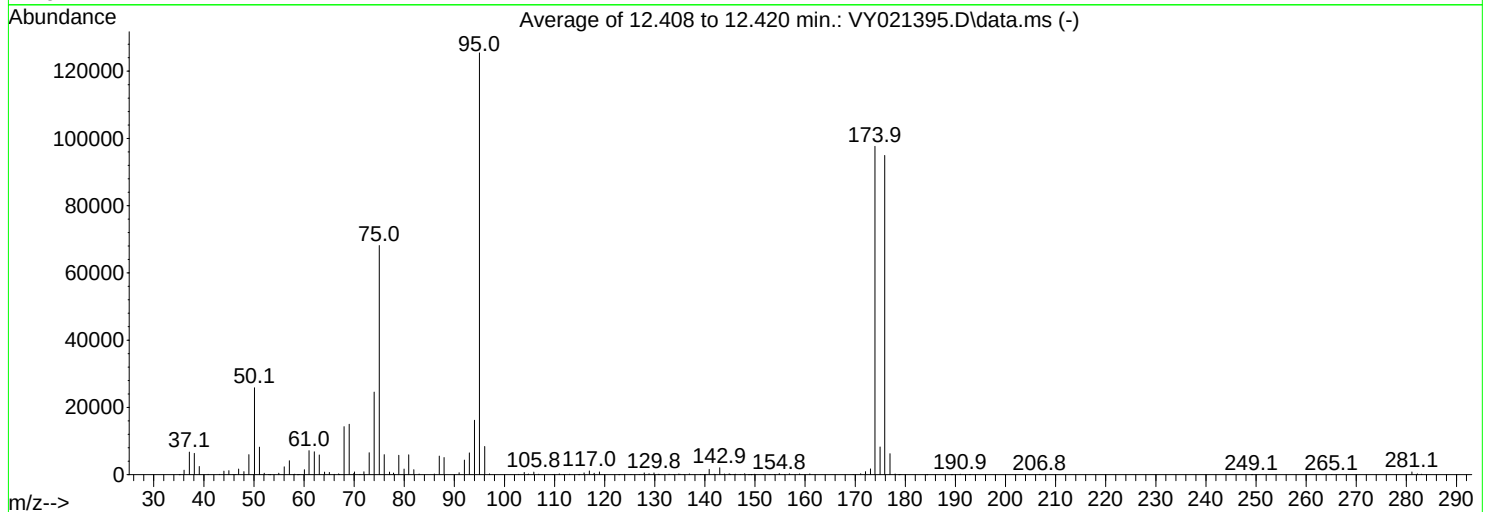


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY030425\
Data File : VY021395.D
Acq On : 04 Mar 2025 08:52
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y030425S.M
Title : SW846 8260
Last Update : Wed Mar 05 12:42:45 2025

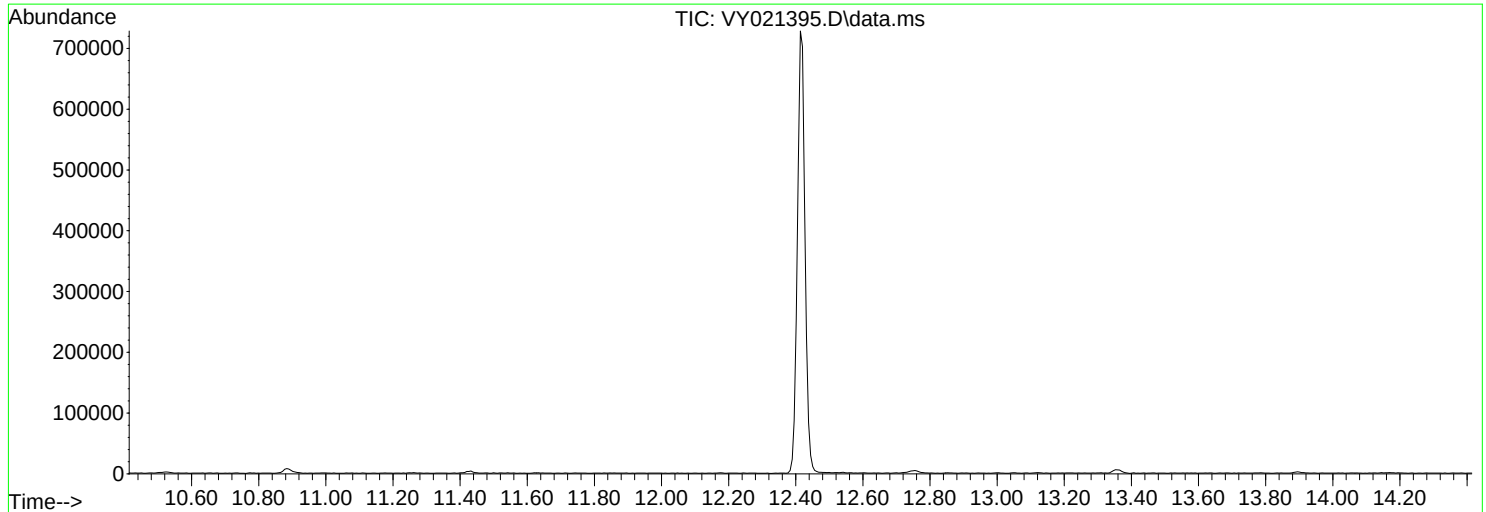

AutoFind: Scans 1753, 1754, 1755; Background Corrected with Scan 1745

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.6	25853	PASS
75	95	30	60	54.3	68152	PASS
95	95	100	100	100.0	125459	PASS
96	95	5	9	6.7	8382	PASS
173	174	0.00	2	1.8	1721	PASS
174	95	50	100	77.8	97645	PASS
175	174	5	9	8.4	8226	PASS
176	174	95	101	97.2	94957	PASS
177	176	5	9	6.6	6262	PASS