

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

LAB CHRONICLE

OrderID:	Q1522	OrderDate:	3/7/2025 10:29:00 AM
Client:	ENTACT	Project:	540 Degraw St, Brooklyn, NY - E9309
Contact:	Jarod Stanfield	Location:	H31,VOA Ref. #3 Water

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q1522-02	TW-WTS-04	WATER	PCB	8082A	03/06/25	03/10/25	03/10/25	03/07/25



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: Q1522

Order ID: Q1522

Client: ENTACT

Project ID: 540 Degraw St, Brooklyn, NY - E9309

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------

Client ID :

Total Concentration: 0.000



QC SUMMARY

Surrogate Summary

SDG No.: **Q1522**

Client: **ENTACT**

Analytical Method: **8082A**

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Rec	Qual	Limits	
								Low	High
I.BLK-PO109425.D	PIBLK-PO109425.D	Tetrachloro-m-xylene	1	20	25.3	126		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	25.3	126		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	24.1	121		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	25.5	127		70 (60)	130 (140)
I.BLK-PO109759.D	PIBLK-PO109759.D	Tetrachloro-m-xylene	1	20	19.1	95		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	17.1	86		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	20.4	102		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	19.0	95		70 (60)	130 (140)
PB167042BL	PB167042BL	Tetrachloro-m-xylene	1	20	18.5	92		30 (16)	150 (158)
		Decachlorobiphenyl	1	20	16.7	84		30 (10)	150 (173)
		Tetrachloro-m-xylene	2	20	19.3	97		30 (16)	150 (158)
		Decachlorobiphenyl	2	20	18.4	92		30 (10)	150 (173)
PB167042BS	PB167042BS	Tetrachloro-m-xylene	1	20	18.0	90		30 (16)	150 (158)
		Decachlorobiphenyl	1	20	17.4	87		30 (10)	150 (173)
		Tetrachloro-m-xylene	2	20	18.6	93		30 (16)	150 (158)
		Decachlorobiphenyl	2	20	19.0	95		30 (10)	150 (173)
PB167042BSD	PB167042BSD	Tetrachloro-m-xylene	1	20	18.2	91		30 (16)	150 (158)
		Decachlorobiphenyl	1	20	17.5	87		30 (10)	150 (173)
		Tetrachloro-m-xylene	2	20	18.9	94		30 (16)	150 (158)
		Decachlorobiphenyl	2	20	18.9	94		30 (10)	150 (173)
Q1522-02	TW-WTS-04	Tetrachloro-m-xylene	1	20	18.1	91		30 (16)	150 (158)
		Decachlorobiphenyl	1	20	14.3	72		30 (10)	150 (173)
		Tetrachloro-m-xylene	2	20	18.8	94		30 (16)	150 (158)
		Decachlorobiphenyl	2	20	15.8	79		30 (10)	150 (173)
I.BLK-PO109773.D	PIBLK-PO109773.D	Tetrachloro-m-xylene	1	20	19.4	97		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	17.2	86		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	20.6	103		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	18.6	93		70 (60)	130 (140)



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q1522

Client: ENTACT

Analytical Method: **8082A** **Datafile :** PO109761.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD		Limits	
								Qual	Low	High	RPD
PB167042BS	AR1016	5	4.60	ug/L	92				40 (61)	140 (112)	
	AR1260	5	4.40	ug/L	88				40 (66)	140 (113)	

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q1522

Client: ENTACT

Analytical Method: **8082A** **Datafile :** PO109762.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD		Limits	
								Qual	Low	High	RPD
PB167042BSD	AR1016	5	4.60	ug/L	92	0			40 (61)	140 (112)	20 (20)
	AR1260	5	4.40	ug/L	88	0			40 (66)	140 (113)	20 (20)

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB167042BL

Lab Name: CHEMTECH

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522

SAS No.: Q1522 SDG NO.: Q1522

Lab Sample ID: PB167042BL

Lab File ID: PO109760.D

Matrix: (soil/water) WATER

Extraction: (Type) SEPF

Sulfur Cleanup: (Y/N) N

Date Extracted: 03/10/2025

Date Analyzed (1): 03/10/2025

Date Analyzed (2): 03/10/2025

Time Analyzed (1): 15:49

Time Analyzed (2): 15:49

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column (1): ZB-MR1 ID: 0.32 (mm)

GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
PB167042BS	PB167042BS	PO109761.D	03/10/2025	03/10/2025
PB167042BSD	PB167042BSD	PO109762.D	03/10/2025	03/10/2025
TW-WTS-04	Q1522-02	PO109764.D	03/10/2025	03/10/2025

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	ENTACT	Date Collected:	03/06/25
Project:	540 Degraw St, Brooklyn, NY - E9309	Date Received:	03/07/25
Client Sample ID:	TW-WTS-04	SDG No.:	Q1522
Lab Sample ID:	Q1522-02	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	990	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	3510C	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109764.D	1	03/10/25 08:48	03/10/25 17:03	PB167042

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.51	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.51	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.51	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.51	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.51	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.51	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.51	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.51	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.51	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	18.8		30 (16) - 150 (158)	94%	SPK: 20
2051-24-3	Decachlorobiphenyl	15.8		30 (10) - 150 (173)	79%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031025\
 Data File : P0109764.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2025 17:03
 Operator : YP/AJ
 Sample : Q1522-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TW-WTS-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 00:59:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.693	171.8E6	98504615	18.151	18.819
2) SA Decachlor...	8.749	8.702	123.3E6	50193516	14.331	15.763

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031025\
Data File : PO109764.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2025 17:03
Operator : YP/AJ
Sample : Q1522-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TW-WTS-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 00:59:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

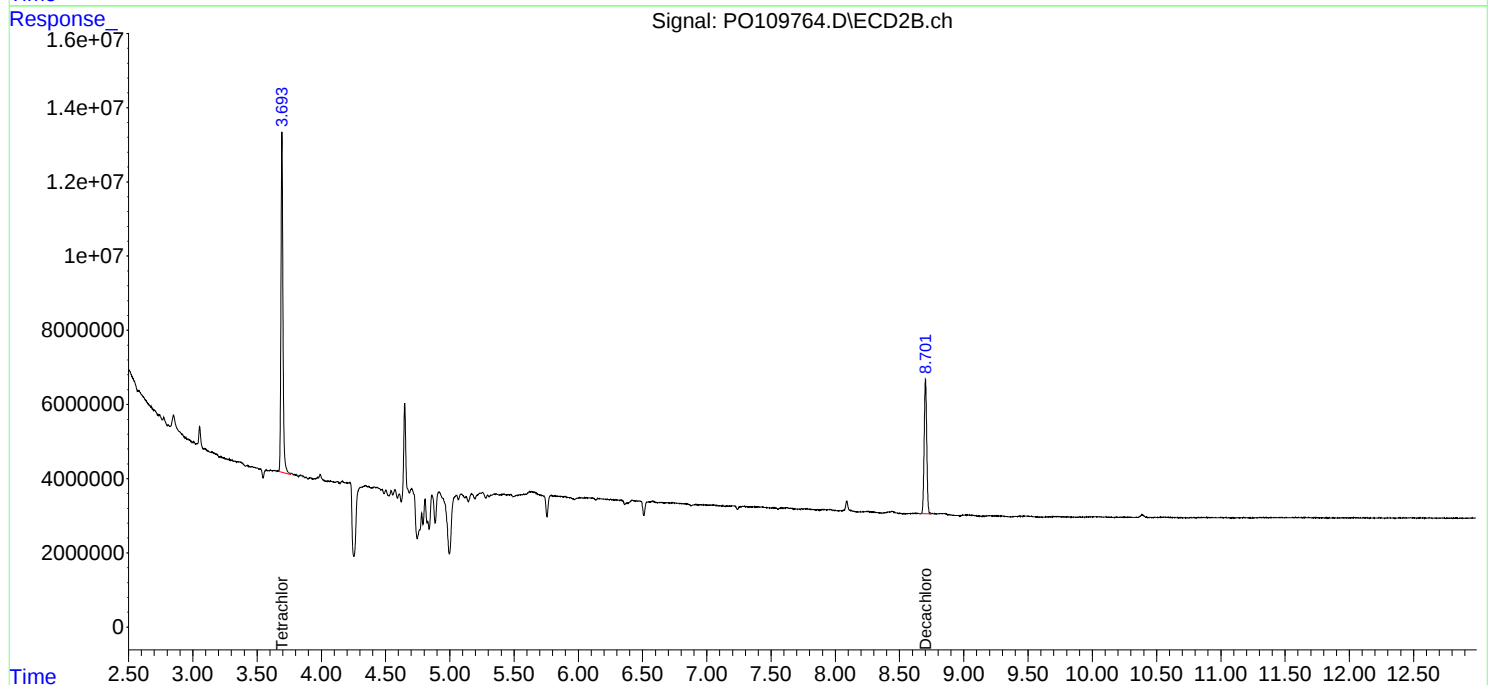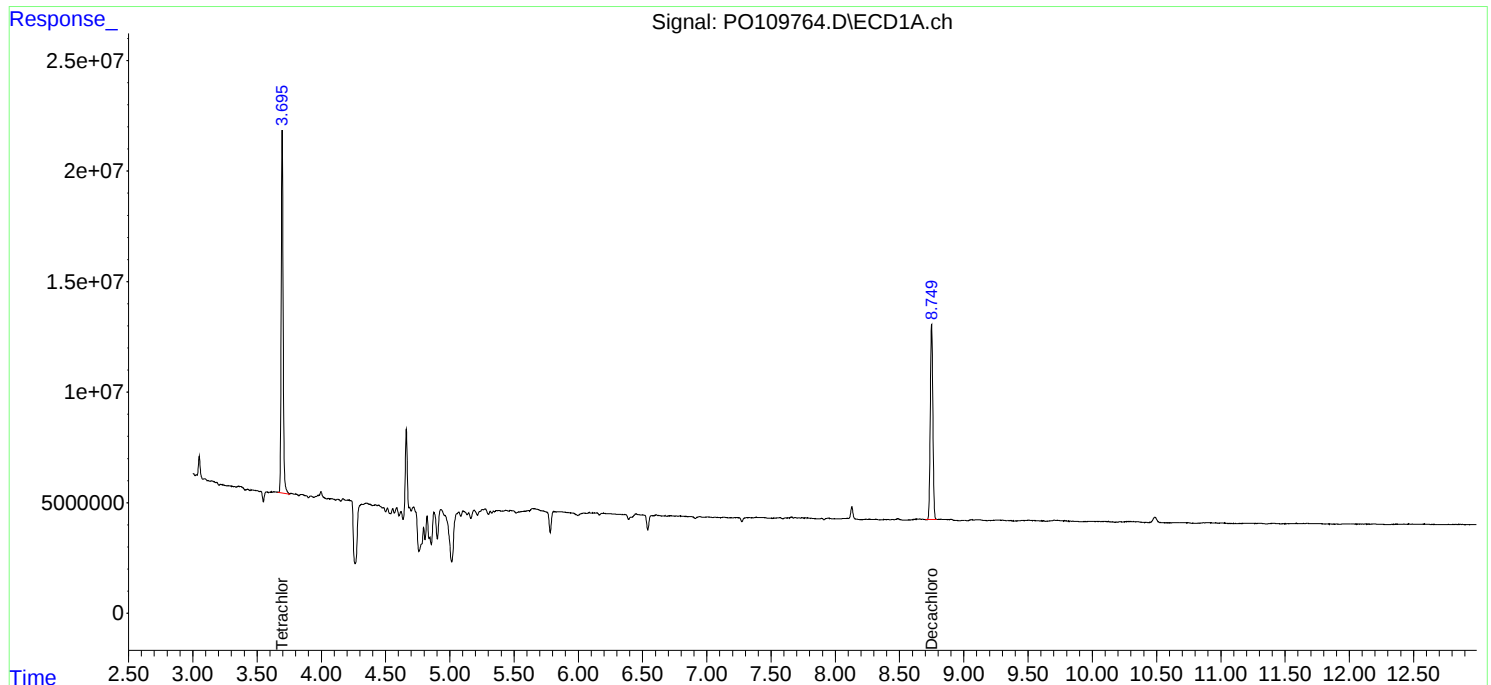


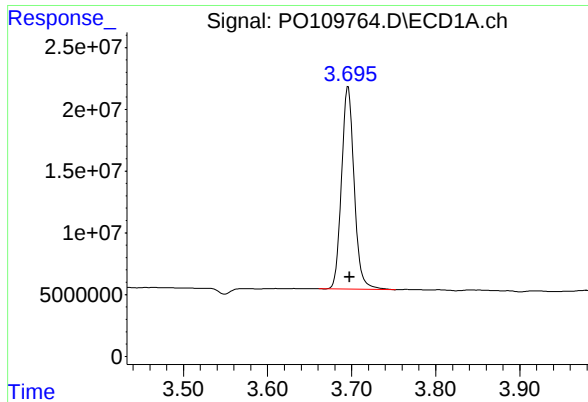

#1 Tetrachloro-m-xylene


R.T.: 3.696 min
Delta R.T.: -0.002 min
Response: 171797868
Conc: 18.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
TW-WTS-04

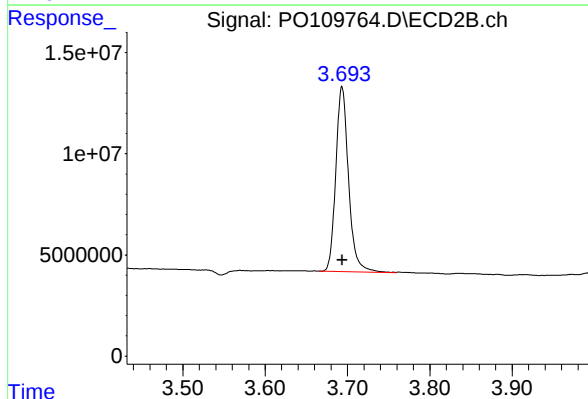


#1 Tetrachloro-m-xylene

R.T.: 3.693 min
Delta R.T.: 0.000 min
Response: 98504615
Conc: 18.82 ng/ml

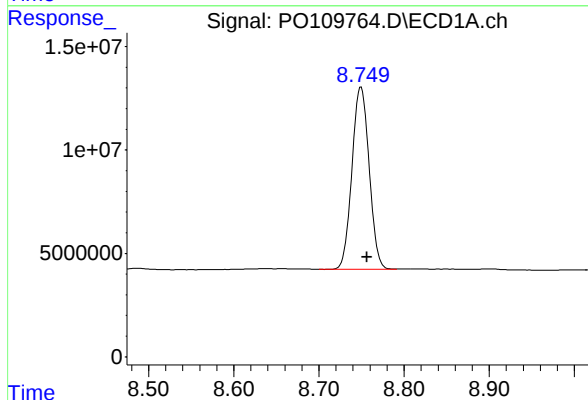

#2 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: -0.007 min
Response: 123269486
Conc: 14.33 ng/ml

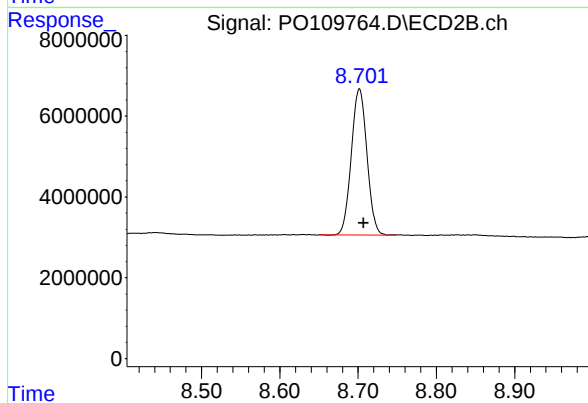

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.005 min
Response: 50193516
Conc: 15.76 ng/ml



CALIBRATION SUMMARY

GC Column: ZB-MR1 ID: 0.32 (mm)

[illegible]

[illegible]

RETENTION TIMES OF INITIAL CALIBRATION

Contract:	<u>ENTA05</u>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q1522</u>	SAS No.:	<u>Q1522</u>	SDG NO.:	<u>Q1522</u>
Instrument ID:	<u>ECD_O</u>	Calibration Date(s):		<u>02/20/2025</u>	<u>02/21/2025</u>		
		Calibration Times:		<u>16:46</u>	<u>01:02</u>		

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID: RT 1000 = PO109426.D RT 750 = PO109427.D
RT 500 = PO109428.D RT 250 = PO109429.D RT 050 = PO109430.D

[illegible]

[illegible]

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: ENTA05
Lab Code: CHEM **Case No.:** Q1522 **SAS No.:** Q1522 **SDG NO.:** Q1522
Instrument ID: ECD_O
Calibration Date(s): 02/20/2025 02/21/2025
Calibration Times: 16:46 01:02

GC Column: ZB-MR1 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO109426.D</u>		CF 750 = <u>PO109427.D</u>			
CF 500 = <u>PO109428.D</u>		CF 250 = <u>PO109429.D</u>		CF 050 = <u>PO109430.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	285955176	296470909	301678880	330073932	327272520	308290283
Aroclor-1016-2	(2)	400344510	409149469	414645114	446605912	434387780	421026557
Aroclor-1016-3	(3)	275712654	284750529	289403798	321232168	307985600	295816950
Aroclor-1016-4	(4)	217819857	224475380	225979744	249359212	241266360	231780111
Aroclor-1016-5	(5)	234915990	244172492	252269048	280073416	279718840	258229957
Aroclor-1260-1	(1)	432857882	445030616	458030860	496965692	497771560	466131322
Aroclor-1260-2	(2)	530613873	540598143	549997768	596865796	607516180	565118352
Aroclor-1260-3	(3)	446055940	458685821	463532386	505033376	504998020	475661109
Aroclor-1260-4	(4)	409227231	417077069	426071740	458083200	447546300	431601108
Aroclor-1260-5	(5)	975246933	982402905	1001465846	1034939896	975352280	993881572
Decachlorobiphenyl		8144381710	8253336907	8542716440	9068866760	9000001000	8601860563
Tetrachloro-m-xylene		9594159870	9382441773	9407964980	9839303320	9101752600	9465124509
Aroclor-1242-1	(1)	241553792	248781753	263582376	278206104	276700060	261764817
Aroclor-1242-2	(2)	330250979	341141312	360022594	377835792	370979720	356046079
Aroclor-1242-3	(3)	230958690	239403319	256570990	271941764	257976860	251370325
Aroclor-1242-4	(4)	181873604	188232188	200194694	210194852	201763980	196451864
Aroclor-1242-5	(5)	192196869	198312276	212424054	232317448	236630280	214376185
Decachlorobiphenyl		7571460160	7783053733	8197005760	8686332120	8704566000	8188483555
Tetrachloro-m-xylene		9236931880	9400204853	9446860340	9568057960	9056865000	9341784007
Aroclor-1248-1	(1)	183385441	189253437	200901320	213658596	210346400	199509039
Aroclor-1248-2	(2)	249519113	262229969	281655510	299590856	298458120	278290714
Aroclor-1248-3	(3)	313646829	324719312	346217716	370103360	392176240	349372691
Aroclor-1248-4	(4)	439951399	452724037	479184310	509535492	504078340	477094716
Aroclor-1248-5	(5)	310476659	318507132	337630456	365736804	380196620	342509534
Decachlorobiphenyl		7703959900	7913043760	8337132500	8816038680	8879579800	8329950928
Tetrachloro-m-xylene		9154374770	9319706587	9763537060	9884300480	9250244600	9474432699
Aroclor-1254-1	(1)	480630669	491242291	514290722	548494120	543375540	515606668
Aroclor-1254-2	(2)	417535343	429223996	451482582	481224324	472406420	450374533
Aroclor-1254-3	(3)	684838056	697322969	725628940	760808456	711178620	715955408
Aroclor-1254-4	(4)	417970360	409808872	428749386	461366848	376062040	418791501
Aroclor-1254-5	(5)	597298518	608943563	631623464	663830224	617819000	623902954
Decachlorobiphenyl		7967092830	8125756000	8528343640	8986366600	8782372000	8477986214
Tetrachloro-m-xylene		9511051460	9602004080	9843620680	9994457760	8495604200	9489347636
Aroclor-1268-1	(1)	1298860853	1294002563	1318124330	1365675636	1344427900	1324218256



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	1196326079	1189492827	1207881780	1246550744	1205280700	1209106426	2
Aroclor-1268-3	(3)	1000400149	998939115	1012813102	1049647308	1029090160	1018177967	2
Aroclor-1268-4	(4)	407507962	408969772	420298422	442140308	445377360	424858765	4
Aroclor-1268-5	(5)	3060378797	3013397139	3036609122	3075360324	2912511720	3019651420	2
Decachlorobiphenyl		14147642890	14125651173	14472115980	15180190720	15441285400	14673377233	4
Tetrachloro-m-xylene		9652630020	9799388160	9953085600	10360200640	9708060200	9894672924	3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522 SAS No.: Q1522 SDG NO.: Q1522

Instrument ID: ECD_O

Calibration Date(s): 02/20/2025 02/21/2025

Calibration Times: 16:46 01:02

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO109426.D</u>		CF 750 = <u>PO109427.D</u>			
CF 500 = <u>PO109428.D</u>		CF 250 = <u>PO109429.D</u>		CF 050 = <u>PO109430.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	144422659	148428763	152032096	167484860	168484300	156170536
Aroclor-1016-2	(2)	205202725	208508729	213432994	229519564	225505040	216433810
Aroclor-1016-3	(3)	112302196	115067393	117212622	128579748	124094120	119451216
Aroclor-1016-4	(4)	94709981	98717735	101165102	112923876	112836120	104070563
Aroclor-1016-5	(5)	124417087	127943616	132644098	146345704	149917060	136253513
Aroclor-1260-1	(1)	217936136	223782013	232739904	251644640	258495520	236919643
Aroclor-1260-2	(2)	255563339	259366392	268832038	291215424	300878620	275171163
Aroclor-1260-3	(3)	239301078	242165468	249897958	270279452	273707020	255070195
Aroclor-1260-4	(4)	193987222	196916529	202218624	218214048	219624820	206192249
Aroclor-1260-5	(5)	436097628	435546231	443785112	464386884	459099080	447782987
Decachlorobiphenyl		2971514290	3027039307	3156019460	3385128400	3381593200	3184258931
Tetrachloro-m-xylene		5186272490	5246400280	5221242400	5478386840	5038748400	5234210082
Aroclor-1242-1	(1)	120966720	124746516	133128702	141428800	141463920	132346932
Aroclor-1242-2	(2)	169605960	173512545	183266616	192017376	189176180	181515735
Aroclor-1242-3	(3)	93390359	96634075	102245092	107691940	99411220	99874537
Aroclor-1242-4	(4)	96389066	101019272	107789002	115338428	114056640	106918482
Aroclor-1242-5	(5)	113196636	117716005	125239314	135801980	136573300	125705447
Decachlorobiphenyl		2727823240	2861750760	3019178360	3243379080	3243962600	3019218808
Tetrachloro-m-xylene		5001213420	5078322907	5254229320	5289448280	4851665000	5094975785
Aroclor-1248-1	(1)	91256927	94139561	100767396	107614600	108857060	100527109
Aroclor-1248-2	(2)	130560541	136645137	146421094	157143508	156628300	145479716
Aroclor-1248-3	(3)	139283148	144897643	155701690	166430352	168727860	155008139
Aroclor-1248-4	(4)	163903044	169411200	180364434	193711724	196594760	180797032
Aroclor-1248-5	(5)	154356880	158447996	169575560	183331920	195308840	172204239
Decachlorobiphenyl		2790488700	2873613467	3038569420	3241156720	3294897400	3047745141
Tetrachloro-m-xylene		4955293160	5040468413	5221131320	5264696400	4750589600	5046435779
Aroclor-1254-1	(1)	243640751	248872624	260914738	280861344	273402140	261538319
Aroclor-1254-2	(2)	212545511	218679507	230680254	249214456	261687520	234561450
Aroclor-1254-3	(3)	339799719	346366689	360950750	378906048	357499640	356704569
Aroclor-1254-4	(4)	192329190	189854227	199746634	214807996	168878980	193123405
Aroclor-1254-5	(5)	278490681	283928981	296376396	314100456	310764660	296732235
Decachlorobiphenyl		2841760820	2921691133	3072525860	3310057280	3280037800	3085214579
Tetrachloro-m-xylene		5117525260	5147853200	5214583540	5337931960	4481650800	5059908952
Aroclor-1268-1	(1)	554131487	553810328	564174560	591076320	593868340	571412207



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	512614105	511079256	520949472	543420336	536655740	524943782	3
Aroclor-1268-3	(3)	413643589	412567932	420525622	442592008	450889440	428043718	4
Aroclor-1268-4	(4)	153729603	155030577	163078820	169661456	165174880	161335067	4
Aroclor-1268-5	(5)	1087226853	1077982207	1085826158	1121186428	1093500600	1093144449	2
Decachlorobiphenyl		4950835750	4972853373	5123922200	5430816080	5582978400	5212281161	5
Tetrachloro-m-xylene		5266816140	5271127760	5328349480	5507659840	5128975000	5300585644	3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522 SAS No.: Q1522 SDG NO.: Q1522

Instrument ID: ECD_O Date(s) Analyzed: 02/20/2025 02/21/2025

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.91	3.81	4.01	131879000
		2	4.00	3.90	4.10	98701000
		3	4.07	3.97	4.17	269838000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.07	3.97	4.17	208928000
		2	4.57	4.47	4.67	116083000
		3	4.81	4.71	4.91	201936000
		4	4.99	4.89	5.09	111220000
		5	5.03	4.93	5.13	81668600
Aroclor-1262	500	1	6.85	6.75	6.95	665842000
		2	7.35	7.25	7.45	1129720000
		3	7.63	7.53	7.73	448264000
		4	7.70	7.60	7.80	829210000
		5	8.19	8.09	8.29	373330000



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522 SAS No.: Q1522 SDG NO.: Q1522

Instrument ID: ECD_O Date(s) Analyzed: 02/20/2025 02/21/2025

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.91	3.81	4.01	68502400
		2	3.99	3.89	4.09	51339800
		3	4.07	3.97	4.17	145428000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.07	3.97	4.17	111462000
		2	4.80	4.70	4.90	103317000
		3	4.97	4.87	5.07	56771800
		4	5.06	4.96	5.16	54894600
		5	5.23	5.13	5.33	58805000
Aroclor-1262	500	1	6.81	6.71	6.91	317212000
		2	7.31	7.21	7.41	498620000
		3	7.60	7.50	7.70	196255000
		4	7.66	7.56	7.76	354890000
		5	8.15	8.05	8.25	143138000

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 16:46
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:01:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:00:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	959.4E6	518.6E6	101.979	99.330
2) SA Decachlor...	8.757	8.706	814.4E6	297.2E6	95.337	94.154
Target Compounds						
3) L1 AR-1016-1	4.792	4.777	286.0E6	144.4E6	947.879	949.948
4) L1 AR-1016-2	4.811	4.797	400.3E6	205.2E6	965.511	961.439
5) L1 AR-1016-3	4.867	4.972	275.7E6	112.3E6	952.692	958.107
6) L1 AR-1016-4	4.988	5.014	217.8E6	94709981	963.891	936.192
7) L1 AR-1016-5	5.246	5.228	234.9E6	124.4E6	931.212	937.977
31) L7 AR-1260-1	6.288	6.261	432.9E6	217.9E6	945.041	936.394
32) L7 AR-1260-2	6.477	6.448	530.6E6	255.6E6	964.756	950.643
33) L7 AR-1260-3	6.845	6.602	446.1E6	239.3E6	962.297	957.595
34) L7 AR-1260-4	7.106	7.073	409.2E6	194.0E6	960.466	959.295
35) L7 AR-1260-5	7.347	7.314	975.2E6	436.1E6	973.819	982.677



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 16:46
Operator : YP/AJ
Sample : AR1660ICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:01:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:00:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

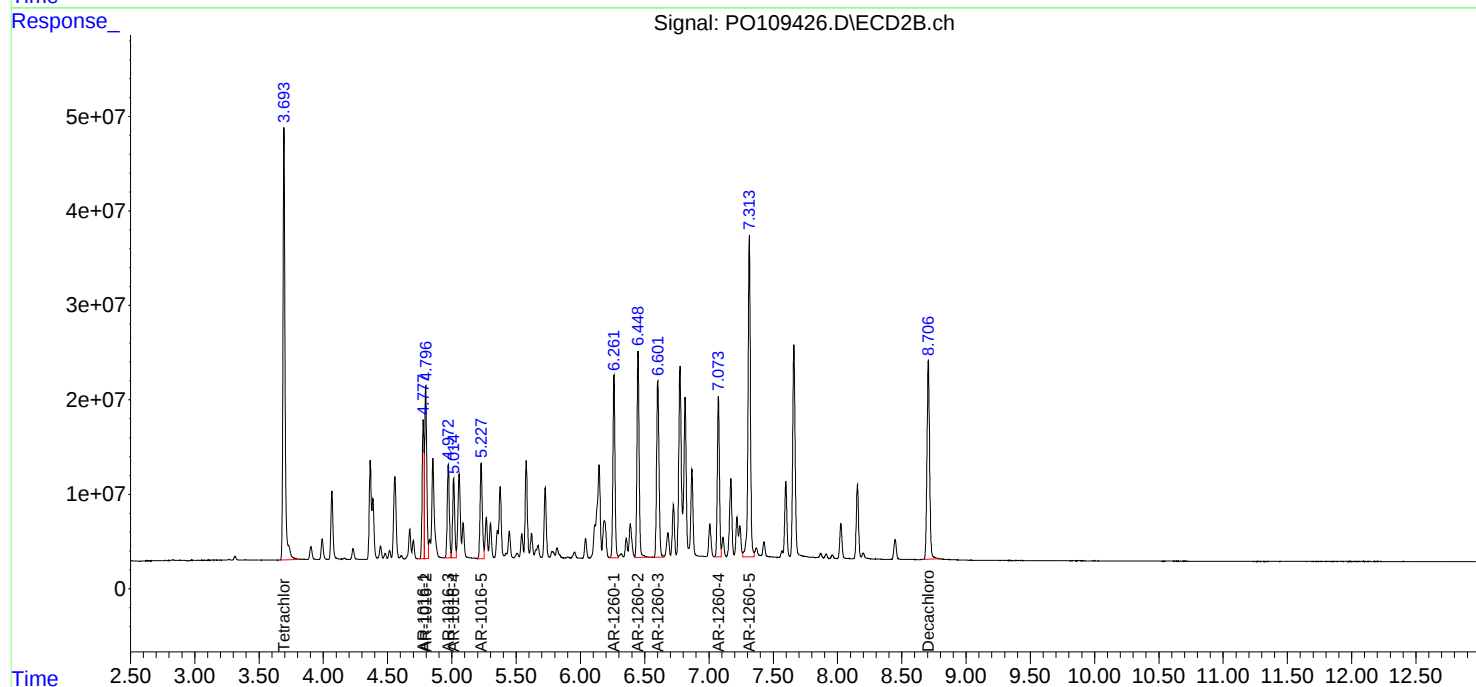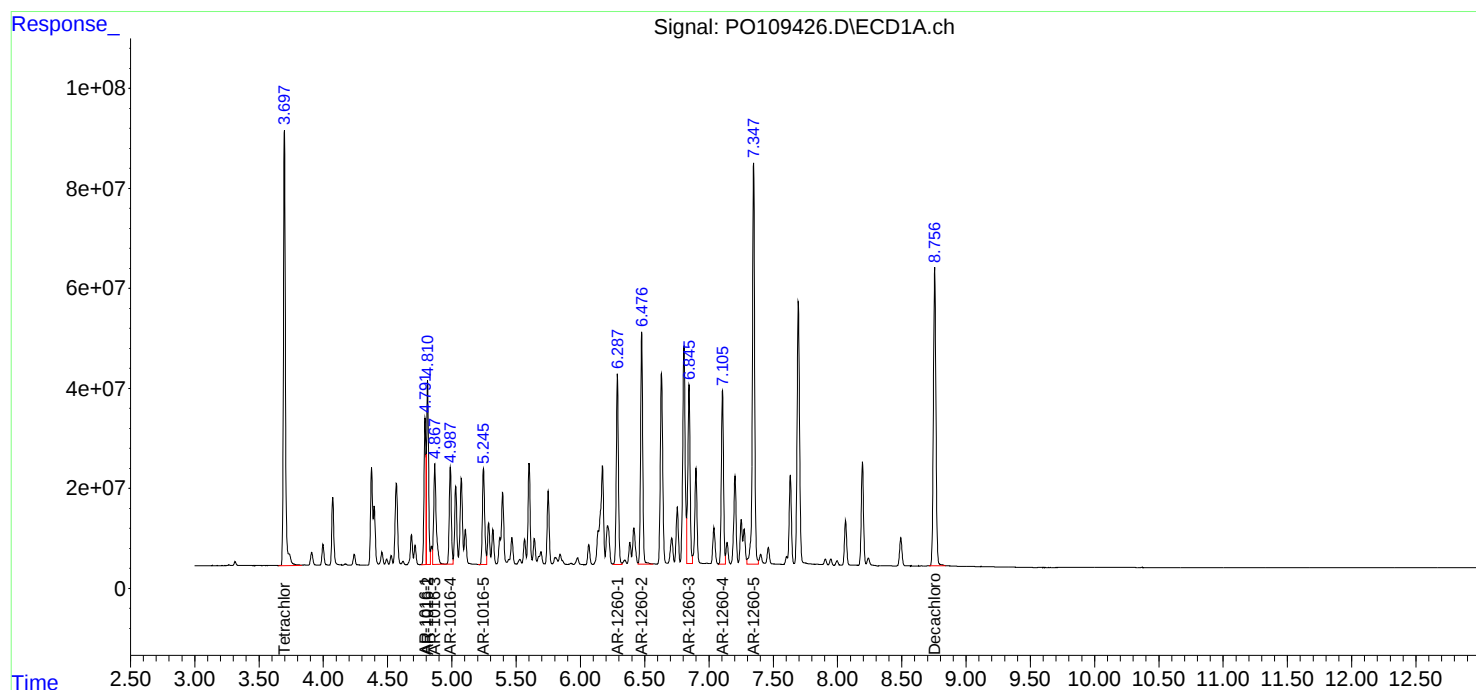

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 17:04
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:01:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:00:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	703.7E6	393.5E6	74.797	75.361
2) SA Decachlor...	8.756	8.707	619.0E6	227.0E6	72.459	71.935
Target Compounds						
3) L1 AR-1016-1	4.792	4.777	222.4E6	111.3E6	737.053	732.224
4) L1 AR-1016-2	4.811	4.797	306.9E6	156.4E6	740.060	732.696
5) L1 AR-1016-3	4.868	4.972	213.6E6	86300545	737.941	736.273
6) L1 AR-1016-4	4.988	5.014	168.4E6	74038301	745.007	731.856
7) L1 AR-1016-5	5.246	5.227	183.1E6	95957712	725.929	723.422
31) L7 AR-1260-1	6.288	6.261	333.8E6	167.8E6	728.713	721.133
32) L7 AR-1260-2	6.477	6.448	405.4E6	194.5E6	737.182	723.592
33) L7 AR-1260-3	6.845	6.602	344.0E6	181.6E6	742.158	726.793
34) L7 AR-1260-4	7.106	7.073	312.8E6	147.7E6	734.167	730.335
35) L7 AR-1260-5	7.347	7.314	736.8E6	326.7E6	735.724	736.076



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 17:04
Operator : YP/AJ
Sample : AR1660ICC750
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:01:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:00:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

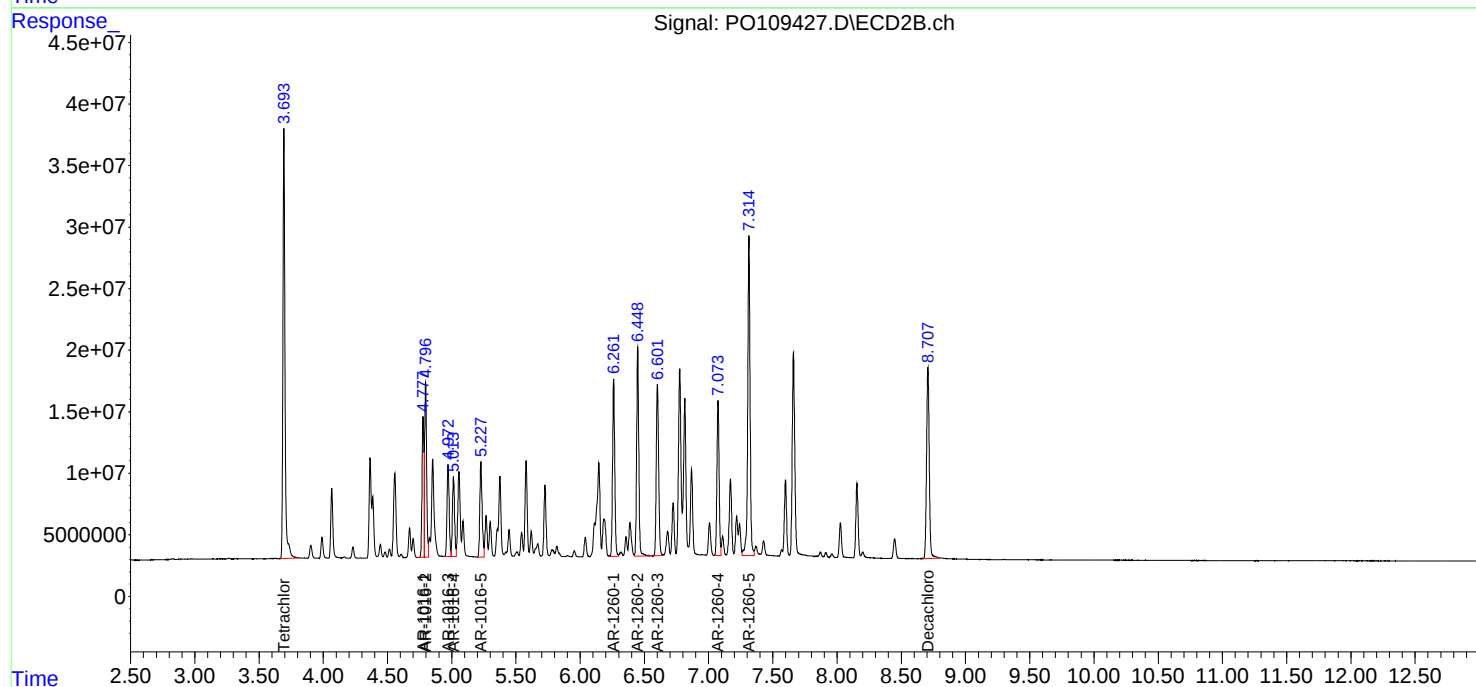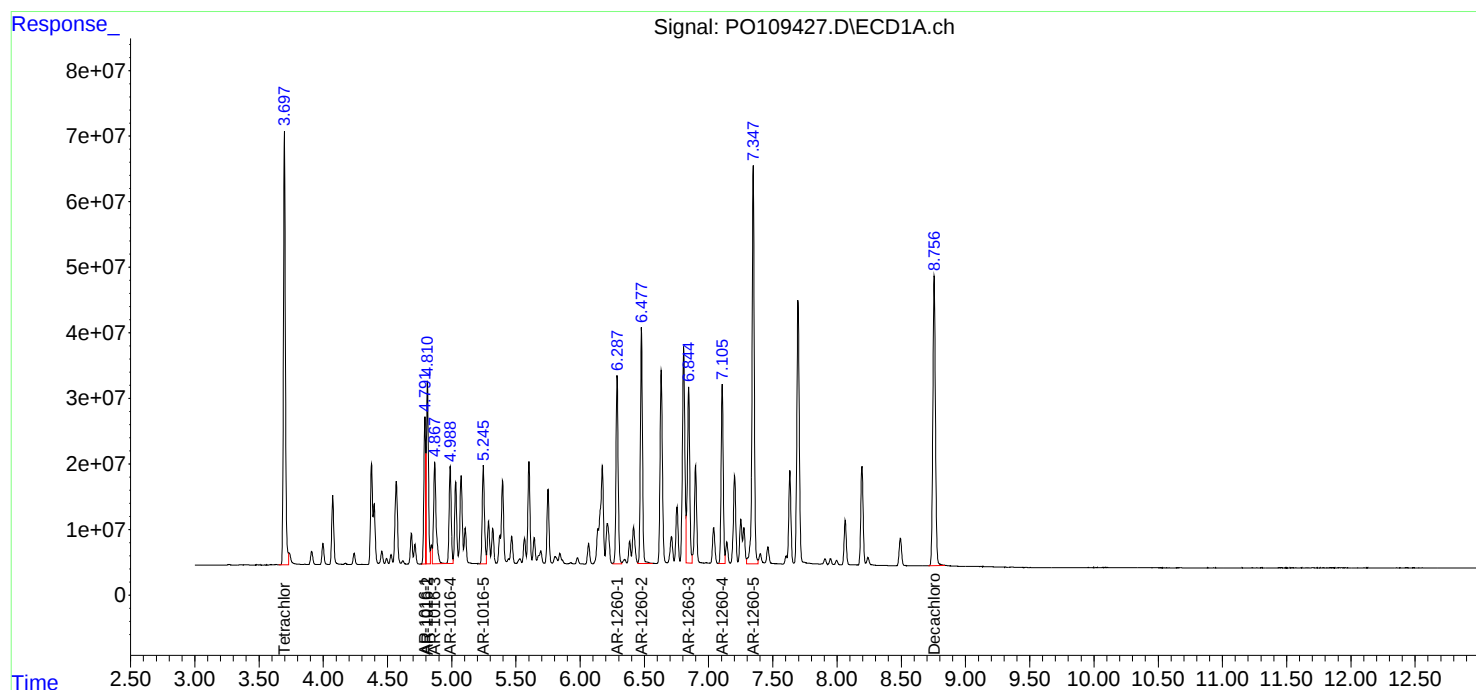

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 17:23
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:01:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:00:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.698	3.694	470.4E6	261.1E6	50.000	50.000
2) SA Decachlor...	8.757	8.707	427.1E6	157.8E6	50.000	50.000
Target Compounds						
3) L1 AR-1016-1	4.791	4.778	150.8E6	76016048	500.000	500.000
4) L1 AR-1016-2	4.811	4.797	207.3E6	106.7E6	500.000	500.000
5) L1 AR-1016-3	4.867	4.972	144.7E6	58606311	500.000	500.000
6) L1 AR-1016-4	4.988	5.014	113.0E6	50582551	500.000	500.000
7) L1 AR-1016-5	5.245	5.227	126.1E6	66322049	500.000	500.000
31) L7 AR-1260-1	6.288	6.261	229.0E6	116.4E6	500.000	500.000
32) L7 AR-1260-2	6.477	6.448	275.0E6	134.4E6	500.000	500.000
33) L7 AR-1260-3	6.846	6.602	231.8E6	124.9E6	500.000	500.000
34) L7 AR-1260-4	7.105	7.074	213.0E6	101.1E6	500.000	500.000
35) L7 AR-1260-5	7.347	7.314	500.7E6	221.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 17:23
Operator : YP/AJ
Sample : AR1660ICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:01:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:00:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

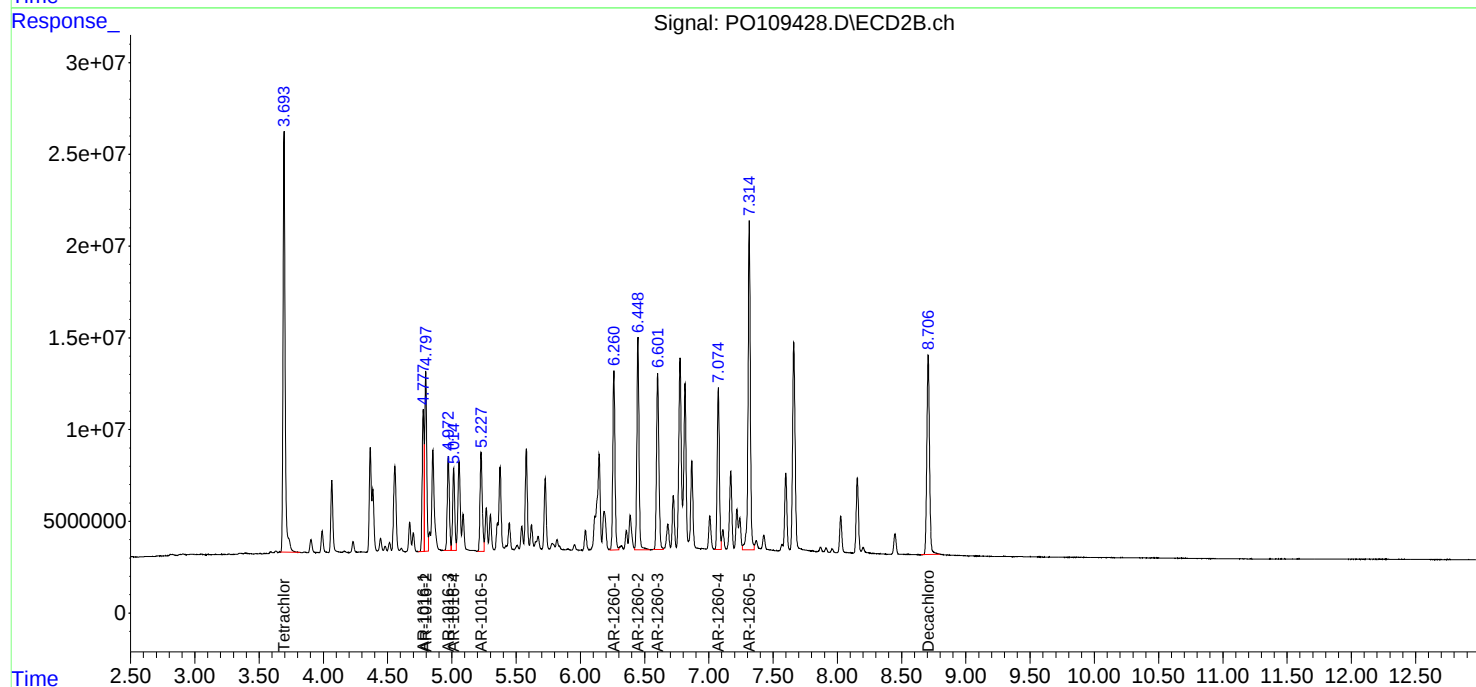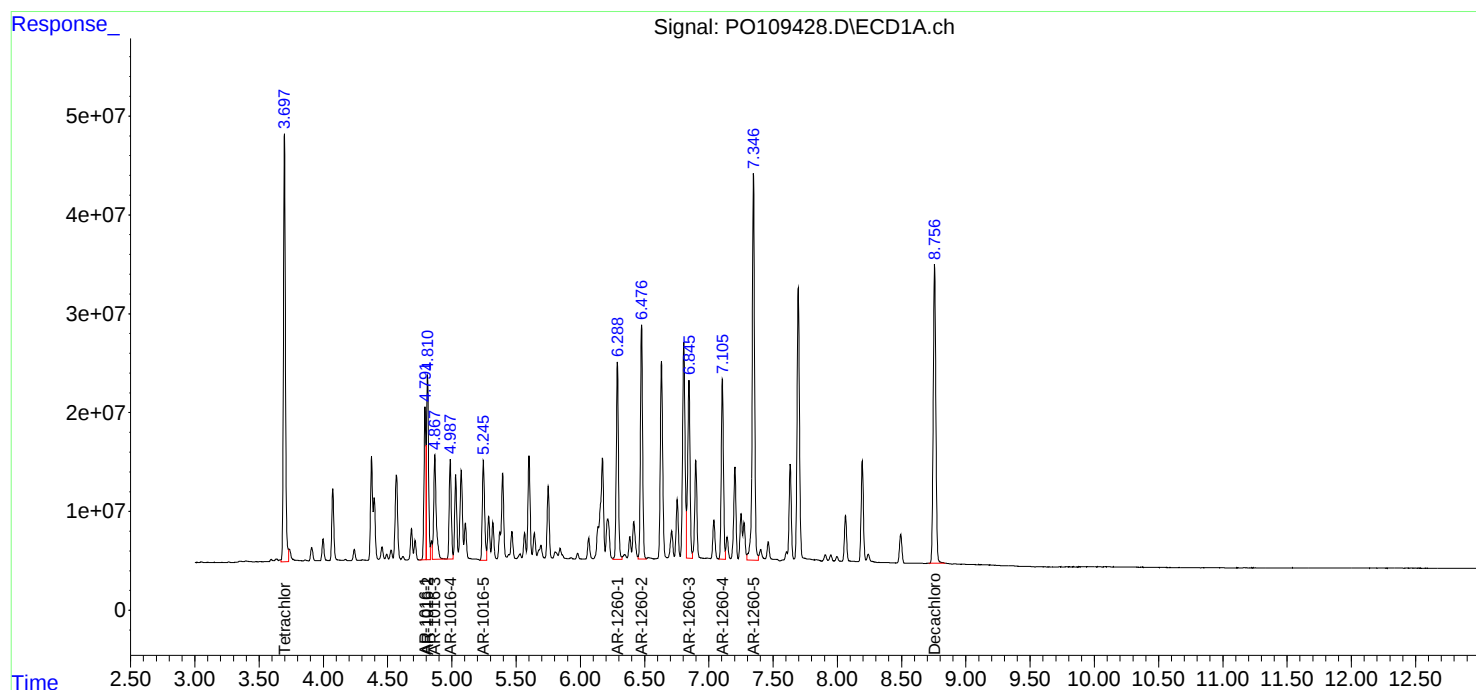

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 17:41
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:02:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:00:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	246.0E6	137.0E6	26.146	26.231
2) SA Decachlor...	8.756	8.706	226.7E6	84628210	26.540	26.815
Target Compounds						
3) L1 AR-1016-1	4.792	4.777	82518483	41871215	273.531	275.410
4) L1 AR-1016-2	4.811	4.797	111.7E6	57379891	269.270	268.843
5) L1 AR-1016-3	4.867	4.972	80308042	32144937	277.495	274.245
6) L1 AR-1016-4	4.988	5.014	62339803	28230969	275.865	279.058
7) L1 AR-1016-5	5.245	5.227	70018354	36586426	277.554	275.824
31) L7 AR-1260-1	6.288	6.261	124.2E6	62911160	271.251	270.307
32) L7 AR-1260-2	6.477	6.448	149.2E6	72803856	271.304	270.815
33) L7 AR-1260-3	6.845	6.602	126.3E6	67569863	272.383	270.390
34) L7 AR-1260-4	7.105	7.073	114.5E6	54553512	268.783	269.775
35) L7 AR-1260-5	7.347	7.313	258.7E6	116.1E6	258.356	261.606



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 17:41
Operator : YP/AJ
Sample : AR1660ICC250
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:02:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:00:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

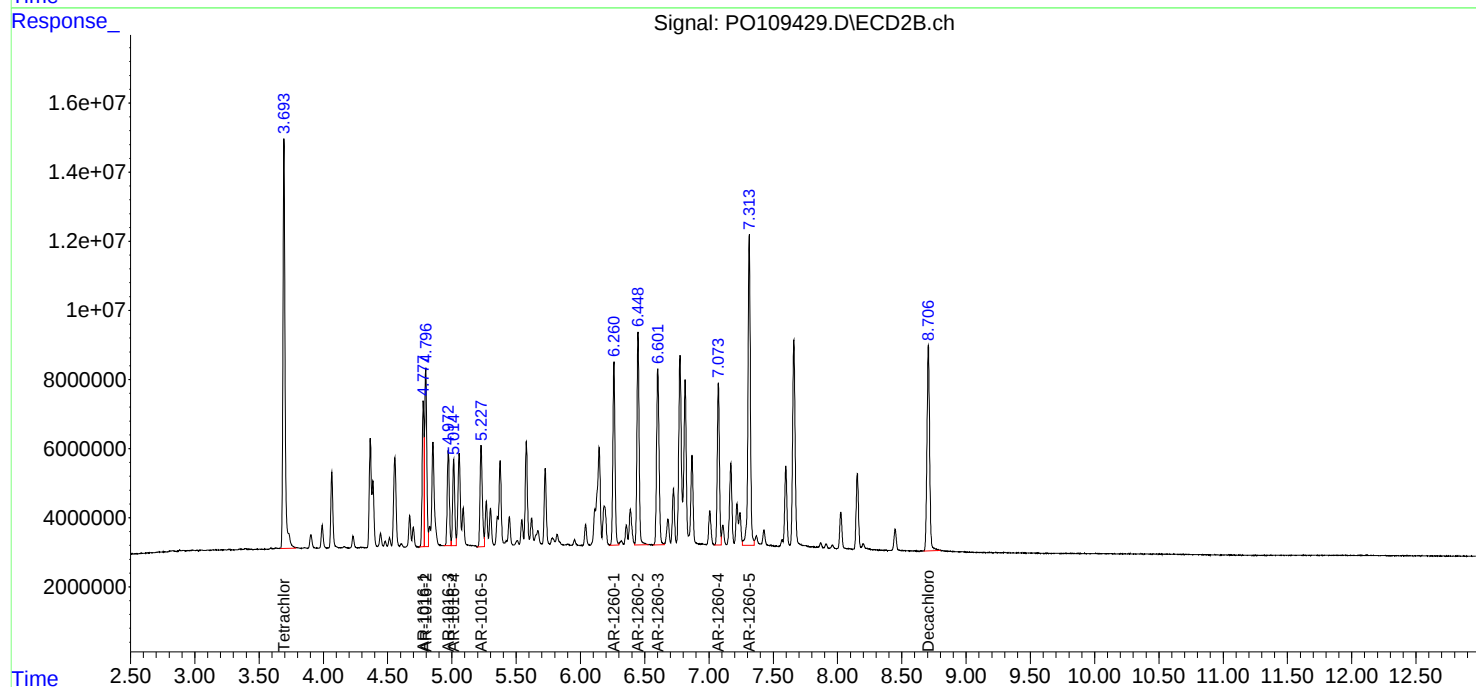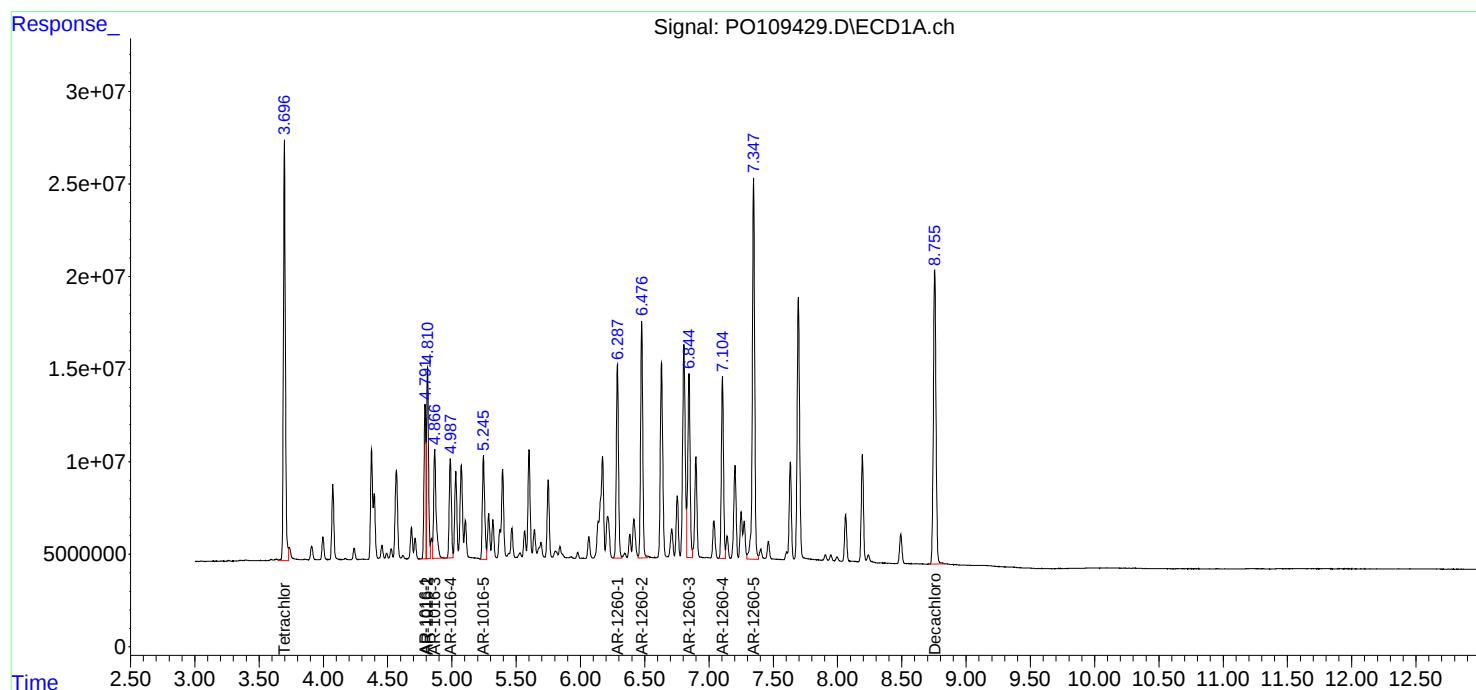

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 17:59
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:02:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:00:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	45508763	25193742	4.837	4.825
2) SA Decachlor...	8.755	8.705	45000005	16907966	5.268	5.357
Target Compounds						
3) L1 AR-1016-1	4.792	4.777	16363626	8424215	54.242	55.411
4) L1 AR-1016-2	4.812	4.796	21719389	11275252	52.381	52.828
5) L1 AR-1016-3	4.867	4.972	15399280	6204706	53.210	52.935
6) L1 AR-1016-4	4.988	5.014	12063318	5641806	53.382	55.768
7) L1 AR-1016-5	5.246	5.227	13985942	7495853	55.441	56.511
31) L7 AR-1260-1	6.287	6.261	24888578	12924776	54.338	55.533
32) L7 AR-1260-2	6.476	6.448	30375809	15043931	55.229	55.960
33) L7 AR-1260-3	6.844	6.601	25249901	13685351	54.473	54.764
34) L7 AR-1260-4	7.104	7.073	22377315	10981241	52.520	54.304
35) L7 AR-1260-5	7.346	7.313	48767614	22954954	48.696	51.725



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 17:59
Operator : YP/AJ
Sample : AR1660ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:02:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:00:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

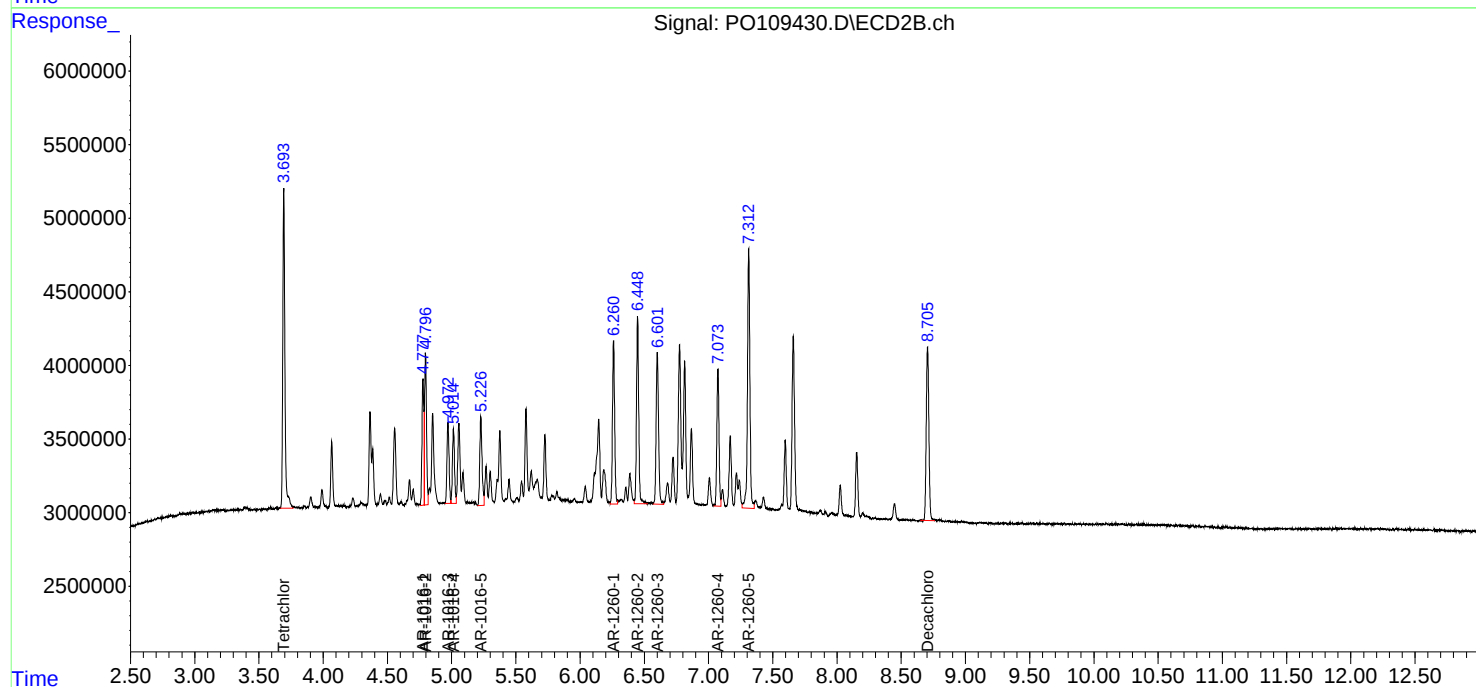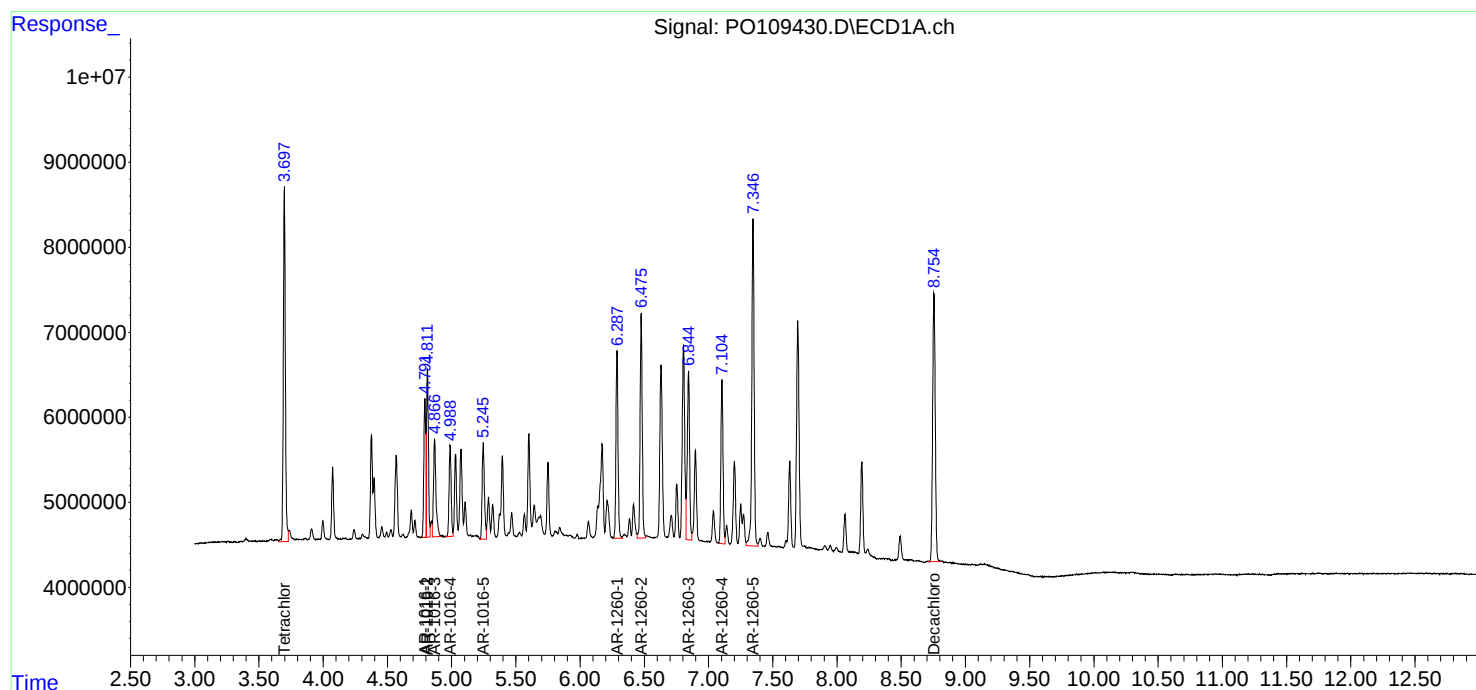

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 18:18
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:14:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:14:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	493.2E6	265.7E6	50.000	50.000
2) SA Decachlor...	8.755	8.707	432.4E6	160.0E6	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	3.910	3.905	65939528	34251207	500.000	500.000
9) L2 AR-1221-2	3.997	3.990	49350500	25669896	500.000	500.000
10) L2 AR-1221-3	4.074	4.066	134.9E6	72714061	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 18:18
Operator : YP/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:14:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:14:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

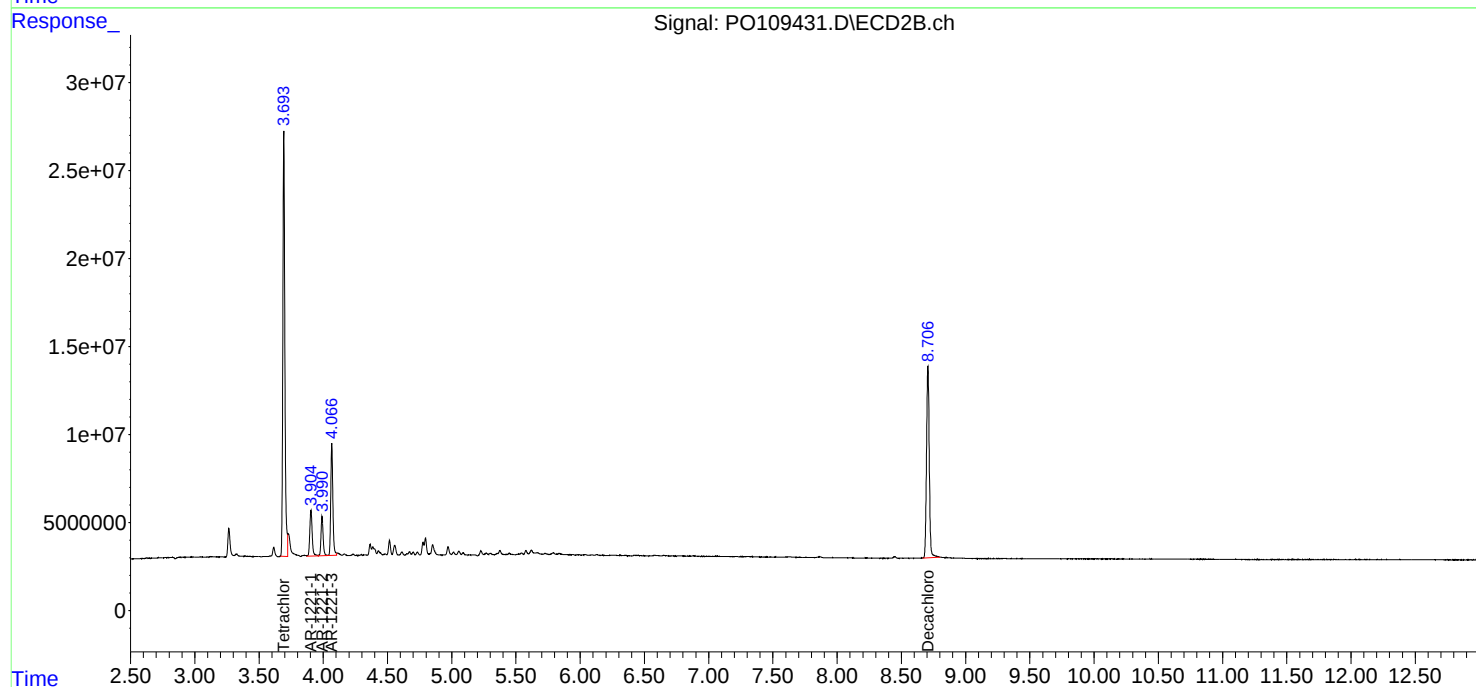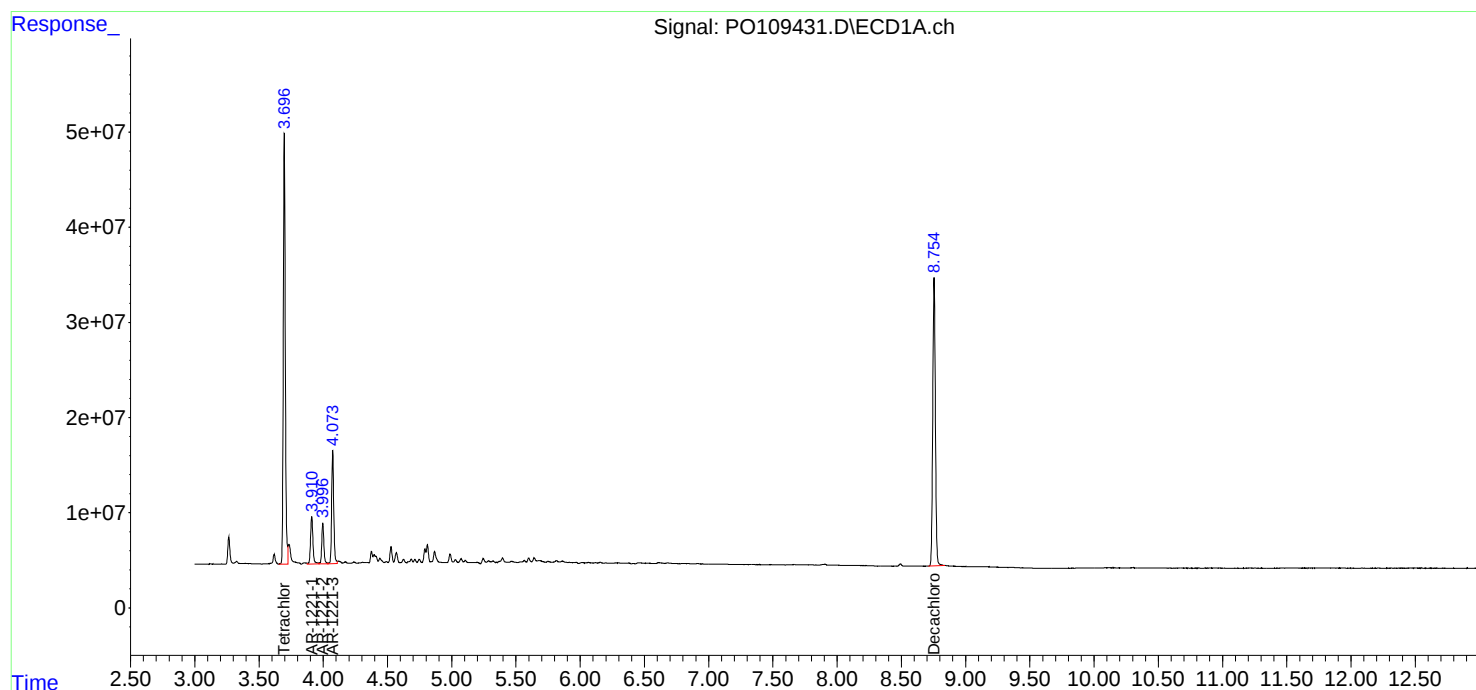

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 18:36
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:23:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:22:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	461.7E6	262.6E6	50.000	50.000
2) SA Decachlor...	8.757	8.706	402.2E6	149.0E6	50.000	50.000
Target Compounds						
11) L3 AR-1232-1	4.074	4.066	104.5E6	55730818	500.000	500.000
12) L3 AR-1232-2	4.569	4.796	58041447	51658633	500.000	500.000
13) L3 AR-1232-3	4.811	4.972	101.0E6	28385926	500.000	500.000
14) L3 AR-1232-4	4.988	5.056	55610100	27447264	500.000	500.000
15) L3 AR-1232-5	5.030	5.227	40834319	29402463	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 18:36
Operator : YP/AJ
Sample : AR1232ICC500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:23:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:22:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

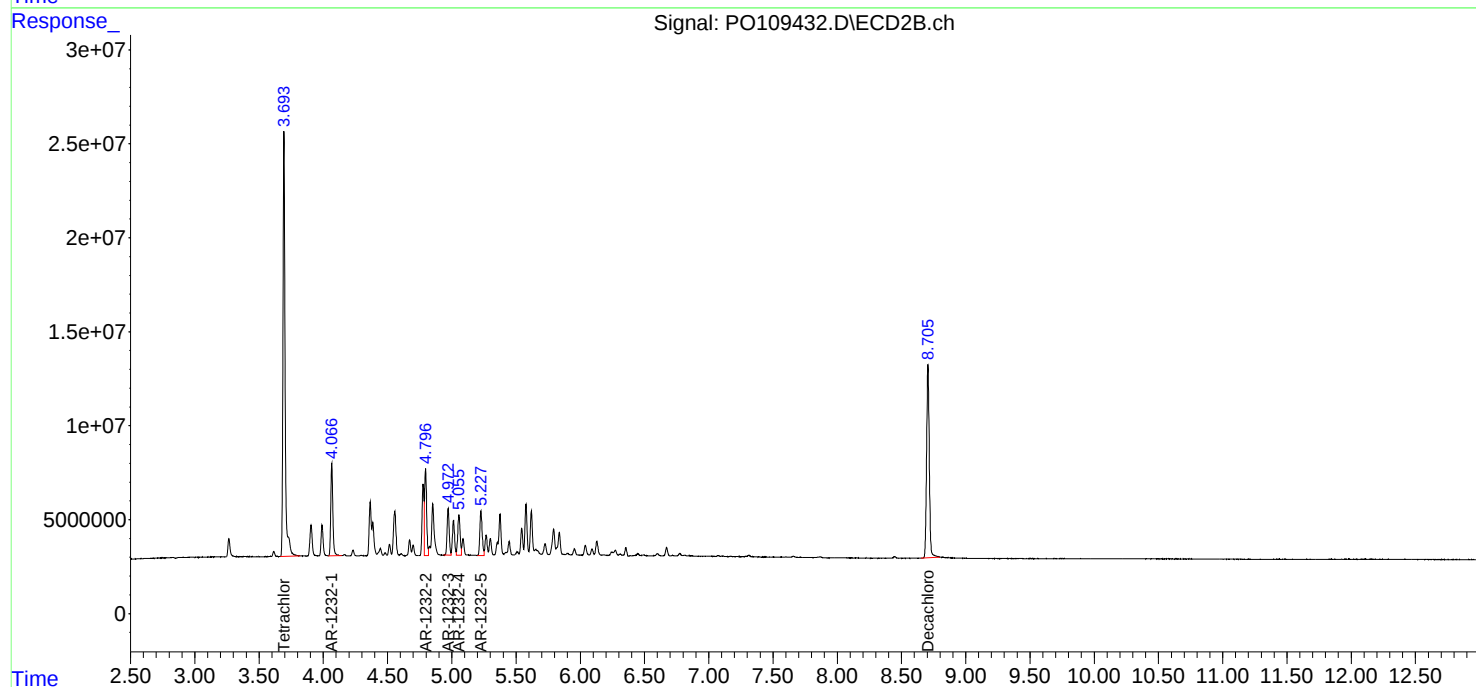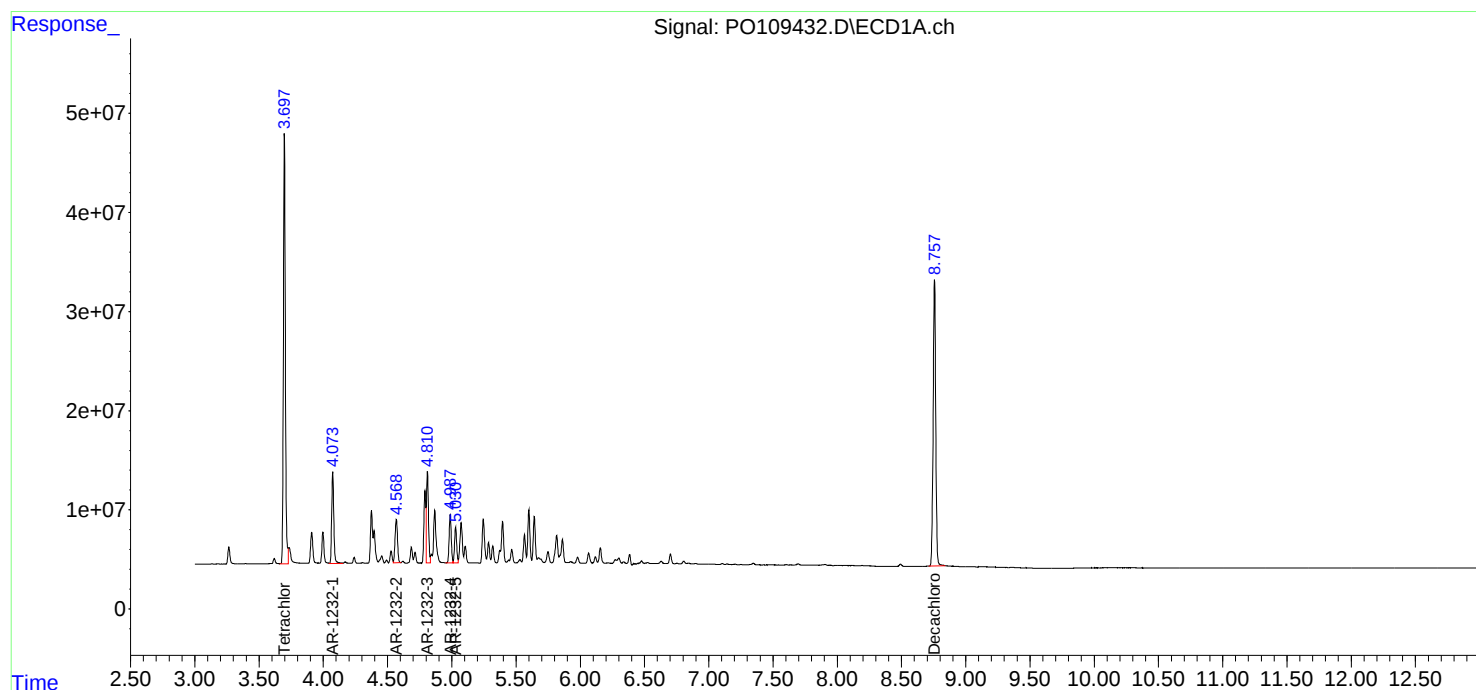

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 18:55
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:27:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:26:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	923.7E6	500.1E6	97.778	95.185
2) SA Decachlor...	8.755	8.706	757.1E6	272.8E6	92.369	90.350
Target Compounds						
16) L4 AR-1242-1	4.792	4.777	241.6E6	121.0E6	916.426	908.645
17) L4 AR-1242-2	4.811	4.797	330.3E6	169.6E6	917.306	925.460
18) L4 AR-1242-3	4.867	4.972	231.0E6	93390359	900.175	913.397
19) L4 AR-1242-4	4.988	5.056	181.9E6	96389066	908.484	894.238
20) L4 AR-1242-5	5.642	5.579	192.2E6	113.2E6	904.779	903.843



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109433.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 18:55
Operator : YP/AJ
Sample : AR1242ICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:27:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:26:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

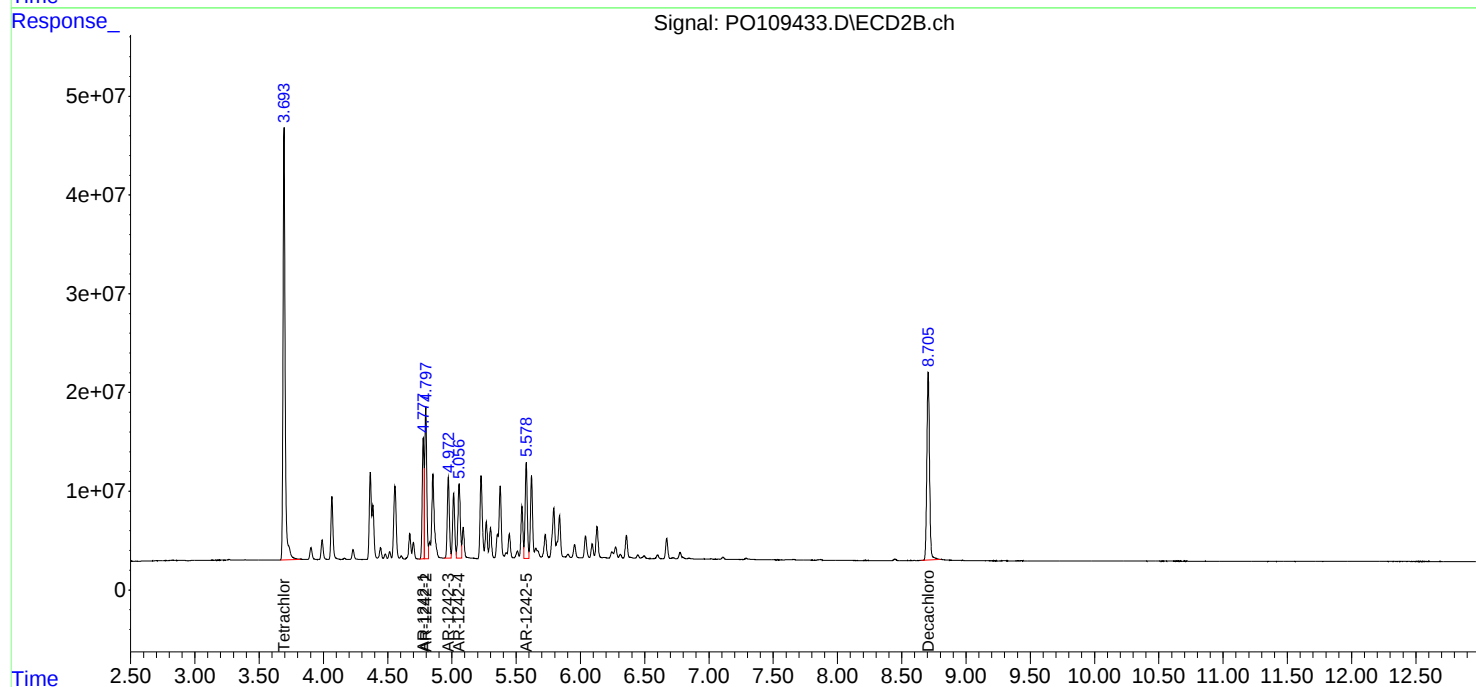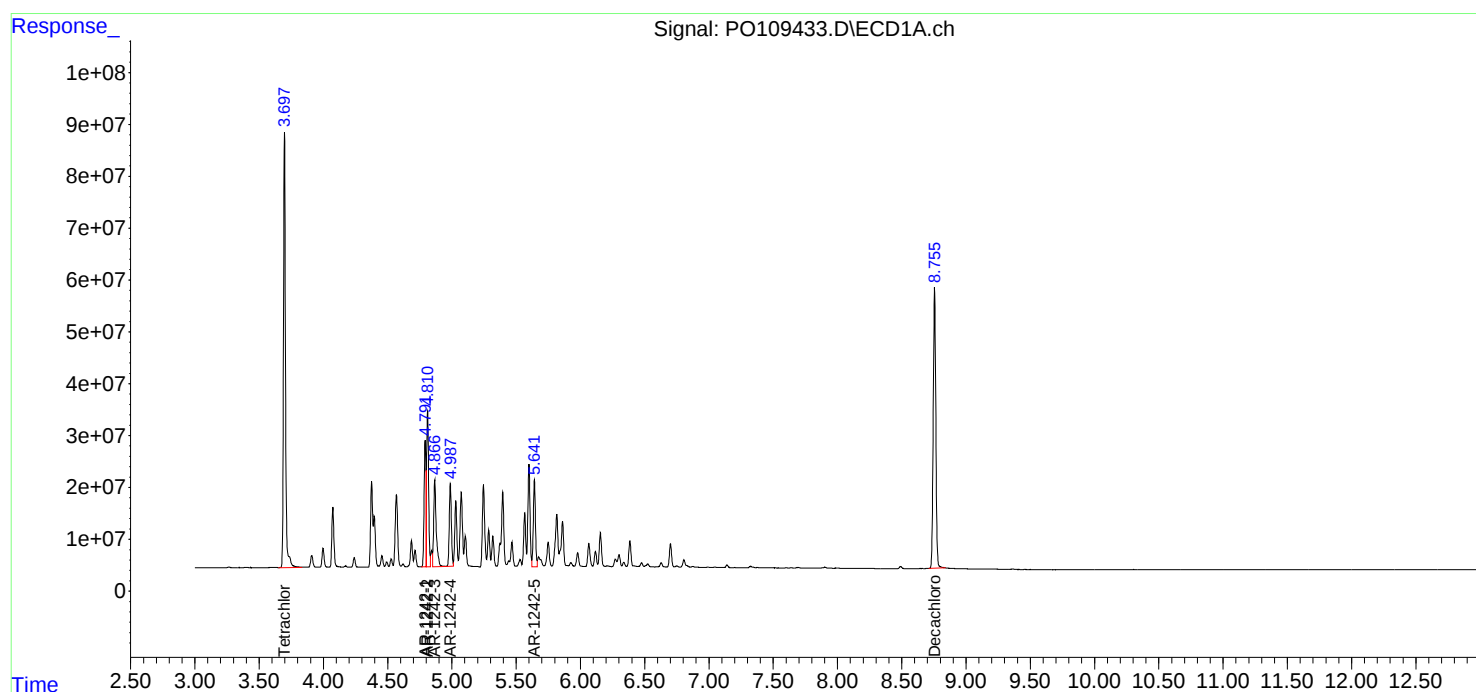

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 19:13
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:27:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:26:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.698	3.694	705.0E6	380.9E6	74.630	72.489
2) SA Decachlor...	8.755	8.706	583.7E6	214.6E6	71.212	71.089
Target Compounds						
16) L4 AR-1242-1	4.792	4.777	186.6E6	93559887	707.886	702.778
17) L4 AR-1242-2	4.812	4.796	255.9E6	130.1E6	710.666	710.082
18) L4 AR-1242-3	4.868	4.972	179.6E6	72475556	699.816	708.841
19) L4 AR-1242-4	4.989	5.057	141.2E6	75764454	705.184	702.896
20) L4 AR-1242-5	5.643	5.578	148.7E6	88287004	700.176	704.946



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 19:13
Operator : YP/AJ
Sample : AR1242ICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:27:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:26:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

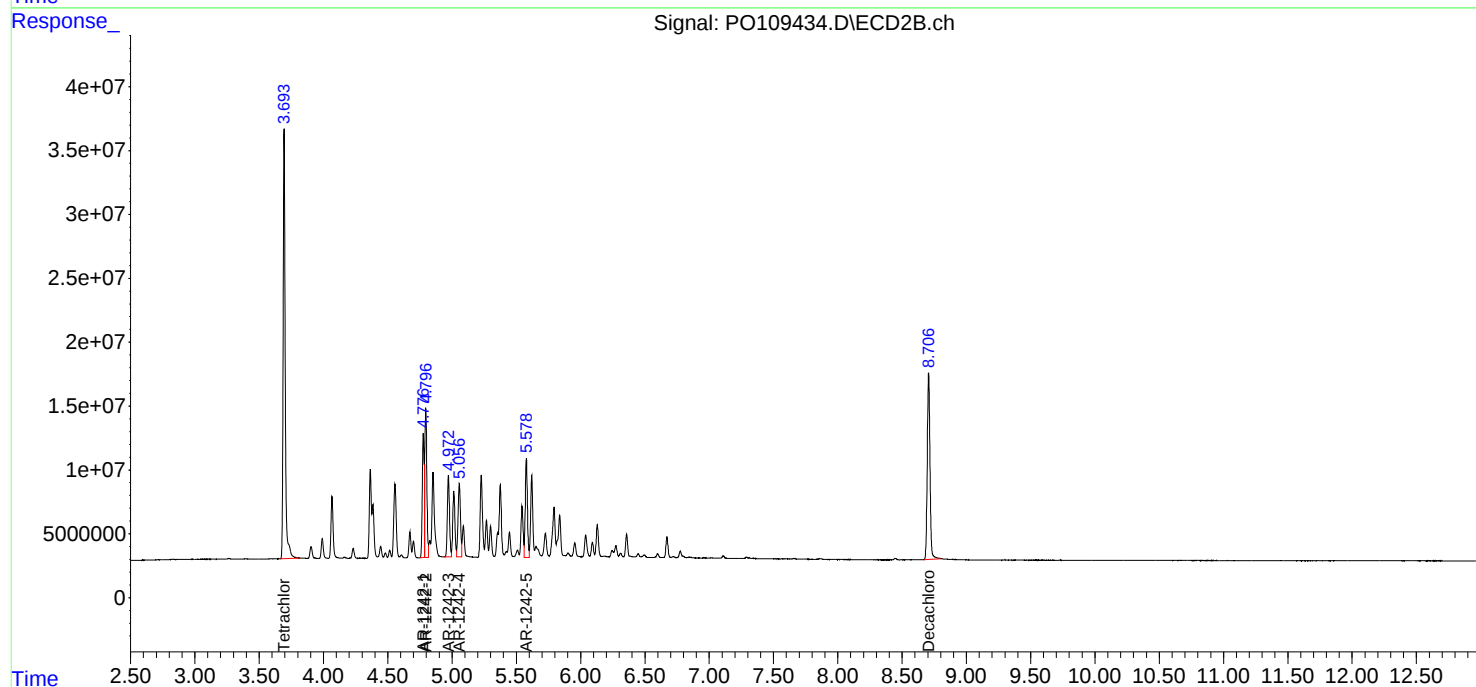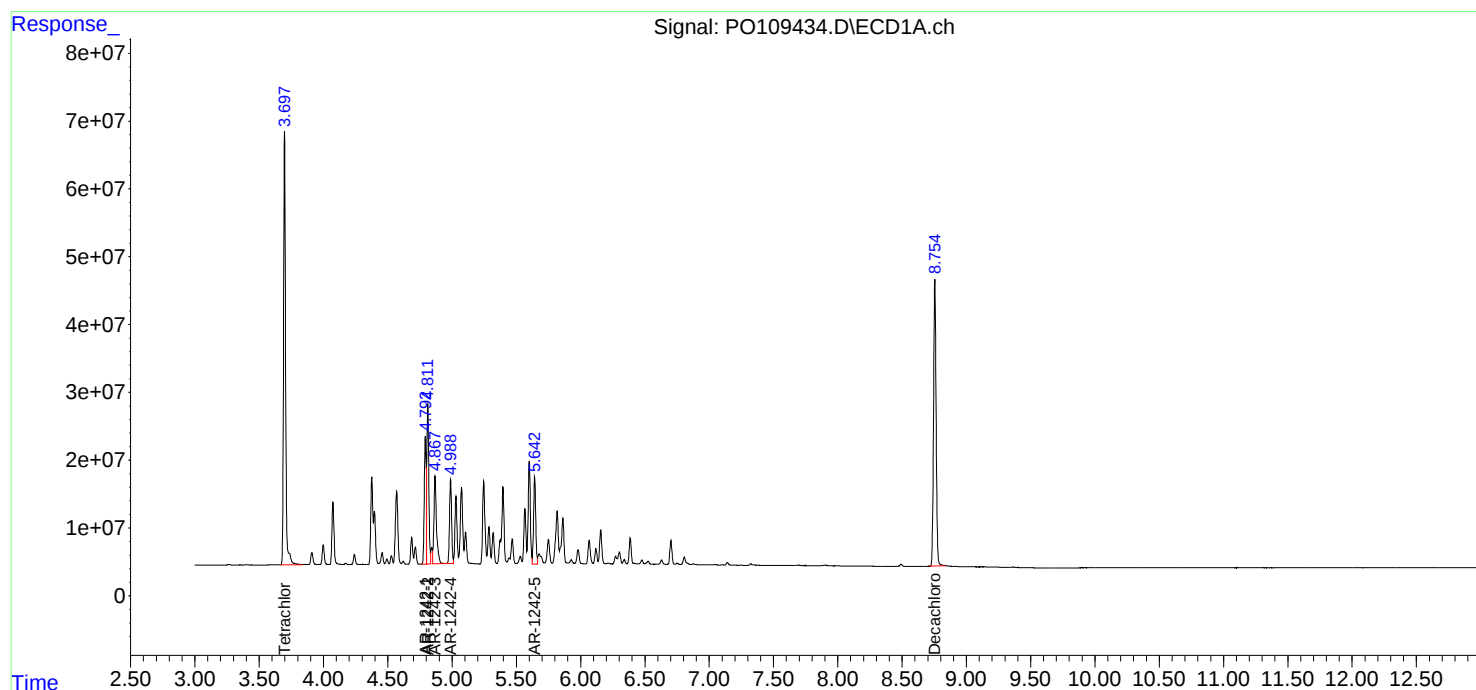

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 19:31
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:28:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:26:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.698	3.694	472.3E6	262.7E6	50.000	50.000
2) SA Decachlor...	8.756	8.707	409.9E6	151.0E6	50.000	50.000
Target Compounds						
16) L4 AR-1242-1	4.792	4.777	131.8E6	66564351	500.000	500.000
17) L4 AR-1242-2	4.811	4.797	180.0E6	91633308	500.000	500.000
18) L4 AR-1242-3	4.868	4.972	128.3E6	51122546	500.000	500.000
19) L4 AR-1242-4	4.989	5.057	100.1E6	53894501	500.000	500.000
20) L4 AR-1242-5	5.642	5.578	106.2E6	62619657	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 19:31
Operator : YP/AJ
Sample : AR1242ICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:28:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:26:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

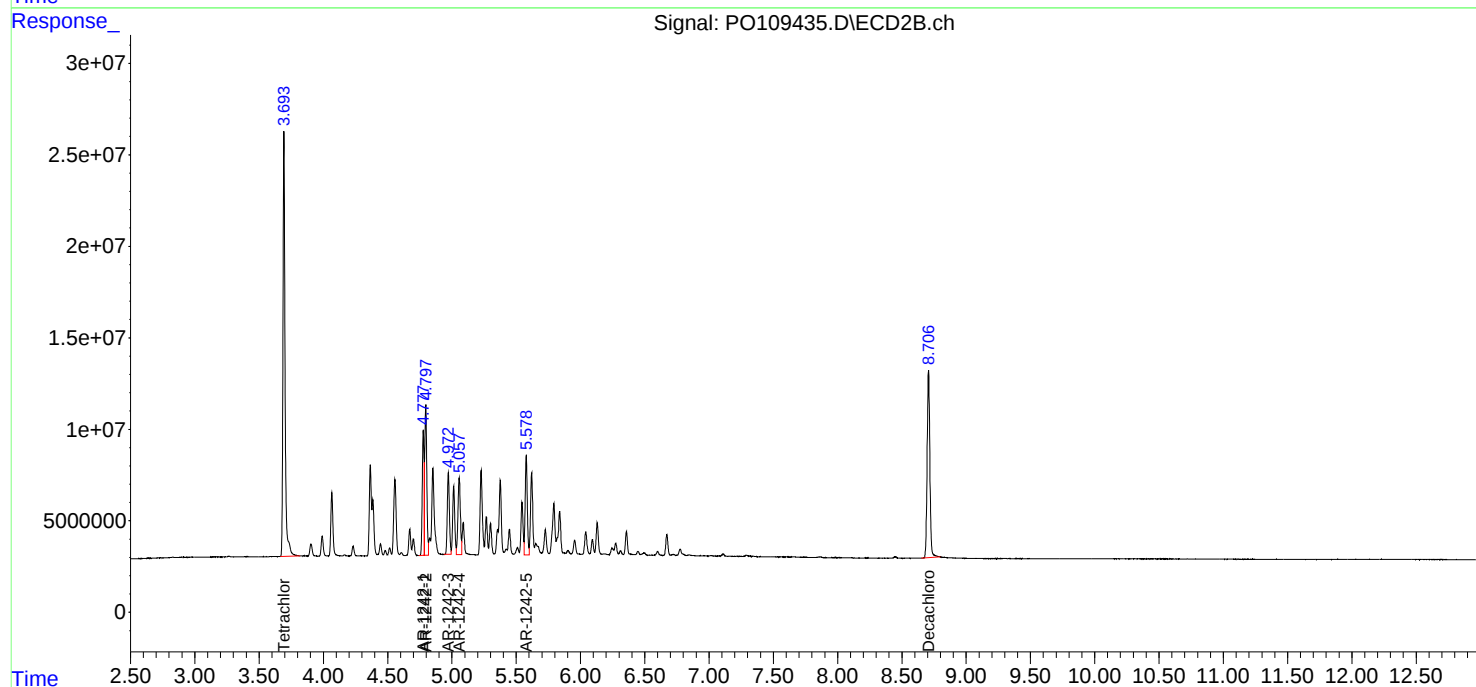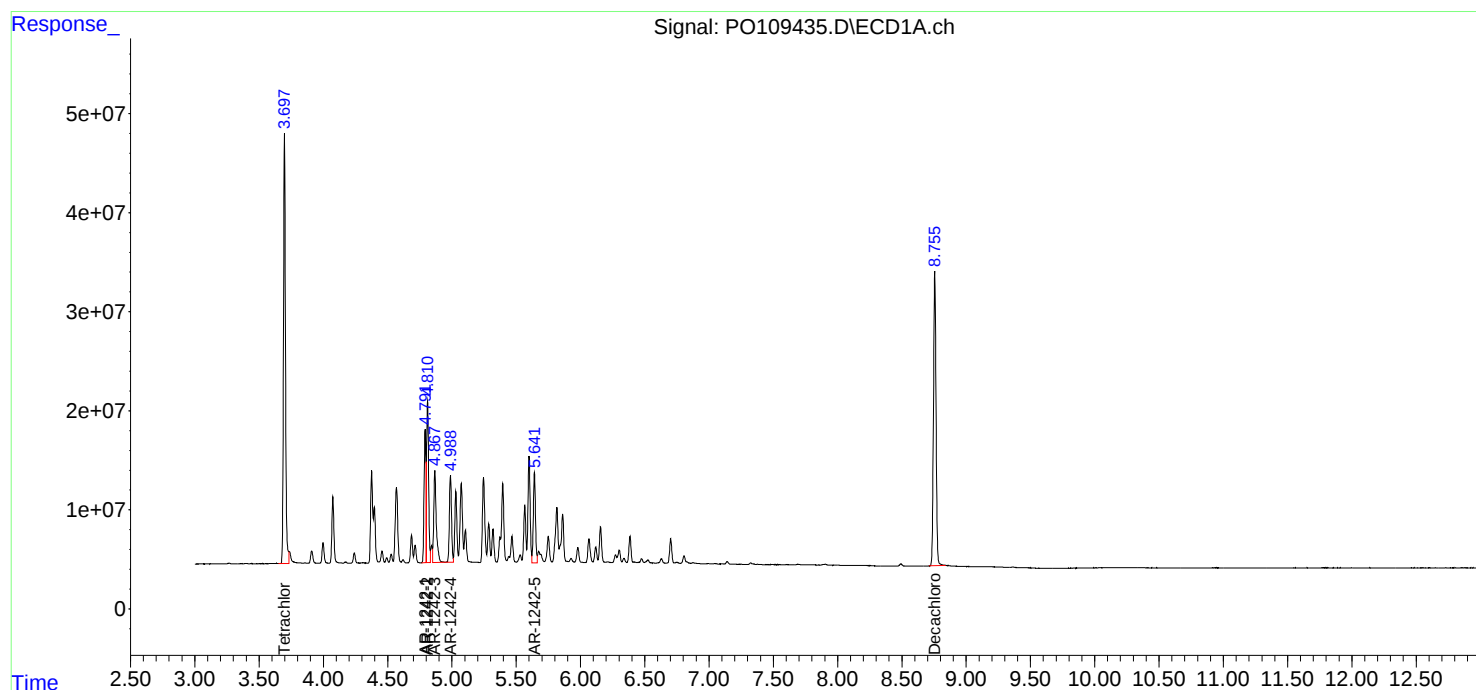

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 19:50
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:28:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:26:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	239.2E6	132.2E6	25.321	25.168
2) SA Decachlor...	8.755	8.706	217.2E6	81084477	26.492	26.856
Target Compounds						
16) L4 AR-1242-1	4.791	4.777	69551526	35357200	263.870	265.587
17) L4 AR-1242-2	4.811	4.796	94458948	48004344	262.369	261.937
18) L4 AR-1242-3	4.867	4.972	67985441	26922985	264.977	263.318
19) L4 AR-1242-4	4.988	5.056	52548713	28834607	262.488	267.510
20) L4 AR-1242-5	5.642	5.578	58079362	33950495	273.412	271.085



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 19:50
Operator : YP/AJ
Sample : AR1242ICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:28:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:26:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

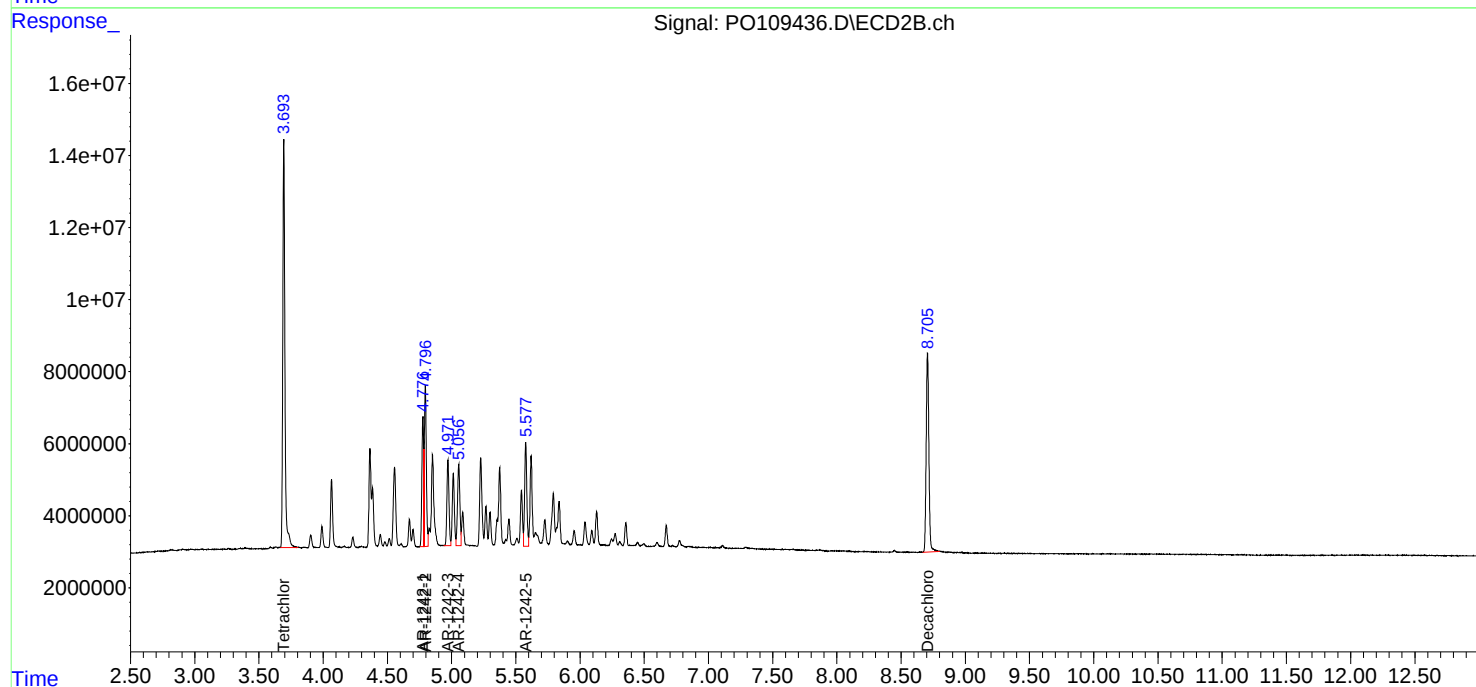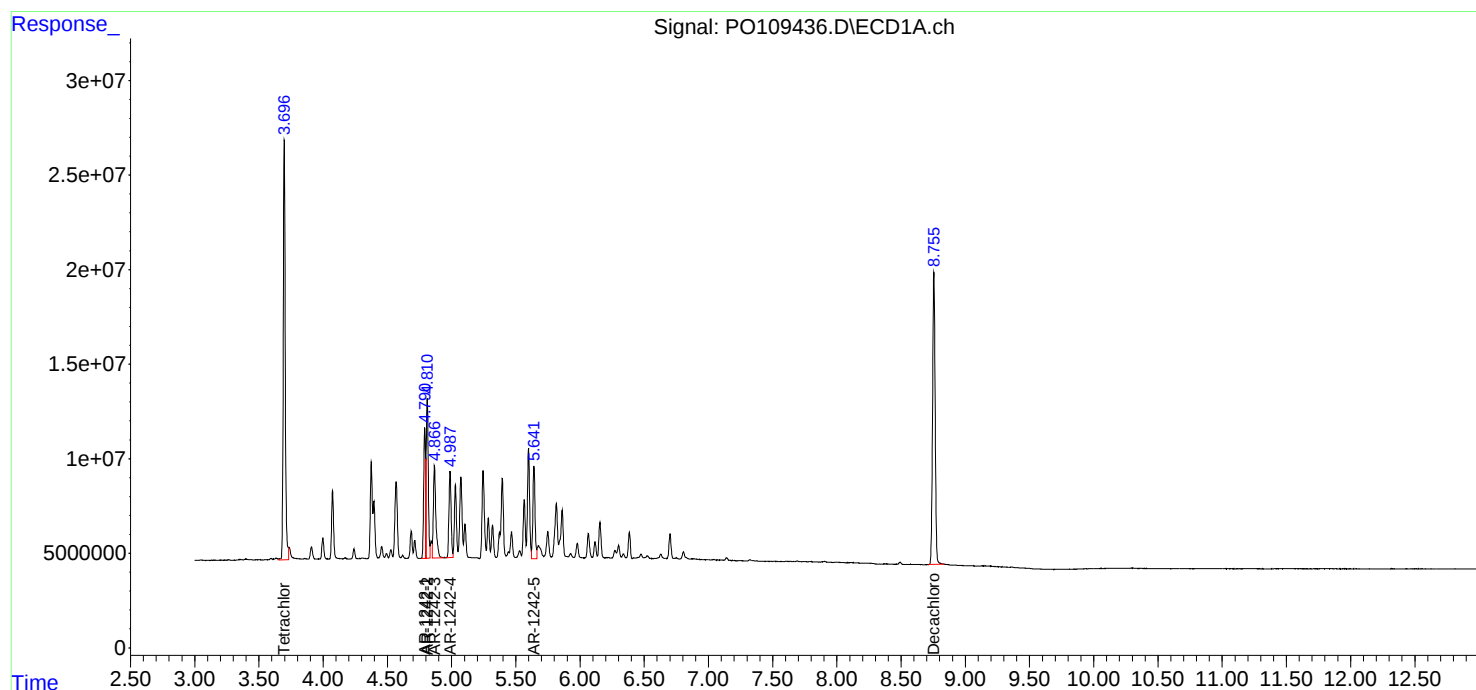

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109437.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 20:08
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2025
 Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:28:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:26:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	45284325	24258325	4.794	4.617
2) SA Decachlor...	8.755	8.706	43522830	16219813	5.310	5.372
Target Compounds						
16) L4 AR-1242-1	4.792	4.777	13835003	7073196	52.488	53.131
17) L4 AR-1242-2	4.811	4.796	18548986	9458809	51.522	51.612
18) L4 AR-1242-3	4.867	4.971	12898843	4970561	50.274	48.614
19) L4 AR-1242-4	4.988	5.055	10088199	5702832	50.392	52.907
20) L4 AR-1242-5	5.641	5.577	11831514	6828665	55.698m	54.525m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
Data File : P0109437.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 20:08
Operator : YP/AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2025
Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:28:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:26:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

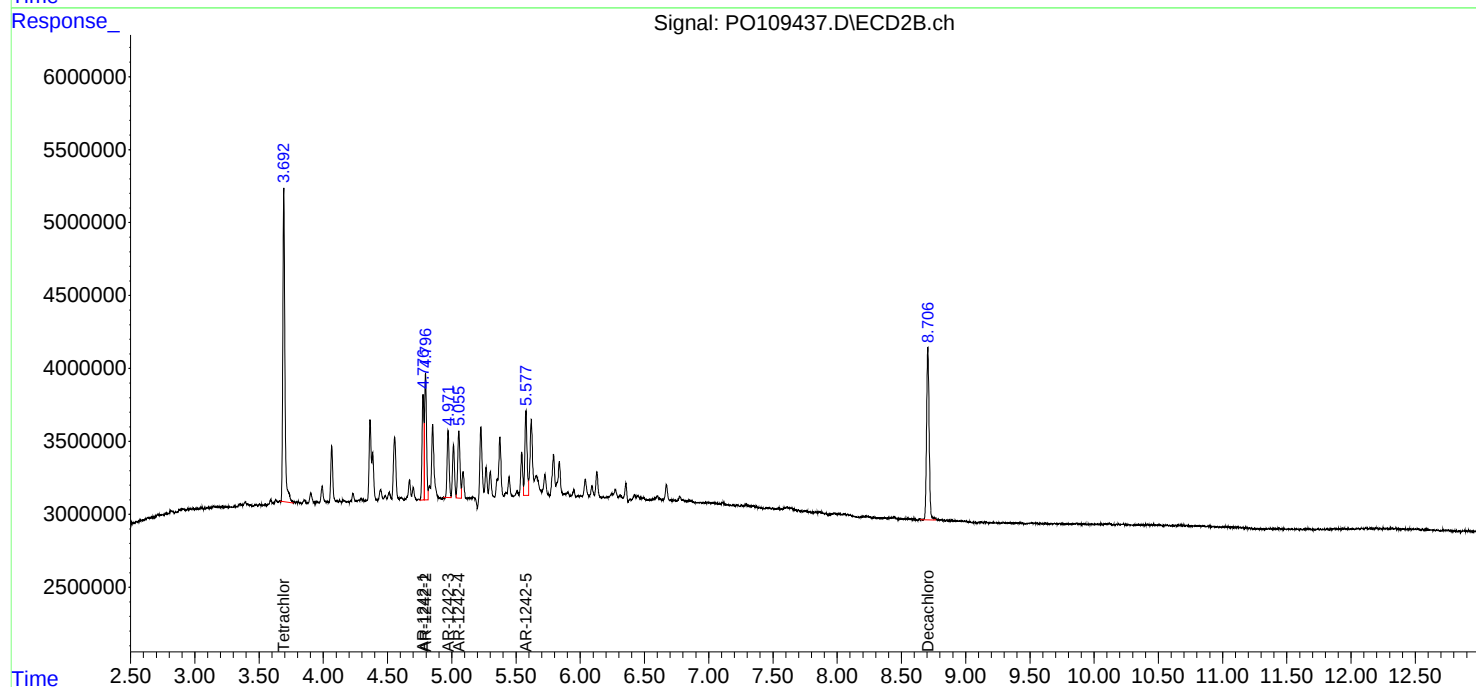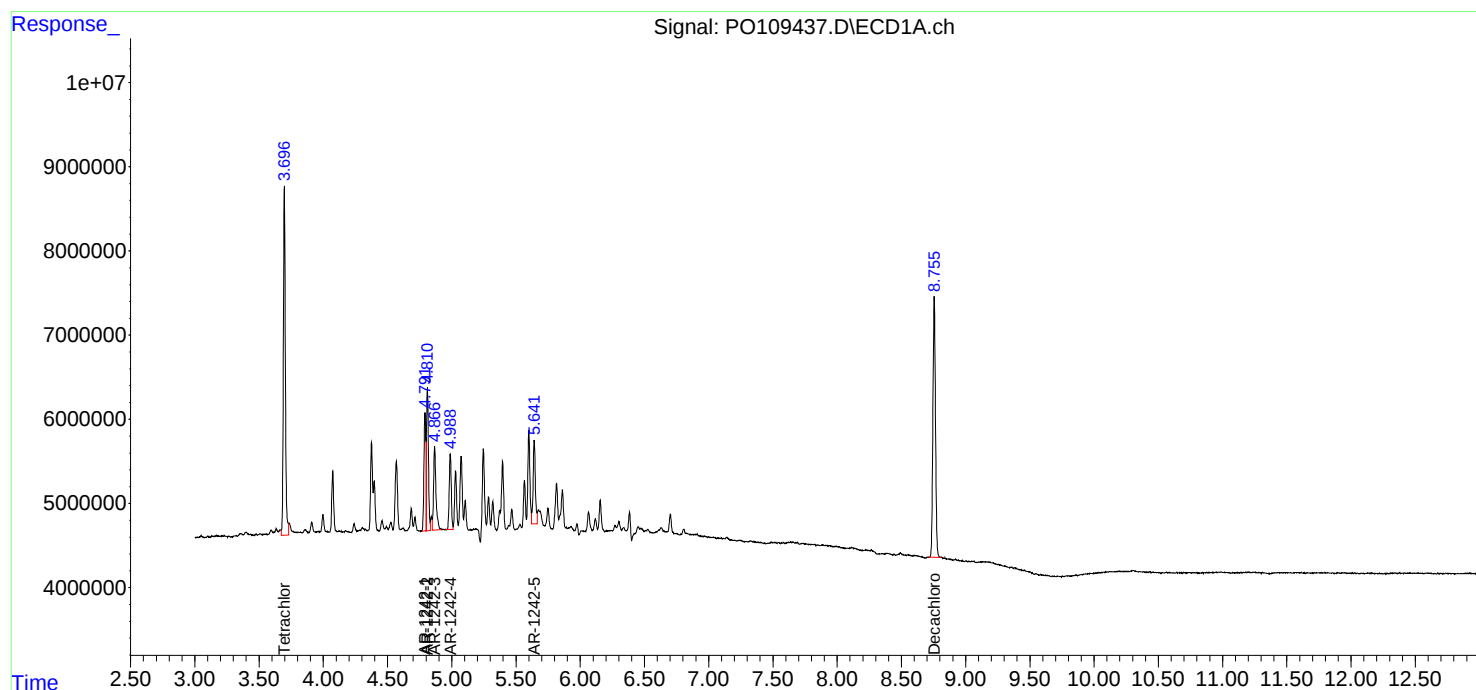

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 20:26
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:45:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:44:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	915.4E6	495.5E6	93.761	94.908
2) SA Decachlor...	8.755	8.706	770.4E6	279.0E6	92.405	91.836
Target Compounds						
21) L5 AR-1248-1	4.791	4.777	183.4E6	91256927	912.814	905.620
22) L5 AR-1248-2	5.030	5.014	249.5E6	130.6E6	885.902	891.678
23) L5 AR-1248-3	5.246	5.057	313.6E6	139.3E6	905.924	894.551
24) L5 AR-1248-4	5.600	5.228	440.0E6	163.9E6	918.126	908.733
25) L5 AR-1248-5	5.642	5.620	310.5E6	154.4E6	919.575	910.254



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 20:26
Operator : YP/AJ
Sample : AR1248ICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:45:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:44:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

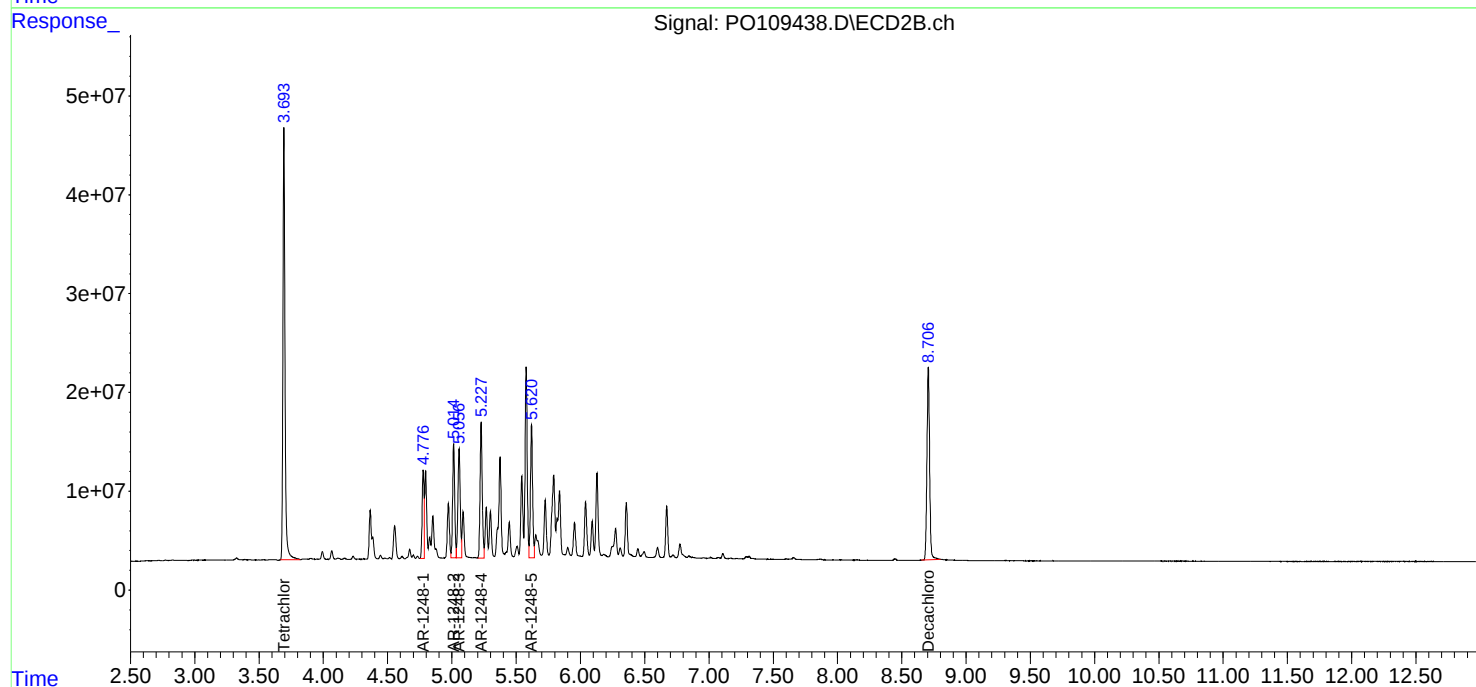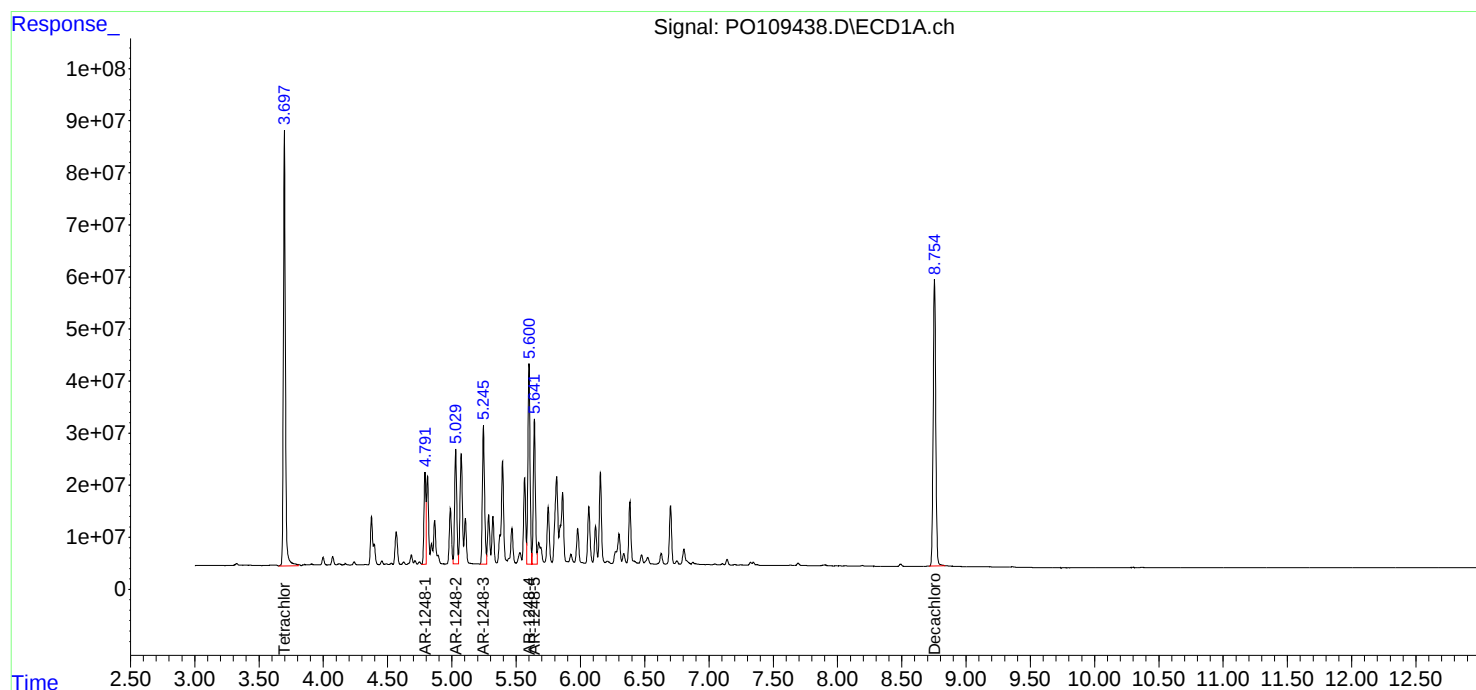

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 20:45
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:48:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:44:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	699.0E6	378.0E6	71.591	72.405
2) SA Decachlor...	8.755	8.706	593.5E6	215.5E6	71.185	70.928
Target Compounds						
21) L5 AR-1248-1	4.791	4.777	141.9E6	70604671	706.516	700.670
22) L5 AR-1248-2	5.030	5.014	196.7E6	102.5E6	698.273	699.925
23) L5 AR-1248-3	5.245	5.056	243.5E6	108.7E6	703.429	697.958
24) L5 AR-1248-4	5.600	5.227	339.5E6	127.1E6	708.585	704.454
25) L5 AR-1248-5	5.642	5.619	238.9E6	118.8E6	707.520	700.785



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 20:45
Operator : YP/AJ
Sample : AR1248ICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:48:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:44:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

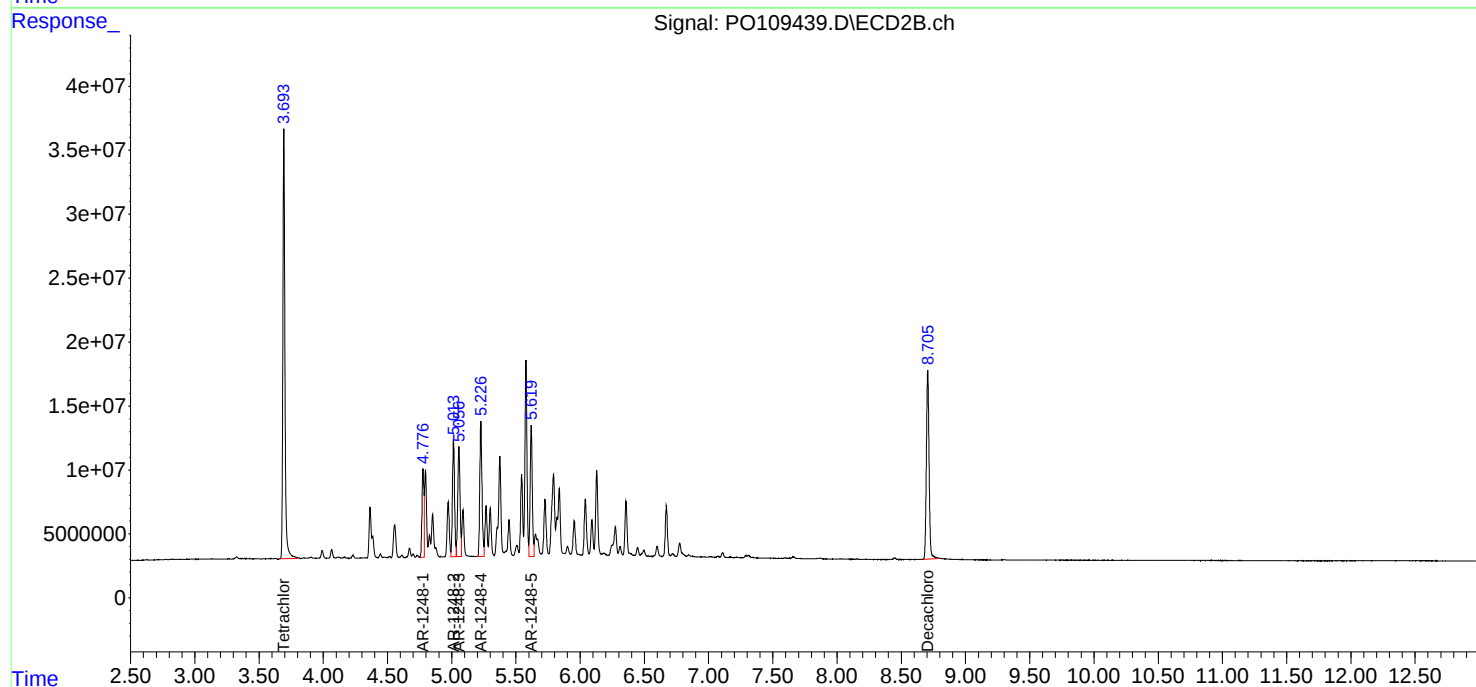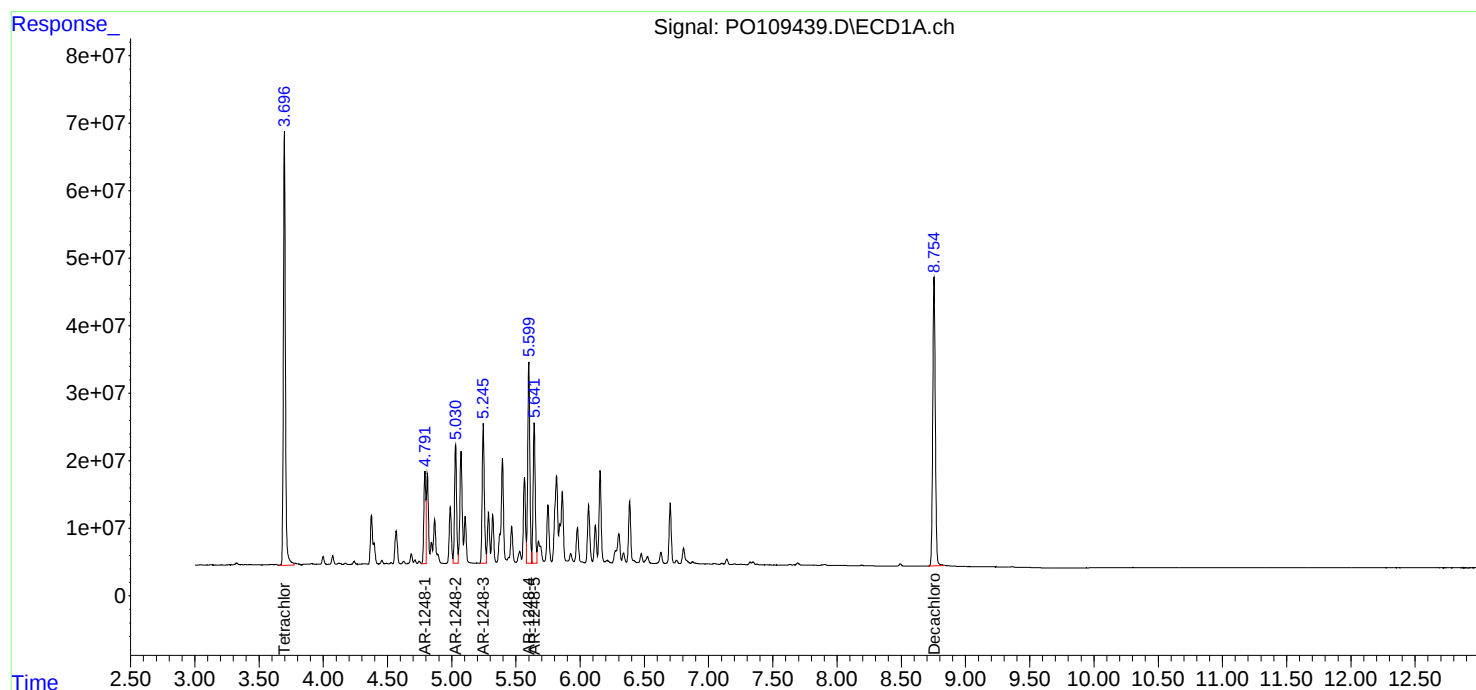

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 21:03
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:48:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:44:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	488.2E6	261.1E6	50.000	50.000
2) SA Decachlor...	8.755	8.706	416.9E6	151.9E6	50.000	50.000
Target Compounds						
21) L5 AR-1248-1	4.792	4.777	100.5E6	50383698	500.000	500.000
22) L5 AR-1248-2	5.030	5.014	140.8E6	73210547	500.000	500.000
23) L5 AR-1248-3	5.245	5.056	173.1E6	77850845	500.000	500.000
24) L5 AR-1248-4	5.601	5.227	239.6E6	90182217	500.000	500.000
25) L5 AR-1248-5	5.642	5.619	168.8E6	84787780	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 21:03
Operator : YP/AJ
Sample : AR1248ICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:48:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:44:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

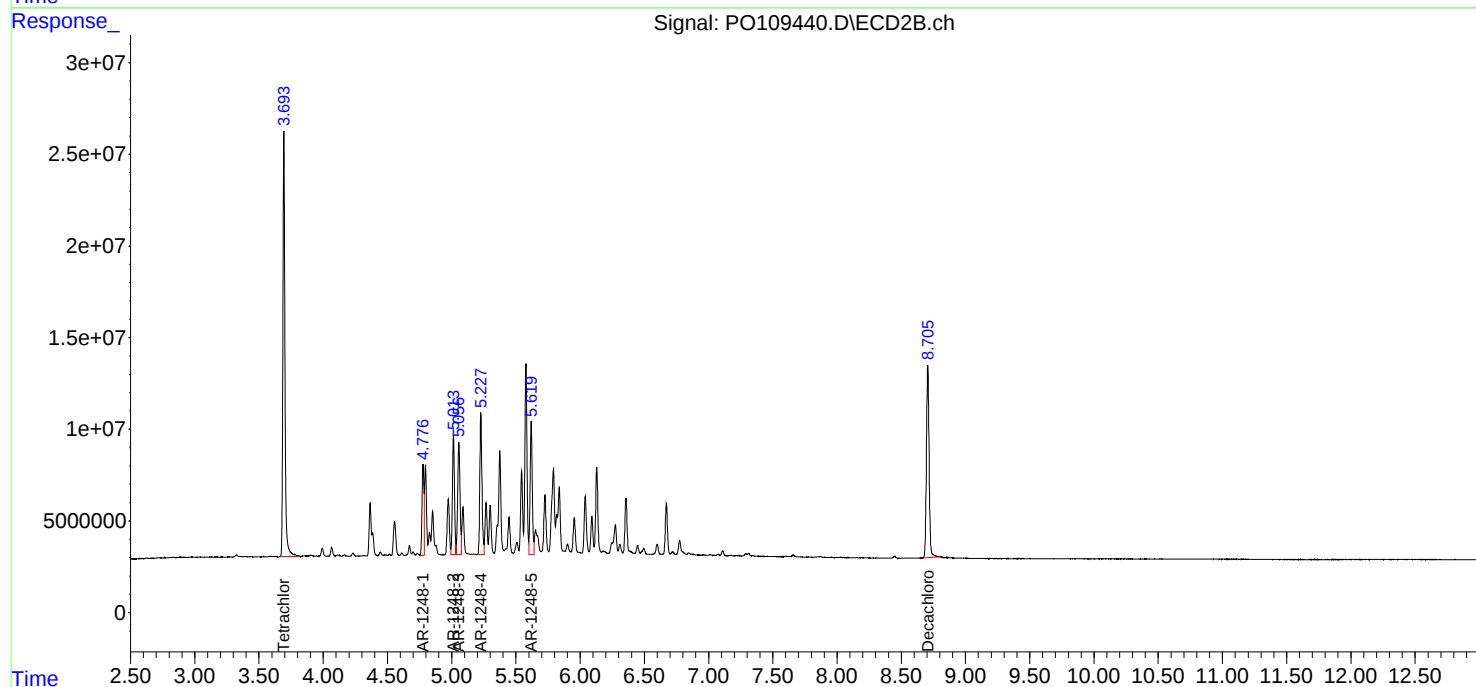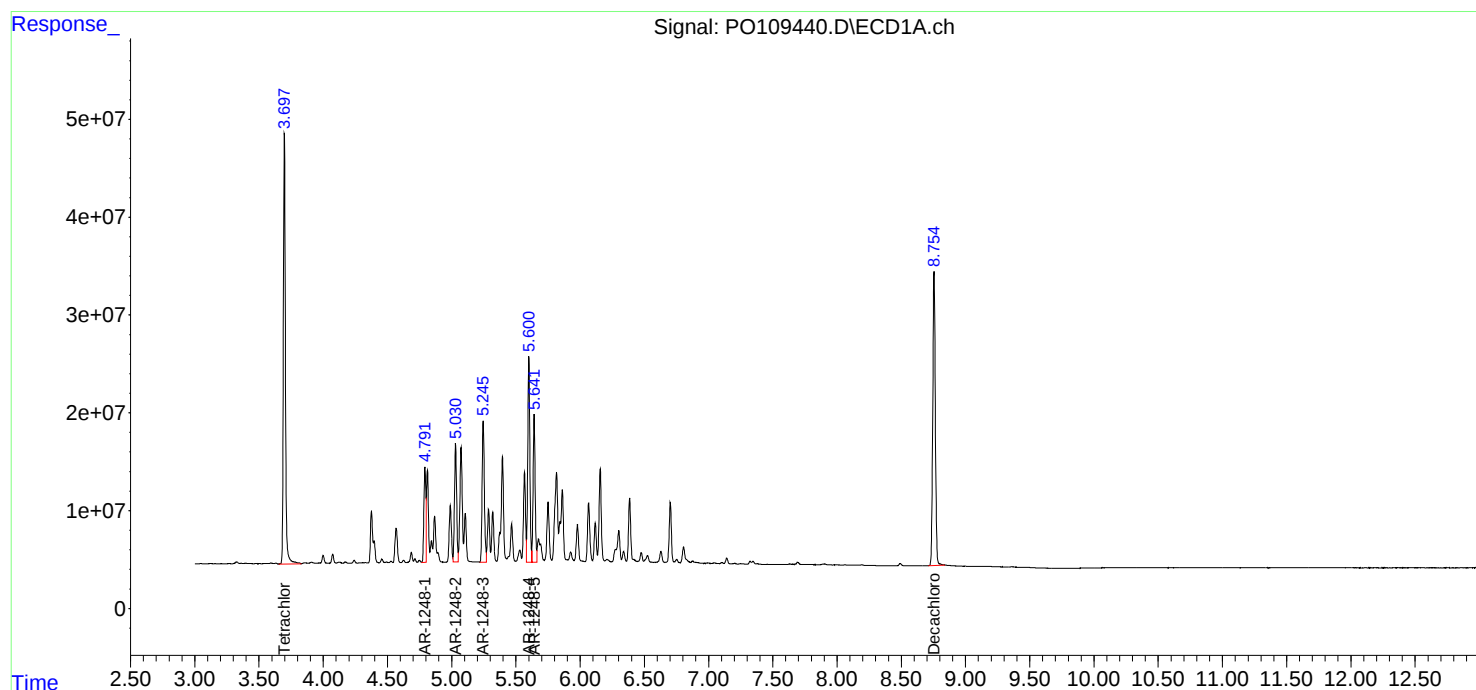

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 21:21
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:48:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:44:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	247.1E6	131.6E6	25.309	25.209
2) SA Decachlor...	8.755	8.705	220.4E6	81028918	26.436	26.667
Target Compounds						
21) L5 AR-1248-1	4.791	4.777	53414649	26903650	265.875	266.988
22) L5 AR-1248-2	5.030	5.014	74897714	39285877	265.920	268.307
23) L5 AR-1248-3	5.245	5.056	92525840	41607588	267.248	267.226
24) L5 AR-1248-4	5.600	5.227	127.4E6	48427931	265.835	268.500
25) L5 AR-1248-5	5.642	5.620	91434201	45832980	270.811	270.281



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 21:21
Operator : YP/AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:48:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:44:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

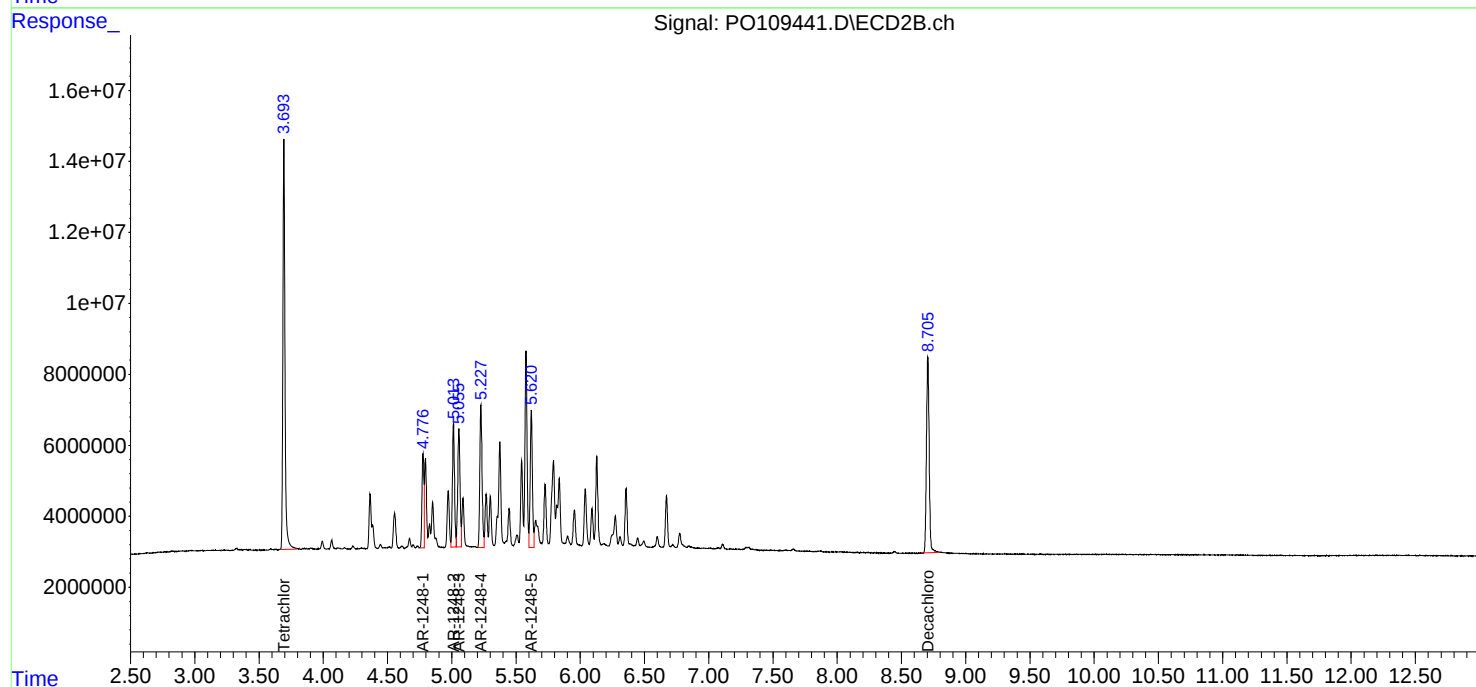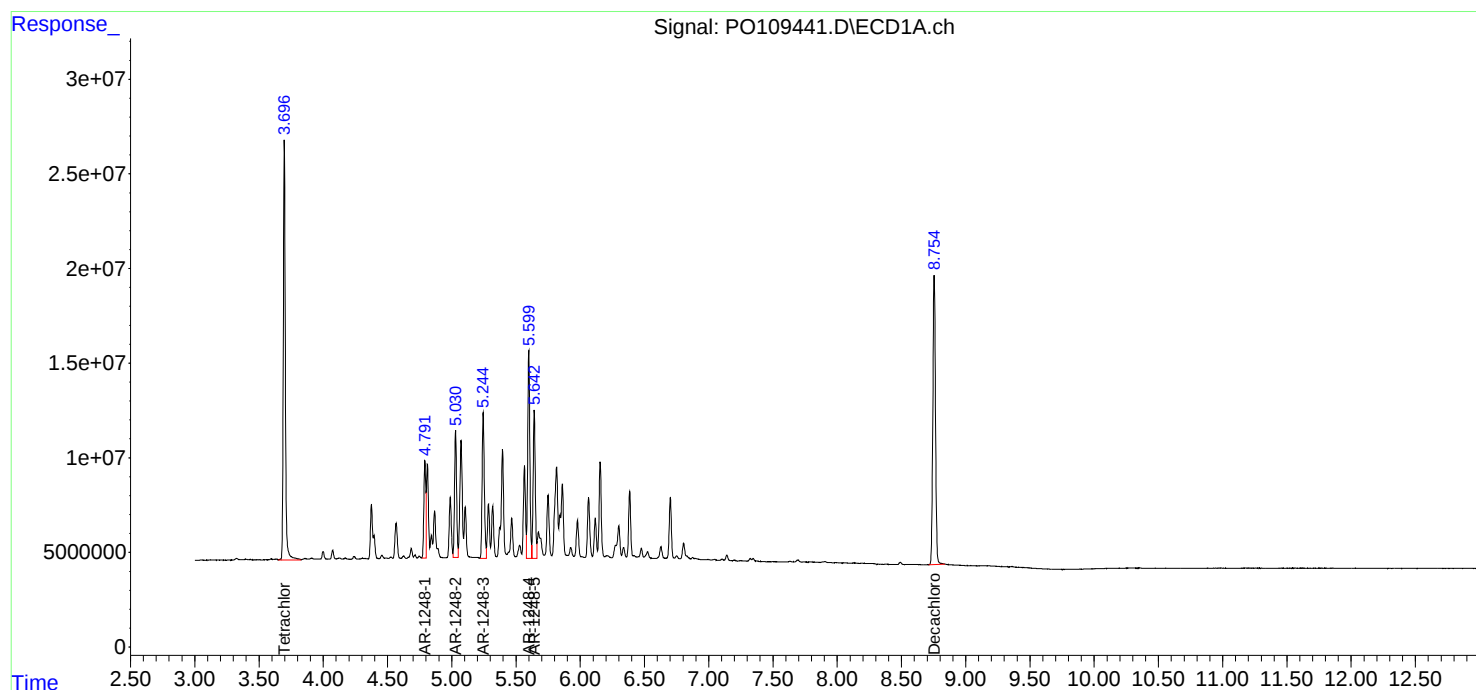

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 21:40
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2025
 Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:49:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:44:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	46251223	23752948	4.737	4.549
2) SA Decachlor...	8.754	8.706	44397899	16474487	5.325	5.422
Target Compounds						
21) L5 AR-1248-1	4.791	4.776	10517320	5442853	52.351	54.014
22) L5 AR-1248-2	5.030	5.013	14922906	7831415	52.983	53.486
23) L5 AR-1248-3	5.245	5.055	19608812	8436393	56.637	54.183
24) L5 AR-1248-4	5.599	5.227	25203917	9829738	52.598m	54.499m
25) L5 AR-1248-5	5.641	5.618	19009831	9765442	56.304m	57.588m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 21:40
Operator : YP/AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2025
Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:49:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:44:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

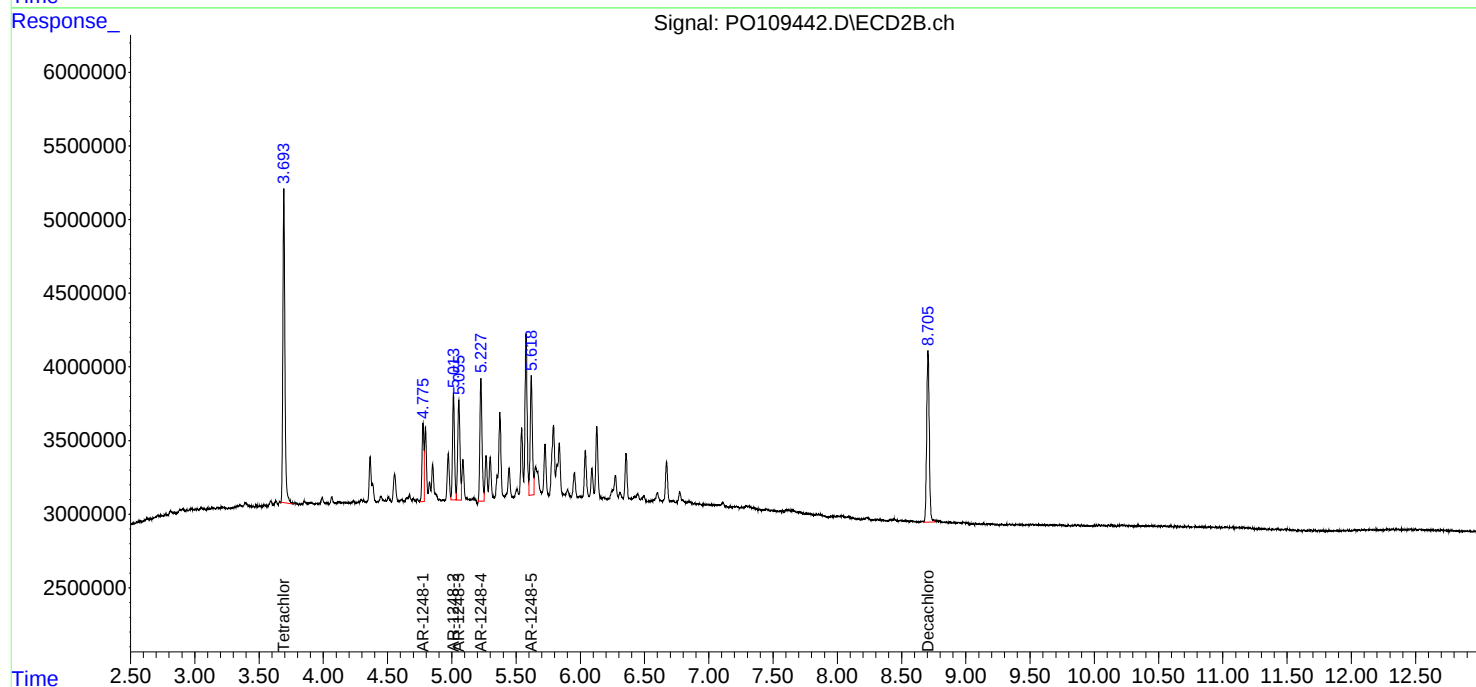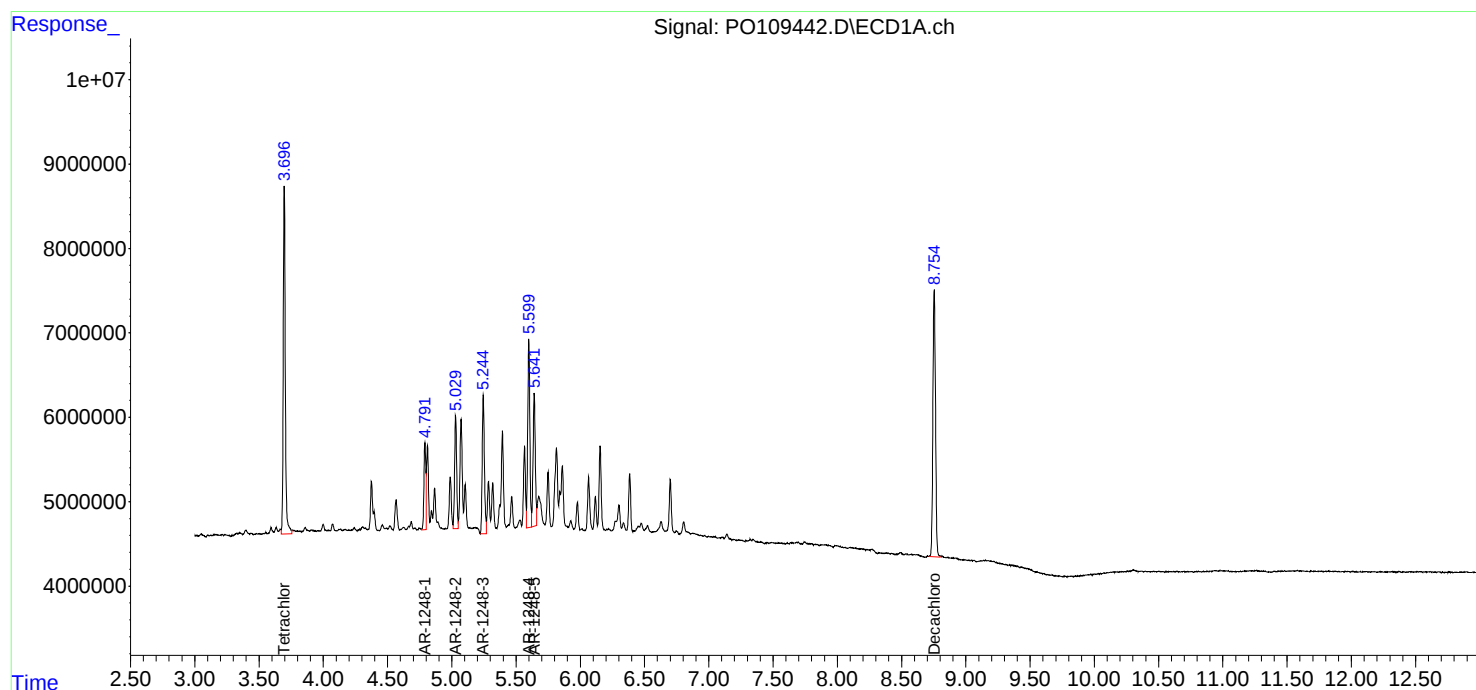

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 21:58
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:05:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 03:04:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	951.1E6	511.8E6	96.621	98.139
2) SA Decachlor...	8.754	8.705	796.7E6	284.2E6	93.419	92.489
Target Compounds						
26) L6 AR-1254-1	5.600	5.578	480.6E6	243.6E6	934.551	933.795
27) L6 AR-1254-2	5.749	5.726	417.5E6	212.5E6	924.809	921.386
28) L6 AR-1254-3	6.155	6.129	684.8E6	339.8E6	943.785	941.402
29) L6 AR-1254-4	6.384	6.357	418.0E6	192.3E6	974.859	962.866
30) L6 AR-1254-5	6.805	6.774	597.3E6	278.5E6	945.656	939.652



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109443.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 21:58
Operator : YP/AJ
Sample : AR1254ICC1000
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:05:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 03:04:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

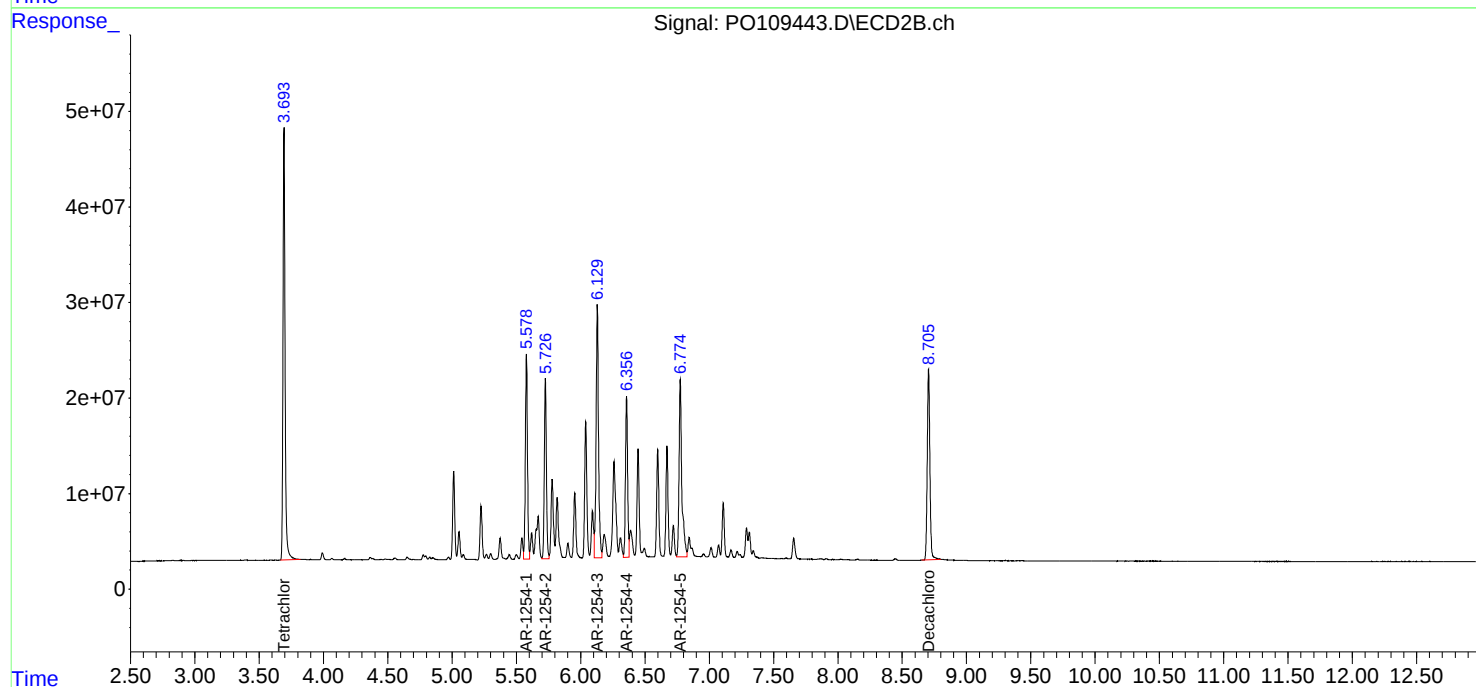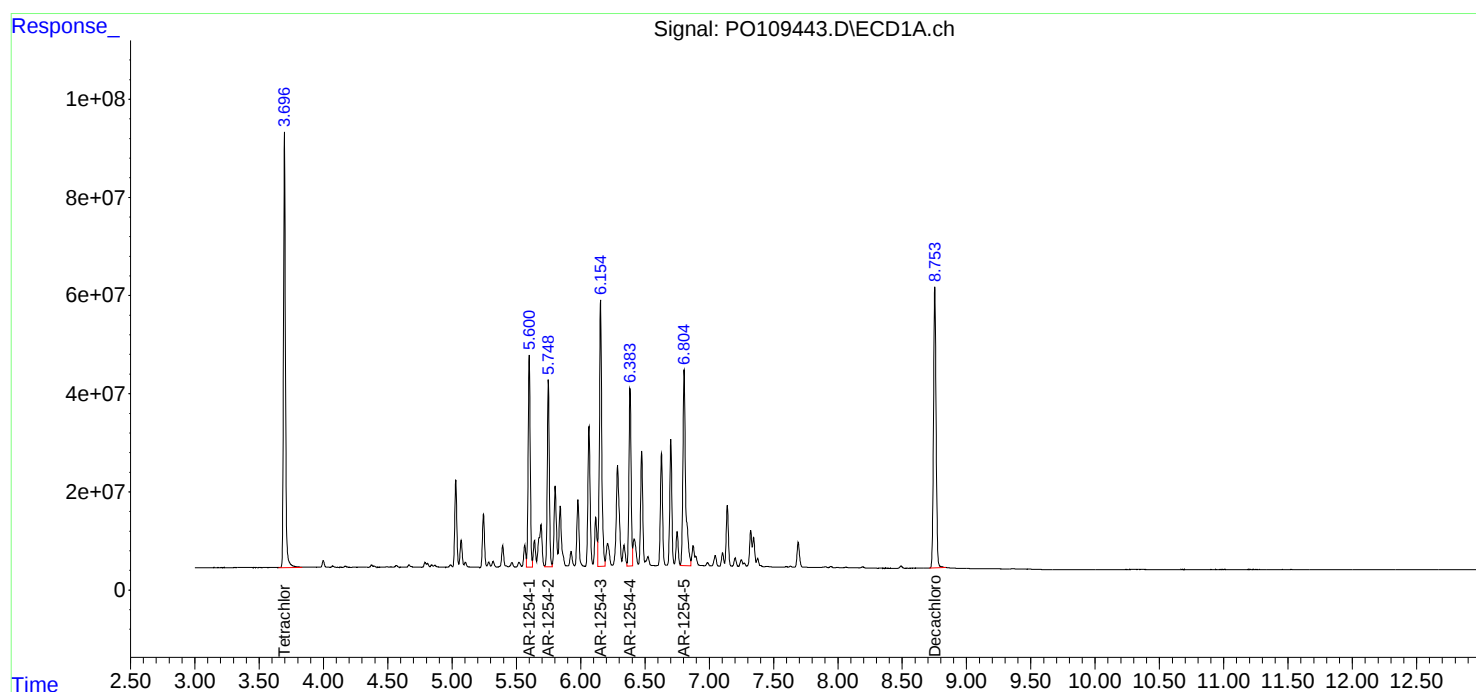

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 22:17
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:05:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 03:04:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	720.2E6	386.1E6	73.159	74.040
2) SA Decachlor...	8.756	8.705	609.4E6	219.1E6	71.460	71.318
Target Compounds						
26) L6 AR-1254-1	5.601	5.579	368.4E6	186.7E6	716.388	715.385
27) L6 AR-1254-2	5.750	5.726	321.9E6	164.0E6	713.024	710.983
28) L6 AR-1254-3	6.156	6.129	523.0E6	259.8E6	720.743	719.697
29) L6 AR-1254-4	6.385	6.357	307.4E6	142.4E6	716.868	712.856
30) L6 AR-1254-5	6.806	6.775	456.7E6	212.9E6	723.070	718.501



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 22:17
Operator : YP/AJ
Sample : AR1254ICC750
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:05:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 03:04:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

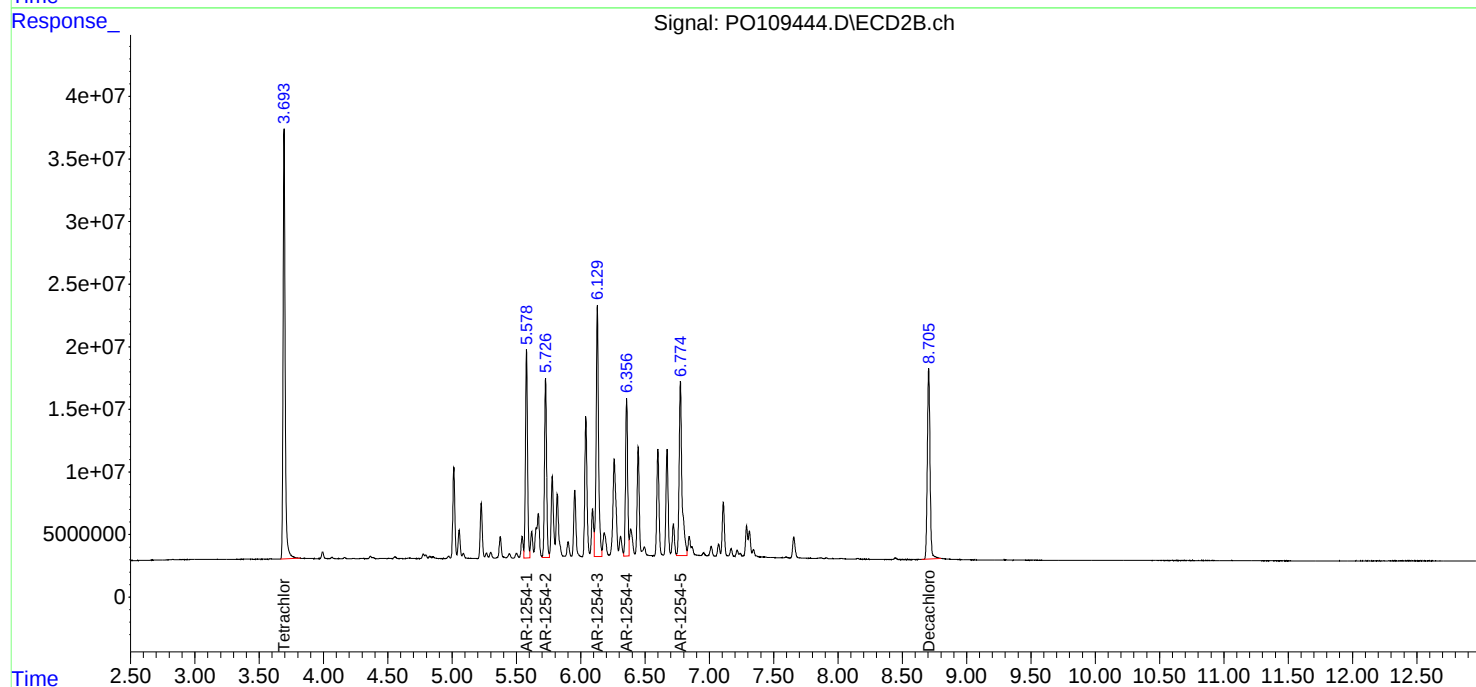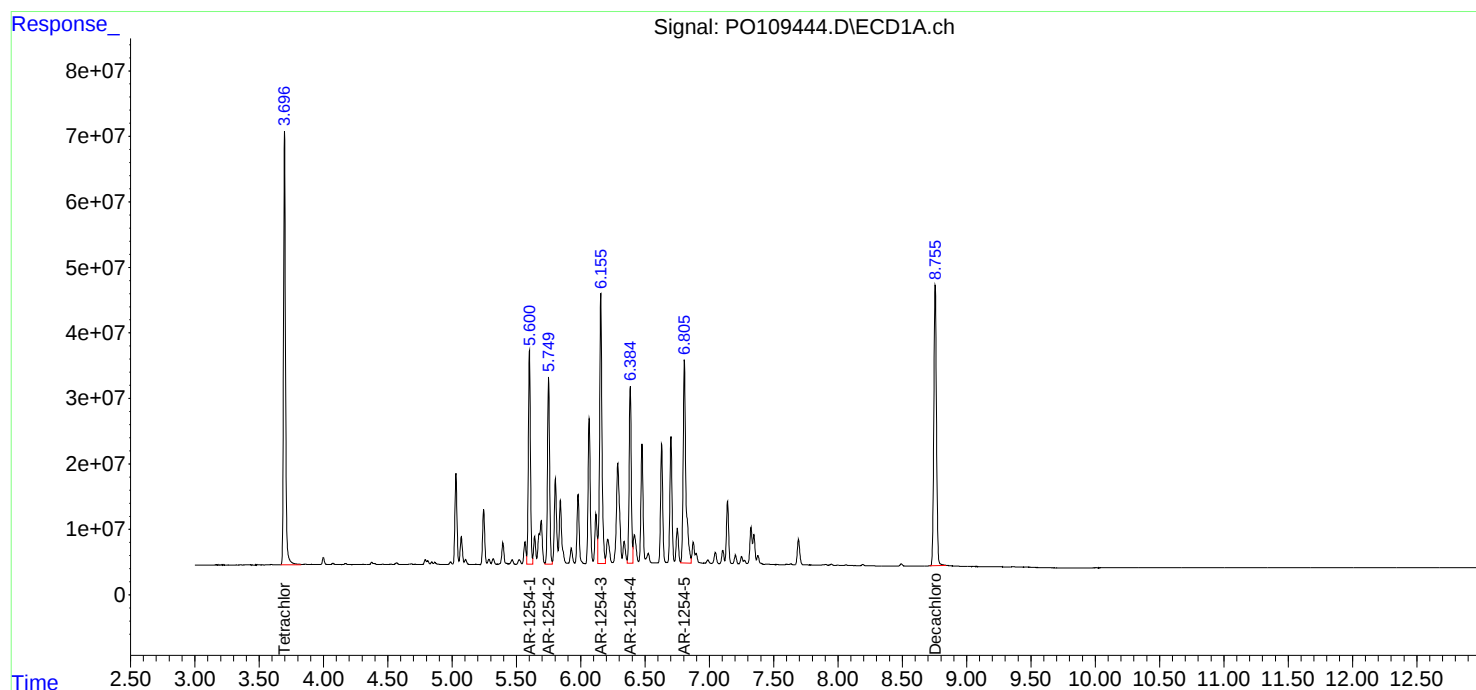

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109445.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 22:35
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:06:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 03:04:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	492.2E6	260.7E6	50.000	50.000
2) SA Decachlor...	8.755	8.705	426.4E6	153.6E6	50.000	50.000
Target Compounds						
26) L6 AR-1254-1	5.601	5.578	257.1E6	130.5E6	500.000	500.000
27) L6 AR-1254-2	5.749	5.726	225.7E6	115.3E6	500.000	500.000
28) L6 AR-1254-3	6.155	6.129	362.8E6	180.5E6	500.000	500.000
29) L6 AR-1254-4	6.385	6.356	214.4E6	99873317	500.000	500.000
30) L6 AR-1254-5	6.805	6.774	315.8E6	148.2E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109445.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 22:35
Operator : YP/AJ
Sample : AR1254ICC500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:06:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 03:04:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

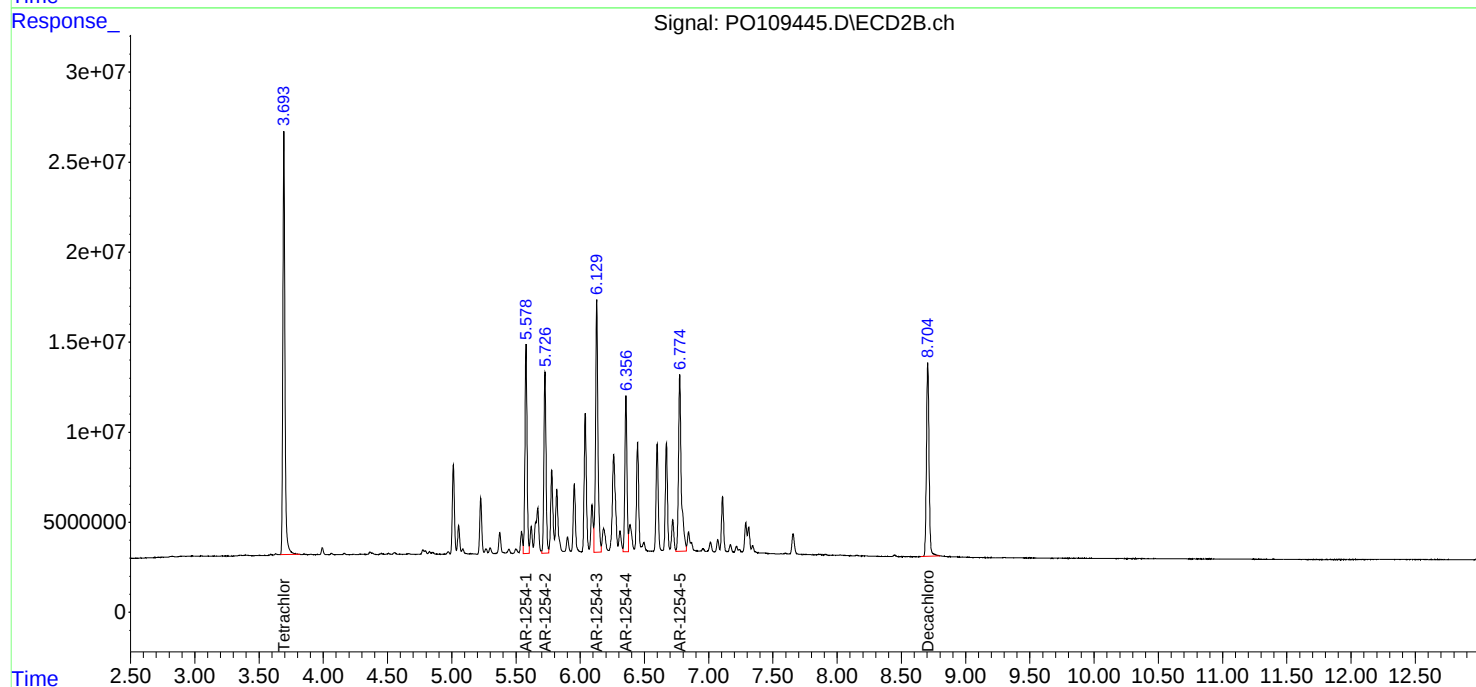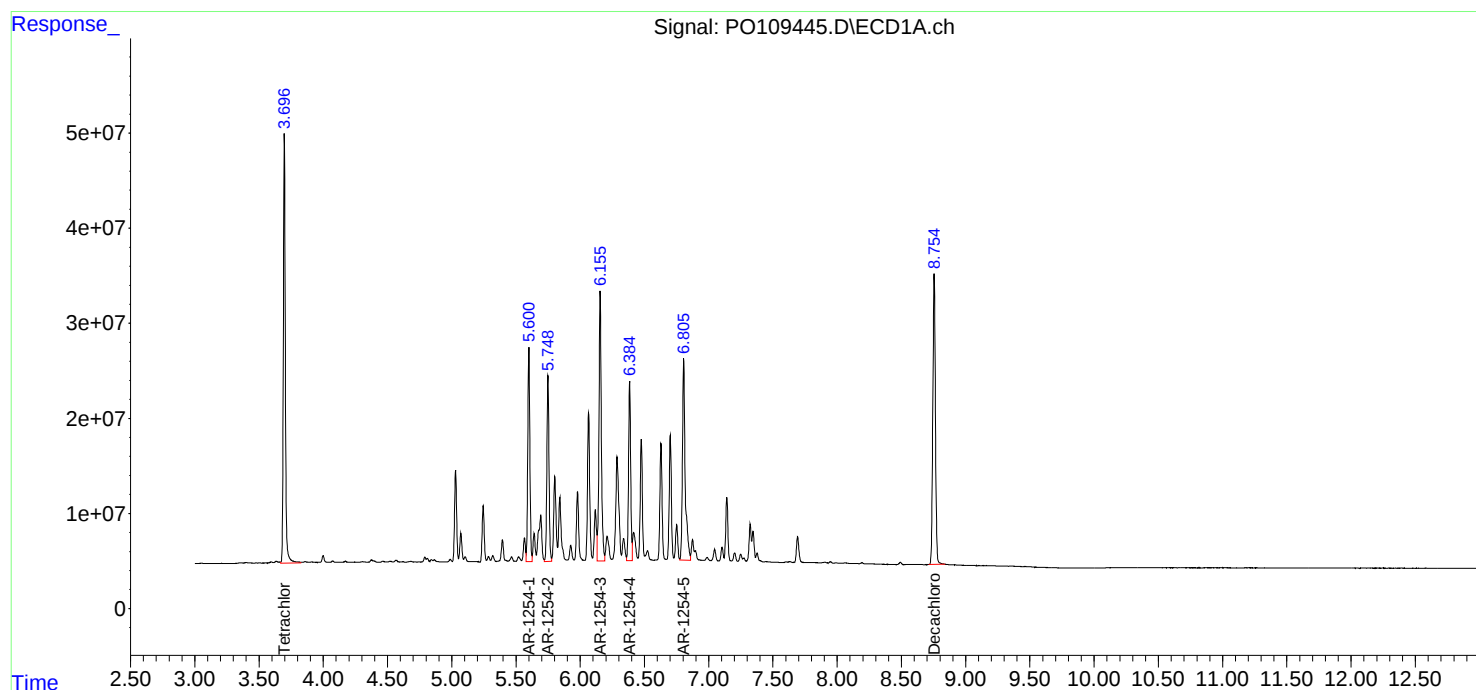

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 22:53
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:06:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 03:04:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	249.9E6	133.4E6	25.383	25.591
2) SA Decachlor...	8.755	8.705	224.7E6	82751432	26.343	26.933
Target Compounds						
26) L6 AR-1254-1	5.600	5.578	137.1E6	70215336	266.626	269.112
27) L6 AR-1254-2	5.749	5.726	120.3E6	62303614	266.469	270.086
28) L6 AR-1254-3	6.155	6.129	190.2E6	94726512	262.120	262.436
29) L6 AR-1254-4	6.385	6.357	115.3E6	53701999	269.019	268.851
30) L6 AR-1254-5	6.805	6.775	166.0E6	78525114	262.748	264.951



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 22:53
Operator : YP/AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:06:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 03:04:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

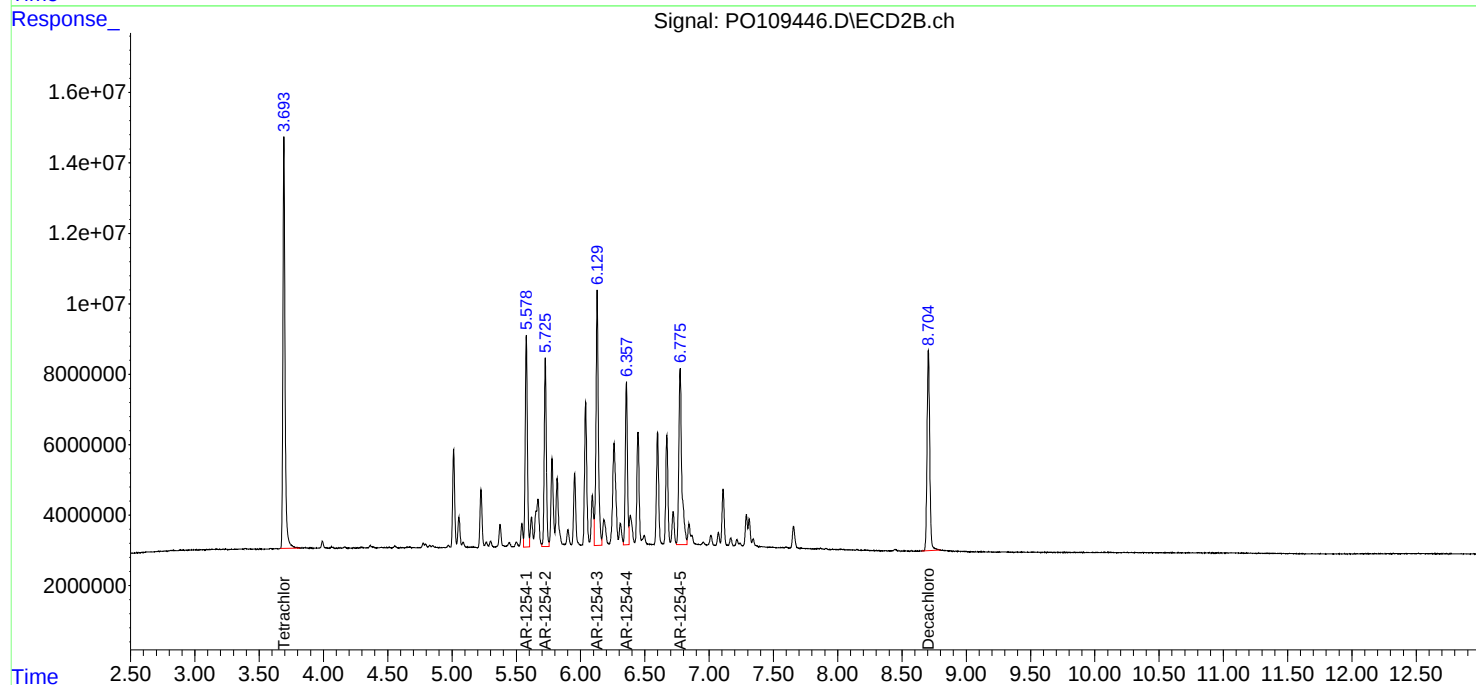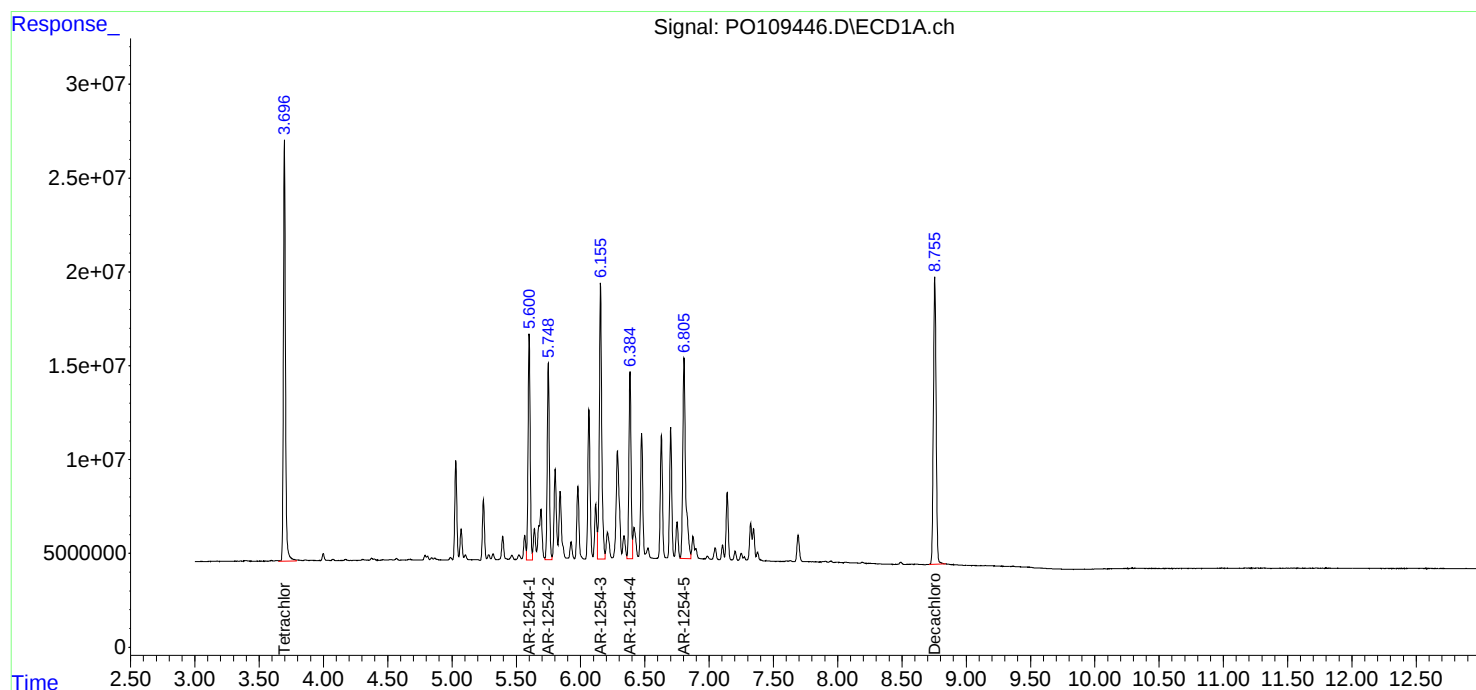

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 23:12
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2025
 Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:06:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 03:04:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.693	42478021	22408254	4.315m	4.297
2) SA Decachlor...	8.755	8.706	43911860	16400189	5.149	5.338
Target Compounds						
26) L6 AR-1254-1	5.601	5.578	27168777	13670107	52.828m	52.393m
27) L6 AR-1254-2	5.749	5.726	23620321	13084376	52.317m	56.721m
28) L6 AR-1254-3	6.156	6.128	35558931	17874982	49.004m	49.522m
29) L6 AR-1254-4	6.384	6.355	18803102	8443949	43.856m	42.273m
30) L6 AR-1254-5	6.806	6.774	30890950	15538233	48.907	52.427

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 23:12
Operator : YP/AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2025
Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:06:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 03:04:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

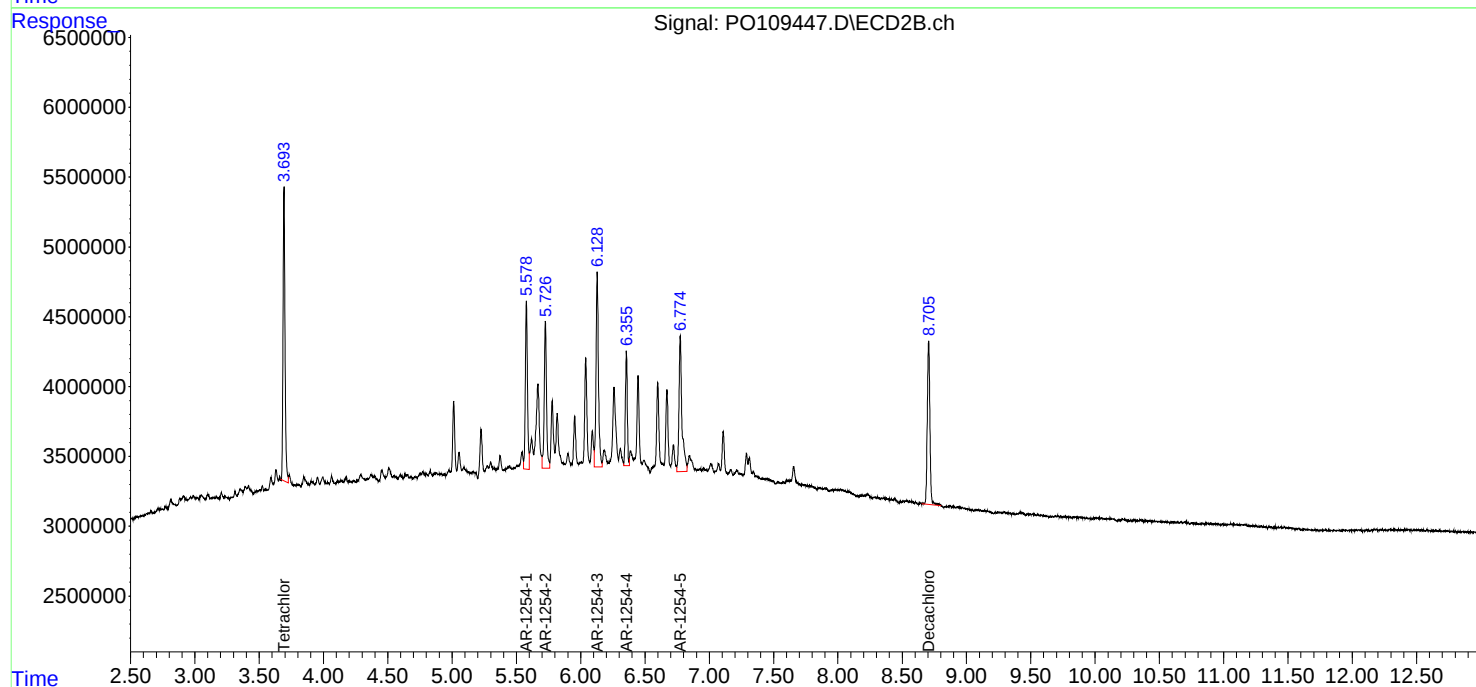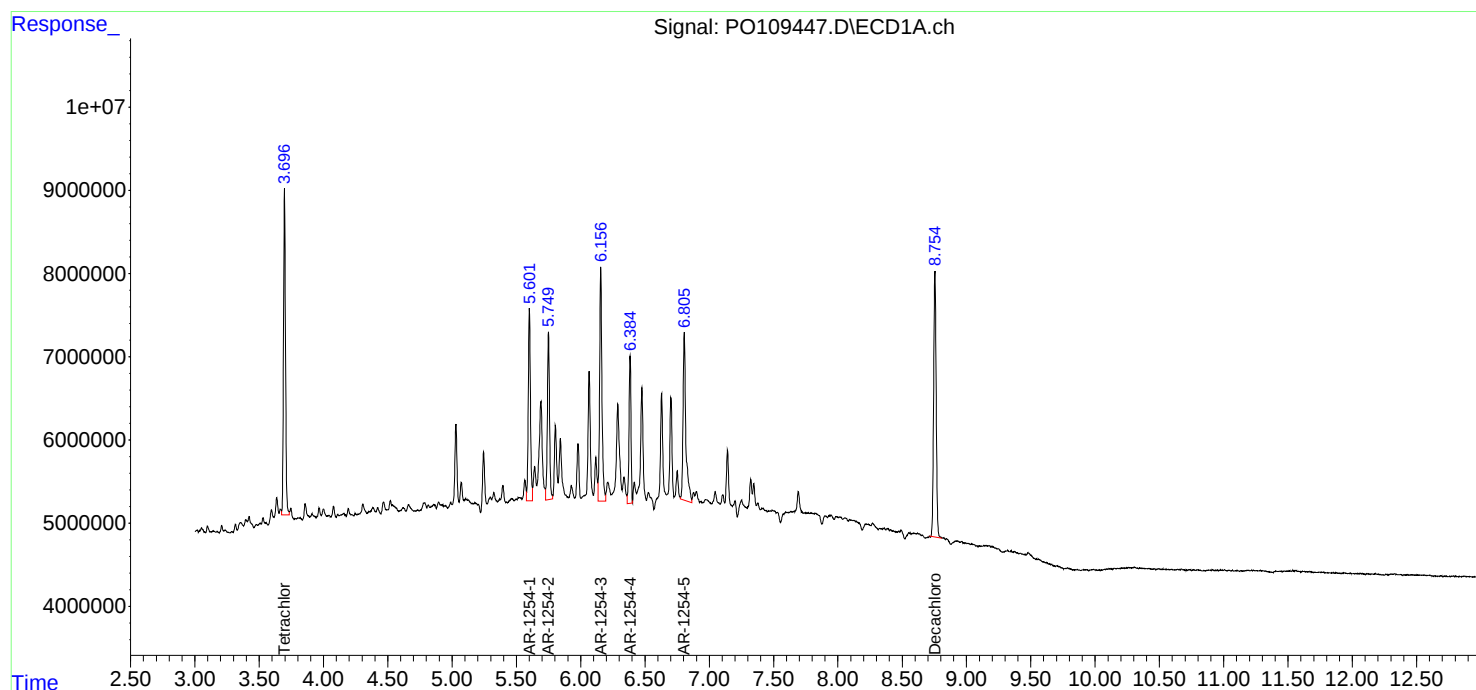

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 23:30
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:11:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:05:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	478.0E6	256.6E6	50.000	50.000
2) SA Decachlor...	8.754	8.705	414.0E6	151.0E6	50.000	50.000
Target Compounds						
36) L8 AR-1262-1	6.845	6.814	332.9E6	158.6E6	500.000	500.000
37) L8 AR-1262-2	7.346	7.313	564.9E6	249.3E6	500.000	500.000
38) L8 AR-1262-3	7.632	7.597	224.1E6	98127525	500.000	500.000
39) L8 AR-1262-4	7.696	7.661	414.6E6	177.4E6	500.000	500.000
40) L8 AR-1262-5	8.193	8.154	186.7E6	71568799	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 23:30
Operator : YP/AJ
Sample : AR1262ICC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:11:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:05:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

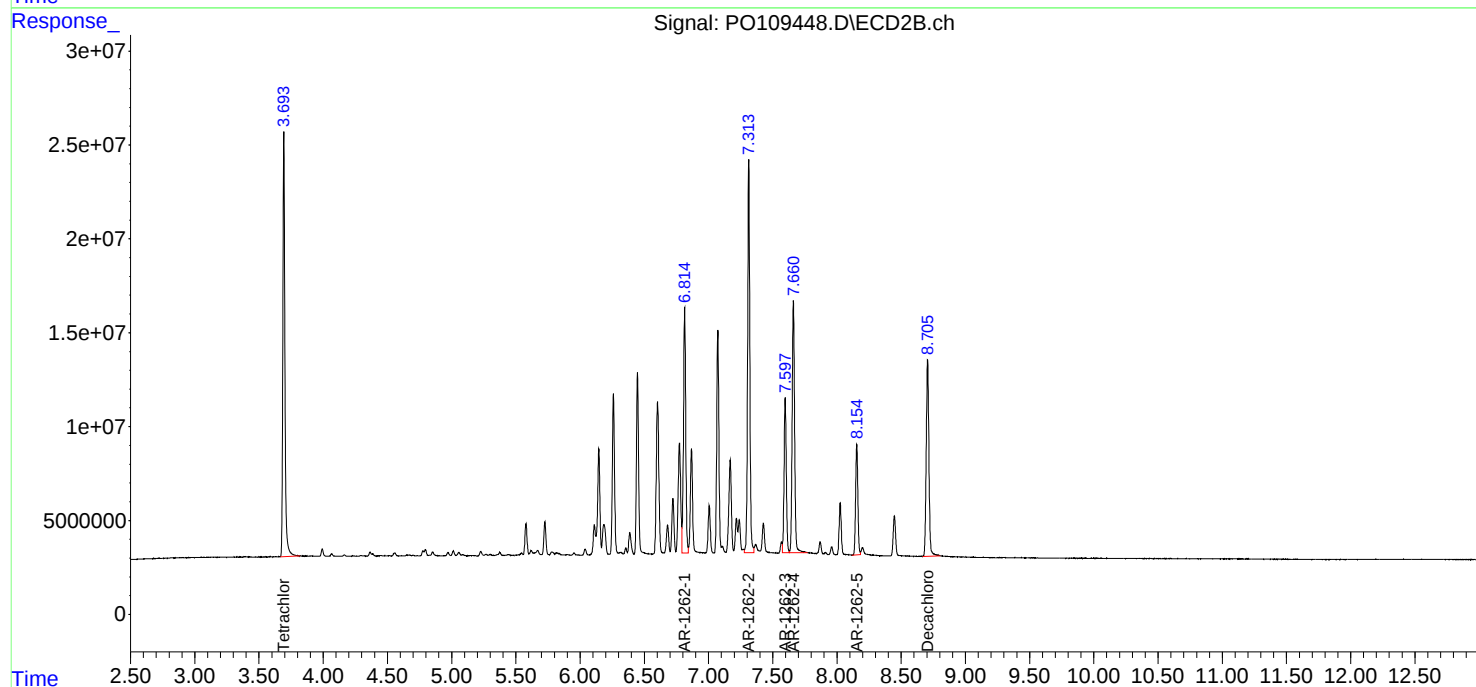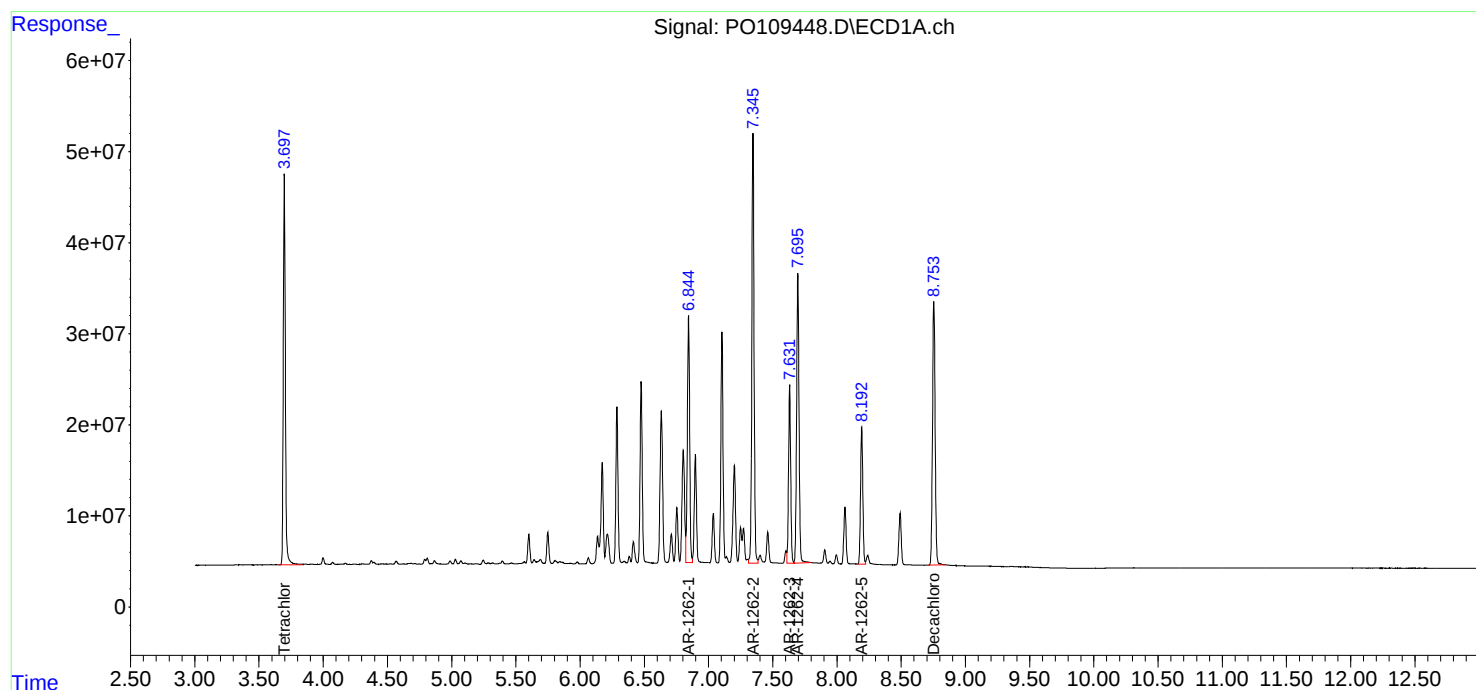

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 23:48
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:17:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:14:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	965.3E6	526.7E6	96.981	98.845
2) SA Decachlor...	8.755	8.706	1414.8E6	495.1E6	97.758	96.622
Target Compounds						
41) L9 AR-1268-1	7.633	7.597	1298.9E6	554.1E6	985.386	982.199
42) L9 AR-1268-2	7.697	7.662	1196.3E6	512.6E6	990.433	984.000
43) L9 AR-1268-3	7.906	7.869	1000.4E6	413.6E6	987.744	983.635
44) L9 AR-1268-4	8.193	8.153	407.5E6	153.7E6	969.568	942.671
45) L9 AR-1268-5	8.493	8.447	3060.4E6	1087.2E6	1007.828	1001.290



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
Data File : P0109449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 23:48
Operator : YP/AJ
Sample : AR1268ICC1000
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:17:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:14:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

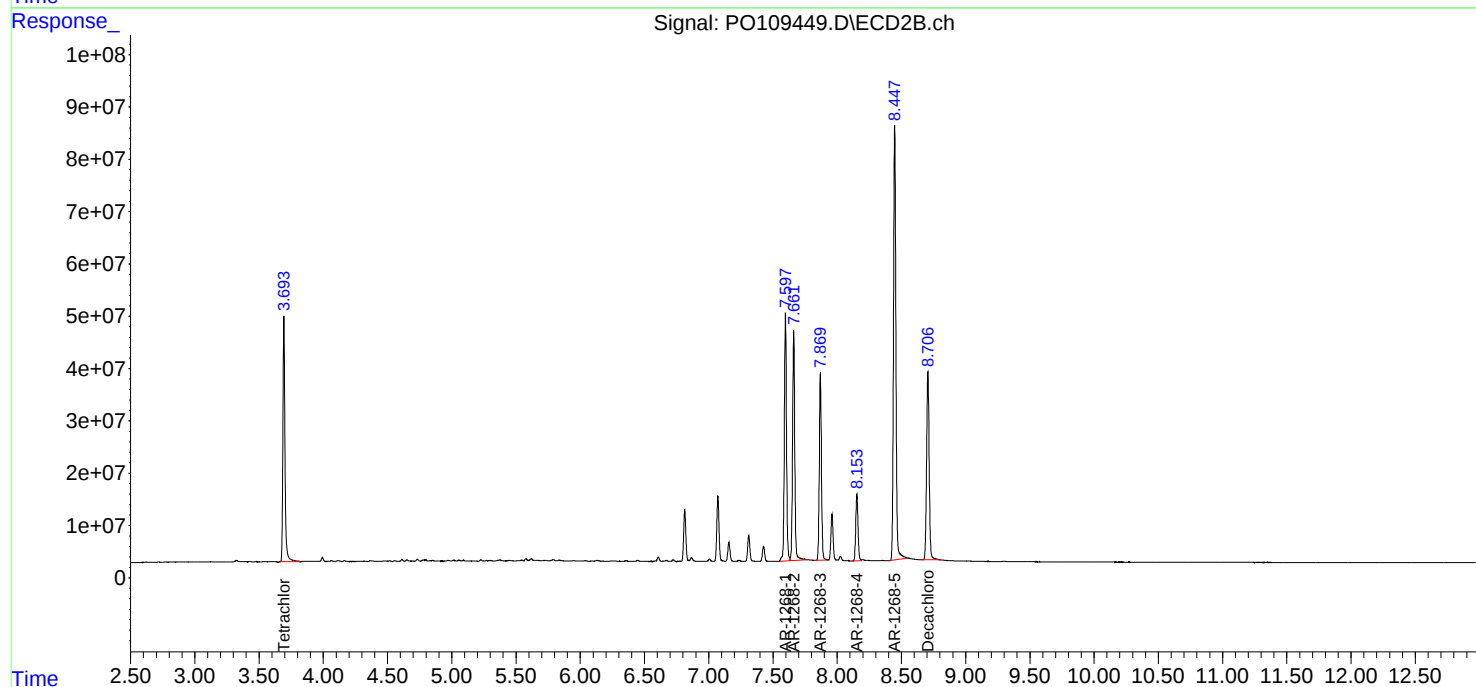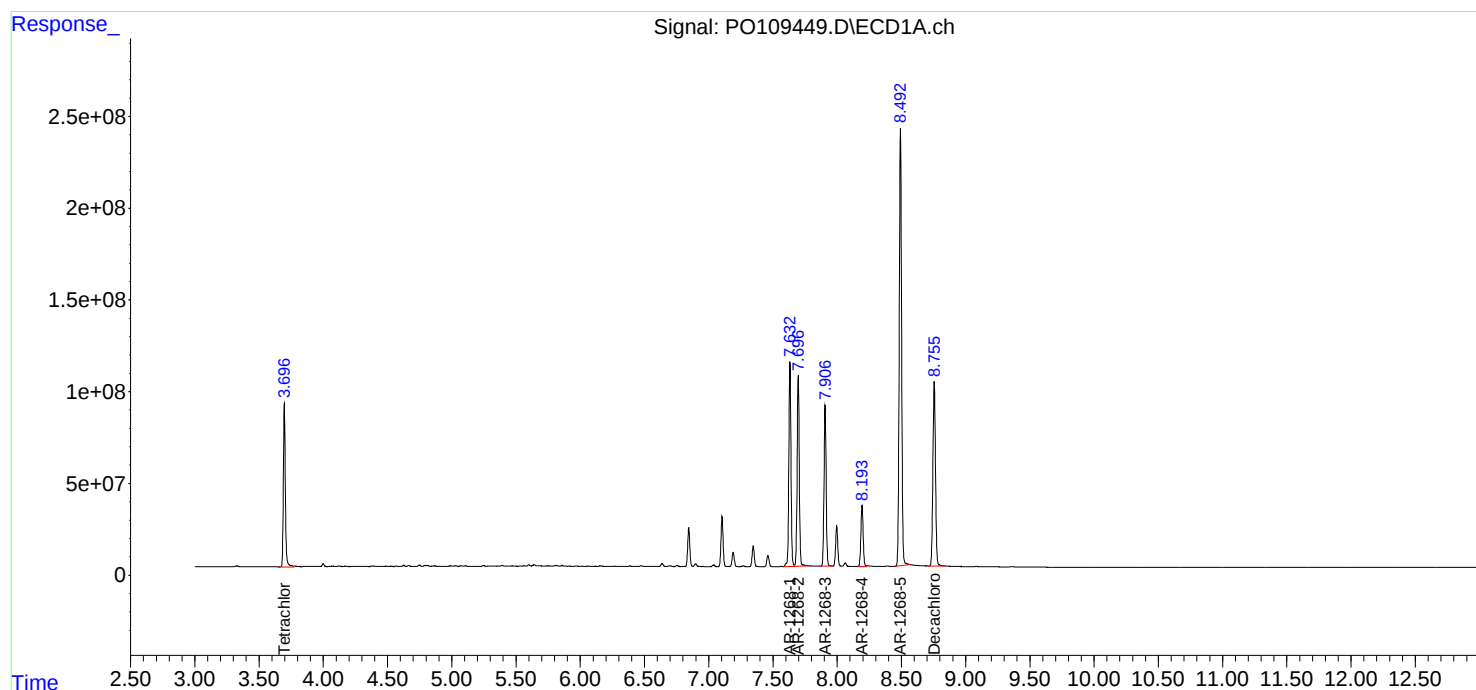

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 00:07
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:17:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:14:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	735.0E6	395.3E6	73.842	74.195
2) SA Decachlor...	8.755	8.705	1059.4E6	373.0E6	73.204	72.789
Target Compounds						
41) L9 AR-1268-1	7.632	7.597	970.5E6	415.4E6	736.275	736.222
42) L9 AR-1268-2	7.697	7.661	892.1E6	383.3E6	738.582	735.790
43) L9 AR-1268-3	7.905	7.870	749.2E6	309.4E6	739.726	735.808
44) L9 AR-1268-4	8.193	8.153	306.7E6	116.3E6	729.785	712.986
45) L9 AR-1268-5	8.492	8.447	2260.0E6	808.5E6	744.267	744.582



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 00:07
Operator : YP/AJ
Sample : AR1268ICC750
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:17:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:14:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

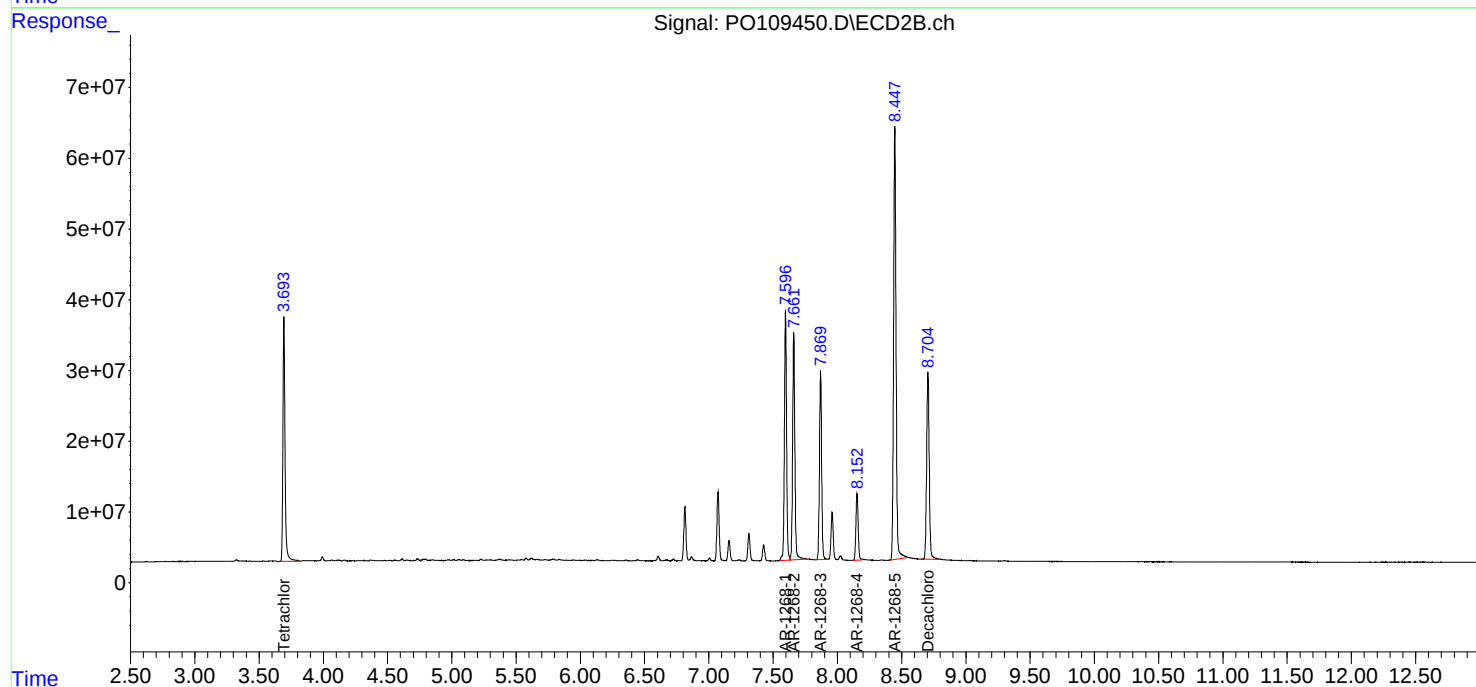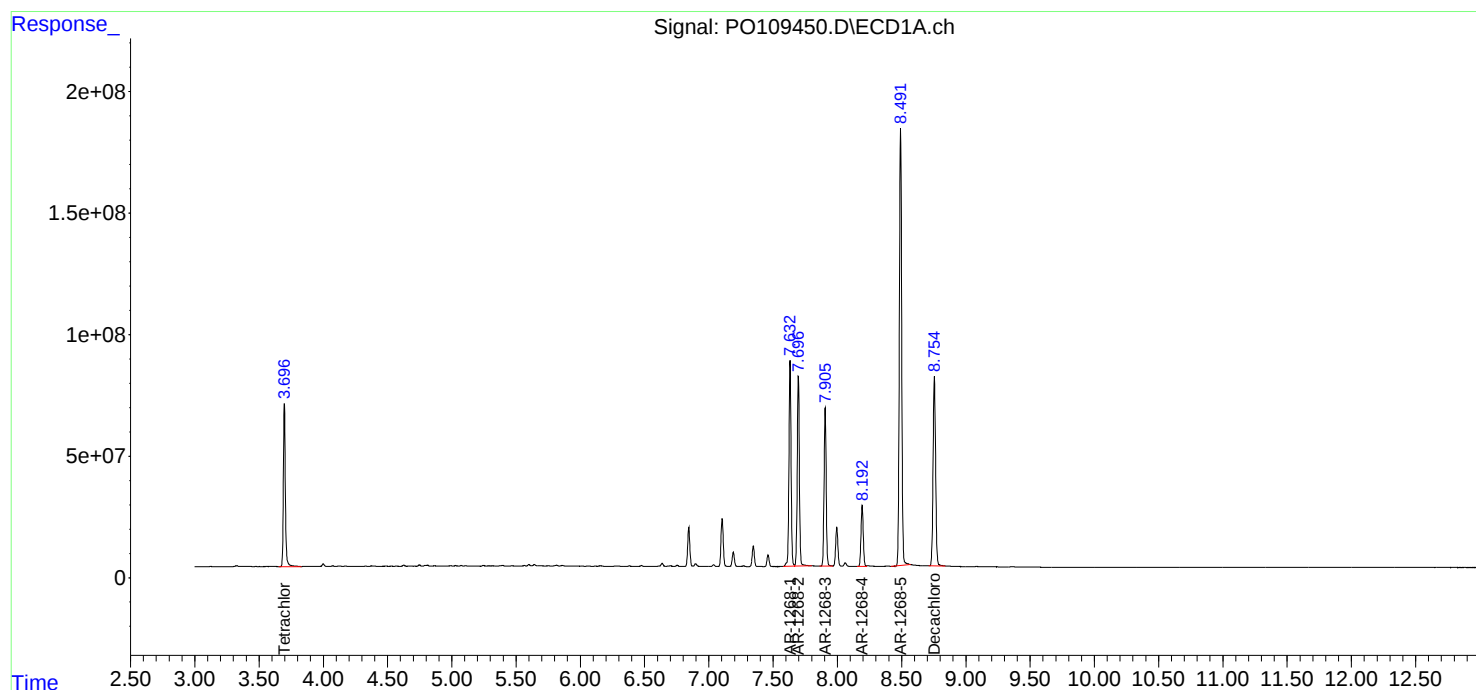

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 00:25
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:17:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:14:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	497.7E6	266.4E6	50.000	50.000
2) SA Decachlor...	8.754	8.705	723.6E6	256.2E6	50.000	50.000
Target Compounds						
41) L9 AR-1268-1	7.632	7.597	659.1E6	282.1E6	500.000	500.000
42) L9 AR-1268-2	7.696	7.662	603.9E6	260.5E6	500.000	500.000
43) L9 AR-1268-3	7.905	7.870	506.4E6	210.3E6	500.000	500.000
44) L9 AR-1268-4	8.193	8.154	210.1E6	81539410	500.000	500.000
45) L9 AR-1268-5	8.492	8.448	1518.3E6	542.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
Data File : P0109451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 00:25
Operator : YP/AJ
Sample : AR1268ICC500
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:17:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:14:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

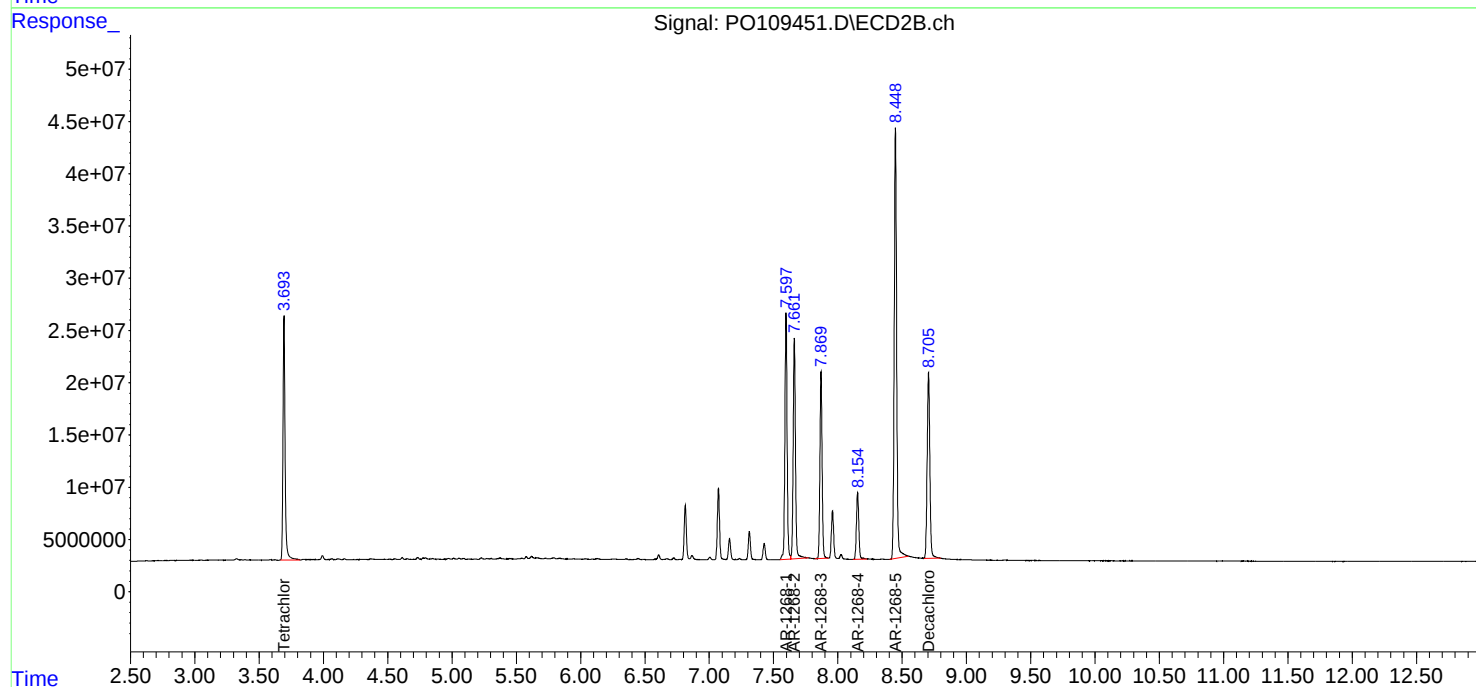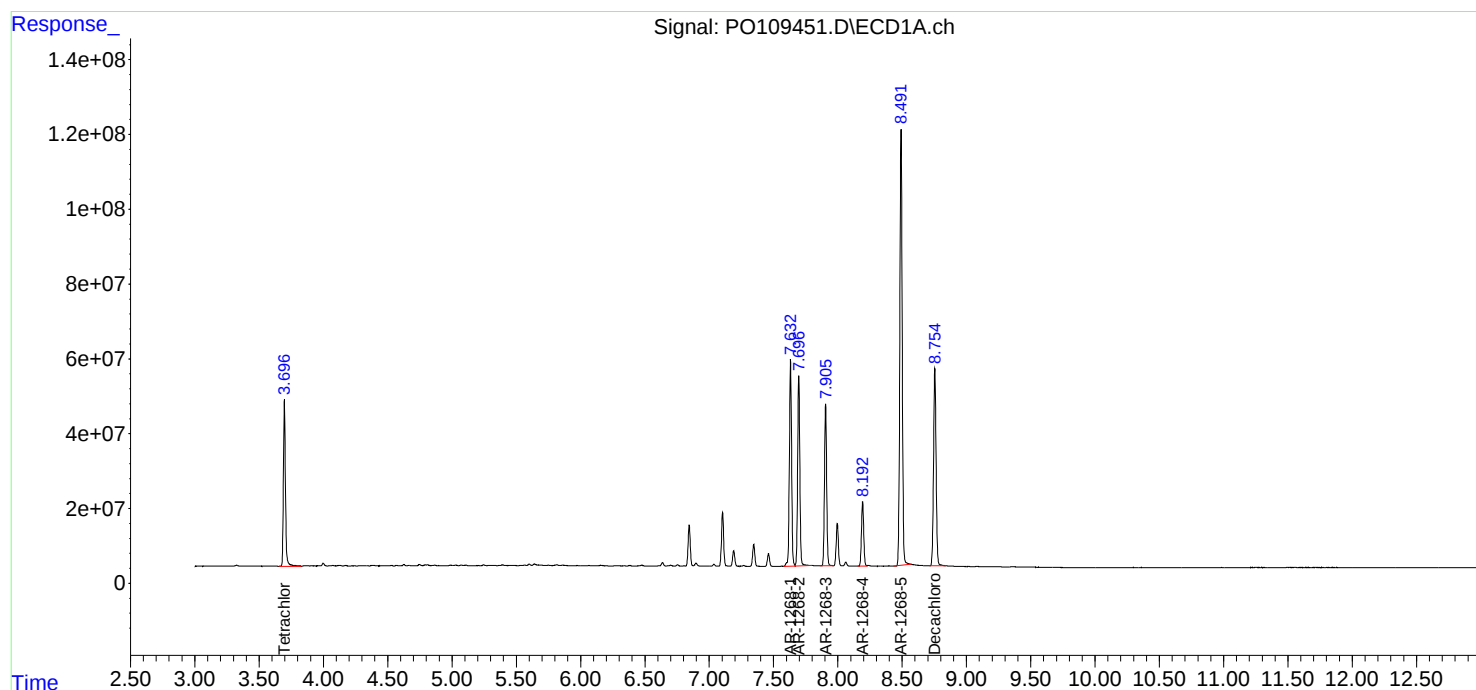

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 00:43
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:17:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:14:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	259.0E6	137.7E6	26.023	25.841
2) SA Decachlor...	8.755	8.705	379.5E6	135.8E6	26.223	26.497
Target Compounds						
41) L9 AR-1268-1	7.632	7.597	341.4E6	147.8E6	259.019	261.921
42) L9 AR-1268-2	7.697	7.661	311.6E6	135.9E6	258.003	260.784
43) L9 AR-1268-3	7.905	7.869	262.4E6	110.6E6	259.092	263.118
44) L9 AR-1268-4	8.193	8.153	110.5E6	42415364	262.992	260.091
45) L9 AR-1268-5	8.492	8.447	768.8E6	280.3E6	253.190	258.141



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 00:43
Operator : YP/AJ
Sample : AR1268ICC250
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:17:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:14:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

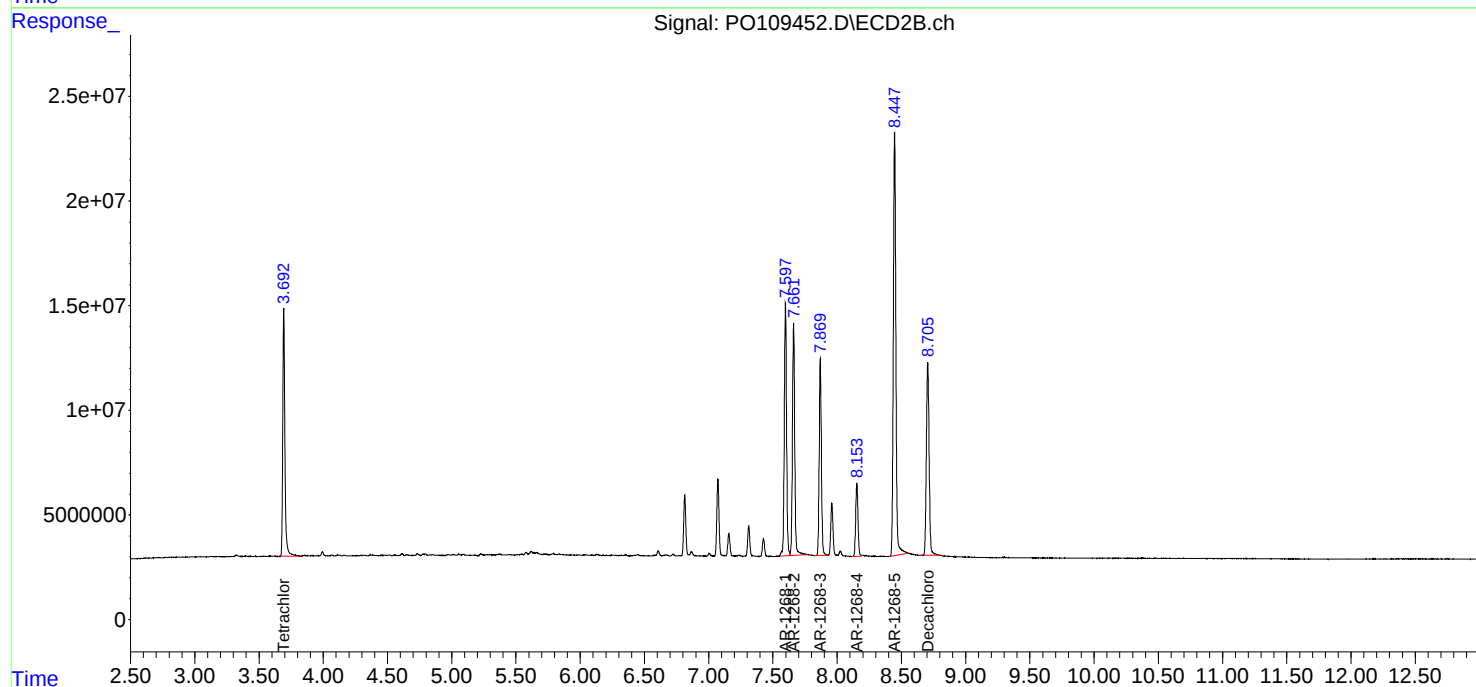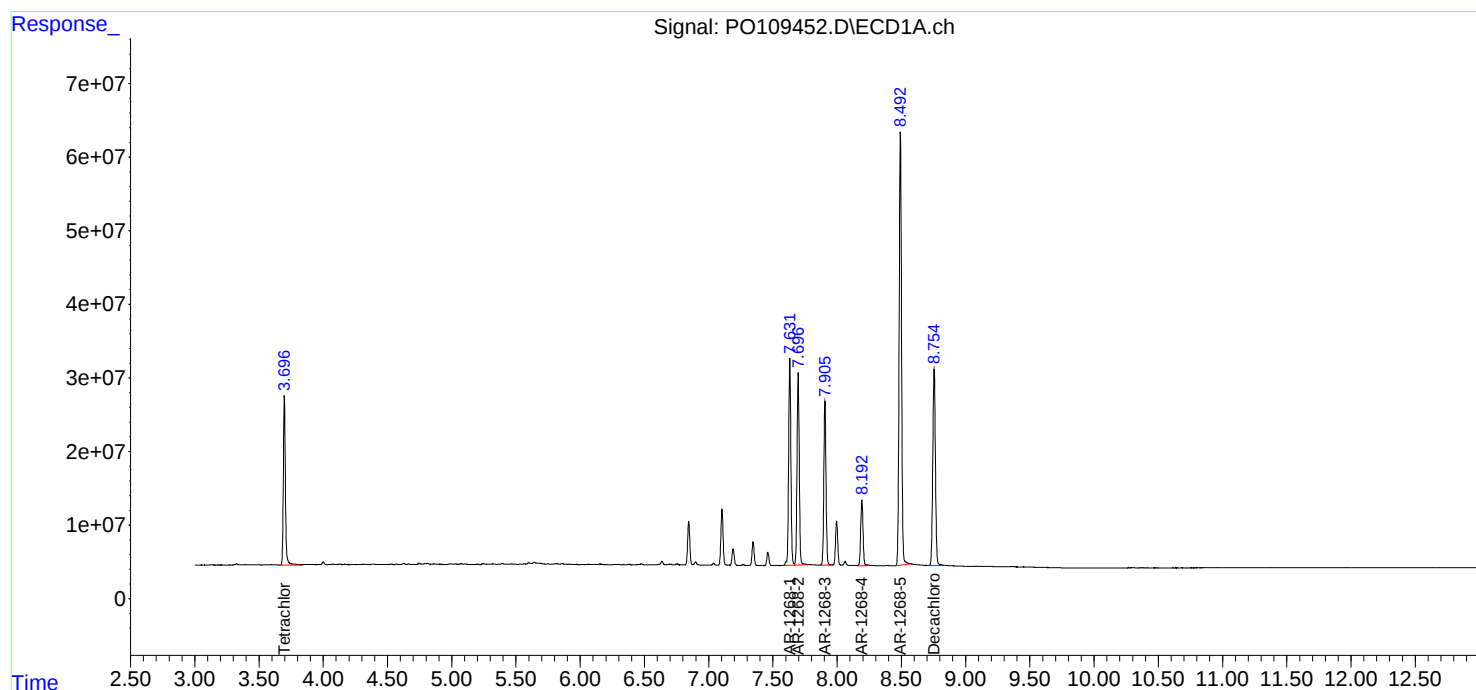

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 01:02
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:18:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:14:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.692	48540301	25644875	4.877	4.813
2) SA Decachlor...	8.754	8.704	77206427	27914892	5.335	5.448
Target Compounds						
41) L9 AR-1268-1	7.632	7.596	67221395	29693417	50.998	52.632
42) L9 AR-1268-2	7.696	7.660	60264035	26832787	49.892	51.507
43) L9 AR-1268-3	7.905	7.869	51454508	22544472	50.804	53.610
44) L9 AR-1268-4	8.191	8.153	22268868	8258744	52.983	50.643
45) L9 AR-1268-5	8.492	8.447	145.6E6	54675030	47.957	50.353



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
Data File : P0109453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 01:02
Operator : YP/AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:18:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:14:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

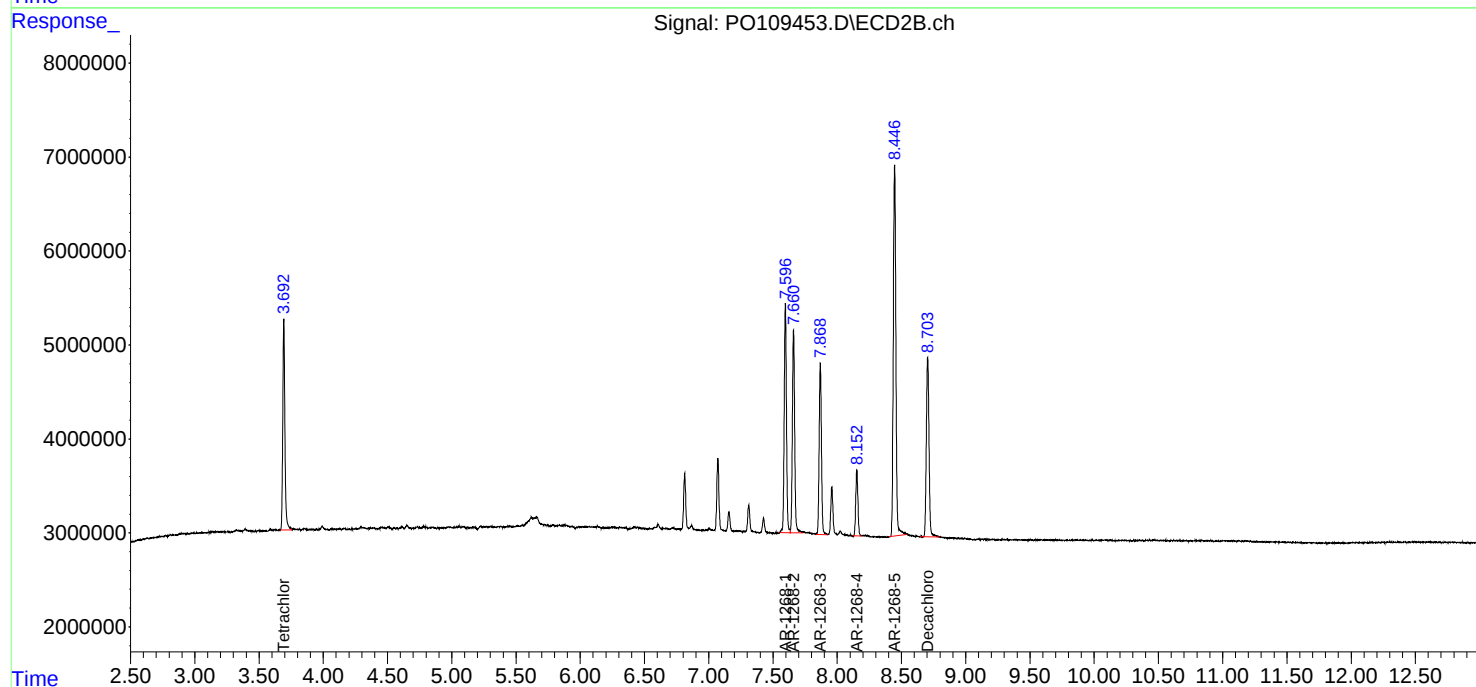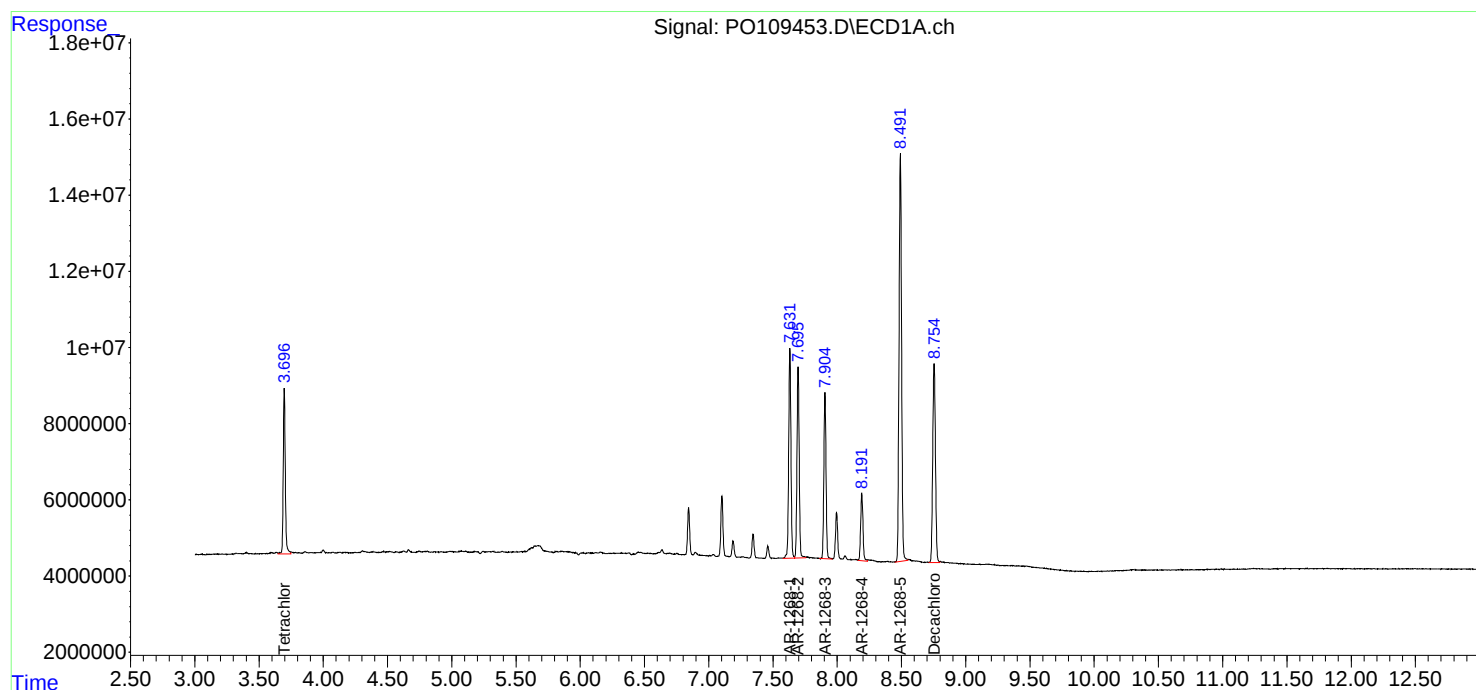

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 01:20
 Operator : YP/AJ
 Sample : P0022025ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO022025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:02:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:00:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.693	485.4E6	269.8E6	51.590	51.681
2) SA Decachlor...	8.754	8.704	443.6E6	158.9E6	51.926	50.342
Target Compounds						
3) L1 AR-1016-1	4.791	4.776	157.1E6	78402892	520.861	515.700
4) L1 AR-1016-2	4.810	4.796	215.0E6	109.8E6	518.628	514.474
5) L1 AR-1016-3	4.866	4.971	152.4E6	60872209	526.733	519.332
6) L1 AR-1016-4	4.987	5.013	119.0E6	52752395	526.672	521.449
7) L1 AR-1016-5	5.245	5.226	131.1E6	68386607	519.681	515.565
31) L7 AR-1260-1	6.286	6.260	235.3E6	118.3E6	513.812	508.238
32) L7 AR-1260-2	6.475	6.447	286.8E6	137.4E6	521.487	511.120
33) L7 AR-1260-3	6.844	6.600	241.2E6	127.7E6	520.450	510.981
34) L7 AR-1260-4	7.105	7.072	220.8E6	103.3E6	518.189	510.781
35) L7 AR-1260-5	7.346	7.312	513.3E6	224.9E6	512.587	506.808



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 01:20
Operator : YP/AJ
Sample : PO022025ICV500
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO022025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:02:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:00:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

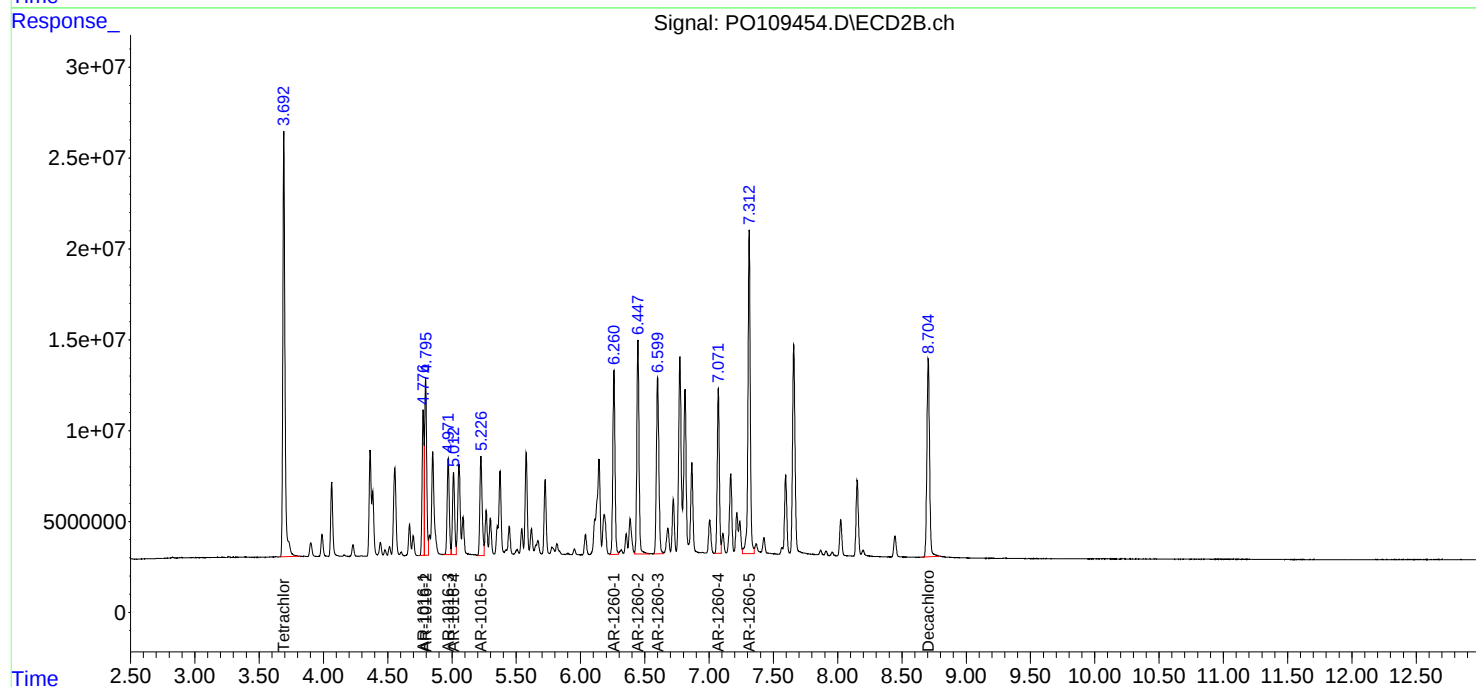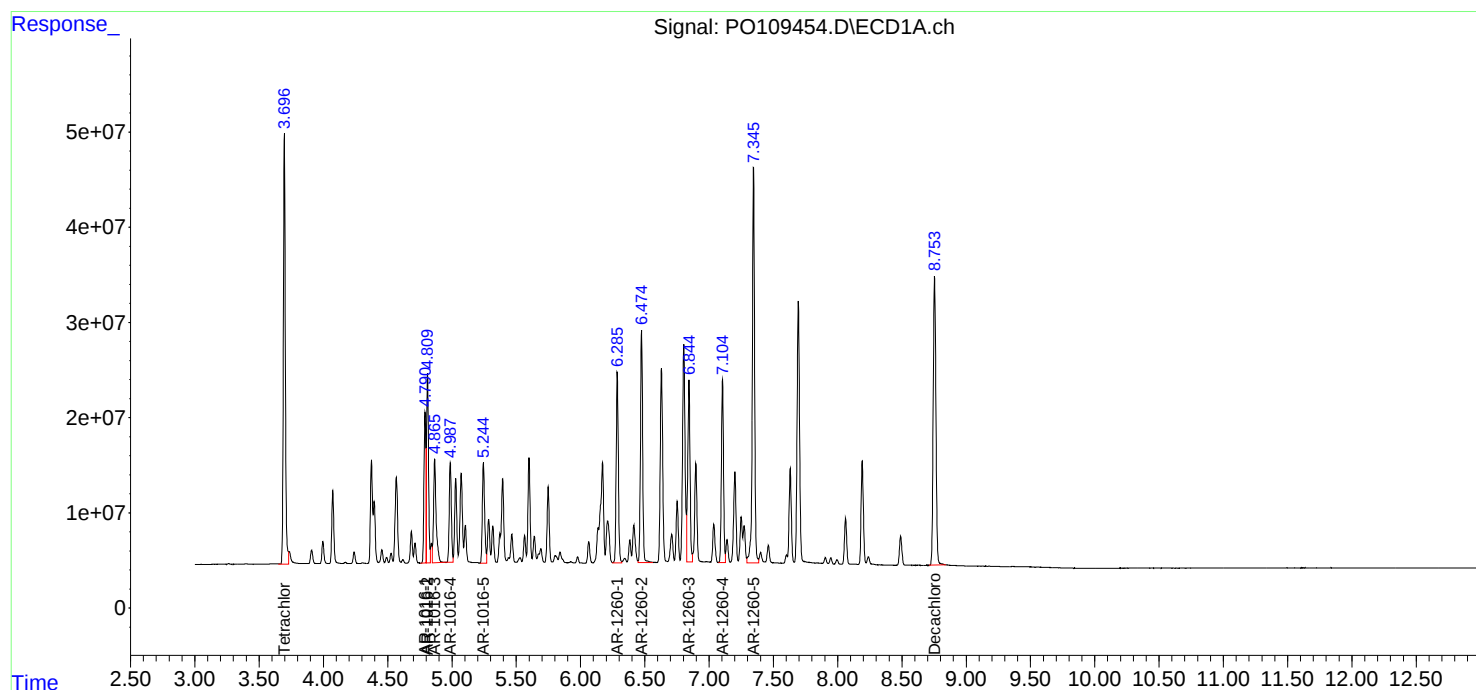

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 01:38
 Operator : YP/AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO022025AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:28:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:26:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	473.0E6	263.5E6	50.071	50.141
2) SA Decachlor...	8.756	8.704	420.7E6	151.7E6	51.323	50.236
Target Compounds						
16) L4 AR-1242-1	4.791	4.777	132.7E6	66474054	503.582	499.322
17) L4 AR-1242-2	4.810	4.795	181.5E6	92310140	503.998	503.693
18) L4 AR-1242-3	4.867	4.971	128.4E6	51844543	500.289	507.061
19) L4 AR-1242-4	4.987	5.055	100.9E6	54380483	503.770	504.509
20) L4 AR-1242-5	5.642	5.577	106.0E6	63476044	499.124	506.838



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 01:38
Operator : YP/AJ
Sample : AR1242ICV500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO022025AR1242

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:28:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:26:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

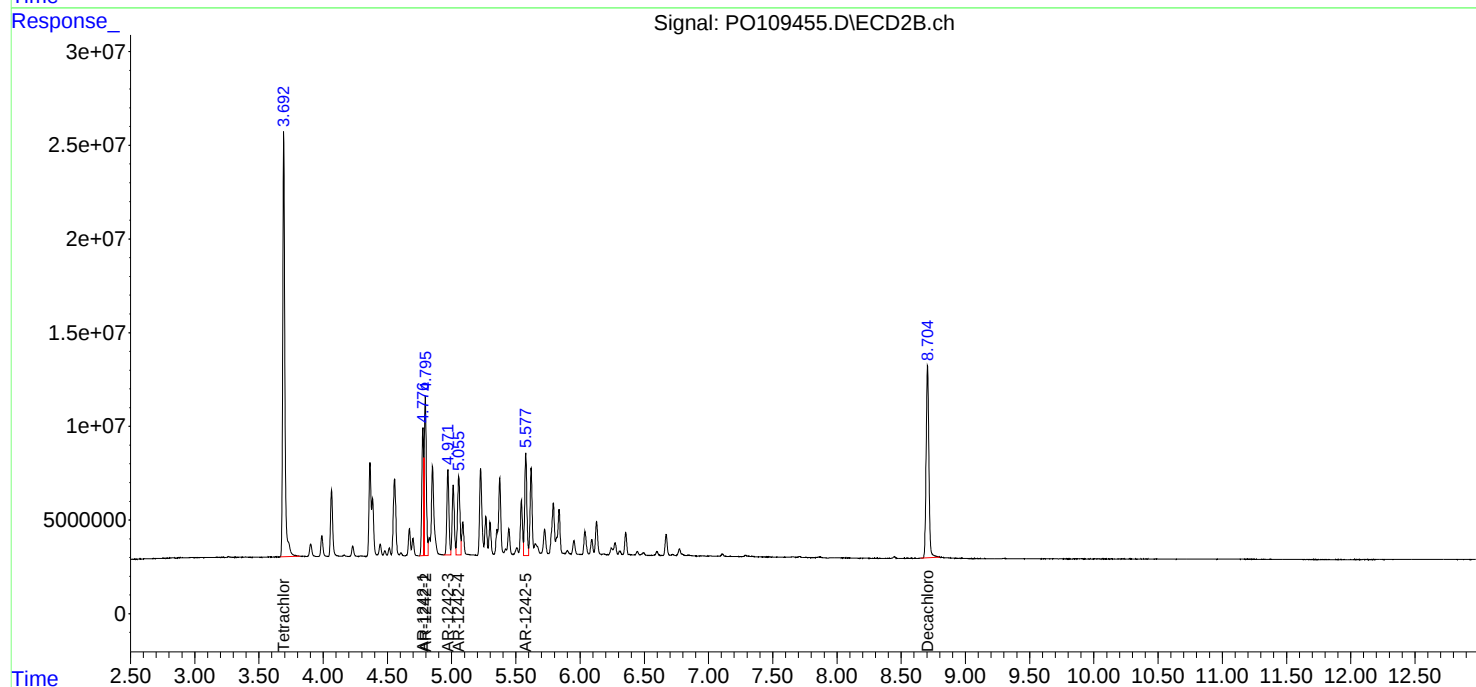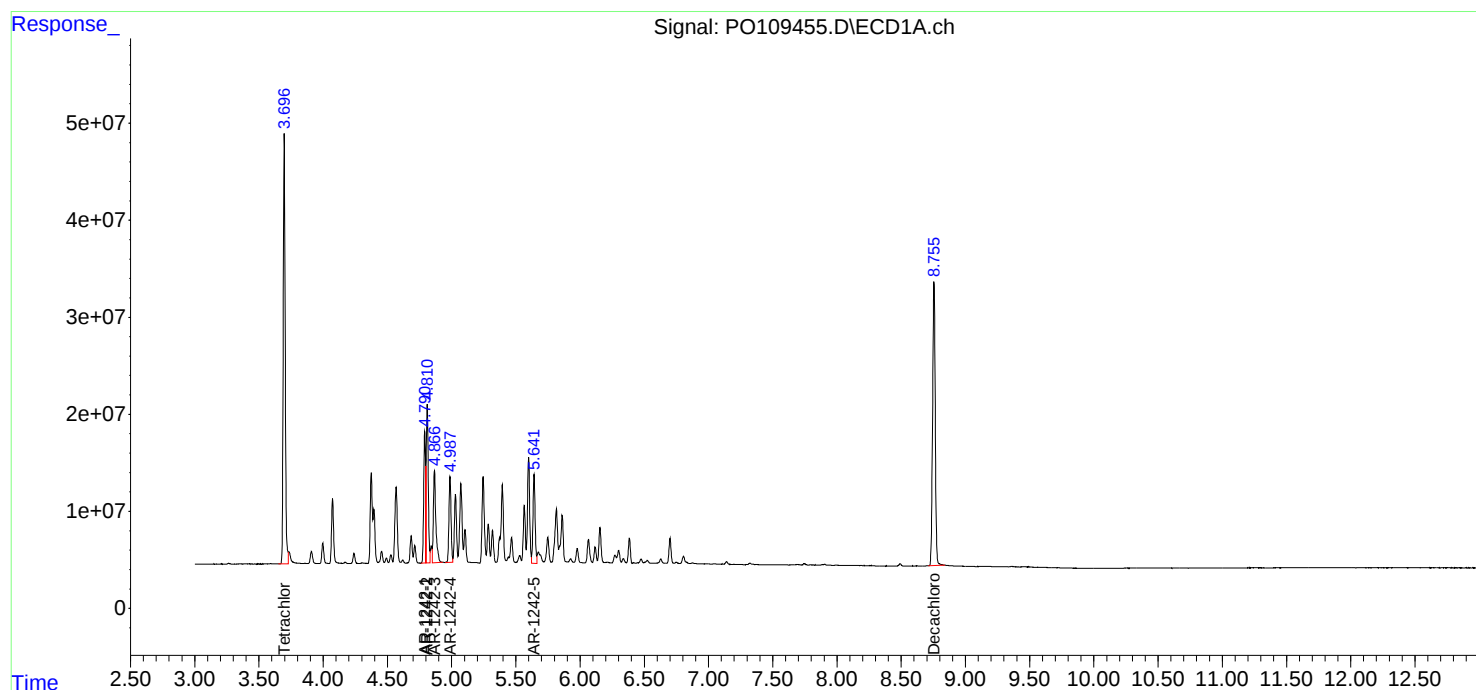

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 01:57
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO022025AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:49:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:44:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.693	490.5E6	262.1E6	50.234	50.194
2) SA Decachlor...	8.754	8.704	425.3E6	152.0E6	51.016	50.037
Target Compounds						
21) L5 AR-1248-1	4.790	4.776	100.9E6	50731291	502.457	503.449
22) L5 AR-1248-2	5.030	5.013	140.5E6	73502388	498.738	501.993
23) L5 AR-1248-3	5.244	5.056	174.2E6	78184021	503.235	502.140
24) L5 AR-1248-4	5.599	5.227	240.3E6	91183159	501.425	505.550
25) L5 AR-1248-5	5.641	5.619	167.5E6	84456599	496.149	498.047



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 01:57
Operator : YP/AJ
Sample : AR1248ICV500
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO022025AR1248

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:49:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:44:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

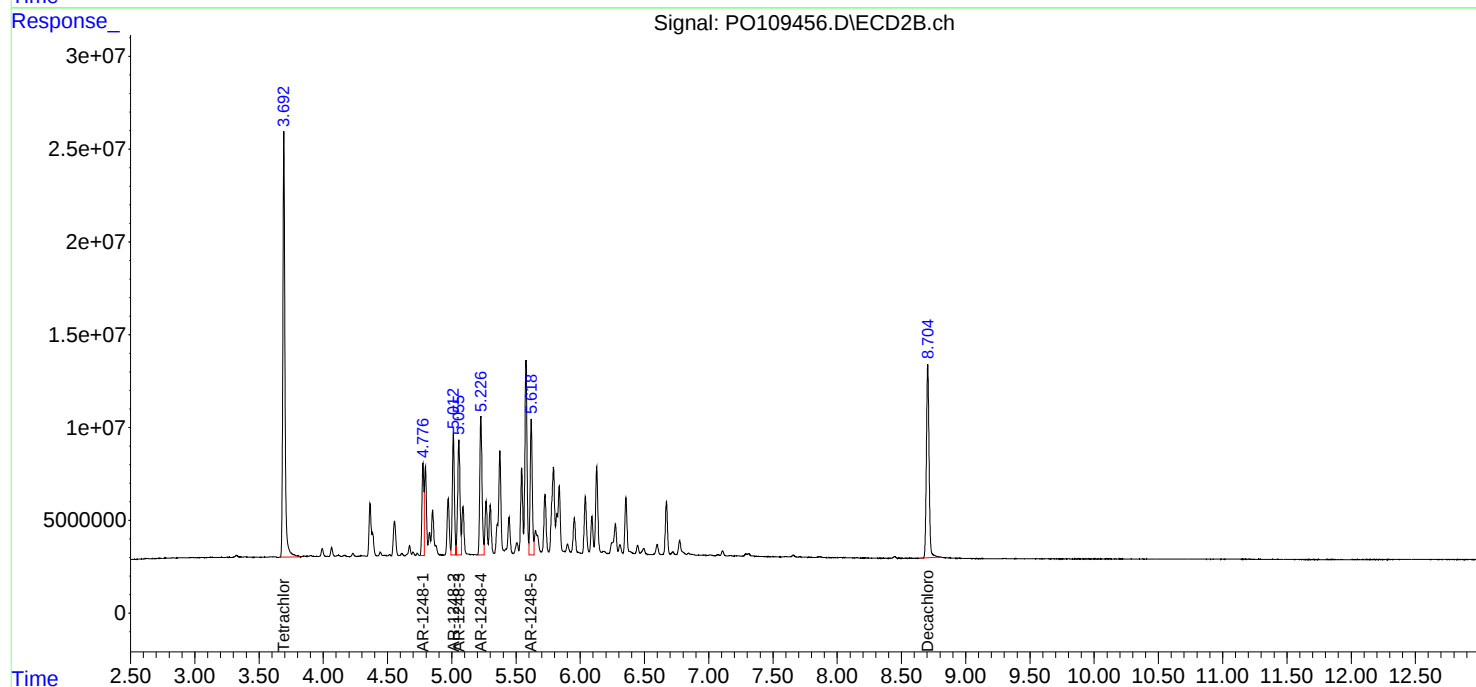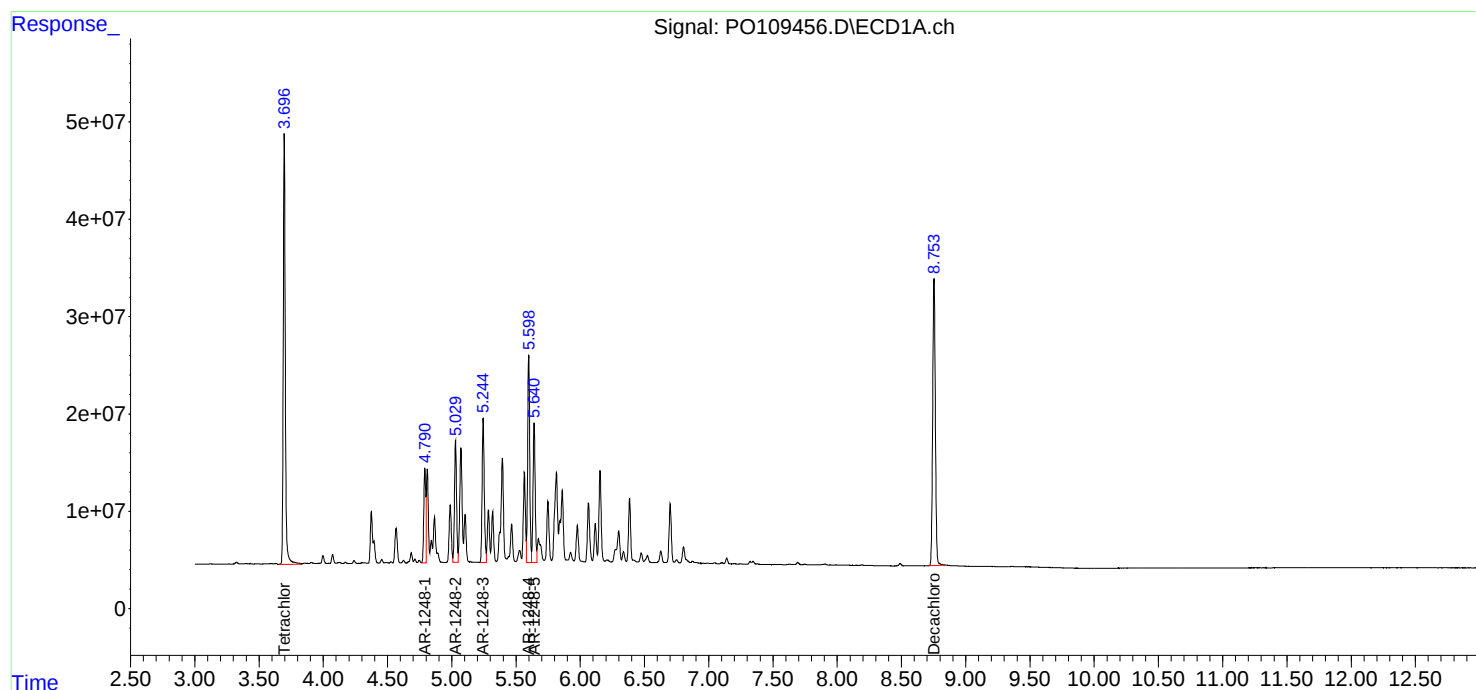

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 02:15
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO022025AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:06:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 03:04:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.693	499.8E6	265.5E6	50.778	50.913
2) SA Decachlor...	8.755	8.705	431.6E6	154.0E6	50.609	50.133
Target Compounds						
26) L6 AR-1254-1	5.600	5.579	259.2E6	131.6E6	503.961	504.534
27) L6 AR-1254-2	5.749	5.727	227.8E6	116.8E6	504.590	506.344
28) L6 AR-1254-3	6.155	6.129	367.1E6	181.9E6	505.885	503.874
29) L6 AR-1254-4	6.385	6.356	217.7E6	101.2E6	507.824	506.393
30) L6 AR-1254-5	6.805	6.775	319.4E6	149.4E6	505.658	504.131



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 02:15
Operator : YP/AJ
Sample : AR1254ICV500
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO022025AR1254

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:06:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 03:04:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

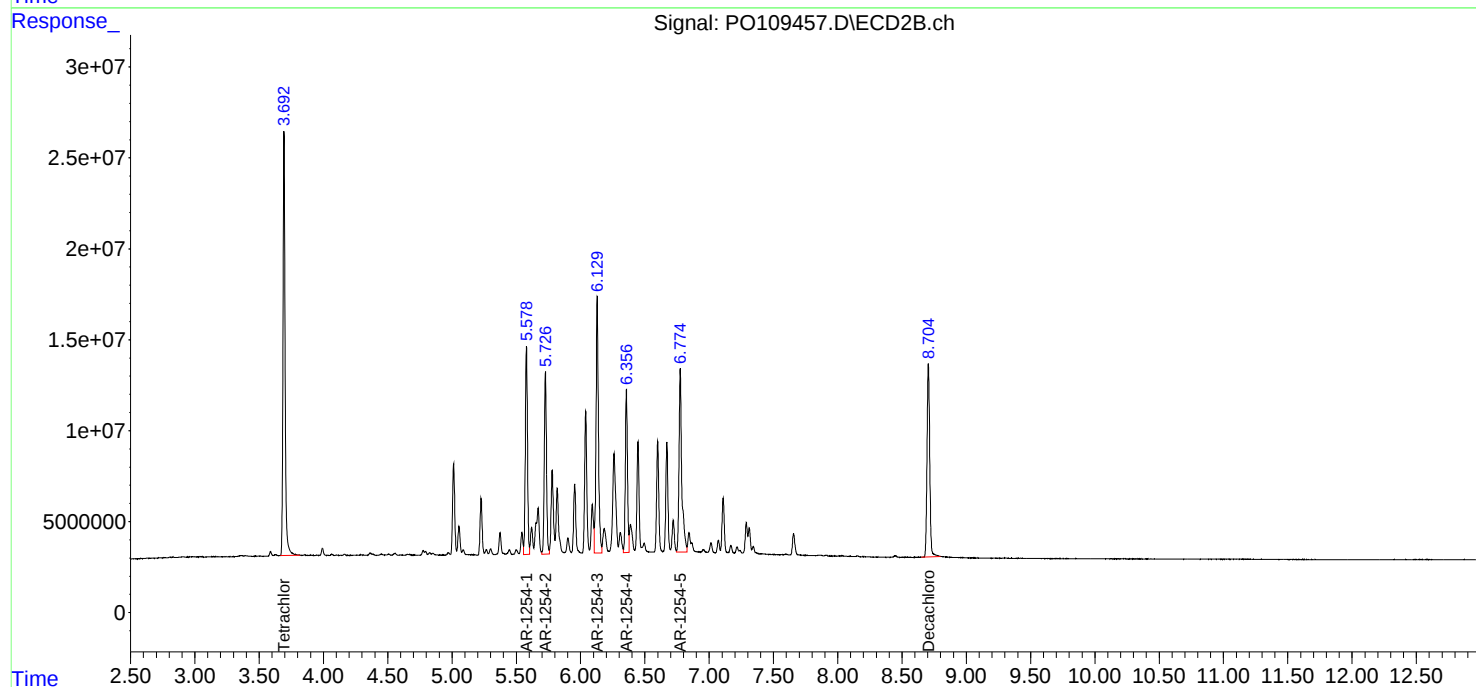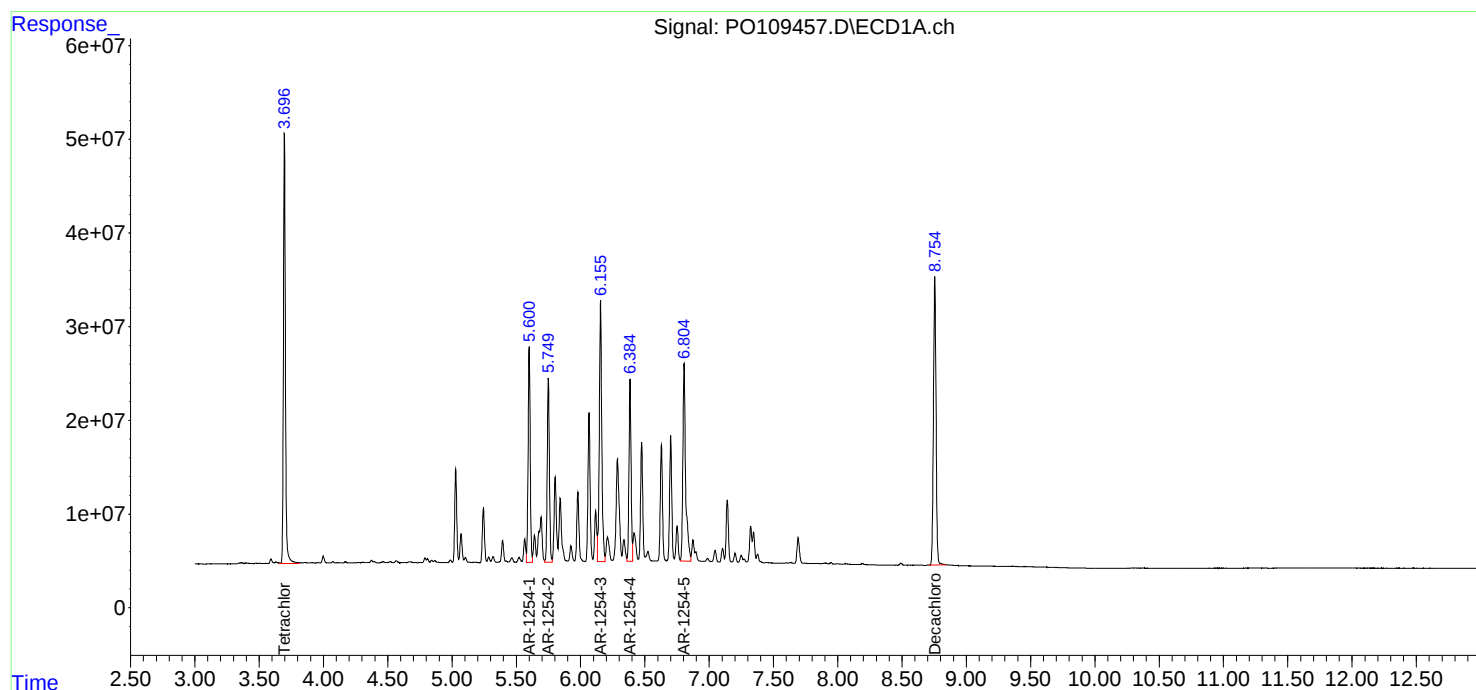

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 02:34
 Operator : YP/AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO022025AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:18:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:14:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.693	505.7E6	272.2E6	50.812	51.081
2) SA Decachlor...	8.754	8.704	737.4E6	260.5E6	50.951	50.843
Target Compounds						
41) L9 AR-1268-1	7.631	7.596	670.6E6	287.4E6	508.735	509.428
42) L9 AR-1268-2	7.696	7.660	616.2E6	265.8E6	510.180	510.135
43) L9 AR-1268-3	7.905	7.868	517.0E6	214.7E6	510.419	510.625
44) L9 AR-1268-4	8.193	8.152	213.4E6	83152742	507.822	509.893
45) L9 AR-1268-5	8.491	8.446	1546.7E6	554.6E6	509.351	510.729



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 02:34
Operator : YP/AJ
Sample : AR1268ICV500
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO022025AR1268

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:18:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:14:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

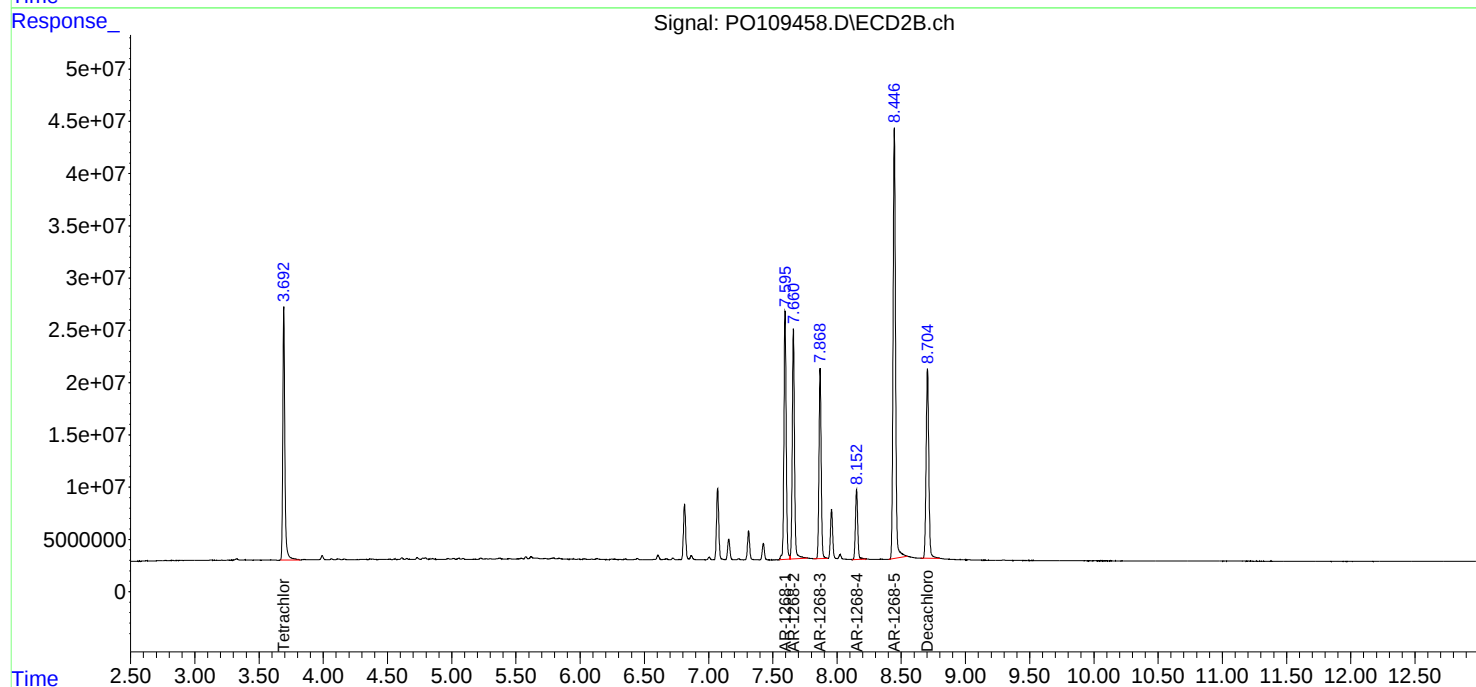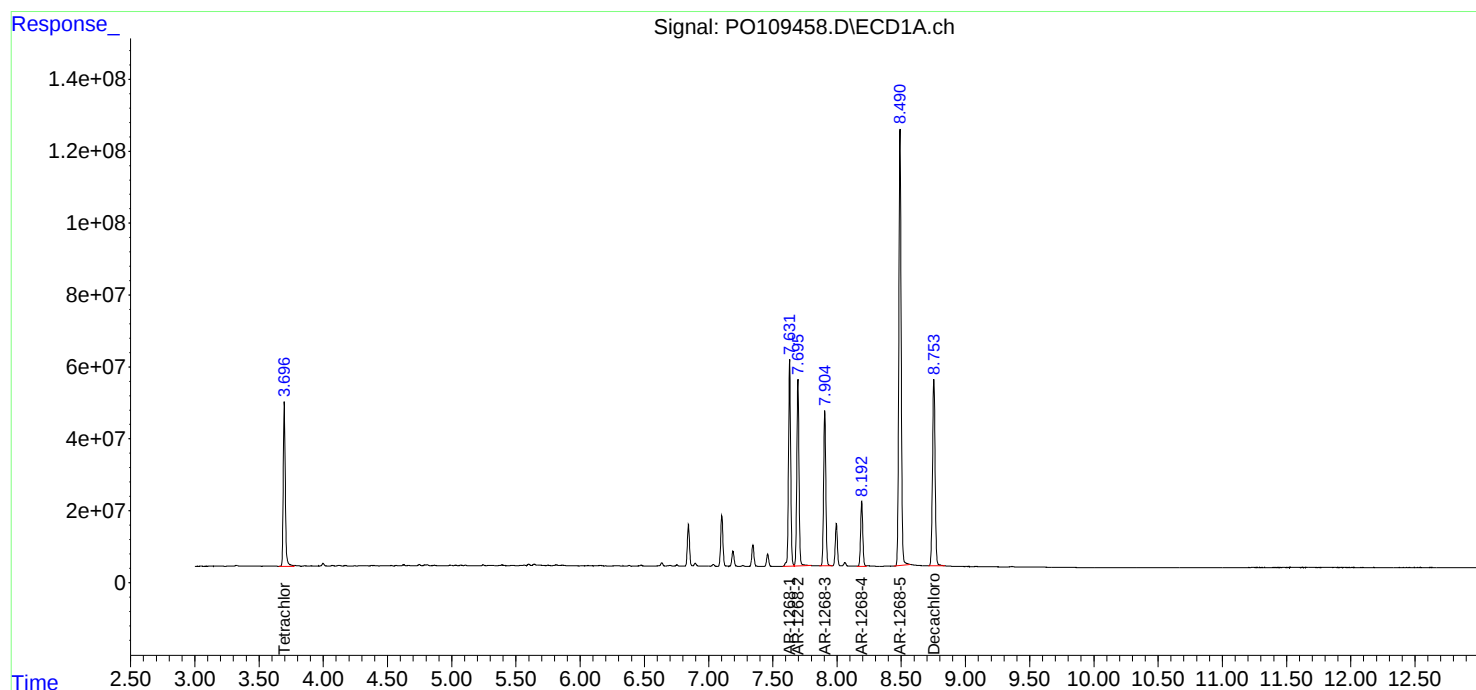



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522 SAS No.: Q1522 SDG NO.: Q1522

Continuing Calib Date: 03/10/2025 Initial Calibration Date(s): 02/20/2025 02/21/2025

Continuing Calib Time: 14:18 Initial Calibration Time(s): 16:46 01:02

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-2	(2)	4.81	4.81	4.71	4.91	0.00
Aroclor-1016-3	(3)	4.86	4.87	4.77	4.97	0.01
Aroclor-1016-4	(4)	4.98	4.99	4.89	5.09	0.01
Aroclor-1016-5	(5)	5.24	5.25	5.15	5.35	0.01
Aroclor-1260-1	(1)	6.28	6.29	6.19	6.39	0.01
Aroclor-1260-2	(2)	6.47	6.48	6.38	6.58	0.01
Aroclor-1260-3	(3)	6.84	6.85	6.75	6.95	0.01
Aroclor-1260-4	(4)	7.10	7.11	7.01	7.21	0.01
Aroclor-1260-5	(5)	7.34	7.35	7.25	7.45	0.01
Tetrachloro-m-xylene		3.70	3.70	3.60	3.80	0.01
Decachlorobiphenyl		8.75	8.76	8.66	8.86	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522 SAS No.: Q1522 SDG NO.: Q1522

Continuing Calib Date: 03/10/2025 Initial Calibration Date(s): 02/20/2025 02/21/2025

Continuing Calib Time: 14:18 Initial Calibration Time(s): 16:46 01:02

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.78	4.78	4.68	4.88	0.00
Aroclor-1016-2	(2)	4.79	4.80	4.70	4.90	0.01
Aroclor-1016-3	(3)	4.97	4.97	4.87	5.07	0.00
Aroclor-1016-4	(4)	5.01	5.01	4.91	5.11	0.00
Aroclor-1016-5	(5)	5.23	5.23	5.13	5.33	0.01
Aroclor-1260-1	(1)	6.26	6.26	6.16	6.36	0.00
Aroclor-1260-2	(2)	6.45	6.45	6.35	6.55	0.00
Aroclor-1260-3	(3)	6.60	6.60	6.50	6.70	0.00
Aroclor-1260-4	(4)	7.07	7.07	6.97	7.17	0.00
Aroclor-1260-5	(5)	7.31	7.31	7.21	7.41	0.00
Tetrachloro-m-xylene		3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl		8.70	8.71	8.61	8.81	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522 SAS No.: Q1522 SDG NO.: Q1522

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 02/20/2025 02/20/2025

Client Sample No.: CCAL01 Date Analyzed: 03/10/2025

Lab Sample No.: AR1660CCC500 Data File : PO109755.D Time Analyzed: 14:18

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.788	4.691	4.891	497.380	500.000	-0.5
Aroclor-1016-2	4.808	4.711	4.911	502.710	500.000	0.5
Aroclor-1016-3	4.864	4.767	4.967	499.300	500.000	-0.1
Aroclor-1016-4	4.984	4.888	5.088	497.350	500.000	-0.5
Aroclor-1016-5	5.242	5.145	5.345	492.520	500.000	-1.5
Aroclor-1260-1	6.283	6.188	6.388	476.930	500.000	-4.6
Aroclor-1260-2	6.472	6.377	6.577	469.660	500.000	-6.1
Aroclor-1260-3	6.840	6.746	6.946	463.460	500.000	-7.3
Aroclor-1260-4	7.101	7.005	7.205	460.840	500.000	-7.8
Aroclor-1260-5	7.343	7.247	7.447	459.090	500.000	-8.2
Decachlorobiphenyl	8.750	8.657	8.857	41.310	50.000	-17.4
Tetrachloro-m-xylene	3.695	3.598	3.798	49.950	50.000	-0.1



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522 SAS No.: Q1522 SDG NO.: Q1522

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 02/20/2025 02/20/2025

Client Sample No.: CCAL01 Date Analyzed: 03/10/2025

Lab Sample No.: AR1660CCC500 Data File : PO109755.D Time Analyzed: 14:18

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.775	4.678	4.878	549.310	500.000	9.9
Aroclor-1016-2	4.794	4.697	4.897	551.780	500.000	10.4
Aroclor-1016-3	4.970	4.872	5.072	551.830	500.000	10.4
Aroclor-1016-4	5.012	4.914	5.114	531.470	500.000	6.3
Aroclor-1016-5	5.225	5.127	5.327	535.450	500.000	7.1
Aroclor-1260-1	6.258	6.161	6.361	514.530	500.000	2.9
Aroclor-1260-2	6.445	6.348	6.548	517.020	500.000	3.4
Aroclor-1260-3	6.599	6.502	6.702	510.860	500.000	2.2
Aroclor-1260-4	7.070	6.974	7.174	501.700	500.000	0.3
Aroclor-1260-5	7.311	7.214	7.414	510.630	500.000	2.1
Decachlorobiphenyl	8.703	8.607	8.807	45.810	50.000	-8.4
Tetrachloro-m-xylene	3.692	3.594	3.794	55.070	50.000	10.1

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031025\
 Data File : PO109755.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2025 14:18
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 14:39:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.695	3.692	472.8E6	288.2E6	49.949	55.069
2) SA Decachlor...	8.750	8.703	355.4E6	145.9E6	41.314	45.808
Target Compounds						
3) L1 AR-1016-1	4.788	4.775	153.3E6	85786248	497.375	549.311
4) L1 AR-1016-2	4.808	4.794	211.7E6	119.4E6	502.707	551.783
5) L1 AR-1016-3	4.864	4.970	147.7E6	65917118	499.298	551.833
6) L1 AR-1016-4	4.984	5.012	115.3E6	55310371	497.348	531.470
7) L1 AR-1016-5	5.242	5.225	127.2E6	72957291	492.522	535.453
31) L7 AR-1260-1	6.283	6.258	222.3E6	121.9E6	476.932	514.528
32) L7 AR-1260-2	6.472	6.445	265.4E6	142.3E6	469.661	517.020
33) L7 AR-1260-3	6.840	6.599	220.5E6	130.3E6	463.462	510.858
34) L7 AR-1260-4	7.101	7.070	198.9E6	103.4E6	460.838	501.695
35) L7 AR-1260-5	7.343	7.311	456.3E6	228.7E6	459.092	510.632



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031025\
Data File : PO109755.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2025 14:18
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 14:39:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

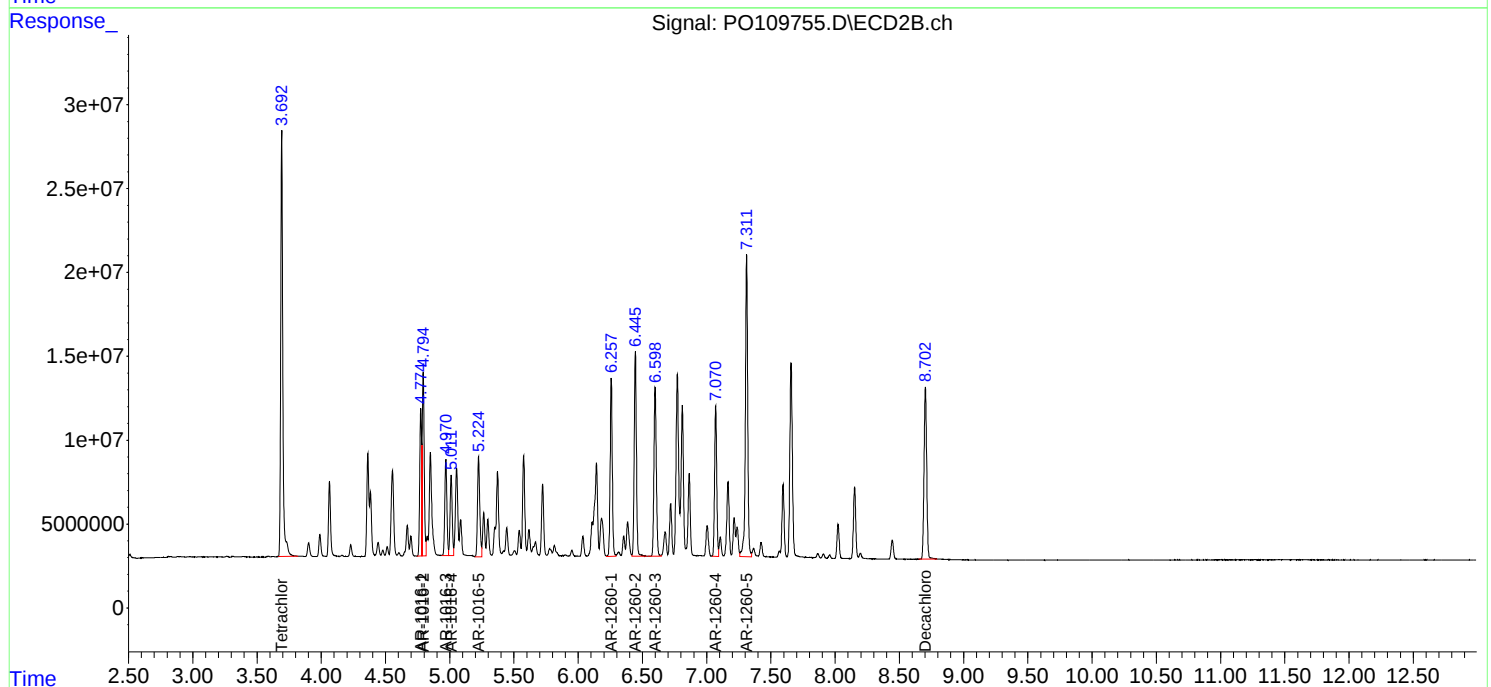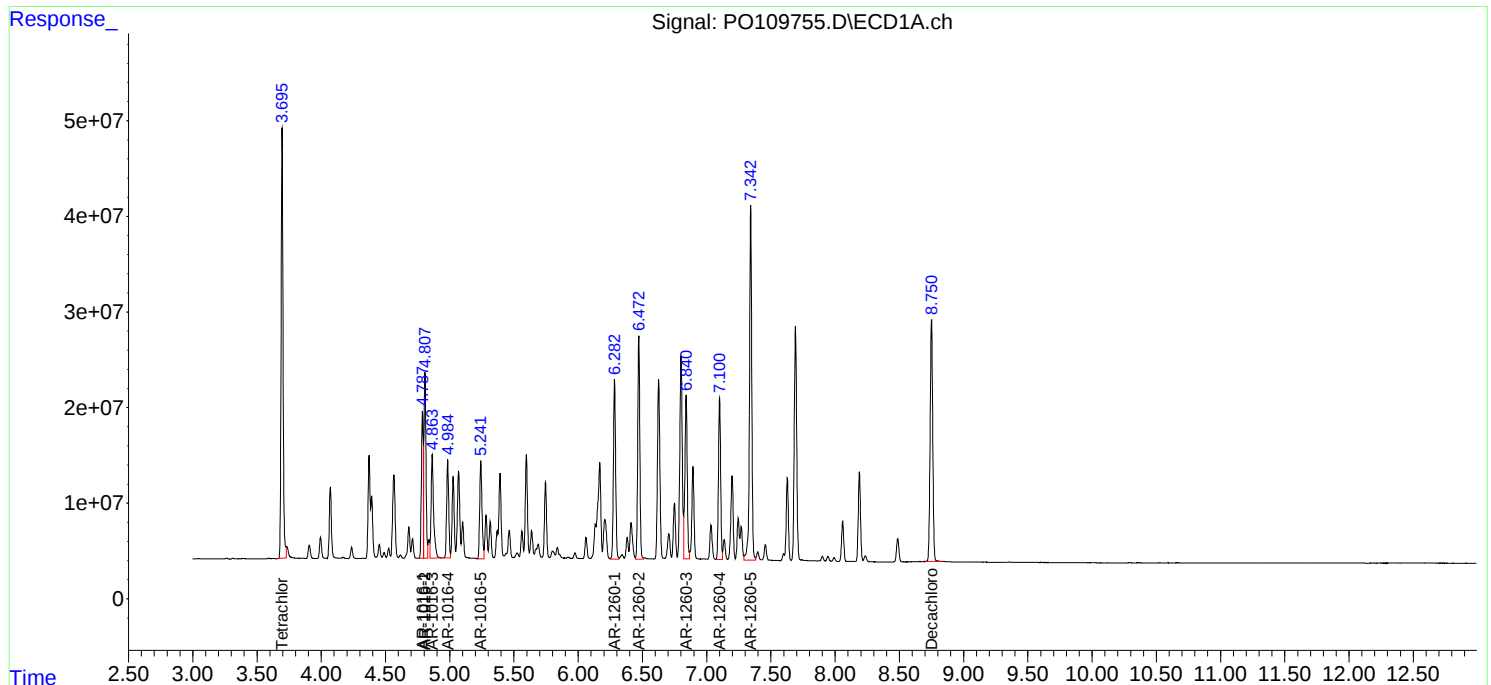



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522 SAS No.: Q1522 SDG NO.: Q1522

Continuing Calib Date: 03/10/2025 Initial Calibration Date(s): 02/20/2025 02/21/2025

Continuing Calib Time: 19:03 Initial Calibration Time(s): 16:46 01:02

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-2	(2)	4.81	4.81	4.71	4.91	0.00
Aroclor-1016-3	(3)	4.86	4.87	4.77	4.97	0.01
Aroclor-1016-4	(4)	4.98	4.99	4.89	5.09	0.01
Aroclor-1016-5	(5)	5.24	5.25	5.15	5.35	0.01
Aroclor-1260-1	(1)	6.28	6.29	6.19	6.39	0.01
Aroclor-1260-2	(2)	6.47	6.48	6.38	6.58	0.01
Aroclor-1260-3	(3)	6.84	6.85	6.75	6.95	0.01
Aroclor-1260-4	(4)	7.10	7.11	7.01	7.21	0.01
Aroclor-1260-5	(5)	7.34	7.35	7.25	7.45	0.01
Tetrachloro-m-xylene		3.70	3.70	3.60	3.80	0.01
Decachlorobiphenyl		8.75	8.76	8.66	8.86	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522 SAS No.: Q1522 SDG NO.: Q1522

Continuing Calib Date: 03/10/2025 Initial Calibration Date(s): 02/20/2025 02/21/2025

Continuing Calib Time: 19:03 Initial Calibration Time(s): 16:46 01:02

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Aroclor-1016-1	(1)	4.78	4.78	4.68	4.88	0.00
Aroclor-1016-2	(2)	4.79	4.80	4.70	4.90	0.01
Aroclor-1016-3	(3)	4.97	4.97	4.87	5.07	0.00
Aroclor-1016-4	(4)	5.01	5.01	4.91	5.11	0.00
Aroclor-1016-5	(5)	5.23	5.23	5.13	5.33	0.01
Aroclor-1260-1	(1)	6.26	6.26	6.16	6.36	0.00
Aroclor-1260-2	(2)	6.45	6.45	6.35	6.55	0.00
Aroclor-1260-3	(3)	6.60	6.60	6.50	6.70	0.00
Aroclor-1260-4	(4)	7.07	7.07	6.97	7.17	0.00
Aroclor-1260-5	(5)	7.31	7.31	7.21	7.41	0.00
Tetrachloro-m-xylene		3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl		8.70	8.71	8.61	8.81	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522 SAS No.: Q1522 SDG NO.: Q1522

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 02/20/2025 02/20/2025

Client Sample No.: CCAL02 Date Analyzed: 03/10/2025

Lab Sample No.: AR1660CCC500 Data File : PO109769.D Time Analyzed: 19:03

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.787	4.691	4.891	515.670	500.000	3.1
Aroclor-1016-2	4.807	4.711	4.911	523.860	500.000	4.8
Aroclor-1016-3	4.864	4.767	4.967	517.840	500.000	3.6
Aroclor-1016-4	4.984	4.888	5.088	512.640	500.000	2.5
Aroclor-1016-5	5.242	5.145	5.345	521.750	500.000	4.4
Aroclor-1260-1	6.283	6.188	6.388	487.690	500.000	-2.5
Aroclor-1260-2	6.472	6.377	6.577	483.630	500.000	-3.3
Aroclor-1260-3	6.840	6.746	6.946	470.450	500.000	-5.9
Aroclor-1260-4	7.100	7.005	7.205	469.560	500.000	-6.1
Aroclor-1260-5	7.342	7.247	7.447	468.410	500.000	-6.3
Decachlorobiphenyl	8.749	8.657	8.857	41.280	50.000	-17.4
Tetrachloro-m-xylene	3.695	3.598	3.798	51.450	50.000	2.9



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522 SAS No.: Q1522 SDG NO.: Q1522

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 02/20/2025 02/20/2025

Client Sample No.: CCAL02 Date Analyzed: 03/10/2025

Lab Sample No.: AR1660CCC500 Data File : PO109769.D Time Analyzed: 19:03

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.775	4.678	4.878	555.990	500.000	11.2
Aroclor-1016-2	4.794	4.697	4.897	566.470	500.000	13.3
Aroclor-1016-3	4.969	4.872	5.072	556.090	500.000	11.2
Aroclor-1016-4	5.012	4.914	5.114	525.520	500.000	5.1
Aroclor-1016-5	5.225	5.127	5.327	528.580	500.000	5.7
Aroclor-1260-1	6.257	6.161	6.361	518.520	500.000	3.7
Aroclor-1260-2	6.445	6.348	6.548	522.170	500.000	4.4
Aroclor-1260-3	6.598	6.502	6.702	513.070	500.000	2.6
Aroclor-1260-4	7.070	6.974	7.174	504.870	500.000	1.0
Aroclor-1260-5	7.310	7.214	7.414	513.060	500.000	2.6
Decachlorobiphenyl	8.702	8.607	8.807	45.310	50.000	-9.4
Tetrachloro-m-xylene	3.693	3.594	3.794	56.080	50.000	12.2

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031025\
 Data File : P0109769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2025 19:03
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 01:01:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.695	3.693	487.0E6	293.5E6	51.452	56.076
2) SA Decachlor...	8.749	8.702	355.1E6	144.3E6	41.279	45.309
Target Compounds						
3) L1 AR-1016-1	4.787	4.775	159.0E6	86829081	515.675	555.989
4) L1 AR-1016-2	4.807	4.794	220.6E6	122.6E6	523.857	566.470
5) L1 AR-1016-3	4.864	4.969	153.2E6	66425148	517.835	556.086
6) L1 AR-1016-4	4.984	5.012	118.8E6	54691334	512.641	525.522
7) L1 AR-1016-5	5.242	5.225	134.7E6	72020656	521.754	528.578
31) L7 AR-1260-1	6.283	6.257	227.3E6	122.8E6	487.690	518.524
32) L7 AR-1260-2	6.472	6.445	273.3E6	143.7E6	483.628	522.167
33) L7 AR-1260-3	6.840	6.598	223.8E6	130.9E6	470.454	513.067
34) L7 AR-1260-4	7.100	7.070	202.7E6	104.1E6	469.563	504.866
35) L7 AR-1260-5	7.342	7.310	465.5E6	229.7E6	468.406	513.061



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031025\
Data File : PO109769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2025 19:03
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 01:01:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

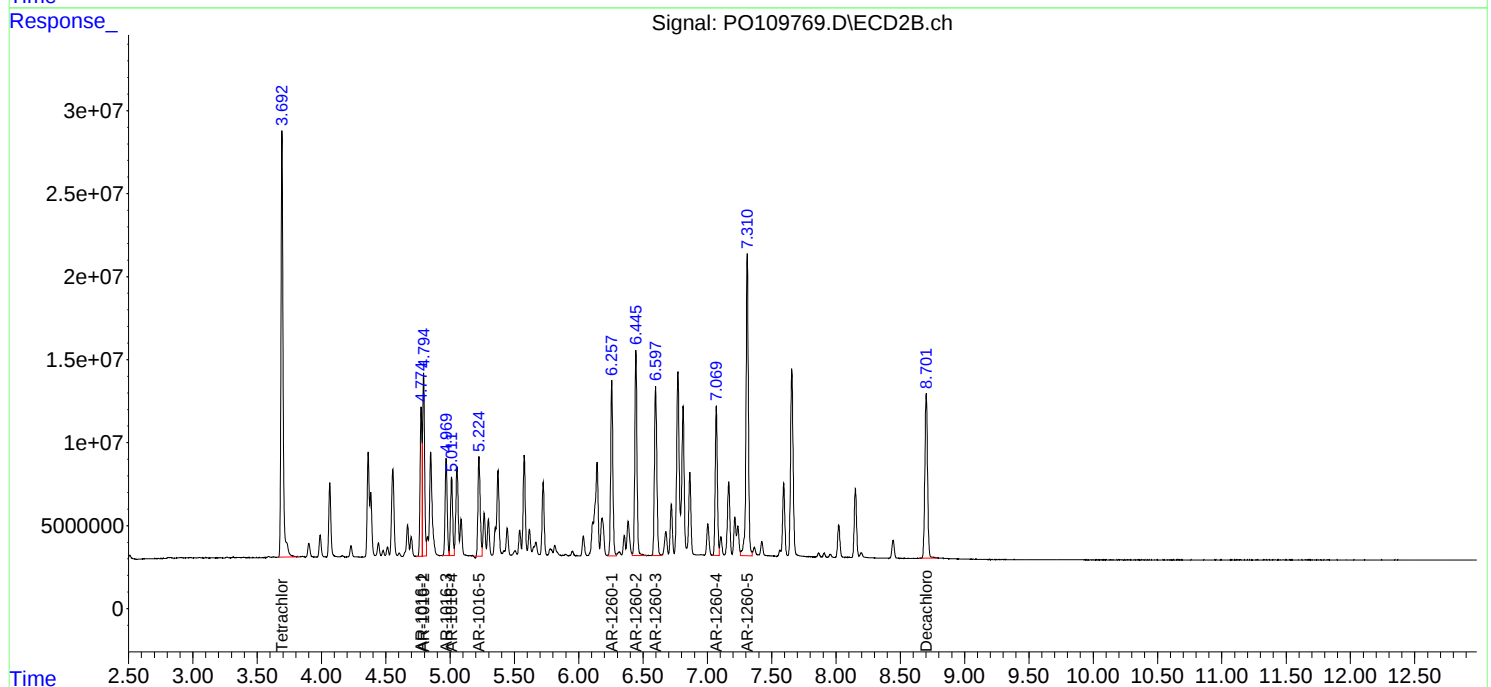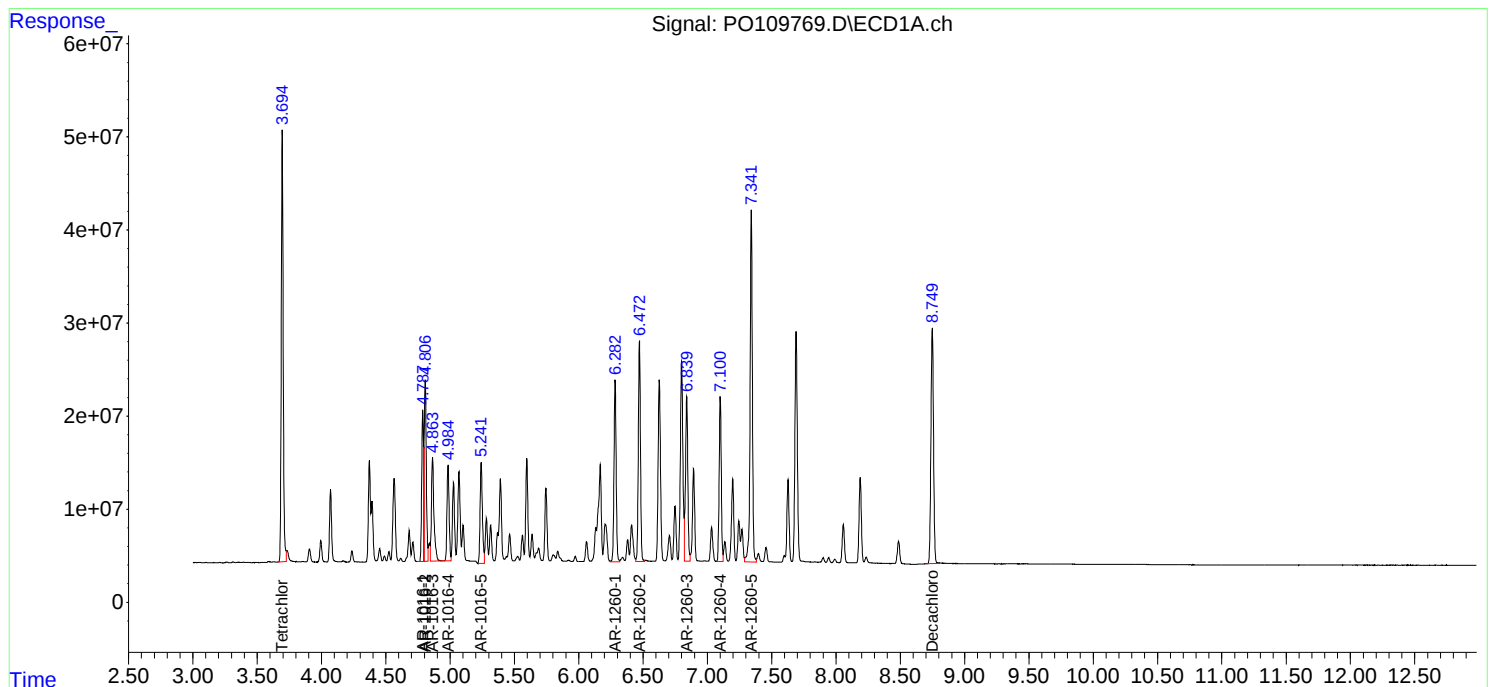

Analytical Sequence

Client: ENTACT

SDG No.: Q1522

Project: 540 Degraw St, Brooklyn, NY - E9309

Instrument ID: ECD_O

GC Column: ZB-MR1

ID: 0.32 (mm)

Inst. Calib. Date(s): 02/20/2025 02/20/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	02/20/2025	16:28	PO109425.D	8.76	3.70
AR1660ICC1000	AR1660ICC1000	02/20/2025	16:46	PO109426.D	8.76	3.70
AR1660ICC750	AR1660ICC750	02/20/2025	17:04	PO109427.D	8.76	3.70
AR1660ICC500	AR1660ICC500	02/20/2025	17:23	PO109428.D	8.76	3.70
AR1660ICC250	AR1660ICC250	02/20/2025	17:41	PO109429.D	8.76	3.70
AR1660ICC050	AR1660ICC050	02/20/2025	17:59	PO109430.D	8.76	3.70
AR1221ICC500	AR1221ICC500	02/20/2025	18:18	PO109431.D	8.76	3.70
AR1232ICC500	AR1232ICC500	02/20/2025	18:36	PO109432.D	8.76	3.70
AR1242ICC1000	AR1242ICC1000	02/20/2025	18:55	PO109433.D	8.76	3.70
AR1242ICC750	AR1242ICC750	02/20/2025	19:13	PO109434.D	8.76	3.70
AR1242ICC500	AR1242ICC500	02/20/2025	19:31	PO109435.D	8.76	3.70
AR1242ICC250	AR1242ICC250	02/20/2025	19:50	PO109436.D	8.76	3.70
AR1242ICC050	AR1242ICC050	02/20/2025	20:08	PO109437.D	8.76	3.70
AR1248ICC1000	AR1248ICC1000	02/20/2025	20:26	PO109438.D	8.76	3.70
AR1248ICC750	AR1248ICC750	02/20/2025	20:45	PO109439.D	8.76	3.70
AR1248ICC500	AR1248ICC500	02/20/2025	21:03	PO109440.D	8.76	3.70
AR1248ICC250	AR1248ICC250	02/20/2025	21:21	PO109441.D	8.76	3.70
AR1248ICC050	AR1248ICC050	02/20/2025	21:40	PO109442.D	8.75	3.70
AR1254ICC1000	AR1254ICC1000	02/20/2025	21:58	PO109443.D	8.75	3.70
AR1254ICC750	AR1254ICC750	02/20/2025	22:17	PO109444.D	8.76	3.70
AR1254ICC500	AR1254ICC500	02/20/2025	22:35	PO109445.D	8.76	3.70
AR1254ICC250	AR1254ICC250	02/20/2025	22:53	PO109446.D	8.76	3.70
AR1254ICC050	AR1254ICC050	02/20/2025	23:12	PO109447.D	8.76	3.70
AR1262ICC500	AR1262ICC500	02/20/2025	23:30	PO109448.D	8.75	3.70
AR1268ICC1000	AR1268ICC1000	02/20/2025	23:48	PO109449.D	8.76	3.70
AR1268ICC750	AR1268ICC750	02/21/2025	00:07	PO109450.D	8.76	3.70
AR1268ICC500	AR1268ICC500	02/21/2025	00:25	PO109451.D	8.75	3.70
AR1268ICC250	AR1268ICC250	02/21/2025	00:43	PO109452.D	8.76	3.70
AR1268ICC050	AR1268ICC050	02/21/2025	01:02	PO109453.D	8.75	3.70
AR1660CCC500	AR1660CCC500	03/10/2025	14:18	PO109755.D	8.75	3.70
IBLK	IBLK	03/10/2025	15:31	PO109759.D	8.75	3.69
PB167042BL	PB167042BL	03/10/2025	15:49	PO109760.D	8.75	3.70
PB167042BS	PB167042BS	03/10/2025	16:07	PO109761.D	8.75	3.70
PB167042BSD	PB167042BSD	03/10/2025	16:26	PO109762.D	8.75	3.70
TW-WTS-04	Q1522-02	03/10/2025	17:03	PO109764.D	8.75	3.70
AR1660CCC500	AR1660CCC500	03/10/2025	19:03	PO109769.D	8.75	3.70
IBLK	IBLK	03/10/2025	20:15	PO109773.D	8.75	3.70

Analytical Sequence

Client: ENTACT

SDG No.: Q1522

Project: 540 Degraw St, Brooklyn, NY - E9309

Instrument ID: ECD_O

GC Column: ZB-MR2

ID: 0.32 (mm)

Inst. Calib. Date(s): 02/20/2025 02/20/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	02/20/2025	16:28	PO109425.D	8.71	3.69
AR1660ICC1000	AR1660ICC1000	02/20/2025	16:46	PO109426.D	8.71	3.69
AR1660ICC750	AR1660ICC750	02/20/2025	17:04	PO109427.D	8.71	3.69
AR1660ICC500	AR1660ICC500	02/20/2025	17:23	PO109428.D	8.71	3.69
AR1660ICC250	AR1660ICC250	02/20/2025	17:41	PO109429.D	8.71	3.69
AR1660ICC050	AR1660ICC050	02/20/2025	17:59	PO109430.D	8.71	3.69
AR1221ICC500	AR1221ICC500	02/20/2025	18:18	PO109431.D	8.71	3.69
AR1232ICC500	AR1232ICC500	02/20/2025	18:36	PO109432.D	8.71	3.69
AR1242ICC1000	AR1242ICC1000	02/20/2025	18:55	PO109433.D	8.71	3.69
AR1242ICC750	AR1242ICC750	02/20/2025	19:13	PO109434.D	8.71	3.69
AR1242ICC500	AR1242ICC500	02/20/2025	19:31	PO109435.D	8.71	3.69
AR1242ICC250	AR1242ICC250	02/20/2025	19:50	PO109436.D	8.71	3.69
AR1242ICC050	AR1242ICC050	02/20/2025	20:08	PO109437.D	8.71	3.69
AR1248ICC1000	AR1248ICC1000	02/20/2025	20:26	PO109438.D	8.71	3.69
AR1248ICC750	AR1248ICC750	02/20/2025	20:45	PO109439.D	8.71	3.69
AR1248ICC500	AR1248ICC500	02/20/2025	21:03	PO109440.D	8.71	3.69
AR1248ICC250	AR1248ICC250	02/20/2025	21:21	PO109441.D	8.71	3.69
AR1248ICC050	AR1248ICC050	02/20/2025	21:40	PO109442.D	8.71	3.69
AR1254ICC1000	AR1254ICC1000	02/20/2025	21:58	PO109443.D	8.71	3.69
AR1254ICC750	AR1254ICC750	02/20/2025	22:17	PO109444.D	8.71	3.69
AR1254ICC500	AR1254ICC500	02/20/2025	22:35	PO109445.D	8.71	3.69
AR1254ICC250	AR1254ICC250	02/20/2025	22:53	PO109446.D	8.71	3.69
AR1254ICC050	AR1254ICC050	02/20/2025	23:12	PO109447.D	8.71	3.69
AR1262ICC500	AR1262ICC500	02/20/2025	23:30	PO109448.D	8.71	3.69
AR1268ICC1000	AR1268ICC1000	02/20/2025	23:48	PO109449.D	8.71	3.69
AR1268ICC750	AR1268ICC750	02/21/2025	00:07	PO109450.D	8.71	3.69
AR1268ICC500	AR1268ICC500	02/21/2025	00:25	PO109451.D	8.71	3.69
AR1268ICC250	AR1268ICC250	02/21/2025	00:43	PO109452.D	8.71	3.69
AR1268ICC050	AR1268ICC050	02/21/2025	01:02	PO109453.D	8.70	3.69
AR1660CCC500	AR1660CCC500	03/10/2025	14:18	PO109755.D	8.70	3.69
IBLK	IBLK	03/10/2025	15:31	PO109759.D	8.70	3.69
PB167042BL	PB167042BL	03/10/2025	15:49	PO109760.D	8.70	3.69
PB167042BS	PB167042BS	03/10/2025	16:07	PO109761.D	8.70	3.69
PB167042BSD	PB167042BSD	03/10/2025	16:26	PO109762.D	8.70	3.69
TW-WTS-04	Q1522-02	03/10/2025	17:03	PO109764.D	8.70	3.69
AR1660CCC500	AR1660CCC500	03/10/2025	19:03	PO109769.D	8.70	3.69
IBLK	IBLK	03/10/2025	20:15	PO109773.D	8.70	3.69

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB167042BS

Contract: ENTA05

Lab Code: CHEM Case No.: Q1522 SAS No.: Q1522 SDG NO.: Q1522

Lab Sample ID: PB167042BS Date(s) Analyzed: 03/10/2025 03/10/2025

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO109761.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.789	4.739	4.839	4.34	4.30	6.74
COLUMN 1	2	4.808	4.758	4.858	4.34		
	3	4.864	4.814	4.914	4.33		
	4	4.985	4.935	5.035	4.32		
	5	5.242	5.192	5.292	4.10		
	1	4.775	4.725	4.825	4.65		
COLUMN 2	2	4.794	4.744	4.844	4.67	4.60	
	3	4.97	4.92	5.02	4.68		
	4	5.012	4.962	5.062	4.49		
	5	5.225	5.175	5.275	4.35		
Aroclor-1260	1	6.284	6.234	6.334	4.30	4.00	9.52
COLUMN 1	2	6.473	6.423	6.523	4.29		
	3	6.841	6.791	6.891	3.73		
	4	7.101	7.051	7.151	3.82		
	5	7.343	7.293	7.393	3.82		
	1	6.257	6.207	6.307	4.58		
COLUMN 2	2	6.445	6.395	6.495	4.57	4.40	
	3	6.598	6.548	6.648	4.59		
	4	7.069	7.019	7.119	3.98		
	5	7.311	7.261	7.361	4.04		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB167042BSD

Contract: ENTA05

Lab Code: CHEM

Case No.: Q1522

SAS No.: Q1522

SDG NO.: Q1522

Lab Sample ID: PB167042BSD

Date(s) Analyzed: 03/10/2025

03/10/2025

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm)

GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO109762.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD	
			FROM	TO				
Aroclor-1016	1	4.788	4.738	4.838	4.37	4.30	6.74	
	2	4.808	4.758	4.858	4.39			
	3	4.864	4.814	4.914	4.36			
	4	4.984	4.934	5.034	4.37			
	5	5.242	5.192	5.292	4.14			
COLUMN 1								
	1	4.775	4.725	4.825	4.64	4.60		
	2	4.794	4.744	4.844	4.73			
	3	4.97	4.92	5.02	4.71			
	4	5.011	4.961	5.061	4.50			
5	5.225	5.175	5.275	4.40				
COLUMN 2								
	1	6.283	6.233	6.333	4.36	4.00	9.52	
	2	6.472	6.422	6.522	4.35			
	3	6.84	6.79	6.89	3.75			
	4	7.101	7.051	7.151	3.85			
5	7.343	7.293	7.393	3.87				
COLUMN 1								
	1	6.257	6.207	6.307	4.62	4.40		
	2	6.445	6.395	6.495	4.64			
	3	6.598	6.548	6.648	4.63			
	4	7.07	7.02	7.12	4.02			
5	7.31	7.26	7.36	4.08				
COLUMN 2								



QC SAMPLE DATA

Report of Analysis

Client:	ENTACT	Date Collected:	
Project:	540 Degraw St, Brooklyn, NY - E9309	Date Received:	
Client Sample ID:	PB167042BL	SDG No.:	Q1522
Lab Sample ID:	PB167042BL	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0 Decanted:
Sample Wt/Vol:	1000 Units: mL	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	3510C		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109760.D	1	03/10/25 08:48	03/10/25 15:49	PB167042

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.3		30 (16) - 150 (158)	97%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.4		30 (10) - 150 (173)	92%	SPK: 20

Comments:

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 E = Value Exceeds Calibration Range
 P = Indicates >25% difference for detected concentrations between the two GC columns
 Q = indicates LCS control criteria did not meet requirements
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 N = Presumptive Evidence of a Compound
 * = Values outside of QC limits
 D = Dilution
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031025\
 Data File : P0109760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2025 15:49
 Operator : YP/AJ
 Sample : PB167042BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB167042BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 00:57:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.695	3.693	174.9E6	101.2E6	18.473	19.332
2) SA Decachlor...	8.750	8.702	143.7E6	58573061	16.708	18.395

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031025\
Data File : PO109760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2025 15:49
Operator : YP/AJ
Sample : PB167042BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB167042BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 00:57:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

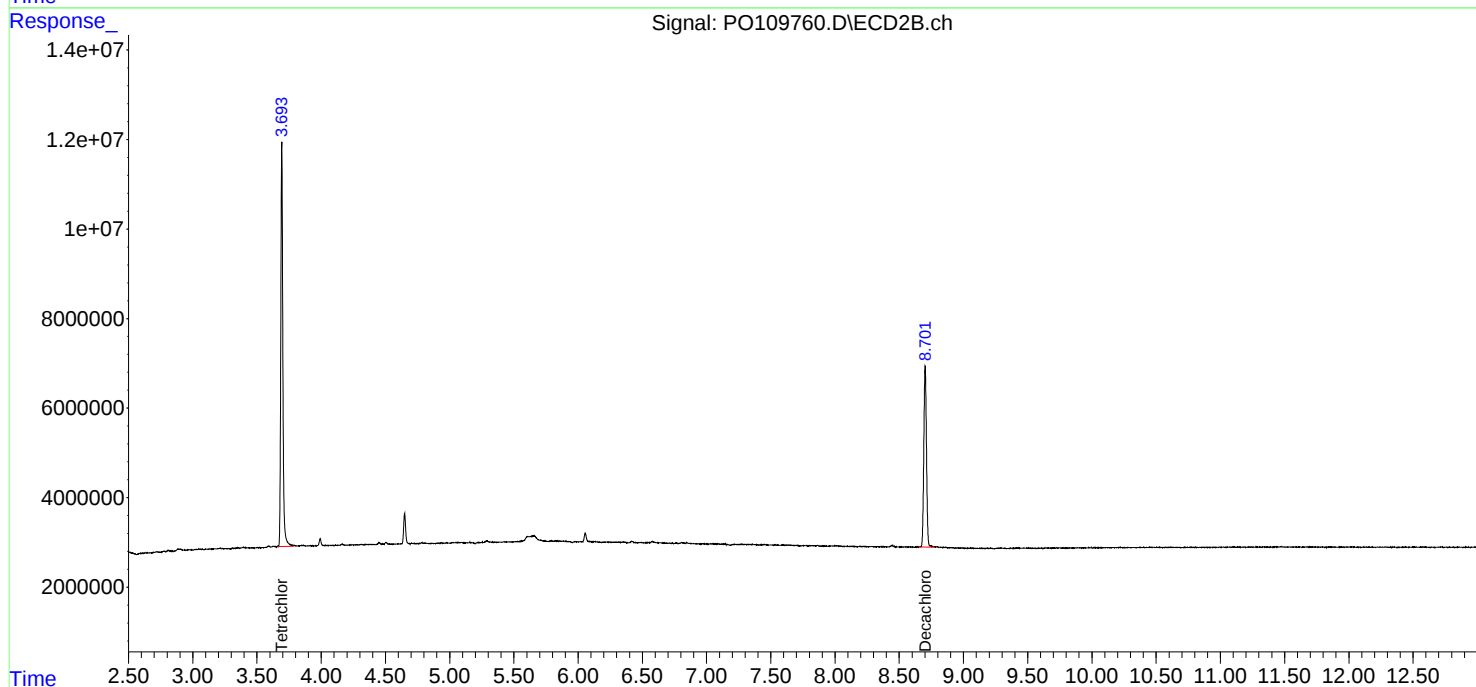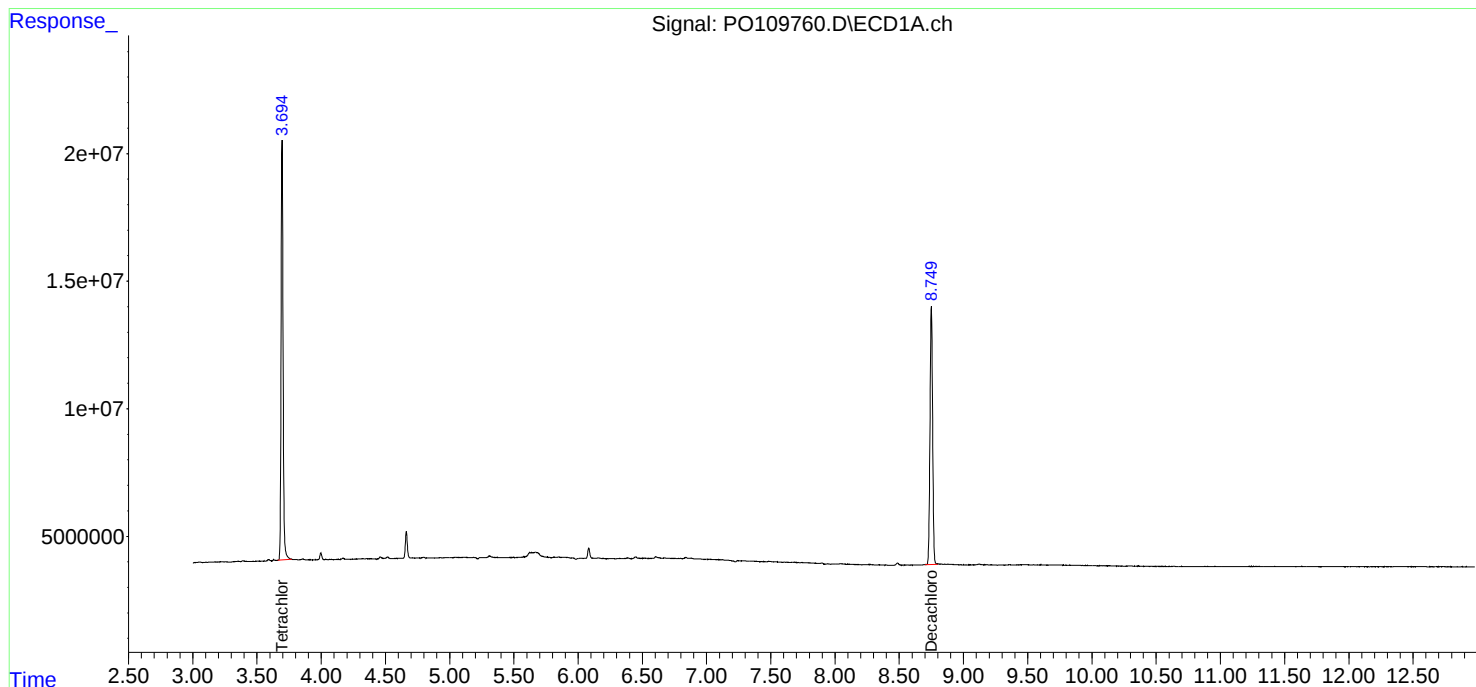


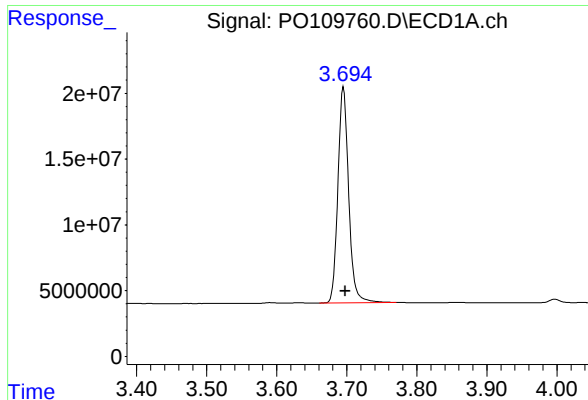

#1 Tetrachloro-m-xylene


R.T.: 3.695 min
Delta R.T.: -0.003 min
Response: 174852252
Conc: 18.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB167042BL

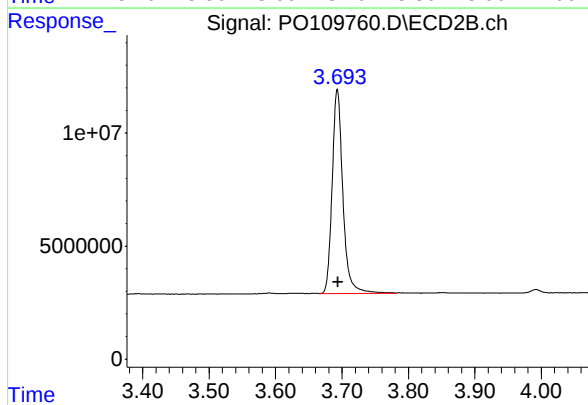


#1 Tetrachloro-m-xylene

R.T.: 3.693 min
Delta R.T.: 0.000 min
Response: 101188520
Conc: 19.33 ng/ml

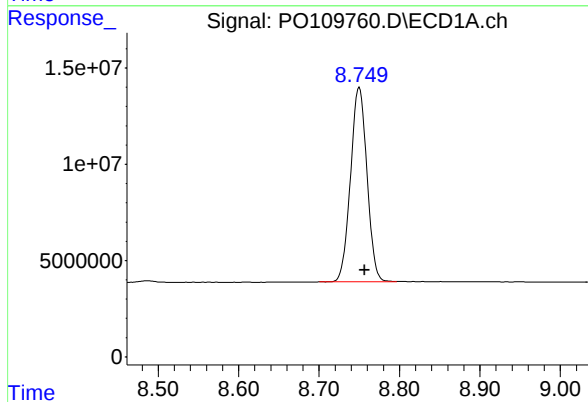

#2 Decachlorobiphenyl

R.T.: 8.750 min
Delta R.T.: -0.007 min
Response: 143719099
Conc: 16.71 ng/ml

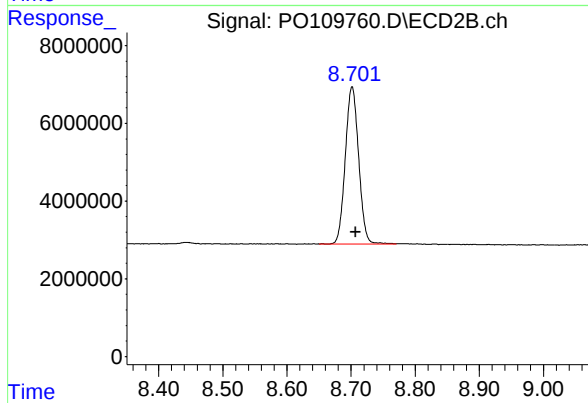

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.005 min
Response: 58573061
Conc: 18.39 ng/ml

Report of Analysis

Client:	ENTACT	Date Collected:	02/20/25
Project:	540 Degraw St, Brooklyn, NY - E9309	Date Received:	02/20/25
Client Sample ID:	PIBLK-PO109425.D	SDG No.:	Q1522
Lab Sample ID:	I.BLK-PO109425.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109425.D	1		02/20/25	PO022025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	24.1		70 (60) - 130 (140)	121%	SPK: 20
2051-24-3	Decachlorobiphenyl	25.3		70 (60) - 130 (140)	126%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 16:28
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:42:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	239.0E6	126.2E6	25.246	24.105
2) SA Decachlor...	8.755	8.707	217.3E6	81112838	25.266	25.473

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 16:28
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:42:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

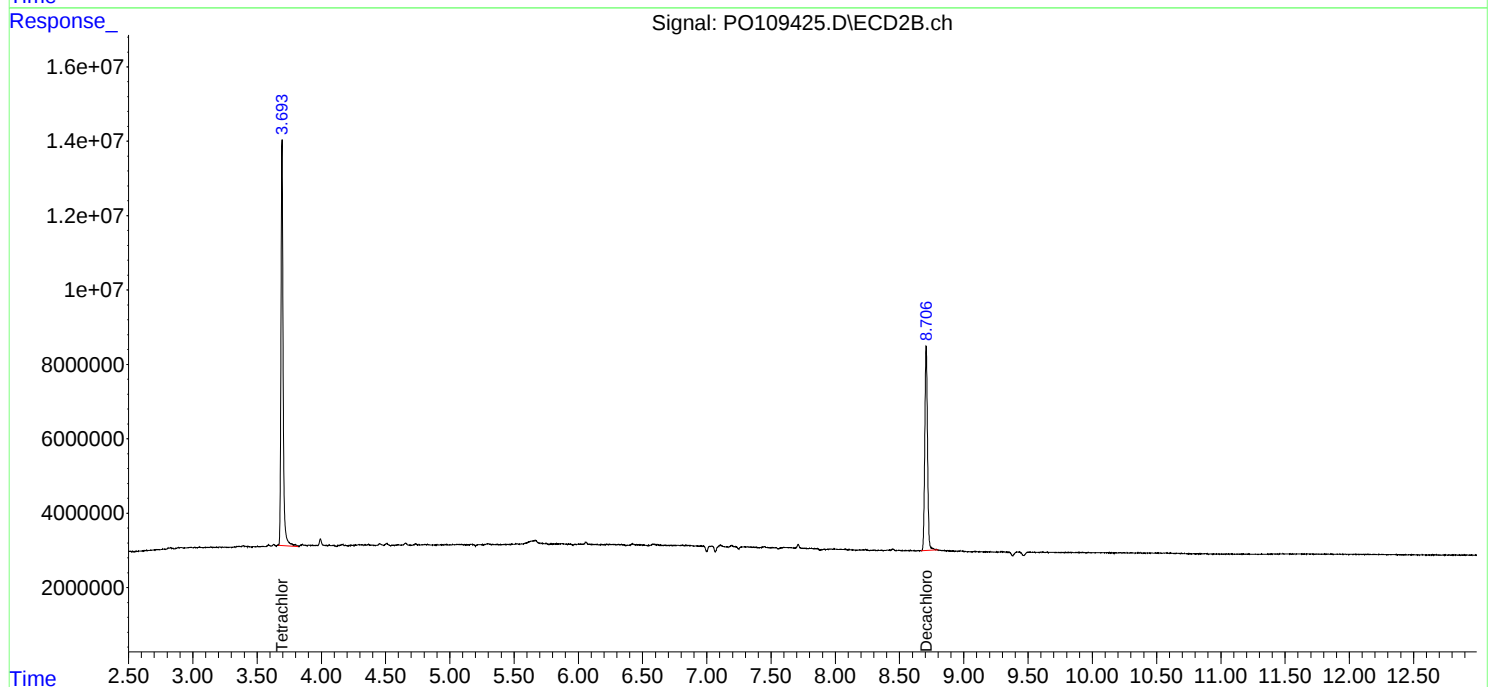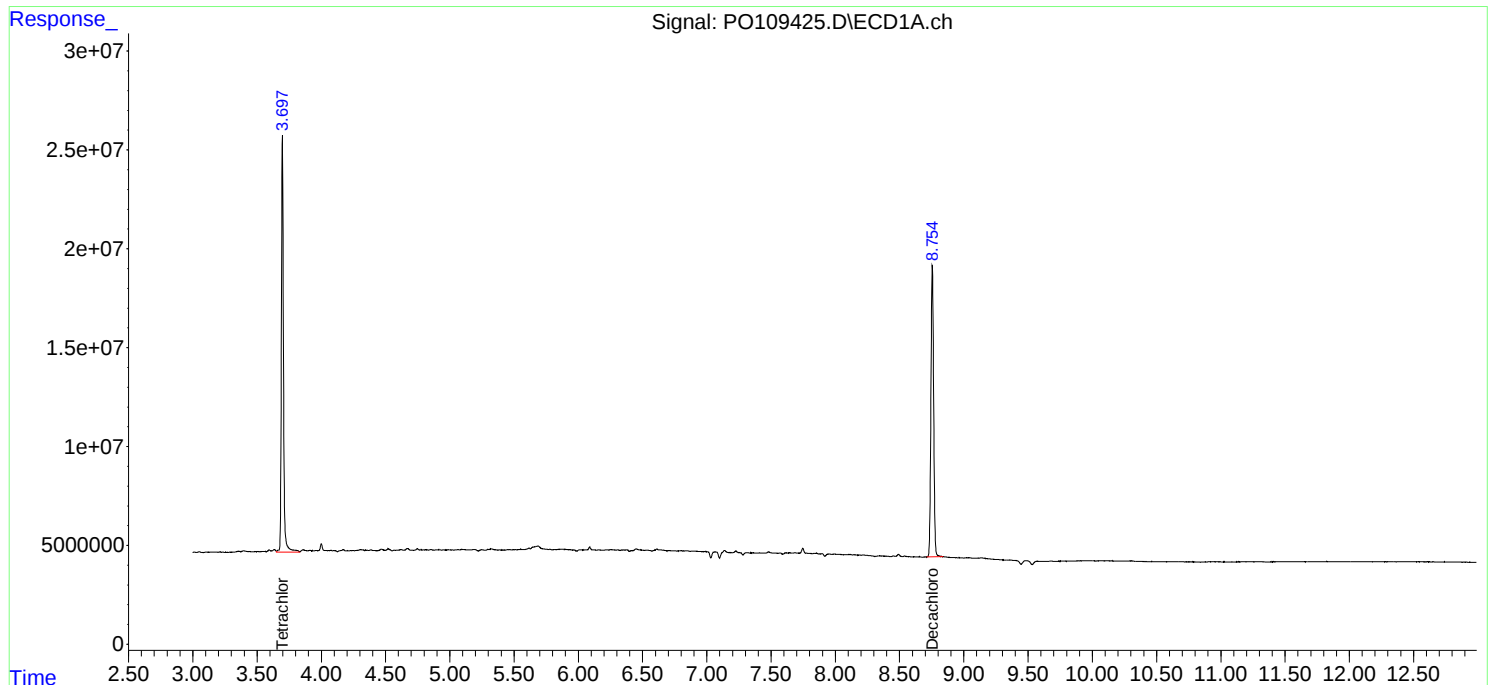


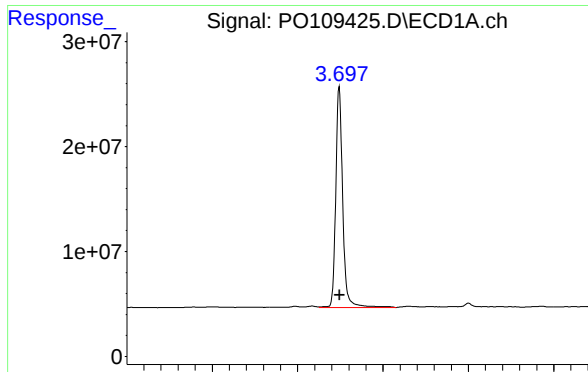

#1 Tetrachloro-m-xylene


R.T.: 3.697 min
Delta R.T.: 0.000 min
Response: 238952889
Conc: 25.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

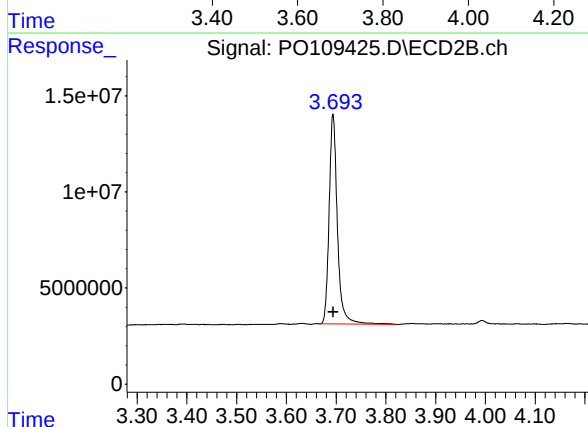


#1 Tetrachloro-m-xylene

R.T.: 3.694 min
Delta R.T.: 0.000 min
Response: 126170966
Conc: 24.11 ng/ml

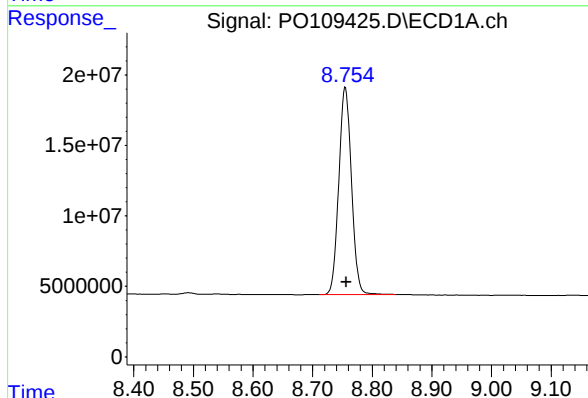

#2 Decachlorobiphenyl

R.T.: 8.755 min
Delta R.T.: -0.002 min
Response: 217333363
Conc: 25.27 ng/ml

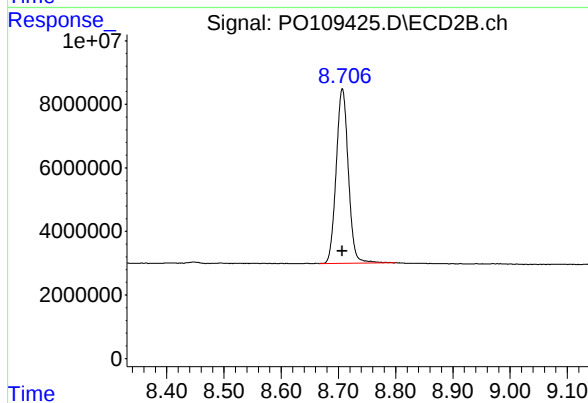

#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: 0.000 min
Response: 81112838
Conc: 25.47 ng/ml

Report of Analysis

Client:	ENTACT	Date Collected:	03/10/25
Project:	540 Degraw St, Brooklyn, NY - E9309	Date Received:	03/10/25
Client Sample ID:	PIBLK-PO109759.D	SDG No.:	Q1522
Lab Sample ID:	I.BLK-PO109759.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109759.D	1		03/10/25	PO031025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.1		70 (60) - 130 (140)	95%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.1		70 (60) - 130 (140)	86%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031025\
 Data File : P0109759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2025 15:31
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 00:57:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.693	3.692	180.3E6	106.9E6	19.046	20.427
2) SA Decachlor...	8.749	8.701	147.5E6	60470440	17.153	18.990

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031025\
Data File : PO109759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2025 15:31
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 00:57:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

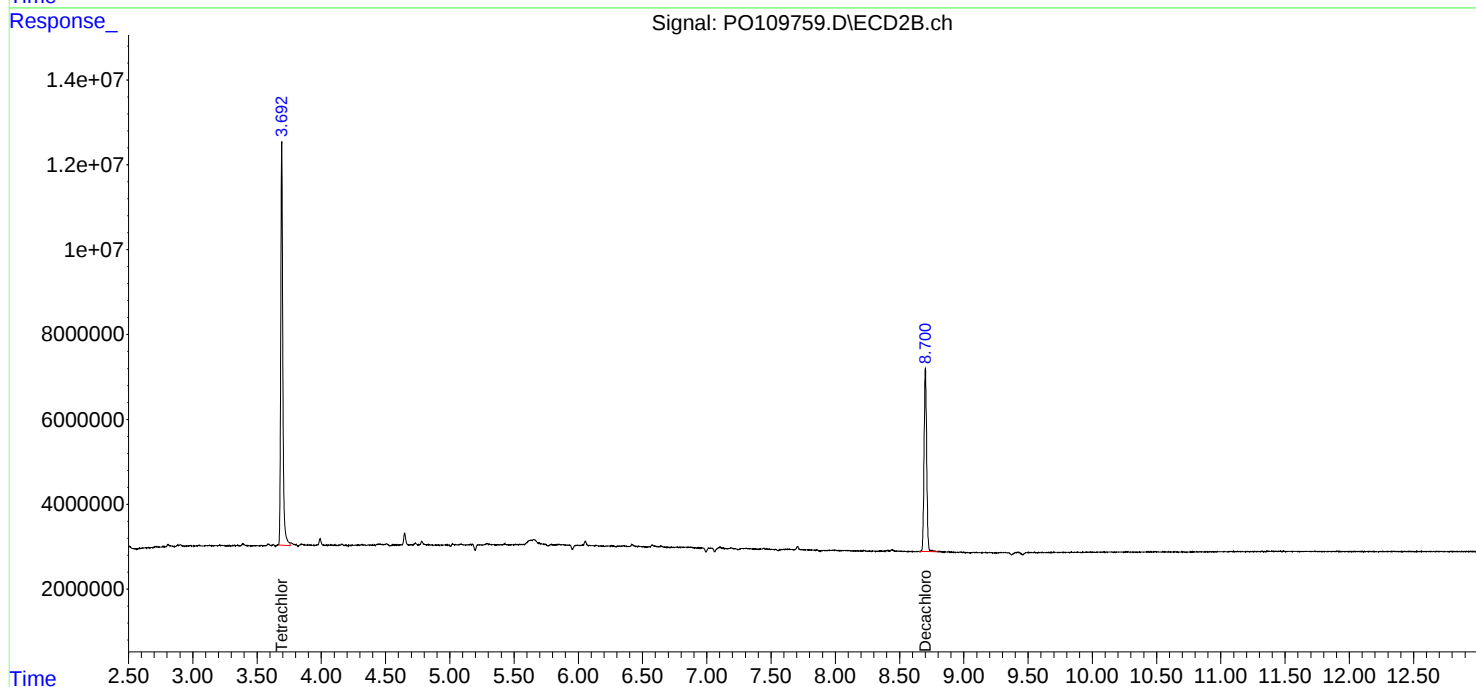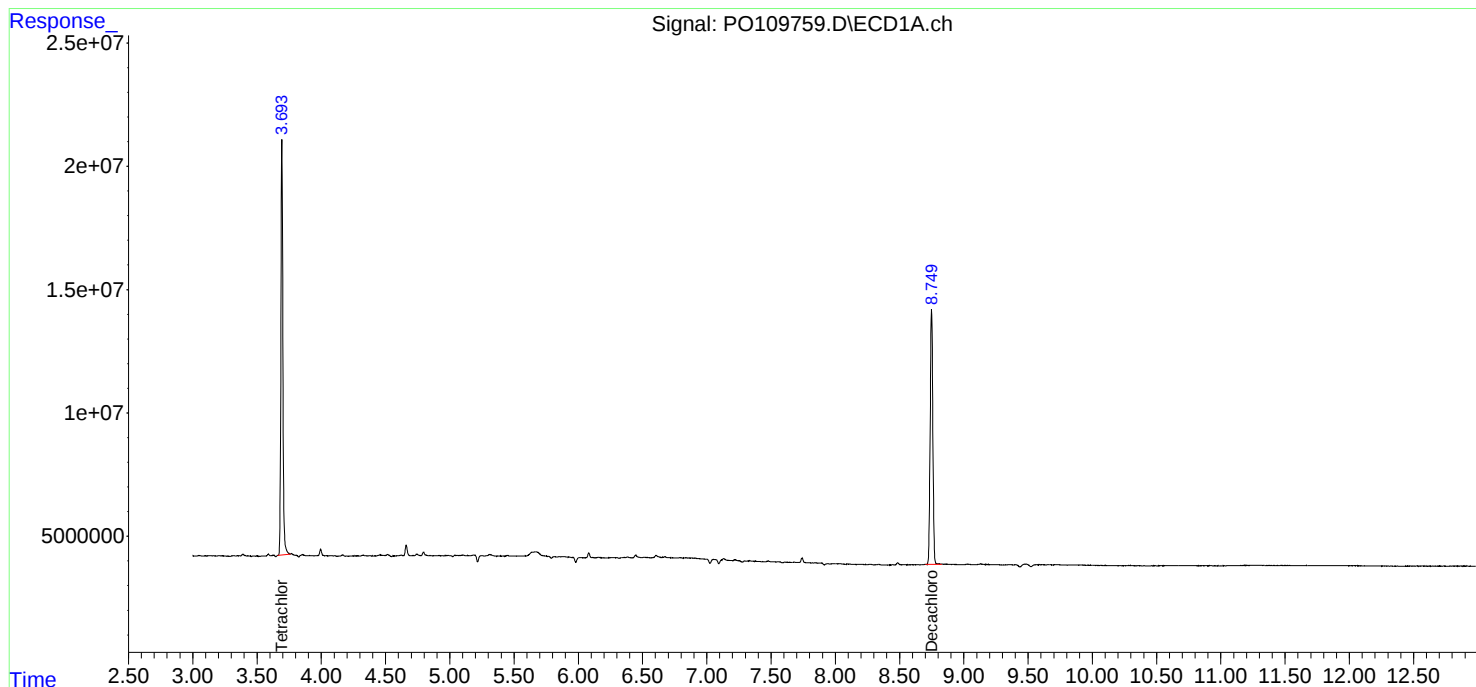


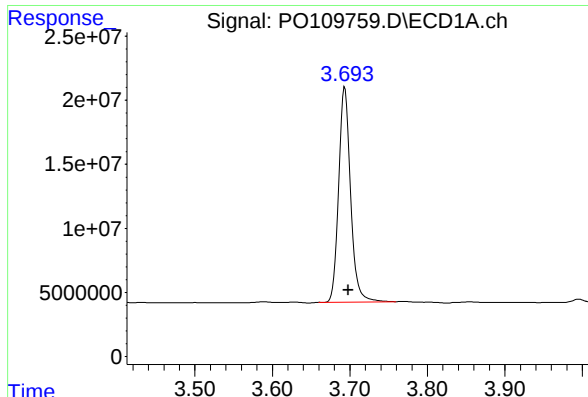

#1 Tetrachloro-m-xylene


R.T.: 3.693 min
Delta R.T.: -0.005 min
Response: 180276959
Conc: 19.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

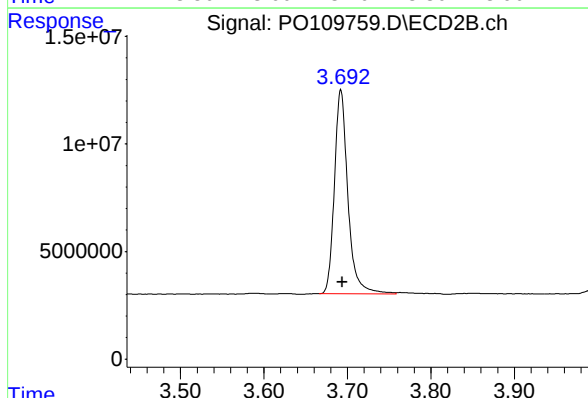


#1 Tetrachloro-m-xylene

R.T.: 3.692 min
Delta R.T.: -0.002 min
Response: 106919447
Conc: 20.43 ng/ml

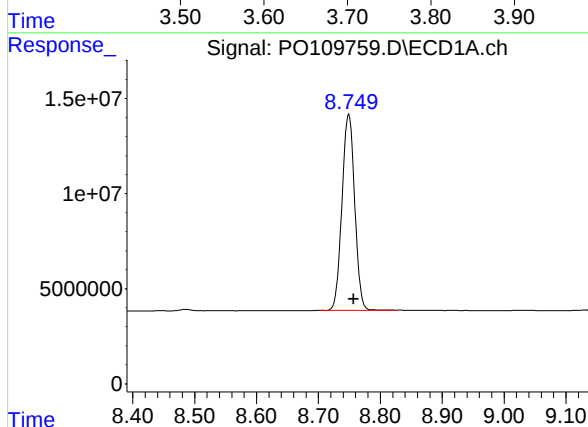

#2 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: -0.008 min
Response: 147545353
Conc: 17.15 ng/ml

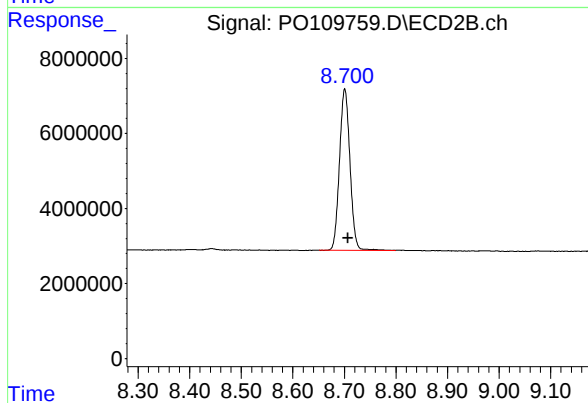

#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: -0.006 min
Response: 60470440
Conc: 18.99 ng/ml

Report of Analysis

Client:	ENTACT	Date Collected:	03/10/25
Project:	540 Degraw St, Brooklyn, NY - E9309	Date Received:	03/10/25
Client Sample ID:	PIBLK-PO109773.D	SDG No.:	Q1522
Lab Sample ID:	I.BLK-PO109773.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109773.D	1		03/10/25	PO031025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.4		70 (60) - 130 (140)	97%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.2		70 (60) - 130 (140)	86%	SPK: 20

Comments:

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 E = Value Exceeds Calibration Range
 P = Indicates >25% difference for detected concentrations between the two GC columns
 Q = indicates LCS control criteria did not meet requirements
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 N = Presumptive Evidence of a Compound
 * = Values outside of QC limits
 D = Dilution
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031025\
 Data File : PO109773.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2025 20:15
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 01:02:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.695	3.692	184.0E6	107.9E6	19.442	20.610
2) SA Decachlor...	8.750	8.701	147.8E6	59111687	17.183	18.564

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031025\
Data File : PO109773.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2025 20:15
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 01:02:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

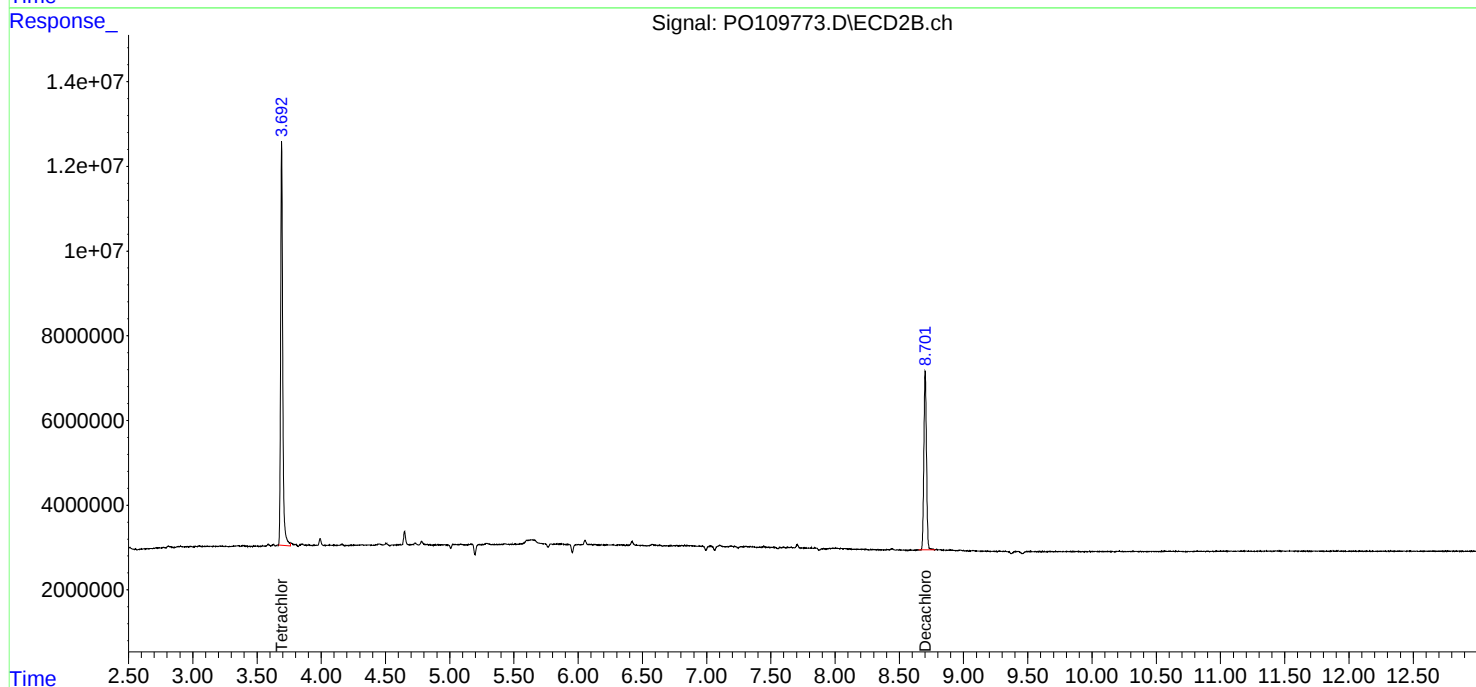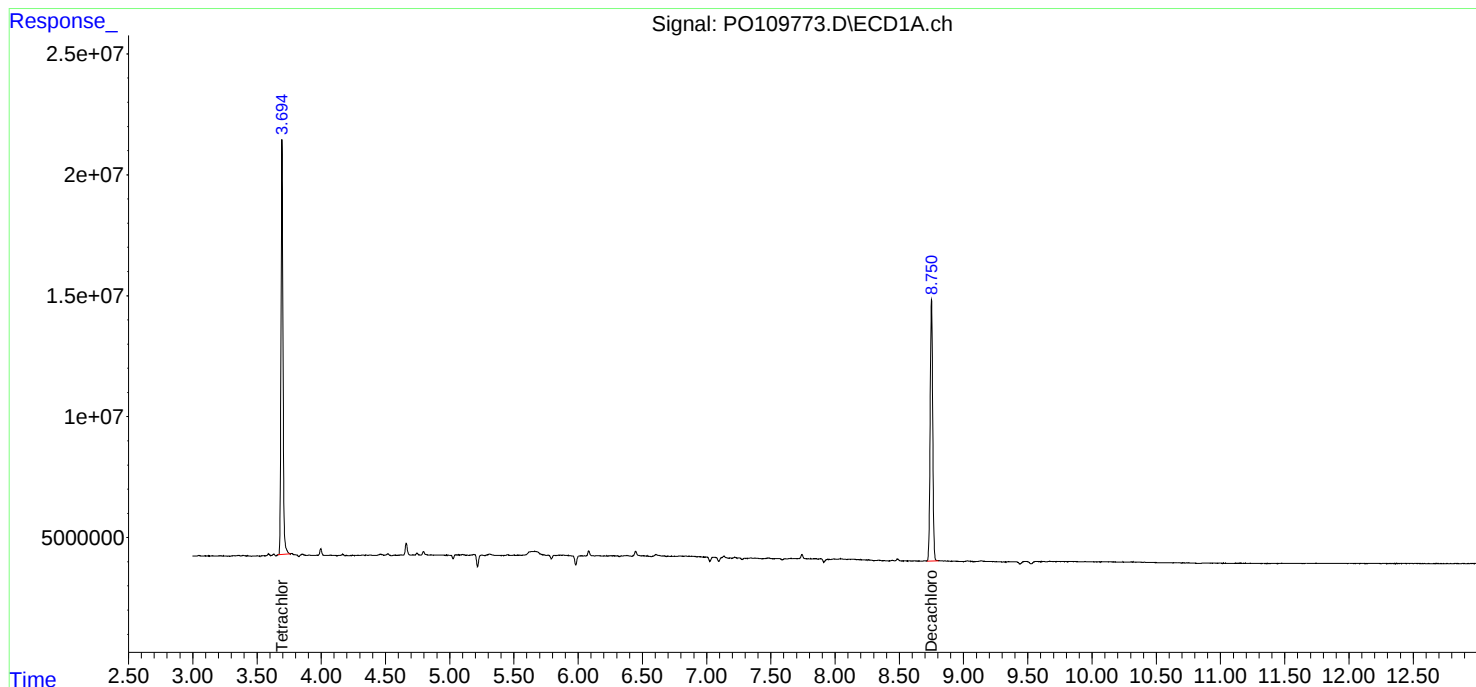


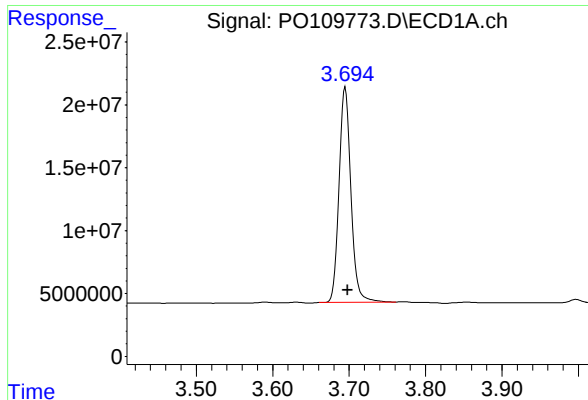

#1 Tetrachloro-m-xylene


R.T.: 3.695 min
Delta R.T.: -0.003 min
Response: 184016227
Conc: 19.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

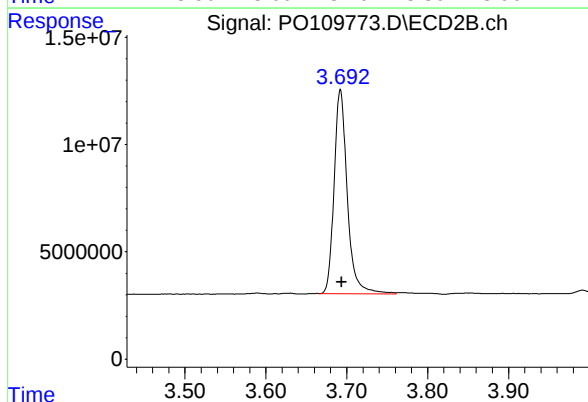


#1 Tetrachloro-m-xylene

R.T.: 3.692 min
Delta R.T.: -0.002 min
Response: 107878206
Conc: 20.61 ng/ml

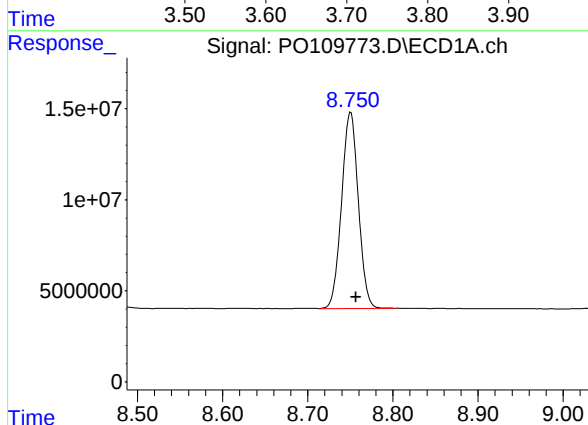

#2 Decachlorobiphenyl

R.T.: 8.750 min
Delta R.T.: -0.006 min
Response: 147807675
Conc: 17.18 ng/ml

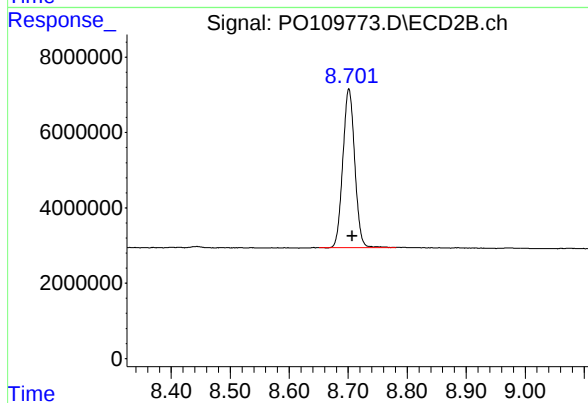

#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: -0.006 min
Response: 59111687
Conc: 18.56 ng/ml

Report of Analysis

Client:	ENTACT	Date Collected:	
Project:	540 Degraw St, Brooklyn, NY - E9309	Date Received:	
Client Sample ID:	PB167042BS	SDG No.:	Q1522
Lab Sample ID:	PB167042BS	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0 Decanted:
Sample Wt/Vol:	1000 Units: mL	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	3510C		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109761.D	1	03/10/25 08:48	03/10/25 16:07	PB167042

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	4.60		0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
11096-82-5	Aroclor-1260	4.40		0.15	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	18.6		30 (16) - 150 (158)	93%	SPK: 20
2051-24-3	Decachlorobiphenyl	19.0		30 (10) - 150 (173)	95%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031025\
 Data File : P0109761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2025 16:07
 Operator : YP/AJ
 Sample : PB167042BS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB167042BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 00:58:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.695	3.693	170.0E6	97565927	17.957	18.640
2) SA Decachlor...	8.750	8.701	149.3E6	60399624	17.352	18.968
Target Compounds						
3) L1 AR-1016-1	4.789	4.775	133.8E6	72546600	434.086	464.534
4) L1 AR-1016-2	4.808	4.794	182.6E6	101.1E6	433.700	467.032
5) L1 AR-1016-3	4.864	4.970	128.0E6	55850250	432.615	467.557
6) L1 AR-1016-4	4.985	5.012	100.1E6	46683917	431.943	448.579
7) L1 AR-1016-5	5.242	5.225	105.9E6	59233276	410.127	434.728
31) L7 AR-1260-1	6.284	6.257	200.4E6	108.6E6	429.991	458.183
32) L7 AR-1260-2	6.473	6.445	242.7E6	125.7E6	429.446	456.896
33) L7 AR-1260-3	6.841	6.598	177.3E6	117.2E6	372.793	459.469
34) L7 AR-1260-4	7.101	7.069	165.1E6	81995583	382.475	397.666
35) L7 AR-1260-5	7.343	7.311	379.4E6	181.0E6	381.786	404.190



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031025\
Data File : PO109761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2025 16:07
Operator : YP/AJ
Sample : PB167042BS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB167042BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 00:58:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

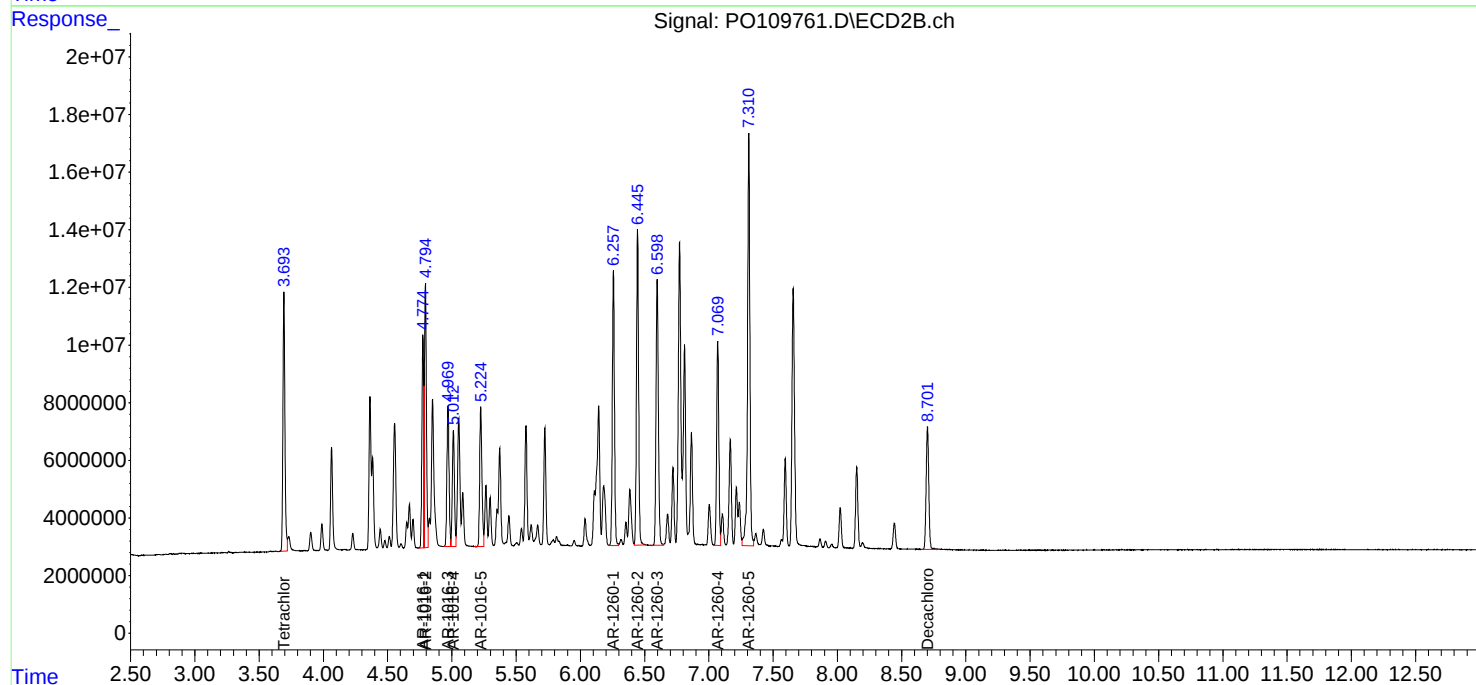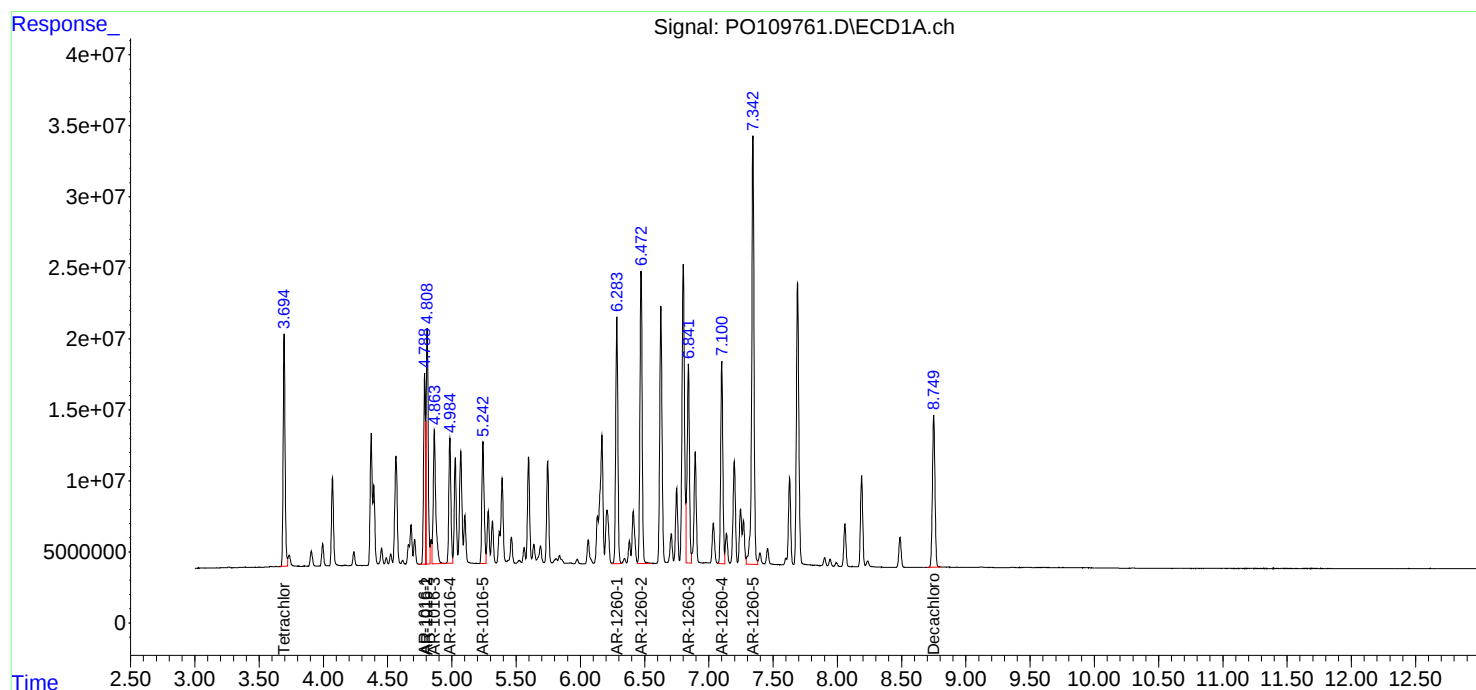

Report of Analysis

Client:	ENTACT	Date Collected:	
Project:	540 Degraw St, Brooklyn, NY - E9309	Date Received:	
Client Sample ID:	PB167042BSD	SDG No.:	Q1522
Lab Sample ID:	PB167042BSD	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0 Decanted:
Sample Wt/Vol:	1000 Units: mL	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	3510C		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109762.D	1	03/10/25 08:48	03/10/25 16:26	PB167042

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	4.60		0.15	0.50	ug/L
11104-28-2	Aroclor-1221	0.23	U	0.23	0.50	ug/L
11141-16-5	Aroclor-1232	0.37	U	0.37	0.50	ug/L
53469-21-9	Aroclor-1242	0.16	U	0.16	0.50	ug/L
12672-29-6	Aroclor-1248	0.12	U	0.12	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.12	U	0.12	0.50	ug/L
11096-82-5	Aroclor-1260	4.40		0.15	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	18.9		30 (16) - 150 (158)	94%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.9		30 (10) - 150 (173)	94%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031025\
 Data File : P0109762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2025 16:26
 Operator : YP/AJ
 Sample : PB167042BSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB167042BSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 00:58:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.695	3.693	172.1E6	98725980	18.182	18.862
2) SA Decachlor...	8.749	8.702	150.5E6	60135723	17.494	18.885
Target Compounds						
3) L1 AR-1016-1	4.788	4.775	134.7E6	72537290	436.766	464.475
4) L1 AR-1016-2	4.808	4.794	184.8E6	102.3E6	438.958	472.693
5) L1 AR-1016-3	4.864	4.970	129.1E6	56202727	436.487	470.508
6) L1 AR-1016-4	4.984	5.011	101.2E6	46871927	436.796	450.386
7) L1 AR-1016-5	5.242	5.225	106.9E6	59997421	413.997	440.337
31) L7 AR-1260-1	6.283	6.257	203.3E6	109.4E6	436.058	461.813
32) L7 AR-1260-2	6.472	6.445	245.9E6	127.8E6	435.098	464.486
33) L7 AR-1260-3	6.840	6.598	178.3E6	118.0E6	374.871	462.724
34) L7 AR-1260-4	7.101	7.070	166.1E6	82790006	384.852	401.519
35) L7 AR-1260-5	7.343	7.310	384.9E6	182.8E6	387.240	408.333



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031025\
Data File : PO109762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2025 16:26
Operator : YP/AJ
Sample : PB167042BSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB167042BSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 00:58:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

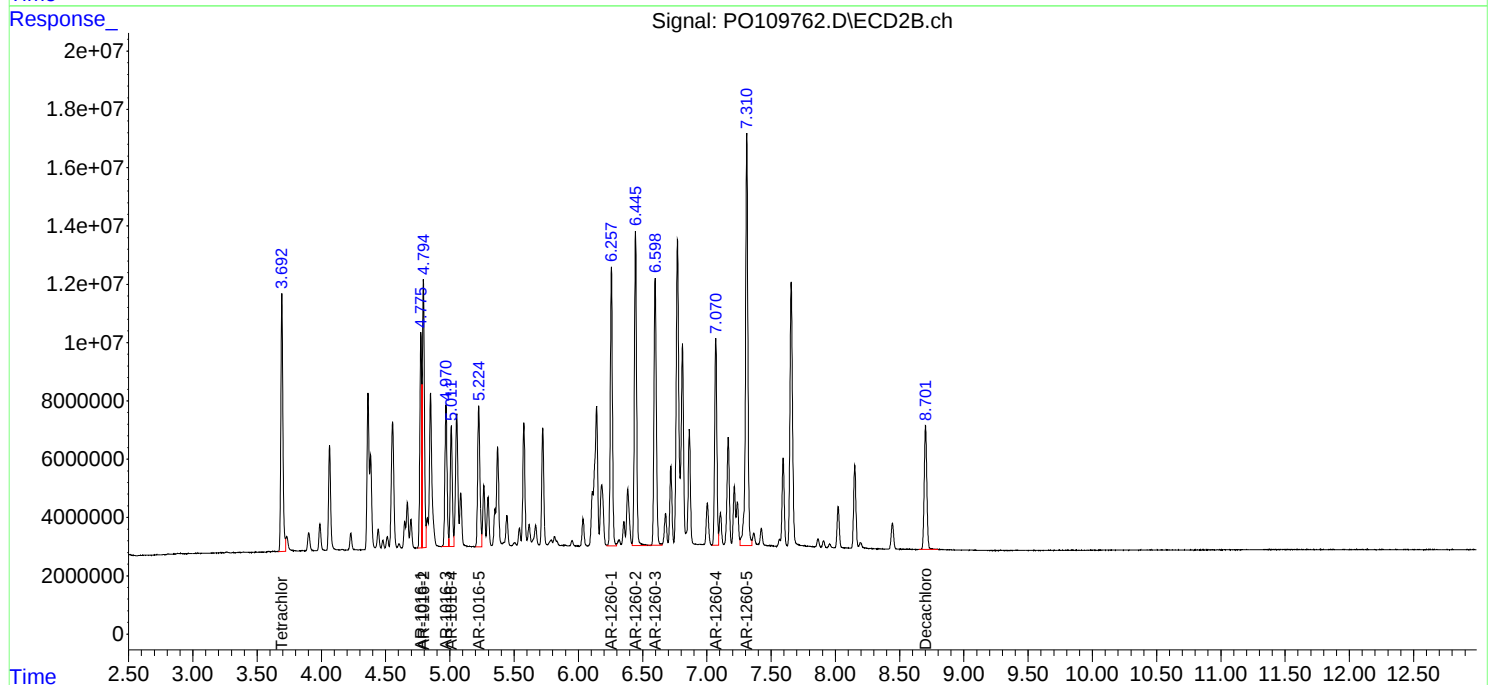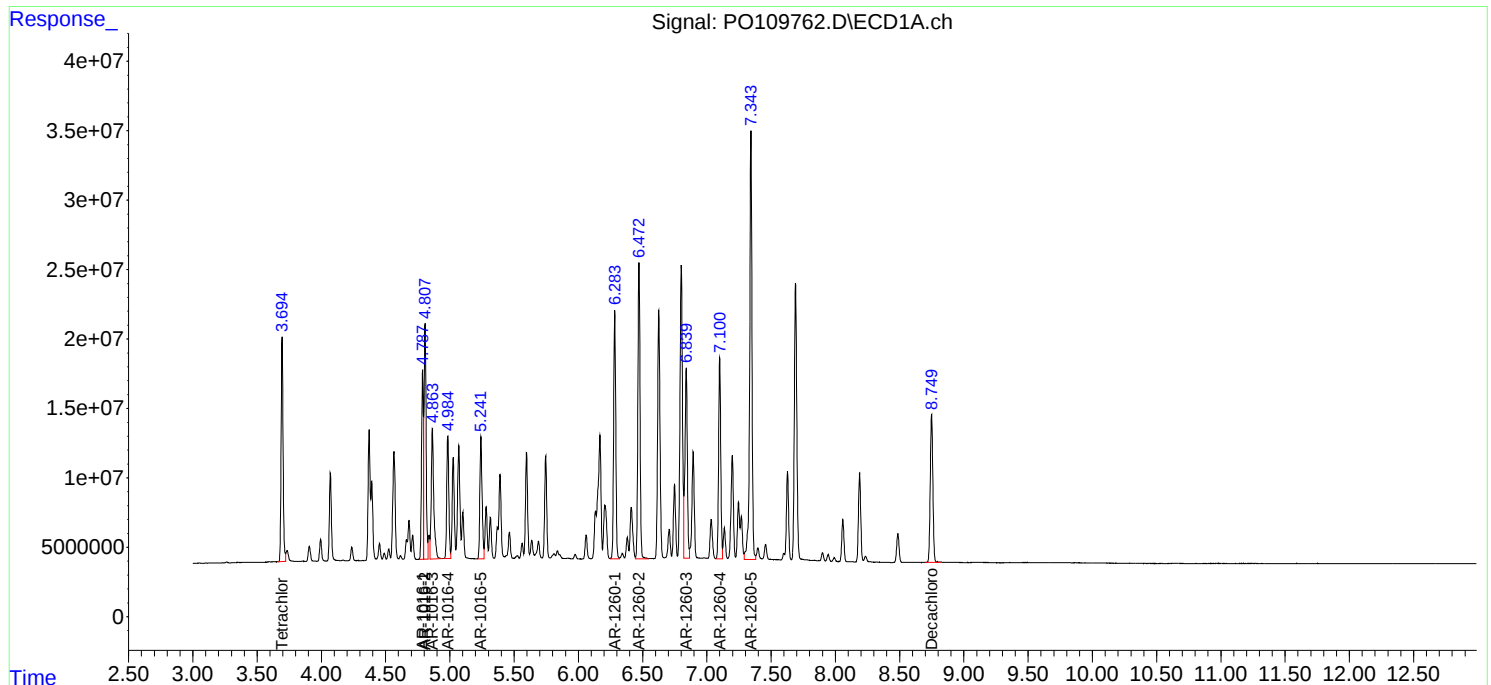

Manual Integration Report

Sequence:

PO022025

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1242ICC050	PO109437.D	AR-1242-5	yogesh	2/21/2025 8:09:35 AM	Ankita	2/21/2025 9:30:25	Peak Integrated by Software
AR1242ICC050	PO109437.D	AR-1242-5 #2	yogesh	2/21/2025 8:09:35 AM	Ankita	2/21/2025 9:30:25	Peak Integrated by Software
AR1248ICC050	PO109442.D	AR-1248-4	yogesh	2/21/2025 8:09:37 AM	Ankita	2/21/2025 9:30:26	Peak Integrated by Software
AR1248ICC050	PO109442.D	AR-1248-4 #2	yogesh	2/21/2025 8:09:37 AM	Ankita	2/21/2025 9:30:26	Peak Integrated by Software
AR1248ICC050	PO109442.D	AR-1248-5	yogesh	2/21/2025 8:09:37 AM	Ankita	2/21/2025 9:30:26	Peak Integrated by Software
AR1248ICC050	PO109442.D	AR-1248-5 #2	yogesh	2/21/2025 8:09:37 AM	Ankita	2/21/2025 9:30:26	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-1	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-1 #2	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-2	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-2 #2	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-3	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-3 #2	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-4	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software

Manual Integration Report

Sequence:

PO022025

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1254ICC050	PO109447.D	AR-1254-4 #2	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	Tetrachloro-m-xylene	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:

PO031025

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1254CCC500	PO109772.D	AR-1254-5	yogesh	3/11/2025 8:31:39 AM	Ankita	3/11/2025 8:52:51	Peak Integrated by Software

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO022025

Review By	yogesh	Review On	2/21/2025 8:09:53 AM
Supervise By	Ankita	Supervise On	2/21/2025 9:30:37 AM
SubDirectory	PO022025	HP Acquire Method	HP Processing Method PO022025
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO109424.D	20 Feb 2025 16:09	YP/AJ	Ok
2	I.BLK	PO109425.D	20 Feb 2025 16:28	YP/AJ	Ok
3	AR1660ICC1000	PO109426.D	20 Feb 2025 16:46	YP/AJ	Ok
4	AR1660ICC750	PO109427.D	20 Feb 2025 17:04	YP/AJ	Ok
5	AR1660ICC500	PO109428.D	20 Feb 2025 17:23	YP/AJ	Ok
6	AR1660ICC250	PO109429.D	20 Feb 2025 17:41	YP/AJ	Ok
7	AR1660ICC050	PO109430.D	20 Feb 2025 17:59	YP/AJ	Ok
8	AR1221ICC500	PO109431.D	20 Feb 2025 18:18	YP/AJ	Ok
9	AR1232ICC500	PO109432.D	20 Feb 2025 18:36	YP/AJ	Ok
10	AR1242ICC1000	PO109433.D	20 Feb 2025 18:55	YP/AJ	Ok
11	AR1242ICC750	PO109434.D	20 Feb 2025 19:13	YP/AJ	Ok
12	AR1242ICC500	PO109435.D	20 Feb 2025 19:31	YP/AJ	Ok
13	AR1242ICC250	PO109436.D	20 Feb 2025 19:50	YP/AJ	Ok
14	AR1242ICC050	PO109437.D	20 Feb 2025 20:08	YP/AJ	Ok,M
15	AR1248ICC1000	PO109438.D	20 Feb 2025 20:26	YP/AJ	Ok
16	AR1248ICC750	PO109439.D	20 Feb 2025 20:45	YP/AJ	Ok
17	AR1248ICC500	PO109440.D	20 Feb 2025 21:03	YP/AJ	Ok
18	AR1248ICC250	PO109441.D	20 Feb 2025 21:21	YP/AJ	Ok
19	AR1248ICC050	PO109442.D	20 Feb 2025 21:40	YP/AJ	Ok,M
20	AR1254ICC1000	PO109443.D	20 Feb 2025 21:58	YP/AJ	Ok
21	AR1254ICC750	PO109444.D	20 Feb 2025 22:17	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO022025

Review By	yogesh	Review On	2/21/2025 8:09:53 AM
Supervise By	Ankita	Supervise On	2/21/2025 9:30:37 AM
SubDirectory	PO022025	HP Acquire Method	HP Processing Method PO022025
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	AR1254ICC500	PO109445.D	20 Feb 2025 22:35	YP/AJ	Ok
23	AR1254ICC250	PO109446.D	20 Feb 2025 22:53	YP/AJ	Ok
24	AR1254ICC050	PO109447.D	20 Feb 2025 23:12	YP/AJ	Ok,M
25	AR1262ICC500	PO109448.D	20 Feb 2025 23:30	YP/AJ	Ok
26	AR1268ICC1000	PO109449.D	20 Feb 2025 23:48	YP/AJ	Ok
27	AR1268ICC750	PO109450.D	21 Feb 2025 00:07	YP/AJ	Ok
28	AR1268ICC500	PO109451.D	21 Feb 2025 00:25	YP/AJ	Ok
29	AR1268ICC250	PO109452.D	21 Feb 2025 00:43	YP/AJ	Ok
30	AR1268ICC050	PO109453.D	21 Feb 2025 01:02	YP/AJ	Ok
31	PO022025ICV500	PO109454.D	21 Feb 2025 01:20	YP/AJ	Ok
32	AR1242ICV500	PO109455.D	21 Feb 2025 01:38	YP/AJ	Ok
33	AR1248ICV500	PO109456.D	21 Feb 2025 01:57	YP/AJ	Ok
34	AR1254ICV500	PO109457.D	21 Feb 2025 02:15	YP/AJ	Ok
35	AR1268ICV500	PO109458.D	21 Feb 2025 02:34	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031025

Review By	yogesh	Review On	3/11/2025 8:31:51 AM
Supervise By	Ankita	Supervise On	3/11/2025 8:52:58 AM
SubDirectory	PO031025	HP Acquire Method	HP Processing Method PO022025
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO109742.D	10 Mar 2025 09:52	YP/AJ	Ok
2	AR1660CCC500	PO109743.D	10 Mar 2025 10:10	YP/AJ	Ok
3	AR1242CCC500	PO109744.D	10 Mar 2025 10:29	YP/AJ	Ok
4	AR1248CCC500	PO109745.D	10 Mar 2025 10:47	YP/AJ	Ok
5	AR1254CCC500	PO109746.D	10 Mar 2025 11:06	YP/AJ	Ok
6	I.BLK	PO109747.D	10 Mar 2025 11:24	YP/AJ	Ok
7	PB167036BL	PO109748.D	10 Mar 2025 11:42	YP/AJ	Ok
8	PB167036BS	PO109749.D	10 Mar 2025 12:01	YP/AJ	Ok
9	Q1530-01	PO109750.D	10 Mar 2025 12:18	YP/AJ	Ok
10	Q1530-02	PO109751.D	10 Mar 2025 12:36	YP/AJ	Ok
11	Q1527-01	PO109752.D	10 Mar 2025 12:55	YP/AJ	Ok
12	Q1527-02	PO109753.D	10 Mar 2025 13:13	YP/AJ	Ok
13	Q1527-03	PO109754.D	10 Mar 2025 13:32	YP/AJ	Ok
14	AR1660CCC500	PO109755.D	10 Mar 2025 14:18	YP/AJ	Ok
15	AR1242CCC500	PO109756.D	10 Mar 2025 14:37	YP/AJ	Ok
16	AR1248CCC500	PO109757.D	10 Mar 2025 14:55	YP/AJ	Ok
17	AR1254CCC500	PO109758.D	10 Mar 2025 15:13	YP/AJ	Ok
18	I.BLK	PO109759.D	10 Mar 2025 15:31	YP/AJ	Ok
19	PB167042BL	PO109760.D	10 Mar 2025 15:49	YP/AJ	Ok
20	PB167042BS	PO109761.D	10 Mar 2025 16:07	YP/AJ	Ok
21	PB167042BSD	PO109762.D	10 Mar 2025 16:26	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031025

Review By	yogesh	Review On	3/11/2025 8:31:51 AM
Supervise By	Ankita	Supervise On	3/11/2025 8:52:58 AM
SubDirectory	PO031025	HP Acquire Method	HP Processing Method PO022025
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	Q1528-02	PO109763.D	10 Mar 2025 16:44	YP/AJ	Ok,M
23	Q1522-02	PO109764.D	10 Mar 2025 17:03	YP/AJ	Ok
24	Q1528-01	PO109765.D	10 Mar 2025 17:21	YP/AJ	Ok,M
25	Q1528-03	PO109766.D	10 Mar 2025 17:39	YP/AJ	Ok
26	Q1529-05	PO109767.D	10 Mar 2025 17:58	YP/AJ	Ok,M
27	Q1529-06	PO109768.D	10 Mar 2025 18:16	YP/AJ	Ok,NR
28	AR1660CCC500	PO109769.D	10 Mar 2025 19:03	YP/AJ	Ok
29	AR1242CCC500	PO109770.D	10 Mar 2025 19:20	YP/AJ	Ok
30	AR1248CCC500	PO109771.D	10 Mar 2025 19:39	YP/AJ	Ok
31	AR1254CCC500	PO109772.D	10 Mar 2025 19:57	YP/AJ	Ok,M
32	I.BLK	PO109773.D	10 Mar 2025 20:15	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO022025

Review By	yogesh	Review On	2/21/2025 8:09:53 AM
Supervise By	Ankita	Supervise On	2/21/2025 9:30:37 AM
SubDirectory	PO022025	HP Acquire Method	HP Processing Method PO022025

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773
Internal Standard/PEM	
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO109424.D	20 Feb 2025 16:09		YP/AJ	Ok
2	I.BLK	I.BLK	PO109425.D	20 Feb 2025 16:28		YP/AJ	Ok
3	AR1660ICC1000	AR1660ICC1000	PO109426.D	20 Feb 2025 16:46		YP/AJ	Ok
4	AR1660ICC750	AR1660ICC750	PO109427.D	20 Feb 2025 17:04		YP/AJ	Ok
5	AR1660ICC500	AR1660ICC500	PO109428.D	20 Feb 2025 17:23		YP/AJ	Ok
6	AR1660ICC250	AR1660ICC250	PO109429.D	20 Feb 2025 17:41		YP/AJ	Ok
7	AR1660ICC050	AR1660ICC050	PO109430.D	20 Feb 2025 17:59		YP/AJ	Ok
8	AR1221ICC500	AR1221ICC500	PO109431.D	20 Feb 2025 18:18		YP/AJ	Ok
9	AR1232ICC500	AR1232ICC500	PO109432.D	20 Feb 2025 18:36		YP/AJ	Ok
10	AR1242ICC1000	AR1242ICC1000	PO109433.D	20 Feb 2025 18:55		YP/AJ	Ok
11	AR1242ICC750	AR1242ICC750	PO109434.D	20 Feb 2025 19:13		YP/AJ	Ok
12	AR1242ICC500	AR1242ICC500	PO109435.D	20 Feb 2025 19:31		YP/AJ	Ok
13	AR1242ICC250	AR1242ICC250	PO109436.D	20 Feb 2025 19:50		YP/AJ	Ok
14	AR1242ICC050	AR1242ICC050	PO109437.D	20 Feb 2025 20:08		YP/AJ	Ok,M
15	AR1248ICC1000	AR1248ICC1000	PO109438.D	20 Feb 2025 20:26		YP/AJ	Ok
16	AR1248ICC750	AR1248ICC750	PO109439.D	20 Feb 2025 20:45		YP/AJ	Ok
17	AR1248ICC500	AR1248ICC500	PO109440.D	20 Feb 2025 21:03		YP/AJ	Ok
18	AR1248ICC250	AR1248ICC250	PO109441.D	20 Feb 2025 21:21		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO022025

Review By	yogesh	Review On	2/21/2025 8:09:53 AM
Supervise By	Ankita	Supervise On	2/21/2025 9:30:37 AM
SubDirectory	PO022025	HP Acquire Method	HP Processing Method PO022025
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248ICC050	AR1248ICC050	PO109442.D	20 Feb 2025 21:40		YP/AJ	Ok,M
20	AR1254ICC1000	AR1254ICC1000	PO109443.D	20 Feb 2025 21:58		YP/AJ	Ok
21	AR1254ICC750	AR1254ICC750	PO109444.D	20 Feb 2025 22:17		YP/AJ	Ok
22	AR1254ICC500	AR1254ICC500	PO109445.D	20 Feb 2025 22:35		YP/AJ	Ok
23	AR1254ICC250	AR1254ICC250	PO109446.D	20 Feb 2025 22:53		YP/AJ	Ok
24	AR1254ICC050	AR1254ICC050	PO109447.D	20 Feb 2025 23:12		YP/AJ	Ok,M
25	AR1262ICC500	AR1262ICC500	PO109448.D	20 Feb 2025 23:30		YP/AJ	Ok
26	AR1268ICC1000	AR1268ICC1000	PO109449.D	20 Feb 2025 23:48		YP/AJ	Ok
27	AR1268ICC750	AR1268ICC750	PO109450.D	21 Feb 2025 00:07		YP/AJ	Ok
28	AR1268ICC500	AR1268ICC500	PO109451.D	21 Feb 2025 00:25		YP/AJ	Ok
29	AR1268ICC250	AR1268ICC250	PO109452.D	21 Feb 2025 00:43		YP/AJ	Ok
30	AR1268ICC050	AR1268ICC050	PO109453.D	21 Feb 2025 01:02		YP/AJ	Ok
31	PO022025ICV500	ICVPO022025	PO109454.D	21 Feb 2025 01:20		YP/AJ	Ok
32	AR1242ICV500	ICVPO022025AR1242	PO109455.D	21 Feb 2025 01:38		YP/AJ	Ok
33	AR1248ICV500	ICVPO022025AR1248	PO109456.D	21 Feb 2025 01:57		YP/AJ	Ok
34	AR1254ICV500	ICVPO022025AR1254	PO109457.D	21 Feb 2025 02:15		YP/AJ	Ok
35	AR1268ICV500	ICVPO022025AR1268	PO109458.D	21 Feb 2025 02:34		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031025

Review By	yogesh	Review On	3/11/2025 8:31:51 AM
Supervise By	Ankita	Supervise On	3/11/2025 8:52:58 AM
SubDirectory	PO031025	HP Acquire Method	HP Processing Method PO022025

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773
Internal Standard/PEM	
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO109742.D	10 Mar 2025 09:52		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO109743.D	10 Mar 2025 10:10		YP/AJ	Ok
3	AR1242CCC500	AR1242CCC500	PO109744.D	10 Mar 2025 10:29		YP/AJ	Ok
4	AR1248CCC500	AR1248CCC500	PO109745.D	10 Mar 2025 10:47		YP/AJ	Ok
5	AR1254CCC500	AR1254CCC500	PO109746.D	10 Mar 2025 11:06		YP/AJ	Ok
6	I.BLK	I.BLK	PO109747.D	10 Mar 2025 11:24		YP/AJ	Ok
7	PB167036BL	PB167036BL	PO109748.D	10 Mar 2025 11:42		YP/AJ	Ok
8	PB167036BS	PB167036BS	PO109749.D	10 Mar 2025 12:01		YP/AJ	Ok
9	Q1530-01	1-WIPE	PO109750.D	10 Mar 2025 12:18	AR1242 Hit	YP/AJ	Ok
10	Q1530-02	2-WIPE	PO109751.D	10 Mar 2025 12:36	AR1242 Hit	YP/AJ	Ok
11	Q1527-01	022825-SEALPOT	PO109752.D	10 Mar 2025 12:55		YP/AJ	Ok
12	Q1527-02	030425-A	PO109753.D	10 Mar 2025 13:13		YP/AJ	Ok
13	Q1527-03	030425-B	PO109754.D	10 Mar 2025 13:32		YP/AJ	Ok
14	AR1660CCC500	AR1660CCC500	PO109755.D	10 Mar 2025 14:18		YP/AJ	Ok
15	AR1242CCC500	AR1242CCC500	PO109756.D	10 Mar 2025 14:37		YP/AJ	Ok
16	AR1248CCC500	AR1248CCC500	PO109757.D	10 Mar 2025 14:55		YP/AJ	Ok
17	AR1254CCC500	AR1254CCC500	PO109758.D	10 Mar 2025 15:13		YP/AJ	Ok
18	I.BLK	I.BLK	PO109759.D	10 Mar 2025 15:31		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031025

Review By	yogesh	Review On	3/11/2025 8:31:51 AM
Supervise By	Ankita	Supervise On	3/11/2025 8:52:58 AM
SubDirectory	PO031025	HP Acquire Method	HP Processing Method PO022025
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	PB167042BL	PB167042BL	PO109760.D	10 Mar 2025 15:49		YP/AJ	Ok
20	PB167042BS	PB167042BS	PO109761.D	10 Mar 2025 16:07		YP/AJ	Ok
21	PB167042BSD	PB167042BSD	PO109762.D	10 Mar 2025 16:26		YP/AJ	Ok
22	Q1528-02	22725	PO109763.D	10 Mar 2025 16:44		YP/AJ	Ok,M
23	Q1522-02	TW-WTS-04	PO109764.D	10 Mar 2025 17:03		YP/AJ	Ok
24	Q1528-01	FERNOT	PO109765.D	10 Mar 2025 17:21		YP/AJ	Ok,M
25	Q1528-03	22425	PO109766.D	10 Mar 2025 17:39		YP/AJ	Ok
26	Q1529-05	60302	PO109767.D	10 Mar 2025 17:58	DCB low in 1st column	YP/AJ	Ok,M
27	Q1529-06	60299	PO109768.D	10 Mar 2025 18:16		YP/AJ	Ok,NR
28	AR1660CCC500	AR1660CCC500	PO109769.D	10 Mar 2025 19:03		YP/AJ	Ok
29	AR1242CCC500	AR1242CCC500	PO109770.D	10 Mar 2025 19:20		YP/AJ	Ok
30	AR1248CCC500	AR1248CCC500	PO109771.D	10 Mar 2025 19:39		YP/AJ	Ok
31	AR1254CCC500	AR1254CCC500	PO109772.D	10 Mar 2025 19:57		YP/AJ	Ok,M
32	I.BLK	I.BLK	PO109773.D	10 Mar 2025 20:15		YP/AJ	Ok

M : Manual Integration

SOP ID: M3510C,3580A-Extraction PCB-14

Clean Up SOP #: Acid Cleanup **Extraction Start Date :** 03/10/2025

Matrix : Water **Extraction Start Time :** 08:48

Weigh By: N/A **Extraction By:** RS **Extraction End Date :** 03/10/2025

Balance check: RJ **Filter By:** RS **Extraction End Time :** 13:30

Balance ID: N/A **pH Meter ID:** N/A **Concentration By:** EH

pH Strip Lot#: E3880 **Hood ID:** 4,5,6,7 **Supervisor By :** RUPESH

Extraction Method: ☒ Separatory Funnel ☐ Continuous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☐ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP24209
Surrogate	1.0ML	200 PPB	PP24217
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3878
Baked Na2SO4	N/A	EP2593
Hexane	N/A	E3877
H2SO4 1:1	N/A	EP2565
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40 ML Vial lot# 03-40BTS721.

KD Bath ID: N/A **Envap ID:** NEVAP-02


KD Bath Temperature: N/A **Envap Temperature:** 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
3/10/25	RS (B4-Lab)	Y-P. Pestir U.
13:35	Preparation Group	Analysis Group

Analytical Method: M3510C,3580A-Extraction PCB-14

Concentration Date: 03/10/2025

Sample ID	Client Sample ID	Test	g /  mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB167042BL	ABLK042	PCB	1000	6	RUPESH	ritesh	10			SEP-8
PB167042BS	ALCS042	PCB	1000	6	RUPESH	ritesh	10			9
PB167042BSD	ALCSD042	PCB	1000	6	RUPESH	ritesh	10			10
Q1522-02	TW-WTS-04	PCB	990	6	RUPESH	ritesh	10	C		11
Q1528-01	FERNOT	PCB	1000	6	RUPESH	ritesh	10	C		12
Q1528-02	22725	PCB	1000	6	RUPESH	ritesh	10	C		13
Q1528-03	22425	PCB	990	6	RUPESH	ritesh	10	C		14
Q1529-05	60302	PCB	980	6	RUPESH	ritesh	10	D		15
Q1529-06	60299	PCB	1000	6	RUPESH	ritesh	10	D		16

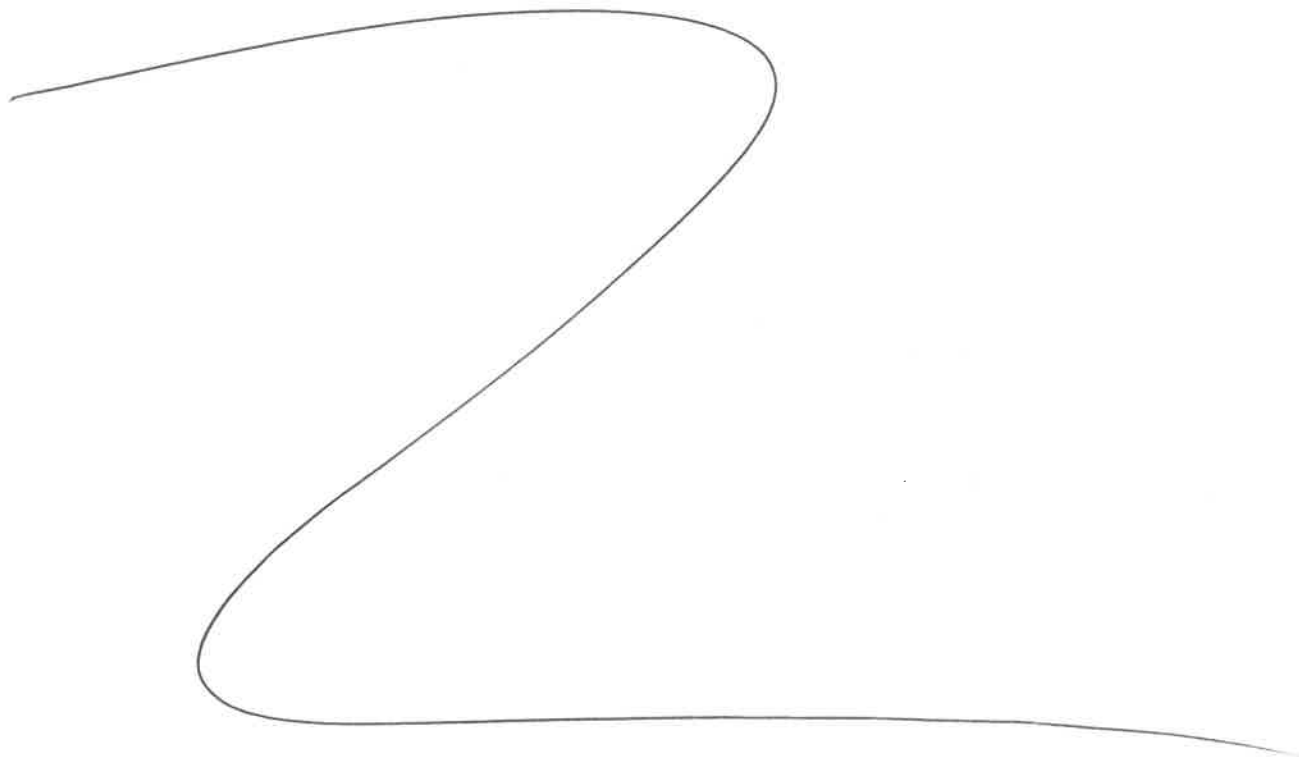

R
3/10

1674008

WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q1528 WorkList ID : 188145 Department : Extraction Date : 03-10-2025 08:43:57

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1522-02	TW-WTS-04	Water	PCB	Cool 4 deg C	ENTA05	H31	03/06/2025	8082A
Q1528-01	FERNOT	Water	PCB	Cool 4 deg C	PSEG03	I31	03/07/2025	8082A
Q1528-02	22725	Water	PCB	Cool 4 deg C	PSEG03	I31	03/07/2025	8082A
Q1528-03	22425	Water	PCB	Cool 4 deg C	PSEG03	I31	03/07/2025	8082A
Q1529-05	60302	Water	PCB	Cool 4 deg C	PSEG03	I31	03/07/2025	8082A
Q1529-06	60299	Water	PCB	Cool 4 deg C	PSEG03	I31	03/07/2025	8082A

Date/Time 3/10/25 8:43
Raw Sample Received by: RJ (Ext 196)
Raw Sample Relinquished by: AP Sr

Date/Time 3/10/25 9:10
Raw Sample Received by: AP Sr
Raw Sample Relinquished by: RJ (Ext 196)

Prep Standard - Chemical Standard Summary

Order ID : Q1522

Test : PCB

Prepbatch ID : PB167042,

Sequence ID/Qc Batch ID: PO031025,

Standard ID :

EP2565,EP2593,PP23733,PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP
23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP2
3757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23
769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775,PP23776,PP23777,PP23778,PP23779,PP23780,PP237
81,PP23782,PP23783,PP23784,PP23785,PP23786,PP23787,PP23788,PP23789,PP23790,PP23946,PP23947,PP2420
9,PP24217,

Chemical ID :

E3551,E3804,E3805,E3825,E3876,E3877,E3878,M5173,P10483,P10500,P11507,P11512,P11521,P11581,P11587,P11
590,P11597,P12698,P12929,P12934,P12947,P12948,P12957,P13033,P13350,P13354,P13372,W3112,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2565	11/20/2024	05/20/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 11/20/2024

FROM 1000.00000ml of M5173 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2593	03/07/2025	07/01/2025	RUPESHKUMAR SHAH	Extraction_SC ALE_2 (EX-SC-2)	None	Riteshkumar Patel 03/07/2025

FROM 4000.00000gram of E3551 = Final Quantity: 4000.000 gram

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP23733	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P13350 + 9.00000ml of E3805 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
202	AR1660 1000/100 ppb working solution 1st source	PP23735	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P10483 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
203	AR1660 750 PPB STD	PP23736	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23735 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
204	AR1660 500 PPB STD	PP23737	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23735 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
205	AR1660 250 PPB STD	PP23738	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23735 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
206	AR1660 50 PPB STD	PP23739	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23737 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
213	AR1221 1000 PPB WORKING SOLUTION	PP23740	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11581 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1079	AR1221 750 PPB STD	PP23741	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23740 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
222	AR1221 500 PPB STD	PP23742	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23740 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1080	AR1221 250 PPB STD	PP23743	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23740 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1081	AR1221 50 PPB STD	PP23744	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23742 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
214	AR1232 1000 PPB WORKING SOLUTION	PP23745	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11587 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1063	AR1232 750 PPB STD	PP23747	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23745 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
223	AR1232 500 PPB STD	PP23748	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23745 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1064	AR1232 250 PPB STD	PP23749	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23745 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1065	AR1232 50 PPB STD	PP23750	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23748 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
215	AR1242 1000 PPB WORKING STD	PP23751	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P12929 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1067	AR1242 750 PPB STD	PP23752	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23751 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
224	AR1242 500 PPB STD	PP23753	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23751 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1068	AR1242 250 PPB STD	PP23754	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23751 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1069	AR1242 50 PPB STD	PP23755	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23753 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
216	AR1248 1000 PPB WORKING STD	PP23756	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P12934 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1075	AR1248 750 PPB STD	PP23757	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23756 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
225	AR1248 500 PPB STD	PP23758	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23756 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1076	AR1248 250 PPB STD	PP23759	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23756 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1077	AR1248 50 PPB STD	PP23760	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23758 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
217	AR1254 1000 PPB WORKING STD	PP23761	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11590 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1071	AR1254 750 PPB STD	PP23762	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23761 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
226	AR1254 500 PPB STD	PP23763	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23761 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1072	AR1254 250 PPB STD	PP23764	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23761 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1073	AR1254 50 PPB STD	PP23765	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23763 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1529	AR1262 1000 PPB Working Solution	PP23766	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P10500 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3753	AR1262 750 PPB STD	PP23767	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23766 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1530	AR1262 500 PPB STD	PP23768	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23766 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3754	AR1262 250 PPB STD	PP23769	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23766 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3755	AR1262 50 PPB STD	PP23770	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23768 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1532	AR1268 1000 PPB Working Solution	PP23771	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11597 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3820	AR1268 750 PPB STD	PP23772	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23771 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1533	AR1268 500 PPB STD	PP23773	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23771 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3821	AR1268 250 PPB STD	PP23774	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23771 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3822	AR1268 50 PPB STD	PP23775	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23773 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
404	AR1660 100 PPM Stock Solution 2nd Source	PP23776	10/03/2024	04/01/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12947 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
405	AR1660 1000/100 PPB ICV STD	PP23777	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 98.50000ml of E3805 + 0.50000ml of PP23733 + 1.00000ml of PP23776 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
406	AR1660 500 PPB ICV	PP23778	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23777 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3789	AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT)	PP23779	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P13372 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3790	AR1221 500 PPB ICV(AGILENT)	PP23780	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23779 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1887	AR1232 1000 PPB Working Sol. 2nd Source	PP23781	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel 10/03/2024

FROM 1.00000ml of P12698 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1889	AR1242 1000 PPB Working Sol. 2nd Source	PP23782	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel 10/03/2024

FROM 1.00000ml of P11507 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1888	AR1232 500 PPB ICV	PP23783	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23781 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1891	AR1242 500 PPB ICV	PP23784	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23782 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1890	AR1248 1000 PPB Working Sol. 2nd Source	PP23785	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11512 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1892	AR1248 500 PPB ICV	PP23786	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23785 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1893	AR1254 1000 PPB Working Sol. 2nd Source	PP23787	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12957 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1894	AR1254 500 PPB ICV	PP23788	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23787 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3757	AR1262 1000 PPB Working Solution second source	PP23789	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P13033 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3758	AR1262 500 PPB STD ICV	PP23790	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23789 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3817	AR1268 1000 ppb Working Soln. 2nd source	PP23946	11/07/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								11/13/2024

FROM 1.00000ml of P11521 + 98.50000ml of E3825 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3823	AR1268 500 PPB STD ICV	PP23947	11/07/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								11/13/2024

FROM 0.50000ml of E3825 + 0.50000ml of PP23946 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3857	5000 PPB PCB SPIKE SOLUTION 2ND SOURCE	PP24209	02/27/2025	08/27/2025	Ankita Jodhani	None	None	Yogesh Patel
								03/06/2025

FROM 0.50000ml of P12948 + 99.50000ml of E3876 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP24217	03/05/2025	08/25/2025	Abdul Mirza	None	None	Yogesh Patel
								03/06/2025

FROM 1.00000ml of P13354 + 999.00000ml of E3876 = Final Quantity: 1000.000 ml

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	07/01/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	11/05/2025	10/01/2024 / Rajesh	09/25/2024 / Rajesh	E3804

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	03/30/2025	09/30/2024 / Rajesh	09/25/2024 / Rajesh	E3805

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	11/06/2025	11/06/2024 / Rajesh	11/01/2024 / Rajesh	E3825

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	08/25/2025	02/25/2025 /	02/12/2025 / Rajesh	E3876

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	243570	08/12/2025	02/12/2025 / Rajesh	02/12/2025 / Rajesh	E3877

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24K1762005	08/14/2025	02/14/2025 / Rajesh	12/27/2024 / Rajesh	E3878

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	0000281827	06/02/2025	06/01/2022 /	04/05/2022 / william	M5173

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul	A0163157	04/03/2025	10/03/2024 / Ankita	03/19/2021 / Abdul	P10483

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane	A0167722	04/03/2025	10/03/2024 / Ankita	03/19/2021 / Ankita	P10500

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-312-1 / Aroclor 1242	0006665550	04/03/2025	10/03/2024 / Ankita	02/21/2022 / Ankita	P11507

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-342-1 / Aroclor 1248	0006626997	04/03/2025	10/03/2024 / Ankita	02/21/2022 / Ankita	P11512

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-382-1 / Aroclor 1268	0006587800	05/07/2025	11/07/2024 / Ankita	02/21/2022 / Ankita	P11521

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul	A0175456	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11581

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul	A0173309	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11587

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	A0175403	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11590

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane	A0181782	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11597

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	91867 / Aroclor 1232 100 ug/mL	020823	04/03/2025	10/03/2024 / Ankita	08/07/2023 / Ankita	P12698

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul	a0203672	04/03/2025	10/03/2024 / Ankita	12/07/2023 / Ankita	P12929

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul	a0202803	04/03/2025	10/03/2024 / Ankita	12/07/2023 / Ankita	P12934

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12947

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	08/27/2025	02/27/2025 / Ankita	12/20/2023 / Yogesh	P12948

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ Arochlor 1254	121823	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12957

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	90165 / Aroclor 1262	112322	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P13033

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	04/03/2025	10/03/2024 / Ankita	04/22/2024 / Abdul	P13350

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	09/05/2025	03/05/2025 / Abdul	04/22/2024 / Abdul	P13354

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-292-1 / Aroclor 1221	0006783205	04/03/2025	10/03/2024 / Ankita	05/02/2024 / Ankita	P13372

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use

Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC



Michelle Bales
Sr. Manager, Quality Assurance

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9262-03
Batch No.: 24C1862008
Manufactured Date: 2024-01-30
Expiration Date: 2025-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.4 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 9/25/24

E 3805

Jamie Croak
Director Quality Operations, Bioscience Production

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

£ 3825

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

 **avantors**™



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 2/12/25

E 3876



Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Certificate of Analysis

1 Reagent Lane
 Fair Lawn, NJ 07410
 201.796.7100 tel
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System
 Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	H303	Quality Test / Release Date	11/07/2024
Lot Number	243570		
Description	HEXANES - OPTIMA		
Country of Origin	United States	Suggested Retest Date	Nov/2029
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A			
Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid
ASSAY (N-HEXANE)	%	>= 60	69
ASSAY (SUM C6 HYDROCARBONS)	%	>= 99.9	>99.9
COLOR	APHA	<= 5	<5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.653 - 0.673	0.669
EVAPORATION RESIDUE	ppm	<= 1	<1
FLUORESCENCE BACKGROUND	ppb	<= 1	<1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 195 NM	ABS. UNITS	<= 1	0.74
OPTICAL ABS AT 210 NM	ABS. UNITS	<= 0.25	0.17
OPTICAL ABS AT 220 NM	ABS. UNITS	<= 0.07	0.05
OPTICAL ABS AT 254 NM	ABS. UNITS	<= 0.005	0.001
PESTICIDE RESIDUE ANALYSIS	NG/L	<= 10	<10
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.375 - 1.385	1.379
SUITABILITY FOR GC/MS		= PASS TEST	PASS TEST
SULFUR COMPOUNDS	%	<= 0.005	<0.005
THIOPHENE	PASS/FAIL	= PASS TEST	PASS TEST
WATER (H2O)	%	<= 0.01	<0.01
WATER-SOLUBLE TITRABLE ACID	MEQ/G	<= 0.0003	0.0001

Recd. by RP on 2/12/25

 E3877

Harout Sahagian - Quality Control Manager - Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.

If there are any questions with this certificate, please call at (800) 227-6701.

*Based on suggested storage condition.

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 24K1762005
Manufactured Date: 2024-10-08
Expiration Date: 2026-01-07
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	2
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	≤ 10	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.5 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	0.0
Chloride (Cl)	$\leq 10 \text{ ppm}$	$< 5 \text{ ppm}$
Water (by KF, coulometric)	$\leq 0.02 \%$	0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3878

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA, 19087 U.S.A. Phone 610.386.1700

Hydrochloric Acid, 36.5–38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis



Material No.: 9530-33
Batch No.: 0000281827
Manufactured Date: 2021/03/30
Retest Date: 2026/03/29
Revision No: 1

Certificate of Analysis

Test	Specification	Result
ACS – Assay (as HCl) (by acid–base titrn)	36.5 – 38.0 %	37.6
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	1
ACS – Specific Gravity at 60°/60°F	1.185 – 1.192	1.189
ACS – Bromide (Br)	<= 0.005 %	< 0.005
ACS – Extractable Organic Substances	<= 5 ppm	< 1
ACS – Free Chlorine (as Cl ₂)	<= 0.5 ppm	< 0.5
Phosphate (PO ₄)	<= 0.05 ppm	< 0.03
Sulfate (SO ₄)	<= 0.5 ppm	< 0.3
Sulfite (SO ₃)	<= 0.8 ppm	0.3
Ammonium (NH ₄)	<= 3 ppm	< 1
Trace Impurities – Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities – Aluminum (Al)	<= 10.0 ppb	0.5
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities – Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities – Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities – Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities – Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities – Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities – Calcium (Ca)	<= 50.0 ppb	15.0
Trace Impurities – Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities – Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities – Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities – Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	3.0
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	1.0
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	< 0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	< 0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.2
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	18.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	< 0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.4
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use

Product Information (not specifications):

Appearance (clear, fuming liquid)

Meets ACS Specifications

Country of Origin: US

Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32039 **Lot No.:** A0163157

Description : Aroclor® 1016/1260 Mix
Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2026 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1016 CAS # 12674-11-2 (Lot 04) Purity ----%	1,007.0 µg/mL	+/- 5.8683 µg/mL Gravimetric +/- 31.9082 µg/mL Unstressed +/- 41.6868 µg/mL Stressed
2	Aroclor 1260 CAS # 11096-82-5 (Lot 07) Purity ----%	1,008.0 µg/mL	+/- 5.8741 µg/mL Gravimetric +/- 31.9399 µg/mL Unstressed +/- 41.7282 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 10476

P 10480

AR
02/19/21

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

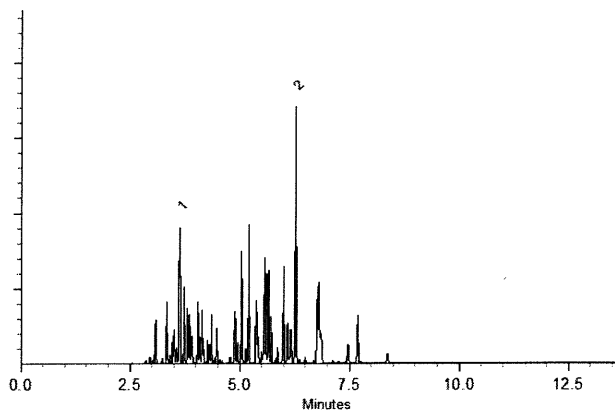

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar - Mix Technician

Date Mixed: 03-Aug-2020

Balance: B442140311

Justine Albertson - Operations Tech-ARM QC

Date Passed: 05-Aug-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32409 Lot No.: A0167722
Description : Aroclor® 1262 Standard
Aroclor® 1262 Standard 1,000 µg/mL, 1mL/ampul, Hexane
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : April 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1262	1,004.0 µg/mL	+/- 5.9635 µg/mL Gravimetric
	CAS # 37324-23-5 (Lot 10849100)		+/- 31.8340 µg/mL Unstressed
	Purity ----%		+/- 41.5787 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P10496
↓
P10500

AJ
09/19/21

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

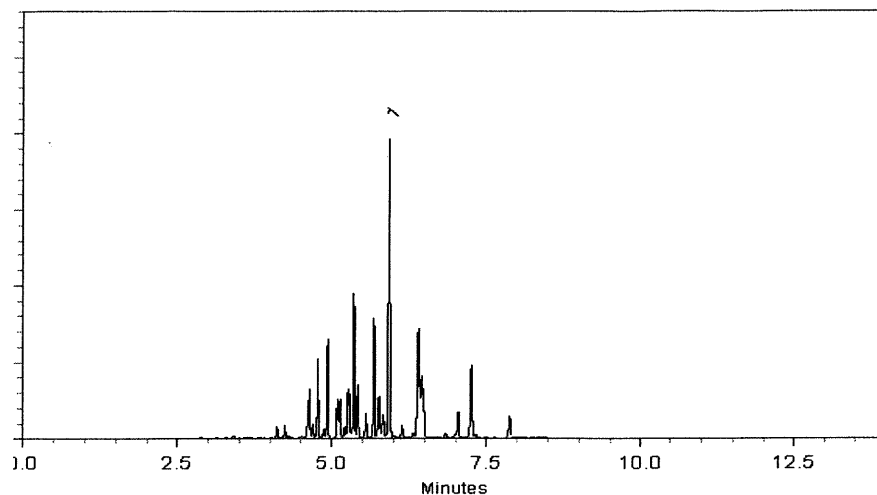

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 03-Jan-2021


Balance: B707717271

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 05-Jan-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1242 Standard

Lot Number: 0006665550

Product Number: PP-312-1

Lot Issue Date: 08-Feb-2022

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 31-Jan-2027

Component Name	CERTIFIED VALUES			CAS#	Analyte Lot
	Concentration	Expanded Uncertainty			
Aroclor 1242	100.4	± 0.5 µg/mL		053469-21-9	NT01020

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P11503
↓
P11507A7
02/21/22

Page: 1 of 2

CSD-QA-015.1

ISO 17034



Agilent

Trusted Answers

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2


www.agilent.com/quality/

CSD-QA-015.1



ISO 17025
Cert No. AT-

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1248 Standard

Lot Number: 0006626997

Product Number: PP-342-1

Lot Issue Date: 17-Aug-2021

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 30-Sep-2025

Component Name	CERTIFIED VALUES		CAS#	Analyte Lot
	Concentration	Expanded Uncertainty		
Aroclor 1248	100.3	± 0.5 µg/mL	012672-29-6	NT01582

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P11508

↓

P11512

AJ

2/21/22

ISO 17034



Agilent

Trusted Answers

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



Certificate of Analysis

P11518
↓
P11522
AJ
02/21/22

Product Name: Aroclor 1268 Standard

Product Number: PP-382-1

Lot Issue Date: 09-Feb-2021

Lot Number: 0006587800

Expiration Date: 31-Mar-2029

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration ± Uncertainty
Aroclor 1268	011100-14-4	RM00937	100.0 ± 0.5 µg/mL

Matrix: isooctane (2,2,4-trimethylpentane)

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.


Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026
Page: 1 of 1

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32007 **Lot No.:** A0175456
Description : Aroclor® 1221 Standard
Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : November 30, 2027 **Storage:** 25°C nominal
Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1221	1,002.0 µg/mL	+/- 5.9516 µg/mL Gravimetric
	CAS # 11104-28-2 (Lot 10210500)		+/- 31.7706 µg/mL Unstressed
	Purity ----%		+/- 41.4958 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 11578
↓
P 11582 / (S)

AR
04/30/22

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

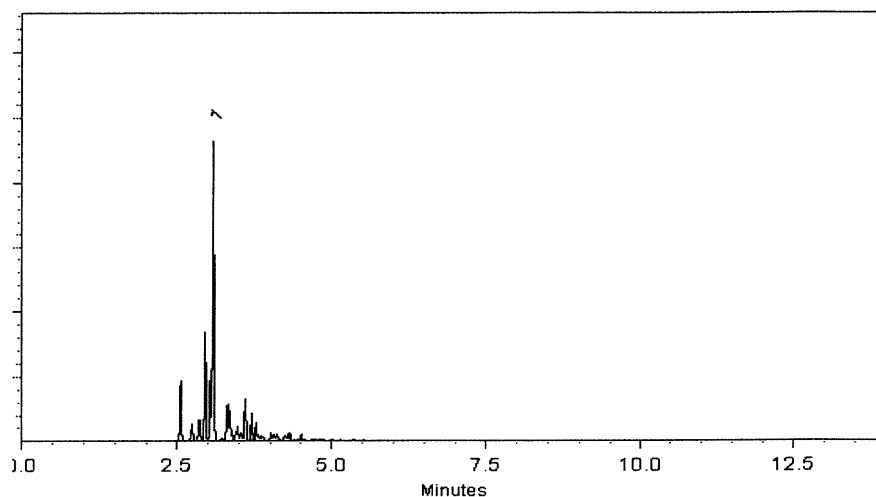

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 16-Aug-2021 Balance: B442140311

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 18-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11578
↓
P11582 / (S)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32008 Lot No.: A0173309
Description : Aroclor® 1232 Standard
Aroclor® 1232 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : September 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1232	1,001.0 µg/mL	+/- 5.9456 µg/mL Gravimetric
	CAS # 11141-16-5 (Lot 15665-01)		+/- 31.7389 µg/mL Unstressed
	Purity ----%		+/- 41.4544 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11583
↓
P11587 / (S)

AR
04/30/22

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

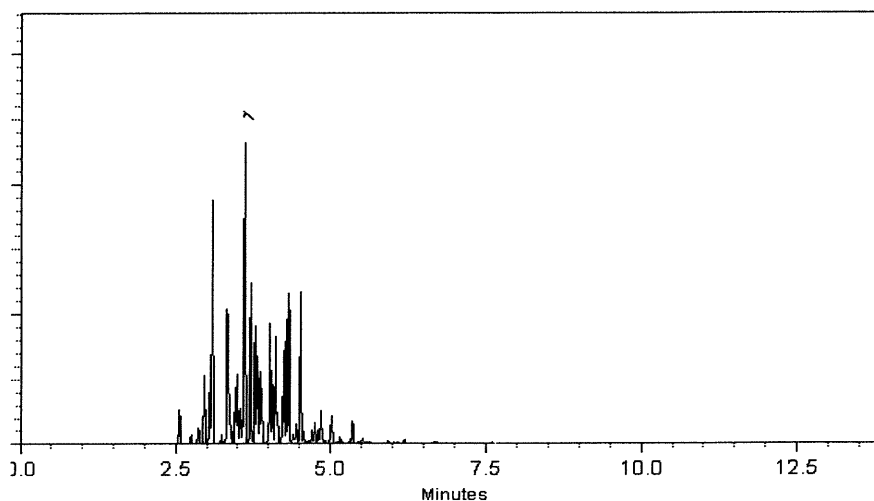

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 13-Jun-2021 **Balance:** B442140311

Alexis Shelow
Alexis Shelow - Operations Tech I

Date Passed: 16-Jun-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11583
↓
P11587 (5)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011 Lot No.: A0175403
Description : Aroclor® 1254 Standard
Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1254 CAS # 11097-69-1 (Lot 124-191-B) Purity ----%	1,000.7 µg/mL	+/- 5.9437 µg/mL Gravimetric +/- 31.7284 µg/mL Unstressed +/- 41.4406 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11588
↓
P11592 / (S)

AR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

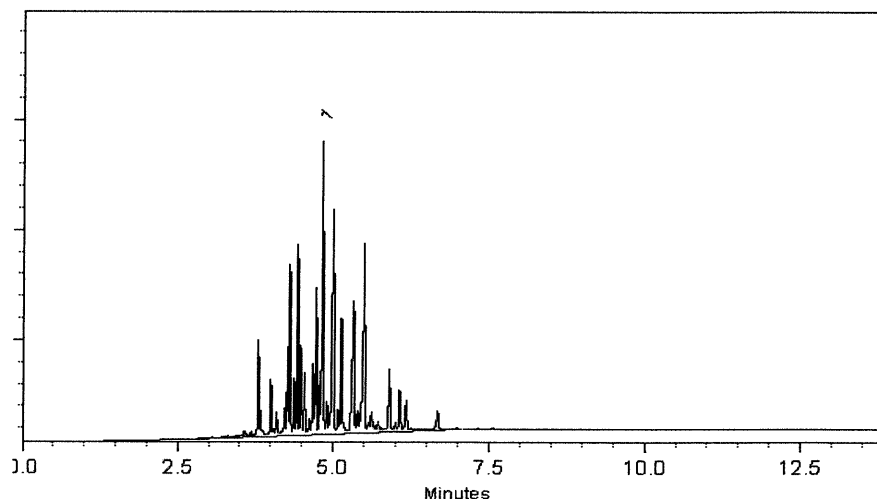

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Cathleen Soltis

Cathleen Soltis - Mix Technician

Date Mixed: 15-Aug-2021

Balance: 1128360905

Alexis Shelow

Alexis Shelow - Operations Tech I

Date Passed: 17-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11588
↓
P11592 / (5)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32410 **Lot No.:** A0181782

Description : Aroclor® 1268 Standard

Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : May 31, 2028 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1268	1,001.4 µg/mL	+/- 5.9480 µg/mL Gravimetric
	CAS # 11100-14-4 (Lot 10947000)		+/- 31.7516 µg/mL Unstressed
	Purity ----%		+/- 41.4710 µg/mL Stressed

Solvent: Hexane

CAS # 110-54-3

Purity 99%

P 11593
↓
P 11597

UAR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

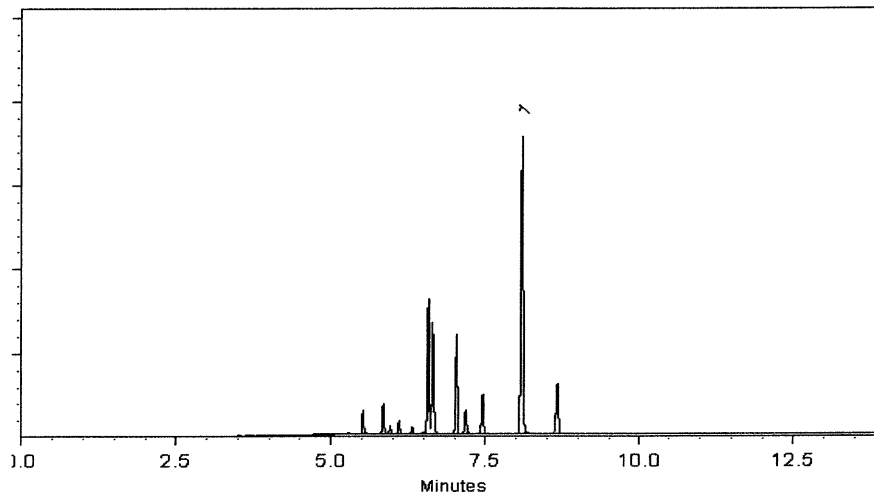

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Penelope S. Riglin
Penelope Riglin - Operations Tech I

Date Mixed: 14-Feb-2022

Balance: 1128360905

Clara Windle
Clara Windle - Operations Technician I

Date Passed: 17-Feb-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 11593 / (5)
↓
P 11597
[Signature]
04/30/2022



CERTIFIED WEIGHT REPORT

Part Number: **91867**
 Lot Number: **020823**
 Description: **WP 037 - Aroclor 1232**
PCB Technical Mixture
 Expiration Date: **020833**
 Recommended Storage: **Ambient (20 °C)**
 Nominal Concentration ($\mu\text{g/mL}$): **100**
 NIST Test ID#: **6UTB**

Solvent(
Aceton


Weight(s) shown below were combined and diluted to (mL): **100.0**
 5E-05 Balance Uncertainty
 0.057 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight (g)
1. Aroclor 1232	17	45-6A	100	100	0.5	0.01000

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measure Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stonier
 Column ID SPB-608 30 meter X 0.53mm X 5 μm film thickness
 Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
 Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
 Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
 Rate = 8°C/min, Total run time = 35 min
 Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
 Standard injection = 1.5 μL , Range=3

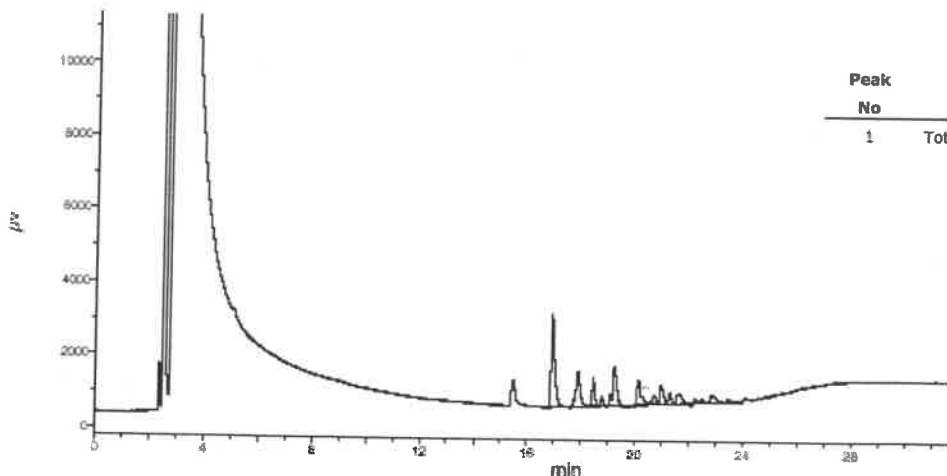




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32009 **Lot No.:** A0203672

Description: Aroclor® 1242 Standard

Aroclor® 1242 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

p12928

→

p12932

AJ

12/27/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Aroclor 1242	53469-21-9	01141	—%	1,004.7 µg/mL	+/- 55.7515

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

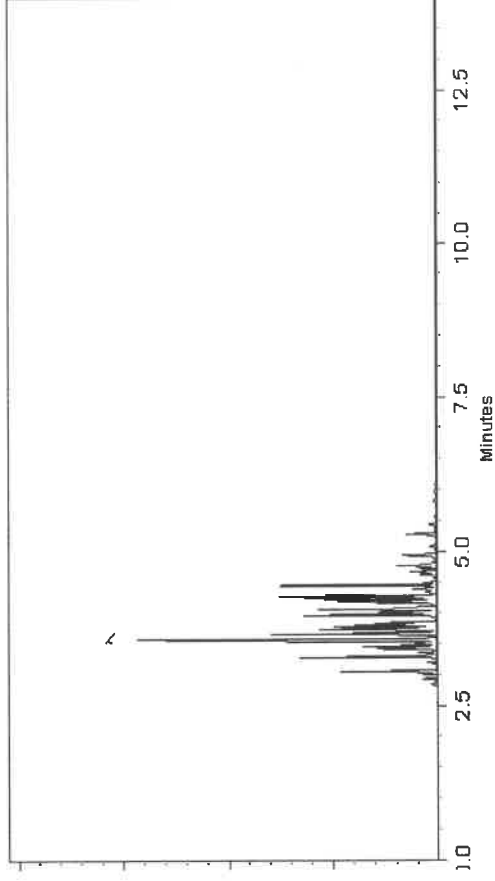

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Boothamer

Russ Boothamer - Operations Technician I

Date Mixed: 26-Oct-2023

Balance Serial #

B442140311

Jennifer Polino

Jennifer Polino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32010 **Lot No.:** A0202803

Description: Aroclor® 1248 Standard

Aroclor® 1248 Standard 1,000µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P1210967
P1210977
P1210973

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1248	12672-29-6	13897600	---%	1,001.7 µg/mL	+/- 55.5850

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

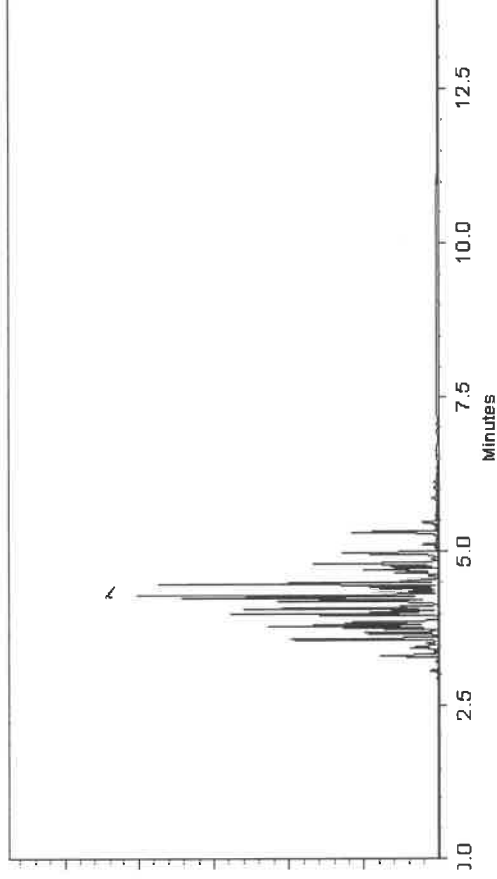

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

[Signature]
Laith Clemente - Operations Technician I

Date Mixed: 03-Oct-2023

Balance Serial # 1128360905

[Signature]
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty


Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

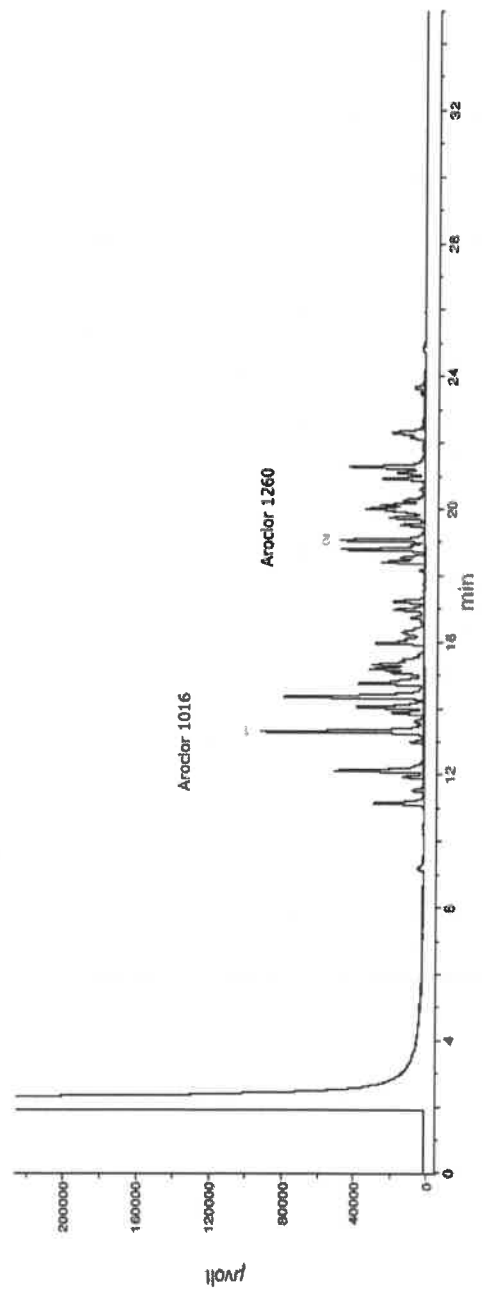



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty


Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

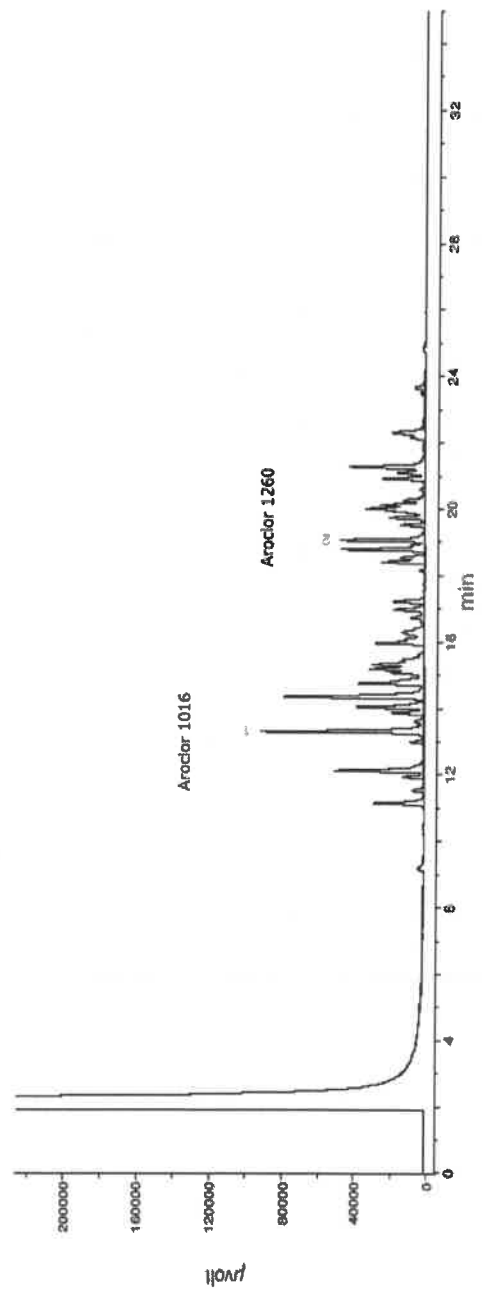



CERTIFIED WEIGHT REPORT

Part Number: 99139
Lot Number: 121823
Description: Aroclor 1254

Expiration Date: 121833
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 100
NIST Test ID#: 6UTB

Volume(s) shown below were combined and diluted to (mL): 20.0
Note: Aroclor 1254 is a mix of isomers.

Solvent(s): Iso-octane
Lot#: 82227

Formulated By: Anthony Mahoney	121823	DATE
Reviewed By: Pedro L. Rentas	121823	DATE


P12956 / Y.P.
12/18/23
P12957

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Initial Uncertainty	Pipette (mL)	Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information		
											(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA) LD50
1. Aroclor 1254	79100	121823	0.10	2.00	0.017	0.017	1003.3	100.1	11097-69-1	1.8	0.5mg/m3 (skin)		or-rat 1295mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X 5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150 °C (Time 1 = 4 min), Temp 2 = 280 °C (Time 2 = 13.5 min)
Rate = 8 °C/min, Total run time = 35 min
Injector temp. = 200 °C, FID Temp. = 300 °C, FID Signal = EDAQ Channel 1
Standard injection = 1.5µL, Range=3

Peak No.	Name	FID RT (min.)
1	Total Aroclor 1254	18.12

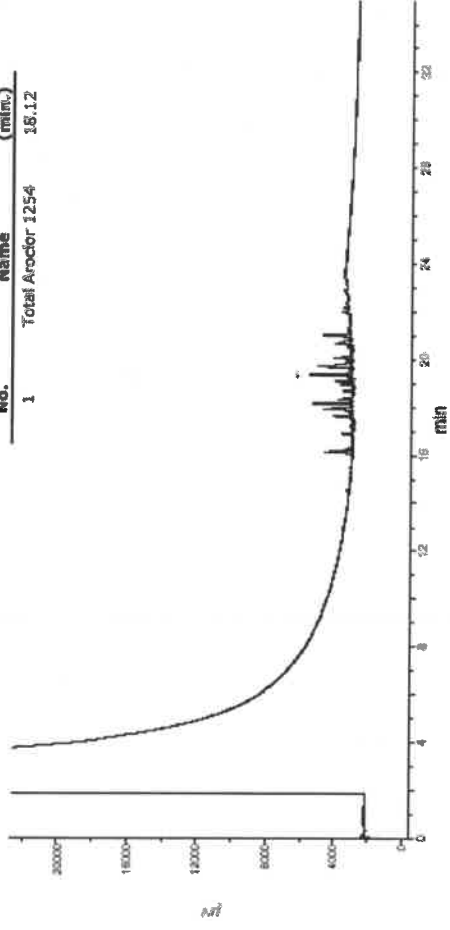



CERTIFIED WEIGHT REPORT

Part Number: 90165
Lot Number: 112322
Description: Atrocior 1262
Expiration Date: 112332
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 6LUTB
Weight(s) shown were combined and diluted to (mL): 50.0

Solvent(s): Hexane
Lot# 273615


SE-05 Balance Uncertainty
0.005 Flask Uncertainty

Formulated By:	Prashant Chauhan	112322	DATE
Reviewed By:	Pedro L. Rentes	112322	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	--------------------	-------------------	-------------------	---------------------	----------------------------------	------	----------------	------

1. Atrocior 1262 444 W-130-05 1000 100 0.2 0.05003 0.05016 1002.7 4.5 37324-23-5 N/A or-tal 11300mg/kg

Method GC/MSD-7.M: Column:(30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (0min.), Temp 2 = 290°C (12.5 min.), Rate = 8°C/min., Injector B = 200°C, Detector B = 290°C.

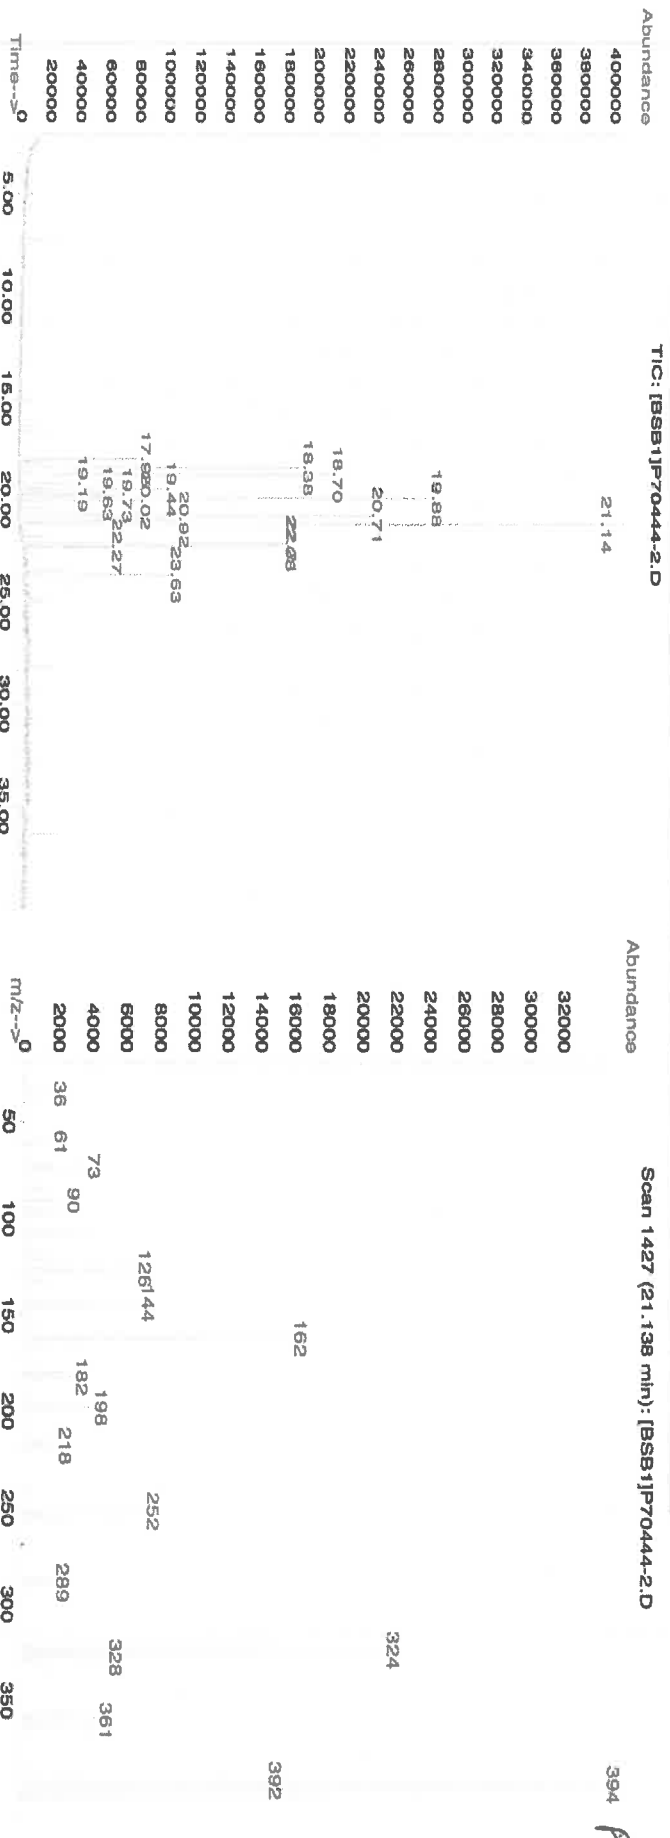

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




Run 20, "P90165 L112322 [1000µg/mL in hexane]"

Run Length: 35.00 min, 21000 points at 10 points/second.
Created: Thu, Dec 8, 2022 at 2:31:02 AM.
Sampled: Sequence "120722-GC3M1", Method "GC3-M1".
Analyzed using Method "GC3-M1".

Comments

GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
Standard injection = 1.5µL, Range=3

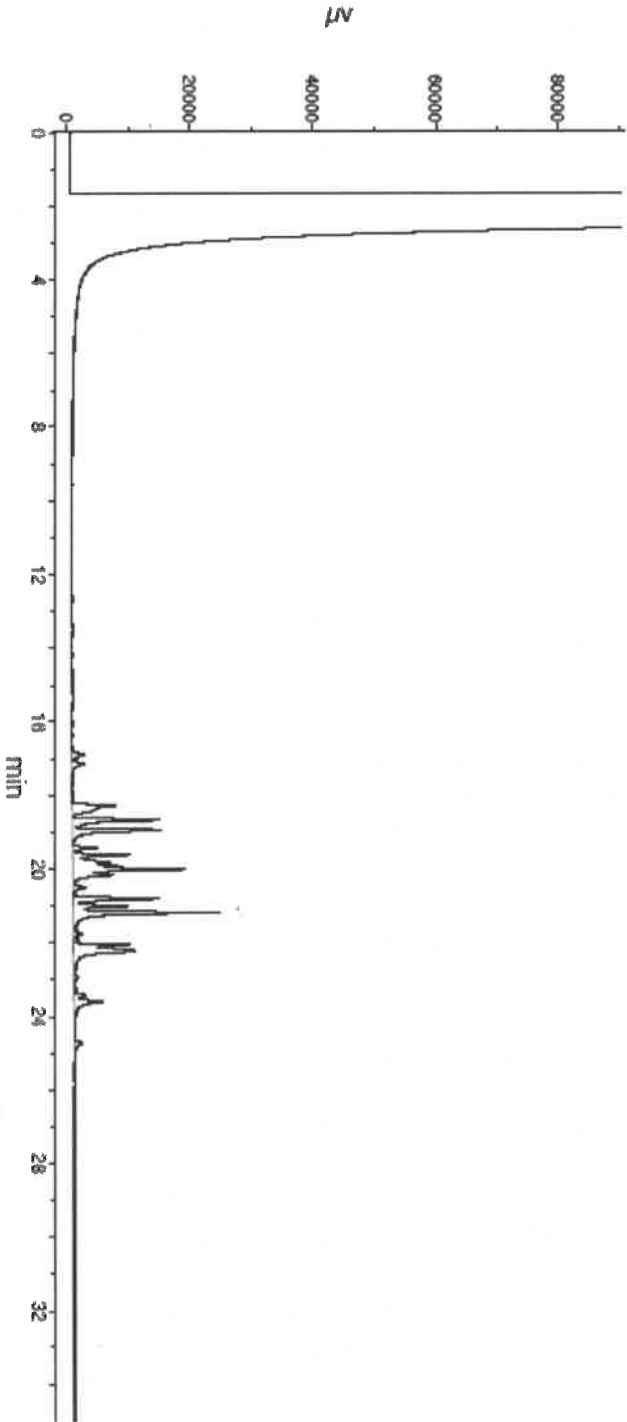



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

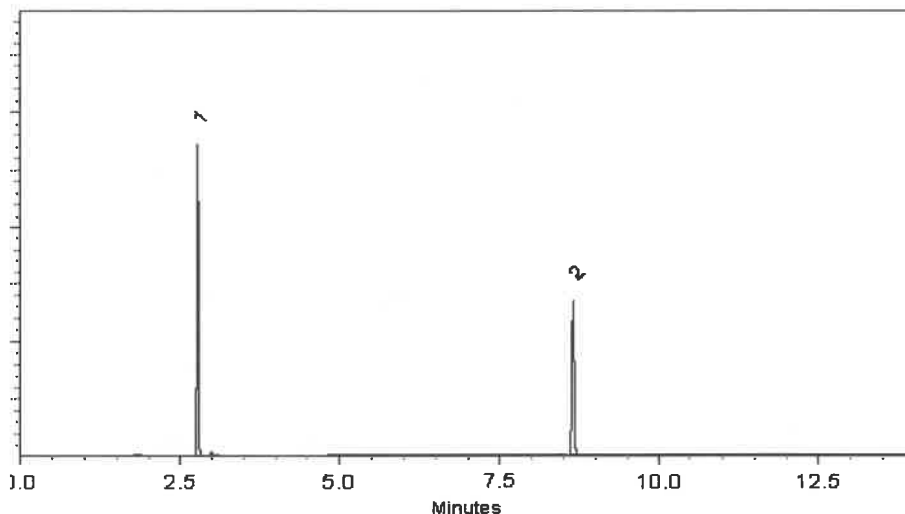


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

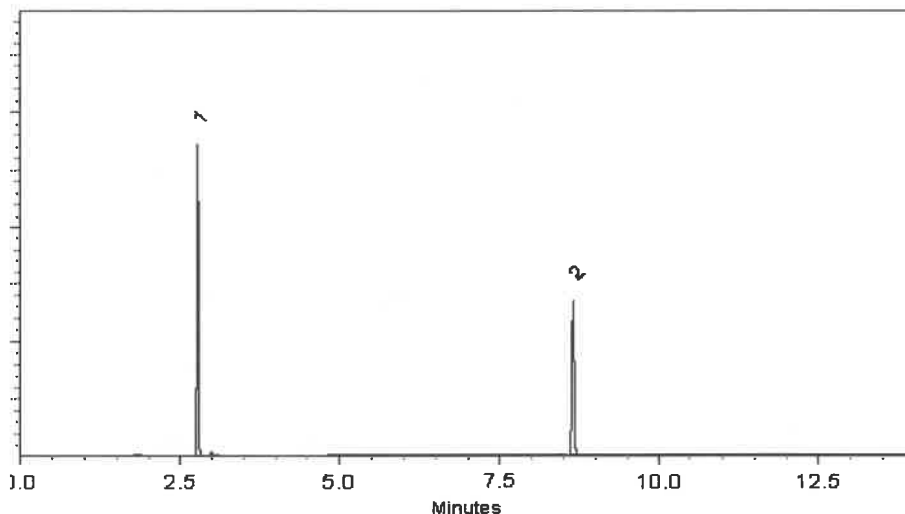


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



ISO 17034

Reference Material Certificate

Product Information Sheet

Product Name: Aroclor 1221 Standard
Product Number: PP-292-1
Storage Conditions: Store at Room Temperature (15° to 30°C).

Lot Number: 0006783205
Lot Issue Date: 20-Feb-2024
Expiration Date: 31-Mar-2032

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1221	100.3 ±	0.5 µg/mL	011104-28-2	NT01017

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13342
AJ
05106124
P13343

Page: 1 of 2

CSD-QA-015.2

ISO 17025
Cert No. AT-1937


250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.2

ISO 17025
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



SHIPPING DOCUMENTS



284 Sheffield Street, Mountainside, NJ 07092

(908) 789-8900 Fax: (908) 788-9222

www.chemtech.net

CHAIN OF CUSTODY RECORD

Alliance Project Number:

Q1522

COC Number: 2042109

Page 1 of 1

CLIENT INFORMATION

COMPANY: ENTACT, LLC

ADDRESS: 150 Bay Street, Suite 806

CITY: Jersey City STATE: NJ ZIP: 07302

ATTENTION: Jarod Stanfield

PHONE: 570-886-0442

FAX:

PROJECT INFORMATION

PROJECT NAME: 540 Degraw St Brooklyn, NY

PROJECT #: E9309

LOCATION: Brooklyn, NY

PROJECT MANAGER: Jarod Stanfield

E-MAIL: jstanfield@entact.com

PHONE: 570-886-0442

FAX:

BILLING INFORMATION

BILL TO: ENTACT, LLC

PO# E9309

ADDRESS: 999 Oakmont Plaza Drive, Suite 300

CITY: Westmont

STATE: IL ZIP: 60559

ATTENTION: Wendy Murray

PHONE: 800-936-8228

ANALYSIS

Metals	Flashpoint + PCB	VOC	SVOC + Chloride (Anions)	BOD+TSS	pH+TSS				
1	2	3	4	5	6	7	8	9	

PRESERVATIVES

COMMENTS

<-- Specify Preservatives
A-HCl B-HNO3
C-H2SO4 D-NaOH
E-ICE F-Other

DATA TURNAROUND INFORMATION

FAX: 5 DAYS*
HARD COPY: 5 DAYS*
EDD 5 DAYS*
* TO BE APPROVED BY ALLIANCE
STANDARD TURNAROUND TIME IS 10 BUSINESS DAYS

DATA DELIVERABLE INFORMATION

- ☐ RESULTS ONLY ☐ USEPA CLP
☐ RESULTS + QC ☐ New York State ASP "B"
☐ New Jersey REDUCED ☐ New York State ASP "A"
☐ New Jersey CLP ☐ Other _____
☐ EDD Format _____

CHEMTECH SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# of Bottles	B	E	E	E	E						
			COMP	GRAB	DATE	TIME		1	2	3	4	5	6	7	8	9		
1.	TW-WTS-03	Surface Water		X	3/6	10:00	1						X					
2.	TW-WTS-04	Surface Water		X	3/6	10:00	1	X	X	X	X	X					pH 1.6	
3.																		
4.																		
5.																		
6.																		
7.																		
8.																		
9.																		
10.																		

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER 1. Jarod Stanfield	DATE/TIME 03/06/25 15:34	RECEIVED BY 1. 3-7-25 0700	Conditions of bottles or coolers at receipt: ☐ Compliant ☐ Non Compliant ☐ Cooler Temp 5.3°C ☐ Ice in Cooler?:
RELINQUISHED BY 2.	DATE/TIME	RECEIVED BY 2.	Comments:
RELINQUISHED BY 3.	DATE/TIME	RECEIVED FOR LAB BY 3.	SHIPPED VIA: CLIENT: ☐ Hand Delivered ☐ Overnight ALLIANCE: ☐ Picked Up ☐ Overnight
Page _____ of _____			Shipment Complete ☐ YES ☐ NO

WHITE - ALLIANCE COPY FOR RETURN TO CLIENT

YELLOW - ALLIANCE COPY

PINK - SAMPLER COPY

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q1522	ENTA05	Order Date : 3/7/2025 10:29:00 AM	Project Mgr :
Client Name : ENTACT		Project Name : 540 Degraw St, Brooklyn, N	Report Type : Level 1
Client Contact : Jarod Stanfield		Receive DateTime : 3/7/2025 7:00:00 AM	EDD Type : Excel NJ
Invoice Name : ENTACT		Purchase Order :	Hard Copy Date :
Invoice Contact : Jarod Stanfield			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q1522-01	TW-WTS-03	Water	03/06/2025	10:00	VOCMS Group4		8260-Low		5 Bus. Days
Q1522-02	TW-WTS-04	Water	03/06/2025	10:00	VOCMS Group4		8260-Low		5 Bus. Days

Relinquished By :



Date / Time : 3.7.25 1232

Received By :



Date / Time : 3.7.25 12:32

Storage Area : VOA Refridgerator Room