


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031025\
Data File : BF141896.D
Acq On : 10 Mar 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

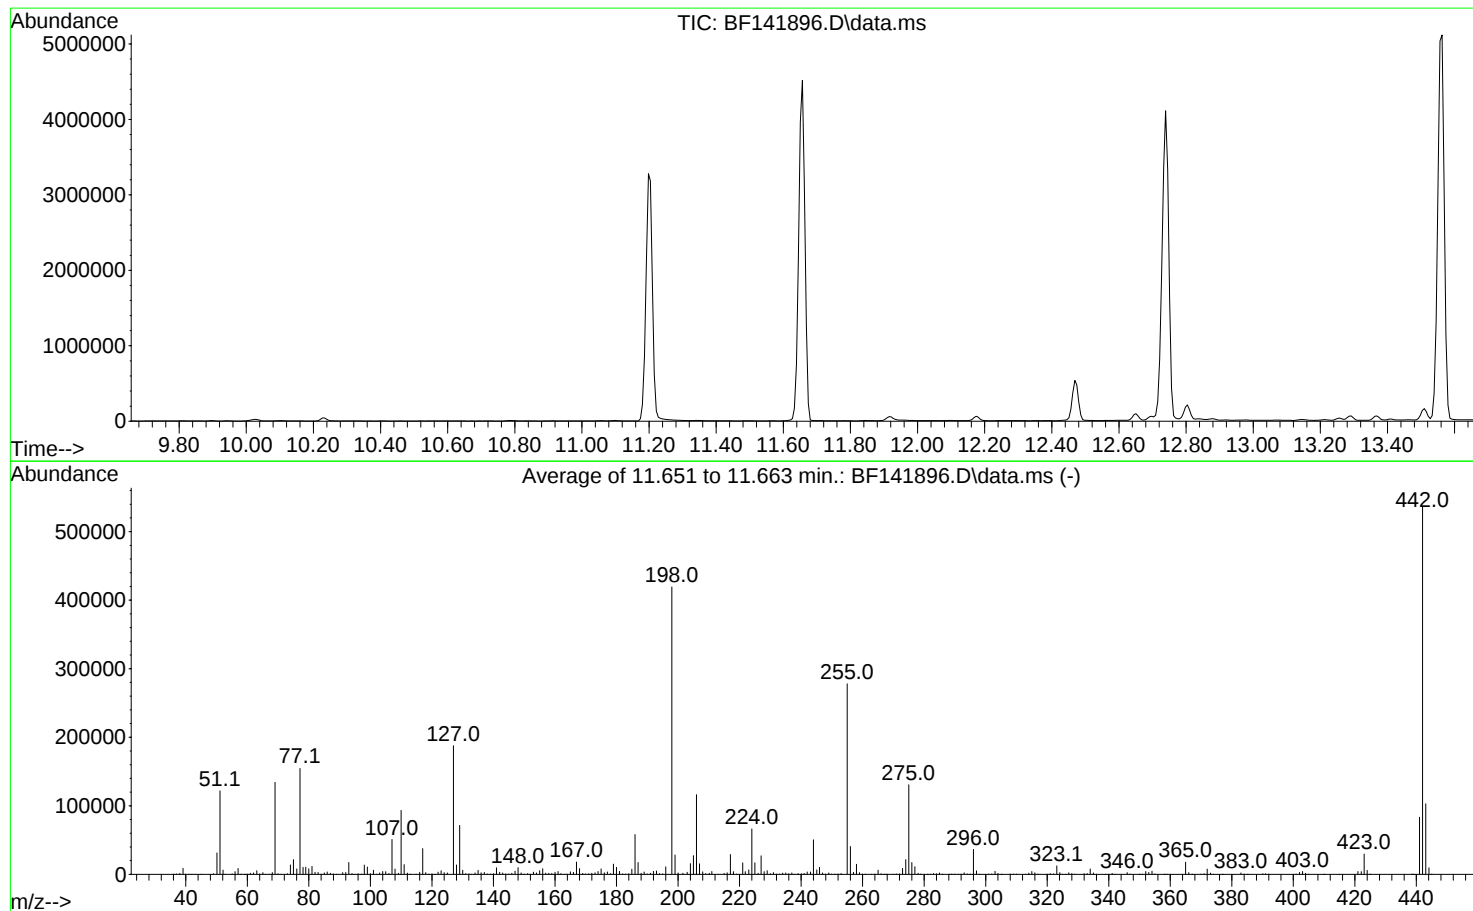

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	121957	PASS
68	69	0.00	2	1.9	2599	PASS
69	198	0.00	100	32.0	134239	PASS
70	69	0.00	2	0.7	949	PASS
127	198	10	80	44.8	187627	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	419221	PASS
199	198	5	9	6.7	28280	PASS
275	198	10	60	31.2	130819	PASS
365	198	1	100	4.2	17803	PASS
441	198	0.01	100	19.9	83389	PASS
442	442	50	100	100.0	536640	PASS
443	442	15	24	19.2	102888	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/10/2025	BNA_F	<u>BF141896.D</u>
Compound Name	Response	Retention Time
DDT	1358235	13.562
DDD	20094	13.292
DDE	930	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21024	1379259	1.52

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031025\
Data File : BF141896.D
Acq On : 10 Mar 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 10 16:16:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

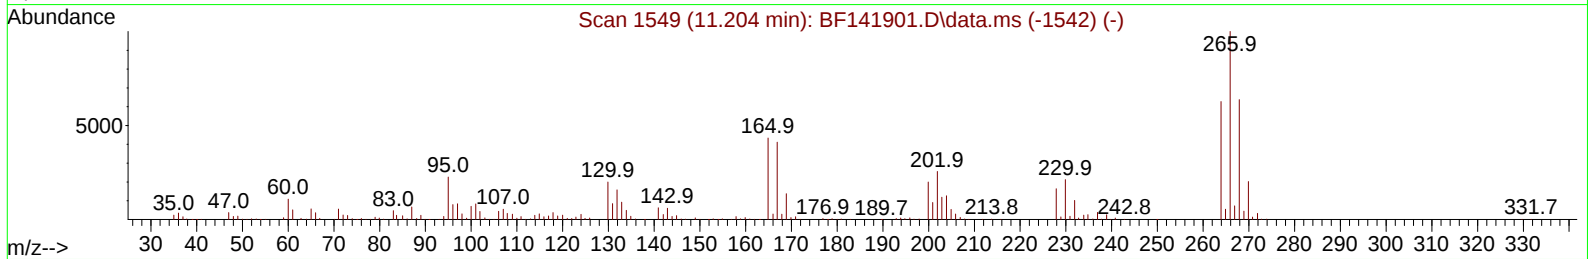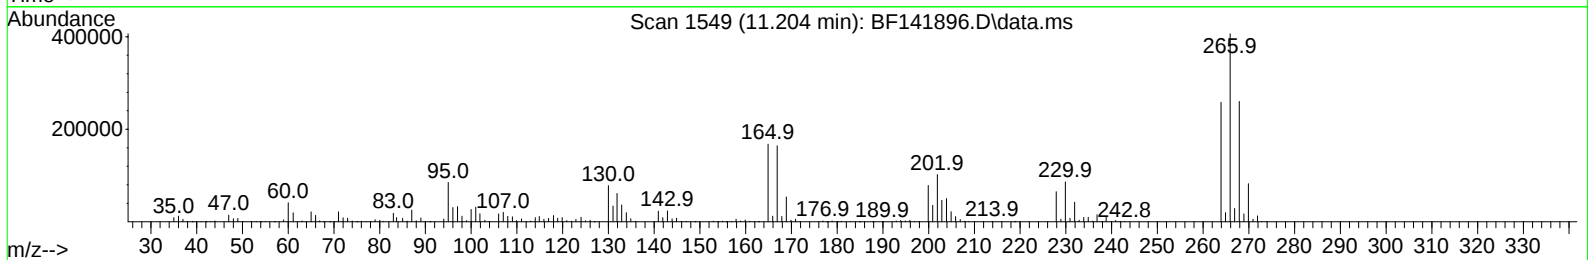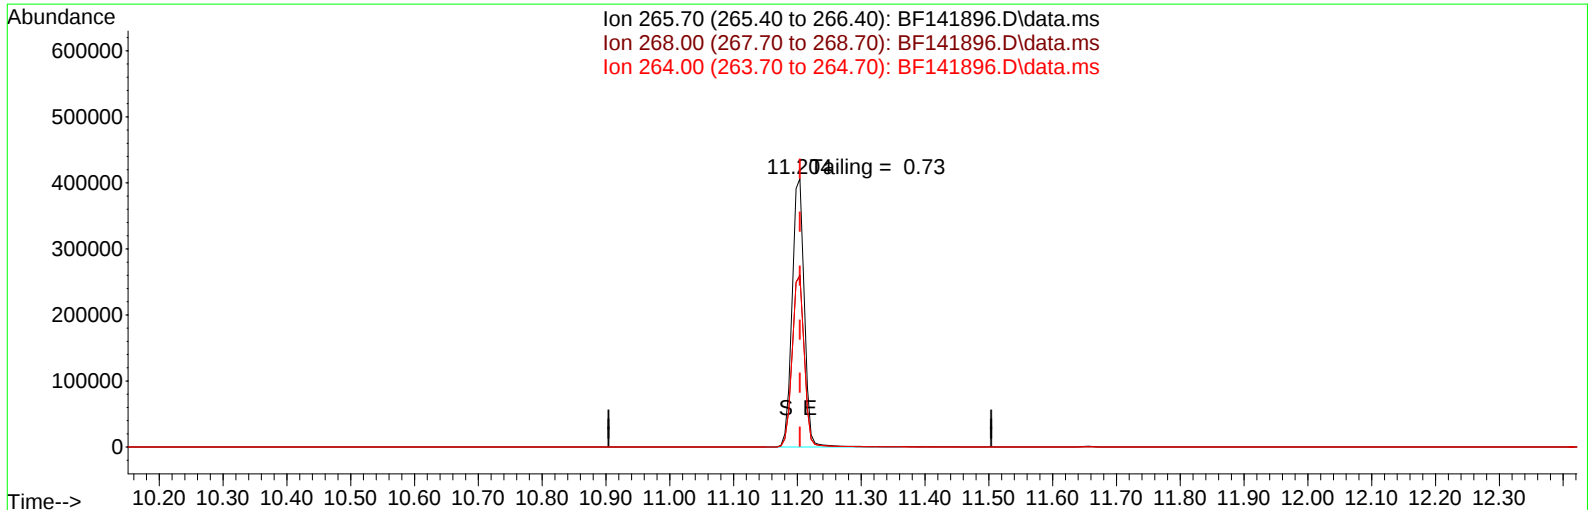

TIC: BF141896.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.000) 118650.09 ng




response 544757

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.05
264.00	62.70	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031025\
Data File : BF141896.D
Acq On : 10 Mar 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 10 16:16:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

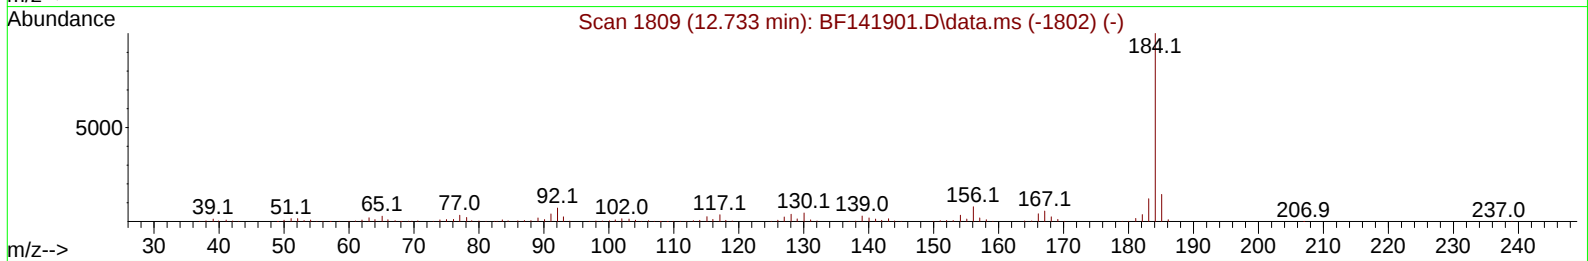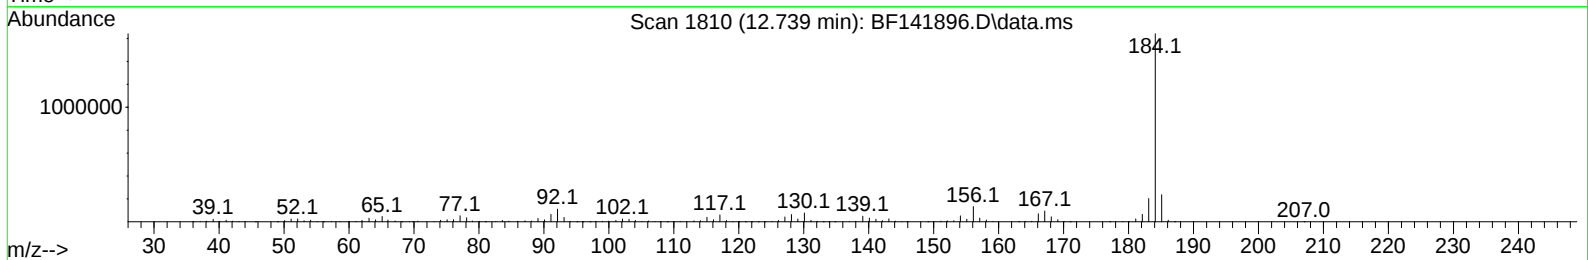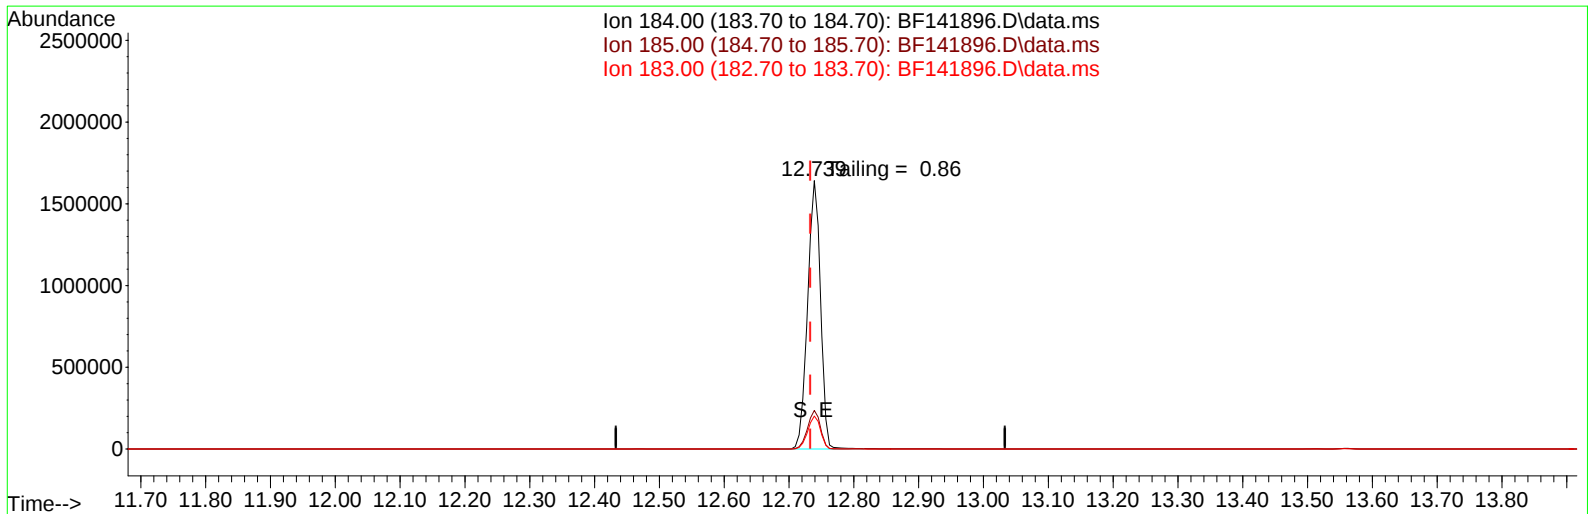

TIC: BF141896.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 203796.44 ng

response 2274676

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.38
183.00	12.10	12.32
0.00	0.00	0.00