


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031125\
Data File : BF141909.D
Acq On : 11 Mar 2025 10:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

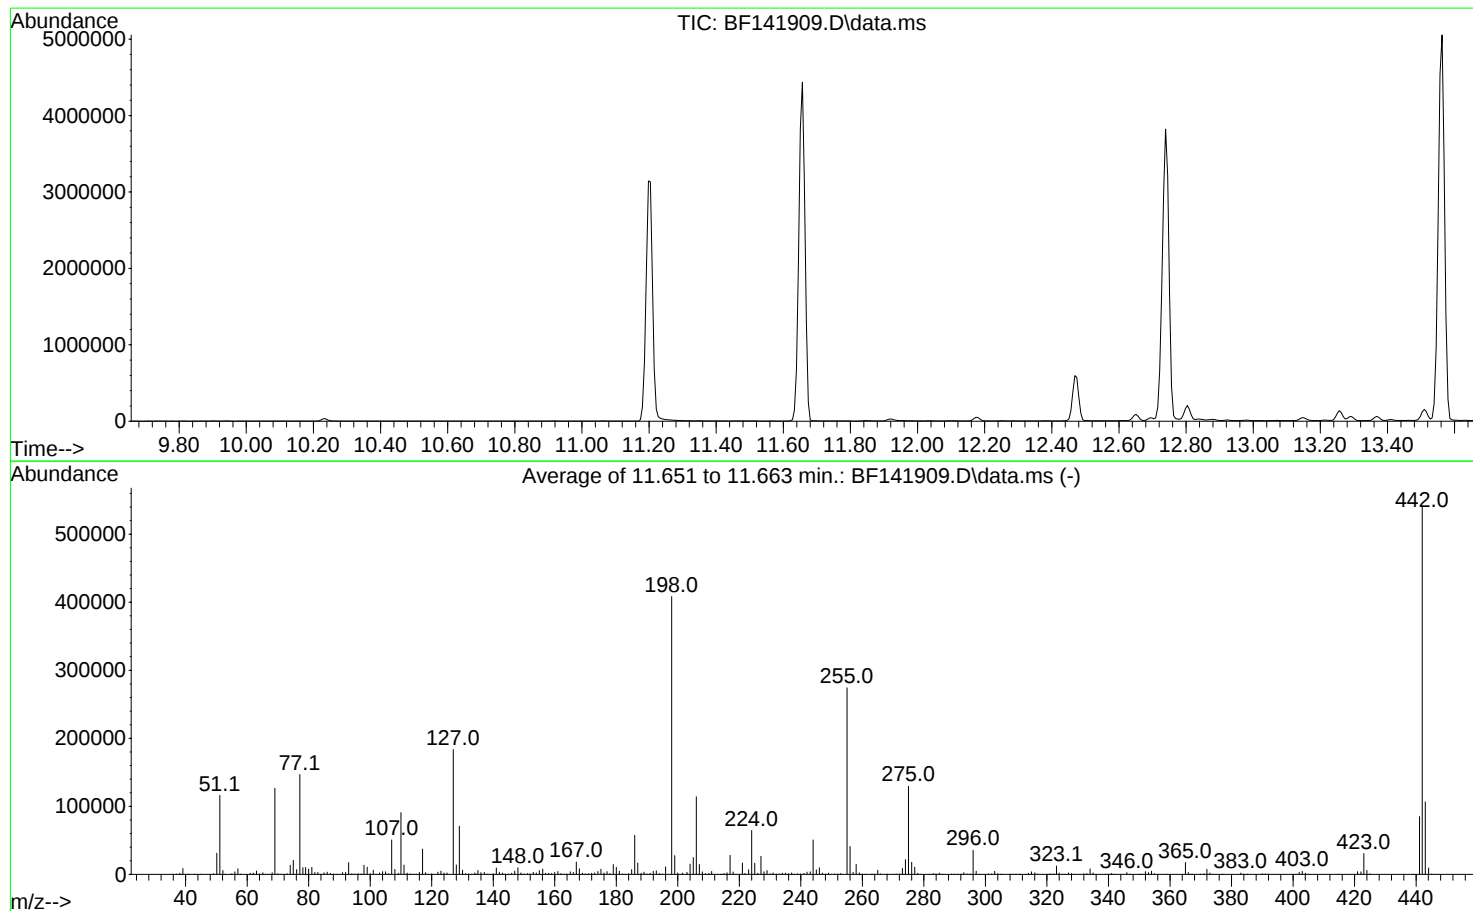

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	116181	PASS
68	69	0.00	2	2.0	2472	PASS
69	198	0.00	100	31.0	126608	PASS
70	69	0.00	2	0.7	857	PASS
127	198	10	80	44.9	183360	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	408427	PASS
199	198	5	9	6.7	27544	PASS
275	198	10	60	31.7	129467	PASS
365	198	1	100	4.3	17493	PASS
441	198	0.01	100	20.8	84915	PASS
442	442	50	100	100.0	540757	PASS
443	442	15	24	19.7	106656	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/11/2025	BNA_F	<u>BF141909.D</u>
Compound Name	Response	Retention Time
DDT	1316072	13.562
DDD	45139	13.257
DDE	1601	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
46740	1362812	3.43

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031125\
Data File : BF141909.D
Acq On : 11 Mar 2025 10:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 11 12:35:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

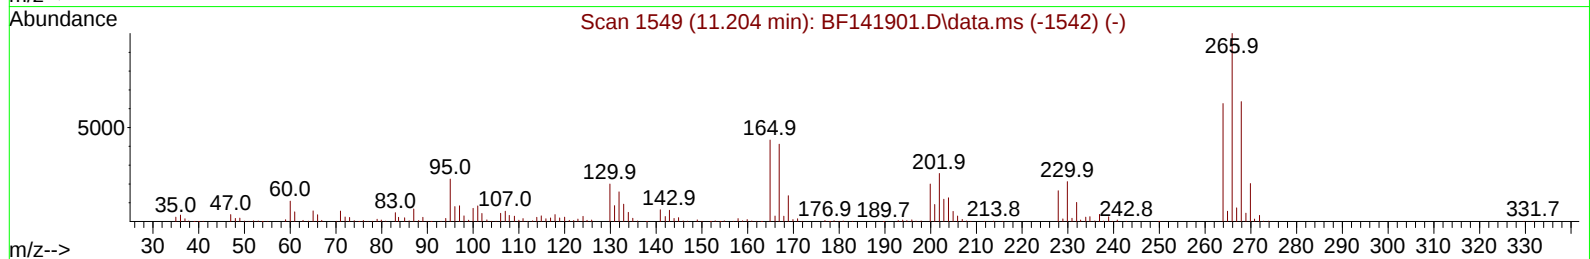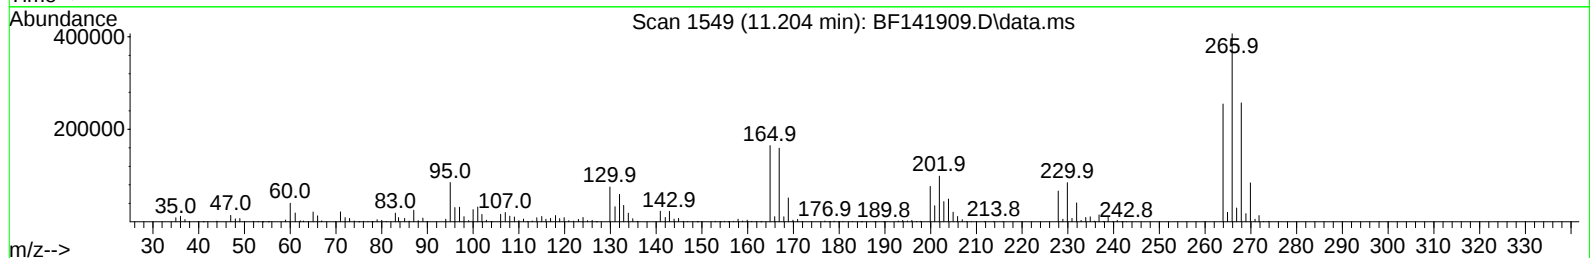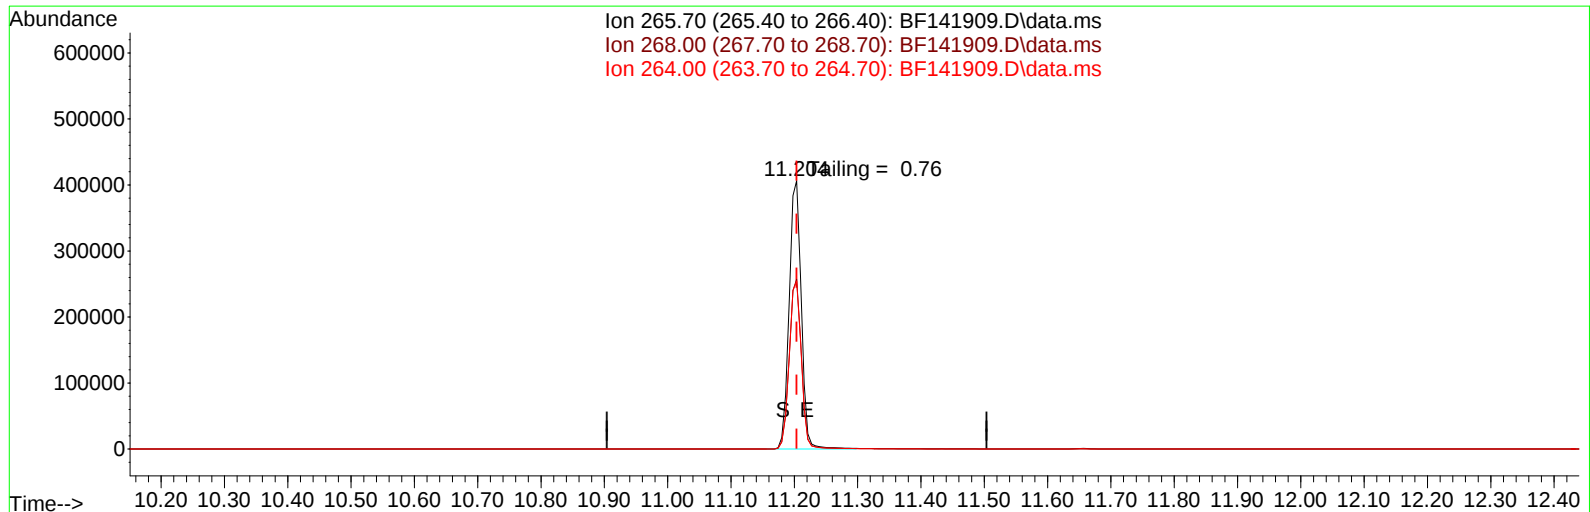

TIC: BF141909.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.000) 72528.27 ng




response 545354

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.26
264.00	62.70	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031125\
Data File : BF141909.D
Acq On : 11 Mar 2025 10:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 11 12:35:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

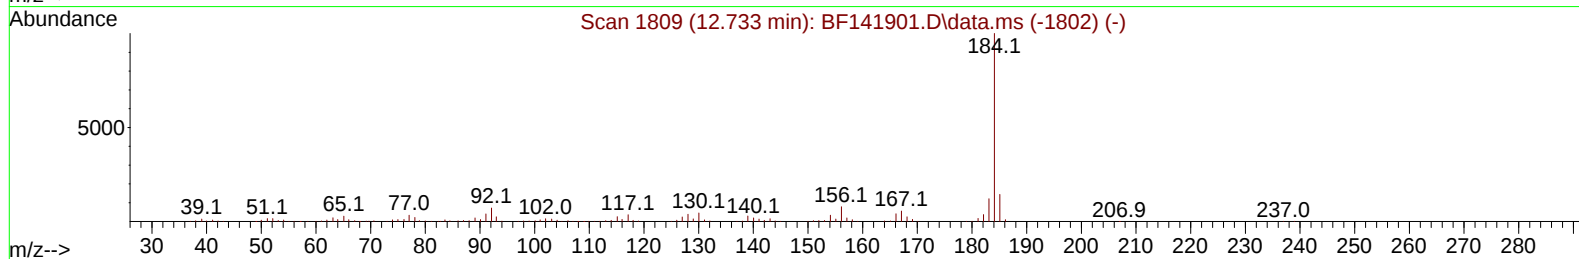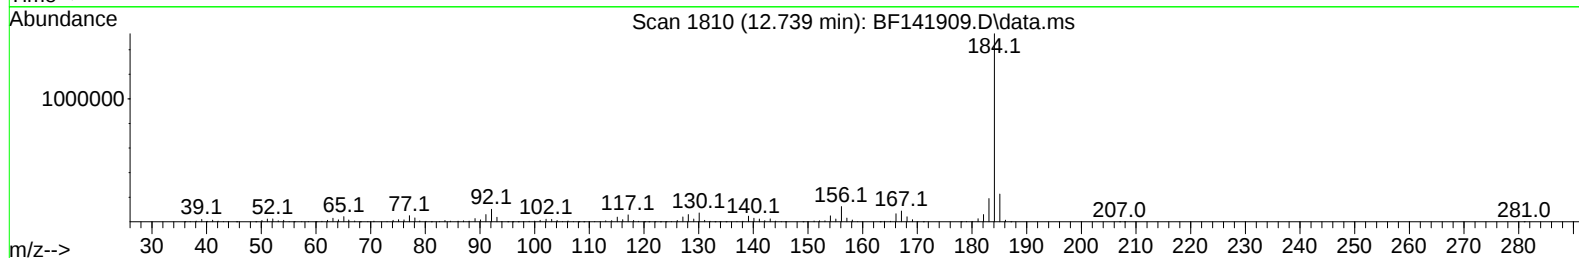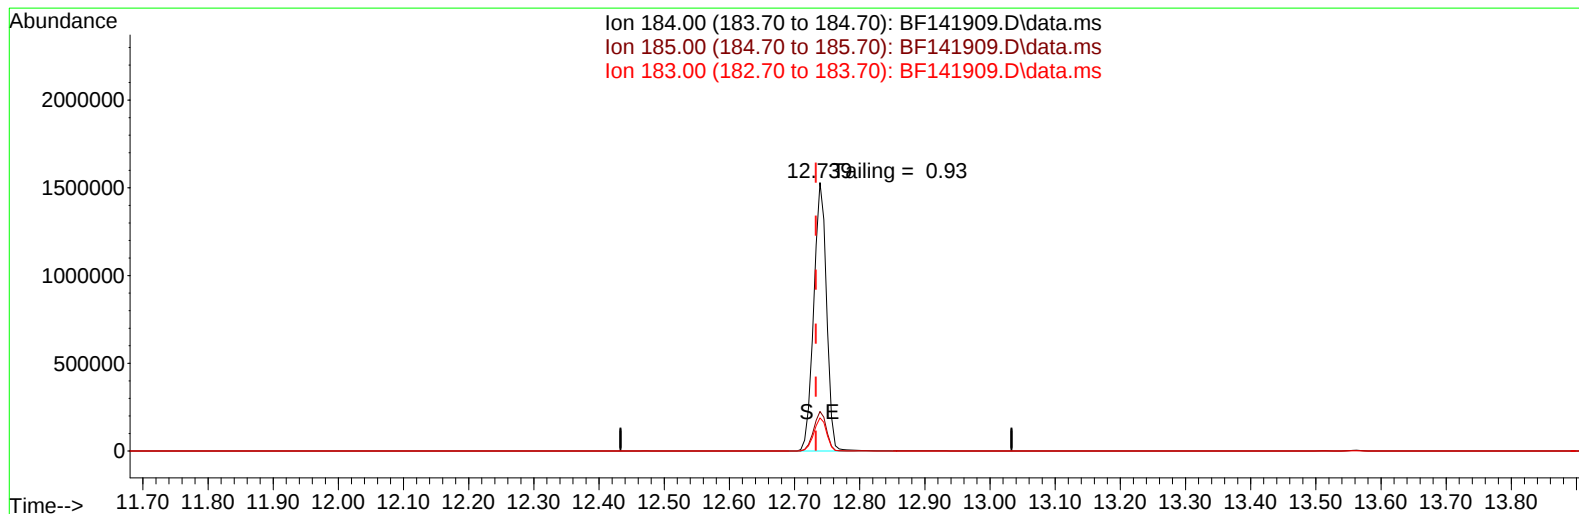

TIC: BF141909.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 151707.91 ng

response 2103912

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.76
183.00	12.10	12.39
0.00	0.00	0.00