
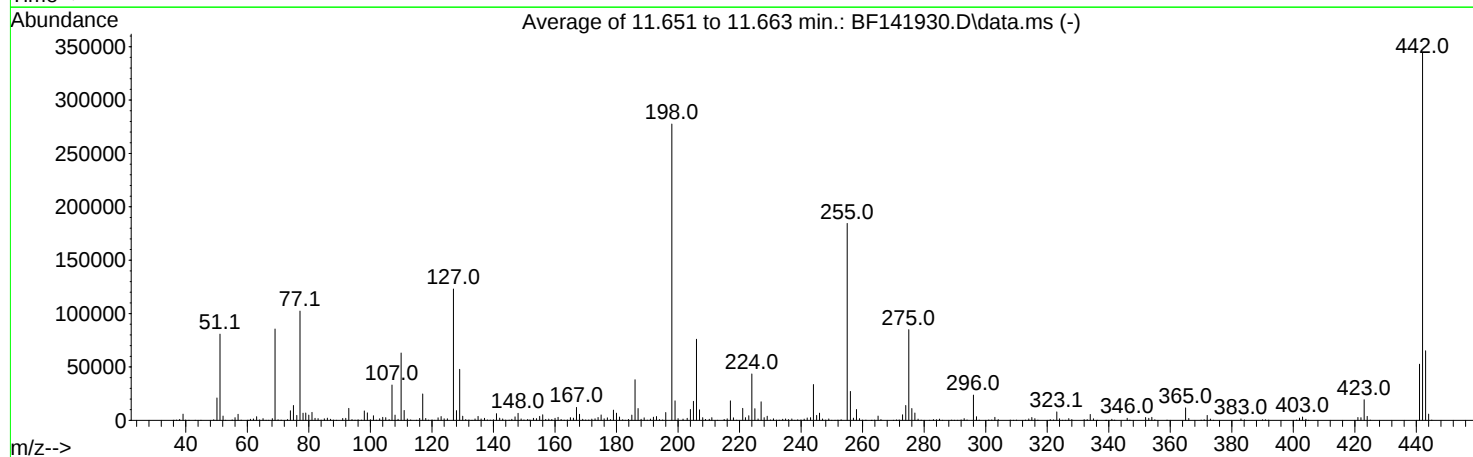


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031225\
Data File : BF141930.D
Acq On : 12 Mar 2025 09:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

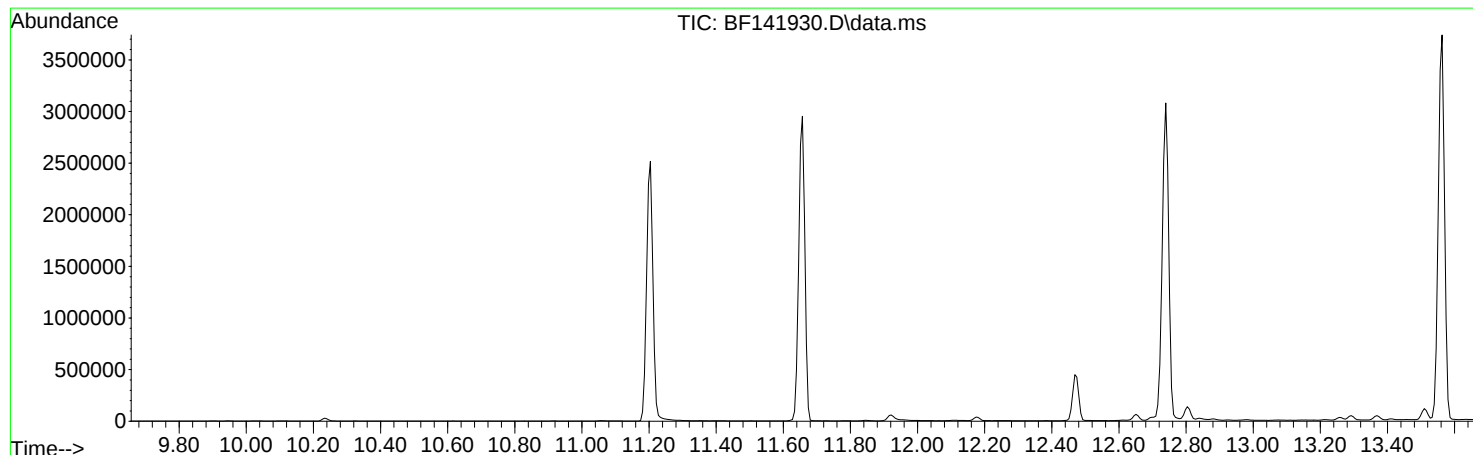




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	80832	PASS
68	69	0.00	2	2.0	1697	PASS
69	198	0.00	100	30.8	85598	PASS
70	69	0.00	2	0.8	654	PASS
127	198	10	80	44.4	123117	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	277568	PASS
199	198	5	9	6.6	18257	PASS
275	198	10	60	30.6	84933	PASS
365	198	1	100	4.2	11734	PASS
441	198	0.01	100	18.9	52571	PASS
442	442	50	100	100.0	344533	PASS
443	442	15	24	18.9	65261	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031225\
Data File : BF141930.D
Acq On : 12 Mar 2025 09:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 12 12:20:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

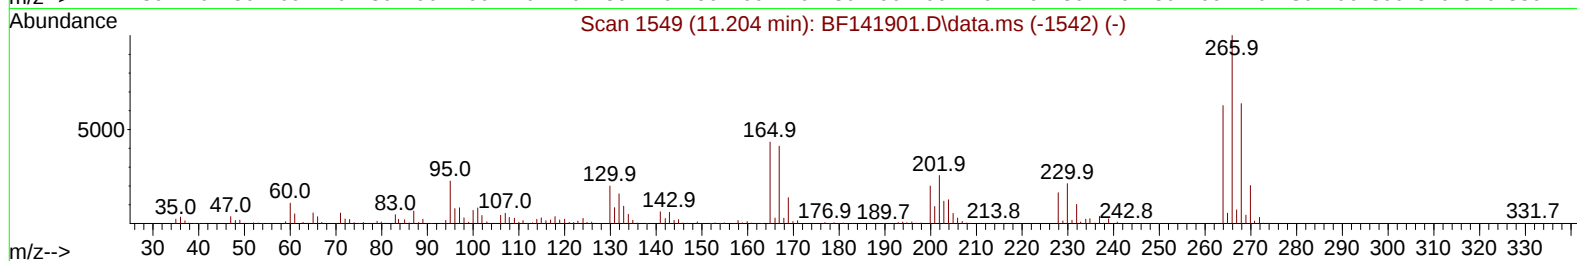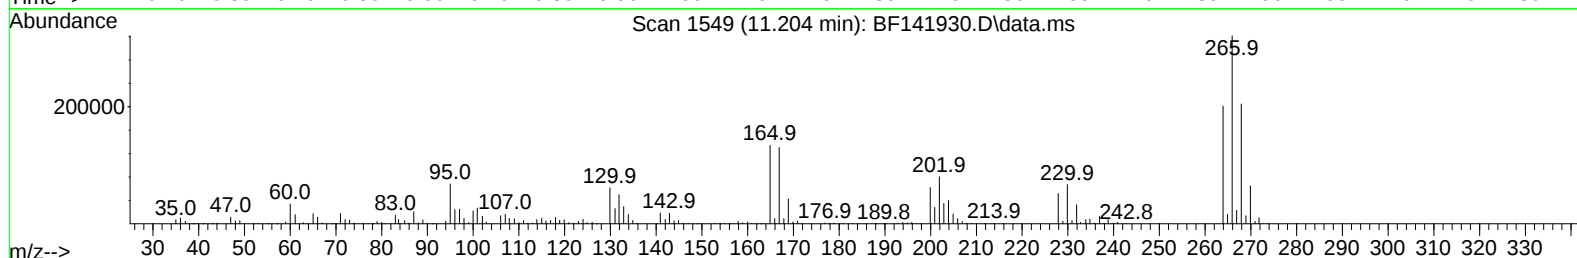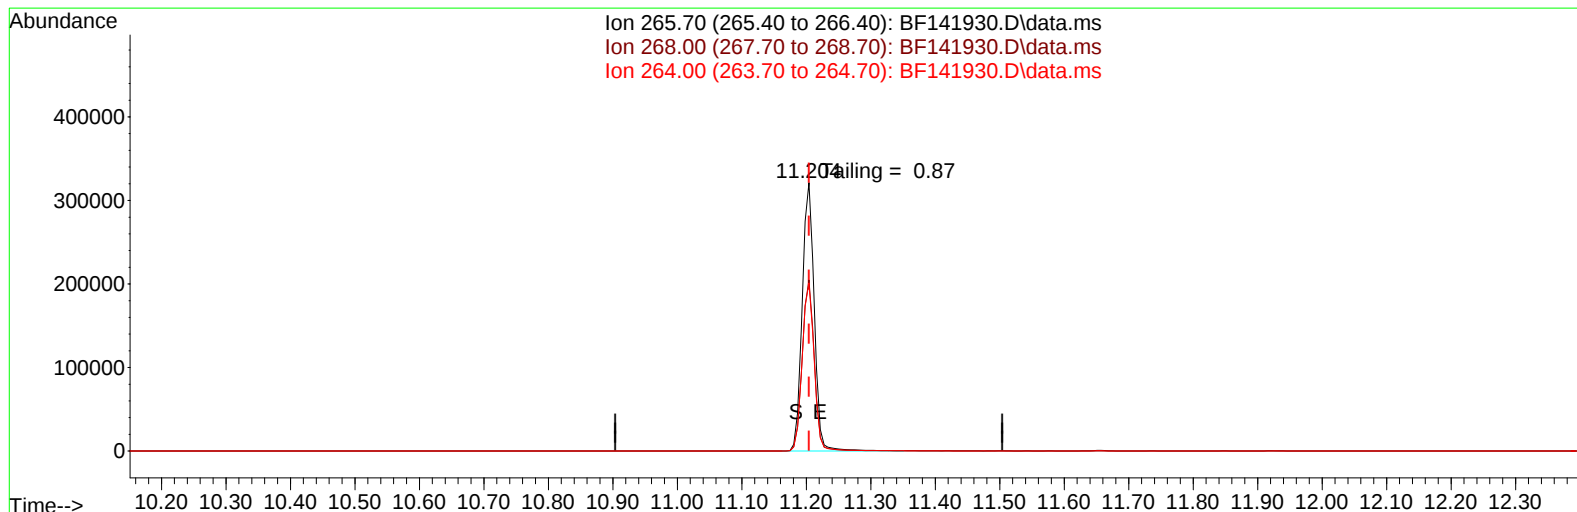

TIC: BF141930.D\data.ms

(70) Pentachlorophenol (C)

11.204min (+ 0.000) 52450.63 ng




response 420204

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.69
264.00	62.70	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031225\
Data File : BF141930.D
Acq On : 12 Mar 2025 09:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 12 12:20:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

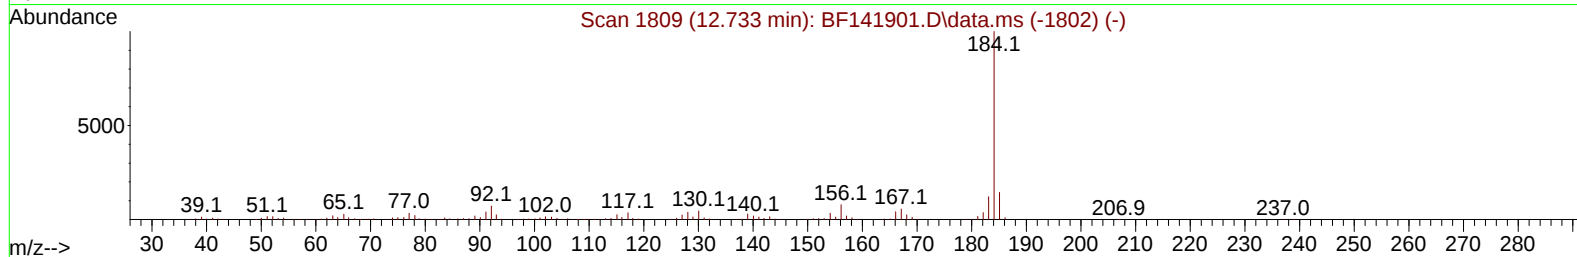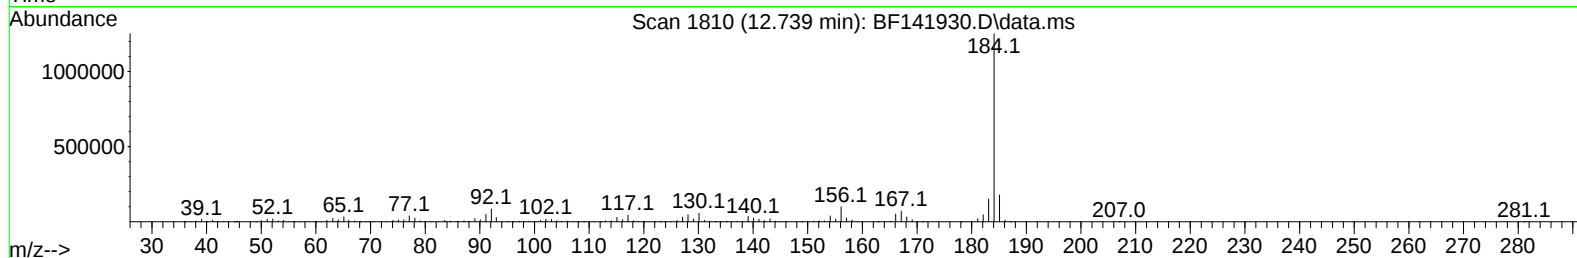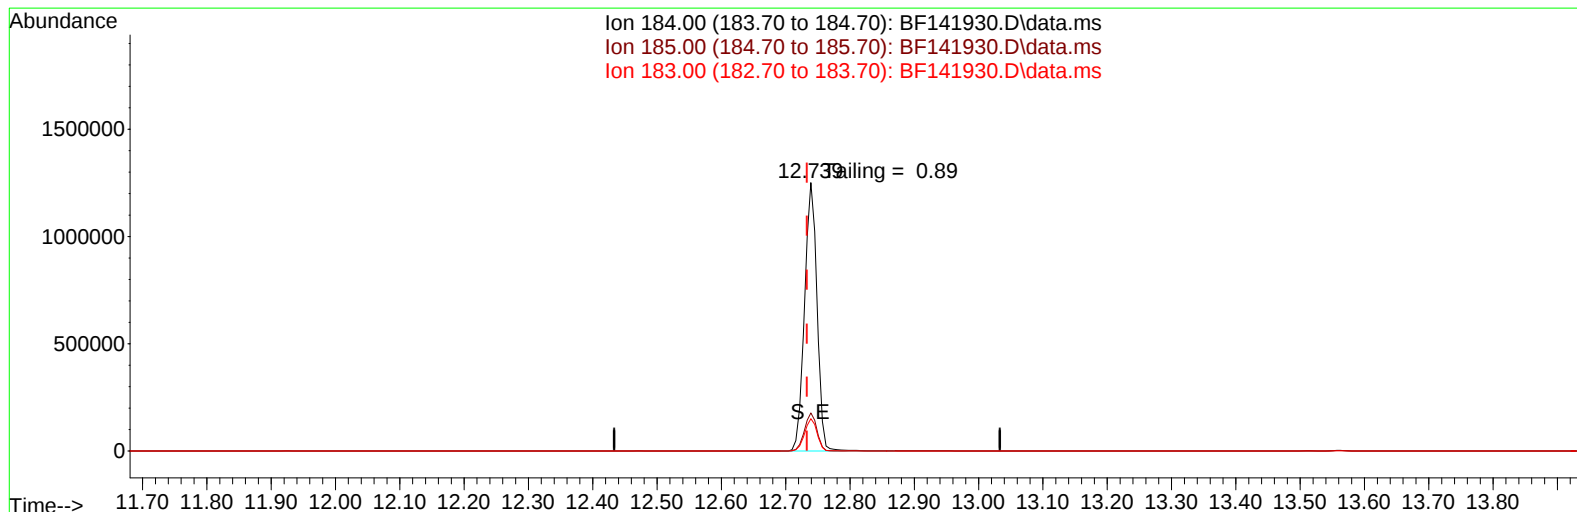

TIC: BF141930.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 143344.46 ng

response 1699937

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.21
183.00	12.10	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/12/2025	BNA_F	<u>BF141930.D</u>
Compound Name	Response	Retention Time
DDT	971282	13.563
DDD	17643	13.292
DDE	640	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18283	989565	1.85

Instrument :
BNA_F
ClientSampleId :
DFTPP