
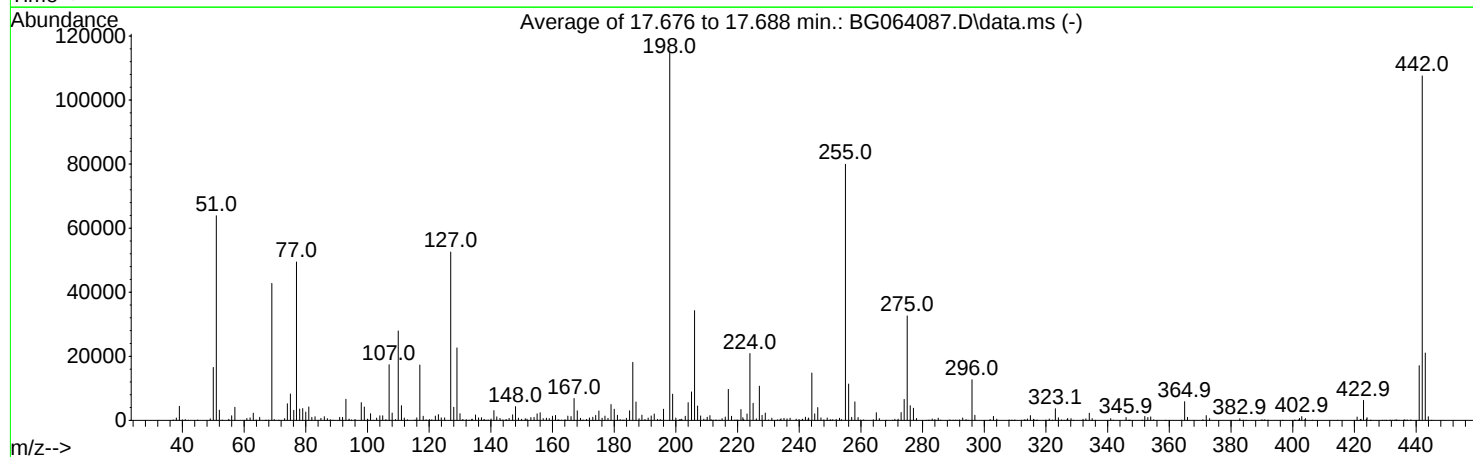


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031125\
Data File : BG064087.D
Acq On : 11 Mar 2025 7:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 05 15:39:19 2025

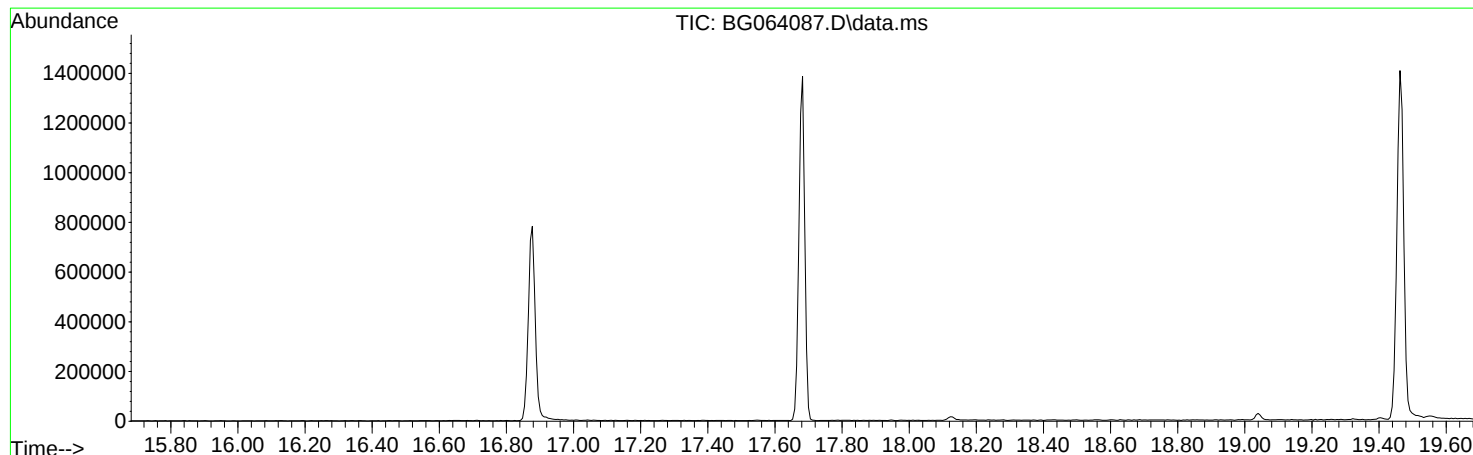

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.6	63893	PASS
68	69	0.00	2	0.3	110	PASS
69	198	0.00	100	37.2	42763	PASS
70	69	0.00	2	0.5	232	PASS
127	198	10	80	45.8	52544	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	114843	PASS
199	198	5	9	7.1	8178	PASS
275	198	10	60	28.4	32643	PASS
365	198	1	100	5.1	5870	PASS
441	198	0.01	100	14.9	17072	PASS
442	442	50	100	100.0	107528	PASS
443	442	15	24	19.5	21019	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/11/2025	BNA_G	<u>BG064087.D</u>
Compound Name	Response	Retention Time
DDT	322741	20.696
DDD	22420	20.262
DDE	0	19.753
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22420	345161	6.50

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031125\
Data File : BG064087.D
Acq On : 11 Mar 2025 7:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 11 10:54:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

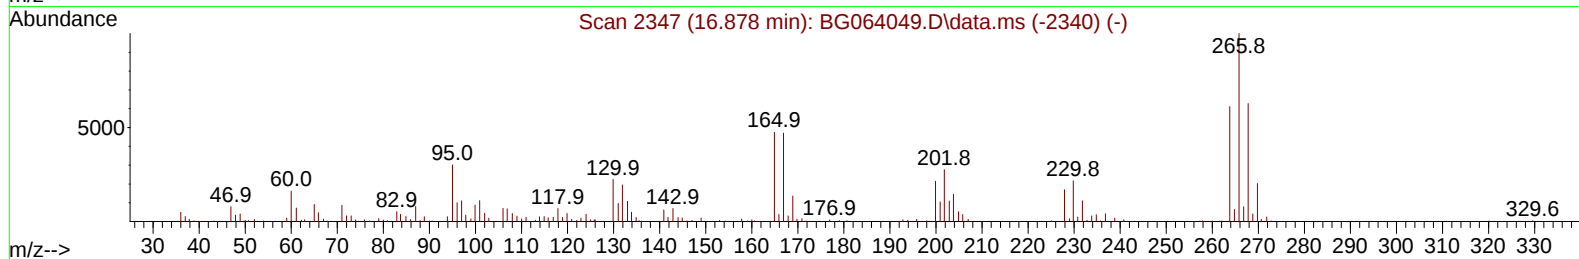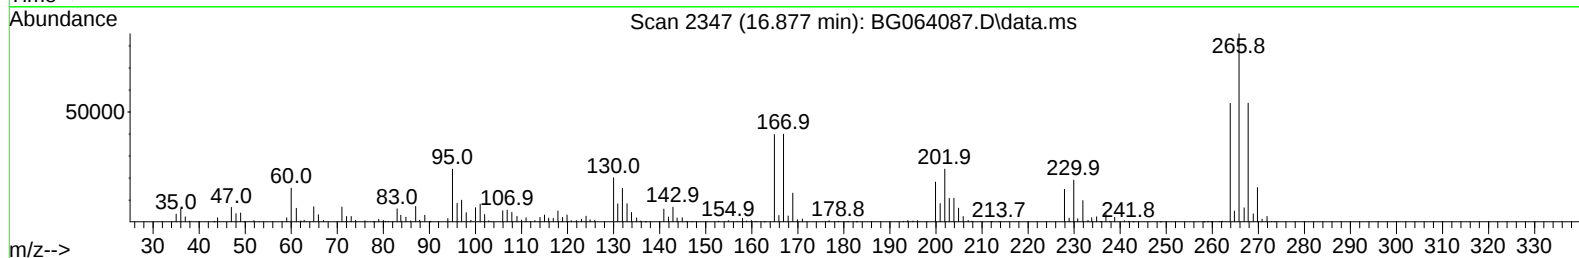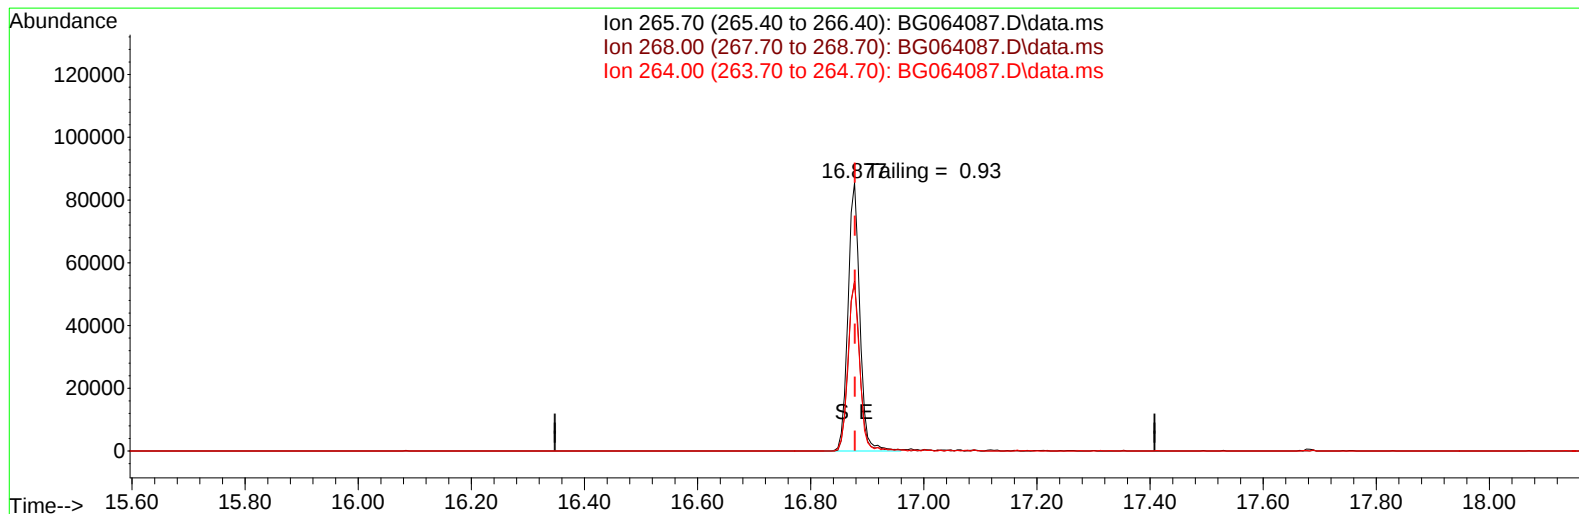

TIC: BG064087.D\data.ms

(70) Pentachlorophenol (C)

16.877min (-0.001) 19891.78 ng




response 124621

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	63.13
264.00	61.10	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031125\
Data File : BG064087.D
Acq On : 11 Mar 2025 7:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 11 10:54:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

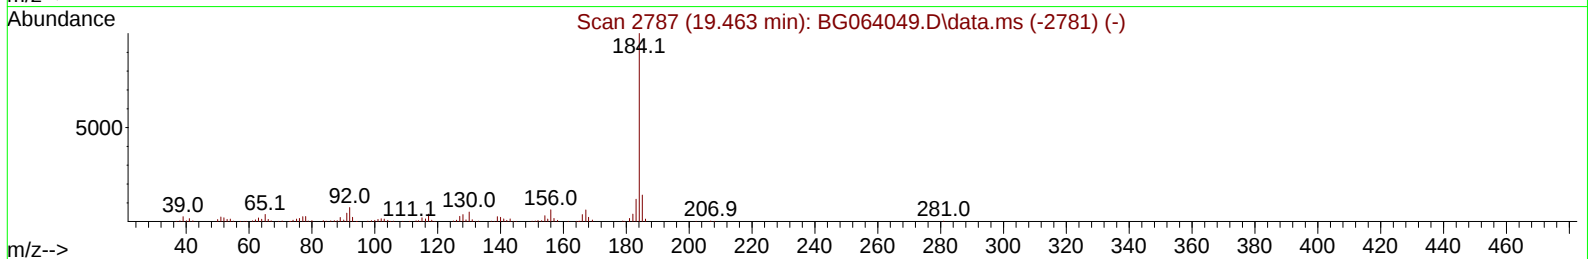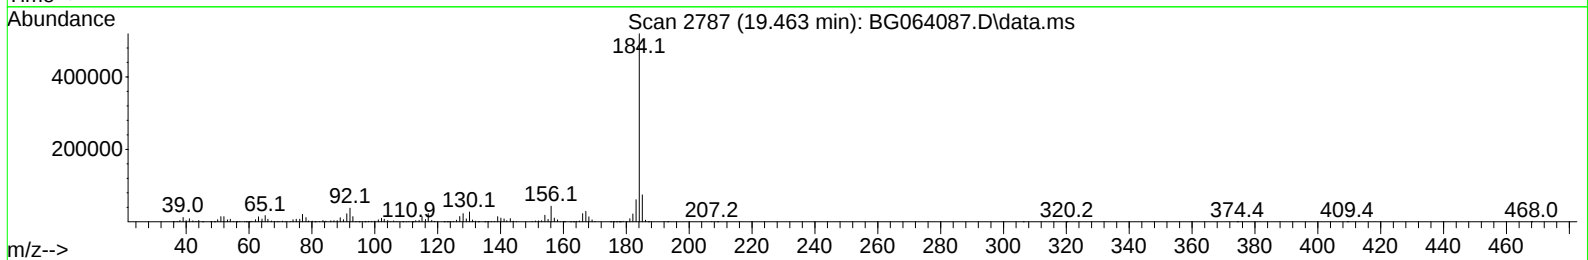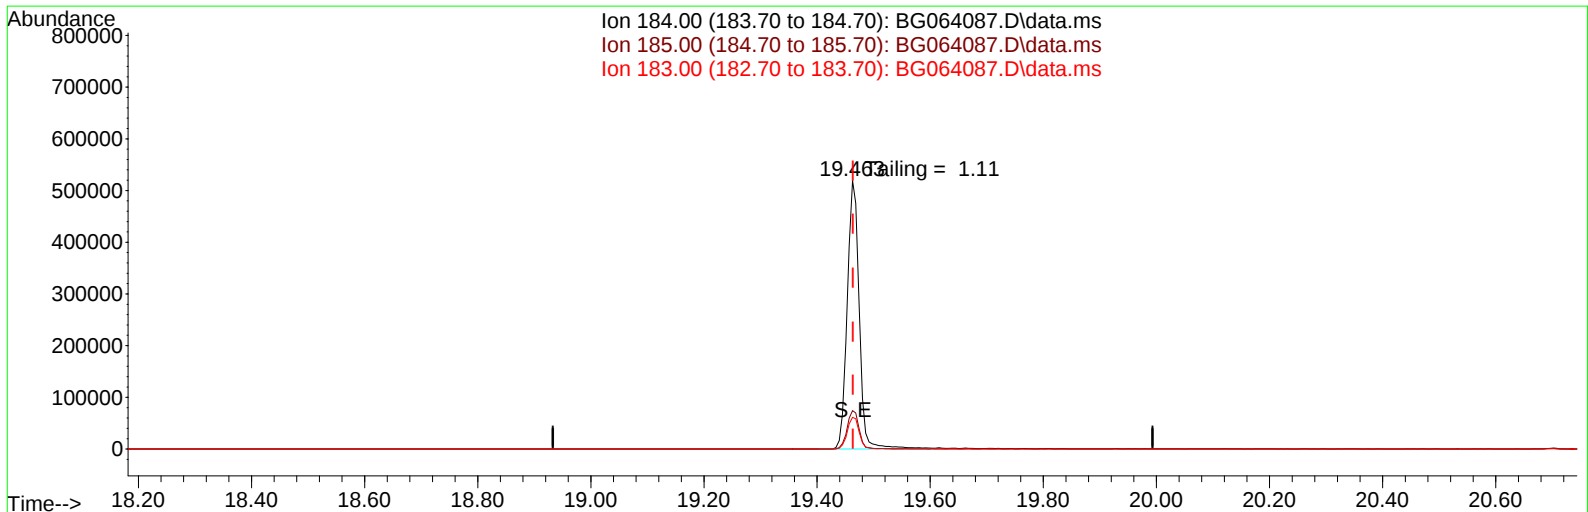

TIC: BG064087.D\data.ms

(77) Benzidine

19.463min (-0.000) 1010322.83 ng m

response 769455

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.30
183.00	11.90	11.82
0.00	0.00	0.00