
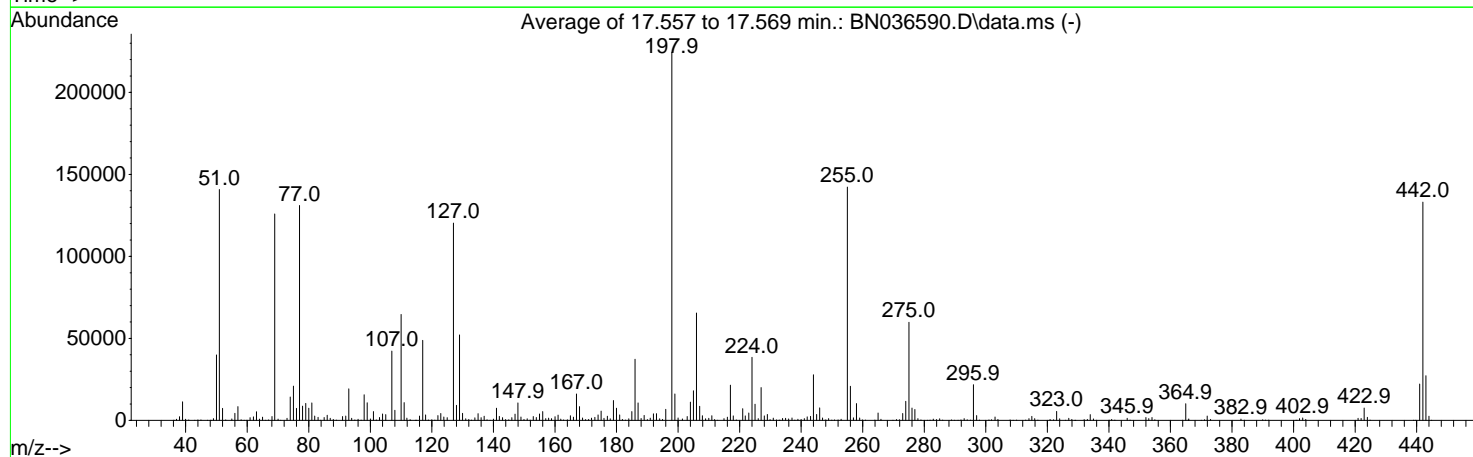


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN031225\  
 Data File : BN036590.D  
 Acq On : 12 Mar 2025 08:35  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN031025.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Mar 10 16:06:28 2025

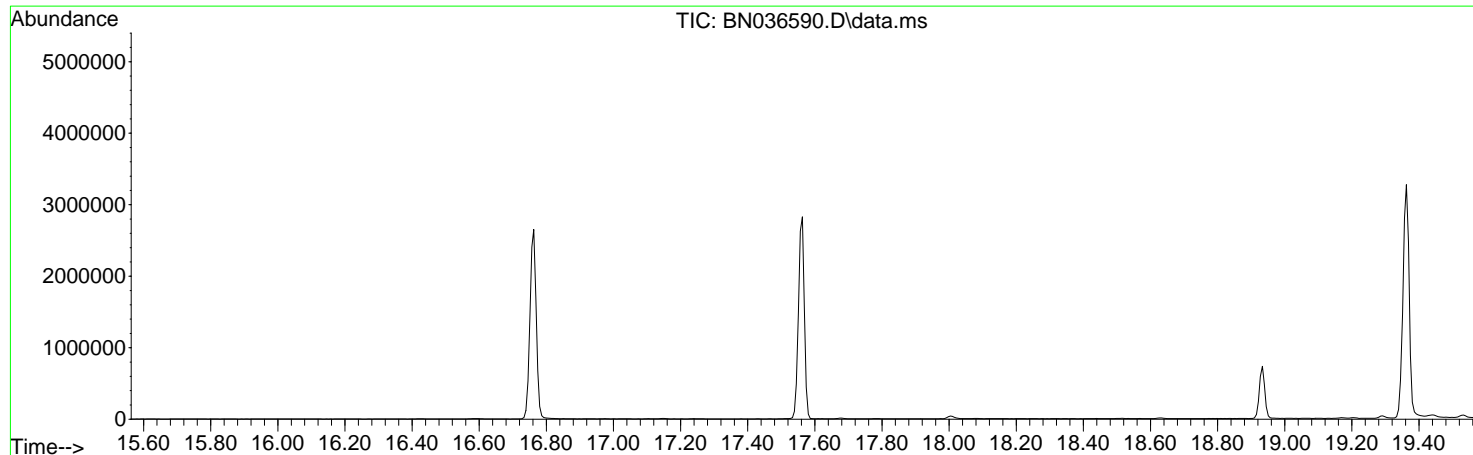




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.8	140749	PASS
68	69	0.00	2	1.8	2300	PASS
69	198	0.00	100	56.1	125881	PASS
70	69	0.00	2	0.6	788	PASS
127	198	10	80	53.6	120285	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	224299	PASS
199	198	5	9	7.2	16143	PASS
275	198	10	60	26.6	59765	PASS
365	198	1	100	4.5	10115	PASS
441	198	0.01	100	9.9	22131	PASS
442	442	50	100	100.0	133088	PASS
443	442	15	24	20.4	27203	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN031225\  
 Data File : BN036590.D  
 Acq On : 12 Mar 2025 08:35  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Mar 12 18:30:53 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 25 04:23:53 2024  
 Response via : Initial Calibration

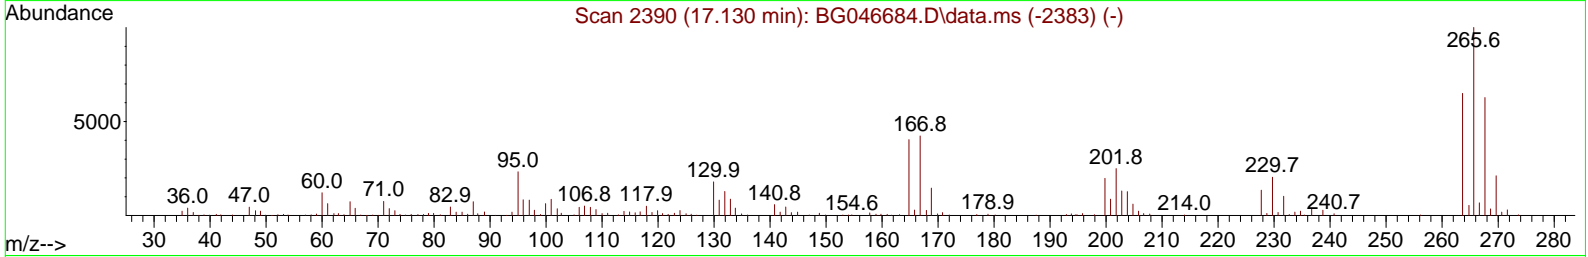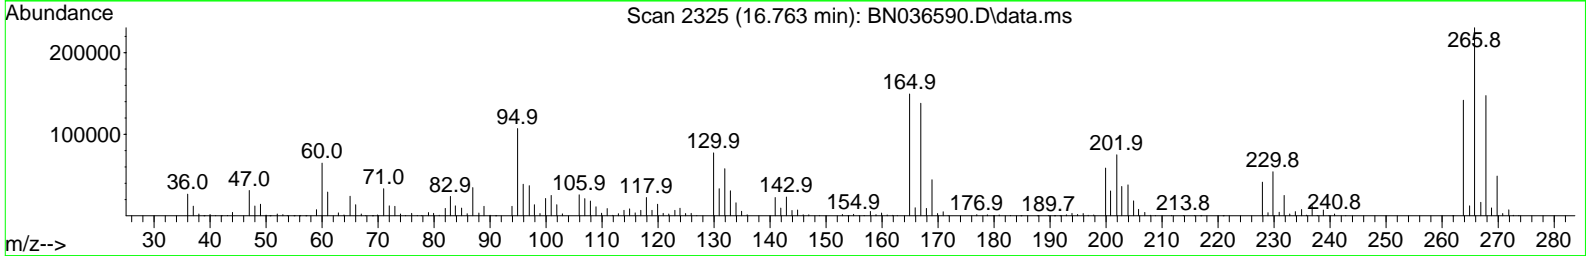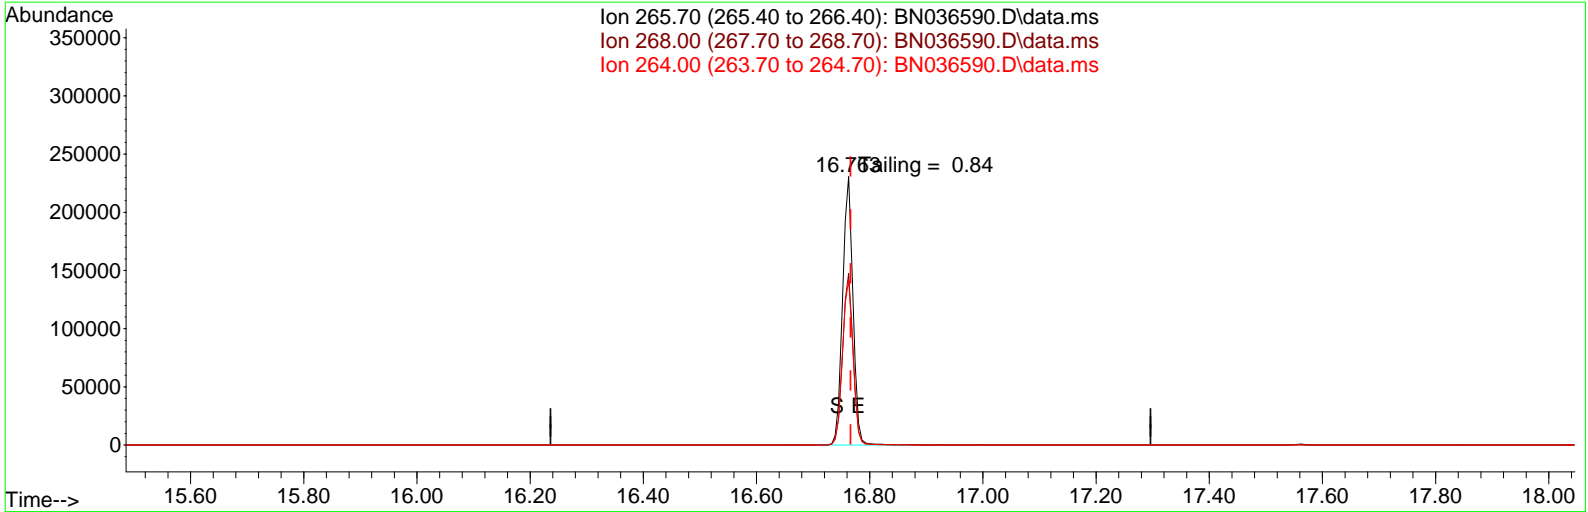

TIC: BN036590.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.003) 21862.92 ng




response 295280

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.93
264.00	61.60	61.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN031225\  
 Data File : BN036590.D  
 Acq On : 12 Mar 2025 08:35  
 Operator : RC/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_N  
**ClientSampleId :**  
 DFTPP

Quant Time: Mar 12 18:30:53 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Dec 25 04:23:53 2024  
 Response via : Initial Calibration

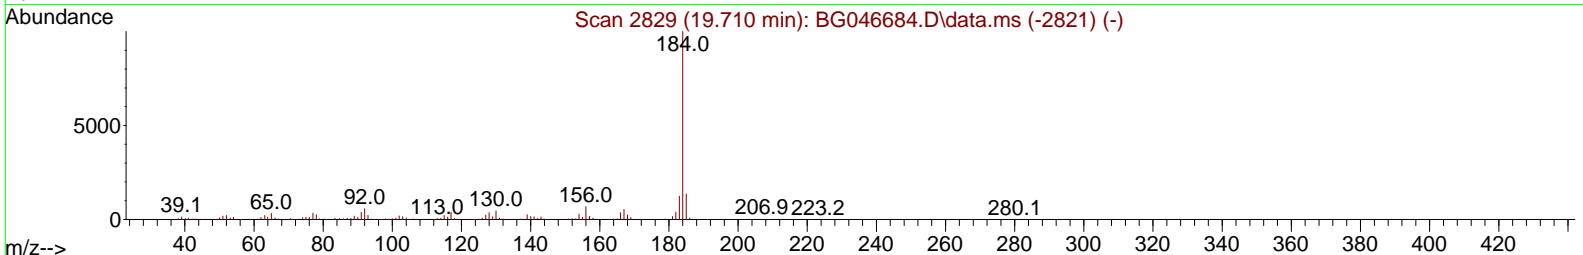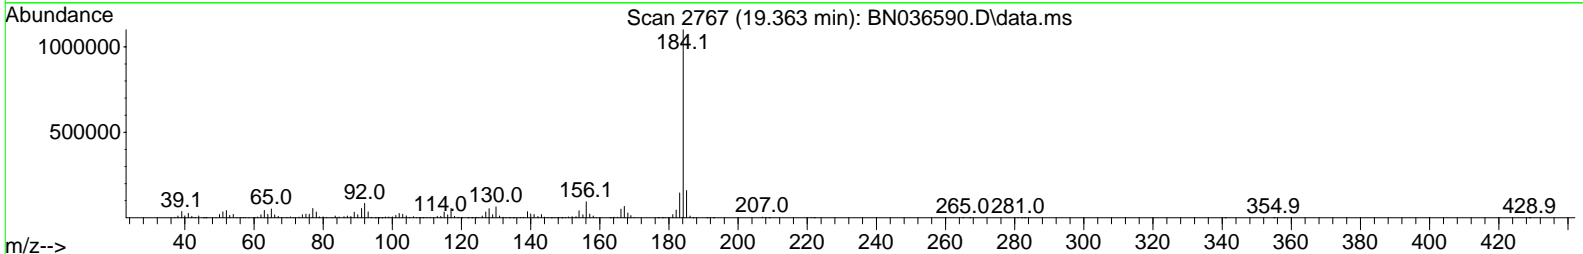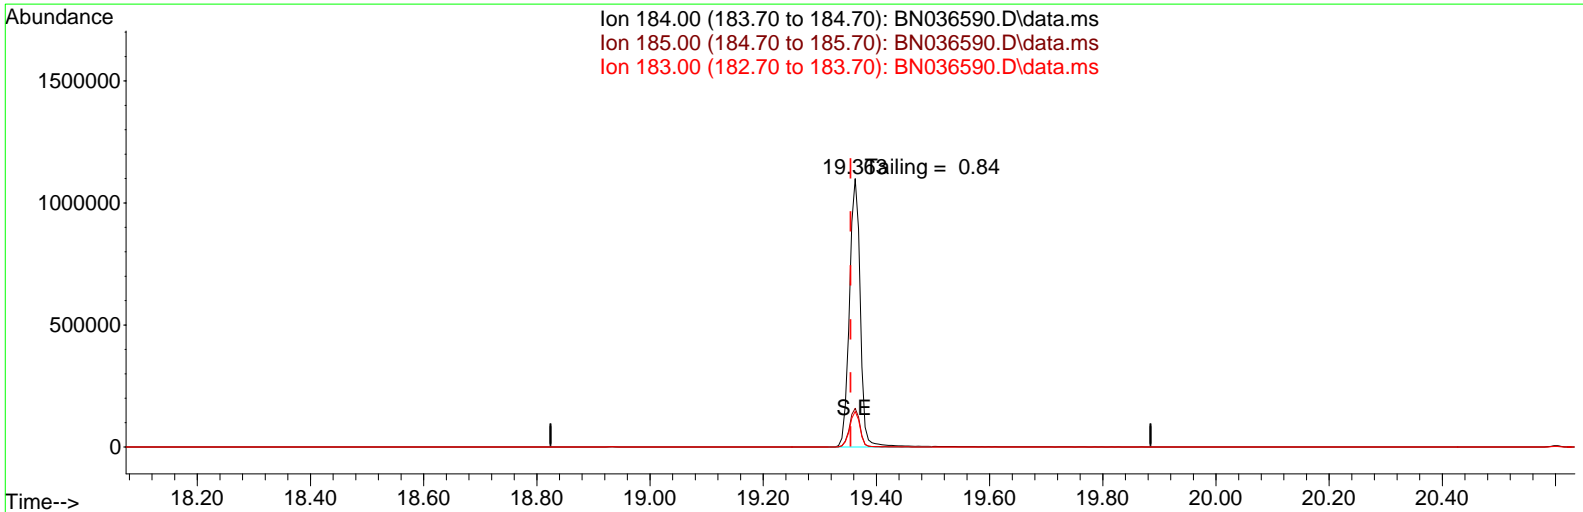

TIC: BN036590.D\data.ms

(77) Benzidine

19.363min (+ 0.008) 0.00 ng

response 1469311

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.46
183.00	13.20	13.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/12/2025	BNA_N	<u>BN036590.D</u>
Compound Name	Response	Retention Time
DDT	1023398	20.598
DDD	10765	20.21
DDE	484	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11249	1034647	1.09

Instrument :  
 BNA\_N  
 ClientSampled :  
 DFTPP