
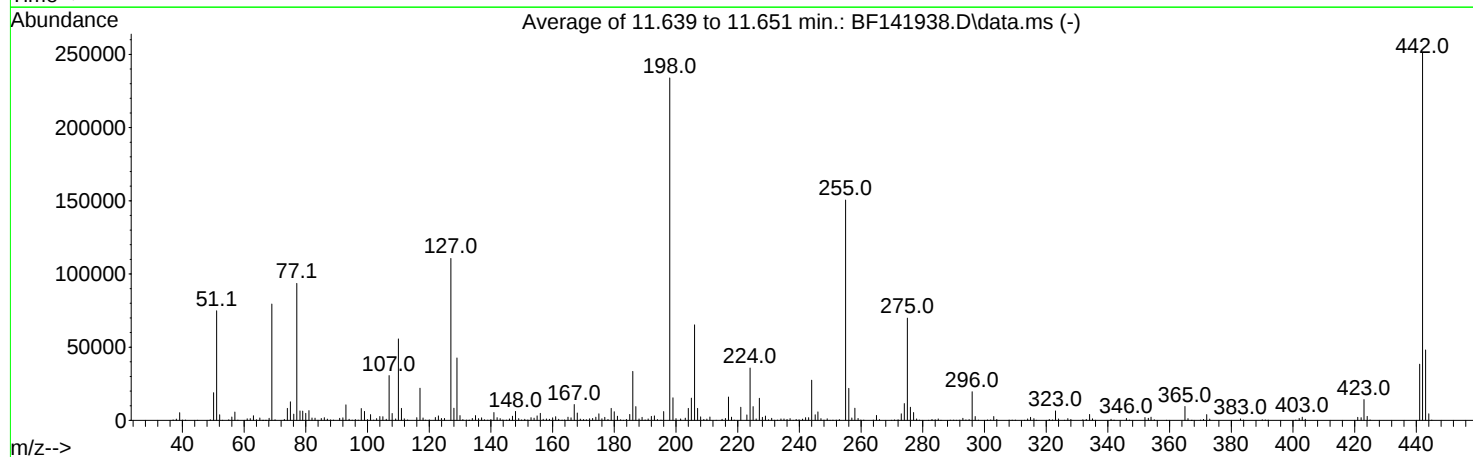


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031325\
Data File : BF141938.D
Acq On : 13 Mar 2025 11:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

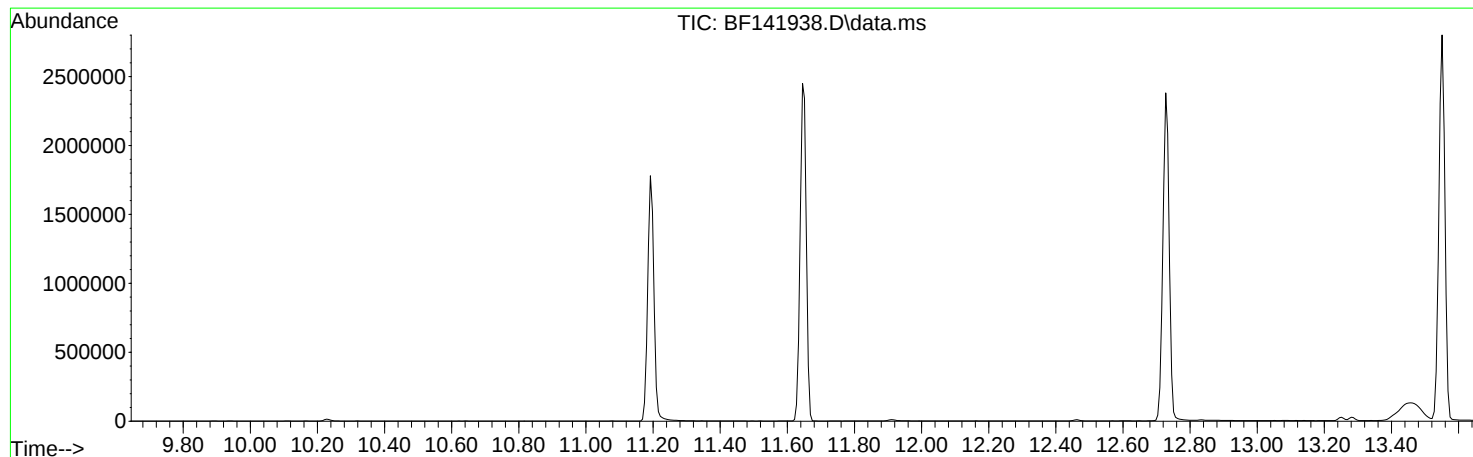



AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	74819	PASS
68	69	0.00	2	1.8	1404	PASS
69	198	0.00	100	34.0	79429	PASS
70	69	0.00	2	0.6	451	PASS
127	198	10	80	47.3	110651	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	233877	PASS
199	198	5	9	6.6	15462	PASS
275	198	10	60	29.9	69864	PASS
365	198	1	100	4.1	9507	PASS
441	198	0.01	100	16.4	38323	PASS
442	442	50	100	100.0	251264	PASS
443	442	15	24	19.1	48053	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031325\
Data File : BF141938.D
Acq On : 13 Mar 2025 11:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 13 13:04:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

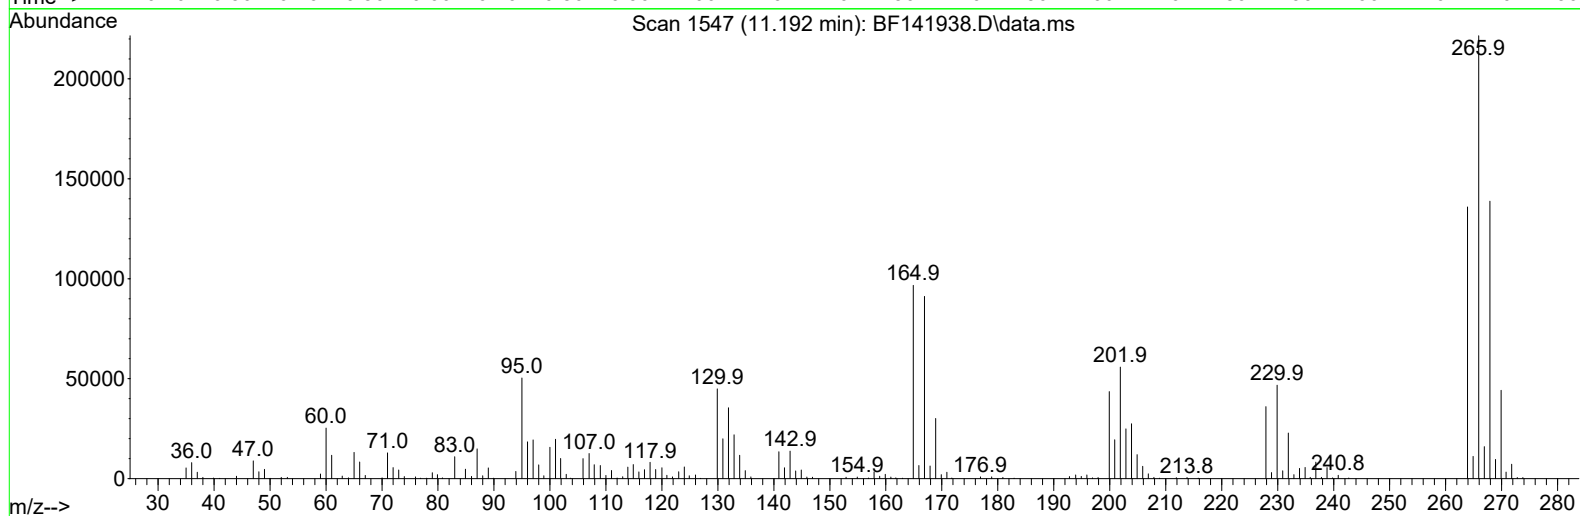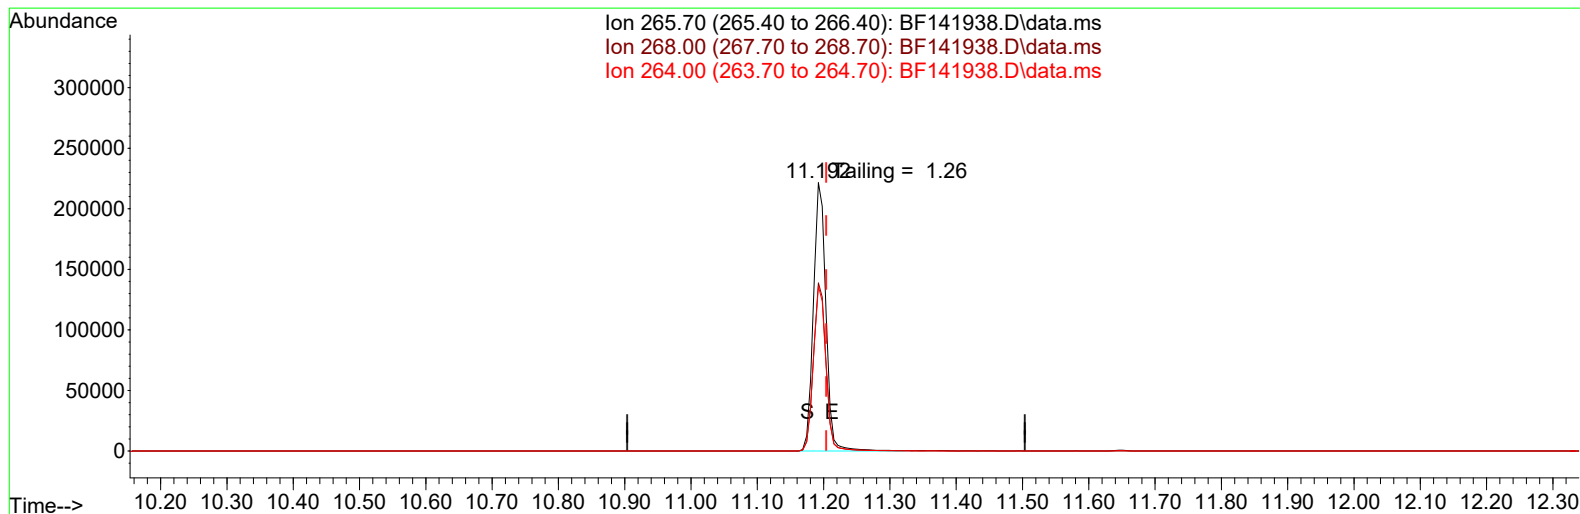

TIC: BF141938.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.012) 133427.78 ng



response 291016

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.65
264.00	62.70	61.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031325\
Data File : BF141938.D
Acq On : 13 Mar 2025 11:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 13 13:04:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

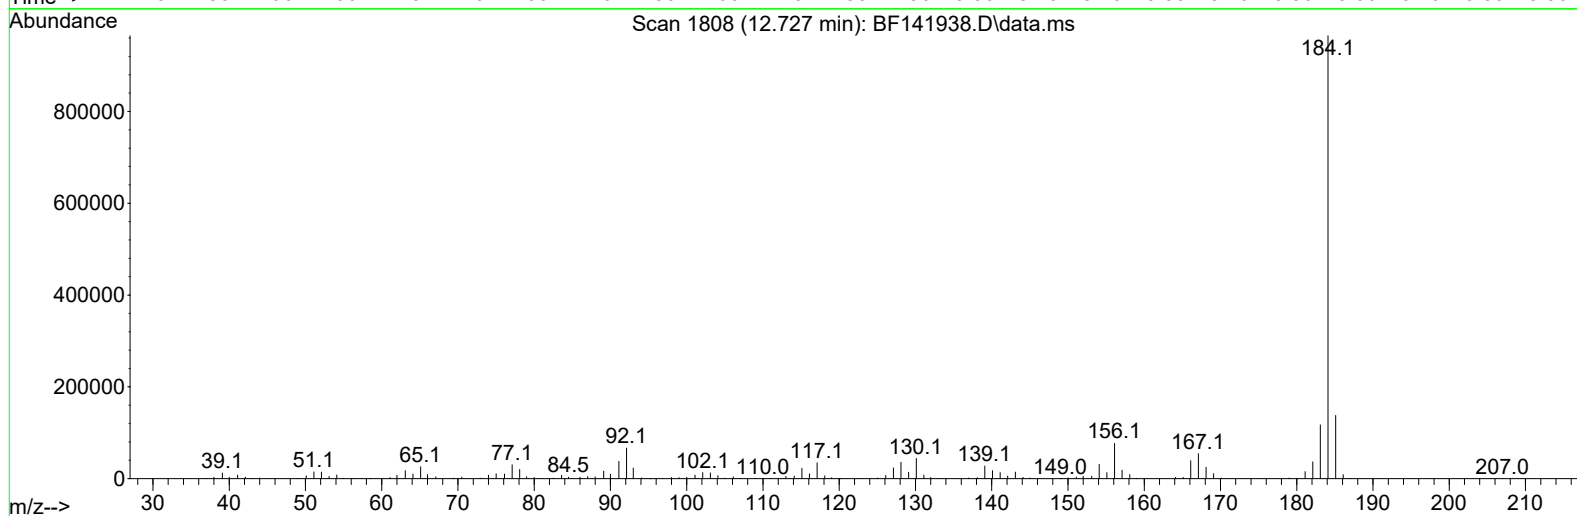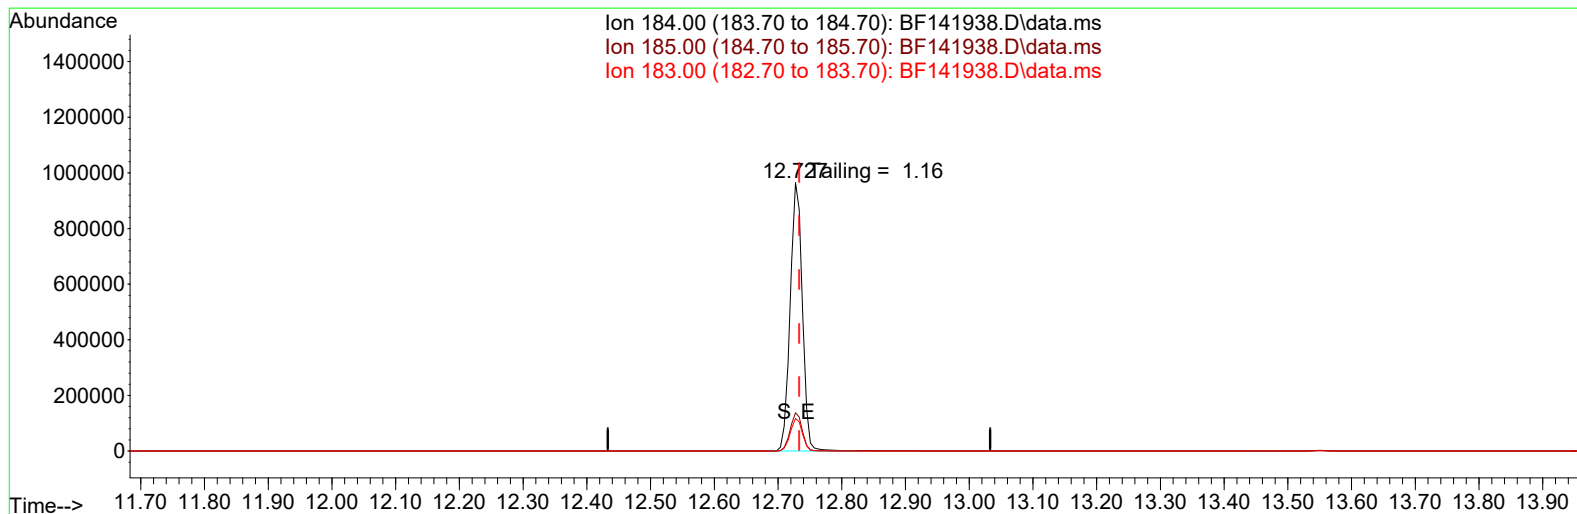

TIC: BF141938.D\data.ms

(77) Benzidine

12.727min (-0.006) 527010.30 ng

response 1286738

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.29
183.00	12.10	12.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/13/2025	BNA_F	<u>BF141938.D</u>
Compound Name	Response	Retention Time
DDT	695260	13.551
DDD	12936	13.251
DDE	425	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13361	708621	1.89

Instrument :
BNA_F
ClientSampleId :
DFTPP