

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031325\
 Data File : BF141944.D
 Acq On : 13 Mar 2025 16:44
 Operator : RC/JU
 Sample : Q1539-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TAPFTA-MW01I-031025-00-T2

Quant Time: Mar 13 17:07:35 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 10 15:46:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	168841	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	662735	20.000	ng	0.00
39) Acenaphthene-d10	9.910	164	386145	20.000	ng	0.00
64) Phenanthrene-d10	11.392	188	718788	20.000	ng	-0.01
76) Chrysene-d12	14.027	240	525213	20.000	ng	-0.01
86) Perylene-d12	15.498	264	377938	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.492	112	744011	73.544	ng	0.00
7) Phenol-d6	6.492	99	585105	45.425	ng	-0.01
23) Nitrobenzene-d5	7.434	82	1226775	104.171	ng	-0.01
42) 2,4,6-Tribromophenol	10.698	330	863116	176.191	ng	0.00
45) 2-Fluorobiphenyl	9.233	172	2455018	96.690	ng	0.00
79) Terphenyl-d14	12.980	244	3069685	86.410	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031325\
Data File : BF141944.D
Acq On : 13 Mar 2025 16:44
Operator : RC/JU
Sample : Q1539-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TAPFTA-MW01I-031025-00-T2

Quant Time: Mar 13 17:07:35 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration




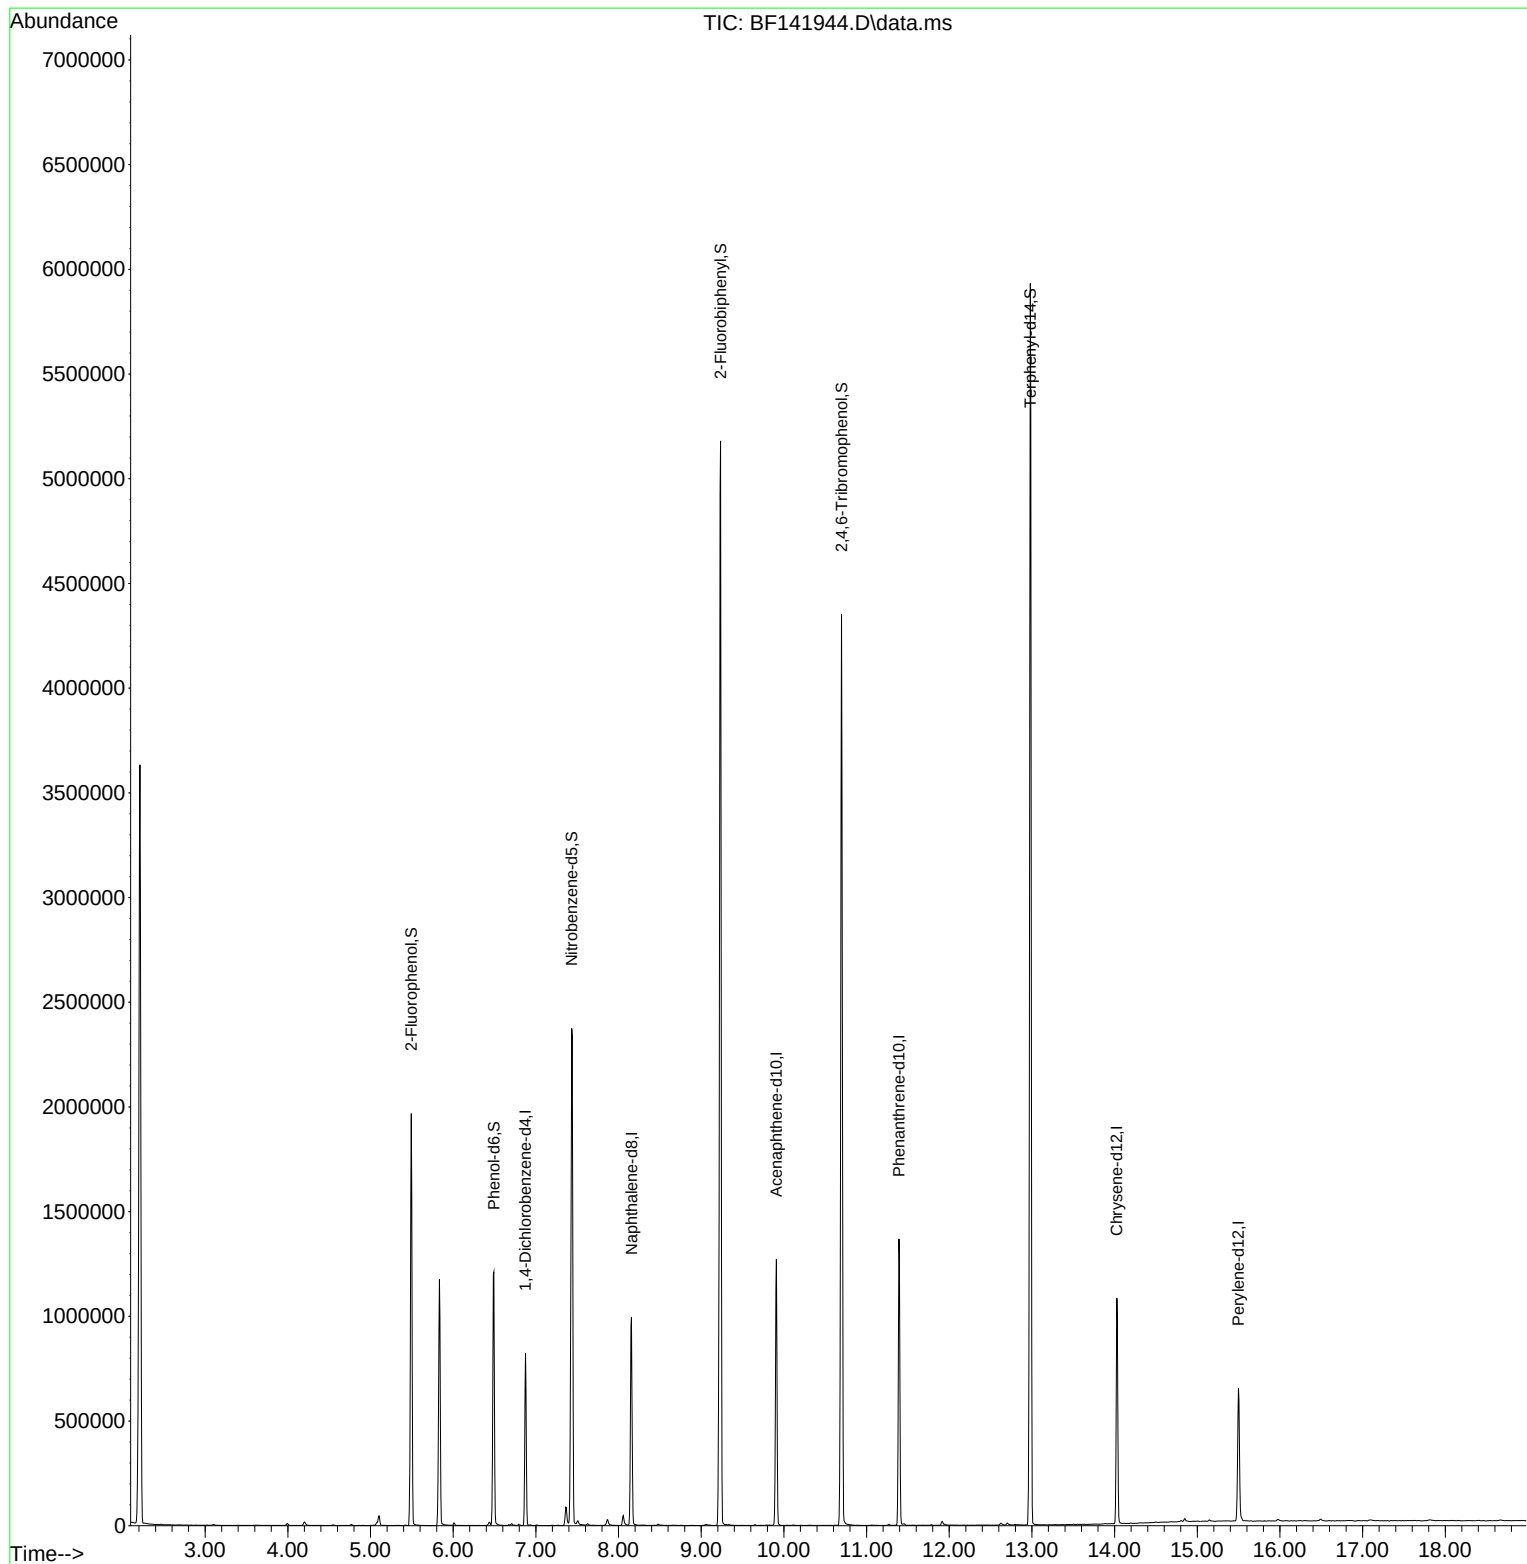


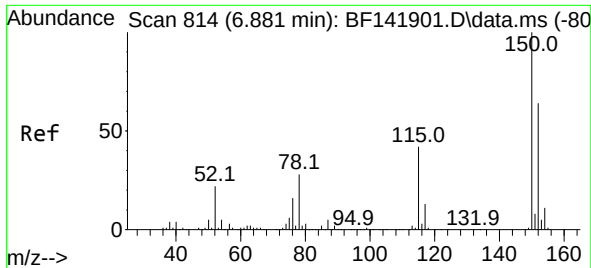

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 814
Delta R.T. -0.006 min
Lab File: BF141944.D
Acq: 13 Mar 2025 16:44




Instrument :
BNA_F
ClientSampleId :
TAPFTA-MW01I-031025-00-T2


Tgt Ion:152 Resp: 168841
Ion Ratio Lower Upper
152 100
150 157.5 127.4 191.2
115 65.9 51.9 77.9

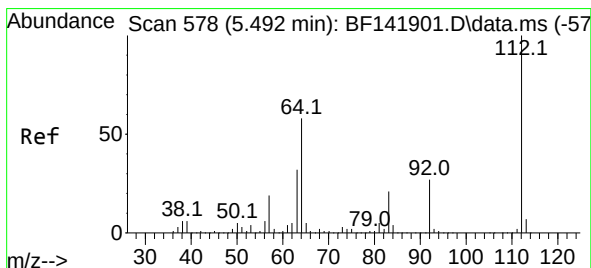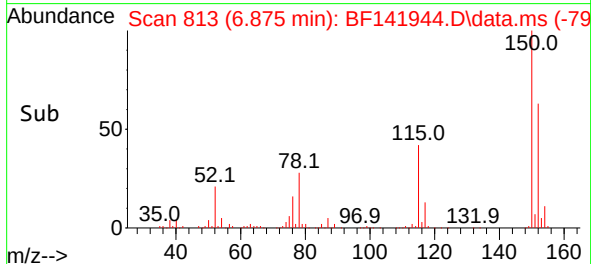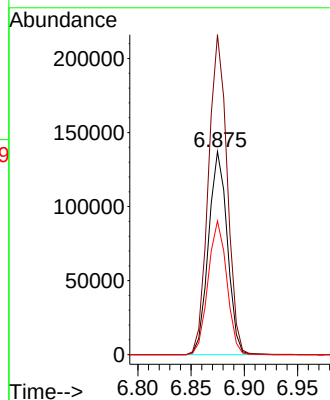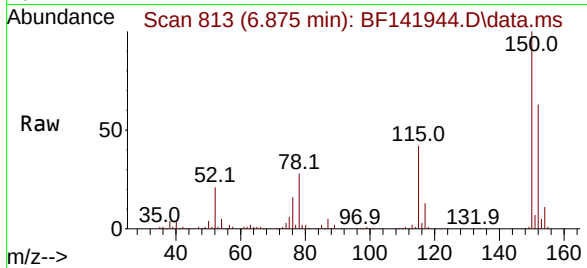

#5
2-Fluorophenol
Concen: 73.544 ng
RT: 5.492 min Scan# 578
Delta R.T. 0.000 min
Lab File: BF141944.D
Acq: 13 Mar 2025 16:44

Tgt Ion:112 Resp: 744011
Ion Ratio Lower Upper
112 100
64 56.8 46.5 69.7
63 30.9 25.4 38.2


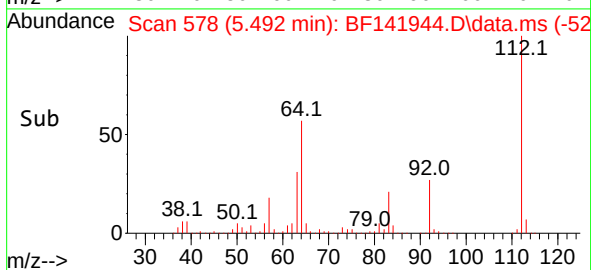
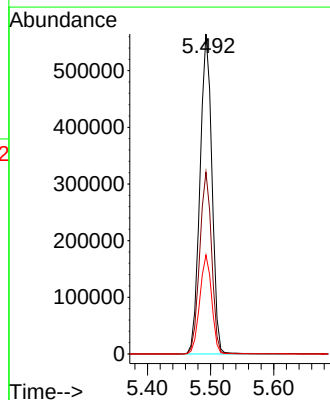
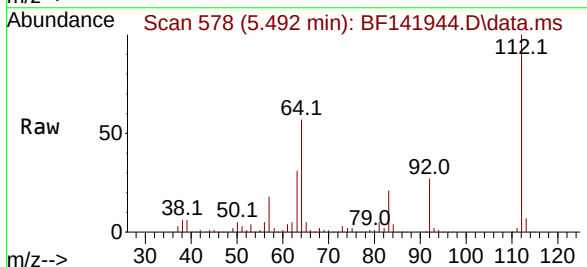


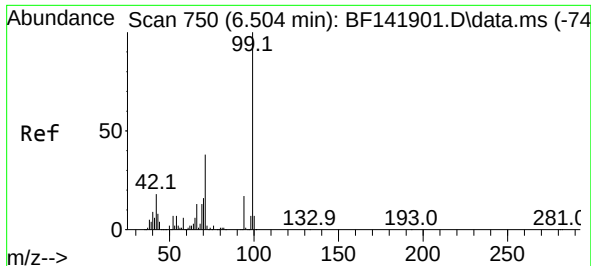

#7
Phenol-d6
Concen: 45.425 ng
RT: 6.492 min Scan# 74
Delta R.T. -0.012 min
Lab File: BF141944.D
Acq: 13 Mar 2025 16:44




Instrument :
BNA_F
ClientSampleId :
TAPFTA-MW01I-031025-00-T2


Tgt Ion: 99 Resp: 585105
Ion Ratio Lower Upper
99 100
42 16.9 14.6 21.8
71 37.5 30.8 46.2

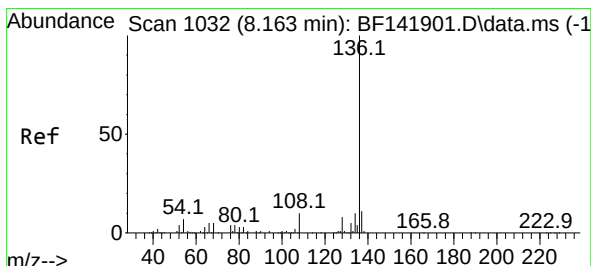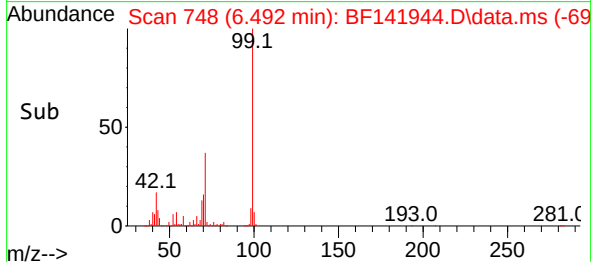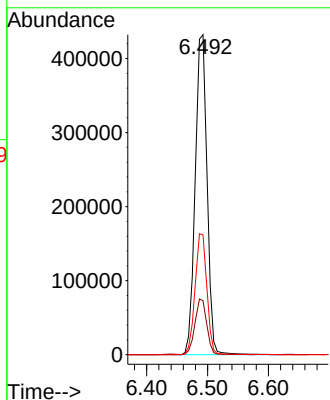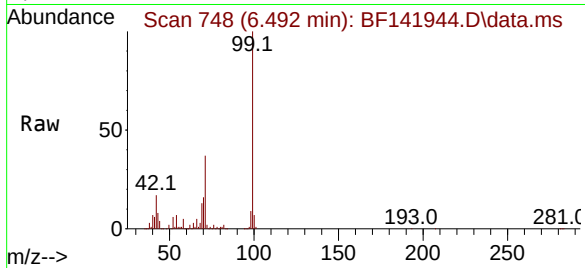

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 1031
Delta R.T. -0.006 min
Lab File: BF141944.D
Acq: 13 Mar 2025 16:44

Tgt Ion: 136 Resp: 662735
Ion Ratio Lower Upper
136 100
137 10.8 8.8 13.2
54 6.7 5.8 8.8
68 4.6 4.1 6.1


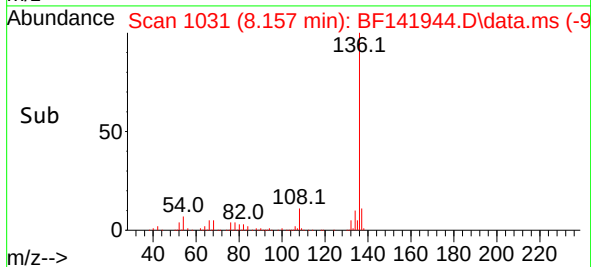
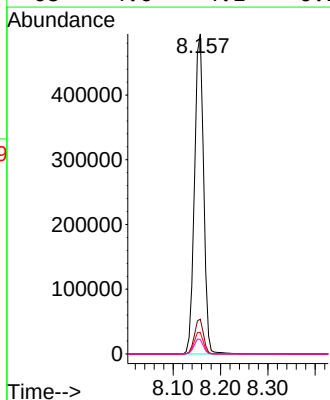
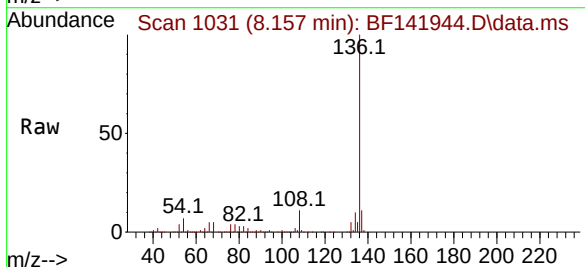


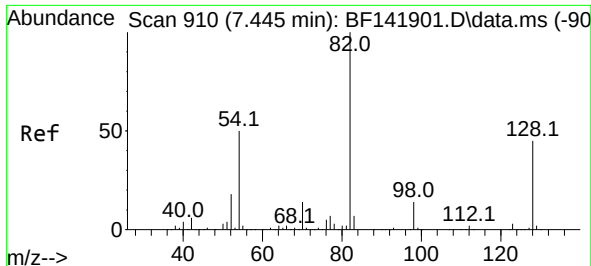

#23
Nitrobenzene-d5
Concen: 104.171 ng
RT: 7.434 min Scan# 90
Delta R.T. -0.012 min
Lab File: BF141944.D
Acq: 13 Mar 2025 16:44




Instrument :
BNA_F
ClientSampleId :
TAPFTA-MW01I-031025-00-T2


Tgt Ion: 82 Resp: 1226775
Ion Ratio Lower Upper
82 100
128 44.4 36.0 54.0
54 49.1 39.6 59.4

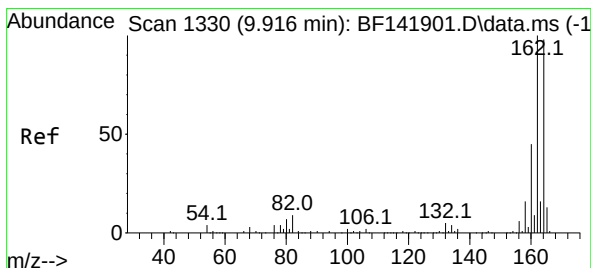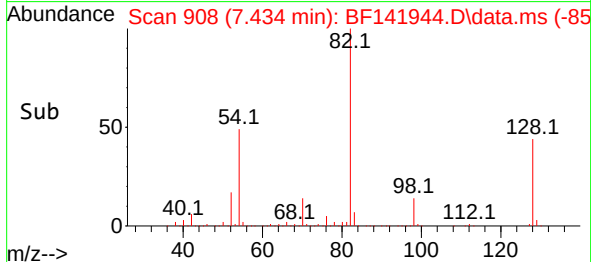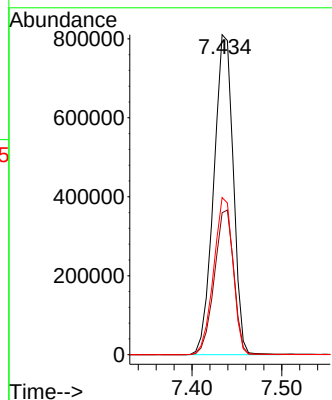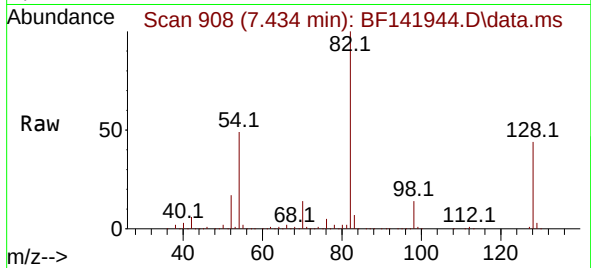

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.910 min Scan# 1329
Delta R.T. -0.006 min
Lab File: BF141944.D
Acq: 13 Mar 2025 16:44

Tgt Ion:164 Resp: 386145
Ion Ratio Lower Upper
164 100
162 103.3 81.8 122.6
160 46.2 36.7 55.1

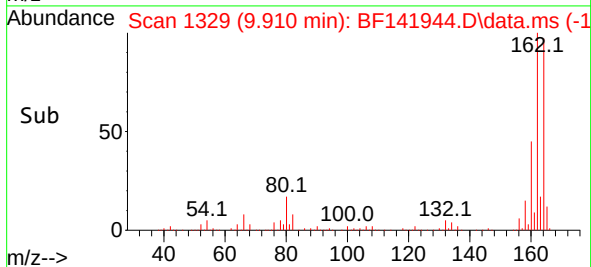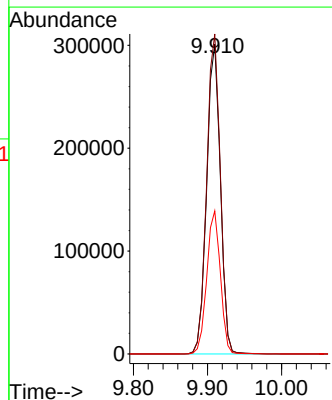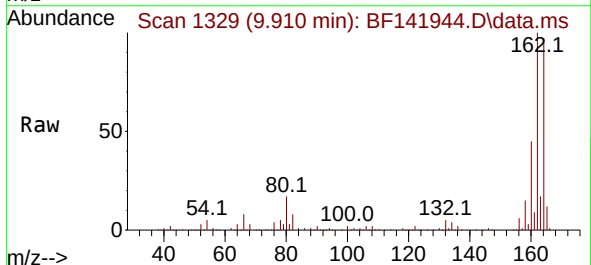

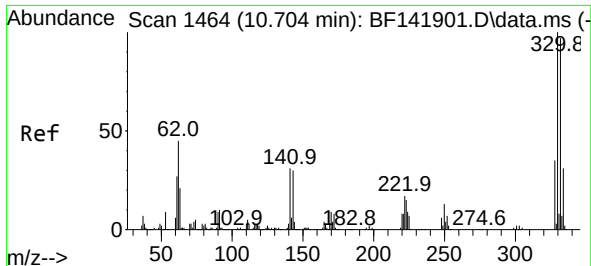

#42

2,4,6-Tribromophenol

Concen: 176.191 ng

RT: 10.698 min Scan# 1463

Delta R.T. -0.006 min

Lab File: BF141944.D

Acq: 13 Mar 2025 16:44

Instrument :

BNA_F

ClientSampleId :

TAPFTA-MW01I-031025-00-T2





Tgt Ion:330 Resp: 863116

Ion Ratio Lower Upper

330 100

332 95.6 77.6 116.4

141 27.4 24.7 37.1

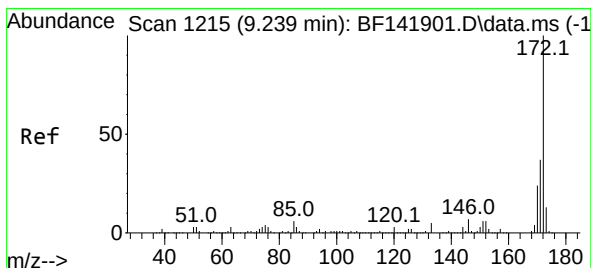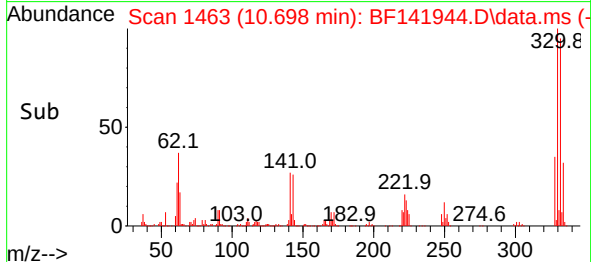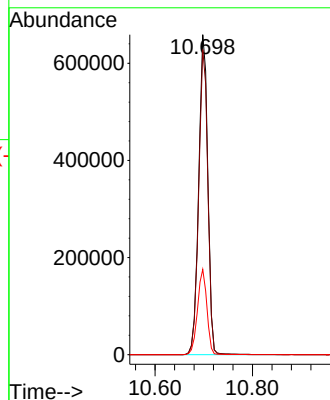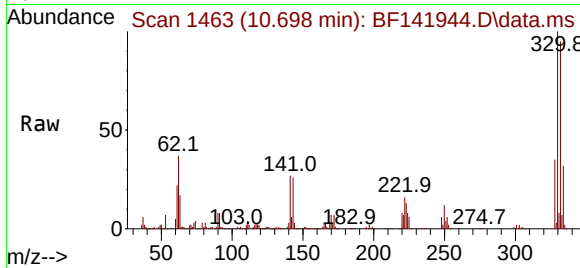

#45

2-Fluorobiphenyl

Concen: 96.690 ng

RT: 9.233 min Scan# 1214

Delta R.T. -0.006 min

Lab File: BF141944.D

Acq: 13 Mar 2025 16:44




Tgt Ion:172 Resp: 2455018


Ion Ratio Lower Upper

172 100

171 36.5 29.3 43.9

170 24.0 19.4 29.0


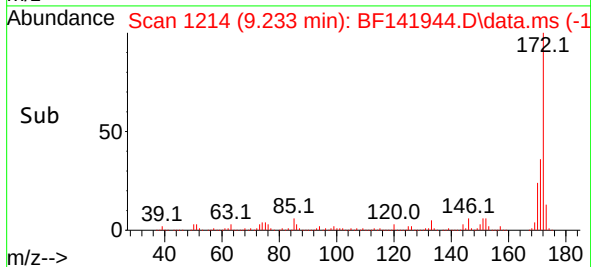
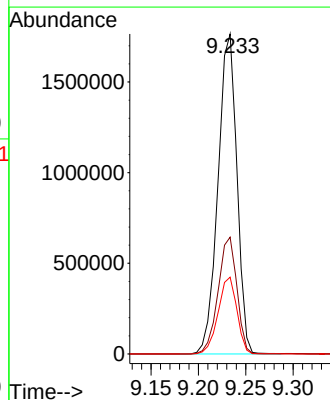
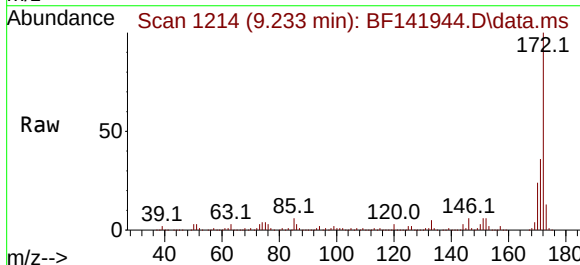


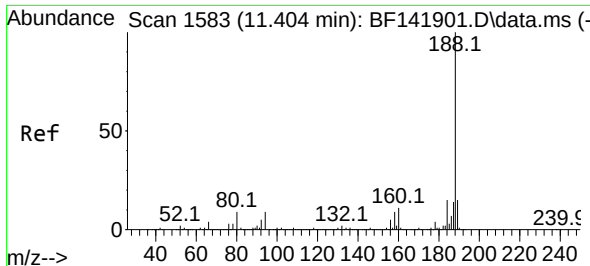

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.392 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF141944.D
Acq: 13 Mar 2025 16:44




Instrument :
BNA_F
ClientSampleId :
TAPFTA-MW01I-031025-00-T2


Tgt Ion:188 Resp: 718788
Ion Ratio Lower Upper
188 100
94 8.6 6.8 10.2
80 9.4 7.6 11.4

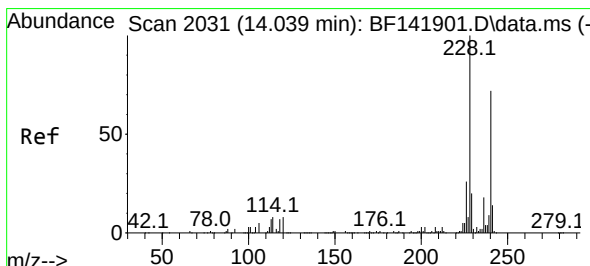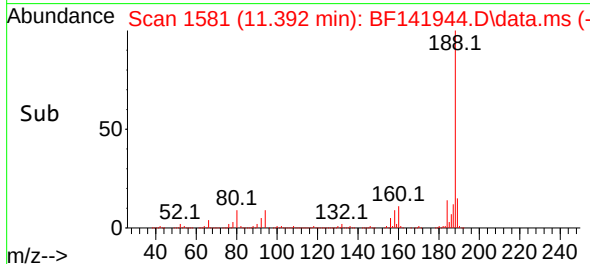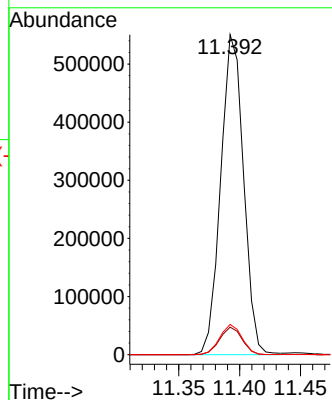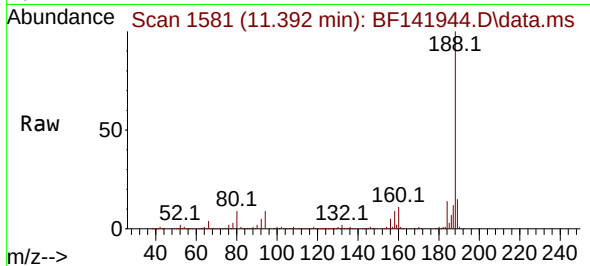

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.027 min Scan# 2029
Delta R.T. -0.012 min
Lab File: BF141944.D
Acq: 13 Mar 2025 16:44

Tgt Ion:240 Resp: 525213
Ion Ratio Lower Upper
240 100
120 9.8 8.4 12.6
236 25.3 20.5 30.7


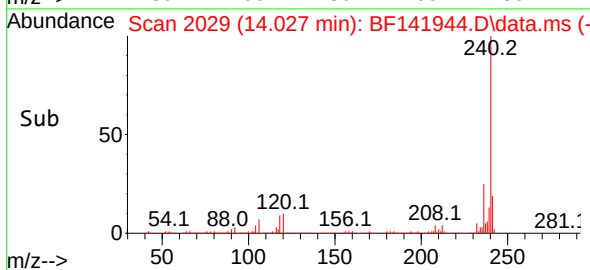
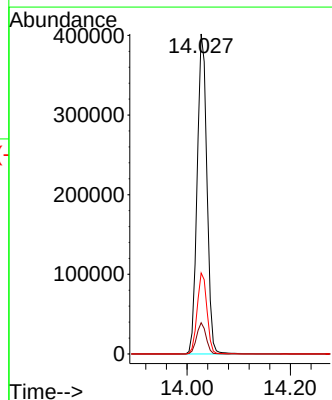
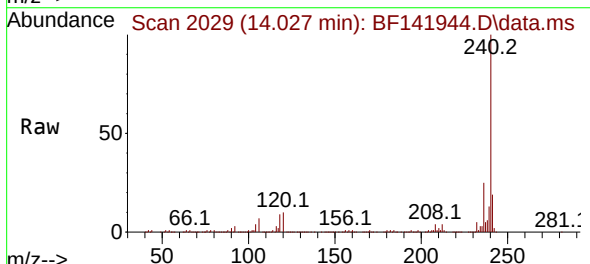


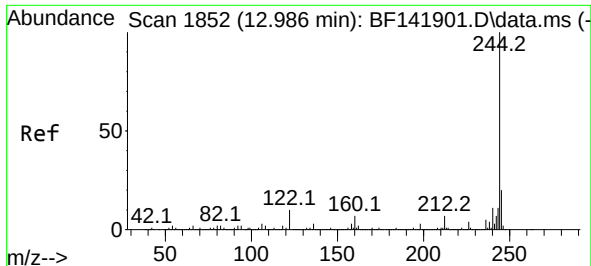

#79
 Terphenyl-d14
 Concen: 86.410 ng
 RT: 12.980 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF141944.D
 Acq: 13 Mar 2025 16:44

Instrument :
 BNA_F
 ClientSampleId :
 TAPFTA-MW01I-031025-00-T2

Tgt Ion:244 Resp: 3069685
 Ion Ratio Lower Upper
 244 100
 212 7.0 6.0 9.0
 122 9.3 7.7 11.5

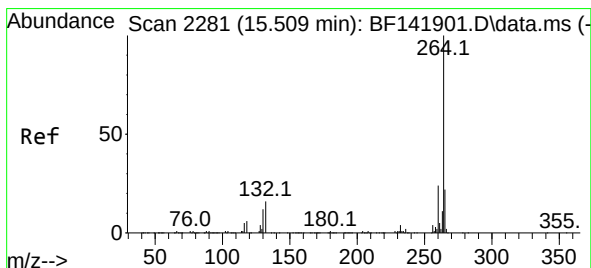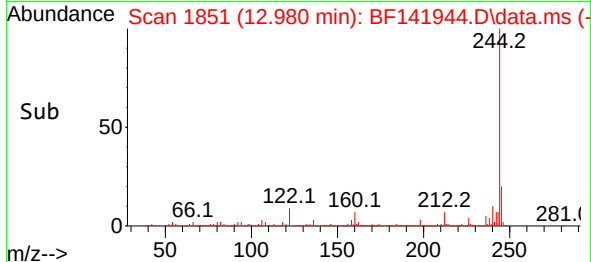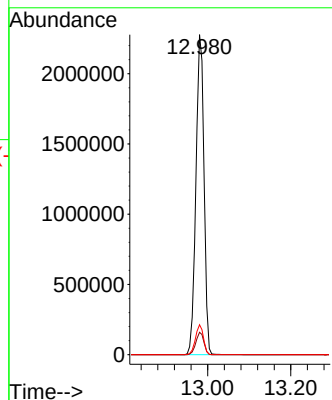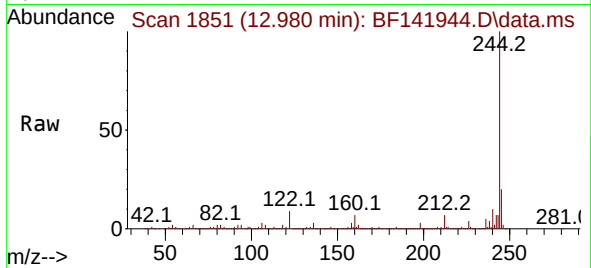

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.498 min Scan# 2279
 Delta R.T. -0.012 min
 Lab File: BF141944.D
 Acq: 13 Mar 2025 16:44

Tgt Ion:264 Resp: 377938
 Ion Ratio Lower Upper
 264 100
 260 22.9 19.1 28.7
 265 21.8 17.5 26.3

