

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031225\
Data File : FF015656.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2025 11:59
Operator : YP\AJ
Sample : PB167095BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB167095BL

Integration File: autoint1.e
Quant Time: Mar 13 02:28:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030325.M
Quant Title :
QLast Update : Mon Mar 03 14:28:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.023	1788083	14.996 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031225\
Data File : FF015656.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2025 11:59
Operator : YP\AJ
Sample : PB167095BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB167095BL

Integration File: autoint1.e
Quant Time: Mar 13 02:28:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030325.M
Quant Title :
QLast Update : Mon Mar 03 14:28:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

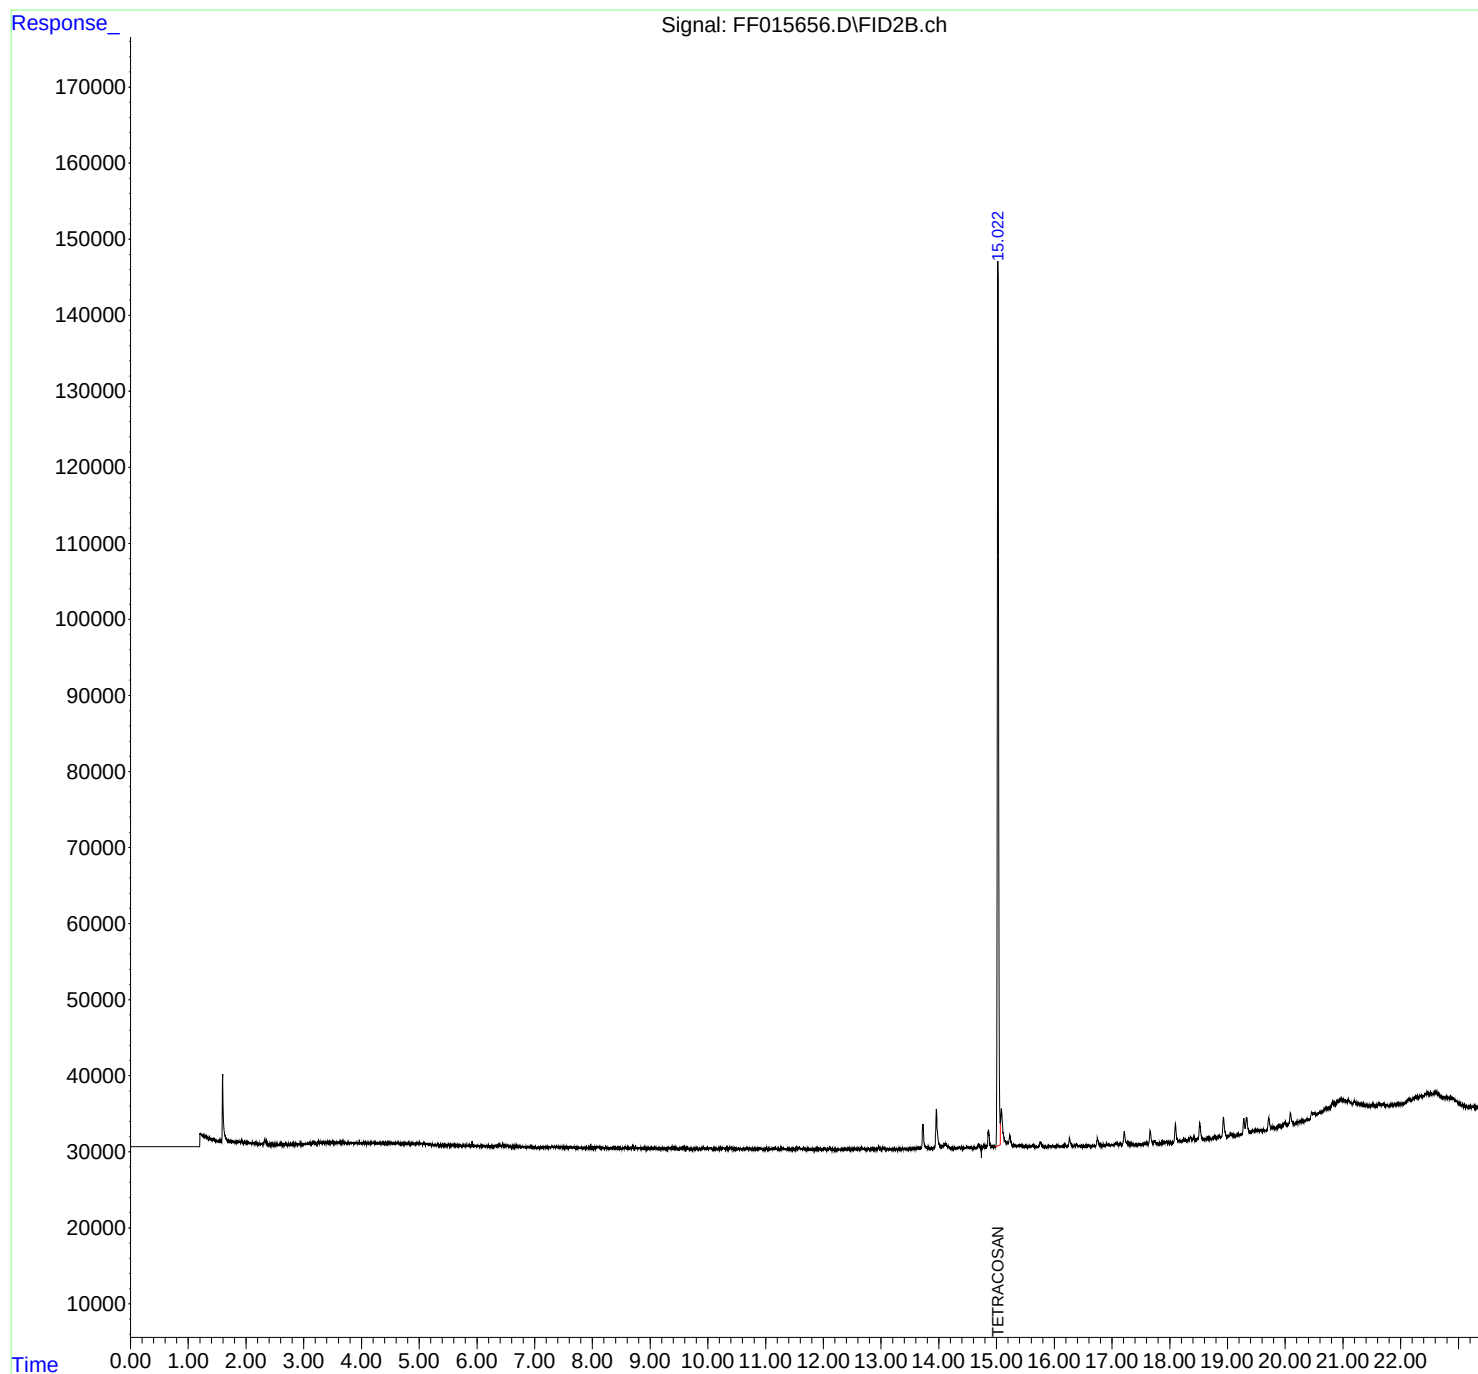

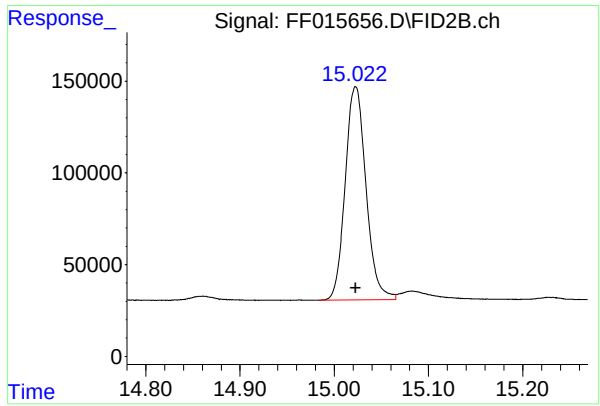

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.023 min
Delta R.T.: 0.000 min
Response: 1788083
Conc: 15.00 ug/ml

Instrument :
FID_F
ClientSampleId :
PB167095BL