

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
 Data File : PL094570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 10:49
 Operator : AR\AJ
 Sample : PSTDICC075
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDICC075

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/12/2025
 Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 17:25:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:20:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.771	201.1E6	263.8E6	74.661	74.715
28)	SA Decachlor...	9.055	7.907	147.1E6	290.1E6	74.529	74.250
Target Compounds							
2)	A alpha-BHC	3.994	3.274	299.7E6	415.1E6	74.590	74.846
3)	MA gamma-BHC...	4.327	3.604	286.8E6	392.3E6	74.491	74.788
4)	MA Heptachlor	4.915	3.942	274.6E6	394.7E6	74.717	74.686
5)	MB Aldrin	5.256	4.221	261.3E6	367.8E6	74.639	74.632
6)	B beta-BHC	4.525	3.905	126.6E6	161.7E6	74.425	74.433
7)	B delta-BHC	4.773	4.133	276.2E6	381.6E6	74.421	74.685
8)	B Heptachlo...	5.683	4.724	234.3E6	338.9E6	74.391	74.396
9)	A Endosulfan I	6.068	5.094	214.1E6	327.1E6	74.379	74.540
10)	B gamma-Chl...	5.939	4.974	236.0E6	360.5E6	74.469	74.458
11)	B alpha-Chl...	6.018	5.038	230.0E6	353.6E6	74.279	74.319
12)	B 4,4'-DDE	6.192	5.226	209.3E6	344.3E6	74.444	74.114
13)	MA Dieldrin	6.343	5.358	223.3E6	363.9E6	74.299	74.605
14)	MA Endrin	6.574	5.634	193.9E6	324.4E6	74.564	74.369
15)	B Endosulfa...	6.793	5.928	187.1E6	317.8E6	74.019	74.259
16)	A 4,4'-DDD	6.710	5.781	152.9E6	270.0E6	74.080	74.117
17)	MA 4,4'-DDT	7.024	6.032	169.4E6	304.6E6	74.825	74.399
18)	B Endrin al...	6.924	6.108	143.4E6	242.5E6	74.079	74.128
19)	B Endosulfa...	7.158	6.331	167.1E6	298.4E6	74.536	73.822
20)	A Methoxychlor	7.500	6.607	86133491	156.4E6	75.871	74.794
21)	B Endrin ke...	7.644	6.836	186.7E6	352.0E6	74.884	74.420
22)	Mirex	8.115	7.015	140.5E6	271.3E6	74.155m	74.275

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031125\
Data File : PL094570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 10:49
Operator : AR\AJ
Sample : PSTDICC075
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :

ECD_L

ClientSampleId :

PSTDICC075

Manual Integrations



APPROVED


Reviewed By :Abdul Mirza 03/12/2025

Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 17:25:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:20:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

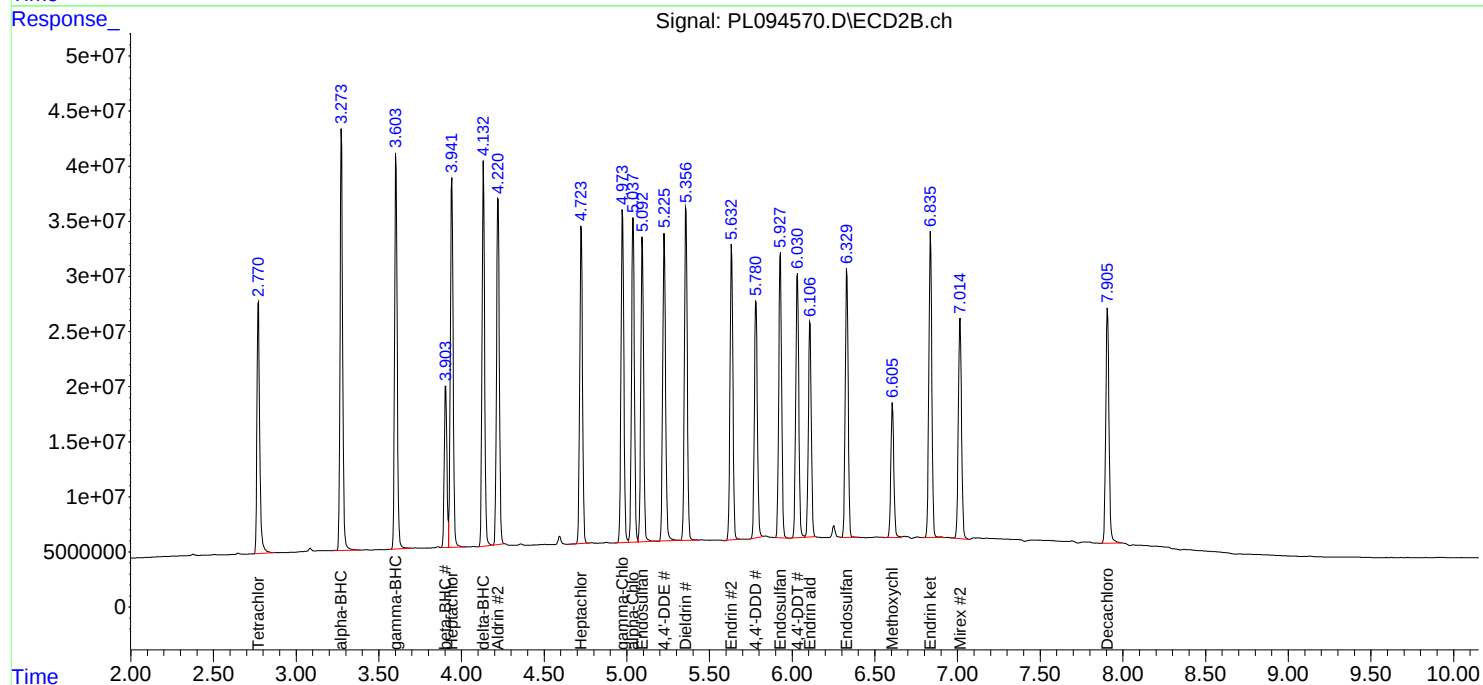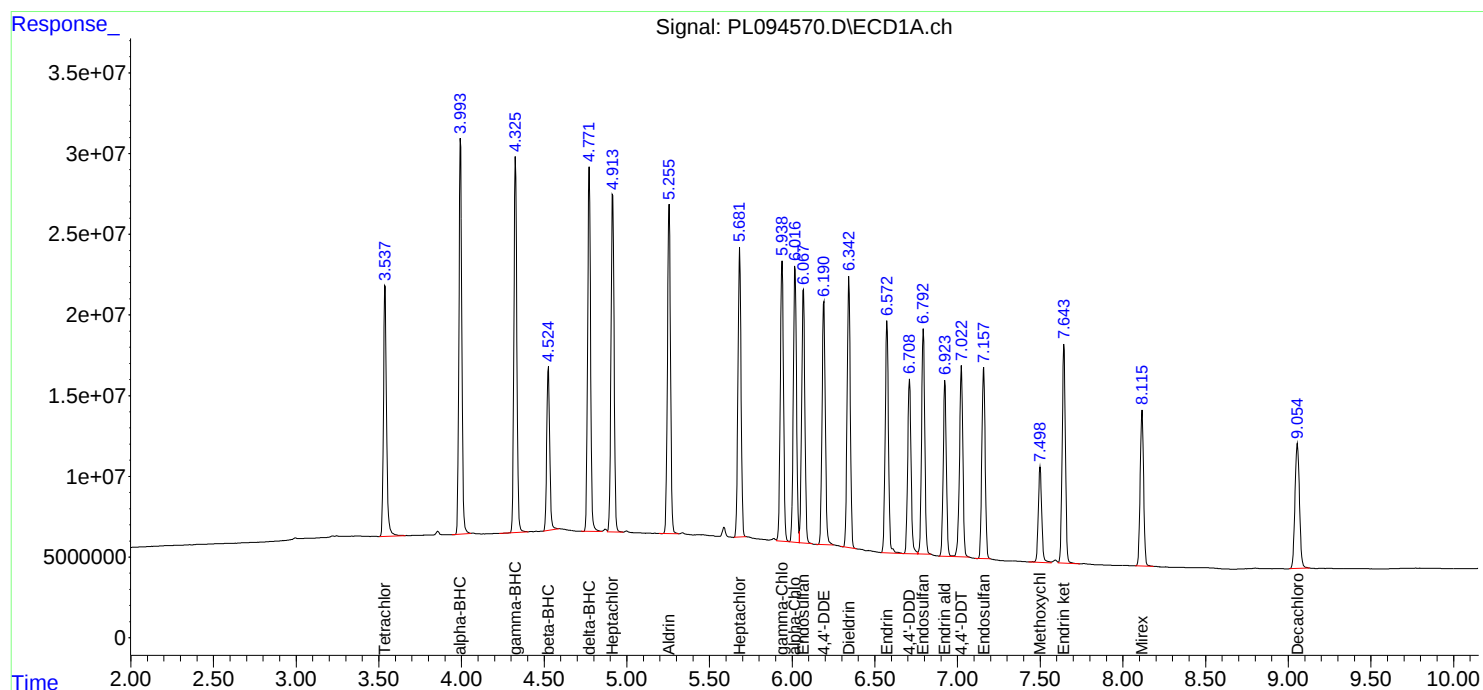

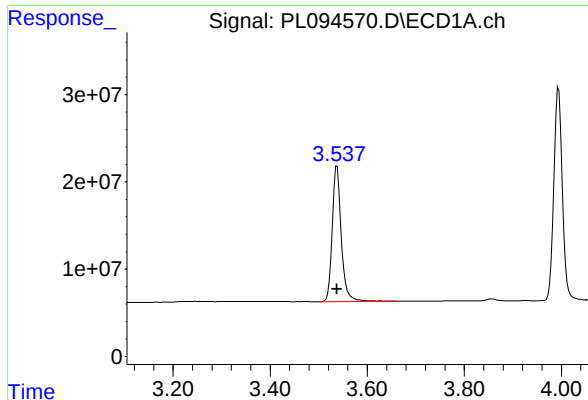


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 201142853
Conc: 74.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

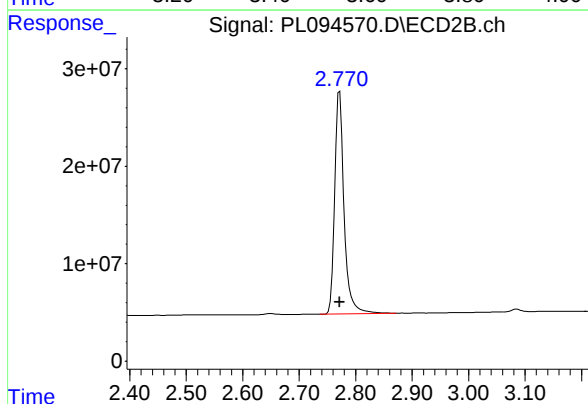


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 263799483
Conc: 74.71 ng/ml

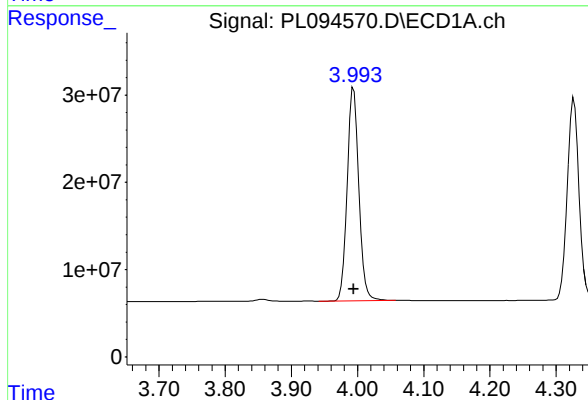


#2 alpha-BHC

R.T.: 3.994 min
Delta R.T.: 0.000 min
Response: 299674738
Conc: 74.59 ng/ml

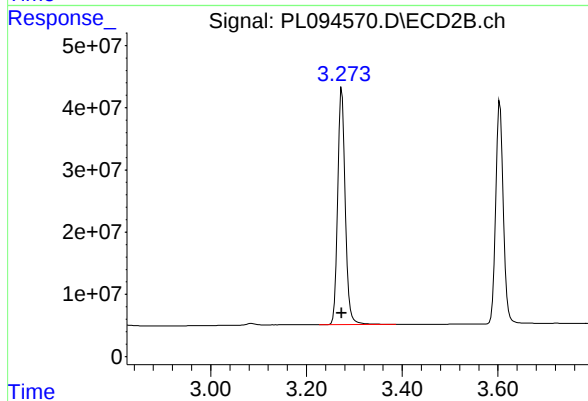

#2 alpha-BHC

R.T.: 3.274 min
Delta R.T.: 0.000 min
Response: 415112906
Conc: 74.85 ng/ml

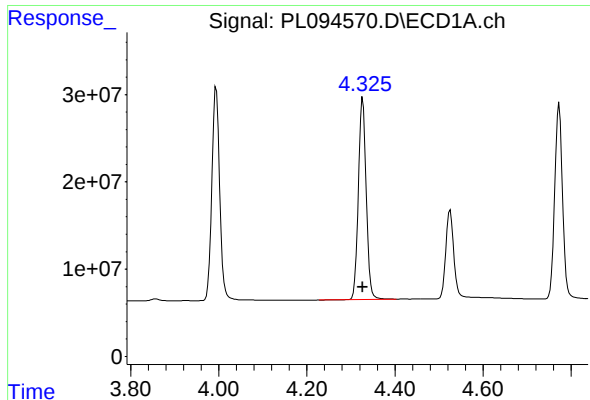


#3 gamma-BHC (Lindane)

R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 286840913
Conc: 74.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

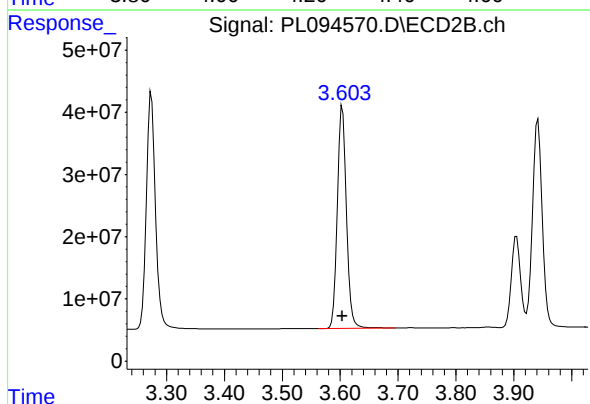


#3 gamma-BHC (Lindane)

R.T.: 3.604 min
Delta R.T.: 0.000 min
Response: 392257185
Conc: 74.79 ng/ml

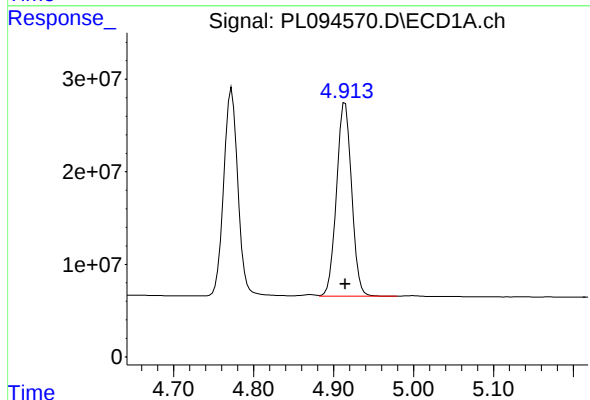


#4 Heptachlor

R.T.: 4.915 min
Delta R.T.: 0.000 min
Response: 274574691
Conc: 74.72 ng/ml

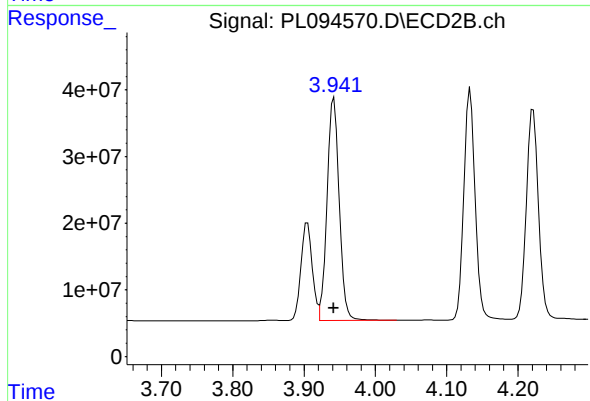

#4 Heptachlor

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 394705067
Conc: 74.69 ng/ml

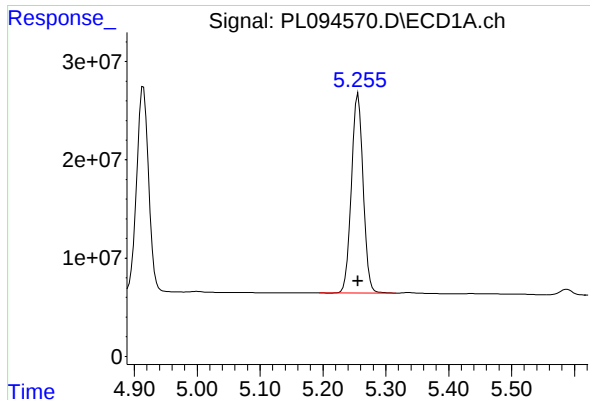


#5 Aldrin

R.T.: 5.256 min
Delta R.T.: 0.000 min
Response: 261288108
Conc: 74.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

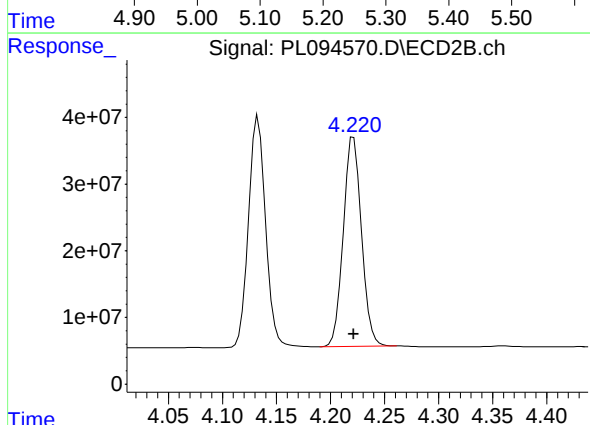


#5 Aldrin

R.T.: 4.221 min
Delta R.T.: 0.000 min
Response: 367798902
Conc: 74.63 ng/ml

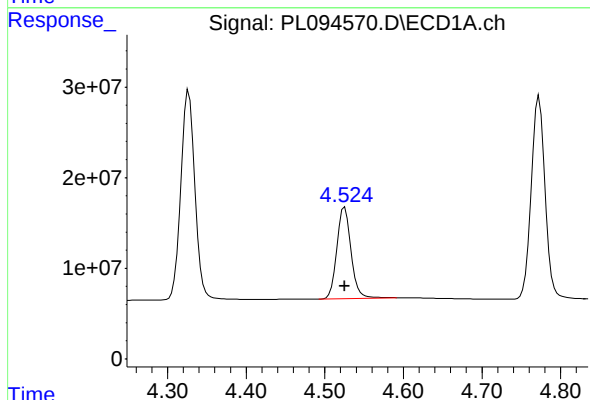


#6 beta-BHC

R.T.: 4.525 min
Delta R.T.: 0.000 min
Response: 126613518
Conc: 74.42 ng/ml

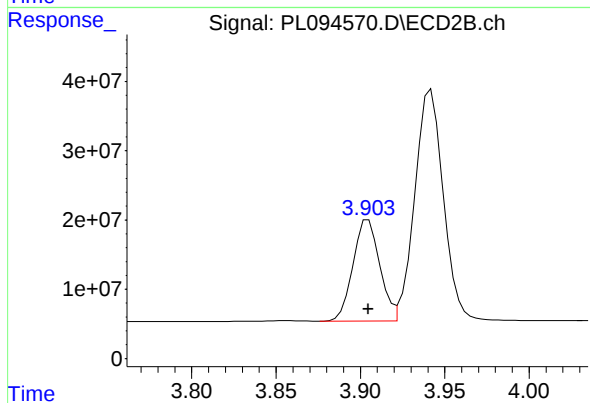

#6 beta-BHC

R.T.: 3.905 min
Delta R.T.: 0.000 min
Response: 161729415
Conc: 74.43 ng/ml

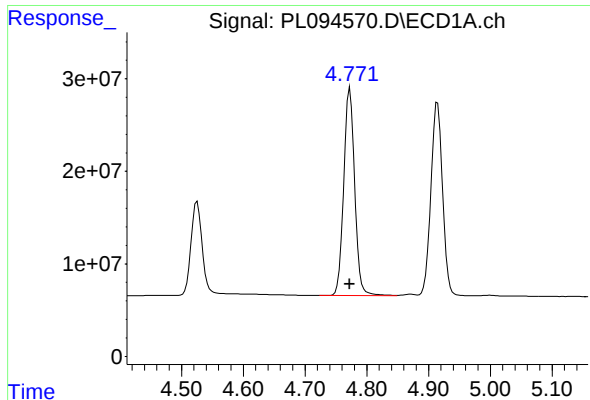


#7 delta-BHC

R.T.: 4.773 min
Delta R.T.: 0.000 min
Response: 276213712
Conc: 74.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

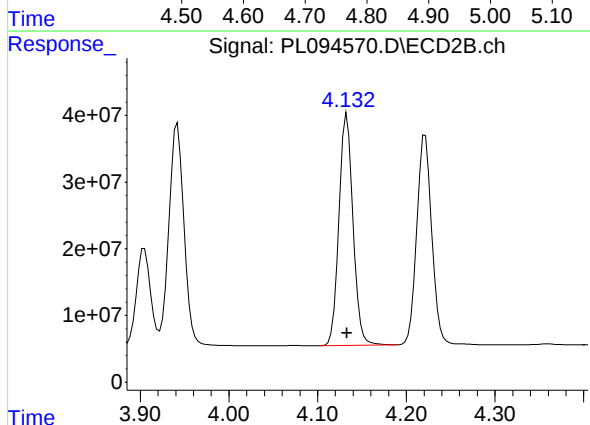


#7 delta-BHC

R.T.: 4.133 min
Delta R.T.: 0.000 min
Response: 381584993
Conc: 74.69 ng/ml

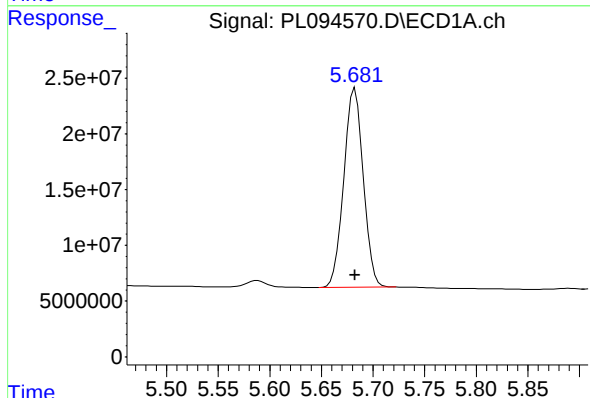


#8 Heptachlor epoxide

R.T.: 5.683 min
Delta R.T.: 0.000 min
Response: 234307611
Conc: 74.39 ng/ml

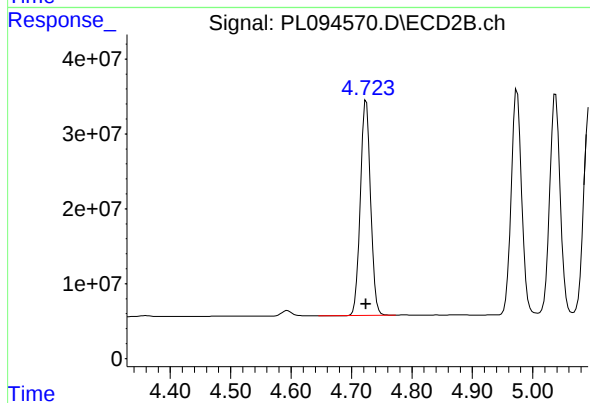

#8 Heptachlor epoxide

R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 338947683
Conc: 74.40 ng/ml

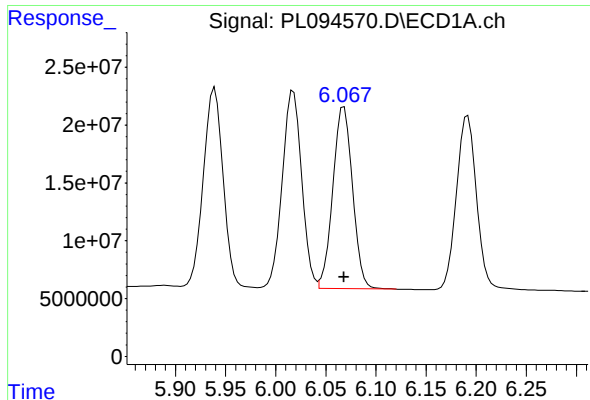


#9 Endosulfan I

R.T.: 6.068 min
Delta R.T.: 0.000 min
Response: 214077097
Conc: 74.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

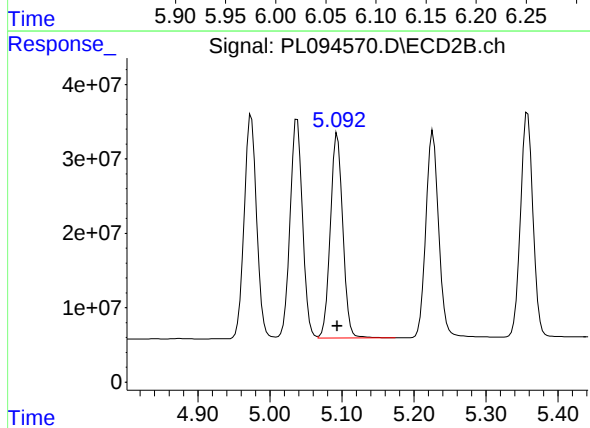


#9 Endosulfan I

R.T.: 5.094 min
Delta R.T.: 0.000 min
Response: 327058959
Conc: 74.54 ng/ml

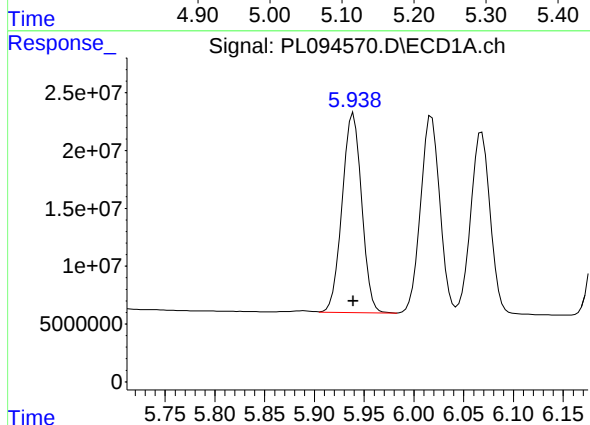


#10 gamma-Chlordane

R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 235979855
Conc: 74.47 ng/ml

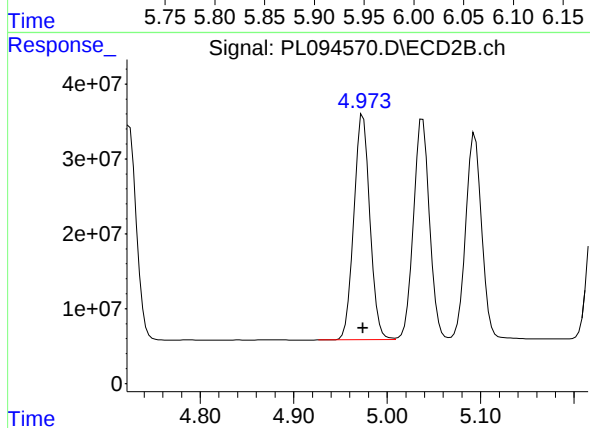

#10 gamma-Chlordane

R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 360471631
Conc: 74.46 ng/ml

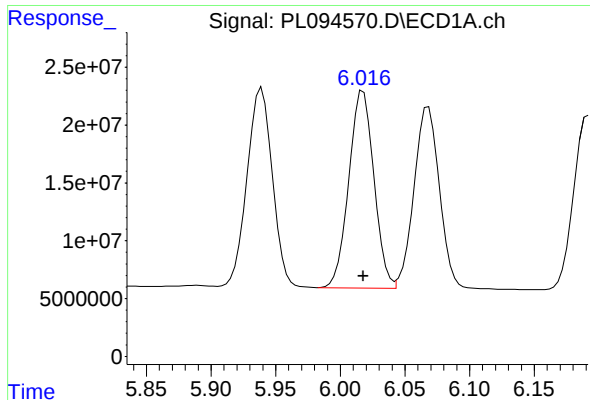


#11 alpha-Chlordane

R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 230043306
Conc: 74.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

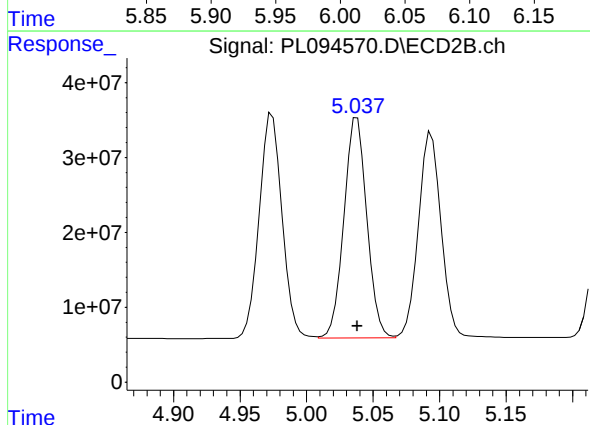


#11 alpha-Chlordane

R.T.: 5.038 min
Delta R.T.: 0.000 min
Response: 353614949
Conc: 74.32 ng/ml

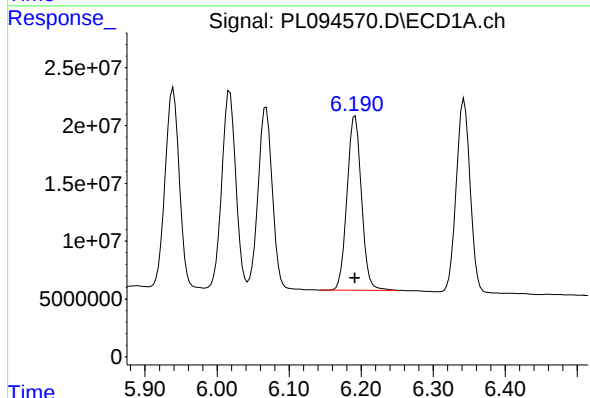


#12 4,4'-DDE

R.T.: 6.192 min
Delta R.T.: 0.000 min
Response: 209341973
Conc: 74.44 ng/ml

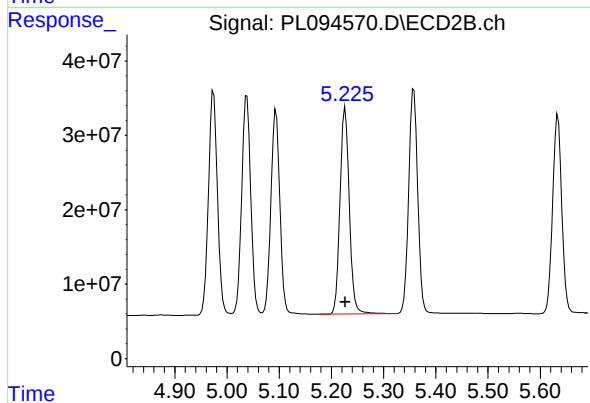

#12 4,4'-DDE

R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 344267084
Conc: 74.11 ng/ml

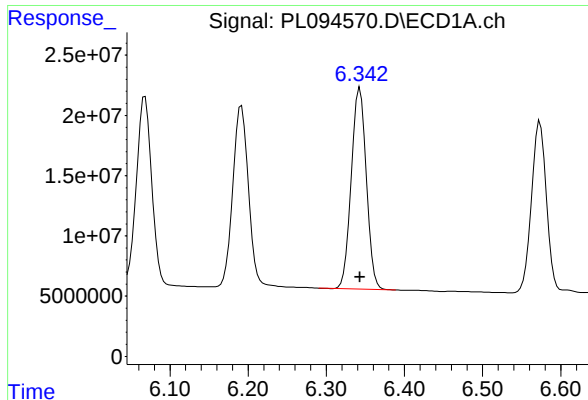


#13 Dieldrin

R.T.: 6.343 min
Delta R.T.: 0.000 min
Response: 223314903
Conc: 74.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

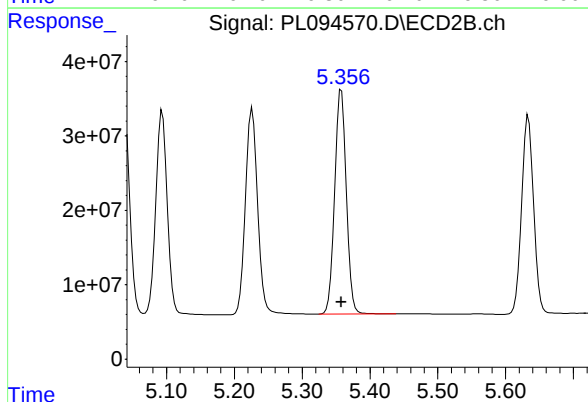


#13 Dieldrin

R.T.: 5.358 min
Delta R.T.: 0.000 min
Response: 363943892
Conc: 74.60 ng/ml

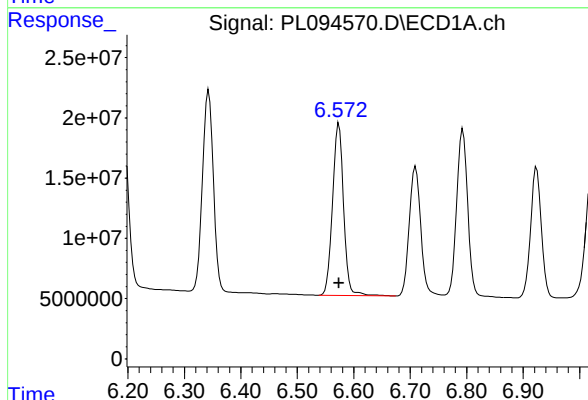


#14 Endrin

R.T.: 6.574 min
Delta R.T.: 0.000 min
Response: 193850510
Conc: 74.56 ng/ml

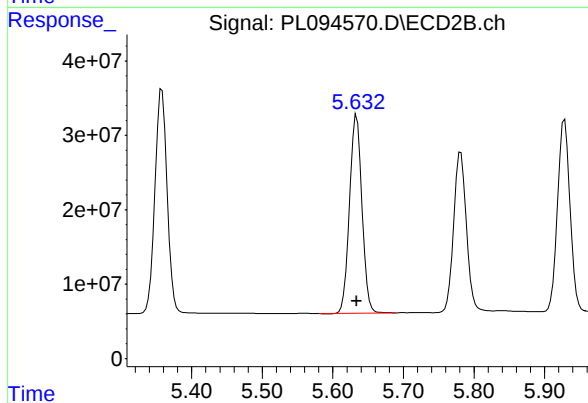

#14 Endrin

R.T.: 5.634 min
Delta R.T.: 0.000 min
Response: 324396614
Conc: 74.37 ng/ml

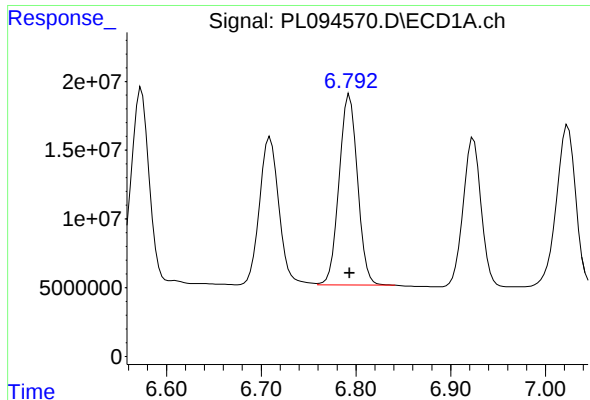


#15 Endosulfan II

R.T.: 6.793 min
Delta R.T.: 0.000 min
Response: 187131432
Conc: 74.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

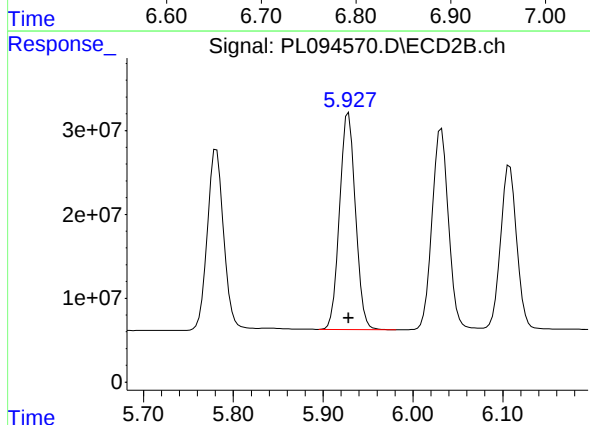


#15 Endosulfan II

R.T.: 5.928 min
Delta R.T.: 0.000 min
Response: 317833183
Conc: 74.26 ng/ml

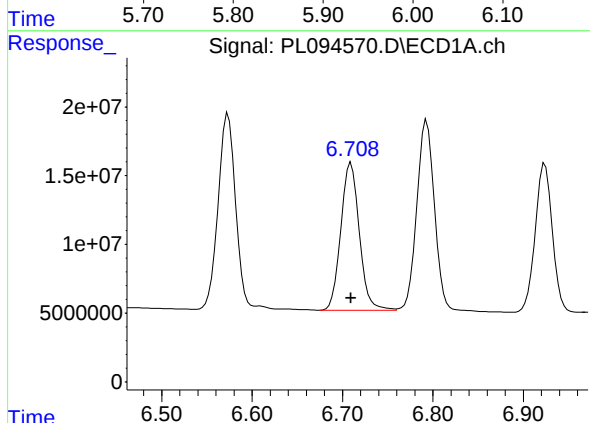


#16 4,4'-DDD

R.T.: 6.710 min
Delta R.T.: 0.000 min
Response: 152854261
Conc: 74.08 ng/ml

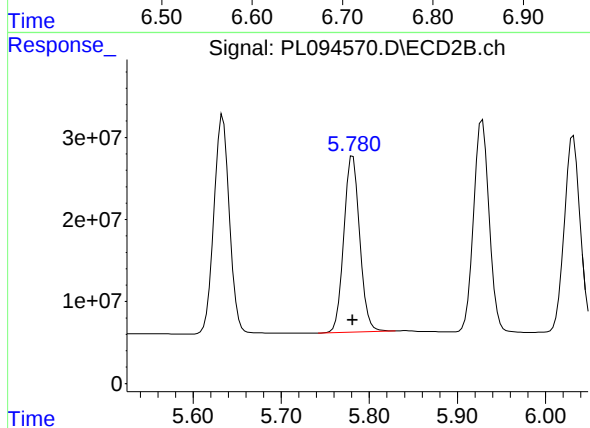

#16 4,4'-DDD

R.T.: 5.781 min
Delta R.T.: 0.000 min
Response: 269957054
Conc: 74.12 ng/ml

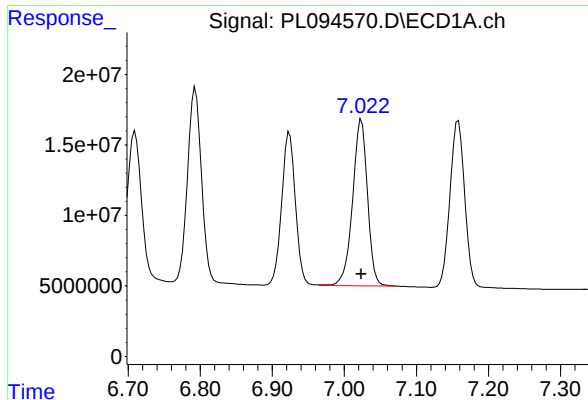


#17 4,4'-DDT

R.T.: 7.024 min
Delta R.T.: 0.000 min
Response: 169409218
Conc: 74.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

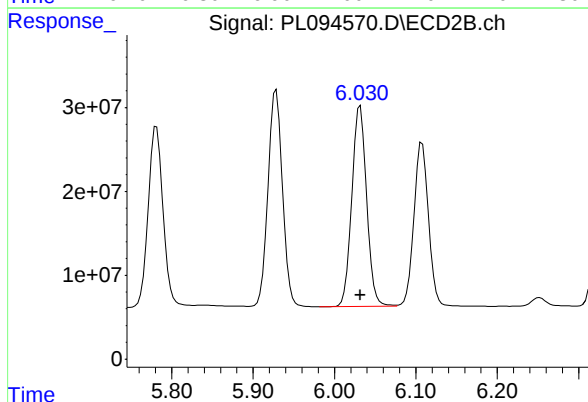


#17 4,4'-DDT

R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 304588533
Conc: 74.40 ng/ml

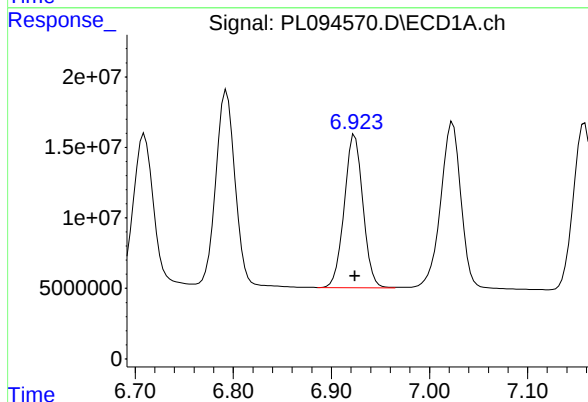


#18 Endrin aldehyde

R.T.: 6.924 min
Delta R.T.: 0.000 min
Response: 143367924
Conc: 74.08 ng/ml

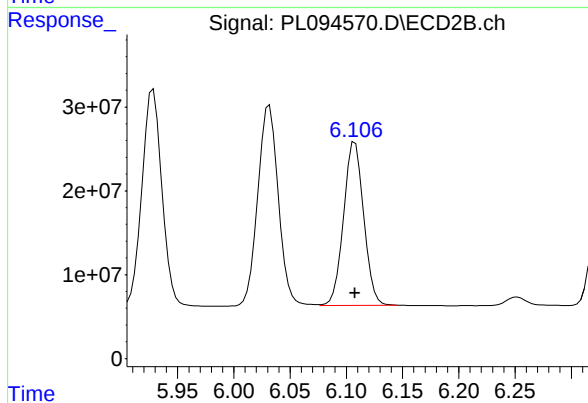

#18 Endrin aldehyde

R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 242485357
Conc: 74.13 ng/ml

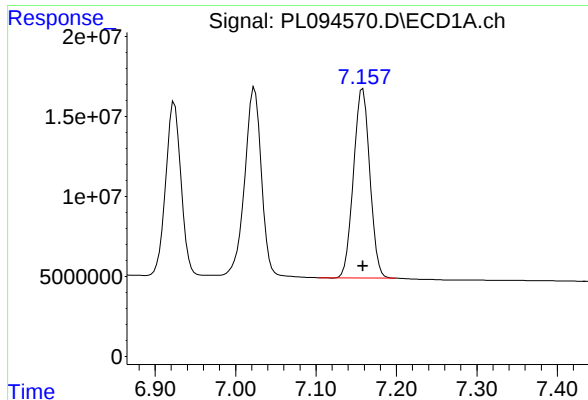


#19 Endosulfan Sulfate

R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 167119326
Conc: 74.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

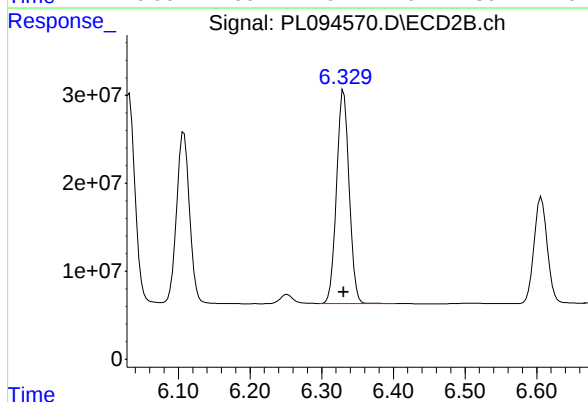


#19 Endosulfan Sulfate

R.T.: 6.331 min
Delta R.T.: 0.000 min
Response: 298376745
Conc: 73.82 ng/ml

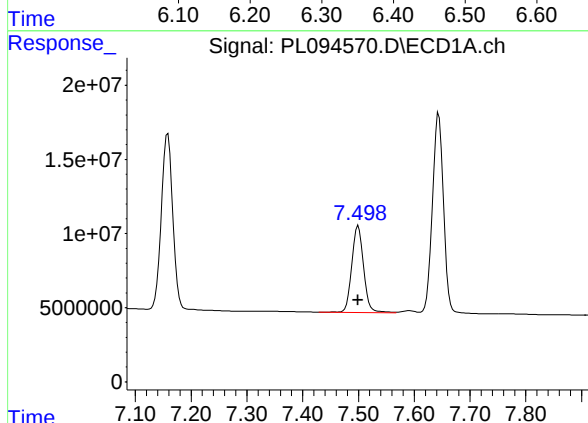


#20 Methoxychlor

R.T.: 7.500 min
Delta R.T.: 0.000 min
Response: 86133491
Conc: 75.87 ng/ml

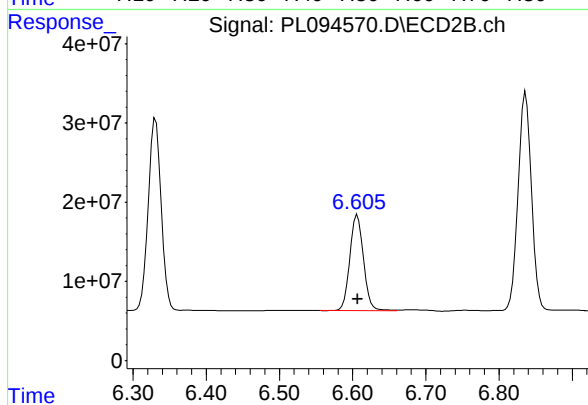

#20 Methoxychlor

R.T.: 6.607 min
Delta R.T.: 0.000 min
Response: 156422121
Conc: 74.79 ng/ml

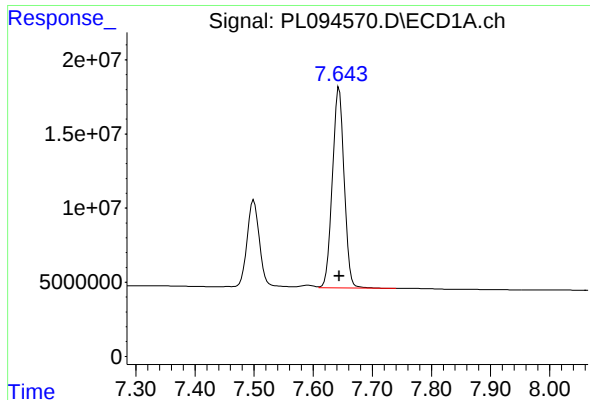


#21 Endrin ketone

R.T.: 7.644 min
Delta R.T.: 0.000 min
Response: 186691823
Conc: 74.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

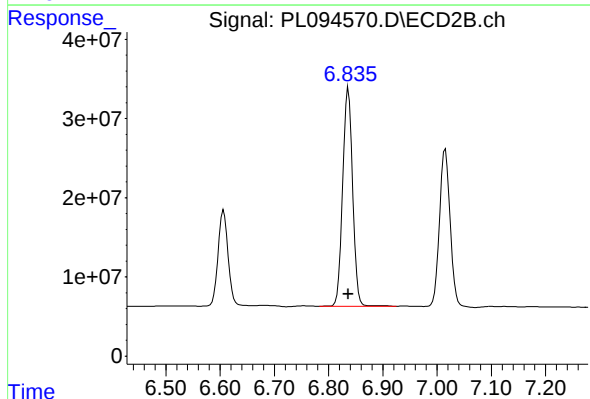


#21 Endrin ketone

R.T.: 6.836 min
Delta R.T.: 0.000 min
Response: 351951268
Conc: 74.42 ng/ml

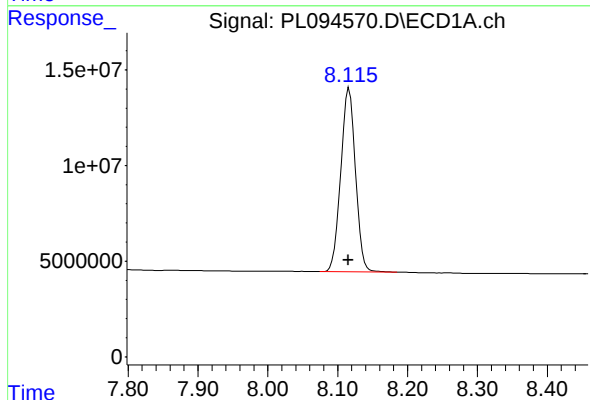


#22 Mirex

R.T.: 8.115 min
Delta R.T.: 0.000 min
Response: 140491044
Conc: 74.15 ng/ml m

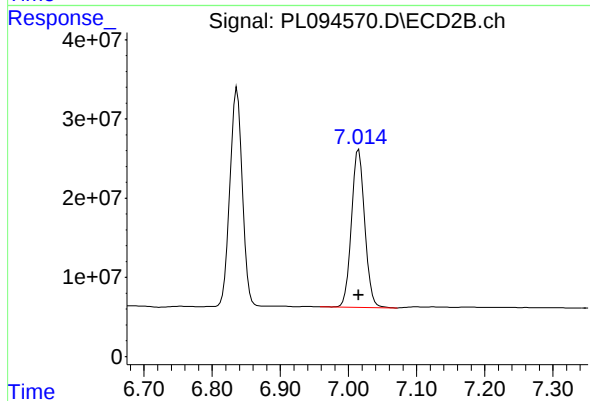

#22 Mirex

R.T.: 7.015 min
Delta R.T.: 0.000 min
Response: 271252738
Conc: 74.27 ng/ml

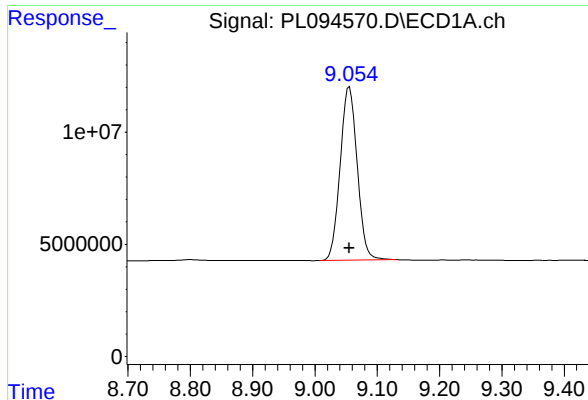


#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 147082223
Conc: 74.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDICC075

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

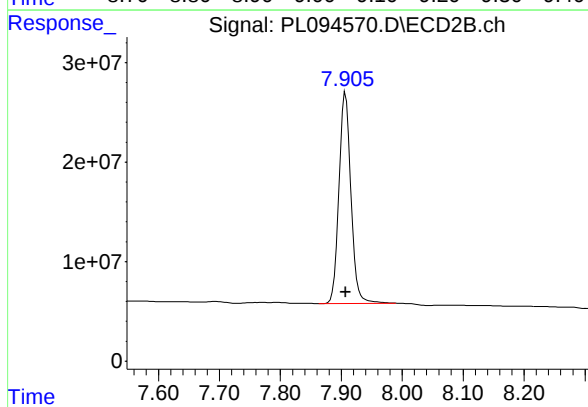

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 290138744
Conc: 74.25 ng/ml