
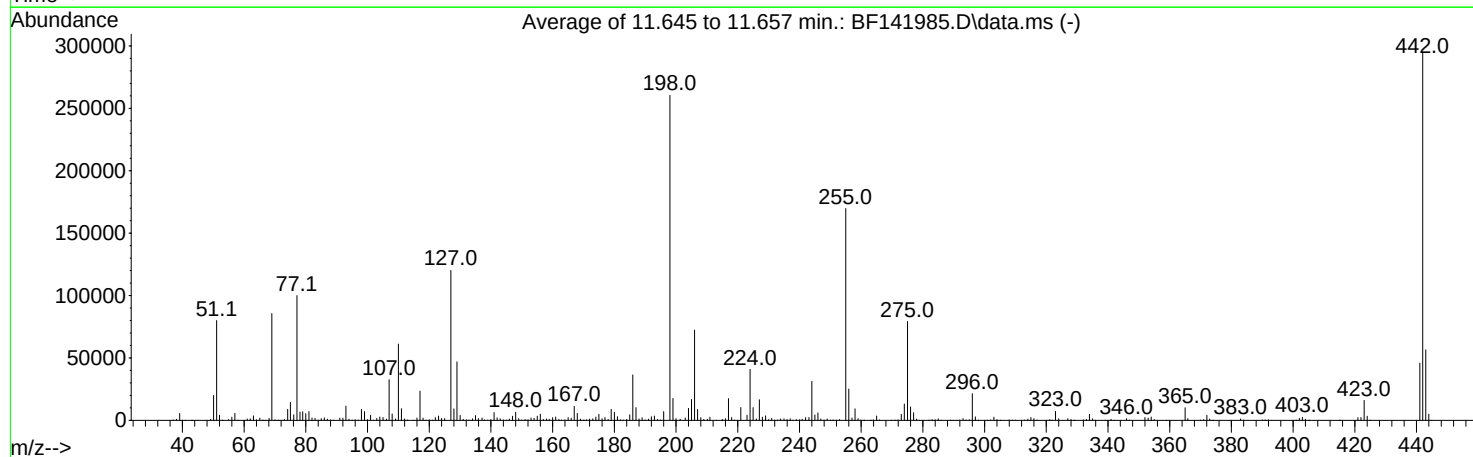


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031825\
Data File : BF141985.D
Acq On : 18 Mar 2025 09:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

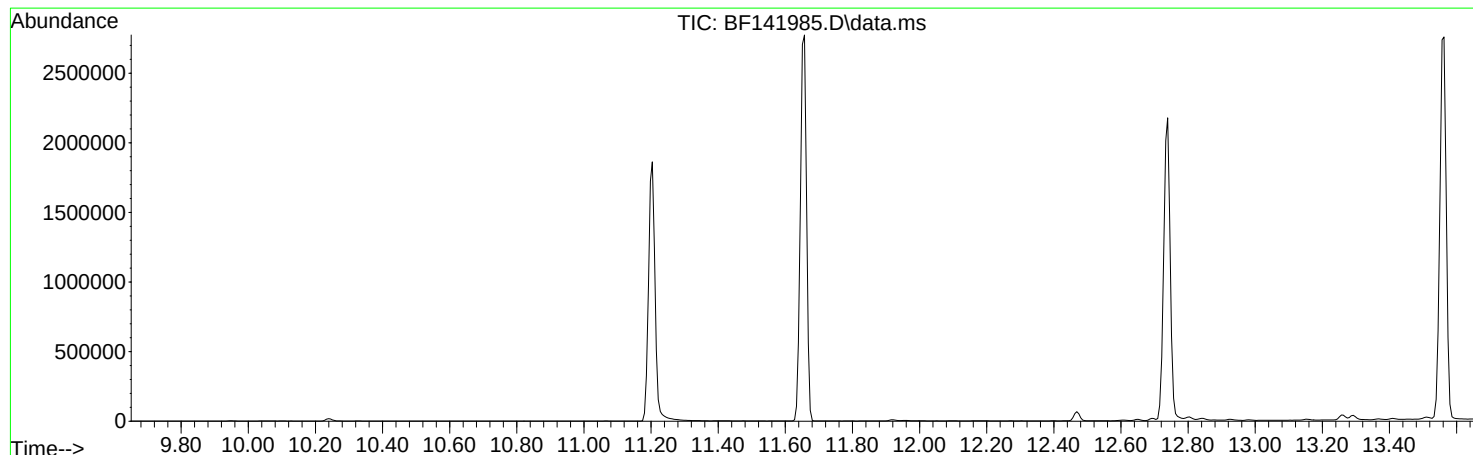

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.7	79971	PASS
68	69	0.00	2	1.9	1651	PASS
69	198	0.00	100	32.9	85619	PASS
70	69	0.00	2	0.5	469	PASS
127	198	10	80	46.1	120128	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	260395	PASS
199	198	5	9	6.8	17608	PASS
275	198	10	60	30.4	79213	PASS
365	198	1	100	3.9	10146	PASS
441	198	0.01	100	17.6	45773	PASS
442	442	50	100	100.0	294741	PASS
443	442	15	24	19.2	56528	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/18/2025	BNA_F	<u>BF141985.D</u>
Compound Name	Response	Retention Time
DDT	746688	13.563
DDD	17727	13.263
DDE	2161	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19888	766576	2.59

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031825\
Data File : BF141985.D
Acq On : 18 Mar 2025 09:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 18 11:21:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

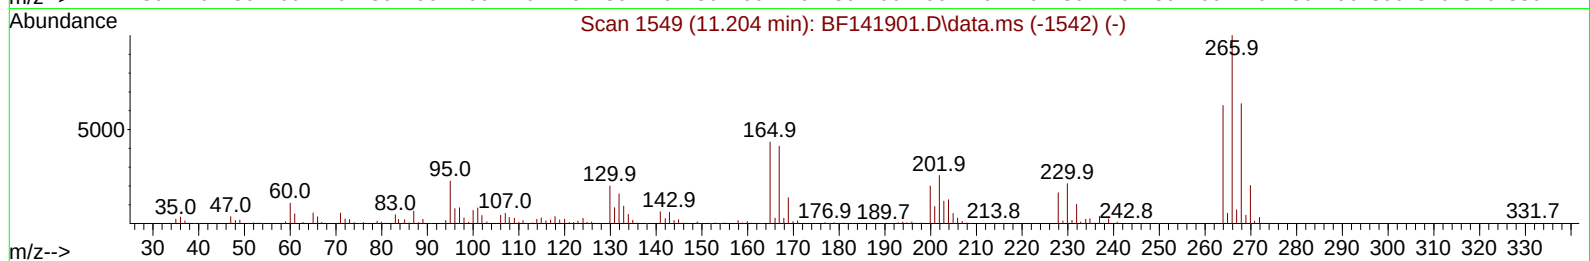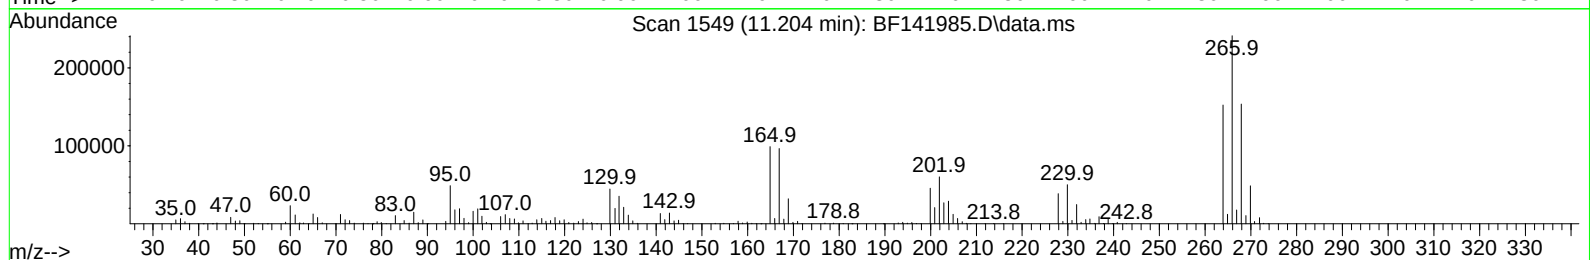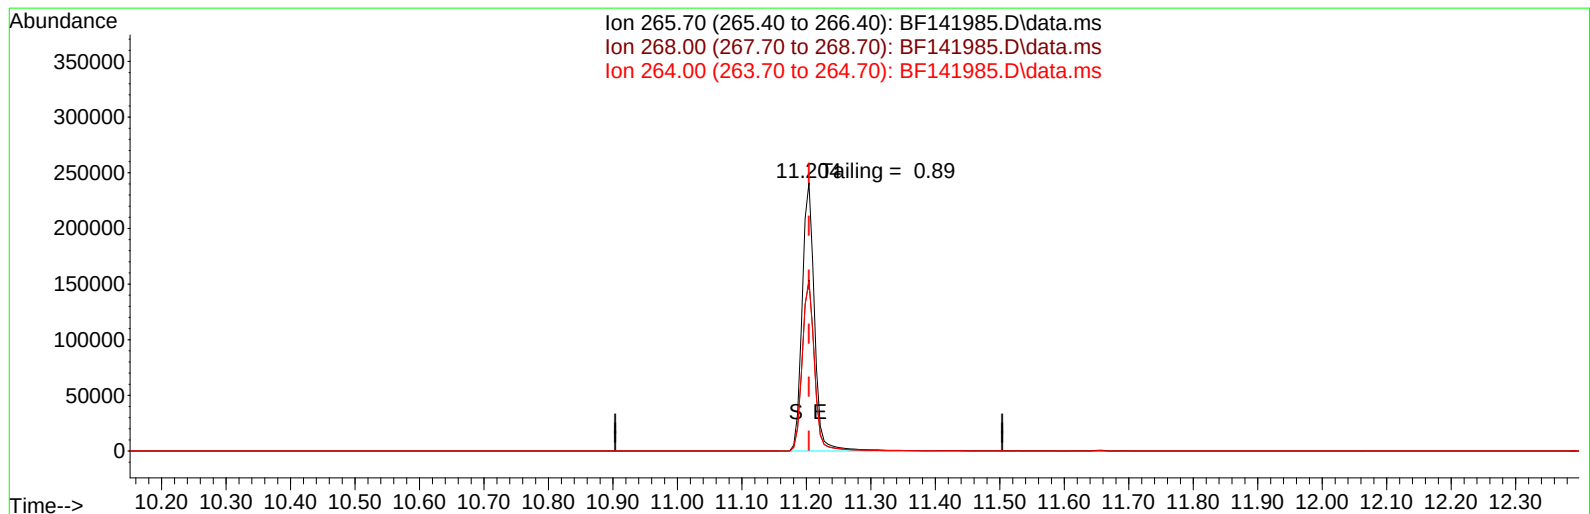

TIC: BF141985.D\data.ms

(70) Pentachlorophenol (C)

11.204min (+ 0.000) 55437.20 ng




response 323218

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.67
264.00	62.70	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031825\
Data File : BF141985.D
Acq On : 18 Mar 2025 09:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 18 11:21:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

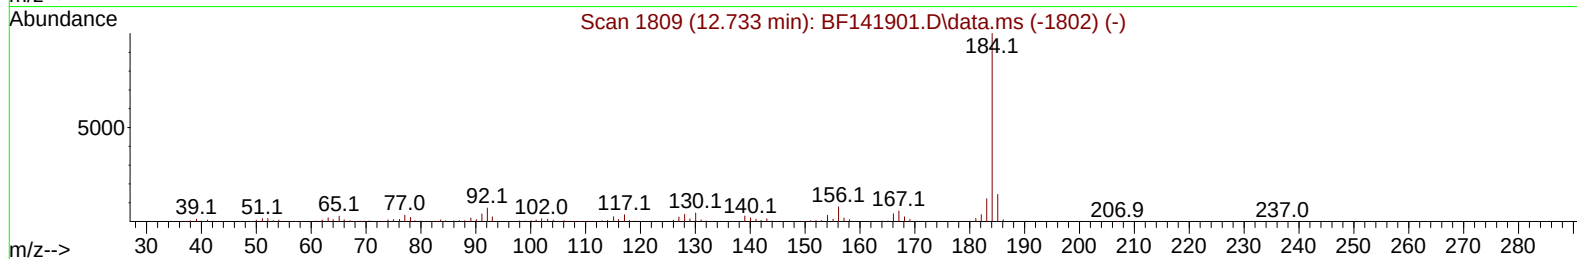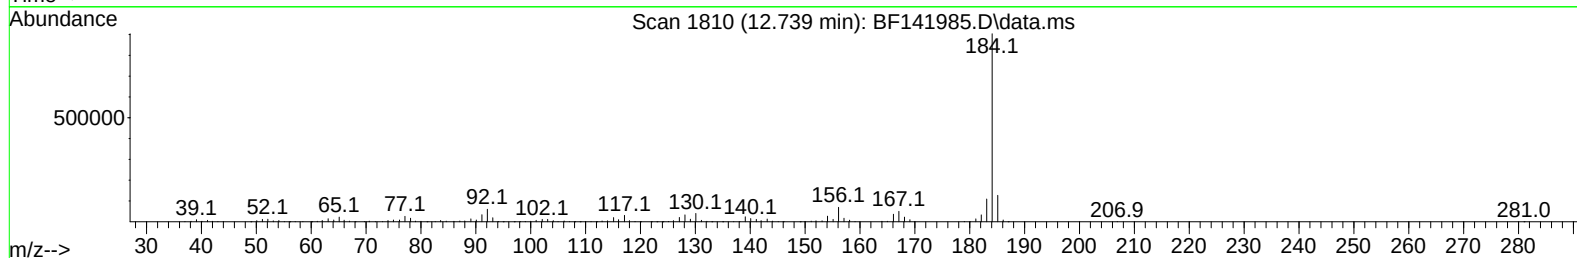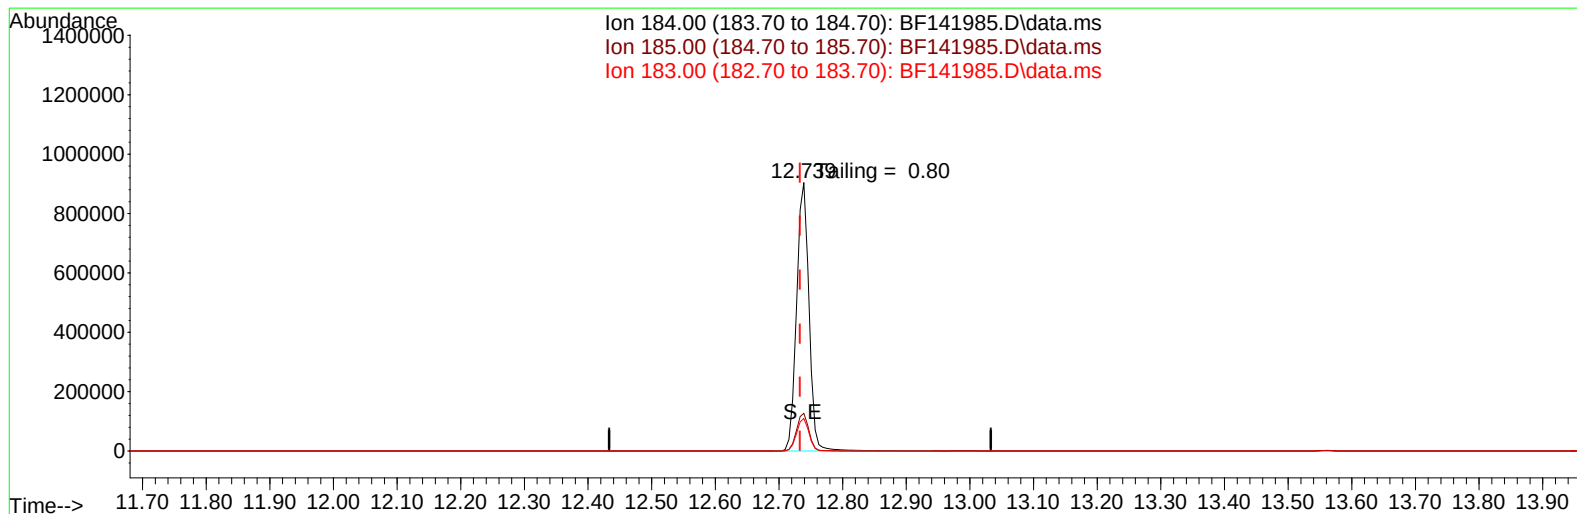

TIC: BF141985.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 128113.33 ng

response 1226172

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.06
183.00	12.10	12.12
0.00	0.00	0.00