

Cover Page

Order ID : Q1574

Project ID : Ave L

Client : G Environmental

Lab Sample Number

Q1574-01
Q1574-02

Client Sample Number

WC1
WC1

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : _____

Date: 3/19/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: Q1574

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication,airbill, sample management lab chronicle, login page)

✓

Check chain-of-custody for proper relinquish/return of samples

✓

Is the chain of custody signed and complete

✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts

✓

Collect information for each project id from server. Were all requirements followed

✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page

✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody

✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results

✓

Do requested analyses on Chain of Custody agree with the log-in page

✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Custody

✓

Were the samples received within hold time

✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle

✓

ANALYTICAL:

Was method requirement followed?

✓

Was client requirement followed?

✓

Does the case narrative summarize all QC failure?

✓

All runlogs and manual integration are reviewed for requirements

✓

All manual calculations and /or hand notations verified

✓

QA Review Signature: MAHESH PATEL

Date: 03/19/2025

LAB CHRONICLE

OrderID:	Q1574	OrderDate:	3/14/2025 11:25:00 AM
Client:	G Environmental	Project:	Ave L
Contact:	Gary Landis	Location:	I41,VOA Ref. #2 Soil

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q1574-01	WC1	SOIL	PCB	8082A	03/12/25	03/14/25	03/17/25	03/14/25
Q1574-01DL	WC1DL	SOIL	PCB	8082A	03/12/25	03/14/25	03/17/25	03/14/25

Hit Summary Sheet
SW-846

SDG No.: Q1574

Order ID: Q1574

Client: G Environmental

Project ID: Ave L

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
Client ID : Q1574-01	WC1 WC1	SOIL	Aroclor-1254	884	E	3.30	17.3	ug/kg
Total Concentration:				884.000				
Client ID : Q1574-01DL	WC1DL WC1DL	SOIL	Aroclor-1254	873	D	16.4	86.6	ug/kg
Total Concentration:				873.000				



QC SUMMARY

Surrogate Summary

SDG No.: **Q1574**

Client: **G Environmental**

Analytical Method: **8082A**

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Rec	Qual	Limits	
								Low	High
I.BLK-PO109425.D	PIBLK-PO109425.D	Tetrachloro-m-xylene	1	20	25.3	126		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	25.3	126		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	24.1	121		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	25.5	127		70 (60)	130 (140)
I.BLK-PO109927.D	PIBLK-PO109927.D	Tetrachloro-m-xylene	1	20	20.0	100		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	17.1	86		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	20.4	102		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	17.4	87		70 (60)	130 (140)
Q1574-01	WC1	Tetrachloro-m-xylene	1	20	18.4	92		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	27.8	139		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	19.8	99		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	23.6	118		30 (32)	150 (175)
Q1574-01DL	WC1DL	Tetrachloro-m-xylene	1	20	20.4	102		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	32.6	163	*	30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	18.6	93		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	23.8	119		30 (32)	150 (175)
I.BLK-PO109939.D	PIBLK-PO109939.D	Tetrachloro-m-xylene	1	20	20.4	102		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	17.6	88		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	20.5	103		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	16.5	83		70 (60)	130 (140)
I.BLK-PP070418.D	PIBLK-PP070418.D	Tetrachloro-m-xylene	1	20	22.0	110		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	23.1	116		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	23.0	115		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	23.5	117		70 (60)	130 (140)
I.BLK-PP070547.D	PIBLK-PP070547.D	Tetrachloro-m-xylene	1	20	19.5	97		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	20.3	101		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	20.5	102		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	20.4	102		70 (60)	130 (140)
PB167143BL	PB167143BL	Tetrachloro-m-xylene	1	20	20.4	102		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	21.2	106		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	21.4	107		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	21.0	105		30 (32)	150 (175)
PB167143BS	PB167143BS	Tetrachloro-m-xylene	1	20	21.4	107		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	21.8	109		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	21.7	108		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	20.0	100		30 (32)	150 (175)
I.BLK-PP070562.D	PIBLK-PP070562.D	Tetrachloro-m-xylene	1	20	20.1	100		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	20.9	104		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	21.2	106		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	20.2	101		70 (60)	130 (140)
Q1572-06MS	C0018MS	Tetrachloro-m-xylene	1	20	20.3	101		30 (32)	150 (144)

() = LABORATORY INHOUSE LIMIT

Surrogate Summary

SDG No.: Q1574

Client: G Environmental

Analytical Method: 8082A

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Rec	Qual	Limits	
								Low	High
Q1572-06MS	C0O18MS	Decachlorobiphenyl	1	20	21.8	109		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	19.0	95		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	34.0	170	*	30 (32)	150 (175)
Q1572-06MSD	C0O18MSD	Tetrachloro-m-xylene	1	20	20.8	104		30 (32)	150 (144)
		Decachlorobiphenyl	1	20	22.3	112		30 (32)	150 (175)
		Tetrachloro-m-xylene	2	20	19.6	98		30 (32)	150 (144)
		Decachlorobiphenyl	2	20	33.2	166	*	30 (32)	150 (175)
I.BLK-PP070572.D	PIBLK-PP070572.D	Tetrachloro-m-xylene	1	20	20.2	101		70 (60)	130 (140)
		Decachlorobiphenyl	1	20	21.0	105		70 (60)	130 (140)
		Tetrachloro-m-xylene	2	20	21.1	105		70 (60)	130 (140)
		Decachlorobiphenyl	2	20	20.5	102		70 (60)	130 (140)

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: Q1574

Client: G Environmental

Analytical Method: 8082A

DataFile : PP070564.D

Lab Sample ID:	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Low	Limits High	RPD
Client Sample ID:	C0018MS											
Q1572-06MS	AR1016	218.8	0	16000	ug/kg	7313	*			40 (55)	140 (146)	
	AR1260	218.8	951	1300	ug/kg	160	*			40 (31)	140 (146)	

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: Q1574

Client: G Environmental

Analytical Method: 8082A

DataFile : PP070565.D

Lab Sample ID:	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Low	Limits High	RPD
Client Sample ID:	C0018MSD											
Q1572-06MSD	AR1016	218.6	0	17000	ug/kg	7777	*	6		40 (55)	140 (146)	30 (20)
	AR1260	218.6	951	1400	ug/kg	205	*	25		40 (31)	140 (146)	30 (20)



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q1574

Client: G Environmental

Analytical Method: 8082A Datafile : PP070549.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD		Limits	
								Qual	Low	High	RPD
PB167143BS	AR1016	166.5	152	ug/kg	91				40 (71)	140 (120)	
	AR1260	166.5	145	ug/kg	87				40 (65)	140 (130)	

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB167143BL

Lab Name: CHEMTECH

Contract: GENV01

Lab Code: CHEM Case No.: Q1574

SAS No.: Q1574 SDG NO.: Q1574

Lab Sample ID: PB167143BL

Lab File ID: PP070548.D

Matrix: (soil/water) Solid

Extraction: (Type) SOXH

Sulfur Cleanup: (Y/N) N

Date Extracted: 03/14/2025

Date Analyzed (1): 03/14/2025

Date Analyzed (2): 03/14/2025

Time Analyzed (1): 22:36

Time Analyzed (2): 22:36

Instrument ID (1): ECD_P

Instrument ID (2): ECD_P

GC Column (1): ZB-MR1 ID: 0.32 (mm)

GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
WC1	Q1574-01	PO109929.D	03/17/2025	03/17/2025
PB167143BS	PB167143BS	PP070549.D	03/14/2025	03/14/2025
C0018MS	Q1572-06MS	PP070564.D	03/15/2025	03/15/2025
C0018MSD	Q1572-06MSD	PP070565.D	03/15/2025	03/15/2025

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	G Environmental	Date Collected:	03/12/25
Project:	Ave L	Date Received:	03/14/25
Client Sample ID:	WC1	SDG No.:	Q1574
Lab Sample ID:	Q1574-01	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	98
Sample Wt/Vol:	30.05	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109929.D	1	03/14/25 12:25	03/17/25 11:02	PB167143

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	4.00	U	4.00	17.3	ug/kg
11104-28-2	Aroclor-1221	4.10	U	4.10	17.3	ug/kg
11141-16-5	Aroclor-1232	3.80	U	3.80	17.3	ug/kg
53469-21-9	Aroclor-1242	4.10	U	4.10	17.3	ug/kg
12672-29-6	Aroclor-1248	6.00	U	6.00	17.3	ug/kg
11097-69-1	Aroclor-1254	884	E	3.30	17.3	ug/kg
37324-23-5	Aroclor-1262	5.10	U	5.10	17.3	ug/kg
11100-14-4	Aroclor-1268	3.70	U	3.70	17.3	ug/kg
11096-82-5	Aroclor-1260	3.30	U	3.30	17.3	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.8		30 (32) - 150 (144)	99%	SPK: 20
2051-24-3	Decachlorobiphenyl	27.8		30 (32) - 150 (175)	139%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031725\
 Data File : P0109929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2025 11:02
 Operator : YP/AJ
 Sample : Q1574-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/18/2025
 Supervised By :mohammad ahmed 03/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 01:31:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.693	3.690	174.6E6	103.8E6	18.451m	19.840m
2) SA Decachlor...	8.746	8.698	239.0E6	74993218	27.781m	23.551m
Target Compounds						
26) L6 AR-1254-1	5.596	5.575	727.6E6	414.4E6	1411.125	1584.419
27) L6 AR-1254-2	5.747	5.725	1385.9E6	754.3E6	3077.166	3215.895
28) L6 AR-1254-3	6.151	6.126	1744.0E6	955.1E6	2435.935	2677.679
29) L6 AR-1254-4	6.381	6.354	792.6E6	405.4E6	1892.559	2098.957
30) L6 AR-1254-5	6.800	6.771	1997.8E6	1021.0E6	3202.124	3440.956

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031725\
Data File : PO109929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2025 11:02
Operator : YP/AJ
Sample : Q1574-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2025
Supervised By :mohammad ahmed 03/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 01:31:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm






#1 Tetrachloro-m-xylene

R.T.: 3.693 min
Delta R.T.: -0.005 min
Response: 174643017
Conc: 18.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2025
Supervised By :mohammad ahmed 03/19/2025




#1 Tetrachloro-m-xylene

R.T.: 3.690 min
Delta R.T.: -0.003 min
Response: 103846867
Conc: 19.84 ng/ml




#2 Decachlorobiphenyl

R.T.: 8.746 min
Delta R.T.: -0.010 min
Response: 238970894
Conc: 27.78 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.698 min
Delta R.T.: -0.009 min
Response: 74993218
Conc: 23.55 ng/ml




#26 AR-1254-1

R.T.: 5.596 min
Delta R.T.: -0.005 min
Response: 727585264
Conc: 1411.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2025
Supervised By :mohammad ahmed 03/19/2025




#26 AR-1254-1

R.T.: 5.575 min
Delta R.T.: -0.003 min
Response: 414386173
Conc: 1584.42 ng/ml




#27 AR-1254-2

R.T.: 5.747 min
Delta R.T.: -0.002 min
Response: 1385877209
Conc: 3077.17 ng/ml



#27 AR-1254-2

R.T.: 5.725 min
Delta R.T.: -0.001 min
Response: 754325007
Conc: 3215.90 ng/ml




#28 AR-1254-3

R.T.: 6.151 min
Delta R.T.: -0.004 min
Response: 1744021014
Conc: 2435.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2025
Supervised By :mohammad ahmed 03/19/2025




#28 AR-1254-3

R.T.: 6.126 min
Delta R.T.: -0.003 min
Response: 955140431
Conc: 2677.68 ng/ml




#29 AR-1254-4

R.T.: 6.381 min
Delta R.T.: -0.003 min
Response: 792587825
Conc: 1892.56 ng/ml



#29 AR-1254-4

R.T.: 6.354 min
Delta R.T.: -0.002 min
Response: 405357688
Conc: 2098.96 ng/ml




#30 AR-1254-5

R.T.: 6.800 min
Delta R.T.: -0.005 min
Response: 1997814415
Conc: 3202.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2025
Supervised By :mohammad ahmed 03/19/2025



#30 AR-1254-5

R.T.: 6.771 min
Delta R.T.: -0.004 min
Response: 1021042534
Conc: 3440.96 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	03/12/25
Project:	Ave L	Date Received:	03/14/25
Client Sample ID:	WC1DL	SDG No.:	Q1574
Lab Sample ID:	Q1574-01DL	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	98
Sample Wt/Vol:	30.05	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109930.D	5	03/14/25 12:25	03/17/25 11:20	PB167143

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	20.1	UD	20.1	86.6	ug/kg
11104-28-2	Aroclor-1221	20.5	UD	20.5	86.6	ug/kg
11141-16-5	Aroclor-1232	18.9	UD	18.9	86.6	ug/kg
53469-21-9	Aroclor-1242	20.4	UD	20.4	86.6	ug/kg
12672-29-6	Aroclor-1248	30.2	UD	30.2	86.6	ug/kg
11097-69-1	Aroclor-1254	873	D	16.4	86.6	ug/kg
37324-23-5	Aroclor-1262	25.6	UD	25.6	86.6	ug/kg
11100-14-4	Aroclor-1268	18.3	UD	18.3	86.6	ug/kg
11096-82-5	Aroclor-1260	16.5	UD	16.5	86.6	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.4		30 (32) - 150 (144)	102%	SPK: 20
2051-24-3	Decachlorobiphenyl	32.6	*	30 (32) - 150 (175)	163%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031725\
 Data File : P0109930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2025 11:20
 Operator : YP/AJ
 Sample : Q1574-01DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC1DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/18/2025
 Supervised By :mohammad ahmed 03/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 01:31:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.691	3.690	38517181	19398431	4.069m	3.706m
2) SA Decachlor...	8.743	8.694	56138249	15115079	6.526m	4.747 #
Target Compounds						
26) L6 AR-1254-1	5.593	5.574	145.7E6	85137355	282.609	325.525
27) L6 AR-1254-2	5.743	5.723	255.1E6	147.3E6	566.324	627.941
28) L6 AR-1254-3	6.148	6.124	398.3E6	195.8E6	556.326	548.986
29) L6 AR-1254-4	6.377	6.352	152.2E6	78620421	363.346	407.099
30) L6 AR-1254-5	6.797	6.769	375.5E6	196.5E6	601.928	662.147

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031725\
Data File : PO109930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2025 11:20
Operator : YP/AJ
Sample : Q1574-01DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC1DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2025
Supervised By :mohammad ahmed 03/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 01:31:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm






#1 Tetrachloro-m-xylene

R.T.: 3.691 min
Delta R.T.: -0.007 min
Response: 38517181
Conc: 4.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC1DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2025
Supervised By :mohammad ahmed 03/19/2025




#1 Tetrachloro-m-xylene

R.T.: 3.690 min
Delta R.T.: -0.004 min
Response: 19398431
Conc: 3.71 ng/ml




#2 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: -0.014 min
Response: 56138249
Conc: 6.53 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: -0.013 min
Response: 15115079
Conc: 4.75 ng/ml




#26 AR-1254-1

R.T.: 5.593 min
Delta R.T.: -0.008 min
Response: 145715232
Conc: 282.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC1DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2025
Supervised By :mohammad ahmed 03/19/2025




#26 AR-1254-1

R.T.: 5.574 min
Delta R.T.: -0.005 min
Response: 85137355
Conc: 325.53 ng/ml




#27 AR-1254-2

R.T.: 5.743 min
Delta R.T.: -0.006 min
Response: 255057892
Conc: 566.32 ng/ml



#27 AR-1254-2

R.T.: 5.723 min
Delta R.T.: -0.003 min
Response: 147290675
Conc: 627.94 ng/ml




#28 AR-1254-3

R.T.: 6.148 min
Delta R.T.: -0.007 min
Response: 398304349
Conc: 556.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC1DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2025
Supervised By :mohammad ahmed 03/19/2025




#28 AR-1254-3

R.T.: 6.124 min
Delta R.T.: -0.004 min
Response: 195825658
Conc: 548.99 ng/ml




#29 AR-1254-4

R.T.: 6.377 min
Delta R.T.: -0.008 min
Response: 152166046
Conc: 363.35 ng/ml



#29 AR-1254-4

R.T.: 6.352 min
Delta R.T.: -0.004 min
Response: 78620421
Conc: 407.10 ng/ml




#30 AR-1254-5

R.T.: 6.797 min
Delta R.T.: -0.009 min
Response: 375544516
Conc: 601.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC1DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/18/2025
Supervised By :mohammad ahmed 03/19/2025



#30 AR-1254-5

R.T.: 6.769 min
Delta R.T.: -0.005 min
Response: 196480360
Conc: 662.15 ng/ml



CALIBRATION SUMMARY

GC Column: ZB-MR1 ID: 0.32 (mm)

[illegible]

[illegible]

RETENTION TIMES OF INITIAL CALIBRATION

Contract:	<u>GENV01</u>						
Lab Code:	<u>CHEM</u>	Case No.:	<u>Q1574</u>	SAS No.:	<u>Q1574</u>	SDG NO.:	<u>Q1574</u>
Instrument ID:	<u>ECD_O</u>	Calibration Date(s):		<u>02/20/2025</u>	<u>02/21/2025</u>		
		Calibration Times:		<u>16:46</u>	<u>01:02</u>		

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID: RT 1000 = PO109426.D RT 750 = PO109427.D
RT 500 = PO109428.D RT 250 = PO109429.D RT 050 = PO109430.D

[illegible]

[illegible]

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: GENV01
Lab Code: CHEM **Case No.:** Q1574 **SAS No.:** Q1574 **SDG NO.:** Q1574
Instrument ID: ECD_O **Calibration Date(s):** 02/20/2025 02/21/2025
Calibration Times: 16:46 01:02

GC Column: ZB-MR1 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO109426.D</u>		CF 750 = <u>PO109427.D</u>			
CF 500 = <u>PO109428.D</u>		CF 250 = <u>PO109429.D</u>		CF 050 = <u>PO109430.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	285955176	296470909	301678880	330073932	327272520	308290283
Aroclor-1016-2	(2)	400344510	409149469	414645114	446605912	434387780	421026557
Aroclor-1016-3	(3)	275712654	284750529	289403798	321232168	307985600	295816950
Aroclor-1016-4	(4)	217819857	224475380	225979744	249359212	241266360	231780111
Aroclor-1016-5	(5)	234915990	244172492	252269048	280073416	279718840	258229957
Aroclor-1260-1	(1)	432857882	445030616	458030860	496965692	497771560	466131322
Aroclor-1260-2	(2)	530613873	540598143	549997768	596865796	607516180	565118352
Aroclor-1260-3	(3)	446055940	458685821	463532386	505033376	504998020	475661109
Aroclor-1260-4	(4)	409227231	417077069	426071740	458083200	447546300	431601108
Aroclor-1260-5	(5)	975246933	982402905	1001465846	1034939896	975352280	993881572
Decachlorobiphenyl		8144381710	8253336907	8542716440	9068866760	9000001000	8601860563
Tetrachloro-m-xylene		9594159870	9382441773	9407964980	9839303320	9101752600	9465124509
Aroclor-1242-1	(1)	241553792	248781753	263582376	278206104	276700060	261764817
Aroclor-1242-2	(2)	330250979	341141312	360022594	377835792	370979720	356046079
Aroclor-1242-3	(3)	230958690	239403319	256570990	271941764	257976860	251370325
Aroclor-1242-4	(4)	181873604	188232188	200194694	210194852	201763980	196451864
Aroclor-1242-5	(5)	192196869	198312276	212424054	232317448	236630280	214376185
Decachlorobiphenyl		7571460160	7783053733	8197005760	8686332120	8704566000	8188483555
Tetrachloro-m-xylene		9236931880	9400204853	9446860340	9568057960	9056865000	9341784007
Aroclor-1248-1	(1)	183385441	189253437	200901320	213658596	210346400	199509039
Aroclor-1248-2	(2)	249519113	262229969	281655510	299590856	298458120	278290714
Aroclor-1248-3	(3)	313646829	324719312	346217716	370103360	392176240	349372691
Aroclor-1248-4	(4)	439951399	452724037	479184310	509535492	504078340	477094716
Aroclor-1248-5	(5)	310476659	318507132	337630456	365736804	380196620	342509534
Decachlorobiphenyl		7703959900	7913043760	8337132500	8816038680	8879579800	8329950928
Tetrachloro-m-xylene		9154374770	9319706587	9763537060	9884300480	9250244600	9474432699
Aroclor-1254-1	(1)	480630669	491242291	514290722	548494120	543375540	515606668
Aroclor-1254-2	(2)	417535343	429223996	451482582	481224324	472406420	450374533
Aroclor-1254-3	(3)	684838056	697322969	725628940	760808456	711178620	715955408
Aroclor-1254-4	(4)	417970360	409808872	428749386	461366848	376062040	418791501
Aroclor-1254-5	(5)	597298518	608943563	631623464	663830224	617819000	623902954
Decachlorobiphenyl		7967092830	8125756000	8528343640	8986366600	8782372000	8477986214
Tetrachloro-m-xylene		9511051460	9602004080	9843620680	9994457760	8495604200	9489347636
Aroclor-1268-1	(1)	1298860853	1294002563	1318124330	1365675636	1344427900	1324218256



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	1196326079	1189492827	1207881780	1246550744	1205280700	1209106426	2
Aroclor-1268-3	(3)	1000400149	998939115	1012813102	1049647308	1029090160	1018177967	2
Aroclor-1268-4	(4)	407507962	408969772	420298422	442140308	445377360	424858765	4
Aroclor-1268-5	(5)	3060378797	3013397139	3036609122	3075360324	2912511720	3019651420	2
Decachlorobiphenyl		14147642890	14125651173	14472115980	15180190720	15441285400	14673377233	4
Tetrachloro-m-xylene		9652630020	9799388160	9953085600	10360200640	9708060200	9894672924	3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Instrument ID: ECD_O

Calibration Date(s): 02/20/2025 02/21/2025

Calibration Times: 16:46 01:02

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO109426.D</u>		CF 750 = <u>PO109427.D</u>			
CF 500 = <u>PO109428.D</u>		CF 250 = <u>PO109429.D</u>		CF 050 = <u>PO109430.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	144422659	148428763	152032096	167484860	168484300	7
Aroclor-1016-2	(2)	205202725	208508729	213432994	229519564	225505040	5
Aroclor-1016-3	(3)	112302196	115067393	117212622	128579748	124094120	6
Aroclor-1016-4	(4)	94709981	98717735	101165102	112923876	112836120	8
Aroclor-1016-5	(5)	124417087	127943616	132644098	146345704	149917060	8
Aroclor-1260-1	(1)	217936136	223782013	232739904	251644640	258495520	7
Aroclor-1260-2	(2)	255563339	259366392	268832038	291215424	300878620	7
Aroclor-1260-3	(3)	239301078	242165468	249897958	270279452	273707020	6
Aroclor-1260-4	(4)	193987222	196916529	202218624	218214048	219624820	6
Aroclor-1260-5	(5)	436097628	435546231	443785112	464386884	459099080	3
Decachlorobiphenyl		2971514290	3027039307	3156019460	3385128400	3381593200	6
Tetrachloro-m-xylene		5186272490	5246400280	5221242400	5478386840	5038748400	3
Aroclor-1242-1	(1)	120966720	124746516	133128702	141428800	141463920	7
Aroclor-1242-2	(2)	169605960	173512545	183266616	192017376	189176180	5
Aroclor-1242-3	(3)	93390359	96634075	102245092	107691940	99411220	5
Aroclor-1242-4	(4)	96389066	101019272	107789002	115338428	114056640	8
Aroclor-1242-5	(5)	113196636	117716005	125239314	135801980	136573300	8
Decachlorobiphenyl		2727823240	2861750760	3019178360	3243379080	3243962600	8
Tetrachloro-m-xylene		5001213420	5078322907	5254229320	5289448280	4851665000	4
Aroclor-1248-1	(1)	91256927	94139561	100767396	107614600	108857060	8
Aroclor-1248-2	(2)	130560541	136645137	146421094	157143508	156628300	8
Aroclor-1248-3	(3)	139283148	144897643	155701690	166430352	168727860	8
Aroclor-1248-4	(4)	163903044	169411200	180364434	193711724	196594760	8
Aroclor-1248-5	(5)	154356880	158447996	169575560	183331920	195308840	10
Decachlorobiphenyl		2790488700	2873613467	3038569420	3241156720	3294897400	7
Tetrachloro-m-xylene		4955293160	5040468413	5221131320	5264696400	4750589600	4
Aroclor-1254-1	(1)	243640751	248872624	260914738	280861344	273402140	6
Aroclor-1254-2	(2)	212545511	218679507	230680254	249214456	261687520	9
Aroclor-1254-3	(3)	339799719	346366689	360950750	378906048	357499640	4
Aroclor-1254-4	(4)	192329190	189854227	199746634	214807996	168878980	9
Aroclor-1254-5	(5)	278490681	283928981	296376396	314100456	310764660	5
Decachlorobiphenyl		2841760820	2921691133	3072525860	3310057280	3280037800	7
Tetrachloro-m-xylene		5117525260	5147853200	5214583540	5337931960	4481650800	7
Aroclor-1268-1	(1)	554131487	553810328	564174560	591076320	593868340	3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	512614105	511079256	520949472	543420336	536655740	524943782	3
Aroclor-1268-3	(3)	413643589	412567932	420525622	442592008	450889440	428043718	4
Aroclor-1268-4	(4)	153729603	155030577	163078820	169661456	165174880	161335067	4
Aroclor-1268-5	(5)	1087226853	1077982207	1085826158	1121186428	1093500600	1093144449	2
Decachlorobiphenyl		4950835750	4972853373	5123922200	5430816080	5582978400	5212281161	5
Tetrachloro-m-xylene		5266816140	5271127760	5328349480	5507659840	5128975000	5300585644	3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Instrument ID: ECD_O Date(s) Analyzed: 02/20/2025 02/21/2025

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.91	3.81	4.01	131879000
		2	4.00	3.90	4.10	98701000
		3	4.07	3.97	4.17	269838000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.07	3.97	4.17	208928000
		2	4.57	4.47	4.67	116083000
		3	4.81	4.71	4.91	201936000
		4	4.99	4.89	5.09	111220000
		5	5.03	4.93	5.13	81668600
Aroclor-1262	500	1	6.85	6.75	6.95	665842000
		2	7.35	7.25	7.45	1129720000
		3	7.63	7.53	7.73	448264000
		4	7.70	7.60	7.80	829210000
		5	8.19	8.09	8.29	373330000



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Instrument ID: ECD_O Date(s) Analyzed: 02/20/2025 02/21/2025

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.91	3.81	4.01	68502400
		2	3.99	3.89	4.09	51339800
		3	4.07	3.97	4.17	145428000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.07	3.97	4.17	111462000
		2	4.80	4.70	4.90	103317000
		3	4.97	4.87	5.07	56771800
		4	5.06	4.96	5.16	54894600
		5	5.23	5.13	5.33	58805000
Aroclor-1262	500	1	6.81	6.71	6.91	317212000
		2	7.31	7.21	7.41	498620000
		3	7.60	7.50	7.70	196255000
		4	7.66	7.56	7.76	354890000
		5	8.15	8.05	8.25	143138000

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 16:46
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:01:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:00:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	959.4E6	518.6E6	101.979	99.330
2) SA Decachlor...	8.757	8.706	814.4E6	297.2E6	95.337	94.154
Target Compounds						
3) L1 AR-1016-1	4.792	4.777	286.0E6	144.4E6	947.879	949.948
4) L1 AR-1016-2	4.811	4.797	400.3E6	205.2E6	965.511	961.439
5) L1 AR-1016-3	4.867	4.972	275.7E6	112.3E6	952.692	958.107
6) L1 AR-1016-4	4.988	5.014	217.8E6	94709981	963.891	936.192
7) L1 AR-1016-5	5.246	5.228	234.9E6	124.4E6	931.212	937.977
31) L7 AR-1260-1	6.288	6.261	432.9E6	217.9E6	945.041	936.394
32) L7 AR-1260-2	6.477	6.448	530.6E6	255.6E6	964.756	950.643
33) L7 AR-1260-3	6.845	6.602	446.1E6	239.3E6	962.297	957.595
34) L7 AR-1260-4	7.106	7.073	409.2E6	194.0E6	960.466	959.295
35) L7 AR-1260-5	7.347	7.314	975.2E6	436.1E6	973.819	982.677



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 16:46
Operator : YP/AJ
Sample : AR1660ICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:01:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:00:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 17:04
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:01:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:00:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	703.7E6	393.5E6	74.797	75.361
2) SA Decachlor...	8.756	8.707	619.0E6	227.0E6	72.459	71.935
Target Compounds						
3) L1 AR-1016-1	4.792	4.777	222.4E6	111.3E6	737.053	732.224
4) L1 AR-1016-2	4.811	4.797	306.9E6	156.4E6	740.060	732.696
5) L1 AR-1016-3	4.868	4.972	213.6E6	86300545	737.941	736.273
6) L1 AR-1016-4	4.988	5.014	168.4E6	74038301	745.007	731.856
7) L1 AR-1016-5	5.246	5.227	183.1E6	95957712	725.929	723.422
31) L7 AR-1260-1	6.288	6.261	333.8E6	167.8E6	728.713	721.133
32) L7 AR-1260-2	6.477	6.448	405.4E6	194.5E6	737.182	723.592
33) L7 AR-1260-3	6.845	6.602	344.0E6	181.6E6	742.158	726.793
34) L7 AR-1260-4	7.106	7.073	312.8E6	147.7E6	734.167	730.335
35) L7 AR-1260-5	7.347	7.314	736.8E6	326.7E6	735.724	736.076



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 17:04
Operator : YP/AJ
Sample : AR1660ICC750
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:01:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:00:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 17:23
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:01:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:00:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.698	3.694	470.4E6	261.1E6	50.000	50.000
2) SA Decachlor...	8.757	8.707	427.1E6	157.8E6	50.000	50.000
Target Compounds						
3) L1 AR-1016-1	4.791	4.778	150.8E6	76016048	500.000	500.000
4) L1 AR-1016-2	4.811	4.797	207.3E6	106.7E6	500.000	500.000
5) L1 AR-1016-3	4.867	4.972	144.7E6	58606311	500.000	500.000
6) L1 AR-1016-4	4.988	5.014	113.0E6	50582551	500.000	500.000
7) L1 AR-1016-5	5.245	5.227	126.1E6	66322049	500.000	500.000
31) L7 AR-1260-1	6.288	6.261	229.0E6	116.4E6	500.000	500.000
32) L7 AR-1260-2	6.477	6.448	275.0E6	134.4E6	500.000	500.000
33) L7 AR-1260-3	6.846	6.602	231.8E6	124.9E6	500.000	500.000
34) L7 AR-1260-4	7.105	7.074	213.0E6	101.1E6	500.000	500.000
35) L7 AR-1260-5	7.347	7.314	500.7E6	221.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 17:23
Operator : YP/AJ
Sample : AR1660ICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:01:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:00:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 17:41
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:02:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:00:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	246.0E6	137.0E6	26.146	26.231
2) SA Decachlor...	8.756	8.706	226.7E6	84628210	26.540	26.815
Target Compounds						
3) L1 AR-1016-1	4.792	4.777	82518483	41871215	273.531	275.410
4) L1 AR-1016-2	4.811	4.797	111.7E6	57379891	269.270	268.843
5) L1 AR-1016-3	4.867	4.972	80308042	32144937	277.495	274.245
6) L1 AR-1016-4	4.988	5.014	62339803	28230969	275.865	279.058
7) L1 AR-1016-5	5.245	5.227	70018354	36586426	277.554	275.824
31) L7 AR-1260-1	6.288	6.261	124.2E6	62911160	271.251	270.307
32) L7 AR-1260-2	6.477	6.448	149.2E6	72803856	271.304	270.815
33) L7 AR-1260-3	6.845	6.602	126.3E6	67569863	272.383	270.390
34) L7 AR-1260-4	7.105	7.073	114.5E6	54553512	268.783	269.775
35) L7 AR-1260-5	7.347	7.313	258.7E6	116.1E6	258.356	261.606



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 17:41
Operator : YP/AJ
Sample : AR1660ICC250
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:02:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:00:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 17:59
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:02:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:00:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	45508763	25193742	4.837	4.825
2) SA Decachlor...	8.755	8.705	45000005	16907966	5.268	5.357
Target Compounds						
3) L1 AR-1016-1	4.792	4.777	16363626	8424215	54.242	55.411
4) L1 AR-1016-2	4.812	4.796	21719389	11275252	52.381	52.828
5) L1 AR-1016-3	4.867	4.972	15399280	6204706	53.210	52.935
6) L1 AR-1016-4	4.988	5.014	12063318	5641806	53.382	55.768
7) L1 AR-1016-5	5.246	5.227	13985942	7495853	55.441	56.511
31) L7 AR-1260-1	6.287	6.261	24888578	12924776	54.338	55.533
32) L7 AR-1260-2	6.476	6.448	30375809	15043931	55.229	55.960
33) L7 AR-1260-3	6.844	6.601	25249901	13685351	54.473	54.764
34) L7 AR-1260-4	7.104	7.073	22377315	10981241	52.520	54.304
35) L7 AR-1260-5	7.346	7.313	48767614	22954954	48.696	51.725



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 17:59
Operator : YP/AJ
Sample : AR1660ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:02:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:00:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 18:18
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:14:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:14:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	493.2E6	265.7E6	50.000	50.000
2) SA Decachlor...	8.755	8.707	432.4E6	160.0E6	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	3.910	3.905	65939528	34251207	500.000	500.000
9) L2 AR-1221-2	3.997	3.990	49350500	25669896	500.000	500.000
10) L2 AR-1221-3	4.074	4.066	134.9E6	72714061	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 18:18
Operator : YP/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:14:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:14:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 18:36
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:23:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:22:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	461.7E6	262.6E6	50.000	50.000
2) SA Decachlor...	8.757	8.706	402.2E6	149.0E6	50.000	50.000
Target Compounds						
11) L3 AR-1232-1	4.074	4.066	104.5E6	55730818	500.000	500.000
12) L3 AR-1232-2	4.569	4.796	58041447	51658633	500.000	500.000
13) L3 AR-1232-3	4.811	4.972	101.0E6	28385926	500.000	500.000
14) L3 AR-1232-4	4.988	5.056	55610100	27447264	500.000	500.000
15) L3 AR-1232-5	5.030	5.227	40834319	29402463	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 18:36
Operator : YP/AJ
Sample : AR1232ICC500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:23:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:22:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 18:55
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:27:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:26:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	923.7E6	500.1E6	97.778	95.185
2) SA Decachlor...	8.755	8.706	757.1E6	272.8E6	92.369	90.350
Target Compounds						
16) L4 AR-1242-1	4.792	4.777	241.6E6	121.0E6	916.426	908.645
17) L4 AR-1242-2	4.811	4.797	330.3E6	169.6E6	917.306	925.460
18) L4 AR-1242-3	4.867	4.972	231.0E6	93390359	900.175	913.397
19) L4 AR-1242-4	4.988	5.056	181.9E6	96389066	908.484	894.238
20) L4 AR-1242-5	5.642	5.579	192.2E6	113.2E6	904.779	903.843



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109433.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 18:55
Operator : YP/AJ
Sample : AR1242ICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:27:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:26:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 19:13
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:27:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:26:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.698	3.694	705.0E6	380.9E6	74.630	72.489
2) SA Decachlor...	8.755	8.706	583.7E6	214.6E6	71.212	71.089
Target Compounds						
16) L4 AR-1242-1	4.792	4.777	186.6E6	93559887	707.886	702.778
17) L4 AR-1242-2	4.812	4.796	255.9E6	130.1E6	710.666	710.082
18) L4 AR-1242-3	4.868	4.972	179.6E6	72475556	699.816	708.841
19) L4 AR-1242-4	4.989	5.057	141.2E6	75764454	705.184	702.896
20) L4 AR-1242-5	5.643	5.578	148.7E6	88287004	700.176	704.946



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 19:13
Operator : YP/AJ
Sample : AR1242ICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:27:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:26:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 19:31
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:28:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:26:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.698	3.694	472.3E6	262.7E6	50.000	50.000
2) SA Decachlor...	8.756	8.707	409.9E6	151.0E6	50.000	50.000
Target Compounds						
16) L4 AR-1242-1	4.792	4.777	131.8E6	66564351	500.000	500.000
17) L4 AR-1242-2	4.811	4.797	180.0E6	91633308	500.000	500.000
18) L4 AR-1242-3	4.868	4.972	128.3E6	51122546	500.000	500.000
19) L4 AR-1242-4	4.989	5.057	100.1E6	53894501	500.000	500.000
20) L4 AR-1242-5	5.642	5.578	106.2E6	62619657	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 19:31
Operator : YP/AJ
Sample : AR1242ICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:28:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:26:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 19:50
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:28:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:26:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	239.2E6	132.2E6	25.321	25.168
2) SA Decachlor...	8.755	8.706	217.2E6	81084477	26.492	26.856
Target Compounds						
16) L4 AR-1242-1	4.791	4.777	69551526	35357200	263.870	265.587
17) L4 AR-1242-2	4.811	4.796	94458948	48004344	262.369	261.937
18) L4 AR-1242-3	4.867	4.972	67985441	26922985	264.977	263.318
19) L4 AR-1242-4	4.988	5.056	52548713	28834607	262.488	267.510
20) L4 AR-1242-5	5.642	5.578	58079362	33950495	273.412	271.085



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 19:50
Operator : YP/AJ
Sample : AR1242ICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:28:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:26:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109437.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 20:08
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2025
 Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:28:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:26:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	45284325	24258325	4.794	4.617
2) SA Decachlor...	8.755	8.706	43522830	16219813	5.310	5.372
Target Compounds						
16) L4 AR-1242-1	4.792	4.777	13835003	7073196	52.488	53.131
17) L4 AR-1242-2	4.811	4.796	18548986	9458809	51.522	51.612
18) L4 AR-1242-3	4.867	4.971	12898843	4970561	50.274	48.614
19) L4 AR-1242-4	4.988	5.055	10088199	5702832	50.392	52.907
20) L4 AR-1242-5	5.641	5.577	11831514	6828665	55.698m	54.525m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
Data File : P0109437.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 20:08
Operator : YP/AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2025
Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:28:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:26:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 20:26
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:45:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:44:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	915.4E6	495.5E6	93.761	94.908
2) SA Decachlor...	8.755	8.706	770.4E6	279.0E6	92.405	91.836
Target Compounds						
21) L5 AR-1248-1	4.791	4.777	183.4E6	91256927	912.814	905.620
22) L5 AR-1248-2	5.030	5.014	249.5E6	130.6E6	885.902	891.678
23) L5 AR-1248-3	5.246	5.057	313.6E6	139.3E6	905.924	894.551
24) L5 AR-1248-4	5.600	5.228	440.0E6	163.9E6	918.126	908.733
25) L5 AR-1248-5	5.642	5.620	310.5E6	154.4E6	919.575	910.254



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 20:26
Operator : YP/AJ
Sample : AR1248ICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:45:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:44:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 20:45
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:48:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:44:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	699.0E6	378.0E6	71.591	72.405
2) SA Decachlor...	8.755	8.706	593.5E6	215.5E6	71.185	70.928
Target Compounds						
21) L5 AR-1248-1	4.791	4.777	141.9E6	70604671	706.516	700.670
22) L5 AR-1248-2	5.030	5.014	196.7E6	102.5E6	698.273	699.925
23) L5 AR-1248-3	5.245	5.056	243.5E6	108.7E6	703.429	697.958
24) L5 AR-1248-4	5.600	5.227	339.5E6	127.1E6	708.585	704.454
25) L5 AR-1248-5	5.642	5.619	238.9E6	118.8E6	707.520	700.785



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 20:45
Operator : YP/AJ
Sample : AR1248ICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:48:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:44:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 21:03
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:48:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:44:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	488.2E6	261.1E6	50.000	50.000
2) SA Decachlor...	8.755	8.706	416.9E6	151.9E6	50.000	50.000
Target Compounds						
21) L5 AR-1248-1	4.792	4.777	100.5E6	50383698	500.000	500.000
22) L5 AR-1248-2	5.030	5.014	140.8E6	73210547	500.000	500.000
23) L5 AR-1248-3	5.245	5.056	173.1E6	77850845	500.000	500.000
24) L5 AR-1248-4	5.601	5.227	239.6E6	90182217	500.000	500.000
25) L5 AR-1248-5	5.642	5.619	168.8E6	84787780	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 21:03
Operator : YP/AJ
Sample : AR1248ICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:48:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:44:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 21:21
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:48:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:44:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	247.1E6	131.6E6	25.309	25.209
2) SA Decachlor...	8.755	8.705	220.4E6	81028918	26.436	26.667
Target Compounds						
21) L5 AR-1248-1	4.791	4.777	53414649	26903650	265.875	266.988
22) L5 AR-1248-2	5.030	5.014	74897714	39285877	265.920	268.307
23) L5 AR-1248-3	5.245	5.056	92525840	41607588	267.248	267.226
24) L5 AR-1248-4	5.600	5.227	127.4E6	48427931	265.835	268.500
25) L5 AR-1248-5	5.642	5.620	91434201	45832980	270.811	270.281



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 21:21
Operator : YP/AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:48:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:44:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 21:40
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2025
 Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:49:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:44:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	46251223	23752948	4.737	4.549
2) SA Decachlor...	8.754	8.706	44397899	16474487	5.325	5.422
Target Compounds						
21) L5 AR-1248-1	4.791	4.776	10517320	5442853	52.351	54.014
22) L5 AR-1248-2	5.030	5.013	14922906	7831415	52.983	53.486
23) L5 AR-1248-3	5.245	5.055	19608812	8436393	56.637	54.183
24) L5 AR-1248-4	5.599	5.227	25203917	9829738	52.598m	54.499m
25) L5 AR-1248-5	5.641	5.618	19009831	9765442	56.304m	57.588m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 21:40
Operator : YP/AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2025
Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:49:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:44:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 21:58
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:05:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 03:04:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	951.1E6	511.8E6	96.621	98.139
2) SA Decachlor...	8.754	8.705	796.7E6	284.2E6	93.419	92.489
Target Compounds						
26) L6 AR-1254-1	5.600	5.578	480.6E6	243.6E6	934.551	933.795
27) L6 AR-1254-2	5.749	5.726	417.5E6	212.5E6	924.809	921.386
28) L6 AR-1254-3	6.155	6.129	684.8E6	339.8E6	943.785	941.402
29) L6 AR-1254-4	6.384	6.357	418.0E6	192.3E6	974.859	962.866
30) L6 AR-1254-5	6.805	6.774	597.3E6	278.5E6	945.656	939.652



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109443.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 21:58
Operator : YP/AJ
Sample : AR1254ICC1000
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:05:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 03:04:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 22:17
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:05:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 03:04:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	720.2E6	386.1E6	73.159	74.040
2) SA Decachlor...	8.756	8.705	609.4E6	219.1E6	71.460	71.318
Target Compounds						
26) L6 AR-1254-1	5.601	5.579	368.4E6	186.7E6	716.388	715.385
27) L6 AR-1254-2	5.750	5.726	321.9E6	164.0E6	713.024	710.983
28) L6 AR-1254-3	6.156	6.129	523.0E6	259.8E6	720.743	719.697
29) L6 AR-1254-4	6.385	6.357	307.4E6	142.4E6	716.868	712.856
30) L6 AR-1254-5	6.806	6.775	456.7E6	212.9E6	723.070	718.501



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 22:17
Operator : YP/AJ
Sample : AR1254ICC750
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:05:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 03:04:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109445.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 22:35
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:06:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 03:04:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	492.2E6	260.7E6	50.000	50.000
2) SA Decachlor...	8.755	8.705	426.4E6	153.6E6	50.000	50.000
Target Compounds						
26) L6 AR-1254-1	5.601	5.578	257.1E6	130.5E6	500.000	500.000
27) L6 AR-1254-2	5.749	5.726	225.7E6	115.3E6	500.000	500.000
28) L6 AR-1254-3	6.155	6.129	362.8E6	180.5E6	500.000	500.000
29) L6 AR-1254-4	6.385	6.356	214.4E6	99873317	500.000	500.000
30) L6 AR-1254-5	6.805	6.774	315.8E6	148.2E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109445.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 22:35
Operator : YP/AJ
Sample : AR1254ICC500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:06:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 03:04:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 22:53
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:06:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 03:04:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	249.9E6	133.4E6	25.383	25.591
2) SA Decachlor...	8.755	8.705	224.7E6	82751432	26.343	26.933
Target Compounds						
26) L6 AR-1254-1	5.600	5.578	137.1E6	70215336	266.626	269.112
27) L6 AR-1254-2	5.749	5.726	120.3E6	62303614	266.469	270.086
28) L6 AR-1254-3	6.155	6.129	190.2E6	94726512	262.120	262.436
29) L6 AR-1254-4	6.385	6.357	115.3E6	53701999	269.019	268.851
30) L6 AR-1254-5	6.805	6.775	166.0E6	78525114	262.748	264.951



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 22:53
Operator : YP/AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:06:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 03:04:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 23:12
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/21/2025
 Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:06:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 03:04:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.693	42478021	22408254	4.315m	4.297
2) SA Decachlor...	8.755	8.706	43911860	16400189	5.149	5.338
Target Compounds						
26) L6 AR-1254-1	5.601	5.578	27168777	13670107	52.828m	52.393m
27) L6 AR-1254-2	5.749	5.726	23620321	13084376	52.317m	56.721m
28) L6 AR-1254-3	6.156	6.128	35558931	17874982	49.004m	49.522m
29) L6 AR-1254-4	6.384	6.355	18803102	8443949	43.856m	42.273m
30) L6 AR-1254-5	6.806	6.774	30890950	15538233	48.907	52.427

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 23:12
Operator : YP/AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/21/2025
Supervised By :Ankita Jodhani 02/21/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:06:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 03:04:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 23:30
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:11:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:05:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	478.0E6	256.6E6	50.000	50.000
2) SA Decachlor...	8.754	8.705	414.0E6	151.0E6	50.000	50.000
Target Compounds						
36) L8 AR-1262-1	6.845	6.814	332.9E6	158.6E6	500.000	500.000
37) L8 AR-1262-2	7.346	7.313	564.9E6	249.3E6	500.000	500.000
38) L8 AR-1262-3	7.632	7.597	224.1E6	98127525	500.000	500.000
39) L8 AR-1262-4	7.696	7.661	414.6E6	177.4E6	500.000	500.000
40) L8 AR-1262-5	8.193	8.154	186.7E6	71568799	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 23:30
Operator : YP/AJ
Sample : AR1262ICC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:11:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:05:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Feb 2025 23:48
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:17:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:14:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	965.3E6	526.7E6	96.981	98.845
2) SA Decachlor...	8.755	8.706	1414.8E6	495.1E6	97.758	96.622
Target Compounds						
41) L9 AR-1268-1	7.633	7.597	1298.9E6	554.1E6	985.386	982.199
42) L9 AR-1268-2	7.697	7.662	1196.3E6	512.6E6	990.433	984.000
43) L9 AR-1268-3	7.906	7.869	1000.4E6	413.6E6	987.744	983.635
44) L9 AR-1268-4	8.193	8.153	407.5E6	153.7E6	969.568	942.671
45) L9 AR-1268-5	8.493	8.447	3060.4E6	1087.2E6	1007.828	1001.290



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
Data File : P0109449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 23:48
Operator : YP/AJ
Sample : AR1268ICC1000
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:17:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:14:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 00:07
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:17:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:14:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	735.0E6	395.3E6	73.842	74.195
2) SA Decachlor...	8.755	8.705	1059.4E6	373.0E6	73.204	72.789
Target Compounds						
41) L9 AR-1268-1	7.632	7.597	970.5E6	415.4E6	736.275	736.222
42) L9 AR-1268-2	7.697	7.661	892.1E6	383.3E6	738.582	735.790
43) L9 AR-1268-3	7.905	7.870	749.2E6	309.4E6	739.726	735.808
44) L9 AR-1268-4	8.193	8.153	306.7E6	116.3E6	729.785	712.986
45) L9 AR-1268-5	8.492	8.447	2260.0E6	808.5E6	744.267	744.582



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 00:07
Operator : YP/AJ
Sample : AR1268ICC750
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:17:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:14:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 00:25
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:17:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:14:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	497.7E6	266.4E6	50.000	50.000
2) SA Decachlor...	8.754	8.705	723.6E6	256.2E6	50.000	50.000
Target Compounds						
41) L9 AR-1268-1	7.632	7.597	659.1E6	282.1E6	500.000	500.000
42) L9 AR-1268-2	7.696	7.662	603.9E6	260.5E6	500.000	500.000
43) L9 AR-1268-3	7.905	7.870	506.4E6	210.3E6	500.000	500.000
44) L9 AR-1268-4	8.193	8.154	210.1E6	81539410	500.000	500.000
45) L9 AR-1268-5	8.492	8.448	1518.3E6	542.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
Data File : P0109451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 00:25
Operator : YP/AJ
Sample : AR1268ICC500
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:17:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:14:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 00:43
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:17:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:14:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	259.0E6	137.7E6	26.023	25.841
2) SA Decachlor...	8.755	8.705	379.5E6	135.8E6	26.223	26.497
Target Compounds						
41) L9 AR-1268-1	7.632	7.597	341.4E6	147.8E6	259.019	261.921
42) L9 AR-1268-2	7.697	7.661	311.6E6	135.9E6	258.003	260.784
43) L9 AR-1268-3	7.905	7.869	262.4E6	110.6E6	259.092	263.118
44) L9 AR-1268-4	8.193	8.153	110.5E6	42415364	262.992	260.091
45) L9 AR-1268-5	8.492	8.447	768.8E6	280.3E6	253.190	258.141



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 00:43
Operator : YP/AJ
Sample : AR1268ICC250
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:17:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:14:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 01:02
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:18:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:14:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.692	48540301	25644875	4.877	4.813
2) SA Decachlor...	8.754	8.704	77206427	27914892	5.335	5.448
Target Compounds						
41) L9 AR-1268-1	7.632	7.596	67221395	29693417	50.998	52.632
42) L9 AR-1268-2	7.696	7.660	60264035	26832787	49.892	51.507
43) L9 AR-1268-3	7.905	7.869	51454508	22544472	50.804	53.610
44) L9 AR-1268-4	8.191	8.153	22268868	8258744	52.983	50.643
45) L9 AR-1268-5	8.492	8.447	145.6E6	54675030	47.957	50.353



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
Data File : P0109453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 01:02
Operator : YP/AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:18:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:14:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 01:20
 Operator : YP/AJ
 Sample : P0022025ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO022025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:02:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:00:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.693	485.4E6	269.8E6	51.590	51.681
2) SA Decachlor...	8.754	8.704	443.6E6	158.9E6	51.926	50.342
Target Compounds						
3) L1 AR-1016-1	4.791	4.776	157.1E6	78402892	520.861	515.700
4) L1 AR-1016-2	4.810	4.796	215.0E6	109.8E6	518.628	514.474
5) L1 AR-1016-3	4.866	4.971	152.4E6	60872209	526.733	519.332
6) L1 AR-1016-4	4.987	5.013	119.0E6	52752395	526.672	521.449
7) L1 AR-1016-5	5.245	5.226	131.1E6	68386607	519.681	515.565
31) L7 AR-1260-1	6.286	6.260	235.3E6	118.3E6	513.812	508.238
32) L7 AR-1260-2	6.475	6.447	286.8E6	137.4E6	521.487	511.120
33) L7 AR-1260-3	6.844	6.600	241.2E6	127.7E6	520.450	510.981
34) L7 AR-1260-4	7.105	7.072	220.8E6	103.3E6	518.189	510.781
35) L7 AR-1260-5	7.346	7.312	513.3E6	224.9E6	512.587	506.808



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 01:20
Operator : YP/AJ
Sample : PO022025ICV500
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO022025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:02:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:00:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 01:38
 Operator : YP/AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO022025AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:28:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:26:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.693	473.0E6	263.5E6	50.071	50.141
2) SA Decachlor...	8.756	8.704	420.7E6	151.7E6	51.323	50.236
Target Compounds						
16) L4 AR-1242-1	4.791	4.777	132.7E6	66474054	503.582	499.322
17) L4 AR-1242-2	4.810	4.795	181.5E6	92310140	503.998	503.693
18) L4 AR-1242-3	4.867	4.971	128.4E6	51844543	500.289	507.061
19) L4 AR-1242-4	4.987	5.055	100.9E6	54380483	503.770	504.509
20) L4 AR-1242-5	5.642	5.577	106.0E6	63476044	499.124	506.838



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 01:38
Operator : YP/AJ
Sample : AR1242ICV500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO022025AR1242

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:28:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:26:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 01:57
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO022025AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 02:49:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 02:44:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.693	490.5E6	262.1E6	50.234	50.194
2) SA Decachlor...	8.754	8.704	425.3E6	152.0E6	51.016	50.037
Target Compounds						
21) L5 AR-1248-1	4.790	4.776	100.9E6	50731291	502.457	503.449
22) L5 AR-1248-2	5.030	5.013	140.5E6	73502388	498.738	501.993
23) L5 AR-1248-3	5.244	5.056	174.2E6	78184021	503.235	502.140
24) L5 AR-1248-4	5.599	5.227	240.3E6	91183159	501.425	505.550
25) L5 AR-1248-5	5.641	5.619	167.5E6	84456599	496.149	498.047



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 01:57
Operator : YP/AJ
Sample : AR1248ICV500
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO022025AR1248

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 02:49:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 02:44:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 02:15
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO022025AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 03:06:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 03:04:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.693	499.8E6	265.5E6	50.778	50.913
2) SA Decachlor...	8.755	8.705	431.6E6	154.0E6	50.609	50.133
Target Compounds						
26) L6 AR-1254-1	5.600	5.579	259.2E6	131.6E6	503.961	504.534
27) L6 AR-1254-2	5.749	5.727	227.8E6	116.8E6	504.590	506.344
28) L6 AR-1254-3	6.155	6.129	367.1E6	181.9E6	505.885	503.874
29) L6 AR-1254-4	6.385	6.356	217.7E6	101.2E6	507.824	506.393
30) L6 AR-1254-5	6.805	6.775	319.4E6	149.4E6	505.658	504.131



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 02:15
Operator : YP/AJ
Sample : AR1254ICV500
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO022025AR1254

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 03:06:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 03:04:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0022025\
 Data File : P0109458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Feb 2025 02:34
 Operator : YP/AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO022025AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 21 04:18:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:14:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.696	3.693	505.7E6	272.2E6	50.812	51.081
2) SA Decachlor...	8.754	8.704	737.4E6	260.5E6	50.951	50.843
Target Compounds						
41) L9 AR-1268-1	7.631	7.596	670.6E6	287.4E6	508.735	509.428
42) L9 AR-1268-2	7.696	7.660	616.2E6	265.8E6	510.180	510.135
43) L9 AR-1268-3	7.905	7.868	517.0E6	214.7E6	510.419	510.625
44) L9 AR-1268-4	8.193	8.152	213.4E6	83152742	507.822	509.893
45) L9 AR-1268-5	8.491	8.446	1546.7E6	554.6E6	509.351	510.729



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Feb 2025 02:34
Operator : YP/AJ
Sample : AR1268ICV500
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO022025AR1268

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:18:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:14:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



RETENTION TIMES OF INITIAL CALIBRATION

Contract: GENV01
Lab Code: CHEM **Case No.:** Q1574 **SAS No.:** Q1574 **SDG NO.:** Q1574
Instrument ID: ECD_P **Calibration Date(s):** 03/11/2025 03/11/2025
Calibration Times: 15:13 23:38

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 = <u>PP070419.D</u>	RT 750 = <u>PP070420.D</u>
RT 500 = <u>PP070421.D</u>	RT 250 = <u>PP070422.D</u>	RT 050 = <u>PP070423.D</u>

COMPOUND		RT 1000	RT 750	RT 500	RT 250	RT 050	MEAN RT	RT WINDOW	
								FROM	TO
Aroclor-1016-1	(1)	5.68	5.68	5.68	5.68	5.68	5.68	5.58	5.78
Aroclor-1016-2	(2)	5.70	5.70	5.70	5.70	5.70	5.70	5.60	5.80
Aroclor-1016-3	(3)	5.76	5.76	5.76	5.76	5.76	5.76	5.66	5.86
Aroclor-1016-4	(4)	5.86	5.86	5.86	5.86	5.86	5.86	5.76	5.96
Aroclor-1016-5	(5)	6.15	6.15	6.15	6.15	6.15	6.15	6.05	6.25
Aroclor-1260-1	(1)	7.27	7.27	7.27	7.27	7.27	7.27	7.17	7.37
Aroclor-1260-2	(2)	7.53	7.52	7.53	7.53	7.53	7.53	7.43	7.63
Aroclor-1260-3	(3)	7.89	7.88	7.88	7.89	7.89	7.88	7.78	7.98
Aroclor-1260-4	(4)	8.11	8.11	8.11	8.11	8.11	8.11	8.01	8.21
Aroclor-1260-5	(5)	8.43	8.43	8.43	8.43	8.43	8.43	8.33	8.53
Decachlorobiphenyl		10.25	10.25	10.25	10.26	10.25	10.25	10.15	10.35
Tetrachloro-m-xylene		4.53	4.52	4.52	4.53	4.53	4.53	4.43	4.63
Aroclor-1232-1	(1)	4.89	4.89	4.89	4.89	4.89	4.89	4.79	4.99
Aroclor-1232-2	(2)	5.41	5.41	5.41	5.41	5.41	5.41	5.31	5.51
Aroclor-1232-3	(3)	5.70	5.70	5.70	5.70	5.70	5.70	5.60	5.80
Aroclor-1232-4	(4)	5.86	5.86	5.86	5.86	5.86	5.86	5.76	5.96
Aroclor-1232-5	(5)	5.95	5.95	5.95	5.95	5.94	5.95	5.85	6.05
Decachlorobiphenyl		10.25	10.25	10.25	10.25	10.26	10.25	10.15	10.35
Tetrachloro-m-xylene		4.53	4.53	4.53	4.53	4.53	4.53	4.43	4.63
Aroclor-1242-1	(1)	5.68	5.68	5.68	5.68	5.68	5.68	5.58	5.78
Aroclor-1242-2	(2)	5.70	5.70	5.70	5.70	5.70	5.70	5.60	5.80
Aroclor-1242-3	(3)	5.76	5.76	5.76	5.76	5.76	5.76	5.66	5.86
Aroclor-1242-4	(4)	5.86	5.86	5.86	5.86	5.86	5.86	5.76	5.96
Aroclor-1242-5	(5)	6.59	6.59	6.59	6.59	6.59	6.59	6.49	6.69
Decachlorobiphenyl		10.25	10.25	10.25	10.25	10.25	10.25	10.15	10.35
Tetrachloro-m-xylene		4.53	4.53	4.53	4.52	4.53	4.53	4.43	4.63
Aroclor-1248-1	(1)	5.68	5.68	5.68	5.68	5.68	5.68	5.58	5.78
Aroclor-1248-2	(2)	5.95	5.95	5.95	5.95	5.95	5.95	5.85	6.05
Aroclor-1248-3	(3)	6.15	6.15	6.15	6.15	6.15	6.15	6.05	6.25
Aroclor-1248-4	(4)	6.55	6.55	6.55	6.55	6.55	6.55	6.45	6.65
Aroclor-1248-5	(5)	6.59	6.59	6.59	6.59	6.59	6.59	6.49	6.69
Decachlorobiphenyl		10.25	10.25	10.25	10.25	10.25	10.25	10.15	10.35
Tetrachloro-m-xylene		4.53	4.52	4.52	4.52	4.52	4.52	4.42	4.62
Aroclor-1254-1	(1)	6.53	6.53	6.53	6.52	6.53	6.53	6.43	6.63
Aroclor-1254-2	(2)	6.74	6.74	6.75	6.74	6.74	6.74	6.64	6.84
Aroclor-1254-3	(3)	7.11	7.11	7.11	7.10	7.11	7.11	7.01	7.21
Aroclor-1254-4	(4)	7.39	7.39	7.39	7.39	7.39	7.39	7.29	7.49
Aroclor-1254-5	(5)	7.81	7.81	7.81	7.80	7.81	7.81	7.71	7.91

RETENTION TIMES OF INITIAL CALIBRATION

Decachlorobiphenyl	10.25	10.25	10.25	10.25	10.25	10.25	10.15	10.35
Tetrachloro-m-xylene	4.53	4.52	4.53	4.52	4.53	4.53	4.43	4.63
Aroclor-1268-1 (1)	8.75	8.74	8.74	8.74	8.75	8.74	8.64	8.84
Aroclor-1268-2 (2)	8.84	8.84	8.83	8.83	8.84	8.84	8.74	8.94
Aroclor-1268-3 (3)	9.07	9.07	9.07	9.07	9.07	9.07	8.97	9.17
Aroclor-1268-4 (4)	9.49	9.49	9.49	9.49	9.49	9.49	9.39	9.59
Aroclor-1268-5 (5)	9.91	9.91	9.90	9.91	9.91	9.91	9.81	10.01
Decachlorobiphenyl	10.25	10.25	10.25	10.25	10.25	10.25	10.15	10.35
Tetrachloro-m-xylene	4.53	4.53	4.52	4.52	4.53	4.53	4.43	4.63

RETENTION TIMES OF INITIAL CALIBRATION

Contract: GENV01

Lab Code: CHEM

Case No.: Q1574

SAS No.: Q1574

SDG NO.: Q1574

Instrument ID: ECD_P

Calibration Date(s):

03/11/2025

03/11/2025

Calibration Times:

15:13

23:38

GC Column: ZB-MR2

ID: 0.32 (mm)

LAB FILE ID:

RT 1000 = PP070419.D

RT 750 = PP070420.D

RT 500 = PP070421.D

RT 250 = PP070422.D

RT 050 = PP070423.D

[illegible]

[illegible]



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Instrument ID: ECD_P Calibration Date(s): 03/11/2025 03/11/2025

Calibration Times: 15:13 23:38

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PP070419.D</u>		CF 750 = <u>PP070420.D</u>			
CF 500 = <u>PP070421.D</u>		CF 250 = <u>PP070422.D</u>		CF 050 = <u>PP070423.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	46284919	48624555	51195480	56320148	56830900	51851200
Aroclor-1016-2	(2)	68727144	72260815	75092688	79473188	62170340	71544835
Aroclor-1016-3	(3)	41881157	43836071	46346194	49629608	45996640	45537934
Aroclor-1016-4	(4)	34693414	37117197	39579046	42287028	41512180	39037773
Aroclor-1016-5	(5)	32535779	33720589	35503344	36571056	34779300	34622014
Aroclor-1260-1	(1)	55067637	58265401	60660348	63250936	56446720	58738208
Aroclor-1260-2	(2)	75483004	79277409	82983970	87347188	85123440	82043002
Aroclor-1260-3	(3)	62678610	64989695	68010270	70682128	62427680	65757677
Aroclor-1260-4	(4)	60990738	64683661	66152948	69503548	65382940	65342767
Aroclor-1260-5	(5)	130557968	135103443	140419232	146528904	130778620	136677633
Decachlorobiphenyl		1005446690	1044219213	1084386360	1134008440	1043654800	1062343101
Tetrachloro-m-xylene		1462968010	1529300040	1575427920	1661278640	1547936200	1555382162
Aroclor-1232-1	(1)	31812517	33409335	34815870	38072588	39676960	35557454
Aroclor-1232-2	(2)	16331114	17367928	17709532	17293972	15638140	16868137
Aroclor-1232-3	(3)	33685372	35206453	37651060	39178940	37126640	36569693
Aroclor-1232-4	(4)	17112653	18207945	18881288	20579940	20189680	18994301
Aroclor-1232-5	(5)	12358074	13019340	13596998	11696560	14140280	12962250
Decachlorobiphenyl		1007346640	1061633867	1110112680	1150608440	1055455400	1077031405
Tetrachloro-m-xylene		1503870440	1587673493	1628432540	1684437880	1564380200	1593758911
Aroclor-1242-1	(1)	39253435	41704367	43482132	47856472	49946320	44448545
Aroclor-1242-2	(2)	58252556	60113944	62228844	66050560	60258320	61380845
Aroclor-1242-3	(3)	35362447	36380501	38652894	41645404	33464760	37101201
Aroclor-1242-4	(4)	29479509	30833784	32552722	35082164	32717220	32133080
Aroclor-1242-5	(5)	29991669	31404576	32011208	32699504	29130640	31047519
Decachlorobiphenyl		1017143570	1063398627	1098678020	1146617040	1019213600	1069010171
Tetrachloro-m-xylene		1483500490	1538532373	1587702840	1655080400	1578490200	1568661261
Aroclor-1248-1	(1)	30241509	31836707	34371560	37879708	36450300	34155957
Aroclor-1248-2	(2)	39839483	41732589	44072986	47187728	39403540	42447265
Aroclor-1248-3	(3)	43671743	45535401	47272778	48829472	45433820	46148643
Aroclor-1248-4	(4)	52673121	54800967	57547552	61348180	63586480	57991260
Aroclor-1248-5	(5)	49495855	52225937	54279376	57435820	54999800	53687358
Decachlorobiphenyl		1018745530	1065079280	1110066380	1164168240	1044426200	1080497126
Tetrachloro-m-xylene		1464367110	1509550200	1593080400	1654989520	1637278400	1571853126
Aroclor-1254-1	(1)	52191144	54776691	58408862	62528540	58393680	57259783

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1254-2	(2)	76163232	79292283	83746208	89006644	77052340	81052141	7
Aroclor-1254-3	(3)	78867294	81324341	86343146	90140028	84184220	84171806	5
Aroclor-1254-4	(4)	65665428	68036704	71633390	75767876	69582520	70137184	5
Aroclor-1254-5	(5)	65604720	67856063	71049052	74607116	70169360	69857262	5
Decachlorobiphenyl		1051774640	1084735960	1131757040	1190025520	1071423800	1105943392	5
Tetrachloro-m-xylene		1491401080	1547951320	1596952960	1679816880	1638007800	1590826008	5
Aroclor-1268-1	(1)	188529701	191493623	201496426	211079324	198399040	198199623	4
Aroclor-1268-2	(2)	162712211	165423828	173208520	180425992	166812140	169716538	4
Aroclor-1268-3	(3)	139964894	142620983	149835492	155687892	143563980	146334648	4
Aroclor-1268-4	(4)	62601215	63262983	66177076	67604984	59759620	63881176	5
Aroclor-1268-5	(5)	401160937	407647449	423231624	443337256	421401480	419355749	4
Decachlorobiphenyl		1797305300	1841882720	1928545440	2018232880	1865263000	1890245868	5
Tetrachloro-m-xylene		1559644910	1556664040	1644040220	1708675120	1710882200	1635981298	5

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: GENV01
Lab Code: CHEM **Case No.:** Q1574 **SAS No.:** Q1574 **SDG NO.:** Q1574
Instrument ID: ECD_P **Calibration Date(s):** 03/11/2025 03/11/2025
Calibration Times: 15:13 23:38

GC Column: ZB-MR2 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PP070419.D</u>		CF 750 = <u>PP070420.D</u>			
CF 500 = <u>PP070421.D</u>		CF 250 = <u>PP070422.D</u>		CF 050 = <u>PP070423.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	31619052	35012463	36116294	39457560	37557300	35952534
Aroclor-1016-2	(2)	44662617	48866077	51001758	55603496	59699380	51966666
Aroclor-1016-3	(3)	24906943	27191785	28703256	30683884	30781120	28453398
Aroclor-1016-4	(4)	19770953	21670935	22902960	24389748	23214920	22389903
Aroclor-1016-5	(5)	25646269	27397575	29268330	32409960	33872260	29718879
Aroclor-1260-1	(1)	45267436	47641613	50061678	53643092	52308080	49784380
Aroclor-1260-2	(2)	60652513	64073769	66616364	70066968	69027800	66087483
Aroclor-1260-3	(3)	52248928	55432315	57823148	61011000	59471320	57197342
Aroclor-1260-4	(4)	47067710	49841909	53961982	55559372	49386640	51163523
Aroclor-1260-5	(5)	123950775	130046140	135804906	136761852	117362580	128785251
Decachlorobiphenyl		935400030	944501173	996009380	1027099200	988797000	978361357
Tetrachloro-m-xylene		901898260	976425347	1019517980	1052535320	1061027800	1002280941
Aroclor-1232-1	(1)	23977464	25043855	25876362	28218616	28432280	26309715
Aroclor-1232-2	(2)	23409194	24148587	25178540	27689696	28634420	25812087
Aroclor-1232-3	(3)	12864968	13117912	13753150	14320588	15988100	14008944
Aroclor-1232-4	(4)	10909254	11094221	11677434	12331552	12548800	11712252
Aroclor-1232-5	(5)	12122932	12663212	13051746	13538632	13963480	13068000
Decachlorobiphenyl		923591970	934486067	965069440	1131453800	1083832600	1007686775
Tetrachloro-m-xylene		981294310	1023698747	1027014040	1102661240	1188146200	1064562907
Aroclor-1242-1	(1)	28374294	28991207	30174104	32528448	32989020	30611415
Aroclor-1242-2	(2)	40120133	40663773	41940388	45612680	49650880	43597571
Aroclor-1242-3	(3)	22172127	22503904	23797688	25561184	25126720	23832325
Aroclor-1242-4	(4)	20777408	21261321	22368954	23941300	21863540	22042505
Aroclor-1242-5	(5)	26011255	26949576	28142034	29660872	28841860	27921119
Decachlorobiphenyl		890780220	996610280	1018649180	1070124720	1151487200	1025530320
Tetrachloro-m-xylene		949681240	969479187	1000171980	1041407720	1043402000	1000828425
Aroclor-1248-1	(1)	21916865	22139940	24138102	25281632	23901120	23475532
Aroclor-1248-2	(2)	28154371	29147072	31604814	33306732	34304240	31303446
Aroclor-1248-3	(3)	29522180	30421332	32954472	34362676	31347200	31721572
Aroclor-1248-4	(4)	34974296	35760019	38441344	40862964	44827240	38973173
Aroclor-1248-5	(5)	34216861	35543065	38522800	40509348	41641320	38086679
Decachlorobiphenyl		933290630	982033680	1000188180	1068098600	1015594400	999841098
Tetrachloro-m-xylene		948607640	978544213	1031768560	1070844800	1068084800	1019570003
Aroclor-1254-1	(1)	49741488	53083060	56518628	60344088	61926700	56322793

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1254-2	(2)	43195538	45981229	48525194	52438220	54392240	48906484	9
Aroclor-1254-3	(3)	69004581	72181184	75732026	81417896	78754240	75417985	7
Aroclor-1254-4	(4)	48529875	50966111	53417608	57048936	53797000	52751906	6
Aroclor-1254-5	(5)	63254548	65263447	68912458	73214624	74627960	69054607	7
Decachlorobiphenyl		966187920	982212947	1086993960	1153126680	1151501200	1068004541	8
Tetrachloro-m-xylene		967205180	984098413	1019987640	1086171680	989309800	1009354543	5
Aroclor-1268-1	(1)	168373725	166057156	179047242	187011272	174871700	175072219	5
Aroclor-1268-2	(2)	142006892	140092196	149842434	153490708	144862740	146058994	4
Aroclor-1268-3	(3)	125351560	120465205	129564250	133099628	133160800	128328289	4
Aroclor-1268-4	(4)	54287293	53233979	56809814	58479952	52090820	54980372	5
Aroclor-1268-5	(5)	364151928	362236821	378313444	380892964	354578080	368034647	3
Decachlorobiphenyl		1632116030	1658280453	1742317540	1836812000	1806314000	1735168005	5
Tetrachloro-m-xylene		1019432100	1034489600	1102868440	1184868600	1114308600	1091193468	6



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Instrument ID: ECD_P Date(s) Analyzed: 03/11/2025 03/11/2025

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	4.73	4.63	4.83	19940100
		2	4.81	4.71	4.91	14608700
		3	4.89	4.79	4.99	44364600
		4	0.00			0
		5	0.00			0
Aroclor-1262	500	1	8.11	8.01	8.21	81718600
		2	8.43	8.33	8.53	164714000
		3	8.75	8.65	8.85	112164000
		4	8.83	8.73	8.93	83803800
		5	9.49	9.39	9.59	58896200



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Instrument ID: ECD_P Date(s) Analyzed: 03/11/2025 03/11/2025

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	4.04	3.94	4.14	14882500
		2	4.13	4.03	4.23	11429100
		3	4.20	4.10	4.30	33421800
		4	0.00			0
		5	0.00			0
Aroclor-1262	500	1	6.96	6.86	7.06	83664000
		2	7.22	7.12	7.32	68729800
		3	7.74	7.64	7.84	65986200
		4	7.81	7.71	7.91	104435000
		5	8.31	8.21	8.41	51550000

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 15:13
 Operator : YP\AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 15:59:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 15:56:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.526	3.829	146.3E6	90189826	96.299	93.878
2) SA Decachlor...	10.254	8.881	100.5E6	93540003	96.223	96.862
Target Compounds						
3) L1 AR-1016-1	5.679	4.917	46284919	31619052	949.625	933.606
4) L1 AR-1016-2	5.700	4.935	68727144	44662617	955.739	933.736
5) L1 AR-1016-3	5.763	5.112	41881157	24906943	949.392	929.187
6) L1 AR-1016-4	5.860	5.154	34693414	19770953	934.220	926.606
7) L1 AR-1016-5	6.153	5.369	32535779	25646269	956.384	934.042
31) L7 AR-1260-1	7.273	6.406	55067637	45267436	951.674	949.709
32) L7 AR-1260-2	7.526	6.594	75483004	60652513	952.665	953.140
33) L7 AR-1260-3	7.886	6.748	62678610	52248928	959.203	949.358
34) L7 AR-1260-4	8.110	7.221	60990738	47067710	959.399	931.760
35) L7 AR-1260-5	8.431	7.462	130.6E6	124.0E6	963.609	954.364



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 15:13
Operator : YP\AJ
Sample : AR1660ICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 15:59:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 15:56:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 15:29
 Operator : YP\AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 16:02:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 15:56:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.524	3.829	114.7E6	73231901	75.332	75.814
2) SA Decachlor...	10.251	8.881	78316441	70837588	74.967	73.894
Target Compounds						
3) L1 AR-1016-1	5.677	4.916	36468416	26259347	748.813	766.713
4) L1 AR-1016-2	5.699	4.935	54195611	36649558	752.436	760.730
5) L1 AR-1016-3	5.761	5.112	32877053	20393839	746.847	757.178
6) L1 AR-1016-4	5.858	5.154	27837898	16253201	749.744	757.786
7) L1 AR-1016-5	6.151	5.369	25290442	20548181	745.593	748.912
31) L7 AR-1260-1	7.270	6.405	43699051	35731210	753.461	749.759
32) L7 AR-1260-2	7.524	6.594	59458057	48055327	750.277	753.444
33) L7 AR-1260-3	7.882	6.748	48742271	41574236	747.281	753.592
34) L7 AR-1260-4	8.108	7.221	48512746	37381432	758.694	743.310
35) L7 AR-1260-5	8.428	7.461	101.3E6	97534605	748.577	750.648



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 15:29
Operator : YP\AJ
Sample : AR1660ICC750
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 16:02:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 15:56:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 15:46
 Operator : YP\AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 15:56:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 15:56:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.524	3.829	78771396	50975899	50.000	50.000
2) SA Decachlor...	10.252	8.881	54219318	49800469	50.000	50.000
Target Compounds						
3) L1 AR-1016-1	5.677	4.917	25597740	18058147	500.000	500.000
4) L1 AR-1016-2	5.699	4.936	37546344	25500879	500.000	500.000
5) L1 AR-1016-3	5.761	5.113	23173097	14351628	500.000	500.000
6) L1 AR-1016-4	5.858	5.154	19789523	11451480	500.000	500.000
7) L1 AR-1016-5	6.151	5.370	17751672	14634165	500.000	500.000
31) L7 AR-1260-1	7.271	6.407	30330174	25030839	500.000	500.000
32) L7 AR-1260-2	7.525	6.595	41491985	33308182	500.000	500.000
33) L7 AR-1260-3	7.883	6.749	34005135	28911574	500.000	500.000
34) L7 AR-1260-4	8.108	7.221	33076474	26980991	500.000	500.000
35) L7 AR-1260-5	8.428	7.462	70209616	67902453	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 15:46
Operator : YP\AJ
Sample : AR1660ICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 15:56:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 15:56:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 16:02
 Operator : YP\AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660ICC250

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/12/2025
 Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 16:15:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 16:15:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.526	3.828	41531966	26313383	26.670	26.644
2) SA Decachlor...	10.255	8.880	28350211	25677480	26.570	26.327m
Target Compounds						
3) L1 AR-1016-1	5.678	4.916	14080037	9864390	278.227	277.469
4) L1 AR-1016-2	5.700	4.935	19868297	13900874	268.896	277.831
5) L1 AR-1016-3	5.762	5.112	12407402	7670971	273.151	275.227
6) L1 AR-1016-4	5.859	5.154	10571757	6097437	275.169	274.862
7) L1 AR-1016-5	6.153	5.369	9142764	8102490	264.374	282.508
31) L7 AR-1260-1	7.272	6.406	15812734	13410773	266.607	272.835
32) L7 AR-1260-2	7.526	6.594	21836797	17516742	268.685	268.035
33) L7 AR-1260-3	7.885	6.749	17670532	15252750	265.362	269.346
34) L7 AR-1260-4	8.110	7.220	17375887	13889843	265.960	269.143
35) L7 AR-1260-5	8.430	7.461	36632226	34190463	265.158	259.725

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

```
Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\  
Data File : PP070422.D  
Signal(s) : Signal #1: ECD1A.ch  Signal #2: ECD2B.ch  
Acq On    : 11 Mar 2025  16:02  
Operator  : YP\AJ  
Sample    : AR1660ICC250  
Misc      :  
ALS Vial  : 6    Sample Multiplier: 1
```



Instrument :
ECD_P
ClientSampleId :
AR1660ICC250

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 16:15:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 16:15:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 16:18
 Operator : YP\AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/12/2025
 Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 16:29:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 16:29:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.526	3.828	7739681	5305139	4.976	5.293
2) SA Decachlor...	10.252	8.882	5218274	4943985	4.912	5.053
Target Compounds						
3) L1 AR-1016-1	5.676	4.917	2841545	1877865	53.987m	52.232
4) L1 AR-1016-2	5.699	4.936	3108517	2984969	42.895m	57.440 #
5) L1 AR-1016-3	5.762	5.113	2299832	1539056	50.765m	54.090
6) L1 AR-1016-4	5.859	5.154	2075609	1160746	53.599m	51.842
7) L1 AR-1016-5	6.151	5.369	1738965	1693613	50.227	56.988
31) L7 AR-1260-1	7.273	6.407	2822336	2615404	48.049	52.535
32) L7 AR-1260-2	7.527	6.594	4256172	3451390	51.877	52.225
33) L7 AR-1260-3	7.885	6.749	3121384	2973566	47.468	51.988
34) L7 AR-1260-4	8.110	7.221	3269147	2469332	50.031	48.460m
35) L7 AR-1260-5	8.431	7.461	6538931	5868129	47.842	45.416m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 16:18
Operator : YP\AJ
Sample : AR1660ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 16:29:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 16:29:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 16:34
 Operator : YP\AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 21:54:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 21:54:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.527	3.829	85559870	52860952	50.000	50.000
2) SA Decachlor...	10.253	8.882	57800559	48491420	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	4.728	4.040	9970034	7441268	500.000	500.000
9) L2 AR-1221-2	4.814	4.127	7304344	5714551	500.000	500.000
10) L2 AR-1221-3	4.889	4.203	22182343	16710871	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 16:34
Operator : YP\AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 21:54:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 21:54:12 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 16:51
 Operator : YP\AJ
 Sample : AR1232ICC1000
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1232ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 21:59:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 21:58:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.828	150.4E6	98129431	92.351	95.548
2) SA Decachlor...	10.253	8.882	100.7E6	92359197	90.743	95.702
Target Compounds						
11) L3 AR-1232-1	4.887	4.202	31812517	23977464	913.736	926.616
12) L3 AR-1232-2	5.413	4.935	16331114	23409194	922.165	929.728
13) L3 AR-1232-3	5.699	5.112	33685372	12864968	894.673	935.420
14) L3 AR-1232-4	5.859	5.197	17112653	10909254	906.329	934.217
15) L3 AR-1232-5	5.949	5.369	12358074	12122932	908.882	928.836



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 16:51
Operator : YP\AJ
Sample : AR1232ICC1000
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1232ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 21:59:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 21:58:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 17:07
 Operator : YP\AJ
 Sample : AR1232ICC750
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1232ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 21:59:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 21:58:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.829	119.1E6	76777406	73.123	74.758
2) SA Decachlor...	10.252	8.882	79622540	70086455	71.725	72.623
Target Compounds						
11) L3 AR-1232-1	4.887	4.203	25057001	18782891	719.701	725.871
12) L3 AR-1232-2	5.413	4.936	13025946	18111440	735.533	719.320
13) L3 AR-1232-3	5.699	5.113	26404840	9838434	701.304	715.359
14) L3 AR-1232-4	5.859	5.198	13655959	8320666	723.254	712.542
15) L3 AR-1232-5	5.949	5.370	9764505	9497409	718.137	727.673



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 17:07
Operator : YP\AJ
Sample : AR1232ICC750
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1232ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 21:59:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 21:58:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 17:23
 Operator : YP\AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:00:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 21:58:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.828	81421627	51350702	50.000	50.000
2) SA Decachlor...	10.252	8.880	55505634	48253472	50.000	50.000
Target Compounds						
11) L3 AR-1232-1	4.887	4.202	17407935	12938181	500.000	500.000
12) L3 AR-1232-2	5.412	4.935	8854766	12589270	500.000	500.000
13) L3 AR-1232-3	5.698	5.112	18825530	6876575	500.000	500.000
14) L3 AR-1232-4	5.859	5.197	9440644	5838717	500.000	500.000
15) L3 AR-1232-5	5.949	5.369	6798499	6525873	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 17:23
Operator : YP\AJ
Sample : AR1232ICC500
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:00:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 21:58:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 17:40
 Operator : YP\AJ
 Sample : AR1232ICC250
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1232ICC250

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/12/2025
 Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:00:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 21:58:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.526	3.829	42110947	27566531	25.860	26.841
2) SA Decachlor...	10.254	8.881	28765211	28286345	25.912	29.310
Target Compounds						
11) L3 AR-1232-1	4.888	4.202	9518147	7054654	273.385	272.629
12) L3 AR-1232-2	5.414	4.935	4323493	6922424	244.134	274.933
13) L3 AR-1232-3	5.700	5.112	9794735	3580147	260.145	260.315
14) L3 AR-1232-4	5.861	5.196	5144985	3082888	272.491	264.004
15) L3 AR-1232-5	5.949	5.369	2924140	3384658	215.058m	259.326

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 17:40
Operator : YP\AJ
Sample : AR1232ICC250
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1232ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:00:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 21:58:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 17:56
 Operator : YP\AJ
 Sample : AR1232ICC050
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1232ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/12/2025
 Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:00:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 21:58:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.526	3.828	7821901	5940731	4.803	5.784
2) SA Decachlor...	10.255	8.881	5277277	5419163	4.754	5.615
Target Compounds						
11) L3 AR-1232-1	4.889	4.201	1983848	1421614	56.981	54.939m
12) L3 AR-1232-2	5.414	4.934	781907	1431721	44.152m	56.863m#
13) L3 AR-1232-3	5.701	5.112	1856332	799405	49.304m	58.125
14) L3 AR-1232-4	5.859	5.196	1009484	627440	53.465m	53.731
15) L3 AR-1232-5	5.943	5.367	707014	698174	51.998m	53.493m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 17:56
Operator : YP\AJ
Sample : AR1232ICC050
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1232ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:00:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 21:58:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 18:12
 Operator : YP\AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:16:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:15:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.828	148.4E6	94968124	93.437	94.952
2) SA Decachlor...	10.252	8.881	101.7E6	89078022	92.579	87.447
Target Compounds						
16) L4 AR-1242-1	5.677	4.916	39253435	28374294	902.749	940.352
17) L4 AR-1242-2	5.699	4.935	58252556	40120133	936.102	956.599
18) L4 AR-1242-3	5.761	5.112	35362447	22172127	914.872	931.692
19) L4 AR-1242-4	5.859	5.197	29479509	20777408	905.593	928.850
20) L4 AR-1242-5	6.589	5.722	29991669	26011255	936.911	924.285



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 18:12
Operator : YP\AJ
Sample : AR1242ICC1000
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:16:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:15:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 18:28
 Operator : YP\AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:16:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:15:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.828	115.4E6	72710939	72.677	72.698
2) SA Decachlor...	10.252	8.880	79754897	74745771	72.592	73.377
Target Compounds						
16) L4 AR-1242-1	5.678	4.916	31278275	21743405	719.336	720.598
17) L4 AR-1242-2	5.700	4.935	45085458	30497830	724.511	727.171
18) L4 AR-1242-3	5.762	5.112	27285376	16877928	705.908	709.226
19) L4 AR-1242-4	5.859	5.196	23125338	15945991	710.396	712.863
20) L4 AR-1242-5	6.590	5.721	23553432	20212182	735.787	718.220



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 18:28
Operator : YP\AJ
Sample : AR1242ICC750
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:16:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:15:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 18:45
 Operator : YP\AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:16:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:15:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm


Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.829	79385142	50008599	50.000	50.000
2) SA Decachlor...	10.253	8.881	54933901	50932459	50.000	50.000
Target Compounds						
16) L4 AR-1242-1	5.678	4.916	21741066	15087052	500.000	500.000
17) L4 AR-1242-2	5.700	4.935	31114422	20970194	500.000	500.000
18) L4 AR-1242-3	5.762	5.113	19326447	11898844	500.000	500.000
19) L4 AR-1242-4	5.859	5.196	16276361	11184477	500.000	500.000
20) L4 AR-1242-5	6.590	5.722	16005604	14071017	500.000	500.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
ECD_P
ClientSampleId :
AR1242ICC500

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 19:01
 Operator : YP\AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:17:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:15:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.524	3.828	41377010	26035193	26.061	26.031
2) SA Decachlor...	10.252	8.882	28665426	26753118	26.091	26.263
Target Compounds						
16) L4 AR-1242-1	5.677	4.916	11964118	8132112	275.150	269.506
17) L4 AR-1242-2	5.699	4.935	16512640	11403170	265.353	271.890
18) L4 AR-1242-3	5.761	5.112	10411351	6390296	269.355	268.526
19) L4 AR-1242-4	5.858	5.197	8770541	5985325	269.426	267.573
20) L4 AR-1242-5	6.589	5.721	8174876	7415218	255.375	263.493



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070433.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 19:01
Operator : YP\AJ
Sample : AR1242ICC250
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:17:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:15:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 19:17
 Operator : YP\AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1242ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/12/2025
 Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:17:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:15:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.828	7892451	5217010	4.971	5.216
2) SA Decachlor...	10.251	8.880	5096068	5757436	4.638	5.652
Target Compounds						
16) L4 AR-1242-1	5.675	4.915	2497316	1649451	57.433m	54.664m
17) L4 AR-1242-2	5.698	4.933	3012916	2482544	48.417m	59.192m
18) L4 AR-1242-3	5.760	5.112	1673238	1256336	43.289m	52.792
19) L4 AR-1242-4	5.858	5.196	1635861	1093177	50.253m	48.870
20) L4 AR-1242-5	6.589	5.721	1456532	1442093	45.501	51.243

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 19:17
Operator : YP\AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:17:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:15:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 19:34
 Operator : YP\AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:28:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:27:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.828	146.4E6	94860764	91.920	91.940
2) SA Decachlor...	10.253	8.881	101.9E6	93329063	91.773	93.312
Target Compounds						
21) L5 AR-1248-1	5.677	4.916	30241509	21916865	879.841	907.978
22) L5 AR-1248-2	5.949	5.154	39839483	28154371	903.943	890.825
23) L5 AR-1248-3	6.152	5.196	43671743	29522180	923.824	895.847
24) L5 AR-1248-4	6.551	5.369	52673121	34974296	915.297	909.809
25) L5 AR-1248-5	6.590	5.763	49495855	34216861	911.872	888.224



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 19:34
Operator : YP\AJ
Sample : AR1248ICC1000
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:28:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:27:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 19:50
 Operator : YP\AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:28:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:27:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.524	3.829	113.2E6	73390816	71.068	71.131
2) SA Decachlor...	10.251	8.881	79880946	73652526	71.961	73.639
Target Compounds						
21) L5 AR-1248-1	5.676	4.916	23877530	16604955	694.689	687.915
22) L5 AR-1248-2	5.948	5.154	31299442	21860304	710.173	691.676
23) L5 AR-1248-3	6.151	5.196	34151551	22815999	722.436	692.349
24) L5 AR-1248-4	6.550	5.369	41100725	26820014	714.205	697.687
25) L5 AR-1248-5	6.589	5.763	39169453	26657299	721.627	691.988



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 19:50
Operator : YP\AJ
Sample : AR1248ICC750
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:28:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:27:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070437.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 20:06
 Operator : YP\AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:28:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:27:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.524	3.828	79654020	51588428	50.000	50.000
2) SA Decachlor...	10.252	8.879	55503319	50009409	50.000	50.000
Target Compounds						
21) L5 AR-1248-1	5.676	4.915	17185780	12069051	500.000	500.000
22) L5 AR-1248-2	5.948	5.153	22036493	15802407	500.000	500.000
23) L5 AR-1248-3	6.151	5.195	23636389	16477236	500.000	500.000
24) L5 AR-1248-4	6.550	5.368	28773776	19220672	500.000	500.000
25) L5 AR-1248-5	6.589	5.762	27139688	19261400	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070437.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 20:06
Operator : YP\AJ
Sample : AR1248ICC500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:28:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:27:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 20:22
 Operator : YP\AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:29:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:27:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.524	3.828	41374738	26771120	25.972	25.947
2) SA Decachlor...	10.251	8.880	29104206	26702465	26.218	26.697
Target Compounds						
21) L5 AR-1248-1	5.676	4.915	9469927	6320408	275.516	261.844
22) L5 AR-1248-2	5.948	5.154	11796932	8326683	267.668	263.462
23) L5 AR-1248-3	6.151	5.196	12207368	8590669	258.233	260.683
24) L5 AR-1248-4	6.550	5.369	15337045	10215741	266.511	265.749
25) L5 AR-1248-5	6.589	5.762	14358955	10127337	264.538	262.892



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 20:22
Operator : YP\AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:29:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:27:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 20:39
 Operator : YP\AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/12/2025
 Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:29:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:27:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.524	3.828	8186392	5340424	5.139	5.176
2) SA Decachlor...	10.252	8.879	5222131	5077972	4.704	5.077
Target Compounds						
21) L5 AR-1248-1	5.675	4.916	1822515	1195056	53.024m	49.509
22) L5 AR-1248-2	5.946	5.154	1970177	1715212	44.703m	54.271
23) L5 AR-1248-3	6.152	5.195	2271691	1567360	48.055	47.561
24) L5 AR-1248-4	6.551	5.368	3179324	2241362	55.247	58.306
25) L5 AR-1248-5	6.588	5.762	2749990	2082066	50.664	54.048

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 20:39
Operator : YP\AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:29:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:27:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 20:55
 Operator : YP\AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:42:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:41:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.828	149.1E6	96720518	93.390	94.825
2) SA Decachlor...	10.251	8.879	105.2E6	96618792	92.933	88.886
Target Compounds						
26) L6 AR-1254-1	6.527	5.722	52191144	49741488	893.548	880.090
27) L6 AR-1254-2	6.743	5.870	76163232	43195538	909.453	890.167
28) L6 AR-1254-3	7.106	6.275	78867294	69004581	913.417	911.168
29) L6 AR-1254-4	7.389	6.503	65665428	48529875	916.687	908.500
30) L6 AR-1254-5	7.806	6.922	65604720	63254548	923.372	917.897



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 20:55
Operator : YP\AJ
Sample : AR1254ICC1000
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:42:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:41:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 21:11
 Operator : YP\AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:42:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:41:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.524	3.828	116.1E6	73807381	72.699	72.361
2) SA Decachlor...	10.250	8.879	81355197	73665971	71.884	67.770
Target Compounds						
26) L6 AR-1254-1	6.526	5.722	41082518	39812295	703.361	704.410
27) L6 AR-1254-2	6.743	5.870	59469212	34485922	710.112	710.681
28) L6 AR-1254-3	7.106	6.275	60993256	54135888	706.405	714.835
29) L6 AR-1254-4	7.388	6.503	51027528	38224583	712.343	715.580
30) L6 AR-1254-5	7.806	6.922	50892047	48947585	716.295	710.286



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 21:11
Operator : YP\AJ
Sample : AR1254ICC750
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:42:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:41:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 21:28
 Operator : YP\AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:43:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:41:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.527	3.827	79847648	50999382	50.000	50.000
2) SA Decachlor...	10.253	8.879	56587852	54349698	50.000	50.000
Target Compounds						
26) L6 AR-1254-1	6.529	5.721	29204431	28259314	500.000	500.000
27) L6 AR-1254-2	6.745	5.869	41873104	24262597	500.000	500.000
28) L6 AR-1254-3	7.108	6.274	43171573	37866013	500.000	500.000
29) L6 AR-1254-4	7.391	6.502	35816695	26708804	500.000	500.000
30) L6 AR-1254-5	7.808	6.921	35524526	34456229	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 21:28
Operator : YP\AJ
Sample : AR1254ICC500
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:43:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:41:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 21:44
 Operator : YP\AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:43:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:41:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.522	3.828	41995422	27154292	26.297	26.622
2) SA Decachlor...	10.247	8.879	29750638	28828167	26.287	26.521
Target Compounds						
26) L6 AR-1254-1	6.524	5.721	15632135	15086022	267.633	266.921
27) L6 AR-1254-2	6.740	5.869	22251661	13109555	265.704	270.160
28) L6 AR-1254-3	7.103	6.274	22535007	20354474	260.994	268.770
29) L6 AR-1254-4	7.386	6.502	18941969	14262234	264.429	266.995
30) L6 AR-1254-5	7.802	6.921	18651779	18303656	262.520	265.607



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070443.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 21:44
Operator : YP\AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:43:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:41:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 22:00
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:43:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:41:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.828	8190039	4946549	5.129	4.850
2) SA Decachlor...	10.249	8.879	5357119	5757506	4.733	5.297
Target Compounds						
26) L6 AR-1254-1	6.527	5.722	2919684	3096335	49.987	54.784
27) L6 AR-1254-2	6.743	5.870	3852617	2719612	46.003	56.045
28) L6 AR-1254-3	7.107	6.275	4209211	3937712	48.750	51.995
29) L6 AR-1254-4	7.388	6.503	3479126	2689850	48.568	50.355
30) L6 AR-1254-5	7.806	6.922	3508468	3731398	49.381	54.147



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 22:00
Operator : YP\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:43:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:41:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070445.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 22:16
 Operator : YP\AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 22:54:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 22:53:51 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.524	3.828	79987375	50598241	50.000	50.000
2) SA Decachlor...	10.249	8.880	55265895	53517923	50.000	50.000
Target Compounds						
36) L8 AR-1262-1	8.107	6.960	40859309	41831981	500.000	500.000
37) L8 AR-1262-2	8.427	7.219	82356816	34364927	500.000	500.000
38) L8 AR-1262-3	8.745	7.743	56082248	32993103	500.000	500.000
39) L8 AR-1262-4	8.830	7.808	41901860	52217661	500.000	500.000
40) L8 AR-1262-5	9.487	8.310	29448112	25775032	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070445.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 22:16
Operator : YP\AJ
Sample : AR1262ICC500
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 22:54:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 22:53:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 22:33
 Operator : YP\AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 23:51:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 23:28:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.527	3.827	156.0E6	101.9E6	94.867	92.435
2) SA Decachlor...	10.254	8.878	179.7E6	163.2E6	93.195	93.675
Target Compounds						
41) L9 AR-1268-1	8.745	7.743	188.5E6	168.4E6	935.648	940.387
42) L9 AR-1268-2	8.839	7.808	162.7E6	142.0E6	939.401	947.708
43) L9 AR-1268-3	9.072	8.015	140.0E6	125.4E6	934.124	967.486
44) L9 AR-1268-4	9.491	8.309	62601215	54287293	945.965	955.597
45) L9 AR-1268-5	9.911	8.613	401.2E6	364.2E6	947.852	962.567



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 22:33
Operator : YP\AJ
Sample : AR1268ICC1000
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 23:51:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 23:28:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 22:49
 Operator : YP\AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 23:51:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 23:28:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.828	116.7E6	77586720	71.014	70.350
2) SA Decachlor...	10.250	8.879	138.1E6	124.4E6	71.630	71.383
Target Compounds						
41) L9 AR-1268-1	8.742	7.744	143.6E6	124.5E6	712.768	695.587
42) L9 AR-1268-2	8.836	7.809	124.1E6	105.1E6	716.292	701.198
43) L9 AR-1268-3	9.069	8.016	107.0E6	90348904	713.888	697.329
44) L9 AR-1268-4	9.489	8.309	47447237	39925484	716.974	702.792
45) L9 AR-1268-5	9.908	8.614	305.7E6	271.7E6	722.384	718.128



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 22:49
Operator : YP\AJ
Sample : AR1268ICC750
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 23:51:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 23:28:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 23:05
 Operator : YP\AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 23:51:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 23:28:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.522	3.827	82202011	55143422	50.000	50.000
2) SA Decachlor...	10.248	8.879	96427272	87115877	50.000	50.000
Target Compounds						
41) L9 AR-1268-1	8.740	7.743	100.7E6	89523621	500.000	500.000
42) L9 AR-1268-2	8.833	7.809	86604260	74921217	500.000	500.000
43) L9 AR-1268-3	9.066	8.015	74917746	64782125	500.000	500.000
44) L9 AR-1268-4	9.487	8.310	33088538	28404907	500.000	500.000
45) L9 AR-1268-5	9.904	8.613	211.6E6	189.2E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 23:05
Operator : YP\AJ
Sample : AR1268ICC500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 23:51:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 23:28:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 23:22
 Operator : YP\AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 23:51:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 23:28:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.523	3.826	42716878	29621715	25.983	26.859
2) SA Decachlor...	10.248	8.877	50455822	45920300	26.163	26.356
Target Compounds						
41) L9 AR-1268-1	8.741	7.742	52769831	46752818	261.890	261.120
42) L9 AR-1268-2	8.834	7.808	45106498	38372677	260.417	256.087
43) L9 AR-1268-3	9.067	8.014	38921973	33274907	259.765	256.822
44) L9 AR-1268-4	9.486	8.308	16901246	14619988	255.394	257.350
45) L9 AR-1268-5	9.905	8.612	110.8E6	95223241	261.876	251.705



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 23:22
Operator : YP\AJ
Sample : AR1268ICC250
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 23:51:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 23:28:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 23:38
 Operator : YP\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/12/2025
 Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 23:57:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 11 23:28:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.528	3.828	8554411	5571543	5.289	5.133
2) SA Decachlor...	10.252	8.879	9326315	9031570	4.918	5.259
Target Compounds						
41) L9 AR-1268-1	8.745	7.743	9919952	8743585	50.063	49.928m
42) L9 AR-1268-2	8.839	7.808	8340607	7243137	48.935	49.489m
43) L9 AR-1268-3	9.072	8.014	7178199	6658040	48.822	52.376m
44) L9 AR-1268-4	9.491	8.309	2987981	2604541	46.032	46.758
45) L9 AR-1268-5	9.910	8.613	21070074	17728904	50.305	47.735

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 23:38
Operator : YP\AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2025
Supervised By :Ankita Jodhani 03/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 23:57:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 11 23:28:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2025 23:54
 Operator : YP\AJ
 Sample : PP031125ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ICVPP031125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:13:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 00:06:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.523	3.827	81467484	52091643	52.378	51.973
2) SA Decachlor...	10.249	8.877	57030864	51101188	53.684	52.231
Target Compounds						
3) L1 AR-1016-1	5.675	4.914	26763573	18466483	516.161	513.635
4) L1 AR-1016-2	5.697	4.933	39150950	25663697	547.223	493.849
5) L1 AR-1016-3	5.760	5.111	24376753	14439904	535.307	507.493
6) L1 AR-1016-4	5.857	5.152	20068166	11515792	514.070	514.330
7) L1 AR-1016-5	6.150	5.367	18221356	14760415	526.294	496.668
31) L7 AR-1260-1	7.269	6.404	31459138	25772586	535.582	517.684
32) L7 AR-1260-2	7.523	6.592	43093099	34068219	525.250	515.502
33) L7 AR-1260-3	7.882	6.746	35379890	29455426	538.034	514.979
34) L7 AR-1260-4	8.106	7.218	34778399	26486148	532.246	517.676
35) L7 AR-1260-5	8.427	7.460	73694362	66685007	539.184	517.800



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 23:54
Operator : YP\AJ
Sample : PP031125ICV500
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP031125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:13:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 00:06:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2025 00:10
 Operator : YP\AJ
 Sample : AR1232ICV500
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ICVPP031125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 05:20:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 05:19:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.828	82637423	51891496	51.851	48.744
2) SA Decachlor...	10.250	8.879	56319561	51738897	52.291	51.344
Target Compounds						
11) L3 AR-1232-1	4.887	4.202	17817484	13234008	501.090	503.008
12) L3 AR-1232-2	5.412	4.934	9000524	12831570	533.581	497.115
13) L3 AR-1232-3	5.698	5.112	19000238	6787601	519.562	484.519
14) L3 AR-1232-4	5.858	5.196	9460626	5871572	498.077	501.319
15) L3 AR-1232-5	5.948	5.368	6697975	6583987	516.729	503.825



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2025 00:10
Operator : YP\AJ
Sample : AR1232ICV500
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP031125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 05:20:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 05:19:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2025 00:27
 Operator : YP\AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ICVPP031125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 02:29:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:28:34 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.522	3.828	80900104	52039514	51.573	51.996
2) SA Decachlor...	10.247	8.877	56432259	50213028	52.789	48.963
Target Compounds						
16) L4 AR-1242-1	5.673	4.914	21829875	15588752	491.127	509.246
17) L4 AR-1242-2	5.695	4.933	32588571	21901951	530.924	502.366
18) L4 AR-1242-3	5.758	5.111	19614357	12116039	528.672	508.387
19) L4 AR-1242-4	5.855	5.195	16599935	11430650	516.600	518.573
20) L4 AR-1242-5	6.586	5.720	17030676	14600485	548.536	522.919



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2025 00:27
Operator : YP\AJ
Sample : AR1242ICV500
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP031125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 02:29:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:28:34 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2025 00:43
 Operator : YP\AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ICVPP031125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:44:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 01:39:22 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.523	3.827	80763365	51993820	51.381	50.996
2) SA Decachlor...	10.249	8.879	57381734	53329390	53.107	53.338
Target Compounds						
21) L5 AR-1248-1	5.675	4.915	17366035	11930350	508.434	508.204
22) L5 AR-1248-2	5.948	5.152	22908060	15777449	539.683	504.016
23) L5 AR-1248-3	6.150	5.195	24248973	16449582	525.454	518.561
24) L5 AR-1248-4	6.549	5.368	29245571	19332171	504.310	496.038
25) L5 AR-1248-5	6.588	5.762	27662486	19099791	515.251	501.482



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2025 00:43
Operator : YP\AJ
Sample : AR1248ICV500
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP031125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:44:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 01:39:22 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2025 00:59
 Operator : YP\AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ICVPP031125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:56:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 01:49:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.827	82035673	53945391	51.568	53.445
2) SA Decachlor...	10.250	8.878	58425643	54856879	52.829	51.364
Target Compounds						
26) L6 AR-1254-1	6.527	5.721	29456235	28994348	514.431	514.789
27) L6 AR-1254-2	6.743	5.869	42978463	24997724	530.257	511.133
28) L6 AR-1254-3	7.106	6.274	43763209	38958184	519.927	516.564
29) L6 AR-1254-4	7.389	6.502	36692419	27576382	523.152	522.756
30) L6 AR-1254-5	7.805	6.921	36360967	35678139	520.504	516.666



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2025 00:59
Operator : YP\AJ
Sample : AR1254ICV500
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP031125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:56:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 01:49:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
 Data File : PP070456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Mar 2025 01:16
 Operator : YP\AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ICVPP031125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:57:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 01:57:27 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.826	82956019	55353504	50.459	50.190
2) SA Decachlor...	10.250	8.877	97699870	88842686	50.660	50.991
Target Compounds						
41) L9 AR-1268-1	8.742	7.742	101.7E6	89726484	504.572	501.133
42) L9 AR-1268-2	8.836	7.807	87505543	76005918	505.203	507.239
43) L9 AR-1268-3	9.069	8.013	75570485	65882951	504.356	508.496
44) L9 AR-1268-4	9.489	8.308	33480982	28268151	505.930	497.593
45) L9 AR-1268-5	9.907	8.612	213.6E6	191.8E6	504.629	506.856



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Mar 2025 01:16
Operator : YP\AJ
Sample : AR1268ICV500
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP031125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:57:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 01:57:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm





284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Continuing Calib Date: 03/17/2025 Initial Calibration Date(s): 02/20/2025 02/21/2025

Continuing Calib Time: 09:13 Initial Calibration Time(s): 16:46 01:02

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-2	(2)	4.81	4.81	4.71	4.91	0.00
Aroclor-1016-3	(3)	4.86	4.87	4.77	4.97	0.01
Aroclor-1016-4	(4)	4.98	4.99	4.89	5.09	0.01
Aroclor-1016-5	(5)	5.24	5.25	5.15	5.35	0.01
Aroclor-1260-1	(1)	6.28	6.29	6.19	6.39	0.01
Aroclor-1260-2	(2)	6.47	6.48	6.38	6.58	0.01
Aroclor-1260-3	(3)	6.84	6.85	6.75	6.95	0.01
Aroclor-1260-4	(4)	7.10	7.11	7.01	7.21	0.01
Aroclor-1260-5	(5)	7.34	7.35	7.25	7.45	0.01
Tetrachloro-m-xylene		3.69	3.70	3.60	3.80	0.01
Decachlorobiphenyl		8.75	8.76	8.66	8.86	0.02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Continuing Calib Date: 03/17/2025 Initial Calibration Date(s): 02/20/2025 02/21/2025

Continuing Calib Time: 09:13 Initial Calibration Time(s): 16:46 01:02

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.77	4.78	4.68	4.88	0.01
Aroclor-1016-2	(2)	4.79	4.80	4.70	4.90	0.01
Aroclor-1016-3	(3)	4.97	4.97	4.87	5.07	0.00
Aroclor-1016-4	(4)	5.01	5.01	4.91	5.11	0.00
Aroclor-1016-5	(5)	5.22	5.23	5.13	5.33	0.01
Aroclor-1260-1	(1)	6.25	6.26	6.16	6.36	0.01
Aroclor-1260-2	(2)	6.44	6.45	6.35	6.55	0.01
Aroclor-1260-3	(3)	6.60	6.60	6.50	6.70	0.01
Aroclor-1260-4	(4)	7.07	7.07	6.97	7.17	0.00
Aroclor-1260-5	(5)	7.31	7.31	7.21	7.41	0.00
Tetrachloro-m-xylene		3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl		8.70	8.71	8.61	8.81	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 02/20/2025 02/20/2025

Client Sample No.: CCAL01 Date Analyzed: 03/17/2025

Lab Sample No.: AR1660CCC500 Data File : PO109923.D Time Analyzed: 09:13

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.787	4.691	4.891	520.420	500.000	4.1
Aroclor-1016-2	4.806	4.711	4.911	532.150	500.000	6.4
Aroclor-1016-3	4.862	4.767	4.967	529.790	500.000	6.0
Aroclor-1016-4	4.983	4.888	5.088	529.650	500.000	5.9
Aroclor-1016-5	5.241	5.145	5.345	513.580	500.000	2.7
Aroclor-1260-1	6.281	6.188	6.388	491.640	500.000	-1.7
Aroclor-1260-2	6.470	6.377	6.577	488.670	500.000	-2.3
Aroclor-1260-3	6.838	6.746	6.946	474.600	500.000	-5.1
Aroclor-1260-4	7.098	7.005	7.205	472.840	500.000	-5.4
Aroclor-1260-5	7.340	7.247	7.447	469.530	500.000	-6.1
Decachlorobiphenyl	8.745	8.657	8.857	40.020	50.000	-20.0
Tetrachloro-m-xylene	3.694	3.598	3.798	52.550	50.000	5.1



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 02/20/2025 02/20/2025

Client Sample No.: CCAL01 Date Analyzed: 03/17/2025

Lab Sample No.: AR1660CCC500 Data File : PO109923.D Time Analyzed: 09:13

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.772	4.678	4.878	539.290	500.000	7.9
Aroclor-1016-2	4.792	4.697	4.897	554.740	500.000	10.9
Aroclor-1016-3	4.967	4.872	5.072	548.600	500.000	9.7
Aroclor-1016-4	5.009	4.914	5.114	529.410	500.000	5.9
Aroclor-1016-5	5.222	5.127	5.327	523.530	500.000	4.7
Aroclor-1260-1	6.254	6.161	6.361	502.590	500.000	0.5
Aroclor-1260-2	6.442	6.348	6.548	501.730	500.000	0.3
Aroclor-1260-3	6.595	6.502	6.702	496.860	500.000	-0.6
Aroclor-1260-4	7.066	6.974	7.174	484.000	500.000	-3.2
Aroclor-1260-5	7.307	7.214	7.414	488.740	500.000	-2.3
Decachlorobiphenyl	8.696	8.607	8.807	39.180	50.000	-21.6
Tetrachloro-m-xylene	3.691	3.594	3.794	52.290	50.000	4.6

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031725\
 Data File : P0109923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2025 09:13
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 06:58:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.694	3.691	497.4E6	273.7E6	52.554	52.291
2) SA Decachlor...	8.745	8.696	344.2E6	124.7E6	40.015	39.176
Target Compounds						
3) L1 AR-1016-1	4.787	4.772	160.4E6	84221887	520.420	539.294
4) L1 AR-1016-2	4.806	4.792	224.1E6	120.1E6	532.155	554.744
5) L1 AR-1016-3	4.862	4.967	156.7E6	65530811	529.786	548.599
6) L1 AR-1016-4	4.983	5.009	122.8E6	55095600	529.647	529.406
7) L1 AR-1016-5	5.241	5.222	132.6E6	71333008	513.583	523.532
31) L7 AR-1260-1	6.281	6.254	229.2E6	119.1E6	491.643	502.589
32) L7 AR-1260-2	6.470	6.442	276.2E6	138.1E6	488.675	501.730
33) L7 AR-1260-3	6.838	6.595	225.7E6	126.7E6	474.598	496.860
34) L7 AR-1260-4	7.098	7.066	204.1E6	99797224	472.841	484.001
35) L7 AR-1260-5	7.340	7.307	466.7E6	218.8E6	469.535	488.739



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031725\
Data File : PO109923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2025 09:13
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 06:58:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm





284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Continuing Calib Date: 03/17/2025 Initial Calibration Date(s): 02/20/2025 02/21/2025

Continuing Calib Time: 16:28 Initial Calibration Time(s): 16:46 01:02

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.79	4.79	4.69	4.89	0.00
Aroclor-1016-2	(2)	4.81	4.81	4.71	4.91	0.00
Aroclor-1016-3	(3)	4.86	4.87	4.77	4.97	0.01
Aroclor-1016-4	(4)	4.98	4.99	4.89	5.09	0.01
Aroclor-1016-5	(5)	5.24	5.25	5.15	5.35	0.01
Aroclor-1260-1	(1)	6.28	6.29	6.19	6.39	0.01
Aroclor-1260-2	(2)	6.47	6.48	6.38	6.58	0.01
Aroclor-1260-3	(3)	6.84	6.85	6.75	6.95	0.01
Aroclor-1260-4	(4)	7.10	7.11	7.01	7.21	0.01
Aroclor-1260-5	(5)	7.34	7.35	7.25	7.45	0.01
Tetrachloro-m-xylene		3.69	3.70	3.60	3.80	0.01
Decachlorobiphenyl		8.75	8.76	8.66	8.86	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Continuing Calib Date: 03/17/2025 Initial Calibration Date(s): 02/20/2025 02/21/2025

Continuing Calib Time: 16:28 Initial Calibration Time(s): 16:46 01:02

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.77	4.78	4.68	4.88	0.01
Aroclor-1016-2	(2)	4.79	4.80	4.70	4.90	0.01
Aroclor-1016-3	(3)	4.97	4.97	4.87	5.07	0.00
Aroclor-1016-4	(4)	5.01	5.01	4.91	5.11	0.00
Aroclor-1016-5	(5)	5.22	5.23	5.13	5.33	0.01
Aroclor-1260-1	(1)	6.26	6.26	6.16	6.36	0.00
Aroclor-1260-2	(2)	6.44	6.45	6.35	6.55	0.01
Aroclor-1260-3	(3)	6.60	6.60	6.50	6.70	0.00
Aroclor-1260-4	(4)	7.07	7.07	6.97	7.17	0.00
Aroclor-1260-5	(5)	7.31	7.31	7.21	7.41	0.00
Tetrachloro-m-xylene		3.69	3.69	3.59	3.79	0.00
Decachlorobiphenyl		8.70	8.71	8.61	8.81	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 02/20/2025 02/20/2025

Client Sample No.: CCAL02 Date Analyzed: 03/17/2025

Lab Sample No.: AR1660CCC500 Data File : PO109935.D Time Analyzed: 16:28

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.787	4.691	4.891	495.420	500.000	-0.9
Aroclor-1016-2	4.806	4.711	4.911	497.010	500.000	-0.6
Aroclor-1016-3	4.862	4.767	4.967	497.830	500.000	-0.4
Aroclor-1016-4	4.983	4.888	5.088	499.000	500.000	-0.2
Aroclor-1016-5	5.240	5.145	5.345	500.320	500.000	0.1
Aroclor-1260-1	6.282	6.188	6.388	468.480	500.000	-6.3
Aroclor-1260-2	6.470	6.377	6.577	466.430	500.000	-6.7
Aroclor-1260-3	6.839	6.746	6.946	449.630	500.000	-10.1
Aroclor-1260-4	7.099	7.005	7.205	446.990	500.000	-10.6
Aroclor-1260-5	7.340	7.247	7.447	446.440	500.000	-10.7
Decachlorobiphenyl	8.747	8.657	8.857	53.600	50.000	7.2
Tetrachloro-m-xylene	3.694	3.598	3.798	47.390	50.000	-5.2



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 02/20/2025 02/20/2025

Client Sample No.: CCAL02 Date Analyzed: 03/17/2025

Lab Sample No.: AR1660CCC500 Data File : PO109935.D Time Analyzed: 16:28

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.773	4.678	4.878	506.990	500.000	1.4
Aroclor-1016-2	4.792	4.697	4.897	518.690	500.000	3.7
Aroclor-1016-3	4.968	4.872	5.072	517.250	500.000	3.5
Aroclor-1016-4	5.010	4.914	5.114	489.360	500.000	-2.1
Aroclor-1016-5	5.223	5.127	5.327	513.620	500.000	2.7
Aroclor-1260-1	6.255	6.161	6.361	474.040	500.000	-5.2
Aroclor-1260-2	6.442	6.348	6.548	476.300	500.000	-4.7
Aroclor-1260-3	6.596	6.502	6.702	469.320	500.000	-6.1
Aroclor-1260-4	7.067	6.974	7.174	450.460	500.000	-9.9
Aroclor-1260-5	7.308	7.214	7.414	446.130	500.000	-10.8
Decachlorobiphenyl	8.697	8.607	8.807	49.430	50.000	-1.1
Tetrachloro-m-xylene	3.692	3.594	3.794	48.820	50.000	-2.4

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031725\
 Data File : P0109935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2025 16:28
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 01:34:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.694	3.692	448.6E6	255.5E6	47.393	48.822
2) SA Decachlor...	8.747	8.697	461.1E6	157.4E6	53.604	49.429
Target Compounds						
3) L1 AR-1016-1	4.787	4.773	152.7E6	79176920	495.422	506.990
4) L1 AR-1016-2	4.806	4.792	209.3E6	112.3E6	497.015	518.690
5) L1 AR-1016-3	4.862	4.968	147.3E6	61786467	497.827	517.253
6) L1 AR-1016-4	4.983	5.010	115.7E6	50928405	499.002	489.364
7) L1 AR-1016-5	5.240	5.223	129.2E6	69982443	500.321	513.619
31) L7 AR-1260-1	6.282	6.255	218.4E6	112.3E6	468.484	474.035
32) L7 AR-1260-2	6.470	6.442	263.6E6	131.1E6	466.430	476.299
33) L7 AR-1260-3	6.839	6.596	213.9E6	119.7E6	449.630	469.317
34) L7 AR-1260-4	7.099	7.067	192.9E6	92881978	446.987	450.463
35) L7 AR-1260-5	7.340	7.308	443.7E6	199.8E6	446.441	446.129



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031725\
Data File : PO109935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2025 16:28
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 01:34:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm





284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Continuing Calib Date: 03/14/2025 Initial Calibration Date(s): 03/11/2025 03/11/2025

Continuing Calib Time: 21:15 Initial Calibration Time(s): 15:13 23:38

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	5.68	5.68	5.58	5.78	0.00
Aroclor-1016-2	(2)	5.70	5.70	5.60	5.80	0.00
Aroclor-1016-3	(3)	5.76	5.76	5.66	5.86	0.00
Aroclor-1016-4	(4)	5.86	5.86	5.76	5.96	0.00
Aroclor-1016-5	(5)	6.15	6.15	6.05	6.25	0.00
Aroclor-1260-1	(1)	7.27	7.27	7.17	7.37	0.00
Aroclor-1260-2	(2)	7.52	7.53	7.43	7.63	0.01
Aroclor-1260-3	(3)	7.88	7.88	7.78	7.98	0.00
Aroclor-1260-4	(4)	8.11	8.11	8.01	8.21	0.01
Aroclor-1260-5	(5)	8.43	8.43	8.33	8.53	0.00
Tetrachloro-m-xylene		4.53	4.52	4.42	4.62	-0.01
Decachlorobiphenyl		10.24	10.25	10.15	10.35	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Continuing Calib Date: 03/14/2025 Initial Calibration Date(s): 03/11/2025 03/11/2025

Continuing Calib Time: 21:15 Initial Calibration Time(s): 15:13 23:38

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.91	4.92	4.82	5.02	0.01
Aroclor-1016-2	(2)	4.93	4.94	4.84	5.04	0.01
Aroclor-1016-3	(3)	5.11	5.11	5.01	5.21	0.00
Aroclor-1016-4	(4)	5.15	5.15	5.05	5.25	0.00
Aroclor-1016-5	(5)	5.37	5.37	5.27	5.47	0.01
Aroclor-1260-1	(1)	6.40	6.41	6.31	6.51	0.01
Aroclor-1260-2	(2)	6.59	6.60	6.50	6.70	0.01
Aroclor-1260-3	(3)	6.74	6.75	6.65	6.85	0.01
Aroclor-1260-4	(4)	7.22	7.22	7.12	7.32	0.00
Aroclor-1260-5	(5)	7.46	7.46	7.36	7.56	0.00
Tetrachloro-m-xylene		3.83	3.83	3.73	3.93	0.00
Decachlorobiphenyl		8.87	8.88	8.78	8.98	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 03/11/2025 03/11/2025

Client Sample No.: CCAL03 Date Analyzed: 03/14/2025

Lab Sample No.: AR1660CCC500 Data File : PP070543.D Time Analyzed: 21:15

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	5.676	5.577	5.777	443.660	500.000	-11.3
Aroclor-1016-2	5.698	5.599	5.799	480.930	500.000	-3.8
Aroclor-1016-3	5.760	5.661	5.861	466.910	500.000	-6.6
Aroclor-1016-4	5.858	5.758	5.958	456.460	500.000	-8.7
Aroclor-1016-5	6.150	6.051	6.251	453.110	500.000	-9.4
Aroclor-1260-1	7.269	7.171	7.371	470.290	500.000	-5.9
Aroclor-1260-2	7.523	7.425	7.625	461.520	500.000	-7.7
Aroclor-1260-3	7.881	7.783	7.983	466.760	500.000	-6.6
Aroclor-1260-4	8.105	8.008	8.208	454.640	500.000	-9.1
Aroclor-1260-5	8.425	8.328	8.528	467.430	500.000	-6.5
Decachlorobiphenyl	10.243	10.152	10.352	46.560	50.000	-6.9
Tetrachloro-m-xylene	4.525	4.424	4.624	46.830	50.000	-6.3



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 03/11/2025 03/11/2025

Client Sample No.: CCAL03 Date Analyzed: 03/14/2025

Lab Sample No.: AR1660CCC500 Data File : PP070543.D Time Analyzed: 21:15

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.912	4.817	5.017	467.760	500.000	-6.4
Aroclor-1016-2	4.932	4.836	5.036	453.880	500.000	-9.2
Aroclor-1016-3	5.108	5.013	5.213	459.150	500.000	-8.2
Aroclor-1016-4	5.150	5.054	5.254	462.340	500.000	-7.5
Aroclor-1016-5	5.365	5.270	5.470	472.460	500.000	-5.5
Aroclor-1260-1	6.401	6.307	6.507	458.750	500.000	-8.3
Aroclor-1260-2	6.589	6.495	6.695	458.120	500.000	-8.4
Aroclor-1260-3	6.743	6.649	6.849	450.000	500.000	-10.0
Aroclor-1260-4	7.215	7.121	7.321	441.280	500.000	-11.7
Aroclor-1260-5	7.456	7.362	7.562	440.290	500.000	-11.9
Decachlorobiphenyl	8.871	8.781	8.981	41.930	50.000	-16.1
Tetrachloro-m-xylene	3.826	3.729	3.929	48.070	50.000	-3.9

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
 Data File : PP070543.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2025 21:15
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 23:47:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:42:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.826	72837798	48174998	46.830	48.065
2) SA Decachlor...	10.243	8.871	49463610	41021745	46.561	41.929
Target Compounds						
3) L1 AR-1016-1	5.676	4.912	23004433	16817234	443.662	467.762
4) L1 AR-1016-2	5.698	4.932	34407759	23586690	480.926	453.881
5) L1 AR-1016-3	5.760	5.108	21262090	13064494	466.909	459.154
6) L1 AR-1016-4	5.858	5.150	17819012	10351658	456.456	462.336
7) L1 AR-1016-5	6.150	5.365	15687675	14041040	453.113	472.462
31) L7 AR-1260-1	7.269	6.401	27624243	22838490	470.294	458.748
32) L7 AR-1260-2	7.523	6.589	37864401	30275766	461.519	458.116
33) L7 AR-1260-3	7.881	6.743	30692750	25738947	466.755	450.002
34) L7 AR-1260-4	8.105	7.215	29707435	22577196	454.640	441.275
35) L7 AR-1260-5	8.425	7.456	63887192	56703176	467.430	440.292



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
Data File : PP070543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2025 21:15
Operator : YP\AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 23:47:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm





284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Continuing Calib Date: 03/15/2025 Initial Calibration Date(s): 03/11/2025 03/11/2025

Continuing Calib Time: 01:51 Initial Calibration Time(s): 15:13 23:38

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	5.68	5.68	5.58	5.78	0.00
Aroclor-1016-2	(2)	5.70	5.70	5.60	5.80	0.00
Aroclor-1016-3	(3)	5.76	5.76	5.66	5.86	0.00
Aroclor-1016-4	(4)	5.86	5.86	5.76	5.96	0.00
Aroclor-1016-5	(5)	6.15	6.15	6.05	6.25	0.00
Aroclor-1260-1	(1)	7.27	7.27	7.17	7.37	0.00
Aroclor-1260-2	(2)	7.52	7.53	7.43	7.63	0.01
Aroclor-1260-3	(3)	7.88	7.88	7.78	7.98	0.00
Aroclor-1260-4	(4)	8.10	8.11	8.01	8.21	0.01
Aroclor-1260-5	(5)	8.42	8.43	8.33	8.53	0.01
Tetrachloro-m-xylene		4.52	4.52	4.42	4.62	0.00
Decachlorobiphenyl		10.24	10.25	10.15	10.35	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Continuing Calib Date: 03/15/2025 Initial Calibration Date(s): 03/11/2025 03/11/2025

Continuing Calib Time: 01:51 Initial Calibration Time(s): 15:13 23:38

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.91	4.92	4.82	5.02	0.01
Aroclor-1016-2	(2)	4.93	4.94	4.84	5.04	0.01
Aroclor-1016-3	(3)	5.11	5.11	5.01	5.21	0.00
Aroclor-1016-4	(4)	5.15	5.15	5.05	5.25	0.00
Aroclor-1016-5	(5)	5.36	5.37	5.27	5.47	0.01
Aroclor-1260-1	(1)	6.40	6.41	6.31	6.51	0.01
Aroclor-1260-2	(2)	6.59	6.60	6.50	6.70	0.01
Aroclor-1260-3	(3)	6.74	6.75	6.65	6.85	0.01
Aroclor-1260-4	(4)	7.21	7.22	7.12	7.32	0.01
Aroclor-1260-5	(5)	7.45	7.46	7.36	7.56	0.01
Tetrachloro-m-xylene		3.83	3.83	3.73	3.93	0.00
Decachlorobiphenyl		8.87	8.88	8.78	8.98	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 03/11/2025 03/11/2025

Client Sample No.: CCAL04 Date Analyzed: 03/15/2025

Lab Sample No.: AR1660CCC500 Data File : PP070558.D Time Analyzed: 01:51

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	5.675	5.577	5.777	457.150	500.000	-8.6
Aroclor-1016-2	5.697	5.599	5.799	495.200	500.000	-1.0
Aroclor-1016-3	5.759	5.661	5.861	478.090	500.000	-4.4
Aroclor-1016-4	5.856	5.758	5.958	468.080	500.000	-6.4
Aroclor-1016-5	6.149	6.051	6.251	469.590	500.000	-6.1
Aroclor-1260-1	7.267	7.171	7.371	498.380	500.000	-0.3
Aroclor-1260-2	7.520	7.425	7.625	477.820	500.000	-4.4
Aroclor-1260-3	7.879	7.783	7.983	476.270	500.000	-4.7
Aroclor-1260-4	8.103	8.008	8.208	464.610	500.000	-7.1
Aroclor-1260-5	8.423	8.328	8.528	479.710	500.000	-4.1
Decachlorobiphenyl	10.241	10.152	10.352	47.630	50.000	-4.7
Tetrachloro-m-xylene	4.524	4.424	4.624	48.060	50.000	-3.9



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 03/11/2025 03/11/2025

Client Sample No.: CCAL04 Date Analyzed: 03/15/2025

Lab Sample No.: AR1660CCC500 Data File : PP070558.D Time Analyzed: 01:51

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.912	4.817	5.017	500.790	500.000	0.2
Aroclor-1016-2	4.930	4.836	5.036	484.340	500.000	-3.1
Aroclor-1016-3	5.108	5.013	5.213	493.000	500.000	-1.4
Aroclor-1016-4	5.149	5.054	5.254	494.170	500.000	-1.2
Aroclor-1016-5	5.364	5.270	5.470	521.050	500.000	4.2
Aroclor-1260-1	6.400	6.307	6.507	477.160	500.000	-4.6
Aroclor-1260-2	6.588	6.495	6.695	473.000	500.000	-5.4
Aroclor-1260-3	6.742	6.649	6.849	465.110	500.000	-7.0
Aroclor-1260-4	7.213	7.121	7.321	453.670	500.000	-9.3
Aroclor-1260-5	7.454	7.362	7.562	455.190	500.000	-9.0
Decachlorobiphenyl	8.871	8.781	8.981	46.060	50.000	-7.9
Tetrachloro-m-xylene	3.826	3.729	3.929	48.770	50.000	-2.5

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
 Data File : PP070558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2025 01:51
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 02:31:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:42:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.524	3.826	74756241	48883903	48.063	48.773
2) SA Decachlor...	10.241	8.871	50596537	45061865	47.627	46.059
Target Compounds						
3) L1 AR-1016-1	5.675	4.912	23703888	18004636	457.152	500.789
4) L1 AR-1016-2	5.697	4.930	35429053	25169506	495.201	484.339
5) L1 AR-1016-3	5.759	5.108	21771400	14027474	478.094	492.998
6) L1 AR-1016-4	5.856	5.149	18272721	11064426	468.078	494.170
7) L1 AR-1016-5	6.149	5.364	16258237	15485105	469.592	521.053
31) L7 AR-1260-1	7.267	6.400	29274222	23755351	498.385	477.165
32) L7 AR-1260-2	7.520	6.588	39202114	31259651	477.824	473.004
33) L7 AR-1260-3	7.879	6.742	31318736	26603333	476.275	465.115
34) L7 AR-1260-4	8.103	7.213	30358624	23211275	464.606	453.668
35) L7 AR-1260-5	8.423	7.454	65565497	58621260	479.709	455.186



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
Data File : PP070558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2025 01:51
Operator : YP\AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 02:31:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm





284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Continuing Calib Date: 03/15/2025 Initial Calibration Date(s): 03/11/2025 03/11/2025

Continuing Calib Time: 05:06 Initial Calibration Time(s): 15:13 23:38

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	5.67	5.68	5.58	5.78	0.01
Aroclor-1016-2	(2)	5.70	5.70	5.60	5.80	0.00
Aroclor-1016-3	(3)	5.76	5.76	5.66	5.86	0.00
Aroclor-1016-4	(4)	5.86	5.86	5.76	5.96	0.00
Aroclor-1016-5	(5)	6.15	6.15	6.05	6.25	0.00
Aroclor-1260-1	(1)	7.27	7.27	7.17	7.37	0.00
Aroclor-1260-2	(2)	7.52	7.53	7.43	7.63	0.01
Aroclor-1260-3	(3)	7.88	7.88	7.78	7.98	0.00
Aroclor-1260-4	(4)	8.10	8.11	8.01	8.21	0.01
Aroclor-1260-5	(5)	8.42	8.43	8.33	8.53	0.01
Tetrachloro-m-xylene		4.52	4.52	4.42	4.62	0.00
Decachlorobiphenyl		10.24	10.25	10.15	10.35	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Continuing Calib Date: 03/15/2025 Initial Calibration Date(s): 03/11/2025 03/11/2025

Continuing Calib Time: 05:06 Initial Calibration Time(s): 15:13 23:38

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.91	4.92	4.82	5.02	0.01
Aroclor-1016-2	(2)	4.93	4.94	4.84	5.04	0.01
Aroclor-1016-3	(3)	5.11	5.11	5.01	5.21	0.00
Aroclor-1016-4	(4)	5.15	5.15	5.05	5.25	0.00
Aroclor-1016-5	(5)	5.36	5.37	5.27	5.47	0.01
Aroclor-1260-1	(1)	6.40	6.41	6.31	6.51	0.01
Aroclor-1260-2	(2)	6.59	6.60	6.50	6.70	0.01
Aroclor-1260-3	(3)	6.74	6.75	6.65	6.85	0.01
Aroclor-1260-4	(4)	7.21	7.22	7.12	7.32	0.01
Aroclor-1260-5	(5)	7.45	7.46	7.36	7.56	0.01
Tetrachloro-m-xylene		3.83	3.83	3.73	3.93	0.00
Decachlorobiphenyl		8.87	8.88	8.78	8.98	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 03/11/2025 03/11/2025

Client Sample No.: CCAL05 Date Analyzed: 03/15/2025

Lab Sample No.: AR1660CCC500 Data File : PP070568.D Time Analyzed: 05:06

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	5.673	5.577	5.777	464.850	500.000	-7.0
Aroclor-1016-2	5.695	5.599	5.799	501.140	500.000	0.2
Aroclor-1016-3	5.757	5.661	5.861	487.390	500.000	-2.5
Aroclor-1016-4	5.855	5.758	5.958	483.220	500.000	-3.4
Aroclor-1016-5	6.147	6.051	6.251	479.270	500.000	-4.1
Aroclor-1260-1	7.266	7.171	7.371	508.310	500.000	1.7
Aroclor-1260-2	7.519	7.425	7.625	490.450	500.000	-1.9
Aroclor-1260-3	7.878	7.783	7.983	488.320	500.000	-2.3
Aroclor-1260-4	8.102	8.008	8.208	471.720	500.000	-5.7
Aroclor-1260-5	8.422	8.328	8.528	487.240	500.000	-2.6
Decachlorobiphenyl	10.239	10.152	10.352	48.570	50.000	-2.9
Tetrachloro-m-xylene	4.522	4.424	4.624	48.550	50.000	-2.9



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 03/11/2025 03/11/2025

Client Sample No.: CCAL05 Date Analyzed: 03/15/2025

Lab Sample No.: AR1660CCC500 Data File : PP070568.D Time Analyzed: 05:06

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.912	4.817	5.017	511.620	500.000	2.3
Aroclor-1016-2	4.930	4.836	5.036	488.190	500.000	-2.4
Aroclor-1016-3	5.107	5.013	5.213	502.650	500.000	0.5
Aroclor-1016-4	5.149	5.054	5.254	495.770	500.000	-0.8
Aroclor-1016-5	5.364	5.270	5.470	540.650	500.000	8.1
Aroclor-1260-1	6.400	6.307	6.507	493.180	500.000	-1.4
Aroclor-1260-2	6.587	6.495	6.695	483.690	500.000	-3.3
Aroclor-1260-3	6.741	6.649	6.849	471.010	500.000	-5.8
Aroclor-1260-4	7.213	7.121	7.321	458.170	500.000	-8.4
Aroclor-1260-5	7.454	7.362	7.562	453.230	500.000	-9.4
Decachlorobiphenyl	8.869	8.781	8.981	46.240	50.000	-7.5
Tetrachloro-m-xylene	3.826	3.729	3.929	49.820	50.000	-0.4

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
 Data File : PP070568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2025 05:06
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 05:29:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:42:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.522	3.826	75517285	49932854	48.552	49.819
2) SA Decachlor...	10.239	8.869	51602626	45241438	48.574	46.242
Target Compounds						
3) L1 AR-1016-1	5.673	4.912	24102790	18394063	464.845	511.621
4) L1 AR-1016-2	5.695	4.930	35853798	25369861	501.137	488.195
5) L1 AR-1016-3	5.757	5.107	22194655	14301994	487.388	502.646
6) L1 AR-1016-4	5.855	5.149	18863726	11100213	483.217	495.769
7) L1 AR-1016-5	6.147	5.364	16593299	16067422	479.270	540.647
31) L7 AR-1260-1	7.266	6.400	29857150	24552460	508.309	493.176
32) L7 AR-1260-2	7.519	6.587	40237821	31965538	490.448	483.685
33) L7 AR-1260-3	7.878	6.741	32110960	26940329	488.323	471.007
34) L7 AR-1260-4	8.102	7.213	30823185	23441586	471.715	458.170
35) L7 AR-1260-5	8.422	7.454	66595335	58369121	487.244	453.228



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
Data File : PP070568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2025 05:06
Operator : YP\AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 05:29:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm



Analytical Sequence

Client: G Environmental

SDG No.: Q1574

Project: Ave L

Instrument ID: ECD_O

GC Column: ZB-MR1

ID: 0.32 (mm)

Inst. Calib. Date(s): 02/20/2025

02/20/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	02/20/2025	16:28	PO109425.D	8.76	3.70
AR1660ICC1000	AR1660ICC1000	02/20/2025	16:46	PO109426.D	8.76	3.70
AR1660ICC750	AR1660ICC750	02/20/2025	17:04	PO109427.D	8.76	3.70
AR1660ICC500	AR1660ICC500	02/20/2025	17:23	PO109428.D	8.76	3.70
AR1660ICC250	AR1660ICC250	02/20/2025	17:41	PO109429.D	8.76	3.70
AR1660ICC050	AR1660ICC050	02/20/2025	17:59	PO109430.D	8.76	3.70
AR1221ICC500	AR1221ICC500	02/20/2025	18:18	PO109431.D	8.76	3.70
AR1232ICC500	AR1232ICC500	02/20/2025	18:36	PO109432.D	8.76	3.70
AR1242ICC1000	AR1242ICC1000	02/20/2025	18:55	PO109433.D	8.76	3.70
AR1242ICC750	AR1242ICC750	02/20/2025	19:13	PO109434.D	8.76	3.70
AR1242ICC500	AR1242ICC500	02/20/2025	19:31	PO109435.D	8.76	3.70
AR1242ICC250	AR1242ICC250	02/20/2025	19:50	PO109436.D	8.76	3.70
AR1242ICC050	AR1242ICC050	02/20/2025	20:08	PO109437.D	8.76	3.70
AR1248ICC1000	AR1248ICC1000	02/20/2025	20:26	PO109438.D	8.76	3.70
AR1248ICC750	AR1248ICC750	02/20/2025	20:45	PO109439.D	8.76	3.70
AR1248ICC500	AR1248ICC500	02/20/2025	21:03	PO109440.D	8.76	3.70
AR1248ICC250	AR1248ICC250	02/20/2025	21:21	PO109441.D	8.76	3.70
AR1248ICC050	AR1248ICC050	02/20/2025	21:40	PO109442.D	8.75	3.70
AR1254ICC1000	AR1254ICC1000	02/20/2025	21:58	PO109443.D	8.75	3.70
AR1254ICC750	AR1254ICC750	02/20/2025	22:17	PO109444.D	8.76	3.70
AR1254ICC500	AR1254ICC500	02/20/2025	22:35	PO109445.D	8.76	3.70
AR1254ICC250	AR1254ICC250	02/20/2025	22:53	PO109446.D	8.76	3.70
AR1254ICC050	AR1254ICC050	02/20/2025	23:12	PO109447.D	8.76	3.70
AR1262ICC500	AR1262ICC500	02/20/2025	23:30	PO109448.D	8.75	3.70
AR1268ICC1000	AR1268ICC1000	02/20/2025	23:48	PO109449.D	8.76	3.70
AR1268ICC750	AR1268ICC750	02/21/2025	00:07	PO109450.D	8.76	3.70
AR1268ICC500	AR1268ICC500	02/21/2025	00:25	PO109451.D	8.75	3.70
AR1268ICC250	AR1268ICC250	02/21/2025	00:43	PO109452.D	8.76	3.70
AR1268ICC050	AR1268ICC050	02/21/2025	01:02	PO109453.D	8.75	3.70
AR1660CCC500	AR1660CCC500	03/17/2025	09:13	PO109923.D	8.75	3.69
IBLK	IBLK	03/17/2025	10:26	PO109927.D	8.75	3.69
WC1	Q1574-01	03/17/2025	11:02	PO109929.D	8.75	3.69
WC1DL	Q1574-01DL	03/17/2025	11:20	PO109930.D	8.74	3.69
AR1660CCC500	AR1660CCC500	03/17/2025	16:28	PO109935.D	8.75	3.69
IBLK	IBLK	03/17/2025	17:42	PO109939.D	8.75	3.69
IBLK	IBLK	03/11/2025	14:57	PP070418.D	10.25	4.53
AR1660ICC1000	AR1660ICC1000	03/11/2025	15:13	PP070419.D	10.25	4.53
AR1660ICC750	AR1660ICC750	03/11/2025	15:29	PP070420.D	10.25	4.52
AR1660ICC500	AR1660ICC500	03/11/2025	15:46	PP070421.D	10.25	4.52
AR1660ICC250	AR1660ICC250	03/11/2025	16:02	PP070422.D	10.26	4.53
AR1660ICC050	AR1660ICC050	03/11/2025	16:18	PP070423.D	10.25	4.53
AR1221ICC500	AR1221ICC500	03/11/2025	16:34	PP070424.D	10.25	4.53

Analytical Sequence

AR1232ICC1000	AR1232ICC1000	03/11/2025	16:51	PP070425.D	10.25	4.53
AR1232ICC750	AR1232ICC750	03/11/2025	17:07	PP070426.D	10.25	4.53
AR1232ICC500	AR1232ICC500	03/11/2025	17:23	PP070427.D	10.25	4.53
AR1232ICC250	AR1232ICC250	03/11/2025	17:40	PP070428.D	10.25	4.53
AR1232ICC050	AR1232ICC050	03/11/2025	17:56	PP070429.D	10.26	4.53
AR1242ICC1000	AR1242ICC1000	03/11/2025	18:12	PP070430.D	10.25	4.53
AR1242ICC750	AR1242ICC750	03/11/2025	18:28	PP070431.D	10.25	4.53
AR1242ICC500	AR1242ICC500	03/11/2025	18:45	PP070432.D	10.25	4.53
AR1242ICC250	AR1242ICC250	03/11/2025	19:01	PP070433.D	10.25	4.52
AR1242ICC050	AR1242ICC050	03/11/2025	19:17	PP070434.D	10.25	4.53
AR1248ICC1000	AR1248ICC1000	03/11/2025	19:34	PP070435.D	10.25	4.53
AR1248ICC750	AR1248ICC750	03/11/2025	19:50	PP070436.D	10.25	4.52
AR1248ICC500	AR1248ICC500	03/11/2025	20:06	PP070437.D	10.25	4.52
AR1248ICC250	AR1248ICC250	03/11/2025	20:22	PP070438.D	10.25	4.52
AR1248ICC050	AR1248ICC050	03/11/2025	20:39	PP070439.D	10.25	4.52
AR1254ICC1000	AR1254ICC1000	03/11/2025	20:55	PP070440.D	10.25	4.53
AR1254ICC750	AR1254ICC750	03/11/2025	21:11	PP070441.D	10.25	4.52
AR1254ICC500	AR1254ICC500	03/11/2025	21:28	PP070442.D	10.25	4.53
AR1254ICC250	AR1254ICC250	03/11/2025	21:44	PP070443.D	10.25	4.52
AR1254ICC050	AR1254ICC050	03/11/2025	22:00	PP070444.D	10.25	4.53
AR1262ICC500	AR1262ICC500	03/11/2025	22:16	PP070445.D	10.25	4.52
AR1268ICC1000	AR1268ICC1000	03/11/2025	22:33	PP070446.D	10.25	4.53
AR1268ICC750	AR1268ICC750	03/11/2025	22:49	PP070447.D	10.25	4.53
AR1268ICC500	AR1268ICC500	03/11/2025	23:05	PP070448.D	10.25	4.52
AR1268ICC250	AR1268ICC250	03/11/2025	23:22	PP070449.D	10.25	4.52
AR1268ICC050	AR1268ICC050	03/11/2025	23:38	PP070450.D	10.25	4.53
AR1660CCC500	AR1660CCC500	03/14/2025	21:15	PP070543.D	10.24	4.53
I.BLK	I.BLK	03/14/2025	22:20	PP070547.D	10.24	4.52
PB167143BL	PB167143BL	03/14/2025	22:36	PP070548.D	10.24	4.52
PB167143BS	PB167143BS	03/14/2025	22:52	PP070549.D	10.24	4.52
AR1660CCC500	AR1660CCC500	03/15/2025	01:51	PP070558.D	10.24	4.52
I.BLK	I.BLK	03/15/2025	02:56	PP070562.D	10.24	4.52
C0018MS	Q1572-06MS	03/15/2025	03:29	PP070564.D	10.24	4.52
C0018MSD	Q1572-06MSD	03/15/2025	03:45	PP070565.D	10.24	4.52
AR1660CCC500	AR1660CCC500	03/15/2025	05:06	PP070568.D	10.24	4.52
I.BLK	I.BLK	03/15/2025	06:11	PP070572.D	10.24	4.52

Analytical Sequence

Client: G Environmental

SDG No.: Q1574

Project: Ave L

Instrument ID: ECD_O

GC Column: ZB-MR2

ID: 0.32 (mm)

Inst. Calib. Date(s): 02/20/2025

02/20/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	02/20/2025	16:28	PO109425.D	8.71	3.69
AR1660ICC1000	AR1660ICC1000	02/20/2025	16:46	PO109426.D	8.71	3.69
AR1660ICC750	AR1660ICC750	02/20/2025	17:04	PO109427.D	8.71	3.69
AR1660ICC500	AR1660ICC500	02/20/2025	17:23	PO109428.D	8.71	3.69
AR1660ICC250	AR1660ICC250	02/20/2025	17:41	PO109429.D	8.71	3.69
AR1660ICC050	AR1660ICC050	02/20/2025	17:59	PO109430.D	8.71	3.69
AR1221ICC500	AR1221ICC500	02/20/2025	18:18	PO109431.D	8.71	3.69
AR1232ICC500	AR1232ICC500	02/20/2025	18:36	PO109432.D	8.71	3.69
AR1242ICC1000	AR1242ICC1000	02/20/2025	18:55	PO109433.D	8.71	3.69
AR1242ICC750	AR1242ICC750	02/20/2025	19:13	PO109434.D	8.71	3.69
AR1242ICC500	AR1242ICC500	02/20/2025	19:31	PO109435.D	8.71	3.69
AR1242ICC250	AR1242ICC250	02/20/2025	19:50	PO109436.D	8.71	3.69
AR1242ICC050	AR1242ICC050	02/20/2025	20:08	PO109437.D	8.71	3.69
AR1248ICC1000	AR1248ICC1000	02/20/2025	20:26	PO109438.D	8.71	3.69
AR1248ICC750	AR1248ICC750	02/20/2025	20:45	PO109439.D	8.71	3.69
AR1248ICC500	AR1248ICC500	02/20/2025	21:03	PO109440.D	8.71	3.69
AR1248ICC250	AR1248ICC250	02/20/2025	21:21	PO109441.D	8.71	3.69
AR1248ICC050	AR1248ICC050	02/20/2025	21:40	PO109442.D	8.71	3.69
AR1254ICC1000	AR1254ICC1000	02/20/2025	21:58	PO109443.D	8.71	3.69
AR1254ICC750	AR1254ICC750	02/20/2025	22:17	PO109444.D	8.71	3.69
AR1254ICC500	AR1254ICC500	02/20/2025	22:35	PO109445.D	8.71	3.69
AR1254ICC250	AR1254ICC250	02/20/2025	22:53	PO109446.D	8.71	3.69
AR1254ICC050	AR1254ICC050	02/20/2025	23:12	PO109447.D	8.71	3.69
AR1262ICC500	AR1262ICC500	02/20/2025	23:30	PO109448.D	8.71	3.69
AR1268ICC1000	AR1268ICC1000	02/20/2025	23:48	PO109449.D	8.71	3.69
AR1268ICC750	AR1268ICC750	02/21/2025	00:07	PO109450.D	8.71	3.69
AR1268ICC500	AR1268ICC500	02/21/2025	00:25	PO109451.D	8.71	3.69
AR1268ICC250	AR1268ICC250	02/21/2025	00:43	PO109452.D	8.71	3.69
AR1268ICC050	AR1268ICC050	02/21/2025	01:02	PO109453.D	8.70	3.69
AR1660CCC500	AR1660CCC500	03/17/2025	09:13	PO109923.D	8.70	3.69
IBLK	IBLK	03/17/2025	10:26	PO109927.D	8.70	3.69
WC1	Q1574-01	03/17/2025	11:02	PO109929.D	8.70	3.69
WC1DL	Q1574-01DL	03/17/2025	11:20	PO109930.D	8.69	3.69
AR1660CCC500	AR1660CCC500	03/17/2025	16:28	PO109935.D	8.70	3.69
IBLK	IBLK	03/17/2025	17:42	PO109939.D	8.70	3.69
IBLK	IBLK	03/11/2025	14:57	PP070418.D	8.88	3.83
AR1660ICC1000	AR1660ICC1000	03/11/2025	15:13	PP070419.D	8.88	3.83
AR1660ICC750	AR1660ICC750	03/11/2025	15:29	PP070420.D	8.88	3.83
AR1660ICC500	AR1660ICC500	03/11/2025	15:46	PP070421.D	8.88	3.83
AR1660ICC250	AR1660ICC250	03/11/2025	16:02	PP070422.D	8.88	3.83
AR1660ICC050	AR1660ICC050	03/11/2025	16:18	PP070423.D	8.88	3.83
AR1221ICC500	AR1221ICC500	03/11/2025	16:34	PP070424.D	8.88	3.83

Analytical Sequence

AR1232ICC1000	AR1232ICC1000	03/11/2025	16:51	PP070425.D	8.88	3.83
AR1232ICC750	AR1232ICC750	03/11/2025	17:07	PP070426.D	8.88	3.83
AR1232ICC500	AR1232ICC500	03/11/2025	17:23	PP070427.D	8.88	3.83
AR1232ICC250	AR1232ICC250	03/11/2025	17:40	PP070428.D	8.88	3.83
AR1232ICC050	AR1232ICC050	03/11/2025	17:56	PP070429.D	8.88	3.83
AR1242ICC1000	AR1242ICC1000	03/11/2025	18:12	PP070430.D	8.88	3.83
AR1242ICC750	AR1242ICC750	03/11/2025	18:28	PP070431.D	8.88	3.83
AR1242ICC500	AR1242ICC500	03/11/2025	18:45	PP070432.D	8.88	3.83
AR1242ICC250	AR1242ICC250	03/11/2025	19:01	PP070433.D	8.88	3.83
AR1242ICC050	AR1242ICC050	03/11/2025	19:17	PP070434.D	8.88	3.83
AR1248ICC1000	AR1248ICC1000	03/11/2025	19:34	PP070435.D	8.88	3.83
AR1248ICC750	AR1248ICC750	03/11/2025	19:50	PP070436.D	8.88	3.83
AR1248ICC500	AR1248ICC500	03/11/2025	20:06	PP070437.D	8.88	3.83
AR1248ICC250	AR1248ICC250	03/11/2025	20:22	PP070438.D	8.88	3.83
AR1248ICC050	AR1248ICC050	03/11/2025	20:39	PP070439.D	8.88	3.83
AR1254ICC1000	AR1254ICC1000	03/11/2025	20:55	PP070440.D	8.88	3.83
AR1254ICC750	AR1254ICC750	03/11/2025	21:11	PP070441.D	8.88	3.83
AR1254ICC500	AR1254ICC500	03/11/2025	21:28	PP070442.D	8.88	3.83
AR1254ICC250	AR1254ICC250	03/11/2025	21:44	PP070443.D	8.88	3.83
AR1254ICC050	AR1254ICC050	03/11/2025	22:00	PP070444.D	8.88	3.83
AR1262ICC500	AR1262ICC500	03/11/2025	22:16	PP070445.D	8.88	3.83
AR1268ICC1000	AR1268ICC1000	03/11/2025	22:33	PP070446.D	8.88	3.83
AR1268ICC750	AR1268ICC750	03/11/2025	22:49	PP070447.D	8.88	3.83
AR1268ICC500	AR1268ICC500	03/11/2025	23:05	PP070448.D	8.88	3.83
AR1268ICC250	AR1268ICC250	03/11/2025	23:22	PP070449.D	8.88	3.83
AR1268ICC050	AR1268ICC050	03/11/2025	23:38	PP070450.D	8.88	3.83
AR1660CCC500	AR1660CCC500	03/14/2025	21:15	PP070543.D	8.87	3.83
I.BLK	I.BLK	03/14/2025	22:20	PP070547.D	8.87	3.83
PB167143BL	PB167143BL	03/14/2025	22:36	PP070548.D	8.87	3.83
PB167143BS	PB167143BS	03/14/2025	22:52	PP070549.D	8.87	3.83
AR1660CCC500	AR1660CCC500	03/15/2025	01:51	PP070558.D	8.87	3.83
I.BLK	I.BLK	03/15/2025	02:56	PP070562.D	8.87	3.83
C0018MS	Q1572-06MS	03/15/2025	03:29	PP070564.D	8.87	3.83
C0018MSD	Q1572-06MSD	03/15/2025	03:45	PP070565.D	8.87	3.83
AR1660CCC500	AR1660CCC500	03/15/2025	05:06	PP070568.D	8.87	3.83
I.BLK	I.BLK	03/15/2025	06:11	PP070572.D	8.87	3.83



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

WC1

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Lab Sample ID: Q1574-01 Date(s) Analyzed: 03/17/2025 03/17/2025

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO109929.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1254	1	5.596	5.546	5.646	479	816	
COLUMN 1	2	5.747	5.697	5.797	1040		
	3	6.151	6.101	6.201	827		
	4	6.381	6.331	6.431	643		
	5	6.8	6.75	6.85	1090		
	1	5.575	5.525	5.625	538		
COLUMN 2	2	5.725	5.675	5.775	1090	884	
	3	6.126	6.076	6.176	909		
	4	6.354	6.304	6.404	713		
	5	6.771	6.721	6.821	1170		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

WC1DL

Contract: GENV01

Lab Code: CHEM Case No.: Q1574 SAS No.: Q1574 SDG NO.: Q1574

Lab Sample ID: Q1574-01DL Date(s) Analyzed: 03/17/2025 03/17/2025

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO109930.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1254	1	5.593	5.543	5.643	480		
	2	5.743	5.693	5.793	962		
	3	6.148	6.098	6.198	945		
	4	6.377	6.327	6.427	617		
	5	6.797	6.747	6.847	1020		
COLUMN 1						805	
	1	5.574	5.524	5.624	553		
	2	5.723	5.673	5.773	1070		
	3	6.124	6.074	6.174	932		
	4	6.352	6.302	6.402	691		
5	6.769	6.719	6.819	1120			
COLUMN 2						873	8.1

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB167143BS

Contract: GENV01

Lab Code: CHEM

Case No.: Q1574

SAS No.: Q1574

SDG NO.: Q1574

Lab Sample ID: PB167143BS

Date(s) Analyzed: 03/14/2025

03/14/2025

Instrument ID (1): ECD_P

Instrument ID (2): ECD_P

GC Column: (1): ZB-MR1 ID: 0.32 (mm)

GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PP070549.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.675	5.625	5.725	146	146	4.03
COLUMN 1	2	5.697	5.647	5.747	157		
	3	5.759	5.709	5.809	146		
	4	5.856	5.806	5.906	141		
	5	6.149	6.099	6.199	142		
	1	4.913	4.863	4.963	156		
COLUMN 2	2	4.932	4.882	4.982	149	152	
	3	5.109	5.059	5.159	153		
	4	5.15	5.1	5.2	152		
	5	5.366	5.316	5.416	150		
Aroclor-1260	1	7.268	7.218	7.318	161	145	0.69
COLUMN 1	2	7.522	7.472	7.572	156		
	3	7.88	7.83	7.93	133		
	4	8.102	8.052	8.152	138		
	5	8.424	8.374	8.474	138		
	1	6.402	6.352	6.452	155		
COLUMN 2	2	6.59	6.54	6.64	152	144	
	3	6.743	6.693	6.793	153		
	4	7.215	7.165	7.265	129		
	5	7.456	7.406	7.506	130		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

C0018MS

Contract: GENV01

Lab Code: CHEM

Case No.: Q1574

SAS No.: Q1574

SDG NO.: Q1574

Lab Sample ID: Q1572-06MS

Date(s) Analyzed: 03/15/2025

03/15/2025

Instrument ID (1): ECD_P

Instrument ID (2): ECD_P

GC Column: (1): ZB-MR1 ID: 0.32 (mm)

GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PP070564.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.675	5.625	5.725	13000	14000	13.33
COLUMN 1	2	5.697	5.647	5.747	17500		
	3	5.762	5.712	5.812	2750		
	4	5.855	5.805	5.905	14100		
	5	6.147	6.097	6.197	24900		
COLUMN 2	1	4.913	4.863	4.963	12500	16000	
	2	4.932	4.882	4.982	15300		
	3	5.109	5.059	5.159	13200		
	4	5.15	5.1	5.2	19500		
	5	5.365	5.315	5.415	20900		
Aroclor-1248	1	5.675	5.625	5.725	19800	18000	11.76
COLUMN 1	2	5.946	5.896	5.996	16400		
	3	6.147	6.097	6.197	18700		
	4	6.547	6.497	6.597	16700		
	5	6.586	6.536	6.636	17900		
COLUMN 2	1	4.913	4.863	4.963	19100	16000	
	2	5.15	5.1	5.2	14000		
	3	5.192	5.142	5.242	15400		
	4	5.365	5.315	5.415	16000		
	5	5.759	5.709	5.809	16400		

IDENTIFICATION SUMMARY FOR MULTICOMPONENT ANALYTES

Aroclor-1260	1	7.268	7.218	7.318	1470	1200	8
	2	7.52	7.47	7.57	1830		
	3	7.878	7.828	7.928	932		
	4	8.099	8.049	8.149	1170		
	5	8.424	8.374	8.474	745		
COLUMN 1							
	1	6.413	6.363	6.463	3280		
	2	6.589	6.539	6.639	896		
	3	6.742	6.692	6.792	1140		
	4	7.215	7.165	7.265	651		
COLUMN 2	5	7.455	7.405	7.505	753	1300	

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

C0018MSD

Contract: GENV01

Lab Code: CHEM

Case No.: Q1574

SAS No.: Q1574

SDG NO.: Q1574

Lab Sample ID: Q1572-06MSD

Date(s) Analyzed: 03/15/2025

03/15/2025

Instrument ID (1): ECD_P

Instrument ID (2): ECD_P

GC Column: (1): ZB-MR1 ID: 0.32 (mm)

GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PP070565.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.675	5.625	5.725	13600	15000	12.5
COLUMN 1	2	5.696	5.646	5.746	18500		
	3	5.763	5.713	5.813	2910		
	4	5.856	5.806	5.906	14900		
	5	6.147	6.097	6.197	26000		
COLUMN 2	1	4.913	4.863	4.963	13100	17000	
	2	4.931	4.881	4.981	16200		
	3	5.109	5.059	5.159	14200		
	4	5.15	5.1	5.2	20600		
	5	5.365	5.315	5.415	22000		
Aroclor-1248	1	5.675	5.625	5.725	20600	19000	11.11
COLUMN 1	2	5.946	5.896	5.996	17000		
	3	6.147	6.097	6.197	19700		
	4	6.548	6.498	6.598	17400		
	5	6.586	6.536	6.636	18500		
COLUMN 2	1	4.913	4.863	4.963	20000	17000	
	2	5.15	5.1	5.2	14700		
	3	5.192	5.142	5.242	16200		
	4	5.365	5.315	5.415	16800		
	5	5.758	5.708	5.808	17100		

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922



QC SAMPLE DATA

Report of Analysis

Client:	G Environmental	Date Collected:	
Project:	Ave L	Date Received:	
Client Sample ID:	PB167143BL	SDG No.:	Q1574
Lab Sample ID:	PB167143BL	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	100 Decanted:
Sample Wt/Vol:	30.01 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP070548.D	1	03/14/25 12:25	03/14/25 22:36	PB167143

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	3.90	U	3.90	17.0	ug/kg
11104-28-2	Aroclor-1221	4.00	U	4.00	17.0	ug/kg
11141-16-5	Aroclor-1232	3.70	U	3.70	17.0	ug/kg
53469-21-9	Aroclor-1242	4.00	U	4.00	17.0	ug/kg
12672-29-6	Aroclor-1248	5.90	U	5.90	17.0	ug/kg
11097-69-1	Aroclor-1254	3.20	U	3.20	17.0	ug/kg
37324-23-5	Aroclor-1262	5.00	U	5.00	17.0	ug/kg
11100-14-4	Aroclor-1268	3.60	U	3.60	17.0	ug/kg
11096-82-5	Aroclor-1260	3.20	U	3.20	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.4		30 (32) - 150 (144)	107%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.2		30 (32) - 150 (175)	106%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
 Data File : PP070548.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2025 22:36
 Operator : YP\AJ
 Sample : PB167143BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB167143BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:59:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:42:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.523	3.826	31678309	21499894	20.367	21.451
2) SA Decachlor...	10.241	8.871	22520411	20574512	21.199	21.030

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
Data File : PP070548.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2025 22:36
Operator : YP\AJ
Sample : PB167143BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB167143BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:59:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm






#1 Tetrachloro-m-xylene


R.T.: 4.523 min
Delta R.T.: 0.000 min
Response: 31678309
Conc: 20.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB167143BL




#1 Tetrachloro-m-xylene

R.T.: 3.826 min
Delta R.T.: -0.003 min
Response: 21499894
Conc: 21.45 ng/ml



#2 Decachlorobiphenyl

R.T.: 10.241 min
Delta R.T.: -0.011 min
Response: 22520411
Conc: 21.20 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.871 min
Delta R.T.: -0.010 min
Response: 20574512
Conc: 21.03 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	02/20/25
Project:	Ave L	Date Received:	02/20/25
Client Sample ID:	PIBLK-PO109425.D	SDG No.:	Q1574
Lab Sample ID:	I.BLK-PO109425.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109425.D	1		02/20/25	PO022025

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	24.1		70 (60) - 130 (140)	121%	SPK: 20
2051-24-3	Decachlorobiphenyl	25.3		70 (60) - 130 (140)	126%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 16:28
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:42:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.697	3.694	239.0E6	126.2E6	25.246	24.105
2) SA Decachlor...	8.755	8.707	217.3E6	81112838	25.266	25.473

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO022025\
Data File : PO109425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Feb 2025 16:28
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 21 04:42:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm






#1 Tetrachloro-m-xylene


R.T.: 3.697 min
Delta R.T.: 0.000 min
Response: 238952889
Conc: 25.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK




#1 Tetrachloro-m-xylene

R.T.: 3.694 min
Delta R.T.: 0.000 min
Response: 126170966
Conc: 24.11 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.755 min
Delta R.T.: -0.002 min
Response: 217333363
Conc: 25.27 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: 0.000 min
Response: 81112838
Conc: 25.47 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	03/17/25
Project:	Ave L	Date Received:	03/17/25
Client Sample ID:	PIBLK-PO109927.D	SDG No.:	Q1574
Lab Sample ID:	I.BLK-PO109927.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000 Units: mL	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	5030		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109927.D	1		03/17/25	PO031725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.0		70 (60) - 130 (140)	100%	SPK: 20
2051-24-3	Decachlorobiphenyl	17.1		70 (60) - 130 (140)	86%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031725\
 Data File : PO109927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2025 10:26
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 01:30:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.693	3.691	189.2E6	106.6E6	19.986	20.362
2) SA Decachlor...	8.745	8.697	147.6E6	55579193	17.153	17.454

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO031725\
Data File : PO109927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2025 10:26
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 01:30:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm






#1 Tetrachloro-m-xylene


R.T.: 3.693 min
Delta R.T.: -0.005 min
Response: 189173180
Conc: 19.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK




#1 Tetrachloro-m-xylene

R.T.: 3.691 min
Delta R.T.: -0.003 min
Response: 106579604
Conc: 20.36 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.745 min
Delta R.T.: -0.012 min
Response: 147551020
Conc: 17.15 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.697 min
Delta R.T.: -0.010 min
Response: 55579193
Conc: 17.45 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	03/17/25
Project:	Ave L	Date Received:	03/17/25
Client Sample ID:	PIBLK-PO109939.D	SDG No.:	Q1574
Lab Sample ID:	I.BLK-PO109939.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO109939.D	1		03/17/25	PO031725

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.4		70 (60) - 130 (140)	102%	SPK: 20
2051-24-3	Decachlorobiphenyl	16.5		70 (60) - 130 (140)	83%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031725\
 Data File : P0109939.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2025 17:42
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 01:35:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 21 04:40:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.693	3.690	192.7E6	107.3E6	20.359	20.501
2) SA Decachlor...	8.746	8.696	151.0E6	52543071	17.560	16.501

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0031725\
Data File : P0109939.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2025 17:42
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 01:35:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0022025.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 21 04:40:23 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm






#1 Tetrachloro-m-xylene


R.T.: 3.693 min
Delta R.T.: -0.005 min
Response: 192701731
Conc: 20.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK




#1 Tetrachloro-m-xylene

R.T.: 3.690 min
Delta R.T.: -0.004 min
Response: 107306369
Conc: 20.50 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.746 min
Delta R.T.: -0.011 min
Response: 151045676
Conc: 17.56 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.696 min
Delta R.T.: -0.010 min
Response: 52543071
Conc: 16.50 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	03/11/25
Project:	Ave L	Date Received:	03/11/25
Client Sample ID:	PIBLK-PP070418.D	SDG No.:	Q1574
Lab Sample ID:	I.BLK-PP070418.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP070418.D	1		03/11/25	pp031125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	22.0		70 (60) - 130 (140)	110%	SPK: 20
2051-24-3	Decachlorobiphenyl	23.1		70 (60) - 130 (140)	116%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070418.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 14:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 03:02:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.526	3.828	34285116	23007566	22.043	22.955
2) SA Decachlor...	10.252	8.880	24539341	22949882	23.099	23.457

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031125\
Data File : PP070418.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2025 14:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 03:02:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm






#1 Tetrachloro-m-xylene


R.T.: 4.526 min
Delta R.T.: 0.002 min
Response: 34285116
Conc: 22.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK




#1 Tetrachloro-m-xylene

R.T.: 3.828 min
Delta R.T.: 0.000 min
Response: 23007566
Conc: 22.96 ng/ml



#2 Decachlorobiphenyl

R.T.: 10.252 min
Delta R.T.: 0.000 min
Response: 24539341
Conc: 23.10 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.880 min
Delta R.T.: -0.001 min
Response: 22949882
Conc: 23.46 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	03/14/25
Project:	Ave L	Date Received:	03/14/25
Client Sample ID:	PIBLK-PP070547.D	SDG No.:	Q1574
Lab Sample ID:	I.BLK-PP070547.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP070547.D	1		03/14/25	pp031425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.5		70 (60) - 130 (140)	97%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.3		70 (60) - 130 (140)	101%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
Data File : PP070547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2025 22:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 23:48:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.521	3.825	30287647	20508990	19.473	20.462
2) SA Decachlor...	10.241	8.871	21532021	19995397	20.268	20.438

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
Data File : PP070547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2025 22:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 23:48:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm






#1 Tetrachloro-m-xylene


R.T.: 4.521 min
Delta R.T.: -0.003 min
Response: 30287647
Conc: 19.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK




#1 Tetrachloro-m-xylene

R.T.: 3.825 min
Delta R.T.: -0.003 min
Response: 20508990
Conc: 20.46 ng/ml



#2 Decachlorobiphenyl

R.T.: 10.241 min
Delta R.T.: -0.011 min
Response: 21532021
Conc: 20.27 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.871 min
Delta R.T.: -0.010 min
Response: 19995397
Conc: 20.44 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	03/15/25
Project:	Ave L	Date Received:	03/15/25
Client Sample ID:	PIBLK-PP070562.D	SDG No.:	Q1574
Lab Sample ID:	I.BLK-PP070562.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP070562.D	1		03/15/25	pp031425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.1		70 (60) - 130 (140)	100%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.2		70 (60) - 130 (140)	101%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
 Data File : PP070562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2025 02:56
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 03:17:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:42:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.524	3.825	31206170	21223856	20.063	21.176
2) SA Decachlor...	10.242	8.871	22186192	19770553	20.884	20.208

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
Data File : PP070562.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2025 02:56
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 03:17:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm






#1 Tetrachloro-m-xylene


R.T.: 4.524 min
Delta R.T.: 0.000 min
Response: 31206170
Conc: 20.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK




#1 Tetrachloro-m-xylene

R.T.: 3.825 min
Delta R.T.: -0.003 min
Response: 21223856
Conc: 21.18 ng/ml



#2 Decachlorobiphenyl

R.T.: 10.242 min
Delta R.T.: -0.010 min
Response: 22186192
Conc: 20.88 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.871 min
Delta R.T.: -0.010 min
Response: 19770553
Conc: 20.21 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	03/15/25
Project:	Ave L	Date Received:	03/15/25
Client Sample ID:	PIBLK-PP070572.D	SDG No.:	Q1574
Lab Sample ID:	I.BLK-PP070572.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP070572.D	1		03/15/25	pp031425

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.097	U	0.097	0.50	ug/L
11104-28-2	Aroclor-1221	0.13	U	0.13	0.50	ug/L
11141-16-5	Aroclor-1232	0.096	U	0.096	0.50	ug/L
53469-21-9	Aroclor-1242	0.12	U	0.12	0.50	ug/L
12672-29-6	Aroclor-1248	0.071	U	0.071	0.50	ug/L
11097-69-1	Aroclor-1254	0.094	U	0.094	0.50	ug/L
11096-82-5	Aroclor-1260	0.081	U	0.081	0.50	ug/L
37324-23-5	Aroclor-1262	0.14	U	0.14	0.50	ug/L
11100-14-4	Aroclor-1268	0.11	U	0.11	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.2		70 (60) - 130 (140)	101%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.5		70 (60) - 130 (140)	102%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
 Data File : PP070572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2025 06:11
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 07:22:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:42:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.523	3.826	31459905	21126630	20.226	21.079
2) SA Decachlor...	10.243	8.871	22297781	20019177	20.989	20.462

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
Data File : PP070572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2025 06:11
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 07:22:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm






#1 Tetrachloro-m-xylene


R.T.: 4.523 min
Delta R.T.: -0.001 min
Response: 31459905
Conc: 20.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK




#1 Tetrachloro-m-xylene

R.T.: 3.826 min
Delta R.T.: -0.003 min
Response: 21126630
Conc: 21.08 ng/ml



#2 Decachlorobiphenyl

R.T.: 10.243 min
Delta R.T.: -0.009 min
Response: 22297781
Conc: 20.99 ng/ml



#2 Decachlorobiphenyl

R.T.: 8.871 min
Delta R.T.: -0.010 min
Response: 20019177
Conc: 20.46 ng/ml

Report of Analysis

Client:	G Environmental	Date Collected:	
Project:	Ave L	Date Received:	
Client Sample ID:	PB167143BS	SDG No.:	Q1574
Lab Sample ID:	PB167143BS	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	100 Decanted:
Sample Wt/Vol:	30.03 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP070549.D	1	03/14/25 12:25	03/14/25 22:52	PB167143

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	152		3.90	17.0	ug/kg
11104-28-2	Aroclor-1221	4.00	U	4.00	17.0	ug/kg
11141-16-5	Aroclor-1232	3.70	U	3.70	17.0	ug/kg
53469-21-9	Aroclor-1242	4.00	U	4.00	17.0	ug/kg
12672-29-6	Aroclor-1248	5.90	U	5.90	17.0	ug/kg
11097-69-1	Aroclor-1254	3.20	U	3.20	17.0	ug/kg
37324-23-5	Aroclor-1262	5.00	U	5.00	17.0	ug/kg
11100-14-4	Aroclor-1268	3.60	U	3.60	17.0	ug/kg
11096-82-5	Aroclor-1260	145		3.20	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.7		30 (32) - 150 (144)	108%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.8		30 (32) - 150 (175)	109%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
 Data File : PP070549.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2025 22:52
 Operator : YP\AJ
 Sample : PB167143BS
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB167143BS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/17/2025
 Supervised By :mohammad ahmed 03/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 01:59:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:42:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.524	3.827	33205418	21721756	21.349	21.672
2) SA Decachlor...	10.242	8.872	23113123	19533518	21.757	19.966
Target Compounds						
3) L1 AR-1016-1	5.675	4.913	22655811	16838908	436.939	468.365
4) L1 AR-1016-2	5.697	4.932	33659019	23292035	470.461	448.211
5) L1 AR-1016-3	5.759	5.109	20019488	13110139	439.622	460.758
6) L1 AR-1016-4	5.856	5.150	16488008	10187202	422.360	454.991
7) L1 AR-1016-5	6.149	5.366	14814899	13366592	427.904	449.768
31) L7 AR-1260-1	7.268	6.402	28474787	23132691	484.775	464.658
32) L7 AR-1260-2	7.522	6.590	38514455	30113094	469.442	455.655
33) L7 AR-1260-3	7.880	6.743	26305571	26221520	400.038	458.439
34) L7 AR-1260-4	8.102	7.215	27028438	19782442	413.641m	386.651
35) L7 AR-1260-5	8.424	7.456	56522478	50192203	413.546	389.736

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
Data File : PP070549.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2025 22:52
Operator : YP\AJ
Sample : PB167143BS
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :

ECD_P

ClientSampleId :

PB167143BS

Manual Integrations



APPROVED

Reviewed By :Yogesh Patel 03/17/2025

Supervised By :mohammad ahmed 03/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 01:59:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Report of Analysis

Client:	G Environmental	Date Collected:	03/12/25
Project:	Ave L	Date Received:	03/14/25
Client Sample ID:	C0018MS	SDG No.:	Q1574
Lab Sample ID:	Q1572-06MS	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	76
Sample Wt/Vol:	30.07	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP070564.D	1	03/14/25 12:25	03/15/25 03:29	PB167143

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	16000	E	5.20	22.3	ug/kg
11104-28-2	Aroclor-1221	5.30	U	5.30	22.3	ug/kg
11141-16-5	Aroclor-1232	4.90	U	4.90	22.3	ug/kg
53469-21-9	Aroclor-1242	5.30	U	5.30	22.3	ug/kg
12672-29-6	Aroclor-1248	18000	E	7.80	22.3	ug/kg
11097-69-1	Aroclor-1254	4.20	U	4.20	22.3	ug/kg
37324-23-5	Aroclor-1262	6.60	U	6.60	22.3	ug/kg
11100-14-4	Aroclor-1268	4.70	U	4.70	22.3	ug/kg
11096-82-5	Aroclor-1260	1300	E	4.20	22.3	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.3		30 (32) - 150 (144)	101%	SPK: 20
2051-24-3	Decachlorobiphenyl	34.0	*	30 (32) - 150 (175)	170%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
 Data File : PP070564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2025 03:29
 Operator : YP\AJ
 Sample : Q1572-06MS
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :

ECD_P

ClientSampleId :

C0018MS

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 03/17/2025

Supervised By :mohammad ahmed 03/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 04:29:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:42:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.523	3.826	31492424	19015081	20.247	18.972
2) SA Decachlor...	10.241	8.872	23103528	33309847	21.748m	34.047m#
Target Compounds						
3) L1 AR-1016-1	5.675	4.913	1545.8E6	1027.1E6	29811.971	28568.783
4) L1 AR-1016-2	5.697	4.932	2869.3E6	1817.2E6	40104.719	34967.922
5) L1 AR-1016-3	5.762	5.109	286.7E6	860.8E6	6295.985	30253.551 #
6) L1 AR-1016-4	5.855	5.150	1261.6E6	998.4E6	32317.971	44590.873 #
7) L1 AR-1016-5	6.147	5.365	1967.9E6	1421.1E6	56839.757m	47818.941
21) L5 AR-1248-1	5.675	4.913	1545.8E6	1027.1E6	45256.716	43752.792
22) L5 AR-1248-2	5.946	5.150	1587.1E6	998.4E6	37389.363	31893.782
23) L5 AR-1248-3	6.147	5.192	1971.4E6	1118.7E6	42719.007m	35266.768
24) L5 AR-1248-4	6.547	5.365	2211.6E6	1421.1E6	38136.398	36464.194
25) L5 AR-1248-5	6.586	5.759	2198.5E6	1430.4E6	40950.306	37557.199
31) L7 AR-1260-1	7.268	6.413	197.7E6	373.7E6	3366.027	7505.712m#
32) L7 AR-1260-2	7.520	6.589	343.1E6	135.4E6	4181.896	2048.218 #
33) L7 AR-1260-3	7.878	6.742	140.0E6	149.3E6	2129.150	2610.828
34) L7 AR-1260-4	8.099	7.215	174.2E6	76097429	2666.075	1487.338 #
35) L7 AR-1260-5	8.424	7.455	232.7E6	221.6E6	1702.840	1720.632

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
Data File : PP070564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2025 03:29
Operator : YP\AJ
Sample : Q1572-06MS
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :

ECD_P

ClientSampleId :

C0018MS

Manual Integrations



APPROVED

Reviewed By :Yogesh Patel 03/17/2025

Supervised By :mohammad ahmed 03/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 04:29:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Report of Analysis

Client:	G Environmental	Date Collected:	03/12/25
Project:	Ave L	Date Received:	03/14/25
Client Sample ID:	C0018MSD	SDG No.:	Q1574
Lab Sample ID:	Q1572-06MSD	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	76
Sample Wt/Vol:	30.09	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PP070565.D	1	03/14/25 12:25	03/15/25 03:45	PB167143

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	17000	E	5.20	22.3	ug/kg
11104-28-2	Aroclor-1221	5.30	U	5.30	22.3	ug/kg
11141-16-5	Aroclor-1232	4.90	U	4.90	22.3	ug/kg
53469-21-9	Aroclor-1242	5.30	U	5.30	22.3	ug/kg
12672-29-6	Aroclor-1248	19000	E	7.80	22.3	ug/kg
11097-69-1	Aroclor-1254	4.20	U	4.20	22.3	ug/kg
37324-23-5	Aroclor-1262	6.60	U	6.60	22.3	ug/kg
11100-14-4	Aroclor-1268	4.70	U	4.70	22.3	ug/kg
11096-82-5	Aroclor-1260	1400	E	4.20	22.3	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.8		30 (32) - 150 (144)	104%	SPK: 20
2051-24-3	Decachlorobiphenyl	33.2	*	30 (32) - 150 (175)	166%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
 Data File : PP070565.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2025 03:45
 Operator : YP\AJ
 Sample : Q1572-06MSD
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :

ECD_P

ClientSampleId :

C0018MSD

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 03/17/2025

Supervised By :mohammad ahmed 03/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 04:30:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 12 02:42:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.523	3.825	32368170	19674300	20.810	19.630
2) SA Decachlor...	10.240	8.872	23727783	32481015	22.335m	33.199m#
Target Compounds						
3) L1 AR-1016-1	5.675	4.913	1606.9E6	1075.9E6	30991.180	29925.656
4) L1 AR-1016-2	5.696	4.931	3025.4E6	1925.6E6	42287.416	37053.656
5) L1 AR-1016-3	5.763	5.109	302.8E6	923.3E6	6649.684	32447.986 #
6) L1 AR-1016-4	5.856	5.150	1331.5E6	1052.2E6	34107.498	46995.572 #
7) L1 AR-1016-5	6.147	5.365	2056.4E6	1493.0E6	59397.064m	50236.412
21) L5 AR-1248-1	5.675	4.913	1606.9E6	1075.9E6	47046.839	45830.829
22) L5 AR-1248-2	5.946	5.150	1650.8E6	1052.2E6	38891.475	33613.751
23) L5 AR-1248-3	6.147	5.192	2074.5E6	1177.9E6	44952.045m	37132.696
24) L5 AR-1248-4	6.548	5.365	2306.8E6	1493.0E6	39778.459	38307.629
25) L5 AR-1248-5	6.586	5.758	2276.2E6	1486.0E6	42397.765	39015.752
31) L7 AR-1260-1	7.268	6.413	204.8E6	389.8E6	3486.616	7830.580m#
32) L7 AR-1260-2	7.519	6.588	361.0E6	140.9E6	4400.150	2132.689 #
33) L7 AR-1260-3	7.878	6.741	145.0E6	156.1E6	2204.937	2728.284
34) L7 AR-1260-4	8.098	7.214	179.0E6	78496874	2739.580	1534.235 #
35) L7 AR-1260-5	8.424	7.455	237.6E6	226.0E6	1738.478	1755.208

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031425\
Data File : PP070565.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2025 03:45
Operator : YP\AJ
Sample : Q1572-06MSD
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :

ECD_P

ClientSampleId :

C0018MSD

Manual Integrations



APPROVED

Reviewed By :Yogesh Patel 03/17/2025

Supervised By :mohammad ahmed 03/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 04:30:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 12 02:42:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm



Manual Integration Report

Sequence:	PO022025	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1242ICC050	PO109437.D	AR-1242-5	yogesh	2/21/2025 8:09:35 AM	Ankita	2/21/2025 9:30:25	Peak Integrated by Software
AR1242ICC050	PO109437.D	AR-1242-5 #2	yogesh	2/21/2025 8:09:35 AM	Ankita	2/21/2025 9:30:25	Peak Integrated by Software
AR1248ICC050	PO109442.D	AR-1248-4	yogesh	2/21/2025 8:09:37 AM	Ankita	2/21/2025 9:30:26	Peak Integrated by Software
AR1248ICC050	PO109442.D	AR-1248-4 #2	yogesh	2/21/2025 8:09:37 AM	Ankita	2/21/2025 9:30:26	Peak Integrated by Software
AR1248ICC050	PO109442.D	AR-1248-5	yogesh	2/21/2025 8:09:37 AM	Ankita	2/21/2025 9:30:26	Peak Integrated by Software
AR1248ICC050	PO109442.D	AR-1248-5 #2	yogesh	2/21/2025 8:09:37 AM	Ankita	2/21/2025 9:30:26	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-1	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-1 #2	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-2	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-2 #2	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-3	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-3 #2	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	AR-1254-4	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:

PO022025

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1254ICC050	PO109447.D	AR-1254-4 #2	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software
AR1254ICC050	PO109447.D	Tetrachloro-m-xylene	yogesh	2/21/2025 8:09:39 AM	Ankita	2/21/2025 9:30:28	Peak Integrated by Software

Manual Integration Report

Sequence:	PO031725	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
Q1574-01	PO109929.D	Decachlorobiphenyl	yogesh	3/18/2025 7:42:53 AM	mohammad	3/19/2025 6:43:23	Peak Integrated by Software
Q1574-01	PO109929.D	Decachlorobiphenyl #2	yogesh	3/18/2025 7:42:53 AM	mohammad	3/19/2025 6:43:23	Peak Integrated by Software
Q1574-01	PO109929.D	Tetrachloro-m-xylene	yogesh	3/18/2025 7:42:53 AM	mohammad	3/19/2025 6:43:23	Peak Integrated by Software
Q1574-01	PO109929.D	Tetrachloro-m-xylene #2	yogesh	3/18/2025 7:42:53 AM	mohammad	3/19/2025 6:43:23	Peak Integrated by Software
Q1574-01DL	PO109930.D	Decachlorobiphenyl	yogesh	3/18/2025 7:42:55 AM	mohammad	3/19/2025 6:43:27	Peak Integrated by Software
Q1574-01DL	PO109930.D	Tetrachloro-m-xylene	yogesh	3/18/2025 7:42:55 AM	mohammad	3/19/2025 6:43:27	Peak Integrated by Software
Q1574-01DL	PO109930.D	Tetrachloro-m-xylene #2	yogesh	3/18/2025 7:42:55 AM	mohammad	3/19/2025 6:43:27	Peak Integrated by Software
AR1254CCC500	PO109953.D	AR-1254-1	yogesh	3/18/2025 7:43:10 AM	mohammad	3/19/2025 6:43:54	Peak Integrated by Software
AR1254CCC500	PO109953.D	AR-1254-1 #2	yogesh	3/18/2025 7:43:10 AM	mohammad	3/19/2025 6:43:54	Peak Integrated by Software
AR1254CCC500	PO109953.D	AR-1254-2	yogesh	3/18/2025 7:43:10 AM	mohammad	3/19/2025 6:43:54	Peak Integrated by Software
AR1254CCC500	PO109953.D	AR-1254-2 #2	yogesh	3/18/2025 7:43:10 AM	mohammad	3/19/2025 6:43:54	Peak Integrated by Software
AR1254CCC500	PO109960.D	AR-1254-1	yogesh	3/18/2025 7:43:16 AM	mohammad	3/19/2025 6:44:04	Peak Integrated by Software
AR1254CCC500	PO109960.D	AR-1254-1 #2	yogesh	3/18/2025 7:43:16 AM	mohammad	3/19/2025 6:44:04	Peak Integrated by Software

Manual Integration Report

Sequence:

PO031725

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1254CCC500	PO109960.D	AR-1254-2	yogesh	3/18/2025 7:43:16 AM	mohammad	3/19/2025 6:44:04	Peak Integrated by Software
AR1254CCC500	PO109960.D	AR-1254-2 #2	yogesh	3/18/2025 7:43:16 AM	mohammad	3/19/2025 6:44:04	Peak Integrated by Software
AR1254CCC500	PO109960.D	Tetrachloro-m-xylene #2	yogesh	3/18/2025 7:43:16 AM	mohammad	3/19/2025 6:44:04	Peak Integrated by Software

Manual Integration Report

Sequence:	pp031125	Instrument	ECD_p
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC250	PP070422.D	Decachlorobiphenyl #2	yogesh	3/12/2025 7:57:06 AM	Ankita	3/12/2025 10:45:04	Peak Integrated by Software
AR1660ICC050	PP070423.D	AR-1016-1	yogesh	3/12/2025 7:57:07 AM	Ankita	3/12/2025 10:45:06	Peak Integrated by Software
AR1660ICC050	PP070423.D	AR-1016-2	yogesh	3/12/2025 7:57:07 AM	Ankita	3/12/2025 10:45:06	Peak Integrated by Software
AR1660ICC050	PP070423.D	AR-1016-3	yogesh	3/12/2025 7:57:07 AM	Ankita	3/12/2025 10:45:06	Peak Integrated by Software
AR1660ICC050	PP070423.D	AR-1016-4	yogesh	3/12/2025 7:57:07 AM	Ankita	3/12/2025 10:45:06	Peak Integrated by Software
AR1660ICC050	PP070423.D	AR-1260-4 #2	yogesh	3/12/2025 7:57:07 AM	Ankita	3/12/2025 10:45:06	Peak Integrated by Software
AR1660ICC050	PP070423.D	AR-1260-5 #2	yogesh	3/12/2025 7:57:07 AM	Ankita	3/12/2025 10:45:06	Peak Integrated by Software
AR1232ICC250	PP070428.D	AR-1232-5	yogesh	3/12/2025 7:57:09 AM	Ankita	3/12/2025 10:45:07	Peak Integrated by Software
AR1232ICC050	PP070429.D	AR-1232-1 #2	yogesh	3/19/2025 6:21:09 AM	mohammad	3/19/2025 6:54:14	Peak Integrated by Software
AR1232ICC050	PP070429.D	AR-1232-2	yogesh	3/19/2025 6:21:09 AM	mohammad	3/19/2025 6:54:14	Peak Integrated by Software
AR1232ICC050	PP070429.D	AR-1232-2 #2	yogesh	3/19/2025 6:21:09 AM	mohammad	3/19/2025 6:54:14	Peak Integrated by Software
AR1232ICC050	PP070429.D	AR-1232-3	yogesh	3/19/2025 6:21:09 AM	mohammad	3/19/2025 6:54:14	Peak Integrated by Software
AR1232ICC050	PP070429.D	AR-1232-4	yogesh	3/19/2025 6:21:09 AM	mohammad	3/19/2025 6:54:14	Peak Integrated by Software

Manual Integration Report

Sequence:	pp031125	Instrument	ECD_p
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1232ICC050	PP070429.D	AR-1232-5	yogesh	3/19/2025 6:21:09 AM	mohammad	3/19/2025 6:54:14	Peak Integrated by Software
AR1232ICC050	PP070429.D	AR-1232-5 #2	yogesh	3/19/2025 6:21:09 AM	mohammad	3/19/2025 6:54:14	Peak Integrated by Software
AR1242ICC050	PP070434.D	AR-1242-1	yogesh	3/12/2025 7:57:12 AM	Ankita	3/12/2025 10:45:18	Peak Integrated by Software
AR1242ICC050	PP070434.D	AR-1242-1 #2	yogesh	3/12/2025 7:57:12 AM	Ankita	3/12/2025 10:45:18	Peak Integrated by Software
AR1242ICC050	PP070434.D	AR-1242-2	yogesh	3/12/2025 7:57:12 AM	Ankita	3/12/2025 10:45:18	Peak Integrated by Software
AR1242ICC050	PP070434.D	AR-1242-2 #2	yogesh	3/12/2025 7:57:12 AM	Ankita	3/12/2025 10:45:18	Peak Integrated by Software
AR1242ICC050	PP070434.D	AR-1242-3	yogesh	3/12/2025 7:57:12 AM	Ankita	3/12/2025 10:45:18	Peak Integrated by Software
AR1242ICC050	PP070434.D	AR-1242-4	yogesh	3/12/2025 7:57:12 AM	Ankita	3/12/2025 10:45:18	Peak Integrated by Software
AR1248ICC050	PP070439.D	AR-1248-1	yogesh	3/12/2025 7:57:14 AM	Ankita	3/12/2025 10:45:19	Peak Integrated by Software
AR1248ICC050	PP070439.D	AR-1248-2	yogesh	3/12/2025 7:57:14 AM	Ankita	3/12/2025 10:45:19	Peak Integrated by Software
AR1268ICC050	PP070450.D	AR-1268-1 #2	yogesh	3/12/2025 7:57:15 AM	Ankita	3/12/2025 10:45:21	Peak Integrated by Software
AR1268ICC050	PP070450.D	AR-1268-2 #2	yogesh	3/12/2025 7:57:15 AM	Ankita	3/12/2025 10:45:21	Peak Integrated by Software
AR1268ICC050	PP070450.D	AR-1268-3 #2	yogesh	3/12/2025 7:57:15 AM	Ankita	3/12/2025 10:45:21	Peak Integrated by Software

Manual Integration Report

Sequence:

pp031125

Instrument

ECD_p

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1242CCC500	PP070465.D	AR-1242-5	yogesh	3/12/2025 7:57:17 AM	Ankita	3/12/2025 10:45:22	Peak Integrated by Software
AR1242CCC500	PP070465.D	AR-1242-5 #2	yogesh	3/12/2025 7:57:17 AM	Ankita	3/12/2025 10:45:22	Peak Integrated by Software

Manual Integration Report

Sequence:	PP031425	Instrument	ECD_p
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PP070500.D	AR-1016-5 #2	yogesh	3/17/2025 8:23:24 AM	mohammad	3/19/2025 6:36:42	Peak Integrated by Software
AR1660CCC500	PP070500.D	AR-1260-1	yogesh	3/17/2025 8:23:24 AM	mohammad	3/19/2025 6:36:42	Peak Integrated by Software
AR1660CCC500	PP070500.D	AR-1260-2	yogesh	3/17/2025 8:23:24 AM	mohammad	3/19/2025 6:36:42	Peak Integrated by Software
AR1660CCC500	PP070515.D	AR-1016-5 #2	yogesh	3/17/2025 8:23:46 AM	mohammad	3/19/2025 6:37:16	Peak Integrated by Software
AR1660CCC500	PP070515.D	AR-1260-1	yogesh	3/17/2025 8:23:46 AM	mohammad	3/19/2025 6:37:16	Peak Integrated by Software
AR1242CCC500	PP070544.D	Decachlorobiphenyl	yogesh	3/17/2025 8:24:05 AM	mohammad	3/19/2025 6:37:57	Peak Integrated by Software
PB167143BS	PP070549.D	AR-1260-4	yogesh	3/17/2025 8:24:07 AM	mohammad	3/19/2025 6:38:01	Peak Integrated by Software
Q1572-06MS	PP070564.D	AR-1016-5	yogesh	3/17/2025 8:24:23 AM	mohammad	3/19/2025 6:38:38	Peak Integrated by Software
Q1572-06MS	PP070564.D	AR-1248-3	yogesh	3/17/2025 8:24:23 AM	mohammad	3/19/2025 6:38:38	Peak Integrated by Software
Q1572-06MS	PP070564.D	AR-1260-1 #2	yogesh	3/17/2025 8:24:23 AM	mohammad	3/19/2025 6:38:38	Peak Integrated by Software
Q1572-06MS	PP070564.D	Decachlorobiphenyl	yogesh	3/17/2025 8:24:23 AM	mohammad	3/19/2025 6:38:38	Peak Integrated by Software
Q1572-06MS	PP070564.D	Decachlorobiphenyl #2	yogesh	3/17/2025 8:24:23 AM	mohammad	3/19/2025 6:38:38	Peak Integrated by Software
Q1572-06MSD	PP070565.D	AR-1016-5	yogesh	3/17/2025 8:24:24 AM	mohammad	3/19/2025 6:38:42	Peak Integrated by Software

Manual Integration Report

Sequence:

PP031425

Instrument

ECD_p

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
Q1572-06MSD	PP070565.D	AR-1221-2	yogesh	3/17/2025 8:24:24 AM	mohammad	3/19/2025 6:38:42	Peak Integrated by Software
Q1572-06MSD	PP070565.D	AR-1248-3	yogesh	3/17/2025 8:24:24 AM	mohammad	3/19/2025 6:38:42	Peak Integrated by Software
Q1572-06MSD	PP070565.D	AR-1260-1 #2	yogesh	3/17/2025 8:24:24 AM	mohammad	3/19/2025 6:38:42	Peak Integrated by Software
Q1572-06MSD	PP070565.D	Decachlorobiphenyl	yogesh	3/17/2025 8:24:24 AM	mohammad	3/19/2025 6:38:42	Peak Integrated by Software
Q1572-06MSD	PP070565.D	Decachlorobiphenyl #2	yogesh	3/17/2025 8:24:24 AM	mohammad	3/19/2025 6:38:42	Peak Integrated by Software

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO022025

Review By	yogesh	Review On	2/21/2025 8:09:53 AM
Supervise By	Ankita	Supervise On	2/21/2025 9:30:37 AM
SubDirectory	PO022025	HP Acquire Method	HP Processing Method PO022025
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO109424.D	20 Feb 2025 16:09	YP/AJ	Ok
2	I.BLK	PO109425.D	20 Feb 2025 16:28	YP/AJ	Ok
3	AR1660ICC1000	PO109426.D	20 Feb 2025 16:46	YP/AJ	Ok
4	AR1660ICC750	PO109427.D	20 Feb 2025 17:04	YP/AJ	Ok
5	AR1660ICC500	PO109428.D	20 Feb 2025 17:23	YP/AJ	Ok
6	AR1660ICC250	PO109429.D	20 Feb 2025 17:41	YP/AJ	Ok
7	AR1660ICC050	PO109430.D	20 Feb 2025 17:59	YP/AJ	Ok
8	AR1221ICC500	PO109431.D	20 Feb 2025 18:18	YP/AJ	Ok
9	AR1232ICC500	PO109432.D	20 Feb 2025 18:36	YP/AJ	Ok
10	AR1242ICC1000	PO109433.D	20 Feb 2025 18:55	YP/AJ	Ok
11	AR1242ICC750	PO109434.D	20 Feb 2025 19:13	YP/AJ	Ok
12	AR1242ICC500	PO109435.D	20 Feb 2025 19:31	YP/AJ	Ok
13	AR1242ICC250	PO109436.D	20 Feb 2025 19:50	YP/AJ	Ok
14	AR1242ICC050	PO109437.D	20 Feb 2025 20:08	YP/AJ	Ok,M
15	AR1248ICC1000	PO109438.D	20 Feb 2025 20:26	YP/AJ	Ok
16	AR1248ICC750	PO109439.D	20 Feb 2025 20:45	YP/AJ	Ok
17	AR1248ICC500	PO109440.D	20 Feb 2025 21:03	YP/AJ	Ok
18	AR1248ICC250	PO109441.D	20 Feb 2025 21:21	YP/AJ	Ok
19	AR1248ICC050	PO109442.D	20 Feb 2025 21:40	YP/AJ	Ok,M
20	AR1254ICC1000	PO109443.D	20 Feb 2025 21:58	YP/AJ	Ok
21	AR1254ICC750	PO109444.D	20 Feb 2025 22:17	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO022025

Review By	yogesh	Review On	2/21/2025 8:09:53 AM
Supervise By	Ankita	Supervise On	2/21/2025 9:30:37 AM
SubDirectory	PO022025	HP Acquire Method	HP Processing Method PO022025
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	AR1254ICC500	PO109445.D	20 Feb 2025 22:35	YP/AJ	Ok
23	AR1254ICC250	PO109446.D	20 Feb 2025 22:53	YP/AJ	Ok
24	AR1254ICC050	PO109447.D	20 Feb 2025 23:12	YP/AJ	Ok,M
25	AR1262ICC500	PO109448.D	20 Feb 2025 23:30	YP/AJ	Ok
26	AR1268ICC1000	PO109449.D	20 Feb 2025 23:48	YP/AJ	Ok
27	AR1268ICC750	PO109450.D	21 Feb 2025 00:07	YP/AJ	Ok
28	AR1268ICC500	PO109451.D	21 Feb 2025 00:25	YP/AJ	Ok
29	AR1268ICC250	PO109452.D	21 Feb 2025 00:43	YP/AJ	Ok
30	AR1268ICC050	PO109453.D	21 Feb 2025 01:02	YP/AJ	Ok
31	PO022025ICV500	PO109454.D	21 Feb 2025 01:20	YP/AJ	Ok
32	AR1242ICV500	PO109455.D	21 Feb 2025 01:38	YP/AJ	Ok
33	AR1248ICV500	PO109456.D	21 Feb 2025 01:57	YP/AJ	Ok
34	AR1254ICV500	PO109457.D	21 Feb 2025 02:15	YP/AJ	Ok
35	AR1268ICV500	PO109458.D	21 Feb 2025 02:34	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031725

Review By	yogesh	Review On	3/17/2025 11:37:36 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:44:23 AM
SubDirectory	PO031725	HP Acquire Method	HP Processing Method
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO109922.D	17 Mar 2025 08:55	YP/AJ	Ok
2	AR1660CCC500	PO109923.D	17 Mar 2025 09:13	YP/AJ	Ok
3	AR1242CCC500	PO109924.D	17 Mar 2025 09:31	YP/AJ	Ok
4	AR1248CCC500	PO109925.D	17 Mar 2025 09:49	YP/AJ	Ok
5	AR1254CCC500	PO109926.D	17 Mar 2025 10:07	YP/AJ	Ok
6	I.BLK	PO109927.D	17 Mar 2025 10:26	YP/AJ	Ok
7	PB167143BL	PO109928.D	17 Mar 2025 10:44	YP/AJ	Not Ok
8	Q1574-01	PO109929.D	17 Mar 2025 11:02	YP/AJ	Dilution
9	Q1574-01DL	PO109930.D	17 Mar 2025 11:20	YP/AJ	Ok,M
10	Q1572-10DL	PO109931.D	17 Mar 2025 13:08	YP/AJ	Ok
11	Q1572-11DL	PO109932.D	17 Mar 2025 13:27	YP/AJ	Ok,M
12	Q1572-12DL	PO109933.D	17 Mar 2025 13:45	YP/AJ	Dilution
13	Q1572-12DL2	PO109934.D	17 Mar 2025 14:03	YP/AJ	Not Ok
14	AR1660CCC500	PO109935.D	17 Mar 2025 16:28	YP/AJ	Ok
15	AR1242CCC500	PO109936.D	17 Mar 2025 16:47	YP/AJ	Ok
16	AR1248CCC500	PO109937.D	17 Mar 2025 17:06	YP/AJ	Ok
17	AR1254CCC500	PO109938.D	17 Mar 2025 17:24	YP/AJ	Ok
18	I.BLK	PO109939.D	17 Mar 2025 17:42	YP/AJ	Ok
19	PB167173BL	PO109940.D	17 Mar 2025 18:01	YP/AJ	Ok
20	PB167173BS	PO109941.D	17 Mar 2025 18:19	YP/AJ	Ok
21	Q1589-01	PO109942.D	17 Mar 2025 18:38	YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031725

Review By	yogesh	Review On	3/17/2025 11:37:36 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:44:23 AM
SubDirectory	PO031725	HP Acquire Method	HP Processing Method
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	Q1589-02	PO109943.D	17 Mar 2025 18:55	YP/AJ	Ok
23	Q1589-03	PO109944.D	17 Mar 2025 19:13	YP/AJ	Ok,M
24	Q1589-04	PO109945.D	17 Mar 2025 19:32	YP/AJ	Ok
25	Q1589-05	PO109946.D	17 Mar 2025 19:50	YP/AJ	Ok,M
26	Q1589-06	PO109947.D	17 Mar 2025 20:08	YP/AJ	Ok
27	Q1589-07	PO109948.D	17 Mar 2025 20:27	YP/AJ	Ok,M
28	Q1589-08	PO109949.D	17 Mar 2025 20:45	YP/AJ	Ok,M
29	AR1660CCC500	PO109950.D	17 Mar 2025 22:43	YP/AJ	Ok
30	AR1242CCC500	PO109951.D	17 Mar 2025 23:38	YP/AJ	Ok
31	AR1248CCC500	PO109952.D	17 Mar 2025 23:57	YP/AJ	Ok
32	AR1254CCC500	PO109953.D	18 Mar 2025 00:15	YP/AJ	Ok,M
33	I.BLK	PO109954.D	18 Mar 2025 00:33	YP/AJ	Ok
34	Q1589-09	PO109955.D	18 Mar 2025 00:52	YP/AJ	Ok,M
35	Q1589-10	PO109956.D	18 Mar 2025 01:10	YP/AJ	Ok,M
36	AR1660CCC500	PO109957.D	18 Mar 2025 03:07	YP/AJ	Ok
37	AR1242CCC500	PO109958.D	18 Mar 2025 04:03	YP/AJ	Ok
38	AR1248CCC500	PO109959.D	18 Mar 2025 04:21	YP/AJ	Ok
39	AR1254CCC500	PO109960.D	18 Mar 2025 04:39	YP/AJ	Ok,M
40	I.BLK	PO109961.D	18 Mar 2025 04:58	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031125

Review By	yogesh	Review On	3/12/2025 7:57:33 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:54:29 AM
SubDirectory	PP031125	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PP070417.D	11 Mar 2025 14:41	YP\AJ	Ok
2	I.BLK	PP070418.D	11 Mar 2025 14:57	YP\AJ	Ok
3	AR1660ICC1000	PP070419.D	11 Mar 2025 15:13	YP\AJ	Ok
4	AR1660ICC750	PP070420.D	11 Mar 2025 15:29	YP\AJ	Ok
5	AR1660ICC500	PP070421.D	11 Mar 2025 15:46	YP\AJ	Ok
6	AR1660ICC250	PP070422.D	11 Mar 2025 16:02	YP\AJ	Ok,M
7	AR1660ICC050	PP070423.D	11 Mar 2025 16:18	YP\AJ	Ok,M
8	AR1221ICC500	PP070424.D	11 Mar 2025 16:34	YP\AJ	Ok
9	AR1232ICC1000	PP070425.D	11 Mar 2025 16:51	YP\AJ	Ok
10	AR1232ICC750	PP070426.D	11 Mar 2025 17:07	YP\AJ	Ok
11	AR1232ICC500	PP070427.D	11 Mar 2025 17:23	YP\AJ	Ok
12	AR1232ICC250	PP070428.D	11 Mar 2025 17:40	YP\AJ	Ok,M
13	AR1232ICC050	PP070429.D	11 Mar 2025 17:56	YP\AJ	Ok,M
14	AR1242ICC1000	PP070430.D	11 Mar 2025 18:12	YP\AJ	Ok
15	AR1242ICC750	PP070431.D	11 Mar 2025 18:28	YP\AJ	Ok
16	AR1242ICC500	PP070432.D	11 Mar 2025 18:45	YP\AJ	Ok
17	AR1242ICC250	PP070433.D	11 Mar 2025 19:01	YP\AJ	Ok
18	AR1242ICC050	PP070434.D	11 Mar 2025 19:17	YP\AJ	Ok,M
19	AR1248ICC1000	PP070435.D	11 Mar 2025 19:34	YP\AJ	Ok
20	AR1248ICC750	PP070436.D	11 Mar 2025 19:50	YP\AJ	Ok
21	AR1248ICC500	PP070437.D	11 Mar 2025 20:06	YP\AJ	Ok

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031125

Review By	yogesh	Review On	3/12/2025 7:57:33 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:54:29 AM
SubDirectory	PP031125	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	AR1248ICC250	PP070438.D	11 Mar 2025 20:22	YPIAJ	Ok
23	AR1248ICC050	PP070439.D	11 Mar 2025 20:39	YPIAJ	Ok,M
24	AR1254ICC1000	PP070440.D	11 Mar 2025 20:55	YPIAJ	Ok
25	AR1254ICC750	PP070441.D	11 Mar 2025 21:11	YPIAJ	Ok
26	AR1254ICC500	PP070442.D	11 Mar 2025 21:28	YPIAJ	Ok
27	AR1254ICC250	PP070443.D	11 Mar 2025 21:44	YPIAJ	Ok
28	AR1254ICC050	PP070444.D	11 Mar 2025 22:00	YPIAJ	Ok
29	AR1262ICC500	PP070445.D	11 Mar 2025 22:16	YPIAJ	Ok
30	AR1268ICC1000	PP070446.D	11 Mar 2025 22:33	YPIAJ	Ok
31	AR1268ICC750	PP070447.D	11 Mar 2025 22:49	YPIAJ	Ok
32	AR1268ICC500	PP070448.D	11 Mar 2025 23:05	YPIAJ	Ok
33	AR1268ICC250	PP070449.D	11 Mar 2025 23:22	YPIAJ	Ok
34	AR1268ICC050	PP070450.D	11 Mar 2025 23:38	YPIAJ	Ok,M
35	PP031125ICV500	PP070451.D	11 Mar 2025 23:54	YPIAJ	Ok
36	AR1232ICV500	PP070452.D	12 Mar 2025 00:10	YPIAJ	Ok
37	AR1242ICV500	PP070453.D	12 Mar 2025 00:27	YPIAJ	Ok
38	AR1248ICV500	PP070454.D	12 Mar 2025 00:43	YPIAJ	Ok
39	AR1254ICV500	PP070455.D	12 Mar 2025 00:59	YPIAJ	Ok
40	AR1268ICV500	PP070456.D	12 Mar 2025 01:16	YPIAJ	Ok
41	AR1660CCC500	PP070457.D	12 Mar 2025 01:32	YPIAJ	Ok
42	AR1232CCC500	PP070458.D	12 Mar 2025 01:48	YPIAJ	Ok
43	AR1242CCC500	PP070459.D	12 Mar 2025 02:04	YPIAJ	Ok
44	I.BLK	PP070460.D	12 Mar 2025 02:21	YPIAJ	Ok

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031125

Review By	yogesh	Review On	3/12/2025 7:57:33 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:54:29 AM
SubDirectory	PP031125	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

45	PB167066BL	PP070461.D	12 Mar 2025 02:37	YP\AJ	Ok
46	Q1502-15	PP070462.D	12 Mar 2025 02:53	YP\AJ	Ok
47	AR1660CCC500	PP070463.D	12 Mar 2025 03:09	YP\AJ	Ok
48	AR1232CCC500	PP070464.D	12 Mar 2025 03:26	YP\AJ	Ok
49	AR1242CCC500	PP070465.D	12 Mar 2025 03:42	YP\AJ	Ok,M
50	I.BLK	PP070466.D	12 Mar 2025 03:58	YP\AJ	Ok

M : Manual Integration

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031425

Review By	yogesh	Review On	3/17/2025 8:24:56 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:39:12 AM
SubDirectory	PP031425	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PP070499.D	14 Mar 2025 07:42	YP\AJ	Ok
2	AR1660CCC500	PP070500.D	14 Mar 2025 07:58	YP\AJ	Ok,M
3	AR1242CCC500	PP070501.D	14 Mar 2025 08:14	YP\AJ	Ok
4	AR1248CCC500	PP070502.D	14 Mar 2025 08:31	YP\AJ	Ok
5	AR1254CCC500	PP070503.D	14 Mar 2025 08:47	YP\AJ	Ok
6	I.BLK	PP070504.D	14 Mar 2025 09:03	YP\AJ	Ok
7	PB167130BL	PP070505.D	14 Mar 2025 09:21	YP\AJ	Ok
8	PB167130BS	PP070506.D	14 Mar 2025 09:37	YP\AJ	Ok
9	Q1562-01	PP070507.D	14 Mar 2025 09:53	YP\AJ	Ok,M
10	Q1562-02	PP070508.D	14 Mar 2025 10:09	YP\AJ	Ok,M
11	Q1562-03	PP070509.D	14 Mar 2025 10:26	YP\AJ	Ok,M
12	Q1562-04	PP070510.D	14 Mar 2025 10:42	YP\AJ	Ok,M
13	Q1562-05	PP070511.D	14 Mar 2025 10:58	YP\AJ	Ok,M
14	Q1562-06	PP070512.D	14 Mar 2025 11:14	YP\AJ	Ok,M
15	Q1562-07	PP070513.D	14 Mar 2025 11:31	YP\AJ	Ok,M
16	Q1562-08	PP070514.D	14 Mar 2025 11:47	YP\AJ	Ok,M
17	AR1660CCC500	PP070515.D	14 Mar 2025 12:36	YP\AJ	Ok,M
18	AR1242CCC500	PP070516.D	14 Mar 2025 12:52	YP\AJ	Ok
19	AR1248CCC500	PP070517.D	14 Mar 2025 13:08	YP\AJ	Ok
20	AR1254CCC500	PP070518.D	14 Mar 2025 13:24	YP\AJ	Ok
21	I.BLK	PP070519.D	14 Mar 2025 13:41	YP\AJ	Ok

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031425

Review By	yogesh	Review On	3/17/2025 8:24:56 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:39:12 AM
SubDirectory	PP031425	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	Q1564-04	PP070520.D	14 Mar 2025 13:57	YP\AJ	Ok,M
23	Q1564-05	PP070521.D	14 Mar 2025 14:13	YP\AJ	Ok,M
24	Q1564-06	PP070522.D	14 Mar 2025 14:29	YP\AJ	Ok,M
25	Q1564-01	PP070523.D	14 Mar 2025 14:45	YP\AJ	Ok,M
26	Q1564-02	PP070524.D	14 Mar 2025 15:02	YP\AJ	Ok,M
27	Q1564-03	PP070525.D	14 Mar 2025 15:18	YP\AJ	Ok,M
28	PB167139BL	PP070526.D	14 Mar 2025 15:34	YP\AJ	Ok
29	PB167139BS	PP070527.D	14 Mar 2025 15:50	YP\AJ	Ok
30	PB167139BSD	PP070528.D	14 Mar 2025 16:06	YP\AJ	Ok
31	AR1660CCC500	PP070529.D	14 Mar 2025 16:55	YP\AJ	Ok
32	AR1242CCC500	PP070530.D	14 Mar 2025 17:11	YP\AJ	Ok
33	AR1248CCC500	PP070531.D	14 Mar 2025 17:28	YP\AJ	Ok
34	AR1254CCC500	PP070532.D	14 Mar 2025 17:44	YP\AJ	Ok
35	I.BLK	PP070533.D	14 Mar 2025 18:00	YP\AJ	Ok
36	Q1553-03	PP070534.D	14 Mar 2025 18:16	YP\AJ	Ok,M
37	Q1563-01	PP070535.D	14 Mar 2025 18:33	YP\AJ	Ok
38	Q1563-02	PP070536.D	14 Mar 2025 18:49	YP\AJ	Ok,M
39	PB167136BL	PP070537.D	14 Mar 2025 19:05	YP\AJ	Ok
40	PB167136BS	PP070538.D	14 Mar 2025 19:21	YP\AJ	Ok
41	Q1566-01	PP070539.D	14 Mar 2025 19:38	YP\AJ	Ok
42	Q1568-01	PP070540.D	14 Mar 2025 19:54	YP\AJ	Ok
43	Q1568-01MS	PP070541.D	14 Mar 2025 20:10	YP\AJ	Ok
44	Q1568-01MSD	PP070542.D	14 Mar 2025 20:26	YP\AJ	Ok,M

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031425

Review By	yogesh	Review On	3/17/2025 8:24:56 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:39:12 AM
SubDirectory	PP031425	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

45	AR1660CCC500	PP070543.D	14 Mar 2025 21:15	YPIAJ	Ok
46	AR1242CCC500	PP070544.D	14 Mar 2025 21:31	YPIAJ	Ok,M
47	AR1248CCC500	PP070545.D	14 Mar 2025 21:48	YPIAJ	Ok
48	AR1254CCC500	PP070546.D	14 Mar 2025 22:04	YPIAJ	Ok
49	I.BLK	PP070547.D	14 Mar 2025 22:20	YPIAJ	Ok
50	PB167143BL	PP070548.D	14 Mar 2025 22:36	YPIAJ	Ok
51	PB167143BS	PP070549.D	14 Mar 2025 22:52	YPIAJ	Ok,M
52	Q1569-01	PP070550.D	14 Mar 2025 23:09	YPIAJ	Ok
53	Q1569-04	PP070551.D	14 Mar 2025 23:25	YPIAJ	Ok,M
54	Q1572-01	PP070552.D	14 Mar 2025 23:41	YPIAJ	Dilution
55	Q1572-02	PP070553.D	14 Mar 2025 23:57	YPIAJ	Dilution
56	Q1572-03	PP070554.D	15 Mar 2025 00:14	YPIAJ	Dilution
57	Q1572-04	PP070555.D	15 Mar 2025 00:30	YPIAJ	Dilution
58	Q1572-05	PP070556.D	15 Mar 2025 00:46	YPIAJ	Dilution
59	Q1572-07	PP070557.D	15 Mar 2025 01:02	YPIAJ	Dilution
60	AR1660CCC500	PP070558.D	15 Mar 2025 01:51	YPIAJ	Ok
61	AR1242CCC500	PP070559.D	15 Mar 2025 02:07	YPIAJ	Ok
62	AR1248CCC500	PP070560.D	15 Mar 2025 02:24	YPIAJ	Ok
63	AR1254CCC500	PP070561.D	15 Mar 2025 02:40	YPIAJ	Ok
64	I.BLK	PP070562.D	15 Mar 2025 02:56	YPIAJ	Ok
65	Q1572-06	PP070563.D	15 Mar 2025 03:12	YPIAJ	Dilution
66	Q1572-06MS	PP070564.D	15 Mar 2025 03:29	YPIAJ	Ok,M
67	Q1572-06MSD	PP070565.D	15 Mar 2025 03:45	YPIAJ	Ok,M

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031425

Review By	yogesh	Review On	3/17/2025 8:24:56 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:39:12 AM
SubDirectory	PP031425	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

68	Q1572-08	PP070566.D	15 Mar 2025 04:01	YP\AJ	Dilution
69	Q1572-09	PP070567.D	15 Mar 2025 04:17	YP\AJ	Dilution
70	AR1660CCC500	PP070568.D	15 Mar 2025 05:06	YP\AJ	Ok
71	AR1242CCC500	PP070569.D	15 Mar 2025 05:22	YP\AJ	Ok
72	AR1248CCC500	PP070570.D	15 Mar 2025 05:39	YP\AJ	Ok
73	AR1254CCC500	PP070571.D	15 Mar 2025 05:55	YP\AJ	Ok
74	I.BLK	PP070572.D	15 Mar 2025 06:11	YP\AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO022025

Review By	yogesh	Review On	2/21/2025 8:09:53 AM				
Supervise By	Ankita	Supervise On	2/21/2025 9:30:37 AM				
SubDirectory	PO022025	HP Acquire Method	HP Processing Method		PO022025		
STD. NAME		STD REF.#					
Tune/Reschk		PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775					
Initial Calibration Stds							
CCC							
Internal Standard/PEM							
ICV/I.BLK							
Surrogate Standard							
MS/MSD Standard							
LCS Standard							

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO109424.D	20 Feb 2025 16:09		YP/AJ	Ok
2	I.BLK	I.BLK	PO109425.D	20 Feb 2025 16:28		YP/AJ	Ok
3	AR1660ICC1000	AR1660ICC1000	PO109426.D	20 Feb 2025 16:46		YP/AJ	Ok
4	AR1660ICC750	AR1660ICC750	PO109427.D	20 Feb 2025 17:04		YP/AJ	Ok
5	AR1660ICC500	AR1660ICC500	PO109428.D	20 Feb 2025 17:23		YP/AJ	Ok
6	AR1660ICC250	AR1660ICC250	PO109429.D	20 Feb 2025 17:41		YP/AJ	Ok
7	AR1660ICC050	AR1660ICC050	PO109430.D	20 Feb 2025 17:59		YP/AJ	Ok
8	AR1221ICC500	AR1221ICC500	PO109431.D	20 Feb 2025 18:18		YP/AJ	Ok
9	AR1232ICC500	AR1232ICC500	PO109432.D	20 Feb 2025 18:36		YP/AJ	Ok
10	AR1242ICC1000	AR1242ICC1000	PO109433.D	20 Feb 2025 18:55		YP/AJ	Ok
11	AR1242ICC750	AR1242ICC750	PO109434.D	20 Feb 2025 19:13		YP/AJ	Ok
12	AR1242ICC500	AR1242ICC500	PO109435.D	20 Feb 2025 19:31		YP/AJ	Ok
13	AR1242ICC250	AR1242ICC250	PO109436.D	20 Feb 2025 19:50		YP/AJ	Ok
14	AR1242ICC050	AR1242ICC050	PO109437.D	20 Feb 2025 20:08		YP/AJ	Ok,M
15	AR1248ICC1000	AR1248ICC1000	PO109438.D	20 Feb 2025 20:26		YP/AJ	Ok
16	AR1248ICC750	AR1248ICC750	PO109439.D	20 Feb 2025 20:45		YP/AJ	Ok
17	AR1248ICC500	AR1248ICC500	PO109440.D	20 Feb 2025 21:03		YP/AJ	Ok
18	AR1248ICC250	AR1248ICC250	PO109441.D	20 Feb 2025 21:21		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO022025

Review By	yogesh	Review On	2/21/2025 8:09:53 AM
Supervise By	Ankita	Supervise On	2/21/2025 9:30:37 AM
SubDirectory	PO022025	HP Acquire Method	HP Processing Method PO022025
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248ICC050	AR1248ICC050	PO109442.D	20 Feb 2025 21:40		YP/AJ	Ok,M
20	AR1254ICC1000	AR1254ICC1000	PO109443.D	20 Feb 2025 21:58		YP/AJ	Ok
21	AR1254ICC750	AR1254ICC750	PO109444.D	20 Feb 2025 22:17		YP/AJ	Ok
22	AR1254ICC500	AR1254ICC500	PO109445.D	20 Feb 2025 22:35		YP/AJ	Ok
23	AR1254ICC250	AR1254ICC250	PO109446.D	20 Feb 2025 22:53		YP/AJ	Ok
24	AR1254ICC050	AR1254ICC050	PO109447.D	20 Feb 2025 23:12		YP/AJ	Ok,M
25	AR1262ICC500	AR1262ICC500	PO109448.D	20 Feb 2025 23:30		YP/AJ	Ok
26	AR1268ICC1000	AR1268ICC1000	PO109449.D	20 Feb 2025 23:48		YP/AJ	Ok
27	AR1268ICC750	AR1268ICC750	PO109450.D	21 Feb 2025 00:07		YP/AJ	Ok
28	AR1268ICC500	AR1268ICC500	PO109451.D	21 Feb 2025 00:25		YP/AJ	Ok
29	AR1268ICC250	AR1268ICC250	PO109452.D	21 Feb 2025 00:43		YP/AJ	Ok
30	AR1268ICC050	AR1268ICC050	PO109453.D	21 Feb 2025 01:02		YP/AJ	Ok
31	PO022025ICV500	ICVPO022025	PO109454.D	21 Feb 2025 01:20		YP/AJ	Ok
32	AR1242ICV500	ICVPO022025AR1242	PO109455.D	21 Feb 2025 01:38		YP/AJ	Ok
33	AR1248ICV500	ICVPO022025AR1248	PO109456.D	21 Feb 2025 01:57		YP/AJ	Ok
34	AR1254ICV500	ICVPO022025AR1254	PO109457.D	21 Feb 2025 02:15		YP/AJ	Ok
35	AR1268ICV500	ICVPO022025AR1268	PO109458.D	21 Feb 2025 02:34		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031725

Review By	yogesh	Review On	3/17/2025 11:37:36 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:44:23 AM
SubDirectory	PO031725	HP Acquire Method	HP Processing Method

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773
Internal Standard/PEM	
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO109922.D	17 Mar 2025 08:55		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO109923.D	17 Mar 2025 09:13		YP/AJ	Ok
3	AR1242CCC500	AR1242CCC500	PO109924.D	17 Mar 2025 09:31		YP/AJ	Ok
4	AR1248CCC500	AR1248CCC500	PO109925.D	17 Mar 2025 09:49		YP/AJ	Ok
5	AR1254CCC500	AR1254CCC500	PO109926.D	17 Mar 2025 10:07		YP/AJ	Ok
6	I.BLK	I.BLK	PO109927.D	17 Mar 2025 10:26		YP/AJ	Ok
7	PB167143BL	PB167143BL	PO109928.D	17 Mar 2025 10:44		YP/AJ	Not Ok
8	Q1574-01	WC1	PO109929.D	17 Mar 2025 11:02	AR1254, Need 5X Dilution	YP/AJ	Dilution
9	Q1574-01DL	WC1DL	PO109930.D	17 Mar 2025 11:20	AR1254 hit	YP/AJ	Ok,M
10	Q1572-10DL	C0022DL	PO109931.D	17 Mar 2025 13:08	AR1248 Hit	YP/AJ	Ok
11	Q1572-11DL	C0023DL	PO109932.D	17 Mar 2025 13:27	AR1248 Hit, DCB high in both column,	YP/AJ	Ok,M
12	Q1572-12DL	C0024DL	PO109933.D	17 Mar 2025 13:45	AR1248 + AR1260 Hit, Need further 10x Dilution	YP/AJ	Dilution
13	Q1572-12DL2	C0024DL2	PO109934.D	17 Mar 2025 14:03	AR1248 + AR1260 Hit, Need more Dilution	YP/AJ	Not Ok
14	AR1660CCC500	AR1660CCC500	PO109935.D	17 Mar 2025 16:28		YP/AJ	Ok
15	AR1242CCC500	AR1242CCC500	PO109936.D	17 Mar 2025 16:47		YP/AJ	Ok
16	AR1248CCC500	AR1248CCC500	PO109937.D	17 Mar 2025 17:06		YP/AJ	Ok
17	AR1254CCC500	AR1254CCC500	PO109938.D	17 Mar 2025 17:24		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031725

Review By	yogesh	Review On	3/17/2025 11:37:36 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:44:23 AM
SubDirectory	PO031725	HP Acquire Method	HP Processing Method
STD. NAME	STD REF.#		
Tune/Reschk	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775 PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773 PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Initial Calibration Stds			
CCC			
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

18	I.BLK	I.BLK	PO109939.D	17 Mar 2025 17:42		YP/AJ	Ok
19	PB167173BL	PB167173BL	PO109940.D	17 Mar 2025 18:01		YP/AJ	Ok
20	PB167173BS	PB167173BS	PO109941.D	17 Mar 2025 18:19		YP/AJ	Ok
21	Q1589-01	KMH809G-1-1	PO109942.D	17 Mar 2025 18:38		YP/AJ	Ok,M
22	Q1589-02	KMH809G-1-2	PO109943.D	17 Mar 2025 18:55		YP/AJ	Ok
23	Q1589-03	KMH809G-2-1	PO109944.D	17 Mar 2025 19:13		YP/AJ	Ok,M
24	Q1589-04	KMH809G-2-2	PO109945.D	17 Mar 2025 19:32		YP/AJ	Ok
25	Q1589-05	0036-1-1	PO109946.D	17 Mar 2025 19:50		YP/AJ	Ok,M
26	Q1589-06	0036-1-2	PO109947.D	17 Mar 2025 20:08		YP/AJ	Ok
27	Q1589-07	9040-1-1	PO109948.D	17 Mar 2025 20:27		YP/AJ	Ok,M
28	Q1589-08	9040-1-2	PO109949.D	17 Mar 2025 20:45		YP/AJ	Ok,M
29	AR1660CCC500	AR1660CCC500	PO109950.D	17 Mar 2025 22:43		YP/AJ	Ok
30	AR1242CCC500	AR1242CCC500	PO109951.D	17 Mar 2025 23:38		YP/AJ	Ok
31	AR1248CCC500	AR1248CCC500	PO109952.D	17 Mar 2025 23:57		YP/AJ	Ok
32	AR1254CCC500	AR1254CCC500	PO109953.D	18 Mar 2025 00:15		YP/AJ	Ok,M
33	I.BLK	I.BLK	PO109954.D	18 Mar 2025 00:33		YP/AJ	Ok
34	Q1589-09	HIH340T-1-1	PO109955.D	18 Mar 2025 00:52	AR1254 Hit	YP/AJ	Ok,M
35	Q1589-10	HIH340T-1-2	PO109956.D	18 Mar 2025 01:10	AR1254 Hit	YP/AJ	Ok,M
36	AR1660CCC500	AR1660CCC500	PO109957.D	18 Mar 2025 03:07		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO031725

Review By	yogesh	Review On	3/17/2025 11:37:36 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:44:23 AM
SubDirectory	PO031725	HP Acquire Method	HP Processing Method
STD. NAME	STD REF.#		
Tune/Reschk	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
Initial Calibration Stds			
CCC			
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		

37	AR1242CCC500	AR1242CCC500	PO109958.D	18 Mar 2025 04:03		YP/AJ	Ok
38	AR1248CCC500	AR1248CCC500	PO109959.D	18 Mar 2025 04:21		YP/AJ	Ok
39	AR1254CCC500	AR1254CCC500	PO109960.D	18 Mar 2025 04:39		YP/AJ	Ok,M
40	I.BLK	I.BLK	PO109961.D	18 Mar 2025 04:58		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031125

Review By	yogesh	Review On	3/12/2025 7:57:33 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:54:29 AM
SubDirectory	PP031125	HP Acquire Method	HP Processing Method PP031125

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773
Internal Standard/PEM	
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PP070417.D	11 Mar 2025 14:41		YPIAJ	Ok
2	I.BLK	I.BLK	PP070418.D	11 Mar 2025 14:57		YPIAJ	Ok
3	AR1660ICC1000	AR1660ICC1000	PP070419.D	11 Mar 2025 15:13		YPIAJ	Ok
4	AR1660ICC750	AR1660ICC750	PP070420.D	11 Mar 2025 15:29		YPIAJ	Ok
5	AR1660ICC500	AR1660ICC500	PP070421.D	11 Mar 2025 15:46		YPIAJ	Ok
6	AR1660ICC250	AR1660ICC250	PP070422.D	11 Mar 2025 16:02		YPIAJ	Ok,M
7	AR1660ICC050	AR1660ICC050	PP070423.D	11 Mar 2025 16:18		YPIAJ	Ok,M
8	AR1221ICC500	AR1221ICC500	PP070424.D	11 Mar 2025 16:34		YPIAJ	Ok
9	AR1232ICC1000	AR1232ICC1000	PP070425.D	11 Mar 2025 16:51		YPIAJ	Ok
10	AR1232ICC750	AR1232ICC750	PP070426.D	11 Mar 2025 17:07		YPIAJ	Ok
11	AR1232ICC500	AR1232ICC500	PP070427.D	11 Mar 2025 17:23		YPIAJ	Ok
12	AR1232ICC250	AR1232ICC250	PP070428.D	11 Mar 2025 17:40		YPIAJ	Ok,M
13	AR1232ICC050	AR1232ICC050	PP070429.D	11 Mar 2025 17:56		YPIAJ	Ok,M
14	AR1242ICC1000	AR1242ICC1000	PP070430.D	11 Mar 2025 18:12		YPIAJ	Ok
15	AR1242ICC750	AR1242ICC750	PP070431.D	11 Mar 2025 18:28		YPIAJ	Ok
16	AR1242ICC500	AR1242ICC500	PP070432.D	11 Mar 2025 18:45		YPIAJ	Ok
17	AR1242ICC250	AR1242ICC250	PP070433.D	11 Mar 2025 19:01		YPIAJ	Ok
18	AR1242ICC050	AR1242ICC050	PP070434.D	11 Mar 2025 19:17		YPIAJ	Ok,M

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031125

Review By	yogesh	Review On	3/12/2025 7:57:33 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:54:29 AM
SubDirectory	PP031125	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248ICC1000	AR1248ICC1000	PP070435.D	11 Mar 2025 19:34		YPIAJ	Ok
20	AR1248ICC750	AR1248ICC750	PP070436.D	11 Mar 2025 19:50		YPIAJ	Ok
21	AR1248ICC500	AR1248ICC500	PP070437.D	11 Mar 2025 20:06		YPIAJ	Ok
22	AR1248ICC250	AR1248ICC250	PP070438.D	11 Mar 2025 20:22		YPIAJ	Ok
23	AR1248ICC050	AR1248ICC050	PP070439.D	11 Mar 2025 20:39		YPIAJ	Ok,M
24	AR1254ICC1000	AR1254ICC1000	PP070440.D	11 Mar 2025 20:55		YPIAJ	Ok
25	AR1254ICC750	AR1254ICC750	PP070441.D	11 Mar 2025 21:11		YPIAJ	Ok
26	AR1254ICC500	AR1254ICC500	PP070442.D	11 Mar 2025 21:28		YPIAJ	Ok
27	AR1254ICC250	AR1254ICC250	PP070443.D	11 Mar 2025 21:44		YPIAJ	Ok
28	AR1254ICC050	AR1254ICC050	PP070444.D	11 Mar 2025 22:00		YPIAJ	Ok
29	AR1262ICC500	AR1262ICC500	PP070445.D	11 Mar 2025 22:16		YPIAJ	Ok
30	AR1268ICC1000	AR1268ICC1000	PP070446.D	11 Mar 2025 22:33		YPIAJ	Ok
31	AR1268ICC750	AR1268ICC750	PP070447.D	11 Mar 2025 22:49		YPIAJ	Ok
32	AR1268ICC500	AR1268ICC500	PP070448.D	11 Mar 2025 23:05		YPIAJ	Ok
33	AR1268ICC250	AR1268ICC250	PP070449.D	11 Mar 2025 23:22		YPIAJ	Ok
34	AR1268ICC050	AR1268ICC050	PP070450.D	11 Mar 2025 23:38		YPIAJ	Ok,M
35	PP031125ICV500	ICVPP031125	PP070451.D	11 Mar 2025 23:54		YPIAJ	Ok
36	AR1232ICV500	ICVPP031125AR1232	PP070452.D	12 Mar 2025 00:10		YPIAJ	Ok
37	AR1242ICV500	ICVPP031125AR1242	PP070453.D	12 Mar 2025 00:27		YPIAJ	Ok

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031125

Review By	yogesh	Review On	3/12/2025 7:57:33 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:54:29 AM
SubDirectory	PP031125	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

38	AR1248ICV500	ICVPP031125AR1248	PP070454.D	12 Mar 2025 00:43		YPIAJ	Ok
39	AR1254ICV500	ICVPP031125AR1254	PP070455.D	12 Mar 2025 00:59		YPIAJ	Ok
40	AR1268ICV500	ICVPP031125AR1268	PP070456.D	12 Mar 2025 01:16		YPIAJ	Ok
41	AR1660CCC500	AR1660CCC500	PP070457.D	12 Mar 2025 01:32		YPIAJ	Ok
42	AR1232CCC500	AR1232CCC500	PP070458.D	12 Mar 2025 01:48		YPIAJ	Ok
43	AR1242CCC500	AR1242CCC500	PP070459.D	12 Mar 2025 02:04		YPIAJ	Ok
44	I.BLK	I.BLK	PP070460.D	12 Mar 2025 02:21		YPIAJ	Ok
45	PB167066BL	PB167066BL	PP070461.D	12 Mar 2025 02:37		YPIAJ	Ok
46	Q1502-15	PT-PCBW-WP	PP070462.D	12 Mar 2025 02:53	AR1232 HIT	YPIAJ	Ok
47	AR1660CCC500	AR1660CCC500	PP070463.D	12 Mar 2025 03:09		YPIAJ	Ok
48	AR1232CCC500	AR1232CCC500	PP070464.D	12 Mar 2025 03:26		YPIAJ	Ok
49	AR1242CCC500	AR1242CCC500	PP070465.D	12 Mar 2025 03:42		YPIAJ	Ok,M
50	I.BLK	I.BLK	PP070466.D	12 Mar 2025 03:58		YPIAJ	Ok

M : Manual Integration

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031425

Review By	yogesh	Review On	3/17/2025 8:24:56 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:39:12 AM
SubDirectory	PP031425	HP Acquire Method	HP Processing Method PP031125

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773
Internal Standard/PEM	
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PP070499.D	14 Mar 2025 07:42		YPIAJ	Ok
2	AR1660CCC500	AR1660CCC500	PP070500.D	14 Mar 2025 07:58		YPIAJ	Ok,M
3	AR1242CCC500	AR1242CCC500	PP070501.D	14 Mar 2025 08:14		YPIAJ	Ok
4	AR1248CCC500	AR1248CCC500	PP070502.D	14 Mar 2025 08:31		YPIAJ	Ok
5	AR1254CCC500	AR1254CCC500	PP070503.D	14 Mar 2025 08:47		YPIAJ	Ok
6	I.BLK	I.BLK	PP070504.D	14 Mar 2025 09:03		YPIAJ	Ok
7	PB167130BL	PB167130BL	PP070505.D	14 Mar 2025 09:21		YPIAJ	Ok
8	PB167130BS	PB167130BS	PP070506.D	14 Mar 2025 09:37		YPIAJ	Ok
9	Q1562-01	BC271227-1-1	PP070507.D	14 Mar 2025 09:53		YPIAJ	Ok,M
10	Q1562-02	BC271227-1-2	PP070508.D	14 Mar 2025 10:09		YPIAJ	Ok,M
11	Q1562-03	BC271227-2-1	PP070509.D	14 Mar 2025 10:26		YPIAJ	Ok,M
12	Q1562-04	BC271227-2-2	PP070510.D	14 Mar 2025 10:42		YPIAJ	Ok,M
13	Q1562-05	EFB643W-1-1	PP070511.D	14 Mar 2025 10:58		YPIAJ	Ok,M
14	Q1562-06	EFB643W-1-2	PP070512.D	14 Mar 2025 11:14		YPIAJ	Ok,M
15	Q1562-07	GHA524R-1-1	PP070513.D	14 Mar 2025 11:31		YPIAJ	Ok,M
16	Q1562-08	GHA524R-1-2	PP070514.D	14 Mar 2025 11:47		YPIAJ	Ok,M
17	AR1660CCC500	AR1660CCC500	PP070515.D	14 Mar 2025 12:36		YPIAJ	Ok,M
18	AR1242CCC500	AR1242CCC500	PP070516.D	14 Mar 2025 12:52		YPIAJ	Ok

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031425

Review By	yogesh	Review On	3/17/2025 8:24:56 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:39:12 AM
SubDirectory	PP031425	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248CCC500	AR1248CCC500	PP070517.D	14 Mar 2025 13:08		YPIAJ	Ok
20	AR1254CCC500	AR1254CCC500	PP070518.D	14 Mar 2025 13:24		YPIAJ	Ok
21	I.BLK	I.BLK	PP070519.D	14 Mar 2025 13:41		YPIAJ	Ok
22	Q1564-04	BC258874-1-2	PP070520.D	14 Mar 2025 13:57		YPIAJ	Ok,M
23	Q1564-05	BC226751-1-1	PP070521.D	14 Mar 2025 14:13		YPIAJ	Ok,M
24	Q1564-06	BC226751-1-2	PP070522.D	14 Mar 2025 14:29		YPIAJ	Ok,M
25	Q1564-01	BC247799-1-1	PP070523.D	14 Mar 2025 14:45		YPIAJ	Ok,M
26	Q1564-02	BC247799-1-2	PP070524.D	14 Mar 2025 15:02		YPIAJ	Ok,M
27	Q1564-03	BC258874-1-1	PP070525.D	14 Mar 2025 15:18		YPIAJ	Ok,M
28	PB167139BL	PB167139BL	PP070526.D	14 Mar 2025 15:34		YPIAJ	Ok
29	PB167139BS	PB167139BS	PP070527.D	14 Mar 2025 15:50		YPIAJ	Ok
30	PB167139BSD	PB167139BSD	PP070528.D	14 Mar 2025 16:06		YPIAJ	Ok
31	AR1660CCC500	AR1660CCC500	PP070529.D	14 Mar 2025 16:55		YPIAJ	Ok
32	AR1242CCC500	AR1242CCC500	PP070530.D	14 Mar 2025 17:11		YPIAJ	Ok
33	AR1248CCC500	AR1248CCC500	PP070531.D	14 Mar 2025 17:28		YPIAJ	Ok
34	AR1254CCC500	AR1254CCC500	PP070532.D	14 Mar 2025 17:44		YPIAJ	Ok
35	I.BLK	I.BLK	PP070533.D	14 Mar 2025 18:00		YPIAJ	Ok
36	Q1553-03	FRAC-TANK-FMI120	PP070534.D	14 Mar 2025 18:16		YPIAJ	Ok,M
37	Q1563-01	437	PP070535.D	14 Mar 2025 18:33		YPIAJ	Ok

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031425

Review By	yogesh	Review On	3/17/2025 8:24:56 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:39:12 AM
SubDirectory	PP031425	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

38	Q1563-02	FERNOT-WATER	PP070536.D	14 Mar 2025 18:49		YPIAJ	Ok,M
39	PB167136BL	PB167136BL	PP070537.D	14 Mar 2025 19:05		YPIAJ	Ok
40	PB167136BS	PB167136BS	PP070538.D	14 Mar 2025 19:21		YPIAJ	Ok
41	Q1566-01	CTWK-COMP	PP070539.D	14 Mar 2025 19:38		YPIAJ	Ok
42	Q1568-01	JC-03-03132025	PP070540.D	14 Mar 2025 19:54		YPIAJ	Ok
43	Q1568-01MS	JC-03-03132025MS	PP070541.D	14 Mar 2025 20:10		YPIAJ	Ok
44	Q1568-01MSD	JC-03-03132025MSD	PP070542.D	14 Mar 2025 20:26		YPIAJ	Ok,M
45	AR1660CCC500	AR1660CCC500	PP070543.D	14 Mar 2025 21:15		YPIAJ	Ok
46	AR1242CCC500	AR1242CCC500	PP070544.D	14 Mar 2025 21:31		YPIAJ	Ok,M
47	AR1248CCC500	AR1248CCC500	PP070545.D	14 Mar 2025 21:48		YPIAJ	Ok
48	AR1254CCC500	AR1254CCC500	PP070546.D	14 Mar 2025 22:04		YPIAJ	Ok
49	I.BLK	I.BLK	PP070547.D	14 Mar 2025 22:20		YPIAJ	Ok
50	PB167143BL	PB167143BL	PP070548.D	14 Mar 2025 22:36		YPIAJ	Ok
51	PB167143BS	PB167143BS	PP070549.D	14 Mar 2025 22:52		YPIAJ	Ok,M
52	Q1569-01	TAP-IDW-SOIL-031325	PP070550.D	14 Mar 2025 23:09		YPIAJ	Ok
53	Q1569-04	TAP-IDW-SOIL-031325	PP070551.D	14 Mar 2025 23:25		YPIAJ	Ok,M
54	Q1572-01	C0AC9	PP070552.D	14 Mar 2025 23:41	DCB high in 2nd column , AR1260 AR1248 Hit , Need dilution 10X,50X	YPIAJ	Dilution
55	Q1572-02	C0O14	PP070553.D	14 Mar 2025 23:57	AR1260 AR1248 Hit , Need dilution 10X,50X	YPIAJ	Dilution

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031425

Review By	yogesh	Review On	3/17/2025 8:24:56 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:39:12 AM
SubDirectory	PP031425	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775 PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773 PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Initial Calibration Stds			
CCC			
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

56	Q1572-03	C0015	PP070554.D	15 Mar 2025 00:14	AR1260 AR1248 Hit , Need dilution 5X,25X	YPIAJ	Dilution
57	Q1572-04	C0016	PP070555.D	15 Mar 2025 00:30	DCB high in 2nd column , AR1260 AR1248 Hit , Need dilution 5X,50X	YPIAJ	Dilution
58	Q1572-05	C0017	PP070556.D	15 Mar 2025 00:46	DCB high in 2nd column , AR1260 AR1248 Hit , Need dilution 10X,100X	YPIAJ	Dilution
59	Q1572-07	C0019	PP070557.D	15 Mar 2025 01:02	AR1260 AR1248 Hit , Need dilution 10X	YPIAJ	Dilution
60	AR1660CCC500	AR1660CCC500	PP070558.D	15 Mar 2025 01:51		YPIAJ	Ok
61	AR1242CCC500	AR1242CCC500	PP070559.D	15 Mar 2025 02:07		YPIAJ	Ok
62	AR1248CCC500	AR1248CCC500	PP070560.D	15 Mar 2025 02:24		YPIAJ	Ok
63	AR1254CCC500	AR1254CCC500	PP070561.D	15 Mar 2025 02:40		YPIAJ	Ok
64	I.BLK	I.BLK	PP070562.D	15 Mar 2025 02:56		YPIAJ	Ok
65	Q1572-06	C0018	PP070563.D	15 Mar 2025 03:12	AR1260 AR1248 Hit , Need dilution 5X,50X	YPIAJ	Dilution
66	Q1572-06MS	C0018MS	PP070564.D	15 Mar 2025 03:29	AR1016 and AR1260 Recovery fail	YPIAJ	Ok,M
67	Q1572-06MSD	C0018MSD	PP070565.D	15 Mar 2025 03:45	AR1016 and AR1260 Recovery fail	YPIAJ	Ok,M
68	Q1572-08	C0020	PP070566.D	15 Mar 2025 04:01	DCB high in 2nd column , AR1248 Hit ,Need dilution 10X	YPIAJ	Dilution
69	Q1572-09	C0021	PP070567.D	15 Mar 2025 04:17	AR1248 Hit , Need dilution 50X	YPIAJ	Dilution
70	AR1660CCC500	AR1660CCC500	PP070568.D	15 Mar 2025 05:06		YPIAJ	Ok
71	AR1242CCC500	AR1242CCC500	PP070569.D	15 Mar 2025 05:22		YPIAJ	Ok

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QC Batch ID # PP031425

Review By	yogesh	Review On	3/17/2025 8:24:56 AM
Supervise By	mohammad	Supervise On	3/19/2025 6:39:12 AM
SubDirectory	PP031425	HP Acquire Method	HP Processing Method PP031125
STD. NAME	STD REF.#		
Tune/Reschk	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
Initial Calibration Stds			
CCC			
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

72	AR1248CCC500	AR1248CCC500	PP070570.D	15 Mar 2025 05:39		YP\AJ	Ok
73	AR1254CCC500	AR1254CCC500	PP070571.D	15 Mar 2025 05:55		YP\AJ	Ok
74	I.BLK	I.BLK	PP070572.D	15 Mar 2025 06:11		YP\AJ	Ok

M : Manual Integration



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 3/17/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:20
In Date: 03/14/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN-1

OVENTEMP OUT Celsius(°C): 105
Time OUT: 08:35
Out Date: 03/15/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLIDS-OVEN

QC:LB135036

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q1569-01	TAP-IDW-SOIL-031325-01	1	1.14	11.74	12.88	10.13	76.6	
Q1569-04	TAP-IDW-SOIL-031325-02	2	1.16	10.92	12.08	9.16	73.3	
Q1572-01	C0AC9	3	1.12	10.23	11.35	8.25	69.7	
Q1572-02	C0014	4	1.15	10.41	11.56	9.32	78.5	
Q1572-03	C0015	5	1.18	10.05	11.23	9.22	80.0	
Q1572-04	C0016	6	1.15	9.00	10.15	7.3	68.3	
Q1572-05	C0017	7	1.14	10.49	11.63	8.97	74.6	
Q1572-06	C0018	8	1.15	9.91	11.06	8.68	76.0	
Q1572-07	C0019	9	1.16	10.15	11.31	8.17	69.1	
Q1572-08	C0020	10	1.13	10.26	11.39	8.8	74.8	
Q1572-09	C0021	11	1.15	10.40	11.55	8.11	66.9	
Q1572-10	C0022	12	1.15	10.39	11.54	8.00	65.9	
Q1572-11	C0023	13	1.14	10.46	11.6	9.91	83.8	
Q1572-12	C0024	14	1.13	10.28	11.41	8.82	74.8	
Q1572-13	C0025	15	1.12	10.22	11.34	8.92	76.3	
Q1572-14	C0026	16	1.19	10.23	11.42	8.82	74.6	
Q1572-15	C0027	17	1.12	10.48	11.6	8.85	73.8	
Q1572-16	C0028	18	1.15	10.11	11.26	9.52	82.8	
Q1573-01	C0AC4	19	1.19	10.51	11.7	8.81	72.5	
Q1573-02	C0AC5	20	1.16	11.03	12.19	8.16	63.5	
Q1573-03	C0AC6	21	1.14	10.38	11.52	7.66	62.8	
Q1573-04	C0AC8	22	1.16	10.28	11.44	7.25	59.2	
Q1573-05	C0029	23	1.18	10.60	11.78	7.09	55.8	
Q1573-06	C0030	24	1.13	10.13	11.26	8.17	69.5	
Q1573-07	C0031	25	1.19	10.24	11.43	8.1	67.5	
Q1573-08	C0032	26	1.15	10.08	11.23	6.7	55.1	
Q1573-09	C0033	27	1.13	10.27	11.4	7.76	64.6	
Q1573-10	C0034	28	1.14	10.42	11.56	9.7	82.1	



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 3/17/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:20
In Date: 03/14/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN-1

OVENTEMP OUT Celsius(°C): 105
Time OUT: 08:35
Out Date: 03/15/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLIDS-OVEN

QC:LB135036

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q1573-11	C0035	29	1.19	11.25	12.44	9.97	78.0	
Q1574-01	WC1	30	1.11	10.31	11.42	11.21	98.0	
Q1578-01	JEC817T-1-1	31	1.00	1.00	2.00	2.00	100.0	pile
Q1578-02	JEC817T-1-2	32	1.00	1.00	2.00	2.00	100.0	pile
Q1579-01	BC271189-1-1	33	1.00	1.00	2.00	2.00	100.0	pile
Q1579-02	BC271189-1-2	34	1.00	1.00	2.00	2.00	100.0	pile
Q1579-03	BC271038-1-1	35	1.00	1.00	2.00	2.00	100.0	pile
Q1579-04	BC271038-1-2	36	1.00	1.00	2.00	2.00	100.0	pile
Q1581-01	TR-06-031425	37	1.14	10.08	11.22	10.54	93.3	
Q1581-02	TR-06-031425-E2	38	1.18	10.18	11.36	10.64	92.9	
Q1584-05	SVOC-GPC-BLANK	39	1.00	1.00	2.00	2.00	100.0	
Q1584-06	PEST-GPC-BLANK	40	1.00	1.00	2.00	2.00	100.0	
Q1584-07	PEST-GPC-BLANK-SPIKE	41	1.00	1.00	2.00	2.00	100.0	
Q1584-08	PCB-GPC-BLANK	42	1.00	1.00	2.00	2.00	100.0	
Q1584-09	PCB-GPC-BLANK-SPIKE	43	1.00	1.00	2.00	2.00	100.0	
Q1584-10	SVOC-GPC2-BLANK	44	1.00	1.00	2.00	2.00	100.0	
Q1584-11	PEST-GPC2-BLANK	45	1.00	1.00	2.00	2.00	100.0	
Q1584-12	PEST-GPC2-BLANK-SPIKE	46	1.00	1.00	2.00	2.00	100.0	
Q1584-13	PCB-GPC2-BLANK	47	1.00	1.00	2.00	2.00	100.0	
Q1584-14	PCB-GPC2-BLANK-SPIKE	48	1.00	1.00	2.00	2.00	100.0	
Q1585-01	OK-02-03142025	49	1.14	10.43	11.57	11.27	97.1	
Q1585-02	OK-02-03142025-E2	50	1.13	10.27	11.4	10.89	95.0	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

135036

WorkList Name : %1-031425 WorkList ID : 188269 Department : Wet-Chemistry Date : 03-14-2025 08:28:30

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1569-01	TAP-IDW-SOIL-031325-01	Solid	Percent Solids	Cool 4 deg C	WEST04	I33	03/13/2025	Chemtech -SO
Q1569-04	TAP-IDW-SOIL-031325-02	Solid	Percent Solids	Cool 4 deg C	WEST04	I33	03/13/2025	Chemtech -SO
Q1572-01	C0AC9	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-02	C0O14	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-03	C0O15	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-04	C0O16	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-05	C0O17	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-06	C0O18	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-07	C0O19	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-08	C0O20	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-09	C0O21	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-10	C0O22	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-11	C0O23	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-12	C0O24	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-13	C0O25	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-14	C0O26	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-15	C0O27	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1572-16	C0O28	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/12/2025	Chemtech -SO
Q1573-01	C0AC4	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/11/2025	Chemtech -SO
Q1573-02	C0AC5	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/11/2025	Chemtech -SO
Q1573-03	C0AC6	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/11/2025	Chemtech -SO

Date/Time 03/14/25 16:10
 Raw Sample Received by: SP WPC
 Raw Sample Relinquished by: JTCM
 Date/Time 03/14/25 17:30
 Raw Sample Received by: JTCM
 Raw Sample Relinquished by: SP WPC

WORKLIST(Hardcopy Internal Chain)

135036

WorkList Name : %1-031425 WorkList ID : 188269 Department : Wet-Chemistry Date : 03-14-2025 08:28:30

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1573-04	C0AC8	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/11/2025	Chemtech -SO
Q1573-05	C0O29	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/11/2025	Chemtech -SO
Q1573-06	C0O30	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/11/2025	Chemtech -SO
Q1573-07	C0O31	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/11/2025	Chemtech -SO
Q1573-08	C0O32	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/11/2025	Chemtech -SO
Q1573-09	C0O33	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/11/2025	Chemtech -SO
Q1573-10	C0O34	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/11/2025	Chemtech -SO
Q1573-11	C0O35	Solid	Percent Solids	Cool 4 deg C	TETR16	I31	03/11/2025	Chemtech -SO
Q1574-01	WC1	Solid	Percent Solids	Cool 4 deg C	GENV01	I41	03/11/2025	Chemtech -SO
Q1578-01	JEC817T-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	I41	03/12/2025	Chemtech -SO
Q1578-02	JEC817T-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	I41	03/14/2025	Chemtech -SO
Q1579-01	BC271189-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	I41	03/14/2025	Chemtech -SO
Q1579-02	BC271189-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	I41	03/14/2025	Chemtech -SO
Q1579-03	BC271038-1-1	Solid	Percent Solids	Cool 4 deg C	PSEG03	I41	03/14/2025	Chemtech -SO
Q1579-04	BC271038-1-2	Solid	Percent Solids	Cool 4 deg C	PSEG03	I41	03/14/2025	Chemtech -SO
Q1581-01	TR-06-031425	Solid	Percent Solids	Cool 4 deg C	PSEG05	I41	03/14/2025	Chemtech -SO
Q1581-02	TR-06-031425-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	I41	03/14/2025	Chemtech -SO
Q1584-05	SVOC-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	03/14/2025	Chemtech -SO
Q1584-06	PEST-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	03/14/2025	Chemtech -SO
Q1584-07	PEST-GPC-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	03/14/2025	Chemtech -SO
Q1584-08	PCB-GPC-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	03/14/2025	Chemtech -SO

Date/Time 03/14/25 16:10
 Raw Sample Received by: SS WCC
 Raw Sample Relinquished by: STCm
 Date/Time 03/14/25 17:30
 Raw Sample Received by: STCm
 Raw Sample Relinquished by: SS WCC

WORKLIST(Hardcopy Internal Chain)

WB 135036

WorkList Name : %1-031425 WorkList ID : 188269 Department : Wet-Chemistry Date : 03-14-2025 08:28:30

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1584-09	PCB-GPC-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	03/14/2025	Chemtech -SO
Q1584-10	SVOC-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	03/14/2025	Chemtech -SO
Q1584-11	PEST-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	03/14/2025	Chemtech -SO
Q1584-12	PEST-GPC2-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	03/14/2025	Chemtech -SO
Q1584-13	PCB-GPC2-BLANK	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	03/14/2025	Chemtech -SO
Q1584-14	PCB-GPC2-BLANK-SPIKE	Solid	Percent Solids	Cool 4 deg C	CHEM02	F11	03/14/2025	Chemtech -SO
Q1585-01	OK-02-03142025	Solid	Percent Solids	Cool 4 deg C	PSEG05	I41	03/14/2025	Chemtech -SO
Q1585-02	OK-02-03142025-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	I41	03/14/2025	Chemtech -SO

Date/Time 03/14/25 16:10
 Raw Sample Received by: JB muel
 Raw Sample Relinquished by: IT (SM)

Date/Time 03/14/25 17:30
 Raw Sample Received by: IT (SM)
 Raw Sample Relinquished by: JB muel

SOP ID: M3541-ASE Extraction-14

Clean Up SOP #: Acid Cleanup

Matrix : Solid

Welgh By: EH

Balance check: RJ

Balance ID: EX-SC-2

pH Strip Lot#: N/A

Extraction By: RJ

Filter By: RJ

pH Meter ID: N/A

Hood ID: 3,7

Extraction Start Date : 03/14/2025

Extraction Start Time : 12:25

Extraction End Date : 03/14/2025

Extraction End Time : 15:25

Concentration By: EH

Supervisor By : RUPESH

Extraction Method: ☐ Seperatory Funnel

☐ Continious Liquid/Liquid

☐ Sonication

☐ Waste Dilution

☒ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP24209
Surrogate	1.0ML	200 PPB	PP24217
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Hexane/Acetone/1:1	N/A	EP2592
Baked Na2SO4	N/A	EP2593
Sand	N/A	E2865
Hexane	N/A	E3877
H2SO4 1:1	N/A	EP2565
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40 ML Vial lot# 03-40 BTS721.

KD Bath ID: N/A

Envap ID: NEVAP-02

KD Bath Temperature: N/A

Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
3/14/25	RS (Ext-Lab)	T-Prest/PLB
15:30	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-14

Concentration Date: 03/14/2025

Sample ID	Client Sample ID	Test	g/mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB167143BL	ABLK143	PCB Group1	30.01	N/A	ritesh	Evelyn	10			U2-1
PB167143BS	ALCS143	PCB Group1	30.03	N/A	ritesh	Evelyn	10			2
Q1569-01	TAP-IDW-SOIL-031325-01	PCB	30.07	N/A	ritesh	Evelyn	10	B	Sludge	3
Q1569-04	TAP-IDW-SOIL-031325-02	PCB	30.03	N/A	ritesh	Evelyn	10	B	Sludge	4
Q1572-01	C0AC9	PCB Group1	30.06	N/A	ritesh	Evelyn	10			5
Q1572-02	C0014	PCB Group1	30.02	N/A	ritesh	Evelyn	10			6
Q1572-03	C0015	PCB Group1	30.10	N/A	ritesh	Evelyn	10			U3-1
Q1572-04	C0016	PCB Group1	30.08	N/A	ritesh	Evelyn	10			2
Q1572-05	C0017	PCB Group1	30.05	N/A	ritesh	Evelyn	10			3
Q1572-06	C0018	PCB Group1	30.03	N/A	ritesh	Evelyn	10			4
Q1572-06MS	C0018MS	PCB Group1	30.07	N/A	ritesh	Evelyn	10			5
Q1572-06MS D	C0018MSD	PCB Group1	30.09	N/A	ritesh	Evelyn	10			6
Q1572-07	C0019	PCB Group1	30.01	N/A	ritesh	Evelyn	10			U6-1
Q1572-08	C0020	PCB Group1	30.04	N/A	ritesh	Evelyn	10			2
Q1572-09	C0021	PCB Group1	30.08	N/A	ritesh	Evelyn	10			3
Q1572-10	C0022	PCB Group1	30.05	N/A	ritesh	Evelyn	10			4
Q1572-11	C0023	PCB Group1	30.03	N/A	ritesh	Evelyn	10			5
Q1572-12	C0024	PCB Group1	30.09	N/A	ritesh	Evelyn	10			6
Q1572-13	C0025	PCB Group1	30.06	N/A	ritesh	Evelyn	10			U7-1
Q1572-14	C0026	PCB Group1	30.03	N/A	ritesh	Evelyn	10			2
Q1572-15	C0027	PCB Group1	30.07	N/A	ritesh	Evelyn	10			3
Q1572-16	C0028	PCB Group1	30.09	N/A	ritesh	Evelyn	10			4
Q1574-01	WC1	PCB	30.05	N/A	ritesh	Evelyn	10	C		5

* Extracts relinquished on the same date as received.

1917125

WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q1572 WorkList ID : 188289 Department : Extraction Date : 03-14-2025 12:16:04

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q1569-01	TAP-IDW-SOIL-031325-01	Solid	PCB	Cool 4 deg C	WEST04	I33	03/13/2025	8082A
Q1569-04	TAP-IDW-SOIL-031325-02	Solid	PCB	Cool 4 deg C	WEST04		03/13/2025	8082A
Q1572-01	C00AC9	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-02	C0014	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-03	C0015	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-04	C0016	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-05	C0017	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-06	C0018	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-07	C0019	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-08	C0020	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-09	C0021	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-10	C0022	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-11	C0023	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-12	C0024	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-13	C0025	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-14	C0026	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-15	C0027	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1572-16	C0028	Solid	PCB Group1	Cool 4 deg C	TETR16	I31	03/12/2025	8082A
Q1574-01	WC1	Solid	PCB	Cool 4 deg C	GENV01	I41	03/12/2025	8082A

Date/Time 3/14/25 12:20
Raw Sample Received by: RJC (Ext Lab)
Raw Sample Relinquished by: OP sm

Date/Time 3/14/25 12:55
Raw Sample Received by: OP sm
Raw Sample Relinquished by: RJC (Ext Lab)

Prep Standard - Chemical Standard Summary

Order ID : Q1574

Test : PCB

Prepbatch ID : PB167143,

Sequence ID/Qc Batch ID: PO031725,pp031425,

Standard ID :

EP2565,EP2592,EP2593,PP23733,PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775,PP23776,PP23777,PP23778,PP23779,PP23780,PP23781,PP23782,PP23783,PP23784,PP23785,PP23786,PP23787,PP23788,PP23789,PP23790,PP23946,PP23947,PP24209,PP24217,

Chemical ID :

E2865,E3551,E3804,E3805,E3825,E3876,E3877,M5173,P10483,P10500,P11507,P11512,P11521,P11581,P11587,P11590,P11597,P12698,P12929,P12934,P12947,P12948,P12957,P13033,P13350,P13354,P13372,W3112,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2565	11/20/2024	05/20/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 11/20/2024

FROM 1000.00000ml of M5173 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	EP2592	02/27/2025	08/12/2025	RUPESHKUMAR SHAH	None	None	Riteshkumar Patel 02/27/2025

FROM 4000.00000ml of E3876 + 4000.00000ml of E3877 = Final Quantity: 8000.000 ml

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2593	03/07/2025	07/01/2025	RUPESHKUMAR SHAH	Extraction_SC ALE_2 (EX-SC-2)	None	Riteshkumar Patel 03/07/2025

FROM 4000.00000gram of E3551 = Final Quantity: 4000.000 gram

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP23733	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel 10/03/2024

FROM 1.00000ml of P13350 + 9.00000ml of E3805 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
202	AR1660 1000/100 ppb working solution 1st source	PP23735	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P10483 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
203	AR1660 750 PPB STD	PP23736	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23735 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
204	AR1660 500 PPB STD	PP23737	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23735 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
205	AR1660 250 PPB STD	PP23738	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23735 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
206	AR1660 50 PPB STD	PP23739	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23737 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
213	AR1221 1000 PPB WORKING SOLUTION	PP23740	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11581 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1079	AR1221 750 PPB STD	PP23741	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23740 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
222	AR1221 500 PPB STD	PP23742	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23740 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1080	AR1221 250 PPB STD	PP23743	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23740 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1081	AR1221 50 PPB STD	PP23744	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23742 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
214	AR1232 1000 PPB WORKING SOLUTION	PP23745	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11587 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1063	AR1232 750 PPB STD	PP23747	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23745 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
223	AR1232 500 PPB STD	PP23748	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23745 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1064	AR1232 250 PPB STD	PP23749	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23745 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1065	AR1232 50 PPB STD	PP23750	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23748 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
215	AR1242 1000 PPB WORKING STD	PP23751	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P12929 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1067	AR1242 750 PPB STD	PP23752	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23751 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
224	AR1242 500 PPB STD	PP23753	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23751 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1068	AR1242 250 PPB STD	PP23754	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23751 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1069	AR1242 50 PPB STD	PP23755	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23753 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
216	AR1248 1000 PPB WORKING STD	PP23756	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P12934 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1075	AR1248 750 PPB STD	PP23757	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23756 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
225	AR1248 500 PPB STD	PP23758	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23756 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1076	AR1248 250 PPB STD	PP23759	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23756 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1077	AR1248 50 PPB STD	PP23760	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23758 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
217	AR1254 1000 PPB WORKING STD	PP23761	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11590 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1071	AR1254 750 PPB STD	PP23762	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23761 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
226	AR1254 500 PPB STD	PP23763	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23761 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1072	AR1254 250 PPB STD	PP23764	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23761 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1073	AR1254 50 PPB STD	PP23765	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23763 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1529	AR1262 1000 PPB Working Solution	PP23766	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P10500 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3753	AR1262 750 PPB STD	PP23767	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23766 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1530	AR1262 500 PPB STD	PP23768	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23766 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3754	AR1262 250 PPB STD	PP23769	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23766 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3755	AR1262 50 PPB STD	PP23770	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23768 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1532	AR1268 1000 PPB Working Solution	PP23771	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11597 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3820	AR1268 750 PPB STD	PP23772	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23771 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1533	AR1268 500 PPB STD	PP23773	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23771 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3821	AR1268 250 PPB STD	PP23774	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23771 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3822	AR1268 50 PPB STD	PP23775	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23773 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
404	AR1660 100 PPM Stock Solution 2nd Source	PP23776	10/03/2024	04/01/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12947 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
405	AR1660 1000/100 PPB ICV STD	PP23777	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 98.50000ml of E3805 + 0.50000ml of PP23733 + 1.00000ml of PP23776 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
406	AR1660 500 PPB ICV	PP23778	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23777 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3789	AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT)	PP23779	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P13372 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3790	AR1221 500 PPB ICV(AGILENT)	PP23780	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23779 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1887	AR1232 1000 PPB Working Sol. 2nd Source	PP23781	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12698 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1889	AR1242 1000 PPB Working Sol. 2nd Source	PP23782	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel 10/03/2024

FROM 1.00000ml of P11507 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1888	AR1232 500 PPB ICV	PP23783	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel 10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23781 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1891	AR1242 500 PPB ICV	PP23784	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23782 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1890	AR1248 1000 PPB Working Sol. 2nd Source	PP23785	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11512 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1892	AR1248 500 PPB ICV	PP23786	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23785 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1893	AR1254 1000 PPB Working Sol. 2nd Source	PP23787	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12957 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1894	AR1254 500 PPB ICV	PP23788	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23787 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3757	AR1262 1000 PPB Working Solution second source	PP23789	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P13033 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3758	AR1262 500 PPB STD ICV	PP23790	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23789 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3817	AR1268 1000 ppb Working Soln. 2nd source	PP23946	11/07/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								11/13/2024

FROM 1.00000ml of P11521 + 98.50000ml of E3825 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3823	AR1268 500 PPB STD ICV	PP23947	11/07/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								11/13/2024

FROM 0.50000ml of E3825 + 0.50000ml of PP23946 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3857	5000 PPB PCB SPIKE SOLUTION 2ND SOURCE	PP24209	02/27/2025	08/27/2025	Ankita Jodhani	None	None	Yogesh Patel
								03/06/2025

FROM 0.50000ml of P12948 + 99.50000ml of E3876 = Final Quantity: 100.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP24217	03/05/2025	08/25/2025	Abdul Mirza	None	None	Yogesh Patel
<u>FROM</u> 1.00000ml of P13354 + 999.00000ml of E3876 = Final Quantity: 1000.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	06/30/2025	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	07/01/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	11/05/2025	10/01/2024 / Rajesh	09/25/2024 / Rajesh	E3804

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	03/30/2025	09/30/2024 / Rajesh	09/25/2024 / Rajesh	E3805

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	11/06/2025	11/06/2024 / Rajesh	11/01/2024 / Rajesh	E3825

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	08/25/2025	02/25/2025 /	02/12/2025 / Rajesh	E3876

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	243570	08/12/2025	02/12/2025 / Rajesh	02/12/2025 / Rajesh	E3877

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	0000281827	06/02/2025	06/01/2022 /	04/05/2022 / william	M5173

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul	A0163157	04/03/2025	10/03/2024 / Ankita	03/19/2021 / Abdul	P10483

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane	A0167722	04/03/2025	10/03/2024 / Ankita	03/19/2021 / Ankita	P10500

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-312-1 / Aroclor 1242	0006665550	04/03/2025	10/03/2024 / Ankita	02/21/2022 / Ankita	P11507

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-342-1 / Aroclor 1248	0006626997	04/03/2025	10/03/2024 / Ankita	02/21/2022 / Ankita	P11512

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-382-1 / Aroclor 1268	0006587800	05/07/2025	11/07/2024 / Ankita	02/21/2022 / Ankita	P11521

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul	A0175456	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11581

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul	A0173309	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11587

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	A0175403	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11590

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane	A0181782	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11597

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	91867 / Aroclor 1232 100 ug/mL	020823	04/03/2025	10/03/2024 / Ankita	08/07/2023 / Ankita	P12698

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul	a0203672	04/03/2025	10/03/2024 / Ankita	12/07/2023 / Ankita	P12929

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul	a0202803	04/03/2025	10/03/2024 / Ankita	12/07/2023 / Ankita	P12934

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12947

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	08/27/2025	02/27/2025 / Ankita	12/20/2023 / Yogesh	P12948

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ Arochlor 1254	121823	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12957

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	90165 / Aroclor 1262	112322	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P13033

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	04/03/2025	10/03/2024 / Ankita	04/22/2024 / Abdul	P13350

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	09/05/2025	03/05/2025 / Abdul	04/22/2024 / Abdul	P13354

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-292-1 / Aroclor 1221	0006783205	04/03/2025	10/03/2024 / Ankita	05/02/2024 / Ankita	P13372

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1


Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use

Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC



Michelle Bales
Sr. Manager, Quality Assurance

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9262-03
Batch No.: 24C1862008
Manufactured Date: 2024-01-30
Expiration Date: 2025-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.4 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 9/25/24

E 3805

Jamie Croak
Director Quality Operations, Bioscience Production

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

£ 3825

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

 **avantors**™



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 2/12/25

E 3876



Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Certificate of Analysis

1 Reagent Lane
 Fair Lawn, NJ 07410
 201.796.7100 tel
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System
 Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	H303	Quality Test / Release Date	11/07/2024
Lot Number	243570		
Description	HEXANES - OPTIMA		
Country of Origin	United States	Suggested Retest Date	Nov/2029
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A			
Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid
ASSAY (N-HEXANE)	%	>= 60	69
ASSAY (SUM C6 HYDROCARBONS)	%	>= 99.9	>99.9
COLOR	APHA	<= 5	<5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.653 - 0.673	0.669
EVAPORATION RESIDUE	ppm	<= 1	<1
FLUORESCENCE BACKGROUND	ppb	<= 1	<1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 195 NM	ABS. UNITS	<= 1	0.74
OPTICAL ABS AT 210 NM	ABS. UNITS	<= 0.25	0.17
OPTICAL ABS AT 220 NM	ABS. UNITS	<= 0.07	0.05
OPTICAL ABS AT 254 NM	ABS. UNITS	<= 0.005	0.001
PESTICIDE RESIDUE ANALYSIS	NG/L	<= 10	<10
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.375 - 1.385	1.379
SUITABILITY FOR GC/MS		= PASS TEST	PASS TEST
SULFUR COMPOUNDS	%	<= 0.005	<0.005
THIOPHENE	PASS/FAIL	= PASS TEST	PASS TEST
WATER (H2O)	%	<= 0.01	<0.01
WATER-SOLUBLE TITRABLE ACID	MEQ/G	<= 0.0003	0.0001

Recd. by RP on 2/12/25

 E3877

Harout Sahagian - Quality Control Manager - Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.

If there are any questions with this certificate, please call at (800) 227-6701.

*Based on suggested storage condition.

Hydrochloric Acid, 36.5–38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis



Material No.: 9530-33
Batch No.: 0000281827
Manufactured Date: 2021/03/30
Retest Date: 2026/03/29
Revision No: 1

Certificate of Analysis

Test	Specification	Result
ACS – Assay (as HCl) (by acid–base titrn)	36.5 – 38.0 %	37.6
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	1
ACS – Specific Gravity at 60°/60°F	1.185 – 1.192	1.189
ACS – Bromide (Br)	<= 0.005 %	< 0.005
ACS – Extractable Organic Substances	<= 5 ppm	< 1
ACS – Free Chlorine (as Cl ₂)	<= 0.5 ppm	< 0.5
Phosphate (PO ₄)	<= 0.05 ppm	< 0.03
Sulfate (SO ₄)	<= 0.5 ppm	< 0.3
Sulfite (SO ₃)	<= 0.8 ppm	0.3
Ammonium (NH ₄)	<= 3 ppm	< 1
Trace Impurities – Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities – Aluminum (Al)	<= 10.0 ppb	0.5
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities – Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities – Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities – Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities – Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities – Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities – Calcium (Ca)	<= 50.0 ppb	15.0
Trace Impurities – Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities – Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities – Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities – Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	3.0
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	1.0
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	< 0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	< 0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.2
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	18.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	< 0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.4
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use

Product Information (not specifications):

Appearance (clear, fuming liquid)

Meets ACS Specifications

Country of Origin: US

Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32039 Lot No.: A0163157
Description : Aroclor® 1016/1260 Mix
Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2026 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1016 CAS # 12674-11-2 (Lot 04) Purity ----%	1,007.0 µg/mL	+/- 5.8683 µg/mL Gravimetric +/- 31.9082 µg/mL Unstressed +/- 41.6868 µg/mL Stressed
2	Aroclor 1260 CAS # 11096-82-5 (Lot 07) Purity ----%	1,008.0 µg/mL	+/- 5.8741 µg/mL Gravimetric +/- 31.9399 µg/mL Unstressed +/- 41.7282 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 10476

P 10480

AR
02/19/21

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar - Mix Technician

Date Mixed: 03-Aug-2020

Balance: B442140311

Justine Albertson - Operations Tech-ARM QC

Date Passed: 05-Aug-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32409 Lot No.: A0167722
Description : Aroclor® 1262 Standard
Aroclor® 1262 Standard 1,000 µg/mL, 1mL/ampul, Hexane
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : April 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1262	1,004.0 µg/mL	+/- 5.9635 µg/mL Gravimetric
	CAS # 37324-23-5 (Lot 10849100)		+/- 31.8340 µg/mL Unstressed
	Purity ----%		+/- 41.5787 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P10496
↓
P10500

AJ
09/19/21

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I


Date Mixed: 03-Jan-2021 **Balance:** B707717271

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 05-Jan-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1242 Standard

Lot Number: 0006665550

Product Number: PP-312-1

Lot Issue Date: 08-Feb-2022

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 31-Jan-2027

Component Name	CERTIFIED VALUES			CAS#	Analyte Lot
	Concentration	Expanded Uncertainty			
Aroclor 1242	100.4	± 0.5 µg/mL		053469-21-9	NT01020

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P11503
↓
P11507

AJ
02/21/22

Page: 1 of 2

CSD-QA-015.1

ISO 17034



Agilent

Trusted Answers

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2


www.agilent.com/quality/

CSD-QA-015.1



ISO 17025
Cert No. AT-

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1248 Standard

Lot Number: 0006626997

Product Number: PP-342-1

Lot Issue Date: 17-Aug-2021

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 30-Sep-2025

Component Name	CERTIFIED VALUES		CAS#	Analyte Lot
	Concentration	Expanded Uncertainty		
Aroclor 1248	100.3	± 0.5 µg/mL	012672-29-6	NT01582

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.


P11508

↓
P11512

AJ

2/21/22

ISO 17034



Agilent

Trusted Answers

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois

QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



Certificate of Analysis

P11518
↓
P11522
AJ
02/21/22

Product Name: Aroclor 1268 Standard

Product Number: PP-382-1

Lot Issue Date: 09-Feb-2021

Lot Number: 0006587800

Expiration Date: 31-Mar-2029

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration ± Uncertainty
Aroclor 1268	011100-14-4	RM00937	100.0 ± 0.5 µg/mL

Matrix: isooctane (2,2,4-trimethylpentane)

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.


Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026
Page: 1 of 1

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32007 Lot No.: A0175456
Description : Aroclor® 1221 Standard
Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1221	1,002.0 µg/mL	+/- 5.9516 µg/mL Gravimetric
	CAS # 11104-28-2 (Lot 10210500)		+/- 31.7706 µg/mL Unstressed
	Purity ----%		+/- 41.4958 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 11578
↓
P 11582 / (S)

AR
04/30/22

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 16-Aug-2021 Balance: B442140311

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 18-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11578
↓
P11582 / (S)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32008 Lot No.: A0173309
Description : Aroclor® 1232 Standard
Aroclor® 1232 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : September 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1232	1,001.0 µg/mL	+/- 5.9456 µg/mL Gravimetric
	CAS # 11141-16-5 (Lot 15665-01)		+/- 31.7389 µg/mL Unstressed
	Purity ----%		+/- 41.4544 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11583
↓
P11587 / (S)

AR
04/30/22

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 13-Jun-2021 **Balance:** B442140311

Alexis Shelow
Alexis Shelow - Operations Tech I

Date Passed: 16-Jun-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11583
↓
P11587 (5)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011 Lot No.: A0175403
Description : Aroclor® 1254 Standard
Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1254 CAS # 11097-69-1 (Lot 124-191-B) Purity ----%	1,000.7 µg/mL	+/- 5.9437 µg/mL Gravimetric +/- 31.7284 µg/mL Unstressed +/- 41.4406 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11588
↓
P11592 / (S)

AR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Cathleen Soltis

Cathleen Soltis - Mix Technician

Date Mixed: 15-Aug-2021

Balance: 1128360905

Alexis Shelow

Alexis Shelow - Operations Tech I

Date Passed: 17-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11588
↓
P11592 / (5)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32410 Lot No.: A0181782
Description : Aroclor® 1268 Standard
Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : May 31, 2028 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1268 CAS # 11100-14-4 Purity ----%	1,001.4 µg/mL (Lot 10947000)	+/- 5.9480 µg/mL Gravimetric +/- 31.7516 µg/mL Unstressed +/- 41.4710 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 11593
↓
P 11597
⑤

UAR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Penelope S. Riglin
Penelope Riglin - Operations Tech I

Date Mixed: 14-Feb-2022

Balance: 1128360905

Clara Windle
Clara Windle - Operations Technician I

Date Passed: 17-Feb-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 11593 / (5)
↓
P 11597
[Signature]
04/30/2022



CERTIFIED WEIGHT REPORT

Part Number: **91867**
 Lot Number: **020823**
 Description: **WP 037 - Aroclor 1232**
PCB Technical Mixture
 Expiration Date: **020833**
 Recommended Storage: **Ambient (20 °C)**
 Nominal Concentration ($\mu\text{g/mL}$): **100**
 NIST Test ID#: **6UTB**

Solvent(
Aceton


Weight(s) shown below were combined and diluted to (mL): **100.0**
 5E-05 Balance Uncertainty
 0.057 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight (g)
1. Aroclor 1232	17	45-6A	100	100	0.5	0.01000

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measure Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stonier
 Column ID SPB-608 30 meter X 0.53mm X 5 μm film thickness
 Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
 Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
 Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
 Rate = 8°C/min, Total run time = 35 min
 Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
 Standard injection = 1.5 μL , Range=3






110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32009 **Lot No.:** A0203672

Description: Aroclor® 1242 Standard

Aroclor® 1242 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

p12928

→

p12932

AJ

12/27/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Aroclor 1242	53469-21-9	01141	—%	1,004.7 µg/mL	+/- 55.7515

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Boothamer

Russ Boothamer - Operations Technician I

Date Mixed: 26-Oct-2023

Balance Serial #

B442140311

Jennifer Polino

Jennifer Polino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32010 **Lot No.:** A0202803

Description: Aroclor® 1248 Standard

Aroclor® 1248 Standard 1,000µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P1219697
P1219697
A1
12104123

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1248	12672-29-6	13897600	---%	1,001.7 µg/mL	+/- 55.5850

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Laith Clemente
Laith Clemente - Operations Technician I

Date Mixed: 03-Oct-2023

Balance Serial # 1128360905

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty


Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3





Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

Weight(s) shown below were combined and diluted to (mL.):
200.0

Balance Uncertainty
0.010

Flask Uncertainty
0.010

SDS Information
(Solvent Safety Info. On Attached pg.)

Expanded Uncertainty
(+/-) (µg/mL)

Actual Conc (µg/mL)

Actual Weight(g)

Target Weight(g)

Purity (%)

Nominal Conc (µg/mL)

Lot Number

RM#

1. Aroclor 1016

15

020491JC

1000

100

0.2

0.20004

0.20060

1002.8

4.0

12674-11-2

N/A

2. Aroclor 1260

21

020491JC

1000

100

0.2

0.20004

0.20081

1003.9


4.0

11086-82-5

0.5mg/m3
orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3





CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

99139
121823
Aroclor 1254

Solvent(s):
Iso-octane

Lot#
82227

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

121833
Ambient (20 °C)
100
6UTB

Volume(s) shown below were combined and diluted to (mL):
Note: Aroclor 1254 is a mix of isomers.

5E-05
0.003
Balance Uncertainty
Flask Uncertainty

20.0
Dilution
Factor

Initial
Vol. (mL)

Uncertainty
Pipette (mL)

Initial
Conc. (µg/mL)

Final
Conc. (µg/mL)

Expanded
Uncertainty
(+/-) (µg/mL)

1.8
11097-69-1

0.5mg/m3 (skin)

orl-rat 1295mg/kg

Formulated By: Anthony Mahoney
Reviewed By: Pedro L. Rentas

121823
DATE

121823
DATE


SDS Information
(Solvent Safety Info. On Attached pg.)
CAS# OSHA PEL (TWA) LD50

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1254	79100	121823	0.10	2.00	0.017	1003.3	100.1	1.8	11097-69-1	0.5mg/m3 (skin)	orl-rat 1295mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X 5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150 °C (Time 1 = 4 min), Temp 2 = 250 °C (Time 2 = 13.5 min)
Rate = 8 °C/min, Total run time = 35 min
Injector temp. = 200 °C, FID Temp. = 300 °C, FID Signal = Etdaq Channel 1
Standard injection = 1.5µL, Range=3

Peak No.	Name	FID RT (min.)
1	Total Aroclor 1254	18.12





CERTIFIED WEIGHT REPORT

Part Number: 90165
Lot Number: 112322
Description: Atrocior 1262
Expiration Date: 112332
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 6LUTB
Weight(s) shown were combined and diluted to (mL): 50.0

Solvent(s): Hexane
Lot# 273615


SE-05 Balance Uncertainty
0.005 Flask Uncertainty

Formulated By:	Prashant Chauhan	112322	DATE
Reviewed By:	Pedro L. Rentes	112322	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	--------------------	-------------------	-------------------	---------------------	----------------------------------	------	----------------	------

1. Atrocior 1262 444 W-130-05 1000 100 0.2 0.05003 0.05016 1002.7 4.5 37324-23-5 N/A or-ral 11300mg/kg

Method GC/MSD-7.M: Column:(30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (0min.), Temp 2 = 290°C (12.5 min.), Rate = 8°C/min., Injector B = 200°C, Detector B = 290°C.



- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




Run 20, "P90165 L112322 [1000µg/mL in hexane]"

Run Length: 35.00 min, 21000 points at 10 points/second.
Created: Thu, Dec 8, 2022 at 2:31:02 AM.
Sampled: Sequence "120722-GC3M1", Method "GC3-M1".
Analyzed using Method "GC3-M1".

Comments

GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
Standard injection = 1.5µL, Range=3





110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl




This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024

Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

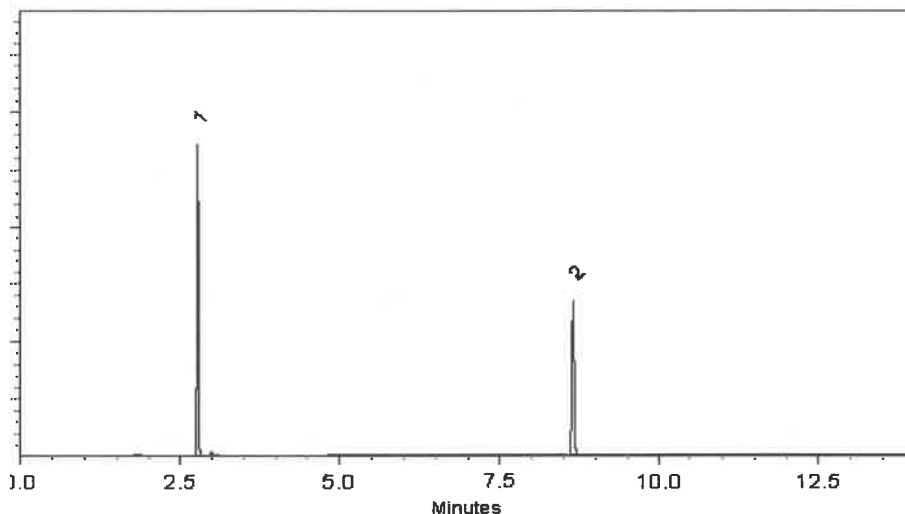


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



ISO 17034

Reference Material Certificate

Product Information Sheet

Product Name: Aroclor 1221 Standard
Product Number: PP-292-1
Storage Conditions: Store at Room Temperature (15° to 30°C).

Lot Number: 0006783205
Lot Issue Date: 20-Feb-2024
Expiration Date: 31-Mar-2032

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1221	100.3 ±	0.5 µg/mL	011104-28-2	NT01017

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13342
AJ
05106124
P13343

Page: 1 of 2

CSD-QA-015.2

ISO 17025
Cert No. AT-1937


250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.2

ISO 17025
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



SHIPPING DOCUMENTS

CLIENT INFORMATION

REPORT TO BE SENT TO:
COMPANY: **Geop Inc**
ADDRESS: **8 CARRIAGE**
CITY: **Succasunna** STATE: **NJ** ZIP: **07876**
ATTENTION:
PHONE: FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME: **Ave L**
PROJECT NO.: LOCATION:
PROJECT MANAGER: **GL**
e-mail:
PHONE: FAX:

CLIENT BILLING INFORMATION

BILL TO: **Geop Inc** PO#:
ADDRESS: **8 CARRIAGE**
CITY: **Succasunna** STATE: **NJ** ZIP: **07876**
ATTENTION: PHONE:
ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) DAYS*
HARDCOPY (DATA PACKAGE): **STANDARD** DAYS*
EDD: DAYS*
*TO BE APPROVED BY CHEMTECH
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☐ Level 2 (Results + QC) ☒ NJ Reduced ☐ US EPA CLP
☐ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
+ Raw Data ☐ Other
☒ EDD FORMAT **add meta excel**

TECP metals
THL metals
PCRA
VOC
BTEX
PCB
PH / Isotobility
EPH

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									COMMENTS
			COMP	GRAB	DATE	TIME		1	2	3	4	5	6	7	8	9	
1.	WC1	501	X		3/13/25	1255	2	X	X	X	X	X	X	X	X		
2.																	
3.																	
4.																	
5.																	
6.																	
7.																	
8.																	
9.																	
10.																	

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER: 1. [Signature]	DATE/TIME: 3/14/25 1110	RECEIVED BY: [Signature]	Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP 2.1°C
RELINQUISHED BY SAMPLER: 2.	DATE/TIME:	RECEIVED BY: 2.	Comments:
RELINQUISHED BY SAMPLER: 3.	DATE/TIME:	RECEIVED BY: 3.	Page ____ of
			CLIENT: ☐ Hand Delivered ☐ Other
			Shipment Complete ☐ YES ☐ NO

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q1574 GENV01
Client Name : G Environmental
Client Contact : Gary Landis
Invoice Name : G Environmental
Invoice Contact : Gary Landis

Order Date : 3/14/2025 11:25:00 AM
Project Name : Ave L
Receive DateTime : 3/14/2025 3:00:00 PM
Purchase Order :

Project Mgr :
Report Type : ~~Level 1~~ *Results only*
EDD Type : Excel NJ
Hard Copy Date :
Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q1574-01	WC1	Solid	03/12/2025	12:55	VOC-TCLVOA-10		8260D		10 Bus. Days

Relinquished By : 

Date / Time : 3/14/25 11:50

Received By : 

Date / Time : 3/14/25 11:50

Storage Area : VOA Refridgerator Room