
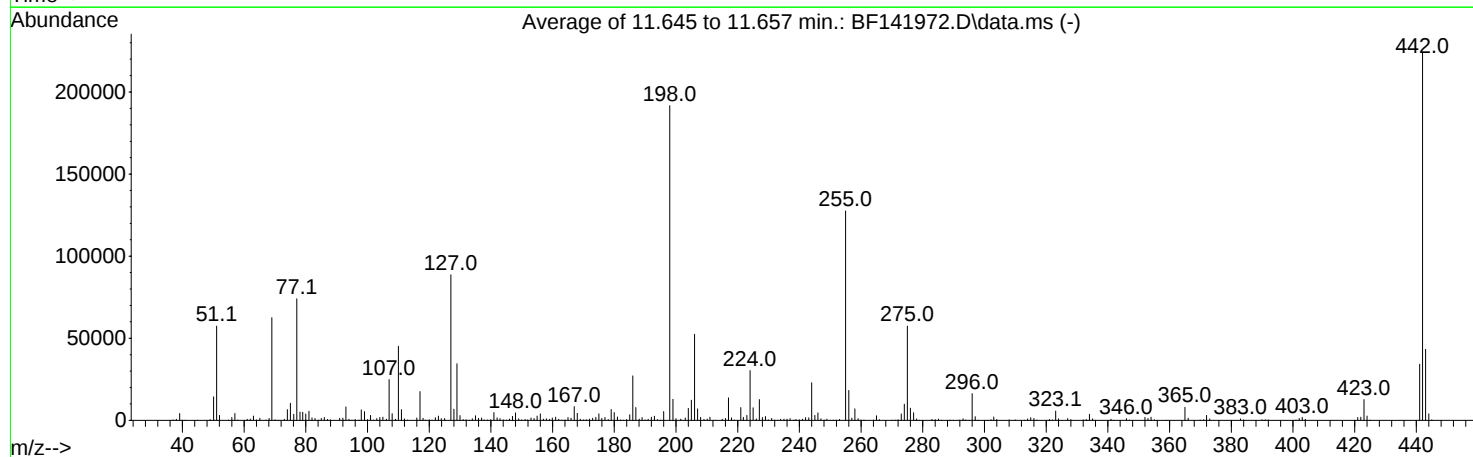


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031725\
Data File : BF141972.D
Acq On : 17 Mar 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

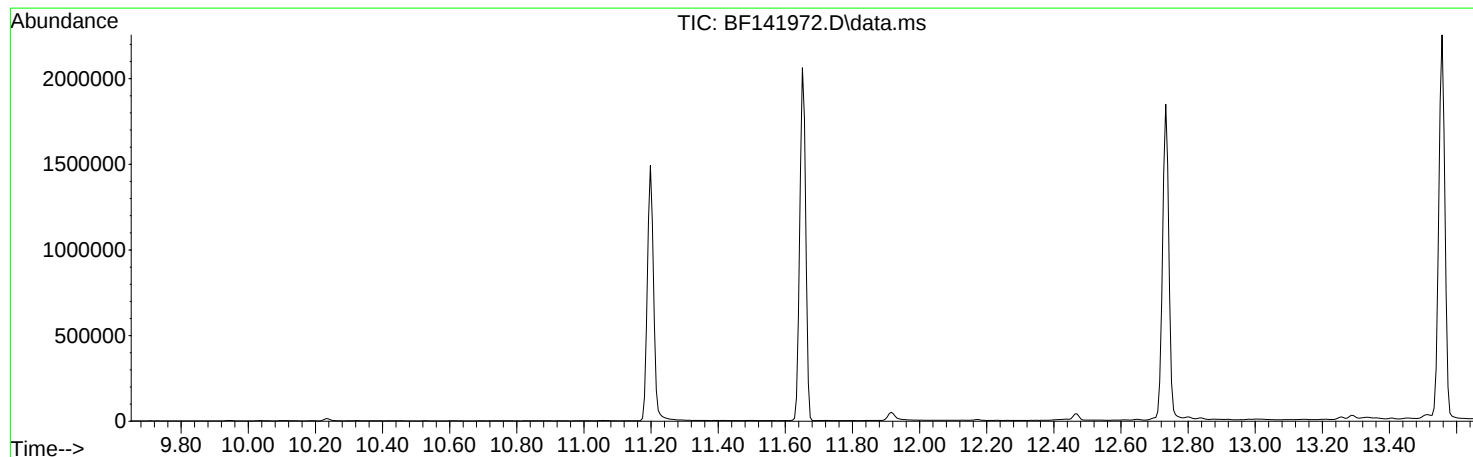

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	57448	PASS
68	69	0.00	2	1.9	1189	PASS
69	198	0.00	100	32.6	62535	PASS
70	69	0.00	2	0.6	365	PASS
127	198	10	80	46.3	88696	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	191723	PASS
199	198	5	9	6.7	12824	PASS
275	198	10	60	30.0	57427	PASS
365	198	1	100	4.2	7964	PASS
441	198	0.01	100	17.9	34259	PASS
442	442	50	100	100.0	224043	PASS
443	442	15	24	19.3	43256	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/17/2025	BNA_F	<u>BF141972.D</u>
Compound Name	Response	Retention Time
DDT	573929	13.557
DDD	10461	13.286
DDE	591	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11052	584981	1.89

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031725\
Data File : BF141972.D
Acq On : 17 Mar 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 17 11:52:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

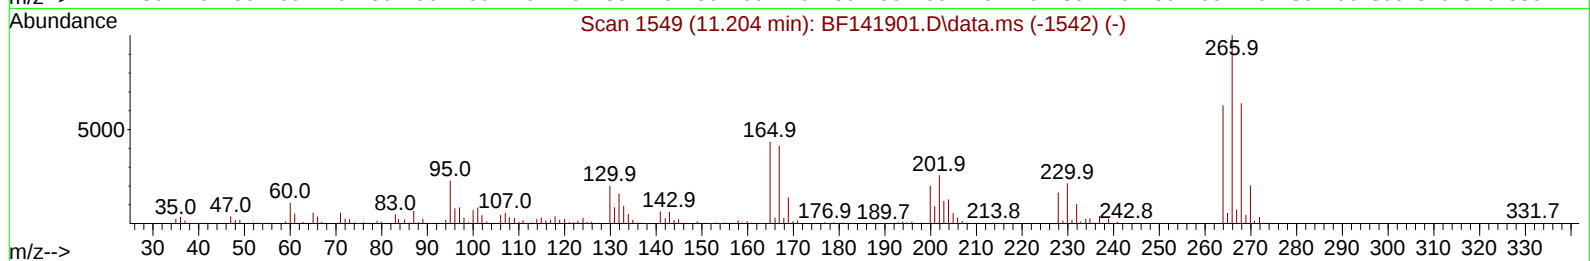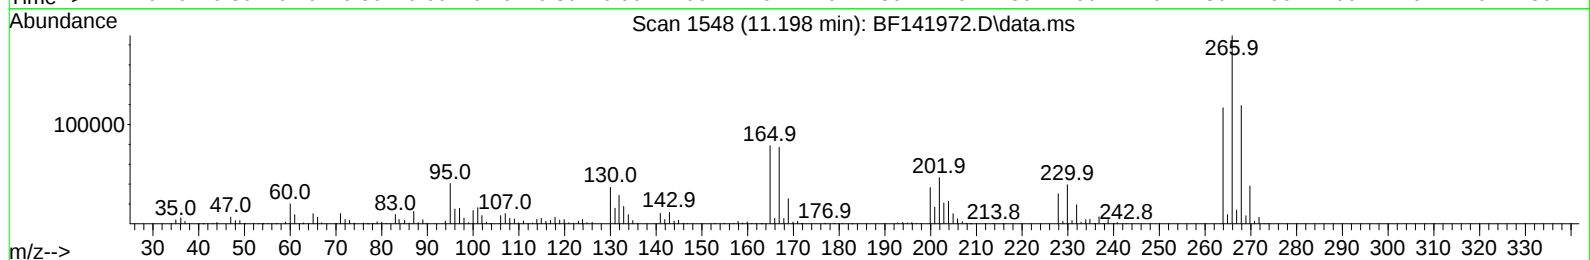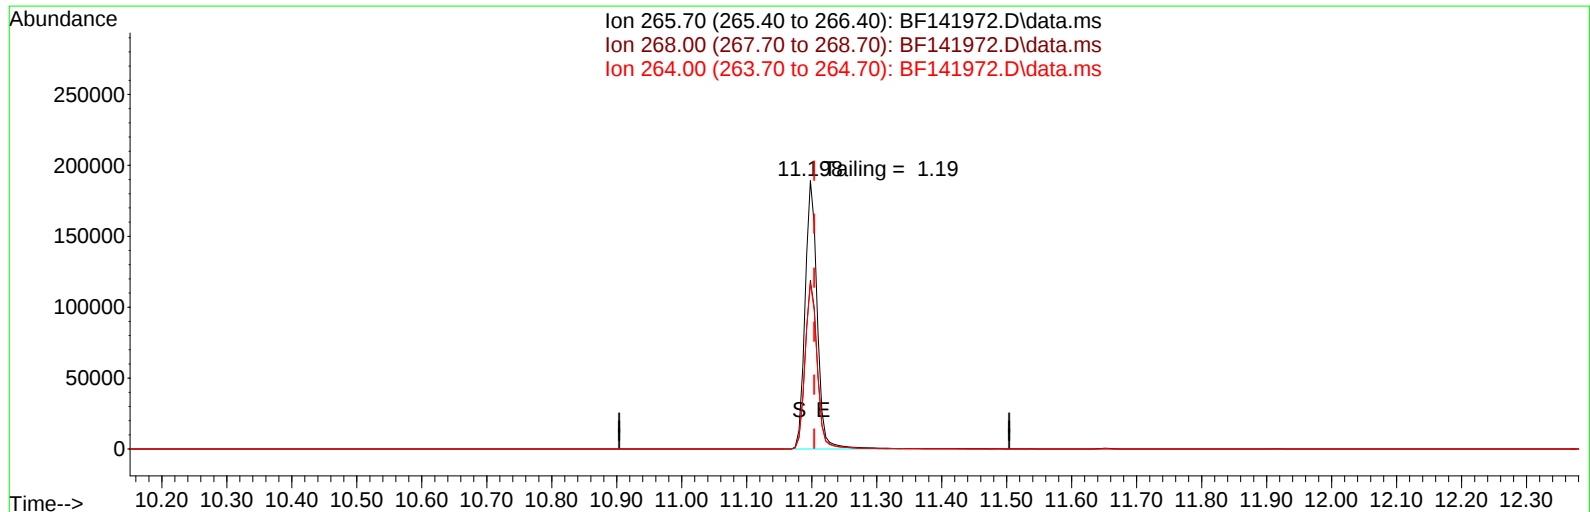

TIC: BF141972.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 60186.83 ng




response 248242

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.83
264.00	62.70	61.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031725\
Data File : BF141972.D
Acq On : 17 Mar 2025 09:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 17 11:52:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

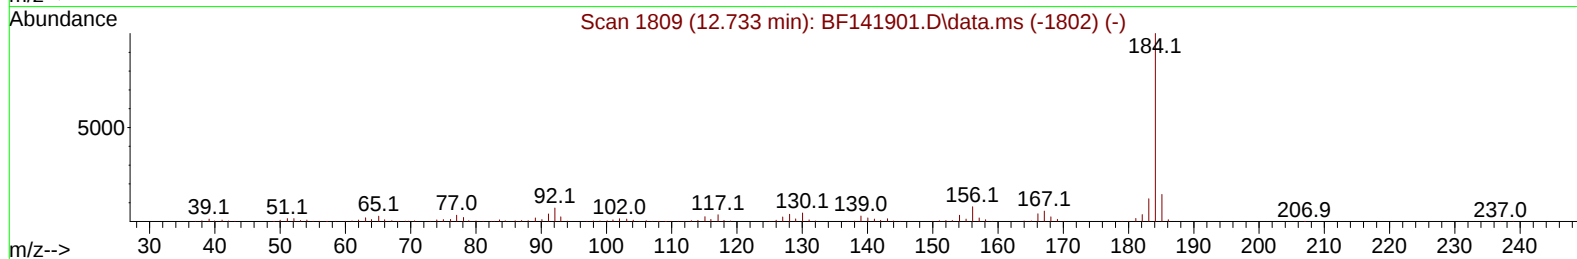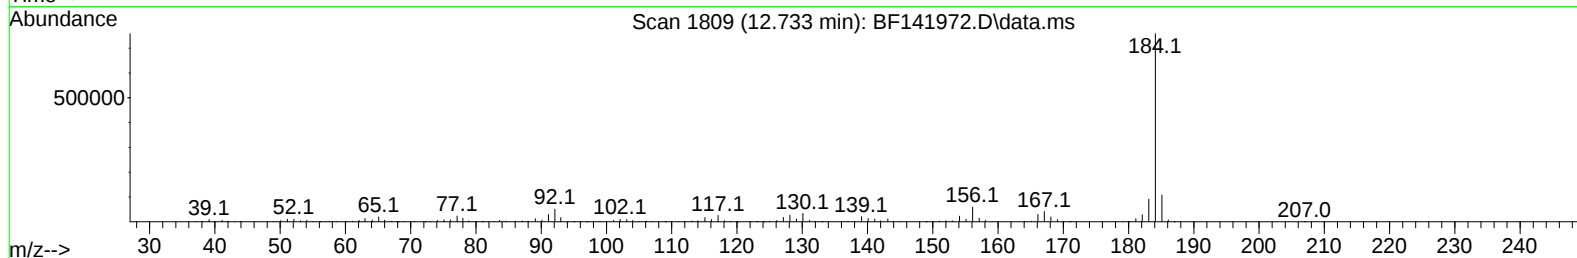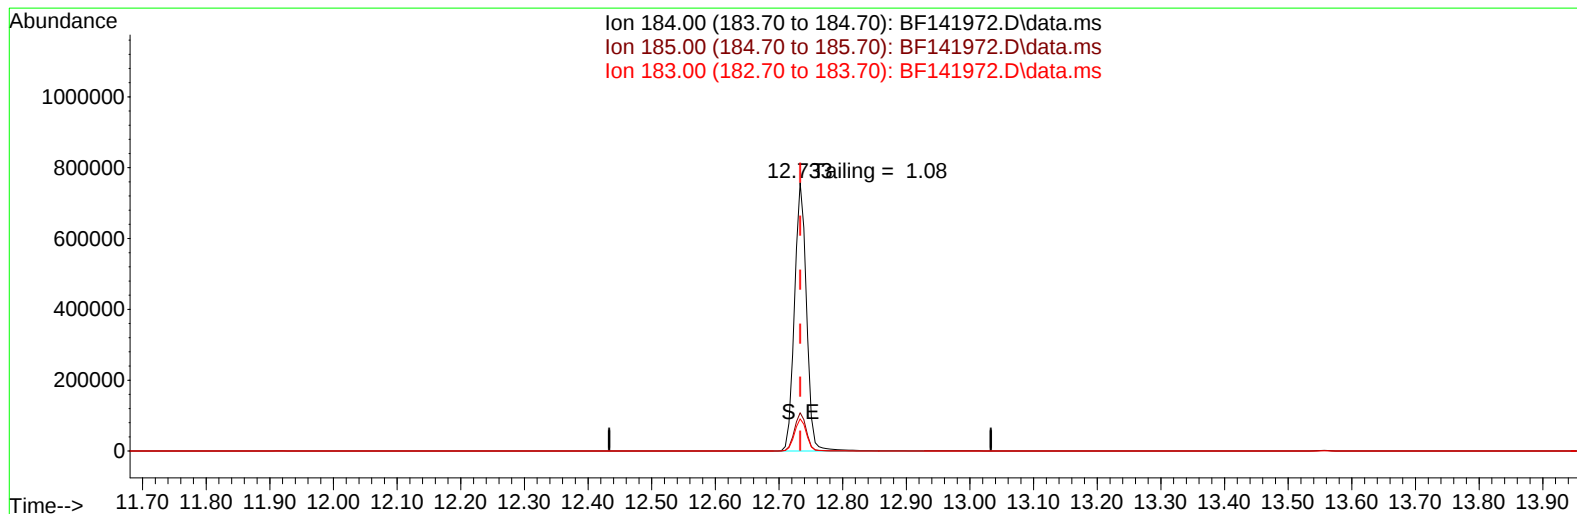

TIC: BF141972.D\data.ms

(77) Benzidine

12.733min (0.000) 175178.85 ng

response 1002071

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.27
183.00	12.10	12.01
0.00	0.00	0.00