
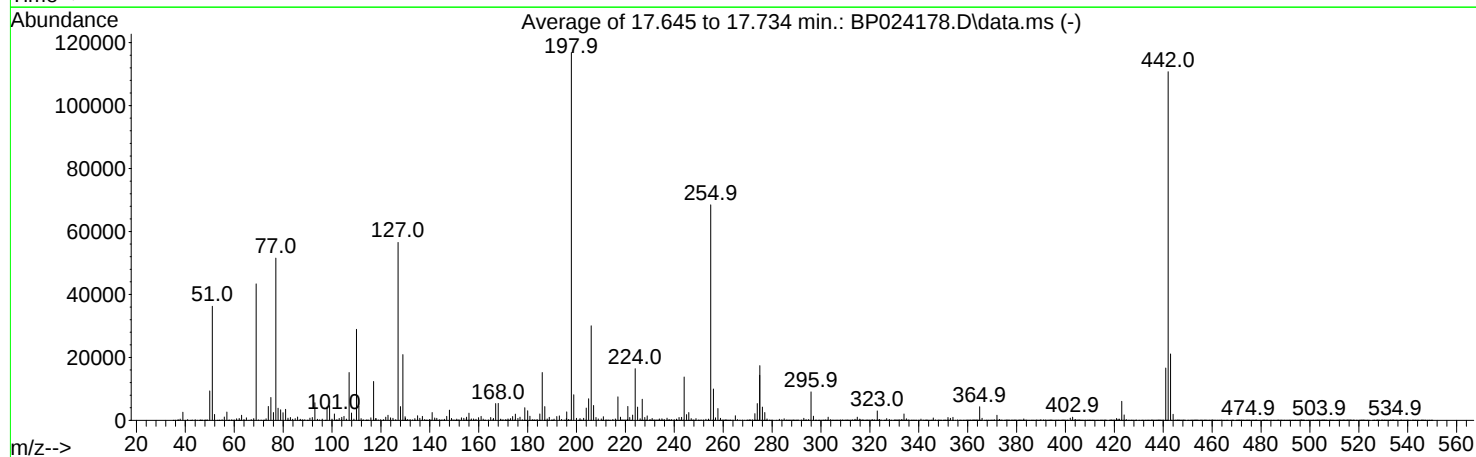


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031825\
Data File : BP024178.D
Acq On : 18 Mar 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\625.1-Tune.M
Title : D
Last Update : Wed Oct 07 11:38:17 2020

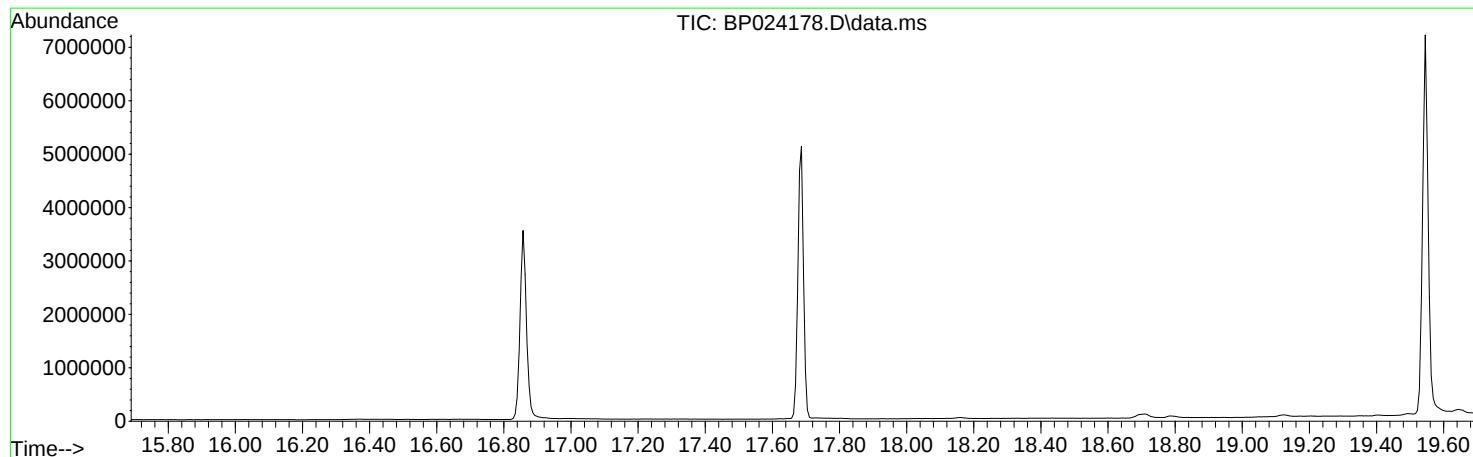




AutoFind: Averaged scan 2475 to 2490; Bkg corrected with scan 2474

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	30	60	31.0	36256	PASS
68	69	0.00	2	1.3	585	PASS
69	69	100	100	100.0	43346	PASS
70	69	0.00	2	0.4	167	PASS
127	198	40	60	48.4	56551	PASS
197	198	0.00	1	0.2	289	PASS
198	198	100	100	100.0	116867	PASS
199	198	5	9	6.9	8120	PASS
275	198	10	30	14.9	17386	PASS
365	198	1	100	3.7	4317	PASS
441	443	0.01	100	78.8	16620	PASS
442	198	40	100	94.8	110745	PASS
443	442	17	23	19.1	21104	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031825\
Data File : BP024178.D
Acq On : 18 Mar 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 18 11:07:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

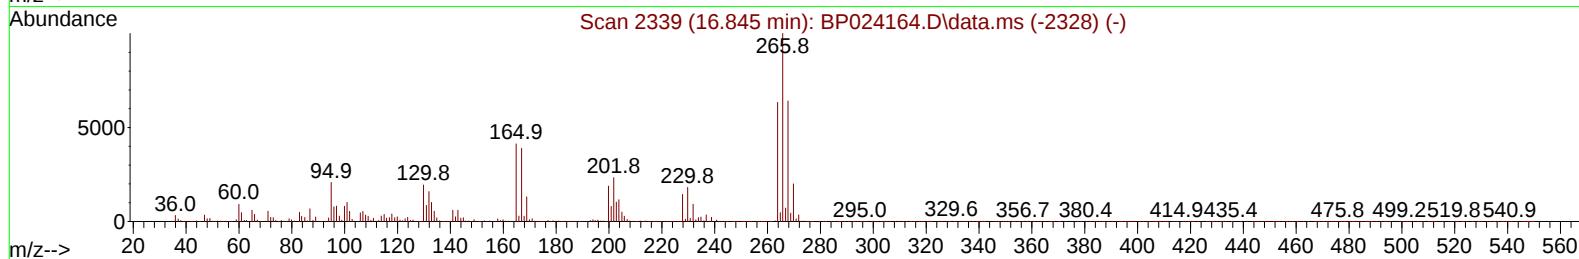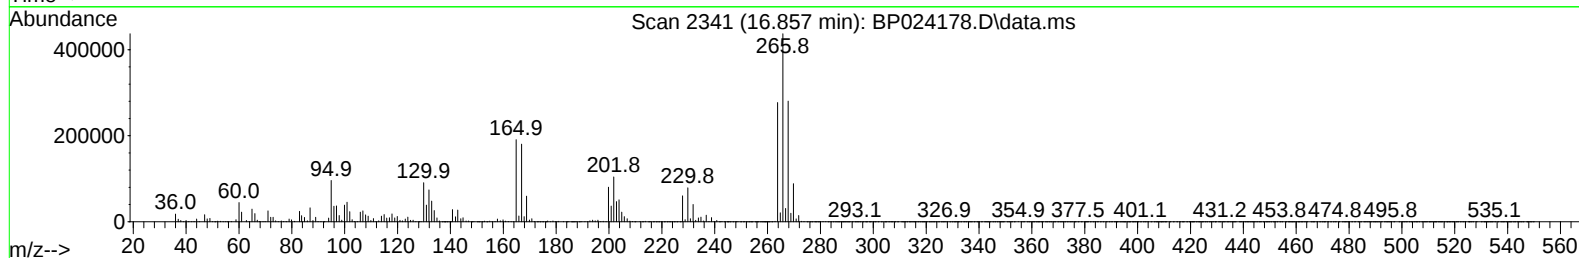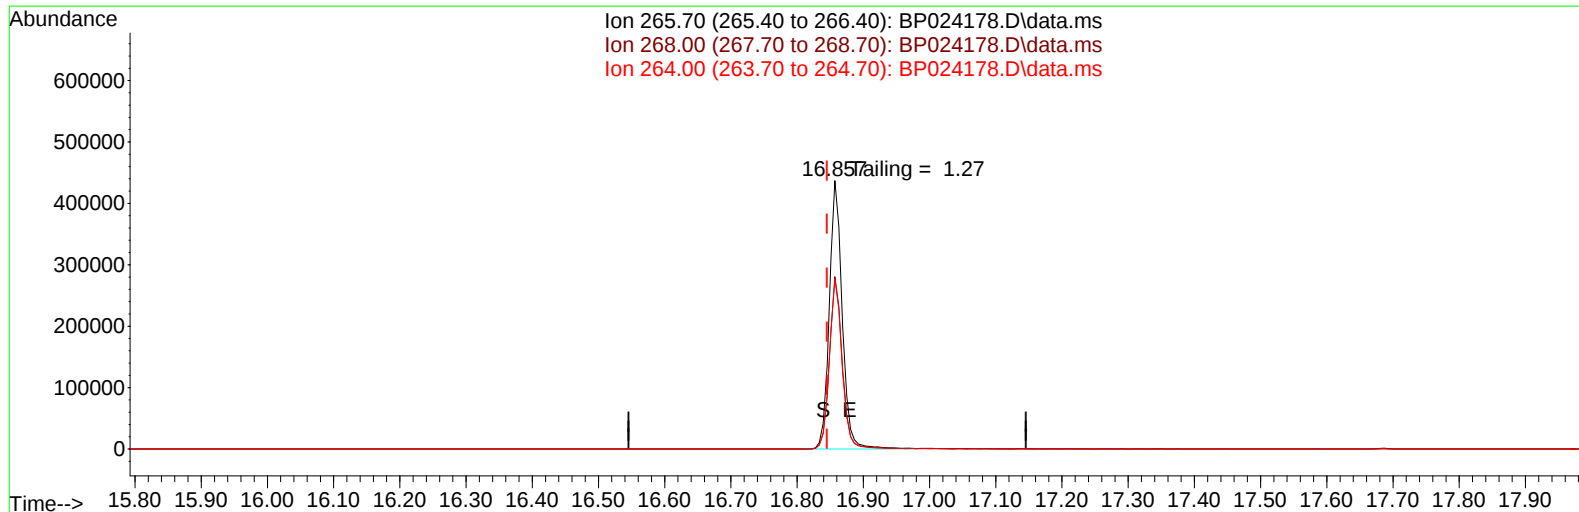

TIC: BP024178.D\data.ms

(70) Pentachlorophenol (C)

16.857min (+ 0.012) 196786.88 ng




response 593684

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.20
264.00	63.30	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031825\
Data File : BP024178.D
Acq On : 18 Mar 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 18 14:43:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

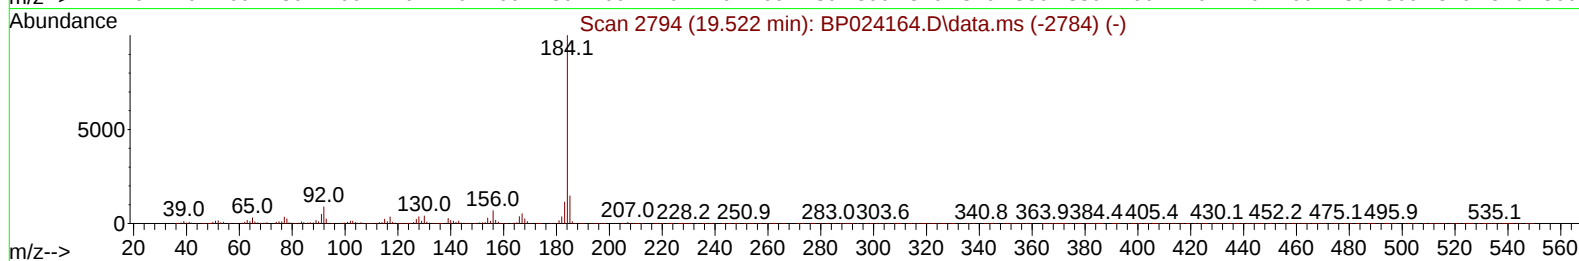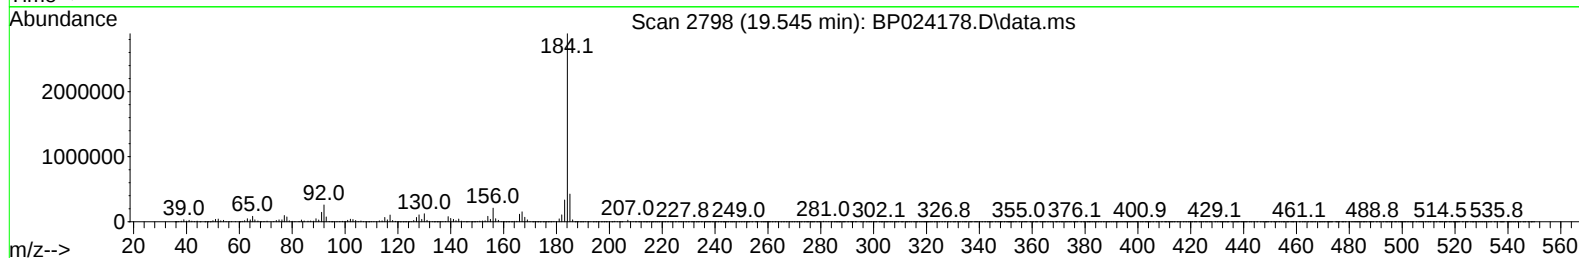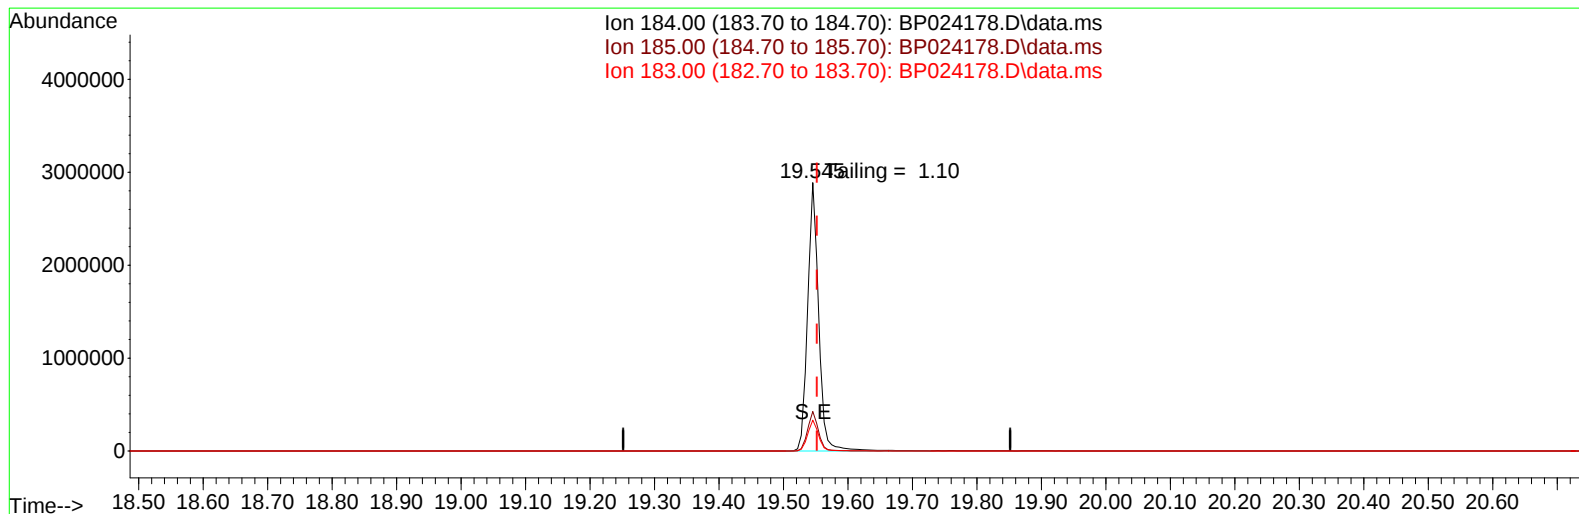

TIC: BP024178.D\data.ms

(77) Benzidine

19.545min (-0.006) 19199.87 ng

response 3449621

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.74
183.00	11.40	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/18/2025	BNA_P	<u>BP024178.D</u>
Compound Name	Response	Retention Time
DDT	1637732	20.845
DDD	20127	20.439
DDE	2174	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22301	1660033	1.34

Instrument :
BNA_P
ClientSampleId :
DFTPP