
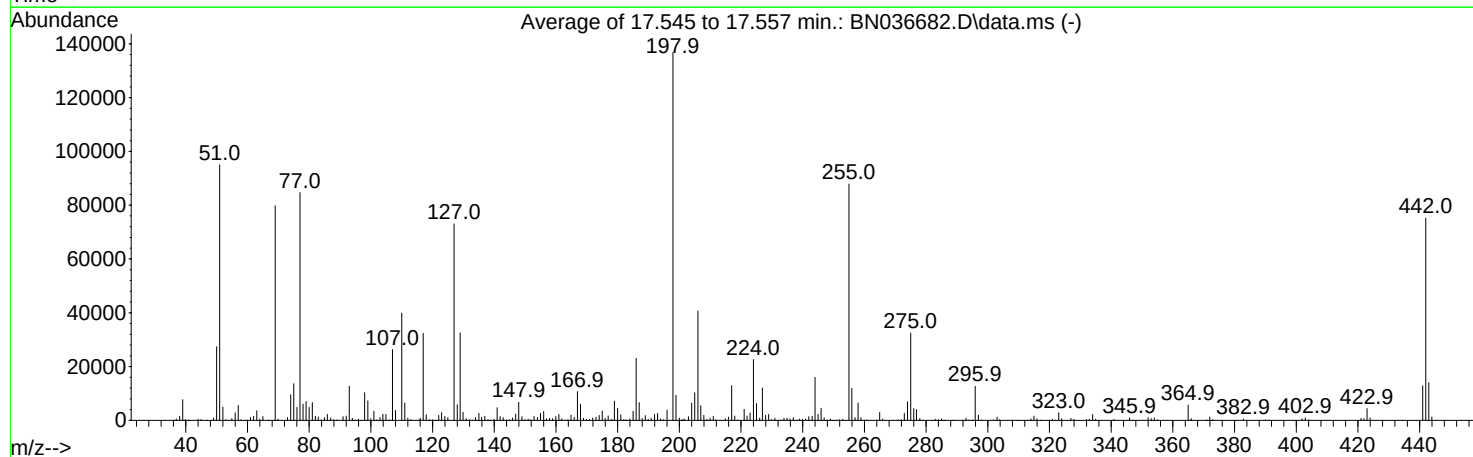


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031825\
Data File : BN036682.D
Acq On : 18 Mar 2025 08:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

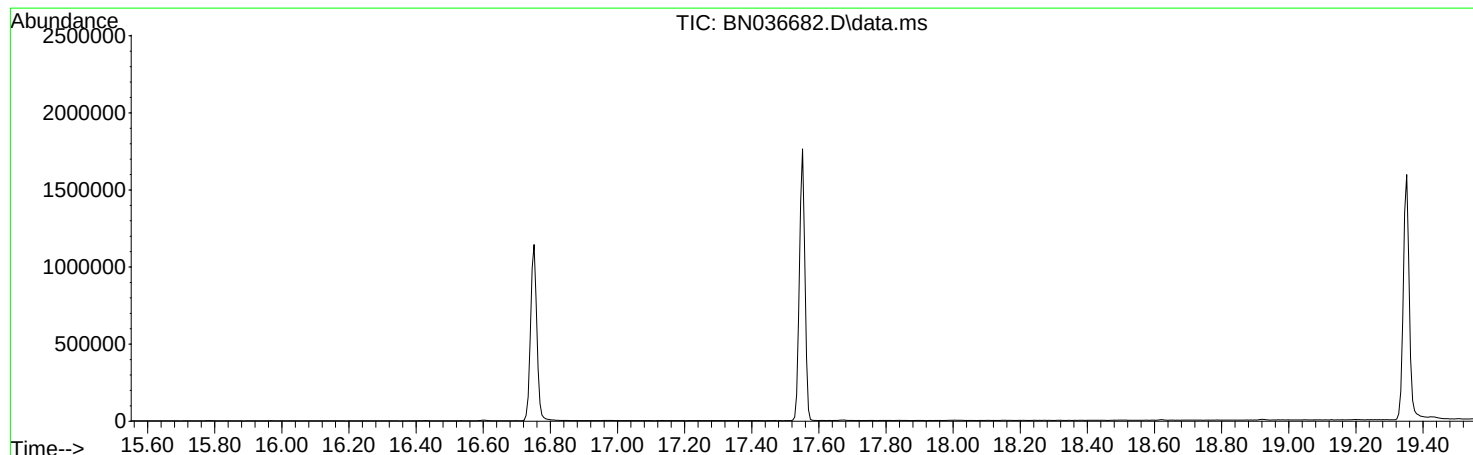




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.5	95037	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	58.3	79763	PASS
70	69	0.00	2	0.6	478	PASS
127	198	10	80	53.4	73040	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	136773	PASS
199	198	5	9	6.8	9344	PASS
275	198	10	60	23.7	32411	PASS
365	198	1	100	4.2	5709	PASS
441	198	0.01	100	9.4	12840	PASS
442	442	50	100	100.0	75131	PASS
443	442	15	24	18.7	14045	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031825\
Data File : BN036682.D
Acq On : 18 Mar 2025 08:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 18 13:19:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 18 01:27:23 2025
Response via : Initial Calibration

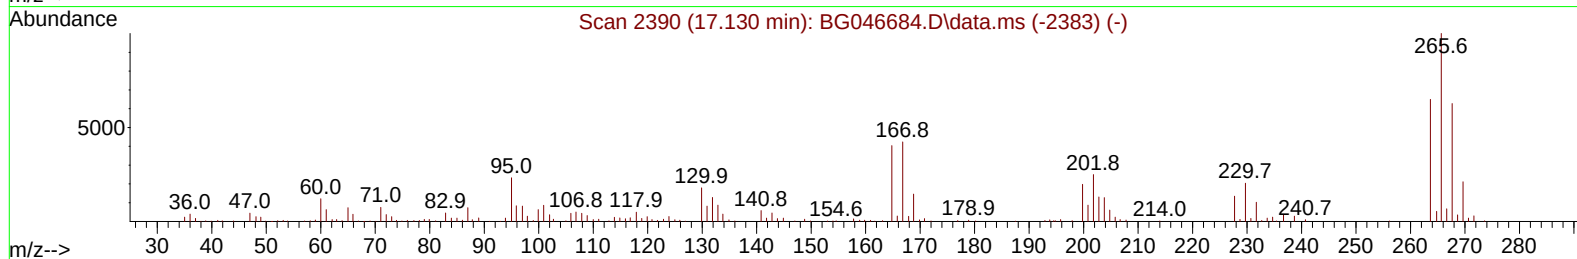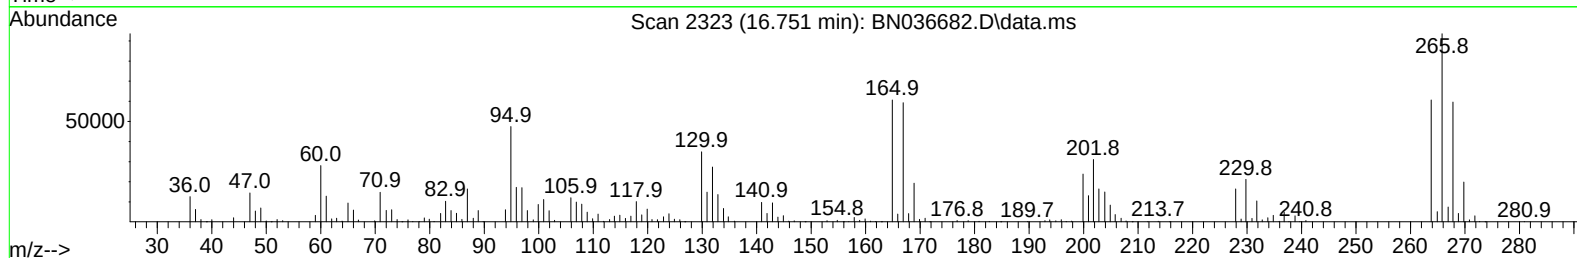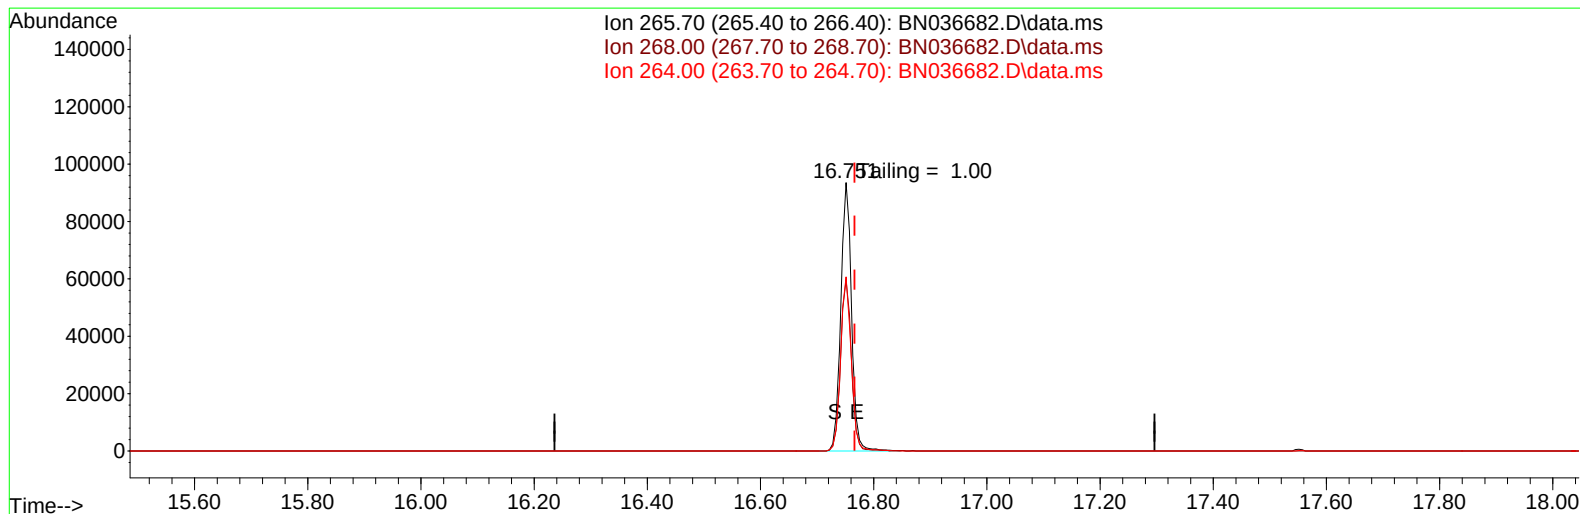

TIC: BN036682.D\data.ms

(70) Pentachlorophenol (C)

16.751min (-0.015) 15755.93 ng




response 123154

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.71
264.00	61.60	64.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN031825\
Data File : BN036682.D
Acq On : 18 Mar 2025 08:42
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 18 13:19:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 18 01:27:23 2025
Response via : Initial Calibration

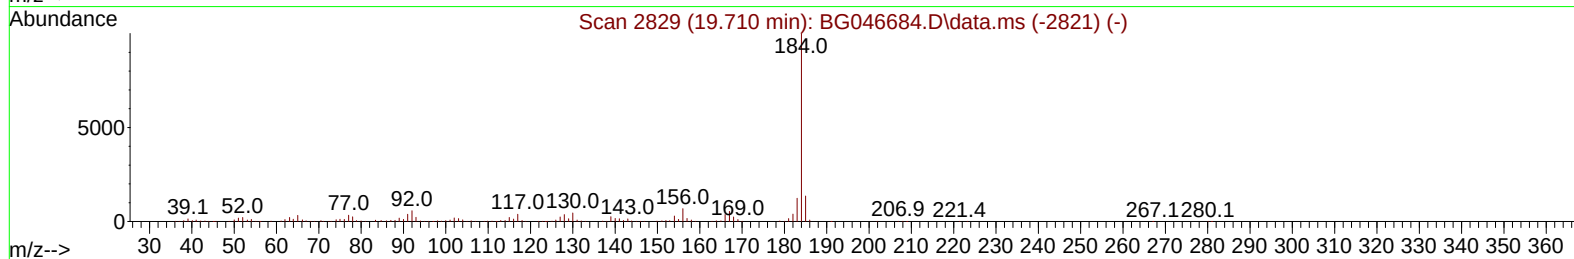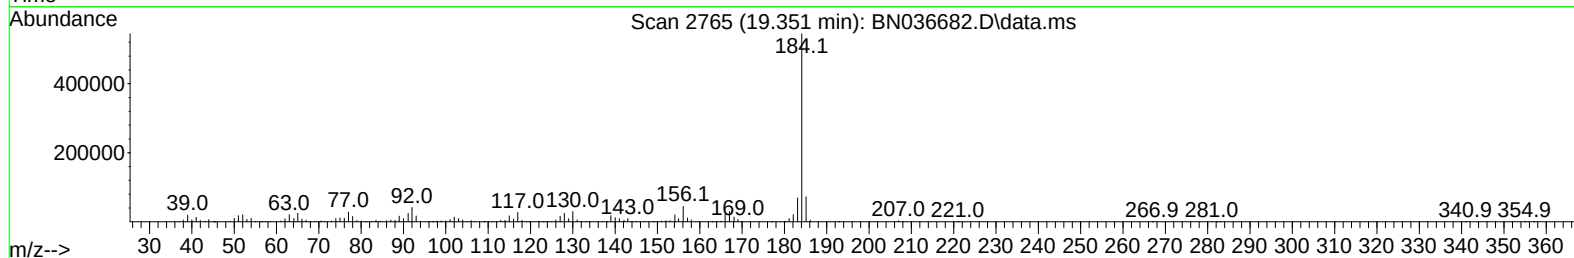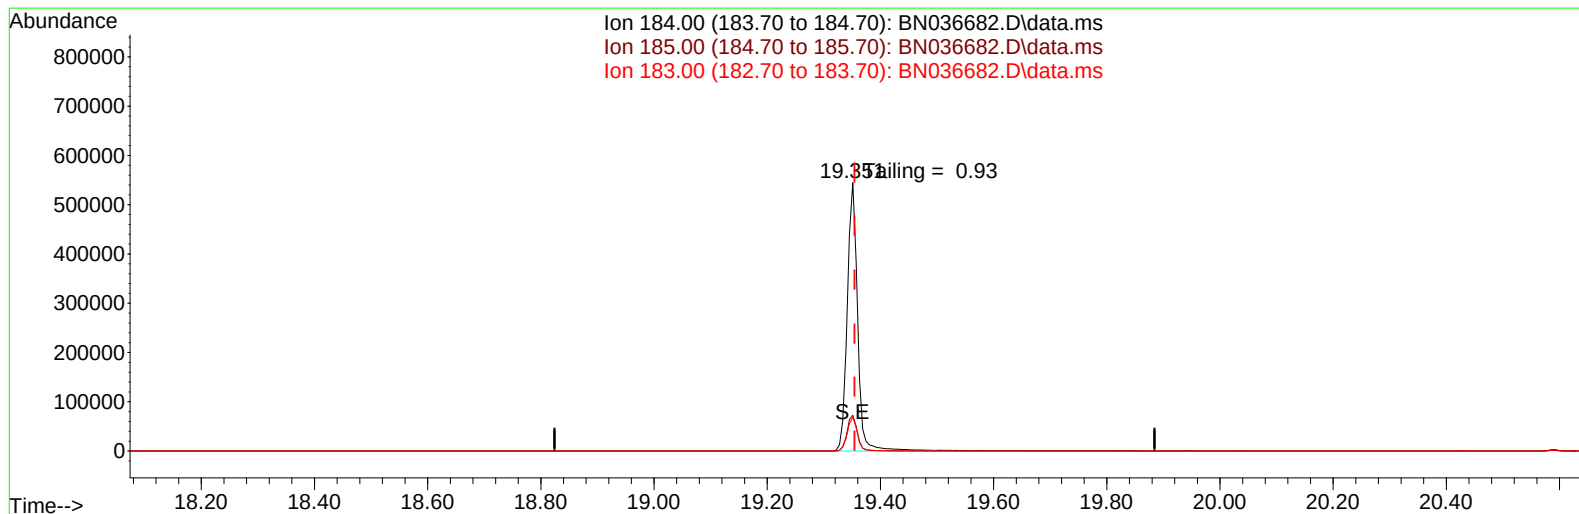

TIC: BN036682.D\data.ms

(77) Benzidine

19.351min (-0.003) 0.00 ng

response 688778

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.35
183.00	13.20	12.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/18/2025	BNA_N	<u>BN036682.D</u>
Compound Name	Response	Retention Time
DDT	424064	20.592
DDD	5924	20.151
DDE	402	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6326	430390	1.47

Instrument :
BNA_N
ClientSampleId :
DFTPP