



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX022125\
Data File : VX045007.D
Acq On : 21 Feb 2025 09:31
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X022125W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Feb 22 01:06:36 2025

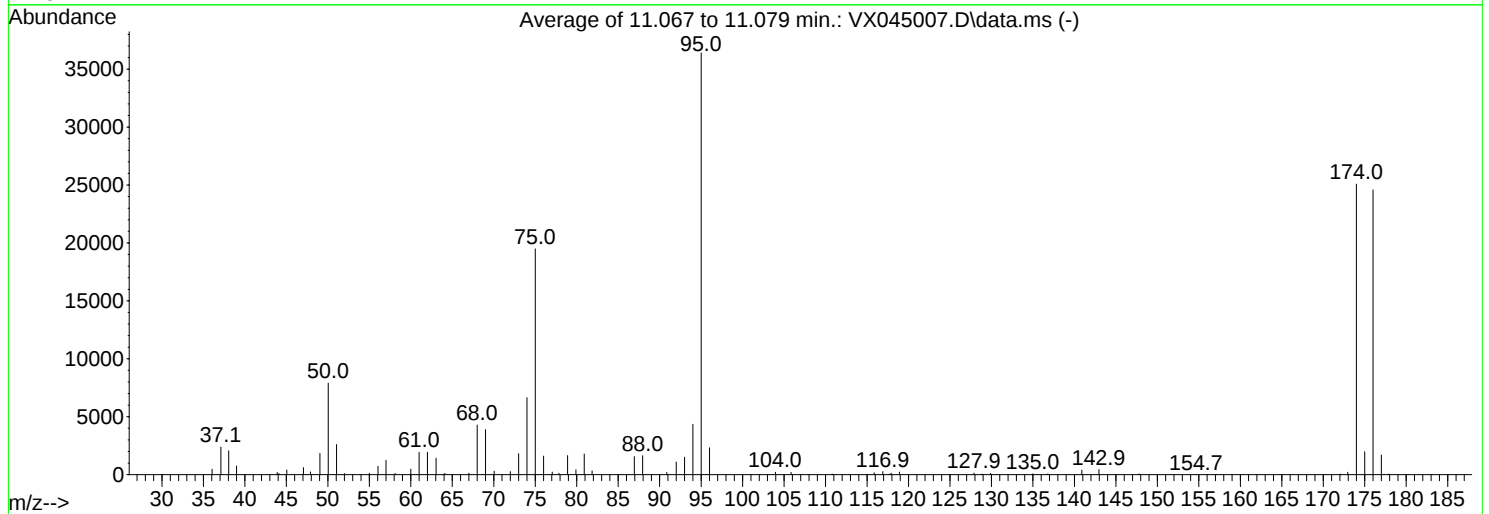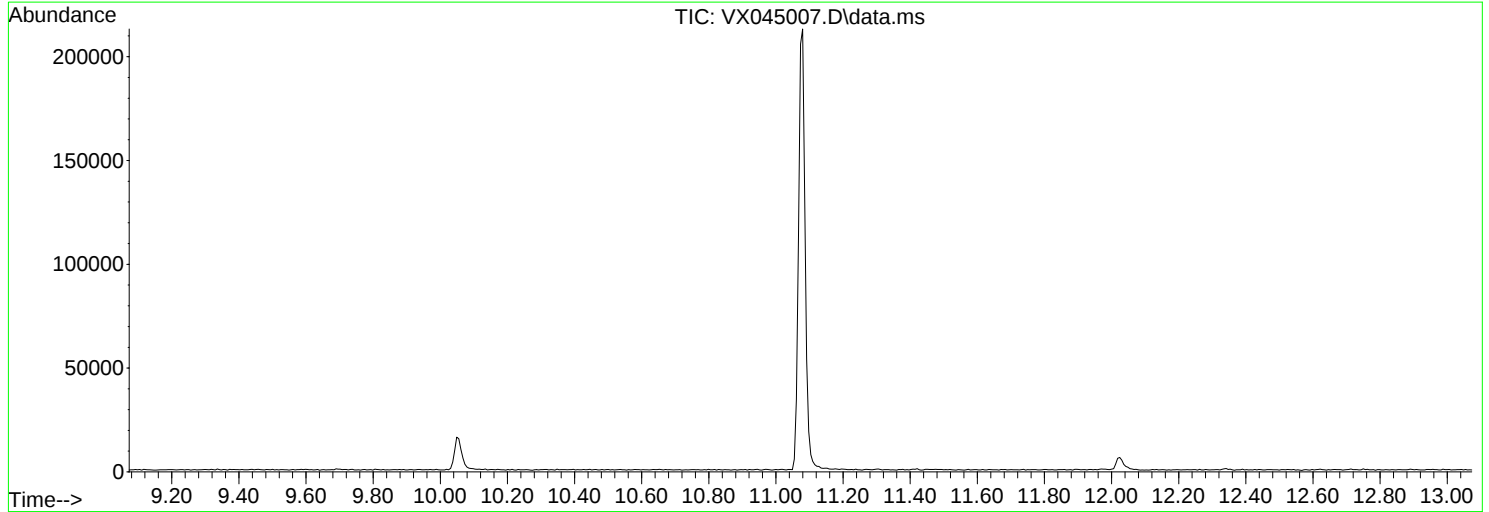

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	7903	PASS
75	95	30	60	53.5	19493	PASS
95	95	100	100	100.0	36408	PASS
96	95	5	9	6.4	2318	PASS
173	174	0.00	2	0.8	213	PASS
174	95	50	100	68.9	25081	PASS
175	174	5	9	7.9	1979	PASS
176	174	95	101	98.0	24589	PASS
177	176	5	9	6.9	1695	PASS