


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX031425\  
Data File : VX045284.D  
Acq On : 14 Mar 2025 09:28  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\624X022125W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
Last Update : Sat Feb 22 01:06:36 2025

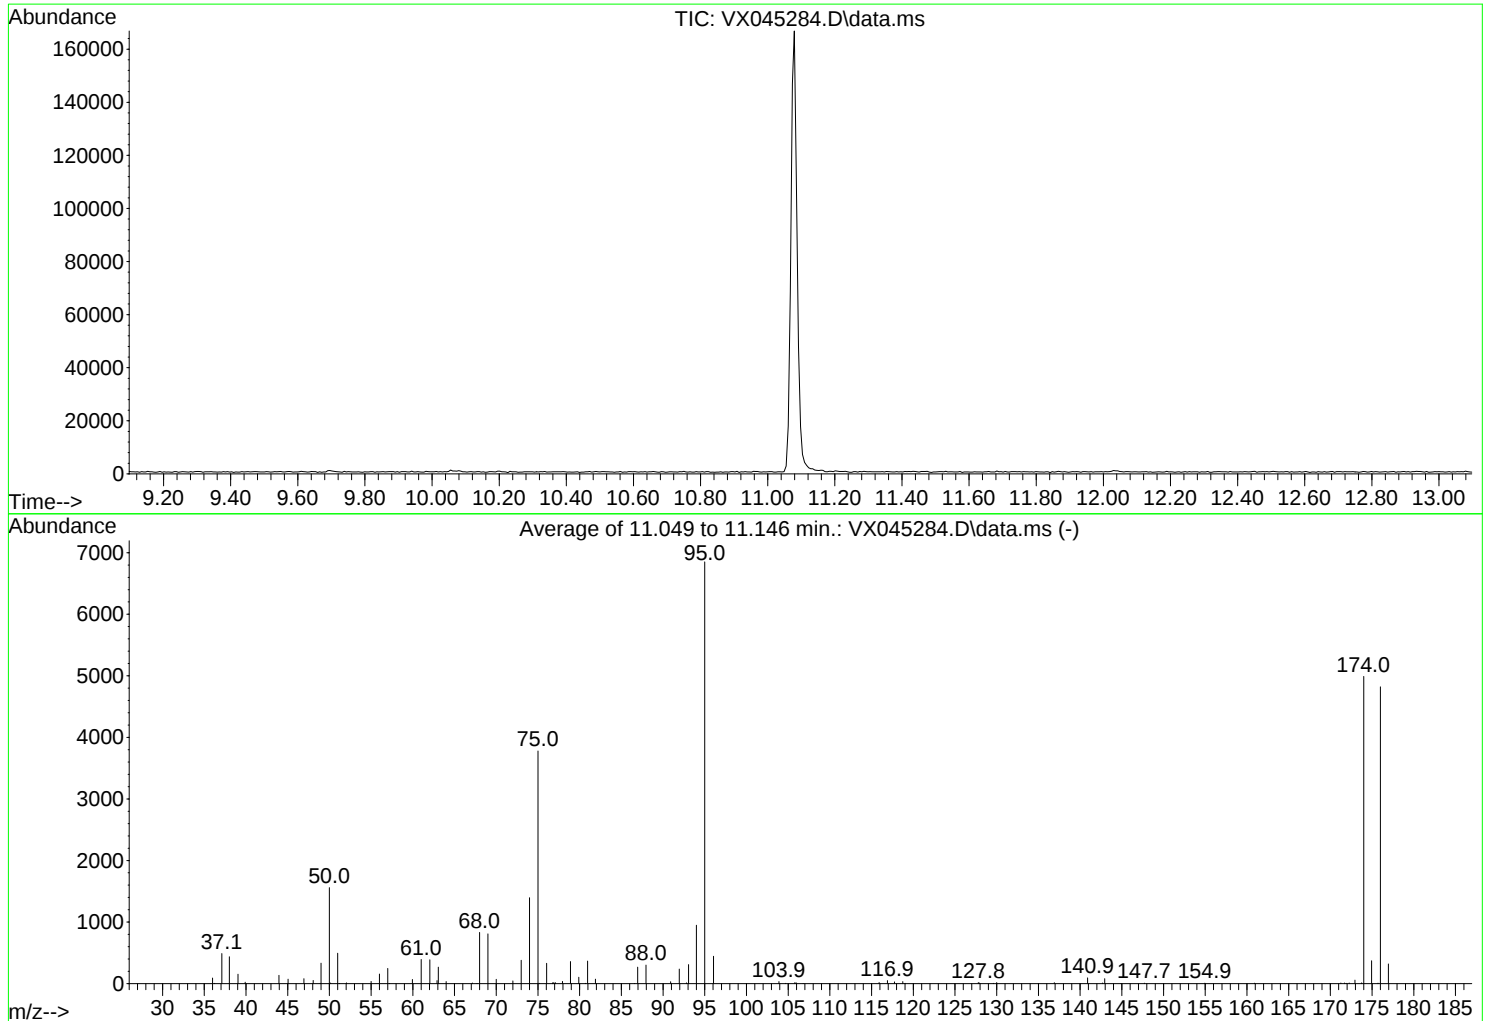

AutoFind: Averaged scan 1634 to 1650; Bkg corrected with scan 1633

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 22.8         | 1559       | PASS                |
| 75             | 95              | 30              | 60              | 55.2         | 3779       | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 6851       | PASS                |
| 96             | 95              | 5               | 9               | 6.5          | 445        | PASS                |
| 173            | 174             | 0.00            | 2               | 1.2          | 58         | PASS                |
| 174            | 95              | 50              | 100             | 72.8         | 4989       | PASS                |
| 175            | 174             | 5               | 9               | 7.4          | 371        | PASS                |
| 176            | 174             | 95              | 101             | 96.7         | 4822       | PASS                |
| 177            | 176             | 5               | 9               | 6.6          | 320        | PASS                |