
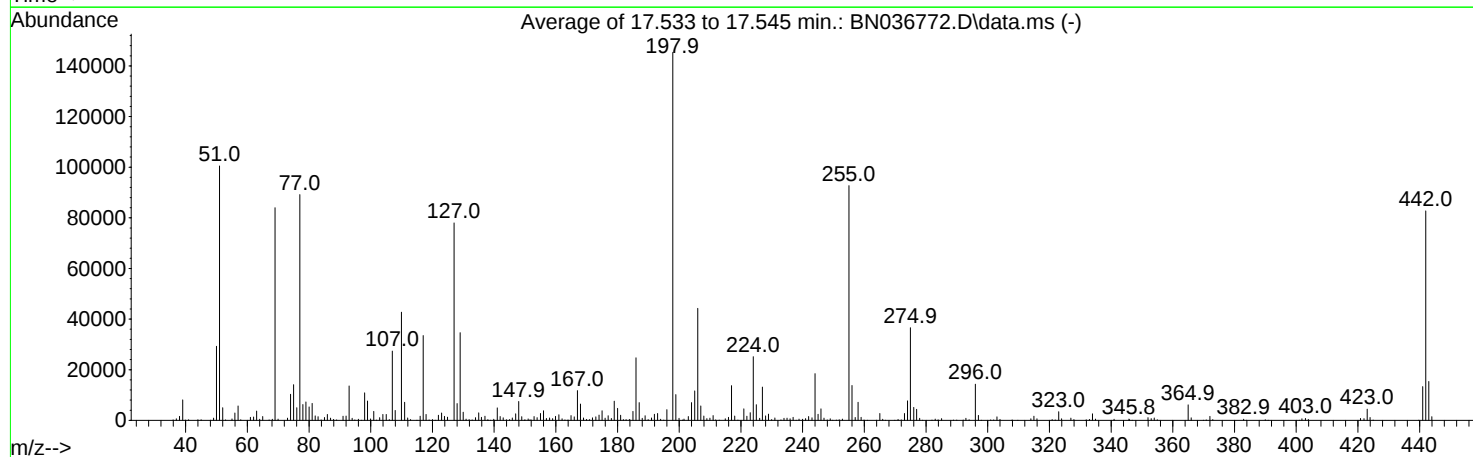


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032825\
Data File : BN036772.D
Acq On : 28 Mar 2025 14:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

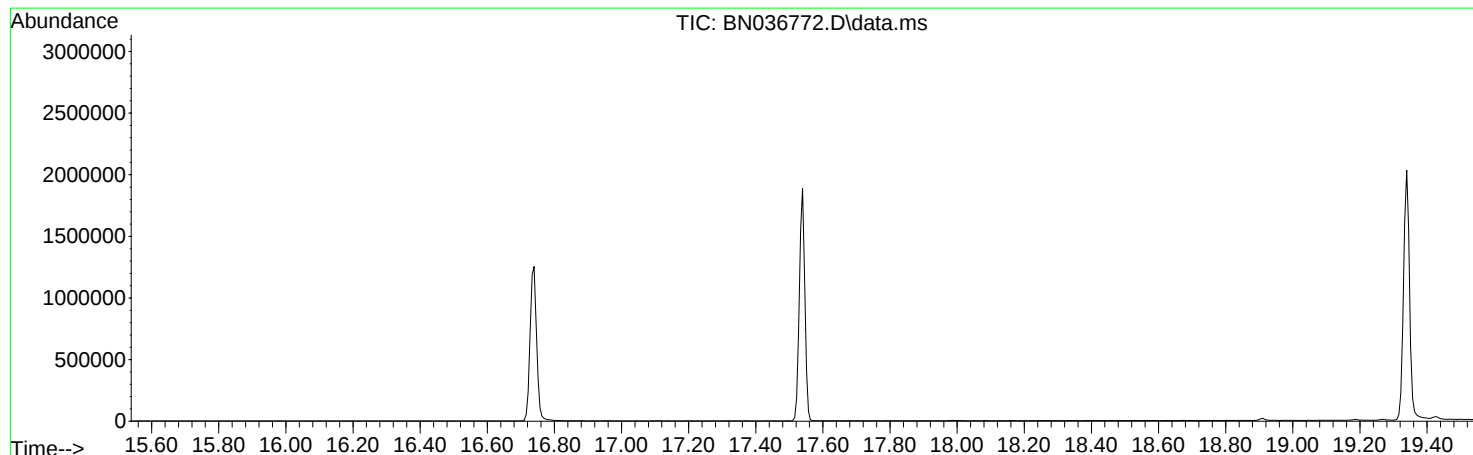




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.1	100475	PASS
68	69	0.00	2	0.6	462	PASS
69	198	0.00	100	57.8	83976	PASS
70	69	0.00	2	0.6	512	PASS
127	198	10	80	53.7	77968	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	145304	PASS
199	198	5	9	7.0	10186	PASS
275	198	10	60	25.2	36616	PASS
365	198	1	100	4.2	6164	PASS
441	198	0.01	100	9.2	13373	PASS
442	442	50	100	100.0	82744	PASS
443	442	15	24	18.6	15354	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032825\
Data File : BN036772.D
Acq On : 28 Mar 2025 14:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 29 04:37:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 29 04:33:53 2025
Response via : Initial Calibration

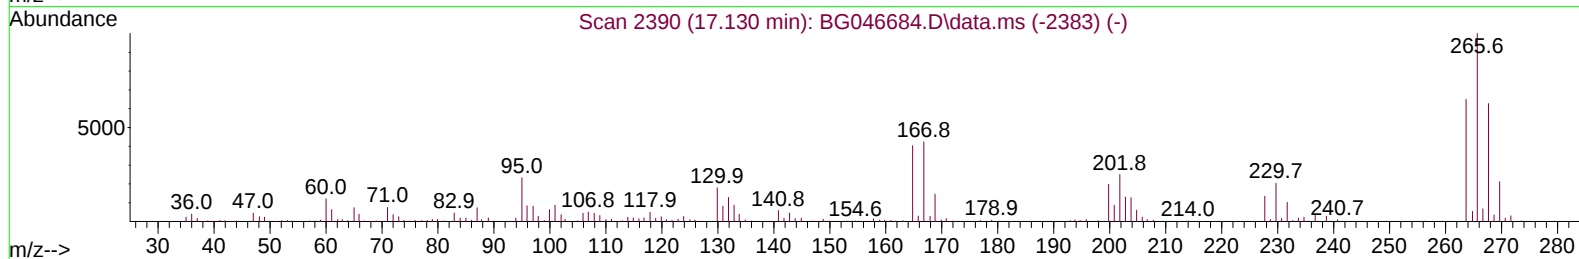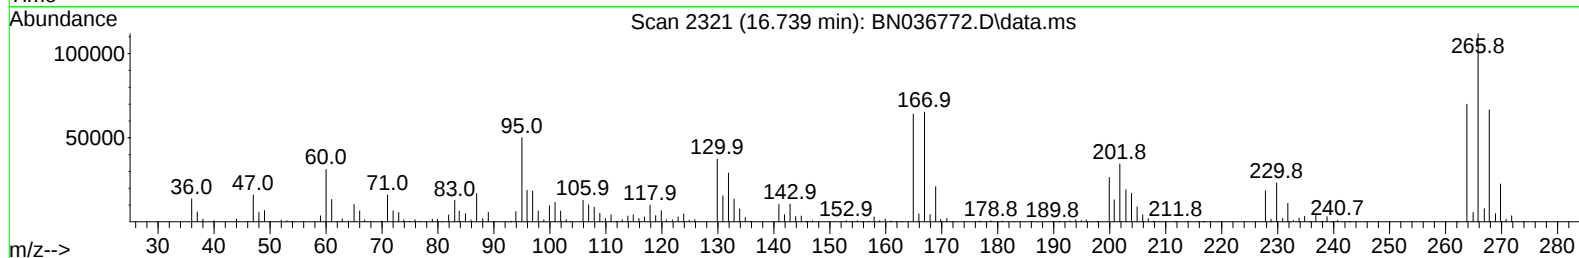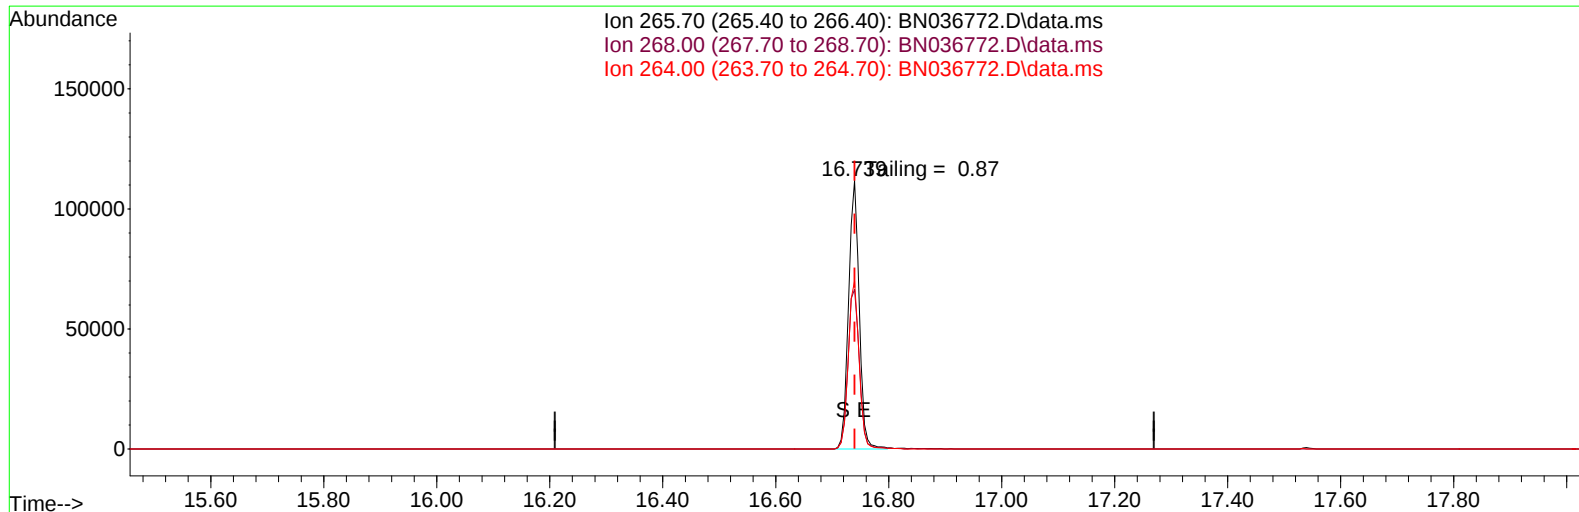

TIC: BN036772.D\data.ms

(70) Pentachlorophenol (C)

16.739min (-0.000) 17915.55 ng




response 146783

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.53
264.00	61.60	62.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032825\
Data File : BN036772.D
Acq On : 28 Mar 2025 14:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 29 04:37:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 29 04:33:53 2025
Response via : Initial Calibration

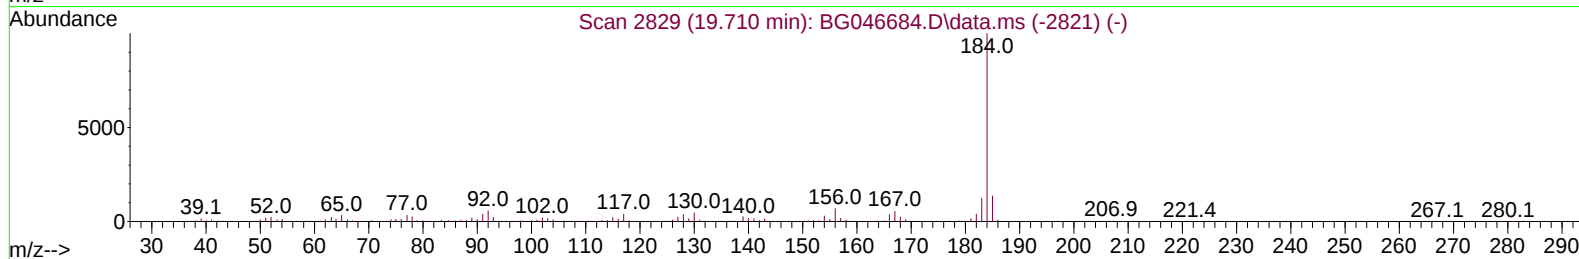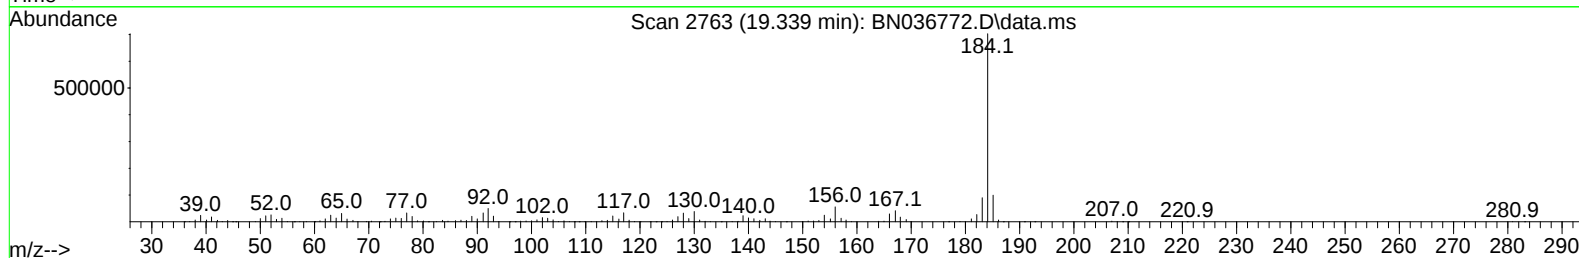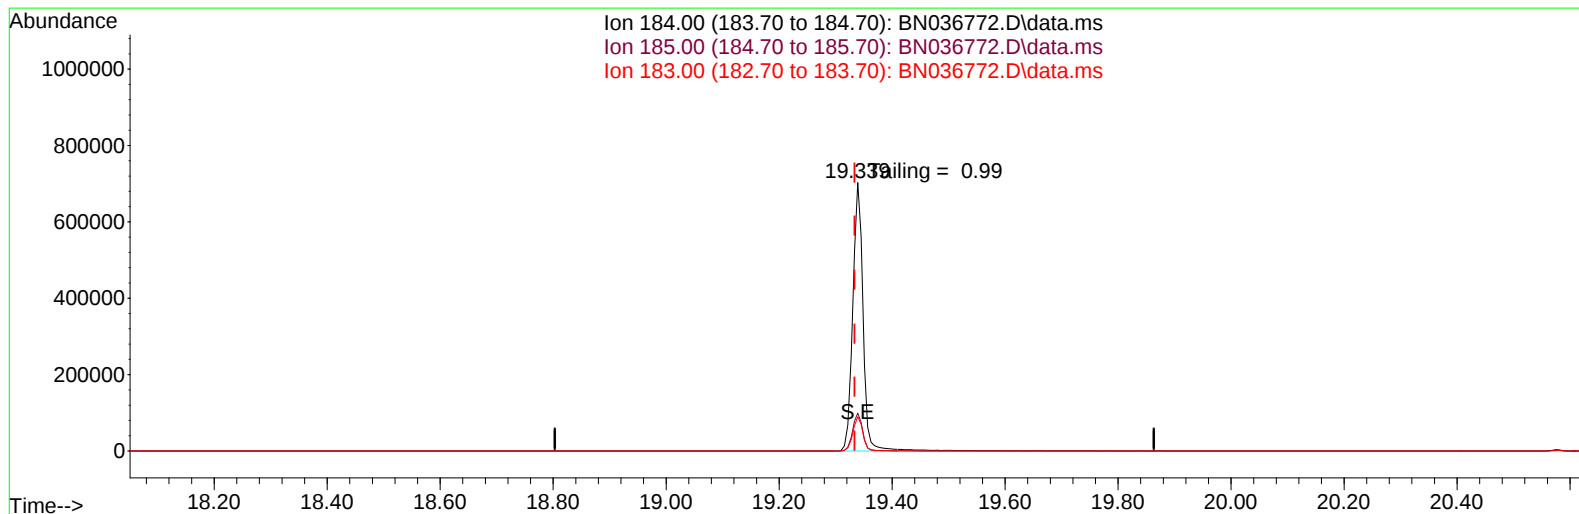

TIC: BN036772.D\data.ms

(77) Benzidine

19.339min (+ 0.006) 0.00 ng

response 891011

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.12
183.00	13.20	12.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/28/2025	BNA_N	<u>BN036772.D</u>
Compound Name	Response	Retention Time
DDT	540432	20.58
DDD	6839	20.186
DDE	318	19.627
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7157	547589	1.31

Instrument :
BNA_N
ClientSampleId :
DFTPP