
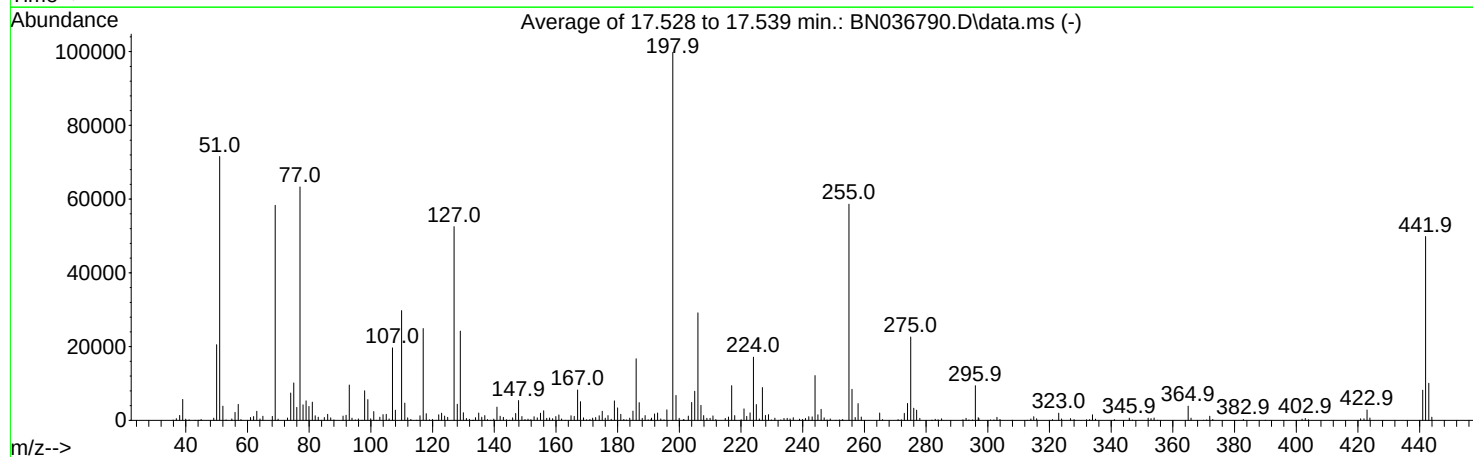


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032825\
Data File : BN036790.D
Acq On : 29 Mar 2025 01:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

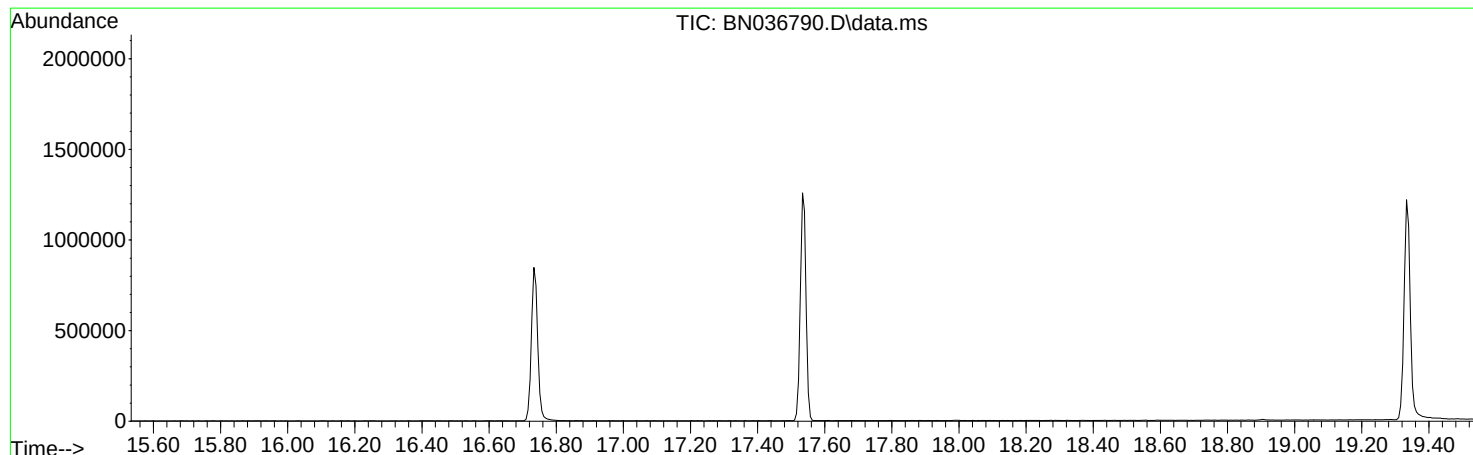

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	71.7	71579	PASS
68	69	0.00	2	1.9	1100	PASS
69	198	0.00	100	58.5	58331	PASS
70	69	0.00	2	0.6	333	PASS
127	198	10	80	52.7	52565	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99763	PASS
199	198	5	9	6.8	6769	PASS
275	198	10	60	22.7	22601	PASS
365	198	1	100	3.9	3887	PASS
441	198	0.01	100	8.2	8219	PASS
442	442	50	100	100.0	49867	PASS
443	442	15	24	20.2	10070	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/28/2025	BNA_N	<u>BN036790.D</u>
Compound Name	Response	Retention Time
DDT	356014	20.575
DDD	5380	20.133
DDE	263	19.628
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5643	361657	1.56

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032825\
Data File : BN036790.D
Acq On : 29 Mar 2025 01:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 01 00:17:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

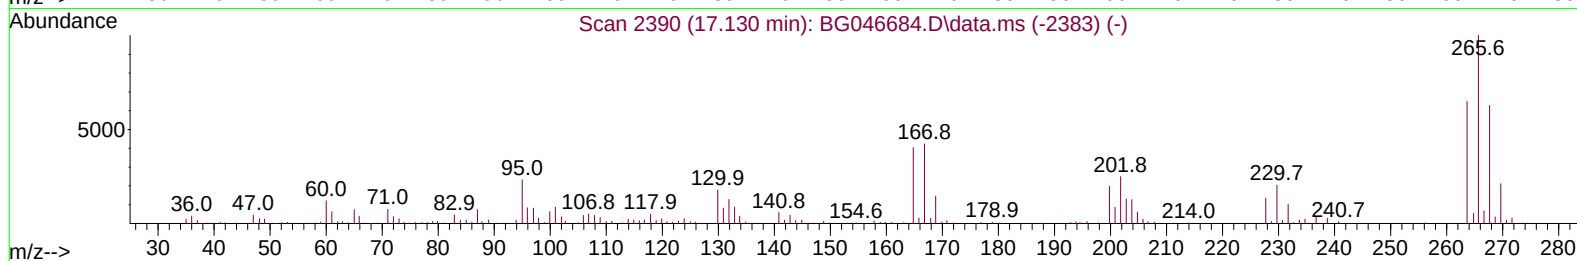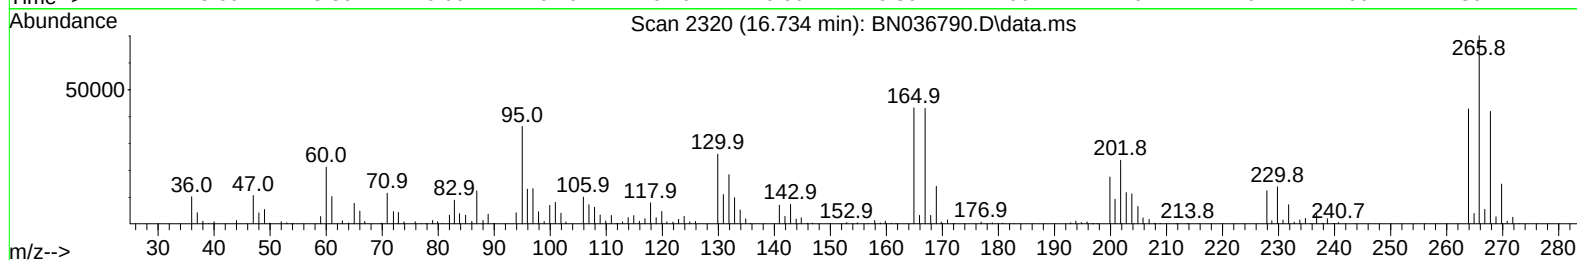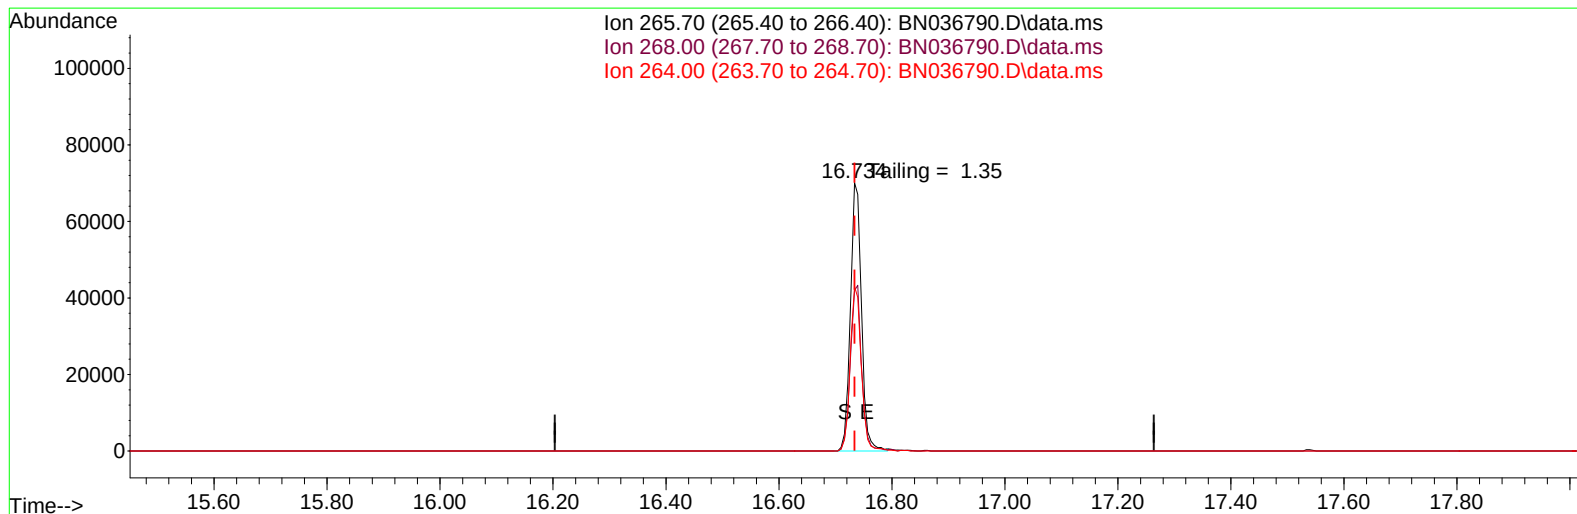

TIC: BN036790.D\data.ms

(70) Pentachlorophenol (C)

16.734min (0.000) 16501.63 ng




response 96219

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.83
264.00	61.60	61.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN032825\
Data File : BN036790.D
Acq On : 29 Mar 2025 01:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 01 00:17:04 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

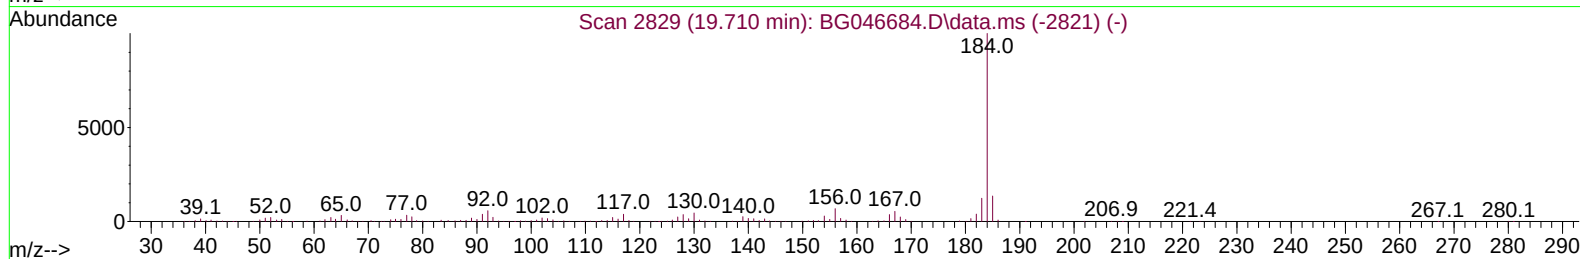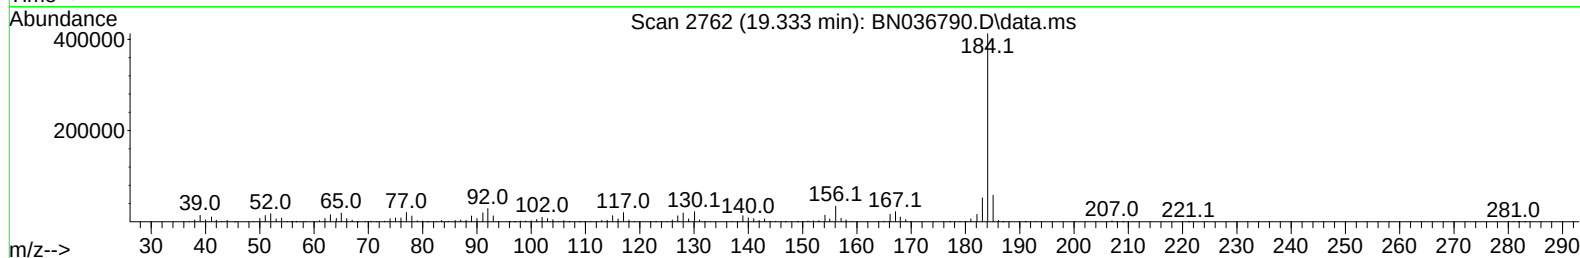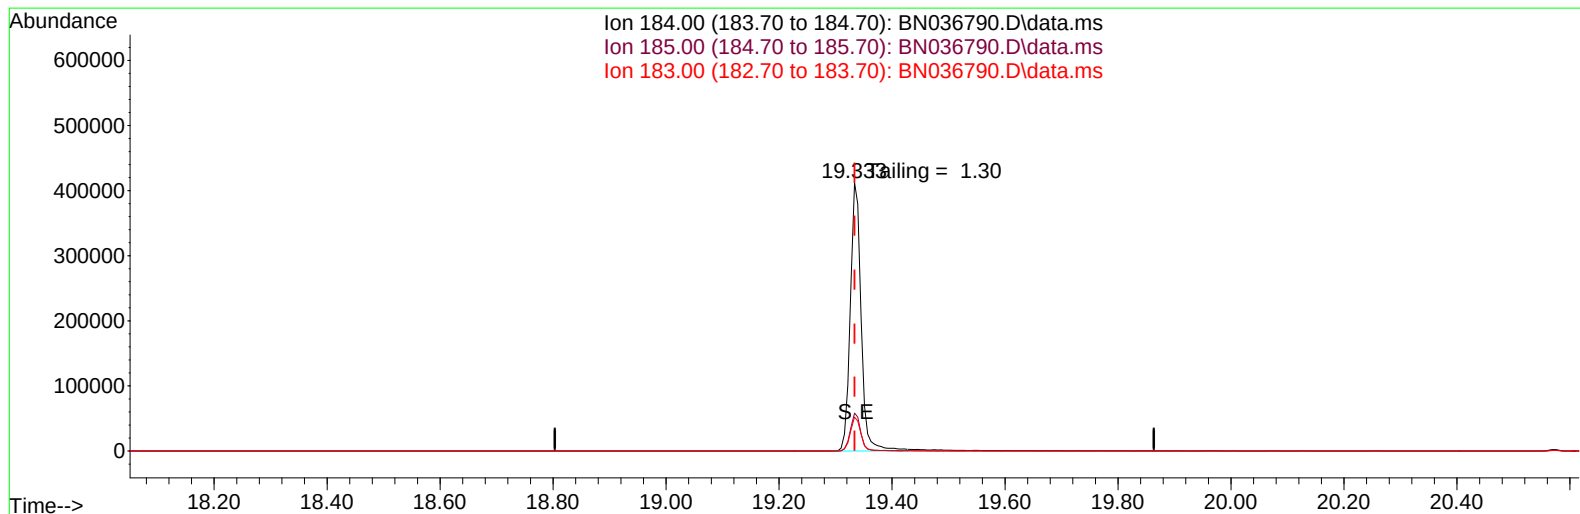

TIC: BN036790.D\data.ms

(77) Benzidine

19.333min (0.000) 0.00 ng

response 556362

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.17
183.00	13.20	12.68
0.00	0.00	0.00