

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032525\
Data File : PP070845.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2025 09:34
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 11:36:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 05:25:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.517	3.820	30843788	24400376	19.830	24.345
2) SA Decachlor...	10.233	8.864	22569739	17869707	21.245	18.265

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP032525\
Data File : PP070845.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2025 09:34
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 11:36:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP031125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 05:25:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

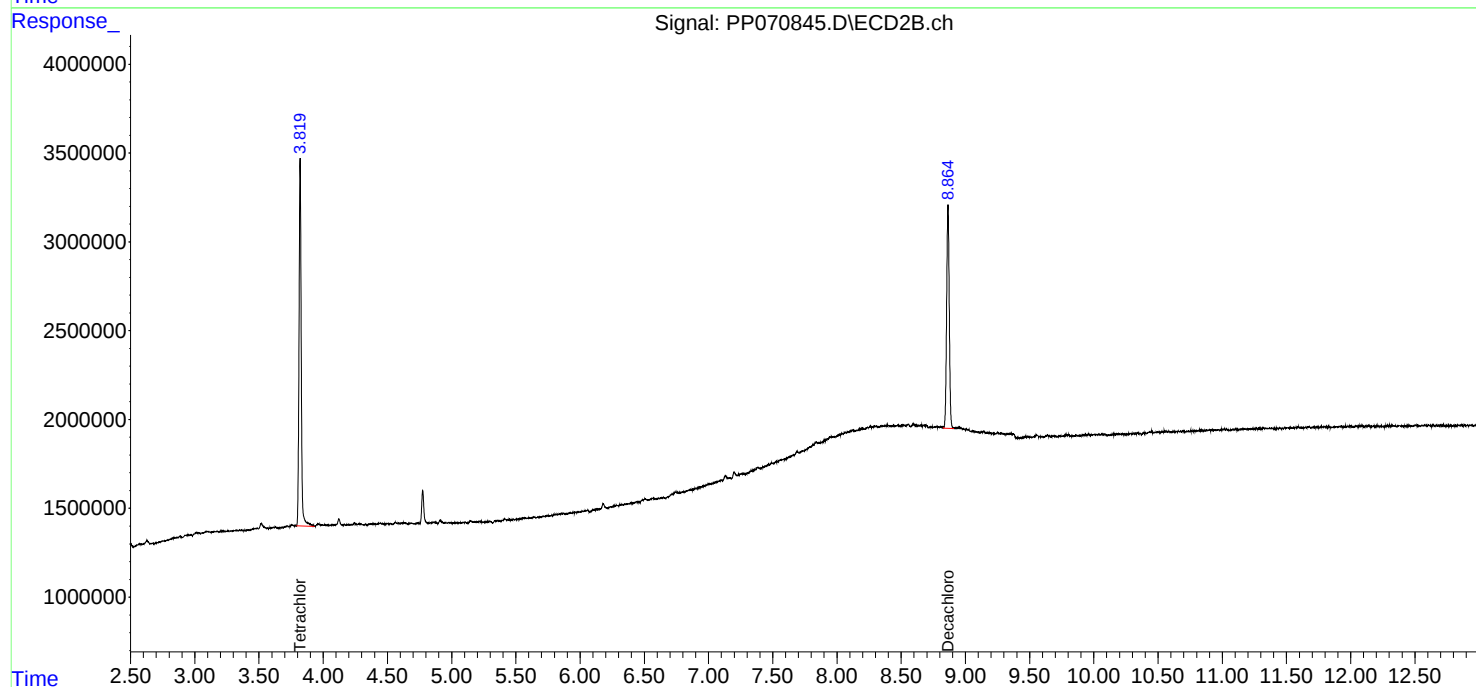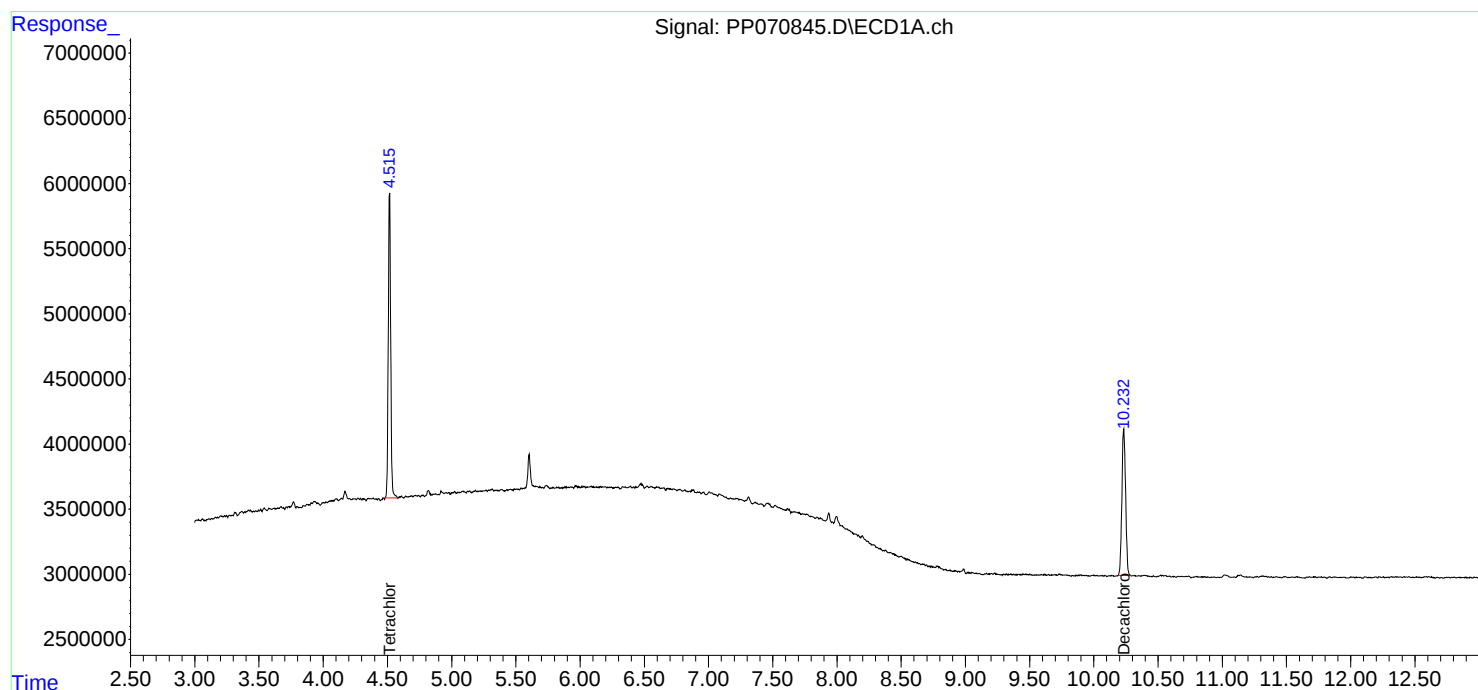


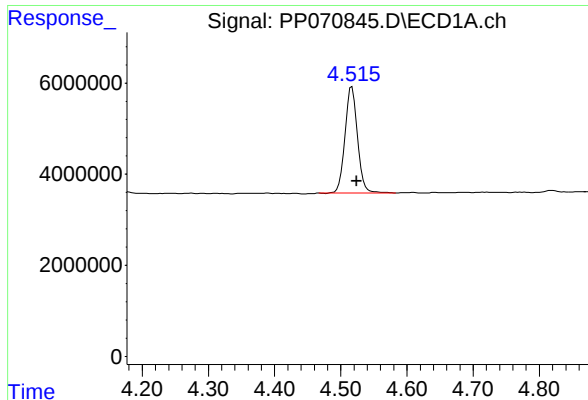

#1 Tetrachloro-m-xylene


R.T.: 4.517 min
Delta R.T.: -0.007 min
Response: 30843788
Conc: 19.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

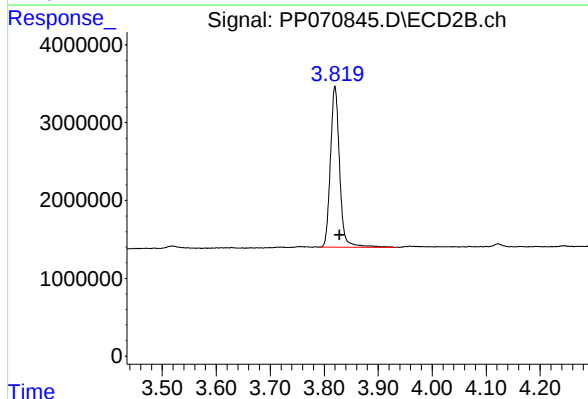


#1 Tetrachloro-m-xylene

R.T.: 3.820 min
Delta R.T.: -0.009 min
Response: 24400376
Conc: 24.34 ng/ml

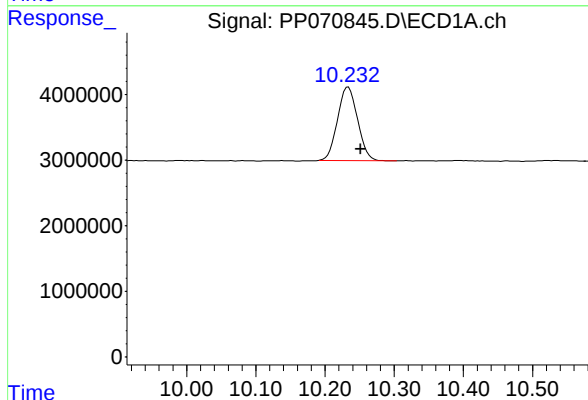

#2 Decachlorobiphenyl

R.T.: 10.233 min
Delta R.T.: -0.018 min
Response: 22569739
Conc: 21.25 ng/ml

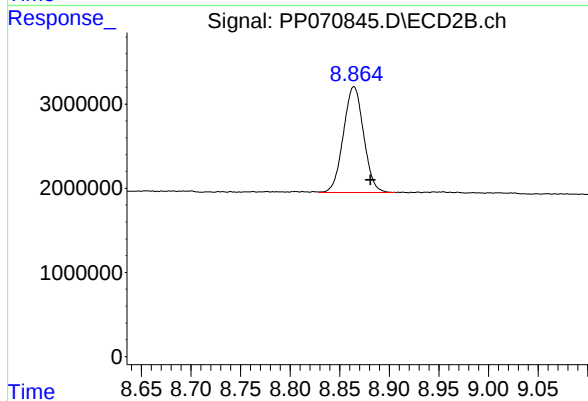

#2 Decachlorobiphenyl

R.T.: 8.864 min
Delta R.T.: -0.017 min
Response: 17869707
Conc: 18.26 ng/ml