
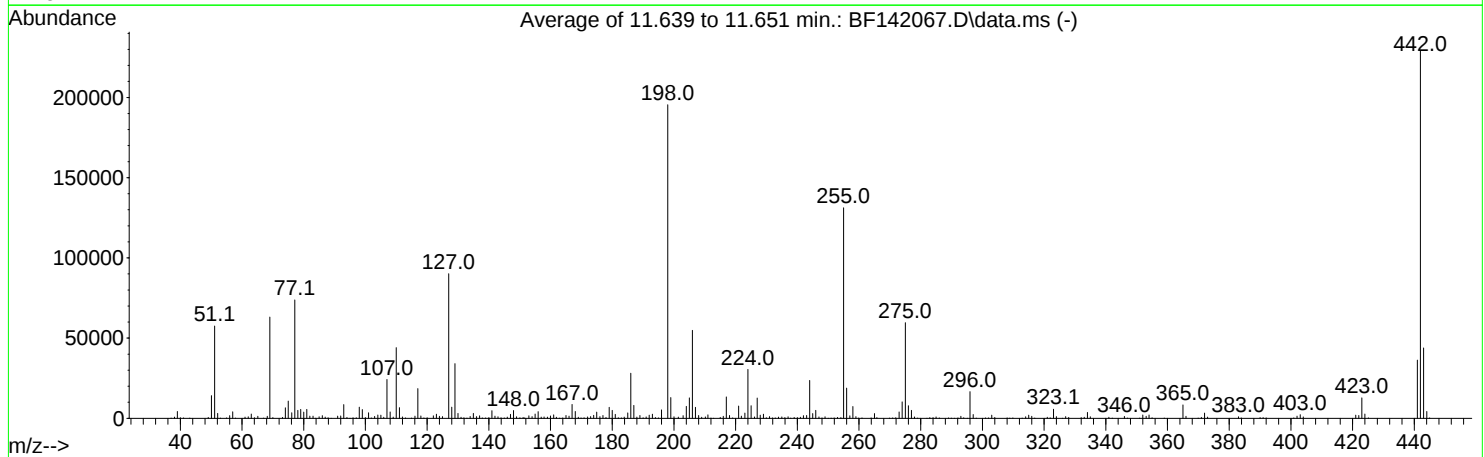


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032525\
Data File : BF142067.D
Acq On : 25 Mar 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

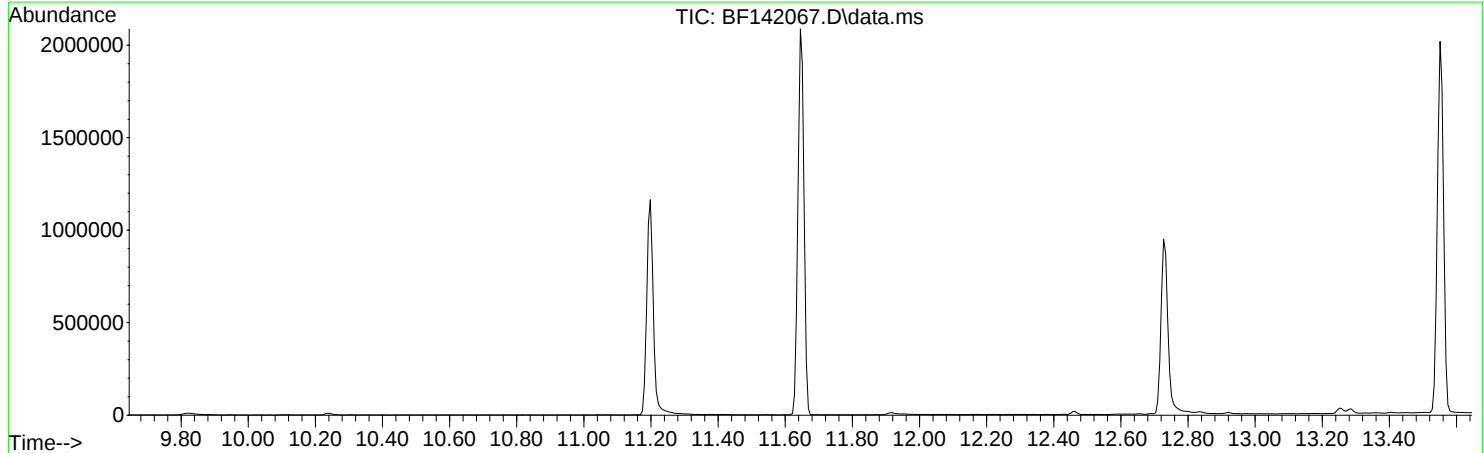




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	57504	PASS
68	69	0.00	2	1.9	1208	PASS
69	198	0.00	100	32.3	63091	PASS
70	69	0.00	2	0.7	436	PASS
127	198	10	80	46.1	90131	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	195499	PASS
199	198	5	9	6.6	12924	PASS
275	198	10	60	30.5	59603	PASS
365	198	1	100	4.2	8301	PASS
441	198	0.01	100	18.5	36256	PASS
442	442	50	100	100.0	229355	PASS
443	442	15	24	19.1	43824	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032525\
Data File : BF142067.D
Acq On : 25 Mar 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 25 11:19:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

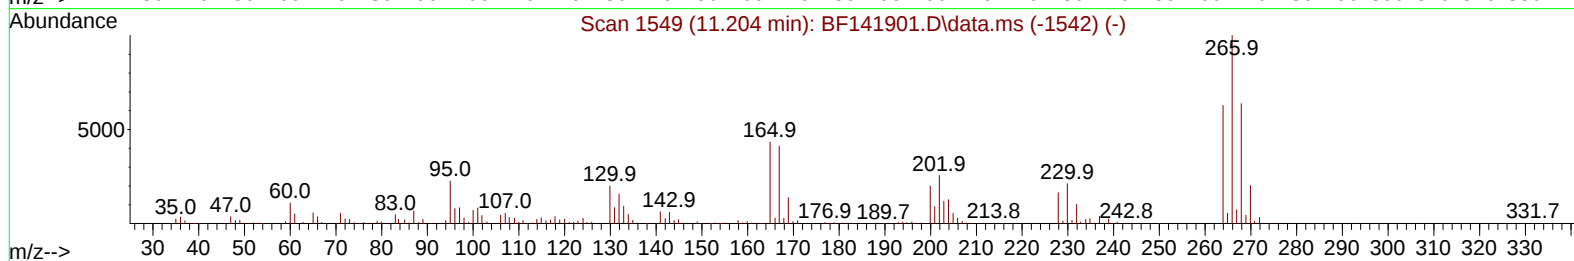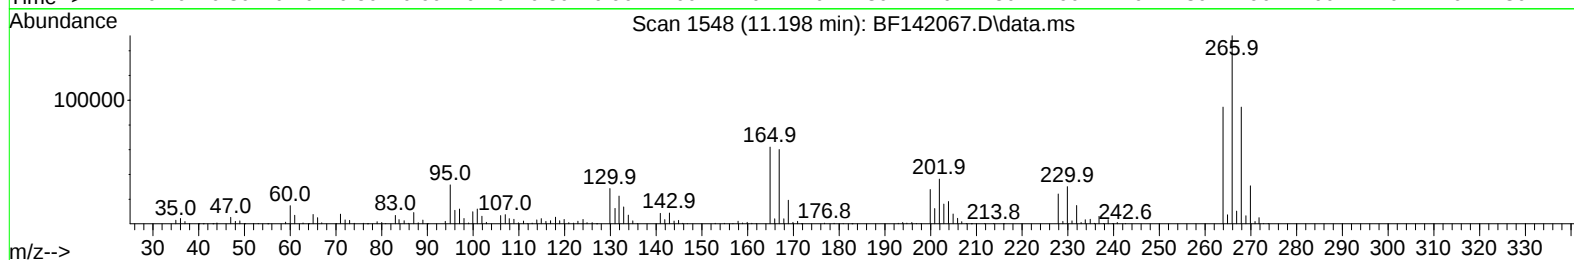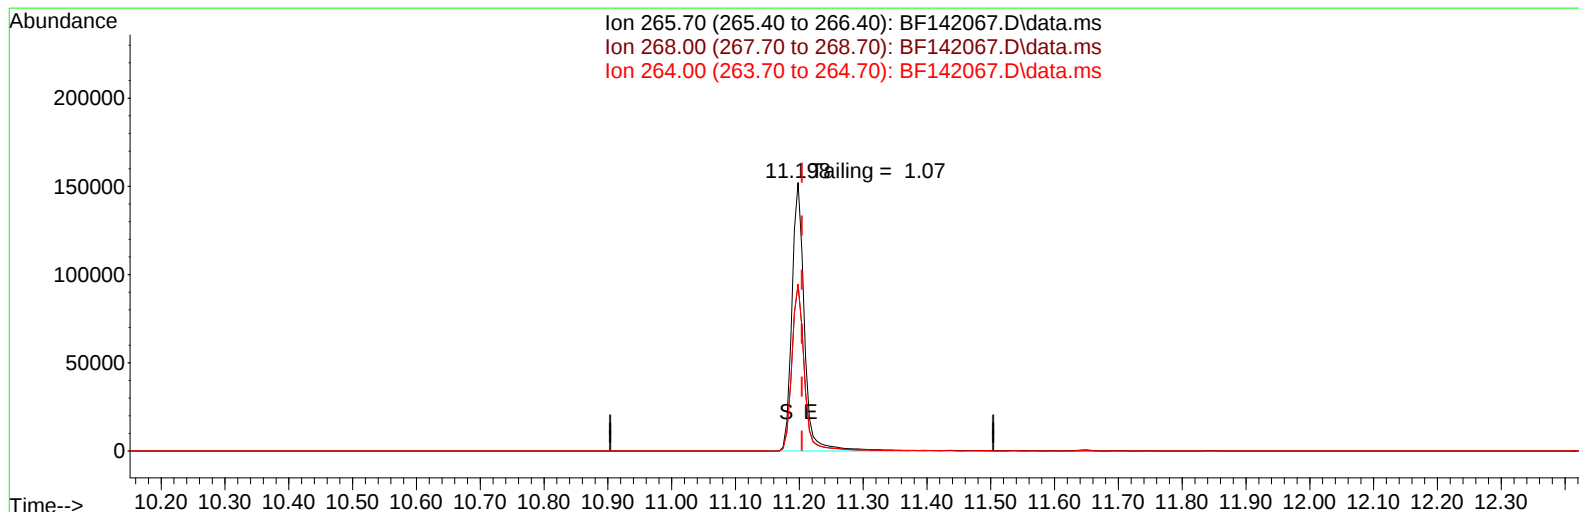

TIC: BF142067.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 96884.65 ng




response 208846

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.08
264.00	62.70	62.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032525\
Data File : BF142067.D
Acq On : 25 Mar 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 25 11:19:21 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

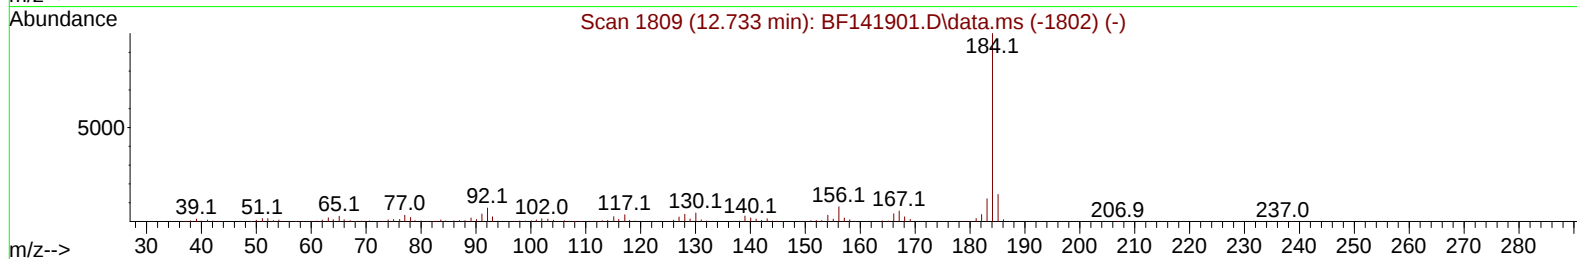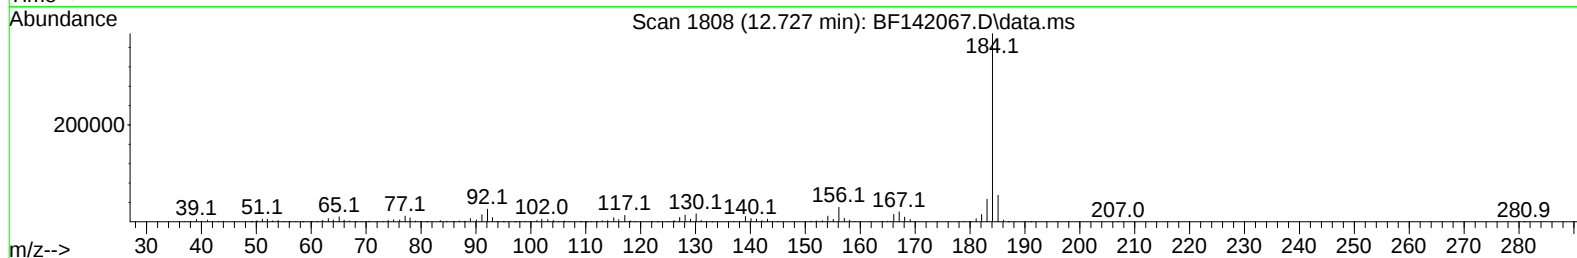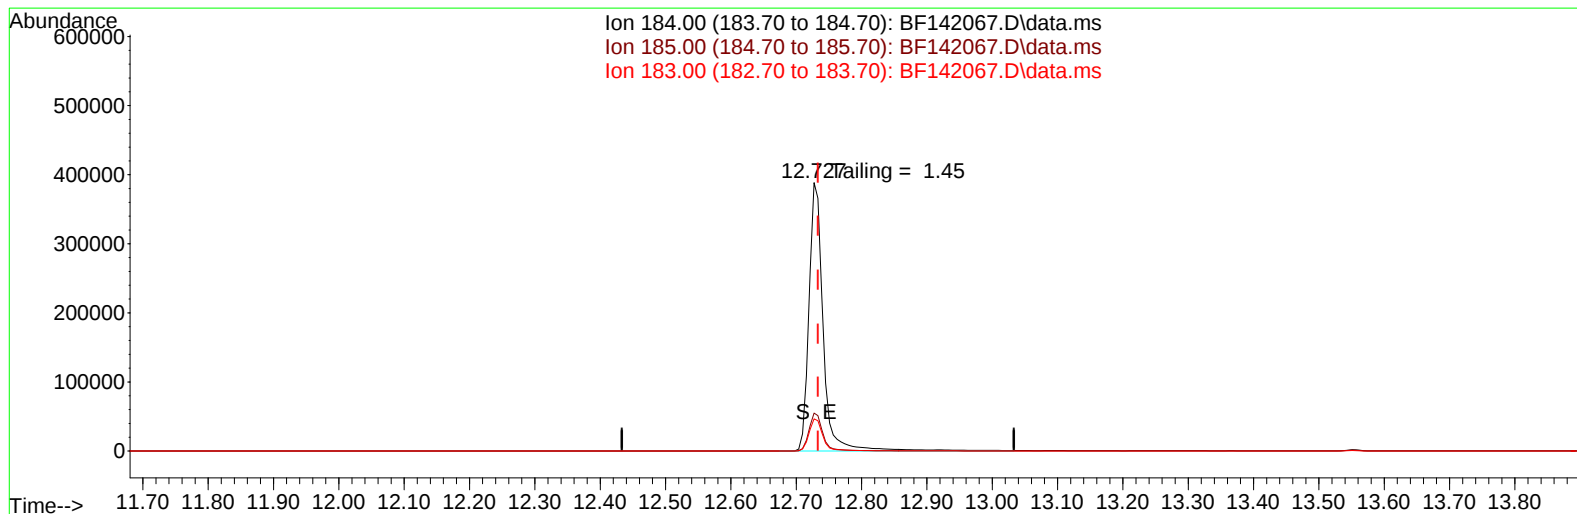

TIC: BF142067.D\data.ms

(77) Benzidine

12.727min (-0.006) 165543.78 ng

response 584341

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.16
183.00	12.10	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/25/2025	BNA_F	<u>BF142067.D</u>
Compound Name	Response	Retention Time
DDT	523081	13.551
DDD	14002	13.251
DDE	1735	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15737	538818	2.92

Instrument :
BNA_F
ClientSampleId :
DFTPP