
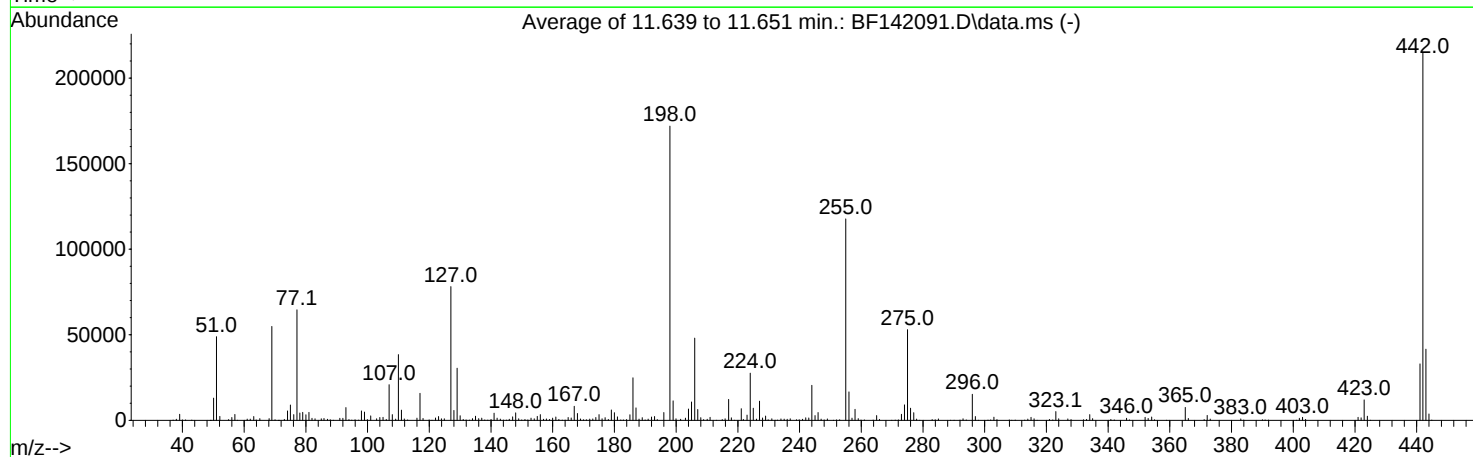


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032625\
Data File : BF142091.D
Acq On : 26 Mar 2025 11:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

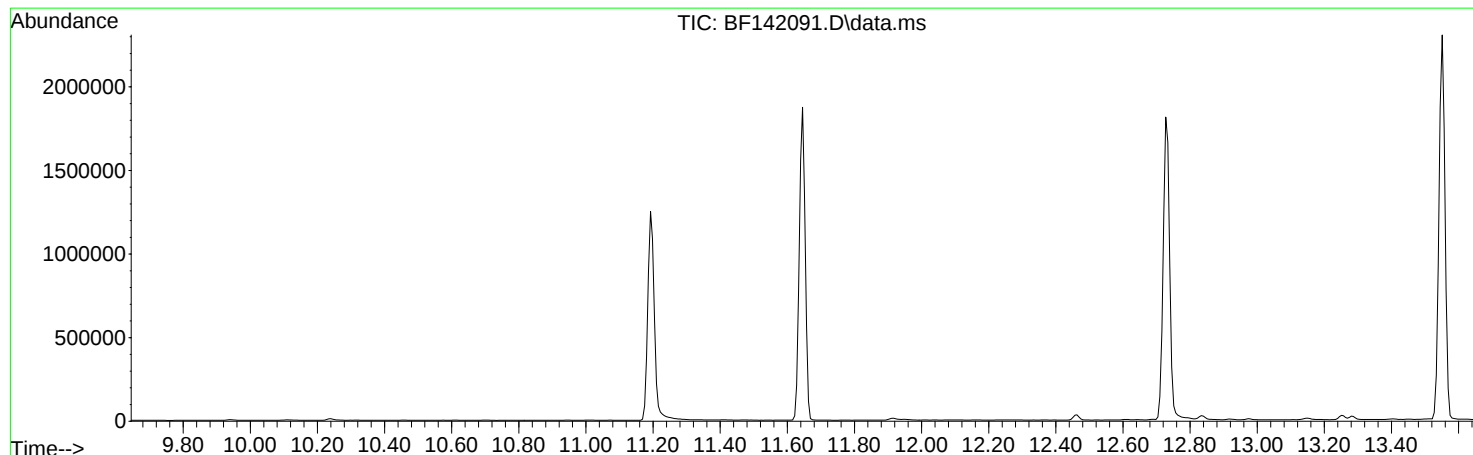




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	48948	PASS
68	69	0.00	2	1.9	1060	PASS
69	198	0.00	100	31.9	54883	PASS
70	69	0.00	2	0.6	350	PASS
127	198	10	80	45.5	78189	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	171947	PASS
199	198	5	9	6.7	11463	PASS
275	198	10	60	30.8	52995	PASS
365	198	1	100	4.4	7579	PASS
441	198	0.01	100	19.2	32997	PASS
442	442	50	100	100.0	214955	PASS
443	442	15	24	19.3	41568	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032625\
Data File : BF142091.D
Acq On : 26 Mar 2025 11:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 26 13:29:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

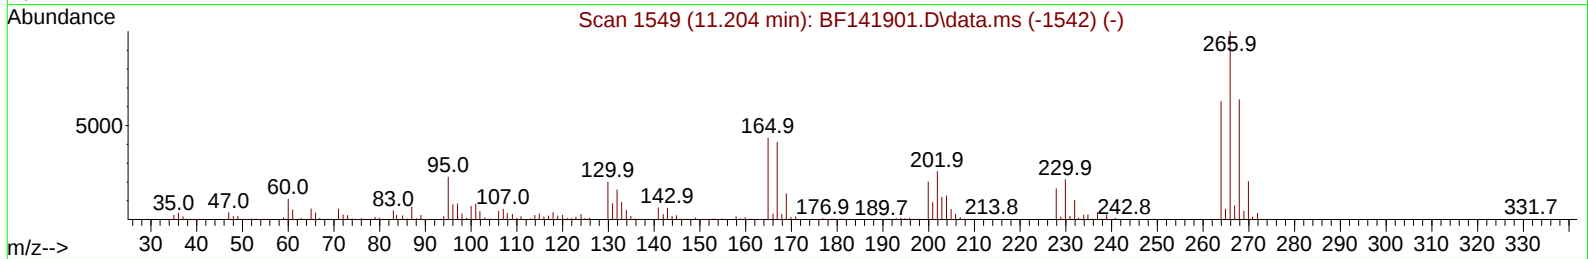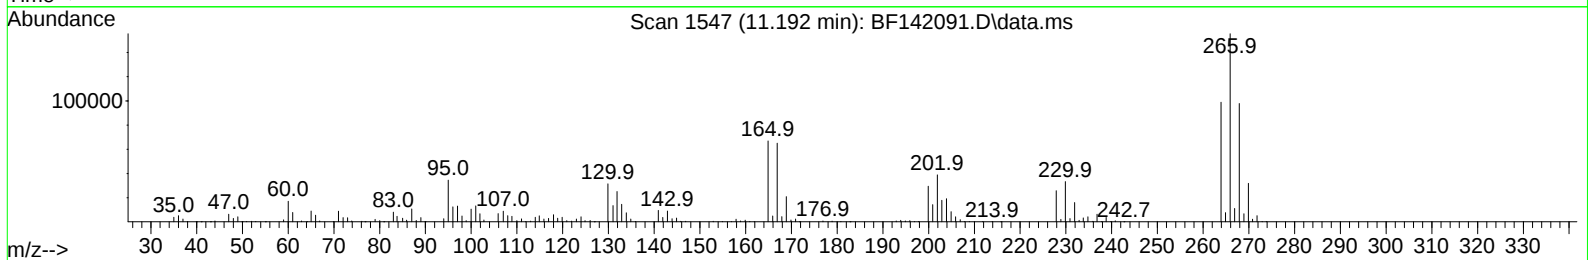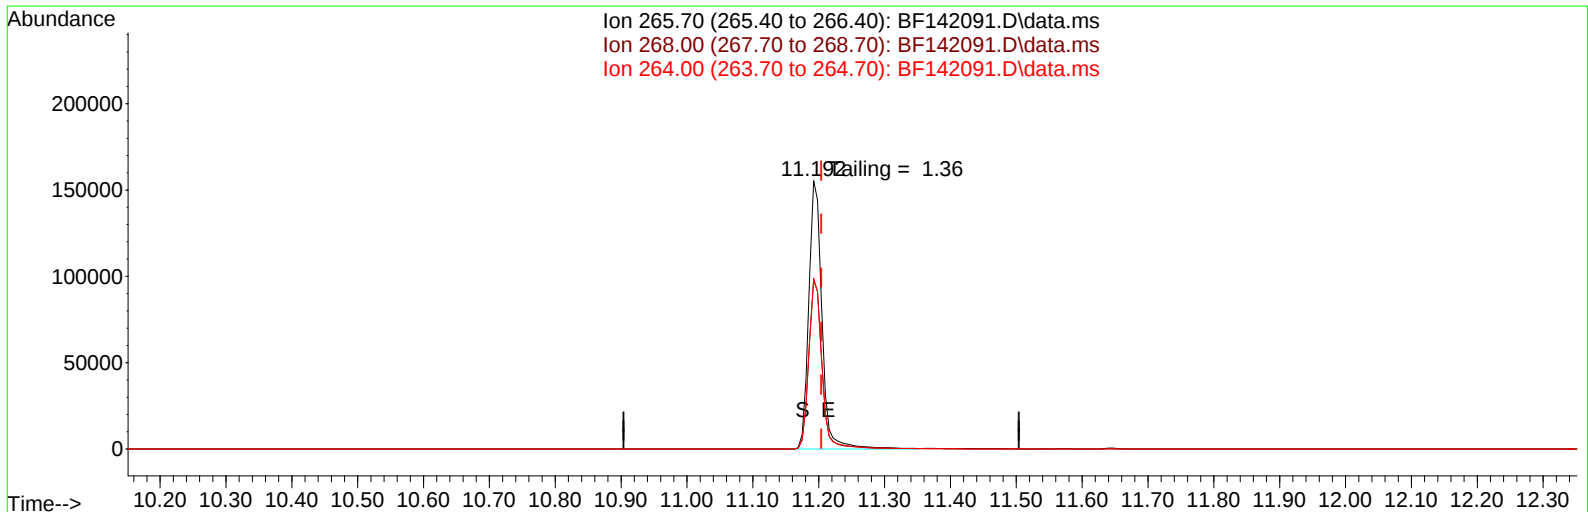

TIC: BF142091.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.011) 22780.12 ng




response 217300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	62.94
264.00	62.70	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032625\
Data File : BF142091.D
Acq On : 26 Mar 2025 11:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 26 13:29:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

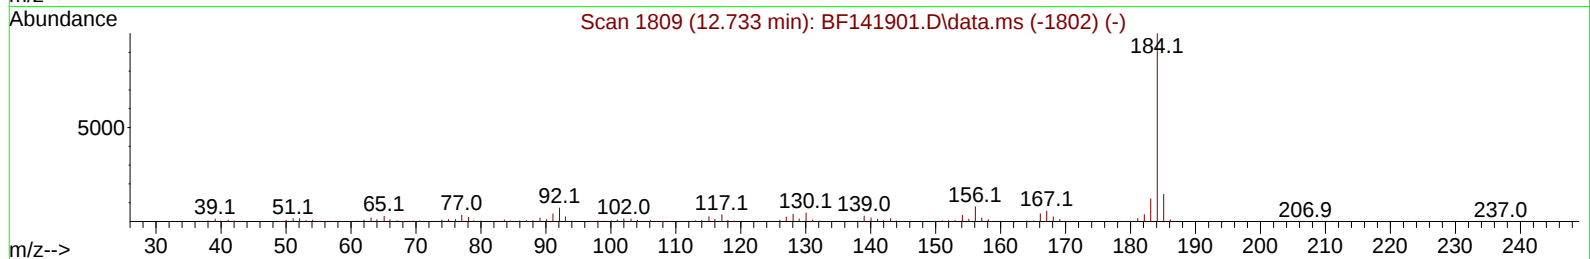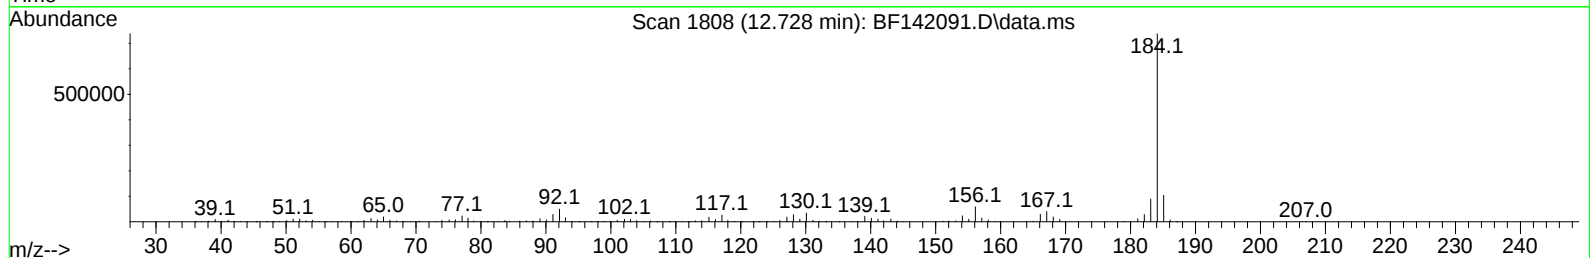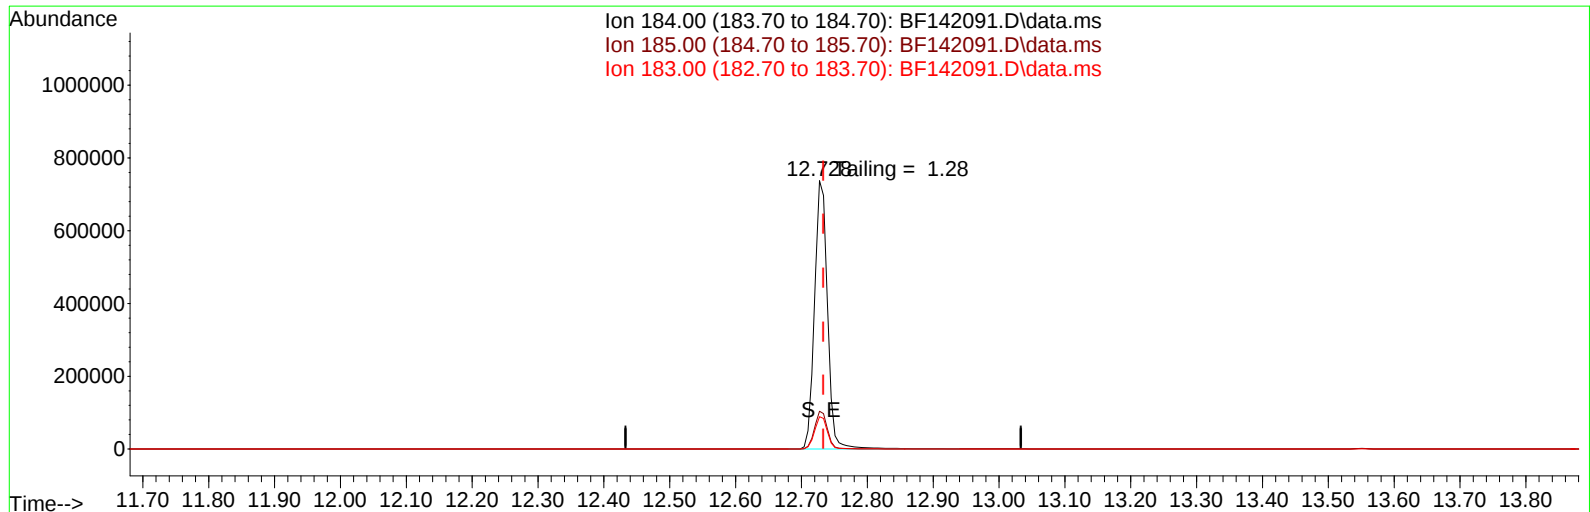

TIC: BF142091.D\data.ms

(77) Benzidine

12.728min (-0.006) 70996.12 ng

response 1009350

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.08
183.00	12.10	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/26/2025	BNA_F	<u>BF142091.D</u>
Compound Name	Response	Retention Time
DDT	582926	13.551
DDD	13634	13.251
DDE	1710	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15344	598270	2.56

Instrument :
BNA_F
ClientSampleId :
DFTPP