

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0032825\
 Data File : P0110102.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2025 17:08
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 18:05:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.691	3.688	167.6E6	96926791	18.409	18.483
2) SA Decachlor...	8.740	8.691	127.9E6	39243274	16.637	16.175

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO032825\
Data File : PO110102.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2025 17:08
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 18:05:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

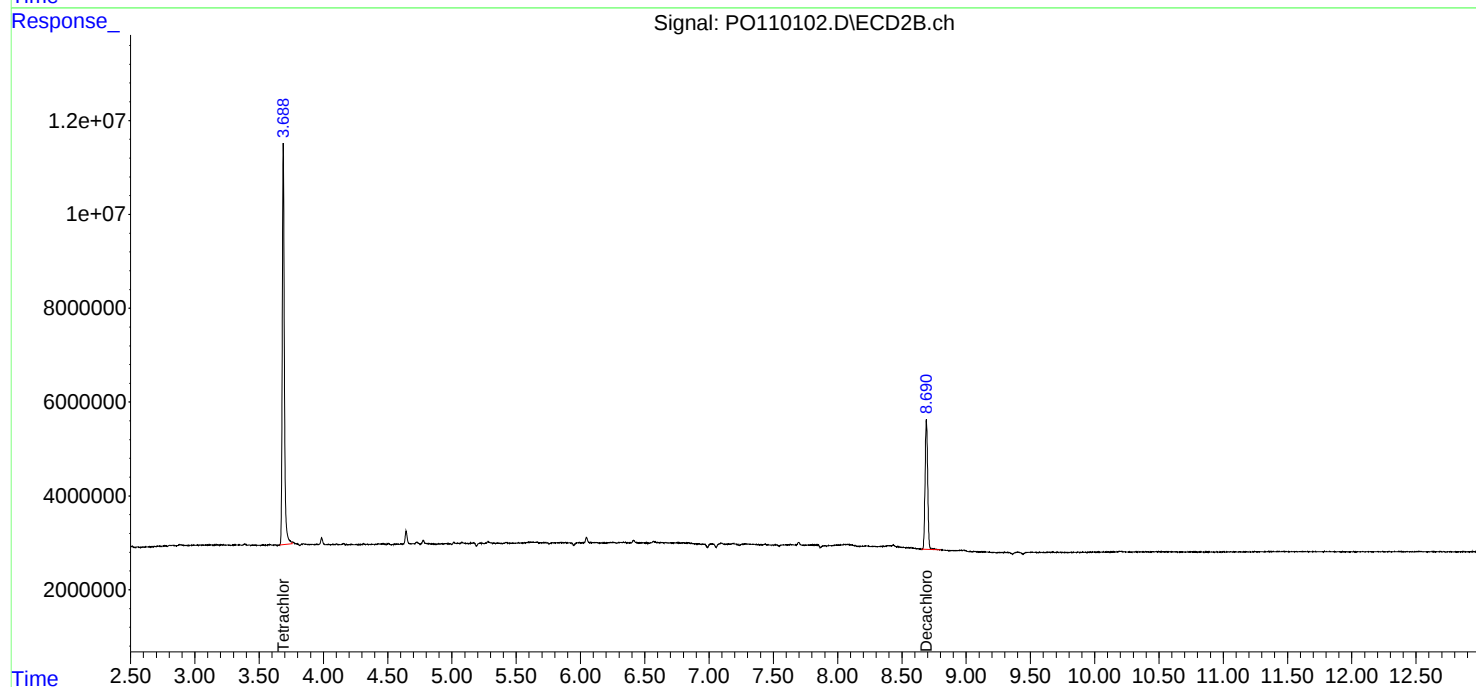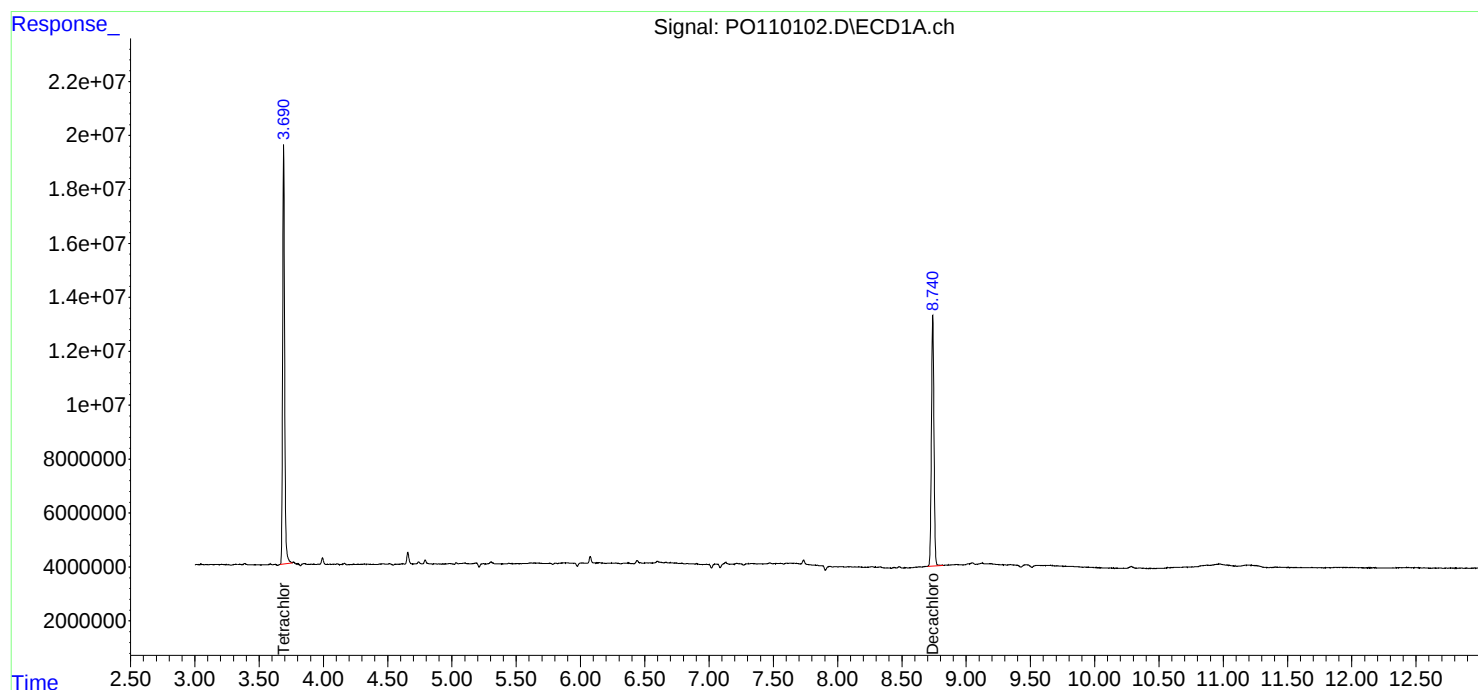


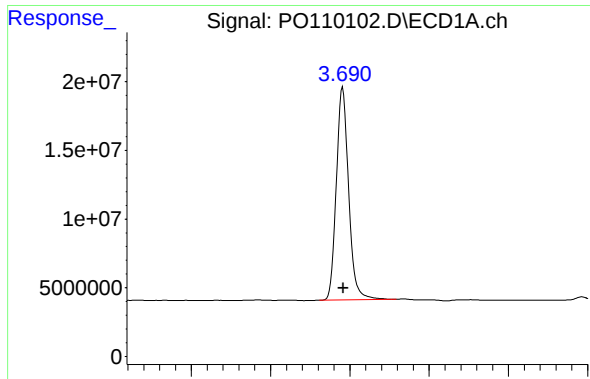

#1 Tetrachloro-m-xylene


R.T.: 3.691 min
Delta R.T.: -0.001 min
Response: 167552340
Conc: 18.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

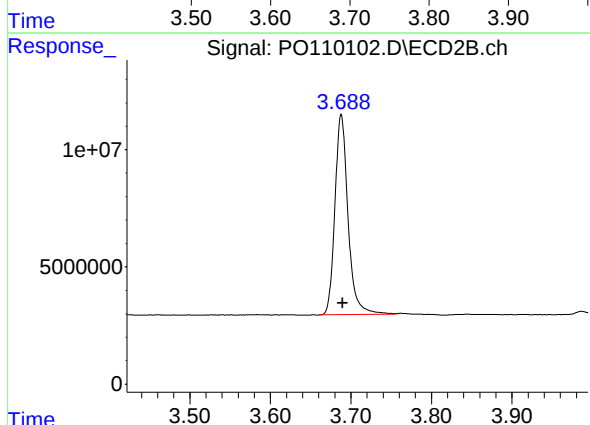


#1 Tetrachloro-m-xylene

R.T.: 3.688 min
Delta R.T.: -0.002 min
Response: 96926791
Conc: 18.48 ng/ml

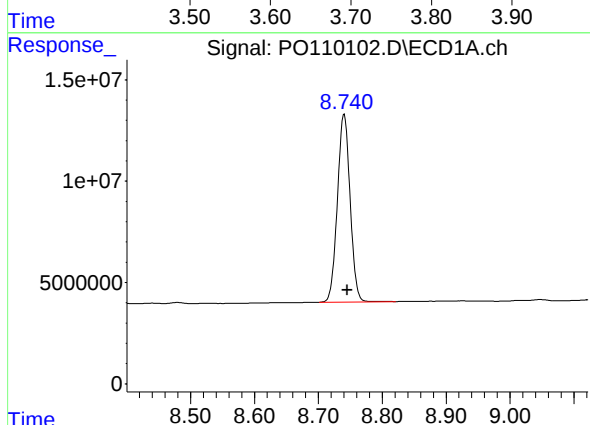

#2 Decachlorobiphenyl

R.T.: 8.740 min
Delta R.T.: -0.005 min
Response: 127918003
Conc: 16.64 ng/ml

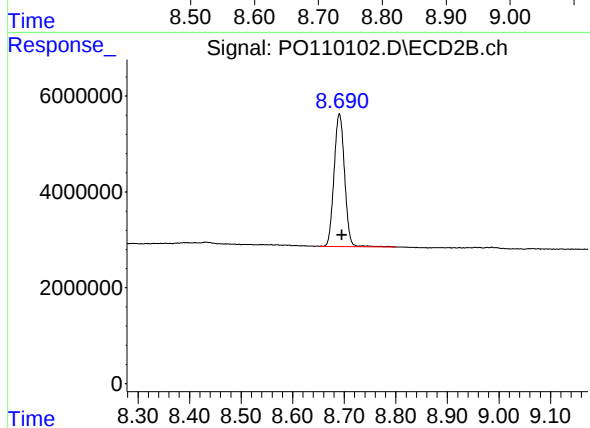

#2 Decachlorobiphenyl

R.T.: 8.691 min
Delta R.T.: -0.005 min
Response: 39243274
Conc: 16.18 ng/ml