

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0033125\
 Data File : P0110129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2025 19:48
 Operator : YP/AJ
 Sample : Q1664-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 P001-BBDGA-001-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:57:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.690	3.689	207.4E6	118.4E6	22.789	22.572
2) SA Decachlor...	8.742	8.694	173.5E6	47750810	22.567	19.682

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO033125\
Data File : PO110129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2025 19:48
Operator : YP/AJ
Sample : Q1664-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
P001-BBDGA-001-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:57:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

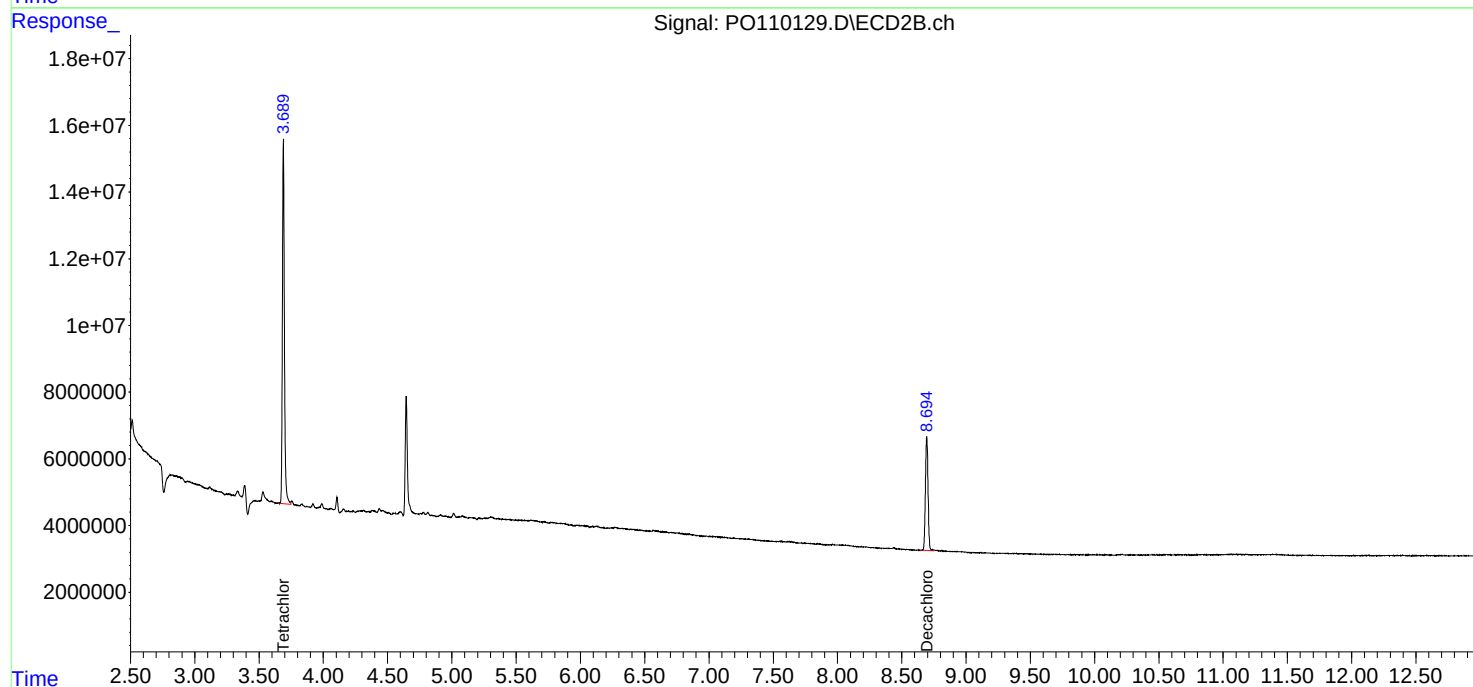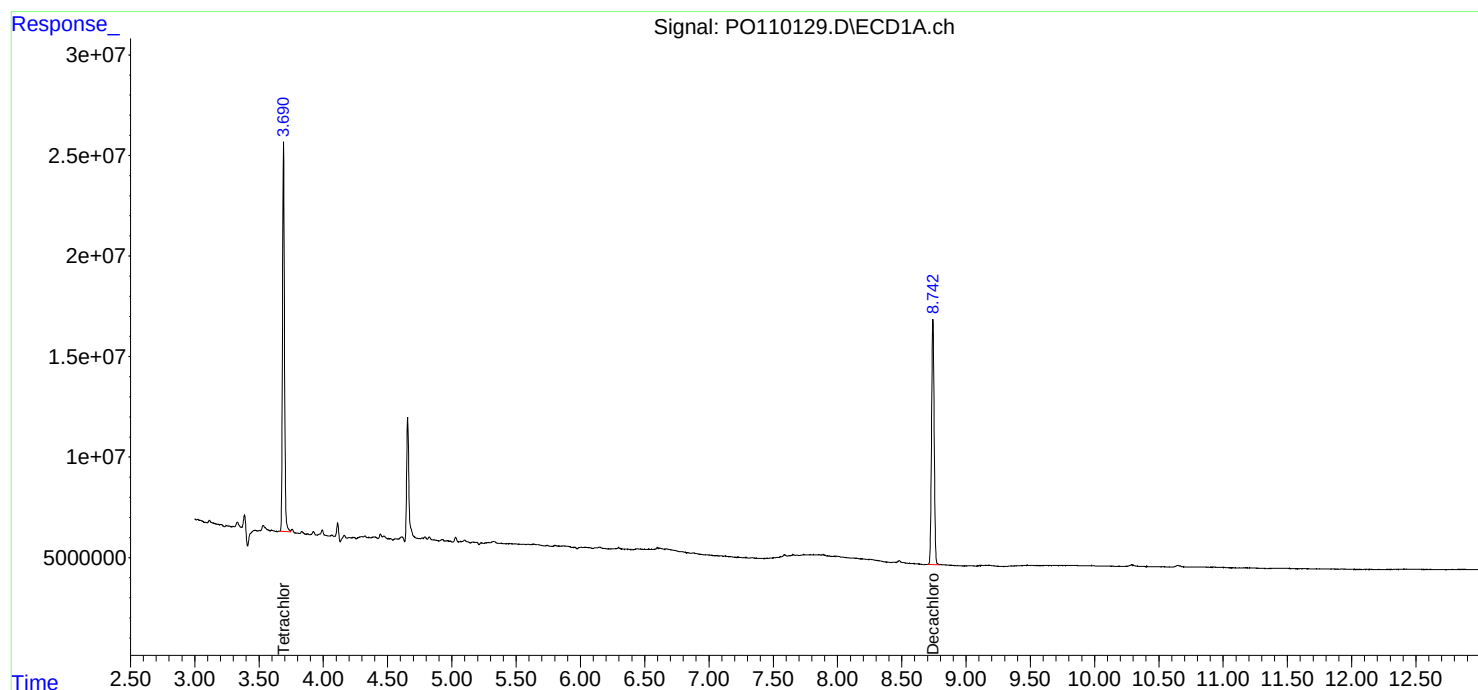


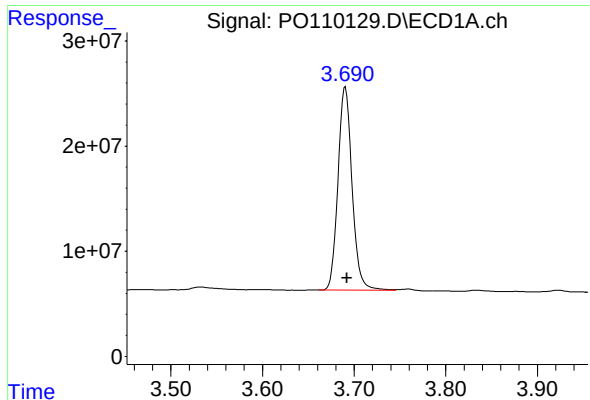

#1 Tetrachloro-m-xylene


R.T.: 3.690 min
Delta R.T.: -0.002 min
Response: 207412554
Conc: 22.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
P001-BBDGA-001-02

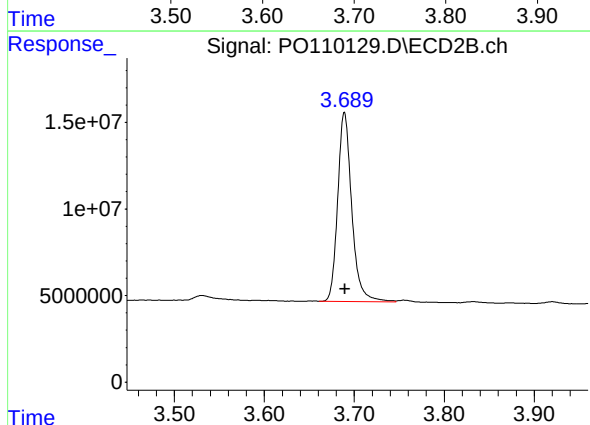


#1 Tetrachloro-m-xylene

R.T.: 3.689 min
Delta R.T.: 0.000 min
Response: 118370174
Conc: 22.57 ng/ml

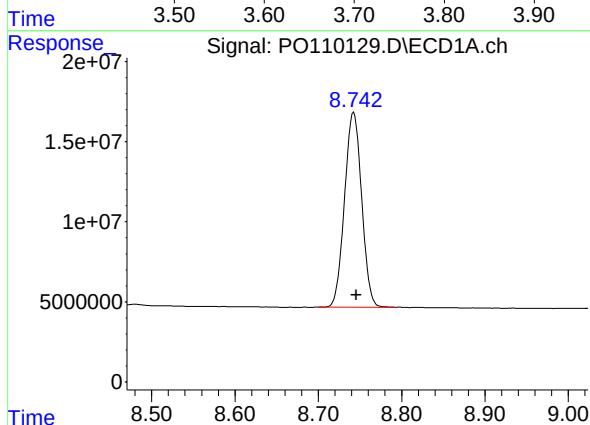

#2 Decachlorobiphenyl

R.T.: 8.742 min
Delta R.T.: -0.003 min
Response: 173512247
Conc: 22.57 ng/ml

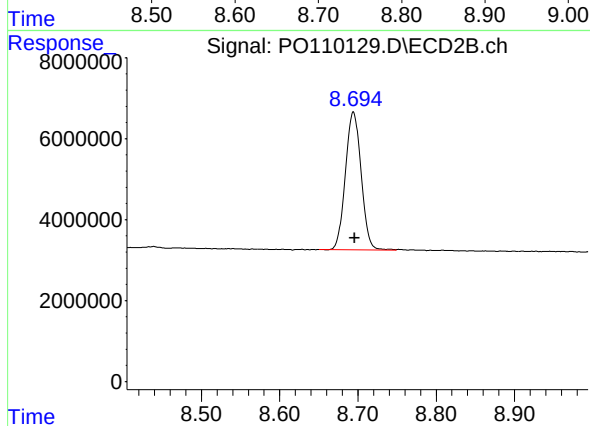

#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: -0.002 min
Response: 47750810
Conc: 19.68 ng/ml