

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033125\
 Data File : PL094974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Mar 2025 21:07
 Operator : AR\AJ
 Sample : Q1664-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P001-BBDGA-005-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/01/2025
 Supervised By :mohammad ahmed 04/07/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 01 02:16:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.769	64980670	92138140	22.956m	25.814m
28) SA Decachlor...	9.054	7.903	56141327	101.6E6	26.639	25.145

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL033125\
Data File : PL094974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Mar 2025 21:07
Operator : AR\AJ
Sample : Q1664-16
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
P001-BBDGA-005-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/01/2025
Supervised By : mohammad ahmed 04/07/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 01 02:16:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

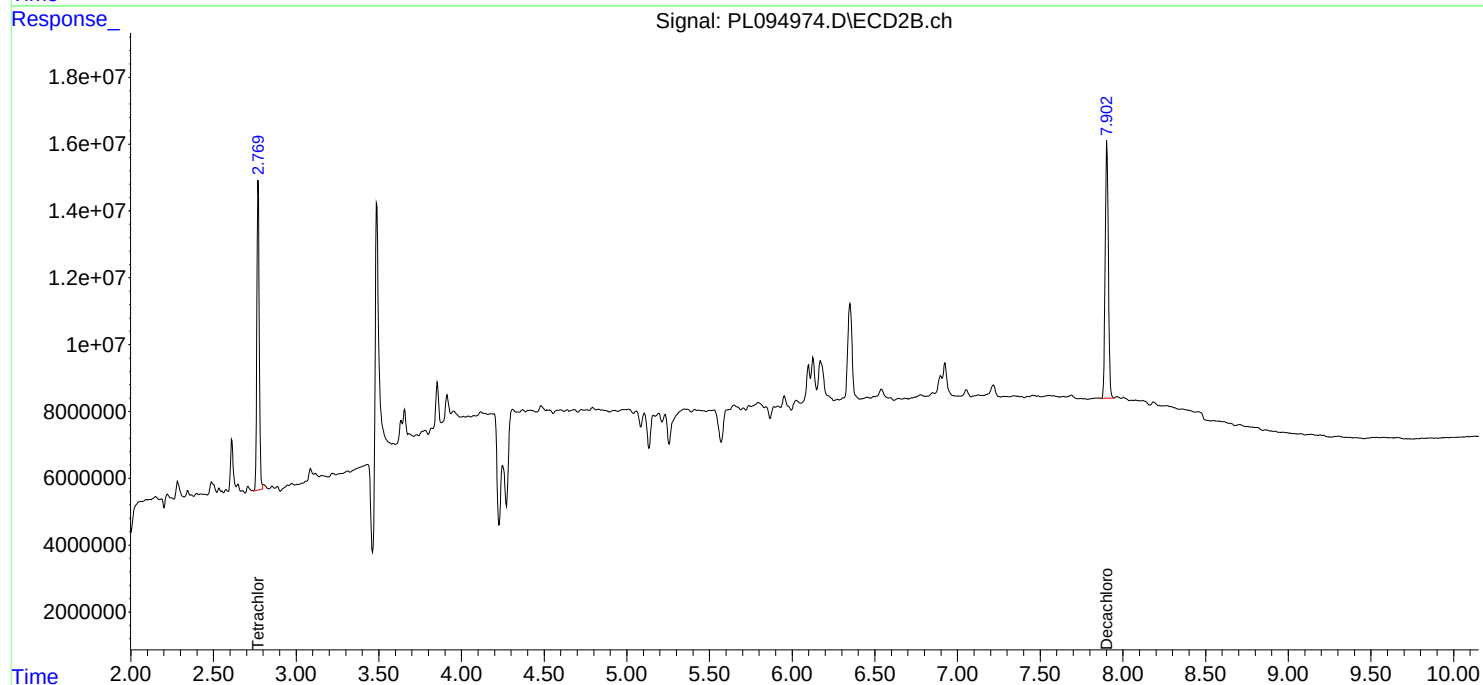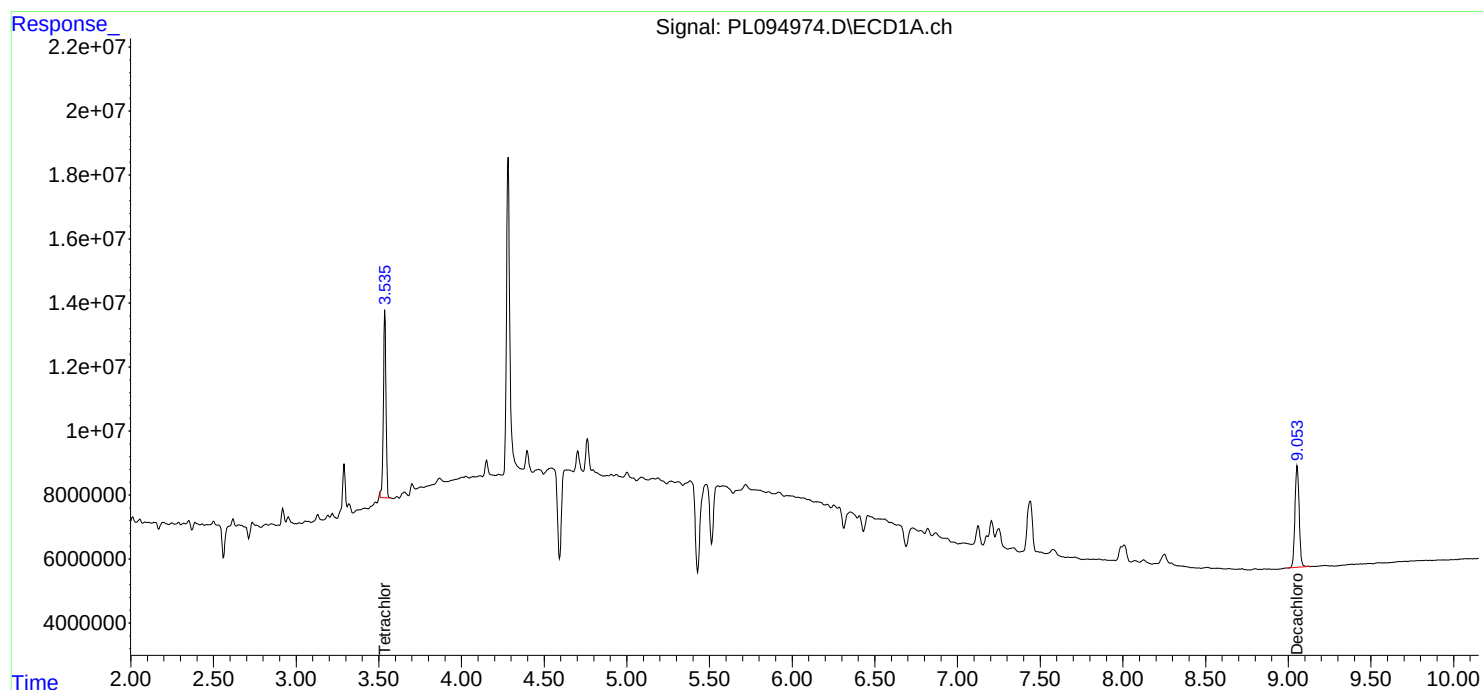

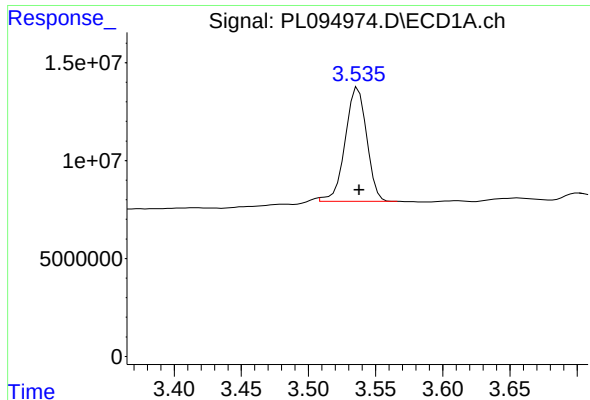


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.003 min
Response: 64980670
Conc: 22.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
P001-BBDGA-005-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/01/2025
Supervised By :mohammad ahmed 04/07/2025

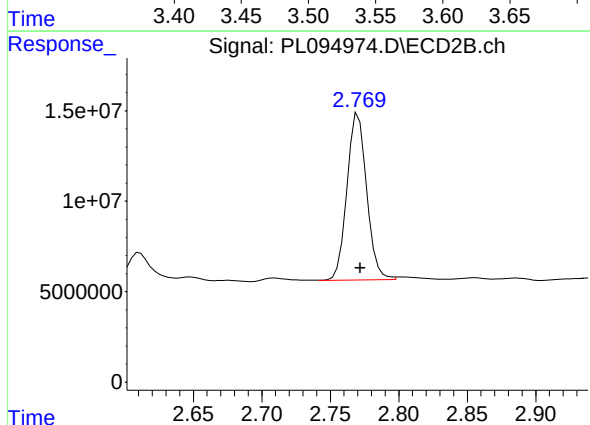


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: -0.003 min
Response: 92138140
Conc: 25.81 ng/ml m

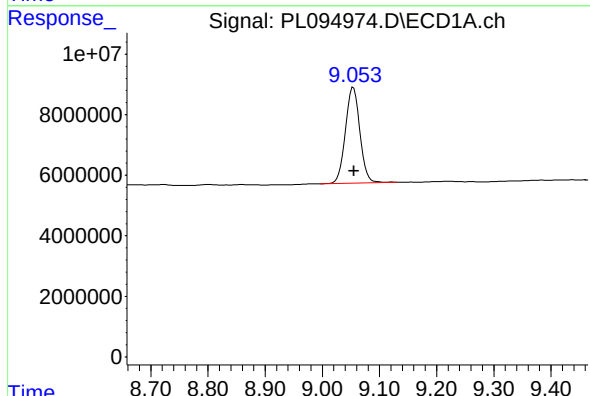

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: -0.001 min
Response: 56141327
Conc: 26.64 ng/ml

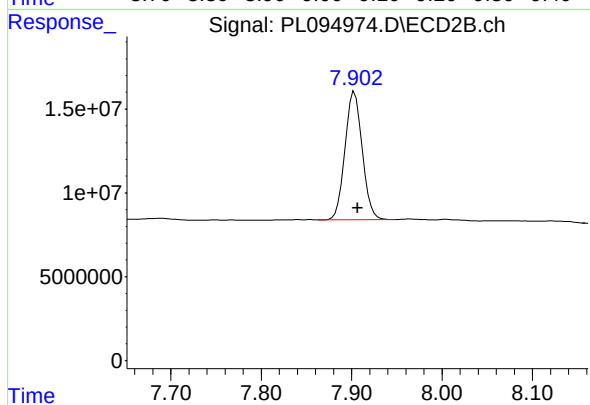

#28 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: -0.004 min
Response: 101569864
Conc: 25.15 ng/ml