
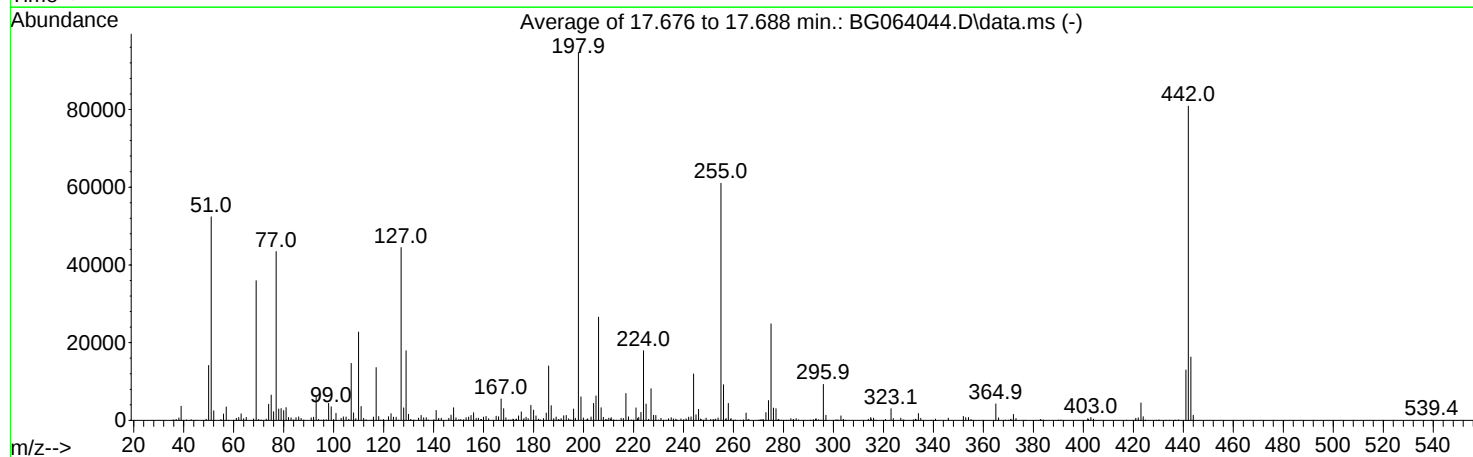


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030525\
Data File : BG064044.D
Acq On : 5 Mar 2025 8:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 05 15:39:19 2025

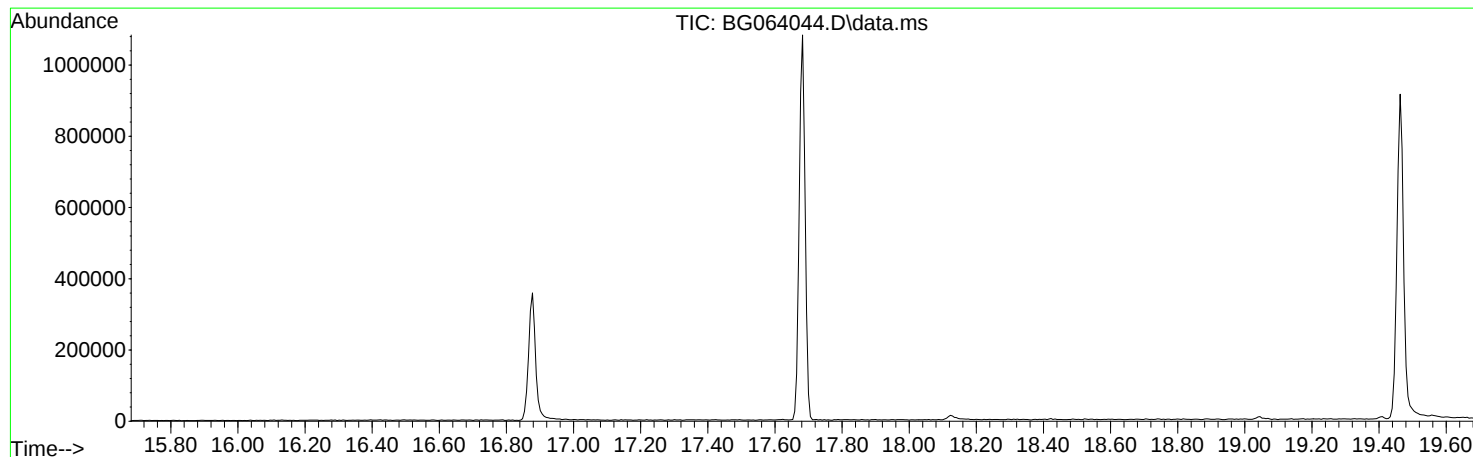

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.3	52392	PASS
68	69	0.00	2	1.1	386	PASS
69	198	0.00	100	38.0	35944	PASS
70	69	0.00	2	0.5	177	PASS
127	198	10	80	47.0	44448	PASS
197	198	0.00	2	0.6	541	PASS
198	198	100	100	100.0	94661	PASS
199	198	5	9	6.4	6065	PASS
275	198	10	60	26.2	24824	PASS
365	198	1	100	4.5	4228	PASS
441	198	0.01	100	13.7	12975	PASS
442	442	50	100	100.0	80851	PASS
443	442	15	24	20.2	16317	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/5/2025	BNA_G	<u>BG064044.D</u>
Compound Name	Response	Retention Time
DDT	173171	20.702
DDD	5056	20.256
DDE	59	19.762
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5115	178286	2.87

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030525\
Data File : BG064044.D
Acq On : 5 Mar 2025 8:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 05 15:40:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

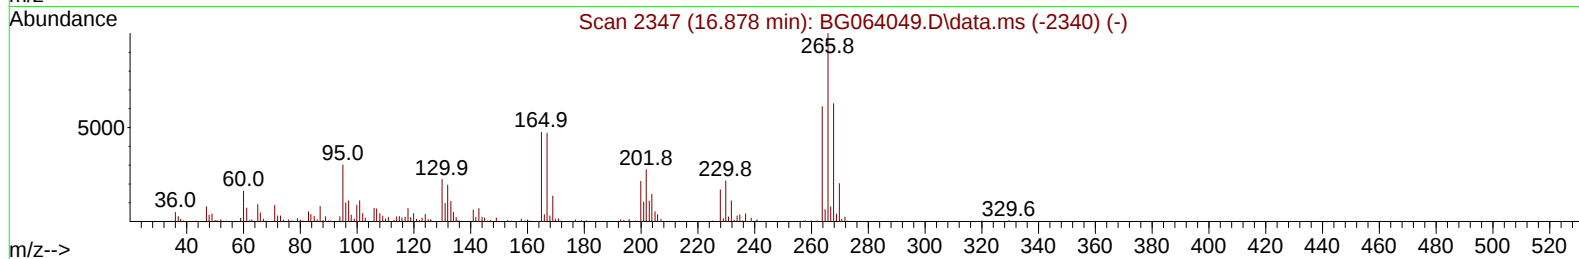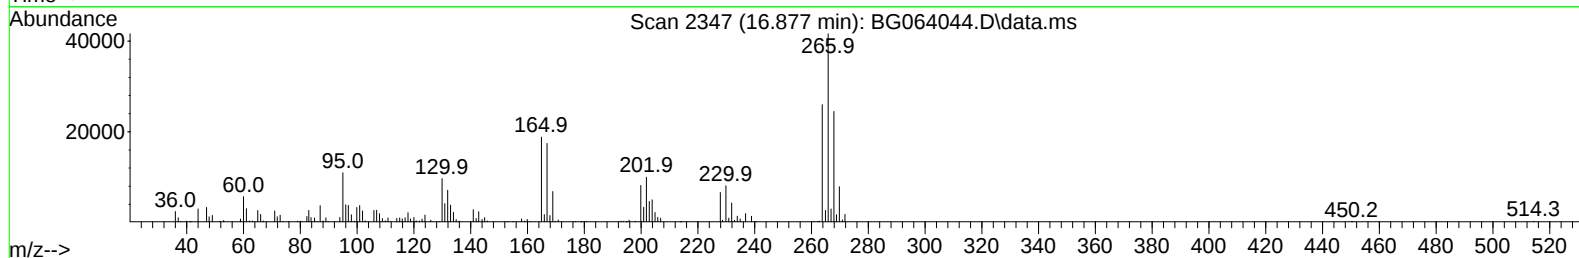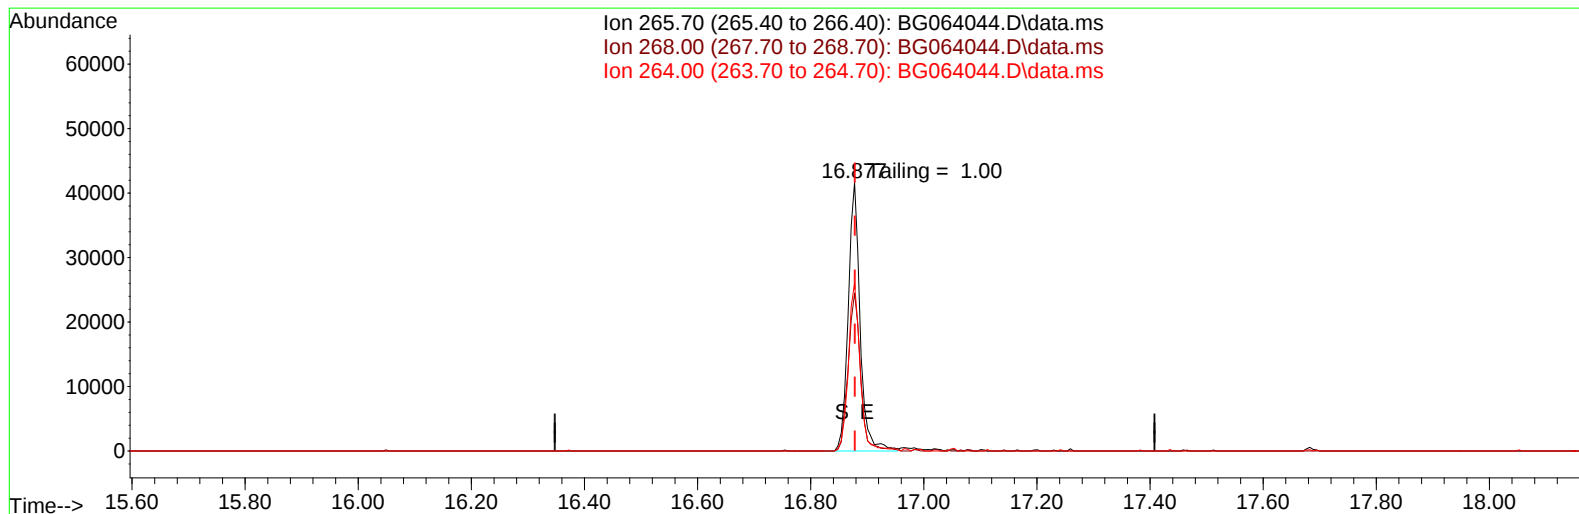

TIC: BG064044.D\data.ms

(70) Pentachlorophenol (C)

16.877min (-0.001) 14067.66 ng




response 60892

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	58.85
264.00	61.10	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030525\
Data File : BG064044.D
Acq On : 5 Mar 2025 8:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 05 15:40:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

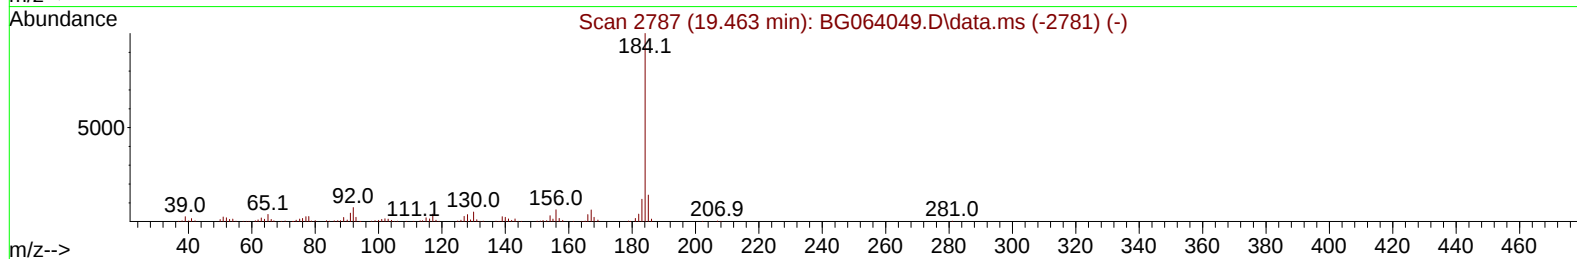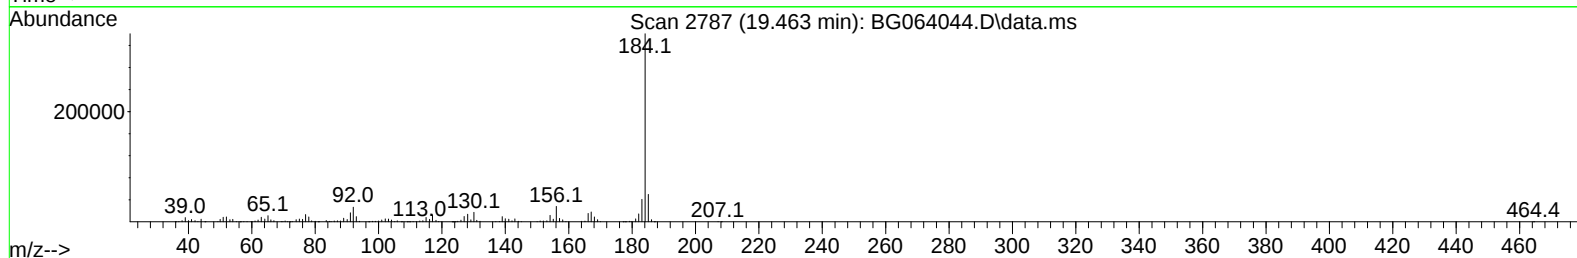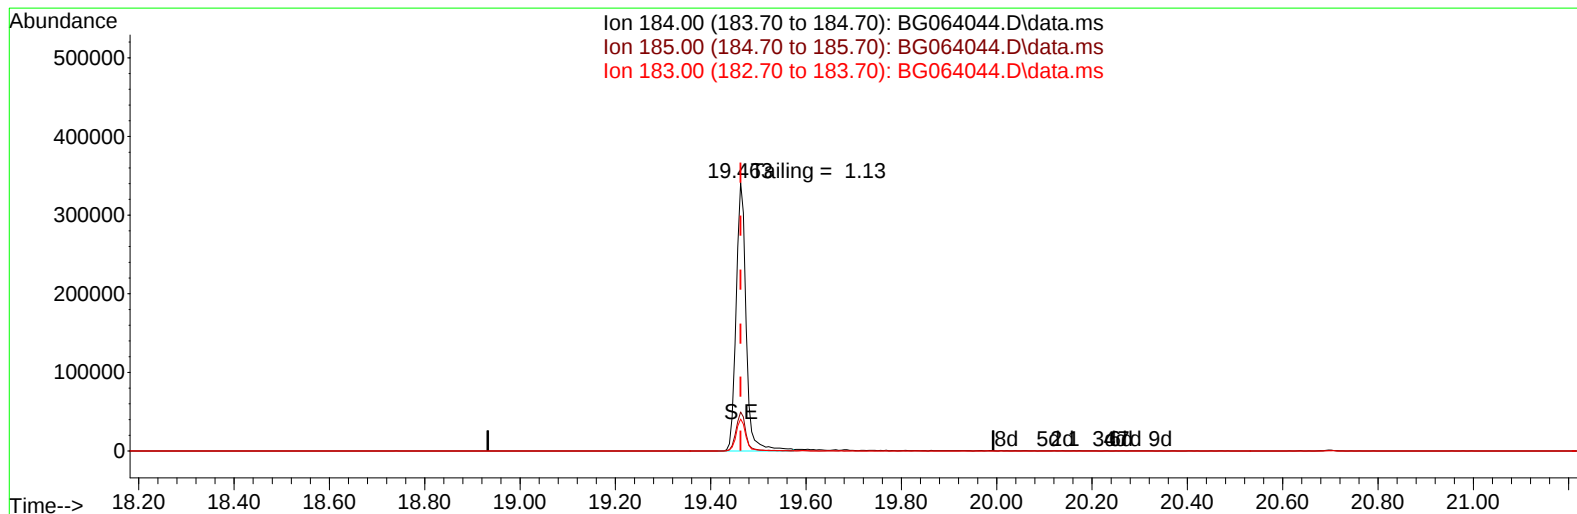

TIC: BG064044.D\data.ms

(77) Benzidine

19.463min (-0.000) 687177.88 ng m

response 523350

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.57
183.00	11.90	11.97
0.00	0.00	0.00