
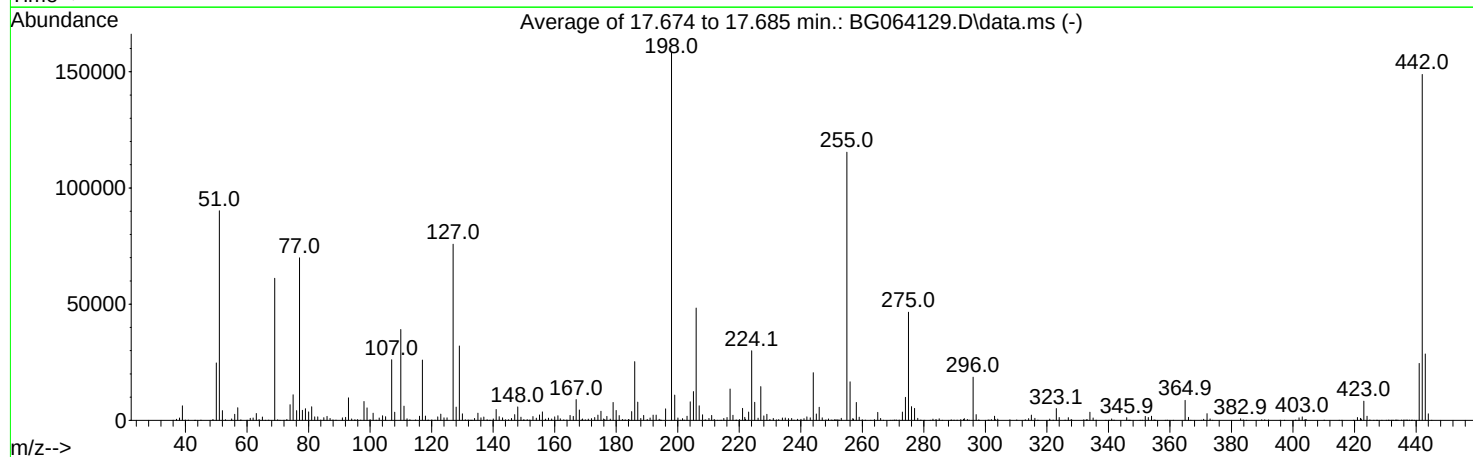


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040125\
Data File : BG064129.D
Acq On : 1 Apr 2025 10:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 05 15:39:19 2025

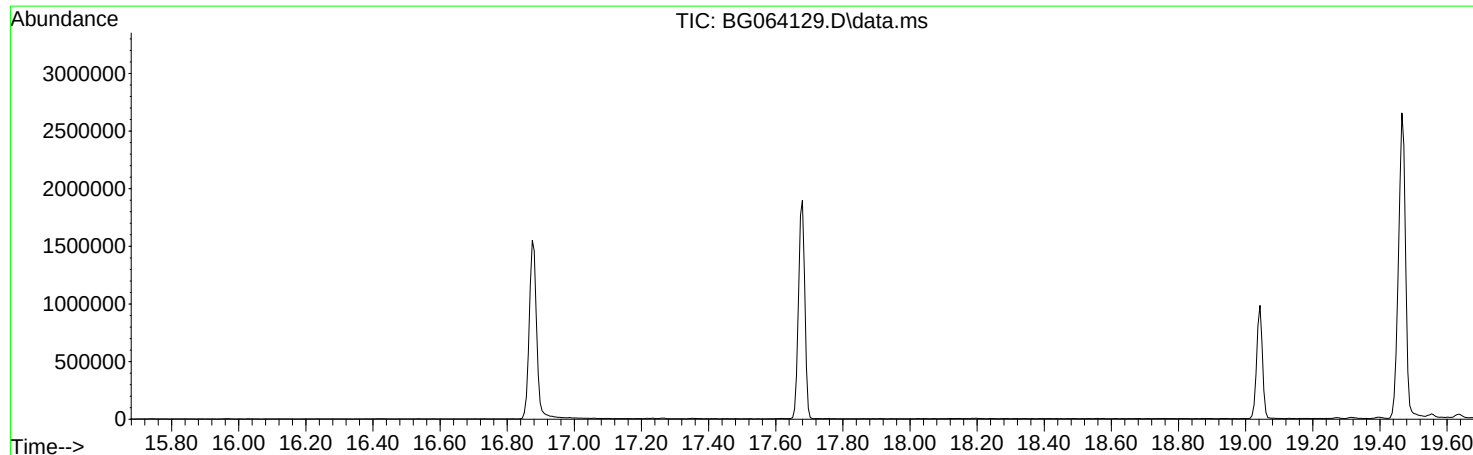

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.0	90163	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.6	61120	PASS
70	69	0.00	2	0.5	294	PASS
127	198	10	80	47.9	75825	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	158291	PASS
199	198	5	9	6.9	10872	PASS
275	198	10	60	29.4	46560	PASS
365	198	1	100	5.4	8613	PASS
441	198	0.01	100	15.5	24488	PASS
442	442	50	100	100.0	148856	PASS
443	442	15	24	19.2	28603	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/1/2025	BNA_G	<u>BG064129.D</u>
Compound Name	Response	Retention Time
DDT	689196	20.699
DDD	16001	20.259
DDE	856	19.753
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16857	706053	2.39

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040125\
Data File : BG064129.D
Acq On : 1 Apr 2025 10:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 01 12:38:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

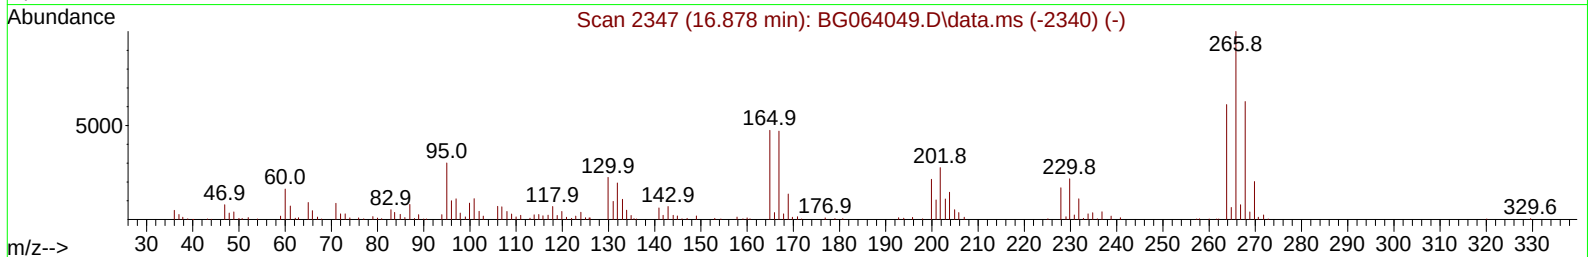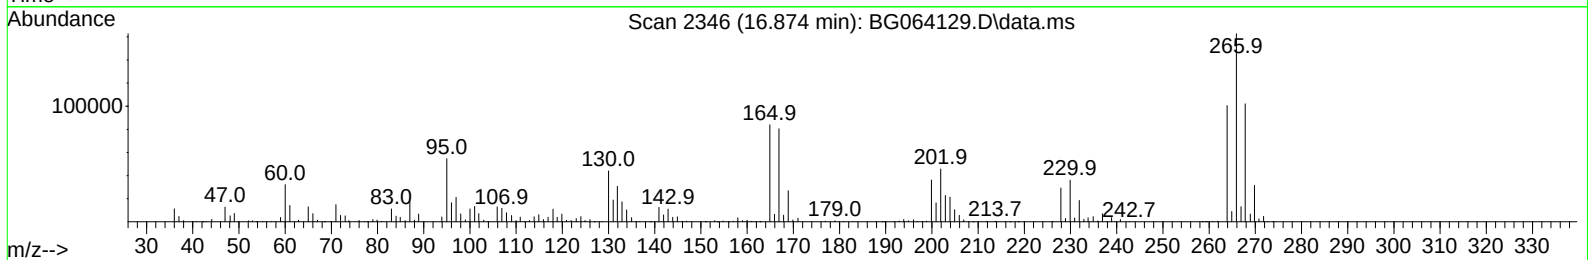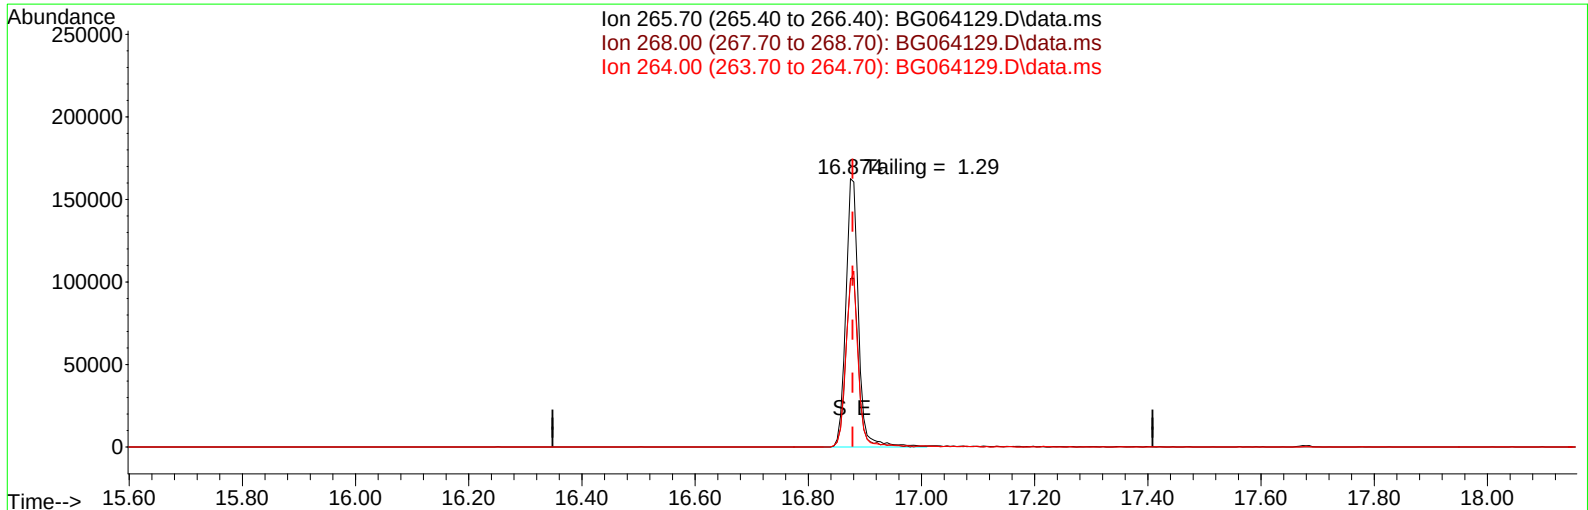

TIC: BG064129.D\data.ms

(70) Pentachlorophenol (C)

16.874min (-0.004) 18192.74 ng




response 250619

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	62.76
264.00	61.10	61.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040125\
Data File : BG064129.D
Acq On : 1 Apr 2025 10:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 01 12:38:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

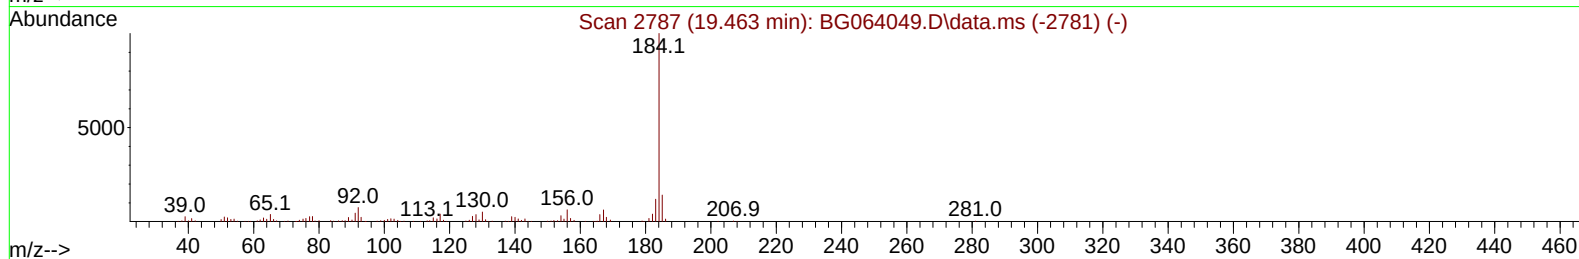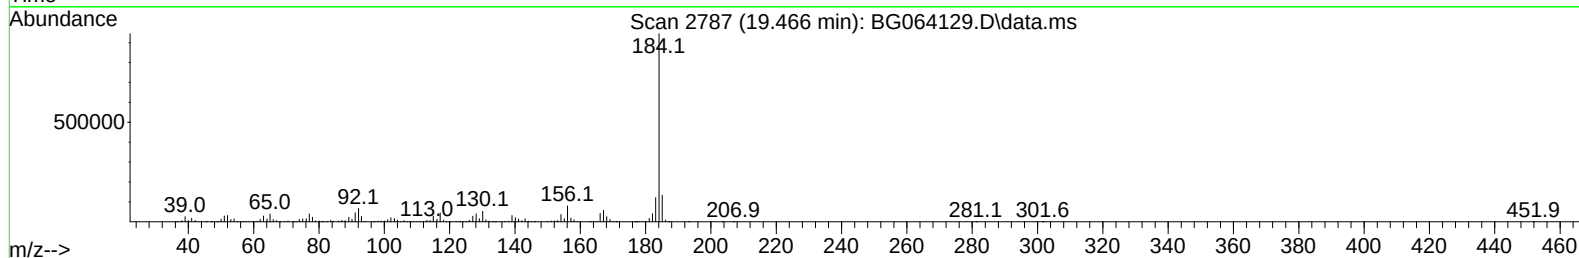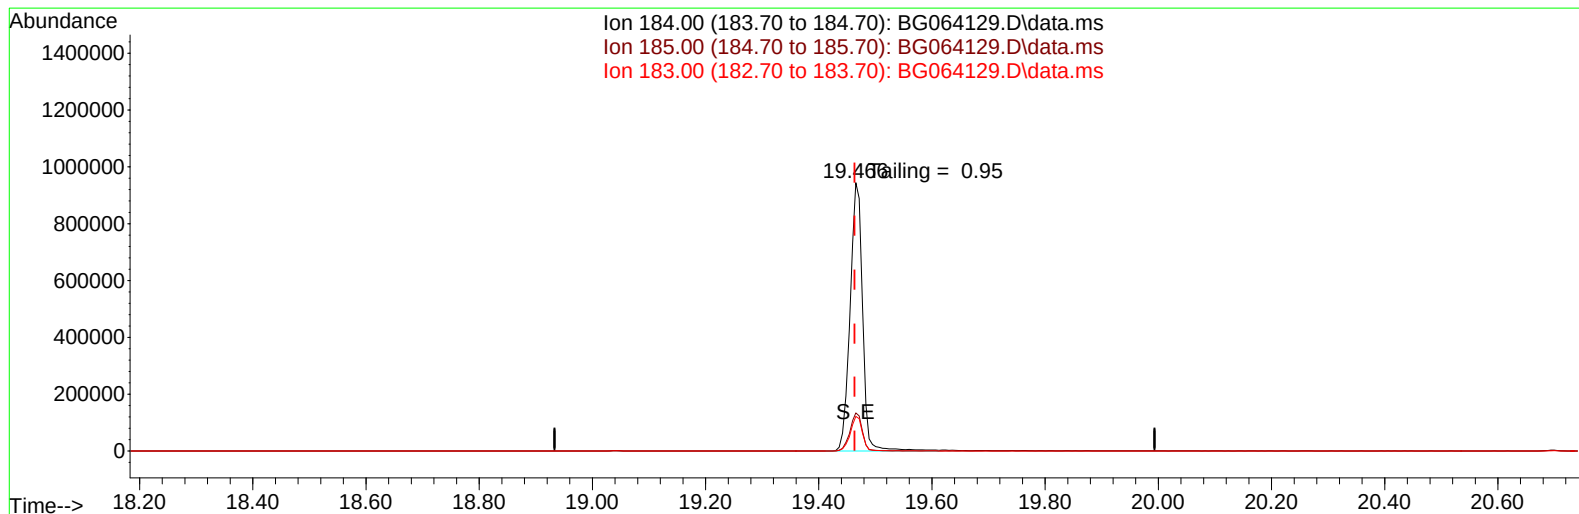

TIC: BG064129.D\data.ms

(77) Benzidine

19.466min (+ 0.003) 44246.31 ng

response 1453902

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.18
183.00	11.90	12.89
0.00	0.00	0.00