
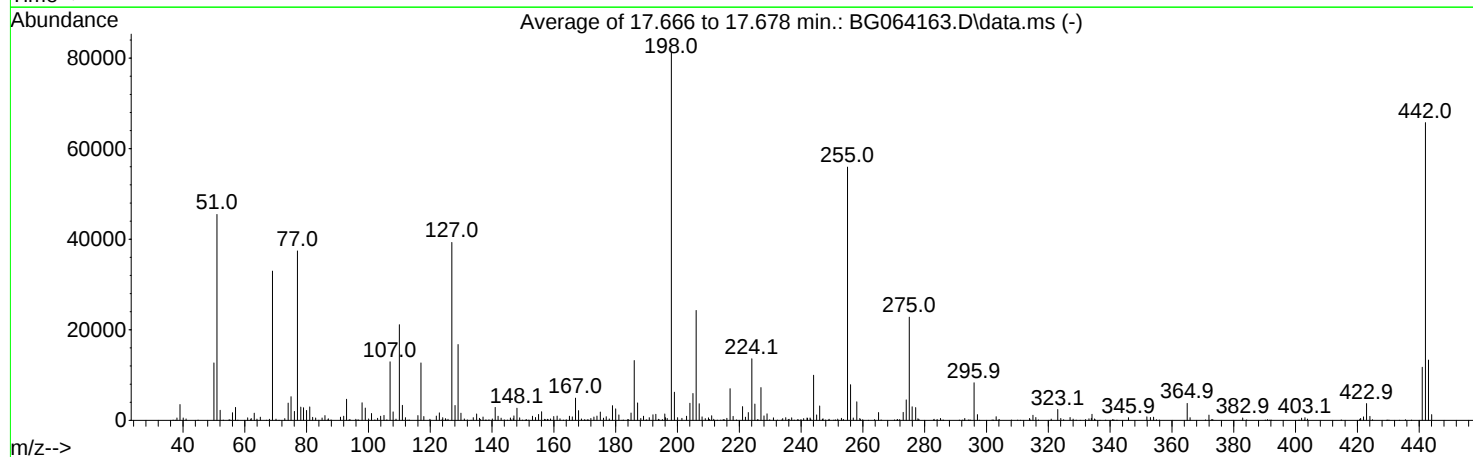


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040325\
Data File : BG064163.D
Acq On : 3 Apr 2025 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Mar 05 15:39:19 2025

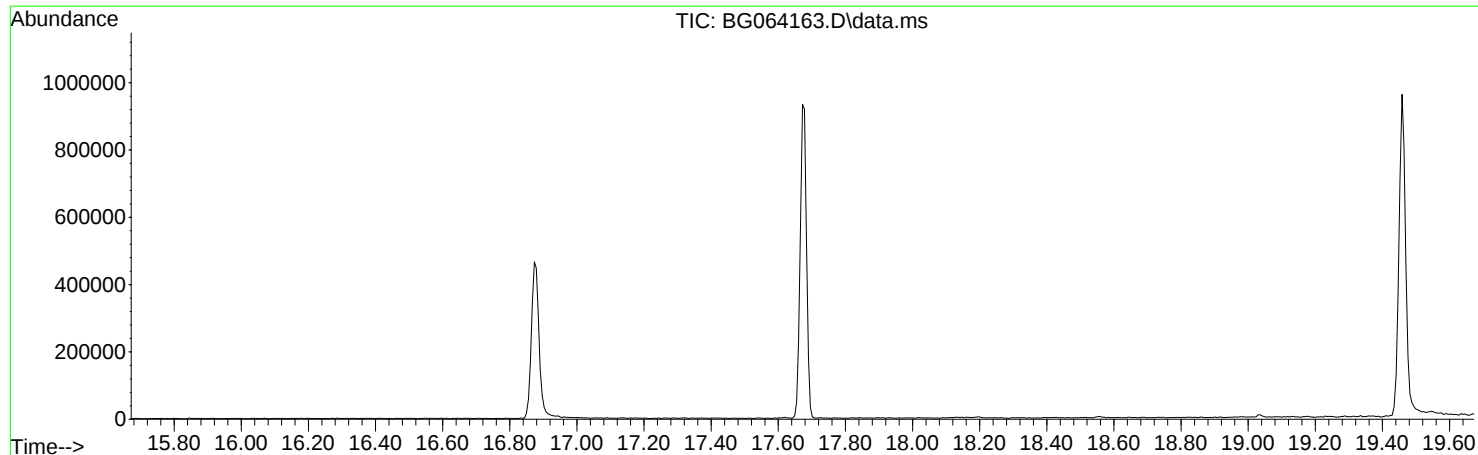




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.0	45483	PASS
68	69	0.00	2	0.8	258	PASS
69	198	0.00	100	40.6	32958	PASS
70	69	0.00	2	0.8	268	PASS
127	198	10	80	48.4	39301	PASS
197	198	0.00	2	0.5	417	PASS
198	198	100	100	100.0	81243	PASS
199	198	5	9	7.7	6234	PASS
275	198	10	60	28.1	22810	PASS
365	198	1	100	4.6	3760	PASS
441	198	0.01	100	14.4	11719	PASS
442	442	50	100	100.0	65776	PASS
443	442	15	24	20.2	13319	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040325\
Data File : BG064163.D
Acq On : 3 Apr 2025 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 03 13:51:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

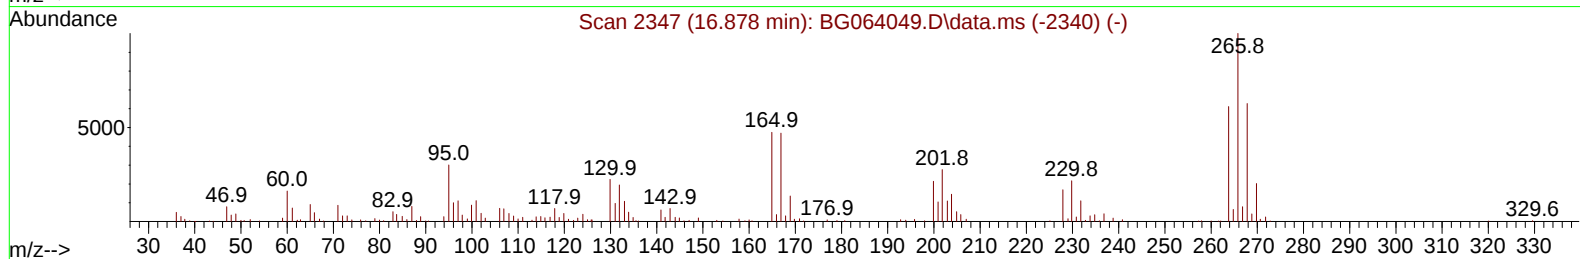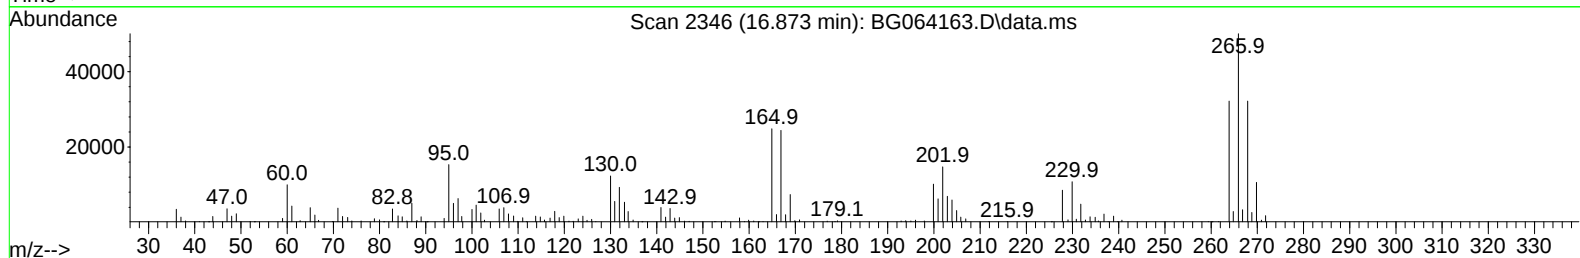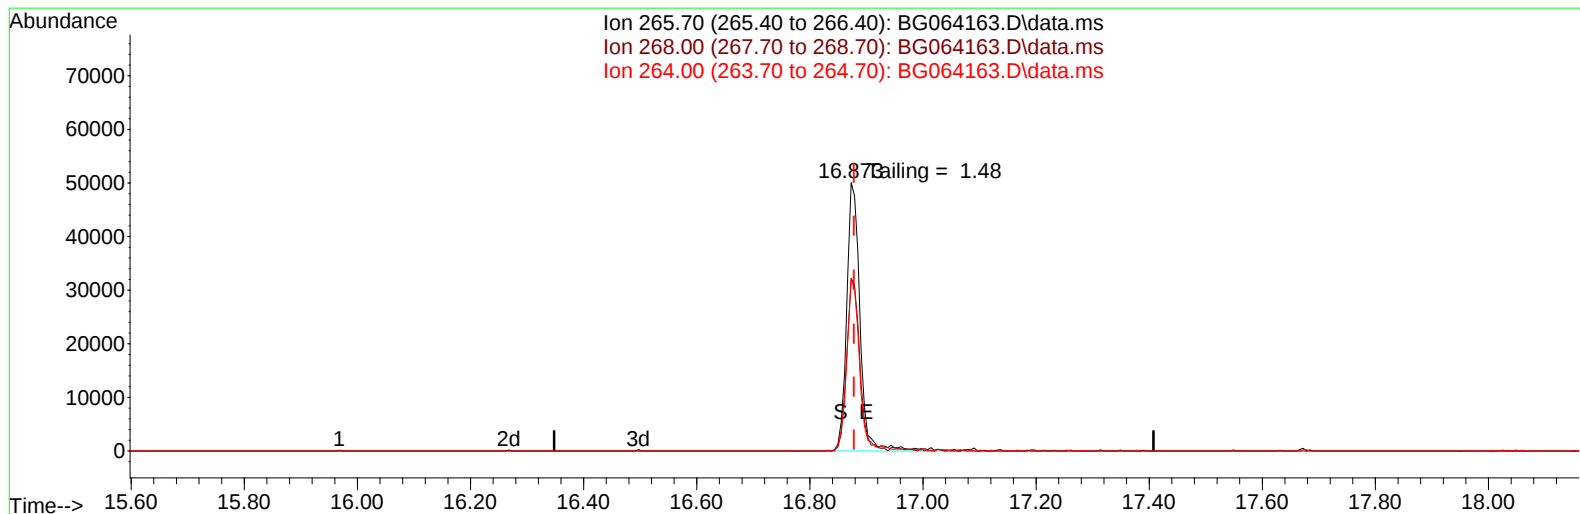

TIC: BG064163.D\data.ms

(70) Pentachlorophenol (C)

16.873min (-0.005) 143328.78 ng m




response 82652

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	64.32
264.00	61.10	64.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040325\
Data File : BG064163.D
Acq On : 3 Apr 2025 12:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 03 13:51:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

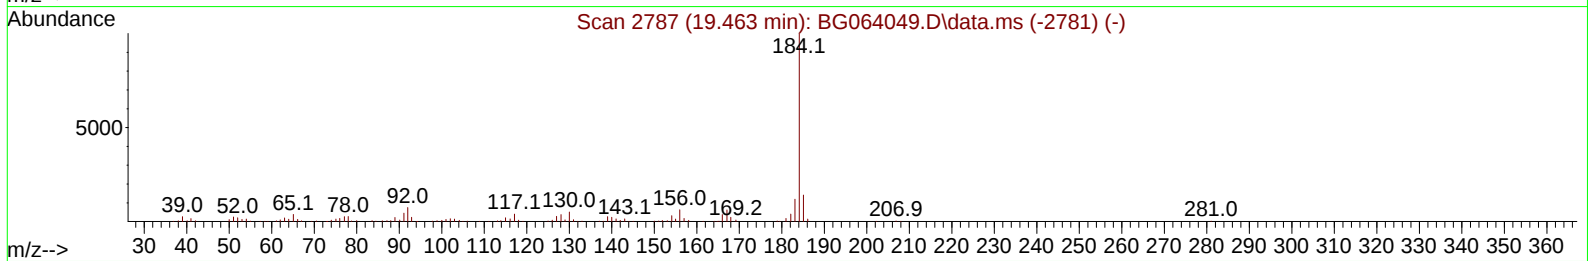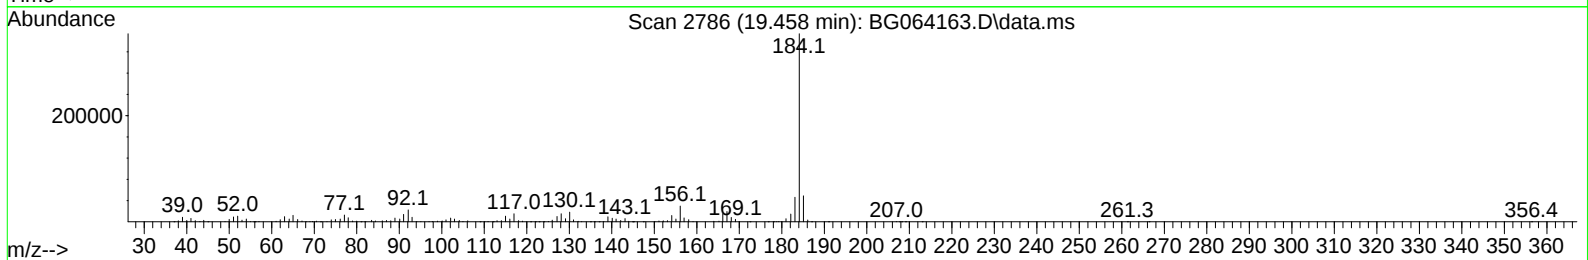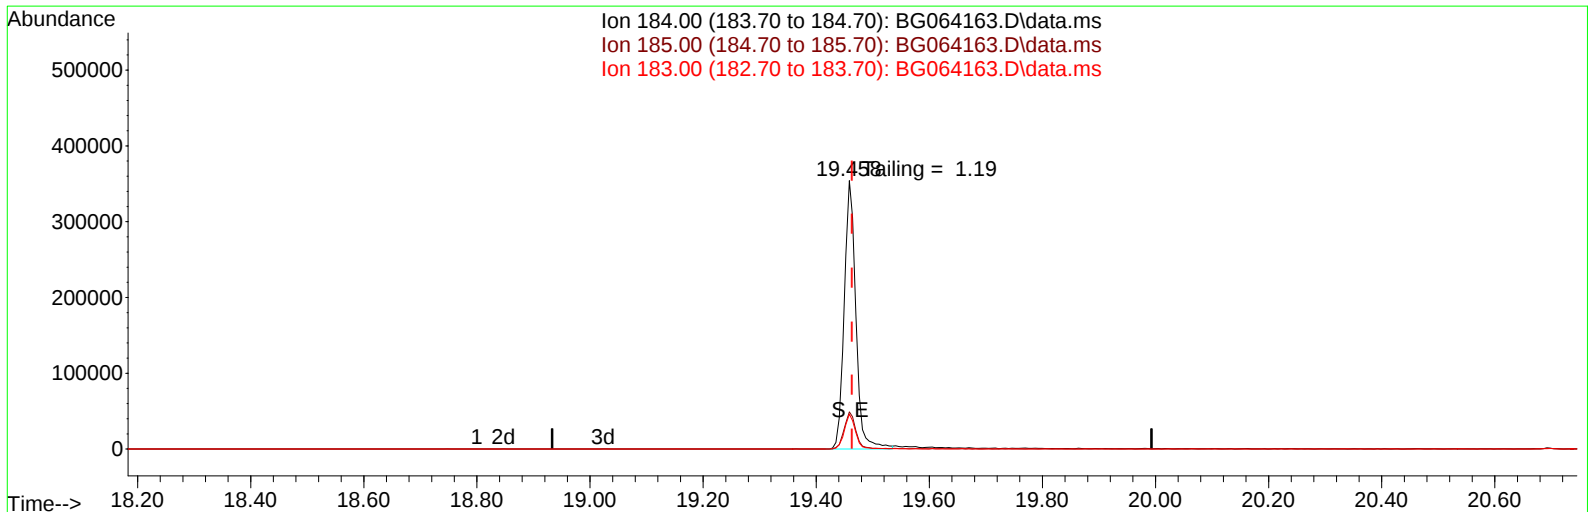

TIC: BG064163.D\data.ms

(77) Benzidine

19.458min (-0.005) 9423.30 ng m

response 527163

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.84
183.00	11.90	13.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/3/2025	BNA_G	<u>BG064163.D</u>
Compound Name	Response	Retention Time
DDT	247452	20.698
DDD	6772	20.257
DDE	773	19.752
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7545	254997	2.96

Instrument :
BNA_G
ClientSampleId :
DFTPP