

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL011425

Review By	sam	Review On	1/15/2025 1:00:29 PM
Supervise By		Supervise On	
SubDirectory	VL011425	HP Acquire Method	TO15AIR.M
		HP Processing Method	VL011425AIR.M
STD. NAME	STD REF.#		
Tune/Reschk	AP2569		
Initial Calibration Stds	AP2571,AP2572,AP2573		
CCC	AP2571		
Internal Standard/PEM	AP2569		
ICV/I.BLK	AP2574,MDL,AP2572,AP2573		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VL041887.D	14 Jan 2025 07:50	SY/MD	Ok
2	VSTDICC0.5	VL041888.D	14 Jan 2025 11:40	SY/MD	Not Ok
3	VSTDICCC010	VL041889.D	14 Jan 2025 12:55	SY/MD	Ok,M
4	VSTDICC002	VL041890.D	14 Jan 2025 13:28	SY/MD	Ok,M
5	VSTDICC001	VL041891.D	14 Jan 2025 13:59	SY/MD	Ok,M
6	VSTDICC0.5	VL041892.D	14 Jan 2025 14:30	SY/MD	Ok,M
7	VSTDICC0.1	VL041893.D	14 Jan 2025 15:01	SY/MD	Ok,M
8	VSTDICC0.03	VL041894.D	14 Jan 2025 15:32	SY/MD	Ok,M
9	VSTDICC015	VL041895.D	14 Jan 2025 16:05	SY/MD	Ok,M
10	VSTDICV010	VL041896.D	14 Jan 2025 17:33	SY/MD	Ok,M
11	VL0114ABL01	VL041897.D	14 Jan 2025 18:34	SY/MD	Ok
12	VL0114ABL02	VL041898.D	14 Jan 2025 19:05	SY/MD	Ok
13	VL0114ABS01	VL041899.D	14 Jan 2025 19:36	SY/MD	Ok,M
14	VIBLK	VL041900.D	14 Jan 2025 20:07	SY/MD	Ok
15	Q1073-04	VL041901.D	14 Jan 2025 20:40	SY/MD	Ok,M
16	Q1073-04DUP	VL041902.D	14 Jan 2025 21:14	SY/MD	Ok,M
17	Q1073-05	VL041903.D	14 Jan 2025 21:47	SY/MD	Ok,M
18	Q1073-06	VL041904.D	14 Jan 2025 22:21	SY/MD	Ok,M
19	Q1073-01	VL041905.D	14 Jan 2025 22:51	SY/MD	Ok,M
20	Q1073-02	VL041906.D	14 Jan 2025 23:22	SY/MD	Ok,M
21	Q1073-03	VL041907.D	14 Jan 2025 23:52	SY/MD	Ok,M

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL011425

Review By	sam	Review On	1/15/2025 1:00:29 PM
Supervise By		Supervise On	
SubDirectory	VL011425	HP Acquire Method	TO15AIR.M
		HP Processing Method	VL011425AIR.M
STD. NAME	STD REF.#		
Tune/Reschk	AP2569		
Initial Calibration Stds	AP2571,AP2572,AP2573		
CCC	AP2571		
Internal Standard/PEM	AP2569		
ICV/I.BLK	AP2574,MDL,AP2572,AP2573		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	VIBLK	VL041908.D	15 Jan 2025 00:22	SY/MD	Ok
23	MDL 0.4	VL041909.D	15 Jan 2025 00:52	SY/MD	Ok,M
24	MDL 0.4	VL041910.D	15 Jan 2025 01:23	SY/MD	Ok,M
25	MDL 0.1	VL041911.D	15 Jan 2025 01:53	SY/MD	Ok,M
26	MDL 0.1	VL041912.D	15 Jan 2025 02:23	SY/MD	Ok,M
27	MDL 0.03	VL041913.D	15 Jan 2025 02:53	SY/MD	Ok,M
28	MDL 0.03	VL041914.D	15 Jan 2025 03:23	SY/MD	Ok,M
29	VSTDCCC010	VL041915.D	15 Jan 2025 08:37	SY/MD	Not Ok

M : Manual Integration

Instrument ID: **MSVOA_L**

Daily Analysis Runlog For Sequence/QC Batch ID # VL020325

Review By	MMDadoda	Review On	2/4/2025 3:44:53 PM
Supervise By		Supervise On	
SubDirectory	VL020325	HP Acquire Method	TO15AIR.M
		HP Processing Method	VL011425AIR.M
STD. NAME	STD REF.#		
Tune/Reschk	AP2569		
Initial Calibration Stds	AP2571,AP2572,AP2573		
CCC	AP2571		
Internal Standard/PEM	AP2569		
ICV/I.BLK	AP2574		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	BFB	VL041957.D	03 Feb 2025 09:47	SY/MD	Ok
2	VSTDCCC010	VL041958.D	03 Feb 2025 10:48	SY/MD	Ok,M
3	VL0203ABL01	VL041959.D	03 Feb 2025 11:34	SY/MD	Ok
4	VL0203ABL02	VL041960.D	03 Feb 2025 12:05	SY/MD	Ok
5	VL0203ABS01	VL041961.D	03 Feb 2025 12:57	SY/MD	Ok,M
6	Q1222-01	VL041962.D	03 Feb 2025 13:57	SY/MD	Ok,M
7	Q1222-01DL	VL041963.D	03 Feb 2025 14:28	SY/MD	Not Ok
8	Q1256-01	VL041964.D	03 Feb 2025 14:59	SY/MD	Ok,M
9	Q1256-01DL	VL041965.D	03 Feb 2025 15:30	SY/MD	Not Ok
10	QC012825 CAN 10439	VL041966.D	03 Feb 2025 16:02	SY/MD	Ok
11	Q1222-02	VL041967.D	03 Feb 2025 16:35	SY/MD	Ok,M
12	Q1222-02DUP	VL041968.D	03 Feb 2025 17:08	SY/MD	Ok,M
13	Q1222-03	VL041969.D	03 Feb 2025 17:41	SY/MD	Ok,M
14	Q1256-02	VL041970.D	03 Feb 2025 18:15	SY/MD	Ok,M
15	Q1168-14 0.03	VL041971.D	03 Feb 2025 21:01	SY/MD	Not Ok
16	Q1168-13 0.03	VL041972.D	03 Feb 2025 21:32	SY/MD	Ok,M
17	Q1168-14 0.03	VL041973.D	03 Feb 2025 22:13	SY/MD	Ok,M
18	QC020325 CAN 10599	VL041974.D	04 Feb 2025 08:03	SY/MD	Ok
19	VSTDCCC010	VL041975.D	04 Feb 2025 08:34	SY/MD	Ok,M

M : Manual Integration

Process Report

Order ID : Q1665

Date	Bottle ID	Lab Sample Number	InComing Vacuum	Canister ID	Can Size	Reg ID	Reg Size	Batch Code	Certification ID
03/31/2025	B2502051	Q1665-19	-8.0	10331	6 L	10206		C2502003	VL042078.D Seq :VL030325 TUNE : VL042074.D ICAL : VL042046.D CCAL : VL042075.D MB : VL042076.D
03/31/2025	B2502051	Q1665-21	-7.5	10332	6 L	10236		C2502002	VL042052.D Seq :VL022625 TUNE : VL042049.D ICAL : VL042046.D CCAL : VL042050.D MB : VL042051.D
03/31/2025	B2502051	Q1665-16	-8.0	10608	6 L	10240		C2502001	VL041974.D Seq :VL020325 TUNE : VL041957.D ICAL : VL041894.D CCAL : VL041958.D MB : VL041960.D
03/31/2025	B2502051	Q1665-09	-5.5	10599	6 L	10207		C2502001	VL041974.D Seq :VL020325 TUNE : VL041957.D ICAL : VL041894.D CCAL : VL041958.D MB : VL041960.D
03/31/2025	B2502051	Q1665-11	-6.3	10598	6 L	10515		C2502001	VL041974.D Seq :VL020325 TUNE : VL041957.D ICAL : VL041894.D CCAL : VL041958.D MB : VL041960.D
03/31/2025	B2502051	Q1665-20	-5.5	10595	6 L	10626		C2502002	VL042052.D Seq :VL022625 TUNE : VL042049.D ICAL : VL042046.D CCAL : VL042050.D MB : VL042051.D

Process Report

Order ID : Q1665

Date	Bottle ID	Lab Sample Number	InComing Vacuum	Canister ID	Can Size	Reg ID	Reg Size	Batch Code	Certification ID
03/31/2025	B2502051	Q1665-07	-6.7	10592	6 L	10558		C2502002	VL042052.D Seq :vl022625 TUNE : VL042049.D ICAL : VL042046.D CCAL : VL042050.D MB : VL042051.D
03/31/2025	B2502051	Q1665-10	-7.1	10492	6 L	10172		C2503001	VL042143.D Seq :VL031425 TUNE : VL042140.D ICAL : VL042046.D CCAL : VL042141.D MB : VL042142.D
03/31/2025	B2502051	Q1665-02	-3.5	10443	6 L	10203		C2501001	VL041853.D Seq :vl010725 TUNE : VL041836.D ICAL : VL041843.D CCAL : VL041838.D MB : VL041846.D
03/31/2025	B2502051	Q1665-01	-8.8	10323	6 L	10478		C2502001	VL041974.D Seq :vl020325 TUNE : VL041957.D ICAL : VL041894.D CCAL : VL041958.D MB : VL041960.D
03/31/2025	B2502051	Q1665-13	-1.8	10315	6 L	10183		C2502003	VL042078.D Seq :VL030325 TUNE : VL042074.D ICAL : VL042046.D CCAL : VL042075.D MB : VL042076.D
03/31/2025	B2502051	Q1665-22	-7.1	10306	6 L	10713		C2502002	VL042052.D Seq :vl022625 TUNE : VL042049.D ICAL : VL042046.D CCAL : VL042050.D MB : VL042051.D
03/31/2025	B2502051	Q1665-18	-8.0	10297	6 L	10190		C2502001	VL041974.D Seq :vl020325 TUNE : VL041957.D ICAL : VL041894.D CCAL : VL041958.D MB : VL041960.D

Process Report

Order ID : Q1665

Date	Bottle ID	Lab Sample Number	InComing Vacuum	Canister ID	Can Size	Reg ID	Reg Size	Batch Code	Certification ID
03/31/2025	B2502051	Q1665-17	-6.7	10294	6 L	10505		C2502003	VL042078.D Seq :VL030325 TUNE : VL042074.D ICAL : VL042046.D CCAL : VL042075.D MB : VL042076.D
03/31/2025	B2502051	Q1665-05	-8.0	10281	6 L	10552		C2502002	VL042052.D Seq :VL022625 TUNE : VL042049.D ICAL : VL042046.D CCAL : VL042050.D MB : VL042051.D
03/31/2025	B2502051	Q1665-14	-7.1	10275	6 L	10482		C2502003	VL042078.D Seq :VL030325 TUNE : VL042074.D ICAL : VL042046.D CCAL : VL042075.D MB : VL042076.D
03/31/2025	B2502051	Q1665-12	-13.7	10271	6 L	10222		C2502002	VL042052.D Seq :VL022625 TUNE : VL042049.D ICAL : VL042046.D CCAL : VL042050.D MB : VL042051.D
03/31/2025	B2502051	Q1665-04	-7.1	10268	6 L	10101		C2501003	VL041954.D Seq :VL012725 TUNE : VL041943.D ICAL : VL041894.D CCAL : VL041944.D MB : VL041946.D
03/31/2025	B2502051	Q1665-15	-6.3	10266	6 L	10696		C2503003	VL042145.D Seq :VL031425 TUNE : VL042140.D ICAL : VL042046.D CCAL : VL042141.D MB : VL042142.D
03/31/2025	B2502051	Q1665-06	-12.0	10198	6 L	10204		C2502002	VL042052.D Seq :VL022625 TUNE : VL042049.D ICAL : VL042046.D CCAL : VL042050.D MB : VL042051.D

Process Report

Order ID : Q1665

Date	Bottle ID	Lab Sample Number	InComing Vacuum	Canister ID	Can Size	Reg ID	Reg Size	Batch Code	Certification ID
03/31/2025	B2502051	Q1665-03	-8.4	10154	6 L	10476		C2502001	VL041974.D Seq :vl020325 TUNE : VL041957.D ICAL : VL041894.D CCAL : VL041958.D MB : VL041960.D
03/31/2025	B2502051	Q1665-08	-7.5	10053	6 L	10168		C2502001	VL041974.D Seq :vl020325 TUNE : VL041957.D ICAL : VL041894.D CCAL : VL041958.D MB : VL041960.D

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041889.D
 Acq On : 14 Jan 2025 12:55
 Operator : SY/MD
 Sample : VSTDICCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 01/15/2025
 Supervised By : Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 21:20:11 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jan 14 16:31:18 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.797	49	152325	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.975	114	449256	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.894	117	400269	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	10.390	95	313194	9.934	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.300%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.502	85	197959	9.541	ppbv	100
3) Chlorodifluoromethane	1.479	51	202651	9.323	ppbv	100
4) Chloromethane	1.538	50	74977	9.608	ppbv	100
5) Vinyl Chloride	1.583	62	71006	8.984	ppbv	100
6) Bromomethane	1.674	94	34817	9.243	ppbv	100
7) Chloroethane	1.709	64	29349	9.544	ppbv	100
8) Dichlorotetrafluoroethane	1.557	85	166754	9.196	ppbv	100
9) Propene	1.486	41	86544	9.665	ppbv	100
10) Heptane	5.001	43	233062	9.738	ppbv	100
11) Trichlorofluoromethane	1.884	101	203374	9.423	ppbv	100
12) 1,1,2-Trichlorotrifluo...	2.146	101	160993	9.517	ppbv	100
13) Ethanol	1.725	45	4155	6.335	ppbv	98
14) Bromoethene	1.787	108	56447	9.114	ppbv	100
15) Acetone	1.842	43	151022	8.255	ppbv	100
16) 1,3-Butadiene	1.612	39	75244	9.163	ppbv	100
17) tert-Butyl alcohol	2.046	59	213109	9.464	ppbv	100
18) 1,1-Dichloroethene	2.039	96	69825	9.158	ppbv	100
19) Isopropyl Alcohol	1.890	45	94532	8.714	ppbv	100
20) Methylene Chloride	2.068	84	59427	8.219	ppbv	100
21) Allyl Chloride	2.101	41	120681	9.526	ppbv	100
22) trans-1,2-Dichloroethene	2.347	96	82326	9.568	ppbv	100
23) Vinyl Acetate	2.470	43	81885	10.281	ppbv	100
24) 1,1-Dichloroethane	2.418	63	154838	9.303	ppbv	100
25) Ethyl Acetate	2.845	43	471257	9.552	ppbv	100
26) Hexane	2.835	57	192009	9.841	ppbv	100
27) Carbon Disulfide	2.156	76	191567	9.921	ppbv	99
28) Methyl tert-Butyl Ether	2.450	73	117898	7.905	ppbv	100
29) Chloroform	2.858	83	291118	9.438	ppbv	100
30) Cyclohexane	3.868	84	164788	9.737	ppbv	100
31) cis-1,2-Dichloroethene	2.729	61	193774	9.432	ppbv	100
32) 1,1,1-Trichloroethane	3.379	97	290126	9.830	ppbv	100
34) 2-Butanone	2.567	43	270263	9.459	ppbv	100
35) Carbon Tetrachloride	3.777	117	291448	10.309	ppbv	100
36) Benzene	3.671	78	396344	9.619	ppbv	100
37) 1,2-Dichloroethane	3.230	62	221352	9.565	ppbv	100
38) Trichloroethene	4.564	130	159253	9.736	ppbv	100
39) 1,2-Dichloropropane	4.331	63	137090	9.484	ppbv	100
40) 1,4-Dioxane	4.606	88	66200	9.075	ppbv #	94
41) Tetrahydrofuran	3.065	42	156141	10.023	ppbv	100
42) Bromodichloromethane	4.509	83	307176	9.900	ppbv	100
43) Methyl Methacrylate	4.897	69	152001	9.930	ppbv	100
44) 2,2,4-Trimethylpentane	4.658	57	654395	9.819	ppbv	100
45) t-1,3-Dichloropropene	6.435	75	151920	10.603	ppbv	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041889.D
 Acq On : 14 Jan 2025 12:55
 Operator : SY/MD
 Sample : VSTDICCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICCC010

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 01/15/2025
 Supervised By :Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 21:20:11 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jan 14 16:31:18 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.622	75	200330	10.649	ppbv	100
47) 1,1,2-Trichloroethane	6.600	97	149634	9.766	ppbv	100
48) Dibromochloromethane	7.402	129	245066	10.368	ppbv	100
49) Bromoform	9.496	173	206751	10.649	ppbv	100
50) 4-Methyl-2-Pentanone	5.778	43	374267	9.615	ppbv	100
51) 2-Hexanone	7.454	43	292941	9.775	ppbv #	100
52) Tetrachloroethene	8.241	164	131334	9.193	ppbv	100
53) Toluene	6.952	91	454085	10.116	ppbv	100
54) 1,2-Dibromoethane	7.668	107	203859	9.679	ppbv	100
56) 1,1,1,2-Tetrachloroethane	8.940	131	192449	9.637	ppbv	99
57) Chlorobenzene	8.937	112	339570	9.197	ppbv	100
58) Ethyl Benzene	9.367	91	620719	9.923	ppbv	100
59) m/p-Xylene	9.564	91	979297m	19.504	ppbv	
60) o-Xylene	9.979	91	490108	9.848	ppbv	100
61) Styrene	9.885	104	234901	10.522	ppbv	100
62) Isopropylbenzene	10.552	105	742261	9.638	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.976	83	300600	9.596	ppbv	100
64) n-propylbenzene	11.002	120	187706	9.646	ppbv	99
65) tert-Butylbenzene	11.542	119	670259	9.550	ppbv	100
66) Benzyl Chloride	11.626	91	46008	10.591	ppbv	100
67) sec-Butylbenzene	11.778	105	920046	9.521	ppbv	100
69) p-Isopropyltoluene	11.937	119	771465	9.694	ppbv	100
70) n-Butylbenzene	12.293	91	759785	9.627	ppbv	100
71) 2-Chlorotoluene	10.914	91	556170	9.763	ppbv	100
72) 4-Ethyltoluene	11.137	105	586667	9.855	ppbv	100
73) 1,3,5-Trimethylbenzene	11.215	105	505443	9.614	ppbv	100
74) 1,2,4-Trimethylbenzene	11.549	105	538665	9.461	ppbv	100
75) 1,3-Dichlorobenzene	11.620	146	310421	9.201	ppbv	100
76) 1,4-Dichlorobenzene	11.684	146	307758	9.324	ppbv	100
77) 1,2-Dichlorobenzene	11.960	146	303196	9.068	ppbv	100
78) Hexachloro-1,3-Butadiene	13.895	225	234457	8.543	ppbv	100
79) Naphthalene	13.526	128	502354	8.764	ppbv	100
80) Naphthalene,2-methyl-	14.471	142	185336	6.819	ppbv	100
81) 1,2,4-Trichlorobenzene	13.452	180	239317	8.553	ppbv	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
Data File : VL041889.D
Acq On : 14 Jan 2025 12:55
Operator : SY/MD
Sample : VSTDICCC010
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICCC010

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 01/15/2025
Supervised By : Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 21:20:11 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Tue Jan 14 16:31:18 2025
Response via : Initial Calibration

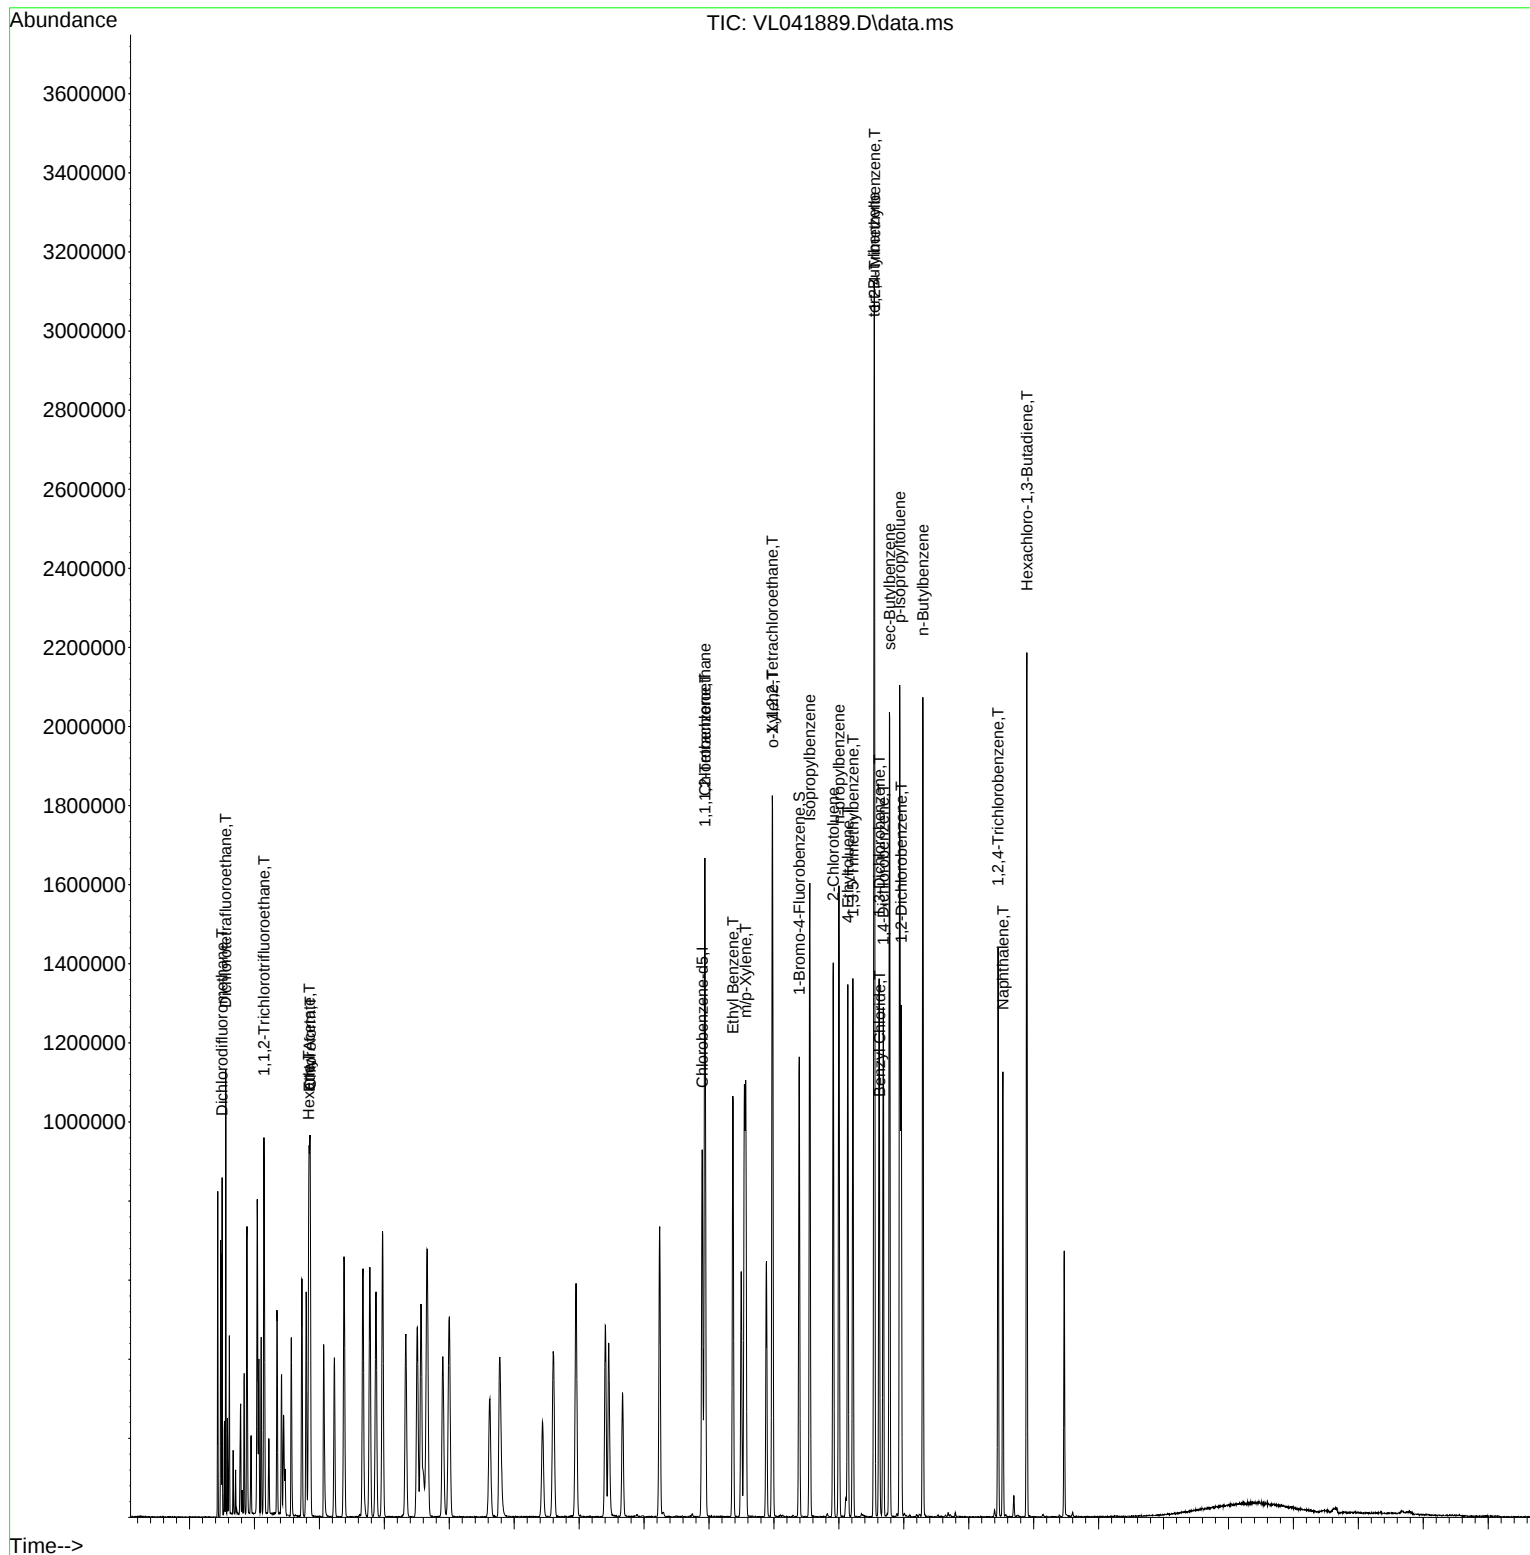

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041890.D
 Acq On : 14 Jan 2025 13:28
 Operator : SY/MD
 Sample : VSTDICC002
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC002

Quant Time: Jan 14 21:20:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Tue Jan 14 16:31:18 2025
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 01/15/2025
 Supervised By : Mahesh Dadoda 01/15/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.797	49	150761	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.971	114	452131	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.894	117	394865	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	10.390	95	313784	10.089	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	100.900%

Target Compounds					Qvalue	
2) Dichlorodifluoromethane	1.502	85	40991	1.996	ppbv	98
3) Chlorodifluoromethane	1.479	51	44207	2.055	ppbv	99
4) Chloromethane	1.538	50	15833	2.050	ppbv	93
5) Vinyl Chloride	1.583	62	15137	1.935	ppbv	99
6) Bromomethane	1.673	94	7486	2.008	ppbv	91
7) Chloroethane	1.709	64	6303	2.071	ppbv #	84
8) Dichlorotetrafluoroethane	1.557	85	36941	2.058	ppbv	99
9) Propene	1.486	41	18248	2.059	ppbv	95
10) Heptane	5.001	43	49302	2.081	ppbv	97
11) Trichlorofluoromethane	1.884	101	43266	2.025	ppbv	97
12) 1,1,2-Trichlorotrifluo...	2.146	101	35162	2.100	ppbv	97
13) Ethanol	1.725	45	1534	2.363	ppbv	84
14) Bromoethene	1.787	108	12163	1.984	ppbv #	95
15) Acetone	1.842	43	37867	2.091	ppbv	99
16) 1,3-Butadiene	1.612	39	16446	2.024	ppbv	100
17) tert-Butyl alcohol	2.049	59	45305	2.033	ppbv	99
18) 1,1-Dichloroethene	2.039	96	15508	2.055	ppbv	97
19) Isopropyl Alcohol	1.894	45	21530	2.005	ppbv	94
20) Methylene Chloride	2.068	84	14399	2.012	ppbv	95
21) Allyl Chloride	2.104	41	25533	2.036	ppbv	97
22) trans-1,2-Dichloroethene	2.350	96	17951	2.108	ppbv	83
23) Vinyl Acetate	2.470	43	16358	2.075	ppbv	99
24) 1,1-Dichloroethane	2.418	63	33175	2.014	ppbv	99
25) Ethyl Acetate	2.848	43	102475	2.099	ppbv	99
26) Hexane	2.835	57	41844	2.167	ppbv	99
27) Carbon Disulfide	2.156	76	39306	2.057	ppbv #	70
28) Methyl tert-Butyl Ether	2.454	73	30355	2.056	ppbv	96
29) Chloroform	2.858	83	63457	2.079	ppbv	94
30) Cyclohexane	3.874	84	34518	2.061	ppbv	97
31) cis-1,2-Dichloroethene	2.729	61	41921	2.062	ppbv	89
32) 1,1,1-Trichloroethane	3.382	97	58965	2.019	ppbv	98
34) 2-Butanone	2.570	43	61381	2.135	ppbv	99
35) Carbon Tetrachloride	3.777	117	59430	2.089	ppbv	95
36) Benzene	3.670	78	85859	2.070	ppbv	96
37) 1,2-Dichloroethane	3.230	62	46786	2.009	ppbv	100
38) Trichloroethene	4.564	130	33773	2.052	ppbv	98
39) 1,2-Dichloropropane	4.334	63	29723	2.043	ppbv	96
40) 1,4-Dioxane	4.619	88	14566m	1.984	ppbv	
41) Tetrahydrofuran	3.072	42	32358	2.064	ppbv	96
42) Bromodichloromethane	4.509	83	63611	2.037	ppbv	99
43) Methyl Methacrylate	4.900	69	31519	2.046	ppbv	99
44) 2,2,4-Trimethylpentane	4.658	57	141602	2.111	ppbv	100
45) t-1,3-Dichloropropene	6.435	75	28818	1.999	ppbv	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041890.D
 Acq On : 14 Jan 2025 13:28
 Operator : SY/MD
 Sample : VSTDICC002
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC002

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 01/15/2025
 Supervised By :Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 21:20:29 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jan 14 16:31:18 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.625	75	39668	2.095	ppbv	94
47) 1,1,2-Trichloroethane	6.600	97	31694m	2.055	ppbv	
48) Dibromochloromethane	7.406	129	48894	2.055	ppbv	99
49) Bromoform	9.496	173	39710	2.032	ppbv	99
50) 4-Methyl-2-Pentanone	5.784	43	81330	2.076	ppbv	98
51) 2-Hexanone	7.457	43	66831	2.216	ppbv #	98
52) Tetrachloroethene	8.241	164	29814	2.074	ppbv	94
53) Toluene	6.952	91	94741	2.097	ppbv	98
54) 1,2-Dibromoethane	7.671	107	44636	2.106	ppbv	96
56) 1,1,1,2-Tetrachloroethane	8.940	131	40249	2.043	ppbv	93
57) Chlorobenzene	8.933	112	77180	2.119	ppbv	94
58) Ethyl Benzene	9.367	91	130554	2.116	ppbv	98
59) m/p-Xylene	9.561	91	214076m	4.322	ppbv	
60) o-Xylene	9.975	91	106458	2.168	ppbv	99
61) Styrene	9.885	104	45490	2.065	ppbv	99
62) Isopropylbenzene	10.552	105	163135	2.147	ppbv	97
63) 1,1,2,2-Tetrachloroethane	9.975	83	67775	2.193	ppbv	99
64) n-propylbenzene	11.001	120	41184	2.145	ppbv	99
65) tert-Butylbenzene	11.542	119	151534	2.189	ppbv	97
66) Benzyl Chloride	11.626	91	8925	2.083	ppbv	97
67) sec-Butylbenzene	11.778	105	211759	2.221	ppbv	99
69) p-Isopropyltoluene	11.937	119	178172	2.270	ppbv	100
70) n-Butylbenzene	12.293	91	174217	2.238	ppbv	99
71) 2-Chlorotoluene	10.914	91	121418	2.161	ppbv	100
72) 4-Ethyltoluene	11.137	105	127115	2.164	ppbv	100
73) 1,3,5-Trimethylbenzene	11.215	105	114342	2.205	ppbv	99
74) 1,2,4-Trimethylbenzene	11.548	105	126939	2.260	ppbv #	89
75) 1,3-Dichlorobenzene	11.616	146	71332	2.143	ppbv	98
76) 1,4-Dichlorobenzene	11.684	146	70219	2.156	ppbv	99
77) 1,2-Dichlorobenzene	11.960	146	71818	2.177	ppbv	100
78) Hexachloro-1,3-Butadiene	13.892	225	60984	2.253	ppbv	99
79) Naphthalene	13.526	128	153268	2.710	ppbv	98
80) Naphthalene,2-methyl-	14.471	142	90910	3.391	ppbv	99
81) 1,2,4-Trichlorobenzene	13.452	180	64653	2.342	ppbv	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041891.D
 Acq On : 14 Jan 2025 13:59
 Operator : SY/MD
 Sample : VSTDICC001
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC001

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 01/15/2025
 Supervised By : Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 21:20:45 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jan 14 16:31:18 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.797	49	151226	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.972	114	453418	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.895	117	393836	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.387 95 312013 10.058 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 100.600%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.502	85	21262	1.032	ppbv	95
3) Chlorodifluoromethane	1.479	51	23396	1.084	ppbv	100
4) Chloromethane	1.534	50	7546	0.974	ppbv	94
5) Vinyl Chloride	1.583	62	8031	1.023	ppbv	97
6) Bromomethane	1.674	94	4139	1.107	ppbv #	81
7) Chloroethane	1.709	64	3093	1.013	ppbv	92
8) Dichlorotetrafluoroethane	1.557	85	18122	1.007	ppbv	100
9) Propene	1.486	41	8719	0.981	ppbv	93
10) Heptane	5.001	43	24438	1.029	ppbv	96
11) Trichlorofluoromethane	1.884	101	21425	1.000	ppbv	98
12) 1,1,2-Trichlorotrifluo...	2.143	101	17187	1.023	ppbv	95
13) Ethanol	1.725	45	650	0.998	ppbv #	29
14) Bromoethene	1.787	108	6736	1.096	ppbv #	88
15) Acetone	1.842	43	19681	1.084	ppbv	95
16) 1,3-Butadiene	1.612	39	8901	1.092	ppbv	98
17) tert-Butyl alcohol	2.049	59	23571	1.054	ppbv	95
18) 1,1-Dichloroethene	2.039	96	7819m	1.033	ppbv	
19) Isopropyl Alcohol	1.894	45	11054	1.026	ppbv #	32
20) Methylene Chloride	2.065	84	7608	1.060	ppbv #	89
21) Allyl Chloride	2.101	41	12451	0.990	ppbv	98
22) trans-1,2-Dichloroethene	2.347	96	8819	1.032	ppbv	96
23) Vinyl Acetate	2.470	43	7181	0.908	ppbv #	93
24) 1,1-Dichloroethane	2.415	63	16623	1.006	ppbv	97
25) Ethyl Acetate	2.845	43	50690	1.035	ppbv	98
26) Hexane	2.836	57	18893	0.975	ppbv	86
27) Carbon Disulfide	2.156	76	18993	0.991	ppbv #	23
28) Methyl tert-Butyl Ether	2.450	73	17955	1.213	ppbv	98
29) Chloroform	2.858	83	31155	1.017	ppbv	97
30) Cyclohexane	3.871	84	18048	1.074	ppbv	96
31) cis-1,2-Dichloroethene	2.729	61	21124	1.036	ppbv	99
32) 1,1,1-Trichloroethane	3.383	97	30396	1.037	ppbv	98
34) 2-Butanone	2.570	43	29280	1.015	ppbv	99
35) Carbon Tetrachloride	3.774	117	27946	0.979	ppbv	96
36) Benzene	3.671	78	43023	1.035	ppbv	93
37) 1,2-Dichloroethane	3.230	62	23402	1.002	ppbv	98
38) Trichloroethene	4.564	130	16954m	1.027	ppbv	
39) 1,2-Dichloropropane	4.331	63	14570	0.999	ppbv	98
40) 1,4-Dioxane	4.613	88	7345m	0.998	ppbv	
41) Tetrahydrofuran	3.075	42	15580m	0.991	ppbv	
42) Bromodichloromethane	4.509	83	29893m	0.955	ppbv	
43) Methyl Methacrylate	4.901	69	15222	0.985	ppbv	95
44) 2,2,4-Trimethylpentane	4.661	57	68050	1.012	ppbv	98
45) t-1,3-Dichloropropene	6.438	75	13220	0.914	ppbv	92

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041891.D
 Acq On : 14 Jan 2025 13:59
 Operator : SY/MD
 Sample : VSTDICC001
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC001

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 01/15/2025
 Supervised By : Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 21:20:45 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jan 14 16:31:18 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.626	75	17749	0.935	ppbv	97
47) 1,1,2-Trichloroethane	6.603	97	15658m	1.013	ppbv	
48) Dibromochloromethane	7.402	129	22169	0.929	ppbv	100
49) Bromoform	9.497	173	17876	0.912	ppbv	100
50) 4-Methyl-2-Pentanone	5.787	43	39436m	1.004	ppbv	
51) 2-Hexanone	7.464	43	28999	0.959	ppbv #	95
52) Tetrachloroethene	8.244	164	14903	1.034	ppbv #	80
53) Toluene	6.956	91	45140m	0.996	ppbv	
54) 1,2-Dibromoethane	7.668	107	21202	0.997	ppbv	96
56) 1,1,1,2-Tetrachloroethane	8.937	131	20255	1.031	ppbv	94
57) Chlorobenzene	8.933	112	38141	1.050	ppbv	98
58) Ethyl Benzene	9.367	91	61537	1.000	ppbv	99
59) m/p-Xylene	9.561	91	99618m	2.016	ppbv	
60) o-Xylene	9.972	91	48888	0.998	ppbv	98
61) Styrene	9.882	104	20285	0.923	ppbv	99
62) Isopropylbenzene	10.549	105	75801	1.000	ppbv	98
63) 1,1,2,2-Tetrachloroethane	9.972	83	33289	1.080	ppbv	97
64) n-propylbenzene	11.002	120	19511	1.019	ppbv	99
65) tert-Butylbenzene	11.539	119	70183	1.016	ppbv	98
66) Benzyl Chloride	11.626	91	3681m	0.861	ppbv	
67) sec-Butylbenzene	11.778	105	96749	1.018	ppbv	97
69) p-Isopropyltoluene	11.937	119	79283	1.013	ppbv	98
70) n-Butylbenzene	12.290	91	80664	1.039	ppbv	99
71) 2-Chlorotoluene	10.911	91	55540	0.991	ppbv	99
72) 4-Ethyltoluene	11.134	105	56973	0.973	ppbv	97
73) 1,3,5-Trimethylbenzene	11.215	105	53550	1.035	ppbv	97
74) 1,2,4-Trimethylbenzene	11.545	105	57352	1.024	ppbv	96
75) 1,3-Dichlorobenzene	11.617	146	34810	1.049	ppbv	99
76) 1,4-Dichlorobenzene	11.681	146	33822	1.041	ppbv	97
77) 1,2-Dichlorobenzene	11.960	146	35516	1.080	ppbv	98
78) Hexachloro-1,3-Butadiene	13.892	225	29210	1.082	ppbv	99
79) Naphthalene	13.523	128	66232	1.174	ppbv	98
80) Naphthalene,2-methyl-	14.468	142	28506	1.066	ppbv	98
81) 1,2,4-Trichlorobenzene	13.452	180	29053	1.055	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
Data File : VL041891.D
Acq On : 14 Jan 2025 13:59
Operator : SY/MD
Sample : VSTDICC001
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC001

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 21:20:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Tue Jan 14 16:31:18 2025
Response via : Initial Calibration

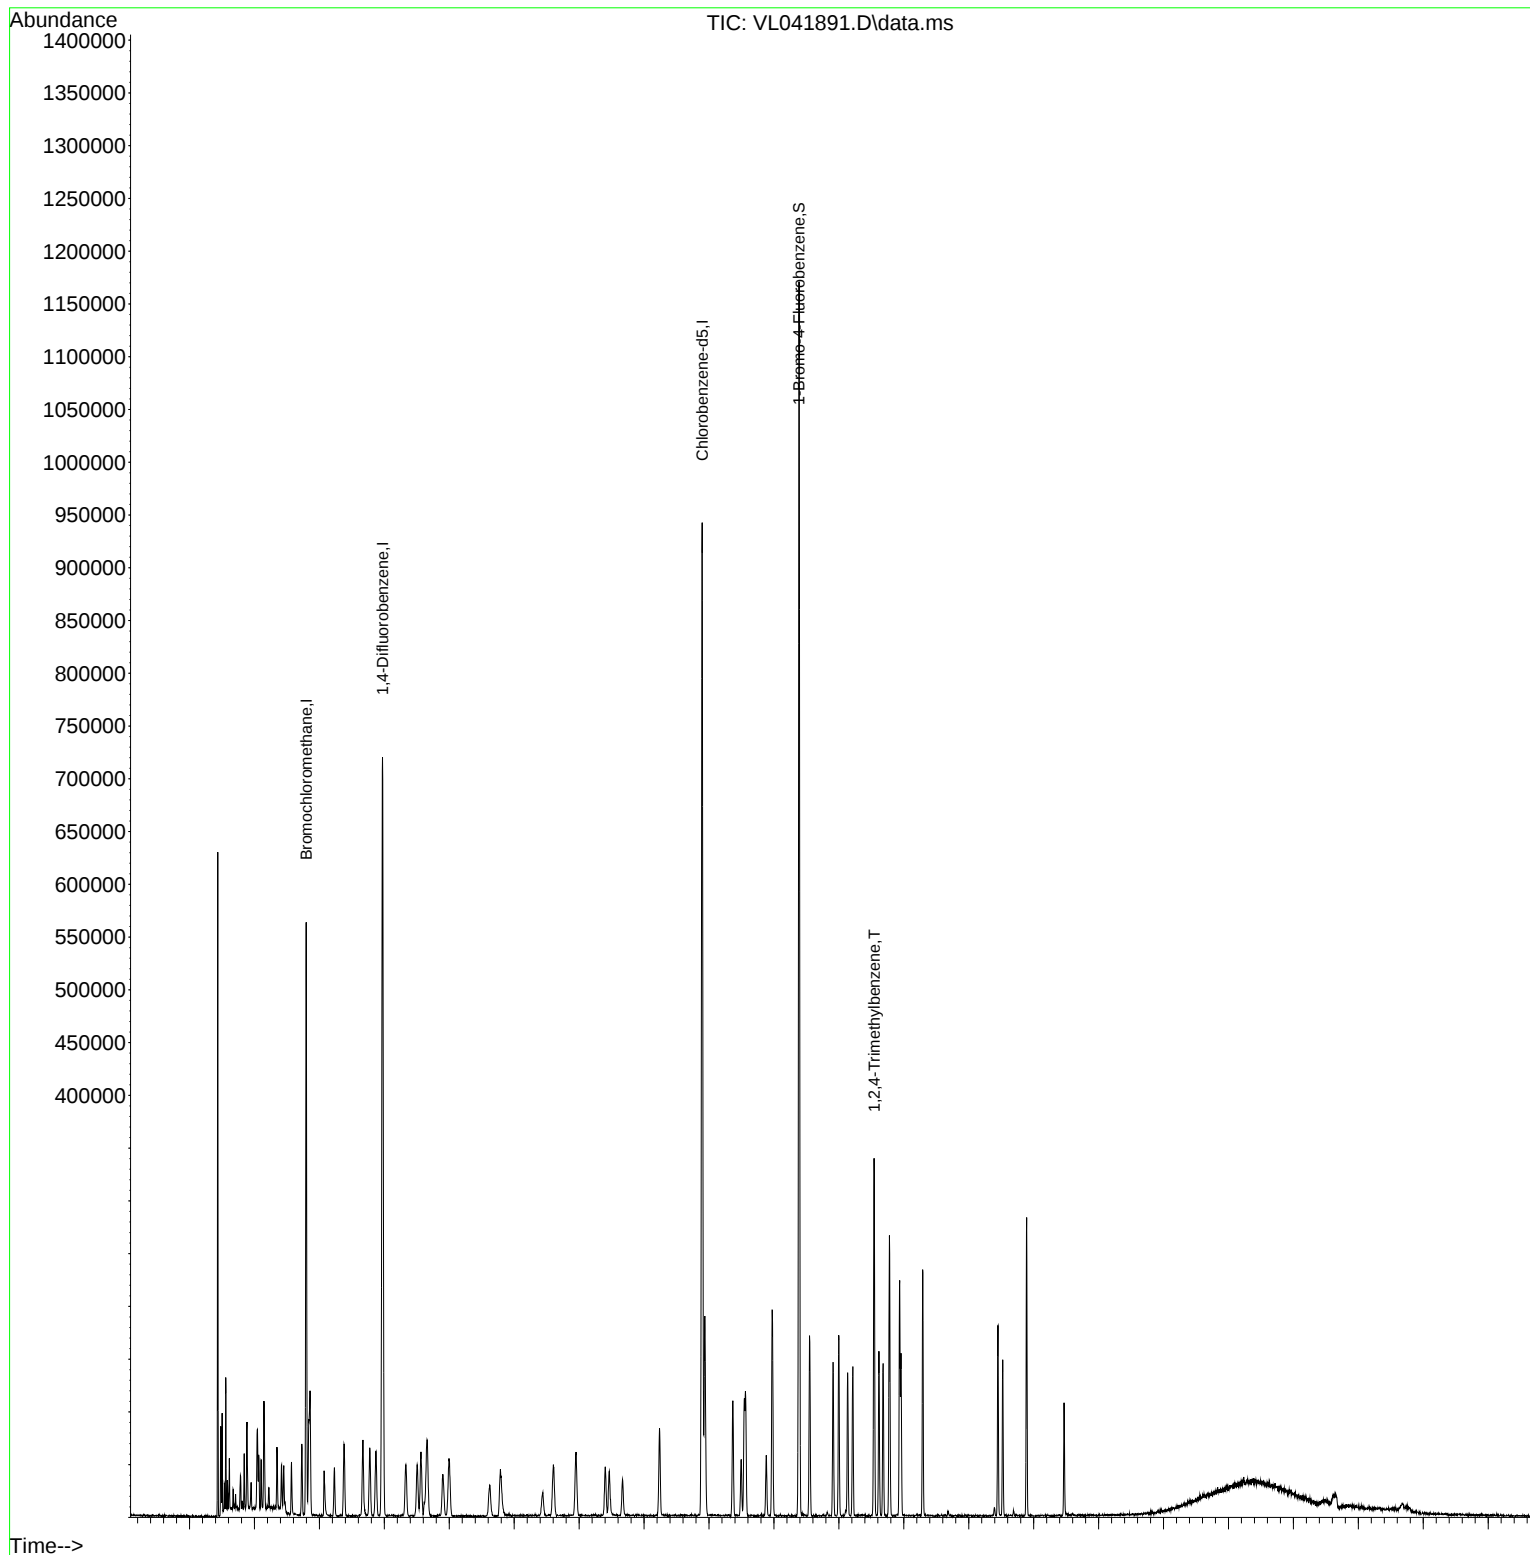

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041892.D
 Acq On : 14 Jan 2025 14:30
 Operator : SY/MD
 Sample : VSTDICC0.5
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.5

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 01/15/2025
 Supervised By : Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 21:21:01 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jan 14 16:31:18 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.790	49	146186	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.968	114	430874	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.891	117	379402	10.000	ppbv	0.00

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene	10.383	95	297462	9.954	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.500%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.499	85	10599	0.532	ppbv	99
3) Chlorodifluoromethane	1.476	51	10582	0.507	ppbv	98
4) Chloromethane	1.534	50	3990	0.533	ppbv	98
5) Vinyl Chloride	1.580	62	4097	0.540	ppbv	94
6) Bromomethane	1.670	94	1852	0.512	ppbv #	78
7) Chloroethane	1.706	64	1532	0.519	ppbv #	77
8) Dichlorotetrafluoroethane	1.557	85	9372	0.539	ppbv	95
9) Propene	1.486	41	4690	0.546	ppbv	85
10) Heptane	4.988	43	11230	0.489	ppbv	95
11) Trichlorofluoromethane	1.881	101	10873	0.525	ppbv	99
12) 1,1,2-Trichlorotrifluo...	2.143	101	8027	0.494	ppbv	90
13) Ethanol	1.725	45	478m	0.759	ppbv	
14) Bromoethene	1.784	108	3071	0.517	ppbv #	94
15) Acetone	1.839	43	10273	0.585	ppbv	99
16) 1,3-Butadiene	1.612	39	4038	0.512	ppbv	99
17) tert-Butyl alcohol	2.046	59	11158	0.516	ppbv #	94
18) 1,1-Dichloroethene	2.036	96	3803	0.520	ppbv	95
19) Isopropyl Alcohol	1.891	45	6317	0.607	ppbv #	32
20) Methylene Chloride	2.065	84	4286	0.618	ppbv	93
21) Allyl Chloride	2.101	41	6553	0.539	ppbv	96
22) trans-1,2-Dichloroethene	2.347	96	4015	0.486	ppbv	89
23) Vinyl Acetate	2.467	43	6381m	0.835	ppbv	
24) 1,1-Dichloroethane	2.415	63	8512	0.533	ppbv	97
25) Ethyl Acetate	2.845	43	23529	0.497	ppbv	97
26) Hexane	2.829	57	9246m	0.494	ppbv	
27) Carbon Disulfide	2.153	76	8847	0.477	ppbv #	1
28) Methyl tert-Butyl Ether	2.447	73	7621	0.532	ppbv	97
29) Chloroform	2.855	83	15360	0.519	ppbv	92
30) Cyclohexane	3.871	84	7579	0.467	ppbv	92
31) cis-1,2-Dichloroethene	2.726	61	10275	0.521	ppbv #	89
32) 1,1,1-Trichloroethane	3.379	97	14198	0.501	ppbv	98
34) 2-Butanone	2.567	43	13981	0.510	ppbv	94
35) Carbon Tetrachloride	3.774	117	12590	0.464	ppbv	89
36) Benzene	3.667	78	19954	0.505	ppbv	95
37) 1,2-Dichloroethane	3.227	62	11613	0.523	ppbv	97
38) Trichloroethene	4.561	130	8199	0.523	ppbv #	89
39) 1,2-Dichloropropane	4.324	63	7526m	0.543	ppbv	
40) 1,4-Dioxane	4.616	88	4031m	0.576	ppbv	
41) Tetrahydrofuran	3.072	42	7183	0.481	ppbv	94
42) Bromodichloromethane	4.499	83	15081m	0.507	ppbv	
43) Methyl Methacrylate	4.891	69	7332m	0.499	ppbv	
44) 2,2,4-Trimethylpentane	4.645	57	31243	0.489	ppbv	95
45) t-1,3-Dichloropropene	6.428	75	6465m	0.470	ppbv	

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041892.D
 Acq On : 14 Jan 2025 14:30
 Operator : SY/MD
 Sample : VSTDICC0.5
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.5

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 01/15/2025
 Supervised By :Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 21:21:01 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jan 14 16:31:18 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.609	75	7986m	0.443	ppbv	
47) 1,1,2-Trichloroethane	6.597	97	7324	0.498	ppbv #	84
48) Dibromochloromethane	7.393	129	10548m	0.465	ppbv	
49) Bromoform	9.493	173	8162	0.438	ppbv	97
50) 4-Methyl-2-Pentanone	5.794	43	19221m	0.515	ppbv	
51) 2-Hexanone	7.454	43	13390	0.466	ppbv #	97
52) Tetrachloroethene	8.238	164	6821m	0.498	ppbv	
53) Toluene	6.946	91	20118	0.467	ppbv	96
54) 1,2-Dibromoethane	7.665	107	10511	0.520	ppbv	89
56) 1,1,1,2-Tetrachloroethane	8.930	131	9524	0.503	ppbv #	1
57) Chlorobenzene	8.930	112	18701	0.534	ppbv #	90
58) Ethyl Benzene	9.364	91	28584	0.482	ppbv #	88
59) m/p-Xylene	9.558	91	45003m	0.946	ppbv	
60) o-Xylene	9.972	91	22370	0.474	ppbv	97
61) Styrene	9.879	104	9788	0.463	ppbv	99
62) Isopropylbenzene	10.545	105	36561	0.501	ppbv	98
63) 1,1,2,2-Tetrachloroethane	9.969	83	15485	0.521	ppbv	98
64) n-propylbenzene	10.995	120	9128	0.495	ppbv	93
65) tert-Butylbenzene	11.536	119	33122	0.498	ppbv	98
66) Benzyl Chloride	11.620	91	1935	0.470	ppbv	99
67) sec-Butylbenzene	11.775	105	45326	0.495	ppbv	98
69) p-Isopropyltoluene	11.931	119	35136	0.466	ppbv	98
70) n-Butylbenzene	12.287	91	35409	0.473	ppbv	96
71) 2-Chlorotoluene	10.908	91	26436	0.490	ppbv	99
72) 4-Ethyltoluene	11.131	105	27363	0.485	ppbv	97
73) 1,3,5-Trimethylbenzene	11.209	105	23183	0.465	ppbv	93
74) 1,2,4-Trimethylbenzene	11.545	105	25777	0.478	ppbv	89
75) 1,3-Dichlorobenzene	11.610	146	16708	0.522	ppbv	100
76) 1,4-Dichlorobenzene	11.678	146	15738	0.503	ppbv	96
77) 1,2-Dichlorobenzene	11.953	146	16364	0.516	ppbv	93
78) Hexachloro-1,3-Butadiene	13.892	225	14162	0.544	ppbv	96
79) Naphthalene	13.520	128	28052	0.516	ppbv	98
80) Naphthalene,2-methyl-	14.468	142	10859	0.422	ppbv	97
81) 1,2,4-Trichlorobenzene	13.445	180	14136	0.533	ppbv	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
Data File : VL041892.D
Acq On : 14 Jan 2025 14:30
Operator : SY/MD
Sample : VSTDICC0.5
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.5

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 21:21:01 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Tue Jan 14 16:31:18 2025
Response via : Initial Calibration

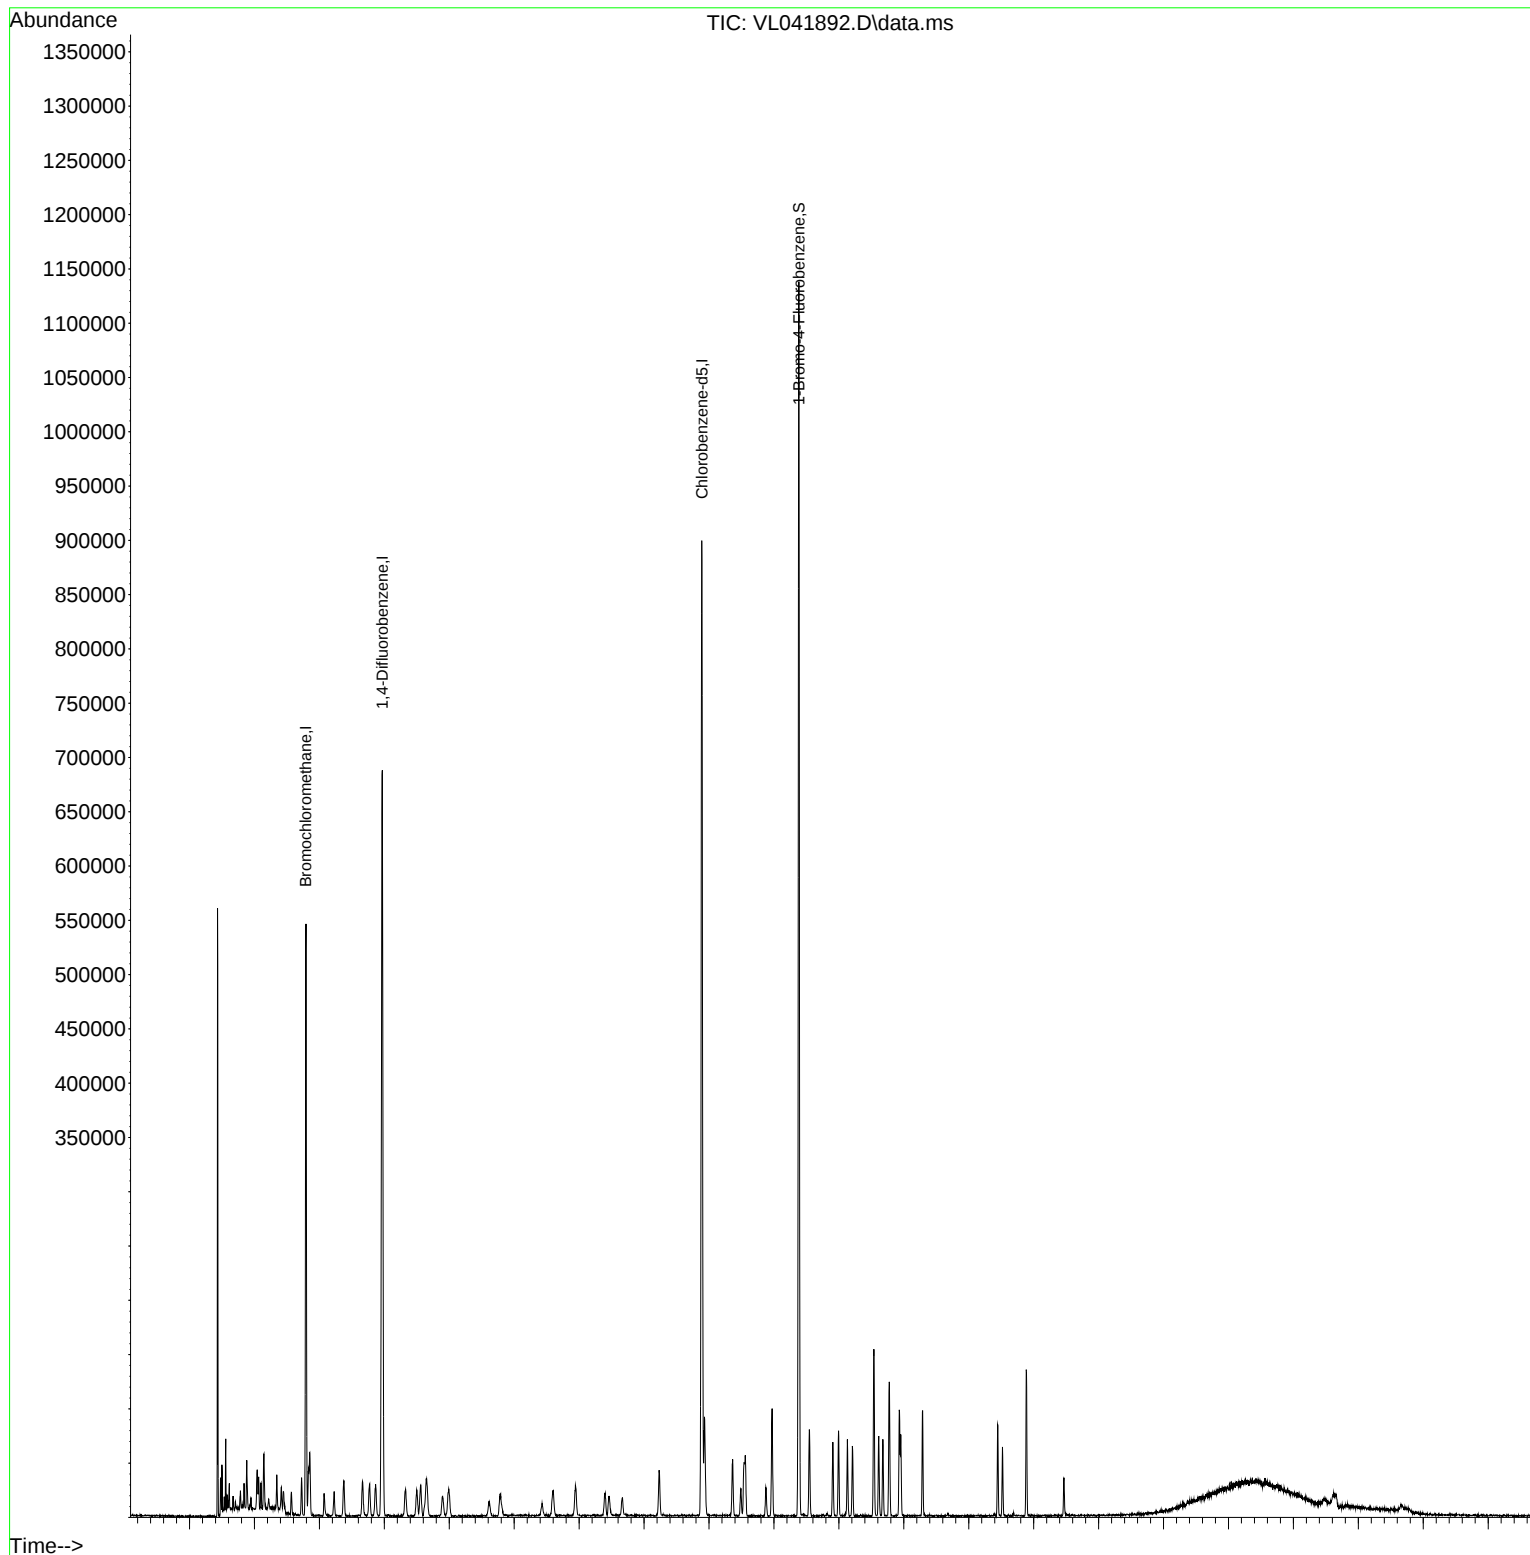

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041893.D
 Acq On : 14 Jan 2025 15:01
 Operator : SY/MD
 Sample : VSTDICC0.1
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 01/15/2025
 Supervised By :Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 22:42:51 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Tue Jan 14 16:31:18 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.793	49	143362	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.968	114	425675	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.891	117	372545	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.387	95	292283	9.961	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.600%
Target Compounds						
5) Vinyl Chloride	1.583	62	828	0.111	ppbv	96
32) 1,1,1-Trichloroethane	3.383	97	2640m	0.095	ppbv	
35) Carbon Tetrachloride	3.768	117	2587m	0.097	ppbv	
38) Trichloroethene	4.557	130	1816m	0.117	ppbv	
52) Tetrachloroethene	8.234	164	1480m	0.109	ppbv	
54) 1,2-Dibromoethane	7.668	107	1872m	0.094	ppbv	
63) 1,1,2,2-Tetrachloroethane	9.976	83	2816	0.097	ppbv	95
79) Naphthalene	13.520	128	3643	0.068	ppbv #	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
Data File : VL041893.D
Acq On : 14 Jan 2025 15:01
Operator : SY/MD
Sample : VSTDICC0.1
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 01/15/2025
Supervised By :Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 22:42:51 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug
QLast Update : Tue Jan 14 16:31:18 2025
Response via : Initial Calibration

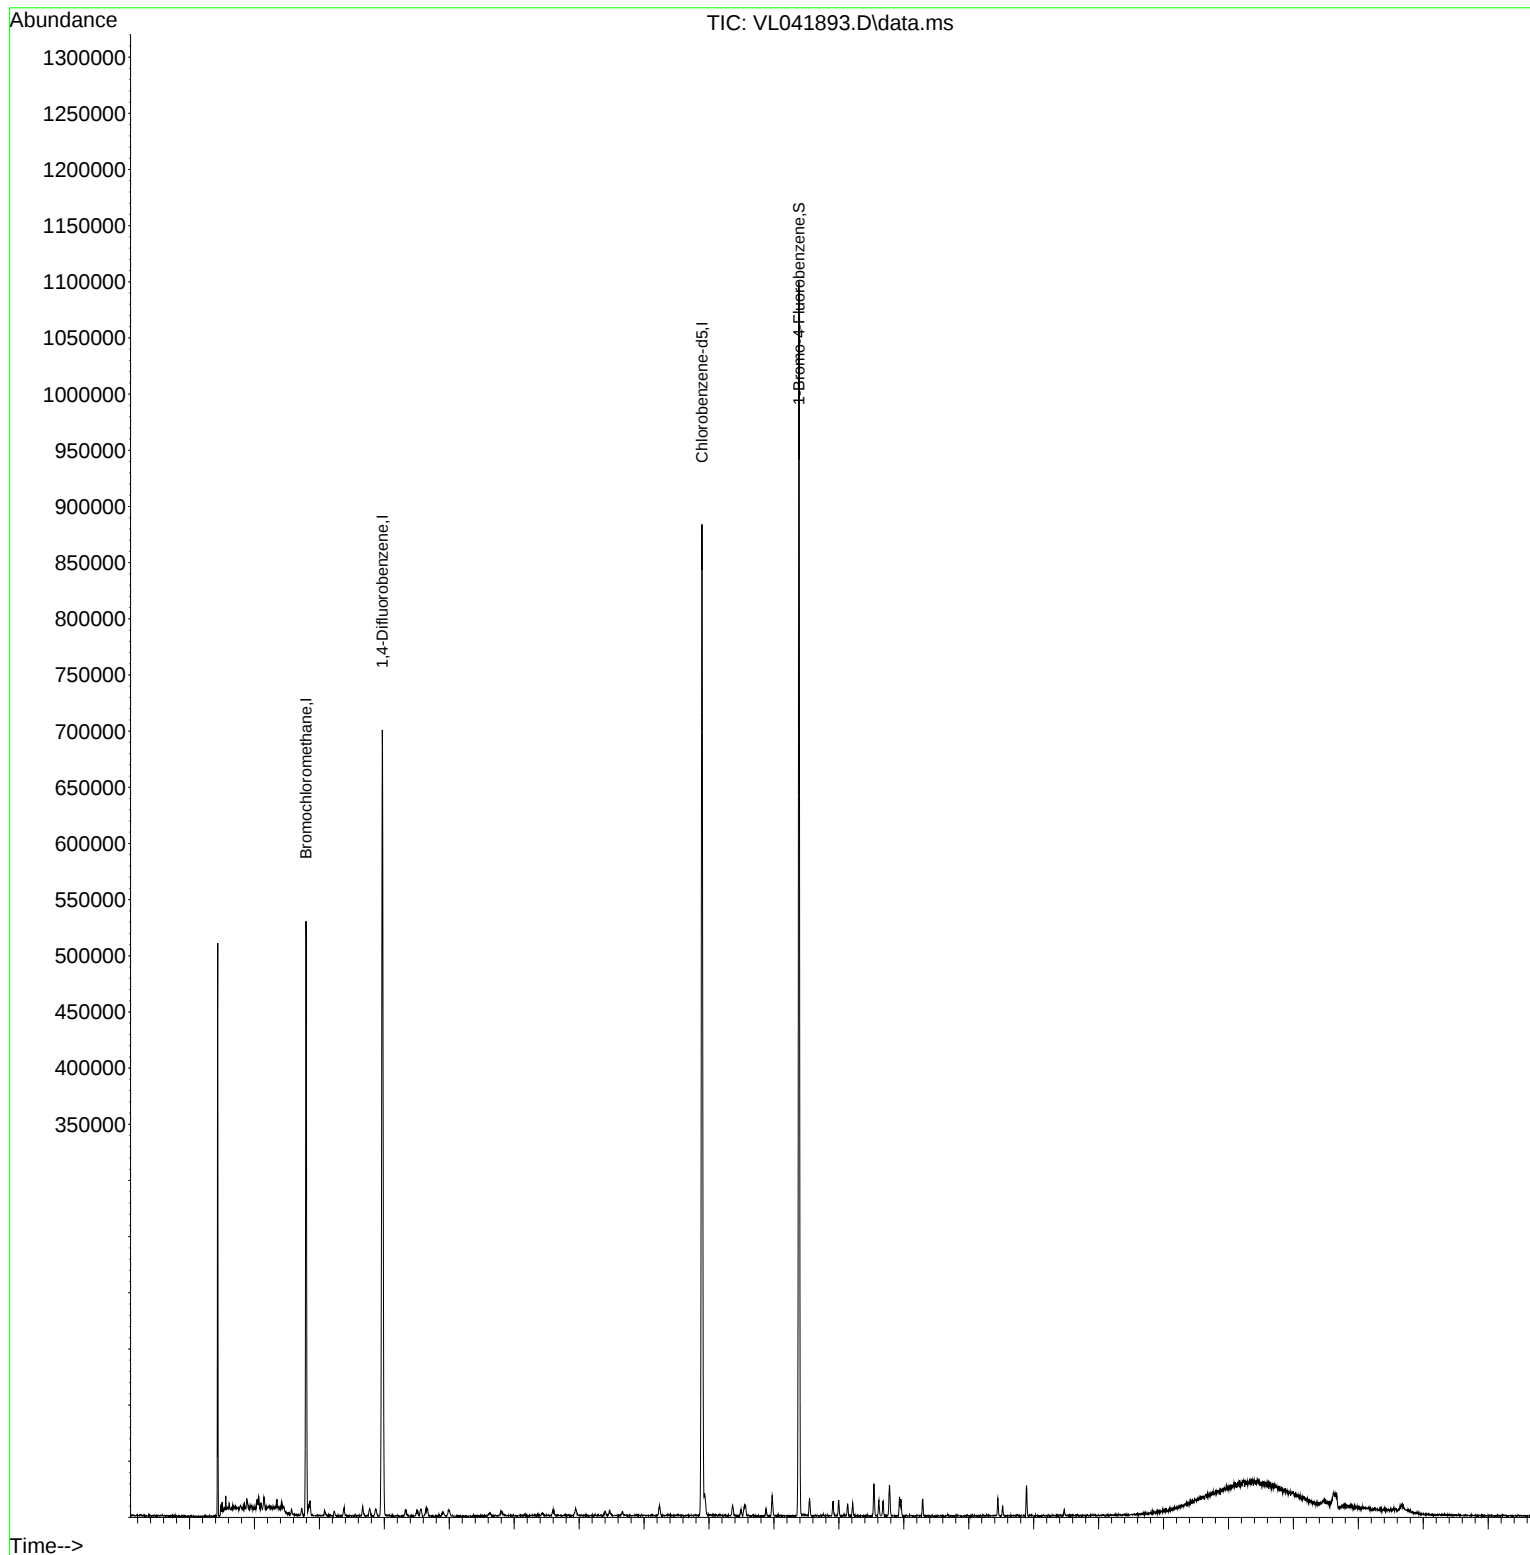

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041894.D
 Acq On : 14 Jan 2025 15:32
 Operator : SY/MD
 Sample : VSTDICC0.03
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC0.03

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 01/15/2025
 Supervised By :Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 21:21:32 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Tue Jan 14 16:31:18 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.793	49	141659	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.972	114	424686	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.891	117	367402	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.387	95	287792	9.945	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.500%
Target Compounds						
					Qvalue	
5) Vinyl Chloride	1.586	62	214m	0.029	ppbv	
32) 1,1,1-Trichloroethane	3.379	97	823	0.030	ppbv	85
35) Carbon Tetrachloride	3.774	117	771	0.029	ppbv #	56
38) Trichloroethene	4.557	130	364m	0.024	ppbv	
52) Tetrachloroethene	8.250	164	408m	0.030	ppbv	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
Data File : VL041894.D
Acq On : 14 Jan 2025 15:32
Operator : SY/MD
Sample : VSTDICC0.03
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VSTDICC0.03

Quant Time: Jan 14 21:21:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug
QLast Update : Tue Jan 14 16:31:18 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 01/15/2025
Supervised By : Mahesh Dadoda 01/15/2025

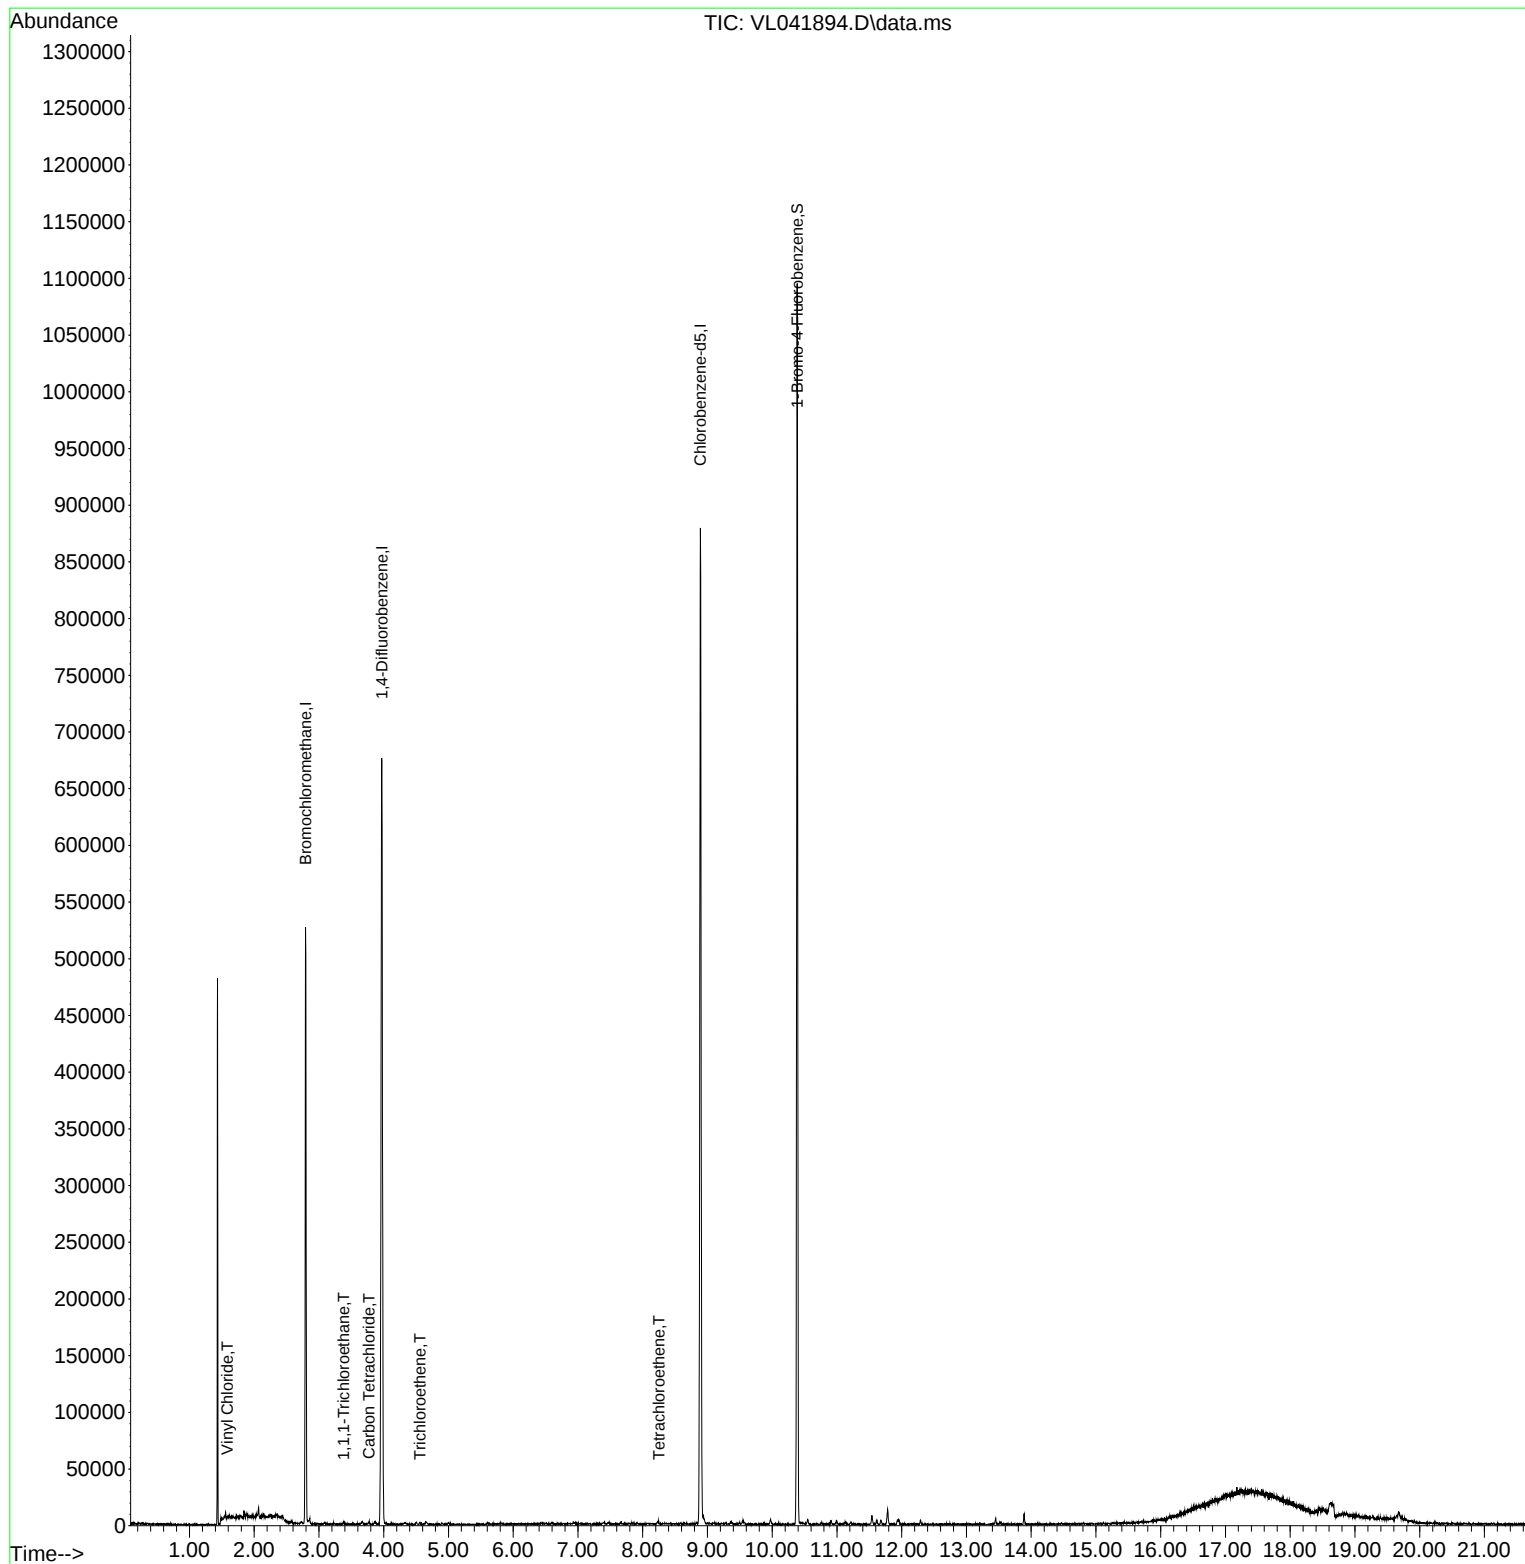

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041895.D
 Acq On : 14 Jan 2025 16:05
 Operator : SY/MD
 Sample : VSTDICC015
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDICC015

Quant Time: Jan 14 21:21:42 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2
 QLast Update : Tue Jan 14 16:31:18 2025
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 01/15/2025
 Supervised By : Mahesh Dadoda 01/15/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.793	49	141652	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.968	114	419859	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.895	117	383799	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.387	95	304042	10.058	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	= 100.600%	
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.502	85	275248	14.266	ppbv	100
3) Chlorodifluoromethane	1.479	51	285437	14.121	ppbv	98
4) Chloromethane	1.534	50	106071	14.617	ppbv	98
5) Vinyl Chloride	1.583	62	104404	14.204	ppbv	98
6) Bromomethane	1.670	94	49415	14.106	ppbv	91
7) Chloroethane	1.709	64	41130	14.383	ppbv	100
8) Dichlorotetrafluoroethane	1.557	85	244666	14.510	ppbv	100
9) Propene	1.486	41	116343	13.972	ppbv	99
10) Heptane	4.998	43	326897	14.688	ppbv	98
11) Trichlorofluoromethane	1.881	101	299656	14.930	ppbv	97
12) 1,1,2-Trichlorotrifluo...	2.143	101	232607	14.787	ppbv	100
13) Ethanol	1.725	45	6109	10.016	ppbv	83
14) Bromoethene	1.784	108	83586	14.513	ppbv	98
15) Acetone	1.839	43	223353	13.128	ppbv	99
16) 1,3-Butadiene	1.612	39	109420	14.329	ppbv	99
17) tert-Butyl alcohol	2.046	59	298424	14.252	ppbv	99
18) 1,1-Dichloroethene	2.039	96	104645	14.759	ppbv	92
19) Isopropyl Alcohol	1.890	45	134050	13.288	ppbv	98
20) Methylene Chloride	2.065	84	88425	13.151	ppbv	98
21) Allyl Chloride	2.101	41	169875	14.419	ppbv	96
22) trans-1,2-Dichloroethene	2.347	96	118169	14.768	ppbv	97
23) Vinyl Acetate	2.470	43	116632	15.747	ppbv	98
24) 1,1-Dichloroethane	2.415	63	230015	14.862	ppbv	99
25) Ethyl Acetate	2.842	43	665170	14.499	ppbv	100
26) Hexane	2.836	57	263948	14.547	ppbv	97
27) Carbon Disulfide	2.156	76	278476	15.509	ppbv	99
28) Methyl tert-Butyl Ether	2.447	73	187986	13.555	ppbv	98
29) Chloroform	2.858	83	413733	14.424	ppbv	98
30) Cyclohexane	3.868	84	233398	14.830	ppbv	99
31) cis-1,2-Dichloroethene	2.729	61	271739	14.223	ppbv	94
32) 1,1,1-Trichloroethane	3.379	97	419117	15.271	ppbv	99
34) 2-Butanone	2.564	43	380813	14.262	ppbv	99
35) Carbon Tetrachloride	3.774	117	426619	16.146	ppbv	97
36) Benzene	3.667	78	553665	14.378	ppbv	100
37) 1,2-Dichloroethane	3.227	62	321362	14.859	ppbv	99
38) Trichloroethene	4.564	130	222328	14.543	ppbv	98
39) 1,2-Dichloropropane	4.328	63	191532	14.179	ppbv	98
40) 1,4-Dioxane	4.596	88	97521	14.305	ppbv #	93
41) Tetrahydrofuran	3.062	42	217707	14.953	ppbv	99
42) Bromodichloromethane	4.502	83	445130	15.351	ppbv	95
43) Methyl Methacrylate	4.894	69	214564	14.999	ppbv	99
44) 2,2,4-Trimethylpentane	4.655	57	909437	14.601	ppbv	100
45) t-1,3-Dichloropropene	6.435	75	218001	16.281	ppbv	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL011425\
 Data File : VL041895.D
 Acq On : 14 Jan 2025 16:05
 Operator : SY/MD
 Sample : VSTDIC015
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDIC015

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 01/15/2025
 Supervised By : Mahesh Dadoda 01/15/2025

Quant Time: Jan 14 21:21:42 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jan 14 16:31:18 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.619	75	281492	16.011	ppbv	98
47) 1,1,2-Trichloroethane	6.597	97	211658	14.782	ppbv	95
48) Dibromochloromethane	7.402	129	356392	16.134	ppbv	100
49) Bromoform	9.493	173	307617	16.953	ppbv	99
50) 4-Methyl-2-Pentanone	5.774	43	533053	14.653	ppbv	99
51) 2-Hexanone	7.451	43	430297	15.363	ppbv #	97
52) Tetrachloroethene	8.237	164	183208	13.721	ppbv	96
53) Toluene	6.949	91	634515	15.126	ppbv	99
54) 1,2-Dibromoethane	7.665	107	295967	15.036	ppbv	93
56) 1,1,1,2-Tetrachloroethane	8.937	131	280809	14.665	ppbv	98
57) Chlorobenzene	8.933	112	479092	13.533	ppbv	99
58) Ethyl Benzene	9.367	91	887072	14.789	ppbv	100
59) m/p-Xylene	9.565	91	1420585m	29.506	ppbv	
60) o-Xylene	9.976	91	704577	14.765	ppbv	100
61) Styrene	9.882	104	342490	15.999	ppbv	99
62) Isopropylbenzene	10.548	105	1063809	14.406	ppbv	100
63) 1,1,2,2-Tetrachloroethane	9.976	83	426347	14.194	ppbv	100
64) n-propylbenzene	10.998	120	266972	14.308	ppbv	100
65) tert-Butylbenzene	11.542	119	947297	14.077	ppbv	98
66) Benzyl Chloride	11.626	91	68623	16.475	ppbv	98
67) sec-Butylbenzene	11.778	105	1292858	13.952	ppbv	100
69) p-Isopropyltoluene	11.937	119	1089109	14.273	ppbv	99
70) n-Butylbenzene	12.290	91	1059002	13.994	ppbv	99
71) 2-Chlorotoluene	10.911	91	797555	14.601	ppbv	100
72) 4-Ethyltoluene	11.134	105	847451	14.846	ppbv	99
73) 1,3,5-Trimethylbenzene	11.215	105	733759	14.556	ppbv	96
74) 1,2,4-Trimethylbenzene	11.549	105	773569	14.170	ppbv	92
75) 1,3-Dichlorobenzene	11.620	146	443828	13.720	ppbv	99
76) 1,4-Dichlorobenzene	11.681	146	447164	14.129	ppbv	99
77) 1,2-Dichlorobenzene	11.956	146	429118	13.385	ppbv	99
78) Hexachloro-1,3-Butadiene	13.892	225	335016	12.731	ppbv	100
79) Naphthalene	13.523	128	724573	13.183	ppbv	99
80) Naphthalene,2-methyl-	14.468	142	278955	10.704	ppbv	99
81) 1,2,4-Trichlorobenzene	13.452	180	342977	12.784	ppbv	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020325\
 Data File : VL041958.D
 Acq On : 03 Feb 2025 10:48
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 02/04/2025
 Supervised By : Mahesh Dadoda 02/04/2025

Quant Time: Feb 04 02:30:31 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jan 14 23:15:42 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.791	49	157470	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.962	114	429487	10.000	ppbv	-0.01
55) Chlorobenzene-d5	8.885	117	371333	10.000	ppbv	0.00
System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.381	95	289698	9.905	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	99.100%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.499	85	218366	10.181	ppbv	100
3) Chlorodifluoromethane	1.477	51	231387	10.298	ppbv	99
4) Chloromethane	1.535	50	86482	10.721	ppbv	97
5) Vinyl Chloride	1.580	62	83248	10.188	ppbv	98
6) Bromomethane	1.667	94	38248	9.822	ppbv	99
7) Chloroethane	1.706	64	34164	10.747	ppbv	99
8) Dichlorotetrafluoroethane	1.554	85	186350	9.941	ppbv	99
9) Propene	1.483	41	95902	10.361	ppbv	98
10) Heptane	4.985	43	266975	10.790	ppbv	97
11) Trichlorofluoromethane	1.878	101	212261	9.513	ppbv	97
12) 1,1,2-Trichlorotrifluo...	2.140	101	162930	9.317	ppbv	99
13) Ethanol	1.722	45	4416	6.513	ppbv	99
14) Bromoethene	1.784	108	60620	9.468	ppbv	100
15) Acetone	1.836	43	176459	9.330	ppbv	99
16) 1,3-Butadiene	1.609	39	86792	10.224	ppbv	99
17) tert-Butyl alcohol	2.043	59	206522	8.872	ppbv	99
18) 1,1-Dichloroethene	2.036	96	74437	9.444	ppbv	93
19) Isopropyl Alcohol	1.888	45	101008	9.007	ppbv	94
20) Methylene Chloride	2.062	84	62977	8.426	ppbv	95
21) Allyl Chloride	2.098	41	126741	9.677	ppbv	98
22) trans-1,2-Dichloroethene	2.344	96	86281	9.700	ppbv	97
23) Vinyl Acetate	2.467	43	84390	9.001	ppbv #	98
24) 1,1-Dichloroethane	2.412	63	171515	9.969	ppbv	100
25) Ethyl Acetate	2.839	43	552271	10.829	ppbv	100
26) Hexane	2.829	57	216097	10.713	ppbv	95
27) Carbon Disulfide	2.153	76	200432	10.041	ppbv	99
28) Methyl tert-Butyl Ether	2.444	73	149839	9.719	ppbv	100
29) Chloroform	2.852	83	333879	10.471	ppbv	100
30) Cyclohexane	3.862	84	183180	10.470	ppbv	98
31) cis-1,2-Dichloroethene	2.723	61	208686	9.825	ppbv	95
32) 1,1,1-Trichloroethane	3.370	97	318650	10.444	ppbv	99
34) 2-Butanone	2.561	43	312946	11.458	ppbv	99
35) Carbon Tetrachloride	3.765	117	320703	11.888	ppbv	99
36) Benzene	3.661	78	444350	11.280	ppbv	97
37) 1,2-Dichloroethane	3.221	62	241263	10.905	ppbv	99
38) Trichloroethene	4.551	130	175365	11.218	ppbv	90
39) 1,2-Dichloropropane	4.322	63	155514	11.255	ppbv	98
40) 1,4-Dioxane	4.590	88	74675	10.701	ppbv #	97
41) Tetrahydrofuran	3.059	42	174208	11.736	ppbv	98
42) Bromodichloromethane	4.496	83	344670	11.620	ppbv	96
43) Methyl Methacrylate	4.888	69	156216	10.675	ppbv	95
44) 2,2,4-Trimethylpentane	4.645	57	751181	11.790	ppbv	99
45) t-1,3-Dichloropropene	6.425	75	148089	10.811	ppbv	98

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020325\
 Data File : VL041958.D
 Acq On : 03 Feb 2025 10:48
 Operator : SY/MD
 Sample : VSTDCCC010
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VSTDCCC010

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 02/04/2025
 Supervised By : Mahesh Dadoda 02/04/2025

Quant Time: Feb 04 02:30:31 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jan 14 23:15:42 2025

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.610	75	202762	11.274	ppbv	99
47) 1,1,2-Trichloroethane	6.590	97	167097	11.410	ppbv	98
48) Dibromochloromethane	7.393	129	269437	11.924	ppbv	99
49) Bromoform	9.487	173	225054	12.125	ppbv	100
50) 4-Methyl-2-Pentanone	5.762	43	428753	11.499	ppbv	98
51) 2-Hexanone	7.445	43	336693	11.752	ppbv #	96
52) Tetrachloroethene	8.231	164	139466	10.211	ppbv	95
53) Toluene	6.940	91	483814	11.275	ppbv	100
54) 1,2-Dibromoethane	7.659	107	229203	11.384	ppbv	97
56) 1,1,1,2-Tetrachloroethane	8.931	131	220185	11.885	ppbv	99
57) Chlorobenzene	8.927	112	386374	11.280	ppbv	98
58) Ethyl Benzene	9.358	91	669174	11.531	ppbv	97
59) m/p-Xylene	9.555	91	1106231m	23.782	ppbv	
60) o-Xylene	9.969	91	555194	12.025	ppbv	98
61) Styrene	9.876	104	246355	11.895	ppbv	99
62) Isopropylbenzene	10.542	105	834260	11.677	ppbv	99
63) 1,1,2,2-Tetrachloroethane	9.966	83	362310	12.280	ppbv	99
64) n-propylbenzene	10.992	120	215585	11.942	ppbv	98
65) tert-Butylbenzene	11.536	119	746398	11.464	ppbv	99
66) Benzyl Chloride	11.620	91	44973	11.160	ppbv	98
67) sec-Butylbenzene	11.772	105	1044912	11.655	ppbv	100
69) p-Isopropyltoluene	11.931	119	867909	11.756	ppbv	99
70) n-Butylbenzene	12.284	91	848499	11.589	ppbv	100
71) 2-Chlorotoluene	10.905	91	615388	11.644	ppbv	98
72) 4-Ethyltoluene	11.128	105	658660	11.926	ppbv	100
73) 1,3,5-Trimethylbenzene	11.209	105	566361	11.613	ppbv	96
74) 1,2,4-Trimethylbenzene	11.542	105	616177	11.666	ppbv	90
75) 1,3-Dichlorobenzene	11.614	146	357966	11.437	ppbv	99
76) 1,4-Dichlorobenzene	11.675	146	352145	11.500	ppbv	100
77) 1,2-Dichlorobenzene	11.950	146	355386	11.457	ppbv	100
78) Hexachloro-1,3-Butadiene	13.886	225	247691	9.729	ppbv	99
79) Naphthalene	13.517	128	553420	10.407	ppbv	99
80) Naphthalene,2-methyl-	14.465	142	173813	6.894	ppbv	97
81) 1,2,4-Trichlorobenzene	13.446	180	251038	9.671	ppbv	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020325\
 Data File : VL041960.D
 Acq On : 03 Feb 2025 12:05
 Operator : SY/MD
 Sample : VL0203ABL02
 Misc : 400mL/MSVOA_L
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0203ABL02

Quant Time: Feb 04 02:33:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
 Quant Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Jan 14 23:15:42 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.790	49	151198	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.965	114	407814	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.888	117	347345	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.380	95	262058	9.579	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	95.800%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020325\
Data File : VL041960.D
Acq On : 03 Feb 2025 12:05
Operator : SY/MD
Sample : VL0203ABL02
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
VL0203ABL02

Quant Time: Feb 04 02:33:07 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Jan 14 23:15:42 2025
Response via : Initial Calibration

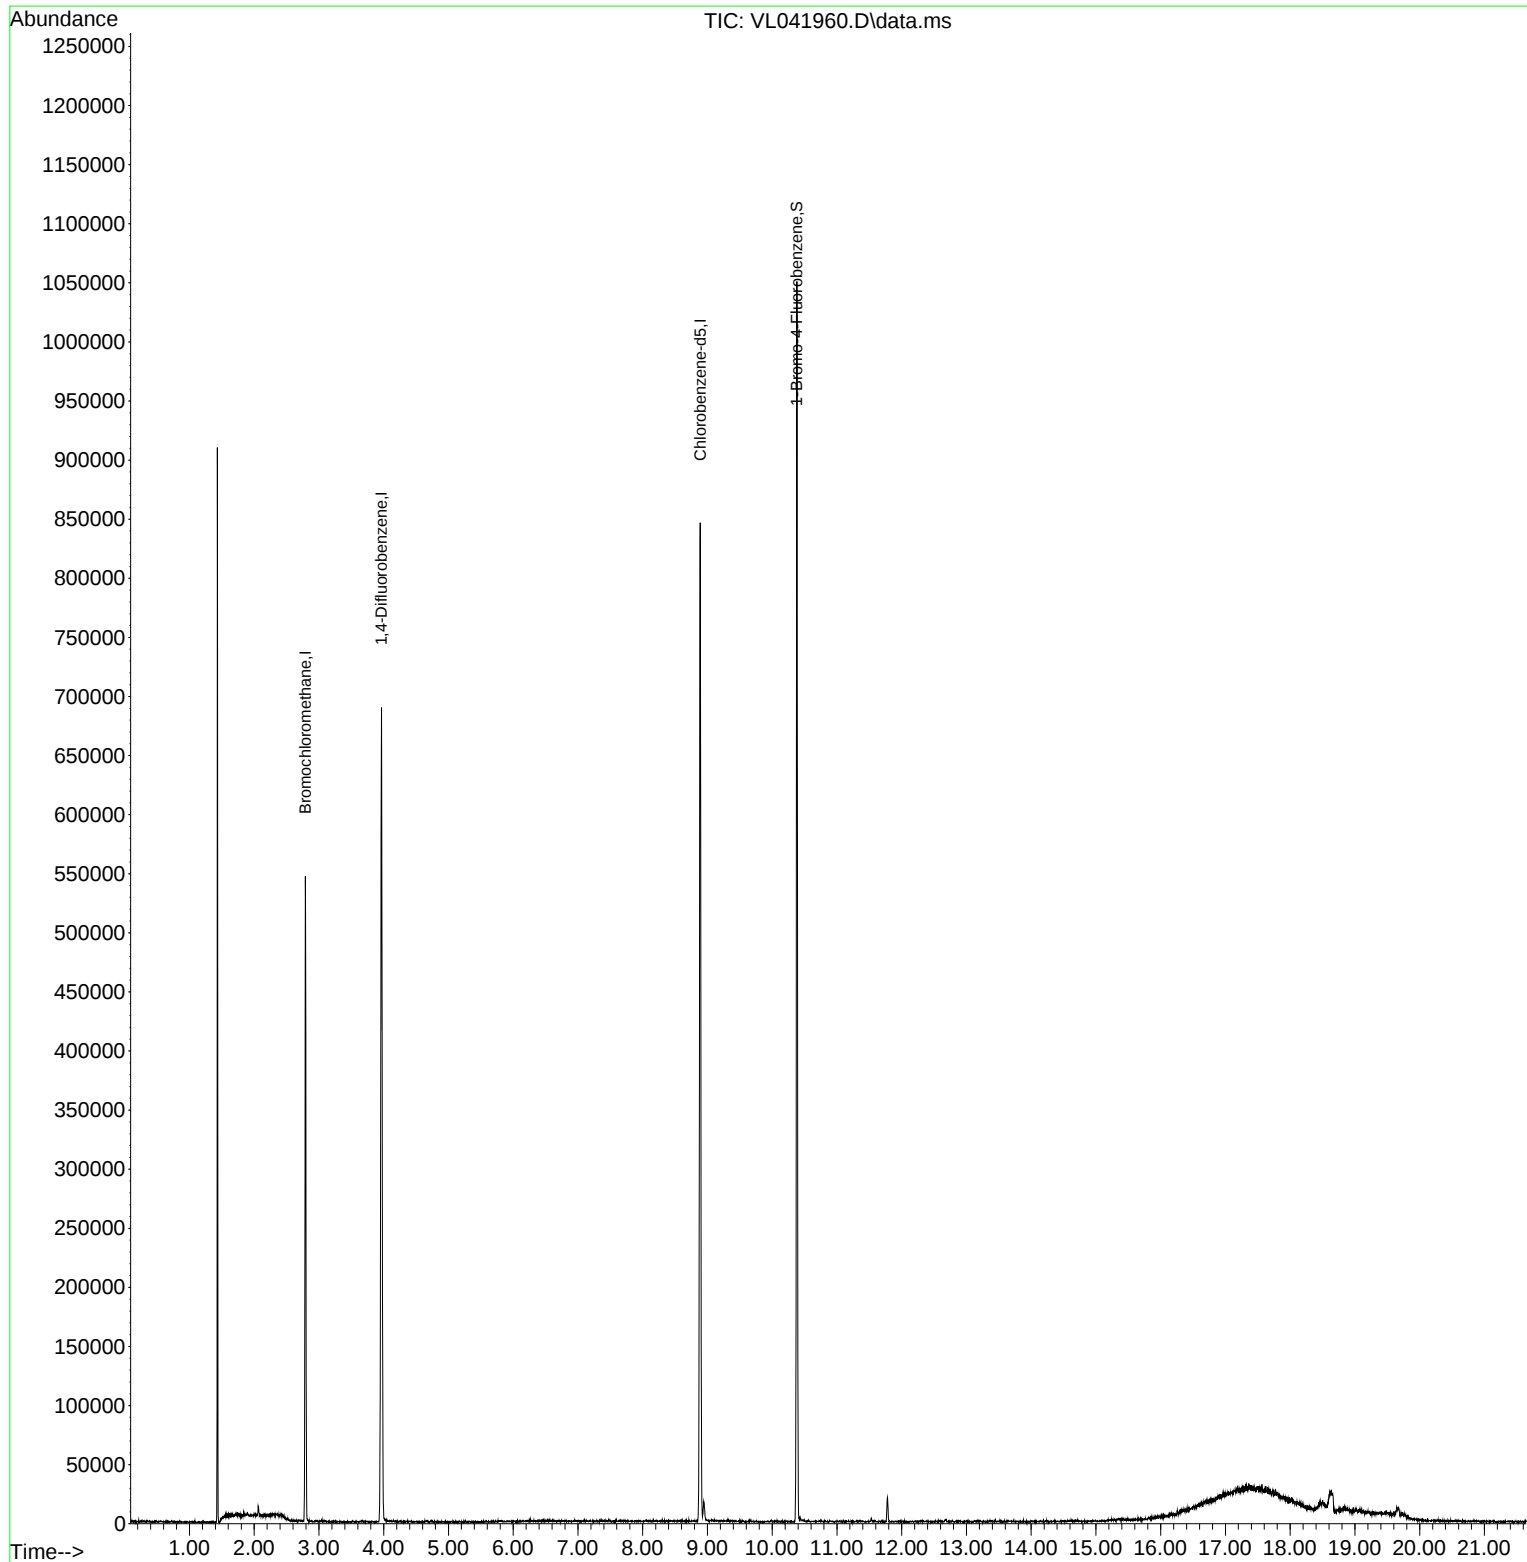

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020325\
 Data File : VL041961.D
 Acq On : 03 Feb 2025 12:57
 Operator : SY/MD
 Sample : VL0203ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0203ABS01

Quant Time: Feb 04 02:34:05 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 2

QLast Update : Tue Jan 14 23:15:42 2025

Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 02/04/2025
 Supervised By : Mahesh Dadoda 02/04/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.790	49	152847	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.965	114	418895	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.882	117	367437	10.000	ppbv	-0.01

System Monitoring Compounds

68) 1-Bromo-4-Fluorobenzene 10.380 95 287209 9.924 ppbv 0.00
 Spiked Amount 10.000 Range 65 - 135 Recovery = 99.200%

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.499	85	203280	9.764	ppbv	99
3) Chlorodifluoromethane	1.476	51	225433	10.336	ppbv	99
4) Chloromethane	1.535	50	81880	10.457	ppbv	94
5) Vinyl Chloride	1.583	62	77713	9.799	ppbv	98
6) Bromomethane	1.670	94	36640	9.694	ppbv	88
7) Chloroethane	1.706	64	31280	10.137	ppbv	94
8) Dichlorotetrafluoroethane	1.557	85	179670	9.875	ppbv	98
9) Propene	1.486	41	91411	10.174	ppbv	99
10) Heptane	4.985	43	161638	6.731	ppbv	99
11) Trichlorofluoromethane	1.881	101	201683	9.312	ppbv	96
12) 1,1,2-Trichlorotrifluo...	2.143	101	164938	9.717	ppbv	98
13) Ethanol	1.722	45	4592	6.978	ppbv	91
14) Bromoethene	1.784	108	57833	9.306	ppbv	99
15) Acetone	1.839	43	165826	9.033	ppbv	98
16) 1,3-Butadiene	1.609	39	83163	10.093	ppbv	98
17) tert-Butyl alcohol	2.043	59	198776	8.797	ppbv	98
18) 1,1-Dichloroethene	2.036	96	70323	9.192	ppbv	97
19) Isopropyl Alcohol	1.891	45	99004	9.096	ppbv	95
20) Methylene Chloride	2.065	84	62278	8.584	ppbv	99
21) Allyl Chloride	2.098	41	122853	9.664	ppbv	98
22) trans-1,2-Dichloroethene	2.344	96	85089	9.855	ppbv	98
23) Vinyl Acetate	2.467	43	86919	9.552	ppbv #	96
24) 1,1-Dichloroethane	2.412	63	166034	9.942	ppbv	99
25) Ethyl Acetate	2.842	43	536156	10.831	ppbv	100
26) Hexane	2.832	57	210051	10.728	ppbv	95
27) Carbon Disulfide	2.153	76	198444	10.242	ppbv	99
28) Methyl tert-Butyl Ether	2.444	73	110198	7.364	ppbv	99
29) Chloroform	2.855	83	325966	10.532	ppbv	96
30) Cyclohexane	3.865	84	173840	10.236	ppbv	98
31) cis-1,2-Dichloroethene	2.726	61	204611	9.925	ppbv	95
32) 1,1,1-Trichloroethane	3.376	97	305623	10.320	ppbv	99
34) 2-Butanone	2.564	43	302190	11.344	ppbv	99
35) Carbon Tetrachloride	3.768	117	309917	11.778	ppbv	97
36) Benzene	3.664	78	426241	11.094	ppbv	99
37) 1,2-Dichloroethane	3.224	62	235620	10.920	ppbv	99
38) Trichloroethene	4.554	130	167629	10.995	ppbv	97
39) 1,2-Dichloropropane	4.318	63	151232	11.221	ppbv	97
40) 1,4-Dioxane	4.590	88	74021	10.876	ppbv #	100
41) Tetrahydrofuran	3.062	42	169798	11.728	ppbv	98
42) Bromodichloromethane	4.496	83	335595	11.600	ppbv	98
43) Methyl Methacrylate	4.884	69	102724	7.197	ppbv	96
44) 2,2,4-Trimethylpentane	4.648	57	725196	11.670	ppbv	99
45) t-1,3-Dichloropropene	6.422	75	145441	10.886	ppbv	94

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020325\
 Data File : VL041961.D
 Acq On : 03 Feb 2025 12:57
 Operator : SY/MD
 Sample : VL0203ABS01
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 VL0203ABS01

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 02/04/2025
 Supervised By :Mahesh Dadoda 02/04/2025

Quant Time: Feb 04 02:34:05 2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M

Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug 2

QLast Update : Tue Jan 14 23:15:42 2025


Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
46) cis-1,3-Dichloropropene	5.609	75	122518	6.985	ppbv	98
47) 1,1,2-Trichloroethane	6.590	97	167038	11.694	ppbv	95
48) Dibromochloromethane	7.390	129	260120	11.803	ppbv	100
49) Bromoform	9.487	173	217089	11.991	ppbv	99
50) 4-Methyl-2-Pentanone	5.765	43	267280	7.350	ppbv	98
51) 2-Hexanone	7.445	43	328817	11.767	ppbv #	96
52) Tetrachloroethene	8.225	164	136143	10.220	ppbv	97
53) Toluene	6.936	91	469033	11.207	ppbv	99
54) 1,2-Dibromoethane	7.655	107	222983	11.356	ppbv	100
56) 1,1,1,2-Tetrachloroethane	8.927	131	214758	11.715	ppbv	99
57) Chlorobenzene	8.924	112	382465	11.284	ppbv	99
58) Ethyl Benzene	9.357	91	646825	11.264	ppbv	98
59) m/p-Xylene	9.555	91	1068374m	23.212	ppbv	
60) o-Xylene	9.966	91	537558	11.766	ppbv	98
61) Styrene	9.872	104	239767	11.699	ppbv	98
62) Isopropylbenzene	10.542	105	802003	11.345	ppbv	99
63) 1,1,2,2-Tetrachloroethane	9.966	83	357905	12.260	ppbv	100
64) n-propylbenzene	10.992	120	208748	11.686	ppbv	99
65) tert-Butylbenzene	11.536	119	731901	11.360	ppbv	99
66) Benzyl Chloride	11.620	91	41013	10.285	ppbv	97
67) sec-Butylbenzene	11.772	105	1015579	11.448	ppbv	99
69) p-Isopropyltoluene	11.931	119	836492	11.451	ppbv	98
70) n-Butylbenzene	12.290	91	824000	11.374	ppbv	100
71) 2-Chlorotoluene	10.905	91	592446	11.329	ppbv	99
72) 4-Ethyltoluene	11.131	105	634050	11.602	ppbv	99
73) 1,3,5-Trimethylbenzene	11.209	105	551677	11.432	ppbv	97
74) 1,2,4-Trimethylbenzene	11.542	105	602744	11.533	ppbv	96
75) 1,3-Dichlorobenzene	11.613	146	348392	11.249	ppbv	99
76) 1,4-Dichlorobenzene	11.678	146	344428	11.367	ppbv	99
77) 1,2-Dichlorobenzene	11.953	146	350456	11.418	ppbv	98
78) Hexachloro-1,3-Butadiene	13.892	225	239328	9.500	ppbv	99
79) Naphthalene	13.523	128	539332	10.249	ppbv	98
80) Naphthalene,2-methyl-	14.468	142	172189	6.902	ppbv	97
81) 1,2,4-Trichlorobenzene	13.452	180	244059	9.502	ppbv	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual Integrations

Quant Time: Feb 04 02:34:05 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_LFri Aug
QLast Update : Tue Jan 14 23:15:42 2025
Response via : Initial Calibration



Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020325\
 Data File : VL041974.D
 Acq On : 04 Feb 2025 08:03
 Operator : SY/MD
 Sample : QC020325 CAN 10599
 Misc : 400mL/MSVOA_L
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_L
 ClientSampleId :
 QC020325 CAN 10599

Quant Time: Feb 04 08:27:00 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
 Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
 QLast Update : Tue Jan 14 23:15:42 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	2.797	49	148524	10.000	ppbv	0.00
33) 1,4-Difluorobenzene	3.975	114	371804	10.000	ppbv	0.00
55) Chlorobenzene-d5	8.898	117	315945	10.000	ppbv	0.00

System Monitoring Compounds						
68) 1-Bromo-4-Fluorobenzene	10.390	95	232316	9.336	ppbv	0.00
Spiked Amount	10.000	Range	65 - 135	Recovery	=	93.400%

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL020325\
Data File : VL041974.D
Acq On : 04 Feb 2025 08:03
Operator : SY/MD
Sample : QC020325 CAN 10599
Misc : 400mL/MSVOA_L
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
QC020325 CAN 10599

Quant Time: Feb 04 08:27:00 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL011425AIR.M
Quant Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
QLast Update : Tue Jan 14 23:15:42 2025
Response via : Initial Calibration

