
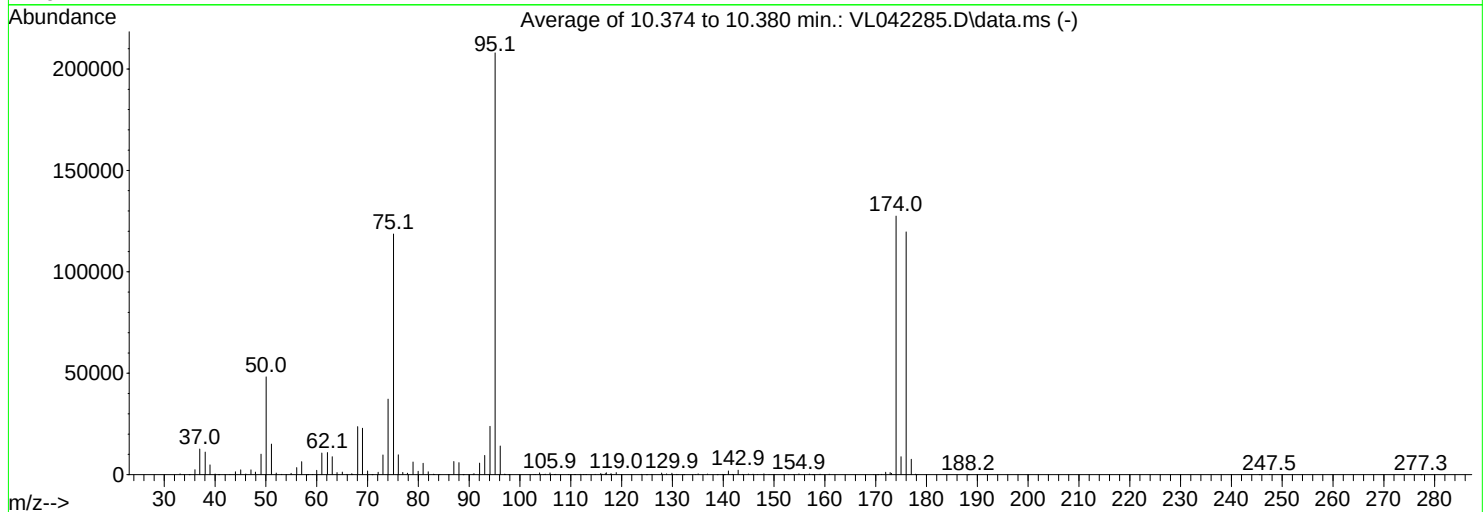


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL040925\
Data File : VL042285.D
Acq On : 09 Apr 2025 09:38
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025

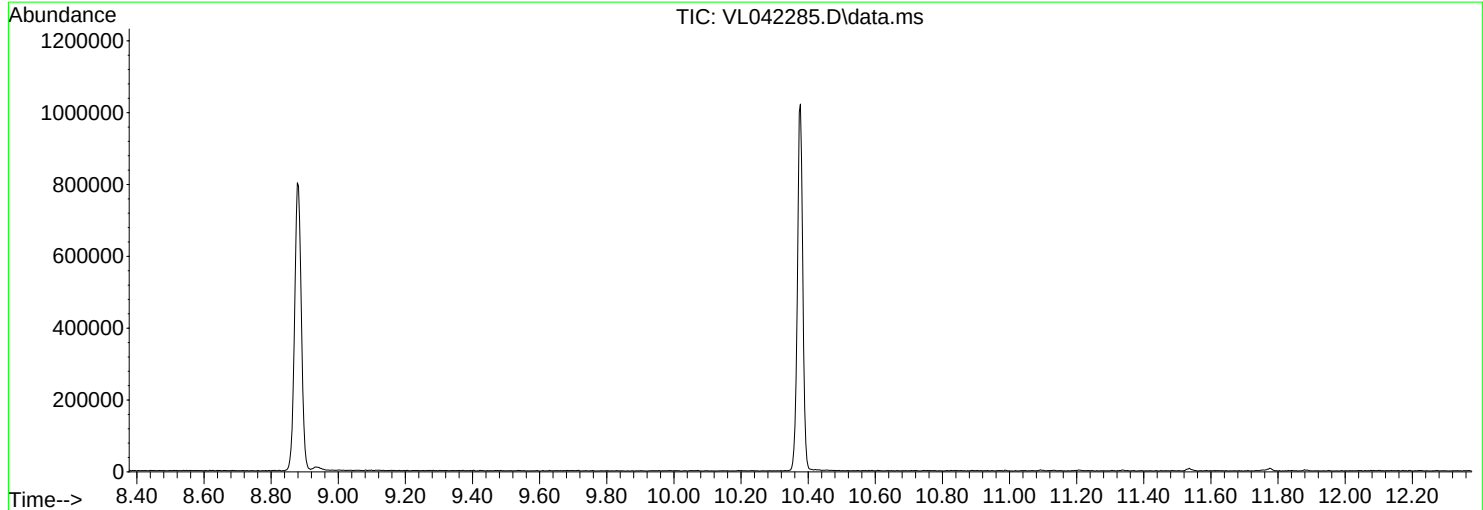

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.2	48216	PASS
75	95	30	66	57.1	118680	PASS
95	95	100	100	100.0	207979	PASS
96	95	5	9	6.8	14091	PASS
173	174	0.00	2	0.8	1054	PASS
174	95	50	120	61.3	127477	PASS
175	174	4	9	6.9	8833	PASS
176	174	93	101	93.9	119656	PASS
177	176	5	9	6.4	7607	PASS

Average of 10.374 to 10.380 min.: VL042285.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	417	44.00	1441	54.95	620	65.05	1261
33.90	94	45.05	2380	56.05	3516	65.95	191
34.90	32	46.05	349	57.05	6411	66.85	42
36.05	2446	47.05	2354	58.00	104	67.10	21
37.00	12645	47.95	1257	58.20	27	68.05	23661
38.05	11110	49.05	10139	59.20	77	69.00	22856
39.00	4835	50.05	48216	60.00	2135	70.00	1792
40.00	285	51.10	15074	61.00	10694	70.90	28
40.70	43	52.05	766	62.10	10932	72.10	1207
41.95	120	53.10	151	63.05	8834	73.05	9735
42.90	87	54.05	105	64.00	1068	74.05	37269

Average of 10.374 to 10.380 min.: VL042285.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	118680	85.90	71	96.10	14091	107.05	179
76.05	9755	86.05	118	96.95	206	109.60	68
76.95	1134	87.00	6464	97.20	139	110.00	75
77.85	699	88.00	5942	97.80	28	110.70	114
78.95	6222	88.80	47	102.75	63	110.90	74
79.95	1641	90.80	279	103.10	96	111.85	172
80.95	5627	90.95	507	103.85	857	112.50	49
81.95	1425	92.05	5692	104.70	125	112.80	63
83.00	204	93.05	9492	104.95	249	113.10	76
83.20	94	94.10	23832	105.90	865	114.80	180
84.20	58	95.10	207979	106.80	78	115.85	485

Average of 10.374 to 10.380 min.: VL042285.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.10	288	127.90	758	140.20	33	150.00	189
116.80	473	128.85	382	141.00	1805	151.90	40
117.00	944	129.90	746	141.80	182	152.90	81
117.80	206	130.85	177	142.00	79	153.85	116
117.95	512	131.10	126	142.95	2193	154.90	405
118.95	998	132.20	19	143.85	183	155.95	119
119.95	112	134.60	74	144.95	304	156.95	348
121.90	73	135.05	382	145.85	215	157.60	42
123.90	168	136.90	304	146.75	89	158.00	85
124.90	17	138.80	18	148.00	408	159.05	270
125.95	151	139.90	129	149.00	121	160.85	202

Average of 10.374 to 10.380 min.: VL042285.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
169.65	95	178.30	58				
170.40	28	188.20	47				
171.15	163	245.50	43				
171.95	1199	247.50	74				
172.85	1054	277.30	17				
173.10	604						
174.00	127477						
175.00	8833						
176.00	119656						
177.00	7607						
177.90	238						