
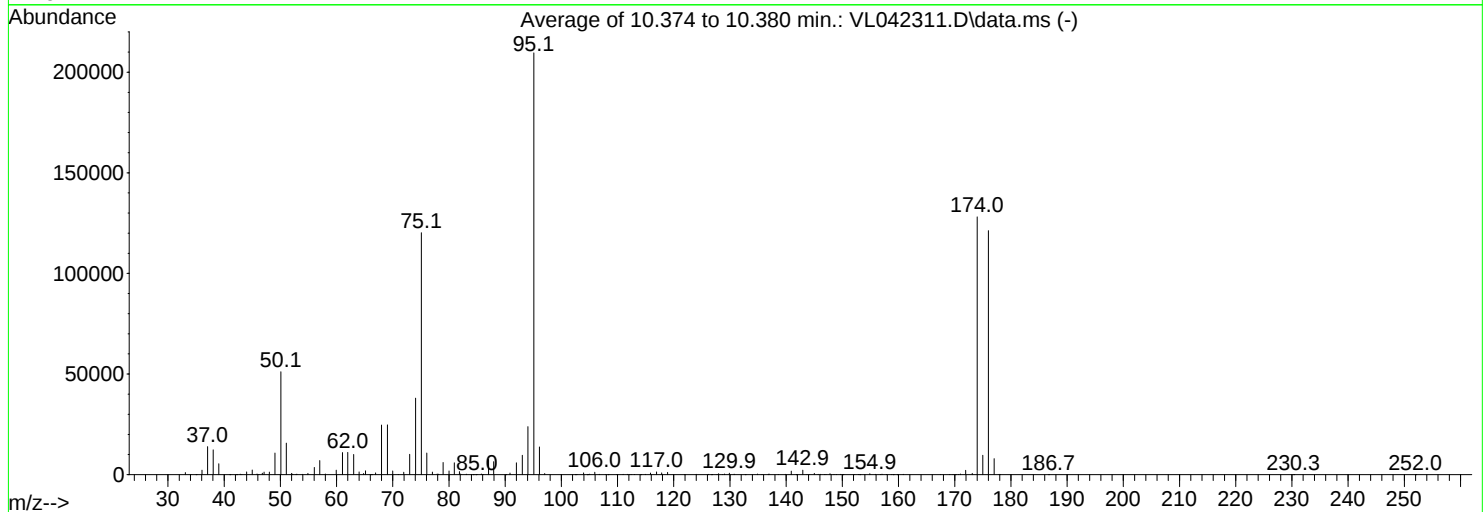


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041125\
Data File : VL042311.D
Acq On : 11 Apr 2025 08:18
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025

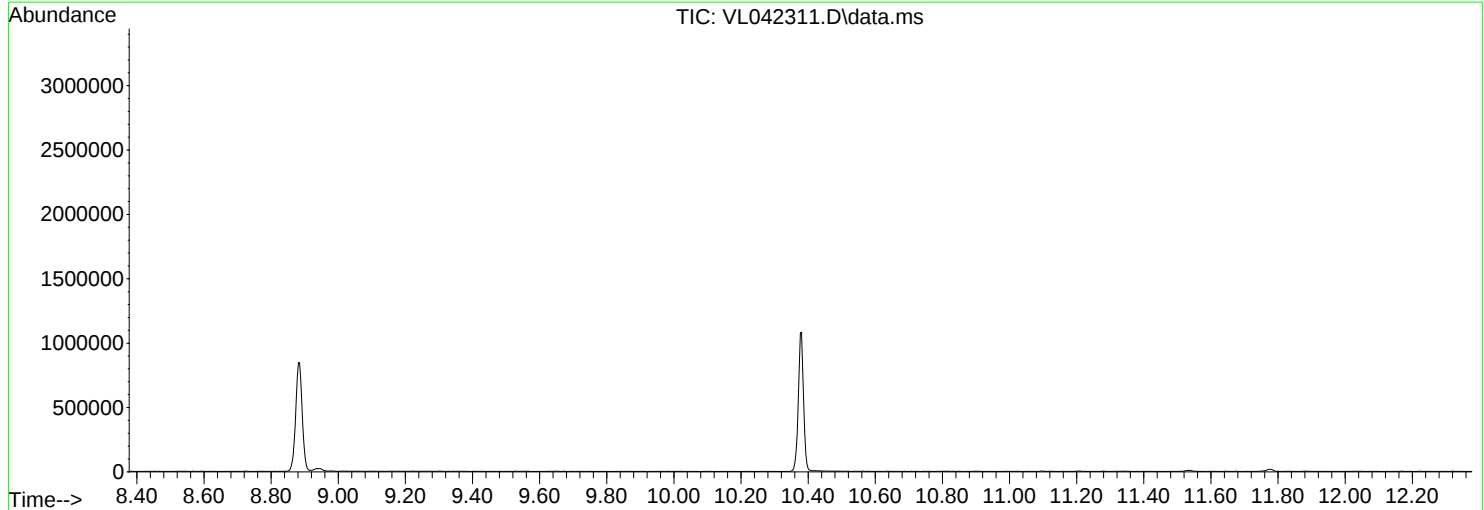

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.4	51160	PASS
75	95	30	66	57.3	120195	PASS
95	95	100	100	100.0	209621	PASS
96	95	5	9	6.6	13755	PASS
173	174	0.00	2	0.5	631	PASS
174	95	50	120	61.1	128109	PASS
175	174	4	9	7.5	9591	PASS
176	174	93	101	94.7	121299	PASS
177	176	5	9	6.6	7977	PASS

Average of 10.374 to 10.380 min.: VL042311.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1074	44.00	1355	52.00	600	62.00	1105
34.05	96	45.00	2304	52.20	280	63.05	1002
35.00	17	45.85	298	52.80	177	64.00	139
36.05	2255	46.00	60	52.95	208	64.80	57
37.05	13891	46.20	116	53.90	189	65.15	1900
38.05	12288	46.80	681	54.90	666	66.00	110
39.05	5453	47.10	1256	56.05	3598	66.20	37
41.00	36	48.05	1306	57.00	7018	66.95	859
42.20	23	49.05	10779	58.00	327	68.00	24645
42.85	273	50.10	51160	59.95	2192	69.05	24747
43.15	59	51.05	15654	61.05	11006	70.00	1869

Average of 10.374 to 10.380 min.: VL042311.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
71.00	70	80.95	5858	87.95	6441	103.95	911
71.95	1172	81.85	1501	90.10	30	104.60	46
73.00	10100	82.10	327	90.85	815	104.80	58
74.05	38011	83.10	250	92.00	5897	105.05	256
75.10	120195	84.00	103	93.05	9587	105.95	1197
76.05	10710	84.30	35	94.05	23856	106.75	167
77.05	1312	84.80	17	95.10	209621	107.90	125
77.90	330	85.00	58	96.10	13755	108.30	43
78.10	257	85.75	322	97.05	573	109.90	58
78.95	6072	86.10	84	102.50	25	111.00	179
80.00	1830	87.05	7571	102.80	54	111.80	181

Average of 10.374 to 10.380 min.: VL042311.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
112.10	69	126.15	133	135.70	80	145.00	641
112.40	78	126.70	31	136.80	149	145.70	170
113.00	96	126.90	52	136.95	291	146.10	164
114.10	19	127.70	80	138.60	58	146.85	116
114.95	134	128.00	516	139.85	134	147.10	95
115.85	782	128.70	54	140.90	1762	147.80	465
116.95	1349	129.05	348	141.80	43	148.50	79
117.85	878	129.90	698	142.00	104	148.95	115
118.90	1137	130.75	256	142.95	2234	149.70	159
121.90	17	132.70	40	143.70	96	150.10	20
124.00	137	134.90	321	144.10	82	152.10	53

Average of 10.374 to 10.380 min.: VL042311.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
152.90	114	160.85	203	176.00	121299		
153.10	22	167.50	57	177.00	7977		
154.00	110	169.10	64	177.90	167		
154.90	451	169.70	56	178.10	103		
155.90	137	170.10	19	186.70	25		
156.80	119	170.65	115	230.30	28		
157.05	257	171.00	345	252.00	28		
157.85	97	171.95	2137				
158.80	104	173.10	631				
159.05	47	174.00	128109				
159.80	23	175.00	9591				