
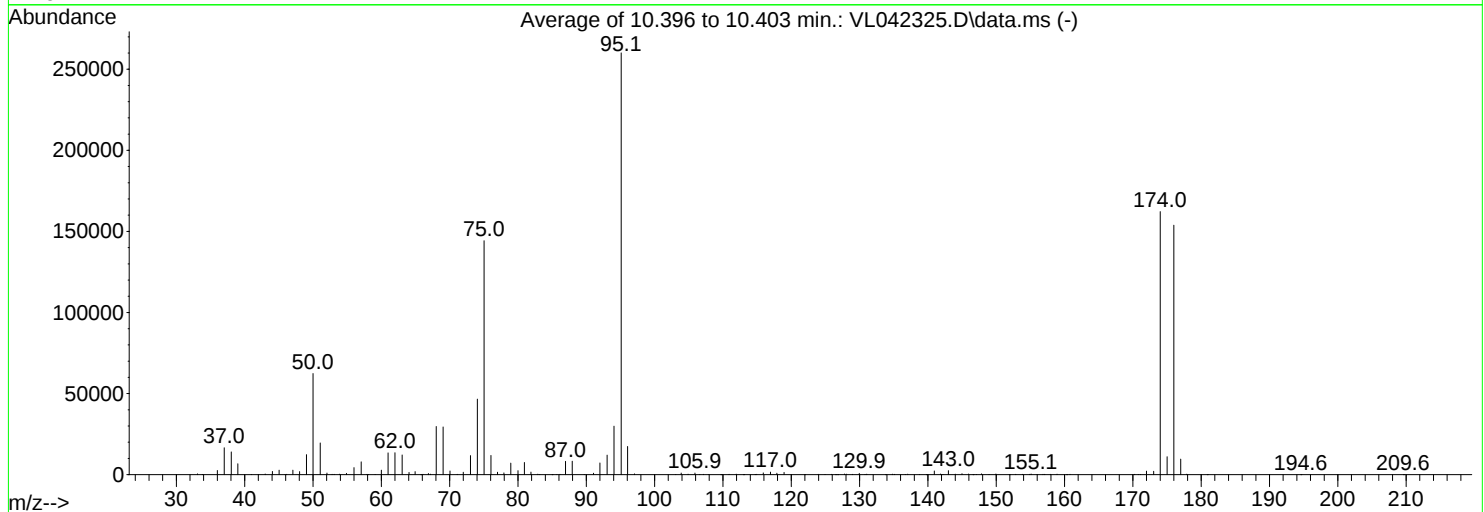


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL041525\
Data File : VL042325.D
Acq On : 15 Apr 2025 07:45
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL032725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Mar 28 02:00:52 2025

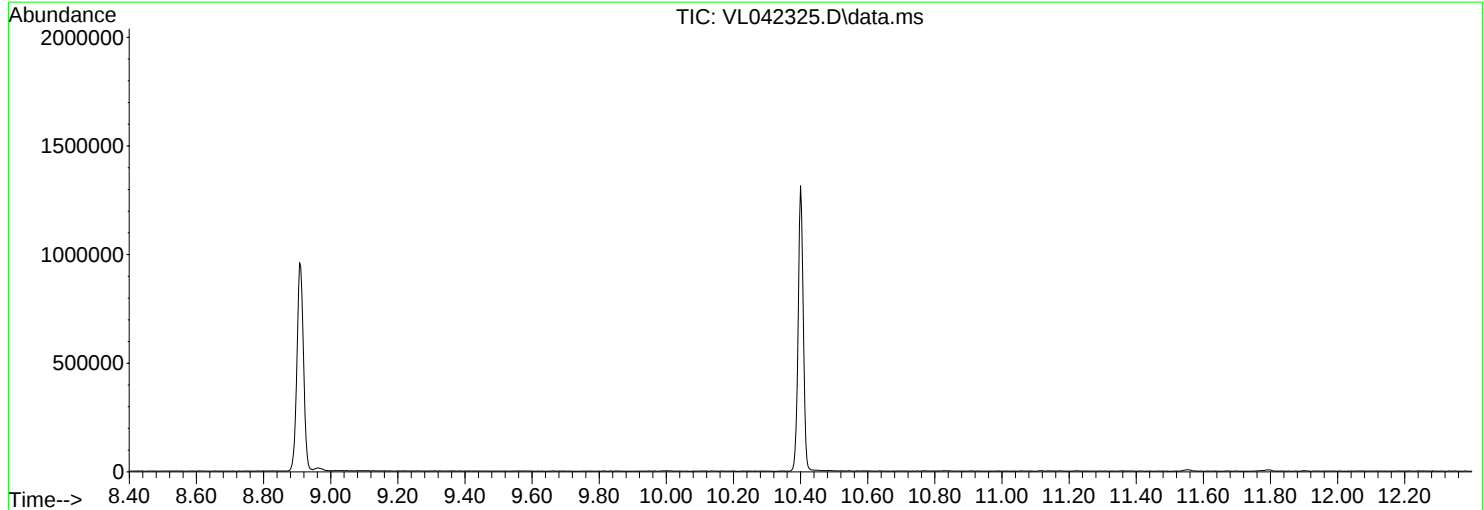

AutoFind: Scans 3185, 3186, 3187; Background Corrected with Scan 3171

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.0	62363	PASS
75	95	30	66	55.5	144299	PASS
95	95	100	100	100.0	260117	PASS
96	95	5	9	6.7	17331	PASS
173	174	0.00	2	1.3	2038	PASS
174	95	50	120	62.4	162261	PASS
175	174	4	9	6.8	11092	PASS
176	174	93	101	94.8	153792	PASS
177	176	5	9	6.2	9603	PASS

Average of 10.396 to 10.403 min.: VL042325.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	527	45.05	2755	53.90	269	64.05	135
33.80	64	45.90	103	54.90	810	64.95	185
33.90	109	46.15	212	56.00	4390	65.80	2
36.00	2597	47.05	2784	57.05	7934	66.10	17
37.00	16567	48.05	1901	57.90	208	66.90	705
38.05	14005	49.05	12367	58.10	142	67.20	281
39.00	6748	50.00	62363	59.10	80	68.05	29680
41.00	129	51.05	19528	60.00	2756	69.05	29389
42.05	149	52.05	1034	61.00	13383	70.05	2291
43.00	410	52.80	160	62.00	13531	71.10	181
44.05	1955	53.10	160	63.05	12163	72.00	1472

Average of 10.396 to 10.403 min.: VL042325.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.05	11788	83.20	99	95.10	260117	109.95	85
74.05	46619	85.00	21	96.05	17331	110.90	165
75.05	144299	85.70	93	97.05	488	111.95	308
76.05	11834	86.15	253	103.10	144	113.00	56
77.00	1527	86.95	8157	103.90	952	113.15	76
77.95	1078	87.95	8281	104.90	256	114.70	76
78.95	7127	89.70	79	105.90	1018	114.80	86
80.00	2469	91.05	904	106.60	86	114.95	162
80.95	7534	92.00	7175	107.15	202	115.90	1065
81.90	1563	93.05	12057	107.95	121	116.95	1597
82.90	327	94.05	29936	109.70	54	117.90	910

Average of 10.396 to 10.403 min.: VL042325.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.95	1420	130.80	65	142.20	102	152.85	224
121.95	46	131.05	349	143.00	2519	153.85	232
123.95	170	133.80	30	144.00	295	154.90	180
124.95	99	134.80	291	145.00	595	155.10	426
125.90	212	135.10	198	145.95	414	156.00	154
126.50	20	136.70	159	146.60	18	156.85	198
126.80	63	137.05	298	147.10	125	157.10	194
127.80	419	138.75	100	147.85	450	157.95	188
128.10	269	139.80	51	148.95	106	158.90	274
128.95	251	140.95	2305	149.95	353	160.30	44
129.95	810	141.85	362	151.90	26	160.80	239

Average of 10.396 to 10.403 min.: VL042325.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
170.25	244	194.60	42				
170.80	64	209.60	24				
171.10	110						
172.00	2175						
173.05	2038						
174.00	162261						
175.00	11092						
176.00	153792						
177.00	9603						
177.90	283						
180.90	23						