
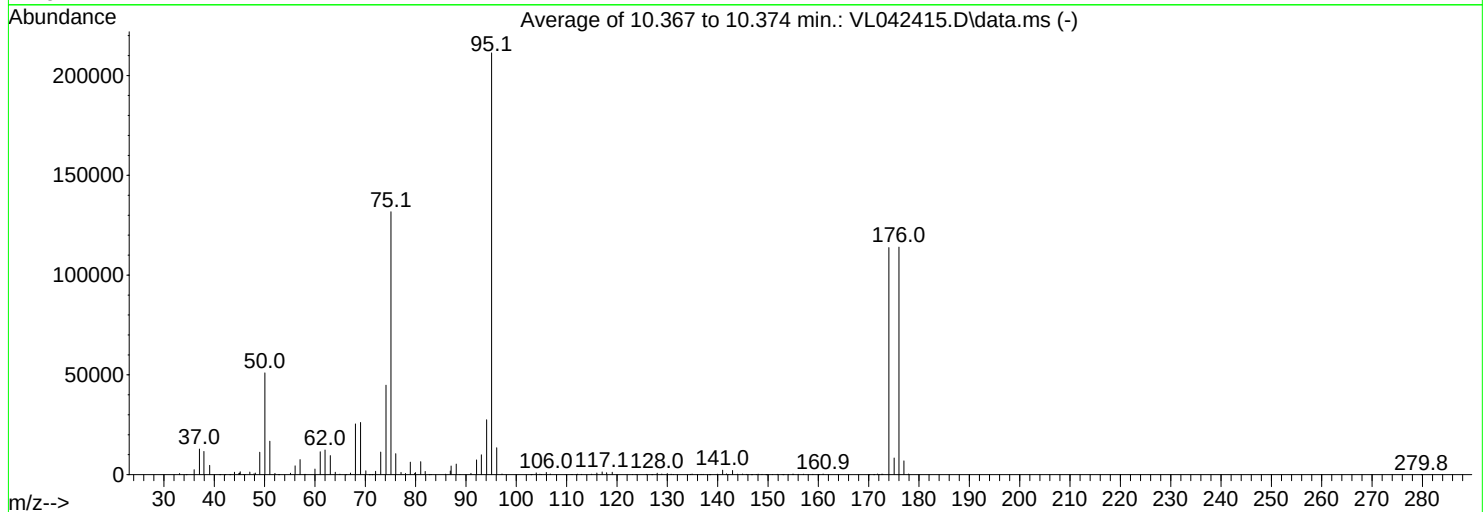


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL042825\
Data File : VL042415.D
Acq On : 28 Apr 2025 07:59
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL041725AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Fri Apr 18 02:14:00 2025

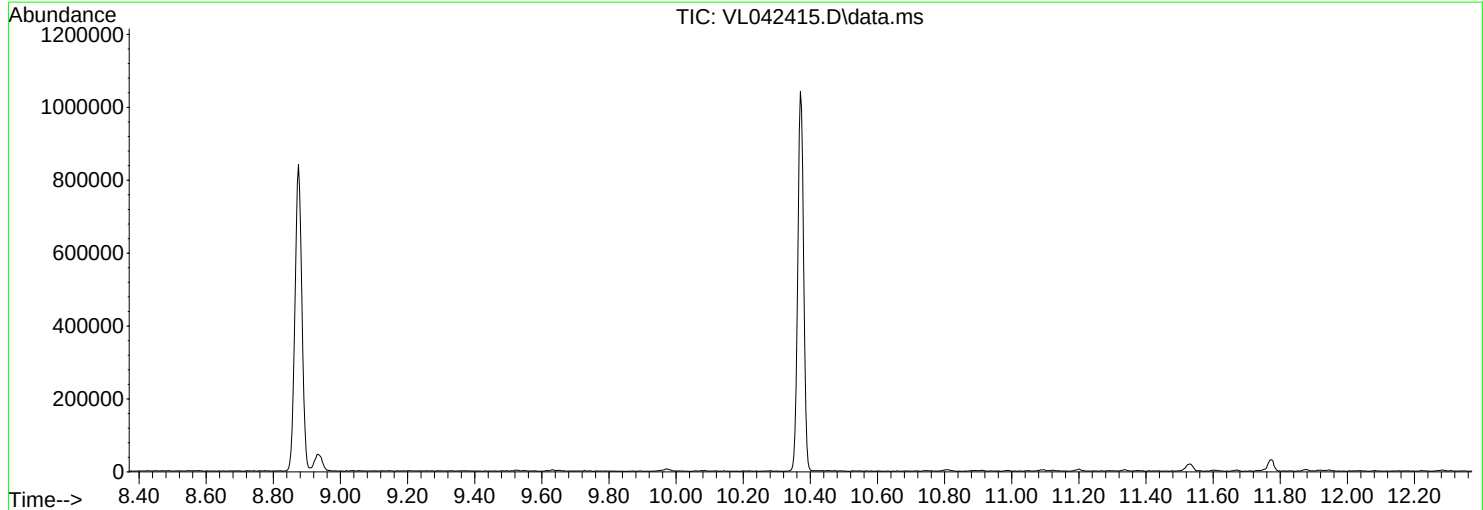

AutoFind: Scans 3176, 3177, 3178; Background Corrected with Scan 3156

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	24.1	51000	PASS
75	95	30	66	62.3	131741	PASS
95	95	100	100	100.0	211371	PASS
96	95	5	9	6.4	13514	PASS
173	174	0.00	2	0.2	277	PASS
174	95	50	120	53.8	113779	PASS
175	174	4	9	7.3	8346	PASS
176	174	93	101	100.2	114021	PASS
177	176	5	9	6.1	6921	PASS

Average of 10.367 to 10.374 min.: VL042415.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	568	45.00	801	52.80	28	64.95	211
34.40	23	45.15	1427	55.15	690	66.10	21
36.00	2525	45.80	97	56.05	4439	67.05	81
37.05	12853	46.15	110	57.05	7539	68.05	2546
37.95	11666	47.05	1286	57.90	141	69.05	26160
39.10	4622	47.90	410	58.15	194	70.10	1912
41.10	44	48.15	784	60.00	2854	70.80	17
42.10	19	49.05	11195	61.05	11453	71.30	23
43.10	21	50.05	51000	62.00	12375	72.05	1693
44.00	1211	51.05	16794	63.05	9540	73.05	11340
44.90	626	52.05	665	64.05	1171	74.10	44853

Average of 10.367 to 10.374 min.: VL042415.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
75.10	131741	85.95	268	97.15	358	111.90	109
76.05	10494	86.90	1875	102.90	23	112.15	279
77.10	1094	87.05	4310	103.10	75	112.95	148
78.00	601	88.05	5267	103.95	877	114.95	268
78.95	6234	88.80	92	104.70	218	116.00	771
79.80	603	91.00	672	105.00	72	117.05	1402
79.95	1072	92.10	7345	105.95	1097	117.95	988
81.00	6517	93.05	9962	106.75	349	119.05	1169
81.90	1590	94.10	27539	109.90	52	123.10	96
82.70	37	95.10	211371	110.90	121	123.80	70
83.10	74	96.10	13514	111.10	106	125.85	142

Average of 10.367 to 10.374 min.: VL042415.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
126.90	17	138.40	17	146.90	96	154.90	249
128.00	742	139.95	260	147.70	89	155.10	242
128.90	337	141.00	2250	148.05	269	156.00	134
130.00	604	141.75	445	148.80	138	157.05	284
130.75	242	142.20	84	149.60	30	158.90	177
131.20	49	142.95	2105	149.90	62	160.00	21
134.60	170	143.95	227	150.90	52	160.95	346
134.90	326	144.95	297	151.85	175	170.00	27
136.00	60	145.75	138	152.80	113	171.00	30
136.70	133	146.00	124	153.00	21	171.75	360
137.10	166	146.70	37	154.05	111	172.10	86

Average of 10.367 to 10.374 min.: VL042415.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.60	261						
172.80	277						
174.00	113779						
175.05	8346						
176.00	114021						
177.00	6921						
177.95	334						
279.80	22						